

[54] **METHOD AND APPARATUS FOR DETECTING OPTICAL PULSES**

2089999 6/1982 United Kingdom .

**OTHER PUBLICATIONS**

[75] Inventors: **James E. Corenman**, Oakland; **Robert T. Stone**, Sunnyvale; **Andras Boross**, Fremont; **Deborah A. Briggs**, San Ramon; **David E. Goodman**, San Francisco, all of Calif.

Goodlin et al., "Systolic Time Intervals in the Fetus and Neonate *Obstetrics and Gynecology*", vol. 34, p. 295 (Feb. 1972).

Goodlin, *Care For The Fetus*, p. 101 (Masson, 1979).  
 Schotz et al., "The Ear Oximeter as a Circulating Monitor," *Anesthesiology*, vol. 19, p. 386 (1958).

Cohen et al., "Self-Balancing System for Medical and Physiological Instrumentation," *IEEE Trans. Bio-Med. Eng.*, vol. BME-18, p. 66, (1971).

Goodlin, "Interpartum Fetal Heart Rate Responses and Plethysmographic Pulse", *Amer. J. Obstet. Gynec.*, vol. 110, p. 210 (1971).

[73] Assignee: **Nellcor Incorporated**, Pleasanton, Calif.

[21] Appl. No.: **840,437**

[22] Filed: **Feb. 24, 1992**

**Related U.S. Patent Documents**

Reissue of:

[64] Patent No.: **4,911,167**  
 Issued: **Mar. 27, 1990**  
 Appl. No.: **175,152**  
 Filed: **Mar. 30, 1988**

*Primary Examiner*—Lee S. Cohen

*Assistant Examiner*—Robert L. Nasser, Jr.

*Attorney, Agent, or Firm*—Townsend and Townsend and Crew

U.S. Applications:

[63] Continuation-in-part of Ser. No. 742,720, Jun. 7, 1985, Pat. No. 4,802,486, which is a continuation of Ser. No. 718,525, Apr. 1, 1985, abandoned.

[51] **Int. Cl.<sup>6</sup>** ..... **A61B 5/00**

[52] **U.S. Cl.** ..... **128/633; 128/665; 356/41**

[58] **Field of Search** ..... 128/632-633, 128/637, 667-668, 670, 671, 687-690, 696, 700, 706, 708

[57] **ABSTRACT**

A method and apparatus for improving the calculation of oxygen saturation and other blood constituents by non-invasive pulse oximeters. The method and apparatus permit more accurate determination of blood flow by collecting time-measures of the absorption signal at two or more wavelengths and processing the collected time-measure to obtain composite pulsatile flow data from which artifacts have been filtered. The processing may occur in the time domain or in the frequency domain. In the preferred time domain embodiment, successive portions of periodic information are weighted and added together in synchrony to obtain the composite pulse information. In the preferred frequency domain embodiment, the time-measure is Fourier transformed into its spectral components to form the composite information. A new method and apparatus for correlating the heartbeat and optical pulse is provided whereby a product of the ECG R-wave and optical pulse signals corresponding to the same heartbeat is obtained, and one signal is time shifted relative to the other until a maximum waveform product corresponding to the heartbeat is determined.

[56] **References Cited**

**U.S. PATENT DOCUMENTS**


Re. 27,042 1/1971 Jorgensen et al. .... 127/700  
 2,827,040 3/1958 Gilford .  
 2,933,081 4/1960 Passannante .

(List continued on next page.)

**FOREIGN PATENT DOCUMENTS**

102816 3/1984 European Pat. Off. .  
 104722 4/1984 European Pat. Off. .  
 104771 4/1984 European Pat. Off. .  
 0104771 4/1984 European Pat. Off. .

**34 Claims, 22 Drawing Sheets**

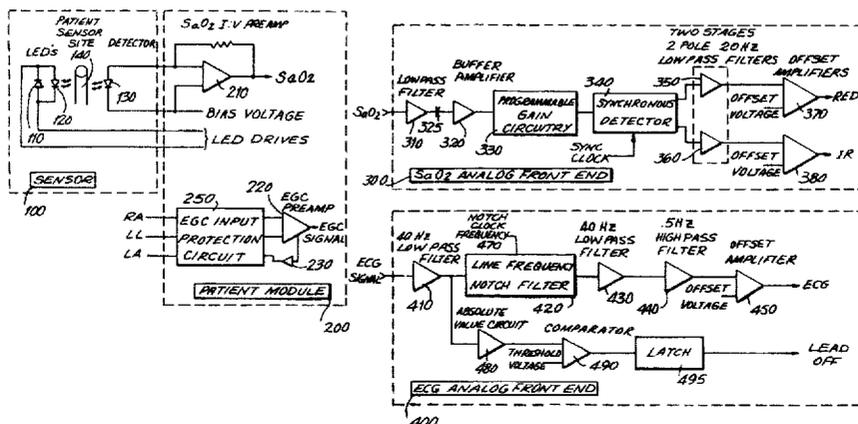

U.S. PATENT DOCUMENTS						
3,318,303	5/1967	Hammacher .....	128/687 X	4,154,230	5/1979 Lee .....	128/661
3,412,729	11/1968	Smith, Jr. .		4,181,134	1/1980 Mason et al. ....	128/689
3,520,295	7/1970	Kelly .		4,216,779	8/1980 Squires et al. ....	128/680
3,590,811	7/1971	Harris .		4,266,554	5/1981 Hamaguri .....	128/633
3,608,545	9/1971	Novack et al. ....	128/700	4,325,384	4/1982 Blaser et al. ....	128/696
3,618,592	11/1971	Stewart .		4,353,998	12/1982 Sawa .	
3,651,806	3/1972	Hirshberg .		4,402,325	6/1983 Sawa .	
3,658,060	4/1972	Eklof .		4,406,658	9/1983 Lattin et al. ....	128/802 X
3,704,706	12/1972	Herczfeld et al. .		4,407,290	10/1983 Wilber .....	128/633
3,734,086	5/1973	Phelps, Sr. .		4,422,458	12/1983 Kravath .....	128/671
3,742,938	7/1973	Stern .....	128/687	4,425,921	1/1984 Fujisaki et al. ....	128/700
3,773,033	11/1973	Rodbard et al. .		4,425,922	1/1984 Conti et al. ....	128/691
3,948,248	4/1976	Zuckerman et al. .		4,440,176	4/1984 Miodownik .....	128/708
3,994,284	11/1976	Voelker .		4,446,868	5/1984 Aronson .....	128/708
3,994,285	11/1976	Doll .		4,446,871	5/1984 Imura .	
3,998,550	12/1976	Konishi et al. ....	356/39	4,450,838	5/1984 Miodownik .....	128/204.23
4,000,461	12/1976	Barber et al. .		4,545,387	10/1985 Balione .	
4,023,563	5/1977	Reynolds et al. .		4,573,478	3/1986 Arnold et al. .	
4,023,564	5/1977	Valiguetta et al. .		4,577,639	3/1986 Simon et al. .	
4,030,485	6/1977	Warner .		4,586,513	6/1986 Hamaguri .	
4,036,211	7/1977	Veth et al. .		4,589,420	5/1986 Adams et al. .	
4,053,911	10/1977	Hudspeth et al. ....	364/415	4,617,937	10/1986 Peel et al. .	
4,063,551	12/1977	Sweeney .		4,653,498	3/1987 New, Jr. et al. ....	128/633
4,086,915	5/1978	Kofsky .....	128/22	4,802,486	2/1989 Goodman et al. ....	128/666 X
				4,824,242	4/1989 Frick et al. .	

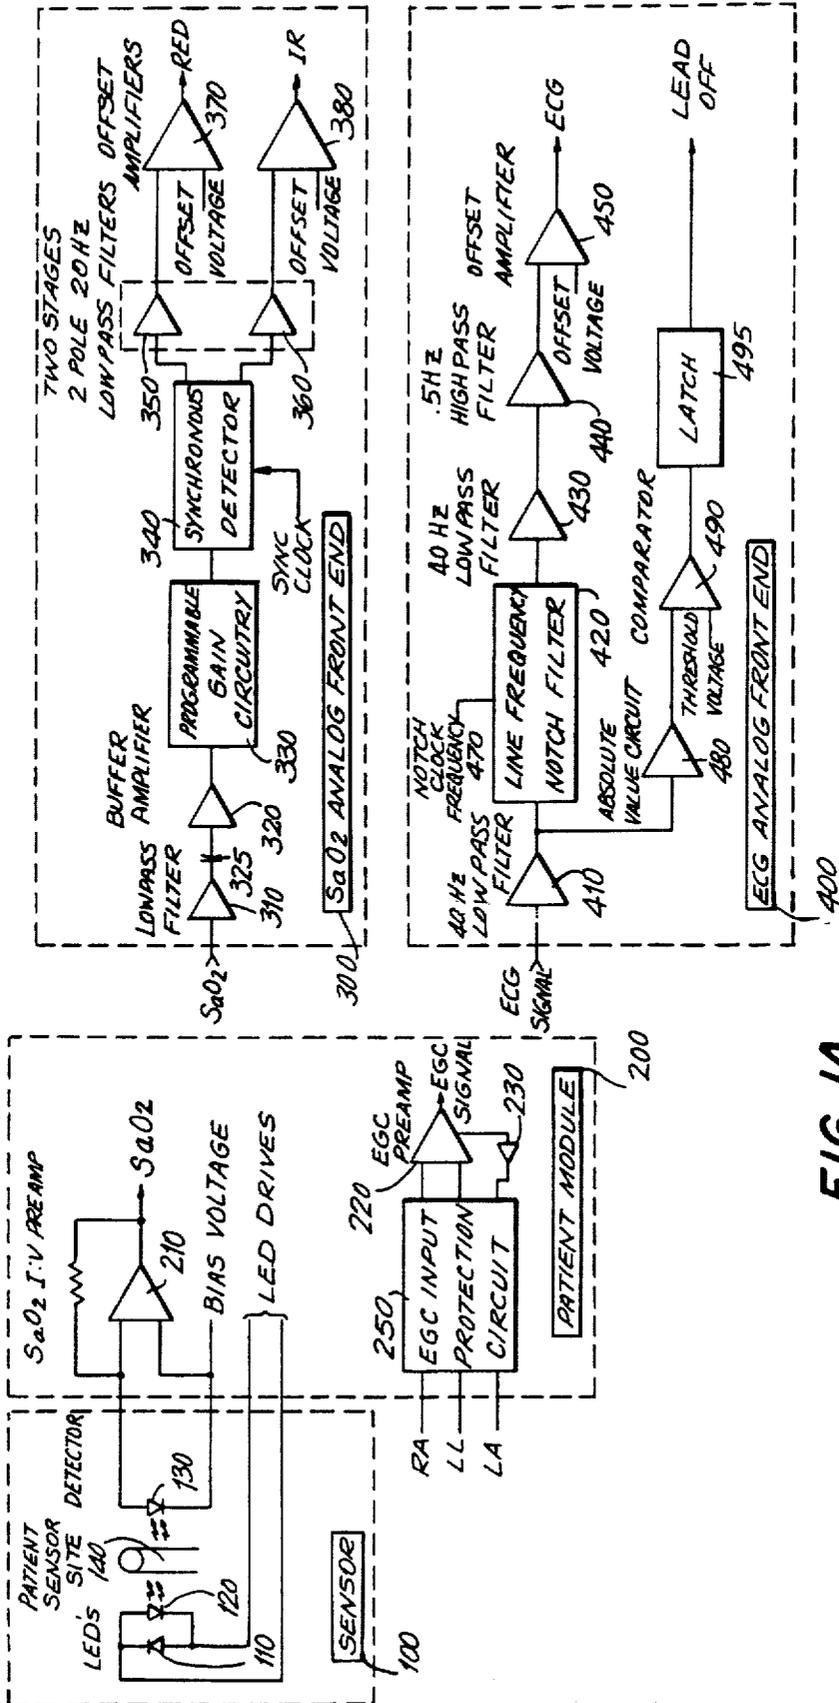


FIG. 1A






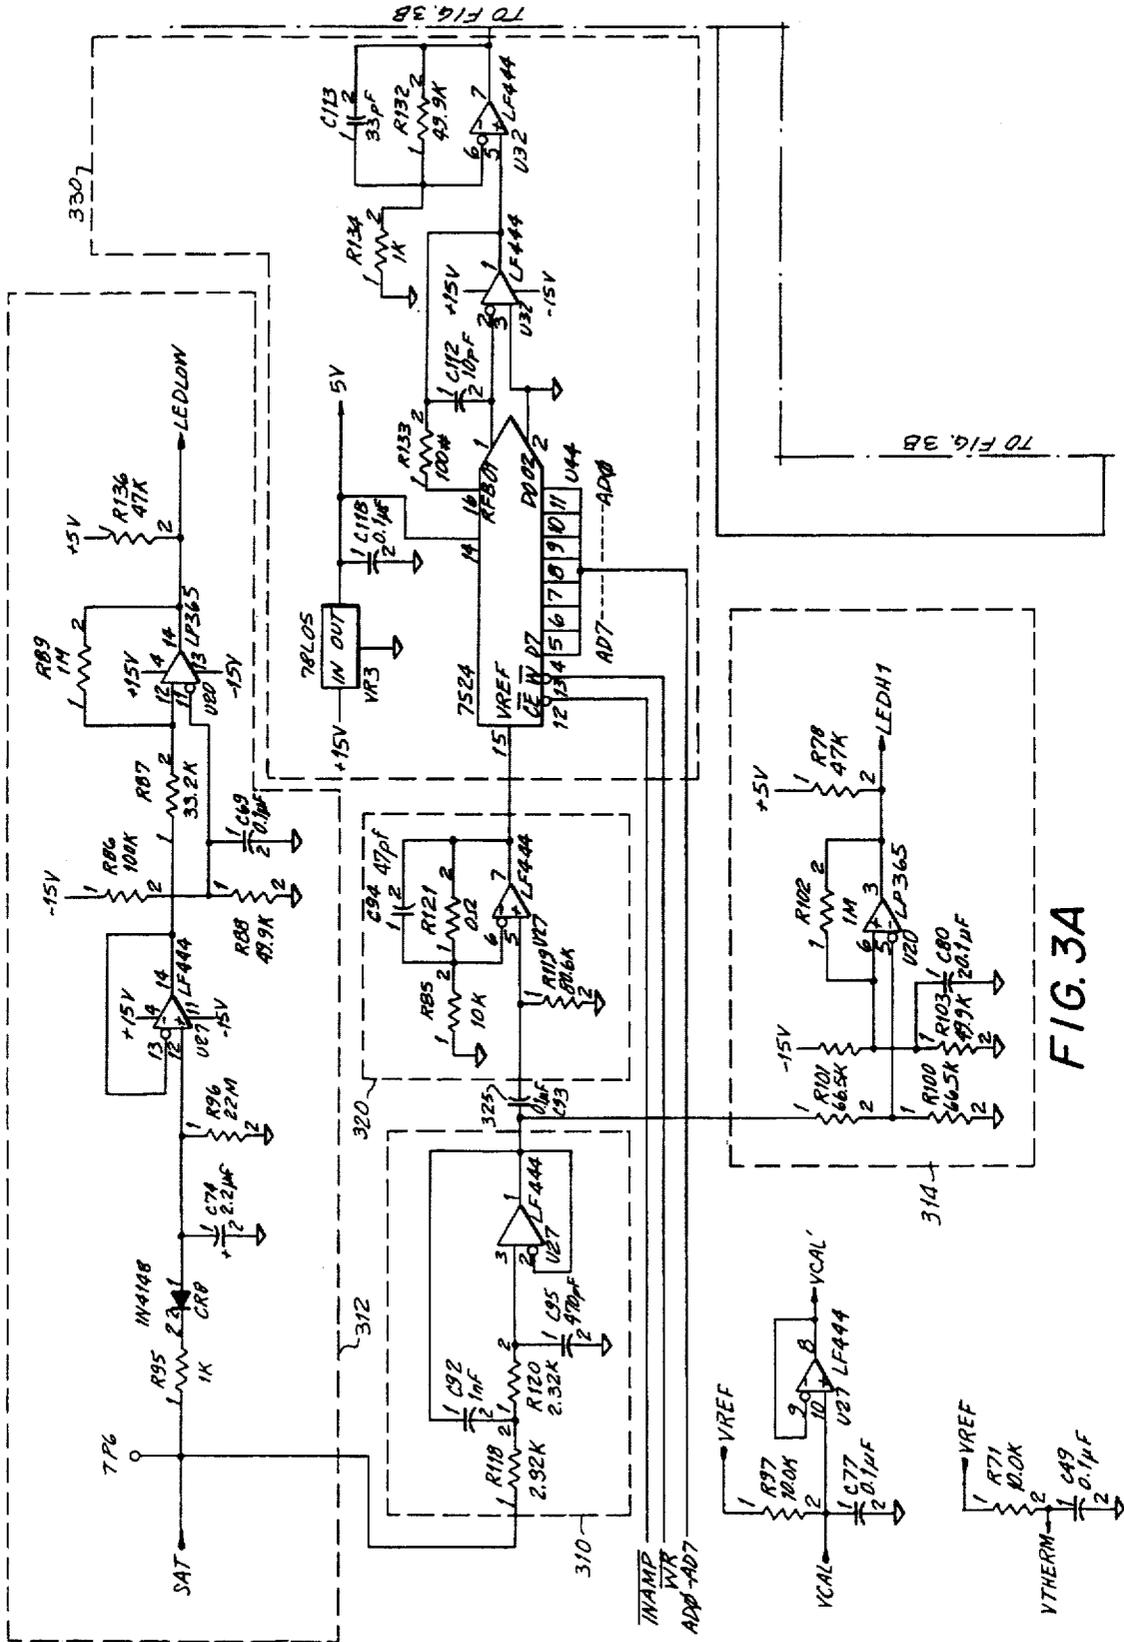


FIG. 3A

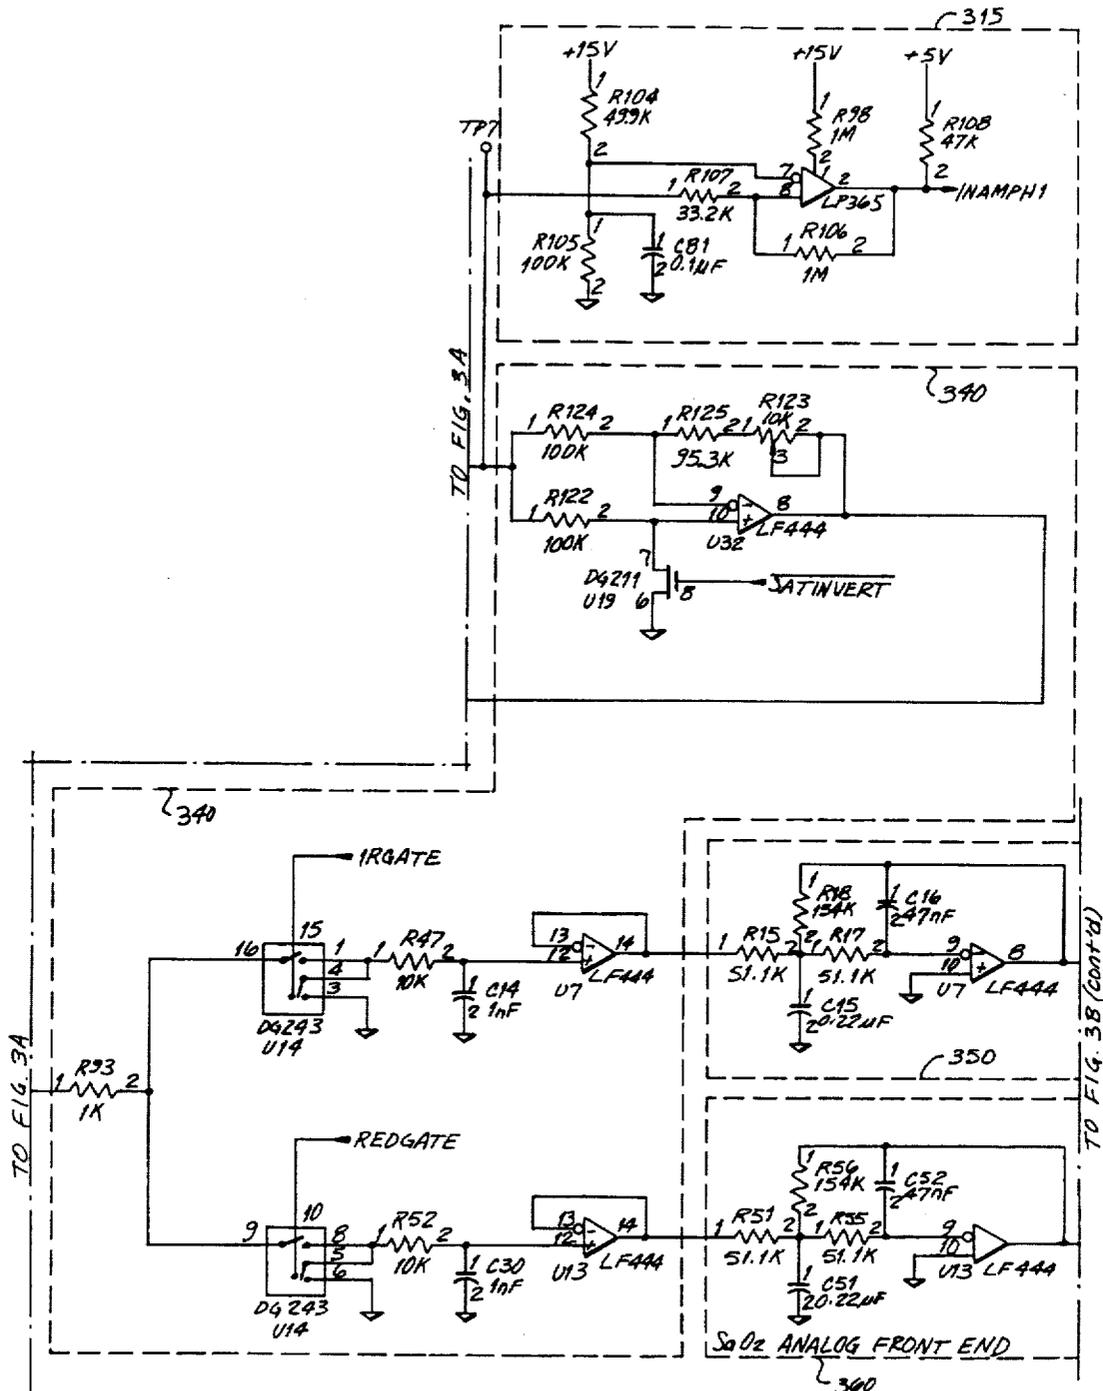

	+15	-15	+5	AGND	DGND
LP365	4	13			16
LF444	4	11			
D6211	13	4	12	5	
D6243	11	14	12	13	
7524				3	

FIG. 3B

FIG. 3B(cont'd)

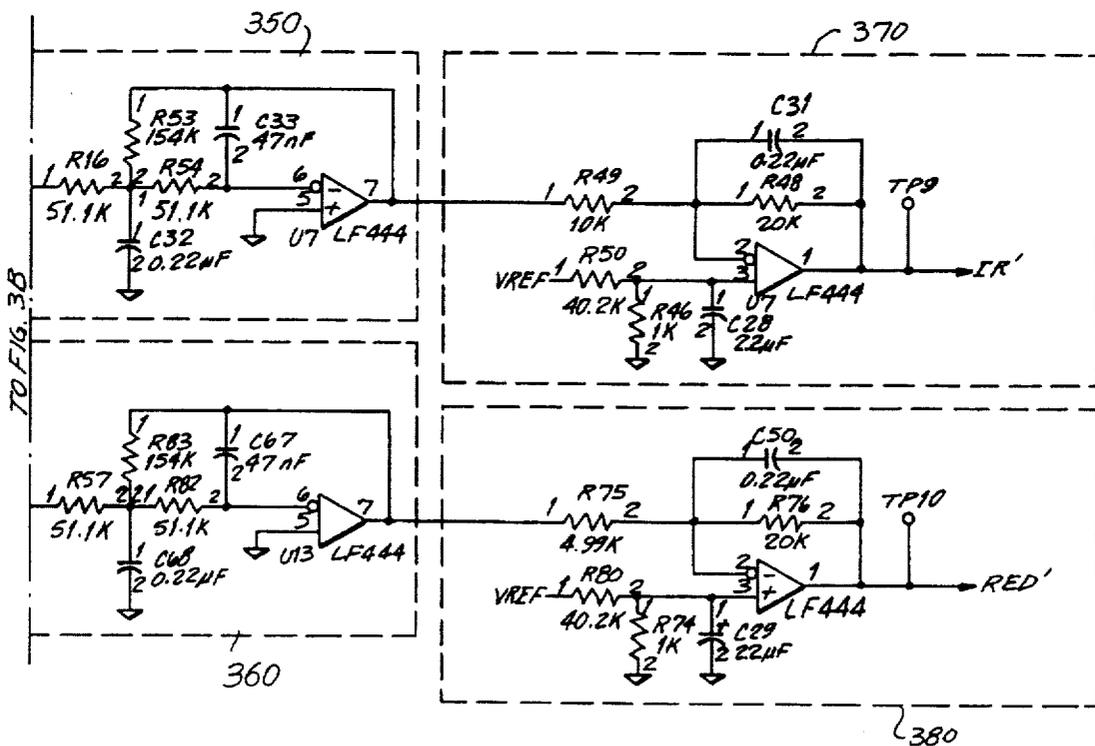


FIG. 4

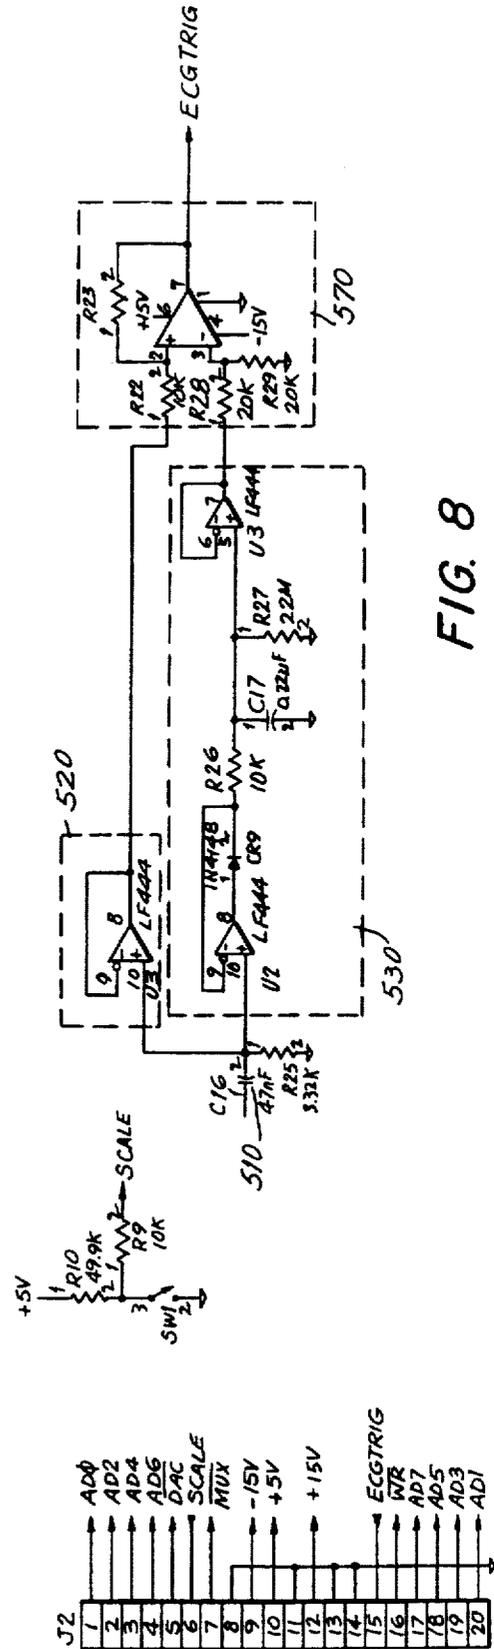
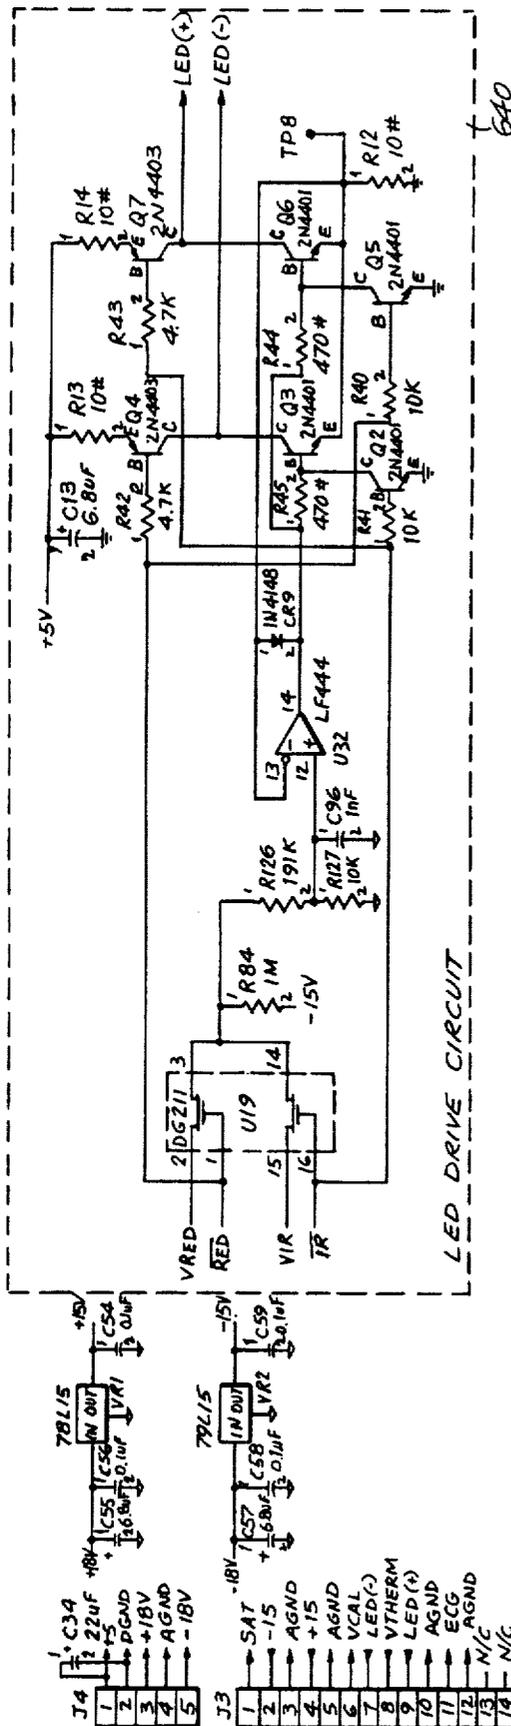


FIG. 8

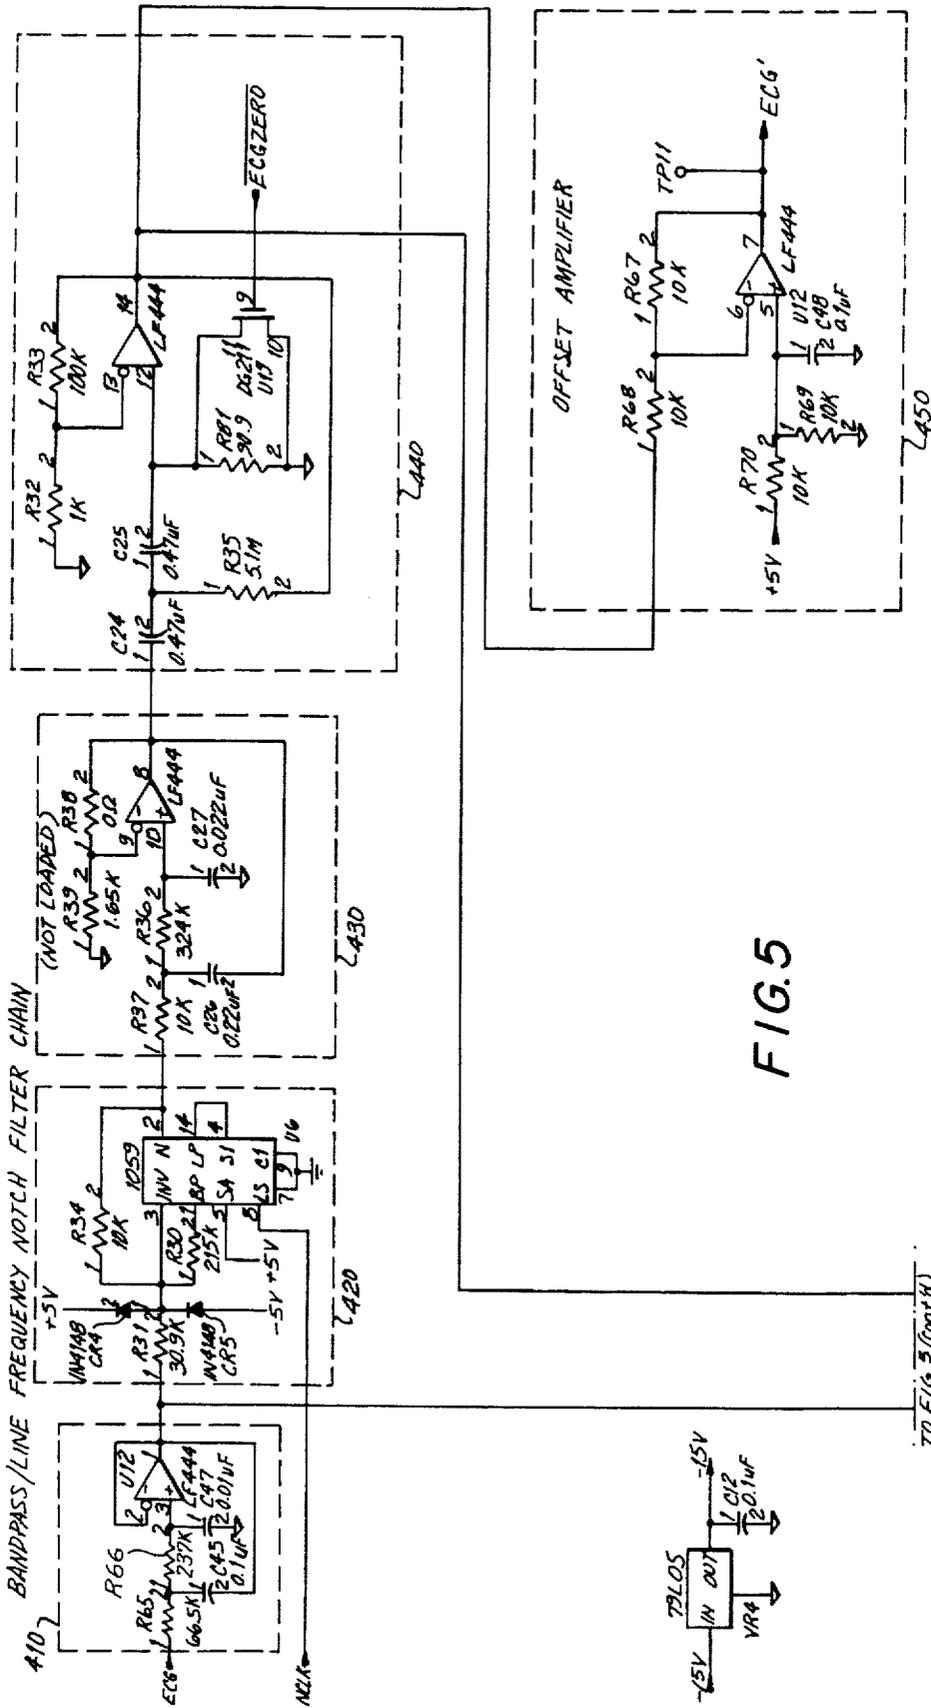


FIG. 5







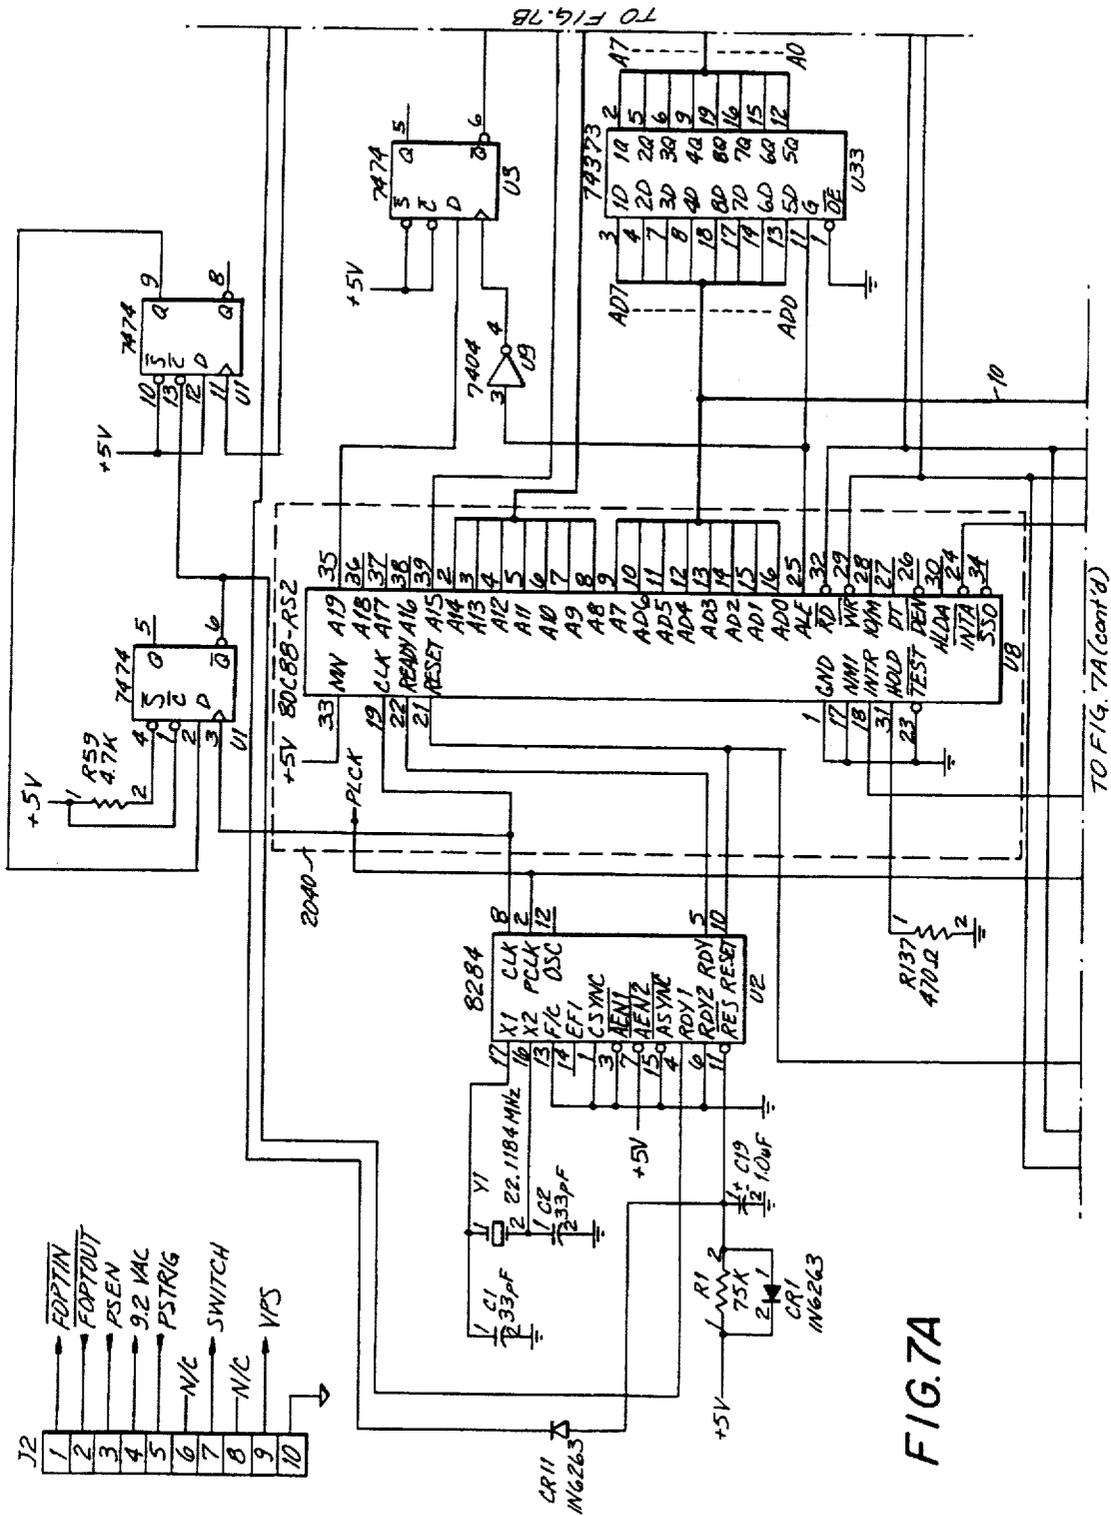


FIG. 7A

TO FIG. 7B

TO FIG. 7A (cont'd)

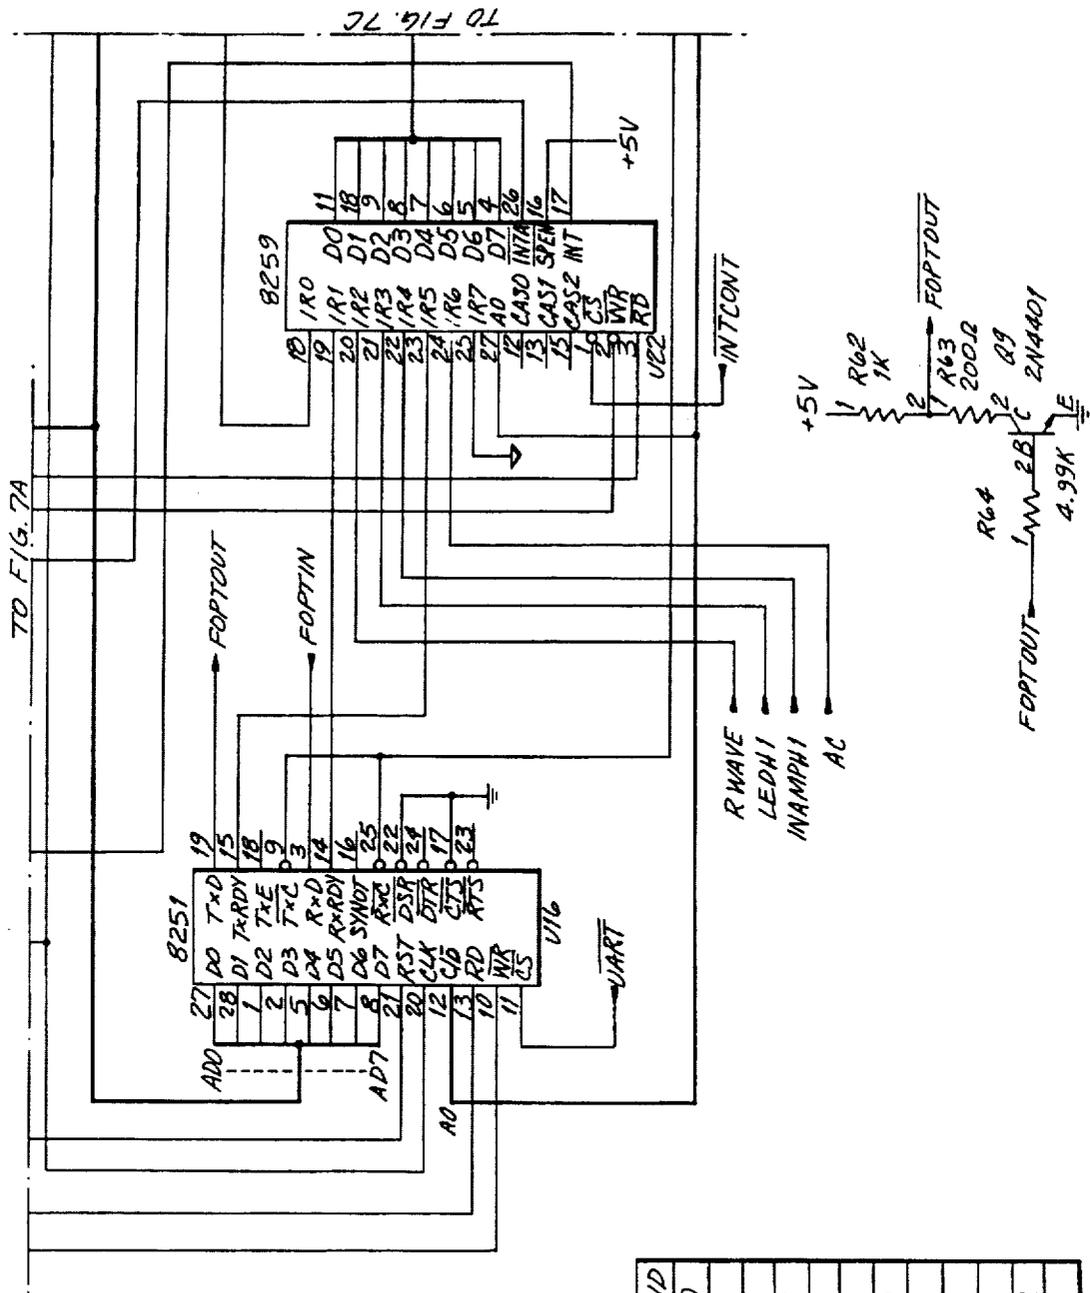


FIG. 7A(cont'd)

+5	DGND
8088	40
8251	26
8253	24
8259	28
8284	18
138	16
374	20
00	14
04	14
393	14
2732	24
27256	28
	20
	4
	12
	14
	9
	8
	10
	7
	7
	7
	12
	14


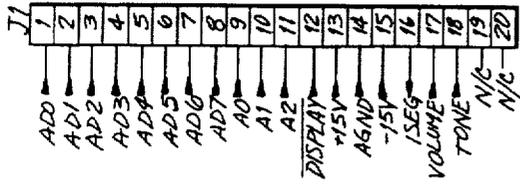


FIG. 7B

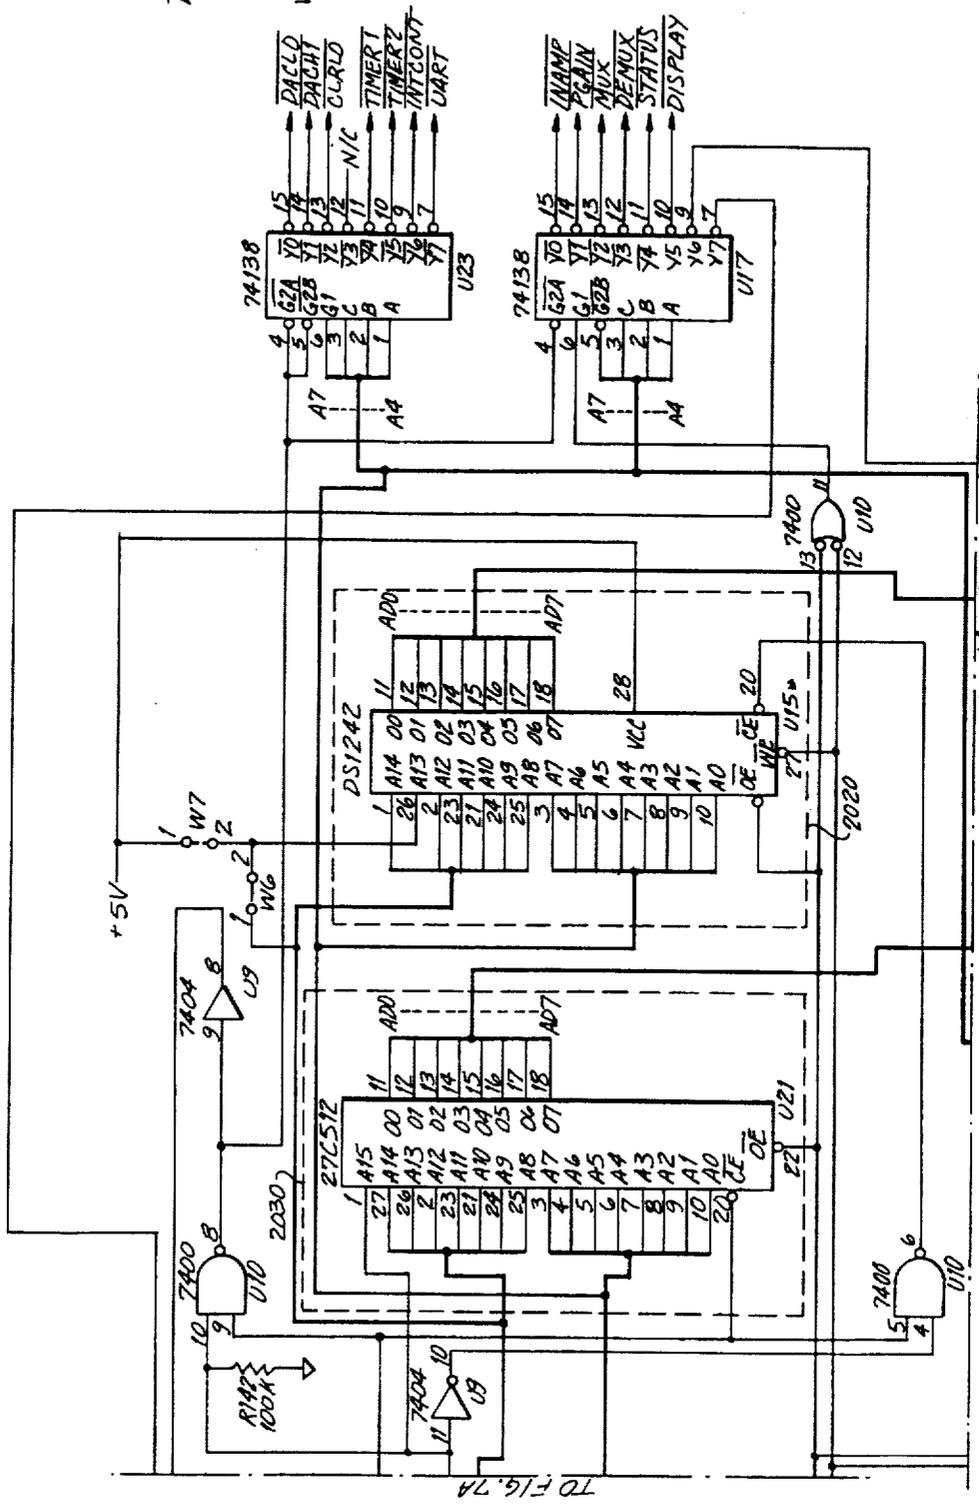

TO FIG. 7C

TO FIG. 7A

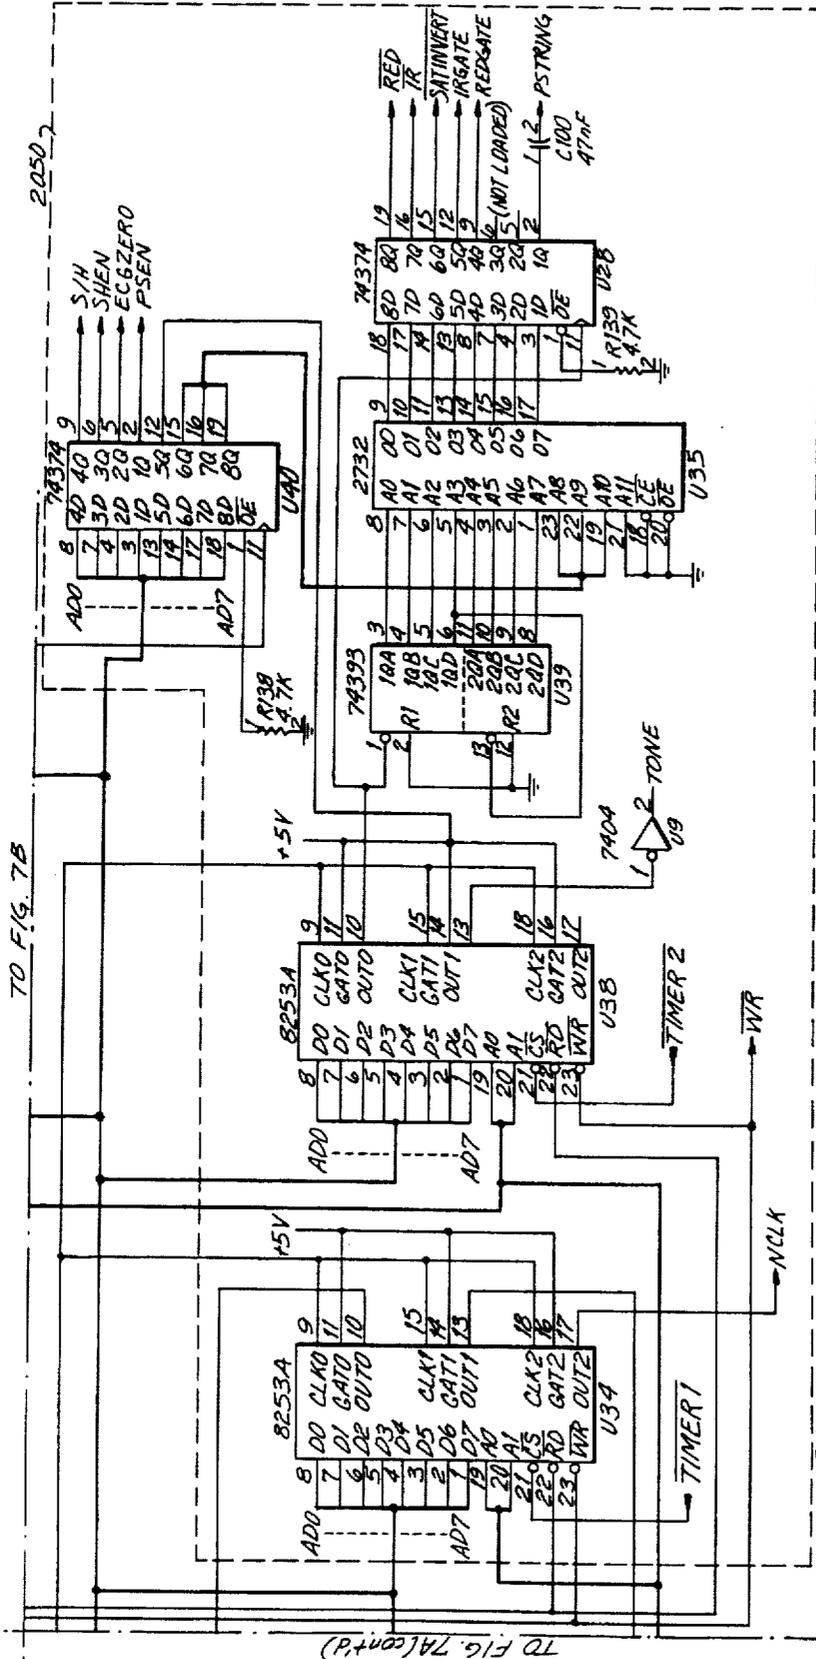


FIG. 7C

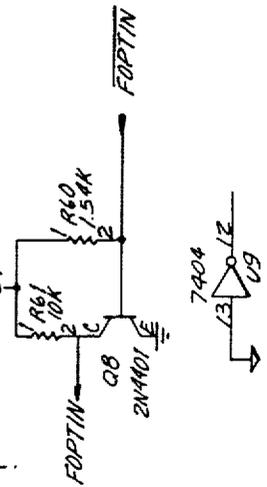


FIG. 9a

SLIDER

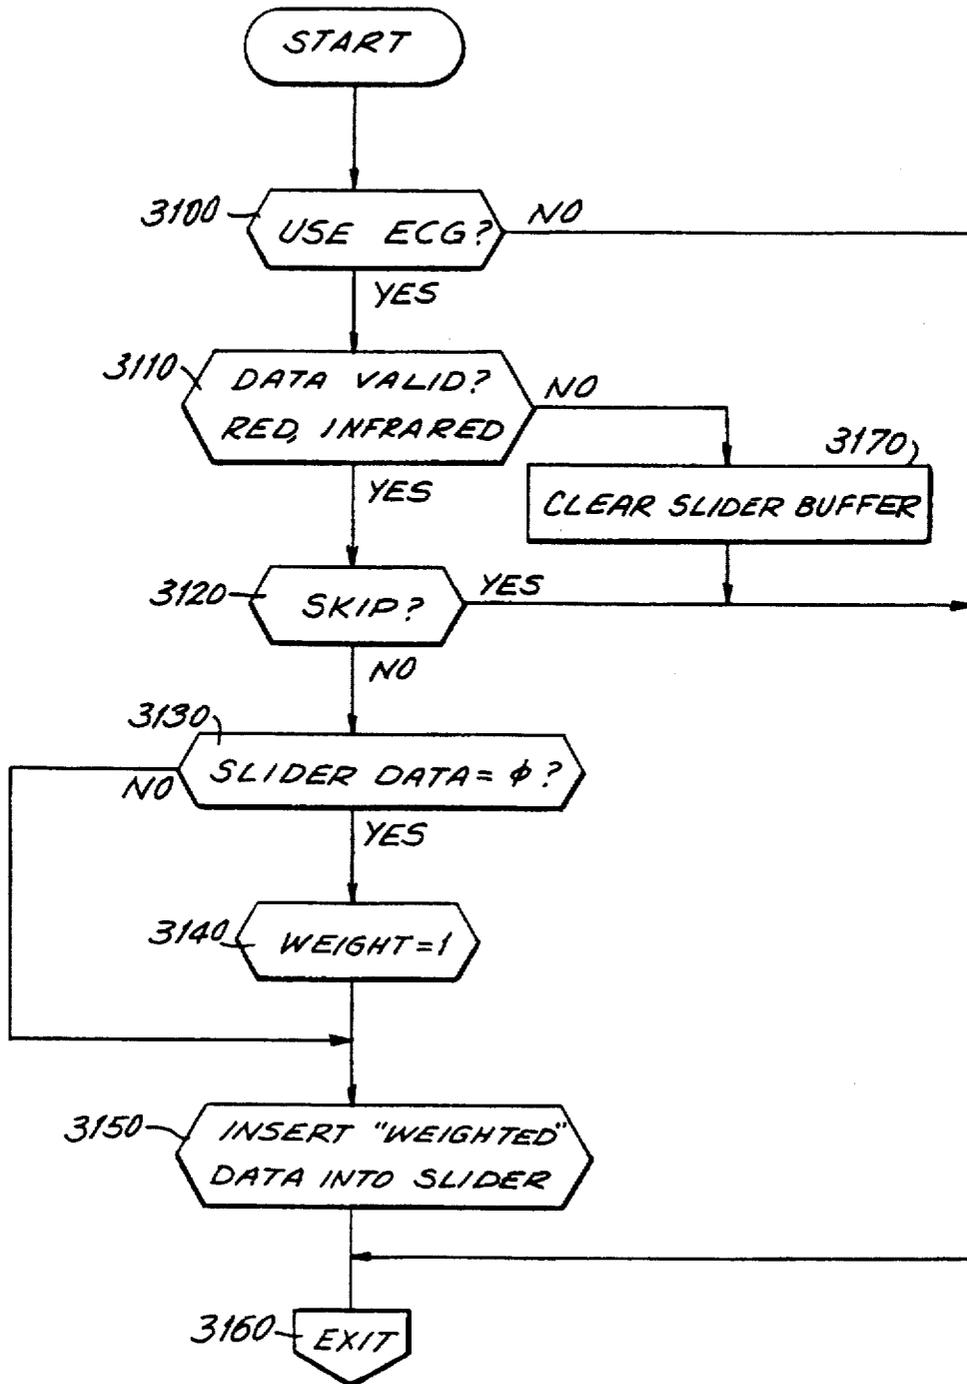
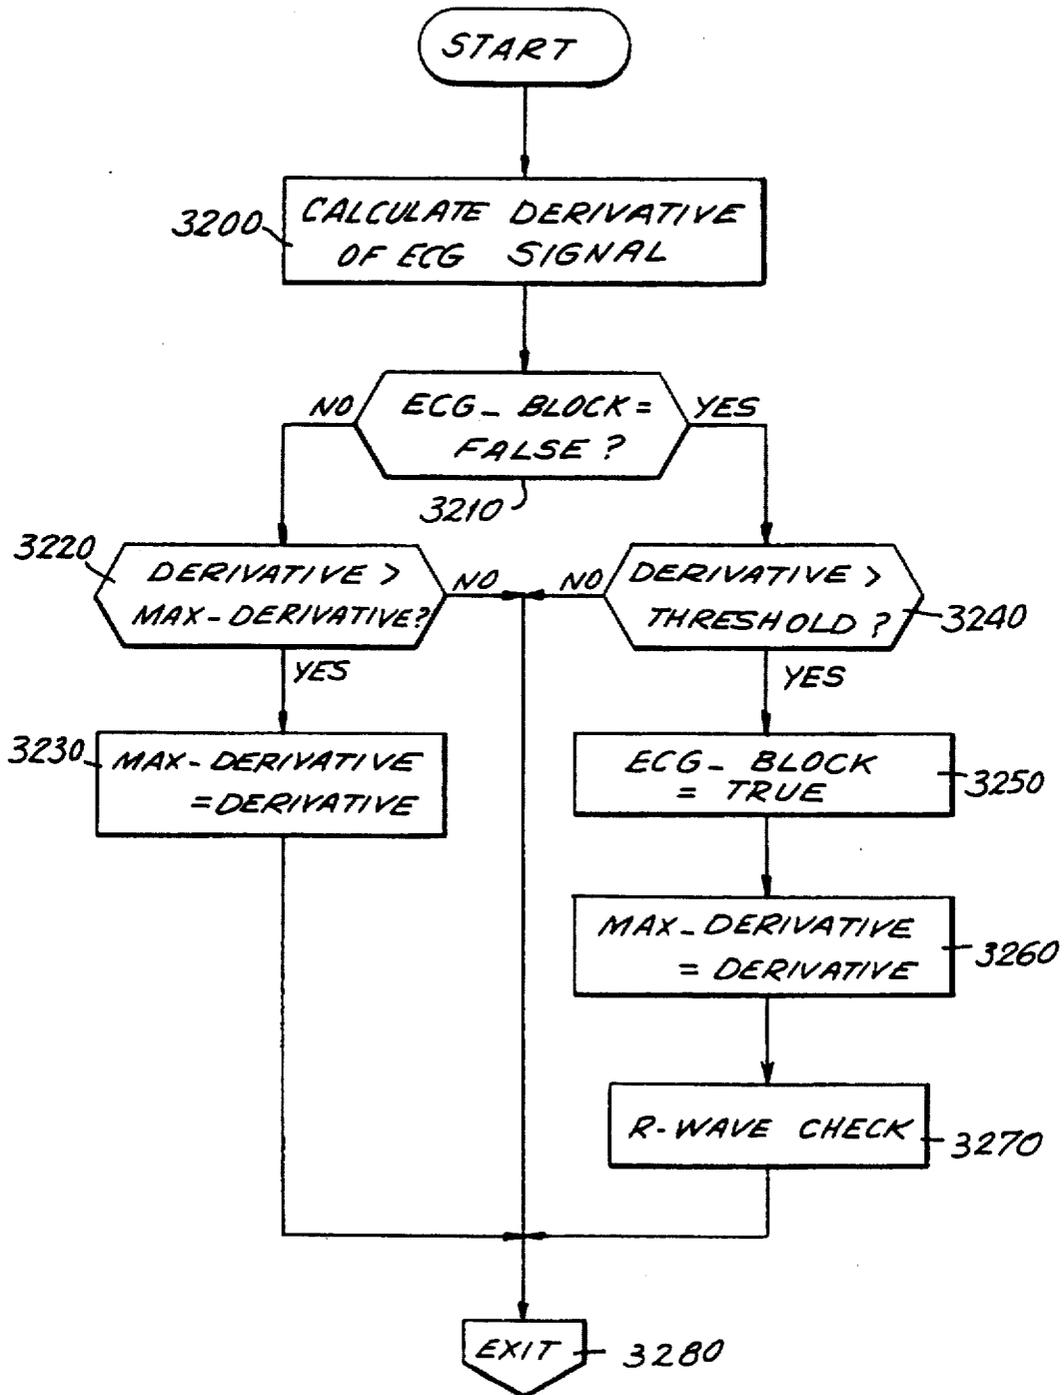


FIG. 9b

ECG-BOX



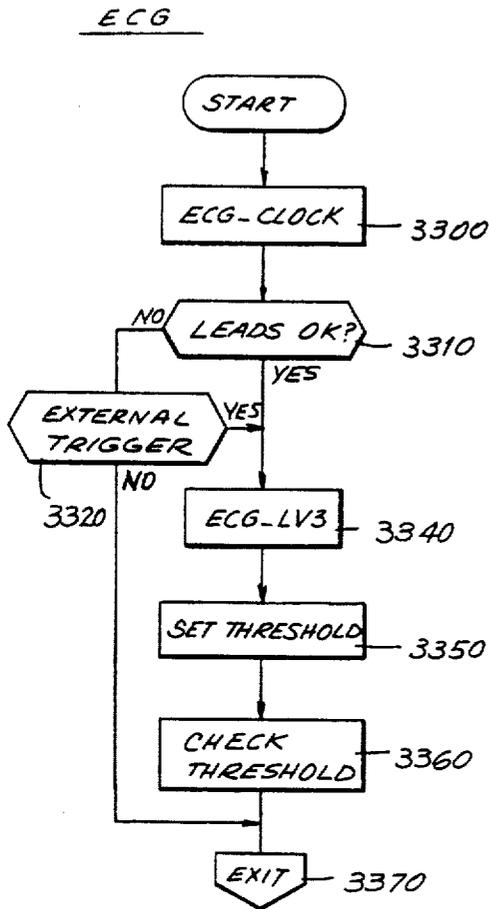


FIG. 9c

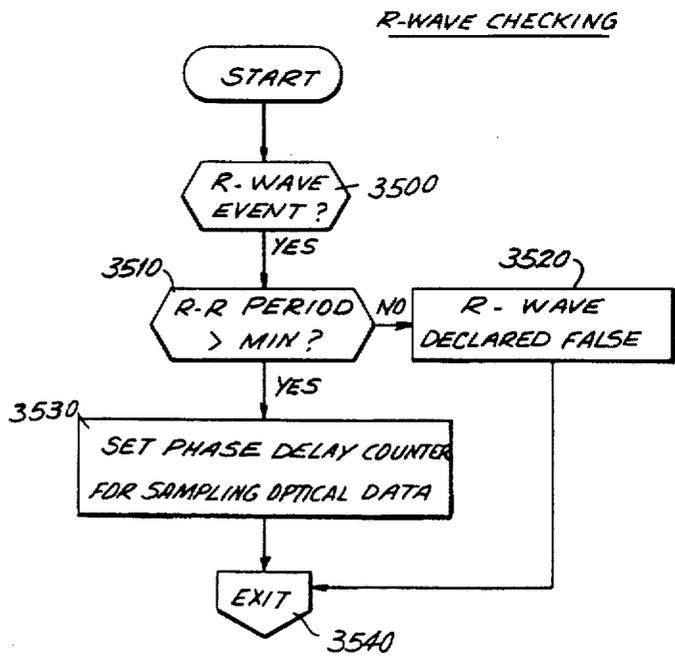


FIG. 9e

ECG - LV3


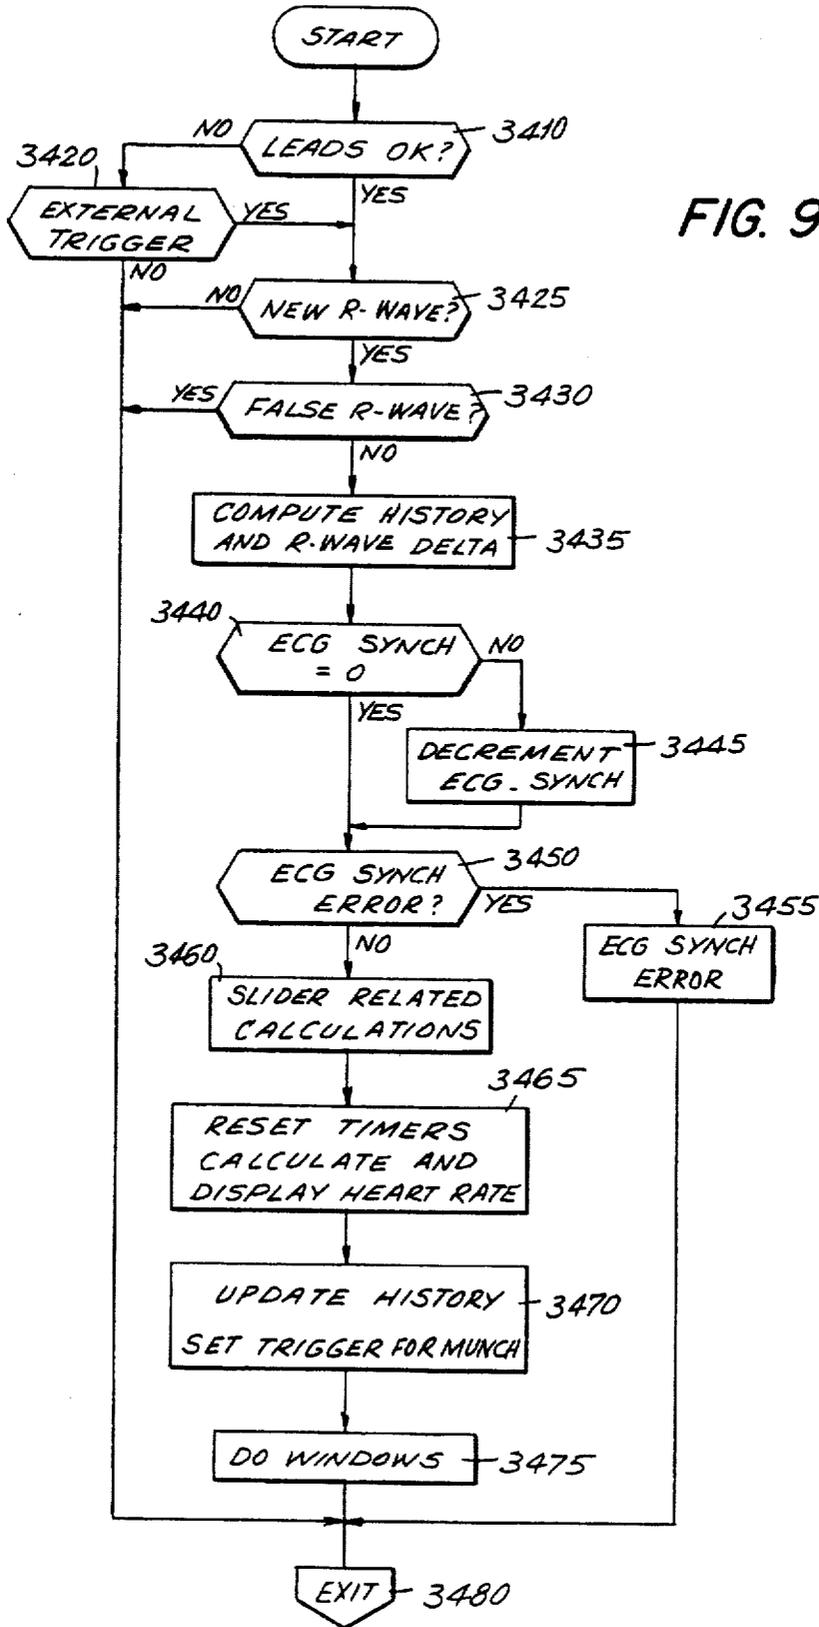



FIG. 9d






FIG. 9f

MAIN LOOP PROCESSING

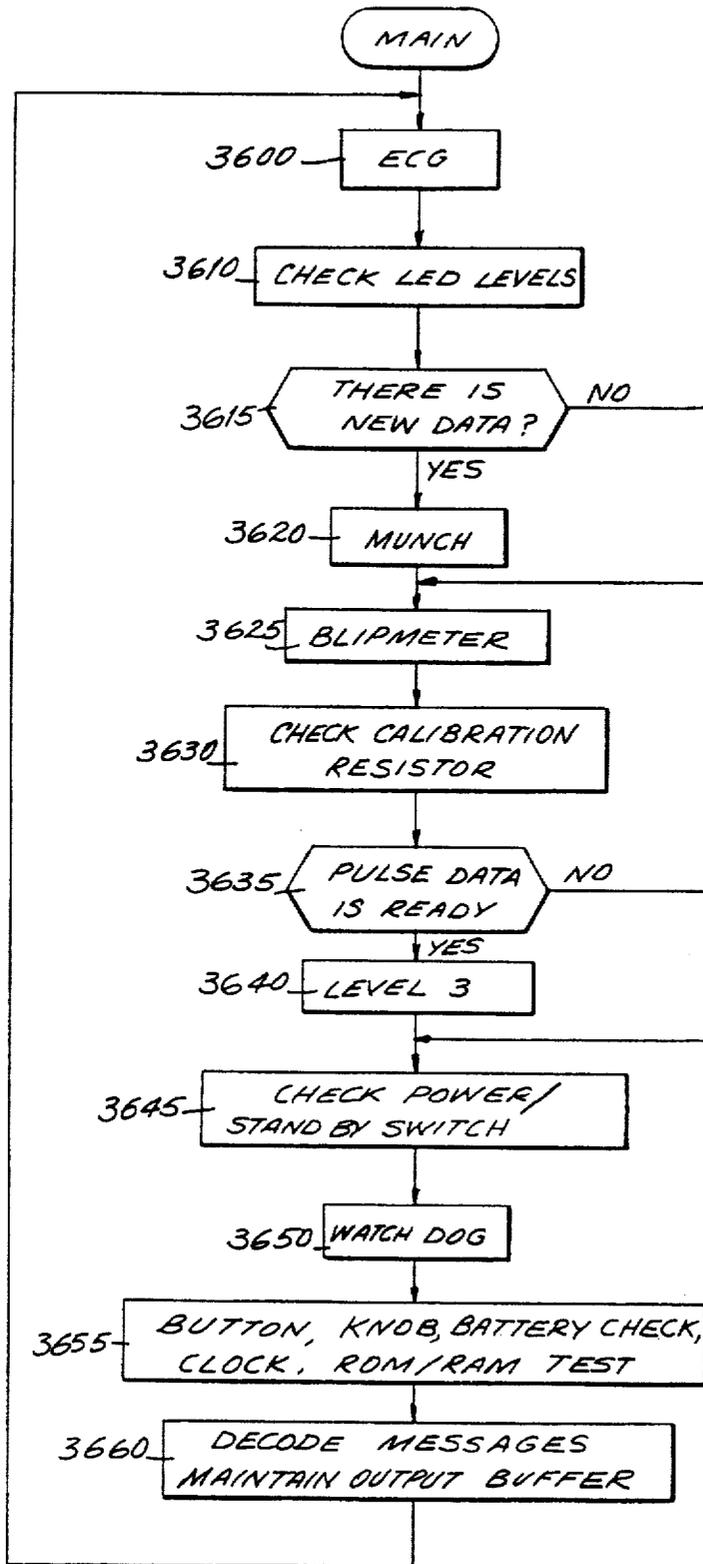

FOURIER OXYMETER FLOWCHART FIG. 10

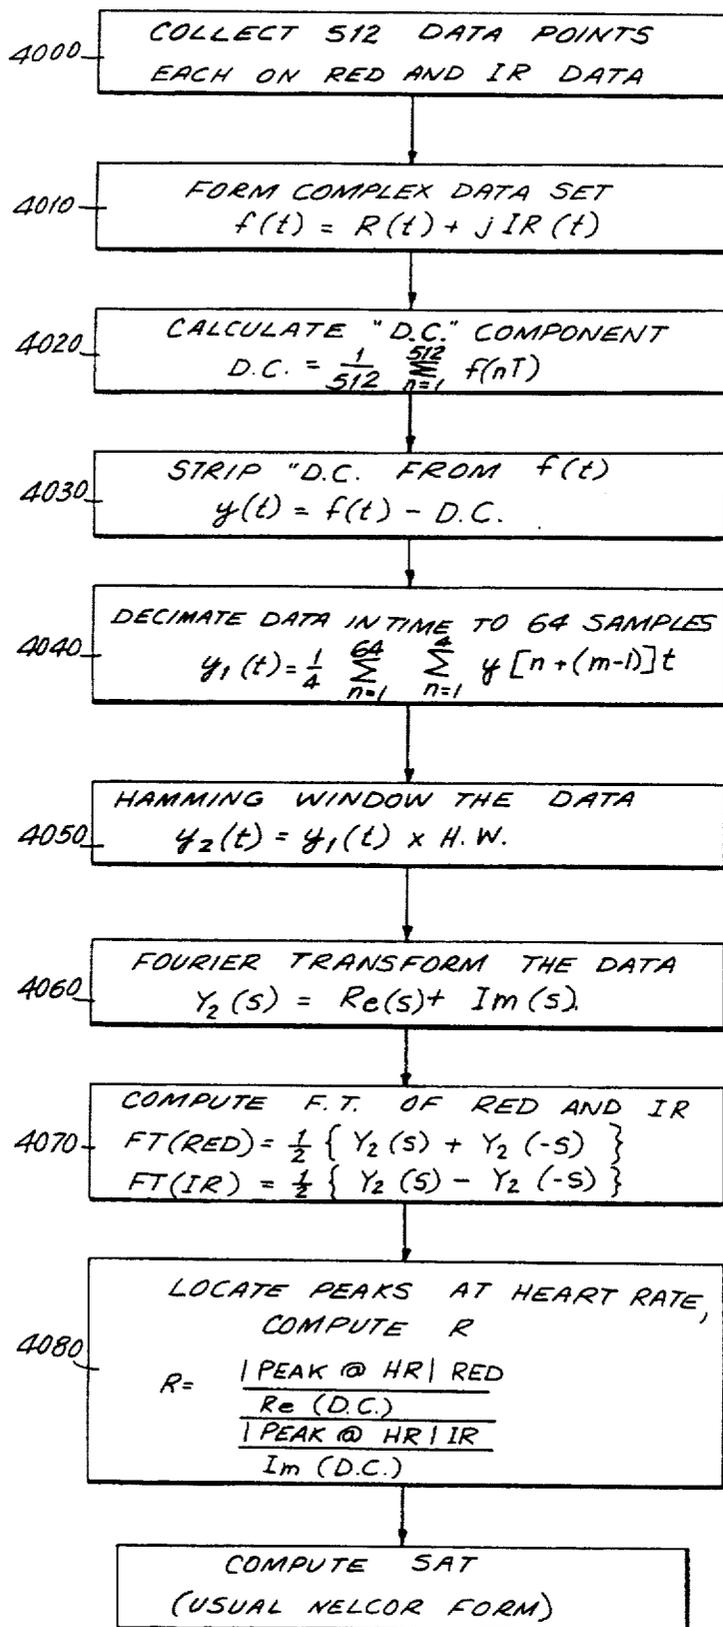

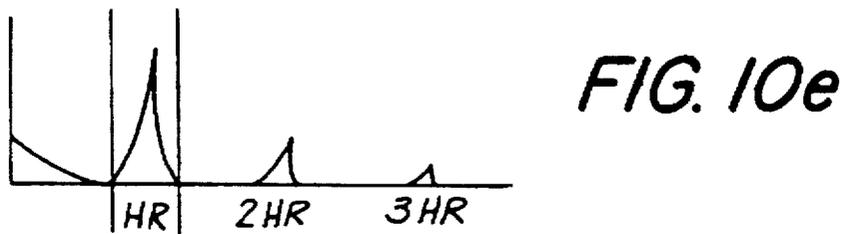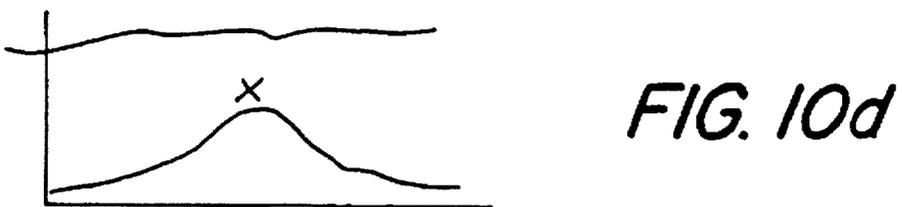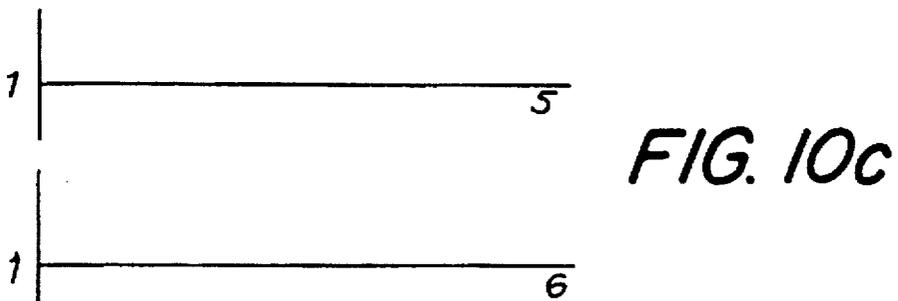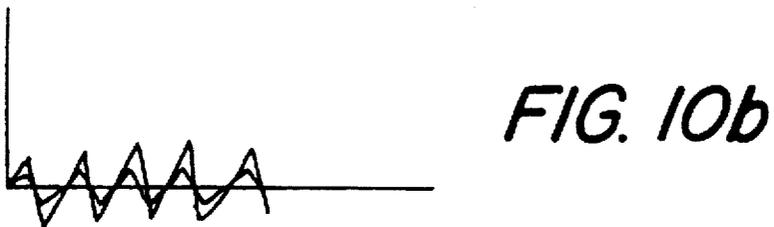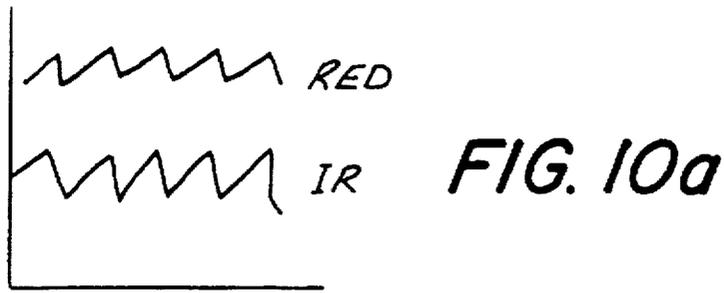

## METHOD AND APPARATUS FOR DETECTING OPTICAL PULSES

Matter enclosed in heavy brackets [ ] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue.

### CROSS REFERENCE TO RELATED APPLICATIONS

This application is a continuation-in-part application of and commonly assigned U.S. application Ser. No. 742,720, now U.S. Pat. No. 4,802,486, entitled Improved Method and Apparatus For Detecting Optical Pulses, filed Jun. 7, 1985 in the names of James E. Corenman and David E. Goodman, which is a continuation of U.S. application Ser. No. 718,525, entitled Improved Method and Apparatus For Detecting Optical Pulses, filed Apr. 1, 1985 in the names of James E. Corenman and David E. Goodman, now abandoned.

This invention relates to non-invasive pulse oximetry and specifically to an improvement on the method and apparatus for photoelectric determination of blood constituents disclosed in U.S. applications Ser. No. 742,720 and 718,525. This specification is accompanied by software appendices A and B.

### BACKGROUND OF THE INVENTION

Non-invasive photoelectric pulse oximetry has been previously described in U.S. Pat. Nos. 4,407,290, 4,266,554, 4,086,915, 3,998,550, 3,704,706, European patent application No. 102,816 published Mar. 13, 1984, European patent application No. 104,772 published Apr. 4, 1984, and European patent application No. 104,771 published Apr. 4, 1984. Pulse oximeters are commercially available from Nellcor Incorporated, Hayward, Calif., U.S.A., and are known as, for example, Pulse Oximeter Model N-100 (herein "N-100 oximeter").

Pulse oximeters typically measure and display various blood flow characteristics including but not limited to blood oxygen saturation of hemoglobin in arterial blood, volume of individual blood pulsations supplying the flesh, and the rate of blood pulsations corresponding to each heartbeat of the patient. The oximeters pass light through human or animal body tissue where blood perfuses the tissue such as a finger, an ear, the nasal septum or the scalp, and photoelectrically sense the absorption of light in the tissue. The amount of light absorbed is then used to calculate the amount of blood constituent being measured.

The light passed through the tissue is selected to be of one or more wavelengths that is absorbed by the blood in an amount representative of the amount of the blood constituent present in the blood. The amount of transmitted light passed through the tissue will vary in accordance with the changing amount of blood constituent in the tissue and the related light absorption.

For example, the N-100 oximeter is a microprocessor controlled device that measures oxygen saturation of hemoglobin using light from two light emitting diodes ("LED's"), one having a discrete frequency of about 660 nanometers in the red light range and the other having a discrete frequency of about 925 nanometers in the infrared range. The N-100 oximeter microprocessor uses a four-state clock to provide a bipolar drive current for the two LED's so that a positive current pulse drives the infrared LED and a negative current

pulse drives the red LED to illuminate alternately the two LED's so that the incident light will pass through, e.g., a fingertip, and the detected or transmitted light will be detected by a single photodetector. The clock uses a high strobing rate, e.g., one thousand five hundred cycles per second, to be easily distinguished from other light sources. The photodetector current changes in response to the red and infrared light transmitted in sequence and is converted to a voltage signal, amplified, and separated by a two-channel synchronous detector—one channel for processing the red light waveform and the other channel for processing the infrared light waveform. The separated signals are filtered to remove the strobing frequency, electrical noise, and ambient noise and then digitized by an analog to digital converter ("ADC"). As used herein, incident light and transmitted light refers to light generated by the LED or other light source, as distinguished from ambient or environmental light.

The light source intensity may be adjusted to accommodate variations among patients' skin color, flesh thickness, hair, blood, and other variants. The light transmitted is thus modulated by the absorption of light in the variants, particularly the arterial blood pulse or pulsatile component, and is referred to as the plethysmograph waveform, or the optical signal. The digital representation of the optical signal is referred to as the digital optical signal. The portion of the digital optical signal that refers to the pulsatile component is labeled the optical pulse.

The detected digital optical signal is processed by the microprocessor the N-100 oximeter to analyze and identify arterial pulses and to develop a history as to pulse periodicity, pulse shape, and determined oxygen saturation. The N-100 oximeter microprocessor decides whether or not to accept a detected pulse as corresponding to an arterial pulse by comparing the detected pulse against the pulse history. To be accepted, a detected pulse must meet certain predetermined criteria, for example, the expected size of the pulse, when the pulse is expected to occur, and the expected ratio of the red light to infrared light of the detected optical pulse in accordance with a desired degree of confidence. Identified individual optical pulses accepted for processing are used to compute the oxygen saturation from the ratio of maximum and minimum pulse levels as seen by the red wavelength compared to the maximum and minimum pulse levels as seen by the infrared wavelength.

Several alternate methods of processing and interpreting optical signal data have been disclosed in the patents and references cited above.

A problem with non-invasive pulse oximeters is that the plethysmograph signal and the optically derived pulse rate may be subject to irregular variants in the blood flow, including but not limited to motion artifact, that interfere with the detection of the blood flow characteristics. Motion artifact is caused by the patient's muscle movement proximate to the oximeter sensor, for example, the patient's finger, ear or other body part to which the oximeter sensor is attached, and may cause spurious pulses that are similar to pulses caused by arterial blood flow. These spurious pulses, in turn, may cause the oximeter to process the artifact waveform and provide erroneous data. This problem is particularly significant with infants, fetuses, or patients that do not remain still during monitoring.

A second problem exists in circumstances where the patient is in poor condition and the pulse strength is very weak. In continuously processing the optical data, it can be difficult to separate the true pulsatile component from artifact pulses and noise because of a low signal to noise ratio. Inability to reliably detect the pulsatile component in the

optical signal may result in a lack of the information needed to calculate blood constituents.

It is well known that electrical heart activity occurs simultaneously with the heartbeat and can be monitored externally and characterized by the electrocardiogram ("ECG") waveform. The ECG waveform, as is known to one skilled in the art, comprises a complex waveform having several components that correspond to electrical heart activity. The QRS component relates to ventricular heart contraction. The R wave portion of the QRS component is typically the steepest wave therein, having the largest amplitude and slope, and may be used for indicating the onset of cardiovascular activity. The arterial blood pulse flows mechanically and its appearance in any part of the body typically follows the R wave of the electrical heart activity by a determinable period of time that remains essentially constant for a given patient. See, e.g., Goodlin et al., "Systolic Time Intervals in the Fetus and Neonate", *Obstetrics and Gynecology*, Vol. 39, No. 2 February 1972, where it is shown that the scalp pulse of fetuses lag behind the ECG "R" wave by 0.03-0.04 second, and U.S. Pat. NO. 3,734, 086.

In prior U.S. application Ser. No. 742,720, copending and commonly assigned, the disclosure (including the software appendix, of which is hereby expressly incorporated by reference, and in corresponding International PCT Application publication No. WO 86/05674 published Oct. 9, 1986, also commonly assigned, there is disclosed an invention for measuring the patient's heart activity and correlating it with the patient's detected blood flow signal to calculate more accurately the patient's oxygen saturation and pulse rate. The correlation includes auto- and cross correlation techniques to enhance the periodic information contained in each individual waveform as well as determine that time relationship of one waveform to another.

Correlating the occurrence of cardiovascular activity with the detection of arterial pulses occurs by measuring an ECG signal, detecting the occurrence of the R-wave portion of the ECG signal, determining the time delay by which an optical pulse in the detected optical signal follows the R-wave, and using the determined time delay between an R-wave, and using the determined time delay between an R-wave and the following optical pulse so as to evaluate arterial blood flow only when it is likely to present a true blood pulse for waveform analysis. The measured time delay is used to determine a time window when, following the occurrence of an R-wave, the probability of finding an optical pulse corresponding to a true arterial pulse is high. The time widow provides an additional criterion to be used in accepting or rejecting a detected pulse as an optical pulse. Any spurious pulses caused by motion artifact or noise occurring outside of that time window are typically rejected and are not used to calculate the amount of blood constituent. Correlating the ECG with the detected optical pulses thereby provided for more reliable measurement of oxygen saturation.

That application and publication refers to a modified N-100 oximeter (the "enhanced N-100 oximeter") whereby the device is provided with an additional heart activity parameter in the form of a detected R-wave from the patient's ECG waveform, in addition to the N-100 pulse oximeter functions, and the microprocessor is modified to include software and memory for controlling and processing the optical signal and heart activity information.

The additional heart activity parameter is independent of the detection of peripheral arterial pulses, e.g., ECG signals, ultrasound, ballistocardiogram, and maybe, accelerometers, nuclear magnetic resonators, electrical impedance techniques, and the like, and provides an identifiable and detectable signal to response to each heartbeat for use by the signal

processing of the oximeter.

It is an object of this invention to provide for improved processing of the detected optical signal containing periodic information corresponding to arterial pulsatile blood flow and aperiodic information corresponding to noise, spurious signals, and motion artifact unrelated to the beating heart and arterial pulsatile blood flow, to improve further the reliability and accuracy of the determination of blood constituent, particularly oxygen saturation of hemoglobin by a non-invasive oximeter device.

It is another object of this invention to provide an improved method and apparatus for collecting successive portions of detected optical signals encompassing periodic information for more than one heartbeat and processing the collected portions to attenuate and filter therefrom aperiodic signal waveforms to provide enhanced periodic information from which the patient's blood constituent can be accurately determined.

It is another object to maintain the enhanced periodic information updated by continuing to add new portions of detected optical signals as they are obtained. It is another object of this invention to create enhanced periodic information by collecting and processing successive portions of detected optical signals wherein the periodic information corresponding to the optical pulses have been added together in phase, synchronized to the occurrence of the patient's ECG and preferably the R-wave signal.

It is another object of this invention to add synchronized periodic information in a weighted fashion so that the most recent portion of detected optical signal is accorded a greater weight in the collected sum than any one prior portion of periodic information data.

It is another object of this invention to create the enhanced periodic information by adding together a predetermined number of the most recent successive portions of detected optical signal, whereby each portion corresponds to a heartbeat event and is given a weight according to its relative age so as to emphasize the newest information in the resultant weighted collective sum.

It is another object of this invention to correlate the periodic information with the ECG R-wave by using a waveform product technique to identify the occurrence of the heartbeat and the optical pulse corresponding to that heartbeat.

It is another object of this invention to evaluate the collected periodic information for a predetermined number of successive portions of the detected optical signal corresponding to a predetermined number of heartbeats in the frequency domain to obtain enhanced periodic information.

It is another object of this invention to Fourier transform a time-measure of detected optical signals including periodic information for N heartbeats to determine the relative maxima at the fundamental frequency N and the minima at the zero frequency for use in determining the light modulation ratio for the amount of blood constituents.

It is another object of this invention to correlate the Fourier Transform of the time-measure of detected optical signals with the Fourier Transform of a time-measure of the ECG signal, and more particularly the R-wave events of the ECG signal, to determine the maxima at the fundamental heart frequency.

It is another object of this invention to correlate the periodic information in a time-measure of the detected optical signal with a time-measure of the detected heart activity, preferably in the form of the ECG signal and more preferably in the form of the R-wave of the ECG signal, to define a predetermined number of samples in a data set and

use frequency domain analysis techniques to evaluate the collected predetermined number of sample data sets to determine the relative maxima at the fundamental frequency.

#### SUMMARY OF THE INVENTION

This invention provides enhanced periodic information with improved rejection of noise, spurious pulses, motion artifact, and other undesired aperiodic waveforms and thereby improves the ability of oximeters to accurately determine amounts of blood constituents.

The present invention provides methods and apparatus for collecting a time-measure of the detected optical signal waveform containing a plurality of periodic information corresponding to arterial pulses caused by the patient's heartbeat and aperiodic information unrelated to pulsatile flow, and processing the collected time-measure of information to obtain enhanced periodic information that is closely related to the most recent arterial pulsatile blood flow. The time-measure may comprise a continuous portion of detected optical signals including a plurality of periodic information from successive heartbeats, or a plurality of discrete portions of detected optical signals including a corresponding plurality of periodic information.

By updating the time-measure of information to include the most recently detected periodic information, and processing the updated measure collectively, an updated enhanced periodic information is obtained (including the new and historical data) from which aperiodic information (including any new aperiodic information) is attenuated. In some embodiments, the updating process includes subtracting detected signals older than a certain relative time from the collected time-measure. Applicants have discovered that by collectively processing a time-measure including successive periodic information to obtain the enhanced periodic information, and using the enhanced periodic information as the basis for making oxygen saturation calculations, the accuracy and reliability of oxygen saturation determinations can be significantly increased. Applicants also have discovered that the time-measures may be collectively processed in either the time domain or the frequency domain.

The amount of a blood constituent, for example, oxygen saturation, can be then determined from this enhanced periodic information (also referred to as composite signal information) by determining the relative maxima and minima in the enhanced periodic information for the respective wavelengths for use in determining the modulation ratios of the known Lambert-Beers equations.

In the preferred embodiment, the detected optical signals are conventionally obtained by passing red (660 nanometers) and infrared (910 nanometers) light through a patient's blood perfused tissue, detecting the transmitted light which is modulated by the blood flow, and providing red and infrared detected optical signals that are preferably separately processed and optionally converted from analog to digital signals, for example, as described above for the Nellcor N-100 oximeter. Portions of the corresponding red and infrared digital signals are then collectively processed in accordance with the present invention and the light modulation ratios are determined based on the resulting enhanced periodic information and used to calculate oxygen saturation.

In the time domain analysis embodiment, the invention provides a method and apparatus for adding together a plurality of successive portions of the detected optical signal waveform whereby one portion of the detected optical signal waveform is added to the following selected portion so that their respective periodic information is added in synchrony,

i.e., in phase. The synchronized sum thus forms a composite portion of detected optical signal information having enhanced periodic information. The following portion is then added to the composite portion so that the new periodic information is added to the prior composite periodic information in synchrony, forming an updated composite portion with update enhanced periodic information. Thereafter, subsequent successive portions of detected optical signal are added to the prior updated composite portion, one at a time, so that the composite and enhanced periodic information are update with each new portion and corresponding heartbeat event.

Weighting functions are applied to the two portions before they are added each other. This provides a scaled or weighted sum that can be adjusted, by selection of the respective weighting functions, to more closely reflect the patient's current condition, rather than the historical condition. In the preferred embodiment, the weighting functions are fractional multipliers which sum to one to provide a stable filter, and are discussed in greater detail below.

The periodic information (optical pulse) generally has the same pulse shape, height, and duration from heartbeat to heartbeat and, as is described in U.S. Ser. No. 742,720, follows heart activity by a determinable period of time.

Applicants have discovered that by synchronizing the occurrence of successive R-waves, it becomes possible to add the corresponding successive portions of the detected optical signal together so that the periodic information (optical pulses) corresponding to the arterial pulse in each portion will add in phase. The weighted magnitude of the new periodic information is reinforced by the existence of the weighted enhanced periodic information at the same time location in accordance with the degree of synchrony. If the new optical pulse is identical to the composite pulse, then the updated result is a composite optical pulse having the same magnitude. If the magnitudes differ, the additive result will differ according to the relative weights.

As a result of the collected, synchronized additive process, any aperiodic information that may be present in the portions of the detected optical signals also are weighted and added to the weighted composite portion waveform. However, because aperiodic signals differ in pulse shape, duration, height, and relative time of occurrence within each portion, and are not synchronous with heart activity, they do not add in phase. Rather, they add in a cancelling manner whereby their weighted sum is spread across the relative time frame of the composite portion.

Applicants have discovered that by processing portions including the periodic information collectively, aperiodic information is attenuated by the absence of any corresponding historical aperiodic signal in the prior composite portion or any subsequent aperiodic at that relative time following heart activity. Further, because the new information can be given a small weight when compared to the absolute weight given the prior composite (as distinguished from the effective lesser weight given to any single prior portion of optical signals as explained below) new aperiodic information is quickly and effectively attenuated, and thus filtered out of the resultant additive portions.

To the extent that any aperiodic information would overlap and thereby obscure some periodic information in a portion, then that aperiodic information would be reinforced by the existing periodic information in the prior composite portion; but only to the extent there was overlap. Thus, the collective processing does not lose optical pulse information hidden by an artifact. Subsequent periodic information lack-

ing "identical" aperiodic information would attenuate any overlapping aperiodic pulse over time.

The collective additive sum having synchronized periodic information waveform thus presents enhanced periodic information that is a composite data set that corresponds to a composite optical pulse from which noise, spurious signals, and motion artifact, have been filtered out. By weighting the collective additive process to favor the most recent information and processing this weighted composite portion as it is update, an accurate estimated optical pulse (enhanced periodic information) that closely reflects the actual conditions is maintained. Basing oxygen saturation determinations on this enhanced optical pulse as it is updated thus provides a more accurate measure than was available by conventional and prior processing techniques.

As discussed in application Ser. No. 742,720, the determinable time period between the R-wave and the optical pulse makes it possible to determine a time window whose time length is long enough to include any likely periodic information, and short enough to exclude detected optical signals that are not of any significant or clinical use in making the determination of the selected blood constituent. A time window can be used in the present invention, following the occurrence of heart activity, to select a portion of detected optical signals for processing in accordance with this invention to reduce the amount of detected optical signal information that must be processed, to improve the rejection of aperiodic signals not proximate to the optical pulse, and to improve the resolution of the oximeter. The timing of the portion can be selected empirically, by considering the time length of the heartbeat pulse and how long it takes for the pulse to travel to the optiCal detection site so that the window is opened before the optiCal pulse maximum occurs at the optical detection site. In the preferred embodiment, the portion of signal is portion that begins 40 ms after the detection of an R-wave event, based on experimentation, and ends after the relative minimum of the optical pulse is detected, which ending time can vary from portion to portion, and may be, for example, about 230 ms after the R-wave event.

The time domain processing of collective weighted portions of the detected optical signal waveforms synchronized by the R-wave of the ECG waveform provides the equivalent of an optimal filter in the frequency domain, whose band-pass elements are those of an ideal heartbeat for the patient under examination. All frequencies which are found in a normal heartbeat are passed with weights of one, and all nonsynchronous frequencies are rejected with attenuation depending on the degree of asynchrony, and the time length of the filter (the effective number of portions processed collectively). As the weight of the periodic information corresponding to the current heartbeat is decreased, greater rejection of the low-frequency aperiodic artifacts occurs, but the delay in reporting the most accurate arterial pulsatile flow increases.

The weighting functions also assure that the new periodic information is not absorbed into the time and amplitude average of the old data. Using fractional weights provides scaling of the new and old composite information sum, and when the fractional weights add to one, stable performance of the filter is assured. Repeated multiplication of the old data by weights less than one accomplish the effective removal of older data, thus limiting in effect the number of periods processed collectively.

In the preferred embodiment, the detected optical signal information is processed in digitized form. Because the successive digitized information is weighted and added, the amount of digital computer memory required to contain the historical and updated composite periodic information only need be as long as the time period for a relative typical heartbeat, so that it can contain the entire time for a selected portion including an optical pulse. This simplified oximeter operation.

In the preferred embodiment, applicants have found that optimal performance occurs when the most recent information is accorded a weight of  $\frac{1}{2}$  and the historical weight-averaged composite information is accorded a weight of  $\frac{1}{4}$ . Weights which are in powers of 2, e.g.,  $\frac{1}{2}$ ,  $\frac{1}{4}$ ,  $\frac{1}{8}$ , etc., are attractive to use with binary digital computers because they require simpler mathematical operations, however, they do not necessarily provide the optimal time and noise attenuation tradeoff in selecting weighting functions.

The resultant enhanced periodic information is a weighted composite optiCal pulse that is evaluated in the same manner that prior oximeters evaluated individual pulses they determined were appropriate optical pulses for determining blood constituents, whether or not the criteria included use of a time window. The relative maxima and minima for each of the red and infrared composite optical pulses are separately determined and used in the modulations ratios for determining amounts of blood constituents, e.g., in the modulation ratio R of the Lambert-Beers equations that are commonly used to determine oxygen saturation of arterial hemoglobins as described below. As additional data sets are taken, the collective set of periodic information is updated. Consequently, the most recent waveform data representing the actual amount of blood constituent is included in the updated composite optical pulse form which the updated oxygen saturation can be determined and displayed. Although the foregoing and following discussions generally discuss only a detected optical signal, it should be understood that both the red and infrared signal are separately obtained and processed by these techniques, except as indicated.

In another embodiment of the time domain embodiment, the time-measure of the detected optical signal is collected in a different manner. The digitized portions of information that are to be weighted, synchronously added together, and processed collectively are accumulated in a memory device having sufficient memory locations for storing separately the raw data for a predetermined number of portions of the detected optical signal. The time of occurrence of the R-wave also may be stored in memory as a pointer for the raw data. This filter embodiment permits assigning a different weighting function to each raw data set corresponding to a different heartbeat in the memory, to improve the attenuation of artifacts and reduce the time needed to estimate the actual arterial pulsatile flow in the detected optical signal.

In this embodiment, for N predetermined heartbeats, the average value of the detected optical signal for those N heartbeats is computed by assigning a weight to each data set and adding the weighted data for each heartbeat synchronously into a buffer with a weight of 1, then dividing by N. After each computation, the data set from the oldest stored heartbeat is subtracted from the buffer. As a new R-wave is detected, the incoming data is added to the buffer, and the result is divided by N for computation of relative amplitudes of the two wavelength (red and infrared) periodic information. Thus, the equivalent delay in determining the arterial oxygen saturation is N/2 times the heartbeat interval. The stored R-wave pointer may be used to correlate the weight-

ing function with the raw data so that the oldest data is given the smallest weight and the most recent data is given the greatest weight, and after each composite heartbeat computation, the oldest data set can be subtracted from the buffer before the following newest data is added.

In an alternate embodiment of the time domain analysis techniques, the ECG and periodic information can be correlated by using a waveform product of the ECG signal and the detected optical signal to determine the location of the optical pulse from which oxygen saturation and heart rate values may be computed. The R-wave of the ECG has the largest slope component within the ECG waveform. In the optical pulse waveform in the portion of detected optical signal, the largest slope is created when the heart contacts to expell blood and thereby produce the arterial pulse. Thus, because of the determinable time interval between the ECG R-wave and the appearance of the optical pulse at the detection site, the detected optical signal can be moved backwards in time, relative to the ECG waveform, an amount equal to the determined time interval so that the portions of maximum slope in the two signals will be aligned, and their product will be at a maximum.

A periodic signals, such as motion artifact, having high slopes will not occur synchronously on the ECG and the detected optical signals. Therefore, once the two periodic waveforms are aligned, the largest slope product of the two will occur at the heart rate interval. Detection of the maximum slope product can be used to pinpoint the occurrence of a heartbeat, and the portion of the detected optical signal that is associated with that maximum slope product can be used for calculating oxygen saturation.

In this embodiment, the time interval between the R-wave and the optical pulse can be determined by collecting a predetermined time measure history of optical and ECG waveform data comprising  $n$  seconds. The time interval must be long enough for the samples to include at least one R-wave and one pule respectively, given that the heartbeat may vary from 20-30 beats per minute at the slowest rates. A measure of six seconds is acceptable. The samples are conventionally digitized and stored in memory. An array of sample-to-sample slopes is obtained for each  $n$  second sample of the ECG waveform and for the second half of each optical pulse waveform sample. The first half of the optical pulse sample is discarded so that when the first optical pulse in the second half is slid backwards, the first R-wave peak it will come upon will be its corresponding R-wave, and also so that the most recent heartbeat data is detected. An optical pulse in the first half of the sample could miss its R-wave.

The number of slope values in the second half of the optical waveform, i.e. the number of data points minus 1 at the given sampling rate of 57 samples per second (every 17.5 msec), is taken as  $m$ , which corresponds to  $n/2$  seconds of data.

A slope product is obtained by multiplying each element of the optical slope array by its corresponding three and one-half points in the ECG slope array (the ECG signal is sampled every 5 msec) and summing the products. This process is repeated for each of the  $m$  optical sample points as the optical waveform slope array is moved backwards relative to the ECG slope array, one optical waveform sample at a time. The backwards slide terminates when the first sample of the ECG waveform is aligned with the first sample of the second half of the optical waveform.

The maximum slope product is found to occur after the optical waveform slop array has been slid  $x$  optical sample points backwards. This establishes the time interval  $t$  between the detection of the ECG R-wave and the detection of the optical pulse produced by the same heart contraction. This time interval  $t$  is expressed in terms of a number of

waveform samples, and is used in the determination of heartbeat occurrence.

Computation of the aligned waveform slope product will yield a slope product value for each optical waveform sample. A percentage of the maximum slope product produced during the establishment of the time interval component can be used to compute a maximum product threshold. For example, a percentage of 75% of the maximum slope product may be used. Thus, when the ECG and optical signal waveform slope product exceeds the maximum product threshold, it is likely that a true pulse has been located.

The "true" pulse, as it appears the detected optical signal, can then be validated and processed using known techniques for calculating oxygen saturation from detected optical signals. For example, the slope product could be used to synchronize the R-wave events so that the corresponding periodic information can be added in phase in accordance with the preferred embodiment of this invention, or the slope product could be used as an additional criterion for accepting the corresponding optical pulse as valid, and the oxygen saturation determination could be based only on the corresponding optical pulse. Alternately, the waveform product for the maximum and minimum values for the red and infrared waveforms could be used as the maximum and minimum values in calculating saturation. Also, one could integrate some portion of the selected waveform product waveform and compare the area of the change to the area of the total signal to obtain the relative transmittance for use in determining saturation. For example one could integrate the portion above a selected threshold and compare that area to the integral of the entire pulse.

Qualified "true" pulses are then used to update the slope product threshold value so that it will change as the patient's condition changes or as the quality of the received signals changes.

Applicants also have discovered that a time-measure of detected optical signals containing a plurality of periodic information corresponding to successive heartbeats can be collectively processed and analyzed using frequency domain techniques. These frequency domain techniques utilize the synchronous nature of the heartbeat and the asynchronous characteristics of noise, spurious signals, and motion artifacts.

In the frequency domain, the optical signals for a given wavelength corresponding to the pulsatile arterial blood flow have spectral components including a zero frequency at the background intensity level, a fundamental frequency at the frequency of the beating heart, and additional harmonic frequencies at multiples of the fundamental frequency. Noise, spurious signals, and motion artifact that appear in the detected optical signal have frequencies that spread across the spectrum. Transient changes in the average background intensity level have frequencies that appear spread out between the zero frequency and the fundamental frequency.

The frequency domain embodiment of the present invention provides a method and apparatus for collecting a time-measure of detected optical signals including a predetermined number of optical pulses, converting the collected detected optical signals into the frequency domain, and analyzing the spectral components of the frequency spectrum thereby to determine the red and infrared relative maxima intensity at the fundamental frequency, and relative minima at the background intensity zero frequency, for use as maxima and minima in the percentage modulation ratio for calculating oxygen saturation.

Applicants have discovered that if the digitized values of the time domain detected optical signals are stored in memory for a period of N heartbeats, and the stored data set is transformed into the frequency domain using Fourier Transforms, the amplitude of the fundamental heartrate is summed for the N heartbeats and appears in the frequency spectrum at a location of N cycles. In contrast, the amplitude of asynchronous signals is 1/m where m is the number of data points in the digitized stored data set, and appear spread across the frequency domain spectrum. The average intensity of the detected optical signal background intensity appears at the spectral line corresponding to zero cycles and corresponds to the average background intensity for that wavelength.

If the detected optical signal for the red and infrared signals is considered as a single complex data set, i.e., having real and imaginary components, only a single Fourier transform is required to analyze the spectral contents of the collective time-measure of the two signals. If F(s) represents the Fourier Transform of the complex data set  $f(t) = \text{Red}(t) + j\text{IR}(t)$  (for Red(t) being the red detected optical signal and IR(t) being the infrared detected optical signal), the Fourier Transform of the real component of f(t) is found by

$$F\{\text{Re}\{f(t)\}\} = \frac{1}{2}\{F(s) + F^*(-s)\}.$$

Similarly, the Fourier transform of the imaginary component of f(t) is found by

$$F\{\text{Im}\{f(t)\}\} = \frac{1}{2j}\{F(s) - F^*(-s)\}.$$

$F^*(-s)$  is the complex conjugate of F(s) with the indexes reversed.

The relative amplitudes of the red and infrared fundamentals at the heartrate has been found to be equivalent to the foregoing time domain techniques for computation of arterial oxygen saturation. The amplitude data may be found by searching the frequency spectrum in the region of expected heart rates for a relative maximum and insuring that this is the fundamental by determining the existence of another relative maximum at twice this rate. This provides a technique for obtaining relative modulation data to calculate arterial oxygen saturation without the need to identify the heart rate independently, e.g., by detecting the ECG. Alternately, the amplitude data at the fundamental may be found by the use of independent heart rate determining mechanism such as ECG or phonoplethysmography or the like to determine a heart rate. However, unlike the time domain techniques, the precise time of occurrence of each heartbeat need not be determined and the optical signal and a heart rate parameter need not be correlated to obtain accurate saturation values. Rather, it is sufficient to obtain an approximate indicator of heart rate, which will facilitate identification of the fundamental frequency and improve saturation reliability.

The number of spectral lines computed is preferably optimized to include the expected range of clinically applicable heartbeats (from 20–250 beats per minute), while the length of the data set is selected by the allowable equivalent delay in displaying measured arterial oxygen saturation. A time-measure of data of, for example, 9–10 seconds represent delays of only 4–5 seconds in the display of computed saturations, and, depending upon the computational speed of the oximeter microprocessor, the time-measure can be updated in a timely fashion every 1 to 2 seconds.

In the preferred embodiment, the optical signal is digitized at 57 samples per second for each red and infrared signal. When 512 data points are accumulated, the data is Fourier transformed, and the red and infrared fundamental maxima are located. The percentage modulation ratio (red/infrared) is computed by dividing the energy at each maxima by the zero cycle background intensity for that wavelength, then dividing the red modulation by the infrared modulation. The resultant ratio, R, is used in the manner set forth in the Lamber-Beers equations for calculating arterial saturation of hemoglobin. The collective data can be updated so that new data points replace the oldest data points by using a push down stack memory or equivalent so that the transform, evaluation and saturation calculation could be made after each new data set was obtained.

An alternative embodiment of the frequency domain analysis technique includes sampling the real time ECG waveform and the real time detected optical signal at high rates, e.g., 1000 samples per second. By examining the ECG wave, the time of occurrence for each heartbeat and the appropriate sample rate to obtain m samples during that heartbeat could be determined. Thus, the data set for each heartbeat can be selected to contain the same number of m samples, where each sample is a fraction of the heartbeat period and N heartbeats contains mxN samples. Taking the Fourier transform of this mxN data set and processing the spectral components of the transform in the same manner as described previously, results in a spectral analysis having several additional advantages. First, the fundamental maximum would always occur at the spectral line for N cycles in "heartbeat" space. Second, any signal present in the data set which did not remain synchronous with the heart, including noise, artifact and transient background intensity changes, would be spread over the heartbeat spectrum. Third, the enhancement in signal-to-noise would be the same for all heart rates. Fourth, because only two spectral lines are of interest, the zero spectral line corresponding to the zero frequency background intensity and the N spectral line corresponding to the number of heartbeats for the data set, the Fourier Transform need only be made at the two frequency components and not of the entire spectrum, and the computation efforts required by the microprocessor are significantly diminished.

The apparatus of the present invention can be used for either time domain or frequency domain analyses, and includes inputs for the plethysmographic detected optical signals and ECG signals of a patient, an analog to digital converter for converting the analog plethysmographic signal to the digital optical signals and for converting the analog ECG signals into digital ECG signals (unless the plethysmographic or ECG signals are provided in digital form), and a digital signal processing section for receiving the digital signals and processing the digital detected optical signal in accordance with one of the foregoing analysis techniques of the present invention, including a microprocessor, memory devices, buffers, software for controlling the microprocessor, and display devices.

In its context, the apparatus of the present invention is a part of an oximeter device which has the capability to detect the red and infrared light absorption, and receive an ECG signal from the patient. In the preferred embodiment, the apparatus of this invention is a part of the Nellcor N-200 Pulse Oximeter (herein the "N-200 oximeter"), a commercially available noninvasive pulse oximeter device manufactured and sold by Nellcor, Incorporated, Hayward, Calif. U.S.A.

The N-200 oximeter is an improved version of the enhanced N-100 oximeter described above and in the prior application Ser. No. 742,720. The N-200 includes circuits that perform many of the same functions as in the N-100 device, but includes some changes, for example, to expand the dynamic range of the device over the N-100 device and to include a 16 bit microprocessor manufactured by Intel Corporation, Model No. 8088. The N-100 oximeter uses an 8 bit microprocessor manufactured by Intel Corporation, Model 8085. The N-200 oximeter includes software for controlling the microprocessor to perform the operations of the preferred embodiment of the time domain analysis techniques of present invention in addition to the conventional oximeter functions, and has some structure and processing methods that are unrelated to the present invention, and therefore are not discussed herein. The software could be modified to perform any of the other time domain or frequency domain analysis techniques of the present invention.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1A and 1B are a block diagram of the apparatus of this invention and the apparatus associated with the present invention.

FIG. 2A is a detailed circuit schematic of the saturation preamplifier in the patient module of FIG. 1.

FIG. 2B is a detailed circuit schematic of the ECG preamplifier and input protection circuit in the patient module of FIG. 1.

FIGS. 3A and 3B are a detailed circuit schematic of the saturation analog front end circuit of FIG. 1.

FIG. 4 is a detailed circuit schematic of the LED drive circuit of FIG. 1.

FIG. 5 is a detailed circuit schematic of the ECG analog front end circuit of FIG. 1.

FIGS. 6A and 6B are a detailed circuit schematic of the analog to digital converter section of FIG. 1.

FIGS. 7A, 7B, and 7C are a detailed circuit schematic of the digital signal processing section of FIG. 1.

FIG. 8 is a detailed circuit schematic of the external ECG circuitry of FIG. 1.

FIGS. 9A, 9B, 9C, 9D, 9E and 9F are flow charts for the time domain ECG and optical signal processing of this invention.

FIG. 10 is a flow chart for the frequency domain optical pulse processing of this invention.

FIGS. 10A, 10B, 10C, 10D and 10E are a series of waveforms corresponding to the flow chart of FIG. 10.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

Referring to FIGS. 1A and 1B, the preferred embodiment of the present invention relates to the apparatus for processing the detected analog optical signal and the analog ECG signal and comprises portions of analog to digital conversion section ("ADC converter") 1000 and digital signal processing section ("DSP") 2000, including the software for driving microprocessor 2040, which processes the digitized optical signals and ECG signals to determine the oxygen saturation of hemoglobin in arterial blood. Associated with the invention, but not forming a part of the invention, is the apparatus for obtaining the detected analog optical signals and the analog ECG signals from the patient that is part of or is

associated with the commercially available Nellcor N-200 Pulse Oximeter. Such apparatus include plethysmograph sensor 100 for detecting optical signals including periodic optical pulses, patient module 200 for interfacing plethysmograph sensor 100 and the conventional ECG electrodes with saturation analog front end circuit 300 and ECG analog front end circuit 400 respectively, saturation analog circuit 300 for processing the detected optical signals into separate red and infrared channels that can be digitized, and ECG analog front end circuit 400 for processing the ECG signal so that it can be digitized. The N-200 oximeter also includes external ECG input circuit 500 for receiving an external ECG signal and processing the signal so that it is compatible with the N-200 processing techniques (as explained below), LED drive circuit 600 for strobing the red and infrared LEDs in plethysmograph sensor 100 at the proper intensity to obtain a detected optical signal that is acceptable for processing, and various regulated power supplies (not shown) for driving or biasing the associated circuits, as well as ADC 1000 and DSP 2000, from line current or storage batteries.

The associated elements are straightforward circuits providing specified functions which are within the skill of the ordinary engineer to design and build. The associated elements are briefly described here, and reference is made to the corresponding detailed schematics in the Figures and circuit element tables set forth below, to place the apparatus for using the present invention in its operating context in the preferred embodiment.

In the preferred embodiment, the invention requires three input signals, the two plethysmograph or detected optical signals (e.g., red and infrared) and the ECG signal of the patient. If analog signals are provided, they must be within or be adjusted by, for example, offset amplifiers, to be within the voltage input range for the ADC. In circumstances where the signals have been digitized already, they must be bit compatible with the digital signal processing devices, DSP.

The plethysmograph signal is obtained in a conventional manner for a non-invasive oximeter, typically by illuminating the patients tissue with red and infrared light in an alternating fashion, in the manner described above for the N-100 oximeter. Referring to FIGS. 1A and 1B, sensor circuit 100 has red LED 110 and infrared LED 120 connected in parallel, anode to cathode, so that the LED drive current alternately illuminates one LED and then the other LED. Circuit 100 also includes photodetector 130, preferably a photodiode, which detects the level of light transmitted through the patient's tissue, e.g., finger 140, as a single, analog optical signal containing both the red and infrared light plethysmographic, detected optical signal waveforms.

Referring to FIGS. 1A, 1B, 2A, and 2B, patient module 200 includes preamplifier 210 for preamplifying the analog detected optical signal of photodetector 130, ECG preamplifier 220 for preamplifying the analog ECG signal detected from the ECG electrodes that would be attached to the patient in a conventional manner, and protection circuitry 250 interposed between instrumentation amplifier 220 and inverter 230 and the three ECG signal leads, to prevent high voltage transients from damaging the ECG preamplifier electronics.

Preamplifier 210 may be an operational amplifier configured as a current to voltage converter, biased by a positive voltage to extend the dynamic range of the system, thereby converting the photocurrent of photo-diode 130 into a usable voltage signal. ECG preamplifier 220 is preferably a high quality instrumentation amplifier which amplifies the differential signal present on the two ECG signal electrodes. The

15

common-mode signal present on the two signal electrodes is inverted by inverter **230** and returned to the patient by the third ECG lead, effectively nulling the common-mode signals. A biasing network on tee two ECG signal leads is provided to aid in the detection of when an ECG electrode lead becomes disconnected from patient module **200** or the patient. Patient module **200** also includes leads for passing the LED drive voltages to LEDs **110** and **120**.

Referring to FIGS. 1A, 1B, 3A and 3B, saturation analog front end circuit **300** receives the analog optical signal from patient module **200** and filters and processes the detected signal to provide separate red and infrared analog voltage signals corresponding to the detected red and infrared optical pulses. The voltage signal is passed through low pass filter **310** to remove unwanted high frequency components above, for example, 100 khz, AC coupled through capacitor **325** to remove the DC component, passed through high pass filter **320** to remove any unwanted low frequencies below, for example, 20 hertz, and passed through programmable gain stage **330** to amplify and optimize the signal level presented to synchronous detector **340**.

Synchronous detector **340** removes any common mode signals present and splits the time multiplexed optical signal into two channels, one representing the red voltage signals and the other representing the infrared voltage signals. Each signal is then passed through respective filter chains having two 2-pole 20 hertz low pass filters **350** and **360**, and offset amplifier **370** and **380**. The filtered voltage signals now contain the signal information corresponding to the red and infrared detected optical signals. Additionally, circuits for use in preventing overdriving the amplifiers in saturation circuit **300** may be applied, for example, level-sensing circuits **312** and **314** (located after low pass filter **310**) for indicating unacceptable LED drive current, and level sensing circuit **315** (located after programmable gain amplifier **330**) for indicating unacceptable input amplifier gain setting.

Referring to FIGS. 1A, 1B, and 8, ECG analog front end circuit **4000** receives the preamplified ECG signal from patient module **200** and processes it for use with the present invention. The analog ECG signal is passed through 2-pole 40 hertz low pass filter **410** for removing unwanted frequencies above 40 hertz, and programmable notch filter **420** for removing unwanted line frequency components. Optionally, circuitry may be provided to measure the line frequency and to select an appropriate clock frequency for the notch filter. The ECG signal is then passed through low pass filter **430**, preferably configured to remove further unwanted components above about 40 hertz, and in particular any frequency components that may have been generated by notch filter **420**. Thereafter, the ECG signal is passed through 2-pole 0.5 hertz high pass filter **440** to remove any low-frequency baseline shifts present in tee original ECG signal, and then passed through offset amplifier **450** to add an offset voltage that the voltage is within the input signal specifications of the analog to digital converter device and the complete waveform will be properly digitized.

It also is desirable to pass the signal output from low pass filter **410** into a circuit that detects whether or not the ECG signal is being detected to identify a "leads-off" condition. The signal voltage is passed through absolute value circuit **480** to take the absolute value of the low pass filter output voltage and sends the value to comparator **490**. Comparator **490** compares the absolute value voltage to a reference threshold or range and, when the absolute value voltage is not within the acceptable range, comparator **490** changes state which change is input to latch **495**, to indicate this condition to, for example, the microprocessor.

16

Referring to FIGS. 1A, 1B and 8, the Nellcor N-200 device also is equipped with external ECG circuit **500** for receiving the ECG signal of a stand alone ECG detector device and processing the ECG signal so that it can be used with the N-200 oximeter and the present invention. Circuit **500** receives the external analog ECG signal, passes it across capacitor **510** to remove any DC offset voltage and then passes the signal through peak detection circuit **530**. A portion of the AC coupled signal also is passed through buffer amplifier **520** and input to comparator **570**. The held peak voltage is used as the reference threshold voltage that is fed to the other input of comparator **570** so that subsequent QRS complexes in the ECG signal that rise above the threshold generate a trigger signal that is transferred to DPS 2000 by an electrically isolated optical serial communication link comprising serial driving opto-isolator **580**, electrically isolated optical link **590**, and corresponding serial driving opto-isolator **2590** in DSP 2000.

Referring to FIGS. 1A, 1B, 6A and 6B, ADC 1000 provides the analog to digital conversions required by the N-200 oximeter. The aforementioned three voltage signals, the red detected optical signal, the infrared detected optical signal, and the ECG signal (preferably the ECG signal from patient module **200**), are input to ADC **1000**. These three signals are conventionally multiplexed and digitized by an expanded range 12-bit analog to digital conversion technique, yielding 16-bit resolution. The input signals are passed through multiplexor **1010** and buffer amplifier **1020**. The converter stage includes offset amplifier **1030**, programmable gain circuitry **1040** which allows a portion of the signal to be removed and the remainder to be further amplified for greater resolution, sample and hold circuit **1050**, comparator **1060**, and 12-bit digital to analog converter **1080**. The buffered signal is passed through offset amplifier **1030** to add a DC bias to the signal wherein a portion of the signal is removed and the balance is amplified by being passed through programmable gain circuitry **1040** to improve the resolution. The amplified signal is then passed through sample and hold circuit **1050**, the output of which is fed to one input of comparator **1060**. The other input of comparator **1060** is the output of digital to analog ("DAC") converter **1080** so that when the inputs to comparator **1060** are the same, the analog voltage at the sample and hold circuit is given the corresponding digital word in DAC converter **1080** which is then stored in an appropriate memory device as the digitized data for the sample, and the next sample is sent to sample and hold circuit **1050** to be digitized.

Referring to FIGS. 1A, 1B, 4, 6A, 6B, 7A, 7B, and 7C, DAC **1080** also generates the sensor LED drive voltages, under the control of microprocessor **2040**, using analog multiplexor **610**, which separates the incoming analog signal into one of two channels for respectively driving the red and infrared LEDs, having respective sample and hold circuits **620** and **630**, and LED driver circuit **640** for converting the respective analog voltage signal into the respective positive and negative bipolar current signals for driving LEDs **110** and **120**.

Alternate techniques of converting the analog signals to digital signals could be used, for example, a 16-bit analog to digital converter.

Referring to FIGS. 1, 7A, 7B and 7C, DSP **2000** controls all aspects of the signal processing operation including the signal input and output and intermediate processing. The apparatus includes 16-bit microprocessor **2040** and its associated support circuitry including data bus **10**, random access memory (RAM) **2020**, read only memory (ROM)

2030, a conventional LED display- device 2010 (not shown in detail), system timing circuit 2050 for providing the necessary clock synchronizing and notch filter frequency signals. In the preferred embodiment, microprocessor 2040 is a model 8088 microprocessor, manufactured by Intel Corporation, Santa Clara, Calif. Alternate microprocessors may be used, such as any of model nos. 8086, 80186, and 80286, also made by Intel Corporation.

Referring to FIGS. 9A, 9B, 9C, 9D, 9E, and 9F and software Appendix A, the flowcharts for the software operation of the preferred embodiment are shown and described. Software appendix A is written in the standard programming language for Intel Model 8088 microprocessor devices.

Similar to the enhanced N-100 oximeter described in U.S. application Ser. No. 742,720, the N-200 oximeter incorporating the present invention is designed to determine the oxygen saturation in one of two modes, an unintegrated mode wherein the oxygen saturation determination is made on the basis of pulses detected in the optical pulse signal that are determined to be optical pulses in accordance with conventional pulse detection techniques, and in an ECG synchronization mode wherein the determination is based on the synchronized additive, composite optical signal information in accordance with the preferred embodiment of the present invention. In an alternate embodiment of the present invention, the determination of saturation in the unintegrated mode may be based on the frequency domain analysis techniques in accordance with this invention with or without the ECG synchronization feature of the time domain analysis techniques.

Referring to FIG. 9F, interrupt programs control the collection and digitization of incoming optical and ECG data. As particular events occur, various software flags are raised which transfer operation to various routines that are called from the Main Loop Processing routine. For example, Main Loop Processing calls the ECG routine at 3600, calls a routine that checks the LED levels at 3610 to make sure that there is enough and not too much light being transmitted, looks for the presence of new data at 3615, and if there is new data, calls the MUNCH routine at 3620, looks for processed pulse data at 3635 and passes such data to the Level13 routine that calculates saturation at 3640, and also runs various maintenance routines related to the oximeter functions which are not pertinent to the present invention, e.g., at 3625, 3630, 3645, 3650, 3655, and 3660 and are not discussed herein. The routines pertinent to the present invention are discussed here. Examples of similar and peripheral other routines may be found in the software appendix to application Ser. No. 742,720.

The detected optical signal waveform is sampled at a rate of 57 samples per second. When the digitized red and infrared signals for a given portion of detected optical signals are obtained, they are stored in a buffer called DATBUF and a software flag indicating the presence of data is set at 3615. This set flag calls a routine referred to as MUNCH as 3620, which processes each new digitized optical signal waveform sample. The MUNCH routine is called once per data point and determines pairs of maximum and minimum amplitudes in the detected signal data and presents the pairs to the Level13 routine. The Level13 routine evaluates the pair of maximum and minimum amplitudes determined by MUNCH, preferably utilizing conventional techniques for evaluating whether a detected pulse is acceptable for processing as an arterial pulse and performs the saturation calculation based on accepted pulses. The MUNCH routine first queries whether or not there is ECG synchronization. If there is ECG synchronization, then the

MUNCH routine obtains from the SLIDER routine the enhanced pulse data on which the ECG synchronized saturation calculation will be mad. If there is not synchronization, MUNCH obtains the sample stored in DATBUF on which the unintegrated saturation calculation will be made.

Referring to FIG. 9A, the SLIDER routine processes each new digitized sample portion of detected optical signal containing the optical pulse to create and maintain the enhanced composite red and infrared optical pulse waveforms, synchronized with the occurrence of successive ECG R-wave events.

The SLIDER routine first inquires whether there is an ECG signal at 3100. If there is not, then the routine aborts to exit at 3160 to main line operation. If there is an ECG signal, then the SLIDER routine continues and checks the validity of the optical signal at 3110. If the digitized sample in the buffer DATBUF for either of the red or infrared channels contains an invalid datapoint, the full content of the slider buffer (SLIDEBUF) is erased and the routine exited. The validity of the data is checked by looking for zeros placed in the buffer. Zeros are placed in the buffer when the signal level of the LEDs changes to permit the 20Hz filters to settle, or if the signal exceeds the voltage limits of the processing electronics. This prevents processing of data known to be bad.

If the data are determined to be valid, then the SLIDER routine queries whether or not the data should be skipped at 3120. The optical signal sampling and data collection and processing of the sampled data are asynchronous processes. On occasion, the data buffer will have several unprocessed samples of data by the time the ECG R-wave event trigger occurs (described below). The R-wave event resets the slider buffer pointer to the beginning of the slider buffer and marks the R-wave data sample in DATBUF SLIDER will not process a data point if the slider buffer pointer is reset already to the beginning of the slider buffer and if the incoming data point was digitized in DATBUF before the data point marked by the R-wave event. Data in the DATBUF buffer prior to the R-wave event are to be skipped. If the data are to be skipped, SLIDER is exited.

If the data are to be processed, SLIDER calculates the updated value for the composite portion waveform sample as "slider data" using the following formula:

$$\text{slider\_data} = \frac{(\text{WEIGHT} - 1)}{\text{WEIGHT}} \times \text{slider\_data} + \frac{1}{\text{WEIGHT}} \times \text{new\_data}$$

wherein "WEIGHT" is the aforementioned fractional weighting fraction; "new data" is the data point taken from the incoming sample in DATBUF, and "slider data" is the pre-existing data point in the composite waveform in the slider buffer (SLIDEBUF) before the new data point is added and becomes the updated data point after the computation.

The computation is performed for each data point in DATBUF and any corresponding pre-existing data in the slider buffer. The occurrence of an R-wave event indicates the beginning of the heartbeat sample.

Before making the computation, SLIDER checks the slider buffer to see if there is any existing data at 3130. If there are data, then at 3150 SLIDER calculates the new value for the composite optical signal. If, however, the slider buffer is empty, then the WEIGHT value is assigned a numerical value of 1 at 3140, and subsequent new data points

will be weighted 100% and the routine continues to calculate a new value for the composite optical signal at 3150 until the occurrence of the next R-wave event corresponding to the following heartbeat and portion of detected optical signal.

The SLIDER routine also performs other housekeeping chores for the processing associated with the slider buffer. First, in the preferred embodiment, the slider buffer is given a specific length and is able to store about three seconds worth of data. If, for whatever reason, the microprocessor does not receive or recognize an R-wave for more than three seconds, the pointer of the slider buffer is set to point to the last location and does not get incremented beyond that location. Subsequently processed samples are each placed in the last location of the buffer until the next accepted R-wave occurs or a time-out condition occurs. Time-out occurs when no further R-wave events are accepted for a predetermined time of, e.g., five seconds. After time out has occurred, MUNCH is notified that ECG synchronization is lost so that saturation calculations will be based only on the optical signals in DATBUF in the unintegrated mode.

Second, SLIDER continuously compares the updated composite waveform in the slider buffer to the previous composite waveform. If there is a large discrepancy, for example, during electromechanical disassociation, SLIDER takes immediate action to disregard the slider buffer data.

Third, to avoid corrupting the integrity of the waveform data in the slider buffer whenever the apparatus hardware or software triggers a change that influences the signal level of the detected optical signal or the optical pulse waveform, the content of the slider buffer is erased.

Referring to FIG. 9B, the ECG BOX routine processes the ECG signal obtained through patient module 200 and analog ECG front end circuit to detect ECG R-wave events. The ECG signal is digitized every 5 msec and the digitized values are maintained in a circular buffer. The R-wave event is detected by observing the derivative of the ECG signal. The derivative is obtained at 3200 by application of the following algorithm:

$$\text{derivative\_ecg\_data}[n] = \text{abs}[-0.5 * \text{ecg\_data}[n - 3] +$$

$$0.5 * \text{ecg\_data}[n - 2] + 0.5 * \text{ecg\_data}[n - 1] - 0.5 * \text{ecg\_data}[n]]$$

where "ecg data[n]" is the digitized value for the ECG signal at sample location n and "ab []" is the absolute value of the bracketed quantity.

The largest magnitude spike in the derivative buffer marks the R-wave. Because the algorithm generates the absolute value of the derivative, the derivative buffer contains two spikes very close to each other, one for the positive-going portion and the other for the negative-going portion of the R-wave. After the first spike is recognized, a timer ecg block is set at 3250 to cause ECG BOX to ignore the second spike.

Once the derivative value is obtained, and if the ecg block timer is not active, then the derivative value is compared to the ECG threshold at 3240. The ECG threshold is a value that is set at about 75% of the previous maximum derivative value. If the derivative is greater than the threshold, ECG BOX starts the ecg block timer by setting ecg block equal to true at 3250, and it replaces the maximum derivative value with the current derivative value at 3260, and calls the R-WAVE CHECKING routine at 3270. After the R-WAVE CHECKING routine is completed (as discussed below), ECG BOX is exited at 3280.

If the derivative is not greater than the threshold, then ECG BOX is exited at 3280. Once the ecg block timer is activated, ECG BOX will continue to calculate the derivative and compare the derivative to the prior maximum derivative value at 3220. If the calculated derivative is greater, then the maximum derivative value is set equal to the current derivative ecg data[n] at 3230 and the routine is exited. Otherwise the routine is exited.

Referring to FIG. 9E, the R-WAVE CHECKING routine receives the detected R-wave event at 3500 and checks the elapsed time since the last R-wave at 3510. If the elapsed time is less than the minimum internal time limit, preferably set at about 200 msec, the R-wave event is marked as a false R-wave event at 3520. If the elapsed time is greater than the minimum limit, then the routine starts a phase-delay timer/counter at 3530. The purpose of the phase-delay counter is to ensure that the optical data is placed into the beginning of the slider buffer after the optical signal minimum from the preceding pulse, but before the signal maximum of the next pulse. The preferred phase-delay period is 40 msec, based on the results of experimentation, and corresponds to the opening of the time window. It may be desirable to have a phase delay period that can be adjusted to accommodate varying optical signal detection conditions for different patients.

The Nellcor N-200 device is equipped with an external ECG input circuit as described above. The main line operating system controlling the operation of the N-200 device receives an interrupt when the external circuit 500 detects an R-wave. On receipt of the interrupt, a message is sent across isolated optical data transmission path 580-590-2590 (FIGS. 1A and 1B) to microprocessor 2040. The microprocessor then indicates to the ECG processing routines that an externally detected R-wave event has occurred, and the R-wave event is passed to the R-WAVE CHECKING routine. The external ECG analog circuit 500 thus performs the same function as the ECG BOX routine, i.e., determination of an R-wave event followed by the R-WAVE CHECKING routine. The ECG BOX routine is given priority over external ECG circuit 500 in passing signals to R-WAVE CHECKING.

Referring to FIG. 9C, the ECG routine provides for ECG synchronization, the initialization for slider buffer use, and various other tasks associated with ECG enhancement of the detected optical signal. The ECG routine is entered from the Main Loop Processing system (FIG. 9F, at 3600). Its first task is to maintain the ECG related counters/timers, such as ecg block and phase-delay, at 3300. Next, at 3310, it checks whether or not the ECG leads from patient module 200 are present, and if not, it checks at 3320 for the presence of an external R-wave event trigger from external ECG circuit 500. If no R-wave event is detected, then the ECG routine is exited at 3370.

At this point in the processing, the main line processing system is receiving R-wave events, either from external circuits 500 or from patient module 200 and ECG BOX. Regardless of the source of the R-wave event, the subsequent processing of the R-wave event is the same.

When an external R-wave event is detected or the ECG leads are present, the ECG routine calls the ECG LV3 routine, shown in FIG. 9D. ECG LV3 runs through a similar patient module 200 lead checking at 3410 or external circuit 500 trigger at 3420 at the ECG routine and if no R-wave event has occurred the routine is exited at 3480. If an

R-wave event is detected, it is first checked at 3425 to determine whether or not it is a new R-wave event, and if it is not, the ECG LV3 routine is exited. If it is a new R-wave event, 3430 uses the false R-wave flag (set by the R-WAVE CHECKING routine) to determine whether or not it was a true or false R-wave event. False R-waves will cause the routine to be exited at this point.

If the R-wave event is determined not to be a false R-wave, then the ECG-LV3 routine builds up a history of R-wave events based on the R-wave to R-wave interval at 3435. The criteria for accepting an R-wave includes the R-R period and the amplitude of the R-wave. For external ECG circuit 500 triggers, the R-wave even is a uniform pulse resulting from a comparison of the R-wave amplitude to a determined threshold signal.

After computing the R-R interval (or R-R delta) and history, the ECG LV3 routine checks to see if the ECG is synchronized at 3440. The ECG is synchronized after receiving the predetermined number, preferably five, acceptable R-wave triggers. For example, the ECG synch counter is initialized at five. The routine tests the ECG synch counter 3440 so that if it is greater than zero, the ECG is determined to be not synched, and then the ECG synch counter is decreased by one at 3455. Thus, when the ECG synch counter is at zero at 3440, indicating that the required prior five acceptable R-wave event have successively occurred, then it is determined that there is ECG synchronization and the device will proceed through MUNCH to calculate oxygen saturation based on the enhanced composite slider buffer calculations. Whether or not there is EC synchronization, any R-wave event is checked again at 3450 against the history and R-R interval, if any, to determine whether there is an error in synchronization. If there is an error, the ECG LV3 routine is exited. If there is no synchronization error, a routine is called at 3460 to compute the maximum length of time after which data in the slider buffer (SLIDEBUF) is disregarded. For example, if there is no prior R-R interval or history, then there will be no error for the first R-wave event. Subsequent true R-wave events will be compared to the prior R-R interval and history and if it appears to be a valid true pulse, then a routine is called to reset slider buffer pointers. However, the saturation calculation will be based upon the slider buffer data only after five R-waves have passed in synch and the synchronization flag is raised. Loss of synchronization resets the ECG synch counter to five.

The ECG LV3 routine also calculates the maximum length of the slider buffer based on the heart rate, which length is preferably 3 seconds or 2.5 times the determined R-R interval, whichever is the smaller. The ECG LV3 routine also maintains the slider pointers and counters, resetting them or clearing them as necessary, resets the ecg timeout and bad R-wave counter, computes and displays heart rate based on the R-R interval at 3465, updates the history buffers and sets the trigger for the MUNCH routine to calculate pulse data for determining oxygen saturation based on the updated slider buffer data at 3470, sets and computes windows for selecting the portion of detected optical signal to be processed for each heartbeat, based on the history and the most recent data at 3475. In the preferred embodiment, the windows are set to open by the R-WAVE CHECKING routine phase-delay counter/timer 40 ms after

the R-wave occurs and before the maximum optical pulse wave has occurred at the detection site, and set to close by the MUNCH routine after a maximum and minimum pair has been found.

Upon exiting ECG LV3, the program returns to the ECG routine and checks the threshold of the derivative buffer of the ECG BOX. If the maximum derivative value is changes substantially, which indicates that the R-wave slope is changing, then the threshold is adjusted.

Referring to FIGS. 10, 10A, 10B, 10C, 10D, 10E and the software appendix B, the flow chart for the software operation of the frequency domain embodiment of the present invention are shown. Software appendix B is written in the Asyst computer language which is a commercially available language.

The routine begins at 4000 with the acquisition of 512 data points for each of the digitized red and infrared optical signals, which are shown graphically at FIG. 10A. At 4010, the complex data set,  $f(t)=\text{Red}(t)+j\text{IR}(t)$ , is formed. At 4020, the "D.C." component is formed by summing all of the data points, and the "D.C." component is then removed from the complex data set by subtraction at 4030, which is graphically shown at FIG. 10B. The resulting data is then decimated in time to 64 samples at 4040, which is illustrated in FIG. 10C, and the time decimated data is then processed by the Hamming Window function at 4050, which result is illustrated in FIG. 10D. Thereafter, the Fourier Transform is taken at 4060. The spectral components of the transform are shown in FIG. 10E. The Fourier Transforms of the red and infrared components are then calculated at 4070 in accordance with the aforementioned equations, and at 4080 the maximum value at the fundamental heart rate and the minimum value at the zero frequency are determined for each of the red and infrared transforms. The saturation ratio R is calculated as:

$$R = \frac{\text{peak at heartrate for red} / \text{Re("D.C.")}}{\text{peak at heartrate for infrared} / \text{Im("D.C.")}}$$

The minimum values for the red and infrared waveforms are taken from the respective real and imaginary components of the "D.C." component. Thereafter, the pulse data is declared ready and saturation is calculated in accordance with the foregoing saturation formula. With each occurrence of the heartbeat, new data is acquired, the 512 data point set is updated and the routine operates to determine the saturation ratio R.

In the preferred embodiment, the blood constituent measured is the oxygen saturation of the blood of a patient. The calculation of the oxygen saturation is made based on the ratio of the pulse seen by the red light compared to the pulse seen by the infrared light in accordance with the following equation:

$$\text{Saturation} = 100\% \times \frac{\text{BR2} - \text{R}(\text{BR1})}{\text{R}(\text{BO1} - \text{BR1}) + \text{BR2} - \text{BO2}}$$

wherein

BO1 is the extinction coefficient for oxygenated hemoglobin at light wavelength 1 (Infrared)

23

BO2 is the extinction efficient for oxygenated hemoglobin at light wavelengths 2 (red)  
 BR1 is the extinction coefficient for reduced hemoglobin at light wavelength 1  
 BR2 is the extinction coefficient for reduced hemoglobin at light wavelength 2  
 light wavelength 1 is infrared light  
 light wavelength 2 is red light  
 and R is the ratio of the optical density of wavelength 2 to wavelength 1 and is calculated as:

$$R = \frac{\ln [I_{max2}/I_{min2}]}{\ln [I_{max1}/I_{min1}]}$$

24

wherein

$I_{max2}$  is the maximum light transmitted at light wavelength 2

$I_{min2}$  is the minimum light transmitted at light wavelength 2

$I_{max1}$  is the maximum light transmitted at light wavelength 1

$I_{min1}$  is the minimum light transmitted at light waveguide 1

The various extinction coefficients are determinable by empirical study as is well known to those of skill in the art. For convenience of calculation, the natural log of the ratios may be calculated by use of the Taylor expansion series for the natural log.

Circuit Tables

<u>REF #</u>	<u>CHIP</u>	<u>MFR PART #</u>	<u>Manufacturer</u>	<u>DESCRIPTION OF CHIP</u>
FIG. 2				
210	U2	LF442	NATIONAL SEMICONDUCTOR	DUAL LOW POWER OP AMP
220	U1	INA101HP	BURR BROWN	INSTRUMENTATION AMP
230	U2	LF442	NATIONAL SEMICONDUCTOR	DUAL LOW POWER OP AMP
FIG. 3.				
312	U27	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
312	U28	LP365N	NATIONAL SEMICONDUCTOR	QUAD VOLTAGE COMPARATOR
310	U27	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP

320	U27	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
330	U44	MP7524LN	MICROPOWER	8-BIT DAC
330	U32	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
330	U32	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
315	U20	LP365N	NATIONAL SEMICONDUCTOR	QUAD VOLTAGE COMPARATOR
340	U32	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
340	U14	DG243CJ	SILICONIX INCORPORATED	ANALOG SWITCH
340	U7	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
340	U13	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
350	U7	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
360	U13	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
370	U7	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
380	U13	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
340	U19	DG211CJ	SILICONIX INCORPORATED	CMOS ANALOG SWITCH
FIG. 4				
640	U19	DG211CJ	SILICONIX INCORPORATED	CMOS ANALOG SWITCH
640	U32	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
FIG. 5				
410	U12	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
420	U6	LTC1059CN	LINEAR TECHNOLOGY	SWITCHED CAPACITOR FILTER
430	U12	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
440	U12	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
440	U19	DG211CJ	SILICONIX INCORPORATED	CMOS ANALOG SWITCH
450	U12	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
480	U5	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
490	U4	LM393N	NATIONAL SEMICONDUCTOR	VOLTAGE COMPARATOR
495	U10	74HC00	TEXAS INSTRUMENTS	HIGH SPEED CMOS
495	U3	74HC74	TEXAS INSTRUMENTS	HIGH SPEED CMOS

FIG. 6

1010	U24	DG528CK	SILICONIX INCORPORATED	OCTAL ANALOG SWITCH
1020	U25	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
1030	U25	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
1040	U38	AD7524LN	ANALOG DEVICES	DAC
1040	U42	74HC374	TEXAS INSTRUMENTS	HIGH SPEED CMOS
1040	U37	LF442N	NATIONAL SEMICONDUCTOR	LOW POWER OP AMP
1050	U36	LF398N	NATIONAL SEMICONDUCTOR	SAMPLE & HOLD OP AMP
1060	U29	LM211P	TEXAS INSTRUMENTS	LOW OFFSET VOLTAGE COMPARATOR
1080	U43	AD7548KN	ANALOG DEVICES	CMOS 12-BIT DAC
1080	U31	LF411ACN	NATIONAL SEMICONDUCTOR	LOW OFFSET OP AMP
1080	U25	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
610	U18	DG528CK	SILICONIX INCORPORATED	OCTAL ANALOG SWITCH
620	U11	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP
630	U11	LF444	NATIONAL SEMICONDUCTOR	QUAD JFET OP AMP

FIG. 7

	U2	82C84A-2	NEC	CMOS 8 MHZ CLOCK GENERATOR
	U1	74HC74	TEXAS INSTRUMENTS	HIGH SPEED CMOS
	U1	74HC74	TEXAS INSTRUMENTS	HIGH SPEED CMOS
2040	U8	MSM80C88RS-2	OKI ELECTRIC	CPU 8MHZ, 125ns
	U3	74HC74	TEXAS INSTRUMENTS	HIGH SPEED CMOS
	U33	74HC374	TEXAS INSTRUMENTS	HIGH SPEED CMOS
	U9	74HC04	TEXAS INSTRUMENTS	HIGH SPEED CMOS
	U3	74HC74	TEXAS INSTRUMENTS	HIGH SPEED CMOS
	U9	74HC04	TEXAS INSTRUMENTS	HIGH SPEED CMOS
	U19	74HC00	TEXAS INSTRUMENTS	HIGH SPEED CMOS
	U9	74HC04	TEXAS INSTRUMENTS	HIGH SPEED CMOS
2030	U21	MBM27C512-25	FUJITSU LIMITED	CMOS 64K X 8 ROM
2020	U15	DS1242	DALLAS SEMICONDUCTOR	CMOS 32K X 8 RAM
	U23	74HC138	TEXAS	HIGH SPEED CMOS

			INSTRUMENTS	
	U17	74HC138	TEXAS	HIGH SPEED CMOS
			INSTRUMENTS	
	U19	74HC00	TEXAS	HIGH SPEED CMOS
			INSTRUMENTS	
	U19	74HC00	TEXAS	HIGH SPEED CMOS
			INSTRUMENTS	
	U16	82C51A	OKI ELECTRIC	CMOS UART
	U22	MSM82C59A-2RS	OKI ELECTRIC	CMOS INTERRUPT CONTROLLER
2050	U34	MSM82C53-2	OKI ELECTRIC	CMOS TRIPLE TIMER
2050	U38	MSM82C53-2	OKI ELECTRIC	CMOS TRIPLE TIMER
2050	U9	74HC04	TEXAS	HIGH SPEED CMOS
			INSTRUMENTS	
2050	U39	74HC393	TEXAS	HIGH SPEED CMOS
			INSTRUMENTS	
2050	U35	D2732A	INTEL	4096 X 8 ROM
			CORPORATION	
2050	U40	74HC374	TEXAS	HIGH SPEED CMOS
			INSTRUMENTS	
2050	U28	74HC374	TEXAS	HIGH SPEED CMOS
			INSTRUMENTS	
FIG. 8				
520	U3	LF444	NATIONAL	QUAD JFET OP AMP
			SEMICONDUCTOR	
530	U2	LF444	NATIONAL	QUAD JFET OP AMP
			SEMICONDUCTOR	
530	U3	LF444	NATIONAL	QUAD JFET OP AMP
			SEMICONDUCTOR	
570	U7	LM311N	NATIONAL	VOLTAGE COMPARATOR W/STROBE
			SEMICONDUCTOR	

```

ECG:
:ECG MAIN "ECG"
ecg_00:
    mov    a1,ecg_sw      ;check if to do any ECG
    or     a1,a1
    jnz    short ecg4

    call   wdg_clock     ;can't do anything if leads off
    call   LEADS_CHK
    jnc    SHORT_ECG1
    jnc    ECG_MODE_EXT_TRIG
    jnc    SHORT_ECG1    ;USING EXTERNAL TRIGGER IF SET
    cmp    ecgfmoflg.1
    je     short ecg0
    cmp    ecgdly.0
    jne    short ecg0
    call   ECG_TMO
    mov    ecgfmoflg.1

ecg0:
    RET

ECG1:
    CALL   ecg_lv3
    call   set_thresh     ;initial threshold adjustment
    call   chk_thresh     ;check and adjust threshold

ECG3:
    MOV    AX,ecdoidr
    ADD    AX,2
    AND    AX,ECG_B_MSK
    MOV    ecdoidr,AX

ecg4:
    cmp    ecg_sync.1
    je     short wdg5
    call   ecg_init1

ecg5:
    ret

; SUBTTL ECG LEVEL 1
    
```

```

ECG LV3:
; COMPUTE HEART RATE FROM ECG R WAVE THIS ROUTINE FIGURES OUT WHETHER EKG
; AND/OR OXIMETER ARE SYNCED. IF EKG ONLY, THEN DO CONFIDENCE CHECKING ON
; PERIOD AND DISPLAY AND ALARM CHECK FOR THE HEART RATE. IF OXIMETER IS SYNCED,
; THEN DETERMINE HEART RATE BY THE R-WAVE PERIOD. IF THE CONFIDENCE IS GOOD,
;
    
```



```

ecgnsyn@a:
mov     first_rmv_seen, 0
call   ecg_nsync_err_ck
jc     ecg_not_sync_ex
dec     ecgsdly
cap     synfig, 0
je     ecg_not_sync_ex
mov     FRATN, 255
mov     CX, RPPER
mov     AX, ECSRATEFACTOR
CALL   COMRAT0
;CALC BUT DON'T DISPLAY YET

ecg_not_sync_ex:
test   ecgnotsyncerr, ecg_amp_err
jnz    ecg_not_sync_ex1
call   ecg_hup
;update ecg history
ecg_not_sync_ex1:
JMP    LV3_RET

ecg_sync_err:
MOV     AL, BADECG
DEC     AL
Jns    ecgserr1
xor     ax, ax
kchg   ecgperiod, ax
mov     rpper, ax
call   ecg_hup
jmp     short ecgserr2

ecgserr1:
MOV     BADECG, AL
mov     rrvavg
add     ax, diflim + 10
;clear ecgperiod if it's too large
;last word in diflim is the
;difference limit for r-r period
cmp     ax, ecgperiod
jae    ecgserr2
mov     ecgperiod, 0

ecgserr2:
jmp     lv3_ret

ecg_sync_err_ck:
mov     bl, 0
test   ecg_mode_ext_trig
jnz    ecgserrk1
mov     ax, ecg_delta
cap     ax, min_pp
ja     ecgserrk1
or     bl, ecg_amp_err
;

ecgserrk1:
push   bx
CALL   FRG_D_CHK
pop    bx
TEST   CURDIF, bits5
;CHECK DIF CODES
;ELASBIT...CHECK IF FAILED PERIOD
;IF NZ, FAILED...DON'T CALC HR
;OUT OF BOUNDARY JUMP SOLVED
or     ECgserrk2
;
;cgserk2:
mov     ecgsyncerr, bl
cap     ecgsyncerr, 0
je     ecgserrk3
;jump if ecgsyncerr = 0
;return carry -> bl != 0
;cgserk3:
ret

ecg_nsync_err_ck:
mov     bl, 0
test   ecg_mode_ext_trig
jnz    ecgserrk1
mov     ax, ecg_delta
cap     ax, min_pp
ja     ecgserrk1
or     bl, ecg_amp_err
;

ecgserrk1:
cap     ecgsdly, 1
;only call ecg_v_chk just before
;about to sync
;
;
;
push   bx
CALL   ECB_v_CHK
pop    bx
TEST   CURvar, bits5
;ECGBIT...CHECK IF FAILED PERIOD
;IF NZ, FAILED...DON'T CALC HR
;OUT OF BOUNDARY JUMP SOLVED
or     ECgserrk2
;
;cgserk2:
mov     ecgnotsyncerr, bl
cap     ecgnotsyncerr, 0
je     ecgserrk3
;jump if ecgnotsyncerr = 0
;return carry -> bl != 0
;cgserk3:
ret

do_slider_stuff:
; ** note = between here and the next set of stars, al contains slide_mode
;
mov     al, slide_mode
mov     elapsed_hr, 0
mov     elapsed_sec, 0
mov     bl, dafrig
cmp     dopidx, bl
je     doslj0
or     al, shld_skip
;for slider - if passed all checks.
;
;
;skip the next few samples if
;dopidx is lagging where diplox
;was when the rwave occurred
;set shld_skip and used_ecg to true.
;

doslj0:
test   al, skip_next_rmv
jz     short doslj1
and    al, not (skip_next_rmv)
mov     slide_mode, al
jmp     short doslj4

```

```

doslj1:
  or      al, use_ecg
  test   al, first_time
  jz     short doslj2
  and    al, not (first_time)
  mov    slide_mode, al
  mov    ax, 0
  jmp    short doslj3

doslj2:
  mov    slide_mode, al
  mov    ax, newwid
  mov    newwid2, ax
  mov    newwid, 0
  mov    newwid2_on, 1
  jmp    short doslj4

doslj3:
  ;;;

doslj4:
  call   clr_newbuf
  mov    newwid, 0
  mov    newwid2_on, 0
  ret
  
```

```

R-WAVE_CHK:
R-WAVE "INTERRUPT" -- CALLED BY THE ACTUAL I.S.R. (ABOVE) OR BY 2.5 MS ROUTINE
  PUSH  AX
  mov    al, ecg_sw
  or     al, al
  jnz    short intr_ret

R-WV1:
  test   first_rvw_fig, 0fffh
  jz     rwv12
  mov    first_rvw_fig, 0
  inc    find_max_pos
  mov    find_cnt, TIME2000
  jmp    intr_ret

R-WV2:
  inc    block_fig
  ior    AX, AX
  cmp    ECG200MS, AL
  je     rwv14

  inc    false_rvw
  jmp    short intr_ret

R-WV4:
  mov    ECG200MS, TIME200
  mov    phase_dly, TIME40

INTR_RET:
  mov    rwv_time_out, TIME5000
  pop   AX
  ret
  
```

```

CHK_TRIG:
; CALLED FROM 2.5 MS INTERRUPT TO CHECK STATUS OF EXTERNAL TRIGGER FLAG
  cmp    front_ecg_tmout, 0
  jne    short chktrig_xit
  mov    AL, EXT_ECG_TRIG
  or     AL, AL
  jz     short chktrig_xit
  xdr    AL, AL
  mov    EXT_ECG_TRIG, AL
  cmp    ext_ecg_blk, 0
  jne    chktrig_xit
  or     ext_ecg_blk, time200*2
  mov    ECG_MODE, EXT_TRIG
  call   ext_trig_tm, ext_trig_tm
  call   R-WAVE_CHK

CHKTRIG_XIT:
  ret
  
```

-----  
: TITLE: ECGATOD  
: FUNCTION: store the ecg signal value in the ecg ring buffer. If front panel ecg input flag is set, send ecg data to the powerbase. Increment the ecgperiod and five\_ms counters. Also sets the ignore\_rwave flag in ecg\_mode if the ecg value isn't within allowable limits.  
: REGS CHANGED. ax, bx, dx  
: CALLS:  
: adcvt, send\_ecg, ecgbox, chktms  
-----

```

ECGATOD:
  inc    ecgperiod
  mov    BX, OFFSET DGROUP: ECGTBL
  call   ADCVT
  mov    BX, ECDIIDX
  push  bx
  cmp    DX, 0ffffh
  jne    atod0
  xdr    dx, dx
  jmp    short atod_1

atod0:
  or     DX, DX
  je     short ATOD_1
  add    DX, GNDV

ATOD_1:
  mov    OFFSET DGROUP: ECG_BUF [BX], DX
  cmp    init_max_min, 1
  je     atod_la
  
```

```

        cmp     dx, ecgmax      ;if a new dc max is found
        jbe    atod_1b
        mov    ecgmax, dx
        jmp    atod_1c
atod_1b:
        cmp     dx, ecgmin     ;else if a new dc min is found
        jae    atod_1c
        mov    ecgmin, dx
        jmp    atod_1c
atod_1a:
        mov    ecgmax, dx
        mov    ecgmin, dx
        mov    init_max_min, 0 ; clear the request to initialize
atod_1c:
        inc    bx
        inc    bx
        and    bx, ECG_B_MSK
        mov    ECDDIDX, bx
        inc    FIVE_MS
        mov    ax, ecgzv
        add    ax, ecgzv
        sub    ax, dx
        jns    atod11
        neg    ax
atod11:
        cmp    ax, 41
        jnb    atod12
        mov    front_ecg_tmout, TM10SEC
        jmp    short atod13
atod12:
        cmp    front_ecg_tmout, 0
        je    atod_1c
        mov    AX, DX
        call   SEND_ECG
atod_13:
        pop    bx
        mov    dx, OFFSET DGROUP: ECG_BUF [BX]
        cmp    dx, max_ecg_lev
        jae    short atod_15a
        cmp    dx, min_ecg_lev
        jbe    short atod_15a
        jmp    short atod_15b
atod_15a:
        or     ecg_mode, ignore_rmv
        mov    ignore_rmv_far, ignore_rmv_time
atod_15b:
        call  ecgbox
        call  chktrns
        ret

ECG_INIT:
        mov    ext_ecg_blk, 0
        mov    ECGSDLY, 4
ecgin0a:
        mov    ECGPSN, 1
        mov    ECGOFV, 0
        mov    ECCTR, 2
        mov    ECGFO, 2
        and    SH_PAT_SAV, ECGDSABL
        mov    DECTAV, DELTA_MIN
        mov    front_ecg_tmout, TM10SEC
ecg_init1:
        mov    ecg_SYNC, 1
-----
: TITLE: ECG_TMO
: FUNCTION: ecg time out
ECG_TMO:
ECG_TMO_2:
        cmp    ecg_SYNC, 1
        je    SHORT TMO_3
        test   ECG_MODE, TMO_FLG
        jz    SHORT TMO_4
        jmp    TMO_1
TMO_4:
        or     ECG_MODE, TMO_FLG
TMO_3:
        mov    b1, ecgsdly
        cmp    ecgsdly, 0
        jne    short tmo_3a
        mov    ecgisecal2, m.1
tmo_3a:
        mov    ECGSDLY, 4
tmo_3a0:
        mov    WINDOWFAC, 3
        mov    MCH_FLG, 1
        mov    ecg_syndly, 4
        ; since chktrns will increment winter1 and 2 as long as winfig1 and 2 are
        ; zero, and since you don't want winter1 or 2 to begin counting
        ; until you're synced on ecg, initialize these variables to something
        ; non zero. dab ///
        mov    winfig1, 2
        mov    winfig2, 2
        mov    winter1, 0
        mov    winter2, 0
        call   clrpdbrs
        call   clr_rr_hist
        mov    first_rmv_seen, 1
        cmp    p1star, 40
        jbe    tmo_33
        mov    p1star, 40
        ; START OUT AT 12.5X
        ; ENABLE MUNCH ON TIMEOUT
        ; dab ///
        ; check pulse timeout counter

```

```

tmo_j3:
MOV     AL,ECG_MODE
AND     OR
OR      AL,NOT (EXT_TRIG)
MOV     ECG_MODE,AL          ;SET IDLE MODE
XOR     AX,AX
MOV     ECG_PERIOD,AX
MOV     RSPER,AX
MOV     ecg_tm,al
MOV     AL,ecg_sync
OR      AL,AL
JNZ     SHORT TMO_1
CMP     SYNFLG,0
JE      SHORT TMO_0
XOR     AX,AX
MOV     FRATE,AL

tmo_j3a:
MOV     RATE,AL
MOV     VRATE,AX
CALL    send_sat           ;update analog output //anb

TMO_0:
CALL    DSPSR
OR      ALMFLG,ECGTMOF
AND     ALMFLG,1 OR ECGTMOF OR PLSTMOF
INC     ECGALMCHK
CALL    ALMCHK
DEC     ECGALMCHK
MOV     CL,LOWRATE OR HIRATE
CALL    CLRITZ
CMP     AL,CTR,0
JE      SHORT TMO_1
MOV     ALMDLY,1

TMO_1:
mov     al,slide_mode      ;for slider - if use_ecg, ///
test   al,use_ecg         ;use_ecg (= false, and ///
jz      short tmo_1a       ;clear munch's parameters ///
and    al,not(use_ecg)    ;
mov     slide_mode,al     ;
mov     perctr,0          ;just for fun, reset perctr ///
mov     al,0              ;
MOV     BX,OFFSET MCHMOD  ;RESET MUNCH'S PARAMETERS ///
MOV     CX,11             ;

tmo_1b:
MOV     BYTE PTR [BX],AL  ;
INC     BX                ;
LOOP   tmo_1b             ;

tmo_1a:
call   rrv_lost
ret

rrv_lost:
mov     rsum,0            ;for ecgbox ///
mov     ecgboxcnt,4       ;ditto ///
mov     ax,thresh_min
mov     max_thresh,ax
mov     max_deriv,ax
mov     first_rvw_flg,1
mov     init_max_min,1
mov     least_rvw_lv3,255
RET

LEADS_CHK:
;CHECK FOR ECG LEADS OFF...SET CARRY IF LEADS ARE OFF
XOR     AX,AX
TEST   STATUS,LEADS_BIT
MOV     CLR_LEADS,AL      ;CLEAR LEADS BIT FOR NEXT TIME
JZ     SHORT LCL_1        ;IF 1,LEADS ARE OK
OR     ECG_MODE,LEADS_OFF ;SET LEADS OFF FLAG
OR     COSTA,ECGOFF
AND    SH_PAT_SAV,ECGDSABL ;DISABLE ECG INPUT TO COMPARATOR
STC
RET

LCL_1:
LCL_2:
AND    ECG_hoe,NOT (LEADS_off); CLEAR BIT
OR     COSTA,NOT ECGOFF
CLC
RET

; Checking and adjusting threshold for ecgboxcar modul
chk_thresh:
test   ecg_block.0ffffh   ;wait til 50 ms is over
jnz    ct_ref
test   block_flg,1       ;adjust just one time after every r-wave
jz     ct_ref
dec    block_flg          ;clear block active flag
mov    ax,old_deriv      ;take 75% of old max
mov    bx,ax
mov    cx,2
shr    bx,cx
mov    ax,bx
mov    bx,max_deriv      ;and 25% of new max
shr    bx,cx
add    ax,bx             ;new average max value
mov    old_deriv,ax
mov    bx,ax             ;and take 75% of this value
shr    bx,cx
sub    ax,bx             ;new threshold
jmp    ct21

```

```

ct2i:   cap      ax,thresh_min    !if threshold ( min
        ja
ct3:    mov      ax,thresh_min    !set min value
ct_ret: mov      max_thresh.ax    !set threshold
        ret

set_thresh:
        test    find_max_req,0fffh
        jz      st1              !return if no max deriv search mode
        test    find_cnt,0ffffh
        jnz     st_ret          !return if inside 2 sec time interval
        mov     find_max_req,0    !reset flag
        mov     ax,max_deriv      !calculate 75% of max deriv value
        mov     old_deriv.ax     !save average max_deriv
        mov     bx,ax
        mov     cx,2
        shr    bx,cx
        sub    ax,bx
        mov     max_thresh.ax    !new threshold value
        inc    set_flg           !check if any r-wave in the next 2 sec
        mov     set_flg_cnt,TIME2000+5
        jmp     min_chk

st1:    test    set_flg,0fffh     !inside the next 2 sec interval
        jz      st_ret          !jump if no
        test    set_flg_cnt,0ffffh
        jnz     st_ret          !jump if ( 2 sec
        mov     set_flg,0        !reset flag
        cap    ecgdiy,0
        ja     st_ret           !jump ecg is synced

        mov     ax,max_thresh
        shr    bx,ax
        shr    bx,1
        shr    bx,1
        shr    bx,1
        sub    ax,bx
        mov     max_thresh.ax    !load min value
        inc    set_flg          !look for max again
        mov     find_cnt,TIME1000+5

min_chk:
        mov     ax,thresh_min    !check threshold value against min_thresh
        cap    ax,max_thresh
        jbe    st_ret
        mov     max_thresh.ax    !load minimum threshold value

st_ret: ret

!calc_slide_tmo calculates how long an interval may elapse since
!the last good R wave before the slider buffer should be cleared.
!It uses 2 and 1/2 times the average R-R period. ///
calc_slide_tmo:
        mov     ax,ravg
        mov     bx,ax
        shl    ax,1
        jc    calc1             !overflow
        shr    bx,1
        add   ax,bx
        jc    calc1             !overflow
        jmp    calc2

calc1:  mov     ax,0ffffh        !set to maximum
calc2:  mov     slide_tmo,ax
        ret

!clr_rr_hist clears the r-r history buffer dab ///
clr_rr_hist:
        mov     cx,8
        mov     di,offset ds:rrper    !clear 8 words from es:di
        push   ds
        pop    es
        xor    ax,ax
        cld
        rep   stosw
        ret

!Ecg boxcar filter.
ecgbox:
        mov     dx,bx
        mov     di,offset ds:ecg_buf  !save ecgdiidx
        cap    word ptr [bx+di],0    !@ data?
        jne    ecgb0
        mov     runsum,0
        mov     ecgboxcnt,4
        mov     cx,0
        jmp    ecgb1
        !yes, initialize the sum, set countdown

ecgb0:  sub     bx,8
        and    bx,ecgmask
        mov    ax,runsum
        cap    [bx],0
        jne    ecgb0b
        !safe to subtract oldest value?
        !no
        !yes

ecgb0b: mov     bx,dx
        add    ax,word ptr [bx+di]    !retrieve ecgdiidx
        mov    runsum,ax
        cap    ecgboxcnt,0
        ja     ecgb2
        !AX contains runsum
        !sums valid yet?
        !yes
        !no
        dec    ecgboxcnt

```

```

    cap    ecgboxcnt, 0           ;sums valid yet to compute entry?
    je     ecgb2
    mov    cx, 0
    jmp    short ecgb1
ecgb2:    shr     AX, 1           ;get 1/2 running sum
    sub    bx, 1
    and    bx, ecgmask
    mov    cx, word ptr [bx + di] ;bx indexes ecgbuff[ecgdiidx-1]
    sub    ax, 2                 ;cx contains ecgbuff[ecgdiidx-1]
    and    bx, ecgmask
    add    cx, word ptr [bx + di] ;bx indexes ecgbuff[ecgdiidx-2]
    ;following code determines whether aidsun ) 1/2 running sum
    ;cx to point to larger value, ax to smaller.
    ;Purpose is to compute aidsun = 1/2 running sum.
    ;On entry ax contains 1/2 running sum.
    cap    cx, ax
    jae    ecgb1a
    xchg   cx, ax
ecgb1a:  sub    cx, ax
ecgb1:   mov    bx, dx
    mov    di, offset ds:ecgboxbuf ;retrieve ecgdiidx
    mov    word ptr [bx + di], cx ;enter answer
    cap    ecg_block, 0
    je     ecgb1b
    mov    cx, max_deriv
    jbe    ecgb12
    mov    max_deriv, cx
    jmp    ecgb12
ecgb1b:  mov    cx, max_thresh
    jbe    ecgb1c
    cap    ecg200ms, 0
    jne    short ecgb1c
    mov    ecg_block, TIME100
ecgb1c:  test   ecg_mode, ignore_rvw ;should ignore rwave because signal railed?
    jz     short ecgb1d
    jmp    short ecgb12
ecgb1d:  cap    first_rvw_flg, 1
    je     short ecgb1ca
    mov    max_deriv, cx
    ;first rwave seen?
    ;yes, don't update max_deriv
ecgb1ca: call   rwave_chk
    rst
ecgb12:  rst
slider:  push   bx
    mov    al, slide_mode
    test   al, use_ecg
    jnz   slide0
    jmp    no_ecg
slide0:  xor    al, al
    cap    mode2, 2
    je     slide1
    mov    al, weight
    ;using ecg
    ;and
    ;if mode2 (beat-beat)
    ;   this_weight = 0
    ;else this_weight = weight
slide1:  mov    this_weight, al
    lea   bx, datbuf
    mov    al, dopidx
    xor    ah, ah
    add    bx, ax
    mov    cx, [bx]
    mov    ax, [bx+2]
    or     cx, ax
    jnz   short slide4
    mov    al, slide_mode
    and    al, not (use_ecg)
    or     al, skip_next_rvw
    ;ir = red = 0
    ;reset using ecg flag to no
    ; & skip next r wave interrupt
    mov    slide_mode, al
    jmp    metermode, 4
    jne   short slide2
    mov    metermode, 3
    jmp    short slide3
slide2:  cap    metermode, 6
    jne   short slide3
    mov    metermode, 5
slide3:  mov    ax, 0
    call  clr_newbuf
    mov    newidx2_on, 0
    jmp    slide4
slide4:  mov    al, dopidx
    cmp    al, dattrig
    mov    al, slide_mode
    jnz   short slide5
    and    al, not (shld skip)
    mov    slide_mode, al
    mov    echmod, 0
    jmp    short slide7
slide5:  test   al, shld_skip
    jz     short slide7
    mov    al, newidx2_on
    or     al, al
    jnz   slide6
    jmp    slide6
slide6:  ;ir and red have data not equal to 0
    ;has dopidx caught up to dattrig?
    ; i.e. to where the ecg occurred
    ;no
    ;yes, then don't skip putting data
    ; into the slider
    ;and per dab insistence !!!
    ;should we skip putting data into
    ; slider buffer?
    ;not skipping
    ;yes skipping
    ; is slider's ptr2 active?
    ; yes.
    ; not on, leave routine

```

```

slide6:      lea    bx, datbuf      ;skip mode - we advance slider's ptr2 alone
             mov    al, dopidx
             xor    ah, ah
             add    bx, ax
             mov    ax, [bx]
             push   bx
             lea    bx, newbuf
             add    bx, newidx2
             mov    cx, [bx]
             push   bx
             call   new_avg
             pop    bx
             mov    [bx], ax
             inc    bx
             inc    bx
             mov    cx, [bx]
             pop    dx
             push   bx
             mov    bx, dx
             inc    bx
             inc    bx
             mov    ax, [bx]
             call   new_avg
             pop    bx
             mov    [bx], ax
             jmp    slide7

slide7:      lea    bx, newbuf      ;not in skip mode - both slider ptrs advanced
             mov    ax, newidx
             add    bx, ax
             push   bx
             mov    cx, [bx]
             or     cx, cx
             jnz   short slide8
             xor    al, al
             mov    this_weight, al

slide8:      lea    bx, datbuf
             mov    al, dopidx
             xor    ah, ah
             add    bx, ax
             pop    cx
             lea    bx, newbuf
             mov    ax, newidx2
             add    dx, ax
             call   put_newbf

no_ecg:      jmp    short slideX

set_flg:     mov    al, slide_mode
             test   al, first_time
             jnz   short slideX
             mov    ax, elapsed_sec
             cmp    ax, slide_time
             jae   short set_flg
             mov    al, elapsed_hr
             cmp    al, 5
             jae   short set_flg
             jmp    short slideX

set_flg:     mov    al, slide_mode
             or     al, first_time
             mov    slide_mode, al

slideX:      pop    bx
             ret

;put_newbf moves entries from datbuf to newbuf using the following
;formula:
;newbuf[newidx] = ((this_weight-1)/this_weight)newbuf[newidx] + (
;1/this_weight)datbuf[dopidx]
;
;This procedure assumes bx points to datbuf[dopidx], cx points to
;newbuf[newidx]. Remember, both IR and red values must be placed.
;dx points to newbuf[newidx2]
put_newbf:
             push   dx
             push   bx
             push   cx
             mov    ax, [bx]
             pop    bx
             push   bx
             mov    cx, [bx]
             call   new_avg
             pop    bx
             mov    [bx], ax
             inc    bx
             inc    bx
             push   bx
             mov    cx, [bx]
             pop    dx
             pop    bx
             push   dx
             inc    bx
             inc    bx
             mov    ax, [bx]
             call   new_avg
             pop    bx
             mov    [bx], ax
;axp:///
             mov    dx, newidx2_on
             ;bx = newidx for the red data
             ;is 2nd newbuf pointer active?

```

```

or      di,di          ; (meanwhile.get 2nd newbuf pointer to ir)
pop     dx             ; no, newidx2 inactive
ja      short putnew0 ; yes, copy ir,red from 1st to 2nd newbuf ptr
dec     bx            ; back up to 1st ir
dec     cx,(bx)       ; & save contents
mov     bx,dx         ; point to 2nd ir
mov     [bx],cx      ; copy into 2nd ir
inc     bx            ; advance to 2nd red
inc     bx            ;
mov     [bx],ax      ; and copy into 2nd red
utnew0:
ret

new_avg - if weight is 0, return datbuff[dopidx] in ax.
         else, return (weight-1)/weight newbuf[newidx] + 1/weight datbuff[dopidx] in ax.
Routine assumes ax = datbuff[dopidx], cx = newbuf[either newidx or newidx2]
improvement - round division returns rather than truncating
ew_avg:
cwp     cx,0          ; zero in newbuf?
ja      short newx    ; yes, then return 100% boxcar
mov     bh,0          ;
mov     bl,this_weight ;
or      bx,bx         ;
jz      short newx    ;
mov     dx,0          ;
div     bx            ; dxax/bx = ax rem dx = datbuff[dopidx]/weight
push    ax            ; leave result
mov     ax,cx         ;
mov     dx,b         ;
div     bx            ; dxax/bx = ax rem dx = newbuf[newidx]/weight
dec     cx            ; get weight - 1
mul     bx            ; ax * bx = dxax = (weight-1)(newbuf[newidx]/weight)
or      dx,dx         ; result too big?
jz      new1         ; no
ppp     ax            ; yes, clear stack
mov     ax,$ffff      ; and return
jmp     newx          ;
new1:
mov     bx,ax         ; leave result
pop     ax            ;
add     ax,bx         ; result too big?
jnc     newx         ; no
mov     ax,$ffff      ; yes, return
newx:
ret

clr_newbuf - routine to clear newbuf. Assume ax contains the index
into newbuf from which to clear it! i.e., clear newbuf from where
ax points to til the end.
lr_newbuf:
lea     bx,newbuf     ; bx points to address from which to clear
mov     cx,newlen     ;
sub     cx,ax         ; cx contains number of bytes to clear
or      cx,cx         ;
jz      short clr2    ; zero is a problem
ja      short clr2    ; so is a negative number
cwp     cx,$000       ;
ja      clr2         ; so is too large a number
shr     cx,1          ; need to know how many words to clear
mov     di,bx         ;
push   ds            ;
pop     es           ;
xor     ax,ax        ; loop counter is fine
cld
rep     stosw        ;
lr2:
ret

```

## Software appendix B

0 D/A.TEMPLATE CHNL0

2 A/D.TEMPLATE CHNLS.23  
2 A/D.TEMPLATE CHNLS.CAL

4 STRING FILE.NAME

INTEGER DIM[ 512 , 2 ] ARRAY RAW.DAT.1  
DIM[ 512 , 2 ] ARRAY RAW.DAT.2  
DIM[ 1 ] ARRAY ISAT  
DIM[ 2048 , 8 ] ARRAY DAT.BUF

SCALAR PTR SCALAR CTR SCALAR HOW.LONG SCALAR PTR.MAX  
SCALAR PTR.MIN SCALAR RCAL SCALAR MINI SCALAR MIN2

## COMPLEX

```

DIM[ 128 ] ARRAY SHORT.DAT
DIM[ 128 ] ARRAY SCONJ.DAT
DIM[ 512 ] ARRAY FOR.DAT
SCALAR FOR.DC

```

## REAL

```

DIM[ 512 ] ARRAY HAMMING.DAT
DIM[ 1024 ] ARRAY SAT.DAT
SCALAR RED.MAX SCALAR IR.MAX SCALAR RNEW
SCALAR SAT SCALAR B01 SCALAR B02 SCALAR B01 SCALAR B02 SCALAR SLOPE
SCALAR INTERCEPT SCALAR QUAL

```

## : set.up

```

HAMMING.DAT [IRAMP
HAMMING.DAT 2. * PI * 512. / COS -.46 * .54 + HAMMING.DAT :=
0 MINI := 0 MINZ := 4095 ISAT :=
1 set.s.optima
5 set.s.points

```

## : SET.TEMPLATE

```

CHNLS.23
RAW.DAT.1 RAW.DAT.2 CYCLIC DOUBLE.TEMPLATE.BUFFERS
.6 CONVERSION.DELAY
CHNL0 ISAT CYCLIC TEMPLATE.BUFFER

```

## : WAIT.FOR.USER

```

SCREEN.CLEAR
10 10 GOTO.XY
INTEN.ON
.* SET LOCATION 24 TO 0 ... THEN: *
.* STRIKE ANY KEY TO BEGIN. * CR
INTEN.OFF
PCKEY ?DROP DROP

```

## : OPEN.DATA.FILE

```

NORMAL.DISPLAY
.* HOW LONG A DATA SET IN MINUTES ? * INPUT 7 * HOW.LONG :=
CR
.* ENTER THE FILE NAME XXXXXXXX.DAT * INPUT FILE.NAME :=
CR .* PLEASE WAIT WHILE THE DATA FILE IS CREATED... *

```

```

FILE.CREATE
COMPLEX DIM[ 512 ] SUBFILE
HOW.LONG TIMES
END
FILE.NAME DEFER> FILE.CREATE

```

## : START.ACQ

```

OAS.INIT
CLEAR.TASKS
CHNL0 1 TASK ARRAY>D/A.OUT
CHNLS.23 2 TASK A/D.IN>ARRAY
17 TASK.PERIOD
PRIME.TASKS
TRIGGER.TASKS

```

```

: STOP.ACQ
  STOP.TASKS
  CLEAR.TASKS
  NORMAL.DISPLAY

```

```

: FIND.BETAS          \ GET BETAS FOR SAT CALC
  RCAL                \ PLACE RCAL ON THE STACK

```

```

CASE
\ RCAL      801      BR1      802      BR2      SLOPE      INTERCEPT
OF          10563    27960    5069    51763    -15743      9237      ENDOF
ENDCASE

```

```

INTERCEPT :=
SLOPE :=
BR2 :=
BOZ :=
BR1 :=
BO1 :=

```

```

: SHORT.FLIP
  128 Z 00
  130 I - PTR :=
  SHORT.DAT [ I ] SCONJ.DAT [ PTR ] :=
  LOOP
  SHORT.DAT [ I ] SCONJ.DAT [ I ] :=
  SCONJ.DAT CONJ SCONJ.DAT :=
  ***** COMPUTE SATURATI...
  QUAL .2 > IF
  BR2 RNEW BR1 * - BO1 BR1 - RNEW * BO2 - BR2 + / 100. *
  SAT :=
  SAT 70. < 1?
  RNEW 4. / SLOPE * INTERCEPT + 4. * 256. /
  SAT :=
  else
  THEN
  SAT 102. > IF 102. SAT := ELSE THEN
  SAT 0. < IF 0. SAT := ELSE THEN
  SAT SAT.DAT [ CTR ] :=
  SAT 100. > IF 100. SAT := ELSE THEN
  SAT 40.95 * FIX ISAT :=
  CR ." SAT = " CR SAT . CR CTR .
  | CTR + CTR :=
  .25 .51 VUPORT.ORIG
  .75 .50 VUPORT.SIZE
  SHORT.DAT ZMAG SUB( 1 , 40 ) Y.AUTO.PLOT PTR.MIN 5 + CR .
  STACK.CLEAR
  ELSE
  THEN

```

```

: SHORT.PROCESS
home screen.clear
FOR.DAT [ISUM SIZ. / DUP FOR.DC := FOR.DAT SWAP - FOR.DAT :=
FOR.DC ZREAL 200. > IF
FOR.DAT ZREAL [IMAX FOR.DAT ZREAL ()min - for.dc zreal /
dup .2 < IF
0. > IF
FOR.DAT HAMMING.DAT * FOR.DAT :=
FOR.DAT SUB[ 1 , 128 , 4 ] FOR.DAT SUB[ 2 , 128 , 4 ]
FOR.DAT SUB[ 3 , 128 , 4 ] FOR.DAT SUB[ 4 , 128 , 4 ] + + + SHORT.DAT :=
SHORT.DAT FFT SHORT.DAT :=
SHORT.FLIP
SHORT.DAT SCONJ.DAT + ZMAG
SUB[ 4 , 30 ] DUP LOCAL.MAXIMA DROP 1 - PTR.MIN :=
SUB[ PTR.MIN , 3 ] [ISUM IR.MAX :=
SHORT.DAT SCONJ.DAT - ZMAG
SUB[ 4 , 30 ] SUB[ PTR.MIN , 3 ] [ISUM RED.MAX :=
RED.MAX FOR.DC ZIMAG / dup 256. / . cr
IR.MAX FOR.DC ZREAL / dup 256. / . cr DUP QUAL := /
. * R = * ? cr RNEW :=
sat.comp
THEN
THEN
ELSE ." TOO SMALL "
THEN
STACK.CLEAR
: GET.IJ
HOW.LONG 1 + 1 DO
BEGIN
?BUFFER.SWITCH
UNTIL
?BUFFER.A/B
IF
RAW.DAT.1 XSECT[ 1 , 1 ] MINI -
.25 .01 VUPORT.ORIG
.75 .50 VUPORT.SIZE
DUP Y.AUTO.PLOT
RAW.DAT.1 XSECT[ 1 , 2 ] MIN2 -
ELSE
RAW.DAT.2 XSECT[ 1 , 1 ] MINI -
.25 .01 VUPORT.ORIG
.75 .50 VUPORT.SIZE
NO.LABELS
DUP Y.AUTO.PLOT
RAW.DAT.2 XSECT[ 1 , 2 ] MIN2 -
THEN
Z=X+IY FOR.DAT :=
FOR.DAT CTR SUBFILE ARRAY>FILE
SHORT.PROCESS
LOOP
1
: IDLE.IT
1 CTR :=
BEGIN
BEGIN
?BUFFER.SWITCH

```

```

UNTIL
?BUFFER.A/B
IF
RAW.DAT.1 XSECT( 1 , 1 ) MIN1 -
.25 .01 VUPOINT.ORIG
.75 .50 VUPOINT.SIZE
DUP Y.AUTO.PLOT
RAW.DAT.1 XSECT( 1 , 2 ) MIN2 -
ELSE
RAW.DAT.2 XSECT( 1 , 1 ) MIN1 -
.25 .01 VUPOINT.ORIG
.75 .50 VUPOINT.SIZE
DUP Y.AUTO.PLOT
RAW.DAT.2 XSECT( 1 , 2 ) MIN2 -
THEN
Z=X+IY FOR.DAT :=
SHORT.PROCESS
?KEY
UNTIL
PCKEY DROP

```

```

: SHOW.IT
STOP.ACQ
NORMAL.DISPLAY
SCREEN.CLEAR
home ." 1 STARTS A DISPLAY ONLY OXIMETER."
CR CR ." 2 DOES OXIMETRY AND STORES DATA FILES."
CR CR ." 3 CHECKS OFFSET CALIBRATION."
CR CR ." 4 READS RED AND IR VOLTAGES."
CR CR ." 5 REPLAYS RECORDED DATA FILES."
CR CR ." 6 RETURNS TO DOS."
CR CR ." 7 CLOSES DATA FILES ON ERRORS."
cr cr ." 8 PRINT INSTRUCTIONS ON SCREEN."
cr cr ." ENTER A SELECTION."
SET.TEMPLATE
) CTR :=
OPEN.DATA.FILE CR
FILE.NAME DEFER> FILE.OPEN
." ENTER RCAL VALUE CODE ( 63 - 84 ) " *INPUT RCAL :=
FIND.BETAS
START.ACQ
GRAPHICS.DISPLAY
GRID.OFF
GET.IT
STOP.ACQ
FILE.CLOSE
NORMAL.DISPLAY
SHOW.IT
CR

: IDLE
SET.TEMPLATE
) CTR :=
." ENTER RCAL VALUE CODE ( 63 - 84 ) " *INPUT RCAL :=

```

```

FIND.BETAS
START.ACQ
GRAPHICS.DISPLAY
GRID.OFF
IOLE.IT
STOP.ACQ
NORMAL.DISPLAY
SHOW.IT
CR

```

```

: CAL.CHECK
  SET.TEMPLATE
  NORMAL.DISPLAY
  SCREEN.CLEAR
  WAIT.FOR.USER
  START.ACQ
  BEGIN
  ?BUFFER.SWITCH
  UNTIL
  STOP.ACQ
  RAW.DAT.1 XSECT( 1 , 1 ) (IMIN DUP MINI := FLOAT 405.5 /
  ." IR zero is " . cr
  RAW.DAT.1 XSECT( 1 , 2 ) (IMIN DUP MIN2 := FLOAT 409.5 /
  ." Red zero is " .
  3000 MSEC.DELAY
  SHOW.IT

```

```

: READ.VOLTS
  cr
  CHNLS.CAL
  A/D.INIT
  A/D.IN 409.5 / ." red volts = " . 409.5 / ." IR volts = " .
  CHNL0 D/A.INIT
  I. CTR :=
  NORMAL.DISPLAY DIR *.DAT
  CR ." ENTER THE FILE TO REPLAY " "INPUT FILE.NAME " :=
  CR FILE.NAME DEFER> ?FILE
  CR ." ENTER RCAL VALUE " $INPUT RCAL :=
  FIND.BETAS
  CR ." WHICH FILE TO BEGIN REPLAY ? " $INPUT
  DUP 1 + CR ." HOW MANY FILES TO REPLAY " $INPUT + SWAP
  graphics.display DO
  I.SUBFILE FOR.DAT FILE>ARRAY
  .25 .01 VUPOINT.ORIG
  .75 .50 VUPOINT.SIZE
  for.dat zreal y.auto.plot
  SHORT.PROCESS
  ISAT [ 1 ] D/A.OUT
  2000 msec.delay
  LOOP
  FILE.CLOSE
  SHOW.IT

```

```

: main.loop
set.up
show.it
begin
  BEGIN
  $input
  ?dup not if
  cr ." Invalid number, re-enter: "
  then
  UNTIL
    case
    1 of idle endof
    2 of doit endof
    3 of cal.check endof
    4 of read.volts endof
    5 of replay.dat endof
    6 of bye endof
    7 of file.close endof
    8 of print.inst endof
    endcase

again
ONERR:

```

```

key-drop
MYSELF

```

```

;
banner: my.banner
CR
."
CR CR CR
."
CR CR CR
."
CP CR
."
CR CR
."
CR CR
."
_iBANNER

```

```

NELLCOR PULSE OXIMETER"
FOR EXPERIMENTAL USE ONLY"
COPYRIGHT 1988"
PROPRIETARY INFORMATION"
ALL RIGHTS RESERVED"
Written by: R. T. Stone, Ph.D."

```

We claim:

1. A method for calculating [the] *an* amount of a blood constituent from the blood flow characteristics of a patient comprising:

detecting an absorption signal corresponding to [the] 5  
absorption of light measured at two or more wave-  
lengths in the patient's tissue including periodic  
changes caused by periodic arterial pulses in the blood  
flow characteristics and aperiodic changes unrelated to  
the patient's heartbeat;

detecting an ECG signal corresponding to the patient's 10  
ECG waveform corresponding to the periodic electrical  
heart activity of the patient;

selecting a first time-measure of the absorption signal 15  
including a maximum and minimum amplitude change  
in absorption;

selecting a second time-measure of the ECG signal 20  
including components corresponding to the occurrence  
of the heartbeat;

correlating the ECG signal and the absorption signal by 25  
multiplying the first time-measure of the absorption  
signal and the second time-measure of the ECG signal  
together to form a waveform product and thereafter  
shifting the time-measure of the absorption signal back-  
wards in time relative to the time-measure of the ECG  
signal and multiplying the shifted and unshifted wave-  
forms together to identify a maximum waveform prod-  
uct corresponding to the product of the ECG signal  
corresponding to the occurrence of the heartbeat and  
the maximum amplitude of the absorption signal;

processing the absorption signal and the determined cor- 30  
relation to identify the periodic changes in the absorp-  
tion signal associated with the determined maximum  
waveform product likely to correspond to arterial  
pulses in the patient's blood flow characteristics; and

calculating the amount of the blood constituent from the 35  
identified periodic changes in the absorption signal.

2. The method of claim 1 wherein the ECG signal further 40  
comprises the R-wave component of the ECG signal so that  
the maximum waveform product corresponds to the product  
of the R-wave component and the maximum of the absorp-  
tion signal.

3. The method of claim 2 wherein the first time-measure 45  
is shorter in length than the second time-measure so that as  
the absorption signal time-measure is shifted backward  
relative to the ECG time-measure the latest maximum  
waveform product corresponds to the most recent heartbeat  
activity in the first and second time-measures.

4. The method of claim 3 wherein the first time-measure 50  
includes a first plurality of maximum amplitudes and the  
second time-measure includes a second plurality of R-wave  
signals so that the maximum waveform product further  
comprises an array of maximum waveform product.

5. Apparatus for calculating [the] *an* amount of a blood 55  
constituent from the blood flow characteristics of a patient  
comprising:

means for photoelectrically detecting an absorption signal 60  
corresponding to [the] absorption of light measured at  
two or more wavelengths in the patient's tissue includ-  
ing periodic changes caused by periodic arterial pulses  
in the blood flow characteristics and aperiodic changes  
unrelated to the patient's heartbeat;

means for electrically detecting an ECG signal corre- 65  
sponding to the patient's ECG waveform correspond-  
ing to the periodic electrical heart activity of the  
patient;

means for selecting a first time-measure of the absorption 5  
signal including a maximum and minimum amplitude  
change in absorption;

means for selecting a second time-measuring of the ECG 10  
signal including components corresponding to the  
occurrence of the heartbeat;

means for correlating the ECG signal and the absorption 15  
signal by multiplying the first time-measure of the  
absorption and the second time-measure of the ECG  
signal together to form a waveform product and there-  
after shifting the time-measure of the absorption signal  
backwards in time relative to the time-measure of the  
ECG signal and multiplying the shifted and unshifted  
waveforms together to identify a maximum waveform  
product corresponding to the product of the ECG signal  
corresponding to the occurrence of the heartbeat and  
the maximum amplitude of the absorption signal;

means for processing the absorption signal and the deter- 20  
mined correlation to identify the periodic changes in  
the absorption signal associated with the determined  
maximum waveform product likely to correspond to  
arterial pulses in the patient's blood flow characteris-  
tics; and

means for calculating the amount of the blood constituent 25  
from the identified periodic changes in the absorption  
signal.

6. The apparatus of claim 5 wherein the means for 30  
electrically detecting an ECG signal further comprises  
means for detecting the R-wave component of the ECG  
signal so that the maximum waveform product corresponds  
to the product of the R-wave component and the maximum  
of the absorption signal.

7. The apparatus of claim 6 wherein the first time-measure 35  
is shorter in length and later in time than the second  
time-measure so that as the absorption signal time-measure  
is shifted backwards relative to the ECG time-measure, the  
latest maximum waveform product corresponds to the most  
recent heartbeat activity in the first and second time-meas-  
ures.

8. The apparatus of claim 7 wherein the first time-measure 40  
includes a first plurality of maximum amplitudes and the  
second time-measure includes a second plurality of R-wave  
signals so that the maximum waveform product further  
comprises an array of maximum waveform products.

9. A method for calculating [the] *an* amount of a blood 45  
constituent from a patient's blood flow characteristics  
including aperiodic information corresponding to artifacts  
and periodic information corresponding to arterial pulses,  
comprising:

*directing light of two or more wavelengths toward the 50*  
*patient's tissue;*

detecting a set of first signals representing [the] absorp- 55  
tion of light measured at *said* two or more wavelengths  
[of light] in the patient's tissue including detected  
information corresponding to changes in absorption as  
a result of changes in the blood flow characteristics;

detecting a second signal representing the occurrences of 60  
a selected portion of [the] *an* ECG waveform of the  
patient;

processing the first and second signals to enhance [the] 65  
periodic information contained in each individual sig-  
nal whereby the first signals are processed in a repeti-  
tive manner, one discrete portion at a time, and the  
occurrence of a selected portion of the patient's ECG  
waveform in the second signal initiates processing of a  
discrete portion of the first signals; and

65

calculating the amount of *said* blood constituent using the enhanced periodic information in the processed portions of the first signals.

10. The method of claim 9 wherein processing the first and second signals further comprises correlating the discrete portions of the first signals and the occurrences of [a] *said* selected portion of the patient's ECG waveform in the second signals.

11. The method of claim 10 wherein detecting the second signal further comprises detecting a signal representing the occurrences of the R wave portion of the ECG waveform of the patient.

12. The method of claim 11 wherein processing the first and second signals further comprises determining whether or not the detected information in the *discrete* portions of the first signals are likely to be arterial pulses by using the determined correlation and preferentially processing detected information determined likely to be arterial pulses for use in calculating *the amount of said blood [constituents] constituent*.

13. The method of claim 12 wherein preferentially processing detected information further comprises rejecting detected information determined not likely to be arterial pulses so that rejected information is not used in calculating the blood constituent.

14. The method of claim 12 wherein processing the first and second signals further comprises determining whether or not detected information in a discrete portion of the first signals is likely to be an arterial pulse by using the determined correlation after each occurrence of an R wave portion in the second signal.

15. The method of claim 11 wherein correlating the first and second signals further comprises:

determining a period of time after the occurrence of [an] *said* R wave in which detected information in the *discrete* portions of the first signals corresponding to blood flow characteristic changes caused by arterial pulses are likely to be detected;

determining that detected signal information in the discrete portions of the first signals are likely to be arterial pulses when detected in the determined period of time after the occurrence of [an] *said* R wave; and

calculating the *amount of said blood [constituents] constituent* further comprises preferentially processing any determined detected information for use in calculating *the amount of said blood [constituents] constituent*.

16. The method of claim 15 wherein preferentially processing detected information further comprises rejecting detected information detected other than in the determined period of time after the R wave occurs so that rejected information is not used in the calculation of *the amount of said blood [constituents] constituent*.

17. The method of claim 15 wherein determining whether or not detected information in a discrete portion of the first signals is acceptable for preferential processing as corresponding to an arterial pulse by using the determined correlation after each occurrence of an R wave portion in the second signal.

18. The method of claim 11 wherein calculating the amount of *said* blood constituent further comprises calculating oxygen saturation of hemoglobin in arterial blood.

19. The method of claim 10 wherein correlating the first and second signals further comprises:

synchronizing the occurrence of a plurality of discrete portions of the first signals;

synchronizing the occurrence of a plurality of occurrences of the R wave portion in the second signal; and

66

correlating the synchronized discrete portions of the [first] *first* signals and the R wave portions.

20. Apparatus for calculating [the] *an* amount of a blood constituent from a patient's blood flow characteristics including arterial pulses and artifacts comprising:

means for photoelectrically detecting a set of first signals representing the absorption of light measured at two or more wavelengths in the patient's tissue including detected information corresponding to changes in absorption as a result of changes in the blood flow characteristics;

means for detecting a second signal representing the occurrences of a selected portion of [the patient's] *an* ECG waveform of the patient;

means for processing the first and second signals to enhance the periodic information contained in each individual signal whereby each occurrence of [a] *said* selected portion in the second signal initiates processing of [a] discrete portions of the first signals so that the information in the first signals are processed in a repetitive manner; and

means for calculating the amount of *said* blood constituent using the enhanced information in the processed portions of the first signals.

21. The apparatus of claim 20 wherein the means for processing the first and second signals further comprises means for correlating the discrete portions of the first signals with the occurrences of [a] *said* selected portion of the patient's ECG waveform in the second signal.

22. The apparatus of claim 21 wherein the means for detecting a second signal further comprises means for detecting a signal corresponding to the occurrences of the R wave portion of the patient's ECG waveform.

23. The apparatus of claim 21 wherein the processing means further comprises:

means for determining whether or not the detected information in the discrete portions of the first signals are likely to be arterial pulses using the determined correlation; and

means for preferentially processing detected information determined likely to be arterial pulses for use in calculating *the amount of said blood [constituents] constituent*.

24. The apparatus of claim 23 wherein the means for preferentially processing detected information further comprises means for rejecting detected information determined not likely to be arterial pulses so that rejected information is not used in calculating *the amount of said blood [constituents] constituent*.

25. The apparatus of claim 23 wherein the processing means further determines whether or not detected information in a discrete portion of the first signals is likely to be an arterial pulse using the determined correlation after each occurrence of an R wave portion in the second signal.

26. The apparatus of claim 21 wherein the means for correlating the first and second signals further comprises:

first determining means for determining a time period after the occurrence of an R wave in which detected information in the first signals corresponding to blood flow characteristic changes caused by arterial pulses are likely to be detected;

second determining means for determining that detected information in the discrete portions of the first signals are likely to be arterial pulses when detected in the determined period of time after the occurrence of [an] *said* R wave; and

67

wherein the means for calculating *the amount of said blood constituent* further comprises means for preferentially processing detected information for use in calculating *the amount of said blood [constituents] constituent*.

27. The apparatus of claim 26 wherein the second determining means further comprises means for rejecting detected information detected other than in the determined period of time after the R wave occurs so that rejected information is not used in calculating *the amount of said blood [constituents] constituent*.

28. The apparatus of claim 26 wherein the second determining means further comprises calculating the amount of whether or not detected information in a discrete portion of the first signals is likely to be an arterial pulse using the determined correlation after each occurrence of an R wave.

29. The apparatus of claim 21 wherein the means for calculating further comprises calculating the amount of oxygen saturation of hemoglobin in arterial blood.

30. A *method of calculating an amount of a blood constituent from the blood flow characteristics of a patient comprising:*

*subjecting the patient's tissue to electromagnetic energy, thereby facilitating the transformation of arterial blood flow in the patient's tissue into a blood flow signal, the blood flow signal corresponding to the arterial blood flow including periodic changes caused by periodic arterial pulses in the blood flow characteristics and changes caused by artifact;*

*detecting the blood flow signal;*

*detecting the occurrence of a heartbeat of the patient;*

*correlating the detected blood flow signal and the occurrence of a heartbeat;*

*processing the blood flow signal and the determined correlation to identify the periodic changes in the blood flow signal likely to correspond to arterial pulses in the*

68

*patient's blood flow characteristics; and calculating the amount of the blood constituent from the identified periodic changes in the blood flow signal.*

31. *The method of claim 30 wherein said blood constituent is the oxygen saturation of hemoglobin in arterial blood.*

32. *The method of claim 31 wherein said step of detecting the blood flow signal comprises detecting an absorption signal corresponding to the absorption of the electromagnetic energy measured at two or more wavelengths in the patient's tissue.*

33. *The method of claim 31 wherein said correlating step comprises the steps of:*

*synchronizing the occurrence of a plurality of changes in the blood flow signal;*

*synchronizing the occurrences of a plurality of selected portions of the heartbeat; and*

*correlating the synchronized changes in the blood flow signal with the synchronized portions of the heartbeat.*

34. *The method of claim 30 wherein said blood constituent is the oxygen saturation of hemoglobin in arterial blood;*

*said step of detecting the blood flow signal comprises detecting an absorption signal corresponding to the absorption of the electromagnetic energy measured at two or more wavelengths in the patient's tissue; and*

*said correlating step comprises the steps of synchronizing the occurrence of a plurality of changes in the blood flow signal,*

*synchronizing the occurrences of a plurality of selected portions of the heartbeat, and*

*correlating the synchronized changes in the blood flow signal with the synchronized portions of the heartbeat.*

\* \* \* \* \*