



US00D960355S

(12) **United States Design Patent**  
**Smith**

(10) **Patent No.:** **US D960,355 S**

(45) **Date of Patent:** **\*\* Aug. 9, 2022**

(54) **DELIVERY SYRINGE**

D926,968 S \* 8/2021 Kern ..... D24/113  
D930,897 S \* 9/2021 Qiu ..... D27/162  
D946,141 S \* 3/2022 Krulevitch ..... D24/113

(71) Applicant: **Ultradent Products, Inc.**, South Jordan, UT (US)

**OTHER PUBLICATIONS**

(72) Inventor: **Wade Robert Smith**, American Fork, UT (US)

Mosaic™ Syringes and Singles, Ultradent, Ultradent.com, [Post-date Unknown], [Site seen Mar. 31, 2022], Seen at URL: <https://www.ultradent.com/products/categories/composites/paste-type-composite/mosaic?group=4022> (Year: 2022).\*  
Glatiramer Acetate Injection, Viatris, Catalog, [Publication date 2021], [Site seen Mar. 31, 2022], Seen at URL: [https://www.viatrisadvocate.com/-/media/viatrisadvocatecom/pdf/ga-2021-0098\\_us\\_viatrisadvocatewelcomepackpatientinjectionbrochure.pdf?la=en](https://www.viatrisadvocate.com/-/media/viatrisadvocatecom/pdf/ga-2021-0098_us_viatrisadvocatewelcomepackpatientinjectionbrochure.pdf?la=en) USE (Year: 2021).\*

(73) Assignee: **ULTRADENT PRODUCTS, INC.**, South Jordan, UT (US)

(\*\*) Term: **15 Years**

\* cited by examiner

(21) Appl. No.: **29/652,606**

(22) Filed: **Sep. 30, 2020**

(51) **LOC (13) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/112; D24/113**

(58) **Field of Classification Search**  
USPC ..... D24/112–114, 108, 133, 127–130, 186  
CPC ..... A61M 5/178; A61M 5/20; A61M 5/31;  
A61M 5/3146; A61M 5/3129; A61M 5/3148; A61M 5/315

*Primary Examiner* — Natasha Vujcic  
*Assistant Examiner* — Gilbert B Ford  
(74) *Attorney, Agent, or Firm* — Maschoff Brennan

See application file for complete search history.

(57) **CLAIM**

The ornamental design for a delivery syringe, as shown and described.

(56) **References Cited**


**U.S. PATENT DOCUMENTS**

D627,061 S \* 11/2010 Van der Stappen ..... D24/113  
D765,239 S \* 8/2016 Hauck ..... D24/113  
D765,240 S \* 8/2016 Hauck ..... D24/113  
D766,425 S \* 9/2016 Hauck ..... D24/113  
D799,026 S \* 10/2017 Jones ..... D24/113  
D878,566 S \* 3/2020 Jansen ..... D24/113  
D878,567 S \* 3/2020 Jansen ..... D24/113  
D884,161 S \* 5/2020 Stewart ..... D24/112  
D907,765 S \* 1/2021 Eriksen ..... A61M 5/24  
D24/112

**DESCRIPTION**

FIG. 1 is a perspective view of a delivery syringe; FIG. 2 is another perspective view of the delivery syringe; FIG. 3 is a top view of the delivery syringe; FIG. 4 is a bottom view of the delivery syringe; FIG. 5 is a left-side view of the delivery syringe; FIG. 6 is a right-side view of the delivery syringe; FIG. 7 is a front view of the delivery syringe; and, FIG. 8 is a rear view of the delivery syringe. The broken lines in the drawings illustrate portions of the delivery syringe and form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

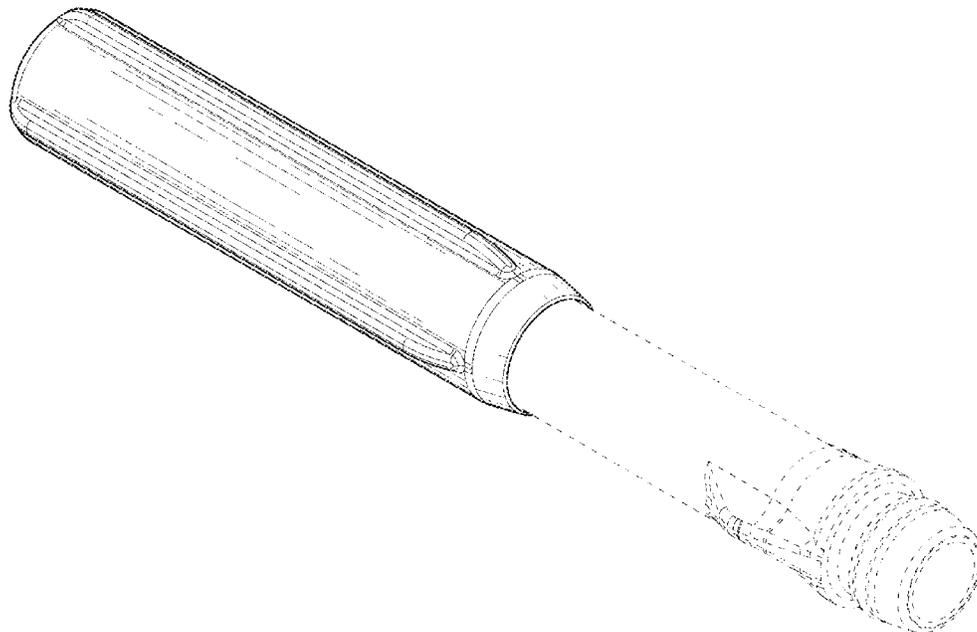

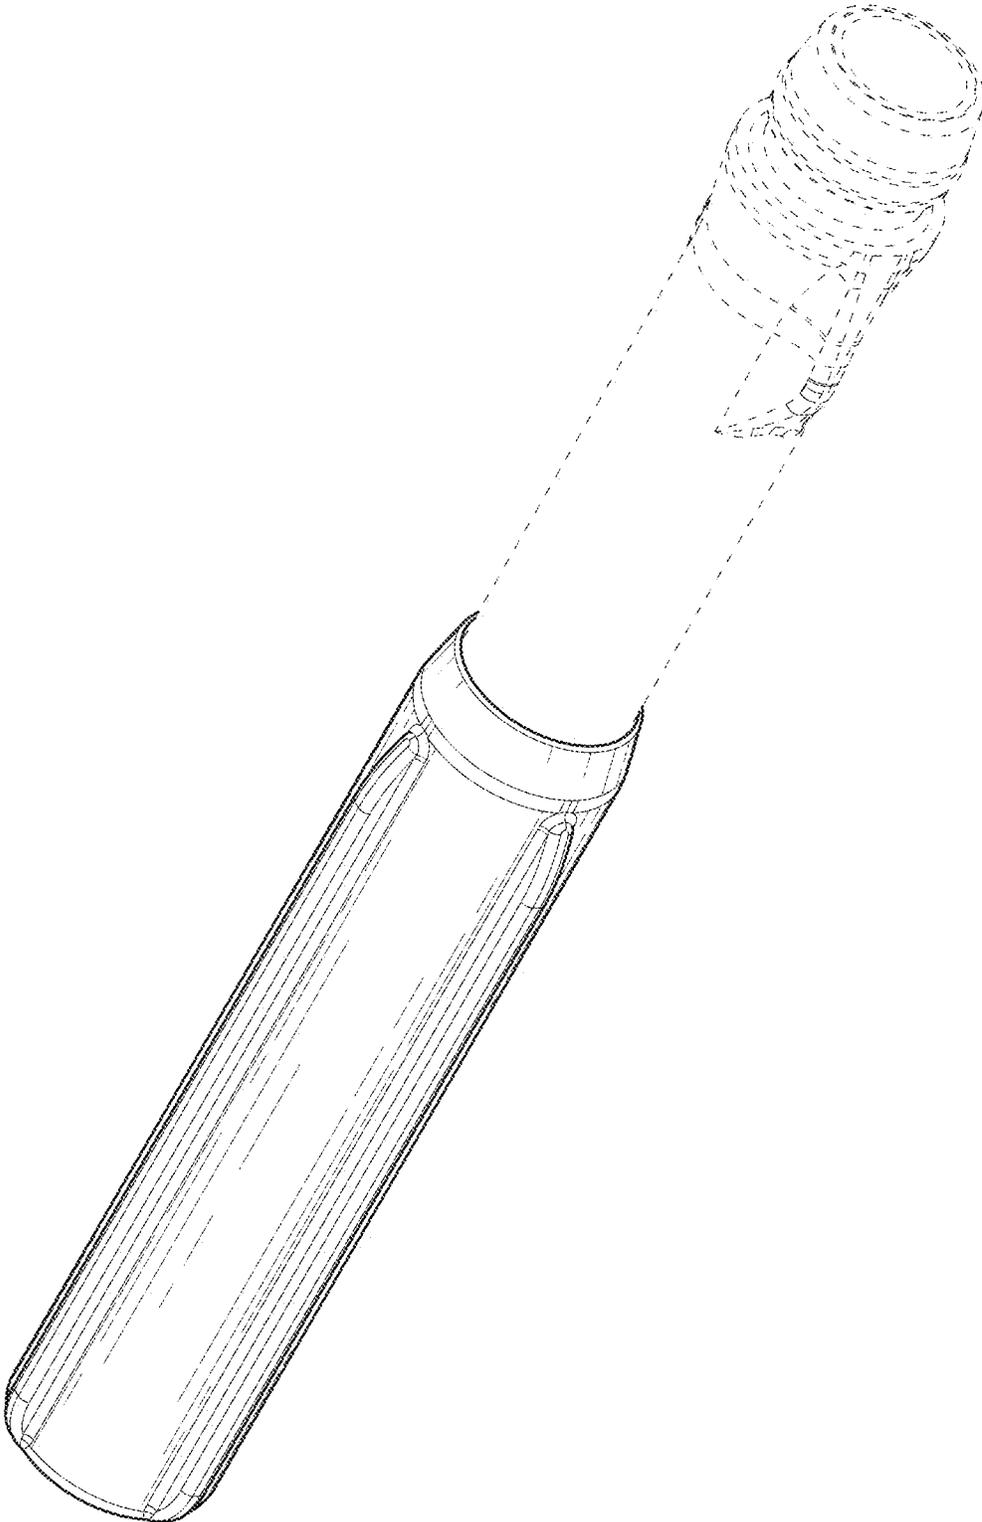


FIG. 1

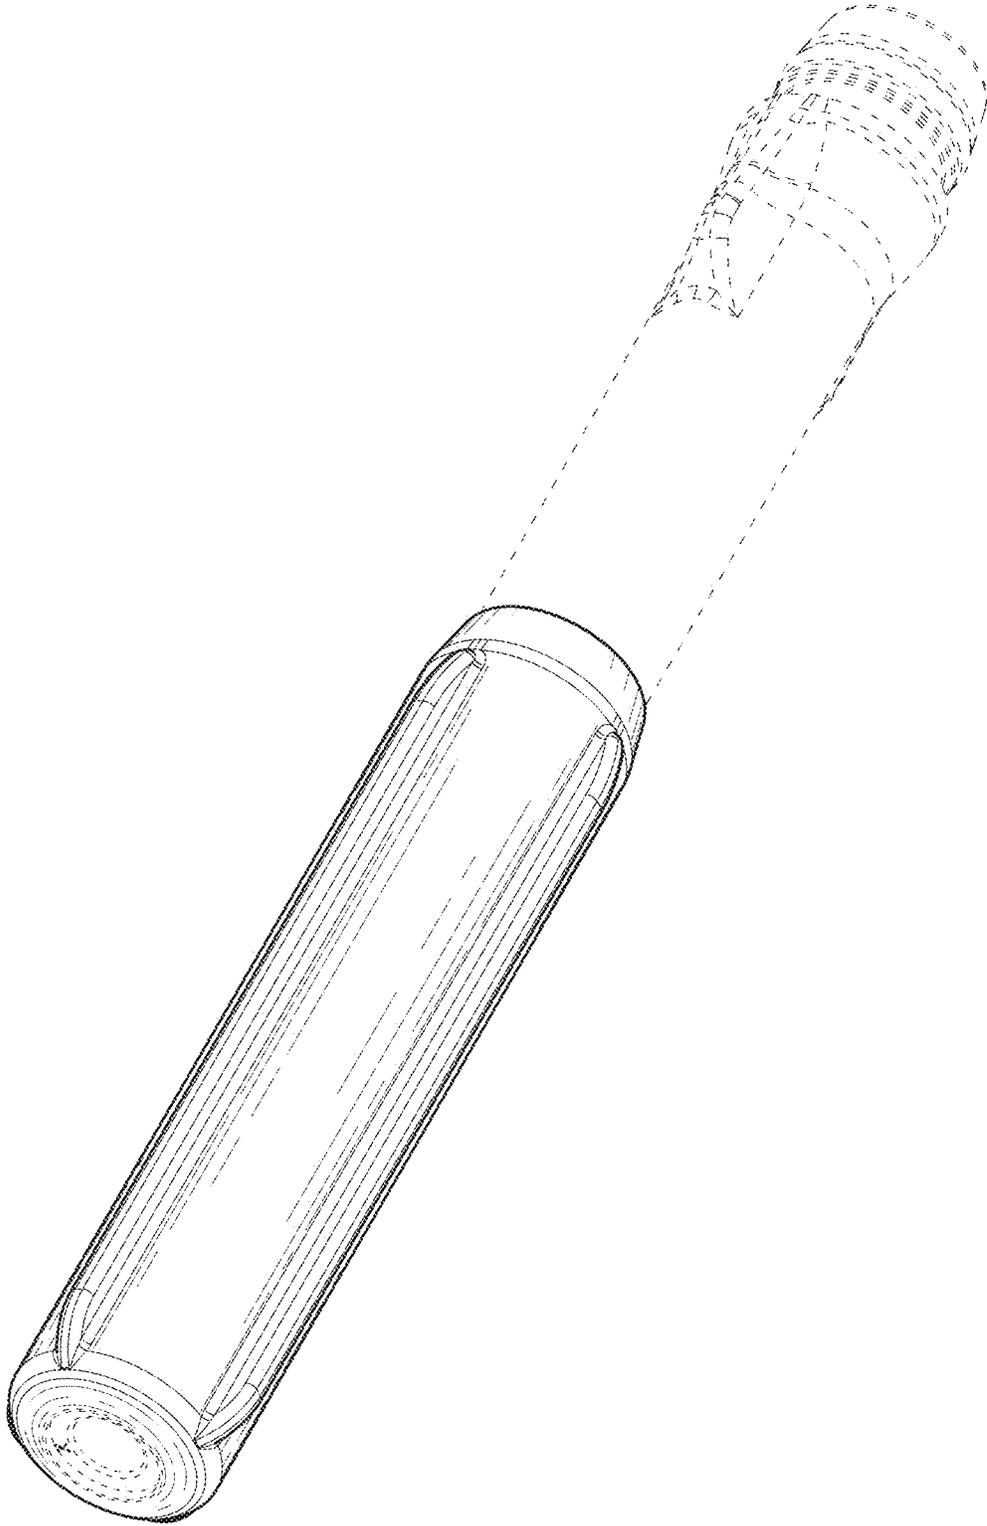


FIG. 2

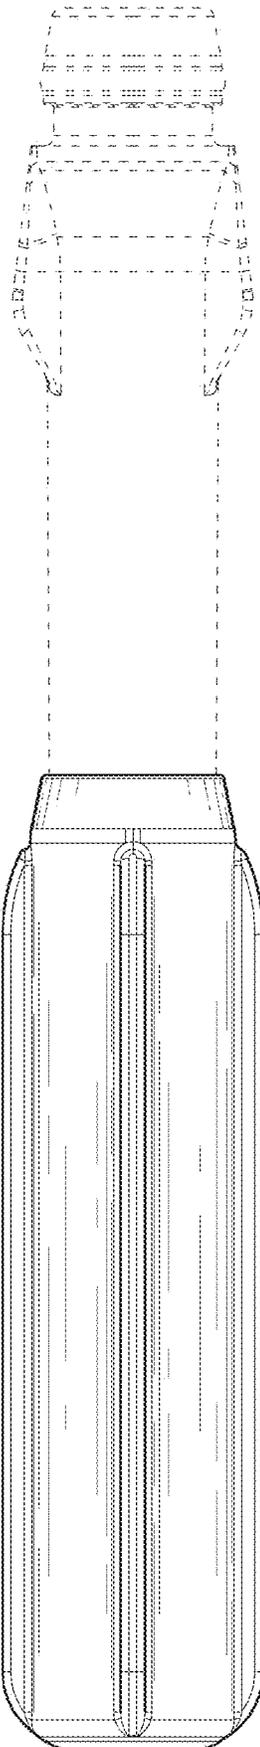


FIG. 3

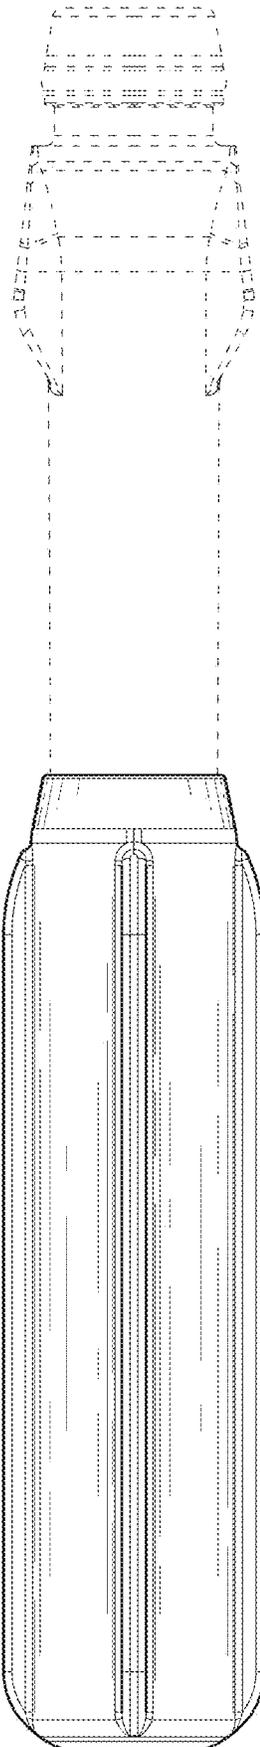


FIG. 4

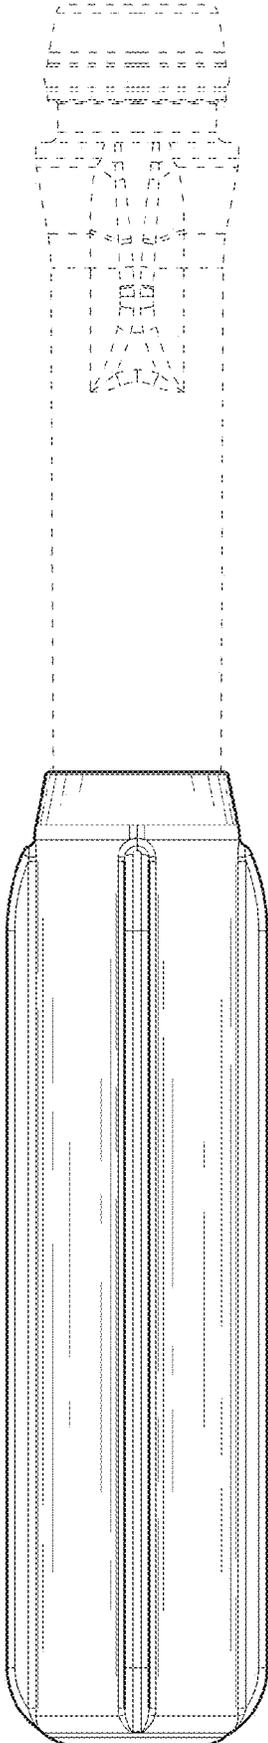


FIG. 5

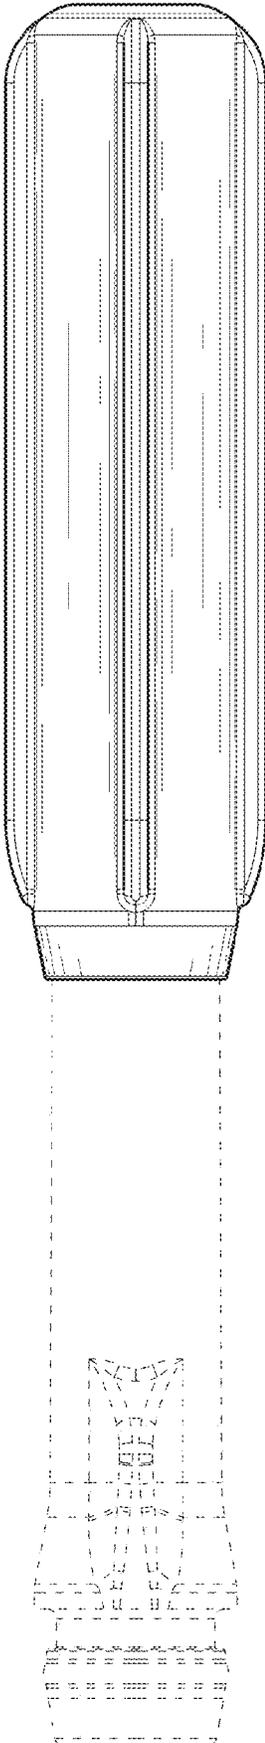


FIG. 6




FIG. 8




FIG. 7