

**(12) PATENT**  
**(19) AUSTRALIAN PATENT OFFICE**

**(11)** Application No. **AU 199712209 B2**  
**(10)** Patent No. **714117**

(54) Title  
**A catheter having a gear-shaped lumen to avert the elimination of fluid flow therein**

(51)<sup>6</sup> International Patent Classification(s)  
**A61M 025/14**

(21) Application No: **199712209** (22) Application Date: **1997.01.16**

(30) Priority Data

(31) Number (32) Date (33) Country  
**08/587624 1996.01.17 US**

(43) Publication Date : **1997.07.24**  
(43) Publication Journal Date : **1997.07.24**  
(44) Accepted Journal Date : **1999.12.16**

(71) Applicant(s)  
**Becton Dickinson and Company**

(72) Inventor(s)  
**William Thomas Antoshkiw; Joseph Choon Chee**

(74) Agent/Attorney  
**F.B. RICE and CO.,139 Rathdowne Street,CARLTON VIC 3053**

(56) Related Art  
**US 1596754**  
**US 4840623**



AU9712209

(12) PATENT ABRIDGMENT (11) Document No. AU-B-12209/97  
(19) AUSTRALIAN PATENT OFFICE (10) Acceptance No. 714117

- (54) Title  
A CATHETER HAVING A GEAR-SHAPED LUMEN TO AVERT THE ELIMINATION OF FLUID FLOW THEREIN
- International Patent Classification(s)  
(51)<sup>8</sup> A61M 025/14
- (21) Application No. : 12209/97 (22) Application Date : 16.01.97
- (30) Priority Data
- |             |           |                             |
|-------------|-----------|-----------------------------|
| (31) Number | (32) Date | (33) Country                |
| 08/587624   | 17.01.96  | US UNITED STATES OF AMERICA |
- (43) Publication Date : 24.07.97
- (44) Publication Date of Accepted Application : 16.12.99
- (71) Applicant(s)  
BECTON DICKINSON AND COMPANY
- (72) Inventor(s)  
WILLIAM THOMAS ANTOSHKIW; JOSEPH CHOON CHEE
- (74) Attorney or Agent  
F.B. RICE & CO., 139 Rathdowne Street, CARLTON VIC 3053
- (56) Prior Art Documents  
US 1596754  
US 4840623
- (57) Claim

### Abstract

5

10

15

20

A catheter designed for improved patency characteristics under forces normally exerted upon the catheter during use. The catheter features an inner wall having one or more protuberances running lengthwise in a manner parallel with the central axis of the catheter. The protuberances include a tip, a root defined along the inner wall, and a pair of sidewalls extending between the tip and the root. The roots of adjacent protuberances are spaced from one another. A fluid path is established between the inner wall and the opposed sidewalls of adjacent protuberances. The opposed sidewalls can be straight. Alternately, at least one of the opposed sidewalls includes a non-linear portion along its length. In response to a force normally exerted upon the catheter during use, the spacing between adjacent roots and, if so provided, the non-linear portion of an opposed sidewall prevents the opposed sidewalls from entering into total contact with one another, thereby preventing occlusion of the fluid path. If desired, to strengthen the catheter against occlusion by a medical adapter attached to the proximal end, one or more support elements may be incorporated at the proximal end of the inner wall.

# AUSTRALIA

## Patents Act 1990

BECTON DICKINSON AND COMPANY

ORIGINAL

### COMPLETE SPECIFICATION STANDARD PATENT



*Invention Title:*



*A catheter having a gear-shaped lumen to avert the elimination of  
fluid flow therein*



The following statement is a full description of this invention including the  
best method of performing it known to us:-

(1/1)

5

10

15

**I. Field of the Invention.**

This invention relates to a catheter having improved patency characteristics, and more particularly, to a catheter having a gear shaped lumen to avert the elimination of fluid flow through the catheter when subjected to bending or torsional forces and being adaptable for use with standard medical adapter and delivery instruments and accessories.

20

**II. Background**

In recent years, there has been a marked increase in the use of catheters by physicians conducting various medical procedures and especially surgical procedures. Catheters are typically elongate tubes formed from medical grade plastics made as polyethylene, polyimide, or even nylon, which define fluid carrying ducts for transporting a medicament from a delivery instrument to body tissue. They are typically introduced into the body cavity through the lumen of a needle or introducer device already pierced into the body. Thereafter, the needle or introducer is threadedly removed about the catheter without displacing the catheter from position within the body. One use of a catheter is found in providing continuous regional anesthesia, and is exemplified, for instance, by the use of epidural catheters to deliver anesthesia to the epidural space of a patient. Catheters are also used for analgesic purposes to provide sustained pain relief following a surgical procedure. Here, the catheter is kept in place following the procedure and analgesic medicaments administered intermittently according to the needs of the patient.

25

30

35

40

The nature of uses for the aforementioned catheters dictate that dimensions, materials, and other characteristics be selected so as to promote

their effective use with minimal trauma or intrusive reaction to the patient. For instance, the outside dimensions of the catheter normally are reduced to as small a diameter as possible so as to minimize the intrusive effects of the catheter to body tissue. Attention must be also paid to the type of material employed for constructing the body of the catheter. In general, catheters such as intended for epidural anesthesia can be formed from a stiff material such as nylon or a soft material such as polyurethane. Both types of materials present certain advantages and certain drawbacks. In a study conducted by M. Jöhr, F. A. Hess, S. Balogh and H. Gerber, "The choice of the epidural catheter: stiff or soft?" (Regional Anesthesia, Volume 17, No. 3S, May-June 1992 Supplement), "stiff" versus "soft" catheters were compared against a number of parameters including difficulty of insertion, sufficiency of the block provided by the catheter, blood aspiration problems, and paraesthesia. In general, it was found that a stiffer catheter might be preferred in view of its easier insertion into the body, but that such catheters provided greater instances of complications including paraesthesia and blood aspiration. Similar conclusions were reached by S. Rolbin, E. Hew, and G. Ogilvie in "A comparison of two types of epidural catheters," Can. J. Anaesth. 1987, 34:5 pp.pp. 459-61. The latter mentioned difficulties such as parasthesia often lead practitioners to prefer catheters made from a softer material so as to minimize trauma caused to the body.

Owing to considerations of diameter and material choice, catheters such as epidural catheters often experience patency difficulties during use. Depending on the forces exerted upon the catheter, the fluid carrying duct defined by the catheter can kink or occlude, particularly at points subject to external pressures such as where a catheter is attached to an injection port site (P. de Long and P. Kansen, "A Comparison of Epidural Catheters With or Without Subcutaneous Injection Ports for Treatment of Cancer Pain," Anesth. Analg. 1994, 78: 94-100). The result is the stoppage of fluid flow through the catheter.

For instance, one area of the catheter particularly prone to occlusion difficulties is the proximal end. Here, the catheter is typically secured to a standardized medical connector, such as a Tuohy-Borst adapter, for mating with a medical delivery device such as a syringe. As is well known, the Tuohy-

Borst adapter includes a gasket portion which applies pressure about the circumference of the catheter. The pressure exerted at or near the proximal end can cause the catheter walls to collapse upon themselves so as to constrict if not eliminate flow of the medicament from the medical delivery device through the catheter.

Catheters can also experience patency difficulties depending on torsional or bending forces normally exerted upon the catheter while in use. For instance, any twisting or bending action imparted upon the catheter during insertion into the body of a patient might cause the catheter walls to collapse upon themselves, thereby constricting or eliminating fluid flow through the catheter. Also, where the catheter is employed for analgesic purposes, any motions by the patient may cause the catheter to twist or bend, possibly eliminating fluid flow.

Another concern is the practitioner's ability to discern fluid flow through the catheter. Catheters are typically formed from materials that are translucent. Certain attempts in the prior art have sought to strengthen the catheter against collapse, for instance, by incorporating metallic components such as coil windings along the length of the catheter. The presence of a largely opaque metallic component along the catheter length can impede the practitioner's ready view of fluid flow, lessening the practitioner's ability to quickly discern certain difficulties, such as blood aspiration. In view of the exigencies of the operating environment, the need to provide the patient with as rapid and efficient an epidural block as possible, the time constraints on operating room facilities, and the like, such problems cause major difficulties to both patient and medical personnel and they merit address.

There exists a need, therefore, for a catheter having improved patency characteristics to avert the elimination of fluid flow, which preserves the strength of the catheter as well as the integrity of the catheter in the body, which provides the practitioner with a ready view of the fluids flowing through the catheter, and which in whole addresses the problems experienced by previous approaches.

### SUMMARY OF THE INVENTION

These and other concerns are addressed by a catheter according to the present invention. While the principles of the present invention are described with particular reference to a catheter, it will be readily apparent and fully appreciated by the skilled artisan that the principles herein discussed can be readily applied to any tube or similar device subject to patency difficulties.

In a first aspect, the present invention provides a catheter having patency properties, comprising a tube having a proximal end, a distal end and a length therebetween, said tube defining a fluid path having a central axis, an outer wall and an inner wall, said inner wall having a plurality of protuberances disposed lengthwise on said inner wall in a direction parallel with the central axis of said tube, each of said protuberances having a tip, a root extending along said inner wall, and a pair of straight sidewalls extending between said tip and said root, each of said roots of said plurality of protuberances being spaced a distance from another of said roots of another of said protuberances along said inner wall so that one of said pair of straight sidewalls of said each protuberances faces in opposed relation to one of said sidewalls of another of said protuberances, and wherein in response to a force experienced during normal use of said catheter, said distance between said roots of said plurality of protuberances prevents said opposed straight sidewalls from entering into total contact with one another to prevent occlusion of the fluid path, and wherein at least one of said protuberances further comprises a radiopaque stripe between said outer wall of said tube and said tip of said protuberance.

In a second aspect, the present invention provides a catheter having patency properties, comprising:

a tube having a proximal end, a distal end and a length therebetween, said tube defining a fluid path having a central axis, an outer wall and an inner wall, said inner wall having a plurality of protuberances disposed lengthwise on said inner wall in a direction parallel with the central axis of said tube, each of said protuberances having a flat tip, a root extending along said inner wall, and a pair of sidewalls each having a non-linear shape extending between said tip and said root, each of said roots of said plurality of protuberances being spaced a distance from another of said roots of






another of said protuberances so that one of said sidewalls of said protuberances faces in opposed relation another sidewall of another of each said protuberances, and wherein in response to a force experienced during normal use of said catheter, said non-linear shape of said opposed sidewalls prevents said opposed sidewalls from entering into total contact with one another to prevent occlusion of the fluid path.

In a preferred embodiment, the plurality of protuberances comprises seven protuberances.

In a further preferred embodiment, the catheter further comprises three tubes as support elements disposed adjacent the proximal end of said tube, wherein in response to a force applied to the proximal end of said tube, said plurality of support elements prevent said proximal end of said tube from being crushed so as to avert occlusion of the fluid path at said proximal end.




The catheter may be formed from a variety of materials. Preferably, the material choice is translucent, allowing the practitioner to discern fluid flow through the catheter. One material choice is nylon. Alternatively, a soft material such as polyurethane may be employed.



Throughout this specification the word "comprise", or variations such as "comprises" or "comprising", will be understood to imply the inclusion of a stated element, integer or step, or group of elements, integers or steps, but not the exclusion of any other element, integer or step, or group of elements, integers or steps.

#### **BRIEF DESCRIPTION OF THE DRAWINGS**



The invention will now be described in greater detail by way of reference to the following drawings, wherein:

Fig. 1 depicts a longitudinal view of a catheter according to the present invention;

Fig. 2 is a longitudinal cross-sectional view taken along line 2-2 of Fig. 1;

Fig. 3a depicts one way to form the protuberances, as seen in cross-section along line 3a-3a of Fig. 1;



Fig. 3b depicts a second way to form the protuberances, as seen in cross-section along line 3b-3b of Fig. 1;

Fig. 4 is a view in cross-section of the proximal end of a prior art catheter subject to constriction by an external force;

5 Fig. 5 is a view in cross-section of the proximal end of a catheter in accordance with the present invention, incorporating one or more support elements at the proximal end to avert constriction by an external force;

Fig. 5a illustrates support elements which can be incorporated at the proximal end of the catheter, as seen in cross-section along line 5a-5a of Fig. 1;

10 Fig. 5b illustrates, in cross-section, the protuberances acting to preserve the fluid path as the catheter is subjected to forces normally experienced in use;

Fig. 6 is a view in cross-section of a catheter in accordance with the present invention being introduced into the body of a patient by an introducer such as an epidural needle; and

15 Fig. 7 is a view in cross-section of a catheter in accordance with the present invention, wherein an introducer such as an epidural needle is being withdrawn around the catheter once the catheter is finally located in the body.

#### **DETAILED DESCRIPTION OF THE INVENTION**

20 Turning now to the drawings, wherein like numerals denote like components, an embodiment of a catheter 10 in accordance with the present invention is depicted in Figs. 1 and 2. Catheter 10, which may be extruded in tube-like form from a material such as polyurethane or nylon, includes a proximal end 12, a distal end 14 and a length therebetween. Catheter 10 also includes an outer wall 16, an inner wall 17, and a fluid carrying lumen 19 within the catheter characterized by a central axis "X". One or more depth marks 80 (Fig. 6) can be printed or otherwise provided on outer wall 16 to assist the practitioner in assessing the relative insertion of catheter 10 into the body cavity. As herein depicted, distal end 14 is closed, with one or more sideports 18 provided between the outer and inner walls of the catheter, adjacent the distal end, to allow fluid flow between catheter 10 and a body cavity. In a preferred construction, three sideports 18 are provided, but the skilled artisan will appreciate that catheter 10 can be configured to incorporate any number of

25

30

sideports 18. It will also be realized by the skilled artisan that catheter 10 may be constructed such that distal end 14 is open.

One drawback of certain prior art catheters is their loss of patency owing to occlusion of the fluid duct when torsional or bending forces are applied to the catheter during normal use. A feature of catheter 10 in accordance with the present invention is to incorporate structure which maintains fluid flow through the catheter notwithstanding torsional or bending forces experienced during normal use of the catheter. For instance, as seen in Figs. 2 and 3a, catheter 10 can be constructed such that fluid carrying lumen 19, when viewed in cross-section (Fig. 3a), appears gear-shaped. Catheter 10 features one or more protuberances 20 formed or otherwise provided along inner wall 17. Protuberances 10 are preferably oriented lengthwise along catheter 10 in a manner parallel with central axis "X" of lumen 19. Here, it will be seen that seven protuberances are provided, but the skilled artisan will appreciate that any number of protruberances appropriate to the size and application of the catheter can be provided. Protuberances 20 each emanate from a root 22 located along inner wall 17 and extend to a tip 24. A pair of sidewalls 26 extend between the tip and root of each protuberance 20.

Fluid carrying lumen 19 is characterized by a main fluid channel 29 and one or more fluid paths 28. Both main fluid channel 29 and each of fluid paths 28 extend along the length of catheter 10. As seen in Fig. 3a, lumen 19 includes a major diameter "Z" as measured at inner wall 17. If a circle "C" is drawn connecting each of tips 24, lumen 19 further defines a minor diameter "Y". The area of catheter 10 located within circle "C" establishes main fluid channel 29 of the lumen. Referring again to Fig. 3a, it will be seen that each of roots 22 of adjacent protuberances 20 are spaced from one another by a respective section 23 of inner wall 17. Accordingly, a fluid path 28 is established, outside of the area of circle "C", between inner wall 17 and each pair of opposed sidewalls 26 of the adjacent protuberances. The overall appearance of lumen 19, when viewed in cross-section, is like that of an internal gear.

The configuration of protuberances 20 preserves the patency of catheter 10 should main fluid channel 29 be subject to occlusion by torsional or bending

forces normally experienced during use. Referring to Fig. 5b, if catheter 10 is subjected to torsional or bending forces normally experienced during use, the spacing between roots 22 of the adjacent protuberances prevent opposed sidewalls 26 from entering into total surface contact with one another. Accordingly, fluid path 28 between inner wall 17 and each pair of opposed sidewalls 26 is prevented from total occlusion, thereby permitting fluid flow through catheter 10 even if main fluid channel 29 is occluded by those forces.

Fig. 3a illustrates that sidewalls 26 may be formed substantially straight-sided. Here also, it is illustrated that root 22 is wider than tip 24 of a given protuberance 20. Thus, sidewalls 26 are canted between the tip and the root, such that fluid path 28 is wider when measured at circle "C" than it is when measured at inner wall 17. The canting of sidewalls 26, coupled with the spacing provided between roots 22 of adjacent protuberances, contributes to preventing opposed sidewalls 26 from entering into total surface contact with one another under torsional or bending forces. It will, however, be appreciated by the skilled artisan that, if desired, sidewalls 26 need not be canted; roots 22 and tips 24 can assume the same width, with the spacing between roots 22 of adjacent protuberances acting alone to avoid total surface contact between opposed sidewalls 26.

Fig. 3b illustrates an alternate way to configure lumen 19' in accordance with the present invention. Here, in lieu of straight sidewalls 26, each of protuberances 20' feature sidewalls 26' displaying at least one non-linear portion along the length of the sidewall. In one configuration, such as that illustrated in Fig. 3b, the non-linear portion can encompass forming sidewalls 26' with a curved portion 27'. As before, each of protuberances 20' are spaced from one another by a respective section 23' of inner wall 17'. In this manner, curved portion 27', coupled with the spacing provided between roots 22' of adjacent protuberances, helps prevent total surface contact between opposed sidewalls 26', thereby preserving fluid path 28'. Also, as earlier described, sidewalls 26' can be canted between roots 22' which are wider than tips 24', further contributing to preserving the patency of the catheter.

Many of the features of the catheter 10 can be modified by the user as need or desire dictate. For instance, while Figures 3a and 3b illustrate that

protuberances 20 (20') are evenly spaced along the inner wall, the skilled artisan will appreciate that, if desired, the spacing can be uneven. Also, while the spacing between adjacent protuberances 20 (20') is depicted as sections 23 (23') of the circumferential length of the circular inner wall 17, it will be realized that the catheter can be formed such that sections 23 (23') assume other shapes, whether linear or non-linear. While tips 24(24') are shown as flat, they can assume any shape, such as peaked or rounded, and can either be sharp or blunt, as desired. In addition, while catheter 10 may be extruded from a single material, it will be evident that the catheter can be co-extruded from differing materials. For instance, protuberances 20 (20') may encompass a material differing from the material employed for the rest of catheter 10. Also in this vein, Figures 1, 3a and 3b illustrate that one or more radiopaque stripes 70 can be incorporated into catheter 10 by extruding an appropriate material into the body of the catheter. For instance, the one or more radiopaque stripes 70 can be conveniently extruded in the catheter 10 between outer wall 16 and one or more of tips 24 (24') of the protuberances.

As was earlier described, one area of a catheter particularly prone to occlusion difficulties is the proximal end. This is particularly true if the catheter is formed from a relatively soft material such as polyurethane. As illustrated in Fig. 4, in the prior art, a catheter 30 is subject to a torsional and/or pinching forces "F" exerted by a medical adapter, such as a Tuohy-Borst adapter, which is attached to the proximal end. Forces "F" can constrict fluid-carrying lumen 39 of the prior art catheter, contributing to patency difficulties.

To further enhance the patency characteristics of a catheter in accordance with the present invention, if desired, one or more tube-like support elements 40 can be inserted into surface contact with inner wall 17 of catheter 10 adjacent the proximal end (see Figs. 5 and 5a). The support elements, for example, can be formed from sections of metallic or plastic cannulae, or they can encompass sections of coil windings. The number or placement of support elements 40 at the proximal end of catheter 10 may be selected by the user according to the length of catheter 10 subject to forces "F". Here, it will be seen that three support elements 40 are provided. It will also be realized by the

skilled artisan that support elements 40 can be incorporated about outer wall 16 of catheter 10.

5 Preferably, each of the support elements 40 are spaced from one another by a distance "A". As illustrated in Fig. 6, catheter 10 is normally inserted into a patient's body cavity via a lumen 52 of an introducer such as an epidural needle 50. After the catheter is located within the desired area of the body cavity, it is taped or otherwise held in place against the patient, and the epidural needle is withdrawn from the body, with the catheter passing through lumen 52 ( see Fig. 7). Most epidural needles 50 include curved distal ends 54. By spacing support elements 40 from one another, proximal end 12 of catheter 10 remains flexible, preventing the proximal end from becoming caught within the curved distal end of epidural needle 50 during withdrawal.

10 Thus, it will be seen that the catheter according to the present invention addresses many of the drawbacks exemplified by the prior art approaches. The catheter displays improved patency properties substantially along its entire length, all the while not obscuring the view of the practitioner during use and permitting the catheter to be formed from a relatively soft material and with a closed ended construction so as to minimize traumatic effects to the patient. The construction also contributes to overall strength and integrity of the catheter along its entire length.

15 20 It will be appreciated and understood by those skilled in the art that further and additional forms of the invention may be devised without departing from the spirit and scope of the appended claims, the invention not being limited to the specific embodiments shown.

THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:

1. A catheter having patency properties, including a tube having a proximal end, a distal end and a length therebetween, said tube defining a fluid path having a central axis, an outer wall and an inner wall, said inner wall having a plurality of protuberances disposed lengthwise on said inner wall in a direction parallel with the central axis of said tube, each of said protuberances having a tip, a root extending along said inner wall, and a pair of straight sidewalls extending between said tip and said root, each of said roots of said plurality of protuberances being spaced a distance from another of said roots of another of said protuberances along said inner wall so that one of said pair of straight sidewalls of said each protuberances faces in opposed relation to one of said sidewalls of another of said protuberances, and wherein in response to a force experienced during normal use of said catheter, said distance between said roots of said plurality of protuberances prevents said opposed straight sidewalls from entering into total contact with one another to prevent occlusion of the fluid path, and wherein at least one of said protuberances further includes a radiopaque stripe between said outer wall of said tube and said tip of said protuberance.



2. A catheter having patency properties, including:  
a tube having a proximal end, a distal end and a length therebetween, said tube defining a fluid path having a central axis, an outer wall and an inner wall, said inner wall having a plurality of protuberances disposed lengthwise on said inner wall in a direction parallel with the central axis of said tube, each of said protuberances having a flat tip, a root extending along said inner wall, and a pair of sidewalls each having a non-linear shape extending between said tip and said root, each of said roots of said plurality of protuberances being spaced a distance from another of said roots of another of said protuberances so that one of said sidewalls of said protuberances faces in opposed relation another sidewall of another of each said protuberances, and wherein in response to a force experienced during normal use of said catheter, said non-linear shape of said opposed sidewalls prevents said opposed sidewalls from entering into total contact with one another to prevent occlusion of the fluid path.



3. The catheter according to claim 1 or claim 2, wherein said plurality of protuberances comprises seven protuberances.

5 4. The catheter according to claim 1 or claim 2, further including three tubes as support elements disposed adjacent the proximal end of said tube, wherein in response to a force applied to the proximal end of said tube, said plurality of support elements prevent said proximal end of said tube from being crushed so as to avert occlusion of the fluid path at said proximal end.

Dated this thirteenth day of September 1999.

**BECTON DICKINSON AND  
COMPANY**

Patent Attorneys for the Applicant:

F B RICE & CO






15 01 97 1208

1/5

12209/97

FIG-1

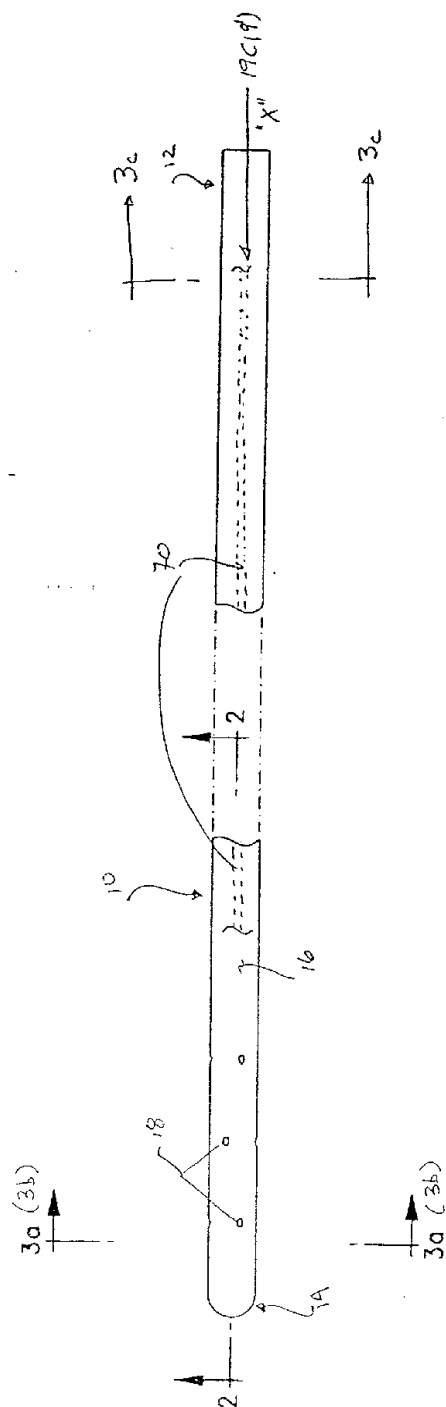

15 01 97 12008

2/5

FIG-2

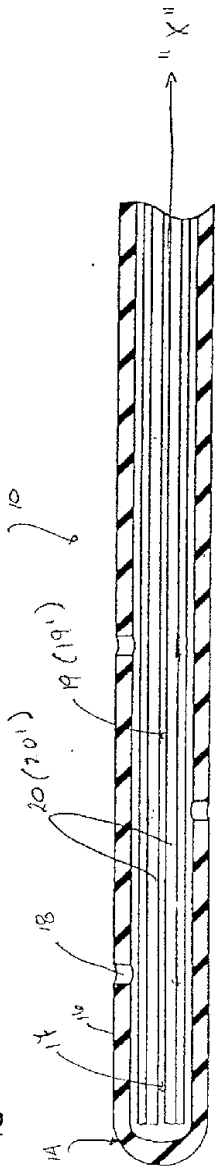


FIG-3a


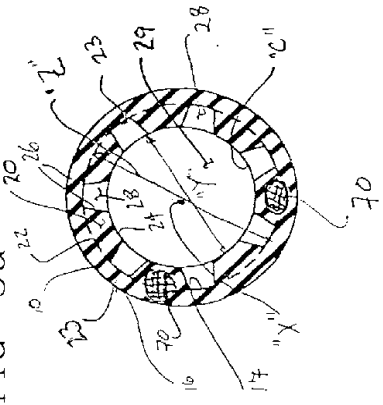


FIG-3b

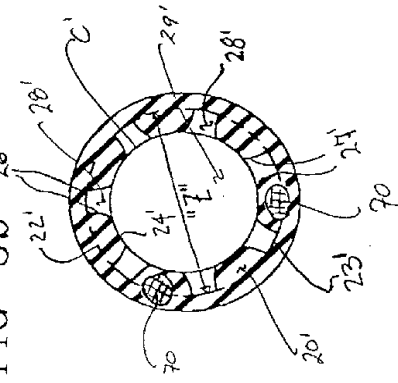

16 01 97 12009

3/5

FIG-4 PRIOR ART


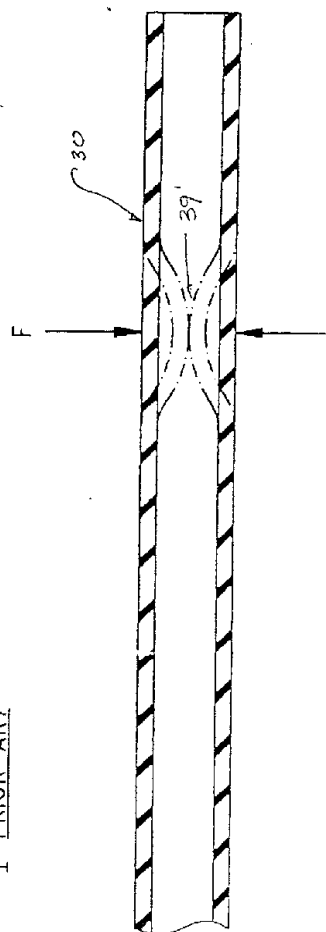


FIG-5

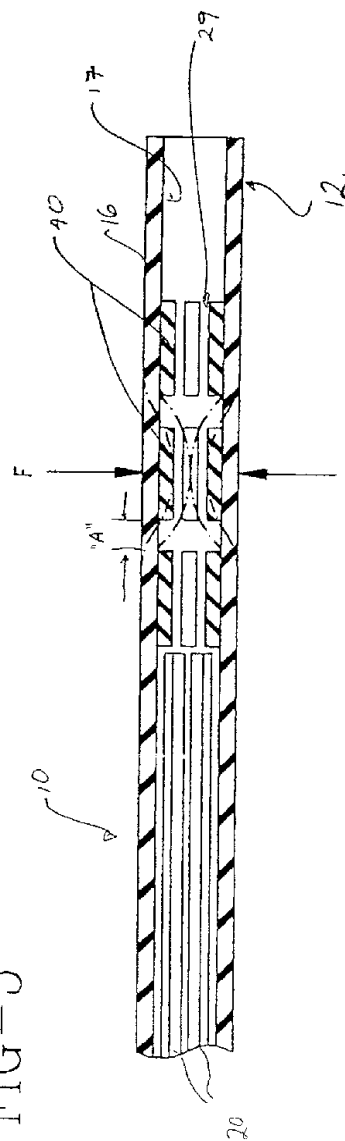

2000  
 2001  
 2002  
 2003  
 2004  
 2005  
 2006  
 2007  
 2008  
 2009  
 2010  
 2011  
 2012  
 2013  
 2014  
 2015  
 2016  
 2017  
 2018  
 2019  
 2020  
 2021  
 2022  
 2023  
 2024  
 2025  
 2026  
 2027  
 2028  
 2029  
 2030  
 2031  
 2032  
 2033  
 2034  
 2035  
 2036  
 2037  
 2038  
 2039  
 2040  
 2041  
 2042  
 2043  
 2044  
 2045  
 2046  
 2047  
 2048  
 2049  
 2050  
 2051  
 2052  
 2053  
 2054  
 2055  
 2056  
 2057  
 2058  
 2059  
 2060  
 2061  
 2062  
 2063  
 2064  
 2065  
 2066  
 2067  
 2068  
 2069  
 2070  
 2071  
 2072  
 2073  
 2074  
 2075  
 2076  
 2077  
 2078  
 2079  
 2080  
 2081  
 2082  
 2083  
 2084  
 2085  
 2086  
 2087  
 2088  
 2089  
 2090  
 2091  
 2092  
 2093  
 2094  
 2095  
 2096  
 2097  
 2098  
 2099  
 2100  
 2101  
 2102  
 2103  
 2104  
 2105  
 2106  
 2107  
 2108  
 2109  
 2110  
 2111  
 2112  
 2113  
 2114  
 2115  
 2116  
 2117  
 2118  
 2119  
 2120  
 2121  
 2122  
 2123  
 2124  
 2125  
 2126  
 2127  
 2128  
 2129  
 2130  
 2131  
 2132  
 2133  
 2134  
 2135  
 2136  
 2137  
 2138  
 2139  
 2140  
 2141  
 2142  
 2143  
 2144  
 2145  
 2146  
 2147  
 2148  
 2149  
 2150  
 2151  
 2152  
 2153  
 2154  
 2155  
 2156  
 2157  
 2158  
 2159  
 2160  
 2161  
 2162  
 2163  
 2164  
 2165  
 2166  
 2167  
 2168  
 2169  
 2170  
 2171  
 2172  
 2173  
 2174  
 2175  
 2176  
 2177  
 2178  
 2179  
 2180  
 2181  
 2182  
 2183  
 2184  
 2185  
 2186  
 2187  
 2188  
 2189  
 2190  
 2191  
 2192  
 2193  
 2194  
 2195  
 2196  
 2197  
 2198  
 2199  
 2200  
 2201  
 2202  
 2203  
 2204  
 2205  
 2206  
 2207  
 2208  
 2209  
 2210  
 2211  
 2212  
 2213  
 2214  
 2215  
 2216  
 2217  
 2218  
 2219  
 2220  
 2221  
 2222  
 2223  
 2224  
 2225  
 2226  
 2227  
 2228  
 2229  
 2230  
 2231  
 2232  
 2233  
 2234  
 2235  
 2236  
 2237  
 2238  
 2239  
 2240  
 2241  
 2242  
 2243  
 2244  
 2245  
 2246  
 2247  
 2248  
 2249  
 2250  
 2251  
 2252  
 2253  
 2254  
 2255  
 2256  
 2257  
 2258  
 2259  
 2260  
 2261  
 2262  
 2263  
 2264  
 2265  
 2266  
 2267  
 2268  
 2269  
 2270  
 2271  
 2272  
 2273  
 2274  
 2275  
 2276  
 2277  
 2278  
 2279  
 2280  
 2281  
 2282  
 2283  
 2284  
 2285  
 2286  
 2287  
 2288  
 2289  
 2290  
 2291  
 2292  
 2293  
 2294  
 2295  
 2296  
 2297  
 2298  
 2299  
 2300  
 2301  
 2302  
 2303  
 2304  
 2305  
 2306  
 2307  
 2308  
 2309  
 2310  
 2311  
 2312  
 2313  
 2314  
 2315  
 2316  
 2317  
 2318  
 2319  
 2320  
 2321  
 2322  
 2323  
 2324  
 2325  
 2326  
 2327  
 2328  
 2329  
 2330  
 2331  
 2332  
 2333  
 2334  
 2335  
 2336  
 2337  
 2338  
 2339  
 2340  
 2341  
 2342  
 2343  
 2344  
 2345  
 2346  
 2347  
 2348  
 2349  
 2350  
 2351  
 2352  
 2353  
 2354  
 2355  
 2356  
 2357  
 2358  
 2359  
 2360  
 2361  
 2362  
 2363  
 2364  
 2365  
 2366  
 2367  
 2368  
 2369  
 2370  
 2371  
 2372  
 2373  
 2374  
 2375  
 2376  
 2377  
 2378  
 2379  
 2380  
 2381  
 2382  
 2383  
 2384  
 2385  
 2386  
 2387  
 2388  
 2389  
 2390  
 2391  
 2392  
 2393  
 2394  
 2395  
 2396  
 2397  
 2398  
 2399  
 2400  
 2401  
 2402  
 2403  
 2404  
 2405  
 2406  
 2407  
 2408  
 2409  
 2410  
 2411  
 2412  
 2413  
 2414  
 2415  
 2416  
 2417  
 2418  
 2419  
 2420  
 2421  
 2422  
 2423  
 2424  
 2425  
 2426  
 2427  
 2428  
 2429  
 2430  
 2431  
 2432  
 2433  
 2434  
 2435  
 2436  
 2437  
 2438  
 2439  
 2440  
 2441  
 2442  
 2443  
 2444  
 2445  
 2446  
 2447  
 2448  
 2449  
 2450  
 2451  
 2452  
 2453  
 2454

FIG-5a


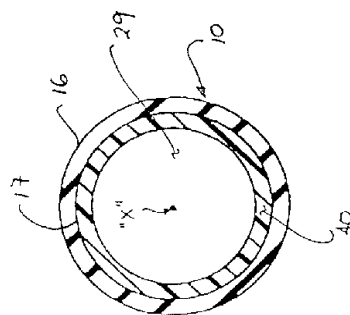


FIG-5b

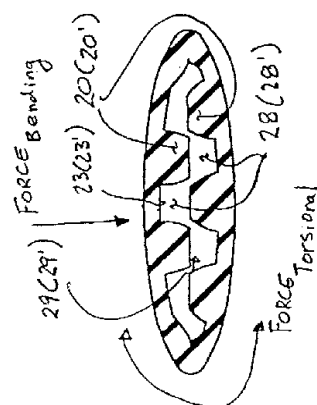

16 01 97 10008

FIG-6

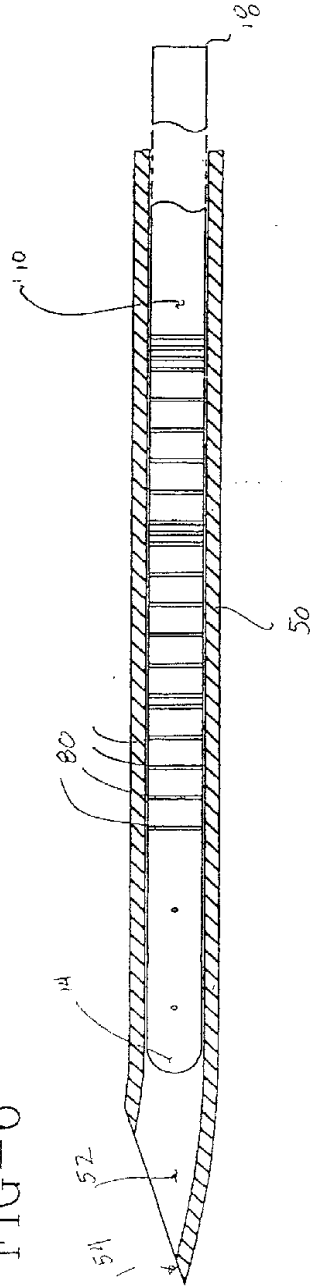


FIG-7

