



US00D932017S

(12) **United States Design Patent**
Lam et al.

(10) **Patent No.:** **US D932,017 S**
(45) **Date of Patent:** **** Sep. 28, 2021**

(54) **MULTI-CONDUCTING LAYER
ELECTROCARDIOGRAM MONITORING
RECORDER**

(71) Applicant: **Quanta Computer Inc.**, Taoyuan (TW)

(72) Inventors: **Barry Lam**, Taoyuan (TW);
Chia-Yuan Chang, Taoyuan (TW);
Jung-Wen Chang, Taoyuan (TW);
Kao-Yu Hsu, Taoyuan (TW)

(73) Assignee: **QUANTA COMPUTER INC.**,
Taoyuan (TW)

(**) Term: **15 Years**

(21) Appl. No.: **29/739,945**

(22) Filed: **Jun. 30, 2020**

(30) **Foreign Application Priority Data**

Mar. 4, 2020 (TW) 109301072

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/167**

(58) **Field of Classification Search**
USPC D24/107, 164–167, 186, 187, 134;
D10/75
CPC . A61B 5/0402; A61B 5/0404; A61B 5/04085;
A61B 5/0416; A61B 5/0432; A61B
5/044; A61B 5/6805; A61B 5/6823; A61B
2560/0412; A61B 2560/0462; A61B 7/02;
A61B 7/04; A61B 7/003; A61B 7/026

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | | |
|--------------|------|---------|-----------|-------|-------------|
| D635,667 | S * | 4/2011 | Soerensen | | D24/134 |
| 9,301,032 | B1 * | 3/2016 | Bello | | A61B 7/003 |
| D865,167 | S * | 10/2019 | Kirgizov | | D24/134 |
| D866,758 | S * | 11/2019 | Chen | | D24/134 |
| D890,347 | S * | 7/2020 | Chang | | D24/167 |
| D890,348 | S * | 7/2020 | Lam | | D24/167 |
| D914,218 | S * | 3/2021 | Govari | | D24/186 |
| 2019/0015004 | A1 * | 1/2019 | Maurizi | | A61B 5/332 |
| 2020/0069203 | A1 * | 3/2020 | Chang | | A61B 5/30 |
| 2020/0289083 | A1 * | 9/2020 | Ogawa | | A61B 7/02 |
| 2020/0352510 | A1 * | 11/2020 | Dhillon | | A61B 5/1491 |

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — McClure, Qualey & Rodack, LLP


(57) **CLAIM**

The ornamental design for a multi-conducting layer electrocardiogram monitoring recorder, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a multi-conducting layer electrocardiogram monitoring recorder showing our new design;
FIG. 2 is a front view thereof;
FIG. 3 is a rear view thereof;
FIG. 4 is a left side view thereof;
FIG. 5 is a right side view thereof;
FIG. 6 is a top plan view thereof;
FIG. 7 is a bottom plan view thereof; and,
FIG. 8 is a bottom perspective view thereof.

1 Claim, 8 Drawing Sheets

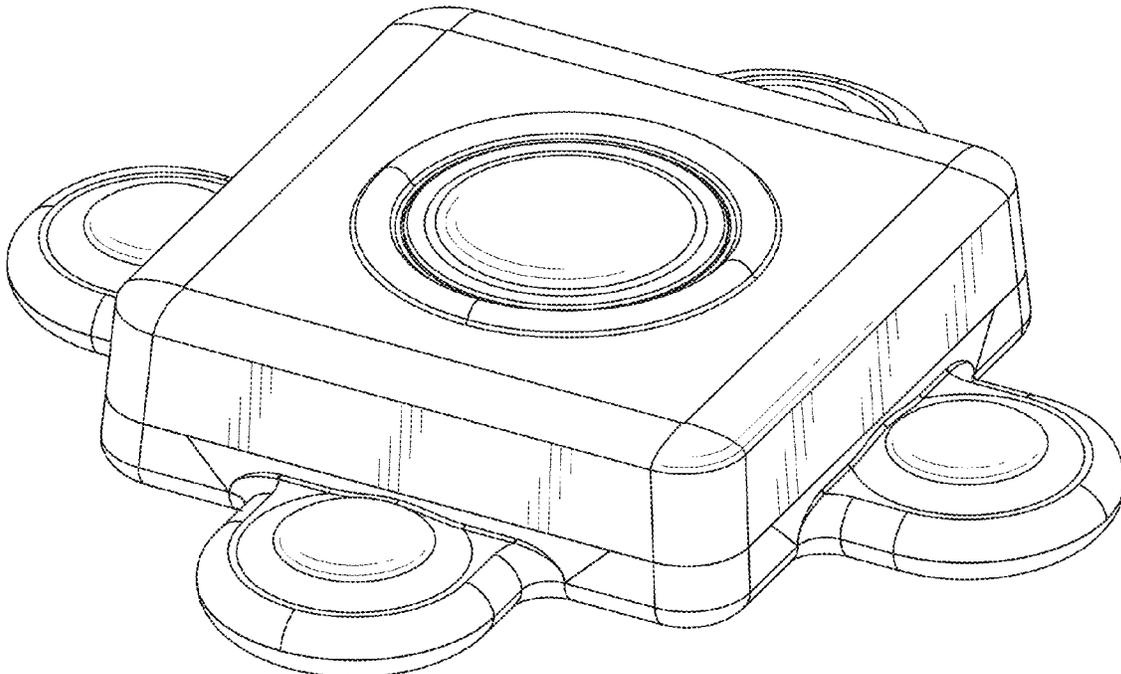

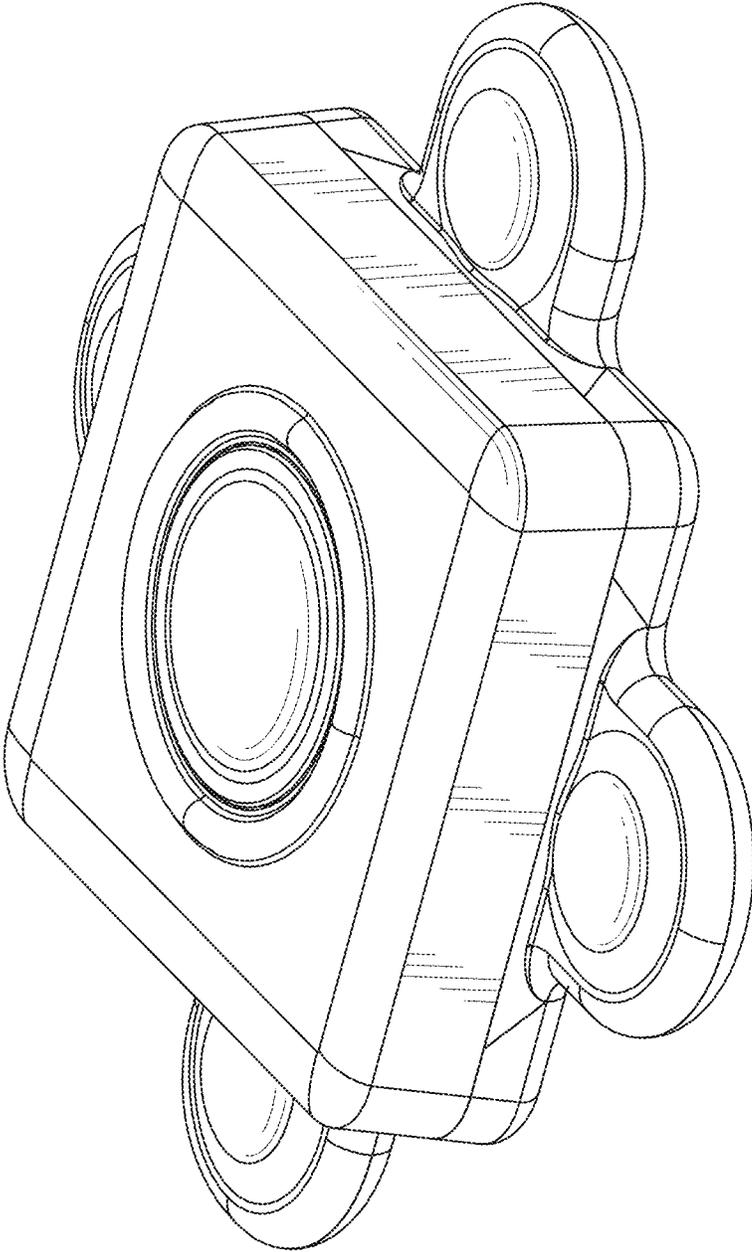


FIG. 1

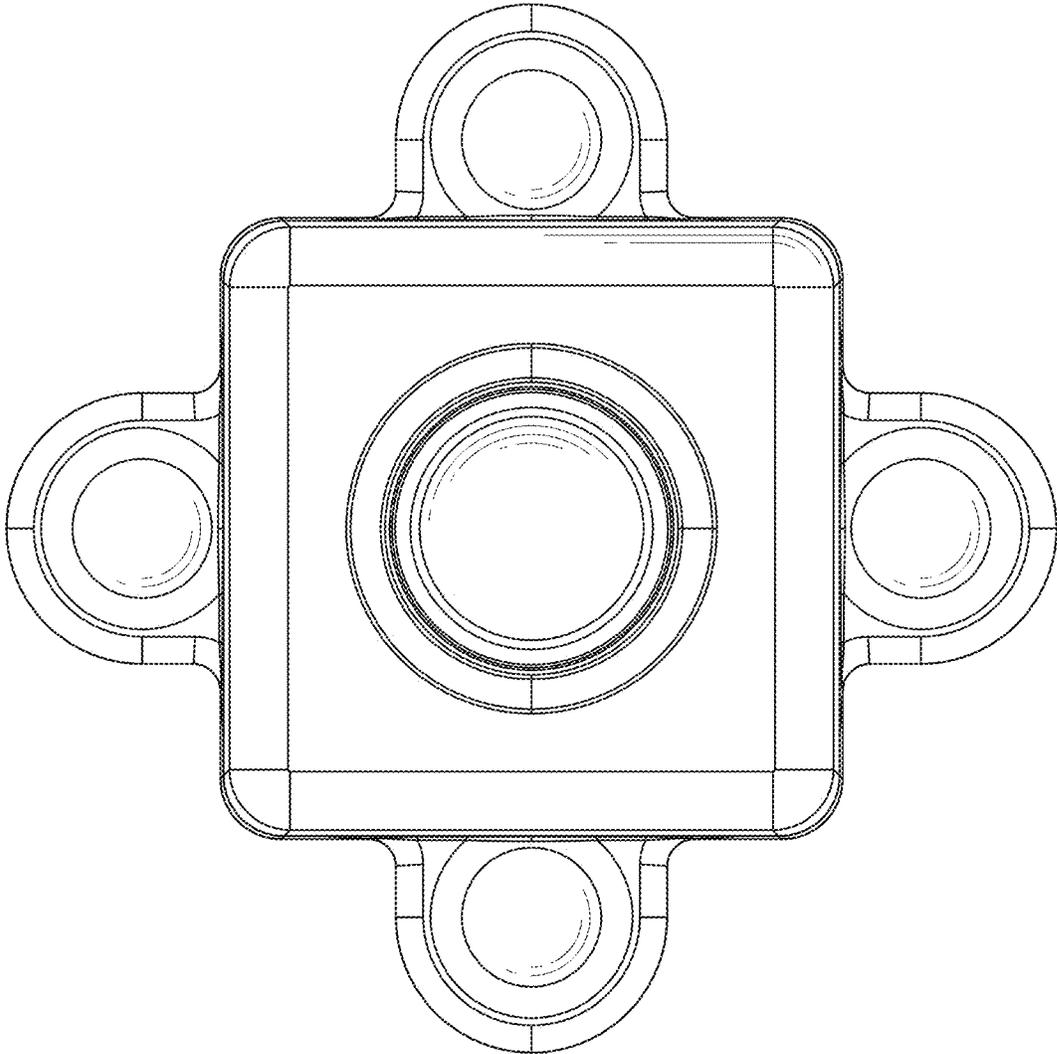


FIG. 2

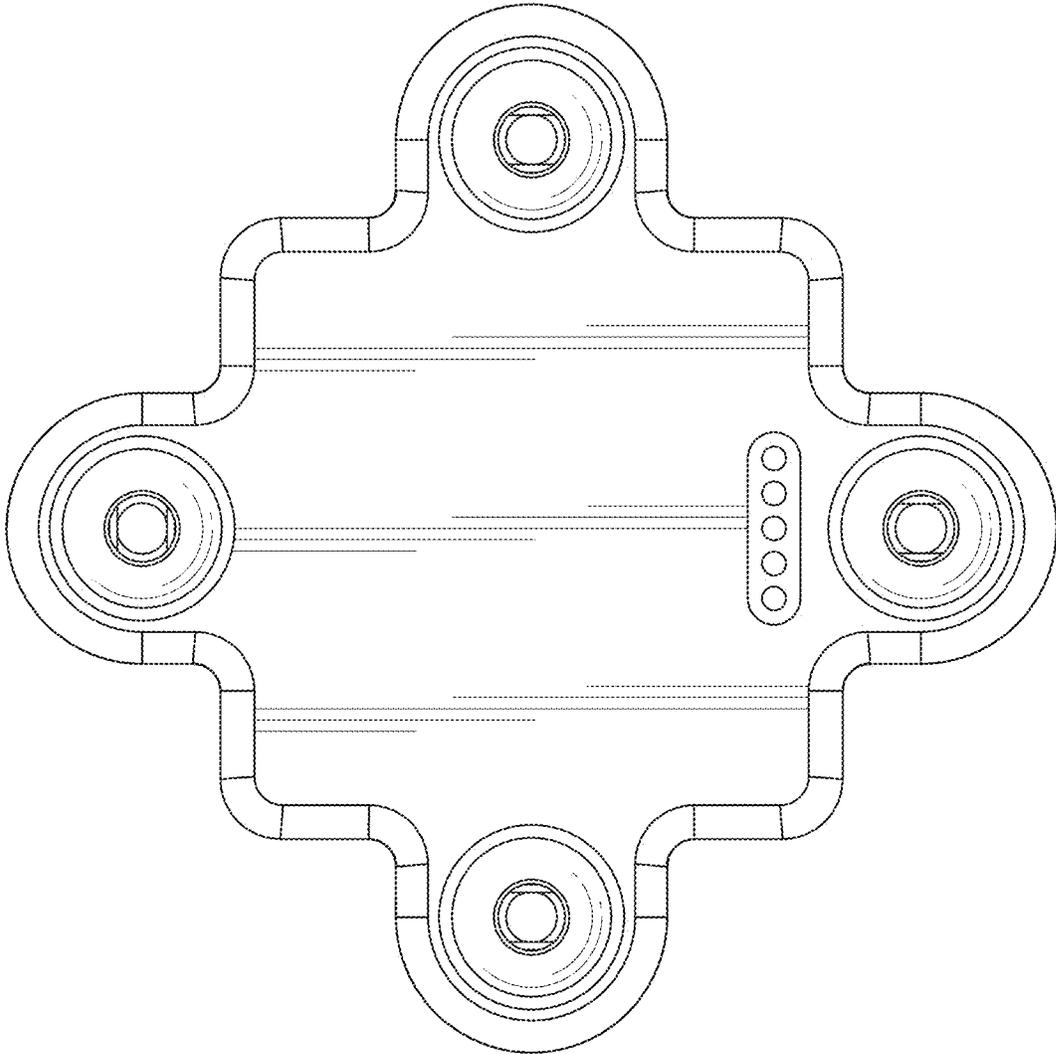


FIG. 3

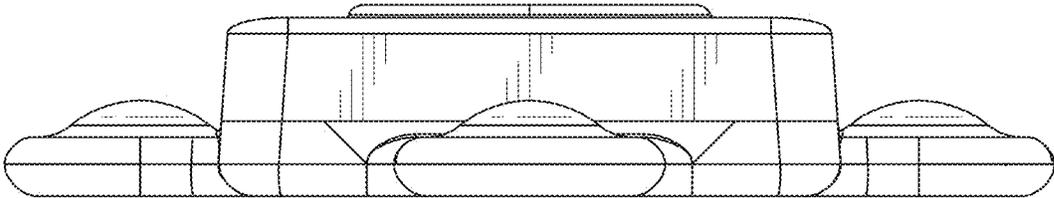


FIG. 4

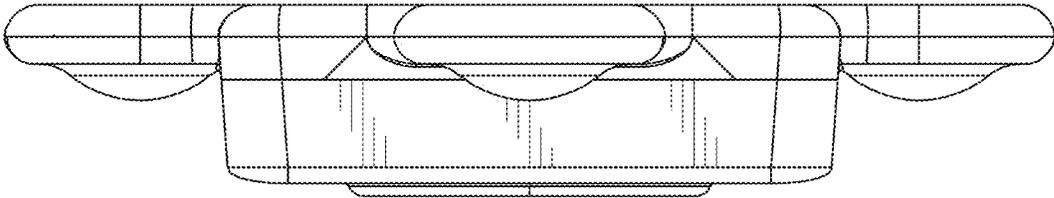


FIG. 5

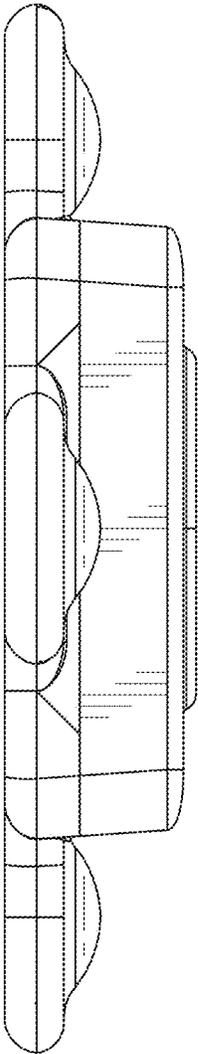


FIG. 6

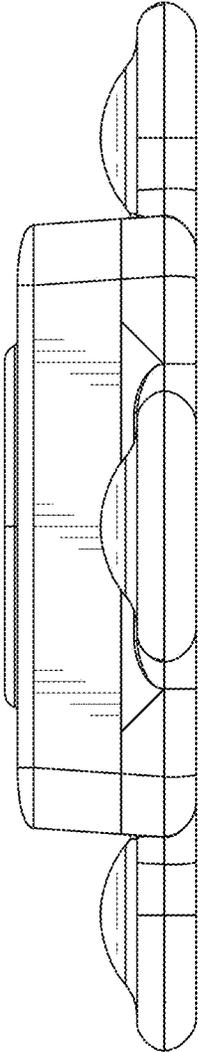


FIG. 7

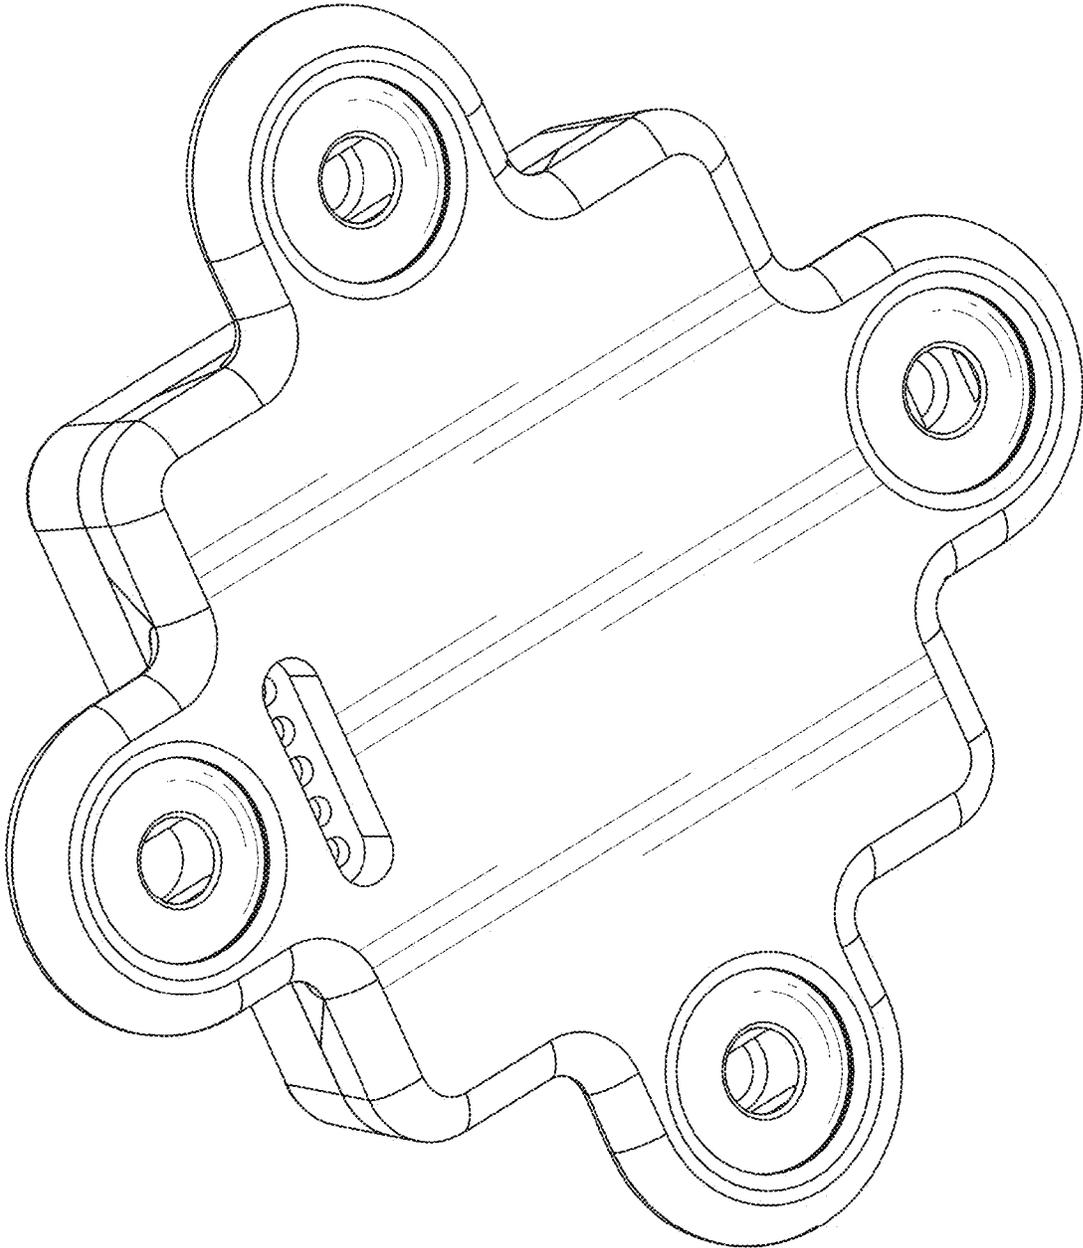


FIG. 8