



US009061156B2

(12) **United States Patent**
Ding et al.

(10) **Patent No.:** **US 9,061,156 B2**
(45) **Date of Patent:** ***Jun. 23, 2015**

(54) **AUTOMATIC SELECTION OF STIMULATION CHAMBER FOR VENTRICULAR RESYNCHRONIZATION THERAPY**

USPC 607/9, 30
See application file for complete search history.

(71) Applicant: **Cardiac Pacemakers, Inc.**, St. Paul, MN (US)

(56) **References Cited**

(72) Inventors: **Jiang Ding**, Shoreview, MN (US); **Julio C. Spinelli**, Lakewood Ranch, FL (US); **Yinghong Yu**, Shoreview, MN (US); **Andrew P. Kramer**, Marine on St. Croix, MN (US)

U.S. PATENT DOCUMENTS

4,712,179 A 12/1987 Heimer
4,809,697 A 3/1989 Causey, III et al.

(Continued)

(73) Assignee: **Cardiac Pacemakers, Inc.**, St. Paul, MN (US)

FOREIGN PATENT DOCUMENTS

WO WO-0041765 7/2000
WO WO-0041766 A1 7/2000

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

OTHER PUBLICATIONS

"U.S. Appl. No. 09/738,407, Final Office Action mailed Jan. 14, 2003", 6 pgs.

This patent is subject to a terminal disclaimer.

(Continued)

(21) Appl. No.: **14/333,674**

Primary Examiner — Amanda Patton

(22) Filed: **Jul. 17, 2014**

(74) *Attorney, Agent, or Firm* — Schwegman Lundberg & Woessner, P.A.

(65) **Prior Publication Data**

US 2014/0330330 A1 Nov. 6, 2014

Related U.S. Application Data

(63) Continuation of application No. 12/480,485, filed on Jun. 8, 2009, now Pat. No. 8,818,511, which is a

(Continued)

(51) **Int. Cl.**

A61N 1/36 (2006.01)

A61N 1/365 (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC *A61N 1/36592* (2013.01); *A61B 5/0472* (2013.01); *A61N 1/3627* (2013.01); *A61N 1/3684* (2013.01)


(58) **Field of Classification Search**

CPC A61N 1/36592; A61N 1/3627; A61N 1/3684; A61B 5/0472

(57) **ABSTRACT**

A method and apparatus for selection of one or more ventricular chambers to stimulate for ventricular resynchronization therapy. Intrinsic intracardia electrograms that include QRS complexes, are recorded from a left and right ventricle. A timing relationship between the intrinsic intracardia electrograms recorded from the left and right ventricle is then determined. In one embodiment, the timing relationship is determined using a delay between a left ventricular and a right ventricular sensed intrinsic ventricular depolarizations and a duration interval of one or more QRS complexes. In one embodiment, the duration of QRS complexes is determined from either intracardiac electrograms or from surface ECG recordings. One or more ventricular chambers in which to provide pacing pulses are then selected based on the timing relationship between intrinsic intracardia electrograms recorded from the right and left ventricle, and the duration of one or more QRS complexes.

20 Claims, 6 Drawing Sheets

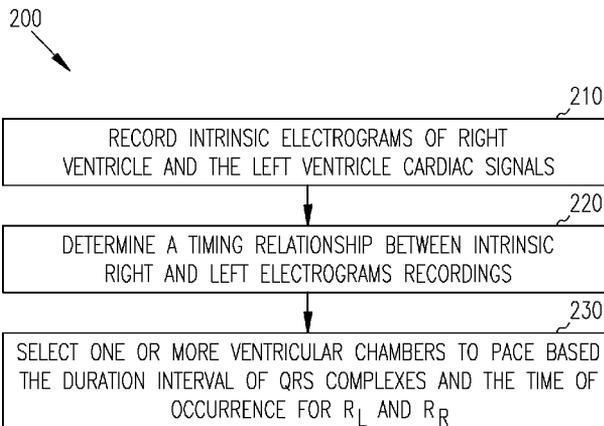

Related U.S. Application Data

continuation of application No. 11/276,007, filed on Feb. 9, 2006, now Pat. No. 7,546,162, which is a continuation of application No. 10/655,569, filed on Sep. 4, 2003, now Pat. No. 6,999,815, which is a continuation of application No. 09/738,407, filed on Dec. 15, 2000, now Pat. No. 6,622,040.

- (51) **Int. Cl.**
A61B 5/0472 (2006.01)
A61N 1/362 (2006.01)
A61N 1/368 (2006.01)

- (56) **References Cited**

U.S. PATENT DOCUMENTS

4,825,869	A	5/1989	Sasmor et al.
4,928,688	A	5/1990	Mower
5,097,831	A	3/1992	Lekholm
5,174,289	A	12/1992	Cohen
5,226,413	A	7/1993	Bennett et al.
5,251,626	A	10/1993	Nickolls et al.
5,267,560	A	12/1993	Cohen
5,282,838	A	2/1994	Hauser et al.
5,292,341	A	3/1994	Snell
5,321,618	A	6/1994	Gessman
5,372,607	A	12/1994	Stone et al.
5,421,830	A	6/1995	Epstein et al.
5,431,691	A	7/1995	Snell et al.
5,456,952	A	10/1995	Garza et al.
5,487,752	A	1/1996	Salo et al.
5,507,782	A	4/1996	Kieval et al.
5,540,727	A	7/1996	Tockman et al.
5,549,654	A	8/1996	Powell
5,594,638	A	1/1997	Iliff
5,607,460	A	3/1997	Kroll et al.
5,630,835	A	5/1997	Brownlee
5,690,690	A	11/1997	Nappholz et al.
5,693,076	A	12/1997	Kaemmerer
5,697,959	A	12/1997	Poore
5,713,937	A	2/1998	Nappholz et al.
5,716,382	A	2/1998	Snell
5,792,203	A	8/1998	Schroepel
5,800,473	A	9/1998	Faisandier
5,817,137	A	10/1998	Kaemmerer
5,833,623	A	11/1998	Mann et al.
5,891,178	A	4/1999	Mann et al.
5,911,132	A	6/1999	Sloane et al.
6,016,442	A	1/2000	Hsu et al.
6,070,101	A	5/2000	Struble et al.
6,091,990	A	7/2000	Hsu et al.
6,129,744	A	10/2000	Boute
6,141,586	A	10/2000	Mower
6,148,234	A	11/2000	Struble
6,168,563	B1	1/2001	Brown
6,249,705	B1	6/2001	Snell
6,272,377	B1	8/2001	Sweeney et al.
6,280,389	B1	8/2001	Ding et al.
6,285,907	B1	9/2001	Kramer et al.
6,304,773	B1	10/2001	Taylor et al.
6,351,675	B1	2/2002	Tholen et al.
6,370,427	B1	4/2002	Alt et al.
6,400,982	B2	6/2002	Sweeney et al.
6,411,847	B1	6/2002	Mower
6,442,432	B2	8/2002	Lee
6,442,433	B1	8/2002	Linberg
6,497,655	B1	12/2002	Linberg et al.
6,526,313	B2	2/2003	Sweeney et al.
RE38,119	E	5/2003	Mower
6,564,104	B2	5/2003	Nelson et al.
6,622,040	B2	9/2003	Ding et al.
6,668,194	B2	12/2003	VanHout
6,669,631	B2	12/2003	Norris et al.
6,999,815	B2	2/2006	Ding et al.
7,070,562	B2	7/2006	Bardy

7,136,707	B2	11/2006	Hall et al.
7,181,285	B2	2/2007	Lindh et al.
7,383,088	B2	6/2008	Spinelli et al.
7,546,162	B2	6/2009	Ding et al.
2001/0031997	A1	10/2001	Lee
2001/0039375	A1	11/2001	Lee et al.
2001/0039503	A1	11/2001	Chan et al.
2002/0016550	A1	2/2002	Sweeney et al.
2002/0120311	A1	8/2002	Lindh et al.
2002/0123672	A1	9/2002	Christophersom et al.
2003/0050803	A1	3/2003	Marchosky
2003/0088290	A1	5/2003	Spinelli et al.
2004/0122487	A1	6/2004	Hatlestad et al.
2004/0133080	A1	7/2004	Mazar
2004/0133246	A1	7/2004	Ding et al.
2004/0143304	A1	7/2004	Hall et al.
2006/0116727	A1	6/2006	Ding et al.
2007/0250125	A1	10/2007	Lindh et al.
2008/0077031	A1	3/2008	Spinelli et al.

OTHER PUBLICATIONS

“U.S. Appl. No. 09/738,407, Non-Final Office Action mailed Aug. 23, 2002”, 6 pgs.
 “U.S. Appl. No. 09/738,407, Notice of Allowance mailed Apr. 7, 2003”, 7 pgs.
 “U.S. Appl. No. 09/738,407, Response filed Mar. 13, 2003 to Final Office Action mailed Jan. 14, 2003”, 10 pgs.
 “U.S. Appl. No. 09/738,407, Response filed Nov. 22, 2002 to Non-Final Office Action mailed Aug. 23, 2002”, 7 pgs.
 “U.S. Appl. No. 09/748,791, Advisory Action mailed Aug. 4, 2004”, 3 pgs.
 “U.S. Appl. No. 09/748,791, Final Office Action mailed Mar. 9, 2004”, 6 pgs.
 “U.S. Appl. No. 09/748,791, Final Office Action mailed Aug. 23, 2005”, 6 pgs.
 “U.S. Appl. No. 09/748,791, Non-Final Office Action mailed Feb. 3, 2005”, 6 pgs.
 “U.S. Appl. No. 09/748,791, Non-Final Office Action mailed Feb. 10, 2006”, 9 pgs.
 “U.S. Appl. No. 09/748,791, Non-Final Office Action mailed Feb. 21, 2003”, 9 pgs.
 “U.S. Appl. No. 09/748,791, Non-Final Office Action mailed Aug. 28, 2002”, 7 pgs.
 “U.S. Appl. No. 09/748,791, Non-Final Office Action mailed Sep. 17, 2003”, 8 pgs.
 “U.S. Appl. No. 09/748,791, Notice of Allowance mailed Sep. 3, 2004”, 7 pgs.
 “U.S. Appl. No. 09/748,791, Notice of Allowance mailed Sep. 20, 2006”, 5 pgs.
 “U.S. Appl. No. 09/748,791, Preliminary Amendment filed Feb. 21, 2001”, 2 pgs.
 “U.S. Appl. No. 09/748,791, Response filed May 10, 2006 to Non-Final Office Action mailed Feb. 10, 2006”, 8 pgs.
 “U.S. Appl. No. 09/748,791, Response filed Jul. 5, 2005 to Non-Final Office Action mailed Feb. 3, 2005”, 7 pgs.
 “U.S. Appl. No. 09/748,791, Response filed Jul. 9, 2004 to Final Office Action mailed Mar. 9, 2004”, 11 pgs.
 “U.S. Appl. No. 09/748,791, Response filed Jul. 21, 2003 to Non-Final Office Action mailed Feb. 21, 2003”, 15 pgs.
 “U.S. Appl. No. 09/748,791, Response filed Nov. 23, 2005 to Final Office Action mailed Aug. 23, 2005”, 7 pgs.
 “U.S. Appl. No. 09/748,791, Response filed Nov. 25, 2002 to Non-Final Office Action mailed Aug. 28, 2002”, 7 pgs.
 “U.S. Appl. No. 09/748,791, Response filed Dec. 17, 2003 to Non-Final Office Action mailed Sep. 17, 2003”, 10 pgs.
 “U.S. Appl. No. 10/008,354, Final Office Action mailed Jul. 12, 2006”, 7 pgs.
 “U.S. Appl. No. 10/008,354, Final Office Action mailed Jul. 19, 2007”, 8 pgs.
 “U.S. Appl. No. 10/008,354, Non-Final office action mailed Jul. 1, 2004”, 5 pgs.
 “U.S. Appl. No. 10/008,354, Non-Final Office Action mailed Apr. 20, 2005”, 8 pgs.

(56)

References Cited

OTHER PUBLICATIONS

"U.S. Appl. No. 10/008,354, Non-Final Office Action mailed Sep. 27, 2006", 7 pgs.
"U.S. Appl. No. 10/008,354, Non-Final Office Action mailed Dec. 19, 2005", 9 pgs.
"U.S. Appl. No. 10/008,354, Notice of Allowance mailed Jan. 23, 2008", 4 pgs.
"U.S. Appl. No. 10/008,354, Notice of Allowance mailed Sep. 28, 2007", 4 pgs.
"U.S. Appl. No. 10/008,354, Response filed Jan. 3, 2005 to Non Final Office Action mailed Jul. 1, 2004", 13 pgs.
"U.S. Appl. No. 10/008,354, Response filed Feb. 27, 2007 to Non Final Office Action mailed Sep. 27, 2006", 17 pgs.
"U.S. Appl. No. 10/008,354, Response filed Mar. 20, 2006 to Non Final Office Action mailed Dec. 19, 2005", 13 pgs.
"U.S. Appl. No. 10/008,354, Response filed Aug. 30, 2005 to Non Final Office Action mailed Apr. 20, 2005", 12 pgs.
"U.S. Appl. No. 10/008,354, Response filed Sep. 12, 2006 to Final Office Action mailed Jul. 12, 2006", 13 pgs.
"U.S. Appl. No. 10/008,354, Response filed Sep. 19, 2007 to Final Office Action mailed Jul. 19, 2007", 15 pgs.
"U.S. Appl. No. 10/655,569, Non-Final Office Action mailed Mar. 28, 2005", 7 pgs.
"U.S. Appl. No. 10/655,569, Notice of Allowance mailed Aug. 25, 2005", 4 pgs.
"U.S. Appl. No. 10/655,569, Response filed Jul. 28, 2005 to Non-Final Office Action mailed Mar. 28, 2005", 8 pgs.
"U.S. Appl. No. 10/655,569, Response to Restriction Requirement filed Mar. 4, 2005", 12 pgs.

"U.S. Appl. No. 10/655,569, Restriction Requirement mailed Feb. 4, 2005", 5 pgs.
"U.S. Appl. No. 11/276,007, Non-Final Office Action mailed Jun. 18, 2008", 10 pgs.
"U.S. Appl. No. 11/276,007, Notice of Allowance mailed Feb. 6, 2009", 5 pgs.
"U.S. Appl. No. 11/276,007, Preliminary Amendment filed Mar. 13, 2006", 3 pgs.
"U.S. Appl. No. 11/276,007, Response filed Oct. 20, 2008 to Non Final Office Action mailed Jun. 18, 2008", 8 pgs.
"U.S. Appl. No. 12/480,485, Final Office Action mailed Jul. 15, 2013", 10 pgs.
"U.S. Appl. No. 12/480,485, Non Final Office Action mailed Nov. 26, 2012", 10 pgs.
"U.S. Appl. No. 12/480,485, Non Final Office Action mailed Dec. 5, 2013", 7 pgs.
"U.S. Appl. No. 12/480,485, Notice of Allowance mailed Apr. 14, 2014", 5 pgs.
"U.S. Appl. No. 12/480,485, Response filed Mar. 4, 2013 to Non Final Office Action mailed Dec. 5, 2013", 6 pgs.
"U.S. Appl. No. 12/480,485, Response filed Mar. 29, 2013 to Non Final Office Action mailed Nov. 26, 2012", 8 pgs.
"U.S. Appl. No. 12/480,485, Response filed Jul. 5, 2012 to Restriction Requirement mailed Jun. 5, 2012", 8 pgs.
"U.S. Appl. No. 12/480,485, Response filed Oct. 15, 2013 to Final Office Action mailed Jul. 15, 2013", 8 pgs.
"U.S. Appl. No. 12/480,485, Restriction Requirement mailed Jun. 5, 2012", 5 pgs.
Mower, Morton, "Method and Apparatus for Treating Hemodynamic Disfunction", U.S. Appl. No. 10/214,474, filed Aug. 8, 2002, entitled, 3 pgs.
US 6,527,714, 03/2003, Bardy (withdrawn)

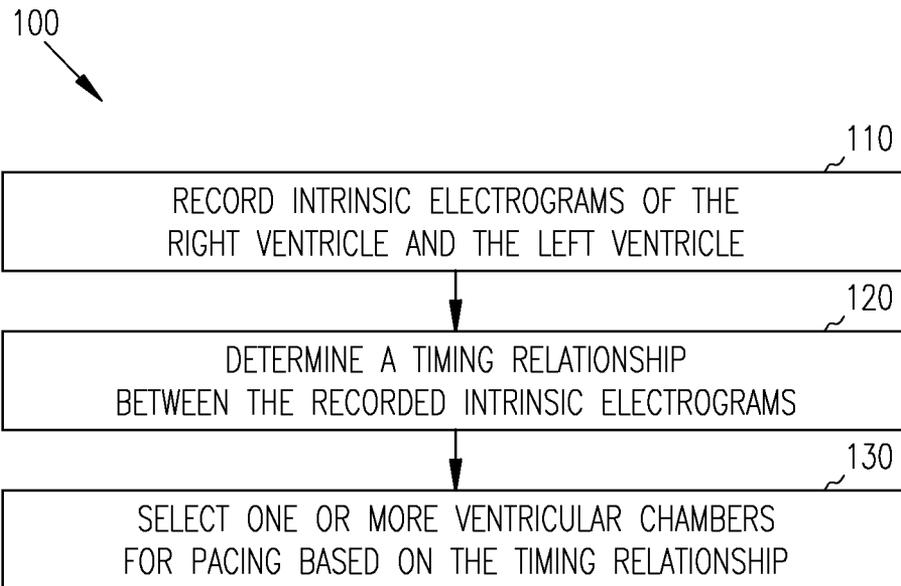


FIG. 1

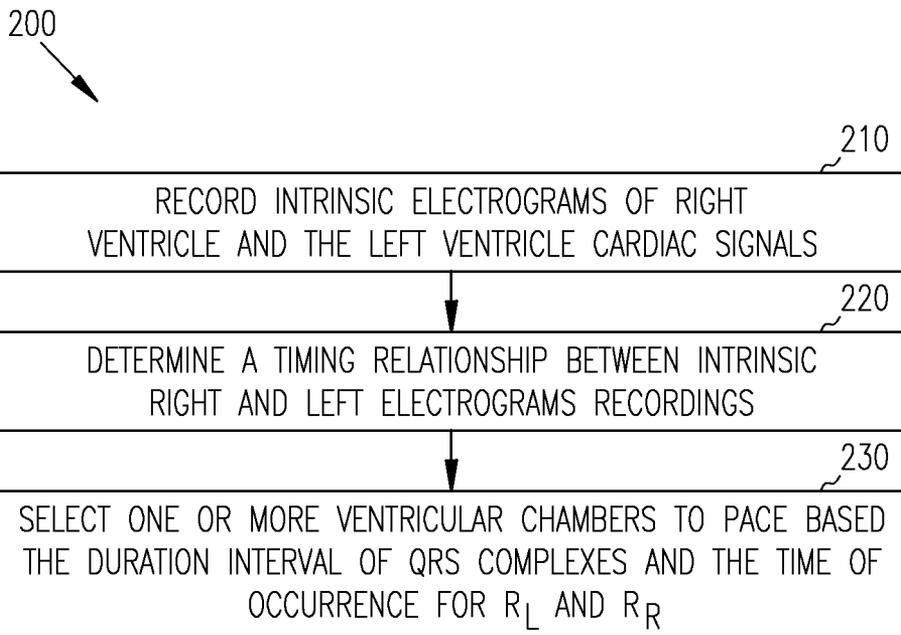


FIG. 2

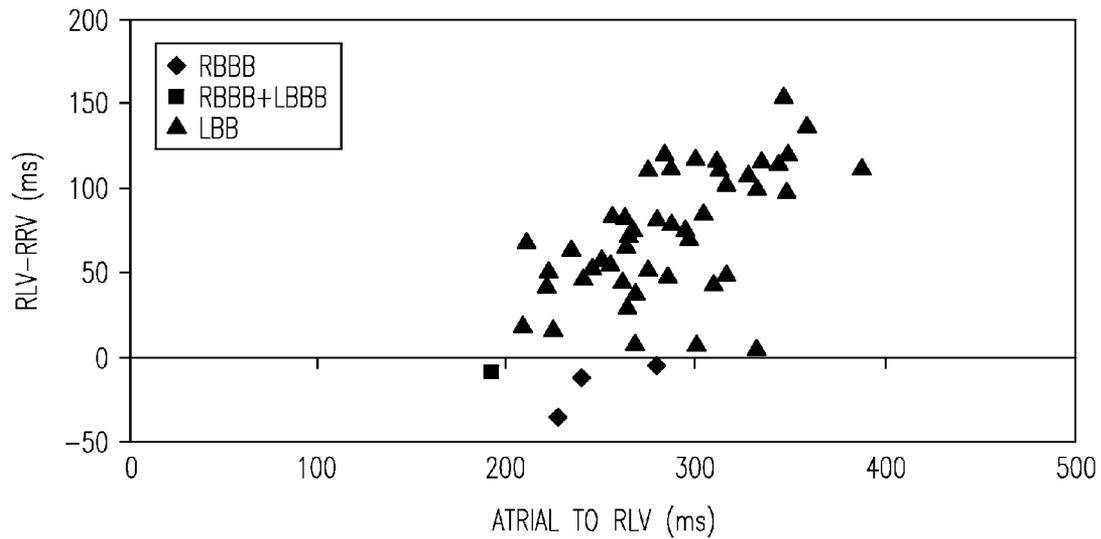


FIG. 3A

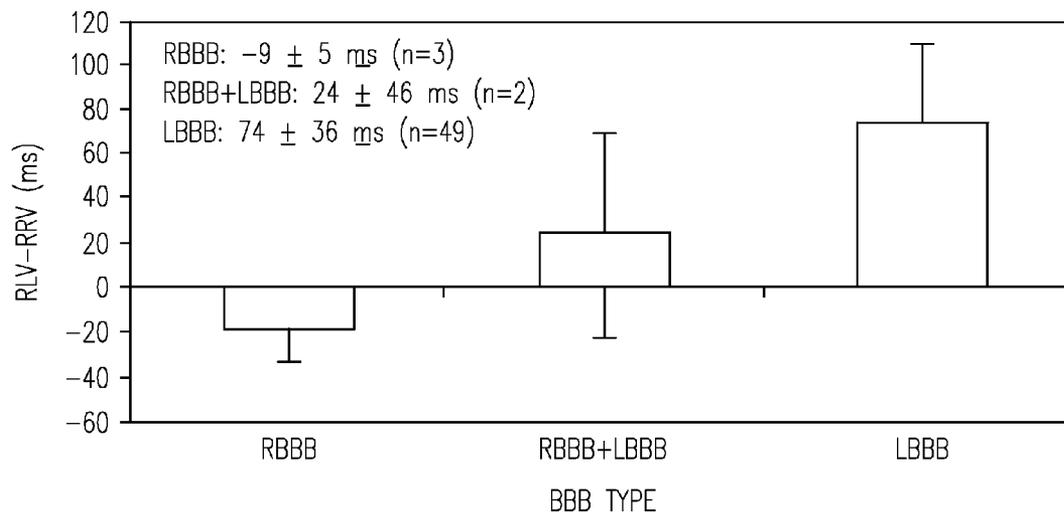


FIG. 3B

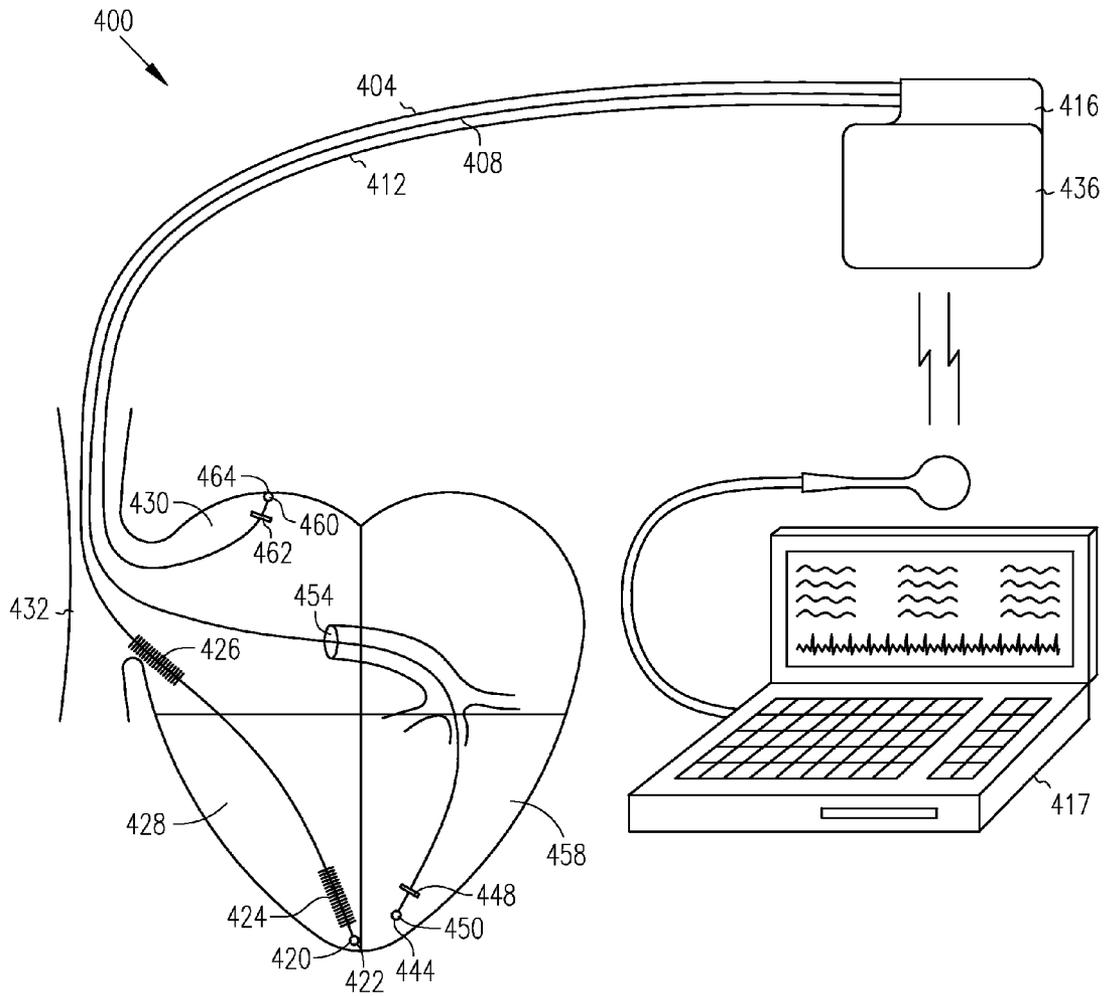


FIG. 4

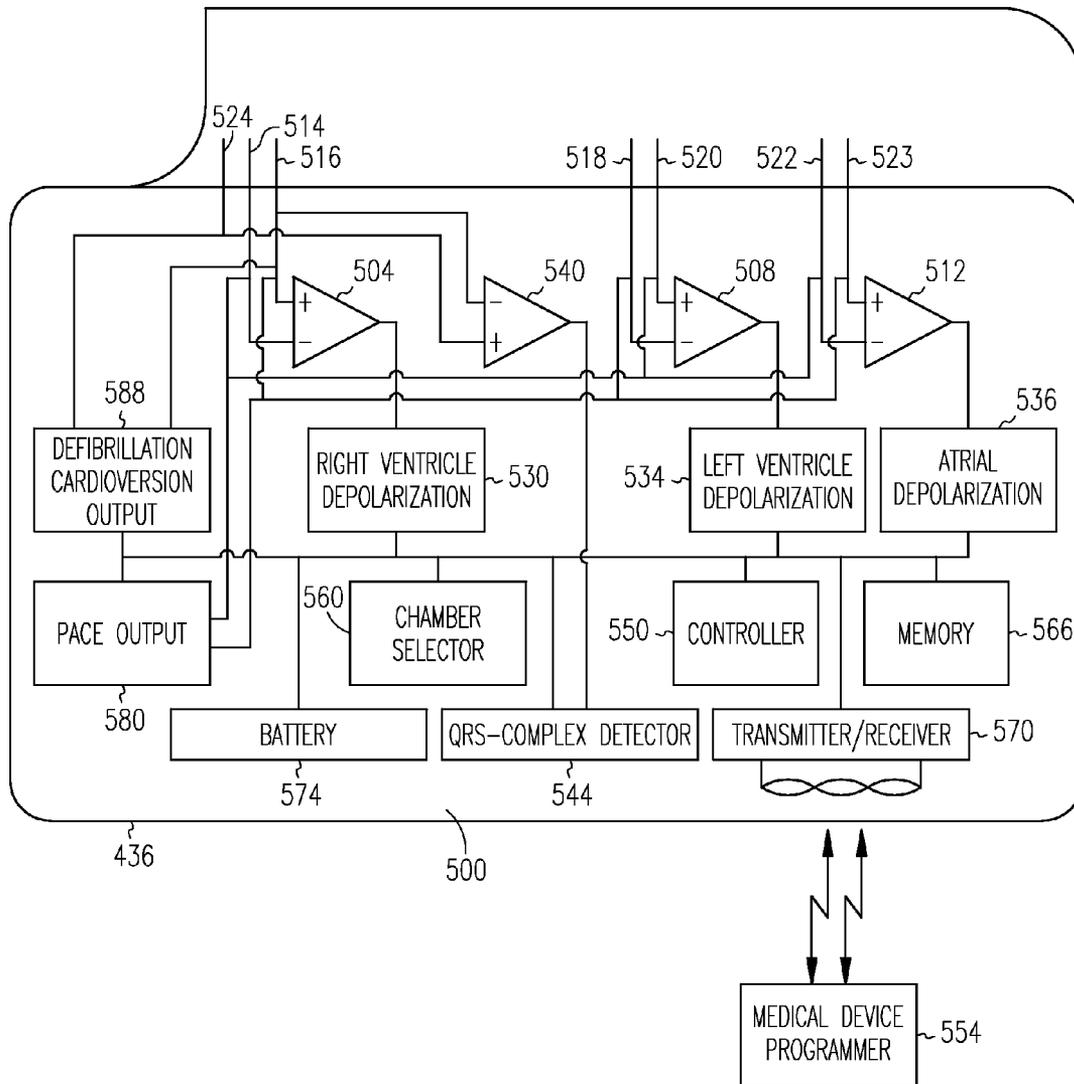


FIG. 5

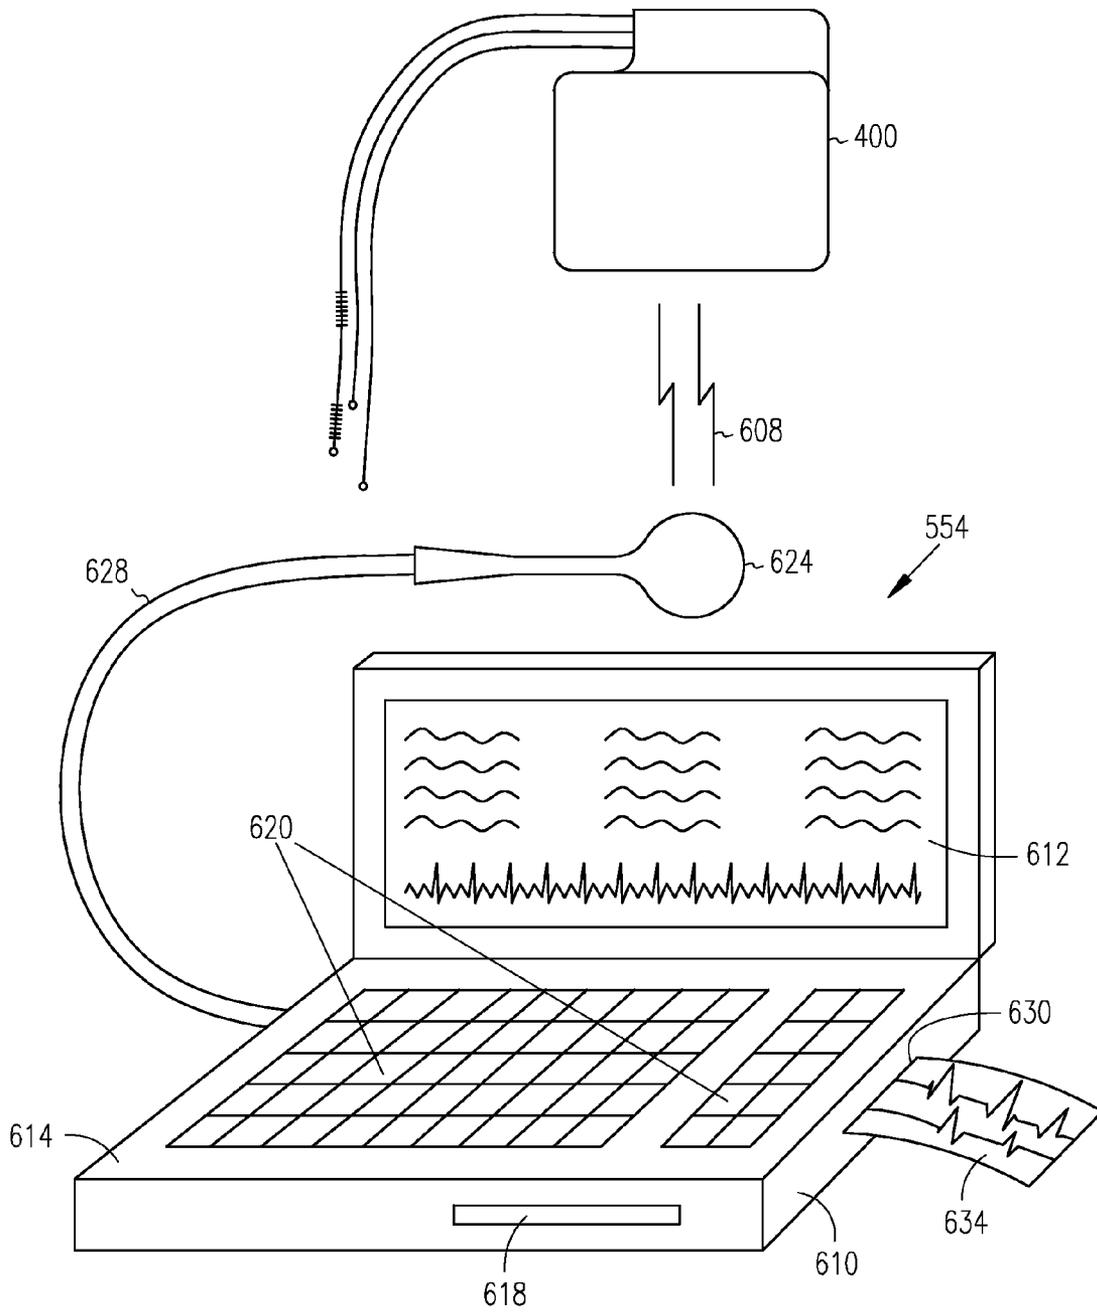


FIG. 6

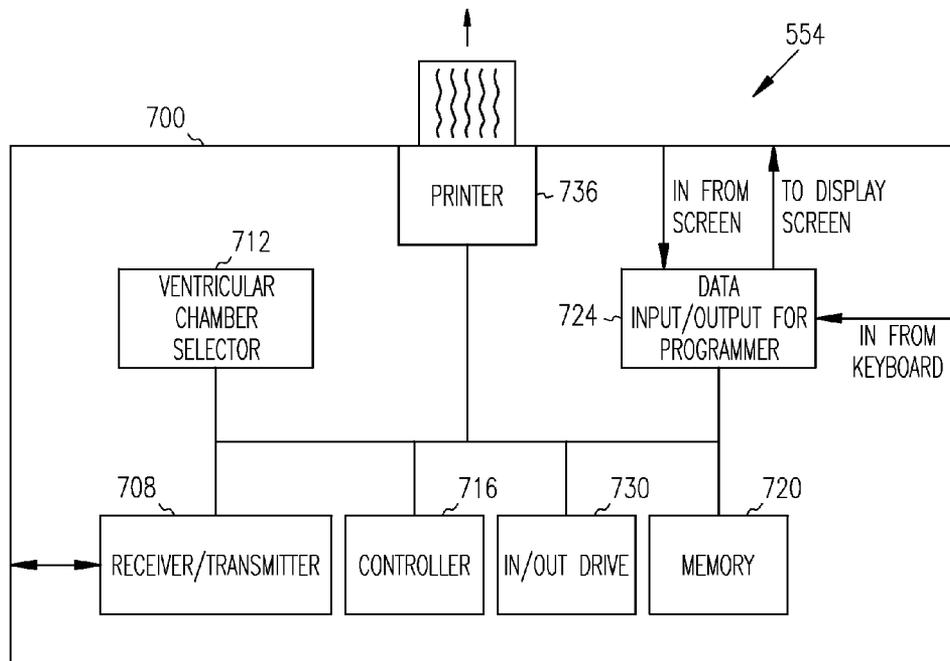


FIG. 7

AUTOMATIC SELECTION OF STIMULATION CHAMBER FOR VENTRICULAR RESYNCHRONIZATION THERAPY

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 12/480,485, filed on Jun. 8, 2009, now issued as U.S. Pat. No. 8,818,511, which is a continuation of U.S. patent application Ser. No. 11/276,007, filed on Feb. 9, 2006, now issued as U.S. Pat. No. 7,546,162, which is a continuation of U.S. patent application Ser. No. 10/655,569, filed on Sep. 4, 2003, now issued as U.S. Pat. No. 6,999,815, which is continuation of U.S. patent application Ser. No. 09/738,407, filed on Dec. 15, 2000, now issued as U.S. Pat. No. 6,622,040, the specifications of which are incorporated herein by reference.

TECHNICAL FIELD

The present invention relates to medical devices and in particular to a medical device for automatically selecting stimulation chamber, or chambers, based on sensed cardiac signals.

BACKGROUND

When functioning properly, the human heart maintains its own intrinsic rhythm, and is capable of pumping adequate blood throughout the body's circulatory system. However, some people have irregular cardiac rhythms, referred to as cardiac arrhythmias. Such arrhythmias result in diminished blood circulation. One mode of treating cardiac arrhythmias uses drug therapy. Drugs are often effective at restoring normal heart rhythms. However, drug therapy is not always effective for treating arrhythmias of certain patients. For such patients, an alternative mode of treatment is needed. One such alternative mode of treatment includes the use of a cardiac rhythm management system. Such systems are often implanted in the patient and deliver therapy to the heart.

Cardiac rhythm management systems include, among other things, pacemakers, also referred to as pacers. Pacers deliver timed sequences of low energy electrical stimuli, called pace pulses, to the heart, such as via an intravascular leadwire or catheter (referred to as a "lead") having one or more electrodes disposed in or about the heart. Heart contractions are initiated in response to such pace pulses (this is referred to as "capturing" the heart). By properly timing the delivery of pace pulses, the heart can be induced to contract in proper rhythm, greatly improving its efficiency as a pump. Pacers are often used to treat patients with bradyarrhythmias, that is, hearts that beat too slowly, or irregularly.

Cardiac rhythm management systems also include cardioverters or defibrillators that are capable of delivering higher energy electrical stimuli to the heart. Defibrillators are often used to treat patients with tachyarrhythmias, that is, hearts that beat too quickly. Such too-fast heart rhythms also cause diminished blood circulation because the heart isn't allowed sufficient time to fill with blood before contracting to expel the blood. Such pumping by the heart is inefficient. A defibrillator is capable of delivering a high energy electrical stimulus that is sometimes referred to as a defibrillation countershock. The countershock interrupts the tachyarrhythmia, allowing the heart to reestablish a normal rhythm for the efficient pumping of blood. In addition to pacers, cardiac rhythm management systems also include, among other things, pacer/

defibrillators that combine the functions of pacers and defibrillators, drug delivery devices, and any other implantable or external systems or devices for diagnosing or treating cardiac arrhythmias.

One problem faced by cardiac rhythm management systems is the treatment of heart failure (also referred to as "HF"). Heart failure, which can result from long-term hypertension, is a condition in which the muscle in the walls of at least one of the right and left sides of the heart deteriorates. By way of example, suppose the muscle in the walls of the left side of the heart deteriorates. As a result, the left atrium and left ventricle become enlarged, and the heart muscle displays less contractility. This decreases cardiac output of blood through the circulatory system which, in turn, may result in an increased heart rate and less resting time between heartbeats. The heart consumes more energy and oxygen, and its condition typically worsens over a period of time.

A deterioration of the heart's conduction system often accompanies heart failure. Normally, intrinsic signals of the heart's conduction system originate in the sinoatrial (SA) node in the upper right atrium. These signals travel through and depolarize the atrial heart tissue to trigger the contraction of the right and left atria. The intrinsic atrial heart signals are received by the atrioventricular (AV) node which, in turn, triggers a subsequent ventricular intrinsic heart signal that travels through the specialized conduction system (Purkinje Fibers) and depolarizes the ventricular heart tissue such that triggered contractions of the right and left ventricles are triggered substantially simultaneously.

In the above example, when the left side of the heart has become enlarged due to heart failure and the conduction system in the left ventricle is blocked, the ventricular intrinsic heart signals may travel through and depolarize the left side of the heart more slowly than in the right side of the heart. This condition is referred to as left bundle branch block (LBBB). As a result, the left and right ventricles do not contract simultaneously, but rather, the left ventricle contracts after the right ventricle. This reduces the pumping efficiency of the heart. Moreover, in the case of LBBB, for example, different regions within the left ventricle may not contract together in a coordinated fashion.

Heart failure can be treated by biventricular (or left-ventricular) coordination therapy that provides pacing pulses to both right and left ventricles. See, e.g., Mower U.S. Pat. No. 4,928,688. Heart failure may also result in an overly long atrioventricular (AV) delay between atrial and ventricular contractions, again reducing the pumping efficiency of the heart. Providing heart failure patients with improved pacing and coordination therapies for improving AV-delay, coordinating ventricular contractions, or otherwise increasing heart pumping efficiency continues to be an area in which improved techniques and therapy protocols are needed.

SUMMARY

The present subject matter provides for improved pacing and coordination therapies for heart failure patients. The present subject matter includes a method and apparatus for recording intrinsic electrograms, including QRS complexes, of left and right ventricles. A timing relationship is then determined between the intrinsic electrograms of the left and the right ventricles. A selection of one or more ventricular chambers in which to provide pacing pulses is then made based on the timing relationship between intrinsic electrograms of the left and the right ventricles.

In one embodiment, determining the timing relationship includes calculating a delay between a left ventricular and a

right ventricular sensed intrinsic ventricular depolarizations and measuring a duration interval of one or more QRS complexes. In one embodiment, intrinsic intracardia electrograms are sensed of the left and right ventricles. The delay is determined by detecting peaks of the sensed intrinsic ventricular depolarizations and calculating the delay between the detected peaks of the intrinsic ventricular depolarizations sensed from the left ventricular and the right ventricles. Additionally, the duration of the QRS complexes are determined from either intracardia electrograms or from surface ECG recordings.

The selection of one or more ventricular chambers then includes selecting one or more ventricular chambers in which to provide pacing pulses based on the duration interval of the QRS complex and the delay between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations. For example, in selecting one or more ventricular chambers, a suggestion to pace in a left ventricle is made when the duration interval of the one or more QRS complexes is greater than or equal to a first threshold value and the difference between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations is greater than a second threshold value. In one embodiment, the first threshold value is 120 millisecond and the second threshold value is zero (0). Alternatively, in selecting one or more ventricular chambers, a suggestion to pace in both the left ventricle and the right ventricle is made when the duration interval of one or more QRS complexes is greater than or equal to the first threshold value and the difference between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations is greater than the second threshold value. Finally, in selecting one or more ventricular chambers, a suggestion to pace in a right ventricle when the duration interval of one or more QRS complexes is greater than or equal to the first threshold value and the difference between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations is less than or equal to the second threshold value. In one embodiment, this suggestion is made through the use of either an implantable pulse generator and/or a medical device programmer.

In one embodiment, the apparatus of the present subject matter includes at least one receiver, where the receiver receives intrinsic intracardia electrograms from the left ventricle and the right ventricle. These electrograms include a left ventricular and a right ventricular sensed intrinsic ventricular depolarizations having QRS complexes. In an additional embodiment, the receiver receives the QRS duration interval of one or more QRS complexes measured from a surface ECG.

The apparatus further includes a controller, where the controller determines a timing relationship between intrinsic electrograms recorded from the left and right ventricle. In one embodiment, the controller calculates a delay between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations and is adapted to receive a duration interval of one or more QRS complexes. In one embodiment, the QRS duration interval is provided to the controller from measurements made from a surface ECG recording. In an alternative embodiment, the controller determines the duration interval of the QRS complexes from the sensed cardiac signals.

The apparatus further includes a ventricular chamber selector. The ventricular chamber selector selects one or more ventricular chambers in which to provide pacing pulses based on the timing relationship between intrinsic intracardia electrograms recorded from the right and left ventricle. In one embodiment, the ventricular chamber selector selects one or

more ventricular chambers in which to provide pacing pulses based on the duration interval of the QRS complexes and the delay between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations, as described above. The apparatus of the present subject matter can be incorporated into a medical device programmer and/or an implantable pulse generator, where the implantable pulse generator includes a first cardiac lead and a second cardiac lead, where the first and second cardiac leads each include electrodes for sensing the intrinsic intracardia electrograms from the left ventricle and the right ventricle.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is one embodiment of a method according to the present subject matter;

FIG. 2 is one embodiment of a method according to the present subject matter;

FIG. 3A shows patient data on a scatter plot of R_{LV} - R_{RV} intervals (ms) vs. Atrial to R_{LV} intervals (ms);

FIG. 3B shows patient data on a bar graph of R_{LV} - R_{RV} intervals (ms) vs. Bundle Branch Block Type;

FIG. 4 is a schematic view of a medical device programmer and an implantable medical device with leads implanted in a heart, where portions of the heart have been removed to show detail, according to one embodiment of the present subject matter;

FIG. 5 is a block diagram of an implantable medical device according to one embodiment of the present subject matter;

FIG. 6 is a perspective view of a medical device programmer and an implantable medical device with leads according to one embodiment of the present subject matter; and

FIG. 7 is a block diagram of a medical device programmer according to one embodiment of the present subject matter.

DETAILED DESCRIPTION

In the following detailed description, reference is made to the accompanying drawings that form a part hereof, and in which is shown by way of illustration specific embodiments in which the invention may be practiced. These embodiments are described in sufficient detail to enable those skilled in the art to practice the invention, and it is to be understood that the embodiments may be combined, or that other embodiments may be utilized and that structural, logical and electrical changes may be made without departing from the spirit and scope of the present invention. The following detailed description is, therefore, not to be taken in a limiting sense, and the scope of the present invention is defined by the appended claims and their equivalents.

The present methods and apparatus will be described in applications involving implantable medical devices for treating heart failure including, but not limited to, implantable pulse generators such as pacemakers, cardioverter/defibrillators, pacer/defibrillators, and biventricular or other multi-site resynchronization devices. However, it is understood that the present methods and apparatus may be employed in unimplanted devices, including, but not limited to, external pacemakers, cardioverter/defibrillators, pacer/defibrillators, biventricular or other multi-site resynchronization devices, monitors, medical device programmers and recorders.

In one embodiment, the present subject matter is implemented in an implantable pulse generator. The implantable pulse generator includes cardiac leads that allow for ventricular cardiac signals to be sensed from left and right ventricular regions of the heart. From information derived from the sensed cardiac signals a selection is made as to which of either

the right, left or both ventricular chambers of the heart is to be paced. In one example, relative delays between intrinsic cardiac depolarizations of the right and left ventricles are used to determine which, or both, ventricular chamber is to be paced. In one embodiment, the ventricle that is activated later (as measured by a later intracardiac lead depolarization) is selected as the stimulation chamber. Since only detection of intracardiac depolarizations are needed, the present subject matter is useful as an automatic site-optimization feature in a ventricular resynchronization therapy device, such as a biventricular stimulation device.

In one embodiment, the suggestion for which ventricular chamber to stimulate (left, right or both) is based on the sensed cardiac conduction between the right and left ventricles of the heart. Different timing relationships between cardiac complexes in the cardiac signals sensed from the right and left ventricular regions can indicate different conduction disorder types. For example, in branch bundle block type disorders regions of the left or right ventricle do not contract together in a coordinated fashion. As a result, the left and right ventricles do not contract simultaneously, but rather, the left ventricle contracts after the right ventricle or vice versa. As a result, the pumping efficiency of the heart is reduced. To increase the pumping efficiency of the heart, identifying and selecting a ventricular pacing location, or locations, that allow for synchronized ventricular contractions would be beneficial to patients with conduction disorder problems. The present subject matter addresses these issues.

FIG. 1 shows one embodiment of a method 100 according to the present subject matter. At 110, intrinsic electrograms of the right ventricle and the left ventricle are recorded. In one embodiment, the electrogram recordings are made from both a right ventricular location and a left ventricular location through the use of electrodes implanted within and/or on the surface of the heart. For example, the electrograms are sensed as unipolar cardiac signals using an implantable pulse generator coupled to one or more cardiac leads implanted in or adjacent the right ventricle and/or left ventricle. In addition, bipolar cardiac signals are sensed from the left and right ventricles so as to allow for ventricular depolarizations to be sensed from around the distal portions of the implanted leads.

At 120, a timing relationship is determined between intrinsic electrograms of the left and right ventricle. In one embodiment, the electrograms include indications of ventricular depolarizations, such as R-waves and/or QRS-complexes that are both indicators of intrinsic ventricular depolarizations. In one embodiment, the timing relationship includes calculating a delay between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations. For example, the delay between left ventricular and the right ventricular sensed intrinsic ventricular depolarizations is taken as the difference between a time of a first ventricular contraction in a first ventricular chamber (e.g., left ventricle or right ventricle) and a time of a second ventricular contraction in a second ventricular chamber (e.g., the right ventricle when the first chamber is the left ventricle and the left ventricle when the first chamber is the right ventricle), where the two ventricular contractions are part of the same cardiac contraction and both contribute to one cardiac cycle of the heart.

Determining the timing relationship also includes measuring a duration interval of one or more QRS complexes. Measuring the duration interval of QRS complexes is accomplished in any number of ways. For example, the duration interval of the QRS complexes is measured manually from a printout of a surface ECG measurement. Alternatively, the duration interval of the QRS complexes is measured electronically from the sensed and recorded cardiac electrograms.

At 130, one or more ventricular chambers in which to provide pacing pulses are then selected based on the timing relationship between intrinsic electrograms of the right and the left ventricles. In one embodiment, the selection at 130 is based on the duration interval of the QRS complex and a calculated delay between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations.

FIG. 2 shows an additional embodiment of a method 200 according to the present subject matter. At 210, intrinsic intracardia electrograms of right ventricular and left ventricular cardiac signals are recorded. In one embodiment, the right and left ventricular cardiac signals are sensed as unipolar cardiac signals using an implantable pulse generator coupled to one or more cardiac leads implanted in or adjacent the right ventricle and/or left ventricle. In one embodiment, a first cardiac signal is sensed from a right ventricular region and a second cardiac signal is sensed from a left ventricular region. In one embodiment, the first cardiac signal is sensed from an apex of the right ventricle, while the second cardiac signal is sensed from a left ventricular free wall. Alternatively, the second cardiac signal is sensed from electrodes implanted transvenously through the coronary sinus so as to position the electrodes adjacent the left ventricle. In an additional embodiment, the electrograms are sensed through the use of a surface 12-lead ECG measurement or a PRM surface ECG system.

At 220, the timing relationship is determined between intrinsic right and left electrograms recordings. In one embodiment, a portion of the timing relationship is determined by calculating a delay between a first ventricular chamber (e.g., left ventricle or right ventricle) and a time of a second ventricular contraction in a second ventricular chamber (e.g., the right ventricle when the first chamber is the left ventricle and the left ventricle when the first chamber is the right ventricle), where the two ventricular contractions are part of the same cardiac contraction and both contribute to one cardiac cycle of the heart. For example, cardiac depolarizations are detected in each of the right and left cardiac signals. In one embodiment, the cardiac depolarizations include R-waves, which are indications of ventricular contractions. The time at which the ventricular contractions occurred is then recorded, where R_L is designated as the time at which the depolarization in the left ventricle occurred and R_R is designated as the time at which the depolarization in the right ventricle occurred. In one embodiment, the time the R-wave occurred is taken as the peak (i.e., the point of maximum deflection during depolarization) of the sensed intrinsic ventricular depolarizations (e.g., the R-waves). The delay between the ventricular chambers is then calculated by taking the difference between the detected peaks of the intrinsic ventricular depolarizations sensed from the left ventricle and the right ventricle (i.e., the difference between R_L and R_R). The difference between R_L and R_R is then used in determining which, or both, ventricular chamber should be paced.

The timing relationship also includes measuring a duration interval of one or more QRS complexes. Measuring the duration interval of QRS complexes is accomplished in any number of ways. For example, the QRS complex duration interval is manually measured. Measuring the QRS complex duration interval is accomplished by sensing the electrograms using any of the above-mentioned techniques and recording/printing the sensed cardiac signal on a paper strip chart recording at 50 millimeters/second. In one embodiment, the QRS complex duration intervals are measured from cardiac signals sensed on leads II, V_1 and V_6 of a 12-lead ECG, where lead V_6 is placed at the midaxillary line, at the same level as lead V_4 . Alternatively, QRS complex duration intervals are measured from cardiac signals sensed from leads II and V_1 of a PRM

surface ECG system, where lead V_1 is placed at the fourth intercostal space, just to the right of the sternum. In one embodiment, the QRS duration is measured from the printout of the cardiac signal using standard practice for determining the start and end of the QRS complex. For example, the QRS duration is measured between a point at which the initial deflection for the Q-wave is sensed and a point where the S-wave returns to baseline of the cardiac signal. Alternatively, the QRS duration is measured from individual leads, where the maximum duration of the QRS interval from among the individual leads is taken as the final result.

At 230, one or more ventricular chambers are selected in which to provide pacing pulses based on the timing relationship between intrinsic electrograms recorded of the right and the left ventricles. In one embodiment, this selection is based on the duration interval of the QRS complexes and the time of occurrence for R_L and R_R . For example, the determination as to the ventricular chamber or chambers to pace is based on the comparison of the duration interval of the QRS complexes to an established value and the value of the difference between R_L and R_R . So, when the duration interval of the QRS complexes is greater than or equal to a first threshold value and the difference between R_L and R_R (i.e., $R_L - R_R$) is greater than a second threshold value, then the patient is likely a left bundle branch block type. In this situation the suggested pacing chamber would be either the left ventricle or biventricular (left ventricle and right ventricle). Alternatively, when the duration interval of the QRS complexes is greater than or equal to the first threshold value and the difference between R_L and R_R (i.e., $R_L - R_R$) is less than or equal to the second threshold value, then the patient is likely a right bundle branch block type. In this situation the suggested pacing chamber would be the right ventricle. In one embodiment, the first threshold value is set at 120 milliseconds and the second threshold value is set at zero (0).

FIGS. 3A and 3B show data collected from fifty four (54) human patients receiving ventricular resynchronization therapy. The data indicate that when QRS complexes have a duration interval greater than or equal to 120 milliseconds, the decision as to whether a patient has a left bundle branch block or a right bundle branch block can be determined by the value of the difference between the R_L and R_R values, as previously described.

As mentioned previously, the present subject matter is implemented in any number of implantable or external medical devices. These medical devices include, but are not limited to, implantable pulse generators, such as pacemakers and cardioverter/defibrillators, pacer/defibrillators, and biventricular or other multi-site resynchronization devices. Other devices include, but are not limited to, external pacemakers, cardioverter/defibrillators, pacer/defibrillators, biventricular or other multi-site resynchronization devices, monitors, medical device programmers and recorders.

FIG. 4 shows one embodiment of an implantable pulse generator system 400 according to the present subject matter. The implantable pulse generator system 400 includes biventricular pacing ability, the ability to sense cardiac signals from and provide pacing pulses to both the right and left ventricular regions of the heart. Examples of biventricular pacemakers include U.S. Pat. Nos. 5,792,203 and 4,928,688, which are hereby incorporated by reference in their entirety.

Biventricular pulse generators have been found to be useful in treating heart failure (HF), a clinical syndrome in which an abnormality of cardiac function causes cardiac output to fall below a level adequate to meet the metabolic demand of peripheral tissues. HF can be due to a variety of etiologies, with ischemic heart disease being the most common. Some

HF patients suffer from some degree of AV block such that their cardiac output can be improved by synchronizing atrial and ventricular contractions with dual-chamber pacing using a short programmed AV delay time. It has also been shown, however, that some HF patients suffer from intraventricular conduction defects (a.k.a. bundle branch blocks). The cardiac outputs of these can be increased by improving the synchronization of right and/or left ventricular contractions. Identifying which, or both, ventricular chamber to pace is then important in treating these cardiac conditions.

In FIG. 4, the implantable pulse generator 400 includes a first cardiac lead 404, a second cardiac lead 408 and a third cardiac lead 412. Each lead 404, 408 and 412 further includes an insulative lead body that includes insulated lead conductors that couple connector pins and/or rings at a proximal end of lead to each electrode on the lead 404, 408 and 412. The implantable pulse generator 400 further includes a connector block 416 adapted to releasably couple leads 404, 408 and 412 to the pulse generator and to couple the electrodes located on the leads to the electronic control circuitry located within the implantable pulse generator 400. The electronic circuitry within the implantable pulse generator 400 senses cardiac signals from the heart and provides electrical pulses, such as pacing and/or defibrillation pulses, under predetermined conditions of the heart. The electronic circuitry also contains transmitting and receiving circuitry for communicating with an external medical device programmer 417.

In the embodiment shown in FIG. 4, the first cardiac lead 404 includes a first ventricular pacing/sensing electrode 420 positioned at or near a distal end 422 of the first cardiac lead 404. The first cardiac lead 404 further includes a first defibrillation electrode 424 and a second defibrillation electrode 426, where the electrodes 424 and 426 are positioned on lead 404 to allow the first pacing/sensing ventricular electrode 420 and the first defibrillation electrode 424 to be positioned in a right ventricle 428 and the second defibrillation electrode 426 positioned in at least a portion of a right atrium 430 and/or a portion of a major vein to the heart, such as the superior vena cava 432.

Electrodes 424 and 426 allow for bipolar cardiac signals to be sensed from the right ventricular region, while electrode 420 allows for unipolar (near-field) cardiac signals to be sensed from the right ventricle. In addition, electrodes 420, 424 and 426 and the implantable pulse generator housing 436, in a "hot can" configuration, allow for different combinations of electrodes and the housing 436 to be used in sensing the cardiac signals from and for delivering electrical energy pulses to at least the right ventricular region of the heart.

The second cardiac lead 408 includes a second ventricular sensing/pacing electrode 444 and a third ventricular sensing/pacing electrode 448. In one embodiment, the second ventricular sensing/pacing electrode 444 is a full or partial annular ring electrode positioned at or near a distal end 450 of the second cardiac lead 408. Alternatively, the second ventricular sensing/pacing electrode 444 is a distal tip electrode positioned at the distal end of the second cardiac lead 408. The third ventricular sensing/pacing electrode 448 is positioned on the lead 408 proximal to the second electrode 444 to allow for the electrodes 444 and 448 to be positioned within a coronary vein 454 and through the coronary veins (such as the lateral or posterior vein) so that the electrodes 444 and 448 are adjacent the left ventricle 458 to allow for sensing intrinsic heart signals from the left ventricle 458 and providing one or more of resynchronization stimulations or defibrillation shocks. In one embodiment, the second cardiac lead 408 of a size and shape adapted to be positioned through the coronary

sinus vein **454** so as to allow the electrodes **444** and **448** to be positioned adjacent the left ventricle **458**.

Electrodes **444** and **448** allow for bipolar cardiac signals to be sensed from and pacing pulses to be delivered to the left ventricular region of the heart. Alternatively, unipolar cardiac signals could be sensed and coordinated paces shocks could be delivered between either electrode **444** or **448** and the housing **436** of the implantable pulse generator.

The third cardiac lead **412** includes a first atrial sensing/pacing electrode **460** and a second atrial sensing/pacing electrode **462**, where both electrodes **460** and **462** are spaced apart and positioned at or near a distal end **464** of the third cardiac lead **412**. In one embodiment, the first atrial sensing/pacing electrode **460** is used in conjunction with the housing **436** for unipolar pacing or sensing from the right atrium **430**. Alternatively, the first and second electrodes **460** and **462** are used to pace bipolarly or to sense bipolar cardiac signals between the two electrodes **460** and **462**. Additional pacing/sensing electrodes can be included on the third cardiac lead **412** to allow for bipolar sensing and pacing of the right atrium **430**.

The apparatus of the present subject matter is not limited to an implantable pulse generator. The apparatus of the present subject matter can be generally considered to be implemented as an automatic site-optimization feature in ventricular resynchronization therapy that can be carried out by an external apparatus (e.g., a medical device programmer or external ventricular resynchronization therapy device) or an implantable pulse generator (e.g., an implantable ventricular resynchronization therapy device such as a pacemaker and/or a cardioverter/defibrillator).

FIG. 5 is a schematic drawing illustrating generally by way of example, but not by way of limitation, one embodiment of the implantable pulse generator **400** coupled by leads **404**, **408** and **412** to the heart. In one such embodiment, the implantable pulse generator **400** provides biventricular resynchronization therapy to coordinate right ventricular and left ventricular contractions, such as for heart failure patients. FIG. 5 shows one embodiment of control circuitry **500** within the implantable pulse generator housing **436**. The housing **436** is electrically conductive and acts as a reference electrode in unipolar pacing and sensing.

In the present embodiment, the implantable pulse generator **400** is adapted to receive the first, second and third leads **404**, **408** and **412**, in connector block **416** and to couple electrodes **420**, **424**, **444**, **448**, **460** and **462** on the cardiac leads to at least one receiver, where the receiver receives intrinsic intracardia electrograms from a left ventricle and a right ventricle. In the present embodiment, the at least one receiver includes cardiac signal amplifiers **504**, **508** and **512** that receive cardiac signals from electrodes **420**, **424**, **444**, **448**, **460** and **462** via contacts **514**, **516**, **518**, **520**, **522** and **523**, respectively. Contact **524** is provided to couple to electrode **426**.

In one embodiment, any combination of bipolar and/or unipolar cardiac signals are sensed using the electrodes **420**, **424**, **444**, **448**, **460** and **462**. For example, a unipolar cardiac signal is sensed from the right ventricle between electrode **422** and the housing **436**. In addition, a unipolar cardiac signal is sensed from the left ventricle between electrode **444** or **448** and the housing **436**. In one embodiment, QRS complex duration intervals are sensed and measured, as described above, from the unipolar cardiac signal sensed from the right ventricle and/or the left ventricle. Finally, a unipolar cardiac signal from the right atrium is sensed from either the first or second atrial sensing/pacing electrode (**460** or **462**) and the housing **436**.

In one embodiment, an output from amplifier **504** is shown coupled to a right ventricular depolarization sensor **530** to allow for a bipolar cardiac signal to be sensed from the right ventricle **428** (FIG. 4) between the first ventricular pacing/sensing electrode **420** and the first defibrillation electrode **424**. The output from amplifier **508** is shown coupled to a left ventricular depolarization sensor **534** to allow for a bipolar cardiac signal to be sensed from the left ventricle **458** (FIG. 4) between the second ventricular sensing/pacing electrode **444** and the third ventricular sensing/pacing electrode **448**. The output from amplifier **512** is shown coupled to an atrial depolarization sensor **536** to allow for a bipolar cardiac signal to be sensed between the first and second atrial sensing/pacing electrodes **460** and **462**.

The control circuitry **500** further includes amplifier **540** that is coupled to the first defibrillation electrode **424** and the second defibrillation electrode **426** to allow for bipolar far-field cardiac signals to be sensed from the heart. From this signal it is possible to measure the duration interval of sensed QRS complexes and to use this value as previously described. In an additional embodiment, the housing **436** is used as an additional electrode in common with the second defibrillation electrode **426** to allow for the far-field cardiac signal to be sensed between the first defibrillation electrode **424** and the second defibrillation electrode **426**/housing **436**. The output from amplifier **540** is shown coupled to a QRS-complex detector **540**. In one embodiment, the QRS-complex detector **540** identifies QRS-complexes detected in the cardiac signal from amplifier **540** and supplies this information to controller **550** either for further processing by the controller **550** or for being transmitted to a medical device programmer **554**, as will be described below.

The information from the right ventricular depolarization sensor **530** and the left ventricular depolarization sensor **534** are then used by the controller **550** to determine the timing relationship between the intrinsic intracardia electrograms recorded from the left and right ventricle. In one embodiment, the controller **550** calculates a delay between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations. In one example, the controller **550** detects peaks of the sensed intrinsic ventricular depolarizations and calculates the delay between the detected peaks of the intrinsic ventricular depolarizations sensed from the left ventricular and the right ventricles.

In addition to calculating the delay, the controller **550** also receives a duration interval of one or more QRS complexes. In one embodiment, the duration interval of the QRS complexes is calculated by the QRS-complex detector **544**. Alternatively, the duration interval is calculated from the paper strip chart recording of the ventricular signals, as previously described, and supplied to the controller **550** from the medical device programmer **554**.

The control circuitry **500** further includes a ventricular chamber selector **560** coupled to the controller **550**. The ventricular chamber selector **560** selects one or more ventricular chambers in which to provide pacing pulses based on the timing relationship between intrinsic intracardia electrograms recorded from the right and left ventricle. In one embodiment, the ventricular chamber selector **560** selects one or more ventricular chambers in which to provide pacing pulses based on the duration interval of the QRS complexes and the delay between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations, as previously discussed. For example, the ventricular chamber selector **560** identifies a left ventricle for pacing when the duration interval of the one or more QRS complexes is greater than or equal to 120 milliseconds and the difference between the left

ventricular and the right ventricular sensed intrinsic ventricular depolarizations is greater than zero (0). Additionally, the ventricular chamber selector **560** identifies both a left ventricle and a right ventricle for pacing when the duration interval of the one or more QRS complexes is greater than or equal to 120 milliseconds and the difference between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations is greater than zero (0). Finally, the ventricular chamber selector **560** identifies a right ventricle for pacing when the duration interval of one or more QRS complexes is greater than or equal to 120 milliseconds and the difference between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations is less than or equal to zero (0).

The controller **550** also analyzes the sensed cardiac signals to determine when and if to deliver electrical energy pulses to the heart. In one embodiment, the microprocessor implements one or more analysis protocols stored in a memory **566** to analyze one or more of the sensed cardiac signals and to provide pacing, cardioversion and/or defibrillation therapy to one or more chambers of the heart under certain predetermined conditions. Memory **566** is also used to store one or more sensed cardiac signals to be downloaded to the medical device programmer **554** for analysis. In one embodiment, the control circuitry **500** communicates with the medical device programmer **554** through a receiver/transmitter **570**, where cardiac signals, programs and operating parameters for the programs for the implantable medical device are transmitted and received through the use of the programmer **556** and the transmitter/receiver **570**. Power for the control circuitry **500** is supplied by a battery **574**.

The controller **550** further controls a pace output circuit **580** and a defibrillation output circuit **588** to provide pacing, cardioversion and/or defibrillation therapy to one or more chambers of the heart under certain predetermined conditions. In one embodiment, the pace output circuit **580** is coupled to contacts **514**, **516**, **518**, **520**, **522** and the housing **436** to allow for pacing between the electrode combinations of **420** and **424**, **420** and the housing **436**, **444** and **448**, **444** or **448** and the housing **436**, **460** and **462**, and **460** and the housing **436**. The defibrillation output circuit **588** is shown coupled to electrodes **424**, **426** and (optionally) housing **436** to allow for defibrillation energy pulses to be delivered to a heart.

FIG. **6** shows one embodiment of a medical device programmer **554** according to the present subject matter. The medical device programmer **554** is adapted to be positioned outside the human body for communication with the implantable pulse generator **400**, as previously described. In one embodiment, a communication link **608** is established between the medical device programmer **554** and the implantable pulse generator **400**, as described above.

In one embodiment, the medical device programmer **554** includes electronic circuitry within a housing **610**, where a graphics display screen **612** is disposed on an upper surface **614** of the housing **610**. The programmer **554** further includes a drive **618** for reading and writing instructions used by the electronic circuitry of the programmer **554**. The graphics display screen **612** is operatively coupled to the electronic circuitry within the housing **610** and is adapted to provide a visual display of graphics and/or data to the user.

The programmer **554** further includes input devices to the electronic circuitry. For example, the programmer **554** includes a touch-sensitive display screen, such that the user interacts with the electronic circuitry by touching identified regions of the screen with either their finger or with a stylus (not shown). In addition, the programmer **554** further

includes an alphanumeric key board **620** for providing information, such as programmable values for the implantable medical device **604**, to the electronic circuitry and the medical device **604**.

The programmer **554** further includes a programming head **624**. The programming head **624** is used to establish the communication link **608** between the electronic circuitry within the programmer **554** and the implantable pulse generator **400**. In one embodiment, the communication link **608** is a radio frequency link. The telemetry link between the implantable pulse generator **400** and the programmer **554** allows the electronic circuitry coupled to the graphics display screen **612** to be coupled to the electronic control circuitry of the implantable pulse generator **400**. The programming head **624** is coupled to the electronic circuitry of the medical device programmer through cable **628**. FIG. **6** also shows the programmer **554** having a printer **630** which allows for cardiac signals received from the implantable pulse generator **400** and displayed on the graphics display screen **612** to be displayed on a paper printout **634**. Adjustments for printer speed and scale of the printed cardiac signals is adjustable through the use of the display screen **612** and the electronic circuitry within the programmer **600**.

FIG. **7** shows one embodiment of control circuitry **700** for the programmer **554**. The control circuitry **700** includes a receiver/transmitter circuit **708**, a ventricular chamber selector **712**, a controller **716**, a memory **720**, a data input/output **724** and an in/out drive **730**. In one embodiment, the receiver/transmitter circuit **708** receives intrinsic intracardia electrograms from a left ventricle and a right ventricle. In one embodiment, the intrinsic intracardia electrograms from the left ventricle and the right ventricle are sensed using an implantable pulse generator, as previously described. The controller **716** then determines a timing relationship between intrinsic intracardia electrograms recorded from the left and right ventricle. In one embodiment, the controller **716** calculates the delay between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations. In one embodiment, the controller **716** detects peaks of the sensed intrinsic ventricular depolarizations and calculates the delay between the detected peaks of the intrinsic ventricular depolarizations sensed from the left ventricular and the right ventricles, as previously described.

The controller is also adapted to receive the duration interval of one or more QRS complexes. In one embodiment, the duration interval of the QRS complexes are measured from a print-out of the sensed electrograms, as previously described, where the electrograms are printed on printer **736** under the control of controller **716** and under the directions provided through the data input/output **724**. The QRS duration interval is then provided through the data input/output **724** via prompts displayed on the display screen **612** (not shown in FIG. **7**) and data received via the keyboard **620** (not shown in FIG. **7**). In an additional embodiment, the QRS duration is measured from printout from a surface ECG and then manually entered into the control circuitry **700**.

The ventricular chamber selector **712** then selects one or more ventricular chambers in which to provide pacing pulses based on the timing relationship between intrinsic intracardia electrograms recorded from the right and left ventricle. In one embodiment, the timing relationship used is based on the duration interval of the QRS complexes and the delay between the left ventricular and the right ventricular sensed intrinsic ventricular depolarizations, as previously described. The results are then displayed on the display screen **612**. The

13

user can then elect to accept the suggested results and program the implantable medical device with the suggested settings.

Although specific embodiments have been illustrated and described herein, it will be appreciated by those of ordinary skill in the art that any arrangement which is calculated to achieve the same purpose may be substituted for the specific embodiment shown. This application is intended to cover any adaptations or variations of the present invention. Therefore, it is intended that this invention be limited only by the claims and the equivalents thereof.

We claim:

1. An implantable cardiac device, comprising:
sensing circuitry for receiving cardiac signals from the right and left ventricles;

pacing circuitry for delivering pacing pulses;

a controller for controlling the operation of the pacing circuitry in accordance with a selected pacing mode;

circuitry for determining a timing relationship between intrinsic ventricular depolarizations of the left and the right ventricles; and,

circuitry for selecting between a right ventricular, left ventricular, or biventricular pacing mode by which to provide pacing pulses based on the timing relationship between intrinsic ventricular depolarizations of the left and the right ventricle, wherein the selected pacing mode determines the manner in which paces are delivered over multiple cardiac cycles.

2. The device of claim 1 wherein the timing relationship between intrinsic ventricular depolarizations of the left and the right ventricle is derived from intracardiac electrograms received by the sensing circuitry.

3. The device of claim 1 wherein the timing relationship between intrinsic ventricular depolarizations of the left and the right ventricle includes an interval between a right ventricular sense R_R and a left ventricular sense L_L .

4. The device of claim 1 further comprising: a receiver/transmitter circuit for communicating with an external device and wherein the circuitry for selecting between a right ventricular, left ventricular, or biventricular pacing mode by which to provide pacing pulses further bases the selection on a QRS duration received from the external device.

5. The device of claim 1 wherein the circuitry for selecting between a right ventricular, left ventricular, or biventricular pacing mode by which to provide pacing pulses includes circuitry for selecting pacing in the left ventricle when the delay between the right ventricular and the left ventricular intrinsic ventricular depolarizations is greater than a threshold value, with the right ventricular depolarization occurring before the left ventricular depolarization.

6. The device of claim 5 wherein the threshold value is zero (0).

7. The device of claim 1 wherein the circuitry for selecting between a right ventricular, left ventricular, or biventricular pacing mode by which to provide pacing pulses includes circuitry for selecting pacing in the right and left ventricles when the delay between the right ventricular and the left ventricular intrinsic ventricular depolarizations is greater than a threshold value, with the right ventricular depolarization occurring before the left ventricular depolarization.

8. The device of claim 7 wherein the threshold value is zero (0).

14

9. The device of claim 1 wherein the circuitry for selecting between a right ventricular, left ventricular, or biventricular pacing mode by which to provide pacing pulses includes circuitry for selecting pacing in the right ventricle when the delay between the left ventricular and the right ventricular intrinsic ventricular depolarizations is greater than a threshold value, with the left ventricular depolarization occurring before the right ventricular depolarization.

10. The device of claim 9 wherein the threshold value is zero (0).

11. A method for operating an implantable cardiac device, comprising:

receiving cardiac signals from the right and left ventricles; delivering pacing pulses in accordance with a selected pacing mode;

determining a timing relationship between intrinsic ventricular depolarizations of the left and the right ventricles; and,

selecting between a right ventricular, left ventricular, or biventricular pacing mode by which to provide pacing pulses based on the timing relationship between intrinsic ventricular depolarizations of the left and the right ventricle, wherein the selected pacing mode determines the manner in which paces are delivered over multiple cardiac cycles.

12. The method of claim 11 wherein the timing relationship between intrinsic ventricular depolarizations of the left and the right ventricle is derived from intracardiac electrograms received by the sensing circuitry.

13. The method of claim 11 wherein the timing relationship between intrinsic ventricular depolarizations of the left and the right ventricle includes an interval between a right ventricular sense R_R and a left ventricular sense L_L .

14. The method of claim 11 further comprising selecting between a right ventricular, left ventricular, or biventricular pacing mode by which to provide pacing pulses where the selection is further based on a QRS duration received from an external device.

15. The method of claim 11 further comprising electing pacing in the left ventricle when the delay between the right ventricular and the left ventricular intrinsic ventricular depolarizations is greater than a threshold value, with the right ventricular depolarization occurring before the left ventricular depolarization.

16. The method of claim 15 wherein the threshold value is zero (0).

17. The method of claim 11 further comprising selecting pacing in the right and left ventricles when the delay between the right ventricular and the left ventricular intrinsic ventricular depolarizations is greater than a threshold value, with the right ventricular depolarization occurring before the left ventricular depolarization.

18. The method of claim 17 wherein the threshold value is zero (0).

19. The method of claim 11 further comprising selecting pacing in the right ventricle when the delay between the left ventricular and the right ventricular intrinsic ventricular depolarizations is greater than a threshold value, with the left ventricular depolarization occurring before the right ventricular depolarization.

20. The method of claim 19 wherein the threshold value is zero (0).

* * * * *