

(12) STANDARD PATENT
(19) AUSTRALIAN PATENT OFFICE

(11) Application No. **AU 2008222757 B2**

- (54) Title
Transdermal analyte monitoring systems and methods for analyte detection
- (51) International Patent Classification(s)
A61B 5/00 (2006.01)
- (21) Application No: **2008222757** (22) Date of Filing: **2008.03.06**
- (87) WIPO No: **WO08/109739**
- (30) Priority Data
- (31) Number (32) Date (33) Country
60/893,563 **2007.03.07** **US**
- (43) Publication Date: **2008.09.12**
(44) Accepted Journal Date: **2011.06.09**
- (71) Applicant(s)
Echo Therapeutics, Inc.
- (72) Inventor(s)
Kost, Joseph; Hurley, James P.; Chuang, Han
- (74) Agent / Attorney
FB Rice, Level 23 44 Market Street, Sydney, NSW, 2000
- (56) Related Art
US 2006/0094944
WO 2000/009203
US 5405366

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
12 September 2008 (12.09.2008)

PCT

(10) International Publication Number
WO 2008/109739 A1

(51) International Patent Classification:
A61B 5/00 (2006.01)

(74) Agents: PABST, Patrea, L. et al.; Pabst Patent Group LLP,
400 Colony Square, 1201 Peachtree Street, Suite 1200, At-
lanta, GA 30361 (US).

(21) International Application Number:
PCT/US2008/056032

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA,
CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE,
EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID,
IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC,
LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN,
MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH,
PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, SV,
SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN,
ZA, ZM, ZW.

(22) International Filing Date: 6 March 2008 (06.03.2008)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/893,563 7 March 2007 (07.03.2007) US

(71) Applicant (for all designated States except US): ECHO
THERAPEUTICS, INC. [US/US]; 10 Forge Parkway,
Franklin, MA 02038 (US).

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,
ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,
FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL,
NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG,
CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(72) Inventors; and


(75) Inventors/Applicants (for US only): CHUANG, Han
[—/US]; 33 Evergreen Circle, Canton, MA 02021 (US).
HURLEY, James, P. [US/US]; 122 Walpole Street, Can-
ton, MA 02021 (US). KOST, Joseph [IL/IL]; 54 Hashita,
84965 Omer (IL).

Published:
— with international search report

[Continued on next page]

(54) Title: TRANSDERMAL ANALYTE MONITORING SYSTEMS AND METHODS FOR ANALYTE DETECTION

Fig. 9. Transdermal glucose sensor with wireless communication

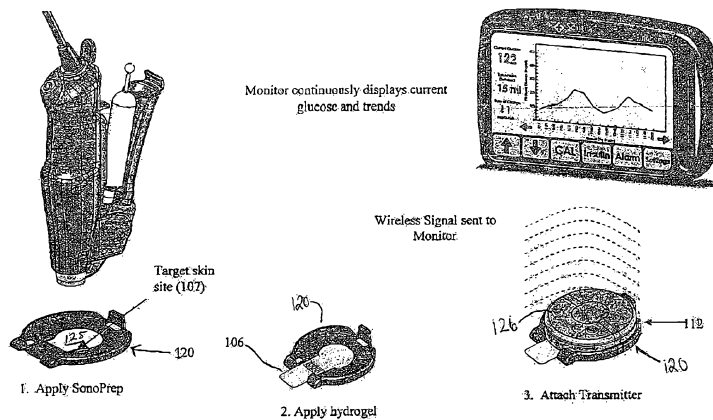

(57) Abstract: Transdermal analyte monitoring systems (TAMS) having increased longevity and improved analyte detection are described herein. Kits for use with the TAMS and methods of using the TAMS and kits are also described. In a preferred embodiment, the TAMS includes a protective, semi-permeable membrane covering the surface of the hydrogel. The protective, semi-permeable membrane contacts with the skin of a user and prevents contamination or fouling of the hydrogel. Optionally, the hydrogel comprises one or more humectants and/or an immobilized enzyme. In another preferred embodiment, the TAMS contains at least one channel or pocket for increasing the amount of oxygen provided to the hydrogel. In one embodiment, a method for improving analyte detection by the TAMS is provided. For example, after the skin porosity is increased by an appropriate pretreatment, a skin preparation wipe is applied to the treated skin area and then the TAMS is applied to the treated area.

WO 2008/109739 A1



-
- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments*

**TRANSDERMAL ANALYTE MONITORING SYSTEMS
AND METHODS FOR ANALYTE DETECTION**

FIELD OF THE INVENTION

5 The present invention is directed to the field of systems and methods for improving non-invasive sampling of biological fluids, and more specifically to systems and methods for improving transdermal analyte detection and quantification.

CROSS-REFERENCE TO RELATED APPLICATION

10 This application claims priority to U.S.S.N. 60/893,563, filed in the U.S. Patent and Trademark Office on March 7, 2007.

BACKGROUND OF THE INVENTION

 The impact that diabetes has on the health of Americans is staggering. According to the American Diabetes Association in 2006
15 approximately 20.8 million Americans were diagnosed with diabetes. The cost of diabetes in 2002 was estimated at \$132 billion. The number of deaths in 2006 attributed to complications associated with diabetes was estimated at 613 Americans per day.

 New and improved systems and methods for treating and detecting
20 diabetes are in high demand. Analytical biosensors provide one type of system that can be used to manage diabetes. Analytical biosensors have been embraced during the last decade as a means of combining the advantages of electrochemical signal transduction with the specificity inherent in biological interactions. For example, the use of continuous glucose monitoring (CGM)
25 to manage diabetes is becoming increasingly popular.

 Despite recent improvements in analytical biosensor systems, the available systems suffer from disadvantages. For example, systems employing a hydrogel sensor typically have short shelf lives and may leak sensor materials onto the skin of a user. Alternatively, bacterial growth or
30 growth of other microorganism can contaminate or foul the biosensor rendering its measurements of analytes unreliable. In some instances, proteins, carbohydrates, cells, or fragments of cells from the user can bind to

the sensor and interfere with measurements. Such binding can also contaminate the biosensor.

Membranes, films or other physical barriers have been used on the surface of sensor electrodes to impede contaminants from reaching the face
5 of the electrode. Typical films which have been employed include cellulose acetate, poly(o-phenylenediamine), polyphenol, polypyrrole, polycarbonate, and NAFION[®], i.e. tetrafluoroethylene-perfluoro-3,6-dioxa-4-methyl-7-octenesulfonic acid copolymer (E.I. du Pont de Nemours & Co.,
Wilmington, Del.). However, these membranes can be difficult to prepare
10 and may not efficiently attach to the reactive surface of the electrode.

Some CGM systems require pretreatment of the skin with a hydrating formulation prior to attachment of the system. For example, with existing biosensor systems, a 10-40 minute skin hydration procedure is typically applied to the target skin site after treatment to increase skin
15 porosity and before sensor application. The hydration procedure results in better sensor performance than is achieved without pretreatment (sensor signal follows well to reference blood glucose reading). Although it enables improved sensor performance, the skin hydration procedure requires undesirable labor, materials and time which may further complicate the
20 procedure for device installation, and hence the cost of the system. Systems that do not require complicated or time consuming skin pretreatment procedures are desirable.

In still other CGM systems, a standard reference glucose method is used to calibrate the glucose sensor and then the sensor reports subsequent
25 glucose readings based on the calibrated electrical signal. In principle, the blood glucose concentration of a test subject should be proportional to the measured electrical signal. For sensors based on the enzymatic conversion of glucose, for example where the enzyme glucose oxidase (GOx) utilizes water and oxygen to convert glucose into hydrogen peroxide (H₂O₂) and
30 glucolactone, the enzymatic conversion is limited by the amount of available oxygen. When the supply of oxygen is limited, such as in interstitial fluid, the concentration of glucose exceeds the concentration of oxygen, the

enzymatic conversion of glucose will be dependent on the oxygen supply, resulting in unreliable sensor glucose reading and hence affecting the sensor performance.

5 Various methods have been reported to mitigate the issue of oxygen limitation. Tierney et al. describes using reverse iontophoresis to limit glucose extraction, maintaining desirable oxygen to glucose balance (M. Tierney et al, *Annals of Medicine*, 32(9):632-641 (2000)). U.S. Patent No. 7,110,803 to Shults et al. discloses using a glucose-limiting membrane layer that has a high oxygen to glucose permeability ratio. U.S. Patent No. 7,108,778 to Simpson et al discloses using an auxiliary electrode to generate
10 oxygen for the sensing chemistry. However, each of these methods requires the addition of extra elements to the CGM system, thereby increasing the cost and complexity of the system. A simple method for increasing the amount of available oxygen to the sensor without increasing the cost and complexity of the system is needed.

15 Therefore, this invention seeks to provide an improved transdermal analyte monitoring system.

It also seeks to provide a method for reducing biofouling and/or contamination in a
20 transdermal analyte monitoring system.

It further seeks to provide methods for improving the accuracy of detection and/or quantification of an analyte by a transdermal analyte monitoring system.

25 Any discussion of documents, acts, materials, devices, articles or the like which has been included in the present specification is not to be taken as an admission that any or all of these matters form part of the prior art base or were common general knowledge in the field relevant to the present invention as it existed before the priority date of each claim of this application.

30
SUMMARY OF THE INVENTION

Transdermal analyte monitoring systems (TAMS) with improved longevity and analyte detection are described herein. Generally, the transdermal analyte detecting system ("TADS") contains a sensor assembly, which includes (1) a hydrophilic polymer

substrate, such as a hydrogel, designed to receive an analyte from the skin, and (2) a sensor body containing a plurality of electrodes, and a display and/or computing device.

5 More particularly, the present invention consists in a transdermal analyte monitoring system comprising:

10 a sensor assembly, wherein the sensor assembly comprises a hydrogel and a sensor body containing a plurality of electrodes, wherein the sensor body is in fluid communications with the hydrogel, wherein the hydrogel comprises a humectant and an enzyme and wherein the humectant is in an effective amount to increase the performance longevity of the transdermal analyte monitoring system, as indicated by decreased signal drift, compared to the same system in the absence of humectant.

15 Throughout this specification the word "comprise", or variations such as "comprises" or "comprising", will be understood to imply the inclusion of a stated element, integer or step, or group of elements, integers or steps, but not the exclusion of any other element, integer or step, or group of elements, integers or steps.

20 In the preferred embodiment, the TAMS includes a semi-permeable membrane at the end of the sensor, which attaches to the hydrophilic polymer substrate. This membrane interfaces with an exterior surface of a

test subject and acts as a barrier between the patient's skin and the hydrophilic polymer substrate. The semi-permeable membrane reduces the amount of biological contamination of the hydrophilic polymer substrate, as compared to the same device in the absence of a semi-permeable membrane, 5 by forming a protective barrier over the exposed surface of the hydrophilic polymer substrate. Additionally, the semi-permeable membrane prevents the hydrophilic polymer substrate from leaking out of the device. The hydrophilic polymer substrate typically includes an enzyme, and optionally includes one or more humectants.

10 In a preferred embodiment, the TAMS contains one or more channels or pockets in the sensor assembly, which increases the amount of oxygen available for reacting the analyte with an enzyme and generating a detectable signal.

In another embodiment, a method for improving analyte detection 15 and/or quantification by a transdermal analyte monitoring system is provided. The method includes treating a region of skin of the organism to increase porosity and subsequently wiping the treated area of skin with a substrate. The substrate can be any suitable absorbent material, such as a pad, woven or non-woven fabric, felt, or gauze. Generally, the substrate 20 contains a wiping reagent, such as a solvent (*e.g.* water, ethanol, or isopropanol), phosphate buffered saline, lactic acid, soap, a surfactant, or a combination thereof. The wiping step prevents the need for a skin hydration step. After the skin is wiped, the transdermal analyte monitoring system is applied.

25 In another embodiment, a kit containing a transdermal analyte detection system and a substrate is provided. The substrate may be impregnated with a wiping reagent. Alternatively, wiping reagents can be separately included in the kit.

BRIEF DESCRIPTION OF THE DRAWINGS

30 Figure 1 shows an exemplary wired transdermal analyte monitoring system (TAMS) for performing continuous analyte monitoring, with the sensor illustrated in an exploded view. Alternatively, the communication

between the sensor and the monitor can be achieved through a wireless link (not shown in Figure 1).

Figure 2 shows a drawing of the sensor body shown in Figure 1.

5 Figure 3 is a bar graph of the percentage of the remaining signal from the exemplary biosensor with and without barrier membranes after 24-hr of *ex vivo* applications, where “n” represents the number of tests.

Figure 4 shows a bar graph of signal drift (%) and 24-hr Mean Absolute Relative Difference (MARD) between the sensor (nA) and blood glucose (BG) levels for the device with different membranes, calibrated every 4 hours. The labels “PES-10K” (Poly (ether sulfone)) and “RC-3k” refer to UF membranes, “UB” refers to covalently activated PES, “0.2PES” refers to uncoated with 0.2 μm pores, “.NAF” refers to Nafion®-coated, and the asterick (*) indicates that for this sensor, MARD is quoted with calibration every 8 hours.

15 Figure 5 shows a bar graph of signal drift (%) and 24-hr MARD when various humectants were included in the hydrogel matrix. Testing was 24-hr *ex vivo* application, and all used a 0.2PES.Naf membrane.

Figure 6 shows a bar graph comparing a biosensor system with covalently immobilized GOx to one without covalent immobilization, using nA to BG correlation (R^2) and MARD, after 4-hour *ex vivo* application.

Figure 7A is a line graph of blood glucose concentrations (mg/dl) versus time (minutes) taken from a continuous, transdermal glucose sensor with a skin preparation wiping procedure performed prior to applying the sensor. Reference blood glucose (“Actual BG”, finger stick blood glucose meter reading, solid line with circles) levels are compared to predicted blood glucose (“Predicted BG”, the sensor’s glucose reading, solid line) levels. The data shows a strong correlation ($r = 0.950$) between the Predicted BG and the Actual BG.

Figure 7B is a line graph of blood glucose concentrations (mg/dl) versus time (minutes) taken from a continuous, transdermal glucose sensor without any skin preparation procedure prior to applying the sensor. Reference blood glucose (“Actual BG”, finger stick blood glucose meter

reading, solid line with circles) levels are compared to predicted blood glucose (“Predicted BG”, the sensor’s glucose reading, solid line) levels. The data shows a poor correlation ($r = 0.309$) between the Predicted BG and the Actual BG.

5 Figure 7C is a line graph of blood glucose concentrations (mg/dl) versus time (minutes) taken from a continuous, transdermal glucose sensor with a 40-minute skin hydration procedure performed prior to applying the sensor. Reference blood glucose (“Actual BG”, finger stick blood glucose meter reading, solid line with circles) levels are compared to predicted blood
10 glucose (“Predicted BG”, the sensor’s glucose reading, solid line) levels. The data shows a strong correlation ($r = 0.947$) between the Predicted BG and the Actual BG.

Figure 8A shows a diagram of the bottom of an exemplary target plate with four air channels.

15 Figure 8B shows a diagram of a front view of an exemplary glucose sensor’s target plate with three cuts of internal air pockets surrounding the central hole for hydrogel chemistry.

Figure 8C shows a diagram of an exemplary sensor housing on top of the target plate to provide an enclosed glucose sensor.

20 Figure 9 is a schematic showing how to use an exemplary wireless transdermal analyte monitoring system (TAMS) for performing continuous analyte monitoring. This system could be used with the glucose sensor illustrated in Figures 8A, 8B, and 8C.

Figure 10 is a Clarke error grid of the data obtained in Study 1A, with
25 222 sensor-blood glucose data points collected from 10 patients.

Figure 11 is a Clarke error grid of the data obtained in Study 1B, with 225 sensor-blood glucose data points collected from 10 patients.

Figure 12 is a Clarke error grid of the data obtained in Study 2C, with 147 sensor-blood glucose data points collected from 10 patients (9 of whom
30 completed the study).

DETAILED DESCRIPTION OF THE INVENTION

I. Transdermal Analyte Monitoring System

Systems and methods for enhancing transdermal analyte detection are described herein. Generally, the transdermal analyte monitoring system
5 (“TAMS”) contains a sensor assembly, which includes (1) a hydrophilic polymer substrate, such as a hydrogel, designed to receive an analyte from the skin, and (2) a sensor body containing a plurality of electrodes, and a display and/or computing device. In the preferred embodiment, the TAMS includes a semi-permeable membrane at the end of the sensor, which
10 attaches to the hydrophilic polymer substrate. This membrane acts as a semi-permeable barrier between the patient’s skin and the hydrophilic polymer substrate.

The TAMS is applied to an area on the skin of an animal; typically the animal is a mammal, and in the preferred embodiment the mammal is a
15 human.

When the system is used, the hydrogel contains enzymes that react continuously with the analyte, thereby generating an electrical signal. Then the electrical signal is detected by the electrode assembly. The electrical signal correlates with an analyte value.

20 The analyte to be monitored can be any analyte of interest, including, but not limited to glucose, lactate, blood gases (e.g. carbon dioxide or oxygen), blood pH, electrolytes, ammonia, proteins or any other biological species that is present in a biological fluid, such as blood, plasma, serum or interstitial fluid.

25 An exemplary TAMS is described in U.S. Publication No. 20060094946 to Kellogg *et al.* and is illustrated herein in Figure 1. The TAMS shown in Figure 1 can be used to carry out continuous monitoring of an analyte, such as glucose. As shown in Figure 1, the TAMS (100) contains a sensor assembly (112), which includes a sensor body (101), a hydrogel disc
30 (106) and a mounting plate (102) as well as other components as described herein, which may be attached to a display or computing device. During operation, the sensor assembly (112) may be positioned adjacent a permeable

region (107) of a user's skin as shown by the dashed line in Figure 1. The sensor assembly (112) may be attached by any suitable means to a display or computing device. Suitable means include a wireless connection or any other means for electrical connection, such as a flexible connecting cable (109). In an embodiment, the sensor assembly (112) is attached to a potentiostat recorder (108), which may include a printed circuit board (111). The connecting cable (109) preferably attaches to the potentiostat recorder (108) using a connector (110) that facilitates removal and attachment of the sensor assembly (112). Suitable means for attachment include a flexible connecting cable (109) and a wireless connection.

A TAMS with a wireless connection is illustrated in Figure 9. The sensor assembly (112) includes a target plate (120), a hydrogel (106) and sensor, and a sensor housing (125). The sensor is coupled with a miniature analyzer which sends data wirelessly to a monitor for data processing and display.

A. Sensor Assembly

The sensor assembly (112) shown in Figures 1 and 2 may be incorporated into any one of a number of detection devices. For instance, this sensor assembly may be incorporated into the receiver to provide for discrete and/or continuous glucose monitoring.

The sensor assembly (112) includes a sensor body (101). The sensor body may include electrodes, as shown in Figure 2, on its surface for electrochemical detection of analytes or reaction products that are indicative of analytes.

A thermal transducer (103), which may be housed within the sensor assembly (112) with a shape that corresponds to that of the sensor body (101), is located between the sensor body (101) and the mounting plate (102). Enzyme-based electrochemical sensors, such as glucose sensors, can be sensitive to temperature fluctuation. The thermal transducer (103) may be used to normalize and report only those changes attributed to a change in analyte or analyte indicator.

The sensor assembly (112) may also contain an adhesive disc (104), which may be attached to the side of the sensor body (101) that faces the thermal transducer (103).

5 The sensor assembly (112) may also contain an adhesive ring (105), which may be attached to the side of the sensor body (101) that is opposite the adhesive disc (104). The cut-out center portion of the adhesive ring (105) preferably exposes some or all of the sensor components on the sensor body (101). The adhesive ring (105) and adhesive disc (104) may have a shape that corresponds to that of the sensor body as shown in Figure 1.

10 The sensor assembly (112) contains a hydrogel disc (106), which may be positioned within the cut-out center portion of the adhesive ring (105) adjacent to a surface of the sensor body (101).

a. Sensor Body

A sensor body (101) is illustrated in detail in Figure 2. The sensor
15 body 101 includes a body layer (207) upon which leads (204, 205, and 206) are patterned. The leads may be formed, for example, by coating metal over the body layer (207) in the desired locations. A working electrode (201), is typically located at the center of the sensor body (101). The working electrode (201) may contain a catalytic and/or conductive material, such as
20 pure platinum, platinized carbon, glassy carbon, carbon nanotube, mezoporous platinum, platinum black, palladium, gold, or platinum-iridium. The working electrode (201) may be patterned over lead (206) so that it is in electrical contact with the lead (206). A counter electrode (202) may contain a stable and conductive material, and preferably contains carbon, which may
25 be positioned about the periphery of a portion of the working electrode (201), as shown in Figure 2. The counter electrode (202) may be patterned over lead (205) so that it is in electrical contact with the lead (205). A reference electrode (203) containing binary oxi-reductive materials which provide consistent redox potential, preferably containing Ag/AgCl, may be
30 positioned about the periphery of another portion of the working electrode (201), as shown in Figure 2. The electrodes (201, 202, and 203) can be formed to roughly track the layout of the electrical leads (206, 205, 204),

respectively, that are patterned in the sensing area of the device. The electrodes (201, 202, and 203) may be screen printed or sputter coated over the electrical leads (206, 205, 204), respectively. The leads can be patterned, using screen printing or other methods known in the art, onto the sensor body (101) in a manner that permits electrical connection to external devices or components. For example, the leads may form a 3X connector pin lead including leads (204, 205, and 206) at the terminus of an extended region of the sensor body, as shown in Figure 2. A standard connector may then be used to connect the sensor electrodes to external devices or components.

10 **b. Hydrophilic Polymer Substrate**

The sensor assembly contains a hydrophilic polymer substrate. The substrate is designed to provide the structure to form an aqueous reservoir in the sensor assembly. The hydrophilic polymer substrate may be in any suitable shape that fits in the sensor assembly. Typically, the hydrophilic polymer substrate is in the shape of the sensor body. A standard form is a disc. The shape is selected to co-ordinate with the shape of the sensor. Optionally, ionic moieties can be incorporated into the hydrophilic polymer substrates to impart added functionalities, such as bioadhesiveness. In the preferred embodiment, the substrate is a hydrogel.

20 Hydrogels are a class of biomaterials utilized for medical and biotechnological applications, such as in contact lenses, biosensors, linings for artificial implants and drug delivery devices. The transdermal analyte monitoring system may utilize one or more of the hydrogel materials described below. Classes of hydrogel materials that may be used in the sensor assembly include agarose based hydrogels, polyethylene glycol diacrylate (PEG-DA)-based hydrogels, and vinyl acetate-based hydrogels including polyethylene glycol diacrylate/polyethyleneimine (PEGDA-PEI) and polyethylene glycol diacrylate-n-vinyl pyrrolidone (PEGDA-NVP).

30 Suitable polymers which can form a hydrogel include, but are not limited to, synthetic or natural polymers. Examples of synthetic polymers include polyacrylic and polymethacrylic acid polymers, cellulose derivatives such as hydroxypropyl cellulose, polyethyleneglycol polymers, copolymers

and block copolymers, and other water swellable, biocompatible polymers. Examples of natural polymers include collagen, hyaluronic acid, gelatin, albumin, polysaccharide, and derivatives thereof. Natural polymers can also be of the type isolated from various plant materials such as psyllium.

5 Structurally, the polymeric hydrogels are three-dimensional macromolecular configurations. They may be produced through several methods: a) synthesis from monomers (cross-linking polymerization); b) synthesis from polymers and polymerization auxiliary (grafting and cross-linking polymerization); c) synthesis from polymers and non-polymerization
10 auxiliary (cross-linking polymers); d) synthesis from polymers with energy sources (cross-linking polymers without auxiliaries) and e) synthesis from polymers (cross-linking by reactive polymer-polymer intercoupling).

The hydrogels can vary in thickness. Typically the hydrogel is about 10 to about 1000 μm , more preferably about 50 to about 700 μm , even more
15 preferably about 200 to about 500 μm .

As shown in Figure 1, a hydrogel disc (106) may be positioned in such a manner that it will face toward the user after folding over onto the mounting plate (102). The sensor body (101) may be connected to the mounting plate (102) using standard connectors with a latch that mates with
20 a corresponding connector interface that is mounted onto the backing plate (102).

i. Agarose-based Hydrogels

Agarose based hydrogels can offer advantages for continuous transdermal analyte monitoring. For instance, agarose-based hydrogels offer
25 one or more of the following features: good response to glucose and hydrogen peroxide due to its high water content, high enzyme loading, good biocompatibility, and excellent permeation and diffusion properties. Agarose based hydrogels are generally compatible with water-soluble analytes. In addition, agarose hydrogels are clean, inexpensive, and/or easy
30 to prepare.

An agarose gel may be formed, for example, from 1-20% agarose in buffer solution containing 0-1 M sodium or potassium phosphate, 0-1 M

sodium chloride, 0-1 M potassium chloride, 0-2 M lactic acid, surfactant such as 0-1 M TRITON[®] X-100 (Union Carbide Chemicals & Plastics Technology Corp.), TWEEN[®] 80 (ICI Americas Inc.) or sodium lauryl sulfate, and any other biocompatible components. Loading of glucose oxidase in agarose hydrogel can be up to 0-20% (by weight), for example, by
5 soaking the solid hydrogel in concentrated glucose oxidase solution, or alternatively by mixing concentrated glucose oxidase powder or solution with agarose solution during its melting stage (15-65° C), followed by cooling and gelling at lower temperature (40° C or lower).

10 **ii. PEG-based Hydrogels**

PEG-based hydrogels can offer several advantages for continuous transdermal analyte monitoring. Structurally, PEG is highly hydrophilic and presents a high degree of solvation in aqueous solvents. The preferential solvation of PEG molecules can effectively exclude proteins from the PEG
15 chain volume, thereby protecting the surface from bio-fouling by proteins. An advantage that can be provided by chemically crosslinked PEG-based hydrogels is that their physical and chemical properties can be modulated by varying the molecular weight of the PEG chains and varying the initiator concentration. For example, increasing the molecular weight of the
20 polyethylene oxide backbone increases the network mesh size. The release of a bioactive molecule, such as an enzyme, can be controlled by control of the network density. Therefore, a hydrogel containing PEGs of a weight average molecular weight of 8 KDa would have a higher rate of release of an entrapped drug than a hydrogel containing PEGs of a weight average
25 molecular weight of 3.3KDa.

Optionally, additives can be incorporated into the hydrogels to impart added functionalities, such as bioadhesiveness. For example, hyaluronic acid or polyacrylic acid can be added to the PEG macromer prior to crosslinking to create bioadhesive hydrogels. In another example, an ionic character can
30 be imparted to the crosslinked hydrogels to provide molecular interaction (e.g. ionic bonds) with entrapped drugs to slow down rates of release of drug from the matrix.

PEG-based hydrogels used in biosensors can provide one or more of the following features: (a) a biocompatible, non-biofouling surface appropriate for long-term exposure to biological fluids without compromise of sensor function, (b) a reservoir for glucose oxidase, (c) a matrix that can
5 be incorporated with ionic moieties to enhance entrapment of glucose oxidase, (d) a matrix that can be modulated in terms of its physical and chemical properties (network density, swelling) by varying the molecular weight of the backbone and (e) a matrix that can be rendered bioadhesive by
10 addition of ionic excipients such as chitosan gluconate, polyacrylic acid, poly(amidoamine), poly(ethyleneimine) and hyaluronic acid.

When the hydrogel is formed from a polyethyleneglycol diacrylate (PEGDA) macromer, polymerization, such as UV polymerization, may occur in a mold that contains a pre-loaded scrim page, which provides a support matrix and a handle for the hydrogel. The PEGDA macromer polymerizes
15 only around the circular head portion of the lollipop-shaped page, leaving the tail section of the page hydrogel-free and useful as a handle (*see* Figure 2 and Figure 9).

Optionally, the PEGDA hydrogel includes an acrylate-PEG-NHS (A-PEG-N) reagent (*e.g.* sold by Nektar), which can function as a linker
20 molecule to covalently link an enzyme, such as the GOx enzyme, to the PEGDA hydrogel network.

iii. Vinyl Acetate-Based Hydrogels

Vinyl acetate-based hydrogels, such as n-vinylpyrrolidone/vinyl acetate copolymer, can exhibit features such as transparency, tackiness, non-
25 toxicity, flexibility, and/or hydrophobicity. Vinyl acetate-based hydrogels typically have a good ability to retain moisture and entrap enzymes, such as glucose oxidase, are biocompatible, and adhere well to skin to improve skin-sensor coupling. As reported by Chuang *et al.*, glucose flux sensor using n-vinylpyrrolidone/vinyl acetate copolymer as the hydrogel showed good
30 performance in tracking the plasma glucose levels of a patient with diabetes during a glucose clamping study. Chuang, *et al.*, "Ultrasonic Pretreatment Enables Continuous Transdermal Glucose Monitoring", Presented at the 4th

Annual Diabetes Technology Meeting Held October 28-30, 2004,
(Philadelphia, PA).

iv. Modified Hydrogels

1. Covalently Immobilized Enzymes

5 Optionally, the hydrogels may be modified to include enzymes and/or
humectants. The enzymes and/or humectants may be entrapped by any
suitable means, including covalent bonding and non-covalent
immobilization. Examples of non-covalent immobilization include, but are
not limited to ionic interactions and physical entrapment. Preferably the
10 enzymes are covalently linked to the hydrogel, such as by using a linker
molecule. In one embodiment, particularly suitable for use in a CGM
system, glucose oxidase is covalently immobilized in the hydrogel disc. For
example, covalent immobilization of GOx into a PEGDA network improves
the effective performance of the device by eliminating GOx diffusion
15 (maintaining bioavailability) and/or by stabilizing the enzyme (maintaining
bioactivity). The PEGDA network provides the structure to contain ~80%
water within its matrix. It acts as an aqueous reservoir to hold vital
components in solution (*e.g.*, buffer salts and osmotic agents), and also
provides a transport medium for the diffusion of the analyte.

20 At a 15% (w/w) PEGDA concentration, most of the GOx can be
retained in the hydrogel by physical entrapment in the mesh. However, at
lower PEGDA concentrations, such as those approaching 10% (w/w), the
more open mesh will not retain GOx, and covalent immobilization is
necessary.

25 *Covalently linking the enzyme to the hydrogel using a linker*

The coupling of the enzyme to the hydrogel may also be
accomplished using a linker. The linker molecule generally contains two or
more functional groups which are able to react with functional groups on the
enzyme and functional groups on the hydrogel. For example, the linker
30 molecule may contain electrophilic groups which react with nucleophilic
groups found in the enzyme and hydrogel, such as hydroxy, thiol, and/or
amino groups. These linkers mediate the conjugation of the enzyme to the

surface of the hydrogel by forming a bond containing a variable number of atoms. The linker molecules can be homofunctional (i.e., the functional groups are identical) or heterofunctional (i.e., the functional groups are different).

5 Suitable linker molecules include, but are not limited to, *N*-Succinimidyl 3-(2-pyridyldithio)propionate (SPDP, 3- and 7-atom spacer), long-chain- SPDP (12-atom spacer), (Succinimidylloxycarbonyl- α -methyl-2-(2-pyridyldithio) toluene) (SMPT, 8-atom spacer), Succinimidyl-4-(*N*-maleimidomethyl)cyclohexane-1-carboxylate) (SMCC, 11-atom spacer) and
10 Sulfosuccinimidyl-4-(*N*-maleimidomethyl)cyclohexane-1-carboxylate, (sulfo-SMCC, 11-atom spacer), *m*-Maleimidobenzoyl-*N*-hydroxysuccinimide ester (MBS, 9-atom spacer), *N*-(γ -maleimidobutyryloxy)succinimide ester (GMBS, 8-atom spacer), *N*-(γ -maleimidobutyryloxy) sulfosuccinimide ester (sulfo-GMBS, 8-atom spacer),
15 Succinimidyl 6-((iodoacetyl) amino) hexanoate (SIAX, 9-atom spacer), Succinimidyl 6-(6-(((4-iodoacetyl)amino)hexanoyl)amino)hexanoate (SIAXX, 16-atom spacer), 1,4-Di-[3'-2'-pyridyldithio]propion-amido]butane (DPDPB, 16-atom spacer), Bismaleimidohexane (BMH, 14-atom spacer), and *p*-nitrophenyl iodoacetate (NPIA, 2-atom spacer). One ordinarily skilled
20 in the art also will recognize that a number of other coupling agents, with different number of atoms, may be used.

Moreover, spacer molecules may be incorporated into the linker to increase the distance between the reactive functional groups at the termini, such as acrylate-polyethylene glycol- *N*-hydroxy succinimide (acrylate-PEG-
25 NHS or A-PEG-*N*). A number of multifunctional PEGs are commercially available from Shearwater Polymers (Huntsville, AL) and Texaco Chemical Co. (Houston, TX). Multi-amino PEGs are available under the name "Jeffamine" and include diamino PEGs and triamino PEGs. In the preferred embodiment, the enzyme is covalently immobilized in the hydrogel using an
30 acrylate-PEG-NHS (A-PEG-*N*).

Covalently linking the enzyme to the hydrogel using a coupling agent

The enzyme can also be coupled directly to the hydrogel by the use of a reagent or reaction that activates a group on the surface of the hydrogel or the enzyme making it reactive with a functional group on the enzyme or hydrogel, respectively, without the incorporation of a coupling agent.

For example, carbodiimides mediate the formation of amide linkages between a carboxylate and an amine or phosphoramidate linkages between phosphate and an amine. Examples of carbodiimides are 1-ethyl-3-(3-dimethylaminopropyl)carbodiimide hydrochloride (EDC), 1-cyclohexyl-3-(2-morpholinoethyl)carbodiimide (CMC), dicyclohexyl carbodiimide (DCC), diisopropyl carbodiimide (DIC), and N,N'-carbonyldiimidazole (CDI). N-ethyl-3-phenylisoxazolium-3'-sulfonate (Woodward's reagent) mediates the formation of amide linkages through the condensation of carboxylates and amines. CDI can also be used to couple amino groups to hydroxyl groups.

15

2. Humectants

In another embodiment, the hydrogel is modified to contain one or more humectants. A humectant is a hygroscopic substance with a strong affinity to form hydrogen bonds with molecules of water. The humectant typically has several hydrophilic groups, such as hydroxyl groups, amines or carboxyl groups. The hydrogel may contain any suitable amount of the humectant to ensure that the hydrogel retains the necessary level of water. Suitable amounts of the humectant in the hydrogel range from 0.1 to 40 % (wt/wt), preferably the amount ranges from 5 to 15% (wt/wt).

Preferably the humectant contains an overall negative charge. Suitable anionic humectants include, but are not limited to, glyceryl triacetate, and negatively charged polyols. Preferred humectants that have been tested include sodium PCA (*i.e.*, a sodium salt of 2-pyrrolidone-5-carboxylic acid) and sodium lactate.

Some small molecule humectants, *i.e.* molecules with molecular weights of less than 1000 Da, may be useful. Examples of useful small-molecule humectants include, but are not limited to, urea, propylene glycol, sodium lactate and sodium pyrrolidone carboxylic acid (PCA).

Some polysaccharide humectants are useful. Examples of useful polysaccharide humectants include, but are not limited to, hyaluronic acid (sodium salt), carrageenan and agarose.

Humectants retain water molecules that would otherwise evaporate from the open system over the period of application. A loss of water in the gel would cause any number of deleterious effects, among them, increased transport resistance, decreased bioavailability of the catalyst that provides the electrical signal (*e.g.* GOx enzyme), loss of interfacial contact area from shrinkage. Any one of the above effects can interfere with device performance.

The humectant improves device consistency by mitigating water loss. Decreased water loss also improves the longevity of the device. As disclosed in Example 2, certain humectants have been shown to prolong device performance (as indicated by decreased signal drift) as compared to a control (without a humectant), while others, such as glycerol and hydroxyethyl urea, were did not increase device performance (as indicated by increased signal drift) as compared to a control (without a humectant) and hence were not beneficial. The preferred humectants increase the performance longevity of a device, while not significantly increasing the error in the readings (such as analyzed by MARD) (*see* Figure 5).

c. Mounting Plate or Target Plate

The mounting plate (102) may have any suitable geometry. The mounting plate connects to the sensor body (101) using standard connectors such as a SLIM/RCPT connector with a latch that mates with a corresponding connector interface that is mounted onto the mounting plate (102). In the wireless system, such as shown in Figure 8A, 8B, and 8C, a target plate (120) is used in place of a mounting plate. Preferably, the mounting plate or target plate is formed from rigid, non-conductive materials with high dielectric constants, such as plastics, which provides firm backing for the sensor body (101) and secure housing for the hydrogel. Suitable materials for the mounting plate include the materials typically used for

printed circuit boards, which not only provide firm backing for the sensor body (101) but also provide printed electrical circuit for the sensor system.

i. Air Pockets or Channels

In one embodiment, the sensor assembly used in the TAMS contains
5 channels or pockets to enable air and/or oxygen to be supplied to the hydrogel or other elements in the sensor assembly that require oxygen to function. One or more air channels and pockets can be located around a hydrogel. The air channels (122) and/or pockets (124) are generally in the form of slits or openings on the mounting plate (102) of a wired system
10 (Figure 1) or the target plate (120) of a wireless system (see Figures 8A and 8B). The channels and pockets not only increase the supply of oxygen (enhanced oxygenation) but also maintain the hydrogel moisture (water). The air channels and pockets can be created by molding, milling, punching, etching or any other mechanical or chemical means.

15 Figures 8A-C show examples of air channels and pockets in the target plate (120) in a wireless TAMS. The wired system (shown in Figures 1 and 2) could be modified in a similar manner to include air pockets and channels. Figure 8A shows a diagram of a rear view of an exemplary glucose sensor's target plate with four air channels (122A, B, C, and D). Figure 8B shows a
20 diagram of a front view of an exemplary glucose sensor's target plate with three cuts (124 A, B, and C) of internal air pockets surrounding the central hole (125) for hydrogel chemistry. Figure 8C shows a diagram of an exemplary wireless sensor housing (126) on top of the target plate (120) to provide an enclosed glucose sensor assembly (112).

25 In one preferred embodiment, the TAMS includes sensors for transdermal analyte detection in which glucose oxidase (GOx, an enzyme) utilizes water and oxygen to convert glucose into hydrogen peroxide (H_2O_2) and gluconolactone. An electrochemical glucose sensor can be designed by using a platinum electrode to break down H_2O_2 and in the mean time
30 generating a continuous electrical current with continuous supply of transdermal glucose flux. If channels or pockets for air or oxygen are included in the sensor assembly, the amount of oxygen supplied to the

hydrogel is increased compared to the same hydrogel in the absence of such air pockets or channels and the hydrogel's moisture level is maintained. This is essential for GOx to convert glucose to hydrogen peroxide, which is subsequently electrochemically oxidized and measured to determine the amount of glucose in the blood.

B. Semi-permeable Membrane

In one preferred embodiment, the TAMS includes a protective, semi-permeable membrane between the surface of the hydrogel and the skin of the user. The protective, semi-permeable membranes can have different pore sizes, composition, charge, reactivity, and thickness. The pores can range from the macroporous (5 μ m) to ultrafiltration (3k) to undefined (NAFION®). "Undefined", as used herein, refers to membranes for which there is currently no standard manner to characterize their pore structure, such as NAFION®. NAFION® contains ionic channels, with sizes ranging from about 1 nm to about 50 nm, depending on the state of hydration

For transdermal analyte monitoring systems, such as CGMs, the attachment of a protective semi-permeable membrane to the outer face of the hydrogel improves the device performance by extending its longevity and reducing contamination of the hydrogel with microorganisms, proteins, cellular material, etc. As an interface between the hydrogel and the porated skin, the membrane can reduce biological contaminants such as proteins, lipids, cellular debris, microorganisms, or combinations thereof.

The protective, semi-permeable membrane can be formed from a variety of polymers, copolymers, or blends thereof. Suitable polymers include hydrophobic polymers such as polytetrafluoroethylene (PTFE); hydrophilic polymers such as Nylon, polyethersulfones (PES), activated PES, (3-mercaptopropyl)trimethylsilane, cellulose acetate, electropolymerized films such as 1,8-diaminonaphthaline and phenylenediamine, and NAFION®-coated PES. NAFION® (tetrafluoroethylene-perfluoro-3,6-dioxo-4-methyl-7-octenesulfonic acid copolymer) is a biocompatible anionic fluoropolymer that can be coated on the hydrogel as a protective layer against physiological contaminants and

biofouling. NAFION® acts as a protective layer based on its hydrophobicity, charge selection, and/or size exclusion.

5 A semi-permeable membrane, such as in the form of a polymeric film, may be coated on an outer surface of the hydrogel layer (106). In general, one or more protective barrier layers may be provided between the hydrogel and the user's skin during operation. The polymer film can be coated on a hydrogel surface using any suitable method, such as by micropipette or by dip-coating the sensor in aqueous or organic polymer solution followed by air drying for several hours before use.

10 In another embodiment, the protective, semi-permeable membrane is attached to only one side of the hydrogel. The interfacial attachment is formed by polymerizing the hydrogel in the presence of the membrane, and forming an Interpenetrating Polymer Network (IPN) in the interfacial region. An IPN is formed when a first polymer (such as a PEGDA hydrogel) is cross-linked in the presence of another polymer network (such as, a
15 polymeric membrane).

In one embodiment, the semi-permeable membrane is negatively-charged (e.g., NAFION®-coated PES) at the hydrogel/skin interface to prevent the loss of negatively-charged components from the hydrogel into
20 the skin. Negatively-charged humectants (e.g., NaPCA) and osmotic agents (e.g., lactic acid) are often included in the hydrogel, and increase the stability of the system.

It is known that protective membranes bind proteins or other biological agents through covalent, electrostatic, hydrophobic, and/or
25 mechanical interactions. As shown by in-house experiments (unpublished) when a membrane was applied between the skin and the hydrogel (during 12-hr *ex vivo* applications), a reduction of protein deposition on the hydrogel was observed. Using extractions and bicinchoninic acid (BCA) protein analysis, an average protein deposition of 32 µg per gel disc was observed
30 without a membrane in place, and an average protein deposition of 14 µg per gel disc was observed when a protective membrane was used.

IV. Methods for Improving Analyte Detection

A. Skin Preparation

In one preferred method of using the TAMS, a skin preparation wipe is applied to the skin prior to application of the TAMS. This skin
5 preparation wipe is used in place of the standard skin hydration procedure currently used in prior art methods. This skin preparation wipe is applied to wipe or clean the surface. It is typically applied to the target skin area by
10 massaging, wiping, padding, rubbing or any other methods to clean the target skin site after a skin pretreatment to increase porosity. This step typically takes a short period of time (as compared to the longer standard hydration
procedures used in the prior art), such as from about 1 to 30 seconds.

The wipe can be formed of a paper, cotton or textile based substrate soaked in agents containing water, phosphate buffered saline, lactic acid, soap, surfactant or any other chemicals, solvents or their mixtures which can
15 be used to clean the target skin area after any skin pretreatment procedure, such as SonoPrep® Ultrasonic Skin Permeation System (Sontra Medical). Preferably, the agents are inorganic or organic solvents such as water, ethanol, isopropanol or a combination thereof. An exemplary formulation of the agent contains 30-95% of isopropanol in water and the wipe material is
20 gauze.

a. Kits

In one embodiment, a kit contains a transdermal analyte detection system and a skin preparation wipe, optionally including wiping reagents such as phosphate buffered saline, lactic acid, soap, surfactant, or a solvent.
25 In one embodiment, the substrate is presoaked with a wiping reagent. In another embodiment, the wiping reagent is provided as a separate component of the kit.

B. Improved Oxygenation of Biosensors

In one preferred embodiment, the sensor assembly is designed to
30 increase oxygen supply to the hydrogel and/or other elements in the sensor assembly that require oxygen to function. Air channels and pockets can be located around a hydrogel. The air channels and pockets are generally in the

form of slits or openings on the mounting plate (102) or target plate (Figure 8). The channels and pockets not only increase the supply of oxygen (enhanced oxygenation) but also maintain the hydrogel moisture (water). Preferably, the mounting plate or target plate is formed from rigid, non-
5 conductive materials with high dielectric constant, such as plastics, which provides firm backing for the sensor body and secure housing for the hydrogel. The air channels and pockets can be created by molding, milling, punching, etching or any other mechanical or chemical means.

IV. Methods of Use

10 The TAMS described herein can be used to monitor biological analytes, for example glucose blood concentrations of a user and/or to deliver therapeutic compounds, as needed. The TAMS is applied to an area on the skin of an animal; typically the animal is a mammal, and in the preferred embodiment the mammal is a human.

15 For example, a prediabetic or diabetic person can use the device to monitor their glucose blood concentration levels and deliver insulin as needed depending on those concentration levels. The insulin can be delivered by the user or by the device. Other analytes can also be monitored.

20 Continuous glucose monitoring can measure the blood concentration of glucose without relying on accumulation of body fluids in the sensor device. In continuous glucose monitoring, for instance, one may prefer to minimize accumulation of both glucose and hydrogen peroxide in the hydrogel so that the current measured by the electrochemical sensor is reflective of the glucose flux through the permeable region of skin in real-
25 time. This advantageously permits continuous real-time transdermal glucose monitoring.

To use the transdermal analyte monitoring systems described herein, first, a region of skin on the user is made more permeable using any suitable method. Typical methods for increasing the skin's permeability include tape
30 stripping, rubbing, sanding, abrasion, laser ablation, radio frequency (RF) ablation, chemicals, sonophoresis, iontophoresis, electroporation, application of permeation enhancing agents. For example, the skin pretreatment

procedure can be the application of low energy ultrasound (e.g. SonoPrep® Ultrasonic Skin Permeation System) or controlled skin abrasion.

When a wireless TAMS is used, typically, the target plate (120) is placed on the skin at the site for increased permeability. Then the skin pretreatment procedure is applied. This method is particularly suitable for use with SonoPrep® as the skin permeation system.

In the preferred embodiment, after the skin pretreatment step, the treated skin is cleaned, such as by wiping or rubbing the treated area of the skin with a skin preparation wipe for a short period of time, such as from about 1 to 30 seconds.

Then the sensor assembly, such as that shown in Figure 1 (wired system) or Figure 9 (wireless system), is attached to the permeable region (107) of skin so that semi-permeable membrane (not shown in Figure 1) is in contact with the permeable skin. When a wireless TAMS is used, typically, the hydrogel and sensor are placed in the target plate and aligned with the center hole (125). Then the sensor housing (126) is attached and connected to the target plate (120) to form the complete sensor assembly (112).

An analyte may be extracted through the treated, permeable region (107) of the user's skin, and pass through the semi-permeable membrane so that it is in contact with the hydrogel disc (106) of the sensor assembly (101).

For example, an analyte, such as glucose, may be transported by diffusion through the semi-permeable membrane and into the hydrogel disc (106) where it can contact glucose oxidase. The glucose then reacts with the glucose oxidase present in the hydrogel disc (106) to form gluconic acid and hydrogen peroxide. Next, the hydrogen peroxide is transported to the surface of the electrode in the sensor body (101) where it is electrochemically oxidized. The current produced in this oxidation is indicative of the rate of hydrogen peroxide being produced in the hydrogel, which is related to the amount of glucose flux through the skin (the rate of glucose flow through a fixed area of the skin). The glucose flux through the skin is proportional to the concentration of glucose in the blood of the user.

The signal from the sensor assembly can thus be utilized to continuously monitor the blood glucose concentration of a user by displaying blood glucose concentration on the potentiostat recorder (108) in a continuous, real-time manner.

5 In principle, any sensor which utilizes the working electrode (201), the counter electrode (202) and the reference electrode (203) to measure hydrogen peroxide can be built in the same way. Examples are biosensors for glucose, lactate or any others using oxidase enzyme incorporated in the hydrogel (106). The electrochemical sensor is preferably operated in
10 potentiostat mode during continuous glucose monitoring. In potentiostat mode, the electrical potential between the working and reference electrodes of a three-electrode cell are maintained at a preset value. The current between the working electrode and the counter electrode is measured. The sensor is maintained in this mode as long as the needed cell voltage and
15 current do not exceed the current and voltage limits of the potentiostat. In the potentiostat mode of operation, the potential between the working and reference electrode may be selected to achieve selective electrochemical measurement of a particular analyte or analyte indicator.

 Other operational modes can be used to investigate the kinetics and
20 mechanism of the electrode reaction occurring on the working electrode surface, or in electroanalytical applications. For instance, according to an electrochemical cell mode of operation, a current may flow between the working and counter electrodes while the potential of the working electrode is measured against the reference electrode. It will be appreciated by those
25 skilled in the art that the mode of operation of the electrochemical sensor may be selected depending on the application.

Examples

**EXAMPLE 1: The use of a protective semi-permeable membrane to form a hydrogel/membrane composite, and improve TAMS
30 performance.**

 The following membranes were tested: [a] Uncoated Polyether sulphone (PES): symmetric with pore sizes of 0.2, 1.2 and 5.0 μm ;

asymmetric with pore sizes of 0.3, 1.0 and 2.0 μm , [b] Nafion[®]-coated PES: each of the 6 different PES pore sizes listed above were also tested with a Nafion[®] coating, [c] Activated PES with aldehyde functional groups (with pores of 0.45 μm), [4] Amphoteric and cationic Nylon 66 (with pores of 0.2 μm), [d] Ultrafiltration membranes: Regenerated Cellulose (RC) with 3.5k MW cutoff; PES with 10k MW cutoff [e] Nafion 1135 sheet, with ~ 35 nm ionic channels.

Formation of a hydrogel/membrane composite: the membrane was cut out as a disc, soaked in buffer and placed at the bottom of the polymerization mold; the scrim page was placed over the membrane; polymer solution was syringed into the mold cavity; the mold was exposed to UV light to form the polymer.

For membranes formed from Nafion[®]-coated PES, the PES membrane was pre-coated with a Nafion[®] solution using an automated coating machine. The coating parameters included machine speed, coating bar size, Nafion[®] solvent, and number of coats, and varied with the pore size of the PES. The coating parameters affect the thickness of the coat, how deep it sinks into the membrane, its consistency, and its longevity. For example, a light surface coating resulted when 0.2 μm PES was singly coated with 5% Nafion[®] solution (in 45% alcohol) at 8 inches/sec using a #20 bar; a deeper coat resulted with multiple coatings of 5.0 μm PES with 20% Nafion[®] solution (in 80% alcohol) using a #20 bar. The depth of the Nafion[®] coating was determined by dyeing the coated membrane with cationic methylene blue.

Where the pore size of the membrane was smaller than the 3.4k PEG macromer (as with 3k cellulose), a smaller 0.75k PEG macromer was used to connect the membrane to the 3.4k PEG network. In this case, when the PEG macromer (at 3.4k Daltons) could not penetrate the pores of the membrane (at 3k Daltons), a 0.75k PEG macromer was used to form two interconnecting IPNs. The 0.75 PEG macromer was first polymerized within one face of the 3k membrane; subsequently, the 3.4k PEG macromer was

polymerized at the new membrane face that now presented a 0.75k PEG network.

24-hr *ex vivo* studies were run to study the effect of each membrane on the glucose sensor's performance. Subject groups that had either no
5 membrane or various types of membranes were compared. The membrane that increased the longevity of the device, without increasing MARD error, was determined to be the preferred membrane. Each membrane was applied to the outer surface of the sensor assembly in a CGM device (supplied by Sontra Medical), which was then applied over the sonicated skin of the
10 subject. In response, the device provided an electrical signal, in nanoamperes (nA), which was calibrated to the blood glucose (BG) of the subject, using a finger-stick blood glucose meter. Throughout the course of the *ex vivo* study (24 hours in length), finger-stick BG samples were taken during the waking hours, at hourly intervals, or at 15-minute intervals near
15 meal times, and were correlated to the signal of the device. Analysis of this correlation provides information about device accuracy, consistency and effective length of performance.

In general, the addition of any membrane to the hydrogel prolonged the use life of the glucose sensor. As shown in Figure 3, in *ex vivo*
20 applications without membranes, only 55% of the subjects had any 24-hr response; with the membrane, 83% of the subjects had a 24-hr response (*see* Figure 3).

There was a difference among membranes, and the criteria used to select the best membrane was the one with the lowest signal drift over 24
25 hours, while still providing good signal correlation (in nA to BG) (i.e. no significant increase in MARD error). A Nafion® coated PES membrane with 5.0 μm pores was determined to be the best candidate because it demonstrated the lowest signal drift of ~ 54% over 24 hrs, and acceptable MARD (*see* Figure 4).

EXAMPLE 2: The inclusion of a humectant in the hydrogel buffer to mitigate water loss, and to improve device performance.

A series of experiments was conducted including various humectants in the hydrogel. Two categories of humectants were tested. The first
5 category contained small-molecule humectants, generally natural moisturizing factors (NMFs), and the second category contained polysaccharides. The following small-molecule humectants were tested: glycerol, urea, hydroxyethyl urea, propylene glycol, sodium lactate (Na
10 lactate) and sodium pyrrolidone carboxylic acid (Na PCA). The following polysaccharide humectants were tested: hyaluronic acid (sodium salt), carrageenan and agarose.

For the small-molecule humectants, each humectant was dissolved in the polymer solution before polymerization. The particular concentration of humectant in the polymer solution was also maintained in the hydrogel
15 buffer. This prevented a humectant concentration gradient that could promote humectant diffusion loss during rinsing and storage.

For the polysaccharide humectants, the same general approach was used as described above for small-molecule humectants. However, certain candidates such as agarose and isolated carrageenan types needed heating for
20 proper solubility, and cooling for gel formation. The PEGDA concentration was dropped to 10 % to increase the polysaccharide solubility.

Screening experiments were first performed to select the best candidates for limited *ex vivo* experiments. Screening experiments involved solubility and drying rate comparisons.

25 24-hr *ex vivo* studies were run to study the effect of each humectant on the glucose sensor's performance. Subject groups that had either no humectant or various types of humectants were compared. The humectant that increased the longevity of the device, without increasing MARD error, was determined to be the preferred humectant. The *ex vivo* experiments
30 involved the application of the device to volunteers for 24 hrs, and then comparing the longevity performance when different humectants were included

Similar to the Example 1, the goal of humectant inclusion study was to prolong the device performance. The results of the test are provided in Figure 5. While many of the humectants showed some promise, including sodium lactate, carrageenan, and agarose, Na PCA consistently provided the lowest signal drift (see Figure 5). Also, when Na PCA was paired with Nafion®-coated PES membranes, there was no water loss over the course of the 24-hr *ex vivo* studies. Data collected from 27 subjects show an actual water gain of 2%. However, typically, there was a water loss for 24-hr studies. In a comparable group of 36 subjects without Na PCA in the study, an average water loss of 19% was observed.

EXAMPLE 3: Covalent immobilization of glucose oxidase (GOx) within a PEGDA hydrogel

A series of experiments was conducted to establish a practical enzyme immobilization strategy. An acrylate-PEG-NHS (A-PEG-N) reagent (Nektar) was chosen as the linker or immobilization reagent. Parameters of concern included the ratio of immobilization reagent to enzyme, reaction sequence, and incubation time.

A pre-polymerization step for incubation of the acrylate-PEG-NHS (A-PEG-N) immobilization reagent to the enzyme was used. 3% GOx was dissolved in the polymerization buffer, and an excess of A-PEG-N at a molar ratio of 7 to 1 was added. A molar ratio of 7 to 1 was chosen to ensure conjugation, without interfering with enzyme activity. The solution was left to incubate overnight at 4°C (a reaction time of 3 hours at room temperature was also effective). PEGDA was added per usual the next day to complete the polymer solution, followed by UV curing.

Evidence that the covalent immobilization was successful was provided by 10% PEGDA polymers containing 3% GOx. Without covalent immobilization, the GOx leached out of a hydrogel disc when placed in a rinse buffer solution, and turn the solution distinctly yellow (UV absorbance at 460 nm = 0.16). With covalent immobilization, the rinse solution did not turn yellow (UV absorbance at 460 nm = 0.02).

Evidence that the enzyme was still active after covalent immobilization was provided by potentiostat testing, which showed no significant differences in responses to a glucose challenge: ~700 nA for the control system, and ~650 nA for the covalently immobilized system.

5 After the covalent immobilization parameters were established, *ex vivo* experiments were conducted to determine if the consistency of the readings by the system had been improved. The *ex vivo* experiments involved the application of the device to volunteers for 4 hrs, and then comparing the performance to a device without covalent immobilization, by
10 performing statistical analysis and calculating the r^2 and MARD values.

In a 4-hr comparative study of *ex vivo* device performance for covalently immobilized GOx vs. non-covalently immobilized GOx, the covalently immobilized GOx system provided better tracking (nA to BG correlation). The results of this study are shown in Figure 6. As shown in
15 Figure 6, after the adoption of the covalently immobilized GOx, *ex vivo* studies provided more consistent tracking, with an r^2 of 0.68, and an MARD of 12.27. In contrast, for the system with non-covalently immobilized GOx, the r^2 value was 0.41, and the MARD was 20.44.

**EXAMPLE 4: Skin preparation procedure for transdermal analyte
20 detection**

A target plate was first applied to the skin. Then, SonoPrep® was applied to the skin site through the target plate. SonoPrep® was then turned on for a period of one second or longer and shut off automatically by the build-in control algorithm of the device. After the skin pretreatment
25 procedure by applying SonoPrep® (Sontra Medical) to increase porosity of the skin, the treated skin site was wiped with a skin preparation wipe. The skin preparation wipe used in this study was gauze pad pre-soaked in 70%/30% of isopropanol/water mixture.

Figures 7A and 7B demonstrate the difference in sensor performance
30 with and without applying a skin preparation wiping procedure on one test subject. As a contrast to the skin preparation wipe procedure, Figure 7C shows the result of the same test subject when a 40-minute hydration

procedure (i.e. prior art procedure) was used. As shown in the figures, wiping the treated skin with the skin preparation wipe shows equivalent performance to 40-minutes skin hydration procedure, and both of these methods perform much better than that without any skin preparation procedure. Removal and/or cleaning of any pore clogging materials by skin preparation wipe is expected to improve transdermal pathways for both analyte extraction and drug delivery.

EXAMPLE 5: Clinical studies with continuous transdermal glucose sensor with three different configurations

10 The glucose biosensor contains an electrochemical sensor and a hydrogel that couple with SonoPrep® ultrasonic permeated skin and continuously draws the glucose into the sensor. The glucose that flows through the skin is consumed by the biosensor as it reacts with glucose oxidase in the hydrogel. This chemical reaction produces a constant electrical signal, which is recorded by the glucose monitor. Due to the enhanced permeation created by SonoPrep and the hydrogel chemistry, the glucose flux detected by the sensor can provide glucose readings through a wireless link every one minute for up to 24 hours. See Figure 9 for schematics of the wireless biosensor system.

20 In each study, the following procedure was used. This procedure is schematically illustrated in Figure 9. First, the target plate was placed on the patient's skin site. Then SonoPrep was applied to the skin site for 5 to 15 seconds (step 1). Then SonoPrep was removed from the target plate. Then the treated skin site was wiped with a skin preparation wipe containing alcohol. Next, the hydrogel and sensor was placed in the target plate (step 2). For each patient, single-use glucose sensors were placed over the SonoPrep treated skin sites. Then the sensor housing was placed over the hydrogel and the sensor assembly was closed (step 3). The sensor was coupled with a miniature analyzer which sent digitized data wirelessly to a monitor for data processing and display (step 3). The glucose sensor signal was referenced to finger stick blood glucose meter readings for Study 1A and Study 1B and to blood glucose was sampled through an IV line for Study 2C.

Table 1 describes the sensor configurations, type of membrane used (if a membrane was present), and type of humectant included in the hydrogel (if a humectant was present) for each of the studies. The sensors used in each of the studies were designed to provide enhanced oxygenation (such as
 5 illustrated in Figures 8A, 8B, and 8C). Additionally, the hydrogels used in each of the studies contained 3% GOx covalently immobilized in 15% PEGDA.

Table 1. Sensor configurations, materials and duration for Each Study

Study #	Sensor configuration	Duration	Membrane	Humectant
1	A	12h	N/A	N/A
1	B	12h	Biodyne B	N/A
2	C	24h	5.0PES.NAF	10% NaPCA

10 ***Study 1 with sensor configuration A***

10 patients with diabetes were tested using the method described above. As noted in Table 1, this study was conducted for 12 hours. The sensor used in this study did not have a membrane over the hydrogel. Additionally, the hydrogel did not contain a humectant.

15 222 data points from this study were analyzed to support development of the blood glucose prediction algorithm. The results are summarized in the Clarke error grid in Figure 10. As shown in Figure 10, the results showed that the sensor could accurately predict blood glucose reading every minute for up to 12 hours with single point calibration after one hour of warm-up
 20 period.

Comparing the biosensor and reference blood glucose measurements, statistical analysis showed the MARD (Mean Absolute Relative Difference) was 12.4%. 98.7% of the data fell in the A+B region of the Clarke error grid with 89.6% in the A region. Excellent data correlation (average $r = 0.87$) was
 25 again demonstrated with this study (see Figure 10). These statistics are summarized in Table 2, along with the statistics for the other studies described in this Example.

Study1 with sensor configuration B

The same study protocol and configuration as in Study1A were used, except that a filter membrane (Biodyne B) was incorporated with the hydrogel. 10 patients with diabetes were tested using the method described
5 above. As noted in Table 1, this study was conducted for 12 hours. The sensor used in this study had a membrane (Biodyne B) over the hydrogel. Additionally, the hydrogel did not contain a humectant.

225 data points were collected from this study. The results are summarized in the Clarke error grid in Figure 11. As shown in Figure 11,
10 the results showed that the sensor could predict blood glucose reading with moderate accuracy, every minute for up to 12 hours with single point calibration after one hour of warm-up period.

Comparing the biosensor and reference blood glucose measurements, statistical analysis showed the MARD (Mean Absolute Relative Difference)
15 was 20.4%. 96.9% of the data fell in the A+B region of the Clarke error grid with 70.7% in the A region. The correlation coefficient between the biosensor and reference blood glucose measurements was 0.64. These statistics are summarized in Table 2, along with the statistics for the other studies described in this Example.

Study2 with sensor configuration C

A 24-hour clinical study was conducted on patients during and after cardiovascular surgery. As noted in Table 1, the sensor used in this study
20 had a membrane (5.0 PES coated with NAFION®) over the hydrogel. Additionally, the hydrogel contained a humectant (10% (wt/wt) Na PCA).

25 During the surgery, the patient's core temperature was brought down to about 20 °C and the patient's heart was put into stop with the aid of a bypass pump for blood circulation. Medication such as insulin and heparin were administrated and blood glucose was sampled through an IV line and analyzed with a blood glucose analyzer.

30 In the first section of the study, it was determined that moisture and betadine (a disinfectant used to prepare the skin prior to surgery) adversely affected the sensor and resulted in device failure. Temporary modifications

to the device configuration and installation procedure (e.g. avoid skin area with betadine) were then implemented to address those issues.

In the second section of the study after the device modification, 10 patients enrolled and nine completed the study. 147 sensor-blood glucose data points were collected and analyzed with the same glucose prediction algorithm developed in Study 1A.

The results are summarized in the Clarke error grid in Figure 12. As shown in Figure 12, the results showed that the sensor could accurately predict blood glucose reading every minute for up to 24 hours, during and post operation.

Comparing the biosensor and reference blood glucose measurements, statistical analysis showed the MARD was 11.2%, and 100% of the data fell in the A+B region of the Clarke error grid with 86.4% in the A region. This study illustrates that with proper device configuration and installation a transdermal glucose monitor can also provide accurate continuous glucose reading for up to 24 hours, even in a surgical ICU setting.

Table 2. Summary table for Statistical Analysis in Clinical Studies

Study #	Setting	# of Subj.	Device config.	# of calibration	Statistics		
					(A+B)% in CEG	MAR D	R2
1	Diabetes	9/10	A	1	98.7	12.4%	0.77
	12h		B	1	96.9	20.4%	0.64
2	Surgical ICU, 24h	9/36	C	2-3	100	11.2%	0.83

20

Those skilled in the art will recognize, or be able to ascertain using no more than routine experimentation, many equivalents to the specific embodiments of the invention described herein. Such equivalents are intended to be encompassed by the following claims.

THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:

1. A transdermal analyte monitoring system comprising:
a sensor assembly, wherein the sensor assembly comprises a hydrogel and a
5 sensor body containing a plurality of electrodes, wherein the sensor body is in fluid
communications with the hydrogel, wherein the hydrogel comprises a humectant and
an enzyme and wherein the humectant is in an effective amount to increase the
performance longevity of the transdermal analyte monitoring system, as indicated by
decreased signal drift, compared to the same system in the absence of humectant.
10
2. The transdermal analyte monitoring system of claim 1, further comprising a
semi-permeable membrane, wherein the membrane is in fluid communication with the
hydrogel.
- 15 3. The transdermal analyte monitoring system of claim 2, wherein the hydrogel
and the semi-permeable membrane form an interpenetrating polymer network.
4. The transdermal analyte monitoring system of claim 1, wherein the hydrogel
comprises a polymer selected from the group consisting of polyethylene glycol
20 diacrylate (PEGDA), agarose, polyethylene glycol diacrylate/polyethylene (PEGDA-
PEI), polyethylene glycol diacrylate-n-vinyl pyrrolidone (PEGDA-NVP), acrylate-
polyethylene glycol – N-hydroxy succinimide (A-PEG-N), and blends and copolymers
thereof.
- 25 5. The transdermal analyte monitoring system of claim 1, wherein the enzyme is
oxidase enzyme.
6. The transdermal analyte monitoring system of claim 1, wherein the enzyme is
covalently immobilized in the hydrogel.
30
7. The transdermal analyte monitoring system of claim 6, the enzyme is covalently
immobilized in the hydrogel using an A-PEG-N.
8. The transdermal analyte monitoring system of claim 1, wherein the humectant is
35 a negatively charged humectant.

9. The transdermal analyte monitoring system of claim 8, wherein the negatively charged humectant is sodium pyrrolidone carboxylic acid (NaPCA).

10. The transdermal analyte monitoring system of claim 1, wherein the sensor
5 assembly comprises at least one channel or picket for providing oxygen to the hydrogel.

11. The transdermal analyte monitoring system of claim 1, wherein the enzyme is immobilized in the hydrogel via non-covalent immobilization.

10

12. A method for increasing analyte detection by a transdermal analyte monitoring system comprising:

(a) treating a region of skin of the user to increase permeability; and

(b) applying the transdermal analyte monitoring system of any one of claims 1

15 to 11.

13. The method of claim 12, further comprising after step (a) and prior to step (b), wiping the treated region of skin with a substrate comprising at least one reagent selected from the group consisting of water, ethanol, isopropanol and glycerol.

20

14. The method of claim 12, wherein the region of skin is treated in step (a) by a method selected from the group consisting of tape stripping, rubbing, sanding, abrasion, laser ablation, radio frequency (RF) ablation, the application of chemicals, sonophoresis, iontophoresis, electroporation, and the application of permeation
25 enhancing agents.

15. The method of claim 13, wherein the substrate is selected from the group consisting of pads, woven and non-woven fabrics, felt and gauze.

30 16. The method of claim 13, wherein the substrate comprises an inorganic or organic solvent.

17. The method of claim 16, wherein the inorganic or organic solvent is selected from the group consisting of water, ethanol, and isopropanol.

35

18. The method of claim 13, wherein the substrate comprises phosphate buffered saline, lactic acid, soap, or a surfactant.
19. The method of claim 12, wherein the analyte to be detected is blood glucose,
5 lactate or other analytes.
20. A kit comprising
the transdermal analyte detection system of any one of claims 1 to 11; and
a substrate comprising phosphate buffered saline, lactic acid, soap, a surfactant,
10 or a solvent.
21. A kit comprising
the transdermal analyte detection system of any one of claims 1 to 11;
a substrate,
15 and a reagent selected from the group consisting of phosphate buffered saline,
lactic acid, soap, a surfactant, and a solvent.
22. A method for enhancing the sensitivity, stability or accuracy of a transdermal
analyte sensor of any one of claims 1 to 11 comprising providing an enhanced supply
20 of oxygen to the hydrogel.
23. The method of claim 22, wherein the source of oxygen is air.

Figure 1

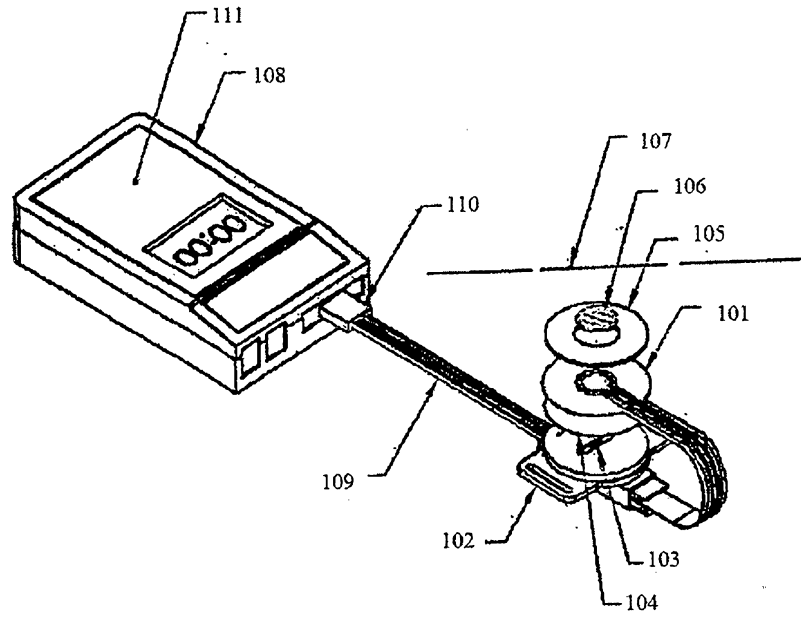


Figure 2

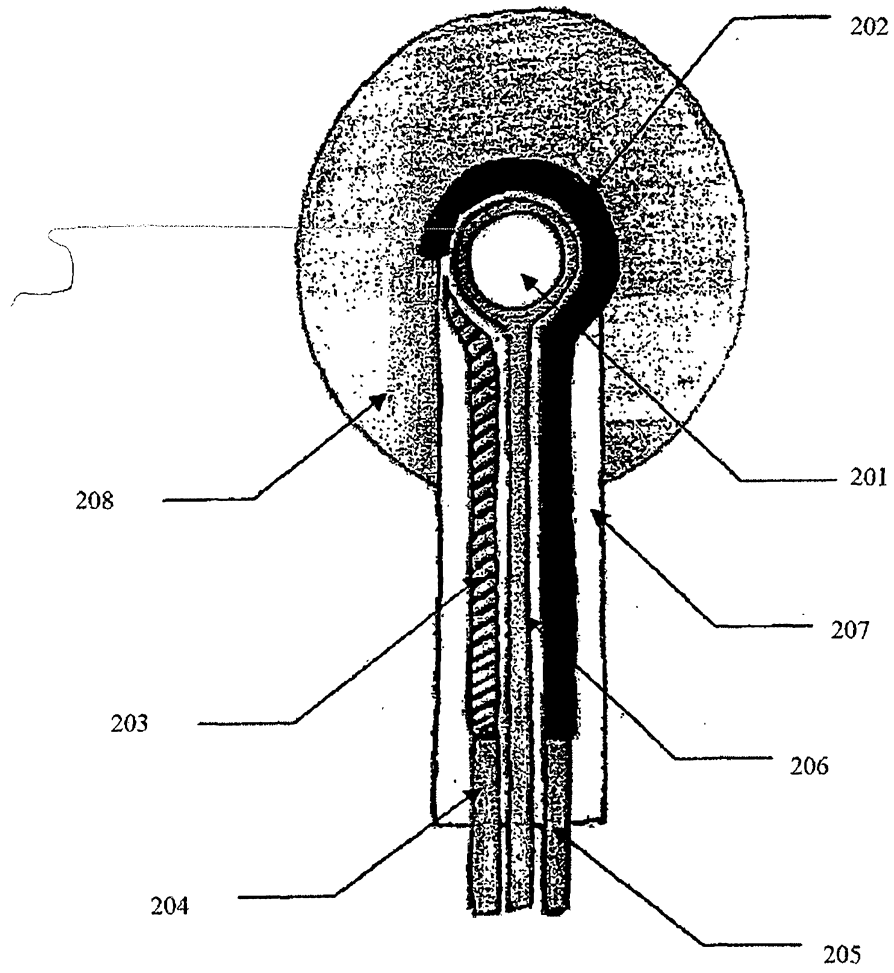


Figure 3

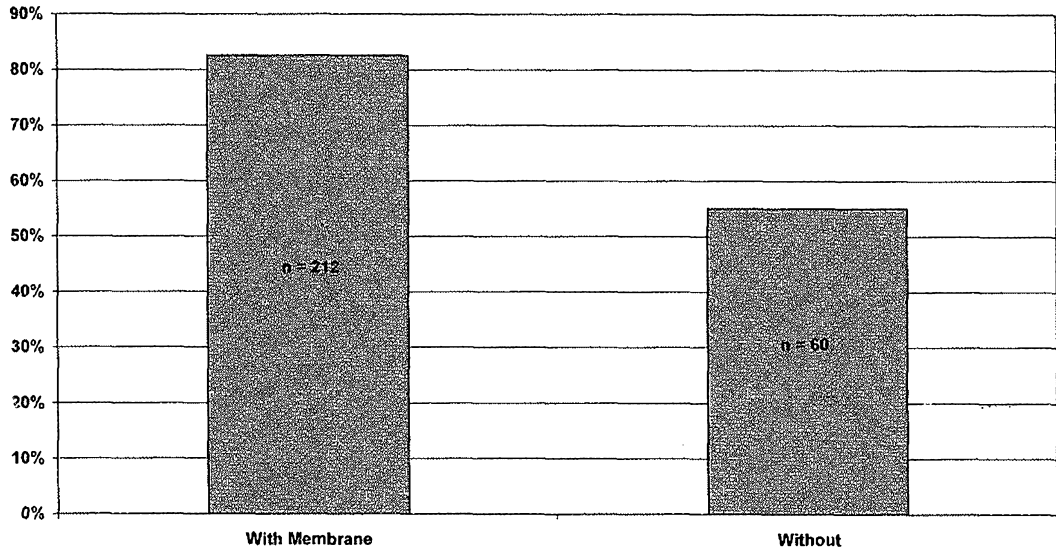


Figure 4

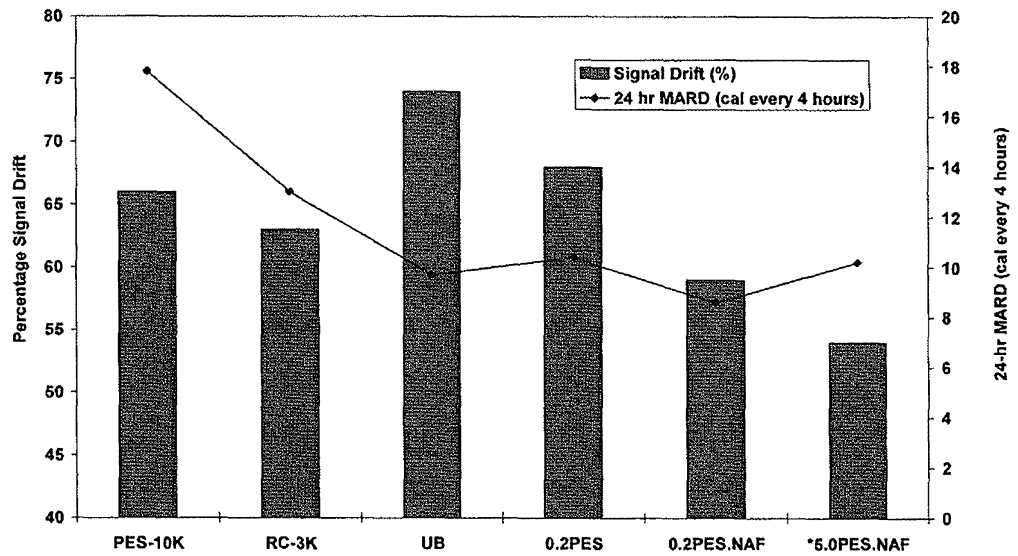


Figure 5

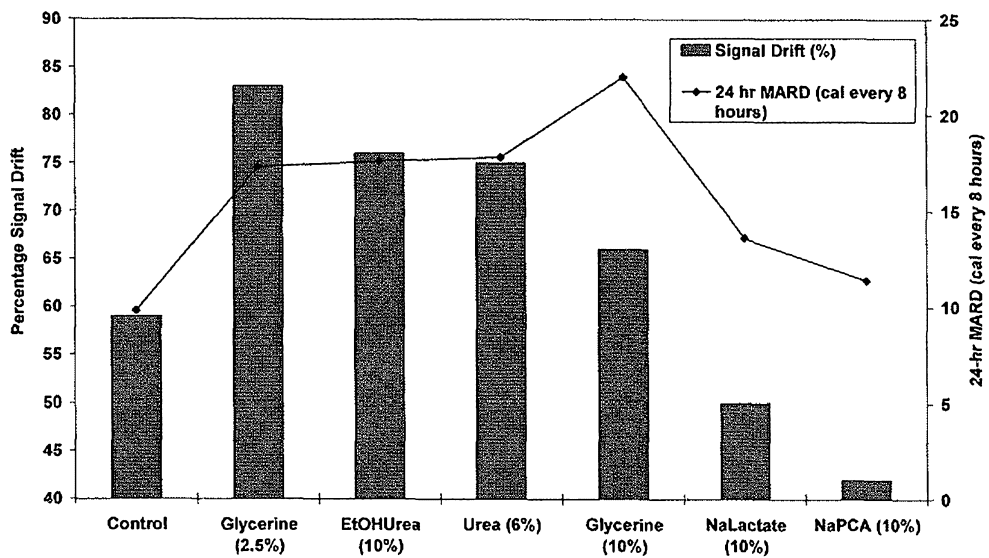


Figure 6

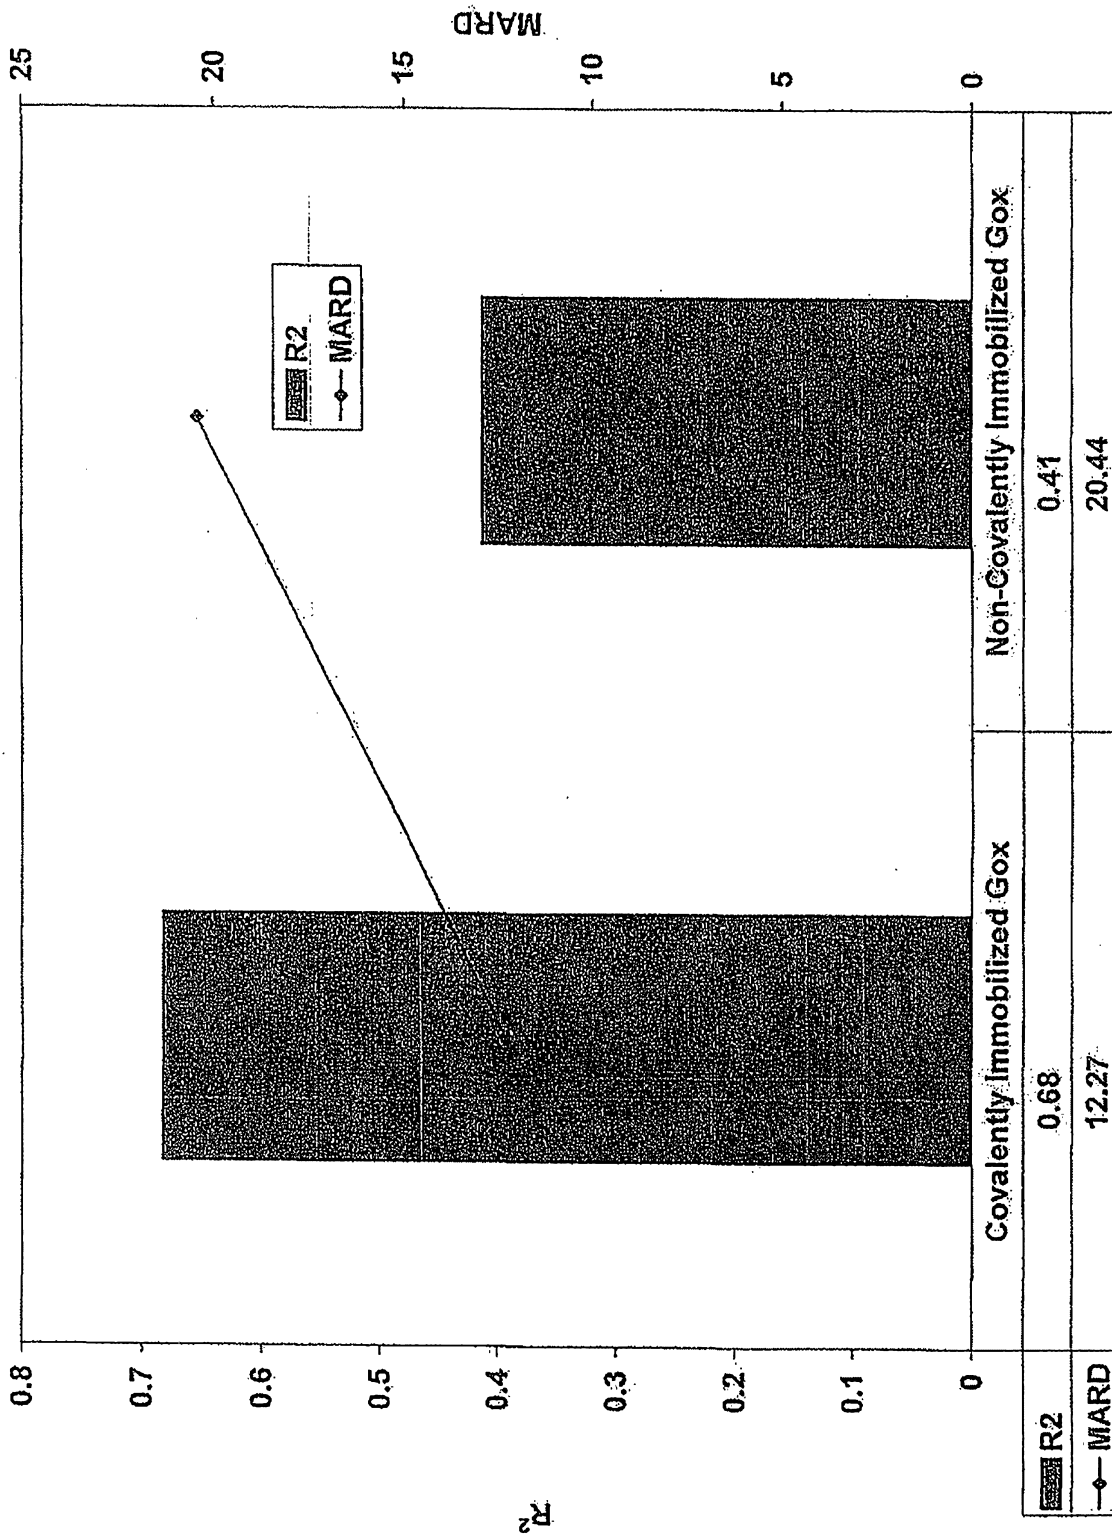


Figure 7A

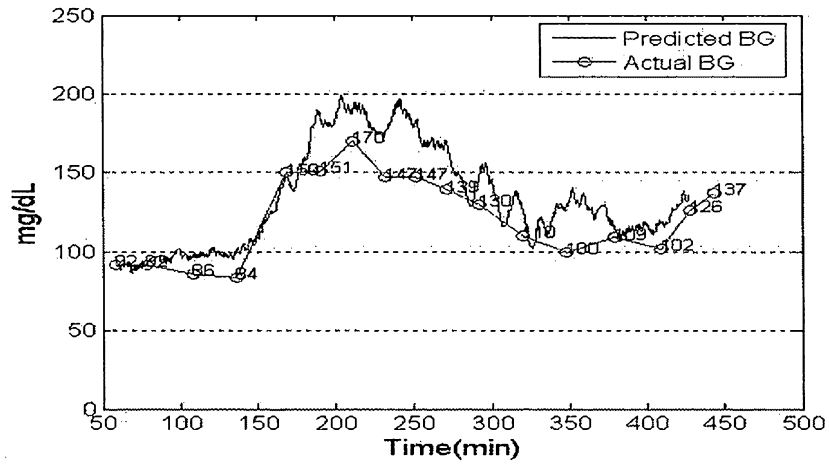


Figure 7B

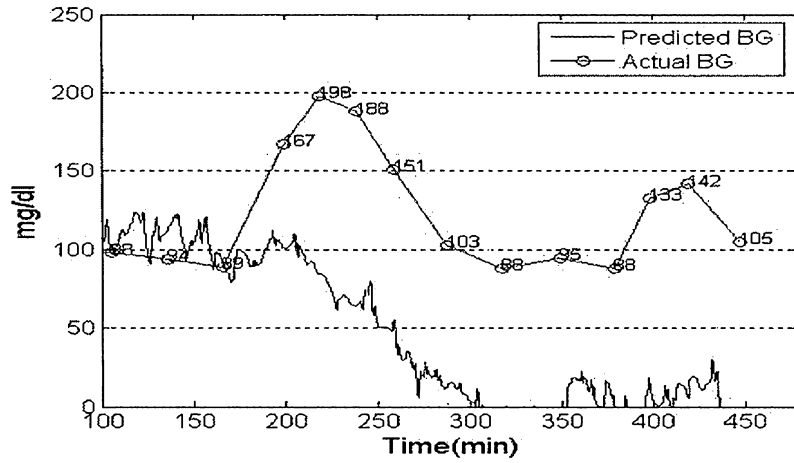
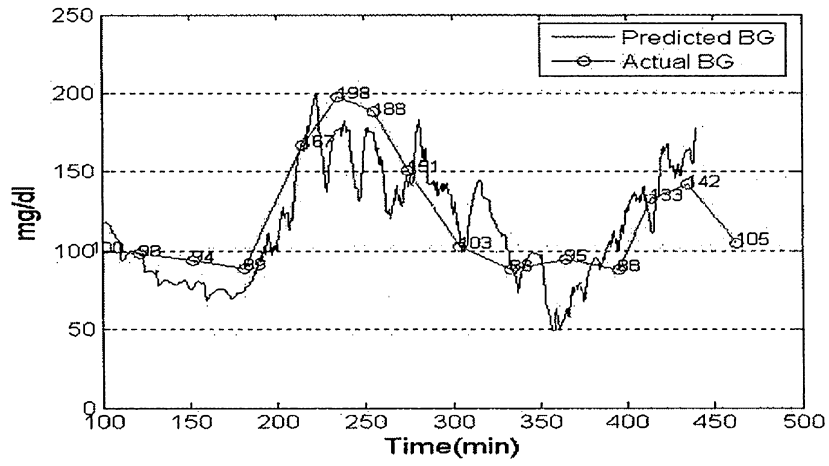


Figure 7C



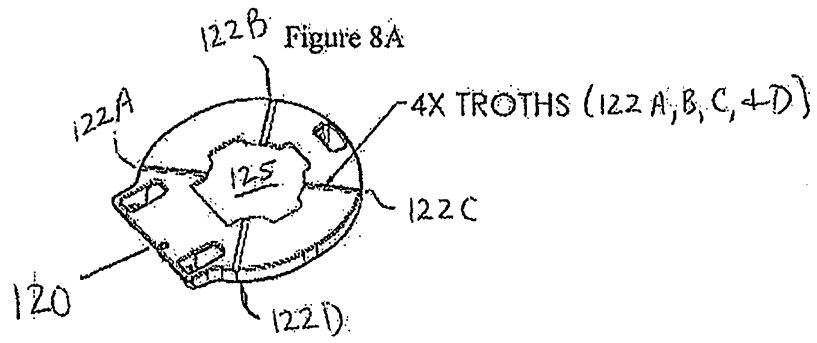


Figure 8A

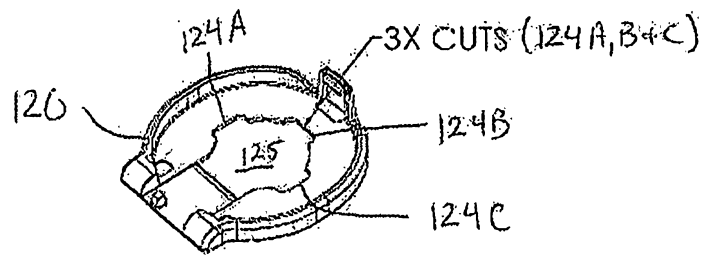


Figure 8B



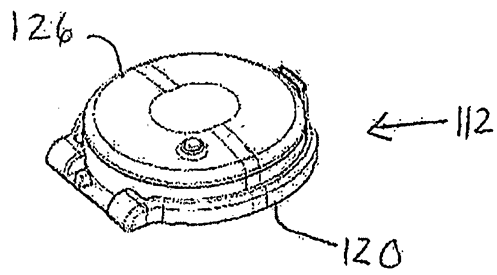


Figure 8C

Fig. 9. Transdermal glucose sensor with wireless communication.

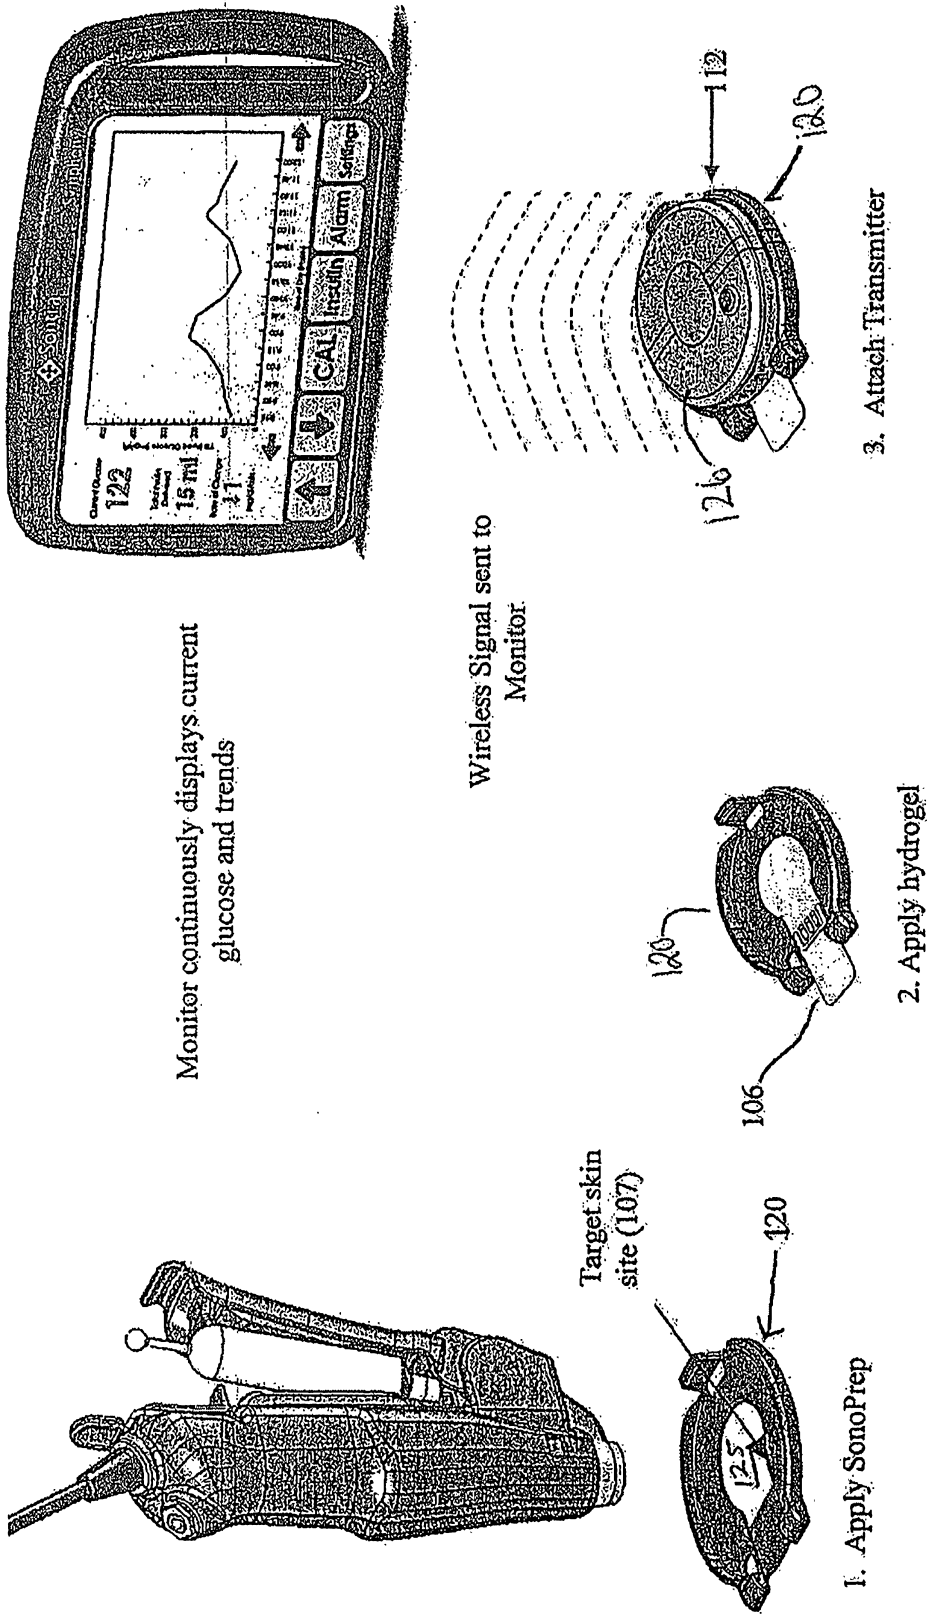

Aggregate MARD 10.74(8h), 12.43(12h),
R2 min/median/max 0.66/0.88/0.98(8h), 0.51/0.77/0.94(12h),

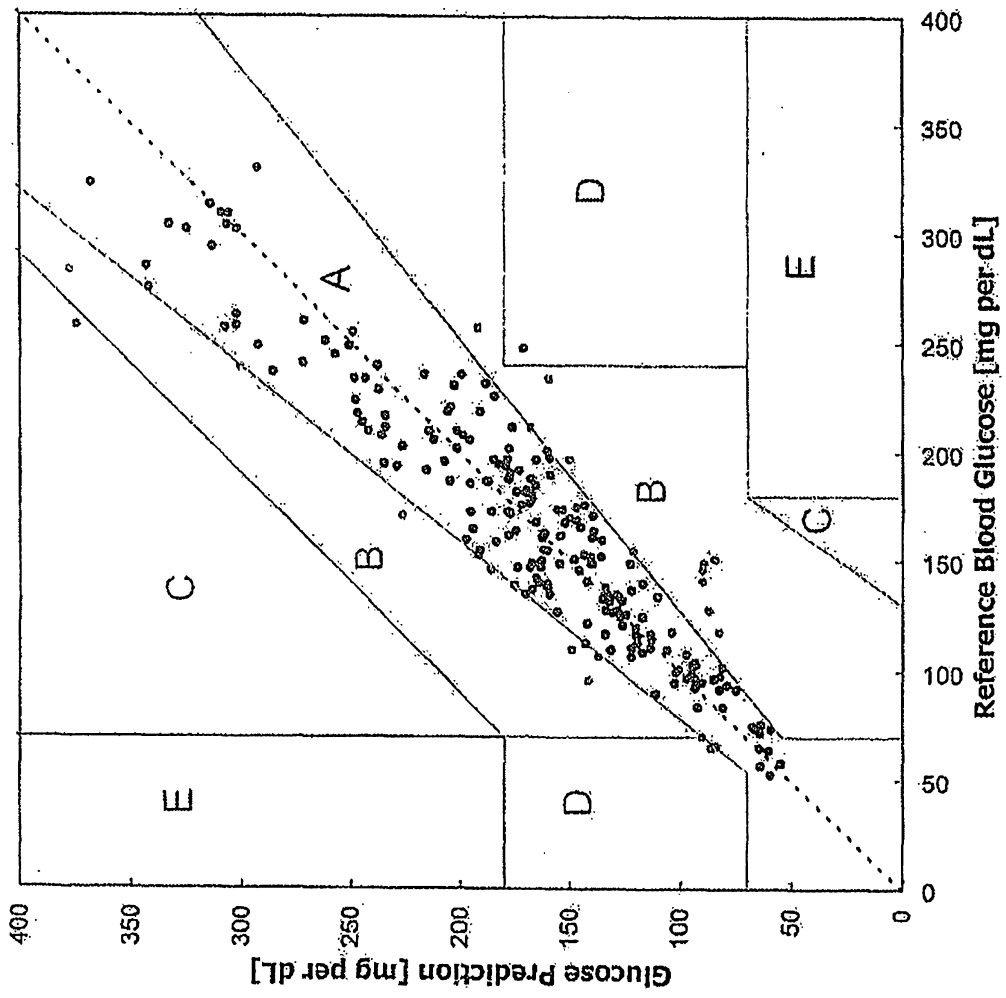

N=222 A 89.64% B 9.01% C 0.45% D 0.90% E 0.90%

Figure 10

Aggregate MARD 17.52(8h), 20.40(12h),
R2 min/median/max 0.25/0.71/0.98(8h), 0.44/0.64/0.87(12h),

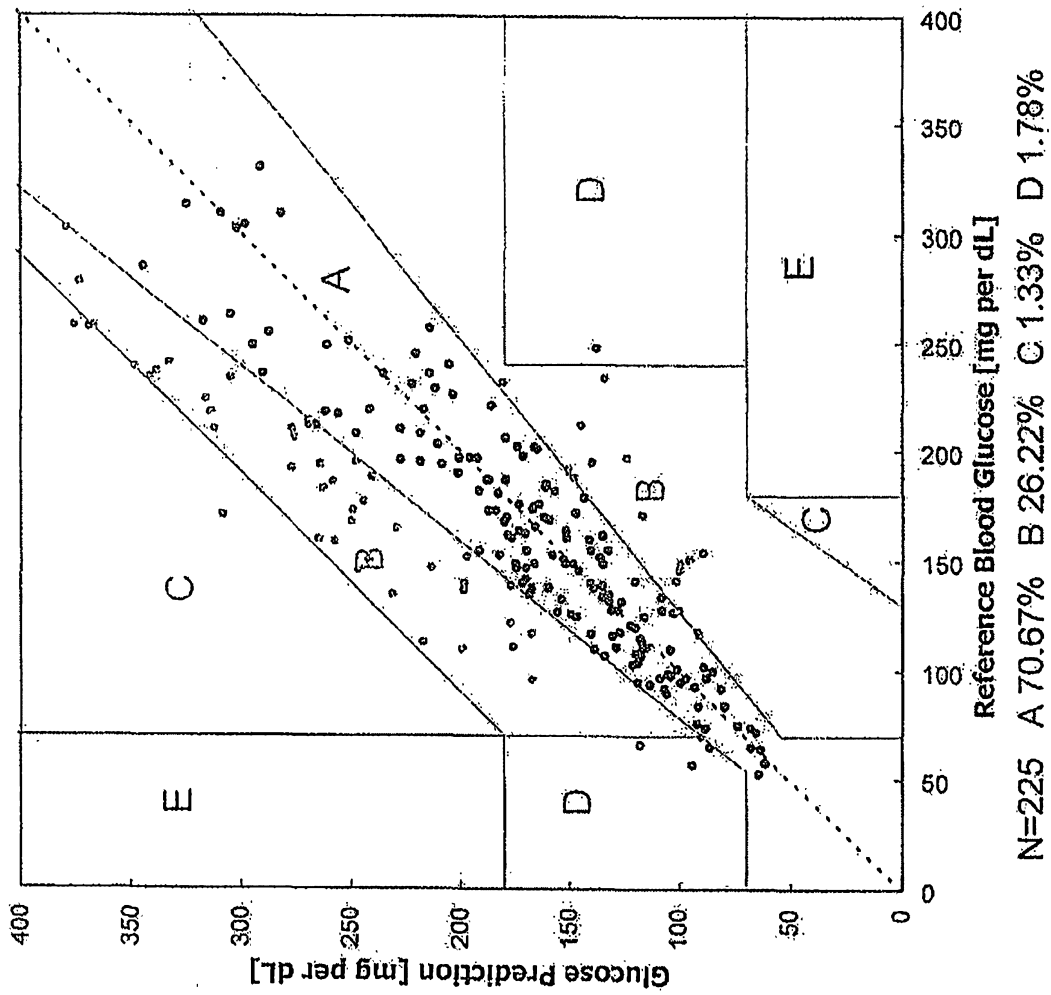


Figure 11

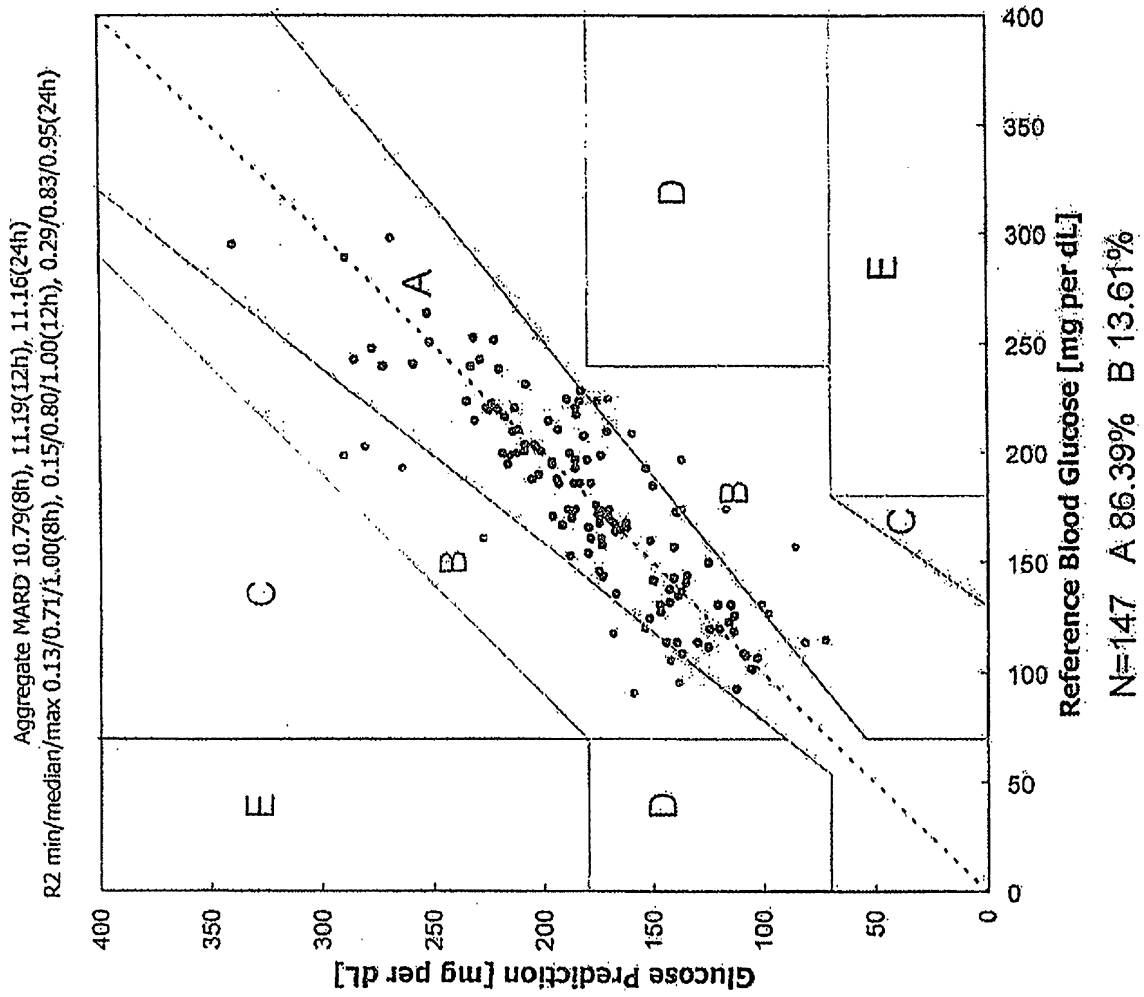


Figure 12