



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : B65D 85/24 // A61M 25/00	A1	(11) International Publication Number: WO 00/47494 (43) International Publication Date: 17 August 2000 (17.08.00)
<p>(21) International Application Number: PCT/SE00/00289</p> <p>(22) International Filing Date: 14 February 2000 (14.02.00)</p> <p>(30) Priority Data: 9900465-7 12 February 1999 (12.02.99) SE</p> <p>(71) Applicant (for all designated States except US): AS-TRAZENECA AB [SE/SE]; S-151 85 Södertälje (SE).</p> <p>(72) Inventors; and (75) Inventors/Applicants (for US only): ISRAELSSON, Anette [SE/SE]; Astra Tech AB, Box 14, S-431 21 Mölndal (SE). PETTERSSON, Agneta [SE/SE]; Astra Tech AB, Box 14, S-431 21 Mölndal (SE). UTAS, Jan [SE/SE]; Astra Tech AB, Box 14, S-431 21 Mölndal (SE).</p> <p>(74) Agent: AWAPATENT AB; Box 11394, S-404 28 Göteborg (SE).</p>		<p>(81) Designated States: AE, AL, AM, AT, AT (Utility model), AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, CZ (Utility model), DE, DE (Utility model), DK, DK (Utility model), DM, EE, EE (Utility model), ES, FI, FI (Utility model), GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KR (Utility model), KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SK (Utility model), SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p>Published <i>With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i></p>
<p>(54) Title: STORAGE PACKAGE AND A METHOD FOR PACKAGING</p> <p>(57) Abstract</p> <p>A storage package (1) contains a medical device (7) having a coated surface (8) which exhibits a reduced friction when wetted with a wetting liquid and a supply of the wetting liquid (9). The package is adapted such that the coated surface of the medical device is maintained contact with the supply of wetting liquid during storage. A good shelf-life for the medical device is achieved and where the medical device is a urethral catheter the catheter is immediately "ready-for-use" after the package has been opened.</p> <div data-bbox="954 1249 1407 2065" data-label="Image"> <p>The diagram shows a cross-section of a storage package (1) containing a medical device (7). The device has a coated surface (8) and is surrounded by a supply of wetting liquid (9). The package is shown in two states: closed (left) and open (right). The device is a long, thin, tapered object, likely a catheter, with a central lumen. The coating (8) is on the outer surface of the device. The wetting liquid (9) is contained within the package, surrounding the device. The package (1) has a top opening (3) and a bottom opening (5). The device (7) is shown in a retracted position (left) and an extended position (right). The coating (8) is shown in a cross-section, indicating its thickness and adherence to the device. The wetting liquid (9) is shown as a liquid layer between the device and the package walls.</p> </div>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon	KR	Republic of Korea	PL	Poland		
CN	China	KZ	Kazakstan	PT	Portugal		
CU	Cuba	LC	Saint Lucia	RO	Romania		
CZ	Czech Republic	LI	Liechtenstein	RU	Russian Federation		
DE	Germany	LK	Sri Lanka	SD	Sudan		
DK	Denmark	LR	Liberia	SE	Sweden		
EE	Estonia			SG	Singapore		

STORAGE PACKAGE AND A METHOD FOR PACKAGINGField of the Invention

The present invention relates to a storage package which contains a medical device having a coated surface which exhibits a reduced friction when wetted and is particularly, although not exclusively, concerned with a storage package which contains a urethral catheter having an elongate shaft which is provided with a surface coating having reduced friction when wetted. The invention further relates to a method for packaging of such a medical device.

Background of the Invention

Urethral catheters are medical devices having an elongate shaft for insertion into the urethra of a patient for *inter alia* drainage of the urine in the patient's bladder, use in treating cancer of the prostate or delivering a medicament. They may be for in-dwelling in the urethra for a number of days or for intermittent self-catherisation.

A fairly recent development in the field of urethral catheters has been the formation on the elongate shaft of a surface coating which exhibits a reduced friction when wetted to facilitate insertion into the urethra. The need for facilitating the insertion of the shaft into the urethra will be readily appreciated when one considers that the outer diameter of the shaft of a catheter is typically greater than the inner diameter of the urethra. In the coated catheter this is achieved by soaking the shaft in a wetting liquid such as sterile water or saline immediately prior to insertion to make the shaft surface slippery. Prior to the development of coated catheters the elongate shafts were simply formed by uncoated plastics tubing, for example of PVC, and to facilitate

insertion of the shaft it was necessary to apply to the shaft a lubricant in the form of a jelly or the like which was rather cumbersome and time-consuming. As examples of friction reducing coatings suitable for application to a catheter shaft there may be mentioned the polyvinyl pyrrolidone (PVP) hydrophilic surface coatings made known in EP-B-0 093 093 and EP-B-0 217 771 (Astra AB).

It is important that the packaging used for catheters having friction-reducing surface coatings be such as to provide the catheter with a long shelf-life because the time that a urethral catheter is held in storage prior to use can be rather lengthy. To this end, the catheter packaging needs to ensure that the friction-reducing coating on the catheter is protected, for instance against the environment. The form that the package takes, however, is complicated if the catheter is to be stored after having been subjected to a sterilising process to alleviate the risk of infection of the urinary tract by the catheter as the package will need to maintain the sterile state of the catheter. Such pre-sterilisation of the catheter has the advantage that the catheter will not need to be sterilised after the catheter storage package is opened and is especially useful when the catheter is a disposable or single-use catheter. A typical pre-sterilising process for surface coated urethral catheters involves exposing the catheter to ethylene oxide gas.

Paper packaging has hitherto been proposed for storing a surface coated urethral catheter which is to be pre-sterilised by ethylene oxide gas because the gas can pass through a paper construction. Thereby, the catheter can be placed in the package and subsequently be exposed to the sterilising gas. To this end, it is conventional for the paper packaging to be formed from a paper construction in which the paper is grid-lacquered with polyethylene and welded around its edge to a laminate of,

for example, polyethylene-polypropylene, polyethylene-polyethylene terephthalate or possibly polyethylene-nylon. A problem encountered with such paper packages, however, is that moisture can ingress into the package during storage. If moisture penetrates to the paper package, the catheter coating will become sticky leading to the coating becoming damaged, destroyed or mutilated through adherence of the coating to the paper component of the package.

10 WO96/30277 (Coloplast A/S) discloses a catheter storage package where the problem of adherence of coated catheters to paper packaging is solved by inserting a plastics material adjacent to the interior surface of the paper so that the catheter cannot come into direct
15 contact with the paper. To still enable ethylene oxide gas to gain access to the catheter surface the plastics material is provided with a number of slits. The drawback of this type of catheter package, however, is that it needs a complicated manufacturing process because the
20 dimensions of the slits in the plastics material have to be carefully regulated so that they do not permit contact of the catheter surface with the paper without in anyway hindering access of the sterilising gas.

WO97/47349 (Astra AB) proposes a solution to this
25 drawback associated with packages of the type disclosed in WO96/30277 by placing a coated urethral catheter in an inner container formed from a material which is permeable to a sterilising agent such as ethylene oxide gas, exposing the inner container to the sterilising agent and
30 then enclosing the inner container in an outer container which is formed from a material which prevents access of moisture to the inner container. This "double pack" arrangement keeps the coating of the catheter sterile and dry until it is required to be used thereby overcoming
35 the problem of the catheter coating becoming sticky due to contact with moisture and then becoming damaged due to adherence with the packaging.

A drawback of the package disclosed in WO97/47349 and the other aforementioned packages is that they do not include a supply for wetting liquid for wetting of the catheter coating prior to use of the catheter. For instance, in the case of the package disclosed in WO96/30277 the catheter coating is wetted by partially opening the package and then introducing sterile water or saline solution into the enclosure containing the catheter. In the case of the package of WO97/47349, on the other hand, the catheter is removed from the package and then soaked in sterile water or saline. Further, a problem with all the above mentioned packages are that the user needs to have access to clean water.

WO97/26937 (Astra AB) discloses a package which includes a supply of sterile wetting liquid in combination with a coated catheter. In this package a coated bladder drainage catheter is positioned in a urine collection bag together with a sealed wetting liquid container, containing sterile wetting liquid. This arrangement is then exposed to ethylene oxide gas to sterilise the catheter and surfaces of the bag and container and subsequently enclosed in a moisture proof outer casing for storage. In use, the outer casing is removed and the wetting liquid container ruptured to release the sterile wetting liquid contained therein into the bag for the catheter to soak in for wetting of the surface coating. The duly wetted catheter is then projected through a removable section of the bag into the urethra with urine drained from the bladder being captured in the collection bag.

As will be appreciated by the foregoing, the development of the prior-art storage packages for a catheter having a friction-reducing surface coating has been in the direction of keeping the coating dry during storage. The present invention is based on the insight that the real problem is not the coating coming into contact with moisture *per se* but more the cyclical effect

of the coating coming into contact with moisture and then drying out.

WO98/19729 (Coloplast A/S) discloses a ready-to-use storage package. The storage package according to this publication is formed by wetting the hydrophilic coating of the catheter with a wetting liquid prior to its encapsulation in the storage package. The walls of the storage package are formed from a gas impermeable material which prevents drying out and keeps the hydrophilic coating wet and "ready-to-use". However, in this ready-to-use package a very limited amount of wetting liquid is supplied. When the catheter is wetted before placing it in the storage package the amount of water is naturally limited only to the amount adopted by the hydrophilic surface, and even in the embodiment where the wetting liquid is supplied after the placement of the catheter in the package, the amount of wetting liquid is limited only to the amount needed for the preparation of the hydrophilic surface of the catheter.

Summary of the Invention

According to the present invention there is provided a storage package which contains a medical device having a coated surface which exhibits a reduced friction when wetted with a wetting liquid and a supply of the wetting liquid. The storage package is characterized in that, during storage, the coated surface of the medical device is constantly maintained in direct contact with said wetting liquid.

The storage package of the present invention therefore differs from that taught in WO98/19729 in that the medical device is maintained in direct contact with the wetting liquid. A problem with the catheter according to WO 98/19729 is that the possibilities for sterilisation are limited. This problem will be discussed more in detail below.

With the present invention there is no need for the coating on the medical device to be subjected to a

wetting step after the package is opened since it is kept wet during storage. The package also provides the medical device with a long shelf-life, e.g. 3-5 years, due to the problem of the coating cyclically becoming wet and then
5 drying out through moisture ingress being alleviated.

A further advantage of the package of the invention is that the medical device and the wetting liquid can be steam sterilised. Hereby, both the medical device and the wetting liquid could be sterilised at the same time,
10 which render the sterilisation process faster and more effective. To make a steam sterilisation of the medical device possible it must be of a material having a melting temperature exceeding 100 °C, and preferably exceeding 130 °C, at least in the part where the surface coating
15 (8) is provided. Such suitable materials may be polyurethanes, polyether block amides, silicon rubber, elastomeric alloys such as Santoprene® and polyolefin alloys based on polypropylene or SEBS (Styrene Ethylene Butadiene Styrene). An example of a polyether block amide
20 that could be used for forming the medical device is Pebax® (Elf Atochem S.A.).

The steam-sterilisation technique is preferred, since it has the advantage over ethylene oxide gas and β - or γ -radiation sterilisation that there is no formation
25 or absorption of harmful reaction products in the wetting liquid, in the catheter material or in the catheter surface coating.

More specifically, a problem with using ethylene oxide sterilisation is that an amount of residual
30 ethylene oxide or degradation products are absorbed by the wetting liquid or the medical device, which could be harmful for the user of the medical device. Further, ethylene oxide could only be used for sterilising the medical device, where after the medical device and
35 sterile wetting liquid must be aseptically packaged. However, the provision of such an aseptic environment for the packaging is both expensive and difficult to achieve

in practice. Those problems with the ethylene oxide sterilisation could be overcome by using steam-sterilisation instead.

Further, a problem with β - or γ -radiation sterilisation is that harmful reaction products are likely to be produced in the medical device. The radiation also starts a degradation process in the material of the medical device, which is typically a plastic material or the like, whereby the shelf-life is shortened. Still further, the medical device has to be sterilised either before it is placed in the package together with the wetting liquid or within a short period thereafter. The pre-sterilisation of the medical device is not preferred, since it requires an aseptic packaging environment, as is discussed above. If a non-sterilised object is placed in a sterilised liquid the liquid is pre-contaminated, and the pre-contamination increases over the time. If the pre-contamination becomes too large, the sterilisation process will not be able to sufficiently sterilise the product. Further, a too large pre-contamination gives rise to large, and possibly harmful endotoxine levels. However, it may be difficult to perform the radiation sterilisation within a prescribed time period, since radiation sterilisation equipment is large and expensive, and it not realistic to have a such an equipment on each packaging facility. However, steam-sterilisation equipment are much less expensive. Hence, all the referred problems with radiation sterilisation could be overcome by using steam-sterilisation instead.

However, it should be understood that the invention is not limited to steam-sterilisation, but other sterilisation processes, such as microwave-sterilisation, with similar performance could be used as well.

In an embodiment of the invention the medical device has a shaft for insertion into a body cavity or body passageway which presents the coated surface. Examples of

such medical devices are catheters such as urethral catheters for bladder drainage. The coated surface may be a surface provided with a hydrophilic coating, for example made in accordance with EP-B-0 093 093 and EP-B-0 217 771 *supra* and the wetting liquid may be an aqueous solution.

Where the medical device has a coated shaft for insertion into a body cavity or body passageway the wetting liquid may contain an osmolality-increasing agent such as sodium chloride and/or a pharmaceutically active substance. The wetting liquid could also contain a substance which acts to maintain the catheter and wetting liquid sterile during an extended storage period, for example an anti-bacterial agent.

In an embodiment of the invention the storage package comprises a container within which the coated surface and the wetting liquid are contained. Further, in this embodiment, the container preferably defines a cavity which houses the coated surface and the wetting liquid is contained in the cavity in a volume sufficient for the coated surface to remain constantly wetted thereby during storage. Preferably, the cavity encloses the whole of the medical device. This facilitates the use of steam sterilisation because the wetting liquid will act to provide a uniform sterilisation temperature around the medical device.

The container may be flexible or stiff and is conveniently constructed so as to be impermeable or substantially impermeable to the wetting liquid. The container may, however, be an inner container with the package further comprising an outer container which encloses the inner container. In this case, the inner container need not be of a construction which is totally impermeable to the wetting liquid if the outer container also has good impermeability to the wetting liquid. The inner container could in this instance be made from polyurethane or polypropylene.

According to the invention there is further provided a method for sterile packaging of a medical device having a surface which exhibits a reduced friction when wetted with a wetting liquid, comprising the steps of: providing
5 a container, placing the medical device in the container together with wetting liquid in such a way that it is maintained in contact with the wetting liquid during storage, and sterilising the medical device and the wetting liquid, and sealing the container.

10 According to the invention there is still further provided a ready-to-use urinary catheter assembly comprising a container, said container containing a urinary catheter having a hydrophilic surface layer which exhibits a reduced friction when wetted with a
15 wetting liquid and a supply of the wetting liquid characterized in that, during storage, the whole of the coated surface is constantly maintained in direct contact with said wetting liquid.

20 These and other objects and features of the invention will become more fully apparent from the following description and appended claims.

Brief description of the drawings

25 In the following, the invention will be explained more in detail by way of an embodiment, and with reference to the appended drawings, on which:

Fig 1 shows a storage package according to a first embodiment of the invention; and

30 Fig 2 shows a storage package with an additional outer container according to a second embodiment of the invention.

Description of Exemplary Embodiment of the Invention

35 By way of example, there is shown in the accompanying Figure 1 a steam sterilised catheter storage package 1 in accordance with the present invention comprising a container 3 formed from two overlapping

blanks of material heat sealed together at their periphery to form a central closed cavity 5. The cavity 5 is filled with a sterile aqueous solution 9 and further houses a urethral bladder drainage catheter 7 having a shaft 8 formed from Pebax® on which there is provided a hydrophilic coating in accordance with European patent No. 0093093 or 0217771 *supra*. However, other materials having a melting temperature exceeding 100 °C, and preferably exceeding 130 °C could be used as well, such as polyurethanes, polyether block amides, silicon rubber, elastomeric alloys such as Santoprene® and polyolefin alloys based on polypropylene or SEBS (Styrene Ethylene Butadiene Styrene).

The blanks of material forming the container 3 are made from a construction, which is impermeable or substantially impermeable to the aqueous solution 9. Further, the blanks are preferably also of a material with a melting temperature exceeding 100 °C, and preferably exceeding 130 °C. As an example, the blanks may comprise a material with barrier properties, rendering it impermeable to the wetting liquid, such as aluminium oxide, polychlorotrifluoroethylene (PCTFE), polyvinylidenechloride (PVDC), an aluminium foil or silicon oxide. Further, the blanks preferably comprise a carrier material and/or a material able to be welded, laminated with the material exhibiting the barrier properties. The skilled man in the art of packaging will know of many other materials and constructions which would work equally as well.

As will be appreciated, the package 1 results in the hydrophilic coating on the shaft 8 of the catheter 7 being maintained in a wet condition during storage. The catheter is therefore immediately ready for insertion into the urethra after the container 3 is opened.

Moreover, the coating on the shaft 8 is not subjected to moisture-induced wetting and drying cycles due to the

coating being stored in a wet condition. The package 1 thus ensures a long shelf-life for the catheter 7.

By reference to fig 2, for added security during storage the container 3 may be enclosed by an outer container 10. The container 3 could also be modified so as to act as an applicator for inserting the catheter shaft 8 into the urethra. There would thus be no risk of the catheter shaft 8 being contaminated during insertion into the urethra since the user would grip the catheter 7 through the material of the container 3. As an example, the container 3 could take the form of a urine collection bag through which the shaft 8 of the catheter 7 is projectable into the urethra of a patient with the urine drained by the catheter 7 being collected in the bag.

While the invention has been illustrated with reference to a urethral bladder drainage catheter it will be appreciated that the invention has equal application for any medical device provided with a coated surface which exhibits a reduced friction when wetted.

Claims

1. A storage package (1) which contains a medical device (7) having a coated surface (8) which exhibits a reduced friction when wetted with a wetting liquid and a supply of the wetting liquid (9) characterized in that, during storage, the coated surface (8) of the medical device (7) is constantly maintained in direct contact with said wetting liquid (9).
2. A storage package (1) as claimed in claim 1, wherein the storage package (1) comprises a container (3) within which the coated surface (8) and the wetting liquid (9) are contained.
3. A storage package (1) as claimed in claim 2, wherein the container (3) defines a cavity (5) which houses the coated surface (8) and the wetting liquid (9) is contained in the cavity (5) in a volume sufficient for the coated surface (8) to remain constantly wetted thereby during storage.
4. A storage package (1) as claimed in claim 3, wherein the cavity (5) is essentially filled with the wetting liquid.
5. A storage package (1) as claimed in claim 3 or 4, wherein the cavity (5) encloses the whole of the medical device.
6. A storage package (1) as claimed in any one of the claims 2-5, wherein the container (3) is of a construction which is impermeable or substantially impermeable to the wetting liquid (9).
7. A storage package (1) as claimed in any one of claims 2 to 6, wherein the container (3) is an inner container and that the package further comprises an outer container which encloses the inner container.
8. A storage package (1) as claimed in any one of the precedings claims, wherein the surface coating (8) is provided on a substrate presented by a polyether block amide.

9. A storage package (1), comprising a container (3) which defines a closed cavity (5), a medical device (7) positioned in the closed cavity (5) having a polyether block amide substrate surface (8) supporting a coating which exhibits a reduced friction when wetted with a wetting liquid, and a volume of the wetting liquid (9) in the closed cavity (5) sufficient for the coating to be maintained constantly wetted thereby during storage.

10. A storage package (1) as claimed in any one of the preceding claims, wherein during storage, essentially the whole coated surface (8) of the medical device (7) is constantly maintained in direct contact with said wetting liquid (9).

11. A storage package (1) as claimed in any one of the preceding claims, wherein during storage, essentially the whole of the medical device (7) is constantly maintained in direct contact with said wetting liquid (9).

12. A storage package (1) as claimed in any one of the preceding claims, wherein the surface coating (8) is provided on a substrate of a material having a melting temperature exceeding 100 °C, and preferably exceeding 130 °C.

13. A storage package (1) as claimed in claim 12, wherein the surface coating (8) is provided on a substrate of a material from the group polyurethanes, polyether block amides, silicon rubber, elastomeric alloys such as Santoprene® and polyolefin alloys based on polypropylene or SEBS (Styrene Ethylene Butadiene Styrene).

14. A storage package (1) according to claim 12 or 13, wherein the medical device is steam-sterilised.

15. A storage package (1) as claimed in any one of the preceding claims as dependent on claim 2 or claim 9, wherein the container is formed of a material having a

melting temperature exceeding 100 °C, and preferably exceeding 130 °C.

16. A storage package (1) as claimed in claim 15, wherein the container is steam-sterilised.

5 17. A storage package (1) as claimed in any one of the preceding claims as dependent on claim 2 or claim 9, wherein the container is impermeable to the wetting liquid.

10 18. A storage package (1) according to any one of the preceding claims, wherein the wetting liquid is steam-sterilised.

15 19. A storage package (1) according to any one of the preceding claims, wherein the wetting liquid (9) contains an osmolality-increasing agent such as sodium chloride and/or a pharmaceutically active substance.

20 20. A ready-to-use urinary catheter assembly comprising a container (3), said container containing a urinary catheter (7) having a hydrophilic surface layer (8) which exhibits a reduced friction when wetted with a wetting liquid and a supply of the wetting liquid (9) characterized in that, during storage, the whole of the coated surface (8) is constantly maintained in direct contact with said wetting liquid (9).

25 21. A method for sterile packaging of a medical device (7) having a surface (8) which exhibits a reduced friction when wetted with a wetting liquid, comprising the following steps:

providing a container;

30 placing the medical device (7) in the container together with wetting liquid (9) in such a way that the surface (8) of the medical device (7) is maintained in contact with the wetting liquid during storage;

sterilising the medical device and the wetting liquid; and

35 sealing the container.

22. The method as claimed in claim 21, wherein the medical device and the wetting liquid are sterilised at the same time.

23. The method as claimed in claim 21 or 22, wherein
5 steam-sterilisation is used for sterilising at least one of the medical device and the wetting liquid.

24. The method as claimed in claim 21 or 22, wherein microwave-sterilisation is used for sterilising at least one of the medical device and the wetting liquid.

10 25. The method as claimed in any one of the claims 21-24, wherein the sterilisation of the wetting liquid is performed after the sealing of the container.

26. The method as claimed in any one of the claims 21-25, wherein the sterilisation of the medical device is
15 performed after the sealing of the container.

27. The method as claimed in any one of the claims 21-26, wherein the volume of wetting liquid (9) placed in the container (3) is sufficient for the coated surface (8) to remain constantly wetted thereby during storage.

20 28. The method as claimed in any one of the claims 21-27, wherein the step of placing wetting liquid in the container comprises placing an amount of wetting liquid in the container such that during storage, essentially the whole coated surface (8) of the medical device (7) is
25 constantly maintained in direct contact with said wetting liquid (9).

29. The method as claimed in any one of the claims 21-28, wherein the step of placing wetting liquid in the container comprises placing an amount of wetting liquid
30 in the container such that during storage, essentially the whole the medical device (7) is constantly maintained in direct contact with said wetting liquid (9).

30. The method as claimed in any one of the claims 21-29, wherein the container (3) is an inner container,
35 comprising the additional step of enclosing the inner container (3) in an additional outer container.

31. The method as claimed in any one of the claims 21-30, wherein the surface (8) which exhibits a reduced friction on the medical device (7) is provided as a surface coating on a substrate of a material having a melting temperature exceeding 100 °C, and preferably exceeding 130 °C.

32. The method as claimed in claim 31, wherein the the surface coating (8) is provided on a substrate of a material from the group polyurethanes, polyether block amides, silicon rubber, elastomeric alloys such as Santoprene® and polyolefin alloys based on polypropylene or SEBS (Styrene Ethylene Butadiene Styrene).


33. The method as claimed in any one of the claims 21-32, wherein a container being formed of a material being substantially impermeable to the wetting liquid is provided.

34. The method as claimed in any one of the claims 21-33, wherein a container being formed of a material having a melting temperature exceeding 100 °C, and preferably exceeding 130 °C, is provided.

35. The method as claimed in any one of the claims 21-34, comprising the further step of adding an osmolality-increasing agent, such as sodium chloride and/or a pharmaceutically active substance to the wetting liquid.

36. The method as claimed in any one of the claims 21-35, wherein the medical device is a urethral catheter and the catheter is immediately "ready-for-use" after the package has been opened.

1/2

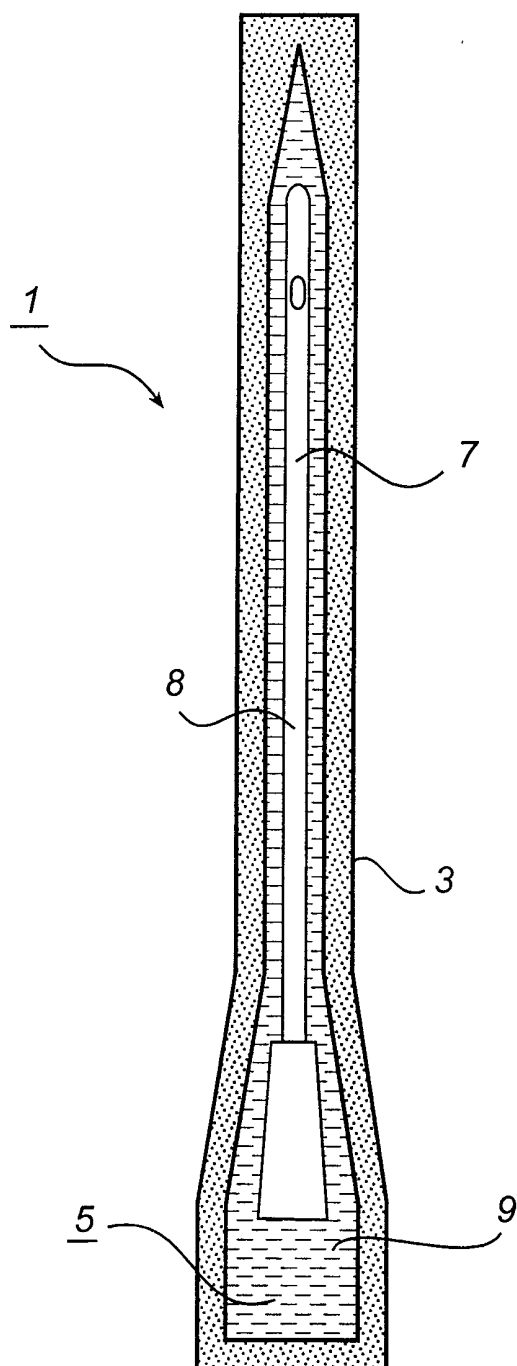*Fig. 1*

2/2

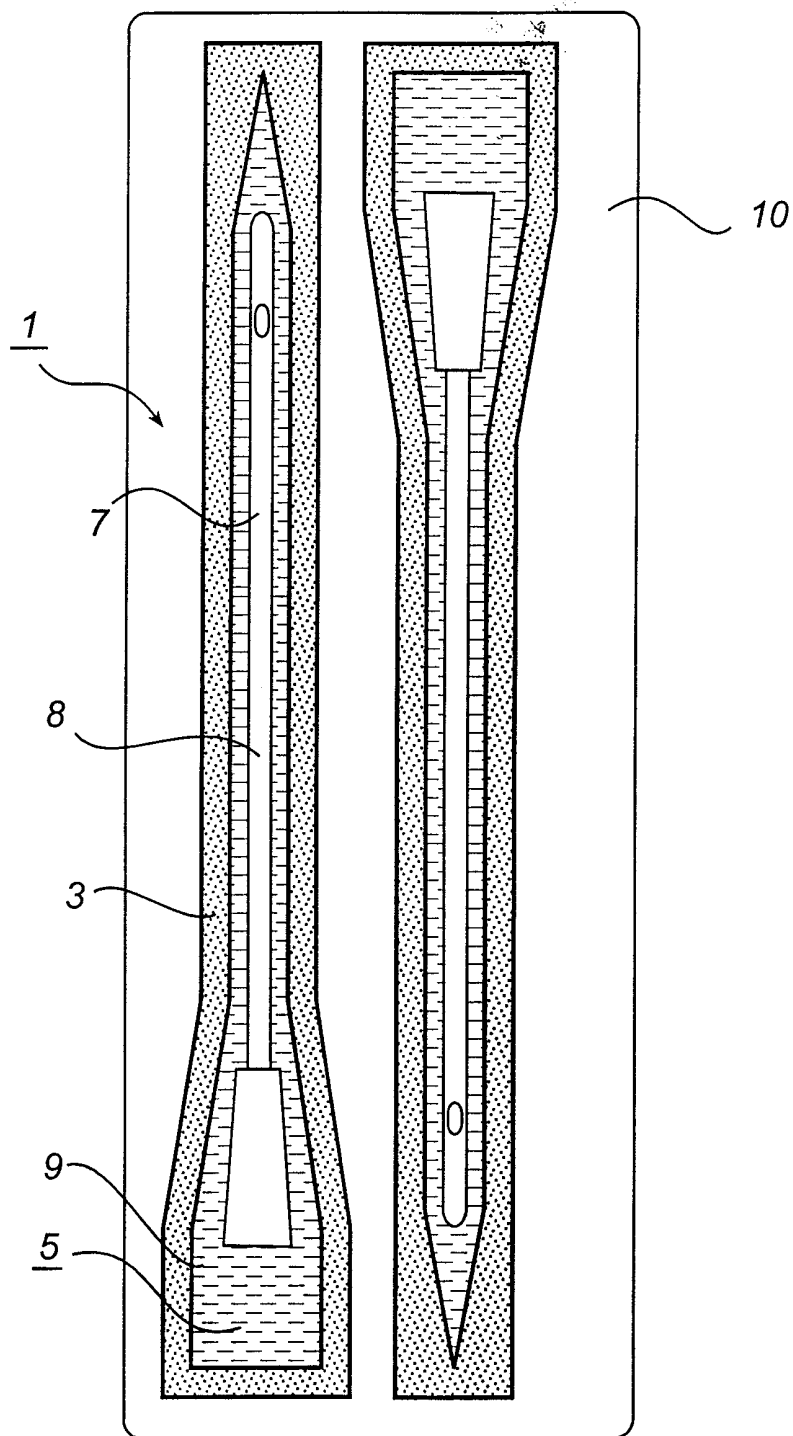


Fig. 2

INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 00/00289

A. CLASSIFICATION OF SUBJECT MATTER

IPC7: B65D 85/24 // A61M 25/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC7: B65D, A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPODOC, WPI

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	WO 9819729 A1 (COLOPLAST A/S), 14 May 1998 (14.05.98), figure 1, claim 1, abstract --	1-6
Y	US 5738213 A (JOHN WHITING ET AL), 14 April 1998 (14.04.98), figure 1, abstract --	1-6
A	WO 9416747 A1 (COLOPLAST A/S), 4 August 1994 (04.08.94), claims 1,5,6,9, abstract --	1-36
A	GB 1498356 A (THE KENDALL COMPANY), 18 January 1978 (18.01.78), claim 1 --	1-36

☒ Further documents are listed in the continuation of Box C.☒ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

19 June 2000

Date of mailing of the international search report

22-06-2000

Name and mailing address of the ISA:

Swedish Patent Office
Box 5055, S-102 42 STOCKHOLM
Facsimile No. +46 8 666 02 86

Authorized officer

Katarina Ekman/MP

Telephone No. +46 8 782 25 00

INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 00/00289

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 3967728 A (ROBERT L. GORDON ET AL), 6 July 1976 (06.07.76), abstract -- -----	1-20

INTERNATIONAL SEARCH REPORT

Information on patent family members

02/12/99

International application No.

PCT/SE 00/00289

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9819729 A1	14/05/98	AU 710581 B AU 710966 B AU 4295297 A AU 4295397 A CZ 9900917 A DK 122496 A EP 0923398 A EP 0935478 A SE 0935478 T3 NO 991120 A NO 992029 A PL 332545 A WO 9811932 A	23/09/99 30/09/99 29/05/98 14/04/98 11/08/99 19/03/98 23/06/99 18/08/99 08/03/99 28/04/99 13/09/99 26/03/98
US 5738213 A	14/04/98	NONE	
WO 9416747 A1	04/08/94	AU 660873 B AU 5880694 A DK 7193 A,B EP 0639990 A	06/07/95 15/08/94 22/07/94 01/03/95
GB 1498356 A	18/01/78	AU 497865 B AU 1376776 A BE 841892 A CA 1029338 A DE 2621503 A IT 1061279 B JP 51141098 A NL 7605026 A NZ 180870 A SE 7605539 A US 4091922 A ZA 7602899 A	18/01/79 17/11/77 01/09/76 11/04/78 25/11/76 28/02/83 04/12/76 18/11/76 03/04/78 17/11/76 30/05/78 27/04/77
US 3967728 A	06/07/76	GB 1465544 A	23/02/77