

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
19 November 2009 (19.11.2009)

PCT

(10) International Publication Number
WO 2009/139968 A2

(51) International Patent Classification:
A61N 1/34 (2006.01)

(21) International Application Number:
PCT/US2009/038741

(22) International Filing Date:
30 March 2009 (30.03.2009)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
12/121,281 15 May 2008 (15.05.2008) US

(71) Applicant (*for all designated States except US*):
BOSTON SCIENTIFIC NEUROMODULATION CORPORATION [US/US]; 25155 Rye Canyon Loop,
Valencia, CA 91355 (US).

(72) Inventors; and

(75) Inventors/Applicants (*for US only*): **PARRAMON, Jordi** [US/US]; 27631 Cobblestone Court, Valencia, CA 91354 (US). **CARBUNARU, Rafael** [VE/US]; 11916 Otsego Street, Valley Village, CA 91607 (US). **HALLER, Matthew, I.** [US/US]; 11815 Hesby Street, Valley Village, CA 91607 (US).

(74) Agent: **LEWIS, Terril, G.**; Wong, Cabello, Lutsch, Rutherford, & Bruculeri L.L.P., 20333 Tomball Parkway, Suite 600, Houston, TX 77070 (US).

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— *with declaration under Article 17(2)(a); without abstract; title not checked by the International Searching Authority*

(54) Title: CURRENT STEERING FOR AN IMPLANTABLE STIMULATOR DEVICE INVOLVING FRACTIONALIZED STIMULATION PULSES

(57) Abstract:



WO 2009/139968 A2

CURRENT STEERING FOR AN IMPLANTABLE STIMULATOR DEVICE INVOLVING FRACTIONALIZED STIMULATION PULSES

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This international application claims priority to U.S. Patent Application Serial Number 12/121,281, filed May 15, 2008, which is incorporated herein by reference in its entirety.

FIELD OF THE INVENTION

[0002] The present invention relates to therapeutic electrical stimulation systems and methods and, more specifically, relates to adjusting electrodes of an implantable stimulator device.

BACKGROUND

[0003] Implantable stimulation devices are devices that generate and deliver electrical stimuli to body nerves and tissues for the therapy of various biological disorders, such as pacemakers to treat cardiac arrhythmia, defibrillators to treat cardiac fibrillation, cochlear stimulators to treat deafness, retinal stimulators to treat blindness, muscle stimulators to produce coordinated limb movement, spinal cord stimulators to treat chronic pain, cortical and deep brain stimulators to treat motor and psychological disorders, and other neural stimulators to treat urinary incontinence, sleep apnea, shoulder subluxation, etc. The present invention may find applicability in all such applications, although the description that follows will generally focus on the use of the invention within a spinal cord stimulation system, such as that disclosed in U.S. Patent 6,516,227, which is incorporated herein by reference in its entirety.

[0004] Spinal cord stimulation is a well-accepted clinical method for reducing pain in certain populations of patients. As shown in Figures 1A, 1B, 2A, and 2B, a Spinal Cord Stimulation (SCS) system typically includes an Implantable Pulse Generator

(IPG) or Radio-Frequency (RF) transmitter and receiver 100 (collectively, “IPGs”), at least one electrode lead 102 and/or 104 having a plurality of electrodes 106, and, optionally, at least one electrode lead extension 120. The electrodes 106 are arranged in a desired pattern and spacing on the lead(s) 102, 104 to create an electrode array 110. Wires 112, 114 within one or more leads(s) 102, 104 connect each electrode 106 in the array 110 with appropriate current source/sink circuitry in the IPG 100.

[0005] In an SCS application, the electrodes lead(s) 102, 104 with the electrodes 106 are typically implanted along the spinal cord 19 (Fig. 2B), and the IPG 100 generates electrical pulses that are delivered through the electrodes 106 to the nerve fibers within the spinal column. The IPG 100 body itself is normally implanted in a subcutaneous pocket, for example, in the patient’s buttocks or abdomen. The electrode lead(s) 102, 104 exit the spinal column and generally attach to one or more electrode lead extensions 120 (Fig. 2), which in turn are typically tunneled around the torso of the patient to the subcutaneous pocket where the IPG 100 is implanted. Alternatively, if the distance between the lead(s) 102, 104 and the IPG 100 is short, the electrode lead(s) 102, 104 may directly connect with the IPG 100 without lead extensions 120. For examples of other SCS systems and other stimulation system, see U.S. Patents 3,646,940 and 3,822,708, which are hereby incorporated by reference in their entireties. Of course, an IPG 100 is an active device requiring energy for operation, which may be provided by an implanted battery or an external power source.

[0006] Precise placement of the lead(s) 102, 104 relative to the target nerves is important for achieving a satisfactory physiological response, and for keeping stimulation thresholds low to conserve battery power. A conventional lead implantation procedure commonly places the leads 102, 104 parallel to the spinal cord column 19 at or near the physiological midline 91, as is shown in Figures 3A and 3B. More particularly, and as best shown in the cross section of Figure 3B, the electrode leads 102, 104 are placed directly on the dura mater 51 within the epidural space 70. (Cerebro-spinal fluid 72 is between the electrode array 110 and the white matter 52 of the spinal cord 19. Dorsal root nerves 50 are shown emanating from grey matter 53). When the leads 102, 104 are placed on opposite sides of the

physiological midline 91 as shown, additional flexibility is provided in the ability to recruit (i.e., stimulate) nerves in the dorsal column, and to treat symptoms manifesting on either the left or right sides of the patient's body.

[0007] In addition to precise placement of the electrode array, proper selection of the electrodes, i.e., determining which of the electrodes 106 in the array should be active in a given patient, is critical for achieving effective stimulation therapy. However, because of the uncertainties of the distances of the electrodes from the neural target, the unknown nature of the specific conductive environment in which the electrode is placed, etc., it generally cannot be known in advance and with precision which combination of active electrodes will be perceived by a patient as providing optimal therapy. As a result, patient therapy generally requires that various electrode combinations be tried and feedback received from the patient as to which of the combinations feels most effective from a qualitative standpoint.

[0008] Various electrode combinations and other stimulation parameters can be tried during initialization by programming the IPG 100 using an external wireless clinician or hand-held controller. (Details concerning such controllers can be found in U.S. Patent Publication 2007/0239228, published October 11, 2007, which is assigned to the present application and which is incorporated herein by reference in its entirety). For example, and as best visualized in Figure 3A, the IPG 100 can be programmed such that electrode E1 comprises an anode (source of current), while E2 comprises a cathode (sink of current). Or, the IPG 100 can be programmed such that electrode E1 comprises an anode, while E9 comprises a cathode. Alternatively, more than one electrode can be used in both the sourcing and sinking of current. For example, electrode E1 could comprise an anode, while both E2 and E9 can comprise cathodes. The amount of current sourced or sunk can also be programmed into the IPG 100. Thus, in the last example, electrode E1 could sink 5 mA, while electrode E2 sources 4 mA and electrode E9 sources 1 mA. The frequency of electrode stimulation pulses, as well as the pulsewidth or duration of such stimulation pulses, is also programmable.

[0009] Ultimately, which electrodes are activated by the IPG 100, and the polarities (cathode v. anode), magnitudes (amount of current), and frequencies of those activated electrodes, are based largely on patient feedback during IPG initialization as noted earlier. Thus, the patient, perhaps assisted by a clinician, will experiment with the various electrode settings, and will report relative levels of comfort and therapeutic effectiveness to arrive at electrode settings that are best for a given patient's therapy.

[0010] In the prior art, patients and/or clinicians used a technique called "field steering" or "current steering" to try and simplify the iterative process for determining a patient's optimal electrode settings during initialization of the IPG. See, e.g., U.S. Patent 6,909,917, which is incorporated herein by reference in its entirety. In current steering, the current sourced or sunk by the electrodes is gradually redistributed by the patient or clinician to different electrodes using a single stimulation timing channel. Such steering can be facilitated using some sort of user interface associated with the external controller, such as a joystick or other directional device. Simple examples of current steering are shown in Figures 4A, 4B, and 5. Starting first with Figure 4A, assume that the IPG 100 has an initial condition, namely that electrode E1 has been programmed to sink 10 mA of current, while electrode E3 has been programmed to source 10 mA of current. This initial condition might be arrived at after some degree of experimentation, and might be a condition at which the patient is feeling a relatively good response, but a response which has not yet been fully optimized.

[0011] In an attempt at further optimization, current steering can commence from these initial conditions. Assume that optimization by current steering will ultimately arrive at the final condition of Figure 4B. As shown, this final condition sinks 10 mA at electrode E2. Thus, during current steering, 10 mA of sink current is moved from E1 (the initial condition) to E2 (the final condition). To do this, electrode E1 is selected and the current sunk from that electrode is moved downward, for example, by clicking downward on the controller's joystick. As shown in Figure 5, this moves some increment of sinking current (as illustrated, a 2 mA increment) from electrode E1 to electrode E2, such that E1 now sinks 8 mA and E2 sinks 2 mA. Another

downward click moves another 2 mA, so that now E1 sinks 6 mA and E2 sinks 4mA, etc., until the full 10 mA is moved to E2 as per the final condition.

[0012] Gradual steering of the current in increments is generally considered advisable to safeguard against abrupt changes of the stimulation field which may be uncomfortable or dangerous for the patient. Abrupt shifting of the entirety of the current from one electrode to another could have unforeseen and undesirable effects. Different nerves are affected by such a change in electrode activation, and it is not necessarily known how moving a full allotment of current would affect those nerves. If the current when applied to the new electrodes (e.g., from E1 to E2) is too low (i.e., sub-threshold), no clinical response would be noticed, even if the electrodes were ultimately suitable choices. If the current is too high (i.e., supra-threshold), the result might be painful (or dangerous) for the patient. Accordingly, incremental movement of the current is considered a good approach.

[0013] However, the illustrated current steering approach requires two different electrodes (e.g., E1 and E2) to simultaneously act as current sinks during the intermediate steering steps. This can be an implementation problem in IPG architectures that don't allow the simultaneous selection of two or more electrodes to act as the source or sink. For example, some simpler IPG architectures may provide only a single current source circuit and a single current sink circuit, which circuits can only be coupled to one electrode at a time. Because such architectures will not support simultaneous activation of two or more electrodes as sinks or sources, the current steering approach of Figure 5 can't be used.

[0014] Other current steering approaches provide additional complexities. For example, the current steering approach illustrated in Figure 6 is disclosed in U.S. Patent Publication 2007/0239228, which was incorporated by reference above. In this approach, steering of the current from one electrode to another occurs by establishing the steered current in a second timing channel. (Because the operation of timing channels are explained in detail in the '228 publication, they are not further explained here). Thus, and as shown, current in the transferring electrode (E1) is initially established in a first timing channel 'A.' As the current is incrementally

steered to receiving electrode E2, that steered current forms in a second timing channel 'B,' such that the pulses in timing channel A and B are non-overlapping. The result after several incremental transfers of current is the final condition in which the sink current resides entirely with electrode E2 is in the second timing channel B.

[0015] This approach of the '228 publication thus requires IPG hardware and software necessary to support different timing channels. Not all IPGs will have such hardware or software, and so will be unable to benefit from the current steering technique of Figure 6. Even in those IPGs that can support multiple timing channels, such a current steering technique is relatively complex, and is potentially limited. For example, although not shown in Figure 6, one skilled in the art will understand that the pulses must generally be followed by either a passive or active current recovery period. Because pulses in the next timing channel cannot be executed until current recovery of the pulses in the preceding timing channel is completed, the ability to use the '228 publication's current steering technique is not guaranteed. For example, if the stimulation pulses are of long duration or of a high frequency, there may simply not be enough time in which to interleave the pulses in the two timing channels, especially when current recovery periods are considered.

[0016] Accordingly, what is needed is an improved method for optimizing electrode activation during the set up of an implantable stimulator device, and this disclosure provides embodiments of such a solution.

BRIEF DESCRIPTION OF THE DRAWINGS

[0017] Figures 1A and 1B show an electrode array and the manner in which it is coupled to the implantable stimulator device in a SCS.

[0018] Figures 2A and 2B show a placement of the percutaneous lead for spinal cord stimulation with an in-line electrode array inserted alongside the spinal cord in the epidural space, in close proximity to the dura mater.

[0019] Figure 3A and 3B show placement of two in-line electrode arrays on the left and right sides of the physiological midline of the spinal cord, respectively, in a perspective view and in cross-section.

[0020] Figures 4A, 4B and 5 show an electrode current steering technique of the prior art.

[0021] Figure 6 shows another electrode current steering technique of the prior art.

[0022] Figures 7A and 7B show how ideally simultaneous pulses can be reconstructed as non-simultaneous fractionalized pulse portions in accordance with an embodiment of the disclosed technique.

[0023] Figures 8A and 8B show how the fractionalized pulse portions can be used in a current steering application.

DETAILED DESCRIPTION

[0024] The description that follows relates to use of the invention within a spinal cord stimulation (SCS) system. However, the invention is not so limited. Rather, the invention may be used with any type of implantable medical device system. For example, the present invention may be used as part of a system employing an implantable sensor, an implantable pump, a pacemaker, a defibrillator, a cochlear stimulator, a retinal stimulator, a stimulator configured to produce coordinated limb movement, a cortical and deep brain stimulator, or in any other neural stimulator configured to treat any of a variety of conditions.

[0025] A method for configuring stimulation pulses in an implantable stimulator device having a plurality of electrodes is disclosed, which method is particularly useful in adjusting the electrodes by current steering during initialization of the device. In one aspect, a set of ideal pulses for patient therapy is determined, in which at least two of the ideal pulses are of the same polarity and are intended to be simultaneously applied to corresponding electrodes on the implantable stimulator device during an initial duration. These pulses are reconstructed into fractionalized

pulses, each comprised of pulse portions. The fractionalized pulses are applied to the corresponding electrodes on the device during a final duration, but the pulse portions of the fractionalized pulses are not simultaneously applied during the final duration.

[0026] An improved current steering technique for an implantable stimulator device is illustrated in Figures 8A and 8B. However, before discussion of that technique, a more fundamental understanding of the technological and biological aspects of the technique are illustrated in Figures 7A and 7B.

[0027] Figure 7A illustrates an intermediary set of pulses as might be desired during current steering. As shown, electrodes E1 and E2 are desired to be simultaneously asserted as pulses 201a and 202a, each providing a 5 mA sink. This condition of simultaneity could be encountered when transferring sink current from E1 to E2, as was illustrated earlier.

[0028] The actual implementation of such idealized pulses according to an aspect of the invention comprises a reconstruction of these ideal pulses 201a and 202a as fractionalized pulses 201b and 202b which are not simultaneous. As can be seen in the magnified illustration at the bottom of Figure 7A, only one fractionalized pulse portion 205 or 206 is asserted at any given time. As such, the fractionalized pulse portions 205 and 206 are interleaved.

[0029] The frequency of the fractionalized pulse portions 205, 206 in the illustrated example equals $1/t_p$, where t_p comprises the pulse portion period. Because the pulse portion period t_p is generally much shorter than the duration of the ideal pulses, t_D , there would typically be many fractional pulse portions 205 or 206 occurring within duration t_D , although only a few such portions are shown in Figure 7A for ease of illustration.

[0030] Stimulation using fractionalized pulses 201b and 202b causes recruited neurons to react to the pulse portions 205 and 206 in an additive manner. For example, for a depolarizing sequence, the transmembrane potential will slowly depolarize on average with each additional pulse portion. The sequence of pulse portions 205 and 206 takes advantage of the non-linear membrane dynamics which

tend to move a recruited neuron towards depolarization. In particular, short pulse portions will tend to open the “m” gates of the sodium channels. As the gates open, the cell membrane will tend to depolarize slightly more. A combination of pulse portions can then depolarize the membrane enough until, as with the ideal pulses 201a and 202a, an action potential is generated in the recruited neurons. In other words, the nerves recruited by the electrodes E1 and E2 will receive effective therapy even though the fractionalized pulses 201b and 202b are interrupted and non-simultaneous unlike their ideal counterparts 201a and 202a.

[0031] The pulse portion period, t_p , may be kept lower than the chronaxie time, which is approximately 100 to 150 microseconds or so. However t_p can also exceed the chronaxie time, although in such an application higher energies (e.g., pulse portion amplitudes) might be required as explained further below. However, effectiveness in therapy, even with increasing energies, would be expected to diminish when t_p exceeds 500 microseconds or so.

[0032] In the illustrated example, the fractionalized pulse portions 205 and 206 have a duty cycle of approximately 50%, such that only one pulse portion 205 or 206 from fractionalized pulses 201b and 202b are asserted at any given time. Note also that the amplitude of those pulse portions 205, 206 (-10 mA) are twice what is called for in the corresponding ideal pulses 201a and 201b (-5 mA). This amplitude relates to the duty cycle of the pulse portions, and stems from the recognition that the total amount of injected charge remains an important first-order variable in effective patient therapy. Thus, when one compares the ideal pulses 201a and 202a with their fractionized actual counterparts 202a and 202b, the amount of charge (i.e., the area under their curves) is same. So, if the duty cycle of the fractionalized portions are 50%, an amplitude of twice would be indicated; if the duty cycle is 33.3% (as might occur should three electrodes need to act as either a source or sink at one time), three times the amplitude would be indicated, etc.

[0033] However, it is not strictly required that the amount of charge in the ideal and fractionalized pulses be equal, and in a given application amplitudes of the fractionalized pulse portions 205 and 206 may need to be adjusted to provide slightly

more or less charge than the injected charge of the ideal pulses 201a and 202a. In one example, and as alluded to above, longer pulse portion periods might require higher amounts of charge than are represented by their ideal counterparts. For example, assuming a 50% duty cycle and a pulse portion period t_p slightly above the chronaxie time, the amplitude of the fractionalized pulse portions 205 and 206 may be higher than double (e.g., 2.1 times) the amplitude of the corresponding ideal pulses 201a and 202a, resulting in a higher amount of charge. If t_p is made even larger, then the amplitude of the fractionalized pulses portions could increase even further (e.g., to 2.2 times), etc.

[0034] Because of the increase in amplitude of the fractionalized pulse portions 205, 206, the current generation circuitry in the IPG 100 must be capable of sustaining higher compliance voltages. See U.S. Published Patent Application 2007/0097719, published May 3, 2007, which is incorporated herein in its entirety, for a further discussion of compliance voltage generation in IPGs.

[0035] Figure 7B illustrates another way in which simultaneous pulses can be reconstructed in accordance with the invention. As with Figure 7A, the ideal pulses 201a and 201b are fractionalized and interleaved as shown at 201c and 202c. However, the fractionalized pulse portions 205' and 206' have the same amplitude (-5 mA) as do their ideal pulse counterparts, but the fractionalized pulses 201c and 202c have a duration t_D' of twice the duration t_D of the ideal pulses. The result, as with Figure 7A, is ideal and fractionalized pulses that are comprised of approximately the same amount of charge. While the reconstruction method of Figure 7B does modify the duration of the ideal pulses (i.e., from t_D to t_D'), such pulse duration modification only affects patient therapy as a second-order variable; the more-important first-order variable of total charge remains essentially unchanged, and so patient therapy is not significantly impacted by the change in duration. Of course, assuming that the amount of charge is kept approximately the same, other durations, both longer and shorter than the duration of the ideal pulses, can be used in the actual fractionalized pulses. The two-fold duration increase shown in Figure 7B is therefore merely exemplary.

[0036] The system may use both techniques—higher pulse amplitude (Fig. 7A) or higher pulse duration (Fig. 7B)—as convenient. For example, the logic in the IPG 100 may choose an appropriate pulse fractionalization strategy that saves energy. Or, the logic in the IPG 100 may choose fractionalization parameters to prevent saturation of the output—e.g., if the amplitude has been maximized then the pulse width or duration is increased, etc.

[0037] There are significant benefits to reconstructing the ideal pulses as fractionalized pulses as shown in Figures 7A and 7B. Even though the patient's nerves biologically sense simultaneous stimulation, the reality is that no more than one electrode is truly active as a source or sink at any given time, given the interleaved fractionalized pulse portions 205 and 206. Therefore, this technique, and the steering technique described subsequently in Figures 8A and 8B, can be implemented in IPGs having simpler architectures in which source or sink circuitry is coupleable to only a single electrode at a time.

[0038] In an actual implementation, there would be some set-up time necessary to switch current sink circuitry from E1 to E2, and so the duty cycles of the fractionalized pulse portions 205 and 206 may be less than an ideal 50% for example. However, such set-up time would be relatively short compared to the pulse portion period t_p , and so such set-up time is negligible and therefore not illustrated in the figures. For example, it may take only a few 0.1 of a microsecond to switch the current from one electrode to another, i.e., from a pulse portion 205 to a pulse portion 206. However, one skilled in the art will realize that the transition times and other non-idealities will mean that the actual charge of the fractionalized pulses may only approximate the charge specified by the ideal pulses.

[0039] Figures 8A and 8B illustrate how the reconfigured fractionalized pulses can be utilized in an improved current steering scheme. As with Figures 5 and 6, Figures 8A and 8B illustrate the simple example of gradually steering 10 mA of sink current from electrode E1 to electrode E2. The initial condition at the top of Figure 8A is defined in a single timing channel, which timing channel specifies the amplitude, duration, and frequency of the ideal stimulation pulses. Starting from that initial

condition, a user (patient or clinician) selects to move an increment (e.g., 2 mA) of sink current from E1 to E2, perhaps by a downward click of a joystick on an external controller as mentioned previously. At this point, the logic in the IPG 100 recognizes the need for sink current to be simultaneously present at both E1 (8 mA) and E2 (2 mA). Accordingly, the logic in the IPG reconstructs these ideal pulses as shown in the second condition of Figure 8A. This second condition reconfigures the pulses as fractionalized pulses. Because these pulses are fractionalized and interleaved, their amplitudes are doubled to (in this example) approximately preserve the desired amount of charge. Thus, the fractionalized pulse portions at E1 (with a duty cycle of approximately 50%), have an amplitude of approximately -16 mA over the same duration as the initial pulses, thus simulating the -8 mA pulse that is desired; the interleaved pulses portions at E2 likewise have an amplitude of approximately -4 mA to simulate the desired -2 mA pulse.

[0040] While the logic in the IPG 100 can be programmed to automatically fractionalize the pulses in a predetermined manner when necessary, it should be noted that this is only an embodiment. The decision on how to perform the fractionalization can also be made by a user with a wireless external controller. For example, a user can access a user interface on the external controller to specify fractionalization parameters such as amplitude, duration, period, etc., with such parameters being wirelessly transmitted to the nonvolatile memory storage in the IPG 100. Because external controllers are well known in the art, they are not discussed further.

[0041] Effecting such fractionalization is achieved in a preferred embodiment by re-writing the timing channel in which the initial condition was specified. In other words, moving from the initial to the second condition does not require the establishment of a second timing channel, because the logic in the IPG 100 preferably re-writes the first timing channel to add the additional electrode (E2), to specify the duty cycle and period (t_p) of the first and second interleaved pulses, etc. This is an improvement over prior art current steering techniques which require the use of steering using additional timing channels, such as the '228 publication referenced earlier. In short, the presently-disclosed current steering technique requires only a single timing channel, making it amenable to IPG architectures having hardware or

software capable of handling only a single timing channel. Having said this, it should be recognized that the invention can also be implemented in IPGs having a plurality of timing channels, and so is not limited to single timing channel devices.

[0042] As shown further in Figure 8A, further user selection to steer another increment of current results in decreasing the amplitude of the fractionalize pulse portions at the transmitting electrode E1 (from -16 mA to -12 mA) while concurrently increasing the amplitude of the fractionized pulse portions at the receiving electrode E2 (from -4 mA to -8 mA). Such adjustment merely requires updating the amplitudes in the first (initial) timing channel, and does not require a second timing channel. Continuing selections eventually result in the final desired condition illustrated at the bottom of Figure 8B, in which the full amount of sink current (-10 mA) is now present entirely at electrode E2. Because this final condition does not require electrode E1 and E2 to both sink current simultaneously, the pulses at E2 can be reconfigured with a 100% duty cycle pulse at its normal amplitude. Again, this happens by re-writing the first timing channel.

[0043] It should be understood that reference to an “electrode on the implantable stimulator device” includes electrodes on the implantable stimulator device, or the electrodes on the associated electrode leads, or any other structure for directly or indirectly stimulating tissue.

[0044] Although particular embodiments of the present invention have been shown and described, it should be understood that the above discussion is not intended to limit the present invention to these embodiments. It will be obvious to those skilled in the art that various changes and modifications may be made without departing from the spirit and scope of the present invention. Thus, the present invention is intended to cover alternatives, modifications, and equivalents that may fall within the spirit and scope of the present invention as defined by the claims.

WHAT IS CLAIMED IS:

1. A method for configuring stimulation pulses in an implantable stimulator device having a plurality of electrodes, comprising:
 - determining a set of pulses for patient therapy, wherein at least two of the pulses are of the same polarity;
 - reconstructing each of the at least two pulses into corresponding fractionalized pulses, wherein each fractionalized pulse is comprised of pulse portions; and
 - applying the at least two fractionalized pulses to corresponding electrodes on the implantable stimulator device during a final duration, wherein the pulse portions of one fractionalized pulse are not simultaneously applied with the pulse portions of another of the fractionalized pulses during the final duration.
2. The method of claim 1, wherein the pulse portions have a period less than the time period at which nerves can respond to electrical stimulation.
3. The method of claim 1, wherein the pulse portions have a period less than 200 microseconds.
4. The method of claim 1, wherein the at least two pulses have first amplitudes, and wherein the pulse portions of each corresponding fractionalized pulse have second amplitudes, and wherein the corresponding first and second amplitudes are different.
5. The method of claim 1, wherein the at least two of the pulses are further determined to be simultaneously applied to corresponding electrodes on the implantable stimulator device during an initial duration, and wherein the initial and final durations are different.

6. The method of claim 1, wherein the at least two of the pulses are further determined to be simultaneously applied to corresponding electrodes on the implantable stimulator device during an initial duration, and wherein the initial and final durations are equal.
7. The method of claim 1, wherein the at least two pulses comprise a initial amount of charge, and wherein the pulse portions of each corresponding fractionalized pulse comprise a final amount of charge.
8. The method of claim 7, wherein the initial and final amounts of charge are approximately equal.
9. The method of claim 1, wherein the fractionalized pulses are defined in a single timing channel in the implantable stimulator device.
10. A method for configuring stimulation pulses in an implantable stimulator device having a plurality of electrodes, comprising:
 - determining a set of pulses for patient therapy, wherein at least two of the pulses are of the same polarity;
 - reconstructing each of the at least two pulses into a plurality of sequential pulse portions; and
 - applying the plurality of sequential pulse portions to corresponding electrodes on the implantable stimulator device during a final duration, wherein the plurality of pulse portions are interleaved during the final duration.
11. The method of claim 10, wherein the pulse portions have a period less than the time period at which nerves can respond to electrical stimulation.
12. The method of claim 10, wherein the at least two pulses have first amplitudes, and wherein the pulse portions of each corresponding fractionalized pulse have

second amplitudes, and wherein the corresponding first and second amplitudes are different.

13. The method of claim 10, wherein the at least two of the pulses are further determined to be simultaneously applied to corresponding electrodes on the implantable stimulator device during an initial duration, and wherein the initial and final durations are different.

14. The method of claim 10, wherein the at least two of the pulses are further determined to be simultaneously applied to corresponding electrodes on the implantable stimulator device during an initial duration, and wherein the initial and final durations are equal.

15. The method of claim 10, wherein the at least two pulses comprise a initial amount of charge, and wherein the pulse portions of each corresponding fractionalized pulse comprise an approximately equal amount of charge.

16. A method for adjusting the electrodes on an implantable stimulator device, comprising:

receiving a command to move an amount of current from a first initial pulse of an initial duration on a first electrode to a second initial pulse on a second electrode;

reconstructing the first and second pulses into corresponding first and second fractionalized pulses, wherein each fractionalized pulse is comprised of pulse portions; and

respectively applying the first and second fractionalized pulses to the first and second electrodes on the implantable stimulator device during a final duration, wherein the pulse portions of first fractionalized pulse are not simultaneously applied with the pulse portions of the second fractionalized pulses during the final duration.

17. The method of claim 16, wherein the pulse portions have a period less than the time period at which nerves can respond to electrical stimulation.
18. The method of claim 16, wherein the pulse portions have a period less than 200 microseconds.
19. The method of claim 16, wherein the first initial pulse has a first amplitudes, the second initial pulse has a second amplitude, the pulse portions of the first fractionalized pulse have a third amplitude, and the pulse portions of the second fractionalized pulse have a fourth amplitude, and wherein the first and third amplitudes are different, and the second and fourth amplitudes are different.
20. The method of claim 16, wherein the first initial pulse has a first amplitudes, the second initial pulse has a second amplitudes, the pulse portions of the first fractionalized pulse have a third amplitude, and the pulse portions of the second fractionalized pulse have a fourth amplitude, and wherein the first and third amplitudes are the same, and the second and fourth amplitudes are the same.
21. The method of claim 16, wherein the initial and final durations are different.
22. The method of claim 16, wherein the initial and final durations are equal.
23. The method of claim 16, wherein the first and second initial pulses respectively comprise first and second amounts of charge, and wherein the pulse portions of the first and second fractionalized pulses respectively comprise approximately the first and second amounts of charge.
24. The method of claim 16, wherein the first initial pulse is defined in a single timing channel in the implantable stimulator device, and wherein the first and second fractionalized pulses are also defined in that timing channel.

25. A method for adjusting the electrodes on an implantable stimulator device, comprising:

receiving a command to move an amount of current from a first initial pulse of an initial duration on a first electrode to a second initial pulse on a second electrode;

reconstructing the first and second pulses into corresponding first and second sets of sequential pulse portions; and

respectively applying the first and second fractionalized pulses to the first and second electrodes on the implantable stimulator device during a final duration, wherein the first and second sets of sequential pulse portions are interleaved during the final duration.

26. The method of claim 25, wherein the pulse portions have a period less than the time period at which nerves can respond to electrical stimulation.

27. The method of claim 25, wherein the first initial pulse has a first amplitude, the second initial pulse has a second amplitude, the pulse portions of the first set have a third amplitude, and the pulse portions of the second set have a fourth amplitude, and wherein the first and third amplitudes are different, and the second and fourth amplitudes are different.

28. The method of claim 25, wherein the first initial pulse has a first amplitude, the second initial pulse has a second amplitude, the pulse portions of the first set have a third amplitude, and the pulse portions of the second set have a fourth amplitude, and wherein the first and third amplitudes are the same, and the second and fourth amplitudes are the same.

29. The method of claim 25, wherein the first and second initial pulses respectively comprise first and second amounts of charge, and wherein the pulse portions of the first and second fractionalized pulses respectively comprise approximately the first and second amounts of charge.

30. The method of claim 25, wherein the first initial pulse is defined in a single timing channel in the implantable stimulator device, and wherein the first and second fractionalized pulses are also defined in that timing channel.

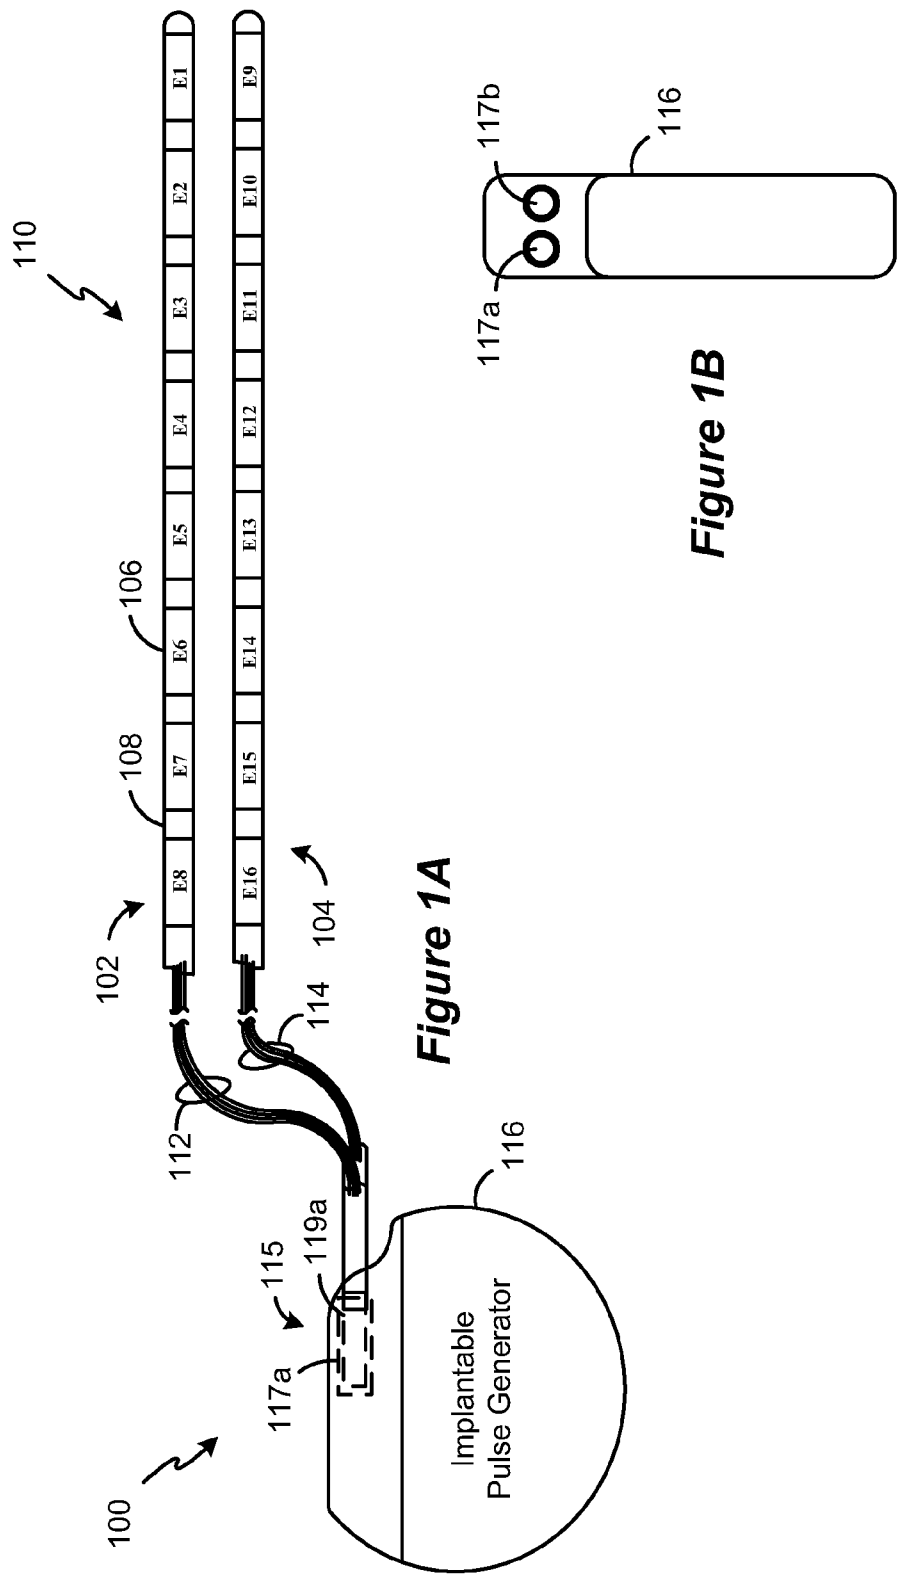


Figure 1A

Figure 1B

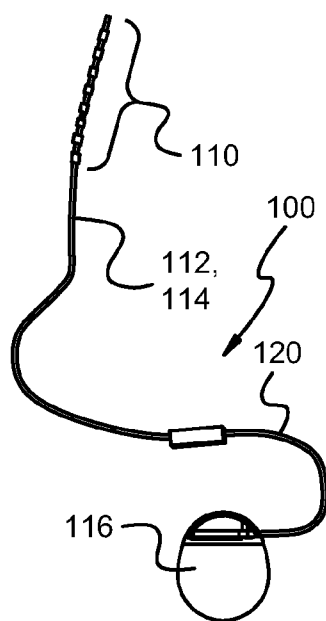
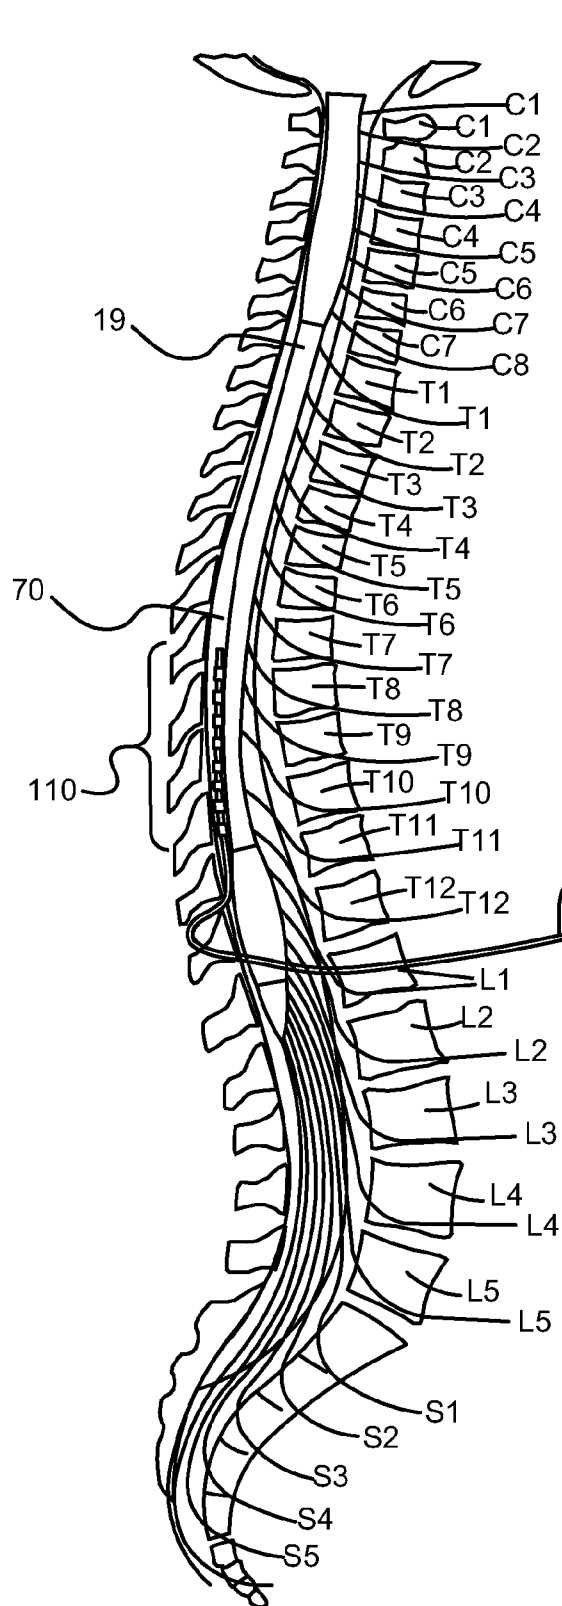


Figure 2A

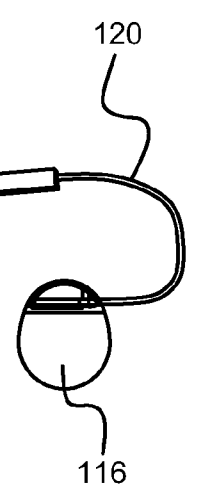
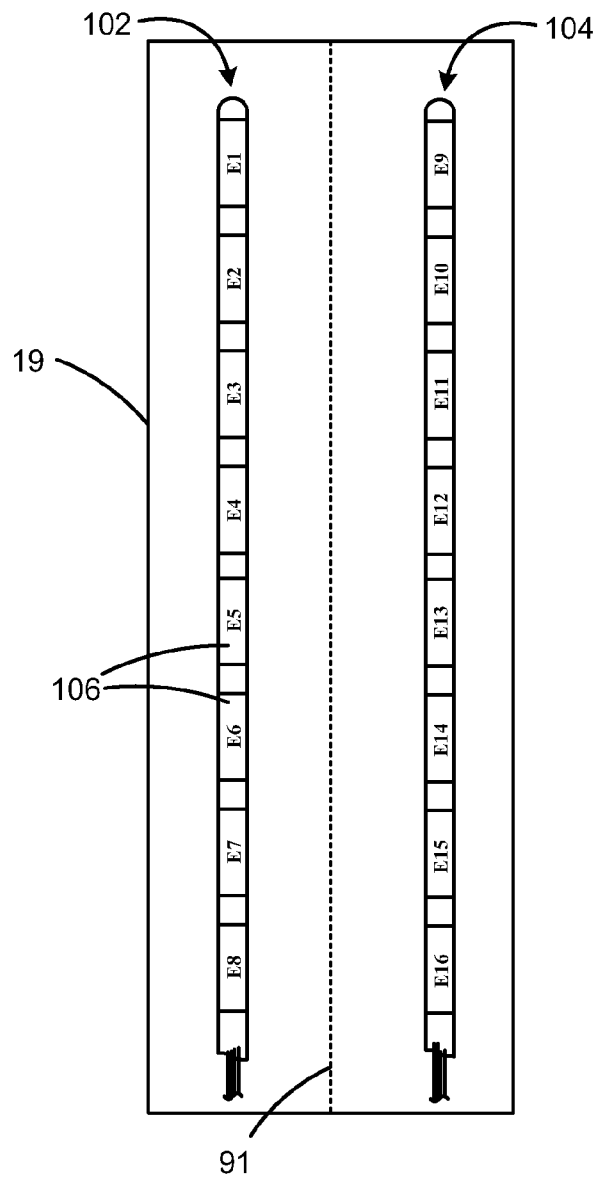


Figure 2B

3/11

**Figure 3A**

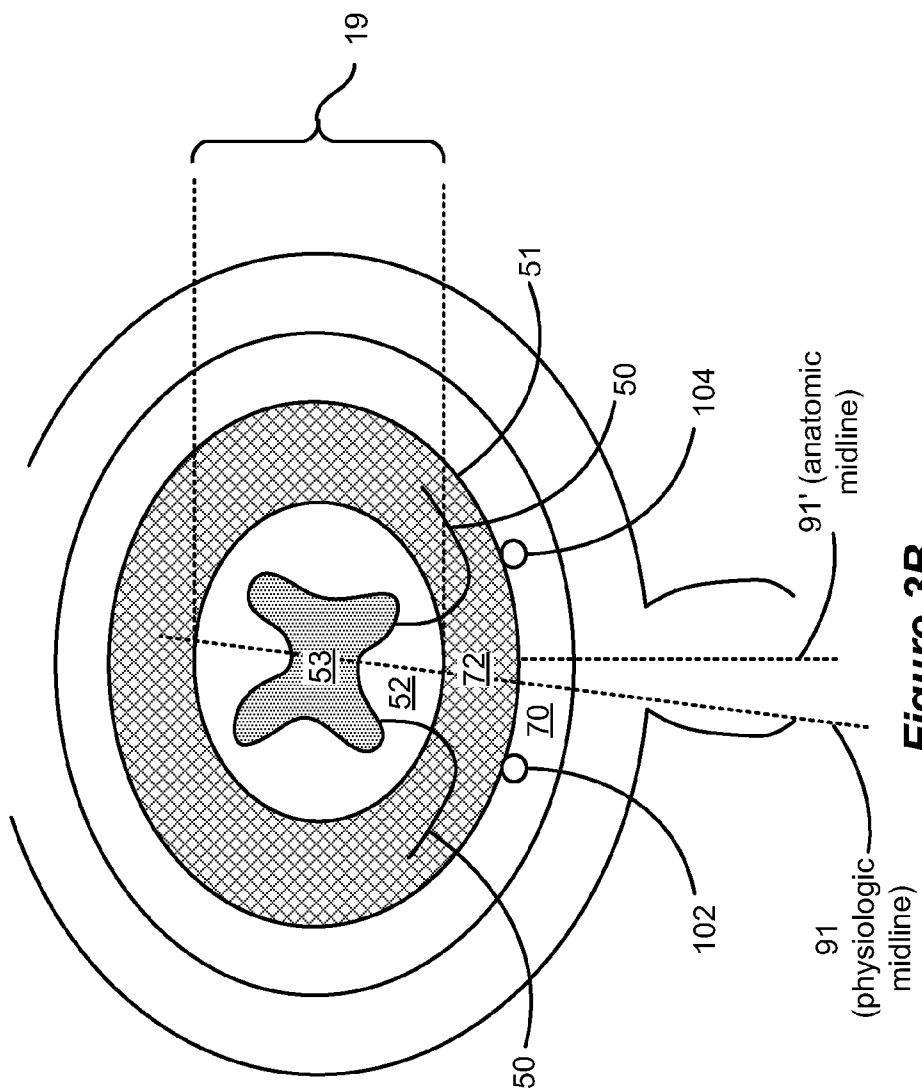


Figure 3B


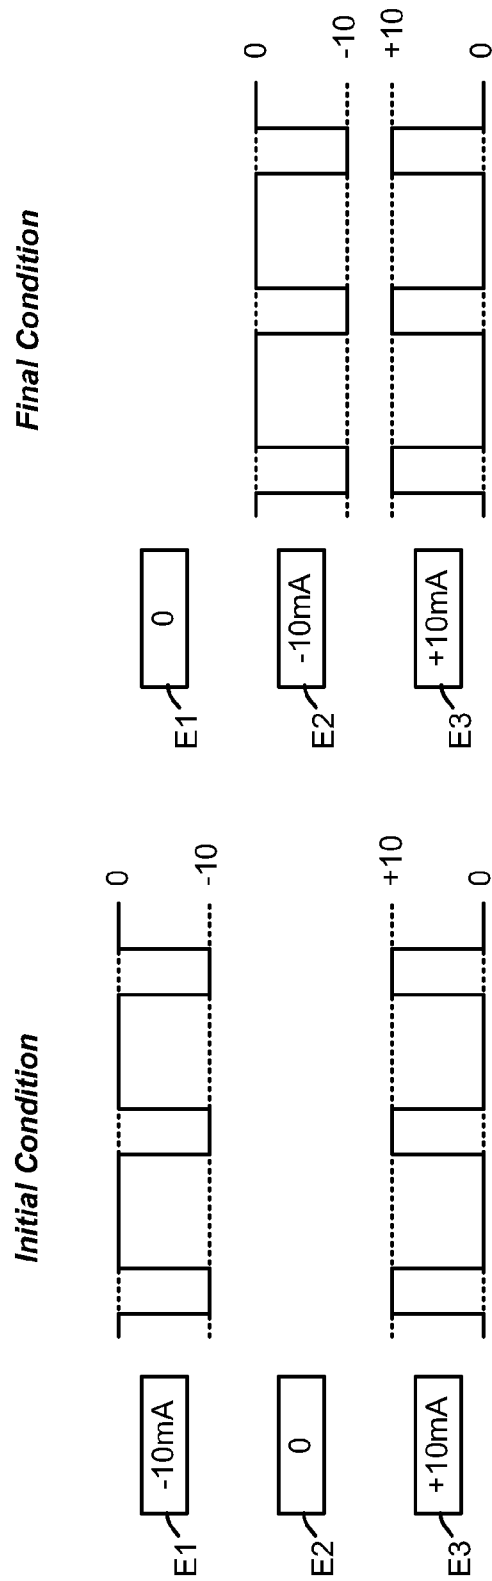



Figure 4B
(prior art)

Figure 4A
(prior art)


6/11

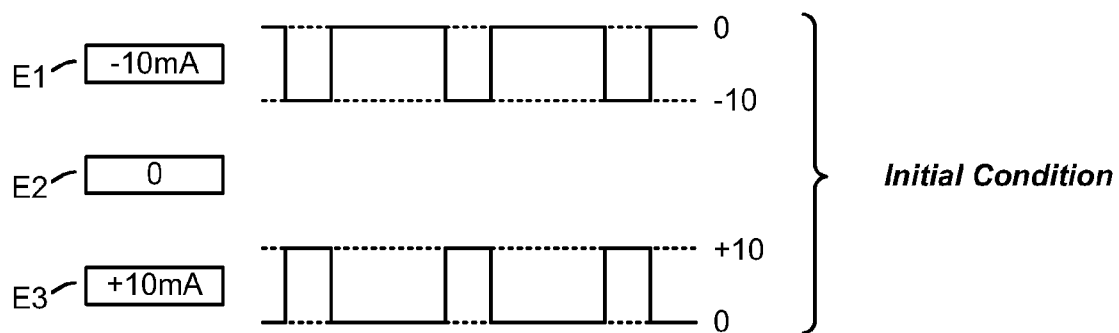

↓ (click down)

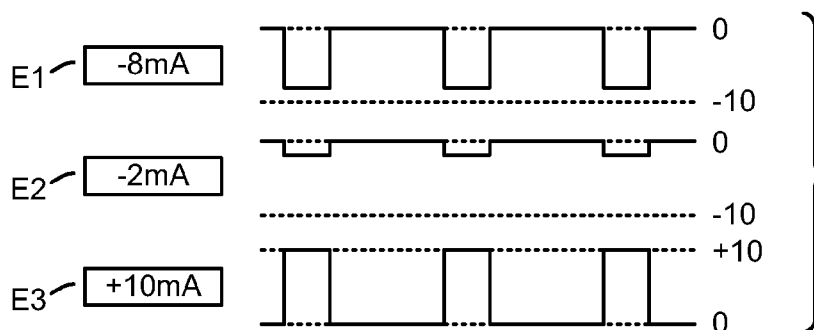

↓ (click down)

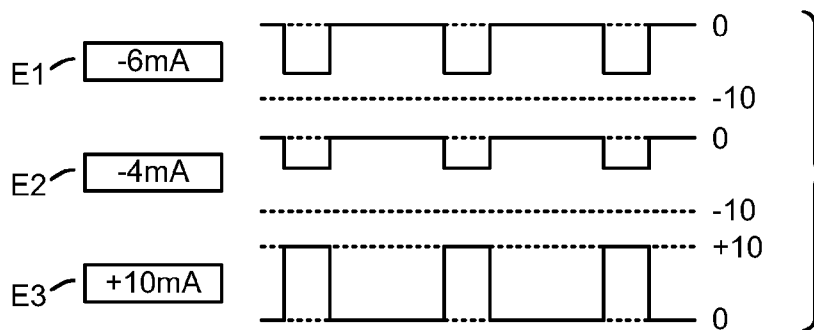


⋮



Figure 5
(prior art)

7/11

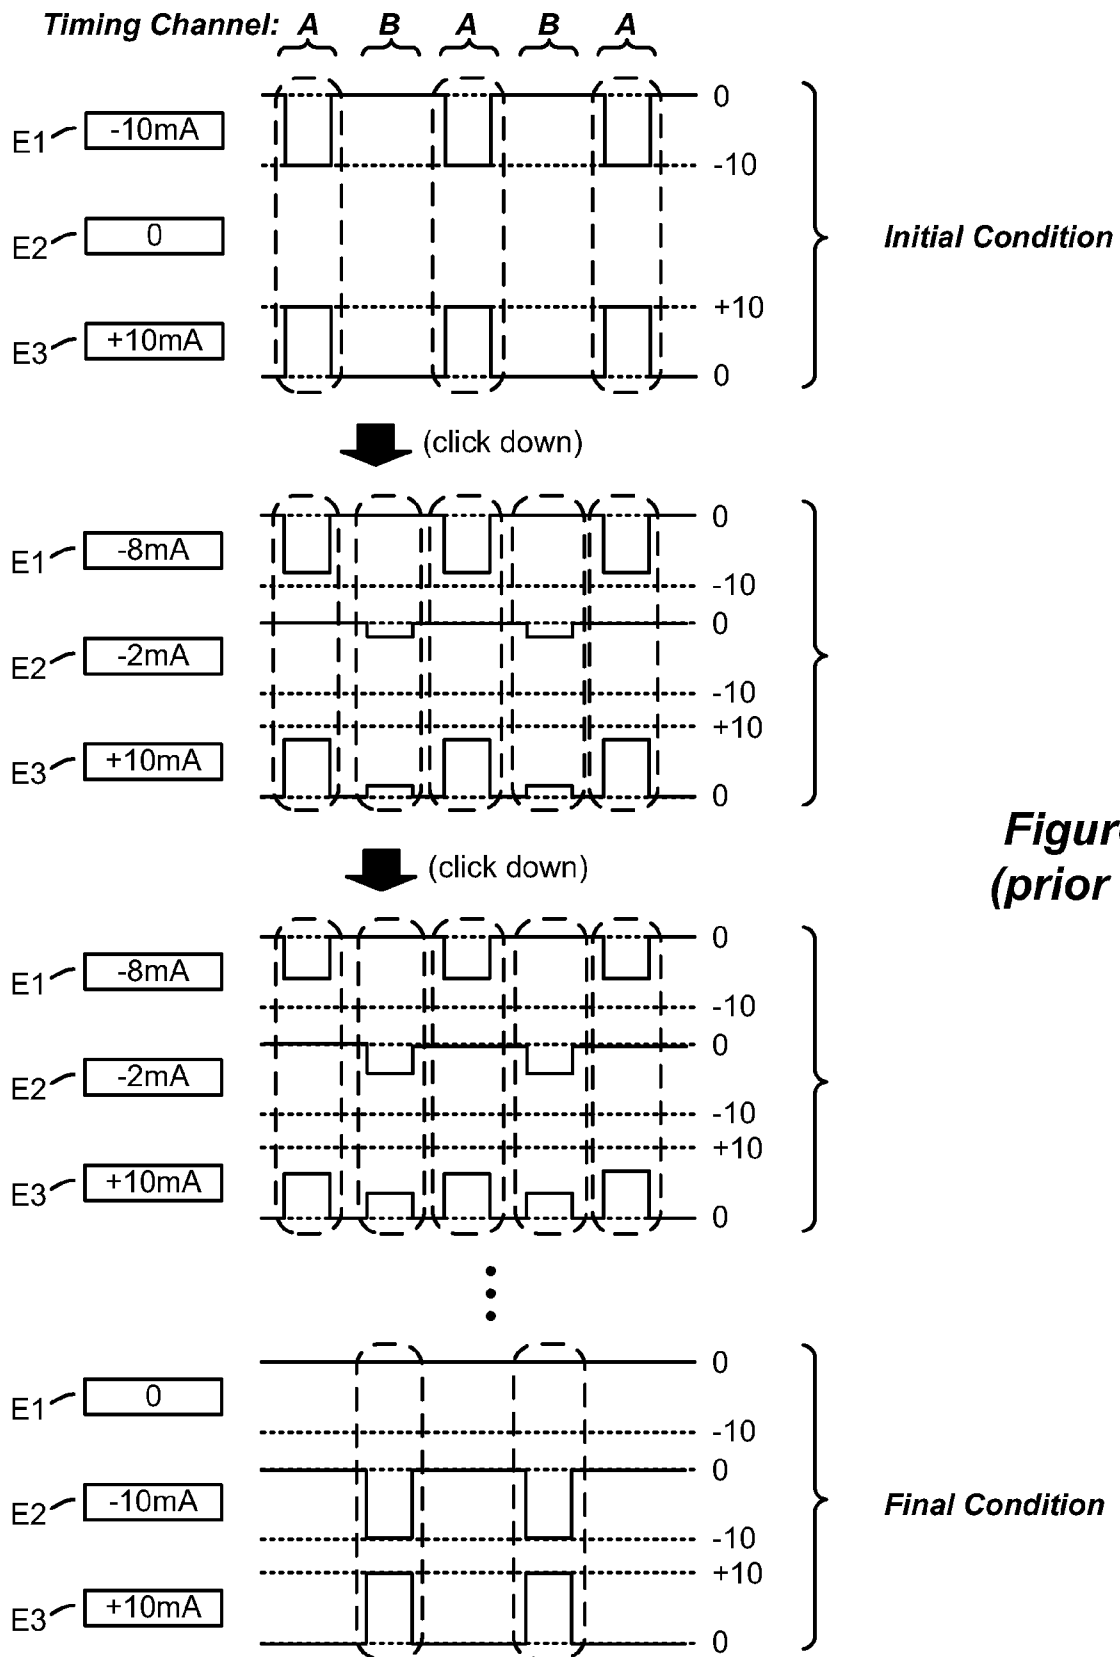

8/11



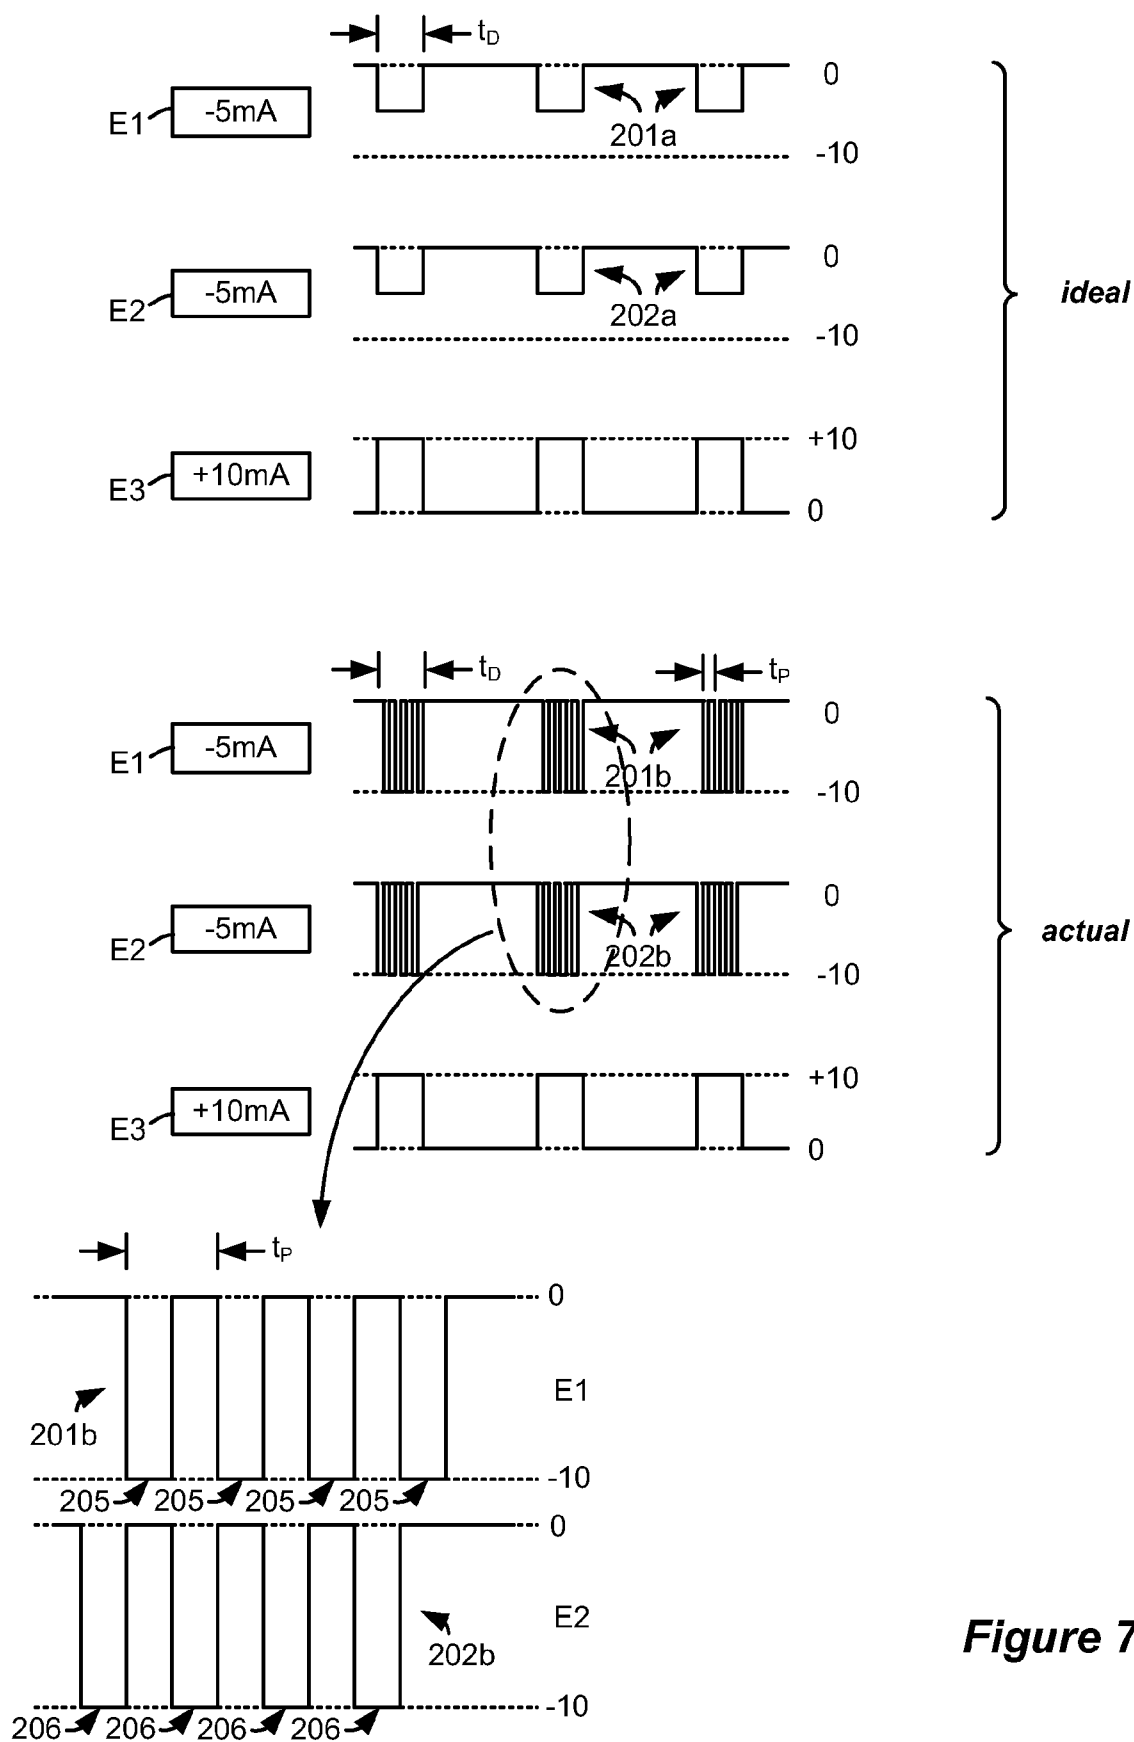


Figure 7A


9/11

**Figure 7B**


10/11

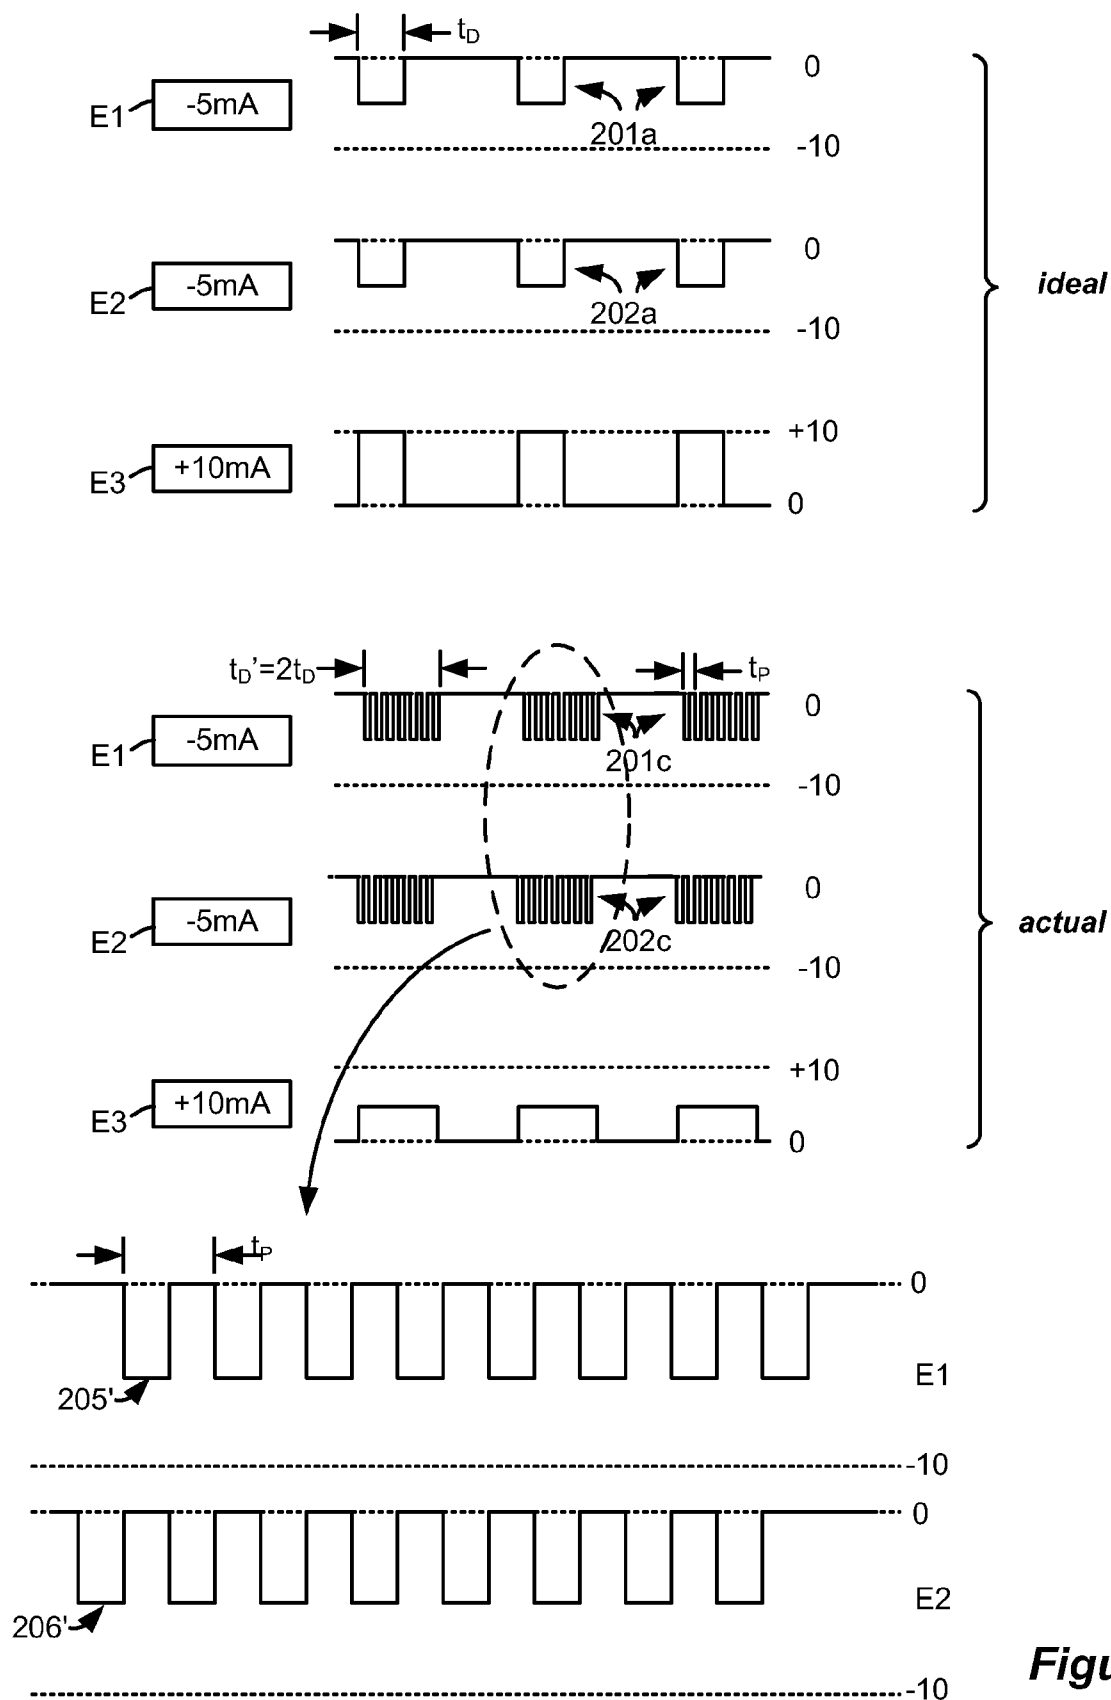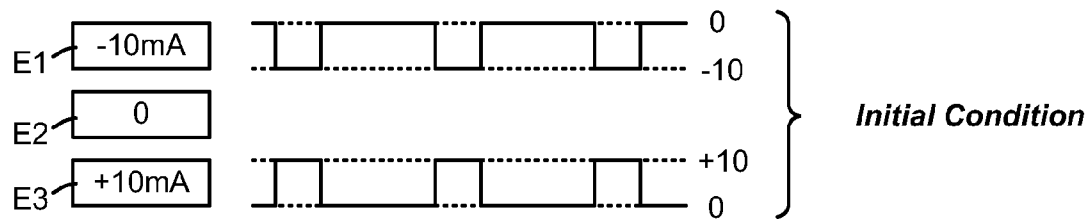

↓ (click down)

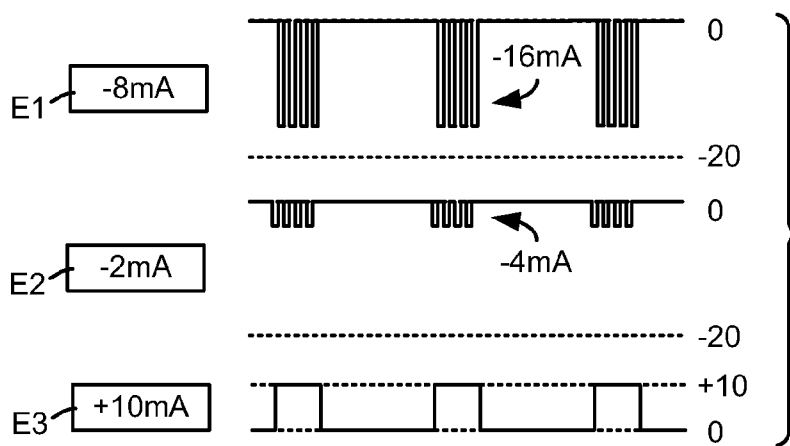

↓ (click down)

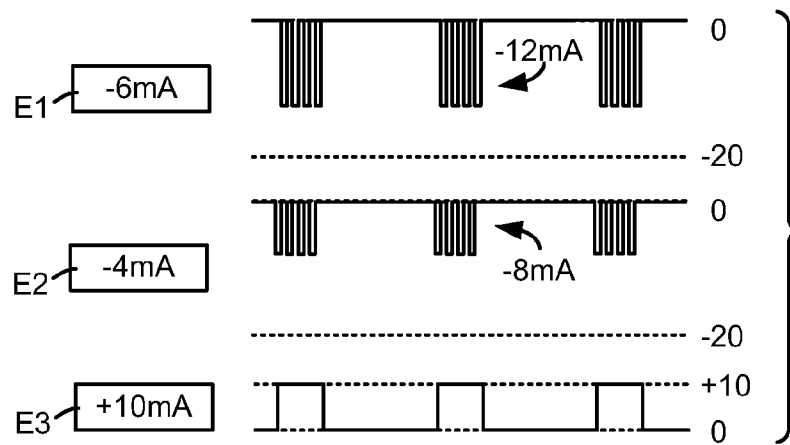


↓ (click down)


Fig. 8B

Figure 8A

Fig. 7A

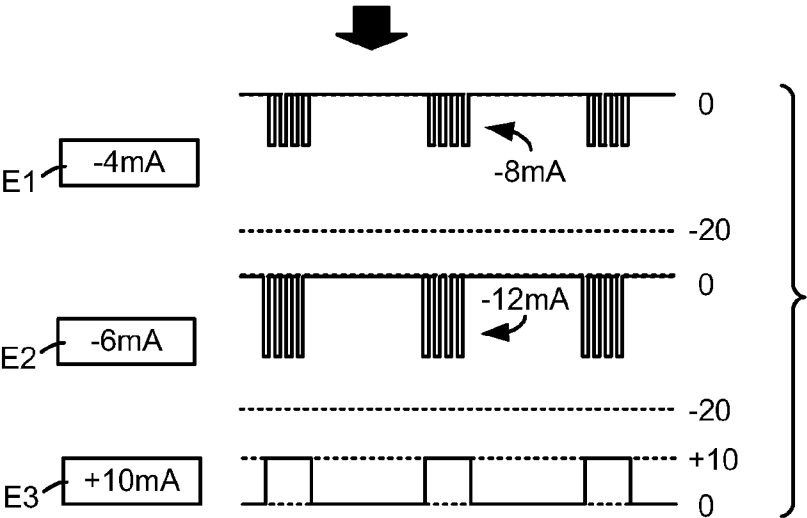

(click down)

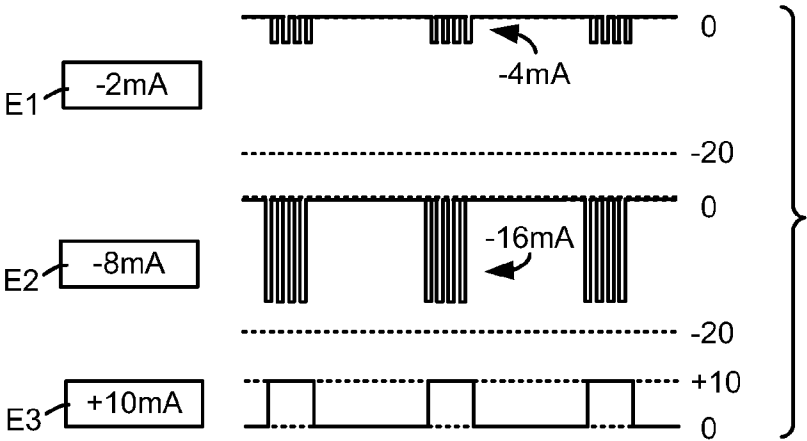

(click down)

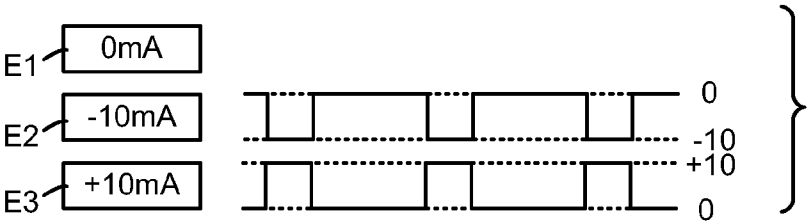


Figure 8B

Final Condition

PCT

DECLARATION OF NON-ESTABLISHMENT OF INTERNATIONAL SEARCH REPORT

(PCT Article 17(2)(a), Rules 13ter.1(c) and Rule 39)

Applicant's or agent's file reference 585-0058WO	IMPORTANT DECLARATION	Date of mailing(day/month/year) 14/07/2009
International application No. PCT/US2009/038741	International filing date(day/month/year) 30/03/2009	(Earliest) Priority date(day/month/year) 15/05/2008
International Patent Classification (IPC) or both national classification and IPC A61N1/34		
Applicant BOSTON SCIENTIFIC NEUROMODULATION CORPORATION		

This International Searching Authority hereby declares, according to Article 17(2)(a), that **no international search report will be established** on the international application for the reasons indicated below

1. ☒ The subject matter of the international application relates to:

- a. ☐ scientific theories
- b. ☐ mathematical theories
- c. ☐ plant varieties
- d. ☐ animal varieties
- e. ☐ essentially biological processes for the production of plants and animals, other than microbiological processes and the products of such processes
- f. ☐ schemes, rules or methods of doing business
- g. ☐ schemes, rules or methods of performing purely mental acts
- h. ☐ schemes, rules or methods of playing games
- i. ☒ methods for treatment of the human body by surgery or therapy
- j. ☒ methods for treatment of the animal body by surgery or therapy
- k. ☐ diagnostic methods practised on the human or animal body
- l. ☐ mere presentations of information
- m. ☐ computer programs for which this International Searching Authority is not equipped to search prior art

2. ☒ The failure of the following parts of the international application to comply with prescribed requirements prevents a meaningful search from being carried out:

☐ the description ☒ the claims ☐ the drawings

3. ☐ A meaningful search could not be carried out without the sequence listing; the applicant did not, within the prescribed time limit:

- ☐ furnish a sequence listing on paper complying with the standard provided for in Annex C of the Administrative Instructions, and such listing was not available to the International Searching Authority in a form and manner acceptable to it.
- ☐ furnish a sequence listing in electronic form complying with the standard provided for in Annex C of the Administrative Instructions, and such listing was not available to the International Searching Authority in a form and manner acceptable to it.
- ☐ pay the required late furnishing fee for the furnishing of a sequence listing in response to an invitation under Rule 13ter.1(a) or (b).

4. ☐ A meaningful search could not be carried out without the tables related to the sequence listings; the applicant did not, within the prescribed time limit, furnish such tables in electronic form complying with the technical requirements provided for in Annex C-bis of the Administrative Instructions, and such tables were not available to the International Searching Authority in a form and manner acceptable to it.

5. Further comments:

Name and mailing address of the International Searching Authority  European Patent Office, P.B. 5818 Patentlaan 2 NL-2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo nl, Fax: (+31-70) 340-3016	Authorized officer Eva San Miguel
--	--

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 203

A meaningful search is not possible on the basis of all claims because all claims are directed to - Method for treatment of the human or animal body by therapy - Rule 39.1(iv) PCT. The independent claims (1, 10, 16, and 25) comprise the step of applying therapeutical stimulation to the human body.

The applicant's attention is drawn to the fact that claims relating to inventions in respect of which no international search report has been established need not be the subject of an international preliminary examination (Rule 66.1(e) PCT). The applicant is advised that the EPO policy when acting as an International Preliminary Examining Authority is normally not to carry out a preliminary examination on matter which has not been searched. This is the case irrespective of whether or not the claims are amended following receipt of the search report or during any Chapter II procedure. If the application proceeds into the regional phase before the EPO, the applicant is reminded that a search may be carried out during examination before the EPO (see EPO Guideline C-VI, 8.2), should the problems which led to the Article 17(2)PCT declaration be overcome.