




(86) Date de dépôt PCT/PCT Filing Date: 2000/07/21
(87) Date publication PCT/PCT Publication Date: 2001/02/01
(45) Date de délivrance/Issue Date: 2009/05/26
(85) Entrée phase nationale/National Entry: 2002/01/24
(86) N° demande PCT/PCT Application No.: US 2000/040449
(87) N° publication PCT/PCT Publication No.: 2001/006935
(30) Priorité/Priority: 1999/07/26 (US09/360,709)

(51) Cl.Int./Int.Cl. *A61B 17/06* (2006.01),
A61F 2/24 (2006.01)
(72) Inventeurs/Inventors:
COHN, WILLIAM, US;
MATHERS, THOMAS P., US
(73) Propriétaires/Owners:
BETH ISRAEL DEACONESS MEDICAL CENTER, US;
GENZYME CORPORATION, US
(74) Agent: BORDEN LADNER GERVAIS LLP

(54) Titre : SYSTÈME DE SUTURE
(54) Title: SUTURE SYSTEM

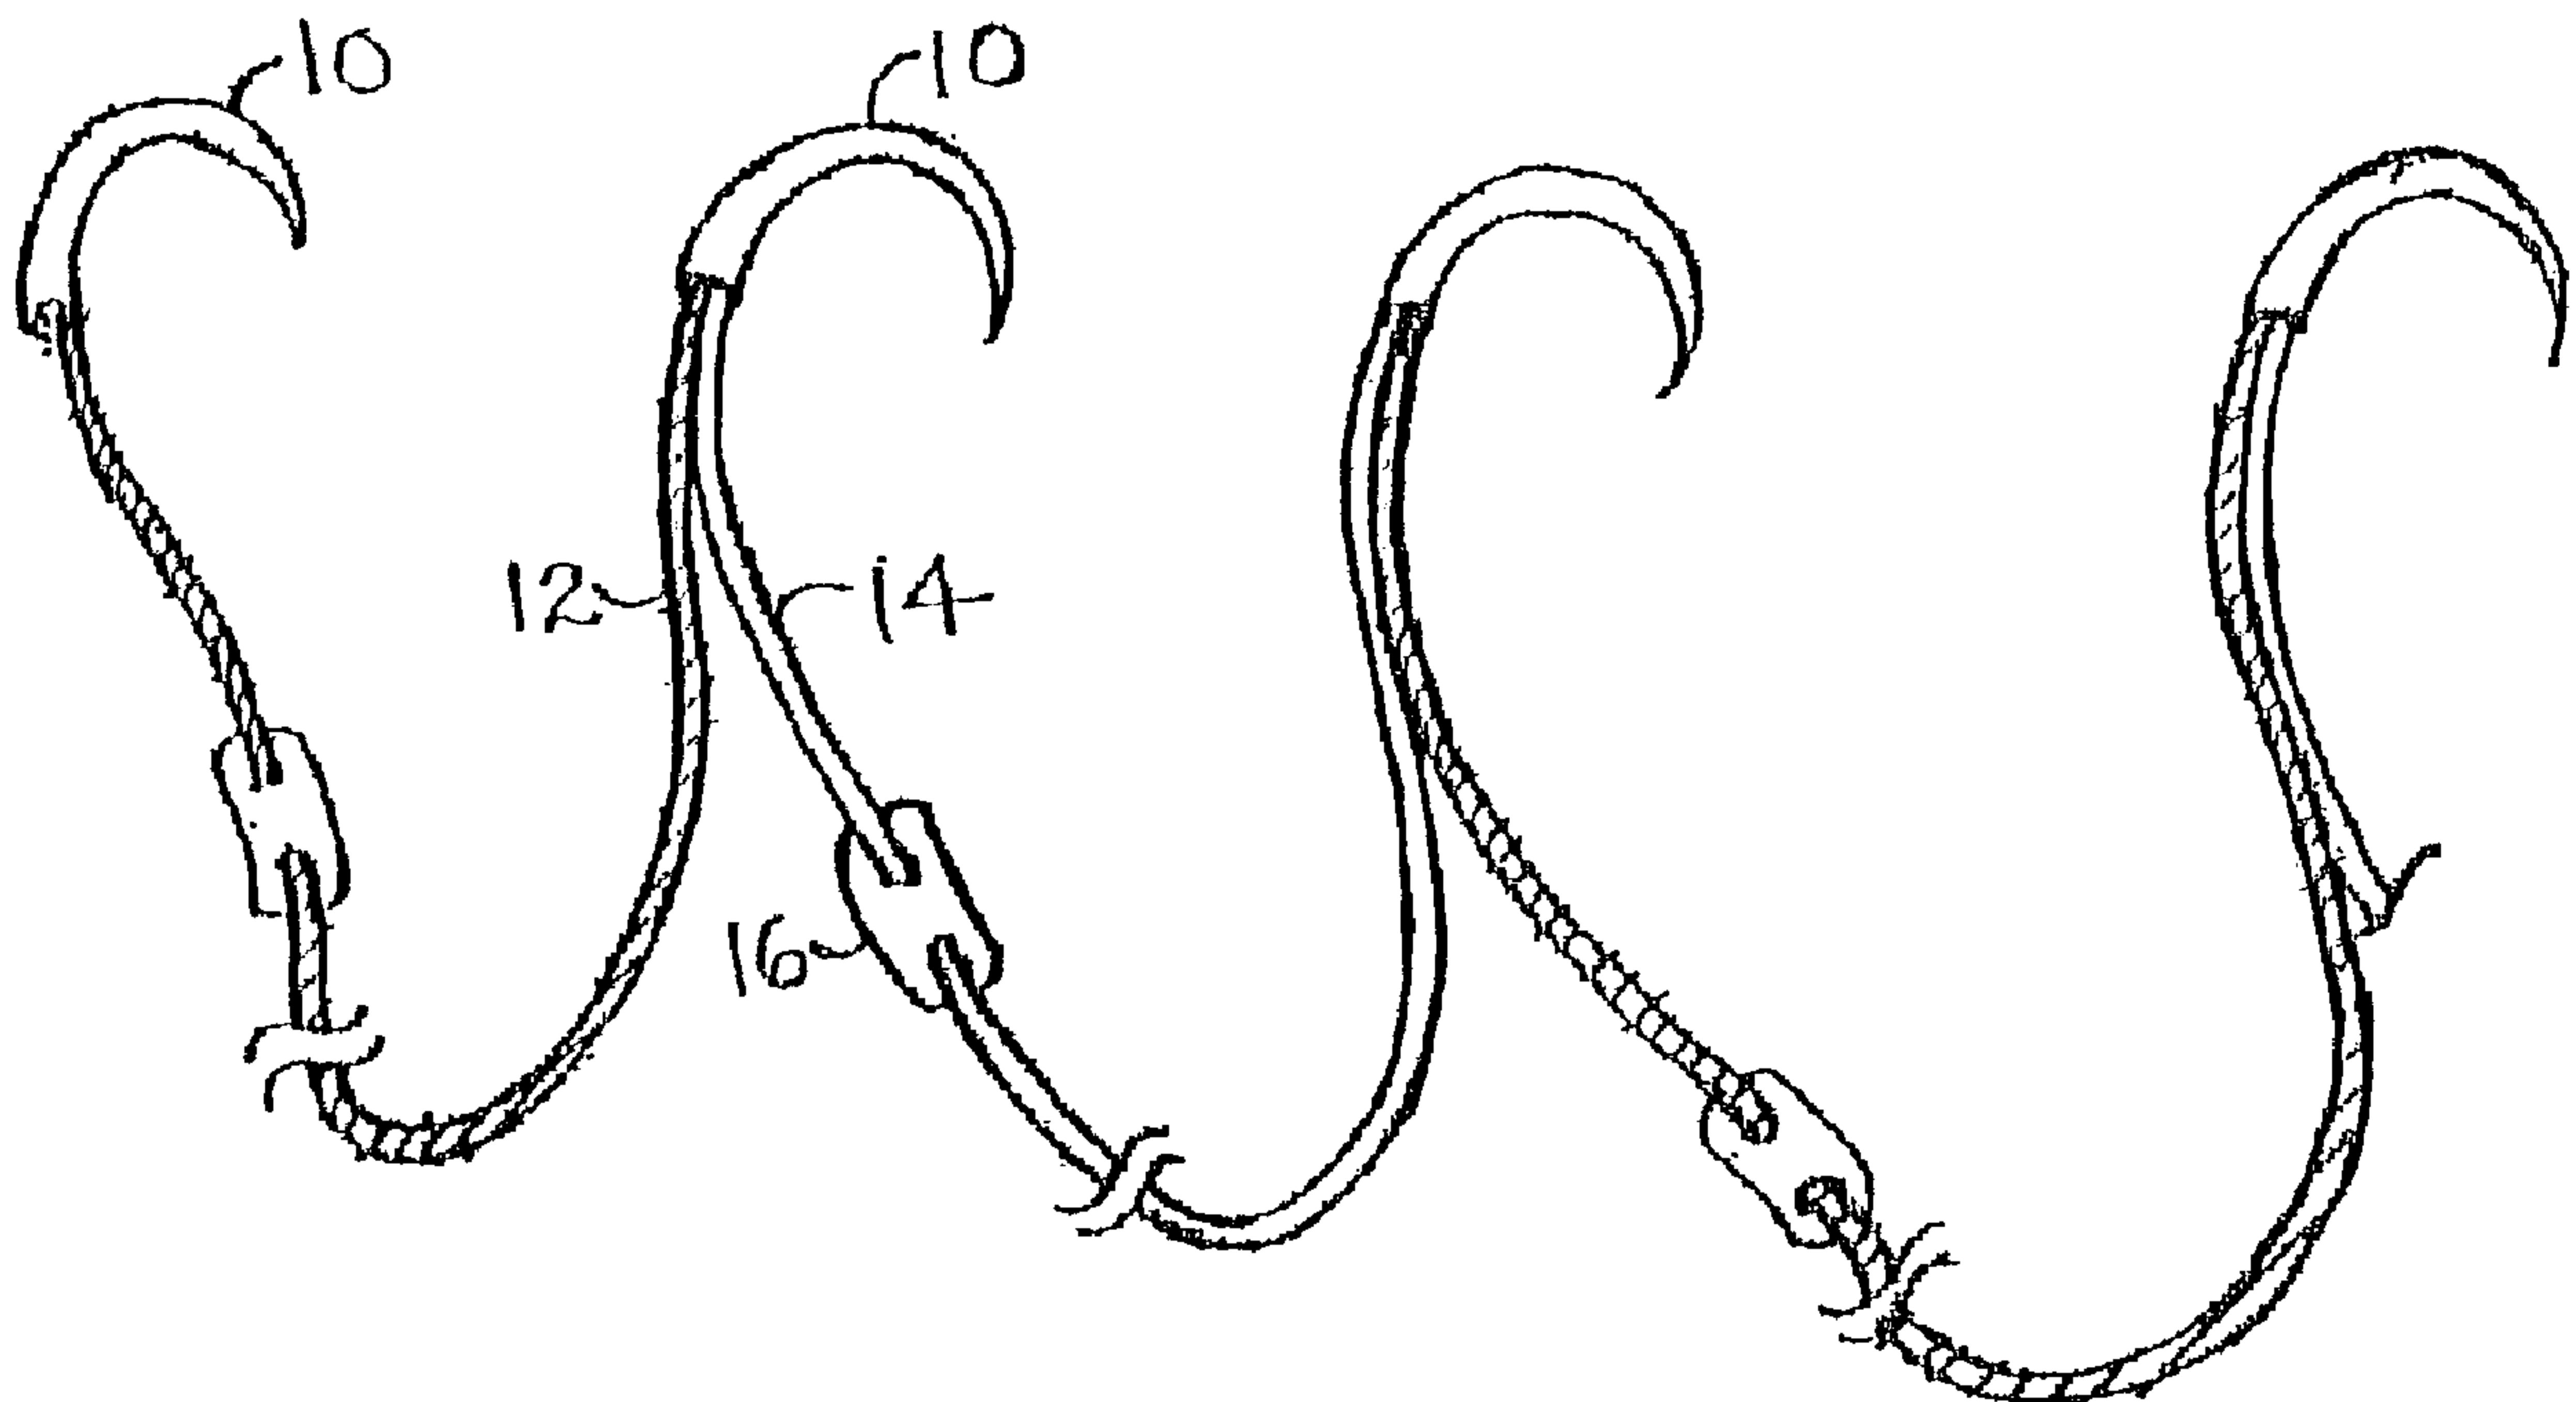

(57) Abrégé/Abstract:

A suture system includes a plurality of double-stranded needles (10) connected in sequence with a single-stranded needle (10) at each end. The double-stranded suture needles (10) incorporate two suture strands (12, 14) into a single needle (10). The suture system of the present invention facilitates the implantation of valve prostheses.

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
1 February 2001 (01.02.2001)

PCT

(10) International Publication Number
WO 01/06935 A1

(51) International Patent Classification⁷: **A61B 17/06**,
A61F 2/24

(US). MATHERS, Thomas, P. [US/US]; 12 Courser
Brook Drive, Newbury, MA 01922 (US).

(21) International Application Number: PCT/US00/40449

(74) Agents: HOOVER, Thomas, O. et al.; Hamilton, Brook,
Smith & Reynolds, P.C., Two Militia Drive, Lexington, MA
02421 (US).

(22) International Filing Date: 21 July 2000 (21.07.2000)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
09/360,709 26 July 1999 (26.07.1999) US

(63) Related by continuation (CON) or continuation-in-part
(CIP) to earlier application:

US 09/360,709 (CON)
Filed on 26 July 1999 (26.07.1999)

(71) Applicants (for all designated States except US): BETH
ISRAEL DEACONESS MEDICAL CENTER [US/US];
330 Brookline Avenue, Boston, MA 02215 (US). GEN-
ZYME CORPORATION [US/US]; One Kendall Square,
Cambridge, MA 02139 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): COHN, William
[US/US]; 104 LaGrange Street, Chestnut Hill, MA 02467

(81) Designated States (national): AE, AG, AL, AM, AT, AU,
AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CR, CU, CZ,
DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR,
HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR,
LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ,
NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM,
TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.


(84) Designated States (regional): ARIPO patent (GH, GM,
KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian
patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European
patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE,
IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG,
CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).

Published:

- With international search report.
- Before the expiration of the time limit for amending the
claims and to be republished in the event of receipt of
amendments.

For two-letter codes and other abbreviations, refer to the "Guid-
ance Notes on Codes and Abbreviations" appearing at the begin-
ning of each regular issue of the PCT Gazette.

(54) Title: SUTURE SYSTEM

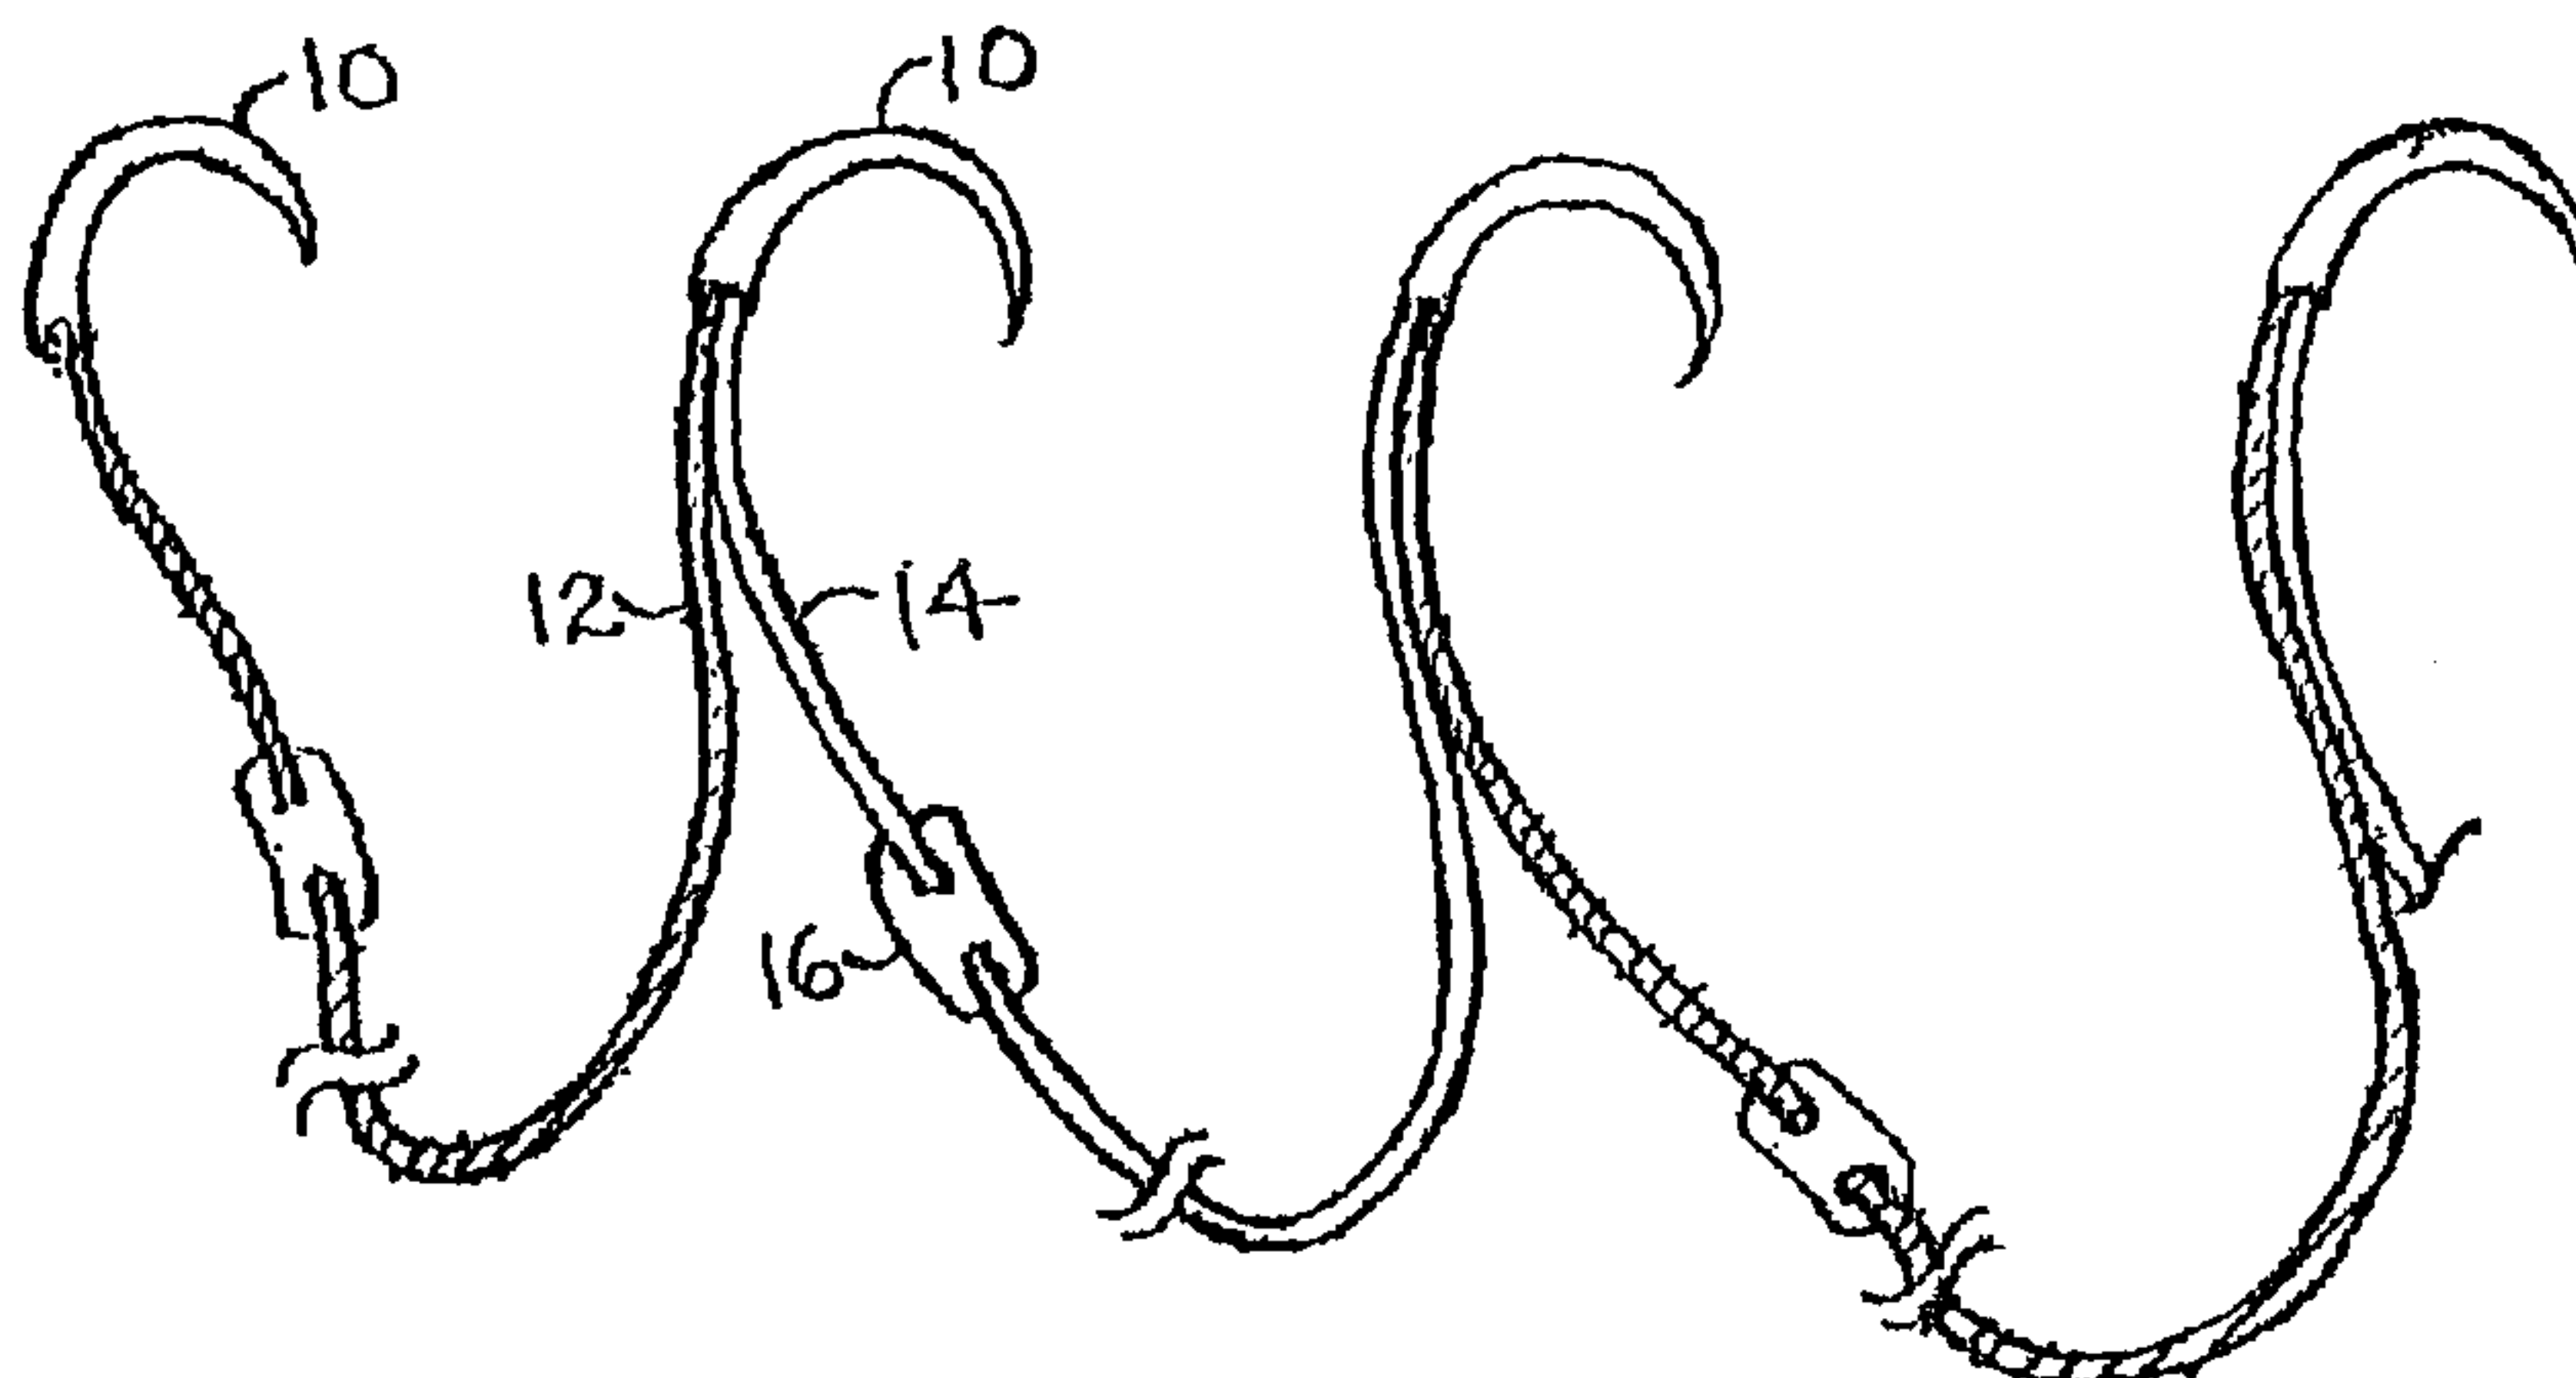

(57) Abstract: A suture system includes a plurality of double-stranded needles (10) connected in sequence with a single-stranded needle (10) at each end. The double-stranded suture needles (10) incorporates two suture strands (12, 14) into a single needle (10). The suture system of the present invention facilitates the implantation of valve prostheses.



WO 01/06935 A1

SUTURE SYSTEM

BACKGROUND OF THE INVENTION

By far the most frequently used technique for implantation of prosthetic valves such as aortic and mitral valves is to use pledgeted mattress sutures. The
5 term "mattress" refers to the fact that each suture passes through the fabric suturing ring or cuff of the prosthetic valve and through the tissue to which the prosthesis will be attached at two points separated, for example, by a gap of about 4 to 8 mm and more preferably between about 4 to 6 mm. To facilitate this, the piece of suture material has two surgical needles pre-attached, one at each end. The term "suture" refers to the composite of suture material and needles. The suture material for valve
10 prosthesis implantation is typically made of nonabsorbable polyester. When the two ends of a single suture, are tied together, a 4-8 mm segment of the circumference of the valve ring and the circumference of the annulus, (the rim of heart tissue that remains after excision of the dysfunctional native valve, and to which the prosthesis is sutured) are compressed tightly together.

15 To decrease the likelihood of the suture pulling through the annular tissue as tension is applied during tying, most surgeons use pledgeted sutures. A "pledget" is a small flat absorbent pad used to protect a wound. It is made from a piece of PTFE coated felt from a polyester material, through which both needles of the suture have been passed. The size of the pledget varies with a preferred size of 4x8 mm.

20 Sutures usually come pre-pledgeted from the manufacturer in multi-packs for valve implantation. When pledgeted sutures are used, generally both needles are passed through the annular tissue as the initial step in such a way that the pledget lies in

-2-

direct contact with the tissue and helps to distribute the force supplied to the 4-8 mm of tissue that lies between the two points of suture penetration. When tied, the annular circumference is compressed between the suturing ring of the prosthesis and the pledget. Multiple sutures are required to create this fluid tight compressive force
5 between the tissue and the prosthesis.

In order to prevent leakage of blood between the prosthetic valve and the tissue annulus post operatively, accurate spacing of the multiple discrete sutures is essential. Tight compression between the tissue and the prosthetic ring is readily achieved if the two ends of the mattress sutures are tightly tied together. Peri-
10 valvular leakage, when it occurs, is more commonly the result of an excessive distance separating two neighboring pledgets. As such, it is essential to pass the first needle (that is to say, the first of any given pair, the pair consisting of the two ends of a single suture) through the annulus as close as possible to the second suture of the neighboring pair. This must be accomplished, however, without actually
15 piercing the preceding suture. Valve sutures are a braided multifilament material and it is possible to pass one suture around or through the interstices of the neighboring strand. Although not always readily apparent at the time, this passing of one suture through the interstices of the adjacent strand may result in suture breakage when the sutures are tied, or in poor seating of the valve due to unevenly
20 distributed tension.

To ensure that the entire circumference of the prosthesis is seated in the annulus in a fluid tight fashion, multiple sutures are required. If the diameter of the annulus is 29 mm, which is quite common in mitral valve replacement, and the mattress sutures are placed such that each encompasses 5 mm of annulus,
25 approximately 18 discrete mattress sutures are required which involves passing 36 needles initially through the tissue, and subsequently through the suturing ring. As described above, every other stitch is technically more demanding and slightly more time consuming because of the increased precision required to pass extremely close to the preceding suture but without piercing it. As space is often quite limited when
30 working inside the heart, the entire exercise can be very demanding. There is thus a

-3-

continued need to provide improved suture devices and systems to accommodate small incisions associated with minimally invasive surgery and to simplify procedures for the implantation of prosthetic valves.

SUMMARY OF THE INVENTION

5 The invention consists of a configuration whereby a plurality of double-stranded needles are connected in sequence with a single-strand needle at each end. Each double-stranded needle incorporates two suture strands or threads on a single needle. In a preferred embodiment, the suture strands can alternate in color. Thus any given pair of needles are connected by a first strand of a first color and the next
10 needle is connected with a second strand of a second color. A plurality of pledgets can be provided on the strands and can be arranged in a "daisy chain" configuration with a single pledget or pad positioned between each pair of needles in the chain.

 In a preferred embodiment, the suture system of the present invention may contain several co-braided monofilament suture strands, where two suture strands of
15 different colors, such as green and white, are co-braided into a single suture strand creating a third suture color or striped suture. This additional color suture provides differentiation between the other suture strands and acts as a visual indicator when tying off the sutures.

 The needle to double suture ratio is greater than 1:1 but does not exceed 3:1.
20 This needle to double suture ratio is defined as the ratio of the needle wire diameter to twice the diameter of the suture. Thus, the needle is at least as large in cross-section as the strands being drawn through tissue by the needle.

 The suture system of the present invention results in a significant reduction and more particularly a reduction of between about forty to fifty percent (40-50%) in
25 the number of needles and steps required to implant a prosthetic heart valve, and also reduces the time required for the procedure and the incidence of suturing errors. The suture system of the present invention provides many advantages to a surgeon. The surgeon can achieve proper spacing of the adjacent sutures which reduces the risk of peri-valvular leakage or interstitial bleeding that can occur as a result of

-4-

using the interrupted sutures of the prior art. Further, there is a reduced risk for the needle to damage the adjacent suture as a result of trying to achieve the exact placement of the adjacent sutures that can occur with the interrupted suture technique. As the suture system of the present invention is provided with an
5 alternating color such as a green and white suture strands and the option of using a third color suture positioned within the suture chain, confusion in determining which pairs of suture strands tie together is also substantially reduced. The spacing between two pledgets does not exceed 1-2 mm and more preferably, the pledgets are in abutting contact with each other.

10 Another preferred embodiment of the present invention includes a method to implant a valve prosthesis using the suture system of the present invention. The method begins, for example, by making a partial or full median sternotomy, thoracotomy or parasternal incision. In this embodiment, the patient is placed on a cardiopulmonary bypass so that the heart can be stopped. The diseased valve is then
15 accessed and excised, and the prosthetic valve then sutured using the suture system of the present invention.

The method further comprises placing the first suture in the tissue using a single-stranded or armed needle. The next double-stranded needle is then taken and a second stitch is placed in the annulus of the valve site approximately 4-6 mm from
20 where the first stitch was placed. Because the second needle is double-stranded, the second stitch places the second stitch of the first suture along with the first stitch of the second suture. The following sutures are placed using the double-stranded needles, 4-6 mm from the previous suture placement until the entire circumference of the valve annulus has been sutured.

25 Once the entire circumference of the valve annulus has been sutured, the prosthetic valve is sutured. The prosthetic valve is held approximately 5 cm above the valve annulus during suturing. The sutures are placed through the cuff of the prosthetic valve using first a single-armed or stranded needle to place the first suture and then using the double-stranded needles placed through the cuff so that the pairs
30 of sutures are evenly spaced around the circumference of the cuff. The prosthetic

-5-

valve is aligned with the valve annulus. Once the sutures have been placed around the entire circumference of the cuff, the valve is lowered into position, the needles are cut off the sutures and the sutures are tied. The optional third color suture aids in tying off the sutures by acting as an additional visual indicator to differentiate
5 between the suture strands associated with each pad or pledget. The prosthetic valve is then tested and the incision is closed.

The suture system of the present invention has different applications for many commonly performed medical procedures. For example, the suture system can be used in surgical procedures to correct ventricular aneurysms, atrial septal
10 defects, and ventricular septal defects. Further, the suture system of the present invention can be used in procedures such as implanting of left ventricular assist devices. Aortic and mitral valve annuloplasty can also use the suture system of the present invention. In a preferred embodiment mechanical or electromechanical systems can be used in holding or manipulating the sutures during surgery.

15 The foregoing and other objects, features and advantages of the invention will be apparent from the following more particular description of preferred embodiments of the invention, as illustrated in the accompanying drawings in which like reference characters refer to the same parts throughout the different views. The drawings are not necessarily to scale, emphasis instead being placed upon
20 illustrating the principles of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 is a schematic illustration of a suture system in accordance with the present invention.

Figure 2 is a schematic illustration of a plurality of sutures in accordance
25 with the present invention.

Figure 3A is a schematic illustration of the suture system in accordance with the present invention during the implantation of a prosthetic valve.

Figure 3B is an enlarged view of a suture shown in Figure 3A.

-6-

Figure 4 is a schematic illustration of a preferred embodiment of the suture system in accordance with the present invention.

Figure 5 is a schematic illustration of another preferred embodiment of the suture system in accordance with the present invention.

5 Figure 6 is a schematic illustration of an embodiment of the suture system of the present invention including three-color sutures.

Figure 7 is a schematic illustration of the suture system being used in a mitral valve replacement procedure including an automated robotic apparatus in accordance with the present invention.

10 Figure 8 is an enlarged view illustrating the pledgets of the suture system as they are sutured during valve replacement surgery.

Figure 9 is a schematic illustration of a prosthetic heart valve being secured using the suture system of the present invention.

15 Figure 10 is a schematic illustration of an aortic valve being secured using the suture system according to the present invention.

Figure 11 is a flowchart of a method for performing a valve prosthesis using the suture system in accordance with the present invention.

DETAILED DESCRIPTION OF THE INVENTION

The present invention relates to a suture system for implanting valved
20 prostheses. Valve implantation, such as cardiac valve implantation, consists of complex suturing process. This includes the placement of multiple mattress sutures in the tissue at the valve site, as well as to the suturing ring or cuff of the valve prostheses. This procedure is complicated by a very small working space inside the arteriotomy or aortotomy in order to excise the diseased native valve, then implant
25 the prosthetic valve. In order to prevent perivalvular leakage and proper seating of the prosthetic valve, the surgeon normally places multiple (i.e., 14 or more) double-ended, pledgeted sutures in mattress or other configuration through both the in-situ annulus of the native, removed valve, and the suturing ring or cuff of the prosthetic valve. The suture strands are made of nonabsorbable polyester and are of a fixed

-7-

length with a needle attached on both ends. The pledgets are made of PTFE or similar material. The pledgets or pads are absorbent patches used to protect a wound. The pledgets are in square, rectangular, oval, circular or other shape with a pair of holes or openings through which a single suture strand passes. The size of the pledget varies with a preferred size of 4x8 mm. In the alternative, a non-pledgeted suture system can also be used with only the suture strands with a needle attached on both ends.

Because of the complex anatomy, precision needed, and small working space, valve implantation suturing is very tedious and slow. Often times, tissue locations are hidden and are difficult to access for suturing. Typically one-third of the stitches are difficult to sew with every other stitch being more difficult to sew because of tight spacing. In order to minimize the risk of perivalvular leakage, a surgeon commonly tries to place each new suture's first needle pass in the annulus and sewing ring as close to the prior suture's exit path in both structures, without actually going through the same entry and exit hole. If the suture were to pass in the same entry and exit hole, the surgeon would most likely split or impale the previous suture, which is commonly referred to as "William Tell." This may cause the suture to break when it is tied or it may cause the valve to leak due to the application of unequal pressure to the valve annulus. Therefore, this occurrence would require the surgeon to remove the previous suture and start over.

The present invention suture system consists of a daisy chain of multiple pre-pledgeted mattress sutures joined at the needles. Referring to Figures 1 and 2, each needle 10 in the chain is attached to two strands of suture 12, 14, rather than a single strand as in the prior art. One of the strands 12 is the first of a pair, in a standard mattress suture. The other, however, is the second strand 14 of the of the preceding neighboring pair. Pairs are of alternating color, for example green or white, to allow for individual pairs to be differentiated at a glance. Pledgets 16 are sewn throughout the sutures. As discussed hereinabove, to ensure that the entire circumference of the prosthesis is seated in the annulus in a fluid tight fashion, multiple sutures are required. If the diameter of the tissue annulus is 29 mm, which is typical in mitral

-8-

valve replacement, and the mattress sutures are placed such that each encompasses 5 mm of annulus, for example, approximately 18 discrete mattress sutures are required (29 mm x 3.14/5mm). As such, in order to place 18 pledgeted sutures the surgeon needs only to pass 20 needles, rather than 36 required by the conventional technique.

5 A single suture system preferably uses at least three needles and can have as many needles as necessary for a given procedure. A preferred embodiment uses multiples of three in a given system such as six, nine, twelve, etc. However, the number in a given system depends upon the specific application. A given suture set can be packaged for sterile delivery and ease of use.

10 Furthermore, the present invention addresses the technical demands imposed by spacing requirements. The two strands that are preferably spaced as close as possible without piercing each other are now attached to the same needle. They therefore pass through the same hole in both the tissue and the prosthetic suturing ring intimately in contact with each other, with no chance of one passing around or
15 through the interstices of the other. The net number of steps required for valve implantation is almost cut in half. In addition, the demands of obtaining close proximity without suture penetration is substantially reduced.

Referring to Figure 3, in order to facilitate the description of this suture system, each needle, suture and pledget is labelled. As such, each suture is defined
20 as 1, 2, 3...etc., each needle 10 is identified on each suture as either 1A, 1B2A, 2B3A, 3B4A,...etc., and each pledget 16 is identified as being attached to its suture 1,2,3...etc. The present invention suture device is a system, which consists of multiple, needles 10 which are pre-attached in either a drilled or channeled configuration to two (2) independent, pre-pledgeted or non-pledgeted sutures of
25 alternating suture 12, 14 colors. In this configuration, the device in accordance with the present invention would be:

-9-

Needle	Suture(s) Attached	Pledget on Suture	Color of Suture (suture #)
1A	1	Yes, on 1	Green(1)
1B2A	1 and 2	Yes, on 1 and 2	White (2)
2B3A	2 and 3	Yes, on 2 and 3	Green (3)
5 3B4A	3 and 4	Yes, on 3 and 4	White (4)
Etc.			

This suture system allows approximately half (50%) as many needle 10 passes by combining two sutures 12, 14 to one needle. This also allows for both sutures to fill the same entry and exit holes in the annulus and suturing ring without splitting, or impaling one another. This suture configuration allows optimal seating of the valve without perivalvular leakage. The time for implantation is also dramatically reduced. Figure 3B is an enlarged view showing the pledget 16 on suture 12. The pre-pledgeted sutures can be packaged for delivering continuously attached valve sutures in a holder for either manual or mechanically aided delivery.

15 Referring to Figures 4 and 5, the suture system of the present invention contains three different colors x, y, and z of suture and shows 6 sutures. The three colors may alternate sequentially or a third color may be utilized in one or both of the end positions of the strand.

When using two colors of suture, for example X and Y, every hole contains 20 both color of suture. Therefore, after the needle 10 has been removed, some confusion can arise as to whether to tie a particular suture to the matching color from the hole on one side or the other of the selected suture. This confusion can also arise at the junction between two different strands of product. Although there are techniques that will enable the surgeon to make a correct determination when tying, 25 the three-color embodiment negates the need for such techniques.

The three-color embodiment facilitates identification of the end of the sutures which must be tied together during the tying process. This facilitation is due to the fact that the color combination of the two sutures in any given hole will be different from the two colors in the two adjacent holes. For example, the color 30 combination in a sequence of holes with suture colors X, Y and Z would be XY, YZ,

-10-

ZX, XY, YZ, ZX, etc. The three colors make it easier to determine which end of the suture to tie together as there is only one matching suture in the two adjacent holes.

Figure 6 illustrates a prosthetic valve 20 being implanted using the three color embodiment of the suture system of the present invention. Note that the valve
5 can have a pair of hinged flaps that are free to rotate between open and closed position. The valve annulus 24 is first sutured along the entire circumference. The prosthetic valve 20 is then sutured along the entire circumference of the cuff 26. The double-stranded needles place the second stitch of the first suture along with the first stitch of the second suture for example. This requires only one needle pass.
10 The two strands are thus as close as possible without piercing each other. The prosthetic valve 20 is aligned with the valve annulus 24 while suturing. Once the sutures 12, 14, 16 have been placed, the needles are cut off the sutures and the sutures are tied. Adjacent like color sutures are tied together as illustrated in Figure 6. The third color suture aids in tying off the sutures by acting as an additional
15 visual indicator to differentiate between the adjacent sutures. The pledgets are placed in an abutting relationship or at a distance from each other depending on the circumstances of each patient. The entire circumference of the prosthesis 20 is seated in the annulus 24 with the pledgets 16 and the tightly tied sutures 12, 14, 16 aiding in preventing leakage between the prosthetic valve 20 and the valve tissue
20 annulus 24.

A number of devices have been proposed for automating the process of suture placement to facilitate valve replacement. A device that takes advantage of the present invention daisy chain configuration has a significant advantage due to increased tolerances with respect to suture spacing. As such, the invention as stated
25 is an important integral part of an automated valve implantation device. Figure 7 illustrates a handheld mechanical automated or robotic placement device 30 that can be used with the suture system of the present invention. A robotic system including a pair of robotic arms 32 assists the suturing system of the present invention. The robotic arms 32 can be manipulated to hold and suture the prosthetic valve 20 to the
30 valve annulus tissue 24 with tight space tolerances. The movement of the robotic

-11-

arms are controlled by the surgeon who can have an optically magnified view of the valve annulus where the prosthetic valve is being implanted. In an alternative embodiment, a camera can assist the surgeon in viewing the area where the prosthetic valve is being implanted. Methods and apparatus for performing
5 minimally invasive cardiac procedures are disclosed in U.S. Patent Nos. 5,855,583, 5,911,036, 5,762,458, 5,807,377, 5,797,900 and 5,792,135.

Figure 8 illustrates the pledgets 16 sutured to the valve annulus tissue 24. The entire circumference of the valve annulus tissue 24 has pledgets 16 sutured thereto. The sutures are tied to the cuff 26 of the prosthetic valve 20 after the
10 prosthetic valve 20 is aligned with the valve annulus 24 and sutured thereto.

Figure 9 illustrates a mitral prosthetic valve 40 having a suturing cuff 42. The sutures are stitched around the circumference of the cuff 42. Figure 10 illustrates an aortic valve suturing process for implanting an aortic prosthetic valve using the suturing system of the present invention.

15 The method for performing the implantation of a valve prosthesis using the suture system of the present invention is illustrated in Figure 11 and begins in step 50 by making a partial or full median sternotomy, thoracotomy, or parasternal incision. The patient is then placed on cardiopulmonary bypass so that the heart can be stopped. Once the diseased valve is accessed, it is excised and the valve annulus
20 is sized to insure proper fit of the new prosthetic valve. The prosthetic valve is then sutured in place after the suture size and needle type are selected according to surgeon preference. The suture system and method of the present invention further includes a particular sequence of steps. In step 52, the surgeon places the first suture in the tissue annulus using either of the single-armed ends of the suture chain. Next
25 in step 54, the surgeon takes the next double-stranded suture and places the second stitch in the annulus approximately 4-6 mm from where the first stitch was placed. Because the second needle is double-stranded, the second stitch places the second stitch of the first suture along with the first stitch of the second suture. This requires only one needle pass as compared to two needle passes required with interrupted

-12-

sutures and there is exact placement of the adjacent suture. In step 56, the surgeon continues placing the sutures using the double armed needles, 4-6 mm from the previous suture placement, until the entire circumference of the valve annulus has been sutured. Again, the needles are double-stranded, thus placing the second stitch
5 of one suture with the first stitch of the next suture with only one needle pass. This reduces the number of needle passes almost in half of the two needle passes required for each suture when using the interrupted suture technique.

In this particular embodiment as illustrated in step 58, once the entire circumference of the tissue annulus has been sutured, the surgeon begins suturing
10 the prosthetic valve. The prosthetic valve is held approximately 5 cm above the valve annulus during suturing. The surgeon, per step 60, takes one of the single-armed needles and places the first suture through the cuff of the prosthetic valve. Then per step 62, the surgeon, continues sewing through the cuff of the prosthetic valve by taking the next double-stranded needle and placing it through the cuff, at a
15 distance from the previous needle's position such that the pairs of strands will be evenly spaced around the cuff. Note that with only one stitch of the double-stranded needle, the second stitch of the first suture along with the first stitch of the second suture is placed. This requires two needle passes when using interrupted sutures. Also, there is exact placement of the adjacent suture. In step 64, the surgeon
20 continues sewing through the cuff of the prosthetic valve using the double-stranded needles. The surgeon places each double-stranded needle through the sewing cuff of the prosthetic valve at a known distance mm from the previous suture placement, until the entire circumference of the valve annulus has been sutured. Careful attention is paid to the alignment of the prosthetic valve to the valve annulus.
25 Again, the needles are double-stranded, thus placing the second stitch of one suture with the first stitch of the next suture with only one needle pass. This reduces the number of needle passes almost in half of the two needle passes required for each suture when using interrupted suture.

Per step 66, once the sutures have been placed around the entire
30 circumference of the cuff, the valve is lowered into position, the needles are cut off

-13-

the sutures and the tying of the sutures begins. The optional third color suture can aid in tying off the sutures by acting as an additional visual indicator to differentiate between the sutures. Then, per step 68, the surgeon removes the excess strand material. The valve is tested to insure unimpaired opening and closing and the
5 incision is closed.

The present invention further includes a valve suture packaging system for delivering continuously attached sutures in a compact holder. The packaging (carrier) design enables the sutures to be used directly from the package at a location close to the surgical incision. The carrier is a compact folder which holds multiple
10 continuously attached sutures. The carrier top flap folds back forming a convenient handle which prevents the package from being compressed, restricting delivery of the sutures. Each suture is separately threaded through holes in the holder preventing the sutures from tangling during removal from the carrier. The structural design has folding panels permitting flexibility to utilize the holder for different
15 suture lengths. Needles are delivered extended from the package providing easy access, and are affixed in a foam strip for needle point protection. Pledgets are positioned above the foam to prevent catching and tangling.

While this invention has been particularly shown and described with references to preferred embodiments thereof, it will be understood by those skilled
20 in the art that various changes in form and details may be made therein without departing from the spirit and scope of the invention as defined by the appended claims.

CLAIMS

1. A suture device for suturing tissue comprising:
a plurality of double threaded needles in sequence, each needle of said plurality of double threaded needles being attached to two different suture strands, including a first suture strand being attached to each double threaded needle of the plurality of double threaded needles having a visual indicator and at least a second suture strand attached to each double threaded needle that is distinguished from the first strand by the visual indicator; and
a first end needle and a second end needle that are each attached at ends of the suture device with a single suture strand.
2. The suture device of claim 1 further comprising attaching a third double-threaded needle to at least two padded sutures.
3. The suture device of claim 1 wherein different suture strands have different indicators.
4. The suture device of claim 1 wherein the suture strands include three different colors.
5. The suture device of claim 3 further comprising tying ends of the sutures for each pad.
6. The suture device of claim 1 wherein a first suture strand is green and another suture strand is white.
7. The suture device of claim 4 wherein a third strand color is formed with a pair of braided strands.
8. A suture device for suturing tissue comprising:
a plurality of double-stranded needles connected in sequence with a single-stranded needle at each end, wherein each double-stranded needle incorporates two suture strands on a single thread and wherein the suture strands can alternate in color; and

-15-

a plurality of pledgets arranged in a chain configuration with a single pledget positioned between each pair of needles in the chain.

9. The suture device of claim 8, wherein the suture strands include strands of at least two different colors.
10. The suture device of claim 8, wherein the suture strands include strands of three different colors.
11. The suture device of claim 8, wherein the device has at least three needles and wherein each needle is connected by at least two suture strands.
12. The suture device of claim 8, wherein each pledget has a pair of apertures such that each suture strand extends through an aperture of said pledget.
13. The suture device of claim 8 further comprising a first needle attached to a single strand and a last needle attached to a single strand.
14. A suture device for suturing a prosthetic device to tissue comprising:

a plurality of at least three connected needles with at least one of the connected needles being attached to a double stranded suture, wherein at least one suture strand of the double stranded suture has a visual indicator that distinguishes it from the second suture strand, and wherein

each suture strand extends between a pair of the connected needles such that the suture strands can be identified with the visual indicator, the needles being removable from the suture strands after insertion through a prosthetic device and the ends of each strand identified and secured together to attach the device to the tissue.
15. The suture device of claim 14 wherein at least one suture strand comprises a co-braided strand.
16. The suture device of claim 14 wherein the suture strands have at least three colors.

-16-

17. The suture device of claim 14 wherein the first indicator comprises a first color and the second indicator comprises a second color.
18. The suture device of claim 14 further comprising a suture strand having a third color comprising a green strand braided with a white strand.
19. The suture device of claim 14 further comprising at least three needles with a first suture strand extending between a first pair of needles and a second suture strand extending between a second pair of needles.
20. The device of Claim 19 further comprising a first pledget attached to the first suture strand and a second pledget attached to the second suture strand.
21. The device of Claim 14 further comprising at least nine needles connected in a chain, each pair of needles having a suture strand extending there between with a pledget attached to each strand.

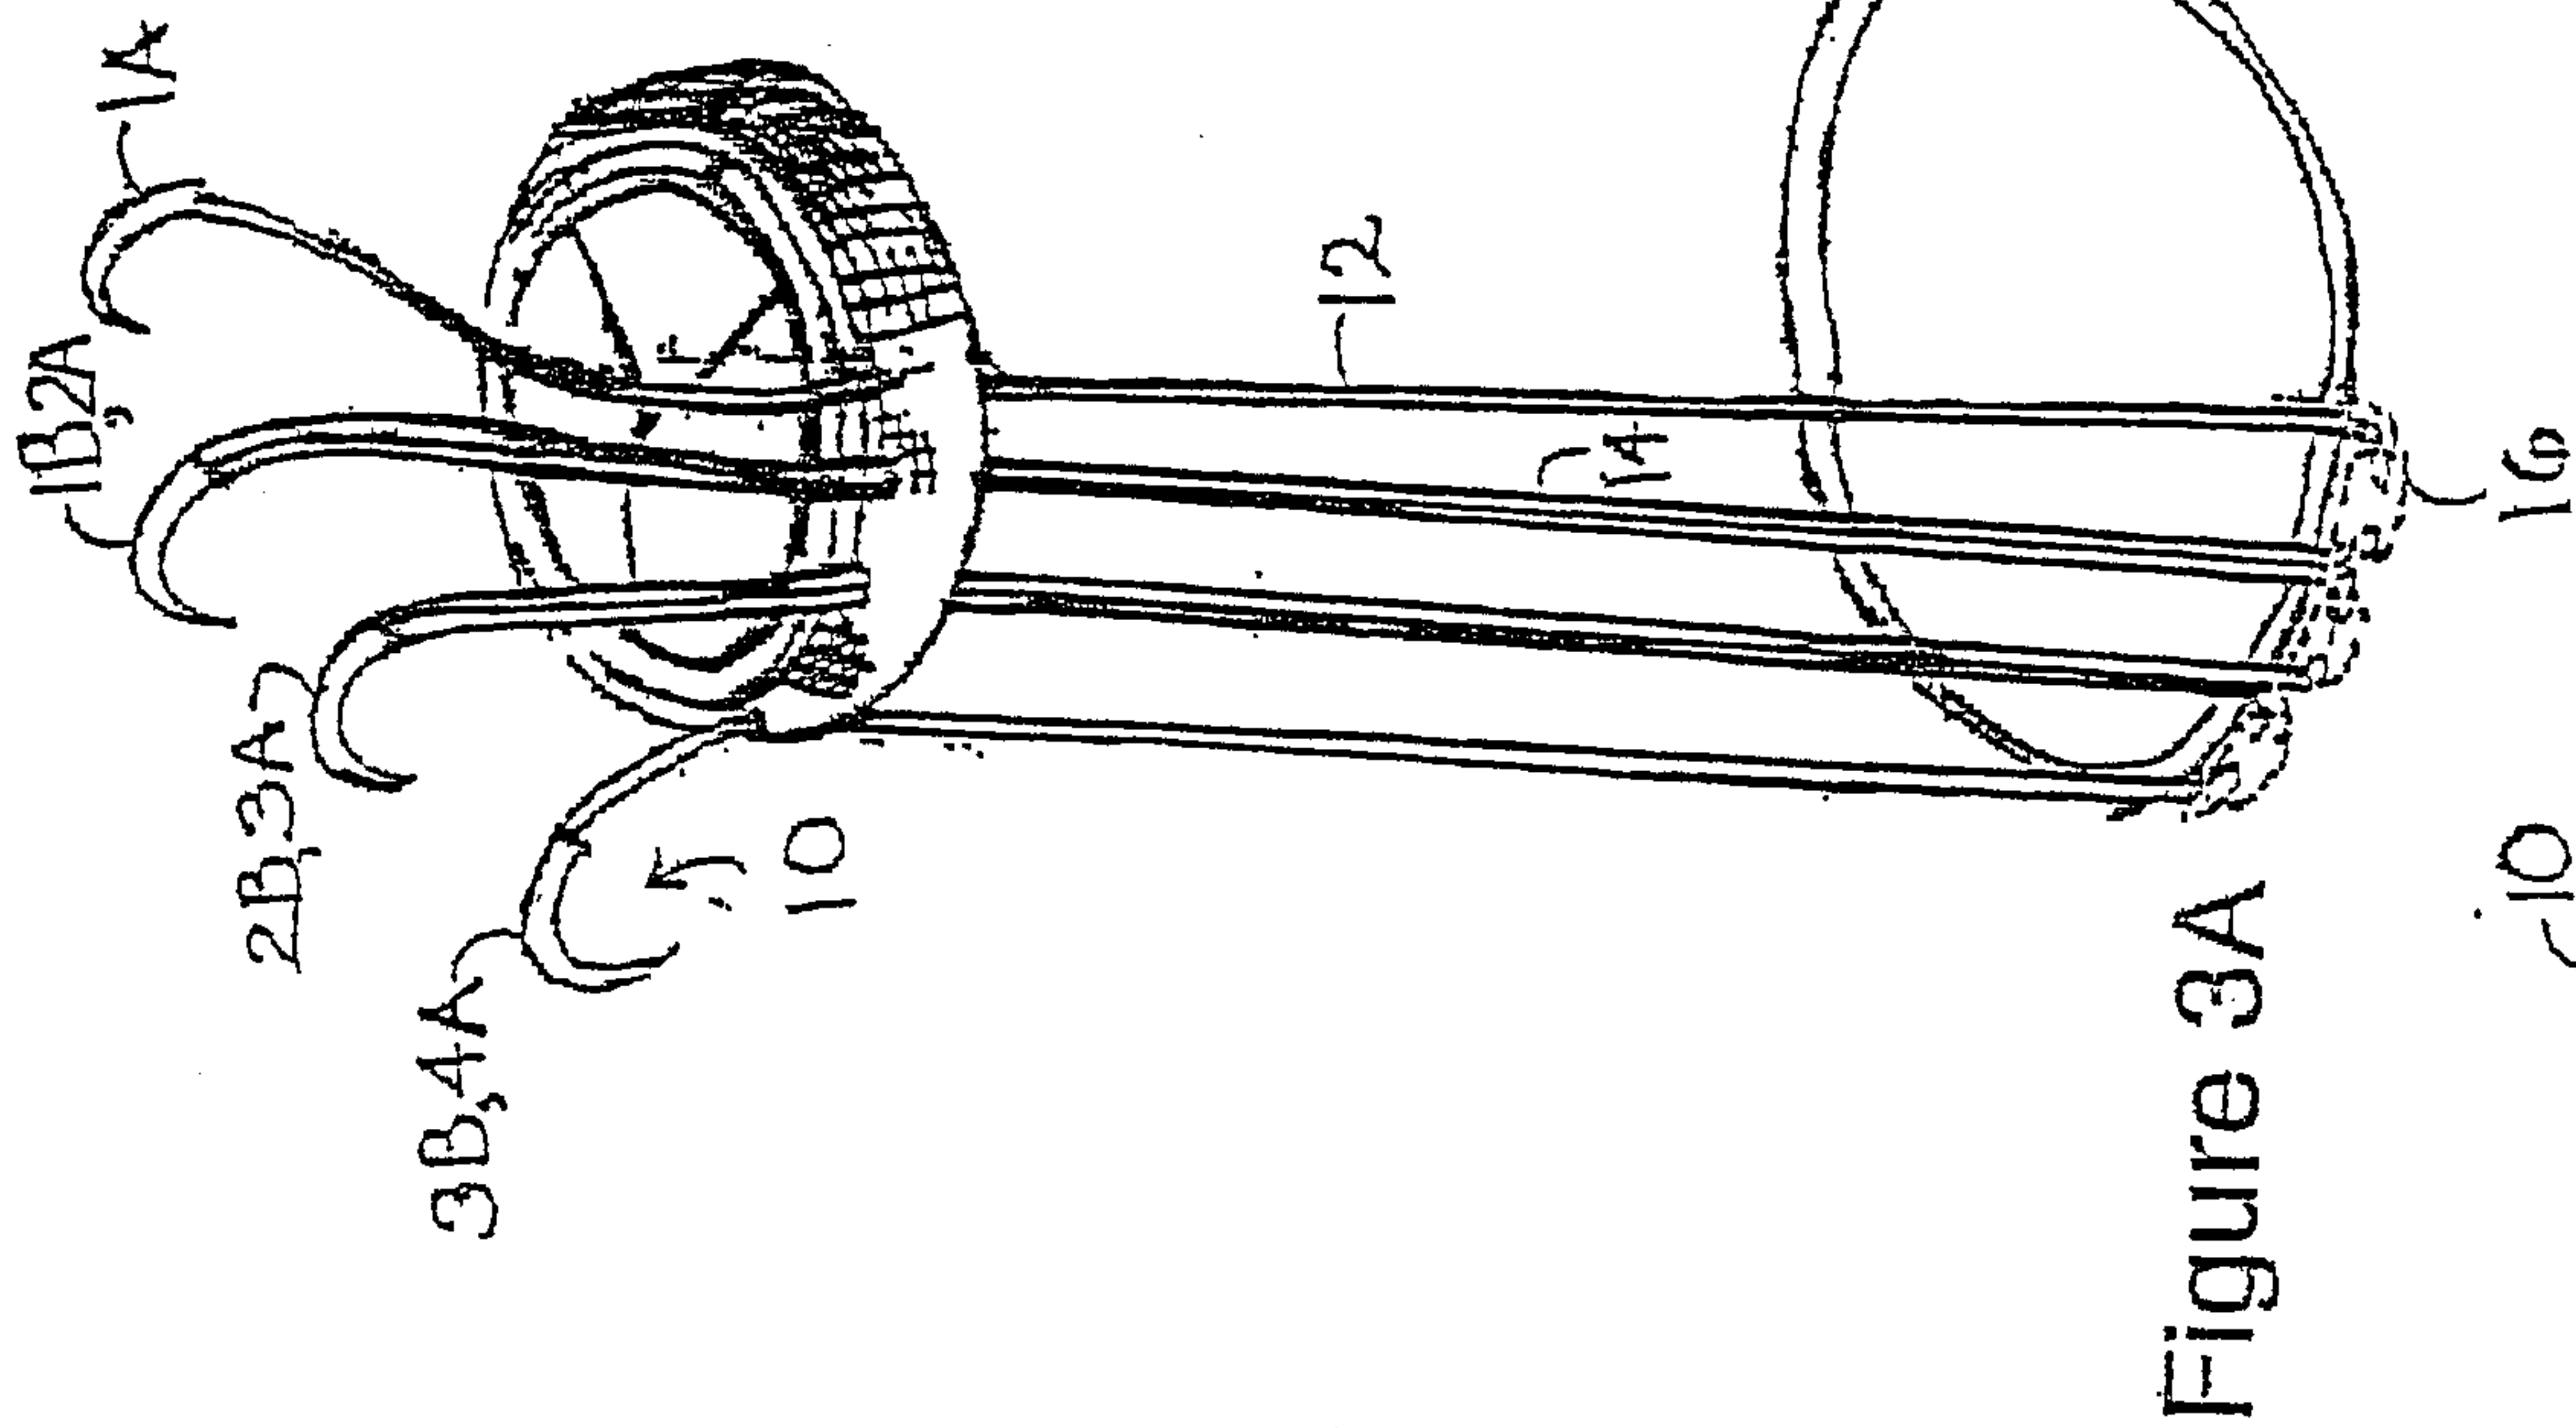


Figure 3A

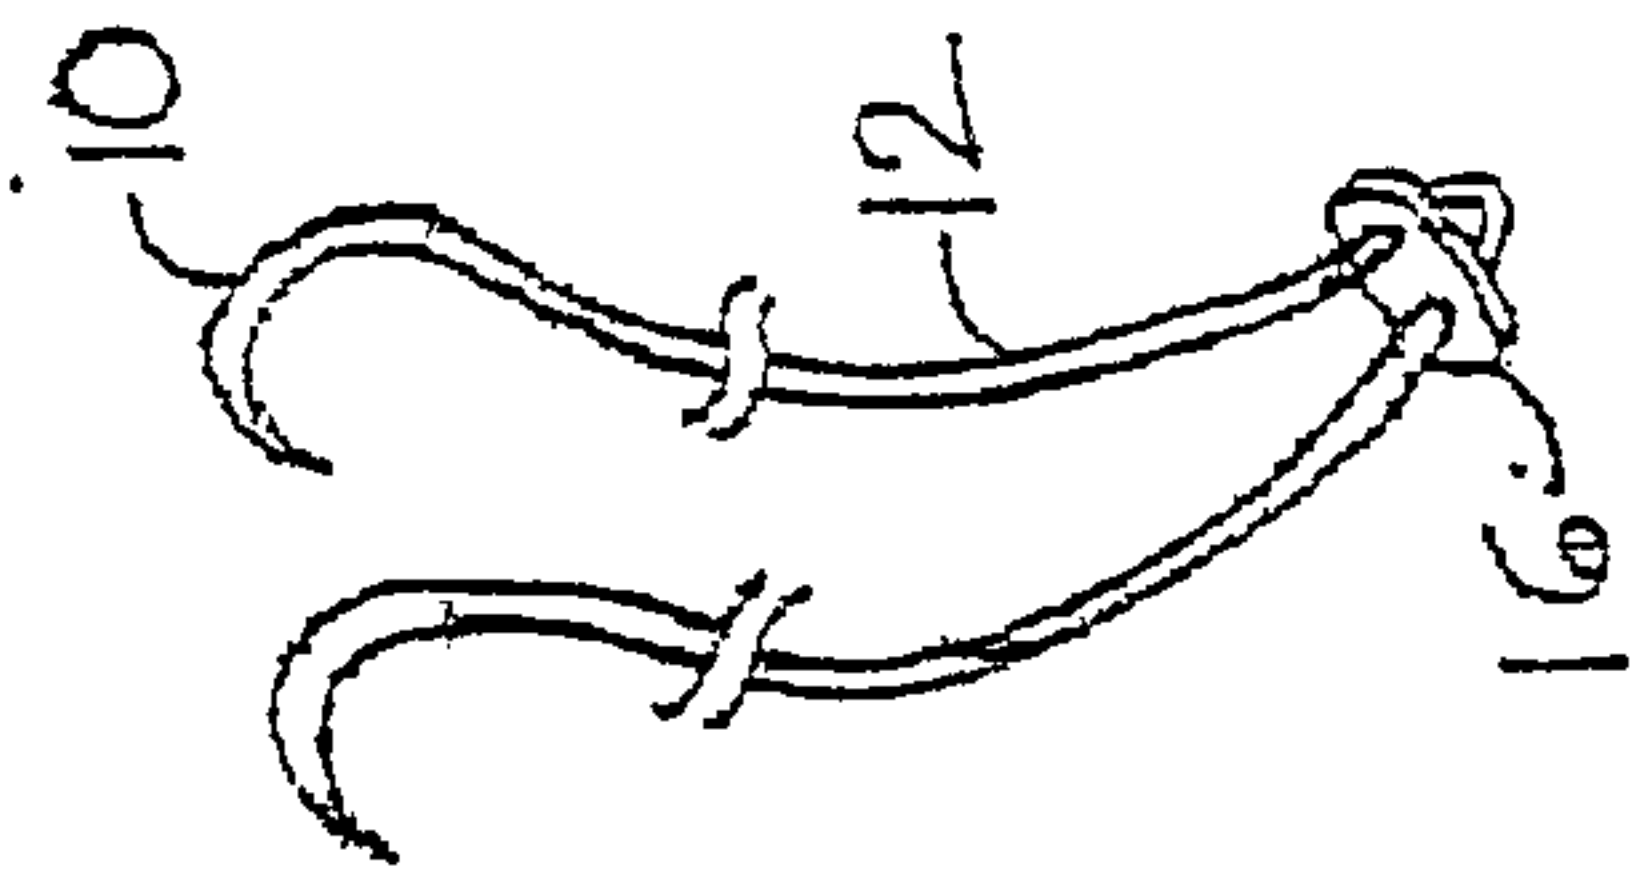


Figure 3B

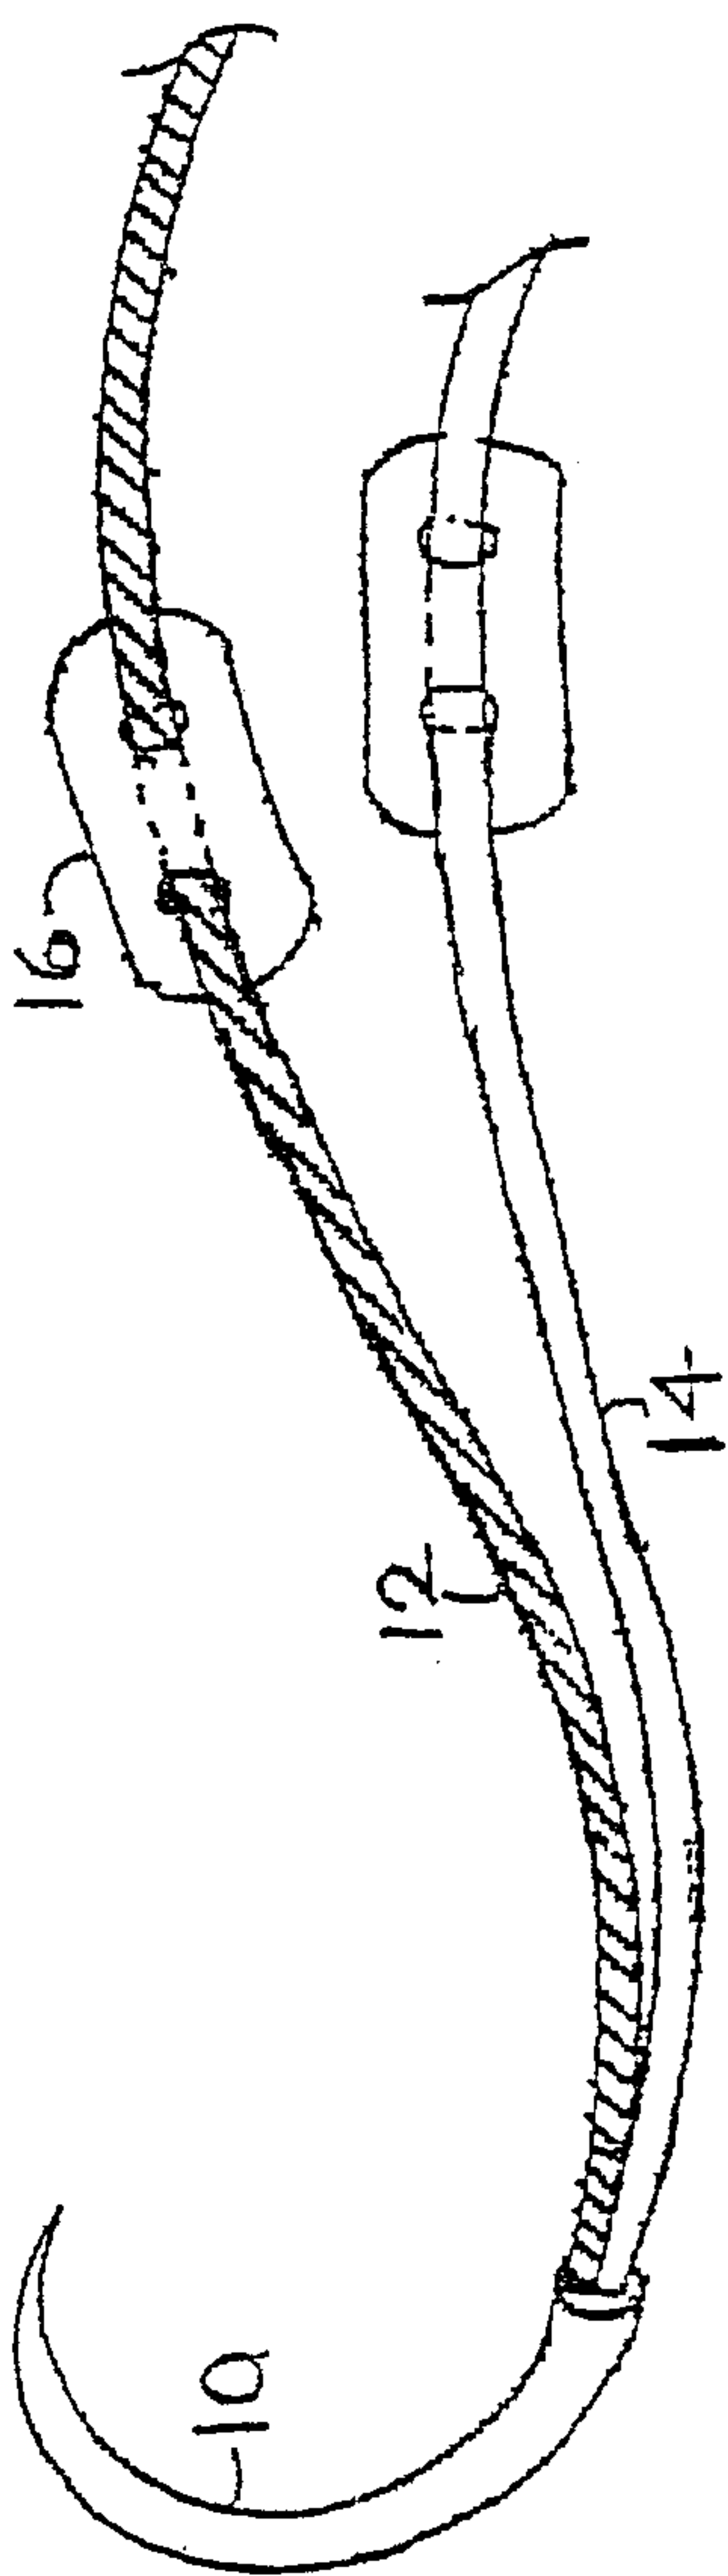


Figure 1

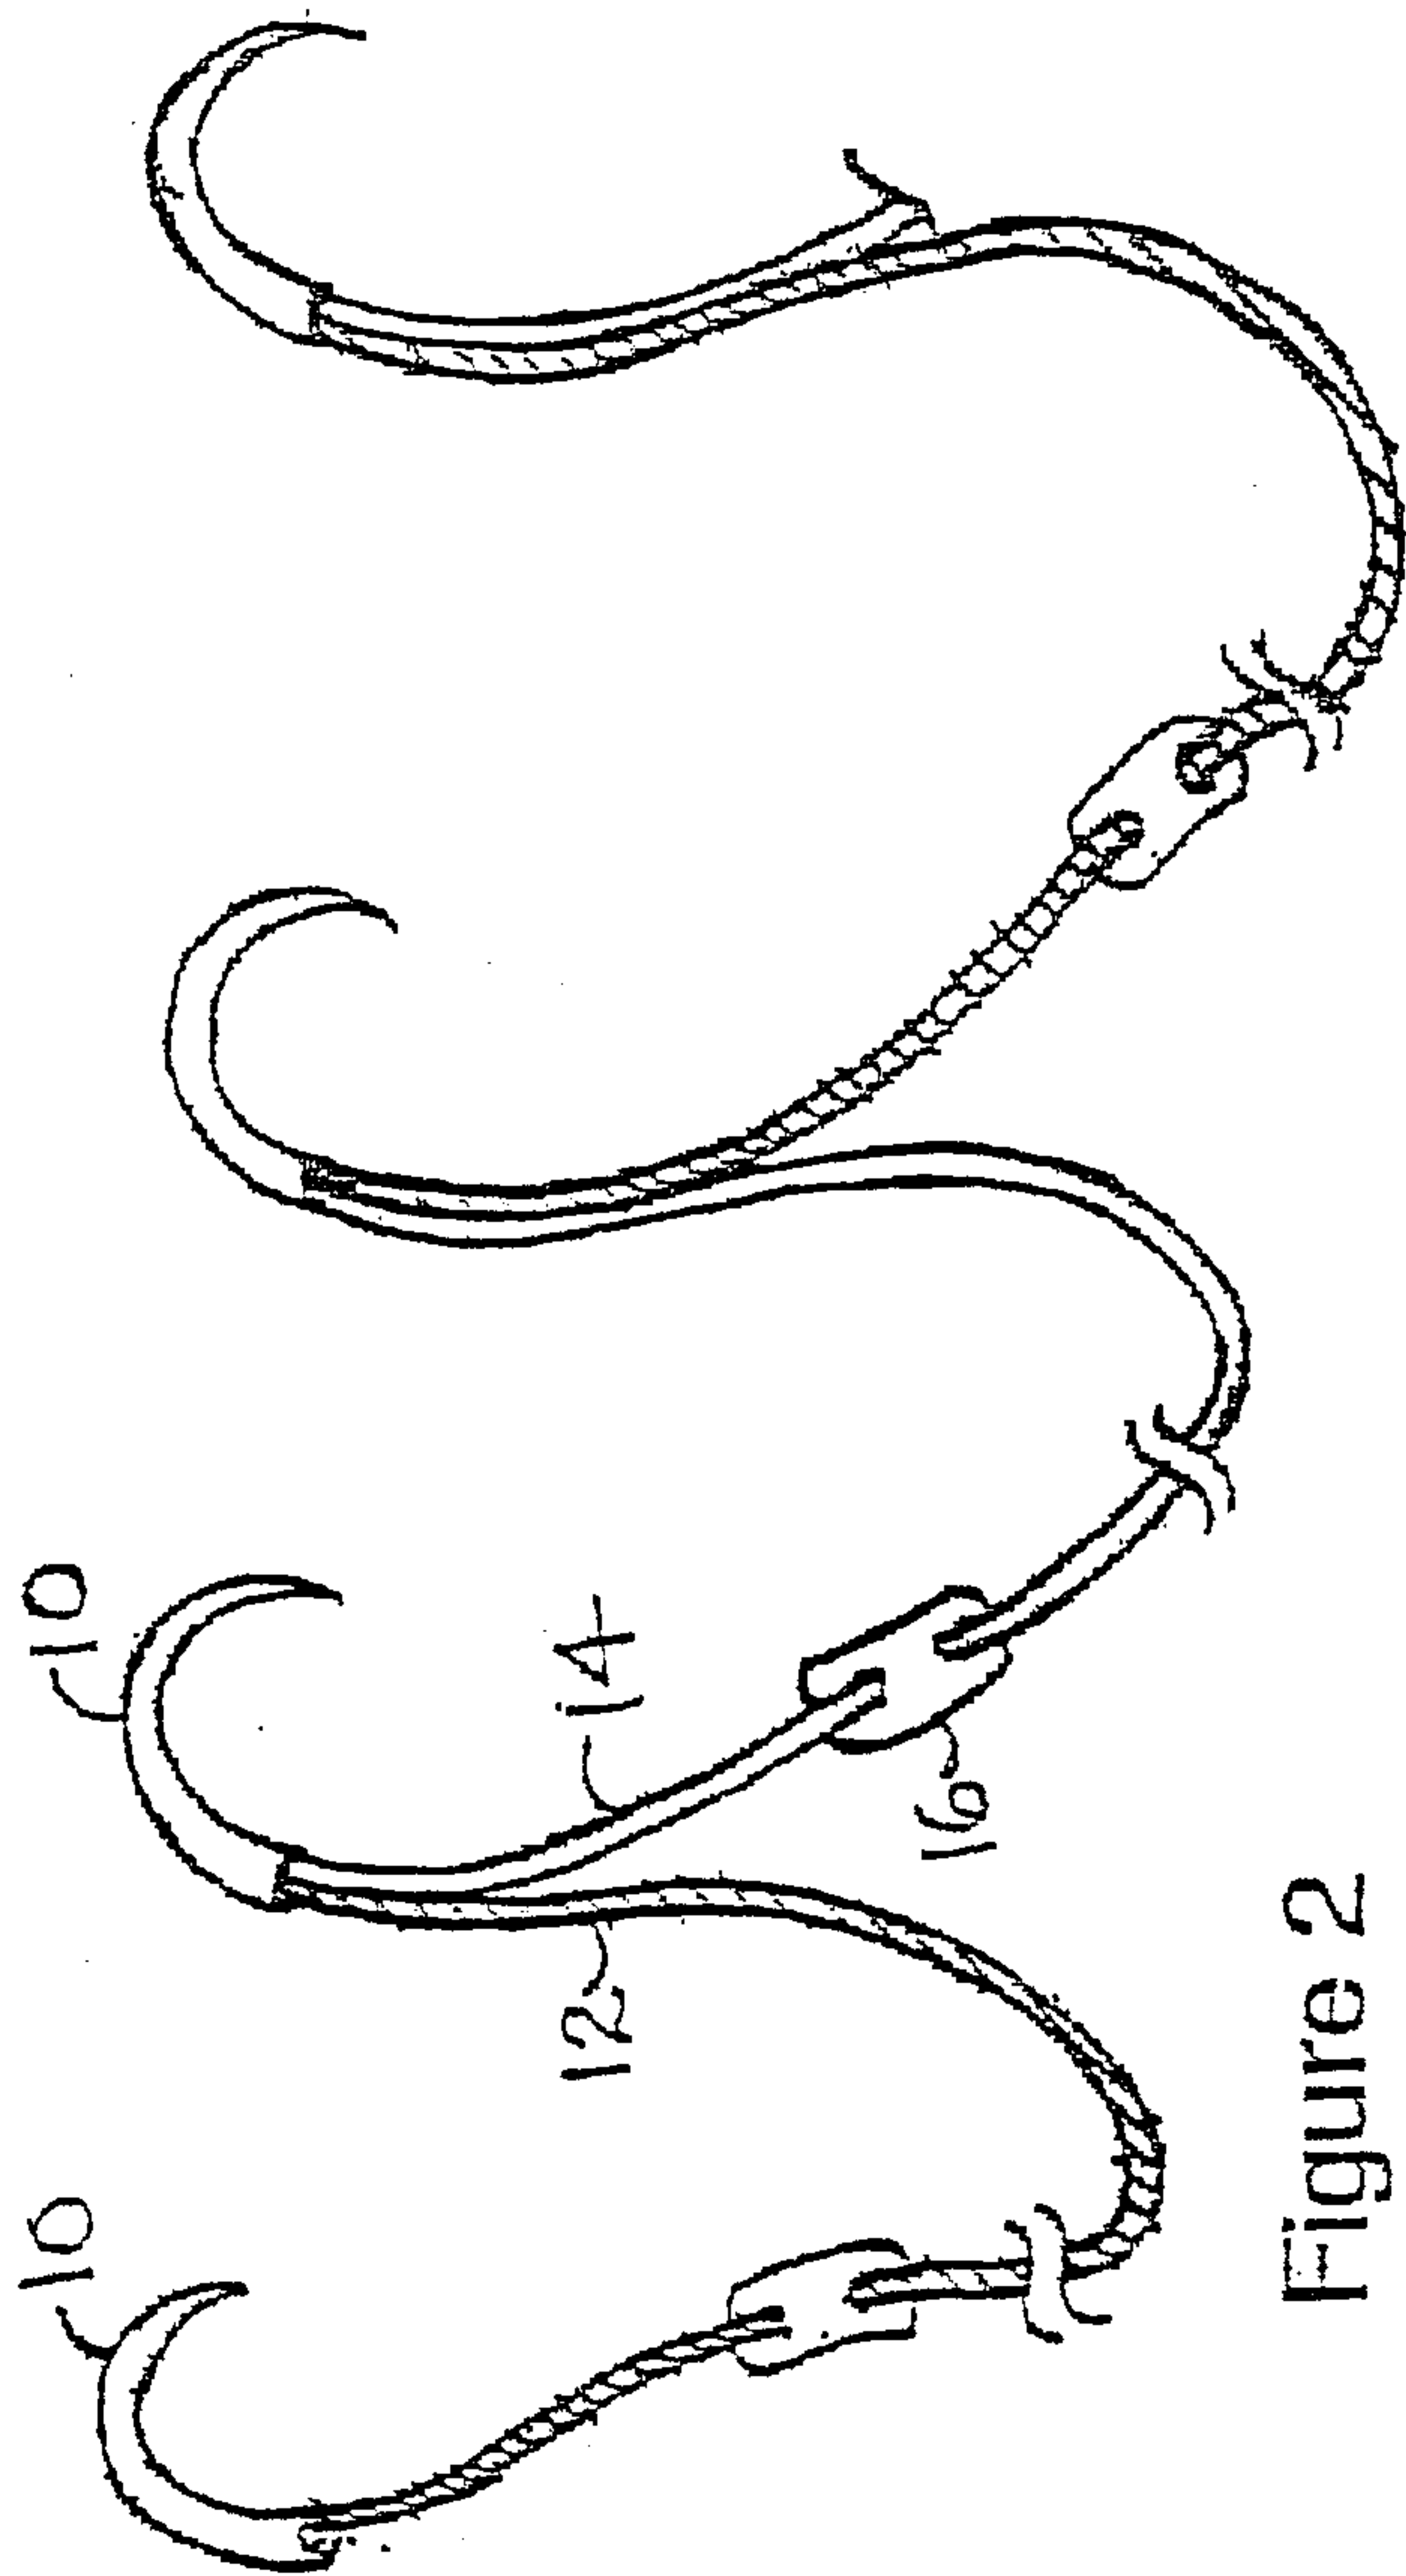


Figure 2

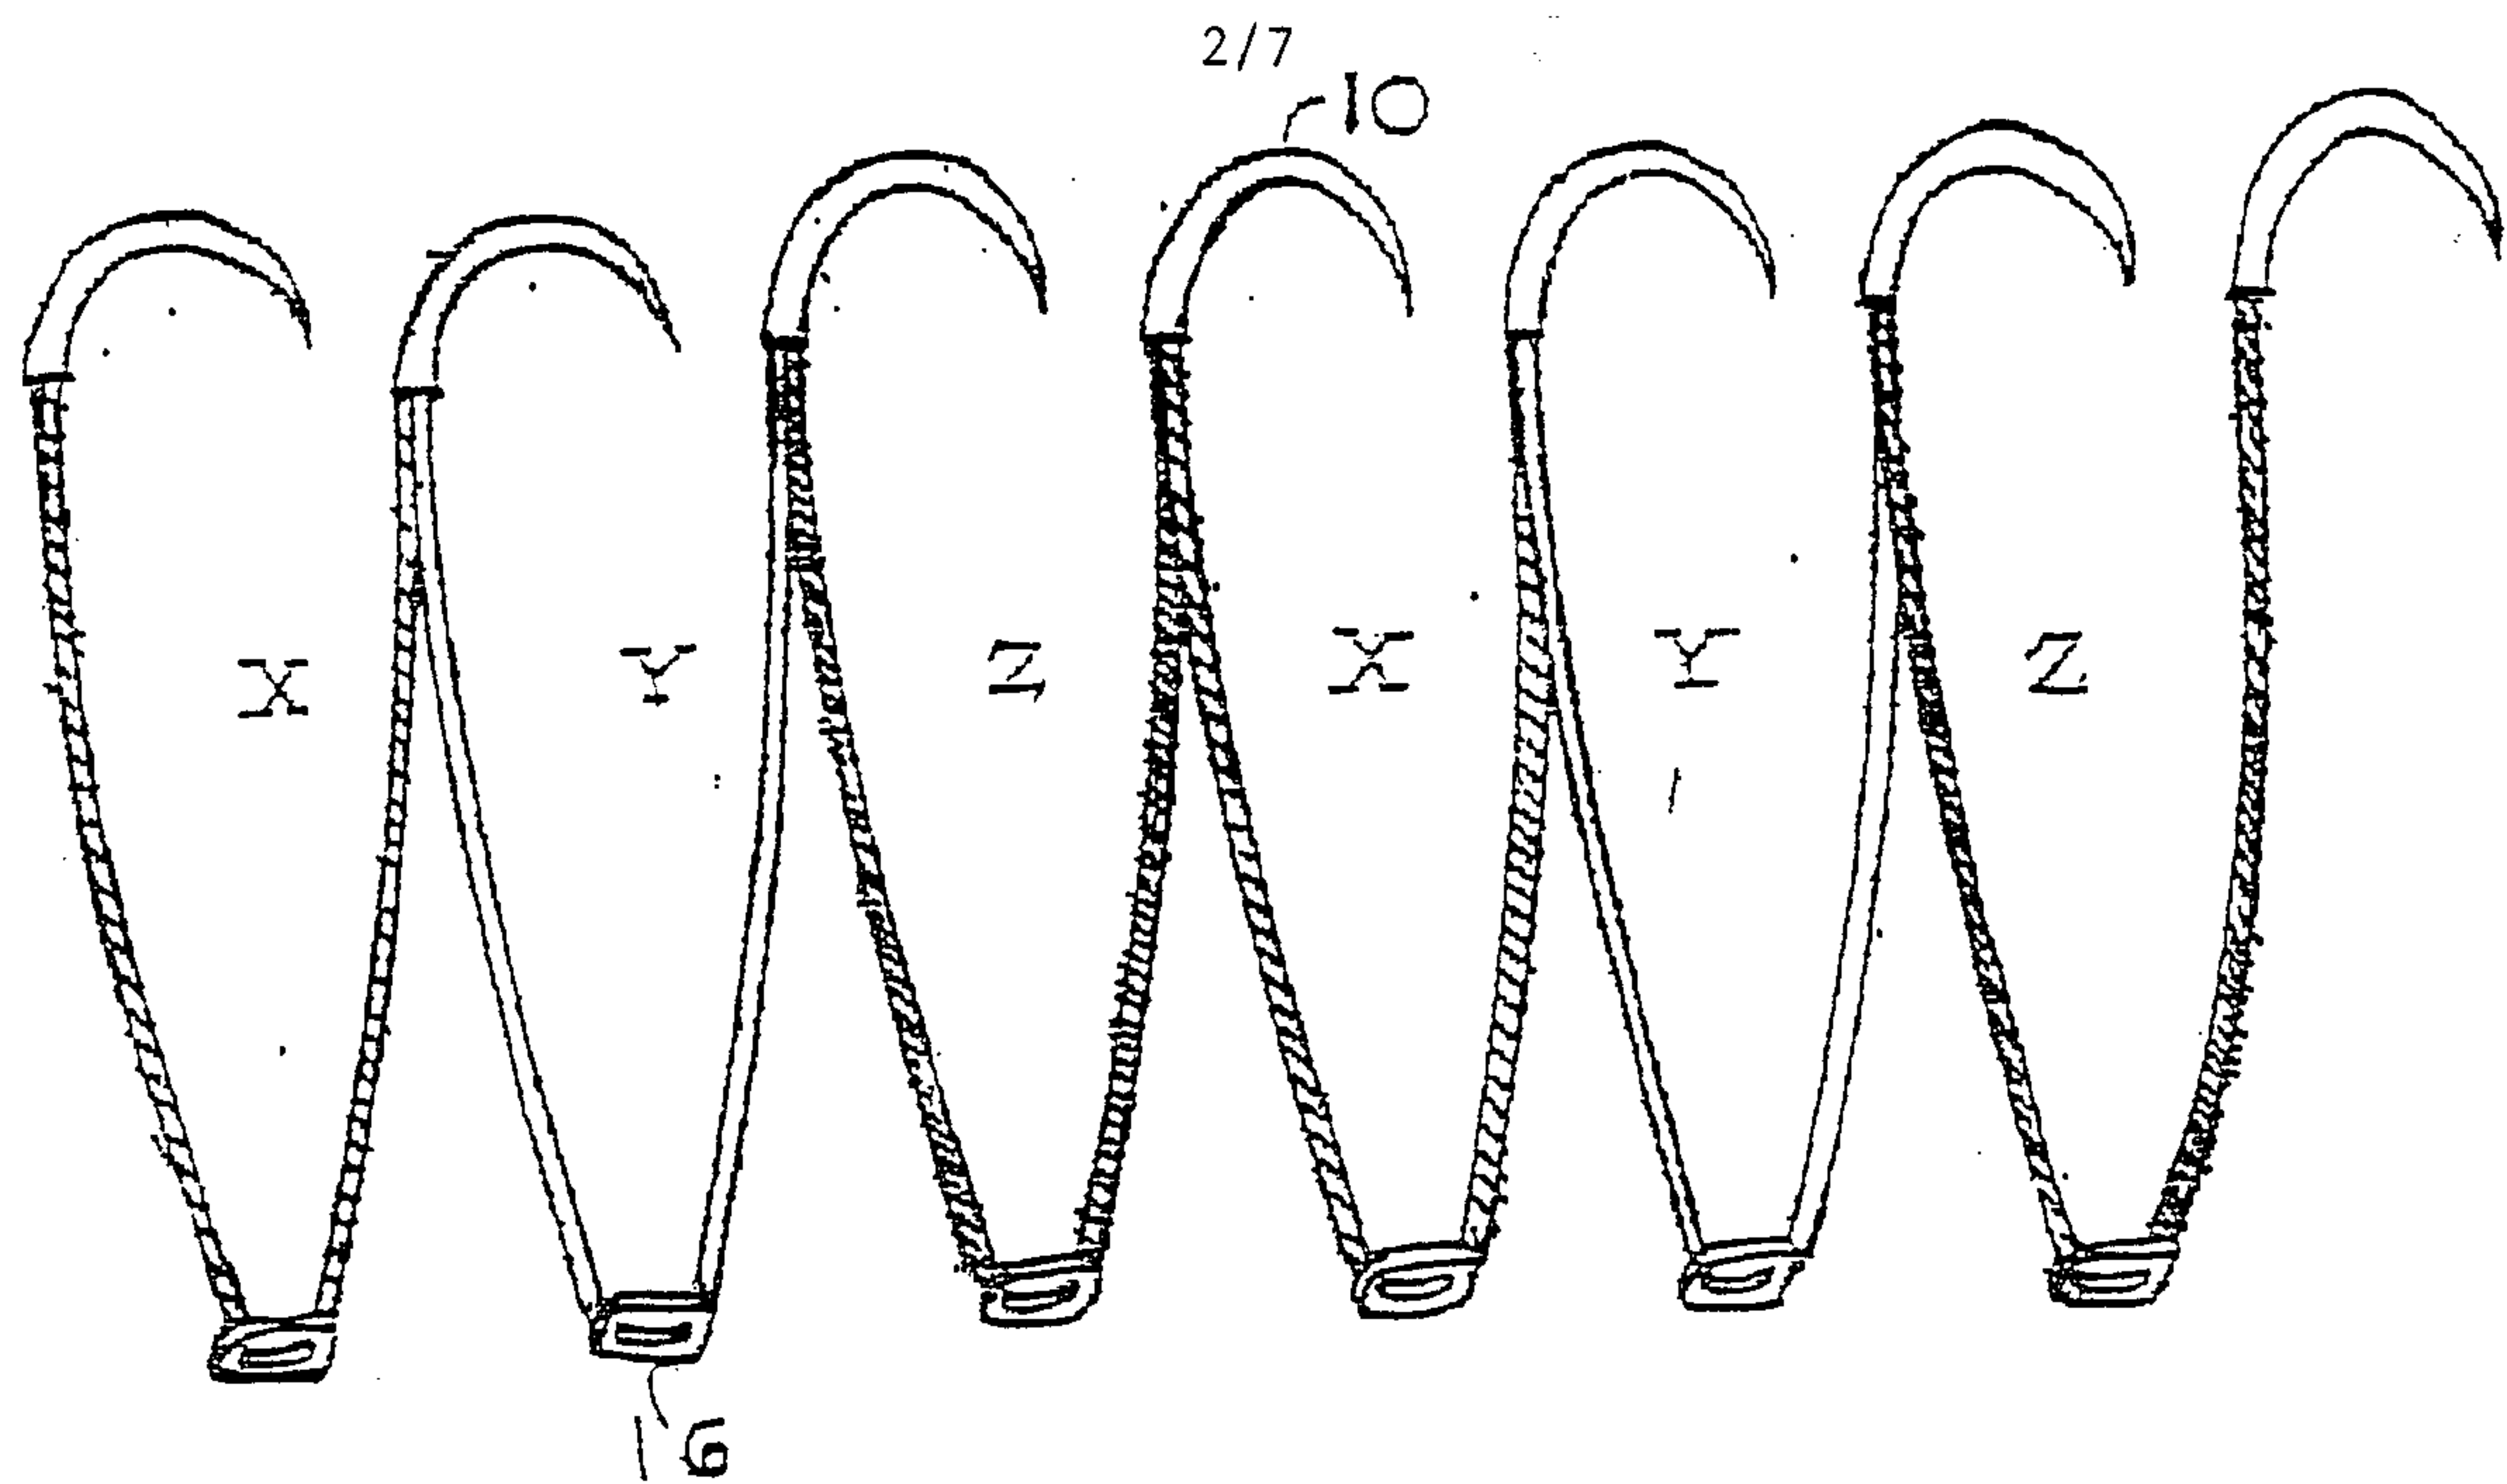


Figure 4

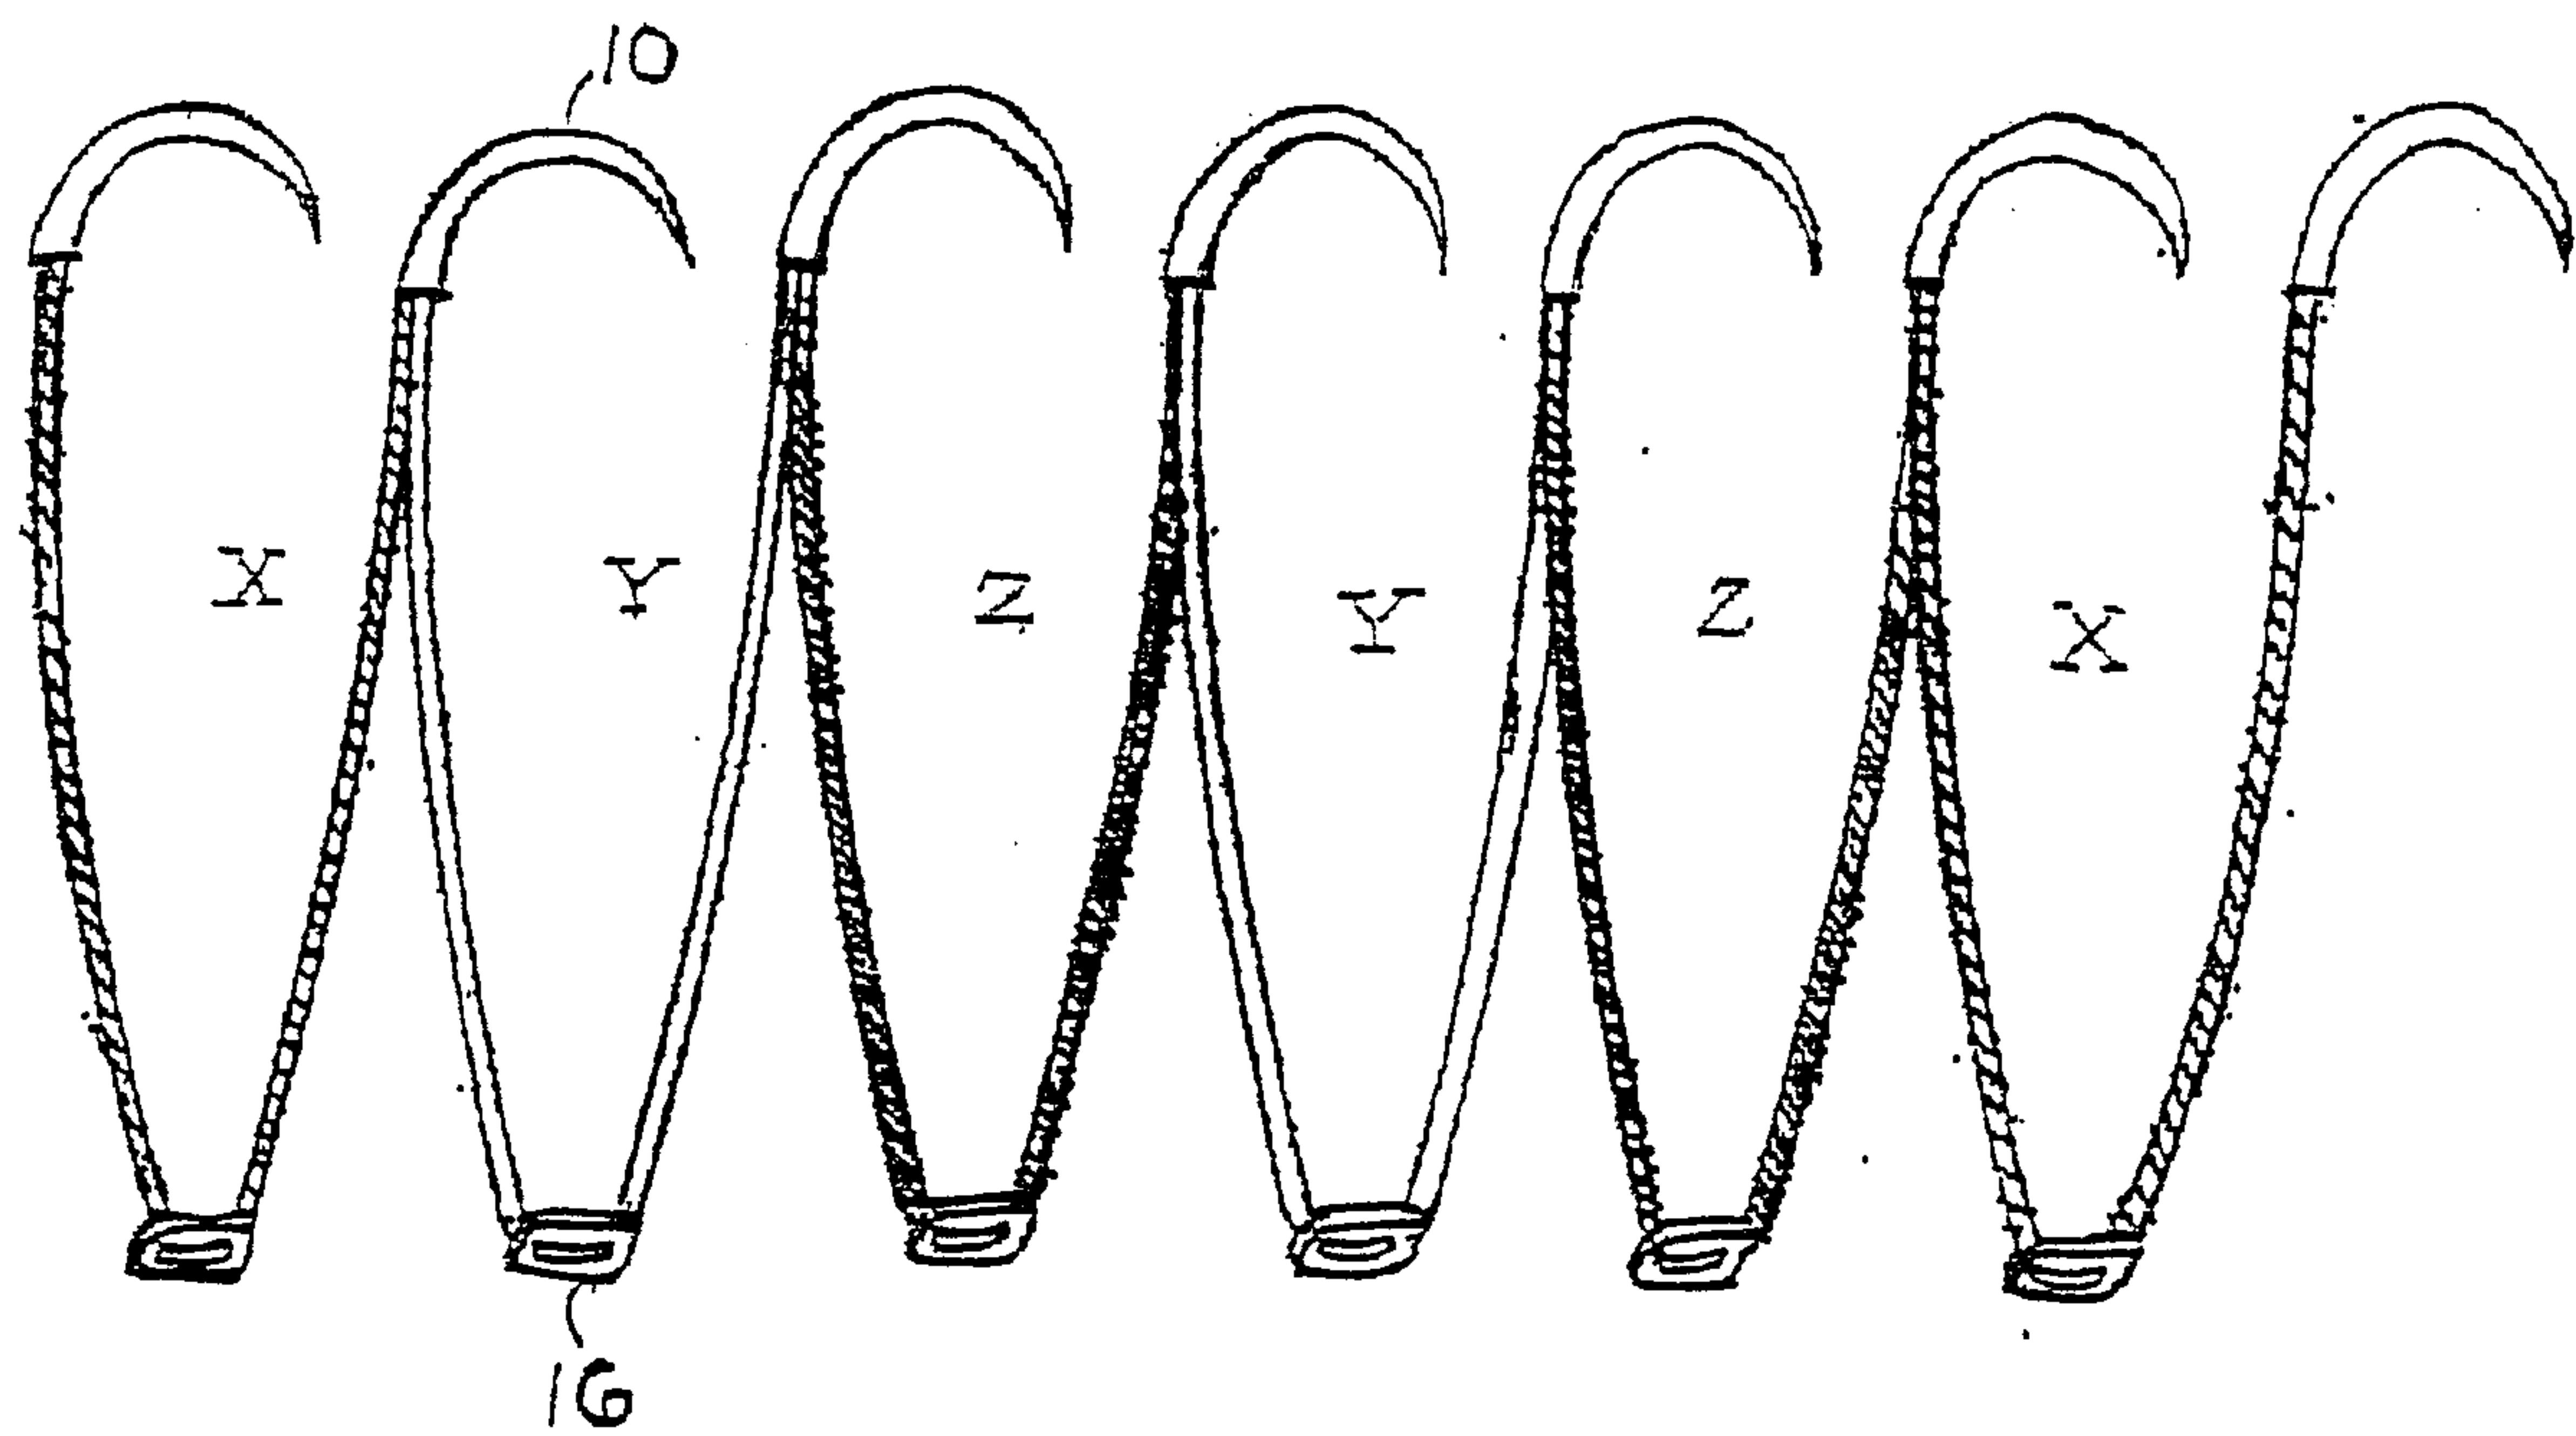


Figure 5

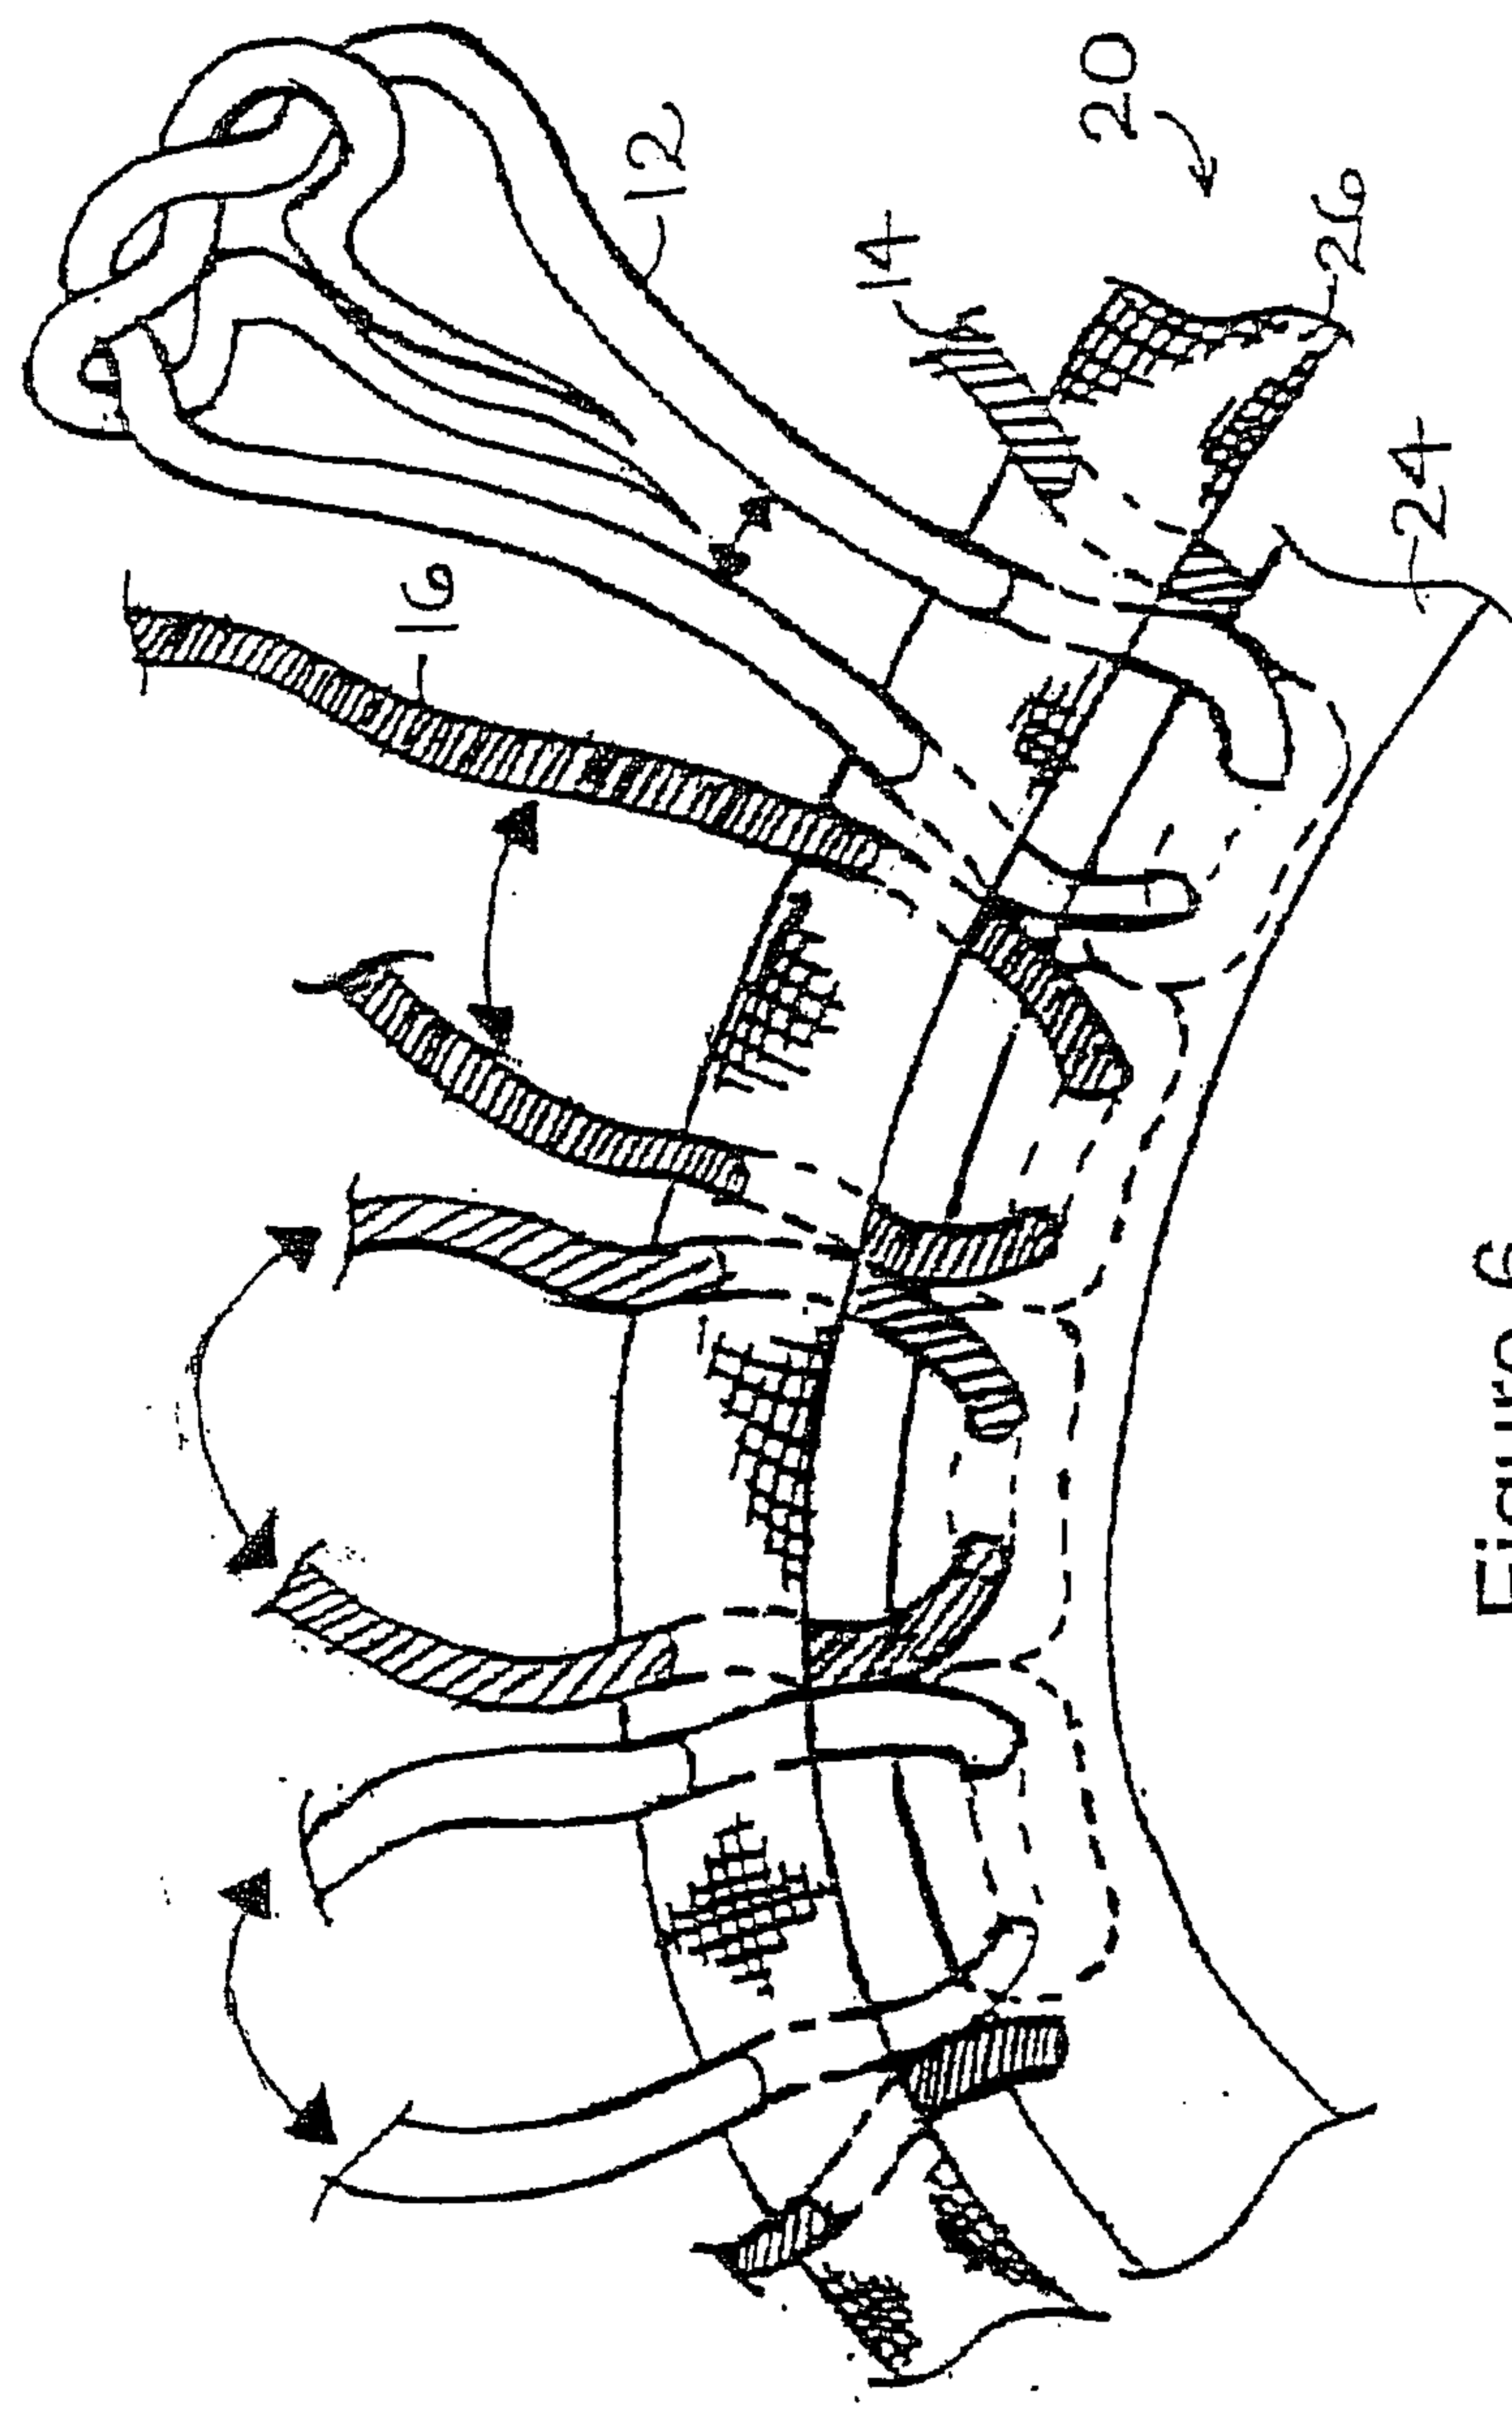


Figure 6

4/7

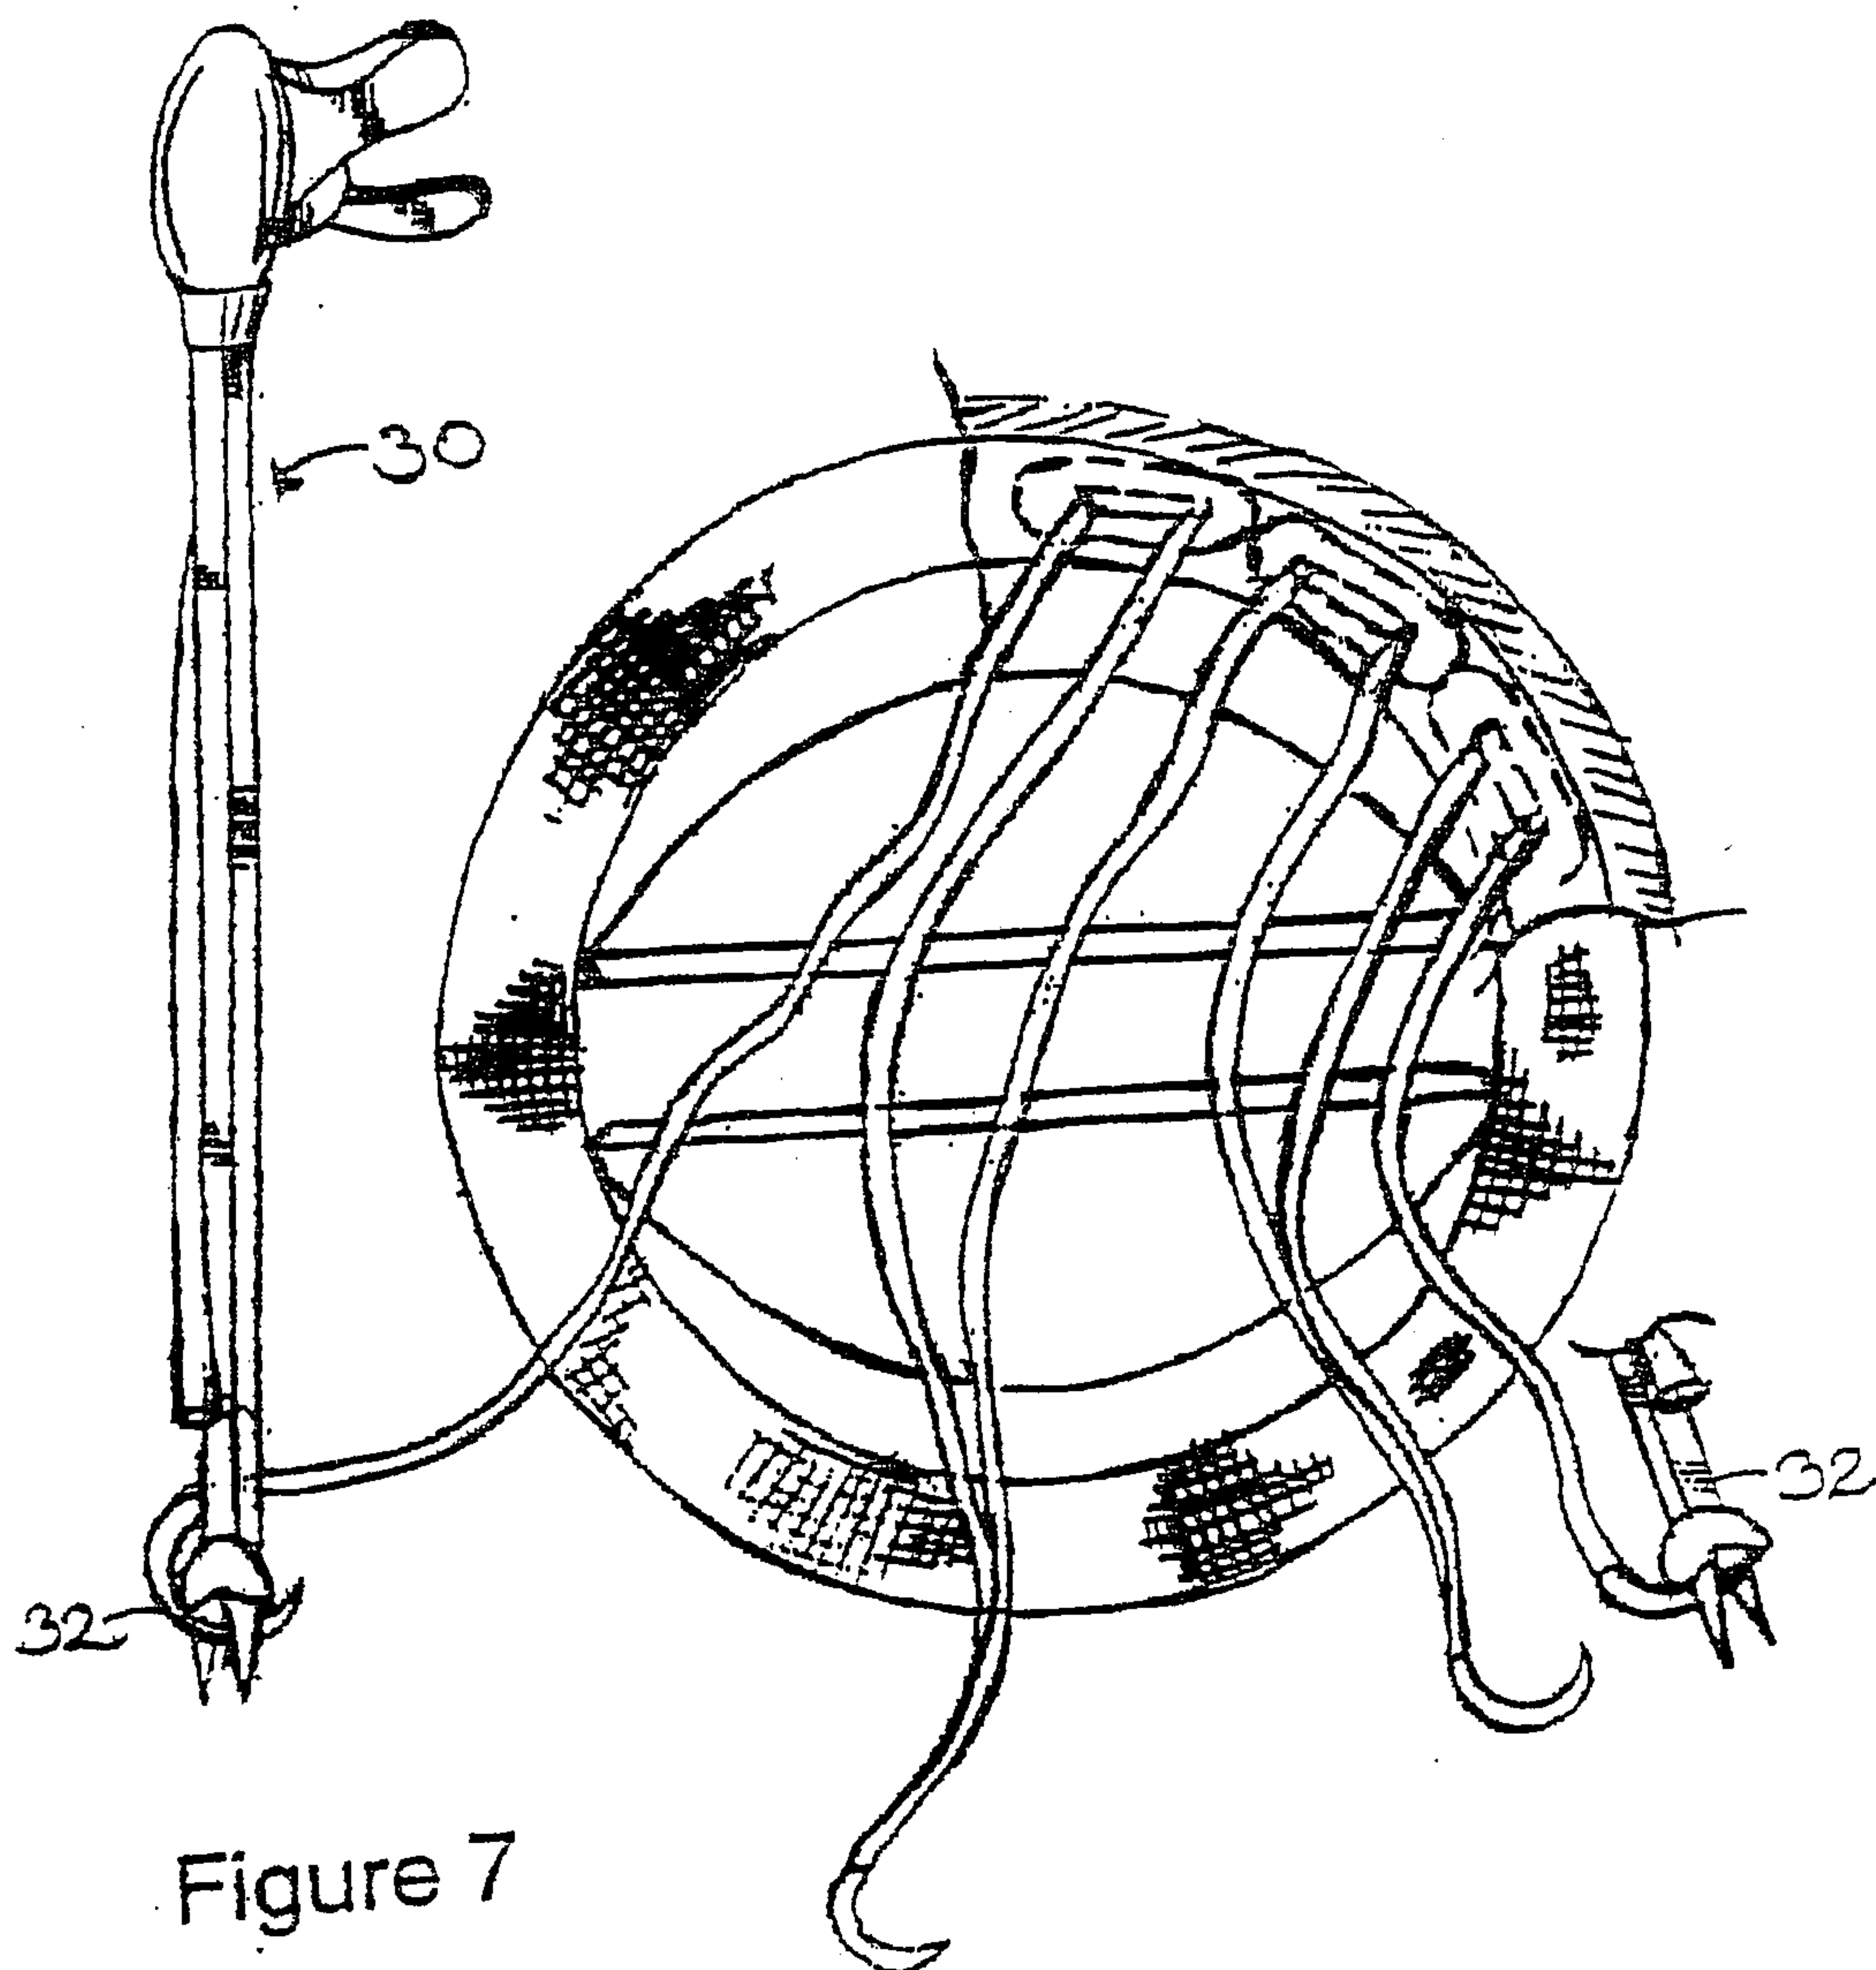


Figure 7

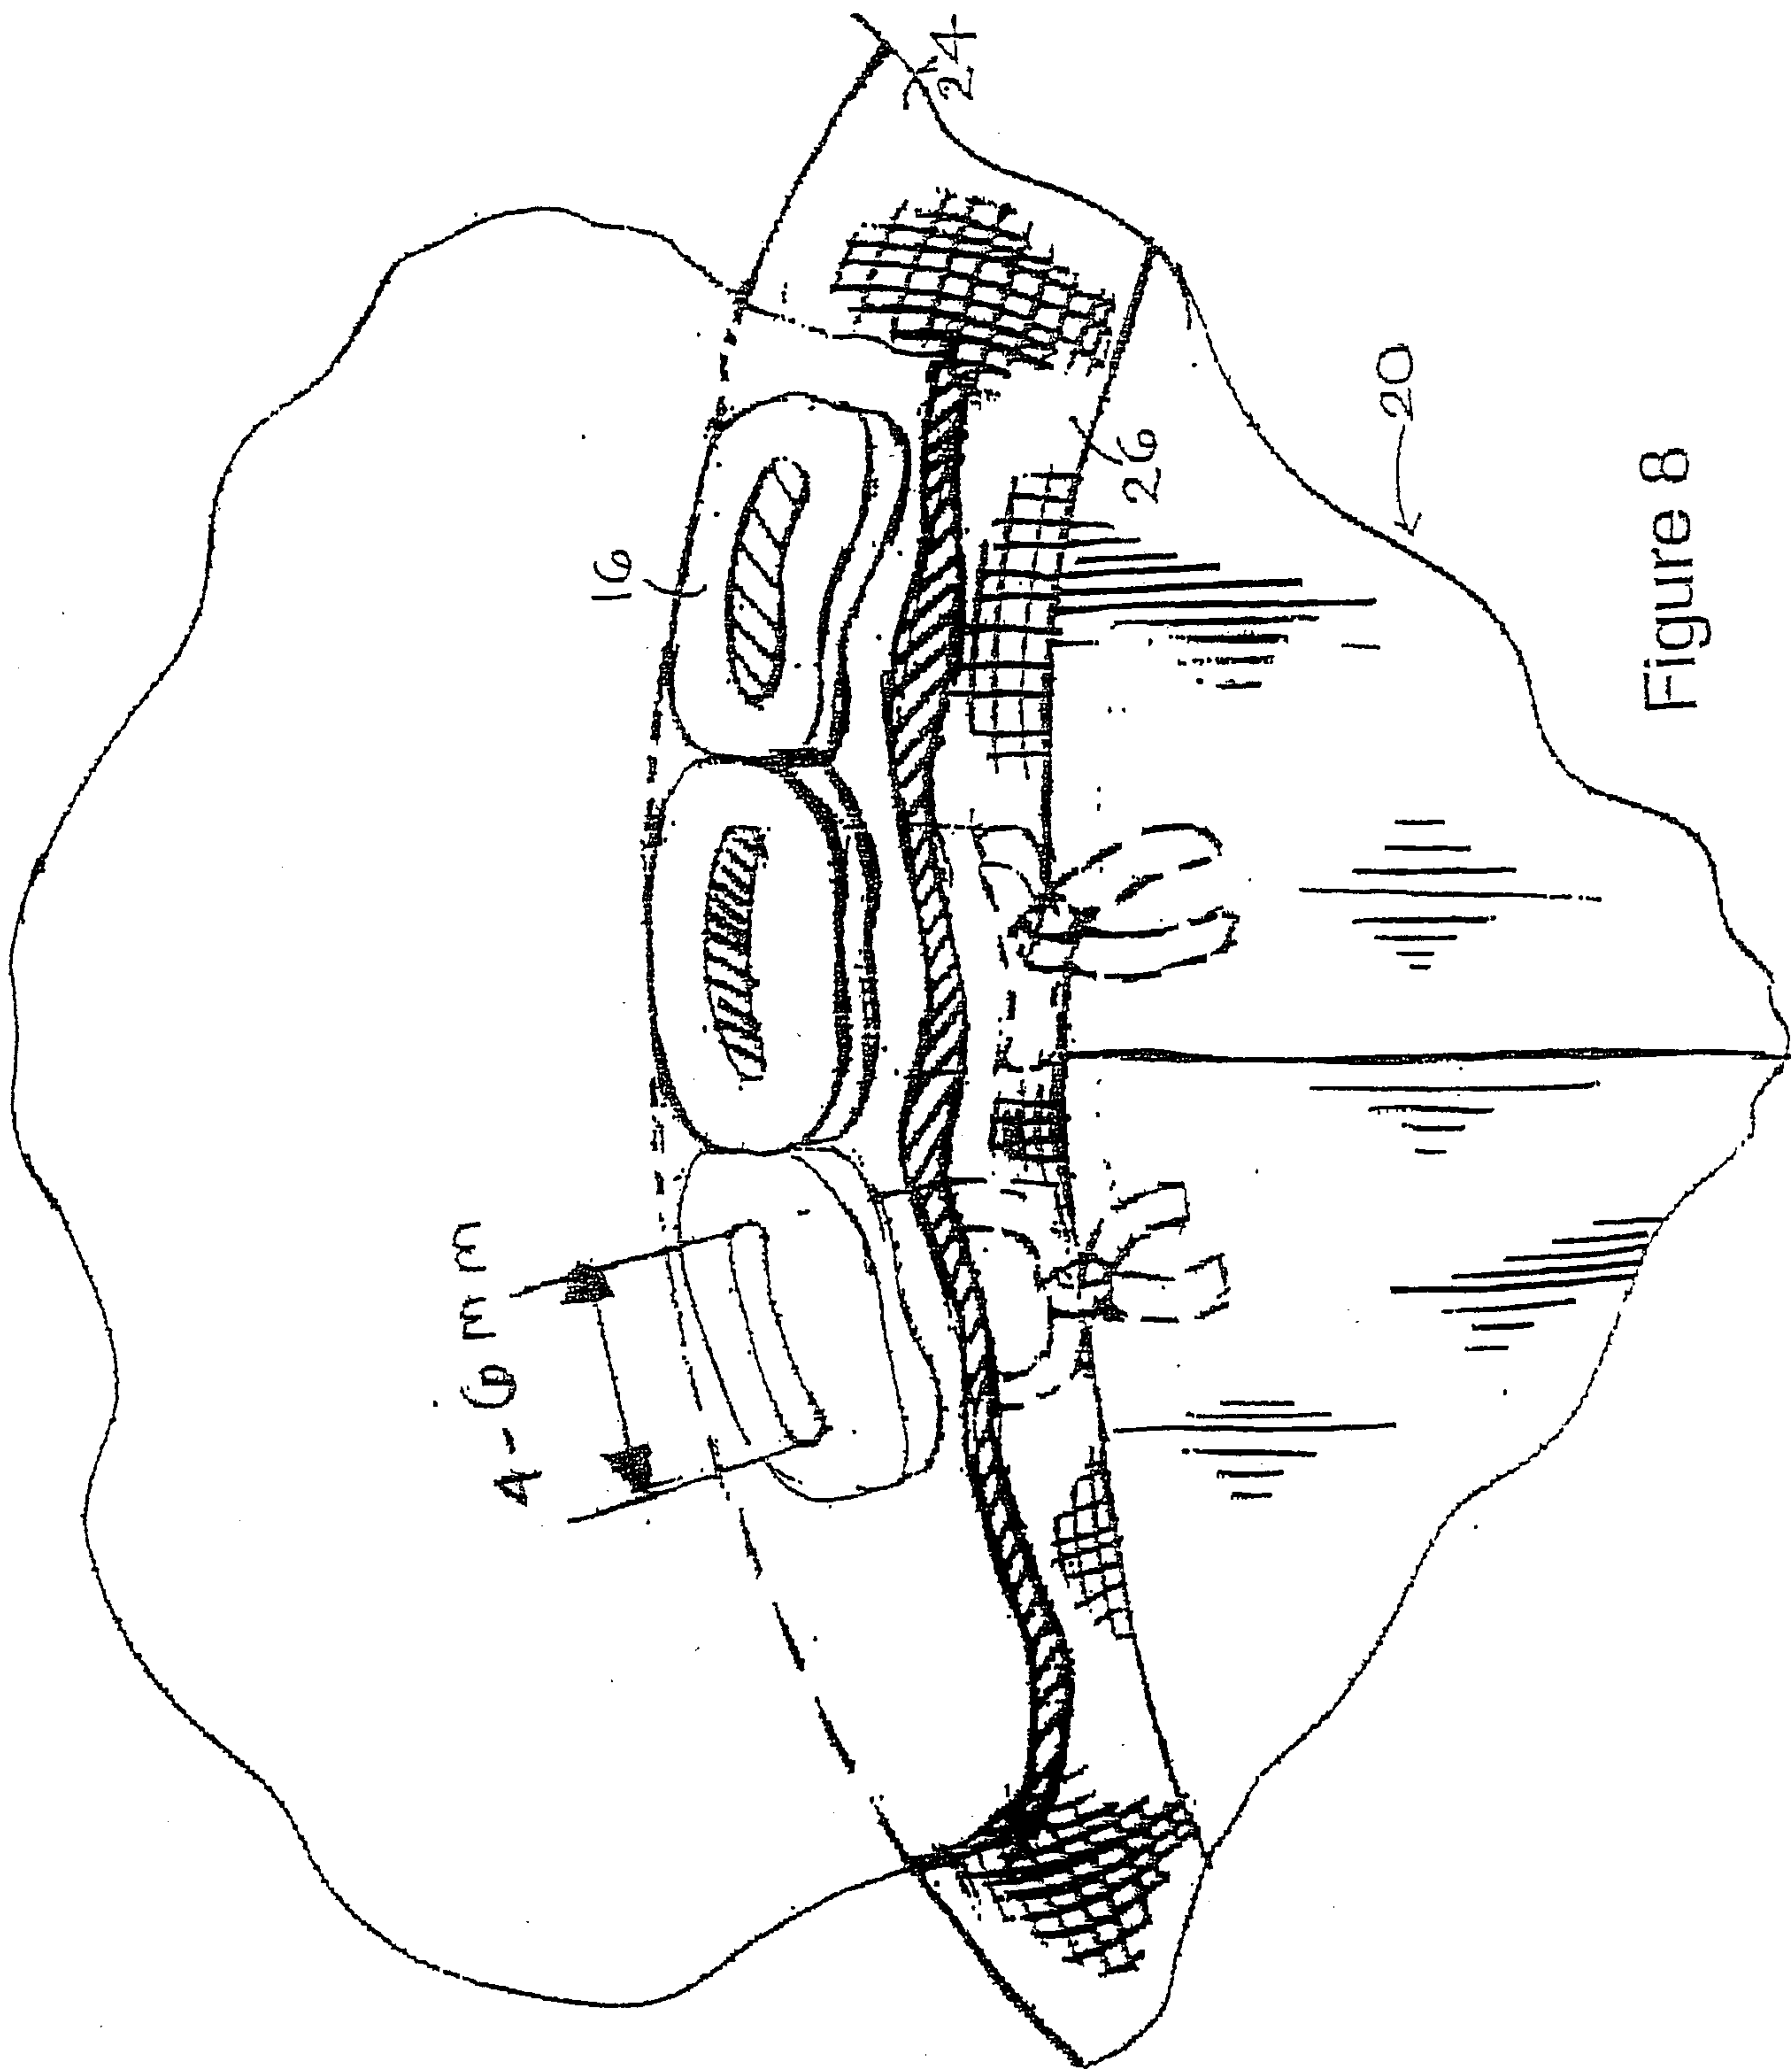


Figure 8

6/7

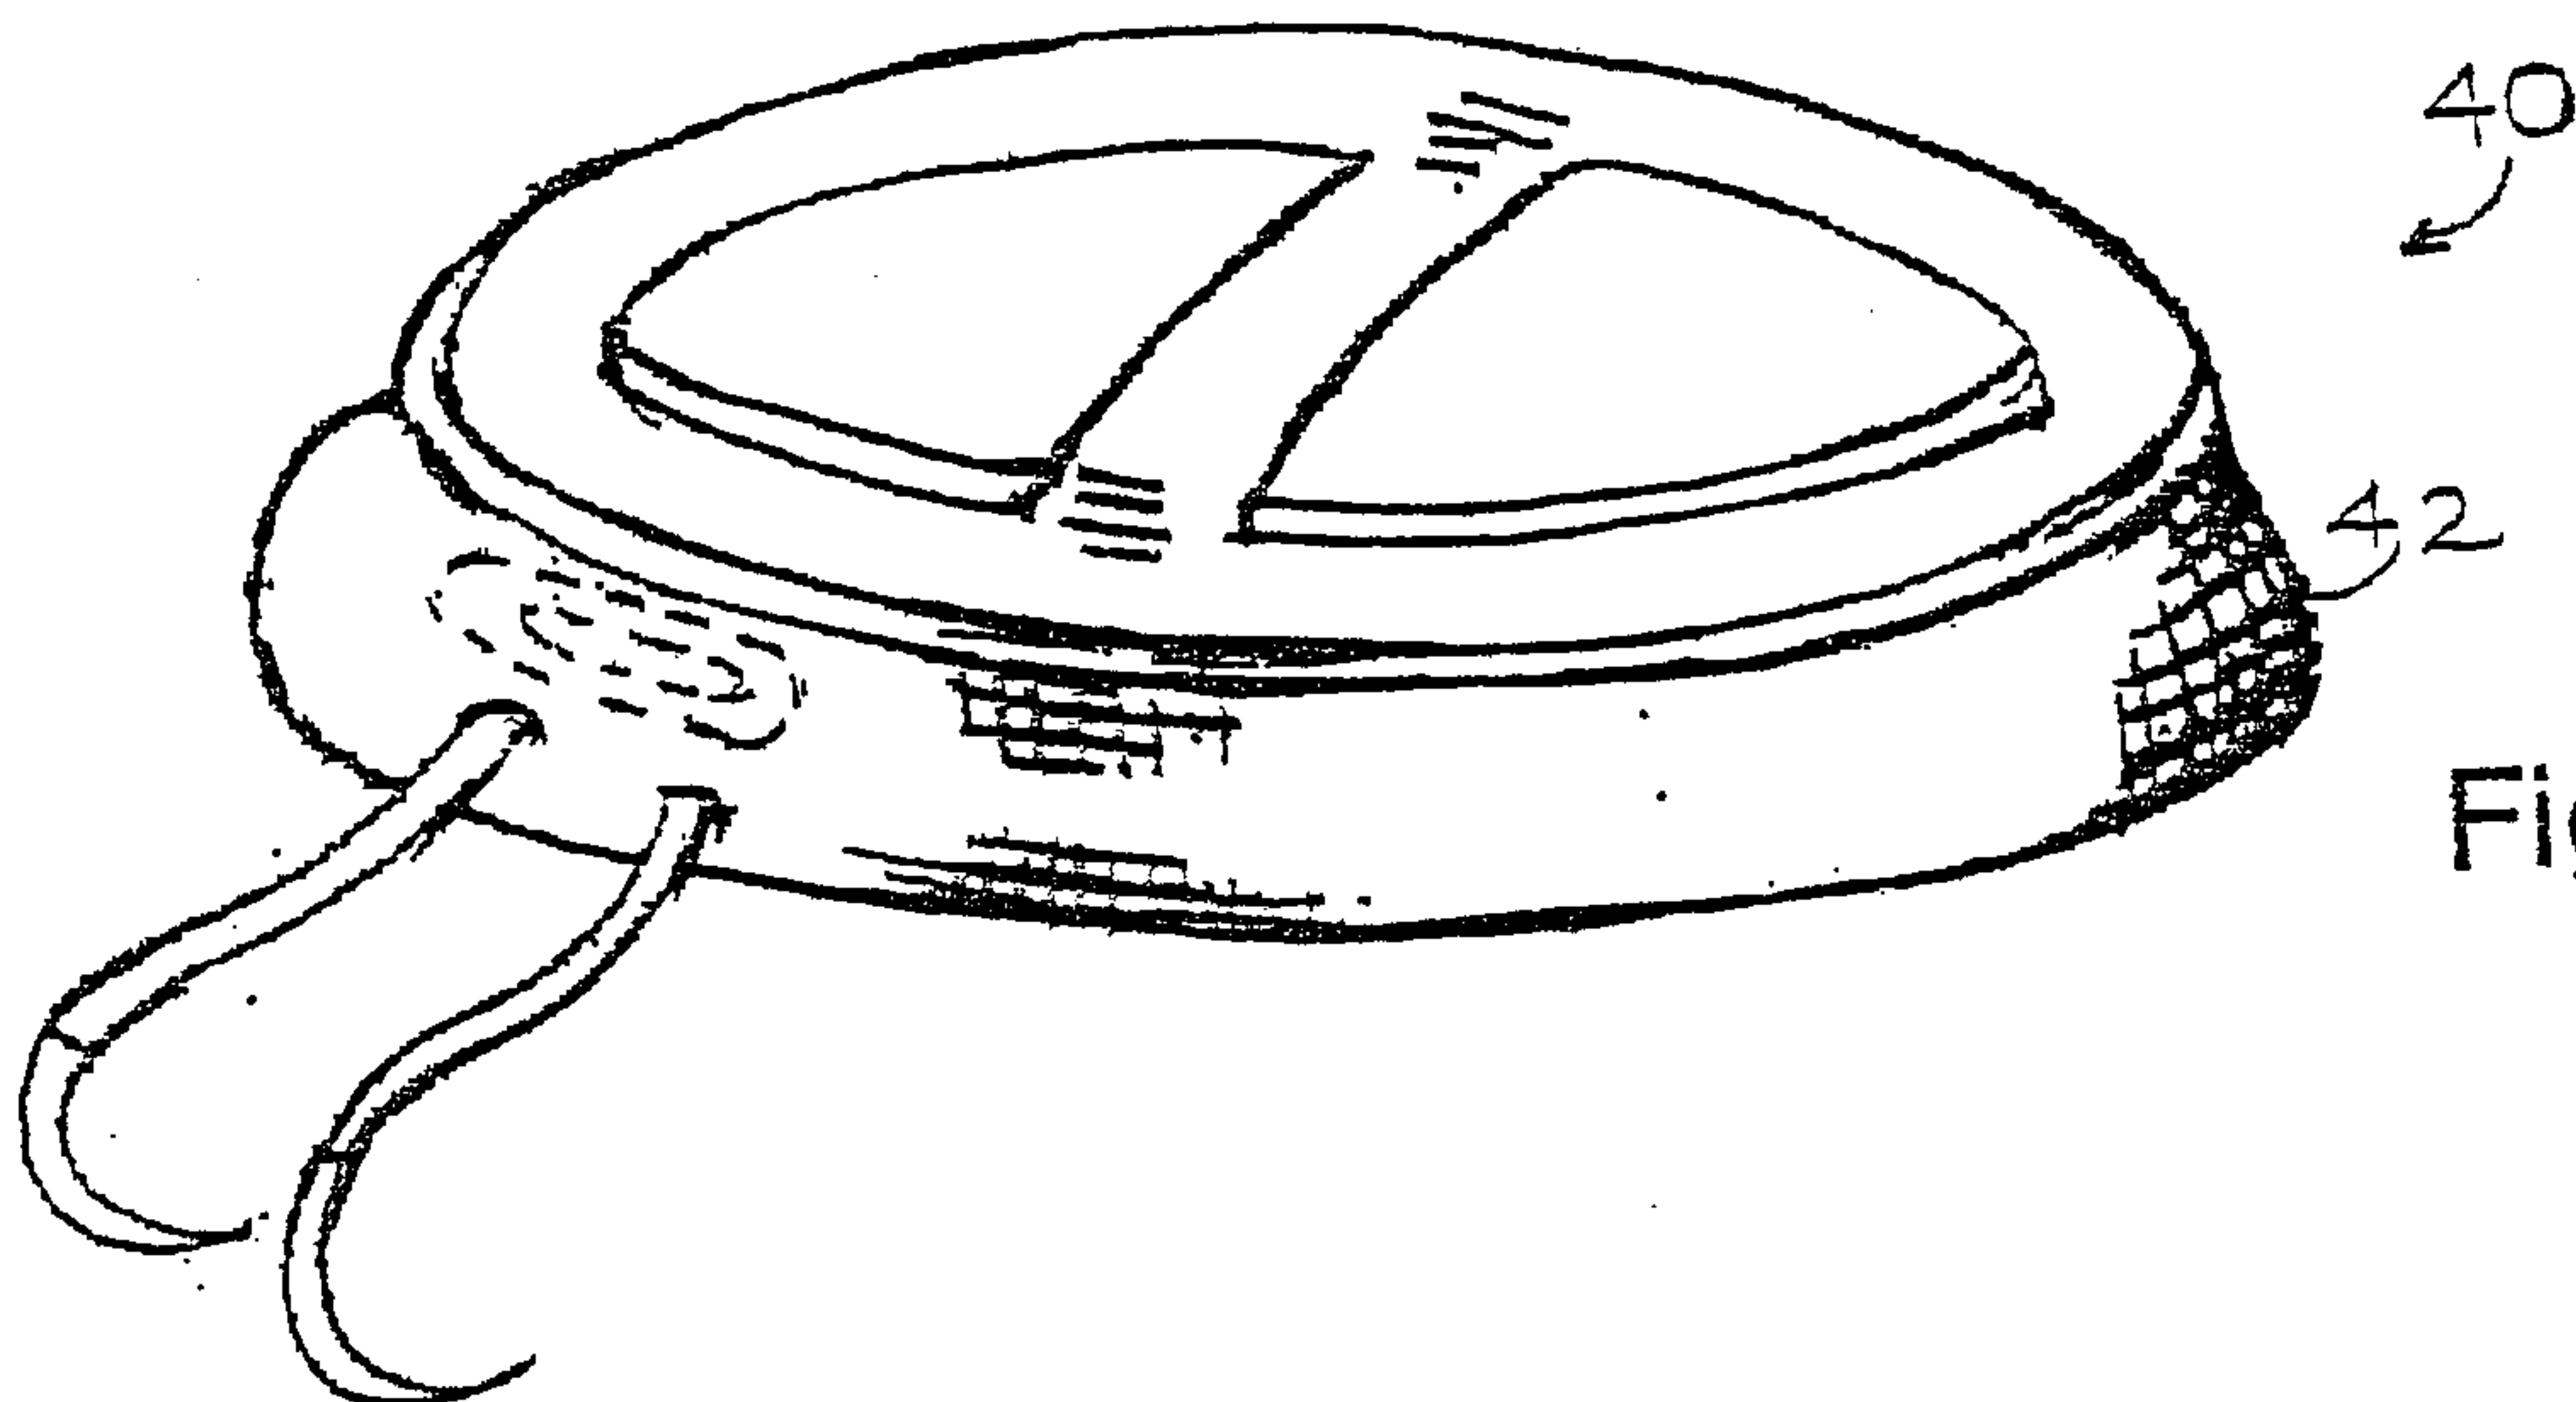


Figure 9

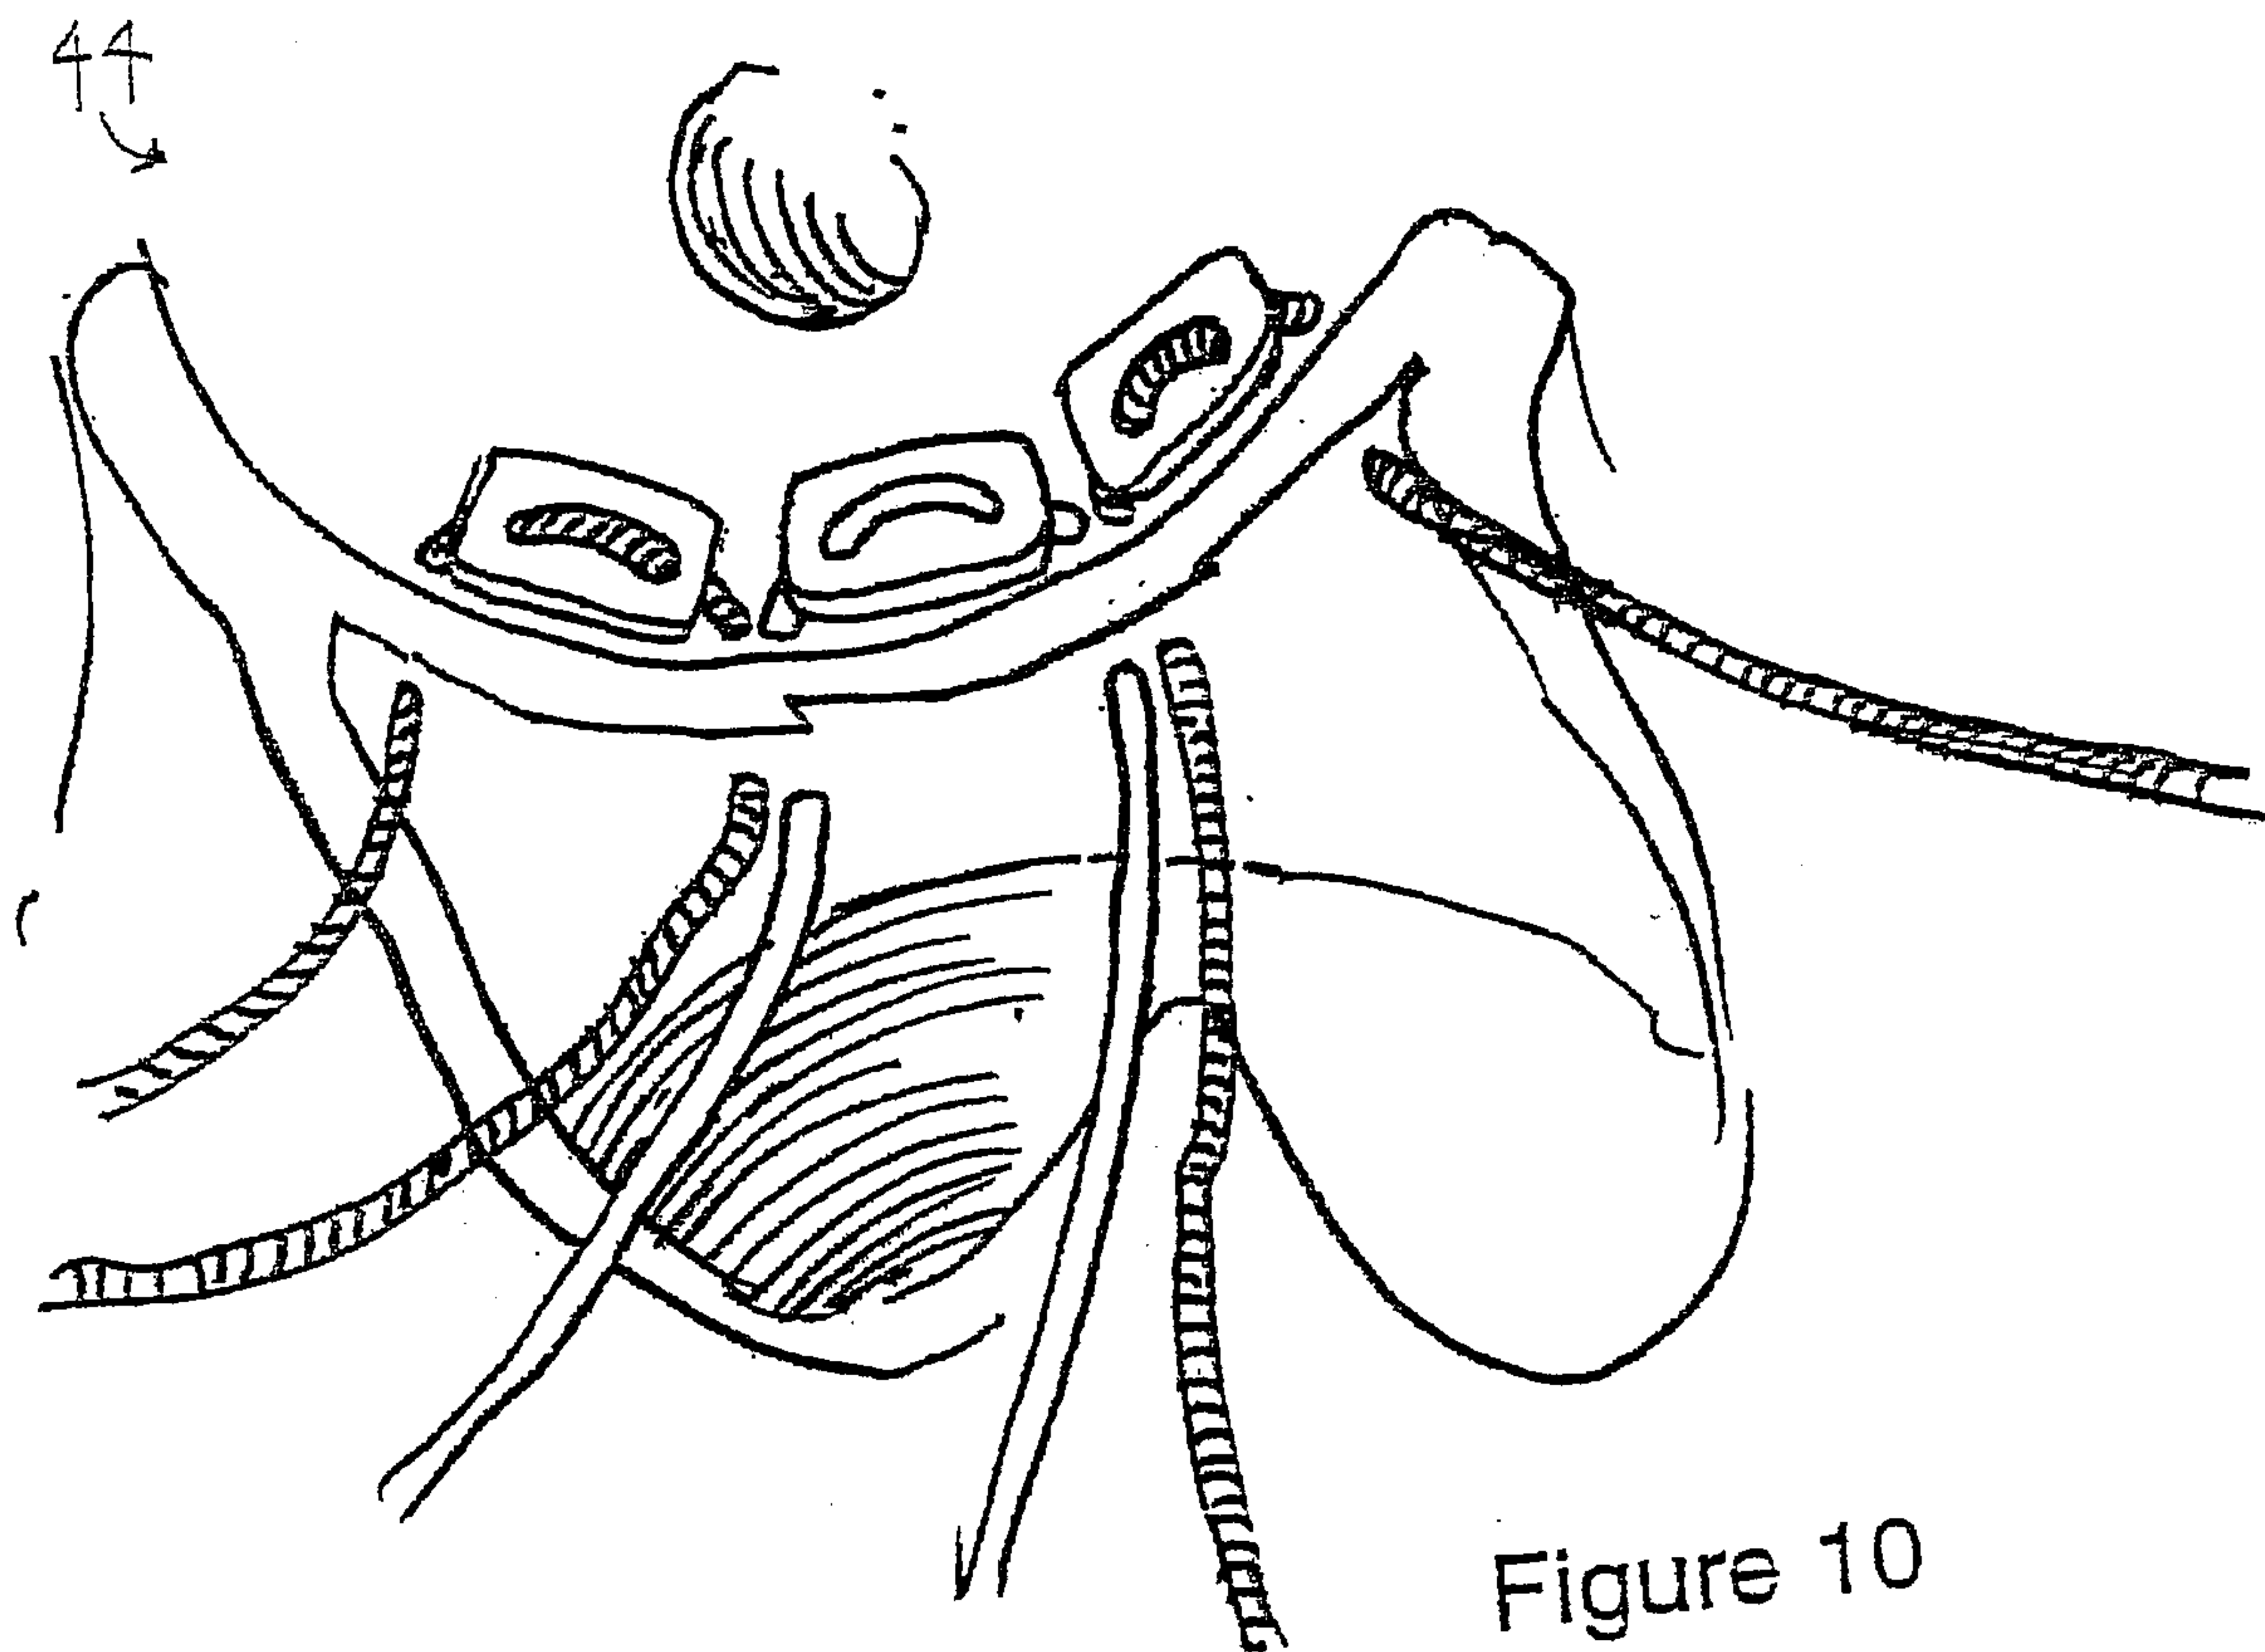


Figure 10

7/7

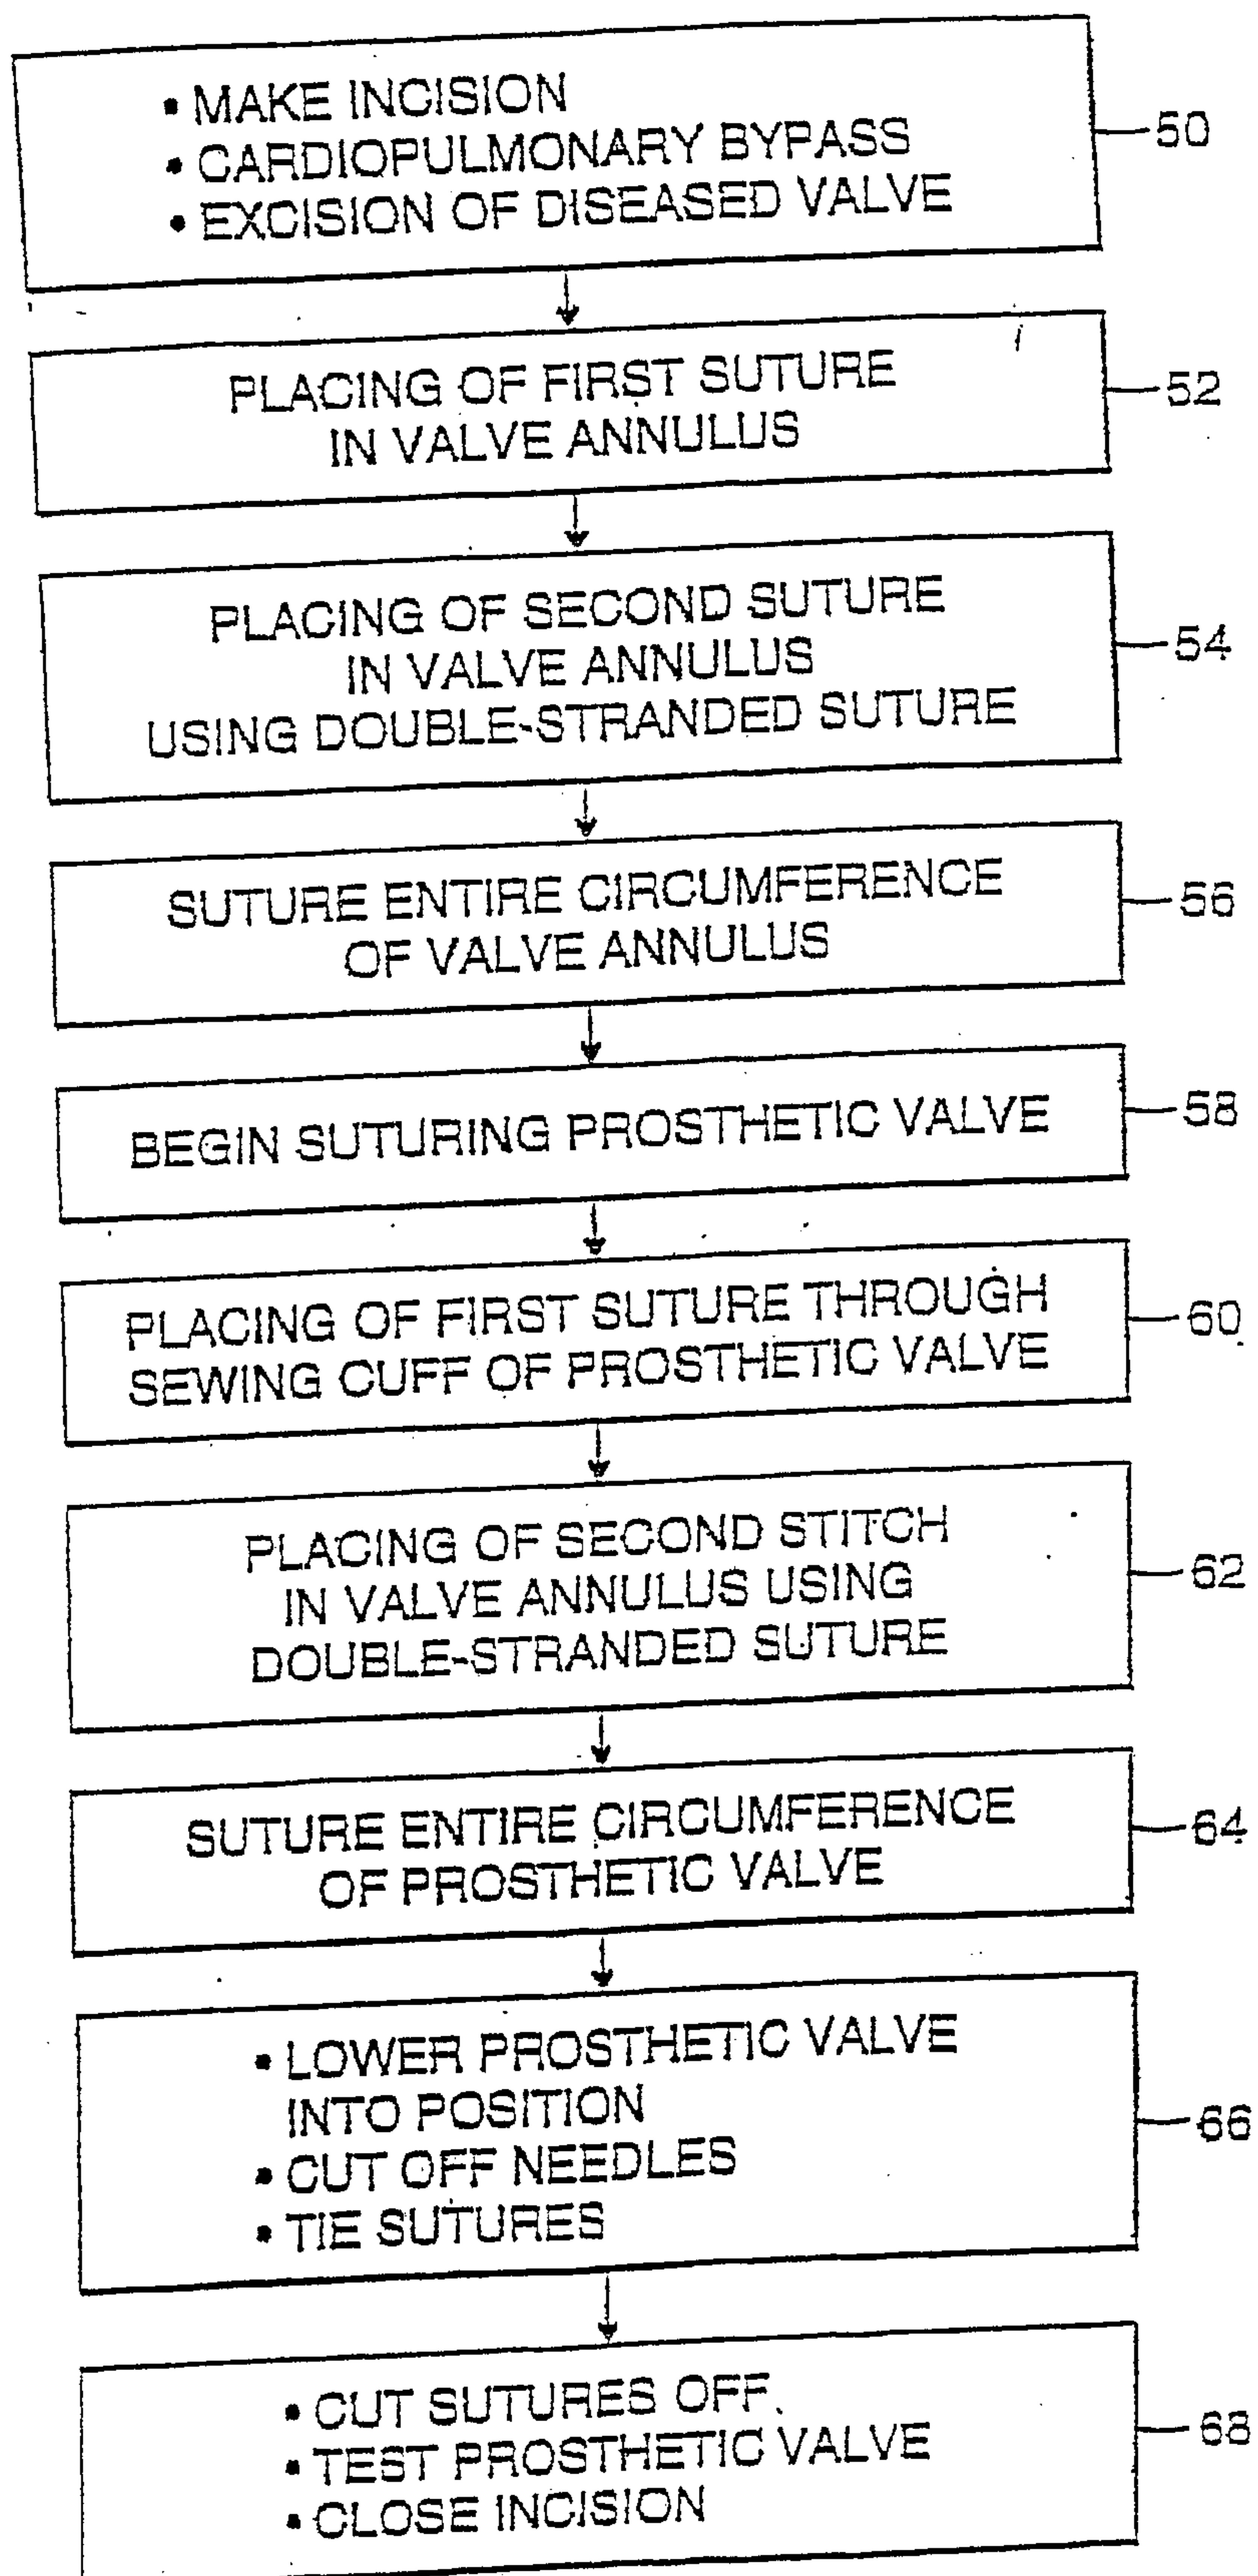


Figure 11

