

(86) Date de dépôt PCT/PCT Filing Date: 2014/01/27  
(87) Date publication PCT/PCT Publication Date: 2014/07/31  
(45) Date de délivrance/Issue Date: 2021/03/16  
(85) Entrée phase nationale/National Entry: 2015/07/22  
(86) N° demande PCT/PCT Application No.: EP 2014/051539  
(87) N° publication PCT/PCT Publication No.: 2014/114794  
(30) Priorités/Priorities: 2013/01/25 (US61/756,633);  
2013/01/25 (EP13152774.9)

(51) Cl.Int./Int.Cl. *A61F 2/24* (2006.01),  
*A61B 5/107* (2006.01)


(72) **Inventeurs/Inventors:**  
KERANEN, OLLI, SE;  
VIRTANEN, JANI, FI;  
PUGH, MARK, IE;  
O'CARROLL, GER, IE;  
MORAN, ADRIAN, IE

(73) **Propriétaire/Owner:**  
MEDTENTIA INTERNATIONAL LTD OY, FI

(74) **Agent:** NORTON ROSE FULBRIGHT CANADA  
LLP/S.E.N.C.R.L. S.R.L.

(54) Titre : DISPOSITIF MEDICAL ET PROCEDE POUR FACILITER LA SELECTION D'UN IMPLANT D'ANNULOPLASTIE

(54) Title: A MEDICAL DEVICE AND METHOD FOR FACILITATING SELECTION OF AN ANNULOPLASTY IMPLANT

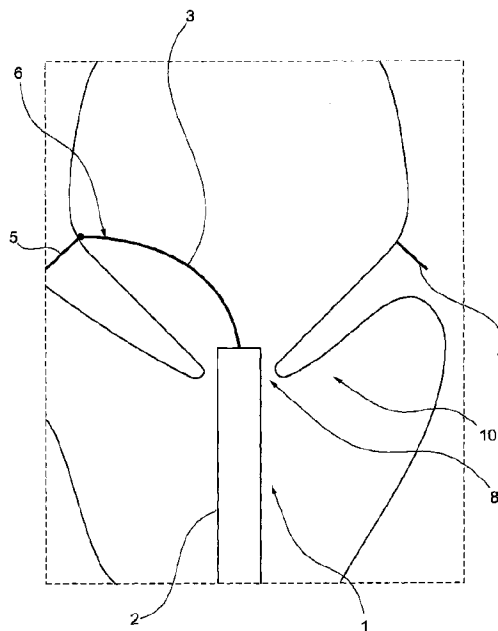

(57) **Abrégé/Abstract:**

A medical device and method for facilitating selection of a shape and/or size of an annuloplasty implant for a patient are disclosed. The device comprises a catheter with a proximal end and a distal end, and an extension member at least partly arranged inside the catheter with an operator end and a measurement end. The measurement end is extendable relative from the distal end of the catheter for apposition with at least one commissure of a cardiac valve. The measurement end of the extension member comprises means for guiding the annuloplasty implant at at least one commissure.

## (12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property  
Organization  
International Bureau



(10) International Publication Number  
**WO 2014/114794 A3**

(43) International Publication Date  
31 July 2014 (31.07.2014)

- (51) International Patent Classification:  
*A61F 2/24* (2006.01) *A61B 5/107* (2006.01)
- (21) International Application Number:  
PCT/EP2014/051539
- (22) International Filing Date:  
27 January 2014 (27.01.2014)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
13152774.9 25 January 2013 (25.01.2013) EP  
61/756,633 25 January 2013 (25.01.2013) US
- (71) Applicant: MEDTENTIA INTERNATIONAL LTD OY  
[FI/FI]; Mäkelankatu 58-60 3rd floor, FI-00510 Helsinki  
(FI).
- (72) Inventors: KERÄNEN, Olli; Anders Möllares väg 56, S-  
237 41 Bjärred (SE). VIRTANEN, Jani; Pyykuja 6,  
Söderkulla, FI-01150 Sipoo (FI). PUGH, Mark; 44  
Woodstream, Coolaney, Co. Sligo (IE). O'CARROLL,  
Ger; Castlebaldwin, Co. Sligo (IE). MORAN, Adrian;  
Ballinfull, Co. Sligo (IE).
- (74) Agent: KIPA; P.O. Box 1065, S-251 10 Helsingborg (SE).
- (81) Designated States (unless otherwise indicated, for every  
kind of national protection available): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,  
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,  
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,  
HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,  
KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME,  
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,  
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,  
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM,  
TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM,  
ZW.

- (84) Designated States (unless otherwise indicated, for every  
kind of regional protection available): ARIPO (BW, GH,  
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,  
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,  
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,  
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,  
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,  
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,  
KM, ML, MR, NE, SN, TD, TG).

## Declarations under Rule 4.17:

— of inventorship (Rule 4.17(iv))

## Published:

— with international search report (Art. 21(3))

[Continued on next page]

(54) Title: A MEDICAL DEVICE AND METHOD FOR FACILITATING SELECTION OF AN ANNULOPLASTY IMPLANT

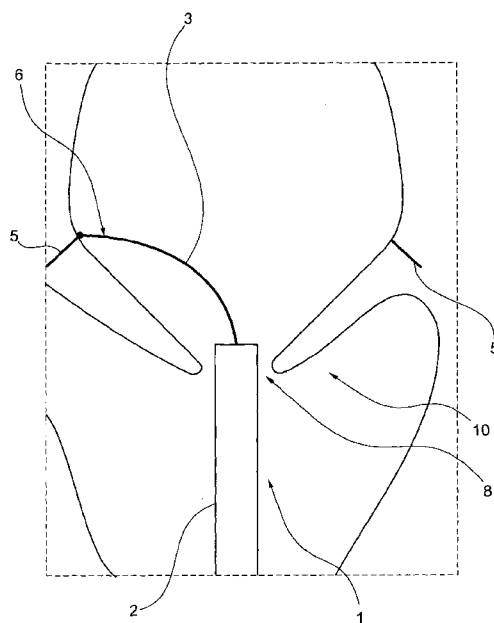


Fig. 1

(57) Abstract: A medical device and method for facilitating selection of a shape and/or size of an annuloplasty implant for a patient are disclosed. The device comprises a catheter with a proximal end and a distal end, and an extension member at least partly arranged inside the catheter with an operator end and a measurement end. The measurement end is extendable relative from the distal end of the catheter for apposition with at least one commissure of a cardiac valve. The measurement end of the extension member comprises means for guiding the annuloplasty implant at at least one commissure.

**WO 2014/114794 A3**



- 
- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))* **(88) Date of publication of the international search report:**  
18 September 2014

## A medical device and method for facilitating selection of an annuloplasty implant

### BACKGROUND OF THE INVENTION

#### 5           **Related applications**

This application is related to application EP13152770.7, PCT/EP2014/051540 "A valve for short time replacement, for taking over the function of and/or for temporary or partial support of a native valve in a heart" filed 25012013, application EP13152769.9, PCT/EP2014/051541 "A medical system, and a device for collecting chordae and/or leaflets" filed 25012013, application  
10 EP13152771.5, PCT/EP2014/051542 "Temporary atrium support device" filed 25012013 and application EP13152768.1, PCT/EP2014/051544 "A system for cardiac valve repair" filed 25012013.

#### **Field of the invention**

15           This disclosure pertains in general to the field of medical devices. More particularly the disclosure relates to a medical device for facilitating a selection of a size and/or shape of an annuloplasty implant.

#### **Description of the Prior Art**

20           It is known that a fit of an annuloplasty implant for reshaping cardiac valves is of great importance to ensure greatest possible effect in the repair of the cardiac valve(s). In US2012/197388 a variety of cardiac valve factors are described for choosing a valve body. There is no disclosure of how the factors are acquired and/or used for selection of the annuloplasty implant.

25           A problem with prior art is how to provide for an easy and reliable way to decide on the shape and/or size of the annuloplasty implant.

A further problem is how to provide for the operator to quickly and with ease visually see which annuloplasty implant the operator should choose. Further problems with prior art include difficulties in positioning such implants.

30           Thus, there is a need for a medical device acquiring the cardiac valve factors and for use in selection of the annuloplasty implant.

### SUMMARY OF THE INVENTION

35           Accordingly, examples of the present disclosure preferably seek to mitigate, alleviate or eliminate one or more deficiencies, disadvantages or issues in the art, such as the above-

identified, singly or in any combination by providing a medical device and a method for use thereof that facilitates a selection of a size and/or shape of an annuloplasty implant.

According to aspects of the invention, a medical device and method for facilitating selection of a shape and/or size of an annuloplasty implant for a patient is provided.

5           According to a first aspect of the invention, a medical device is provided, wherein the medical device comprises a catheter with a proximal end and a distal end. The medical device further comprises an extension member at least partly arranged inside the catheter with an operator end and a measurement end and wherein the measurement end of the extension member is extendable relative from the distal end of the catheter for apposition with at least one  
10 commissure of a cardiac valve, such as a mitral valve of the patient. The measurement end of the extension member comprises means for guiding the annuloplasty implant at at least one commissure.

          According to a second aspect of the invention, a method is provided, wherein the method is providing for facilitating selection of a shape and/or size of an annuloplasty implant.  
15       The method comprises providing a medical device such as the medical device for facilitating the selection of a shape and/or size of an annuloplasty implant as described above. The method further comprises positioning, preferably minimally invasively, a distal end of the catheter of the medical device at a cardiac valve of a patient. The method further comprises extending a measurement end of an extension member relative from a distal end of the catheter, bringing the  
20 measurement end in apposition with at least one commissure of the cardiac valve, such as a mitral valve of said patient. The method comprises further guiding the annuloplasty implant to at least one commissure by use of the extension member comprising means for guiding the annuloplasty implant.

          Some examples of the disclosure provide for easy positioning of an implant at a valve.

25           Some examples of the disclosure provide for efficient stabilizing of the valve before positioning an implant.

          Some examples of the disclosure provide for atraumatic guiding and positioning of an implant.

30           Some examples of the disclosure provide for an easy and reliable way to decide on the shape and/or size of the annuloplasty implant.

          Some examples of the disclosure also provide for the operator to quickly and with ease visually see which annuloplasty implant the operator should choose.

          Some examples of the disclosure also provide for easy use and movement of the extension member and catheter.

Some examples of the disclosure also provide for easy use and movement of the extension member and catheter independently of each other.

Some examples of the disclosure also provide for an extension member comprising a suitable material compatible with and for use in a catheter and in a heart.

5        Some examples of the disclosure also provide for a distance between two commissures to be measured immediately and relatively short amount of time.

Some examples of the disclosure also provide for an easier to control extension member due to shared alignment of two separable sections with the direction of a catheter.

10       Some examples of the disclosure also provide for an extension member that are easier to apposition with the two commissures due to the extension members having two separable extensions, or sections, being synchronized when extended.

Some examples of the disclosure also provide for easier manufacturing of the extension member comprising two separable sections since the extension member and the two separable extensions are made in one piece.

15       Some examples of the disclosure also provide for an increased breaking resistance and/or improved rotational force of an extension member and two separable sections.

Some examples of the disclosure also provide for an extension member and two separable sections to be manufactured from different material and thus have different material properties with respect to bending, rotation and/or biocompatibility.

20       Some examples of the disclosure also provide for a more reliable indication of when an extension member is at apposition or in contact to or with at least one commissure.

Some examples of the disclosure also provide for attaching at least one anchor at the at least one commissure to so that an annuloplasty implant can be anchored.

25       Some examples of the disclosure also provide for an annuloplasty implant to be anchored at different locations from different entering points at the commissure which provides for stabilizing the annuloplasty implant at these suitable locations.

Some examples of the disclosure also provide for an annuloplasty implant, which preferably has the shape of a helix ring, to be rotated into place at the cardiac valve by use of anchors.

30       Some examples of the disclosure also provide for a rotation of an extension member relative to a catheter.

Some examples of the disclosure also provide for a sliding of an extension member inside a catheter.

35       Some examples of the disclosure also provide for a synchronised movement of a catheter and an extension member.

Some examples of the disclosure also provide for a synchronised movement of a catheter and an extension member where the extension member and the catheter is engaged so that when movement of the catheter is performed the extension member is moved in the same way as the catheter.

5           Some examples of the disclosure also provide for an extended length of an extension member from a substantially centre position in a cardiac valve to an at least one commissure resulting in a measure on a size and/or shape of an annuloplasty implant.

          Some examples of the disclosure also provide for an extension member comprising two separable sections separable towards two commissures to result in a measure of a width  
10       between the two commissures which is very accurate and quickly acquired.

          Some examples of the disclosure also provide for an extension of the extension member from a catheter to be performed out from the proximal end of the catheter.

          Some examples of the disclosure also provide for an extension of the extension member from a catheter to be performed out through the sidewall of the catheter at a proximal  
15       end of the catheter.

          Some examples of the disclosure also provide for an indication of when at least one commissure has been found to be performed more reliable by use of a maneuver force detection unit.

          Some examples of the disclosure also provide for an indication of an apposition or  
20       contact to an at least one commissure by comparing a measured applied maneuver force with a predefined commissure value for triggering the indication.

          Some examples of the disclosure also provide for an operator to locate at least one commissure and attach anchors for an annuloplasty implant at the at least one commissure in one go and with the same device, saving time compared to needed to use a second instrument for  
25       attaching anchors.

          It should be emphasized that the term "comprises/comprising" when used in this specification is taken to specify the presence of stated features, integers, steps or components but does not preclude the presence or addition of one or more other features, integers, steps, components or groups thereof.

30

## **BRIEF DESCRIPTION OF THE DRAWINGS**

          These and other aspects, features and advantages of which examples of the disclosure are capable of will be apparent and elucidated from the following description of examples of the  
35       present disclosure, reference being made to the accompanying drawings, in which

Fig. 1 is a cross-sectional view of an example of a medical device for facilitating a selection of a size and/or shape of an annuloplasty implant positioned at cardiac valves;

Figs. 2a-b is a side view of another example of a medical device for facilitating a selection of a size and/or shape of an annuloplasty implant positioned at cardiac valves;

5 Fig. 3 is a cross-sectional view of another example of a medical device for facilitating a selection of a size and/or shape of an annuloplasty implant positioned at cardiac valves;

Figs. 4a-b is a side view of another example of a medical device for facilitating a selection of a size and/or shape of an annuloplasty implant positioned at cardiac valves;

10 Fig. 5 is a cross-sectional view of another example of a medical device for facilitating a selection of a size and/or shape of an annuloplasty implant positioned at cardiac valves;

Fig. 6 is a flowchart of a method for facilitating a selection of a size and/or shape of an annuloplasty implant;

15 Fig. 7 is a side view of another example of a medical device for facilitating a selection of a size and/or shape of an annuloplasty implant comprising a means for limiting leaflet movement; and

Figs. 8a-b, are views of another example of the device in Fig. 7.

## DESCRIPTION OF THE PREFERRED EMBODIMENTS

20 Specific examples of the disclosure will now be described with reference to the accompanying drawings. This disclosure may, however, be embodied in many different forms and should not be construed as limited to the examples set forth herein; rather, these examples are provided so that this disclosure will be thorough and complete, and will fully convey the scope of the disclosure to those skilled in the art. The terminology used in the detailed description of the examples illustrated in the accompanying drawings is not intended to be limiting of the disclosure. In the drawings, like numbers refer to like elements.

The following description focuses on an example of the present disclosure applicable to a medical device and in particular to a medical device for facilitating selection of a shape and/or size of an annuloplasty implant.

30 In an example of the disclosure according to Fig. 1 a medical device 1 for facilitating selection of a shape and/or size of an annuloplasty implant for a patient. The medical device 1 comprises a catheter 2 with a proximal end and a distal end 8. The medical device 1 further comprises an extension member 3 at least partly arranged inside the catheter 2 with an operator end and a measurement end 9 and wherein the measurement end 9 of the extension member 3  
35 is extendable relative from the distal end of the catheter 2 for apposition with at least one



commissure 5 of a cardiac valve 10, such as a mitral valve of the patient and wherein a measure related to the selection of the annuloplasty implant shape and/or size is based on at least an extended length of the measurement end of the extension member 3 from the distal end of the catheter 2, positioned at the cardiac valve, to the at least one commissure 5. By use of the

5 medical device 1 providing the measure related to the selection of the shape and/or size of the annuloplasty implant an operator of the medical device 1 is facilitated to in an easy and reliable way decide on the shape and/or size of the annuloplasty implant.

Catheter 2 used herein this disclosure is of well known types and wherein the catheter 2 is capable of comprising at least an extension member 3 according to this disclosure. Additionally

10 the catheter 2 is capable of being rotated and/or otherwise steered into position at the cardiac valve from a desired position in or outside the body by the operator.

In an example the extension member 3 is a rod or alternatively a pole and/or another long thin member with a cylindrical, circular, squared or rectangular base, capable of being arranged in the catheter 2. In an example illustrated in Fig. 2a the extension member 3 is a rod

15 extended perpendicular from the catheter 2 outwards towards the commissure. In another example illustrated in Fig. 2b the extension member is of a semi-circular shape such as a leaf shaped and where the semi-circular shape is directed towards the at least one commissure and has a spring action for apposition to at least one commissure. Another example of the extension member is illustrated in Fig. 2c where the extension member has an oval cone shape for

20 apposition to at least one commissure. The oval cone shape is in example formed of at least one extending sheet. In another example the oval cone shape is formed from several braided, extending or interwoven shape members.

In another example the extension member 3 is rotationally arranged in the catheter 2 for apposition with the at least one commissure 5. In another example the extension member 3 is

25 slidably arranged in the catheter 2. These arrangements allow for easy use and movement of the extension member 3 and catheter 2. Alternatively, the arrangement allows for easy use and movement independently of each other.

The extension member 3 is made of a suitable material compatible with and for use in a catheter 2 and in a heart, such as of titanium, nitinol, polymer, carbon fiber, textiles, all in solid

30 forms or in braided or sandwich structure forms, etc. The extension member 3 has a length that is at least as long as the catheter 2 and a distance from the catheter 2 to the at least one commissure 5. The extension member 3 is preferably long enough to be operated at the operator end by the proximal end of the catheter 2 and still extendable at the measurement end at the distal end of the catheter 2, i.e. the extension member 3 extends out of and from the catheter 2 at

35 both ends of the catheter 2 when used by the operator.

In another example of the extension member 3 the extension member 3 has a length wherein the measurement end of the extension member 3 only extends out and from the distal end of the catheter 2 and the operator end of the extension member 3 is arranged at level with the proximal end of the catheter 2, i.e. the extension member 3 only extends from the catheter 2 at the distal end of the catheter 2 when used by the operator. By using the manoeuvrable extension member 3 the operator measures a distance from the catheter 2 at the cardiac valve to the at least one commissure 5 and bases the size and/or shape of the annuloplasty implant on the distance.

In one example the measure related to the annuloplasty implant's shape and/or size is indicated at the operator end of the extension member 3. By having the operator end of the extension member 3 indicating the measure related to the size and/or shape of the annuloplasty implant, the operator can quickly and with ease visually see which annuloplasty implant the operator should choose.

As illustrated in Figs. 3, 4a and 4b, another example of the measurement end of the extension member 3 comprises two sections 3a, 3b, separable towards each of the mitral valve's commissures 5. By using two sections 3a, 3b, that are separable towards two commissures 5 at the mitral valve a distance between the two commissures 5 is measured immediately and faster than when using the extension member 3 without the two separable sections 3a, 3b.

In other example the two separable sections 3a, 3b, are upon extension from the catheter 2 aligned in a plane extending along a direction of the proximal end of the catheter 2. By having the two separable sections 3a, 3b, aligned and extended in the plane parallel to the direction of the catheter 2 the two sections 3a, 3b, will be easier to control due to their shared alignment with the direction of the catheter 2. This can be illustrated in Fig. 4b where the separable sections 3a, 3b, of the extension member 3 are separated perpendicular to the catheter 2.

Further illustrated in Fig. 4b, in yet another example the two separable sections 3a, 3b, separate with an opposite inclined separation angle. By having the two sections 3a, 3b, separate with opposite inclined angle of separation the two separable sections 3a, 3b, extend the same distance outwards towards the commissures 5 and thus are easier to apposition with the two commissures 5 due to their synchronised extension.

The two separable sections 3a, 3b, are in one example an integral continuation of the extension member 3. By having the two separable sections 3a, 3b, being the integral continuation of the extension member 3 the two separable sections 3a, 3b, better responds to manoeuvres, such as rotation and/or extension of the extension member 3 performed by the operator. Additionally, a requirement for manufacturing of the extension member 3 is greatly reduced since

the extension member 3 and the two separable extensions are made in one piece. In one example the two separable sections 3a, 3b, and the extension member's 3 mechanical aspects such as increased breaking resistance and/or improved rotational force, are greatly improved because the extension member 3 and the two separable sections 3a, 3b, are sized and/or shaped dependent on each other.

Alternatively, the two separable sections 3a, 3b, are joined to the measurement end of the extension member 3. By allowing the two separable sections 3a, 3b, to be joined at the measurement end of the extension member 3 they may be manufactured from a different material than the extension member 3 and thus have other material properties with respect to bending, rotation and/or biocompatibility.

In another example illustrated in Fig. 4a the extension member 3 comprises two separable sections 3a, 3b, which further comprises a c-shaped or claw shaped end. This claw shaped end is large enough to encompass an edge of a valve leaflet when aligned at the at least one commissure so that the extension member is further secured at the at least one commissure.

In one example the medical device 1 further comprises a force detection unit connected to the extension member 3 for detection of a manoeuvre force applied to the extension member 3. By using the force detection unit for detecting the manoeuvre force applied to the extension member 3 it is possible to get a further more reliable indication of when the extension member 3 is at apposition or in contact to or with at least one commissure 5.

In a further example of the extension member 3, as illustrated in Fig. 5, the measurement end of the extension member 3 comprises anchoring means 6 for attaching anchors 7 at at least one commissure 5 for the annuloplasty implant. Alternatively, one anchor 7 is attached at one commissure 5. By having the extension member 3 comprising anchoring means 6 for attaching anchors 7 for the annuloplasty implant it is possible to detect the location of the at least one commissure 5 and following the localization attach anchors 7 at the commissure 5 so that the annuloplasty implant can be anchored. This allows for fast deployment of the annuloplasty implant after the at least one commissure 5 is found and the size and/or shape of the annuloplasty implant has been chosen. In an example the anchoring means 6 is a claw or similar that allows for gripping the anchors.

In one example, the anchors 7 comprise at least one guiding unit or ring, as also illustrated in Fig. 5. By using at least one guiding unit or rings as anchors 7 the annuloplasty implant, which preferably has the shape of a helix ring, is rotated into place at the cardiac valve by use of the anchors 7. For example, when using rings as anchors 7 the annuloplasty implant is inserted through and slides in the rings securing the annuloplasty implant at the commissures 5.

In an example the anchors 7 are arranged in the atrium and catch and guides an upper part of the

helix ring. In another example the anchors 7 are arranged in the ventricle and catch and guides a lower part of the helix ring. In yet another example the anchors 7 are arranged in both the atrium and the ventricle, which is illustrated in Fig. 5, and catch both parts of the helix ring and part of the annulus. This allows for the helix ring to be anchored in different ways from different entering points at the commissure and provides for stabilizing the helix ring at suitable locations.

As discussed above, in one example the anchoring means 6 comprises anchors 7 that are used as guides, i.e. guiding means, for the annuloplasty implant at the at least one commissure. In another example the anchors 7 are used alternatively and/or in addition, as means for guiding the annuloplasty implant at the at least one commissure before the anchors 7 may be attached at the at least one commissure. This allows the user to both measure the correct size of the annuloplasty implant and guide the annuloplasty implant into place in an easy way without removing the medical device 1 when placed at the at least one commissure 5 and at the same time avoid attaching the anchors 7 at the at least one commissure, thus reducing the time for deploying the annuloplasty implant in the patient. In this example, the means for guiding is may be generally open or c-shaped which allows the annuloplasty implant to be guided into place in the heart without attaching the means for guiding at the at least one commissure and which allows for removal of the means for guiding, after the annuloplasty implant is implanted in the patient, through the opening of the c-shape. Fig. 8b shows the extension member comprising guiding means 7 that are generally open or C-shaped for guiding an implant into place. Other shapes that can be used are substantially loop-shaped, triangle-shaped, ring-shaped, such as shown in Fig. 8a, or any other suitable shape that allows for guiding the annuloplasty implant into place and/or allows for removing the means for guiding when the annuloplasty implant is implanted in the heart. As shown in Figs. 8a-b the extension member may have guiding means 7 at each the two lateral parts of the extension member that are to be placed at the commissures.

In a further example of the extension member 3, as illustrated in Fig. 7, the measurement end of the extension member 3 is shaped and/or formed as one coherent member 3. The extension member 3 may thus be formed as a continuous single or one-piece loop, i.e. a closed design. By using the extension member 3 formed from one piece closed design the member 3 is much more stable in its construction and easier to manoeuvre in the heart. Further, the continuous loop provides for particularly efficient stabilization of the anatomy and improving the precision by which the implant can be placed at the valve. Further, the continuous loop minimizes undesired interference with the chordae in the heart that would otherwise be the risk when having projections, edges, kinks etc. The extension member may comprise a continuous loop having a distal portion 8 being curved outwardly in a direction from the distal end of the catheter, see Fig. 8a. Such curved shape further reduces the risk of damaging any chordae due

the smooth shape. In the example in Fig. 8a, the distal portion 8 bridges the two guiding means 7 on the extension member. This provides for an atraumatic extension member that effectively stabilizes the valve, while at the same time providing guiding means for the implant. The principle of use and mode of use is the same as for the other examples of extension members 3 described in this application. Hence, the measurement, expansion, material and so on are the same and operates in the same way.

In another example, as also illustrated in figure 7, the extension member 3 comprises a leaflet limiter 3d. The leaflet limiter 3d is not limited to be used only with the coherent extension member 3 but the other types of extension members 3 disclosed in this application may also have the leaflet limiter 3d. The leaflet limiter 3d limits abnormal movement, such as prolapse, of the leaflets into the atrium. Such abnormal movement may arise if a chordae, or several chordae, that usually limits the movement of the leaflet is completely destroyed and the leaflet may thus freely move in the left atrium and/or left chamber. The leaflet limiter 3d is made of a material that expands with the extension member 3, and it may be made of the same material as the extension member 3. The leaflet limiter 3d may also be such that it can be bent, twisted or otherwise collapsed into the catheter 2 and then assume a desired shape when released from the catheter 2. Alternatively, the leaflet limiter 3d is expanded by a spring back motion and/or force when exited from the catheter 2 with the extension member 3d. The example of the leaflet limiter 3d shown in fig. 7 is a crossbar that extends between two anchoring points of the extension member 3 and is projected laterally from an intersecting plane of the anchoring points of the extension member 3. The leaflet limiter 3d may be of one piece or be made up of several pieces and/or have a number of different shapes and/or have various placements. One example of a shape that limits but not damage the leaflet(s) when hindering the movement into the atrium would be to have a simple straight projection outwards towards the leaflets from the extension member 3 with a blunt end, which can limit the movement but not damage the leaflet(s) when hindering the movement into the atrium. Preferably, the extension member 3 has two leaflet limiters 3d, one on each side of the extension member 3 for each leaflet when the extension member 3 is arranged at the commissures. But, there could also be only one leaflet limiter 3d. This could be the case if it is known that one leaflet is already damaged and moving freely when starting the procedure of measuring and/or deciding the size of the annuloplasty implant.

In an example according to the disclosure and as illustrated in Fig. 6 is a method for facilitating selection of a shape and/or size of an annuloplasty implant. The method comprises providing 100 a medical device 1 such as the medical device 1 for facilitating the selection of a shape and/or size of an annuloplasty implant as described above. The method further comprises positioning 200, preferably minimally invasively, a distal end of the catheter 2 of the medical

device 1 at a cardiac valve of a patient. The method further comprises extending 300 a measurement end of an extension member 3 relative from a distal end of the catheter 2, bringing the measurement end in apposition with at least one commissure 5 of the cardiac valve, such as a mitral valve of said patient. The method also comprises basing 400 the annuloplasty implant's

5 shape and/or size on at least an extended length of the extension member 3 relative from the distal end of the catheter 2 to the at least one commissure 5. By using the medical device 1 for facilitating the selection of the shape and/or size of the annuloplasty implant comprising the catheter 2 and the extension member 3 it is possible to base the size/and or shape of the annuloplasty implant on the extension of the extension member 3 relative from the catheter 2.

10 In one example, the catheter 2 is positioned in a substantially centre position at the cardiac valves. Following the extension member 3 is extended from the distal end of the catheter 2 by an operator pushing the extension member 3 from the proximal end of the catheter 2 through the catheter 2 and out at the distal end of the catheter 2. The measurement end of the extended extension member 3 is positioned at, appositioned, or in contact with the commissure 5.

15 The positioning of the extension member 3 is performed in a number of way such as by rotating the extension member 3 relative to the catheter 2, sliding the extension member 3 inside the catheter 2, by synchronised movement of the catheter 2 and the extension member 3 and/or by synchronised movement of the catheter 2 and the extension member 3 where the extension member 3 and the catheter 2 is engaged so that when movement of the catheter 2 is performed

20 the extension member 3 is moved in the same way as the catheter 2.

The extended length of the extension member 3 from the substantially centre position to the commissure 5 gives the operator a measure on the size and/or shape of the annuloplasty implant. The extended length is in one example used as basis for the radius of the annuloplasty implant. In another example an assumption that the cardiac valve is symmetrical together with the

25 extended length of the extension member 3 is used as basis for the width of the annuloplasty device.

In another example of the method for facilitating selection of a shape and/or size of an annuloplasty implant the basing of the annuloplasty implant's shape and/or size is based on a measured valve width between two commissures 5 of the cardiac valve by the extension of the

30 measurement end of the extension member 3 relative from the catheter 2 to the two commissures 5. Basing the selection of the annuloplasty implant on the distance between the two commissures 5 gives a better fit of the annuloplasty implant than when only using one commissure 5. In one example the width between the two commissures 5 are measured by sweeping the extension member 3 from one commissure 5 to the other commissure 5.

In another example the width is obtained between the two commissures 5 by arranging of two separable sections 3a, 3b, of the extension member 3 separable towards the commissures 5. The use of the extension member 3 comprising two separable sections 3a, 3b, separable towards the commissures 5 results in the width between the commissures 5 being measured  
 5 more accurately and faster than any presently known method. When obtaining the width between the commissures 5 by use of the extension member 3 comprising two separable sections 3a, 3b, the operator positions the catheter 2 at the cardiac valve and extends the extension member 3. The two separable sections 3a, 3b, separate outwards towards the commissures 5 when they passes the distal end of the catheter 2 by the operator pushing the extension member 3 through  
 10 the catheter 2 from the proximal end of the catheter 2. Depending on the pushed distance of the extension member 3 i.e. extended distance of the extension member 3 and the two separable sections 3a, 3b, the width of the commissures 5 is known. The separation of the two separable sections 3a, 3b, is preferably at a predefined angle and/or settles at the predefined angle when measuring the width between the commissures 5. The extension of the extension member 3 from  
 15 the catheter 2 may be performed in several ways such as, out from the proximal end of the catheter 2 and/or out through the sidewall of the catheter 2 at the proximal end.

In one example the method further comprises measuring an applied manoeuvre force on the extension member 3 while manoeuvring the extension member 3 to apposition the measurement end with the at least one commissure 5 and, indicating when the measurement end  
 20 is apposition with the at least one commissure 5 based on the measured applied manoeuvre force. By measuring the applied manoeuvre force on the extension member 3 applied by the operator the indication of when at least one commissure 5 has been found is performed more reliable than by use of tactile indication through the extension member 3. The measurement of the applied manoeuvre force may e.g. be measured by a force detection unit.

25 In one example if the force detection unit is used, the force detection unit bases the indication of the apposition to the at least one commissure 5 by comparing the measured applied manoeuvre force with a predefined commissure 5 value for triggering the indication of the apposition of the measurement end with the at least one commissure 5.

30 In another example of the method for facilitating selection of a shape and/or size of an annuloplasty implant an indication is based on a measured force for stretching the extension member 3 between two commissures 5. By measuring the force needed to extend and/or stretch the extension member 3 outwards towards the two commissures 5 it is possible to detect when the two commissures 5 have been found since the two commissures 5 have a difference in flexibility compared to other tissue in the atrium.

In yet another example the method comprises anchoring at least one anchor at at least one commissure 5 by use of the extension member 3 comprising anchoring means. By using at least one anchor at at least one commissure 5 by using the extension member 3 the operator can attach anchors for the annuloplasty device in one go and with the same device, saving time compared to needed to use a second instrument for attaching anchors. In one example the anchoring means 6 comprises anchors 7, or guiding means, that are used as guides for the annuloplasty implant at the at least one commissure. In another example the anchors 7 are used alternatively and/or in addition, as means for guiding the annuloplasty implant at the at least one commissure before the anchors 7 are attached at the at least one commissure. This allows the user to both measure the correct size of the annuloplasty implant and guide the annuloplasty implant into place in an easy way without removing the medical device 1 when placed at the at least one commissure 5 and at the same time avoid attaching the anchors 7 at the at least one commissure, thus reducing the time for deploying the annuloplasty implant in the patient. In this example, the means for guiding is preferably c-shaped which allows the annuloplasty implant to be guided into place in the heart without attaching the means for guiding at the at least one commissure and allows for removal of the means for guiding after the annuloplasty implant is implanted in the patient through the opening of the c-shape. Other shapes that can be used are loop-shaped, ring-shaped or any other suitable shape that allows for guiding the annuloplasty implant into place and/or allows for removing the means for guiding when the annuloplasty implant is implanted in the heart.

The present disclosure has been described above with reference to specific examples. However, other examples than the above described are equally possible within the scope of the disclosure. Different method steps than those described above, performing the method by hardware or software, may be provided within the scope of the disclosure. The different features and steps of the disclosure may be combined in other combinations than those described. The scope of the disclosure is only limited by the appended patent claims.

30



## Claims

1. A medical device for facilitating selection of a shape and/or size of an annuloplasty implant for a patient, comprising:
  - a catheter with a proximal end and a distal end,
  - an extension member at least partly arranged inside the catheter with an operator end and a measurement end,
  - wherein the measurement end of the extension member is extendable relative from the distal end of the catheter for apposition with at least one commissure of a cardiac valve,
  - wherein a measure related to the selection of the annuloplasty implant's shape and/or size is based on at least an extended length of the measurement end of the extension member from the distal end of the catheter, when positioned at the cardiac valve, to the at least one commissure, and
  - wherein the measurement end of the extension member comprises means for guiding the annuloplasty implant at at least one commissure.
2. The medical device according to claim 1, wherein the means for guiding is loop-shaped or c-shaped.
3. The medical device according to any one of claims 1-2, wherein the measure related to the annuloplasty implant's shape and/or size is indicated at the operator end of the extension member.
4. The medical device according to any one of claims 1-3, wherein the measurement end of the extension member comprises two sections separable towards each of the mitral valve's commissures.
5. The medical device according to claim 4, wherein the two separable sections are upon extension from the catheter aligned in a plane extending along a direction of the proximal end of the catheter.
6. The medical device according to claims 4 or 5, wherein the two separable sections separate with an opposite inclined separation angle.
7. The medical device according to any one of claims 4-6, wherein the two separable sections are an integral continuation of the extension member.
8. The medical device according to any one of claims 5-7, wherein the two separable sections are joined to the measurement end of the extension member.

9. The medical device according to any one of claims 1-8, further comprising a force detection unit connected to the extension member for detection of a manoeuvre force applied to the extension member.

10. The medical device according to any one of claims 1-9, wherein the extension member is rotationally arranged in the catheter for apposition with the at least one commissure.

11. The medical device according to any one of claims 1-10, wherein the measurement end of the extension member comprises anchoring means for attaching anchors at at least one commissure for the annuloplasty implant.

12. The medical device according to claim 11, wherein the anchors comprise at least one guiding unit or ring.

13. The medical device according to any one of claims 1-12, further comprising a leaflet limiter arranged at the extension member.

14. The medical device according to claim 13, wherein the leaflet limiter is self-expandable from a delivery mode to an expanded mode.

15. The medical device according to any one of claims 1-4 and 10-14, wherein the extension member is formed as a continuous single or one-piece loop.

16. The medical device according to claim 15, wherein the continuous loop has a distal portion being curved outwardly in a direction from the distal end of the catheter.

1/8

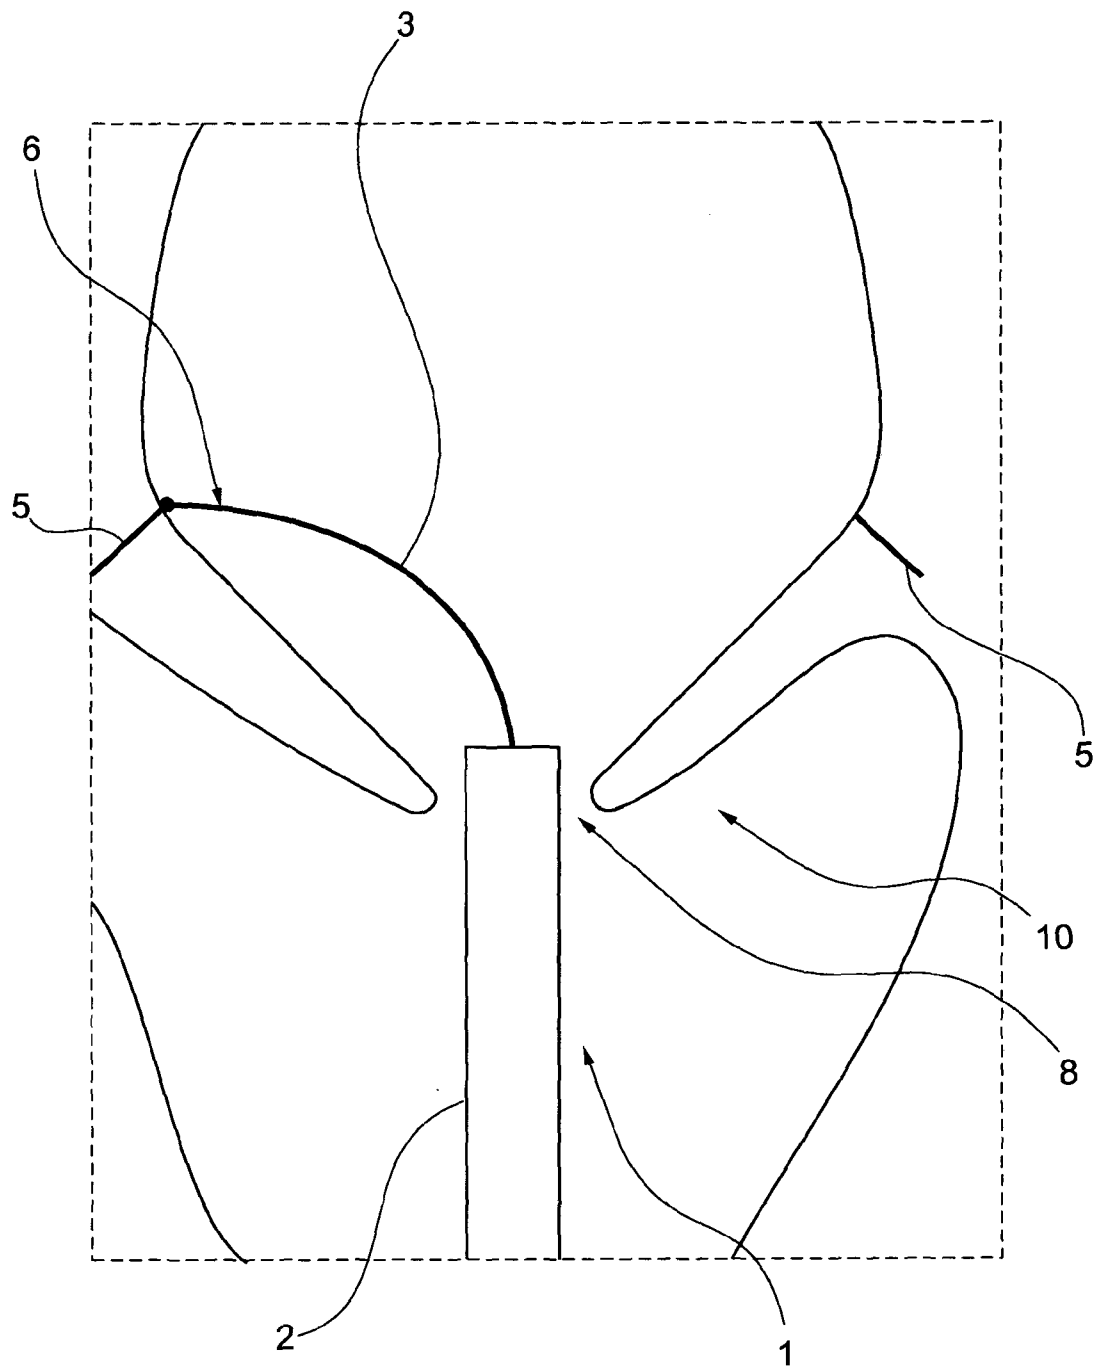


Fig. 1

2/8

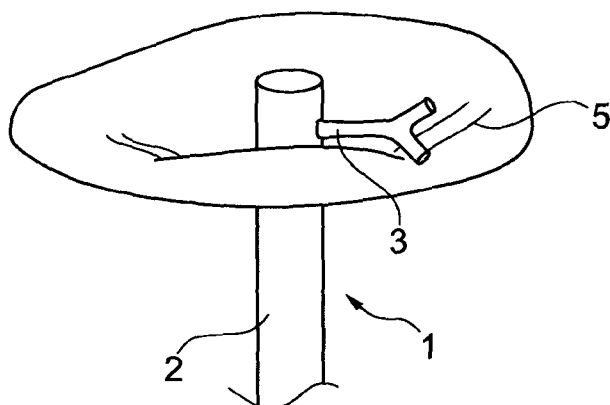


Fig. 2a

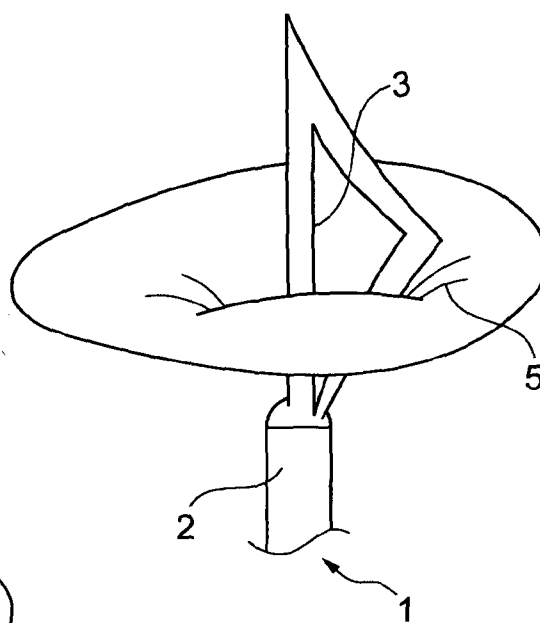


Fig. 2b

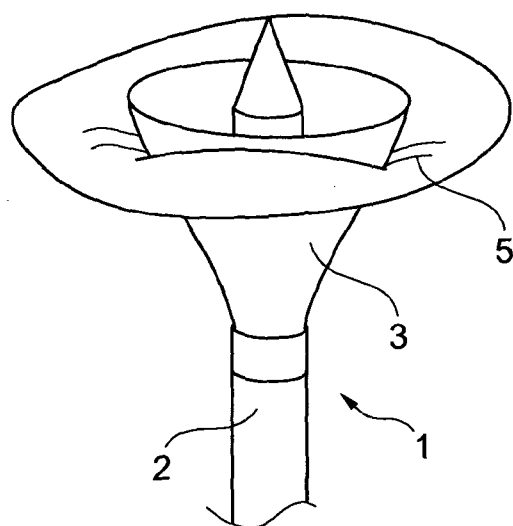


Fig. 2c

3/8

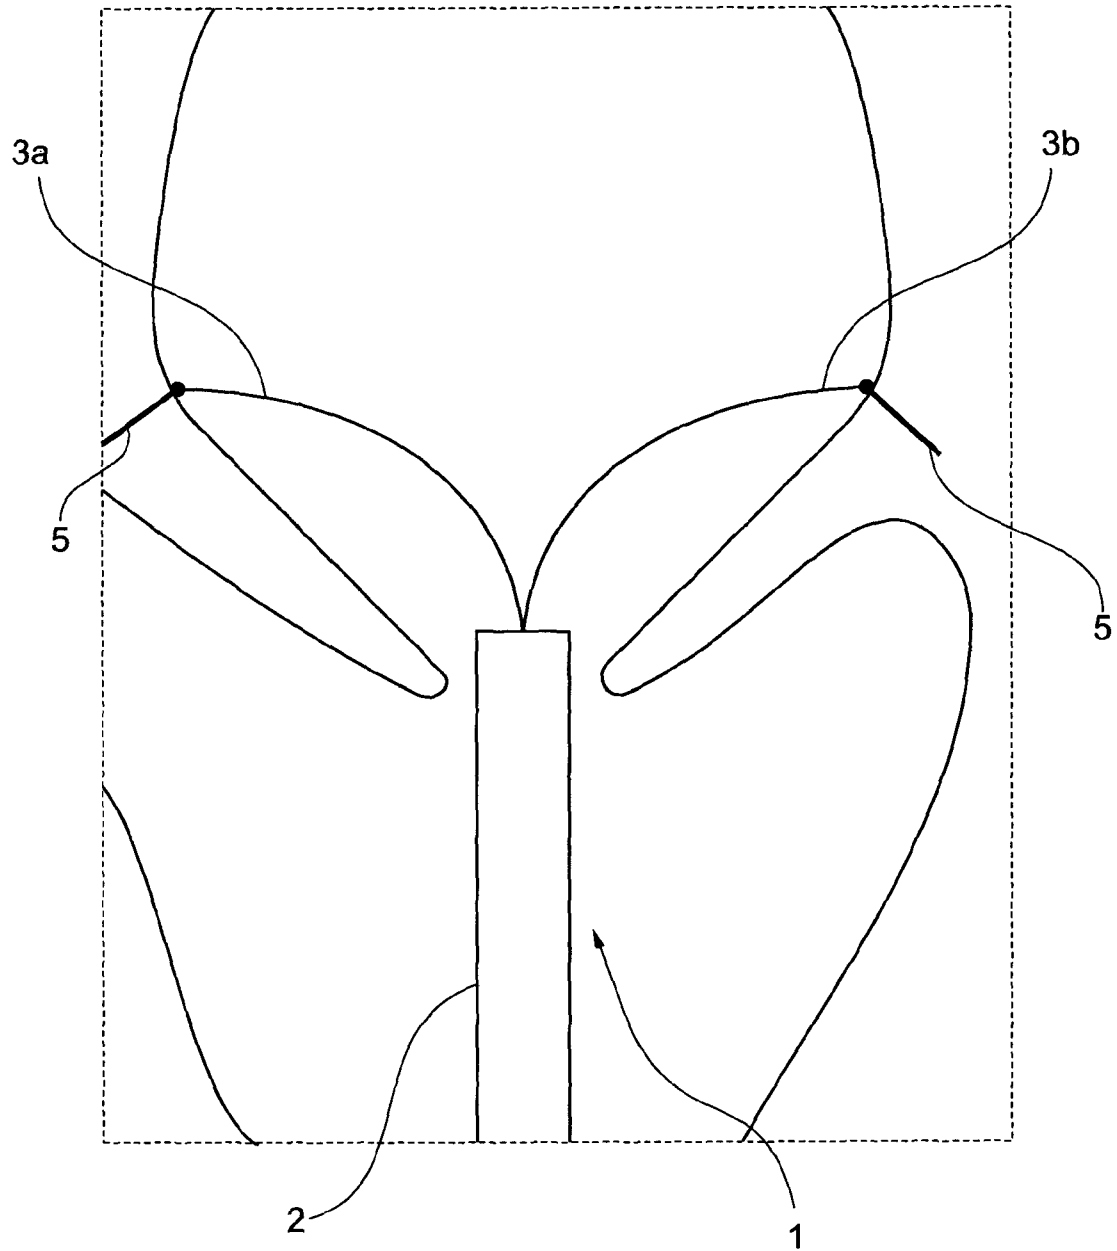


Fig. 3

4/8

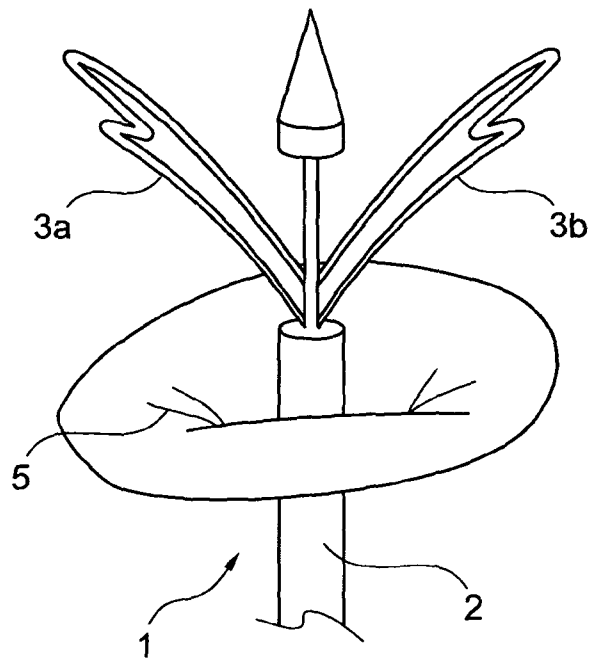


Fig. 4a

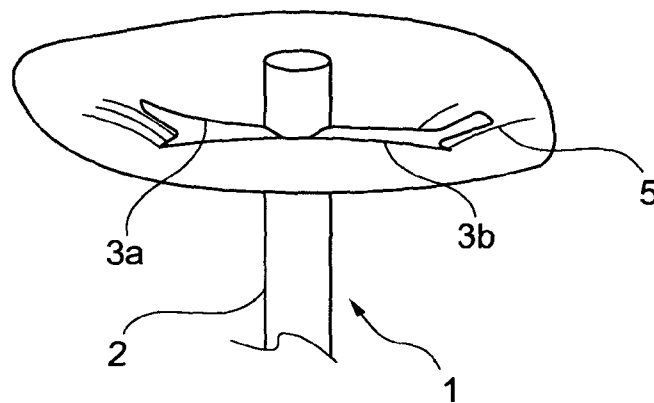


Fig. 4b

5/8

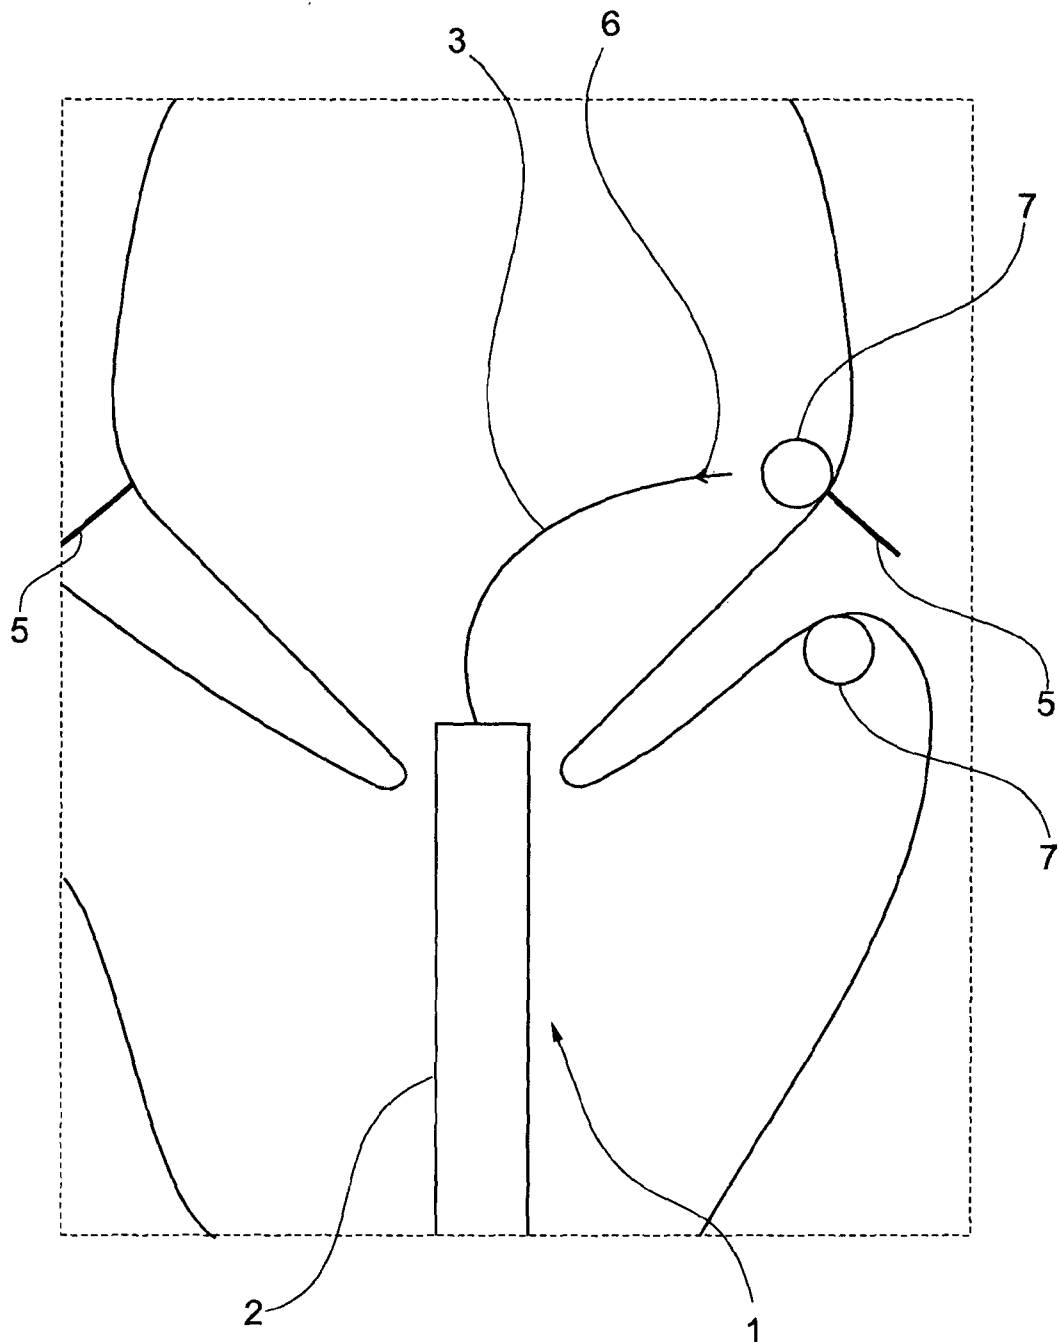


Fig. 5

6/8

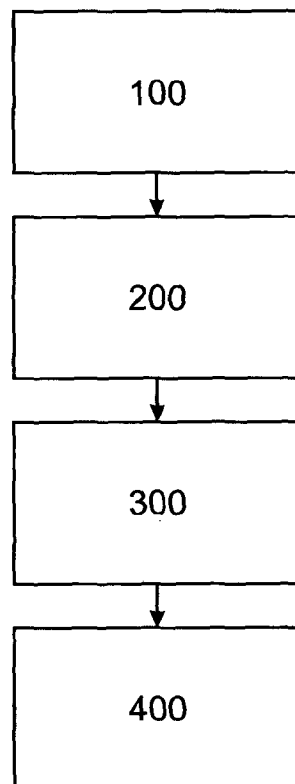


Fig. 6



7/8

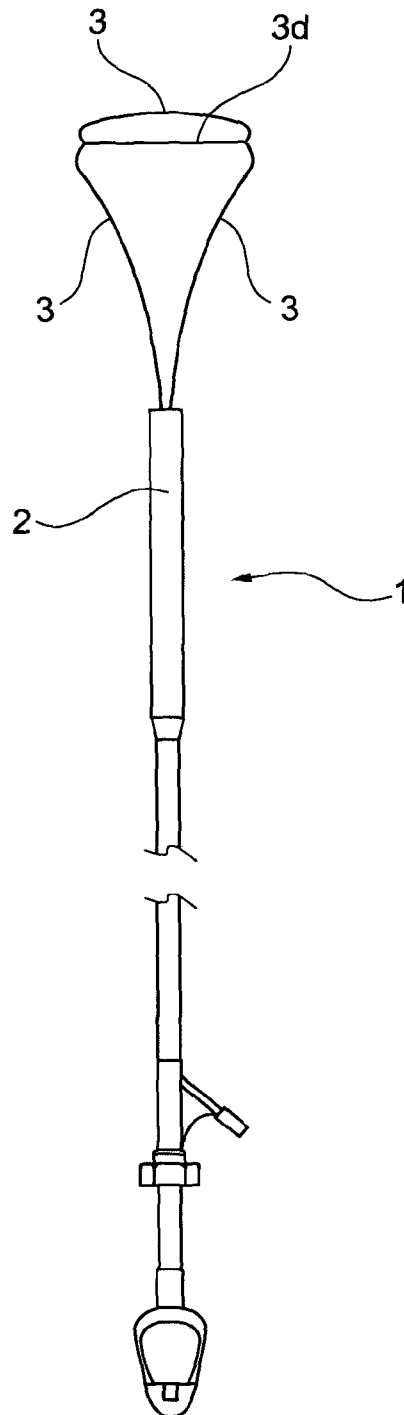


Fig. 7

8/8

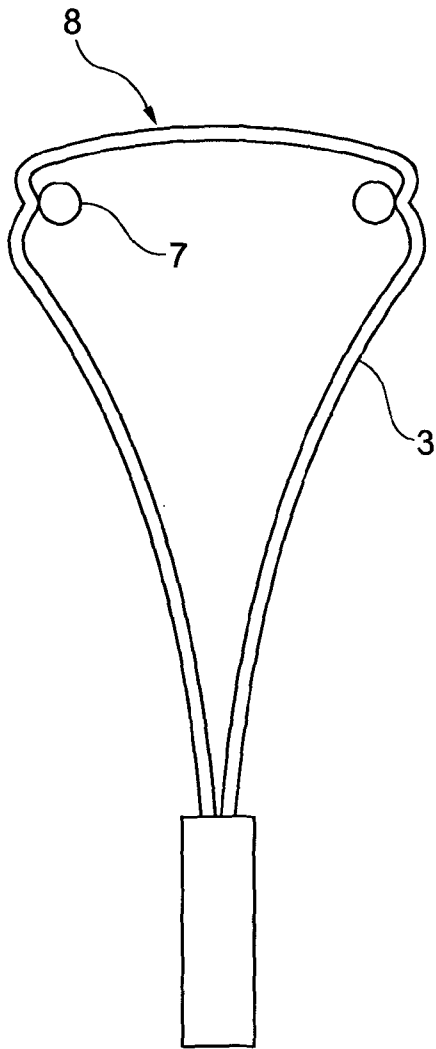


Fig. 8a

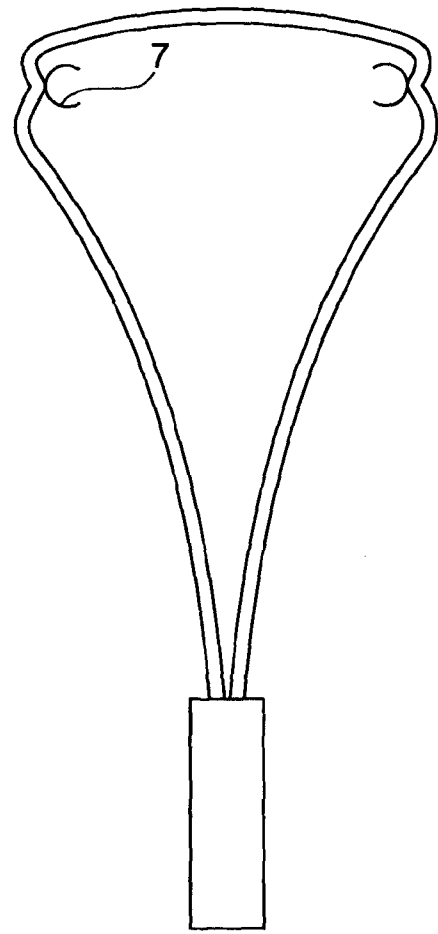


Fig. 8b

