



- (51) International Patent Classification:
A61B 5/053 (2006.01) *A61M 1/14* (2006.01)
- (21) International Application Number:
PCT/EP2013/001257
- (22) International Filing Date:
26 April 2013 (26.04.2013)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
EP 12002955 26 April 2012 (26.04.2012) EP
61/638,514 26 April 2012 (26.04.2012) US
- (71) Applicant: **FRESENIUS MEDICAL CARE
DEUTSCHLAND GMBH** [DE/DE]; Else-Kröner-Straße
1, 61352 Bad Homburg (DE).
- (72) Inventors: **WABEL, Peter**; Chopinweg 12, 64287 Darm-
stadt (DE). **CHAMNEY, Paul**; 37 Trooper Road, Aldbury
near Tring, Herts HP23 5RW (GB). **GROEBER, Tobias**;
Leipziger Ring 25, 63150 Heusenstamm (DE). **MOISSEL,
Ulrich**; Ysenburger Strasse 5, 61184 Karben (DE).

WIESKOTTEN, Sebastian; Georg-Sachse-Str. 33, 64372
Ober-Ramstadt (DE).


(74) Agent: **BOBBERT & PARTNER**; Patentanwälte, Post-
fach 1252, 85422 Erding (DE).

(81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP,
KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD,
ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI,
NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU,
RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ,
TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA,
ZM, ZW.

(84) Designated States (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,

[Continued on next page]

(54) Title: ELECTRODES FOR A BIO-IMPEDANCE MEASURING DEVICE, AND DEVICES USED DURING DIALYSIS

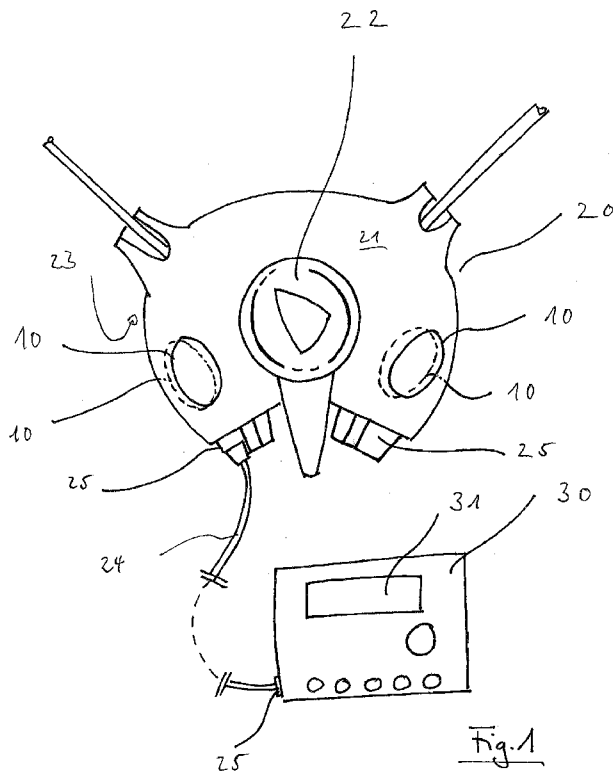

(57) Abstract: The present invention relates to electrodes (10) for a bio-impedance measuring device (30) or a body composition monitor, the electrodes (10) being integral with or being attached to a surface of at least one device belonging to a group of electronic and/or non-electronic devices used in the preparation of a dialysis treatment or during dialysis, in particular during peritoneal dialysis, the group preferably consisting of organizers (20) of a continuous ambulatory peritoneal dialysis system (CAPD), automated peritoneal dialysis devices, automated peritoneal dialysis-cyclers (APD-Cycler) (40), bioelectrical impedance analyzers (BIA) (30), body composition monitors (BCM), hand-held electrodes holders (50) for the electrodes, and dialysis apparatuses. The invention also relates to devices and methods used during dialysis.



MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, **Published:**
SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, — *with international search report (Art. 21(3))*
GW, ML, MR, NE, SN, TD, TG).

Description

5

**Electrodes for a bio-impedance measuring device, and devices
used during dialysis**

The present invention relates to electrodes according to
10 claim 1 for realising at least one bioelectrical impedance
analysis to estimate the hydration and/or the nutritional
status of dialysis patients before, during or after dialysis
treatment. It further relates to a device to be used before or
during dialysis or while preparing a dialysis treatment, in
15 particular peritoneal dialysis, ultrafiltration,
hemofiltration, hemodiafiltration, hemo-ultrafiltration or
hemodialysis, according to claim 8, to a dialysis apparatus
according to claim 14, and to a method for determining
parameters for estimating the hydration or the nutritional
20 status of a dialysis patient according to claim 16. The
present invention further relates to a non-transitory
computer-readable medium with an executable program stored
thereon according to claim 20, to a computer program and to a
computer program product comprising computer program code.

25

In certain treatment procedures such as dialysis (hereinafter,
this term and the term dialysis treatment each encompass
peritoneal dialysis, ultrafiltration, hemodialysis,
hemofiltration, hemo-ultrafiltration, hemodiafiltration and
30 the like) excess body fluid is removed from the patient's
body. An accurate knowledge of the patient's hydration state
before starting a treatment session is desirable for
determining the most appropriate dialysis treatment, for
controlling of the dialysis apparatus, and for determining and
35 achieving the patient's post treatment target weight.

For example, peritoneal dialysis is often conducted by the patient alone at home and without being constantly monitored or supervised by medically trained staff. In fact, home
5 peritoneal dialysis patients are seen by the dialysis staff in charge only every 4-12 weeks. Therefore, hydration state measurements made in a professional setting are made only every now and then. For that reason, it is particularly important for peritoneal dialysis to be provided with accurate
10 methods and devices in order to easily determine by oneself the present hydration state between examinations that are carried out by the medical staff every 4-12 weeks.

There are some methods available to estimate the hydration
15 state of a patient including assessment of weight changes, edema, jugular venous pressure, blood pressure, the measurement of hematocrit, of natriuretic peptides (ANP, Pro-BNP, and BNP), cyclic guanine monophosphate (cGMP) and/or inferior vena cava diameter. These methods are not all
20 clinically useful because of limited accuracy or practicability or both.

The estimation of the patient's hydration (also referred to as the patient's hydration state) before a dialysis treatment
25 session using bio-impedance analysis can be a useful step toward revealing the patient's hydration status. Bio-impedance techniques measuring body fluid content are advantageous in that they are non-invasive, relatively cheap, generally easily to perform and reliable if carried out correctly. Further they
30 can in theory be carried out by the patient himself and even without professional supervision. However, these clinical methods are still too cumbersome for some patients. Also, when carried out, the results depend strongly on how accurately the electrodes used for the bio-impedance measurement are placed
35 by the patient. In practice, it has turned out that a number

of patients are not capable of using the electrodes which have to be placed on both arms, one arm and one foot, both feet, or the like in the intended manner. In consequence, the results stemming from bio-impedance measurements - if carried out at all - and their interpretation can suffer remarkably.

It is therefore an object of the present invention to provide electrodes intended for a bioelectrical impedance measurement and to suggest devices for a bioelectrical impedance measurement or for a dialysis treatment or both, and a corresponding method.

This object is solved by the feature combinations of the independent claims.

15

The electrodes according to the present invention, i.e., one, two, or more electrodes, or one, two, or more pairs of electrodes, for a bio-impedance measuring device are being intended and/or prepared to be used with a bio-impedance measuring device. The electrodes are integral with or attached to or into a portion or a surface (or intended to be attached) of at least one device selected from a group of electronic and/or non-electronic devices used in the preparation of a dialysis treatment or during dialysis of any kind as set forth above, for example during peritoneal dialysis or hemodialysis. In some embodiments according to the present invention, said group consists of at least one item of organizers of a continuous ambulatory peritoneal dialysis system (CAPD), organizer for so-called stay-safe-dialysis-bags, automated peritoneal dialysis devices, automated peritoneal dialysis-cyclers (APD-Cycler), bioelectrical impedance analyzers (BIA), body composition monitors (BCM), hand-held electrodes holders for the electrodes and dialysis apparatuses.

A 'dialysis apparatus' or a 'dialysis machine' or 'dialysis device' within the meaning of the present invention may be an apparatus configured or embodied for carrying out a dialysis treatment within the meaning thereof as set forth above.

5 Hence, a dialysis apparatus or machine according to the present invention may be a peritoneal dialysis machine, a hemodialysis machine, a hemofiltration machine, a hemo-ultrafiltration machine, a hemodiafiltration machine and the like or combinations thereof.

10

The device according to the present invention is used during dialysis or while preparing a dialysis treatment or intended to be used during dialysis or while preparing a dialysis treatment, in particular peritoneal dialysis or any other kind
15 of dialysis. The device comprises at least one (or two or more) integrated and/or attached electrode or pairs of electrodes according to the present invention.

The dialysis apparatus according to the present invention
20 comprises at least one electrode according to the present invention, the device according to the present invention, or both, or is in signal communication therewith to receive results of measurements carried out by means of the electrodes.

25

The method for determining parameters for estimating the hydration or the nutritional status of a dialysis patient according to the present invention encompasses touching at least two electrodes according to the present invention with
30 at least two body portions while the electrodes are connected to a bioelectrical impedance analyzer or a body composition monitor or both. The method further comprises collecting and processing the information gained by of the electrodes in a processing element in at least one bioelectrical impedance
35 analyzer and/or body composition monitor.

The present invention also relates to a non-transitory computer-readable medium with an executable program stored thereon, wherein the program instructs a programmable computer system to perform the steps of any of the embodiments of the method according to the present invention as described herein.

The present invention also relates to a computer program and to a computer program product comprising computer program code portions adapted to perform any of the embodiments of the method according to the present invention as described herein.

The present invention also relates to the use of the electrodes according to the present invention, of the device according to the present invention and of the dialysis apparatus according to the present invention.

Developments of the present invention are each also the subject of the dependent claims.

The use of the expression 'may be' or 'may have' and so on, is to be understood herein synonymously with 'preferably is' or 'preferably has', respectively, and so on, and is intended to illustrate exemplary embodiments according to the present invention.

Embodiments according to the present invention may comprise one, some or all of the following features in arbitrary combinations.

In some embodiments according to the present invention, if reference is made to "the steps of any of the embodiments of the method according to the present inventions", in particular in connection with the non-transitory computer-readable medium with an executable program stored thereon, the computer

program or the computer program product comprising computer program code, "the steps" may be understood as referring only to steps that will be carried out by a device or in an automatic manner.

5

In certain embodiments according to the present invention, the non-transitory computer-readable medium with an executable program stored thereon comprises electrodes, a processor and/or any other device needed for carrying out the steps, or
10 is connected therewith.

In some embodiments, the electrodes according to the present invention are detachably attached to the electronic and/or a non-electronic device.

15

In certain embodiments, the electrodes according to the present invention are non-detachably attached to the electronic and/or a non-electronic device.

20 In some embodiments according to the present invention, at least one electrode is a non-disposable and/or reusable electrode or intended to be used several times without being removed from a surface it has been attached to in the time between two measurements (taking place on different days).

25

In certain embodiments according to the present invention, a first electrode and a second electrode are integrated or arranged having a distance between them which is particularly in the range of 2.5 to 15 cm, and more particularly in a range
30 of 4 to 7.5 cm.

In some embodiments, the electrodes according to the present invention have at least one connection element intended and/or configured to connect at least one electrode to at least one

bioelectrical impedance analyzer or to at least one body composition monitor or both.

In certain embodiments according to the present invention, a
5 first electrode and a second electrode are arranged on different surfaces of the electronic or non-electronic device.

In some embodiments according to the present invention, these surfaces are the front side and rear side, in others these
10 surfaces are the left and the right side, the upper and the bottom side or any combination of two arbitrary sides mentioned herein.

In certain embodiments, the device according to the present
15 invention is selected from a group consisting of organizers of a continuous ambulatory peritoneal dialysis system, automated peritoneal dialysis devices, automated peritoneal dialysis-cyclers, dialysis machines, and hand-held electrodes holders.

20 In some embodiments according to the present invention, the device is or comprises a bioelectrical impedance analyzer or body composition monitor or both or is - in a wireless or a non-wireless manner - connected thereto.

25 In certain embodiments according to the present invention, the device is configured or arranged, e.g., by means of a corresponding device, to start measuring the bioelectrical impedance and/or the body composition measurements automatically upon touching one, at least one, two, three,
30 four or more of the electrodes by the patient. To this end, in particular embodiments according the present invention sensors are provided which detect the presence of the fingers or other body sections of the patient on the device. The presence may be detected by resistance, skin resistance, skin temperature,
35 pressure or the like. The presence may also be detected by

contact buttons which close an electrical circuit once they are touched or pressed by the patient.

5 In some embodiments according to the present invention, the device comprises a button or switch or element that has to be pushed, switched, inserted, attached or otherwise activated or operated before a bioelectrical impedance and/or body composition measurement may be started at all. The activation or operation of the button, switch or element may be a pre-
10 condition necessary to bring the device into a mode in which the measurement can be started (whereas the measurement cannot be started before this mode has been selected). Of course, it may be provided that for starting the measurement it may not be sufficient that the system has entered into above mentioned
15 modus; additionally some action from the patient may be required such as touching some sensors as described above, or the like.

In certain embodiments according to the present invention, for
20 starting the bioelectrical impedance and/or body composition measurement a disc with a dial or another element such as a connector, for example a so-called stay safe connector (which may be a part or a disc of a so-called stay safe (organizer) which is commercially distributed by Fresenius Medical Care,
25 Germany), has to be inserted into or connected with the device according to the present invention. The connector, disc or element may have the function of a key such that a measurement cannot be started before the 'key' is connected with the device. The connector, disc or element may be required to
30 start a treatment in which the device according to the present invention is used.

In some embodiments according to the present invention, it may be provided that it is not sufficient to have the connector,
35 the disc or another element inserted into or connected with

the device. In these embodiments according to the present invention, it might be requested that the connector, the disc or the element has to be brought into a particular position on the device before measuring the bioelectrical impedance and/or body composition is enabled. For example, the disc might have to be rotated into a pre-set position or the element, if embodied as a switch, might have to be switched in a predetermined manner. In certain embodiments according to the present invention, a device for checking whether the connector, the disc or the element is in the pre-set position or not is provided. For example, the disc may have to be connected with the device and be turned into a pre-determined position before the patient is allowed to measure his bioelectrical impedance and/or body composition.

In certain embodiments according to the present invention, an element of the device such as a switch for selecting between two or more operating states or modes of the device may be provided. Based on the operating state that is presently selected by means of the switch a measurement may be allowed or blocked. In some embodiments according to the present invention, a sensor is provided for detecting in which operating state or modus the device is.

Since the results achieved by a bioelectrical impedance and/or body composition measurement may depend on circumstances such as a stage of a simultaneously conducted dialysis treatment, and since measurements conducted during some stages of the treatment might result in different findings compared to the measurements conducted during other stages of the same treatment session, in some embodiments of the present invention the patient is given an acoustical, optical or any other hint indicating that a bioelectrical impedance and/or body composition should or should not be carried out right now, or the like. For example, the patient might be informed

by a tone or any other signal that he should start his measurement now. Such a signal might be given, e. g., right before his peritoneum is going to be filled or emptied or while the peritoneum is emptied. The signal might be sent
5 based on the operating state of the device or the treatment device as detected by a suitable sensor.

In some embodiments according to the present invention, the device comprises another device for sending a measurement
10 result to a dialysis machine, to a medical monitoring centre, the doctor in charge, to a clinic, to a hospital, to a dialysis centre, and/or the like.

In certain embodiments according to the present invention, the
15 measurement results are sent or signalled in a wireless manner.

In some embodiments according to the present invention, the device comprises another device for sending a warning signal
20 (a text message, for example, or any other signal) to a medical monitoring centre, the doctor in charge, to a clinic, to a hospital, to a dialysis centre, and/or the like, once the measurement results have exceeded an upper or lower threshold. This allows an easy determination for the remote working
25 recipient to assess if or when the patient should be seen by a doctor or by medical staff in general.

In particular embodiments according to the present invention, the dialysis apparatus is an apparatus for peritoneal
30 dialysis, hemodialysis, hemofiltration, and/or hemodiafiltration or for any other dialysis treatment as set forth above.

In certain embodiments according to the present invention, the
35 dialysis apparatus comprises a control unit, the control unit

being configured to control - with or without feedback control - the dialysis treatment based on the signal representing the results of the measurement carried out by means of the electrodes.

5

In some embodiments of the method according to the present invention, the at least two body portions for touching the at least two electrodes according to the present invention are two fingers of one hand, or at least two fingers of different
10 hands, or two fingers of each hand, or any part of a hand and any part of a foot, or any part of both feet, or another two separate parts of the body.

In certain embodiments, the method according to the present
15 invention encompasses manually inputting information into the bioelectrical impedance analyzer and/or to the body composition monitor about the patient's parameters as for example height, weight, age, sex and/or with what part of the patient's body the electrodes have been touched.

20

In some embodiments, the method according to the present invention additionally comprises adjusting the treatment parameters of a dialysis treatment to the results of the bioelectrical impedance analysis.

25

In certain embodiments, the method according to the present invention comprises starting the bioelectrical impedance measurement solely by touching at least one electrode, two electrodes or two pairs of electrodes.

30

In some embodiments, the method according to the present invention comprises adjusting or controlling the dialysis treatment in an automatic manner based on a measurement result achieved by the method according to the present invention.

35

In certain embodiments, the method according to the present invention comprises filtering of the measurement results and in particular of the measured body resistance or any other mathematical scatter or noise reduction. This may enhance the accuracy of the input data used for a subsequent determination of the overhydration (herein also referred to as the overhydration state) or used for a body composition calculation, and for giving the patient a more precise feedback on his status.

The filtering or mathematical scatter or noise reduction may encompass the use of a Kalman filter, a mean, an average, or the like and combination thereof.

In certain embodiments, the method according to the present invention comprises obtaining first bioimpedance measurement data of a patient from a first type of bioimpedance measurement, deriving bioimpedance calibration data from the first bioimpedance measurement data for calibrating second bioimpedance measurement data from a second type of bioimpedance measurement, obtaining the second bioimpedance measurement data from a second bioimpedance measurement of the patient, and calibrating the second bioimpedance measurement data using the calibration data to determine the overhydration parameter or the body composition parameter of the patient.

In some embodiments according to the present invention the step of obtaining first bioimpedance measurement data comprises performing a first bioimpedance measurement.

In certain embodiments, the method according to the present invention the step of performing a first bioimpedance measurement comprises measuring a bioimpedance spectrum of the patient at one frequency or at multiple frequencies.

In some embodiments, the method according to the present invention comprises receiving bioimpedance calibration data derived from first bioimpedance measurement data obtained by a first type of bioimpedance measurement, the bioimpedance calibration data being suitable for calibrating second bioimpedance measurement data from a second type of bioimpedance measurement, obtaining the second bioimpedance measurement data from a second bioimpedance measurement of the patient and calibrating the second bioimpedance measurement data using the calibration data to determine the overhydration parameter or the body composition parameter of the patient.

In certain embodiments, the method according to the present invention the step of obtaining the second bioimpedance measurement data comprises performing a second bioimpedance measurement.

In certain embodiments, the method according to the present invention the step of performing a second bioimpedance measurement comprises measuring a bioimpedance of the patient at a single frequency.

In certain embodiments, the method according to the present invention comprises obtaining a plurality of bioimpedance measurements of the second type at different times to generate a time series of bioimpedance measurements, performing time analysis of the time series to determine whether a current bioimpedance measurement of the time series deviates significantly from previous bioimpedance measurements of the time series, and generating an indication that a new measurement of the first type of bioimpedance measurements should be performed or a warning message.

In certain embodiments, the method according to the present invention the step of deriving the calibration data comprises

using bioimpedance reference data correlating bioimpedance measurement results of the first type and bioimpedance measurement results of the second type.

5 In certain embodiments, the method according to the present invention comprises a step of deriving the reference data, wherein the first type of bioimpedance measurements comprises a first type of electrode configuration, wherein the second type of bioimpedance measurements comprises a second type of
10 electrode configuration, and wherein the step of deriving the reference data comprises applying a conversion factor between a first format considering a measurement using the first type of electrode configuration and a second format considering a measurement using the second type of electrode configuration.

15

In some embodiments, the method according to the present invention comprises obtaining the first bioimpedance measurement data, deriving the bioimpedance calibration data from the first bioimpedance measurement data, providing the
20 bioimpedance calibration data to a device for determining the overhydration parameter or the body composition parameter.

In some embodiments, the method according to the present invention comprises performing a plurality of bioimpedance
25 reference measurements, each comprising a first reference measurement of the first type of bioimpedance measurement and a second reference measurement of the second type of bioimpedance reference measurement and correlating data from the first and the second reference measurements to obtain the
30 bioimpedance reference data.

The devices, apparatuses and machines according to the present invention comprise in particular embodiments of the present invention devices, monitors and the like which are adapted

and/or configured for carrying out at least one or all of the steps described in here.

For example, the device or the dialysis apparatus according to the present invention comprises in some embodiments a data provisioning unit for obtaining first bioimpedance measurement data of a patient from a first type of bioimpedance measurement, a processing unit for deriving bioimpedance calibration data from the first bioimpedance measurement data for calibrating second bioimpedance measurement data from a second type of bioimpedance measurement, a data obtaining unit for obtaining the second bioimpedance measurement data from a second bioimpedance measurement of the patient, and a calibration unit for calibrating the second bioimpedance measurement data using the calibration data to determine the overhydration parameter or the body composition parameter of the patient.

In certain embodiments of the present invention, the device or the dialysis apparatus according to the present invention or both comprise a measurement unit for performing a bioimpedance measurement for obtaining the first bioimpedance measurement data.

In certain embodiments of the present invention, the measurement unit is adapted to measure the bioimpedance spectrum of the patient at multiple frequencies.

The device or the dialysis apparatus according to the present invention comprises in some embodiments a receiving unit for receiving bioimpedance calibration data derived from first bioimpedance measurement data obtained by a first type of bioimpedance measurement, the bioimpedance calibration data being suitable for calibrating second bioimpedance measurement data from a second type of bioimpedance measurement, a data

obtaining unit for obtaining the second bioimpedance measurement data from a second bioimpedance measurement, of the patient, and a calibration unit for calibrating the second bioimpedance measurement data using the calibration data to
5 determine the overhydration parameter or the body composition parameter of the patient.

In certain embodiments of the present invention, the device or the dialysis apparatus according to the present invention
10 comprises a measurement unit for performing a bioimpedance measurement for obtaining the second bioimpedance measurement data.

In some embodiments of the present invention, the measurement
15 unit is adapted to measure the bioimpedance of the patient at a single frequency.

In certain embodiments according to the present invention the expressions 'bio-impedance analyzer', 'bioelectrical impedance analyzer', 'bio-impedance measuring device' and 'bio-impedance
20 analysis', or 'bioelectrical impedance analysis' relate to bio-impedance measuring devices or bioelectrical impedance analysis methods that are known in the art. In some embodiments according to the present invention, such devices
25 use the 50 kHz current frequency vector and/or the multifrequency bio-impedance measurement or spectroscopy.

In some embodiments according to the present invention, the bio-impedance measuring device is a monitor as described in
30 WO 2006/002685 A1. The respective disclosure of WO 2006/002685 A1 is hereby incorporated in the present application by way of reference. Of course, the present invention must not be understood to be limited to monitors obtaining data by bio-impedance measurements as is described
35 in WO 2006/002685 A1. Other bio-impedance measurement methods

known in the art and also any other devices known in the art are also contemplated and encompassed by the present invention.

5 In certain embodiments according to the present invention, the bio-impedance measuring device is configured to measure the extracellular fluid volume over total body water (ECV/TBW) ratio, extracellular fluid volume over body mass (ECV/BM), and/or extracellular over intracellular volume (ECV/ICV).

10

In some embodiments according to the present invention, the device according to the present invention and/or the dialysis apparatus according to the present invention comprise a device for signalling or sending the measurement results achieved by means of the method according to the present invention to an electronic medical card of the patient comprising personal and/or treatment data of the patient for saving or storing the measurement results for a later use thereof.

20 The present invention also relates to devices, apparatuses, and the like, which are adapted, configured, arranged, programmed or the like to carry out each of the methods according to the present invention or single steps thereof.

25 Any embodiment according to the present invention may have one or more of the above or in the following mentioned advantages in any combination.

Since the electrodes intended for measuring the body's resistance at one or more frequencies or for measuring the bio-impedance of a patient's body by a bio-impedance measuring device are suggested herein to be integral with or permanently attached to at least one device of the above mentioned group according to the present invention, the patient does not need help in placing the electrodes on his limbs. Rather, it is

35

quite easy to handle and use the electrodes and the devices according to the present invention. Therefore, the patient is capable of measuring his body fluid content whenever and as frequently as he wishes to. This is believed to increase the patient's compliance regarding using the device for measuring on a frequent basis. This may obviously result in higher quality treatment.

Also, since the patient does not have to place the electrodes anywhere on his limbs but has only to put his fingers or other parts of the body onto electrodes that are both attached to a device and determined to be used in a particular way, the patient cannot fail to use the electrodes in the only correct manner. This obviously results in higher quality measurements. Besides, the measurements carried out are performed in a reproducible way. The results achieved can be compared to results gained earlier in a more reliable manner.

Further, since the electrodes according to the present invention are intended to be used more often than only once - in contrast to disposable electrodes known from the prior art - and since they may be reusable, waste material does not have to be disposed of after every single measurement. This implies the advantages well-known to the skilled person.

The electrodes according to the present invention may have a shape that only allows their use by pre-defined parts of the body, e. g. the fingers. Hence, the accuracy of the measurements carried out by means of those electrodes may be enhanced as their shape does not allow for contact with other body parts, e.g., the foot if this was not intended by the manufacturer.

Also, if at least some electrodes according to the present invention are arranged on different surfaces of the electronic

or non-electronic device of the above mentioned group, for example both on the front side and on the rear side, an incorrect use of the electrodes is further ruled out. Again this may lead to better measurement results.

5

In certain embodiments of the present invention, the devices comprise a device for signalling or sending the measurement results to a medical monitoring centre, to the doctor in charge, to a clinic, to a hospital, to a dialysis centre, and/or the like. Any of those recipients - such as the medical monitoring centre - can check for plausibility of the results, developments of the body fluid content and the like and contact and inform the patient if necessary to prevent harm.

10

15

If, as is also contemplated by embodiments of the present invention, the devices according to the present invention comprise a device for signalling or sending the measurement results to a dialysis apparatus, the device or the dialysis apparatus can check for plausibility of the results, developments of the body fluid content and the like and adapt or amend automatically the treatment or certain parameters thereof or suggest to do so to the patient or the doctor if necessary to prevent harm or to improve the treatment outcome or both by controlling the dialysis apparatus effectively.

20

25

Many characteristics of the patient such as for example age, sex, weight, height and some other conditions such as changing sodium and water intake, position of the body, position of the electrodes during measurement and the like can have some effect on the measurement results. Hence, the accuracy of the bio-impedance measurement can be further improved if the bioelectrical impedance analyzer or body composition monitor comprises an input element for manually inputting at least some (or all) of the above mentioned conditions to the bio-

30

impedance device or the body composition monitor, be it by the patient himself or by the medical staff.

5 If certain signals as related to herein are transmitted in a wireless manner, all advantages known to the skilled person can be achieved.

10 If the bio-impedance measuring device starts automatically measuring once the patient has placed, for example, his fingers on the electrodes, operating a switch for starting the measurement is no longer required. This can render the operation of the devices involved in the measurements less cumbersome. The patient may receive a signal, an alarm or the like once the measurement is finished, or not.

15

The electrodes according to the present invention can be advantageously used to upgrade conventional devices of the above mentioned group of electronic and/or non-electronic devices used in the preparation of a dialysis treatment or during dialysis, in particular by means of sticking or gluing them to said devices. For example, this can happen by using a pad comprising the electrodes. This way it is easy and also economical to achieve the advantages discussed above while maintaining existing devices that are already in operation.

25

If for starting the bioelectrical impedance and/or body composition measurement a disc with a dial or another element has to be inserted into or connected with the device according to the present invention, the patient would notice that he has forgotten to insert or connect the disc or the element since he would not be able to carry out measurements. This way, the risk of overlooking to insert or connect elements that have to be inserted or connected for a proper function of, e. g., the blood treatment apparatus or the extracorporeal blood circuit is reduced.

35

In the following, the present invention will be exemplarily specified with reference to the appended drawing. In the drawing, identical reference numerals designate same or
5 identical elements, wherein:

Fig. 1 shows a top view of an organizer according to the present invention having two electrodes on its upper side;

10 Fig. 2 shows a perspective view of an ADP-cycler according to the present invention having four electrodes;

15 Fig. 3 shows a top view of a hand-held electrodes holder according to the present invention;

Fig. 4 shows a bottom view of the hand-held electrodes holder of Fig. 3; and

20 Fig. 5 shows schematically a perspective view of an organizer according to the present invention on a stand.

Fig. 1 schematically shows a top view of an organizer 20 in accordance with a first embodiment of the present invention having four electrodes 10. Below the organizer 20, Fig. 1 schematically shows a conventional bio-impedance measuring device 30.

30 Two of said electrodes 10 are placed on the top side 21 of the organizer 20, lateral to the disk having a dial 22 (the dial 22 also being called a stay safe connector herein). Two other electrodes 10 are placed on the bottom side 23 of the organizer 20 and shown by dotted lines in Fig. 1. This way,
35 the organizer 20 comprises a first pair of electrodes 10 (left

from the dial 22) and a second pair of electrodes 10 (right from the dial 22).

In order to check his body composition or bioelectrical
5 impedance, the patient has to place his thumbs on the two
electrodes 10 of the top side 21 and his forefingers on the
two electrodes 10 of the bottom side 23 of the organizer 20
for a bio-impedance measurement. The electrodes 10 are placed
in such a manner that the patient can hold the organizer 20
10 with two hands and can reach every electrode 10 with the
corresponding finger without effort. The position of the
particular finger on the electrode is pre-determined by the
form, configuration, position and/or shape of the
electrode 10. This pre-determination makes the measurement
15 reliable and reproducible.

In the embodiment according to the present invention shown in
Fig. 1, the organizer 20 is connected to the bio-impedance
measuring device 30 and/or a body composition monitor by means
20 of a connecting element 24 connected to or plugged into a
terminal or notch 25 of the organizer 20. In alternative
embodiments according to the present invention, a wireless
connection is provided instead of the connecting element 24
shown in Fig. 1. By means of wireless connection, the patient
25 is less hampered by electric wires.

In some embodiments according to the present invention like
the one shown in Fig. 1, the bio-impedance measuring device 30
is turned on or starts measuring automatically by touching the
30 four electrodes 10 with the fingers.

The result of the measurement can be displayed on the
display 31 of the bio-impedance measuring device 30. The bio-
impedance measuring device 30 can include an alarm modus to
35 alert the patient if the results of measurements are below or

above pre-determined target values or if the results do not make sense. The alarm signal or alert can reach only the patient, with a sound or a message on the display of the bio-impedance measuring device 30, or it can reach a medical monitoring centre. The same applies to the measurement results. They can also be transferred to the medical monitoring centre. In addition or as an alternative, the measurement results can be sent to the dialysis device. In particular embodiments, the measurement results sent to the dialysis device can be used to automatically control the treatment.

The bio-impedance measuring device 30 below the organizer 20 can be replaced for a body composition monitor.

15

Fig. 2 shows a perspective view of a conventional ADP-cycler 40 (automated peritoneal dialysis-cycler) according to the present invention having four electrodes 10 according to the present invention on its surfaces, the electrodes 10 being integral or attached to the ADP-cycler 40.

20

Two of the electrodes 10 are placed on the upper surface or upper part 41 of the ADP-cycler and another two on both lateral surfaces or lateral parts 42 (one of them being indicated by dotted lines), so that a patient can effortlessly reach the electrodes 10 of the upper part 41 of the device with his thumbs and the electrodes 10 of the lateral parts 42 with his forefingers or with his middle fingers.

25

Upon touching of the electrodes 10 or upon activating a switch or the like the measurement automatically takes place. The results of the measurement can be displayed on a display 43.

30

In this embodiment of the present invention the bio-impedance measuring device 30 is integrated into the ADP-cycler 40.

35

In other embodiments according to the present invention, the bio-impedance measuring device 30 is different from or non-integral with the ADP-cycler 40. It may be connected to the
5 ADP-cycler 40 by a connecting element 44.

A conventional ADP-cycler 40 can be upgraded or interlinked by means of wires or wireless with a separate bio-impedance measuring device 30 by attaching four electrodes 10 according
10 to the present invention to the casing, housing or the like of the ADP-cycler 40.

Fig. 3 shows a top view of a hand-held electrodes holder 50 according to the present invention. The representation of
15 Fig. 3 shows two electrodes 10 for the thumbs of the patient. The embodiment of the hand-held electrodes holder 50 shown in Fig. 3 is quite simple. Simply spoken, it may be a casing 51 comprising the electrodes 10 on its surfaces.

20 The hand-held electrodes holder 50 may have terminals or sockets 52 for connecting the hand-held electrodes holder 50 to another apparatus, e.g., for connecting the electrodes 10 to a bio-impedance measuring device 30 by means of connecting elements not shown. In further embodiments according to the
25 present invention, the connection is wireless. More sophisticated embodiments according to the present invention include an input element 53 for inputting patient-related information that can be helpful to achieve a more accurate measurement result such as, for example, height, sex, age,
30 etc.

The hand-held electrodes holder 50 includes in certain embodiments according to the present invention a bio-impedance measuring device 30, too. In this case the patient may not

need any device except for the hand-held electrodes holder 50 to perform a complete bio-impedance analysis.

The hand-held electrodes holder 50 according to the present
5 invention may comprise a display 54.

Fig. 4 shows a bottom view of the hand-held electrodes holder 50 of Fig. 3. In Fig. 4, the two electrodes 10 for the forefingers or the middle fingers of the patient are shown.

10

Fig. 5 shows an example of an organizer 20, which is held on a moveable stand 60. The organizer 20 has four electrodes 10 positioned like in Fig. 2. The electrodes 10 are placed on the surface of the organizer 20 and are connected to a bio-
15 impedance measuring device 30, which constitutes a separate unit from the organizer 20 and has been placed below it. The connection can be wireless.

The bio-impedance measuring device 30 can be embodied as in
20 every other embodiment or configuration as shown by the figures or as described above.

The entire disclosure of the priority documents EP 12002955 and US 61/638,514 is herewith incorporated into the present
25 application by reference.

Reference numerals list

| | | |
|----|----|---|
| | 10 | electrodes |
| 5 | 20 | organizer |
| | 21 | top side of the organizer |
| | 22 | disk with dial |
| | 23 | bottom side of the organizer |
| | 24 | connecting element |
| 10 | 25 | terminal or notch |
| | 30 | bio-impedance measuring device |
| | 31 | display of the bio-impedance measuring device |
| | 32 | alarm modus button |
| | 40 | ADP-cycler |
| 15 | 41 | upper part of the ADP-cycler |
| | 42 | lateral parts of the ADP-cycler |
| | 43 | display of the ADP-cycler |
| | 44 | connecting element of the ADP-cycler |
| | 50 | hand-held electrodes holder |
| 20 | 51 | casing |
| | 52 | connecting element of the hand-held electrodes holder |
| | 53 | input element |
| | 54 | display of the hand-held electrodes holder |
| | 60 | stand |
| 25 | | |

Claims

1. Electrodes (10) for a bio-impedance measuring device (30)
or a body composition monitor, the electrodes (10) being
5 integral with or being attached to a surface of at least
one device belonging to a group of electronic and/or non-
electronic devices used in the preparation of a dialysis
treatment or during dialysis, in particular during
peritoneal dialysis, the group preferably consisting of
10 organizers (20) of a continuous ambulatory peritoneal
dialysis system (CAPD), automated peritoneal dialysis
devices, automated peritoneal dialysis-cyclers (APD-
Cycler) (40), bioelectrical impedance analyzers (BIA) (30),
body composition monitors (BCM), hand-held electrodes
15 holders (50) for the electrodes, and dialysis apparatuses.
2. Electrodes (10) according to claim 1, wherein the
electrodes (10) are detachably attached to the electronic
and/or a non-electronic device.
20
3. Electrodes (10) according to claim 1, wherein the
electrodes (10) are non-detachably attached to the
electronic and/or a non-electronic device.
- 25 4. Electrodes (10) according to any one of the claims 1 to 3,
wherein at least one electrode (10) is a non-disposable
and/or reusable electrode.
5. Electrodes (10) according to any one of the preceding
30 claims, wherein a first electrode (10) and a second
electrode (10) are integrated or arranged having a distance
between them, which is particularly in the range of 2.5 to
15cm, and more particularly in a range of 4 to 7.5cm.

6. Electrodes (10) according to any one of the preceding claims, wherein the electrodes (10) have at least one connection element (24) to connect at least one electrode (10) to at least one bioelectrical impedance analyzer (30) or/and at least one body composition monitor.
7. Electrodes (10) according to any one of the preceding claims, wherein a first electrode (10) and a second electrode (10) are arranged on different surfaces of the electronic or non-electronic device.
8. Device for use during dialysis or while preparing a dialysis treatment or being intended to be used during dialysis or while preparing a dialysis treatment, in particular peritoneal dialysis, comprising at least one integrated and/or attached electrode (10) according to any one of the preceding claims.
9. Device according to claim 8, the device being selected from the group consisting of organizers (20) of a continuous ambulatory peritoneal dialysis system, automated peritoneal dialysis devices, automated peritoneal dialysis-cyclers (40), hand-held electrodes holders (50), and dialysis machines.
10. Device according to claim 8 or claim 9, the device being or comprising a bioelectrical impedance analyzer (30), a body composition monitor or both, or being connected thereto.
11. Device according to claim 10, wherein the device is configured to start measuring the bioelectrical impedance or the body composition measurements or both upon touching at least one of the electrodes.

12. Device according to claim 10, wherein the device is configured to start measuring or to allow measuring the bioelectrical impedance or the body composition measurements, or both, upon or by inserting a dial or another element such as a connector, in particular a stay safe connector, into the device.

13. Device according to any of claims 8 to 12, wherein the device comprises a device for sending a measurement result to a dialysis apparatus, to a medical monitoring centre, to a medical card of the patient, or to at least two of the aforementioned recipients.

14. Dialysis apparatus, the dialysis apparatus comprising at least one of the electrodes (10) according to any one of claims 1 to 7, or the device of claims 8 to 13, or both, or being in signal communication therewith to receive results of measurement carried out by means of the electrodes.

15. Dialysis apparatus according to claim 14, the dialysis apparatus comprising a control unit, the control unit being configured to control the dialysis treatment based on the signal representing the results of measurement carried out by means of the electrodes.

16. Method for determining parameters for estimating the hydration or the nutritional status of a dialysis patient comprising the steps:

- touching at least two electrodes (10) according to any one of the claims 1 to 7 with at least two body portions, the electrodes (10) being connected to a bioelectrical impedance analyzer (30) or a body composition monitor or both; and

- collecting and processing information received from the electrodes (10) in a processing element of a bioelectrical impedance analyzer (30) or a body composition monitor or both.

5

17. Method according to claim 16, comprising the step:

- adjusting the treatment parameters of a dialysis treatment to the results of a bioelectrical impedance analysis carried out by the bioelectrical impedance analyzer (30) or the body composition monitor or both.

10

18. Method according to any of claims 16 to 17, comprising the step:

15

- starting the bioelectrical impedance measurement by touching of at least one electrode (10).

20

19. Method according to any of claims 16 to 18, comprising the step:

- adjusting or controlling the dialysis treatment in an automatic manner based on a measurement result achieved by the method of the method of claims 16 to 18.

25

20. Non-transitory computer-readable medium with an executable program stored thereon, wherein the program instructs a programmable computer system to perform the steps of any of the methods according to any of claims 16 to 19.

30

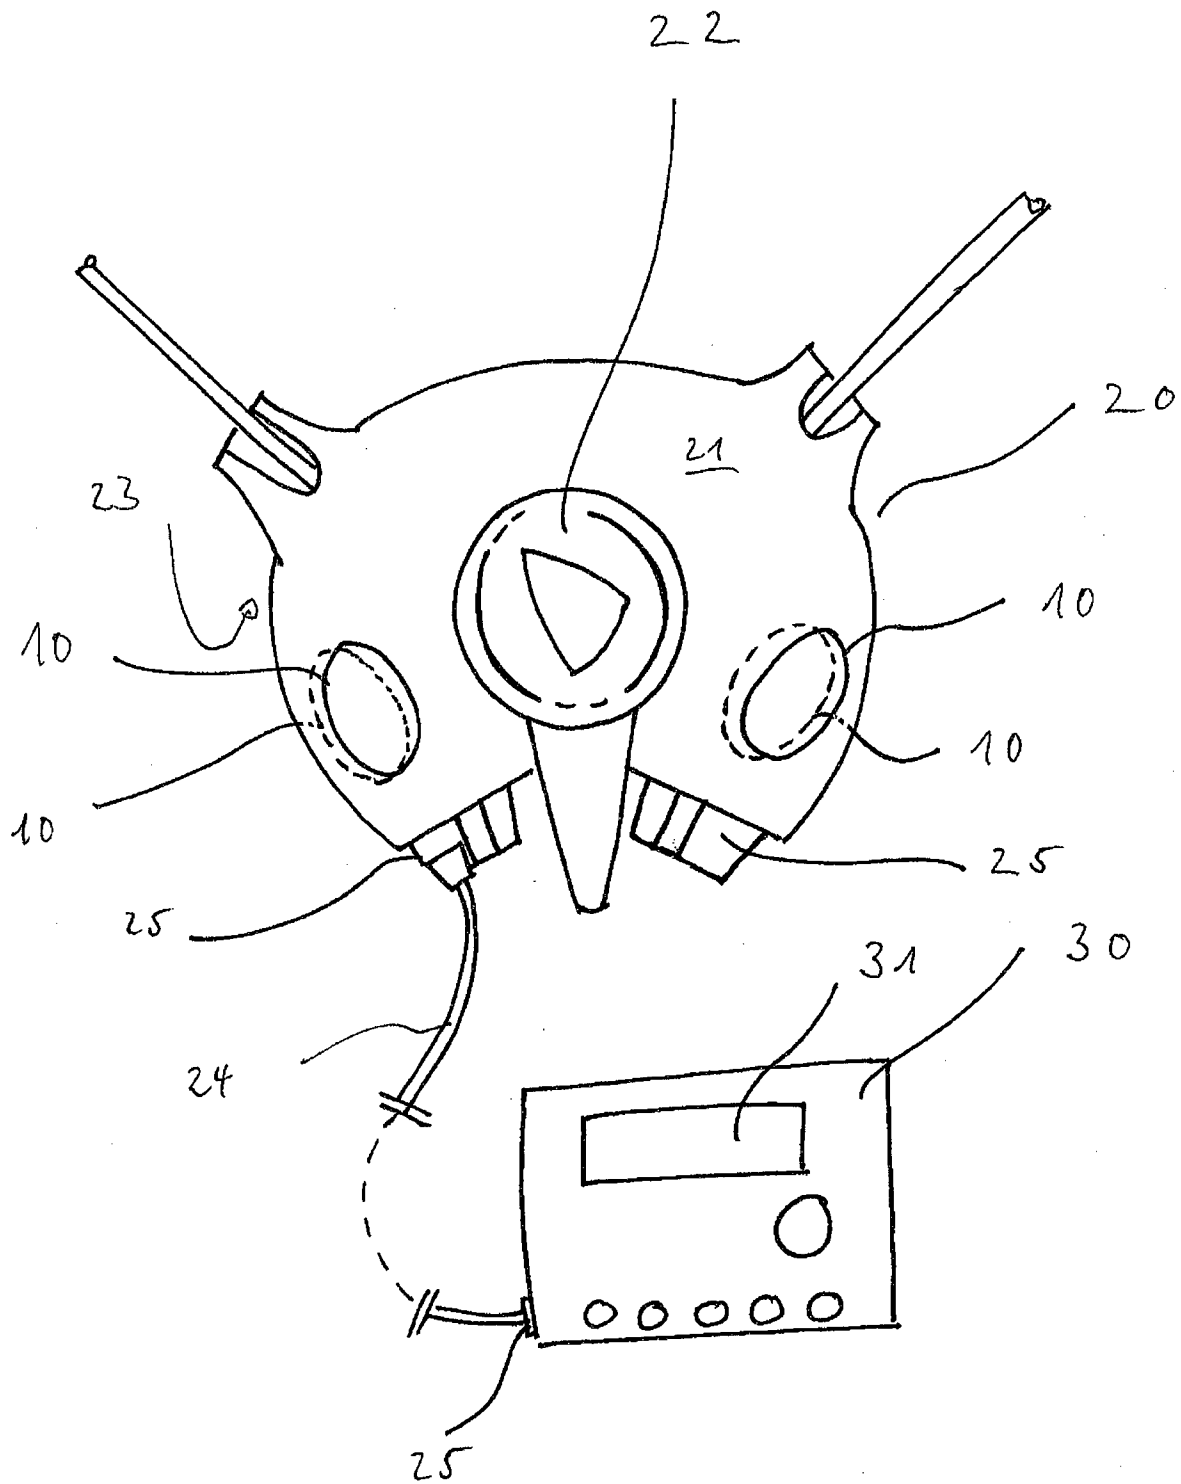


Fig. 1

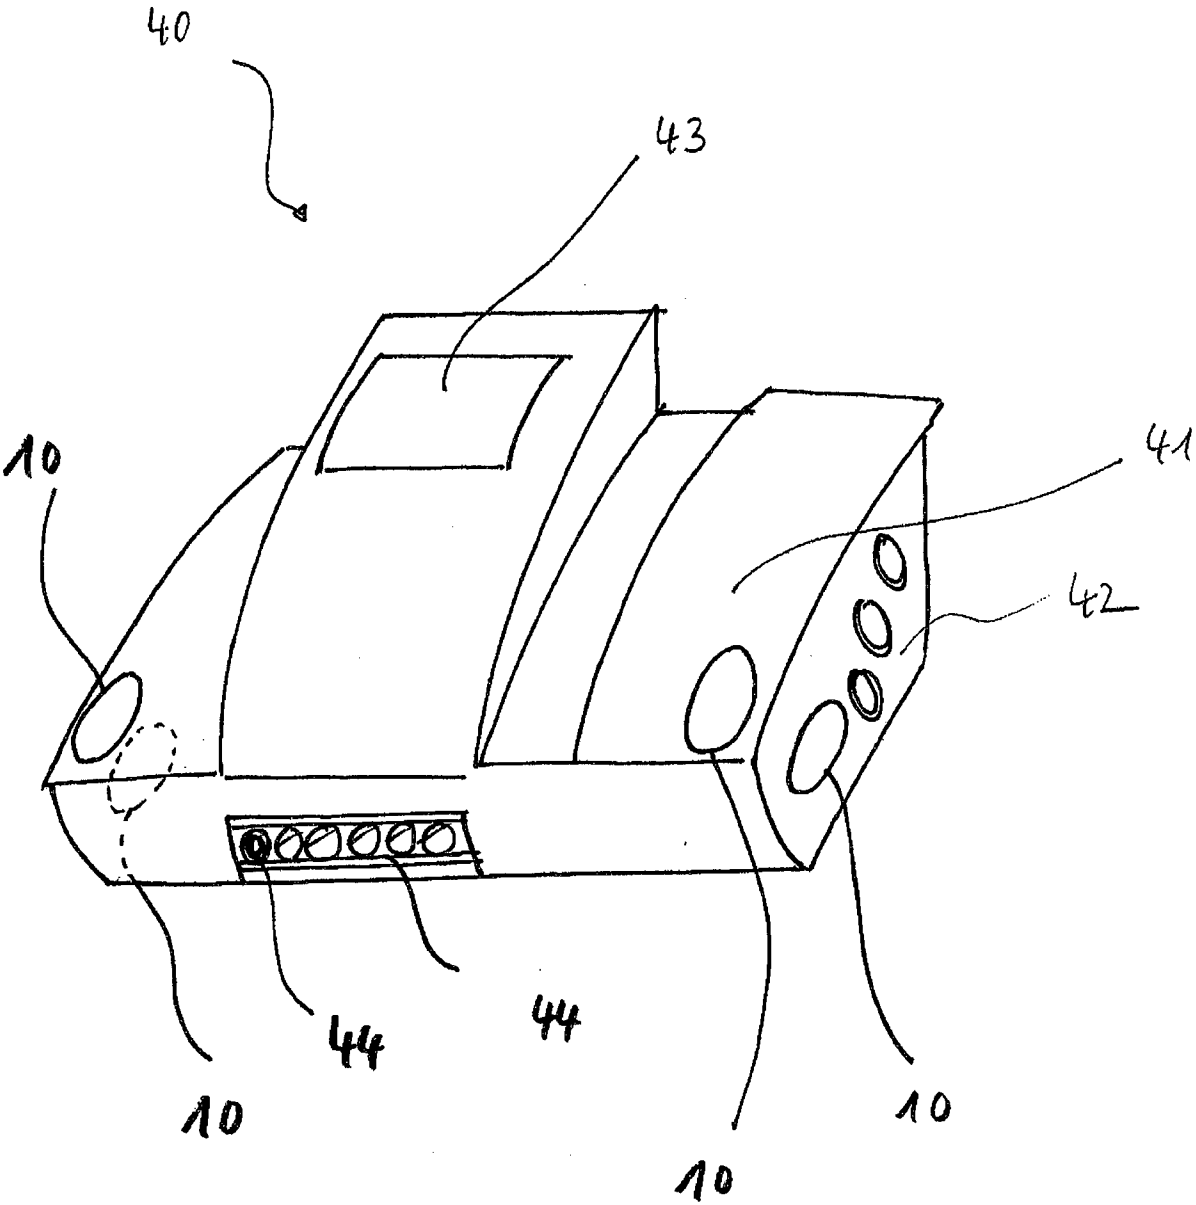


Fig. 2

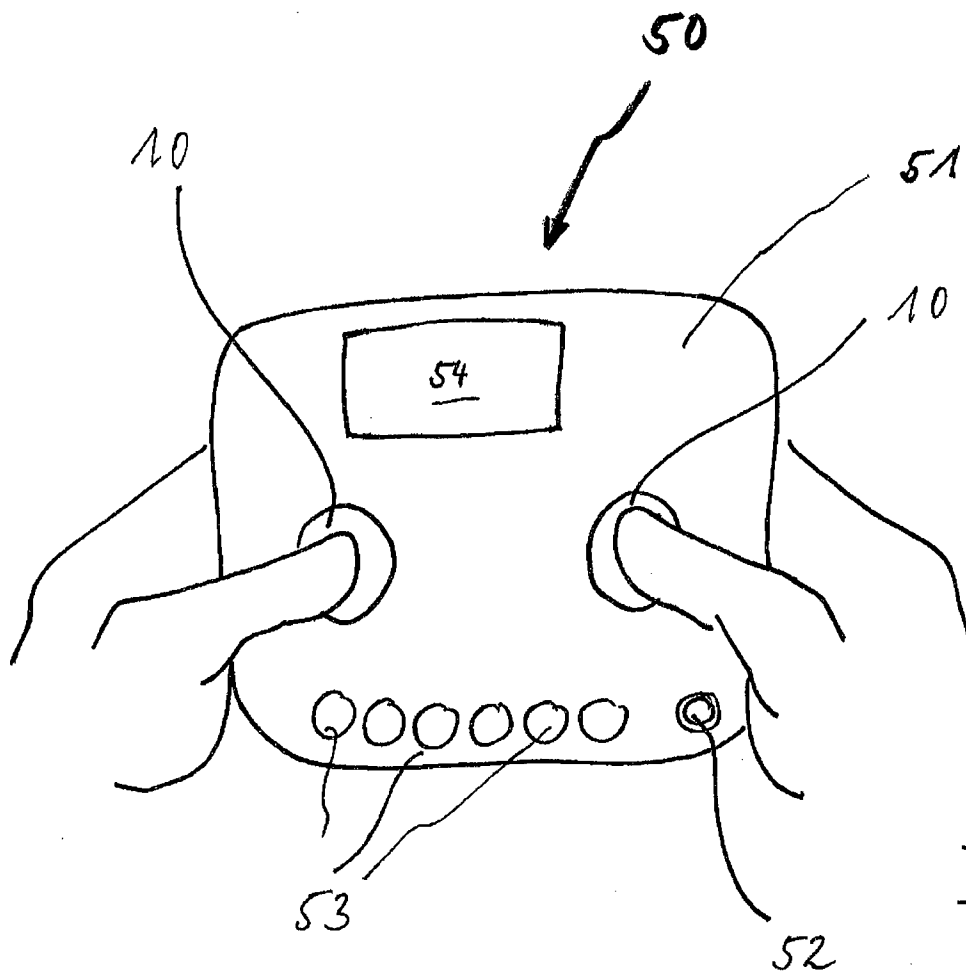


Fig. 3

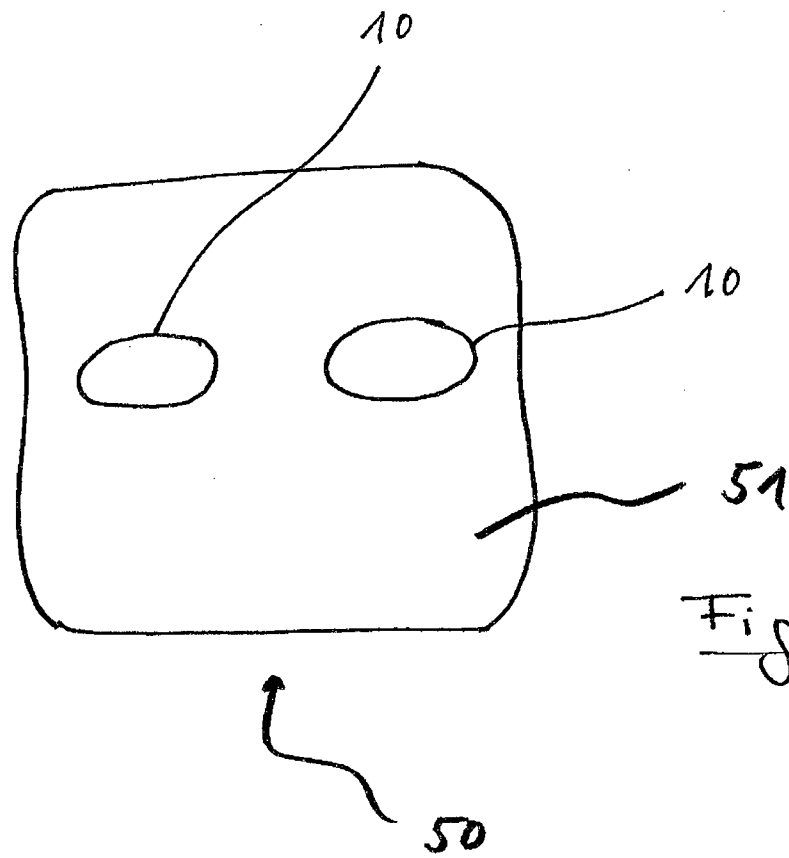


Fig. 4

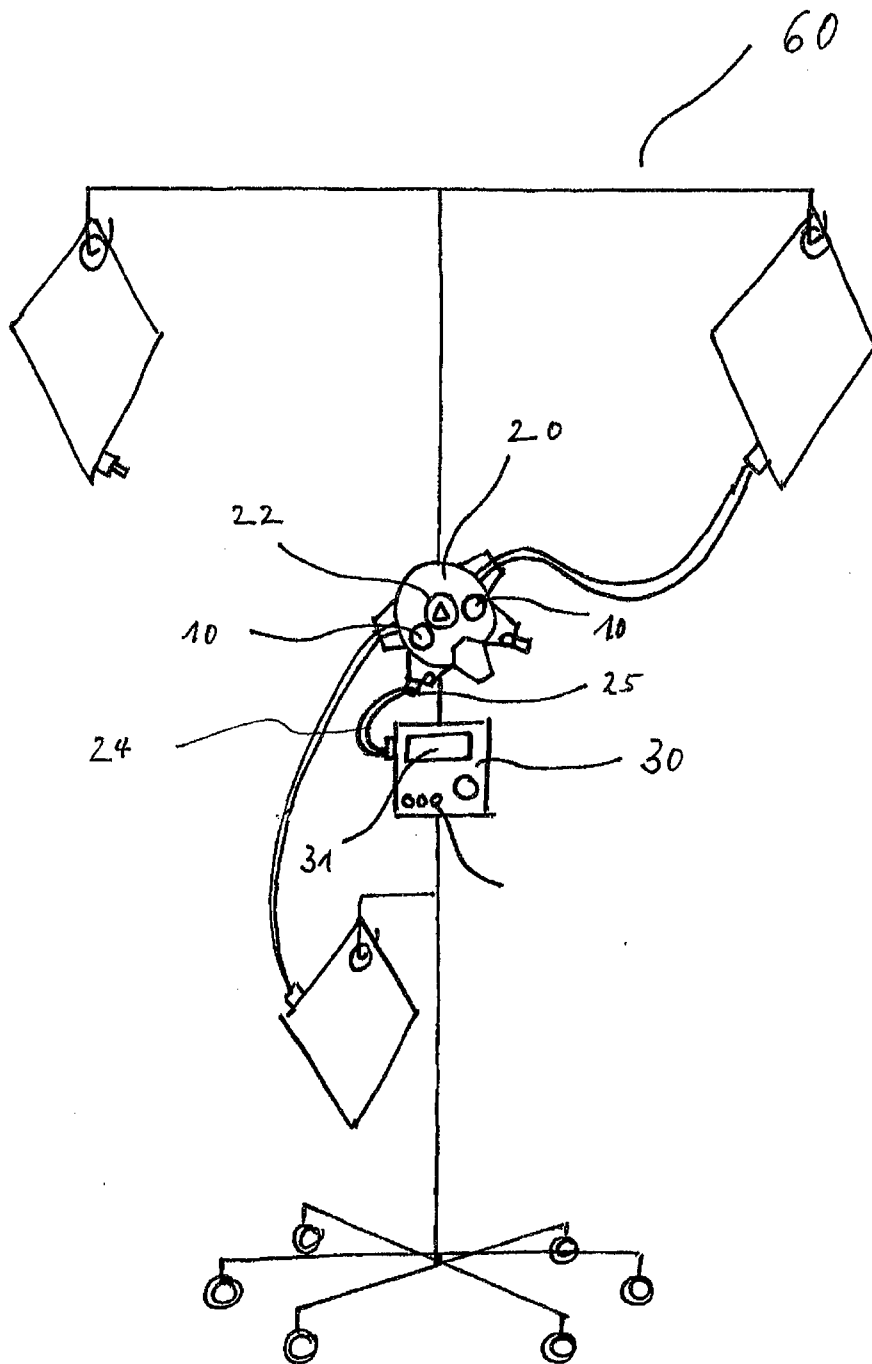


Fig. 5

INTERNATIONAL SEARCH REPORT

International application No

PCT/EP2013/001257

A. CLASSIFICATION OF SUBJECT MATTER

INV. A61B5/053 A61M1/14
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data, BIOSIS, COMPENDEX, EMBASE, INSPEC

C. DOCUMENTS CONSIDERED TO BE RELEVANT

| Category* | Citation of document, with indication, where appropriate, of the relevant passages | Relevant to claim No. |
|-----------|---|---------------------------------------|
| X | US 4 370 983 A (LICHTENSTEIN ERIC S [US]) 1 February 1983 (1983-02-01) column 3, line 64 - column 4, line 2 column 6, line 40 - line 60 column 16, line 40 - column 17, line 33 column 20, line 53 - column 21, line 62 figures 4-7A ----- | 1,3-5, 8-10, 13-17,19 |
| X | US 2012/035432 A1 (KATRA RODOLPHE [US] ET AL) 9 February 2012 (2012-02-09) | 1,2,5, 8-10,13, 16,17, 19,20 |
| Y | paragraph [0022] | 11,18 |
| A | paragraph [0026] - paragraph [0028] paragraph [0035] - paragraph [0040] paragraph [0043] - paragraph [0048] figures 1-7 ----- -/- | 15 |



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

29 July 2013

Date of mailing of the international search report

06/08/2013

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Görlach, Tobias

INTERNATIONAL SEARCH REPORT

International application No

PCT/EP2013/001257

| C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT | | |
|--|--|-------------------------------------|
| Category* | Citation of document, with indication, where appropriate, of the relevant passages | Relevant to claim No. |
| X | DE 10 2010 031530 A1 (FRESENIUS MEDICAL CARE DE GMBH [DE]) 19 January 2012 (2012-01-19) | 1,3-8, 10,12, 13,16, 17,19 |
| A | paragraph [0017] paragraph [0055] - paragraph [0061] figures 3,4 | 9,15 |
| X | ----- US 2005/070778 A1 (LACKEY ROBERT P [US] ET AL) 31 March 2005 (2005-03-31) paragraph [0006] paragraph [0026] - paragraph [0051] paragraph [0063] - paragraph [0067] paragraph [0079] - paragraph [0082] figures 1-6,10A-B | 1,5,8 |
| A | ----- WO 2009/036321 A1 (CORVENTIS INC [US]; LIBBUS IMAD [US]; AMURTHUR BADRI [US]) 19 March 2009 (2009-03-19) paragraph [0086] - paragraph [0092] figures 1A,1G-J | 2,5,6 |
| Y | ----- US 2009/182204 A1 (SEMLER HERBERT J [US] ET AL) 16 July 2009 (2009-07-16) | 11,18 |
| A | paragraph [0032] - paragraph [0033] paragraph [0073] - paragraph [0079] paragraph [0097] - paragraph [0139] paragraph [0142] - paragraph [0151] figures 4,8A-11C | 1-10, 12-17, 19,20 |
| | ----- | |

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/EP2013/001257

| Patent document cited in search report | Publication date | Patent family member(s) | Publication date |
|---|---------------------|-----------------------------|-------------------------------|
| US 4370983 | A | 01-02-1983 | DE 3068781 D1 06-09-1984 |
| | | EP 0027470 A1 29-04-1981 | |
| | | JP S56500993 A 23-07-1981 | |
| | | US 4370983 A 01-02-1983 | |
| | | US 4464172 A 07-08-1984 | |
| | | WO 8002376 A1 13-11-1980 | |
| ----- | | | |
| US 2012035432 | A1 | 09-02-2012 | NONE |
| ----- | | | |
| DE 102010031530 | A1 | 19-01-2012 | DE 102010031530 A1 19-01-2012 |
| | | EP 2595531 A1 29-05-2013 | |
| | | WO 2012010588 A1 26-01-2012 | |
| ----- | | | |
| US 2005070778 | A1 | 31-03-2005 | AU 2004266725 A1 03-03-2005 |
| | | CA 2539547 A1 03-03-2005 | |
| | | EP 1677674 A2 12-07-2006 | |
| | | EP 2382920 A1 02-11-2011 | |
| | | JP 2007502675 A 15-02-2007 | |
| | | JP 2012143574 A 02-08-2012 | |
| | | US 2005070778 A1 31-03-2005 | |
| | | US 2008039700 A1 14-02-2008 | |
| | | WO 2005018432 A2 03-03-2005 | |
| ----- | | | |
| WO 2009036321 | A1 | 19-03-2009 | EP 2195076 A1 16-06-2010 |
| | | US 2009076559 A1 19-03-2009 | |
| | | WO 2009036321 A1 19-03-2009 | |
| ----- | | | |
| US 2009182204 | A1 | 16-07-2009 | NONE |
| ----- | | | |