



US 20070167681A1

(19) **United States**(12) **Patent Application Publication****Gill et al.**(10) **Pub. No.: US 2007/0167681 A1**(43) **Pub. Date: Jul. 19, 2007**(54) **PORTABLE IMAGING SYSTEM
EMPLOYING A MINIATURE ENDOSCOPE**

No. 10/042,126, filed on Oct. 19, 2001, now Pat. No. 6,863,651.

(76) Inventors: **Thomas J. Gill**, Weston, MA (US);
James E. McDonald, Monson, MA (US)**Publication Classification**(51) **Int. Cl.****A61B 1/04** (2006.01)**A61B 1/00** (2006.01)(52) **U.S. Cl.** **600/112**; 600/131; 600/182;
600/179; 600/109

Correspondence Address:

**WEINGARTEN, SCHURGIN, GAGNEBIN &
LEBOVICI LLP
TEN POST OFFICE SQUARE
BOSTON, MA 02109 (US)**


(57)

ABSTRACT

A cart or man-portable system and method for performing endoscopic procedures is provided. A portable display device, such as a laptop computer, is coupled to a handle comprising a miniature camera and fiber optic illumination subsystem. A sterile disposable portion is fitted over the illumination subsystem and inserted into a target area on a patient. Images of the target area are conveyed from the camera to the display device while an endoscopic procedure is performed, thus facilitating real-time diagnosis during the procedure.

(21) Appl. No.: **11/512,715**(22) Filed: **Aug. 30, 2006****Related U.S. Application Data**

(63) Continuation-in-part of application No. PCT/US06/08342, filed on Mar. 8, 2006, which is a continuation-in-part of application No. 11/075,827, filed on Mar. 8, 2005, which is a continuation-in-part of application

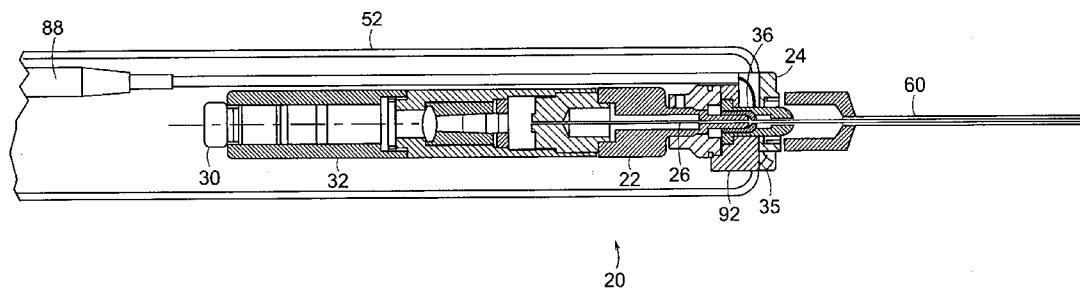

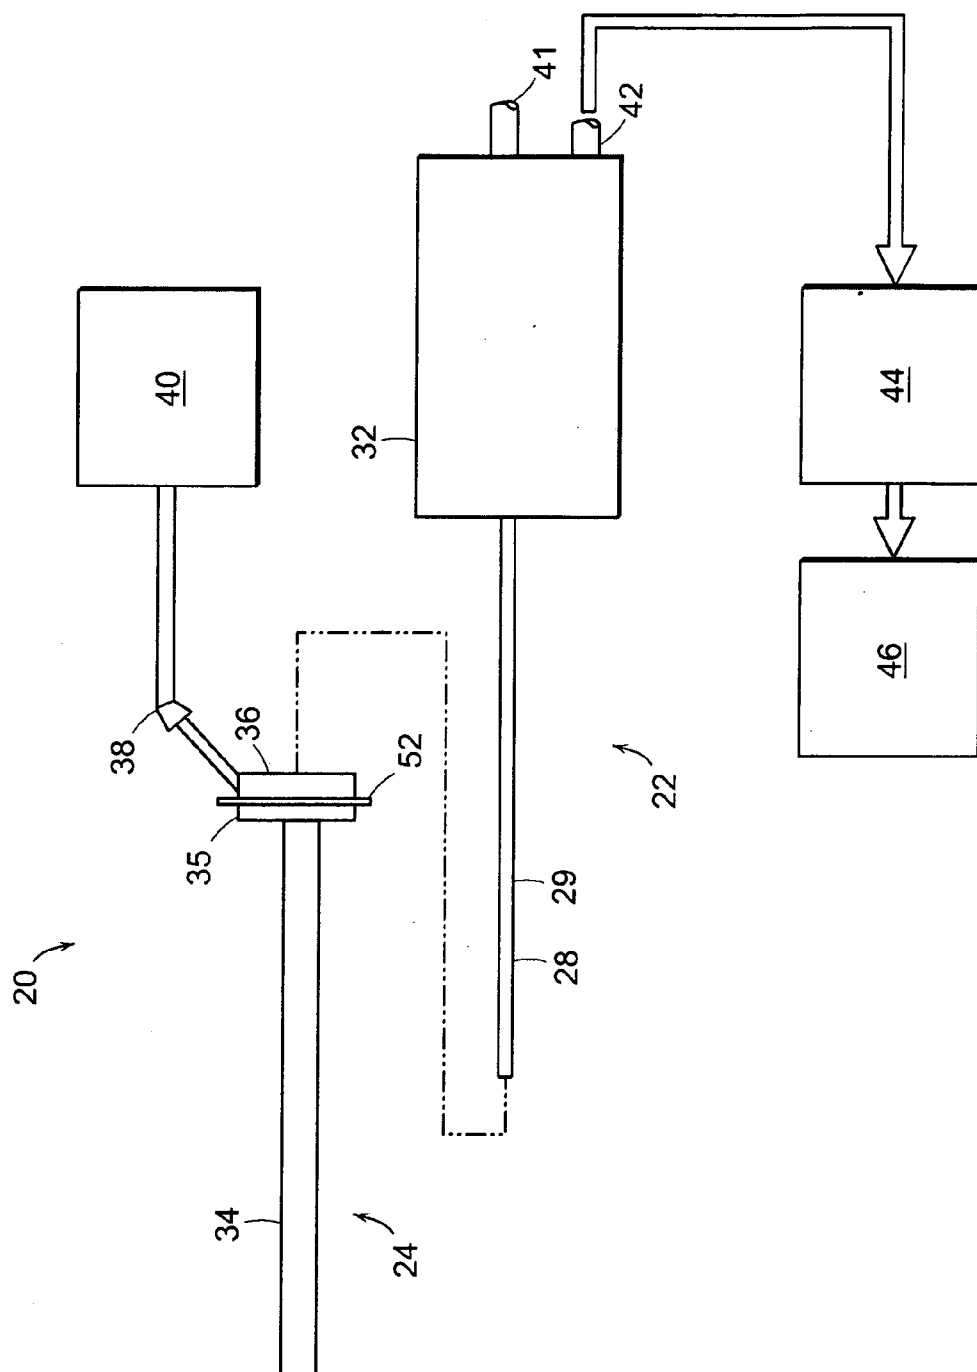


FIG. 1

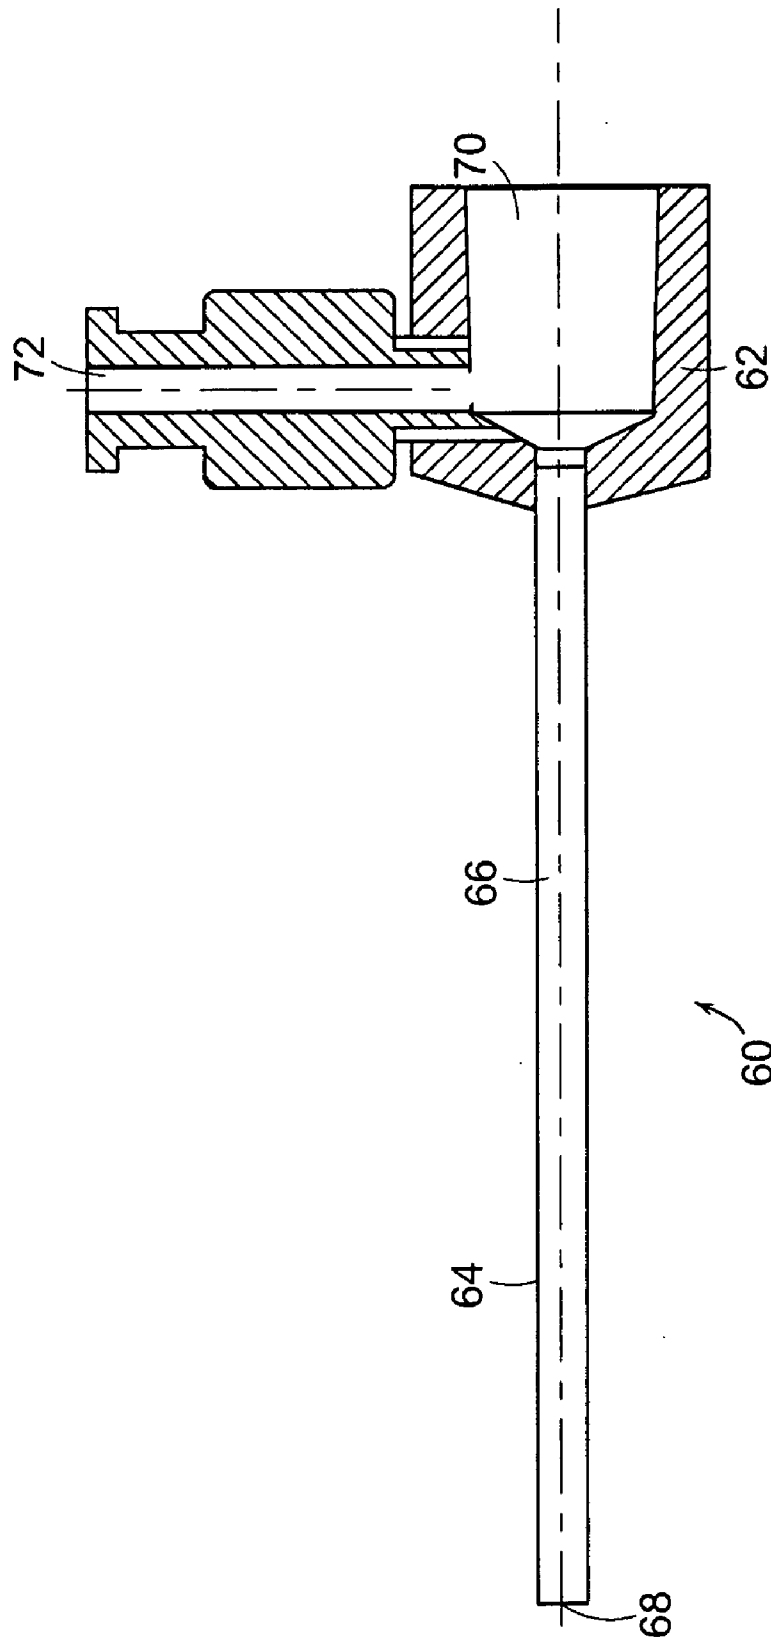


FIG. 2

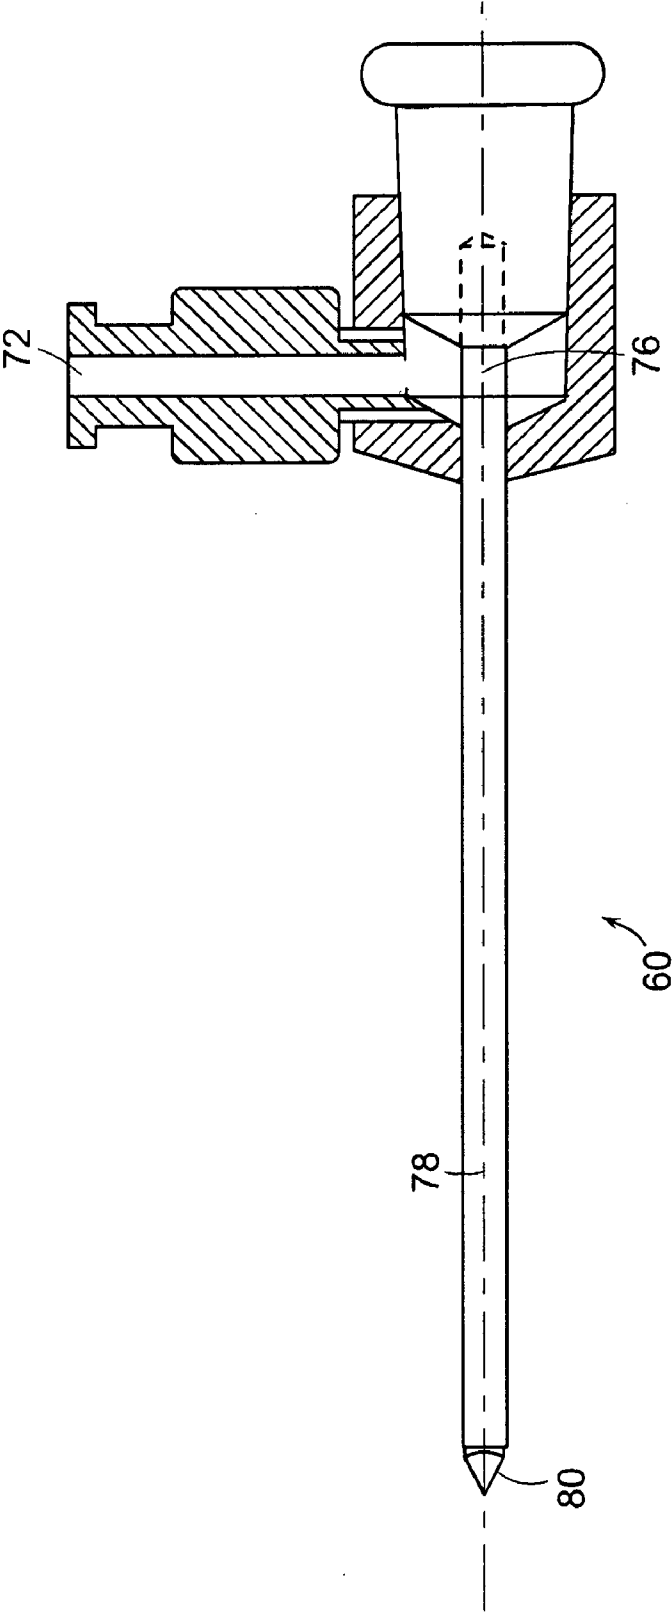
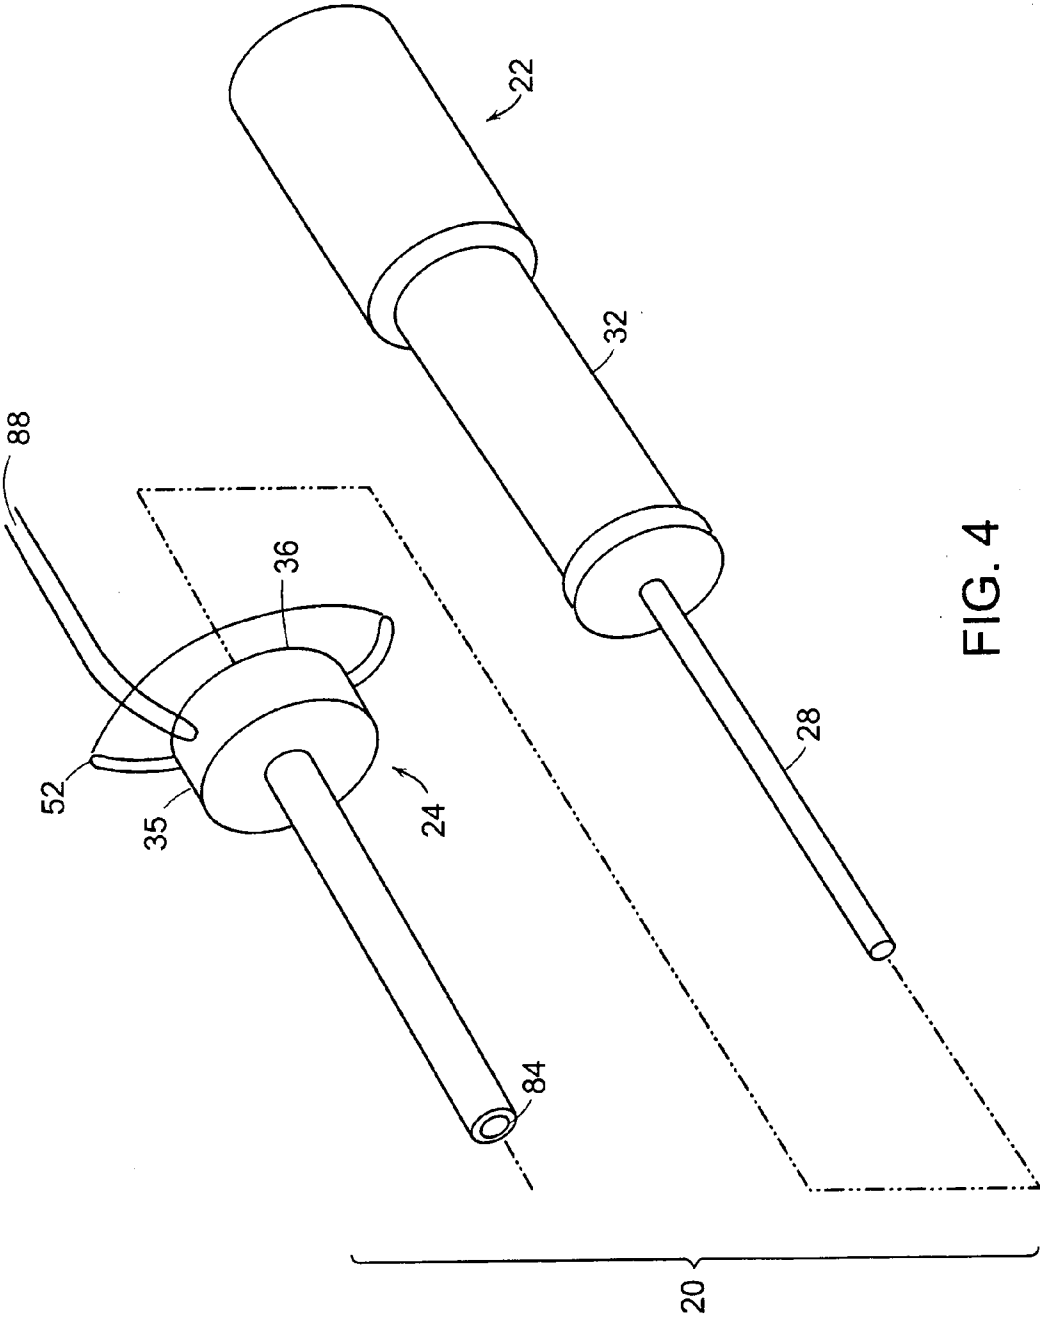


FIG. 3



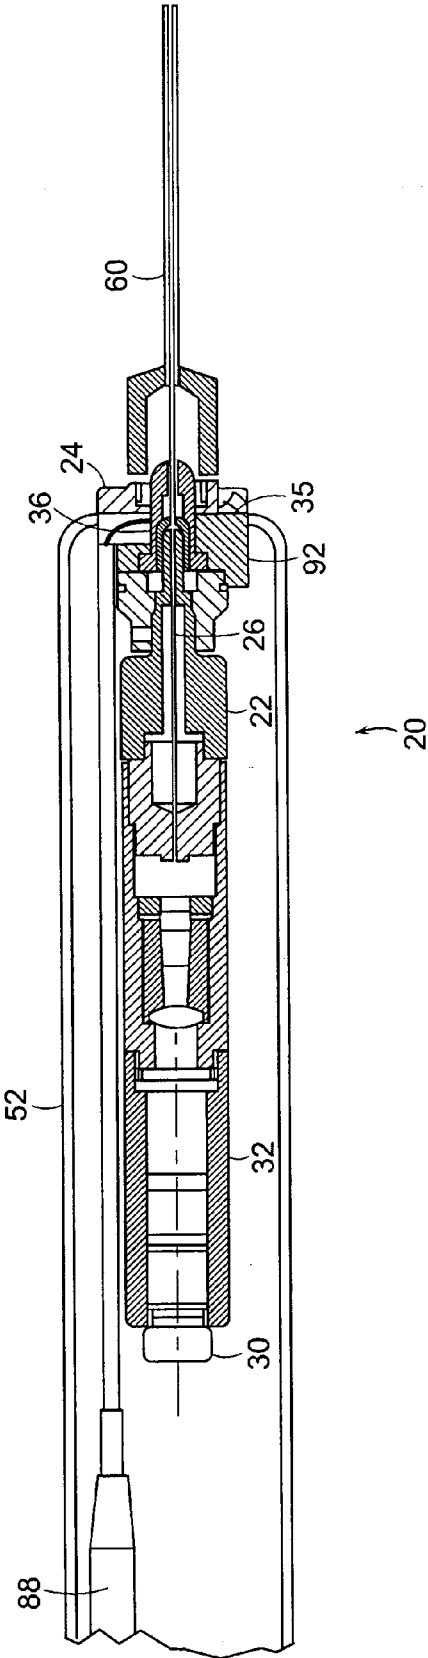


FIG. 5

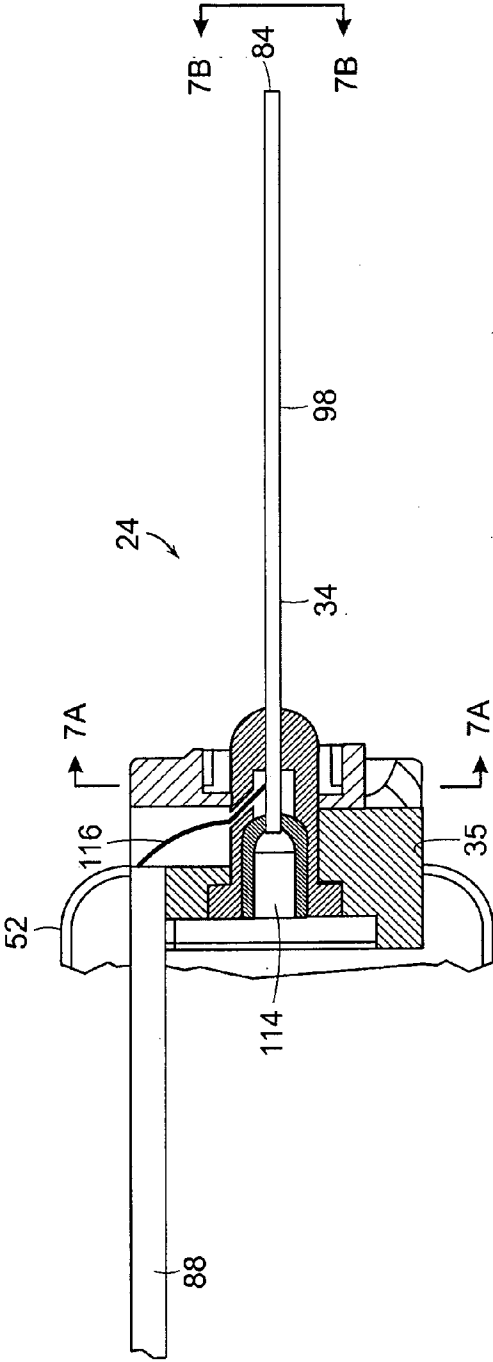


FIG. 6A

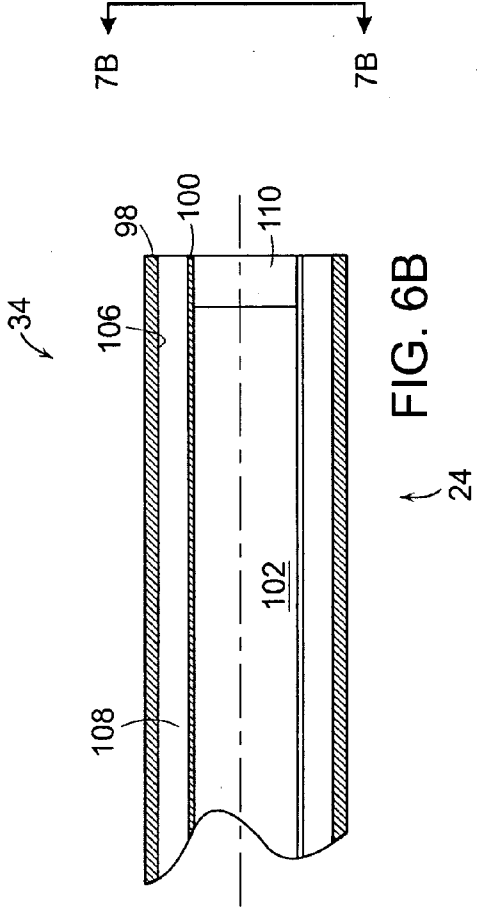


FIG. 6B

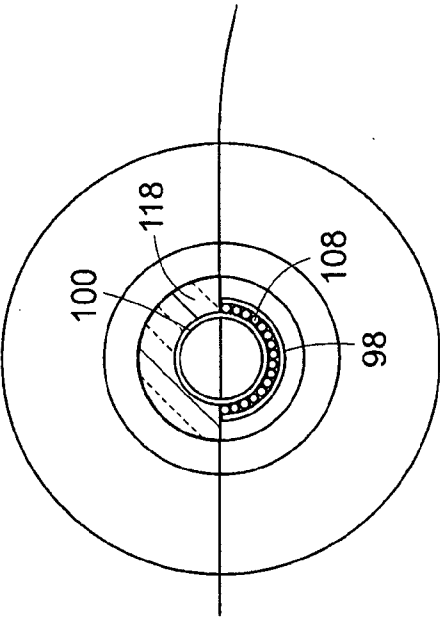


FIG. 7A

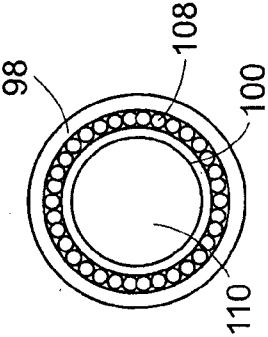


FIG. 7B

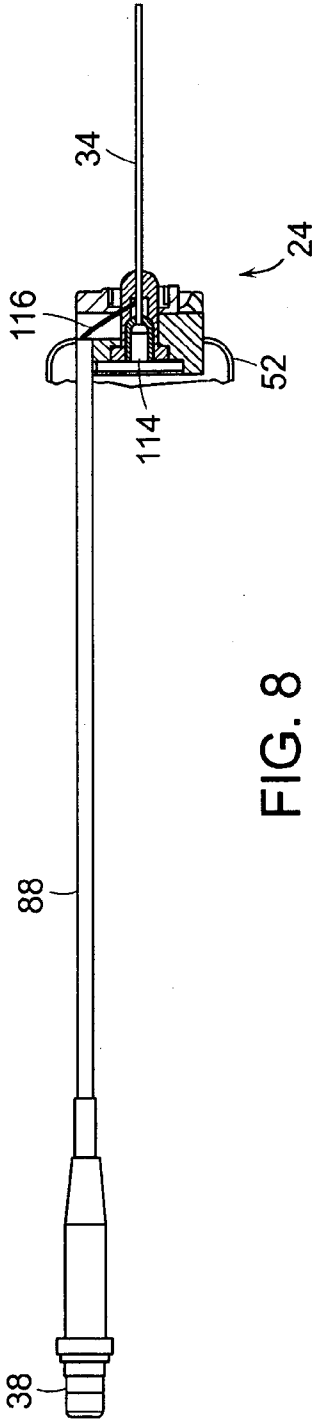


FIG. 8

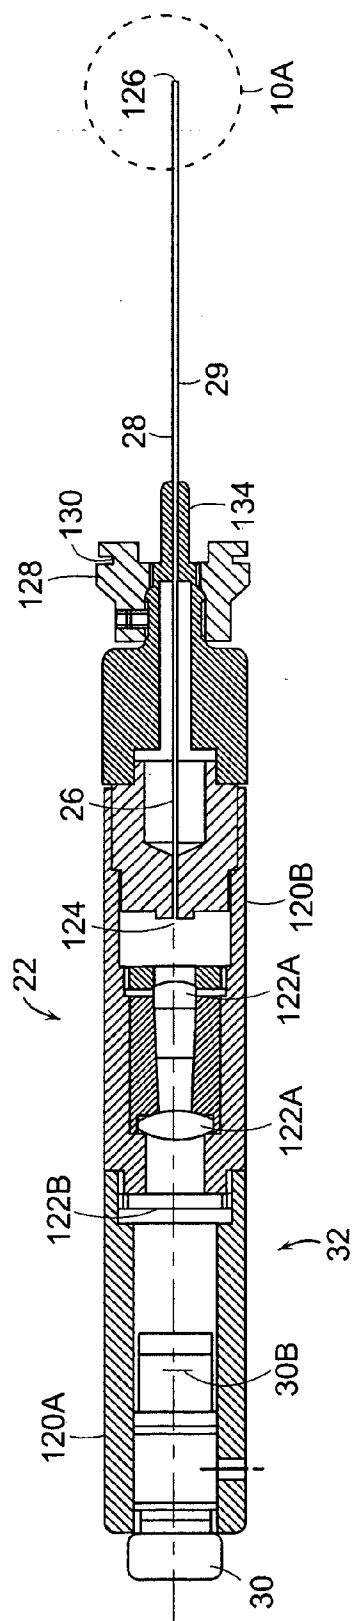
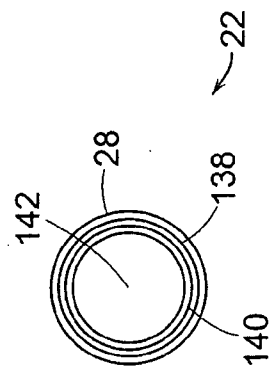

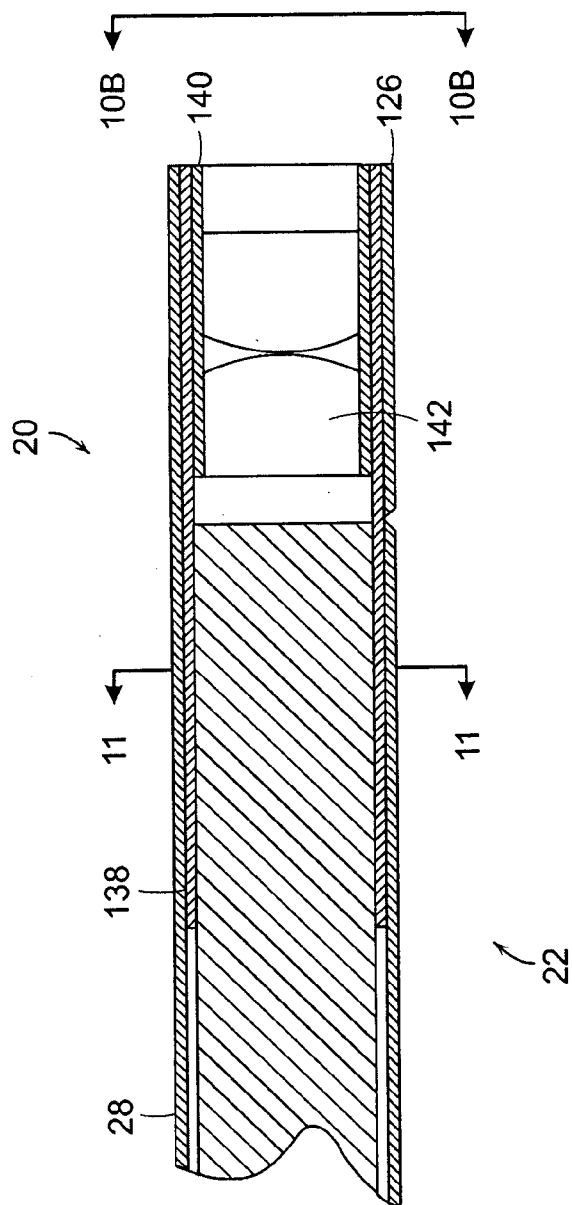


FIG. 9



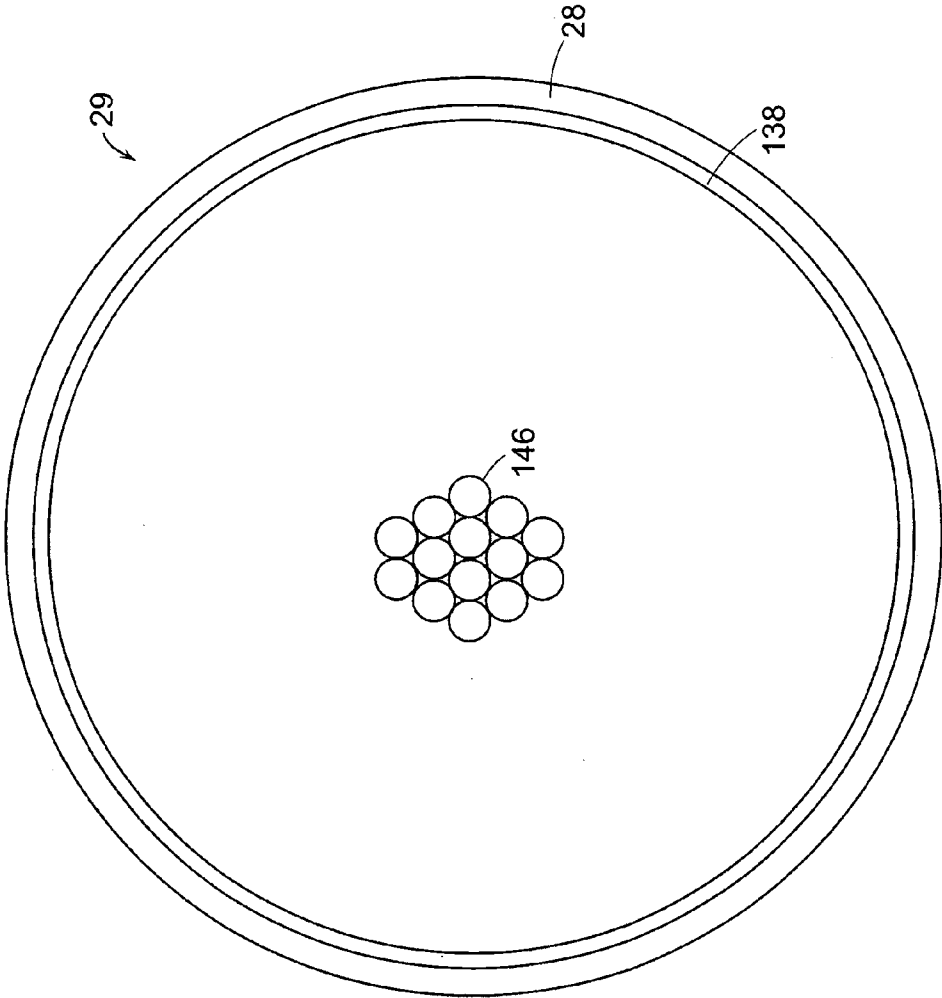


FIG. 11

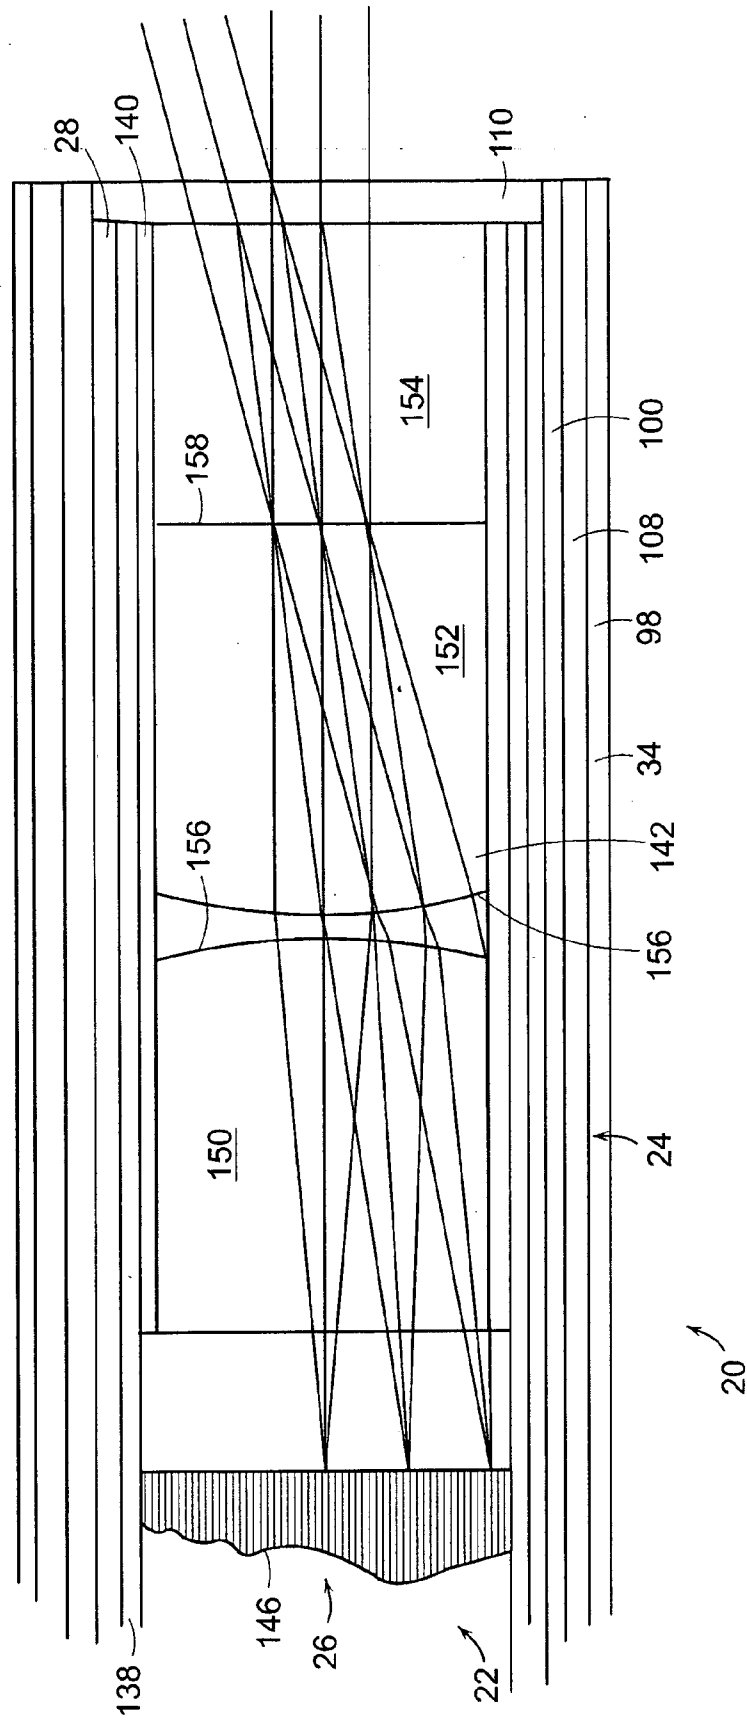


FIG. 12

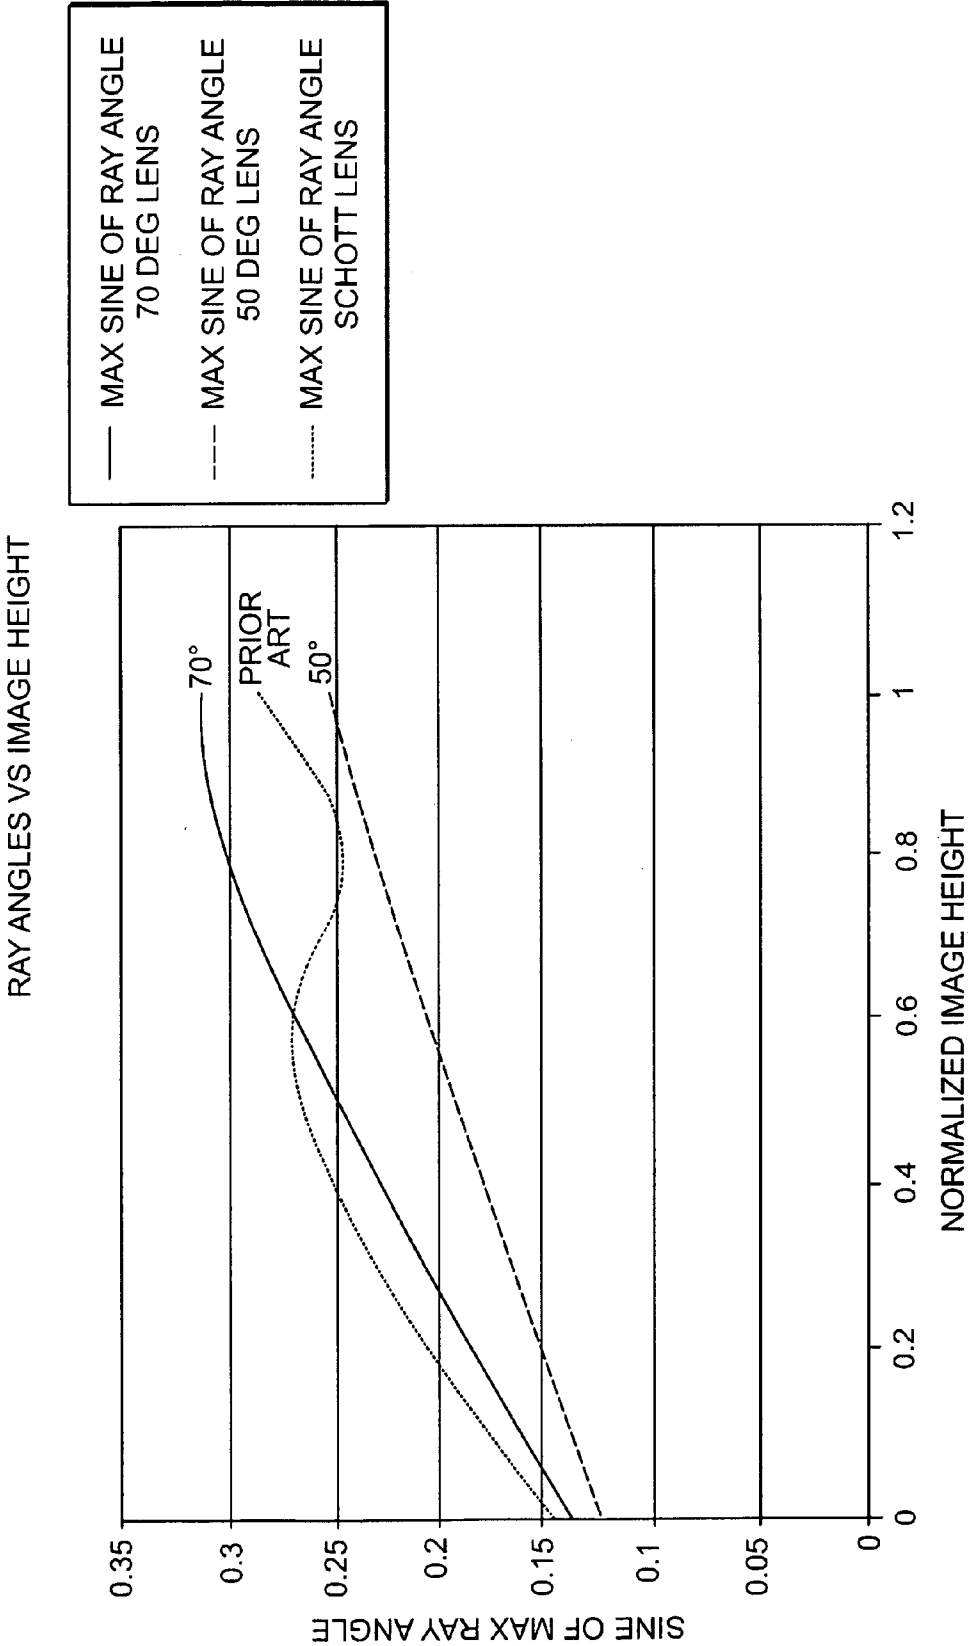


FIG. 13


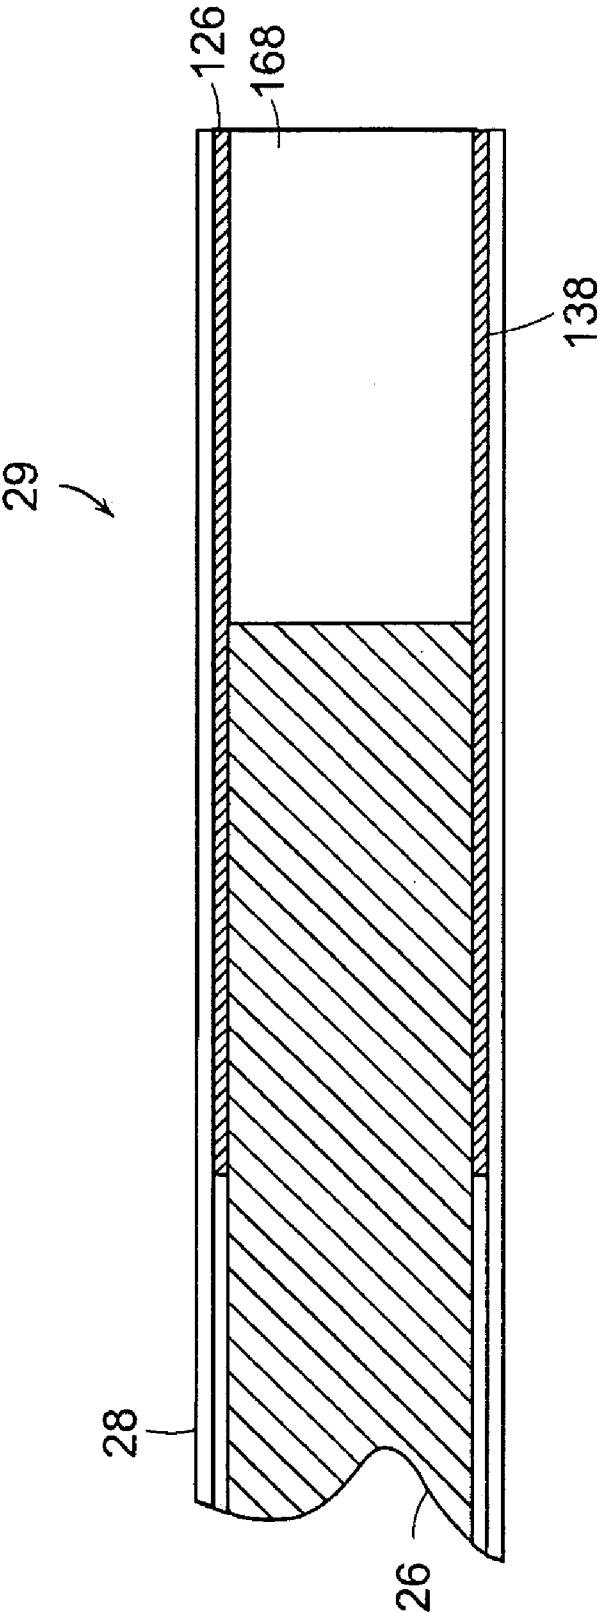


FIG. 14

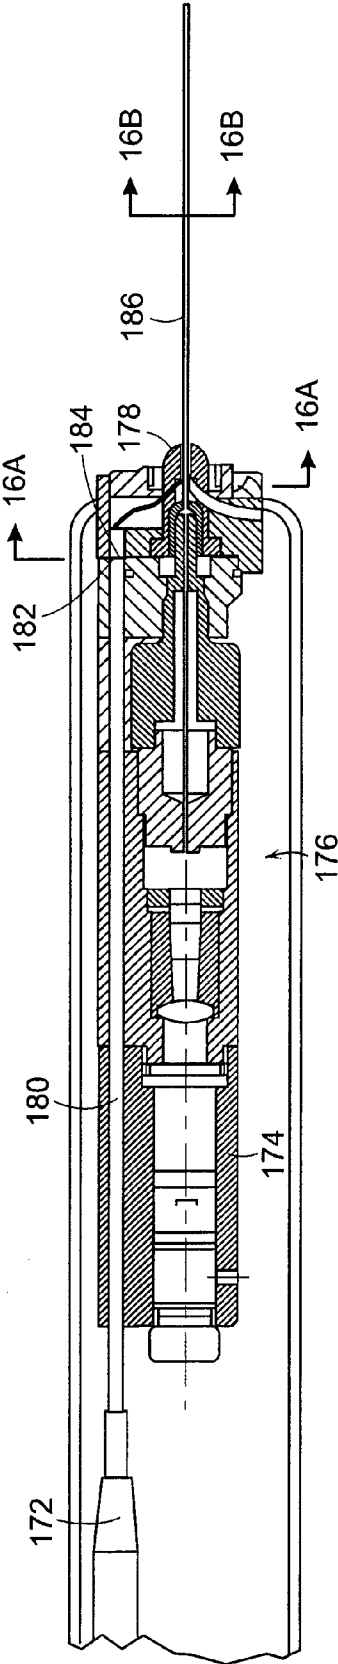

170

FIG. 15

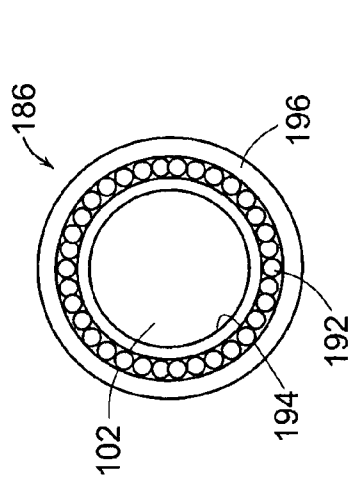


FIG. 16B

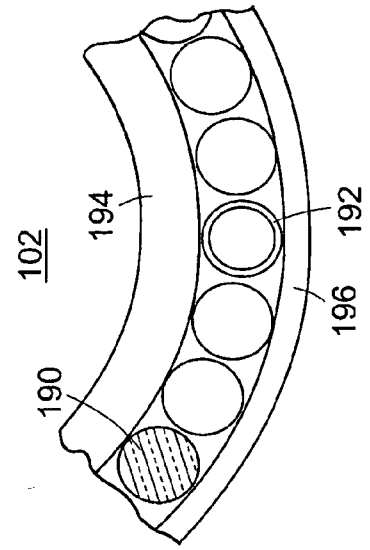


FIG. 16C

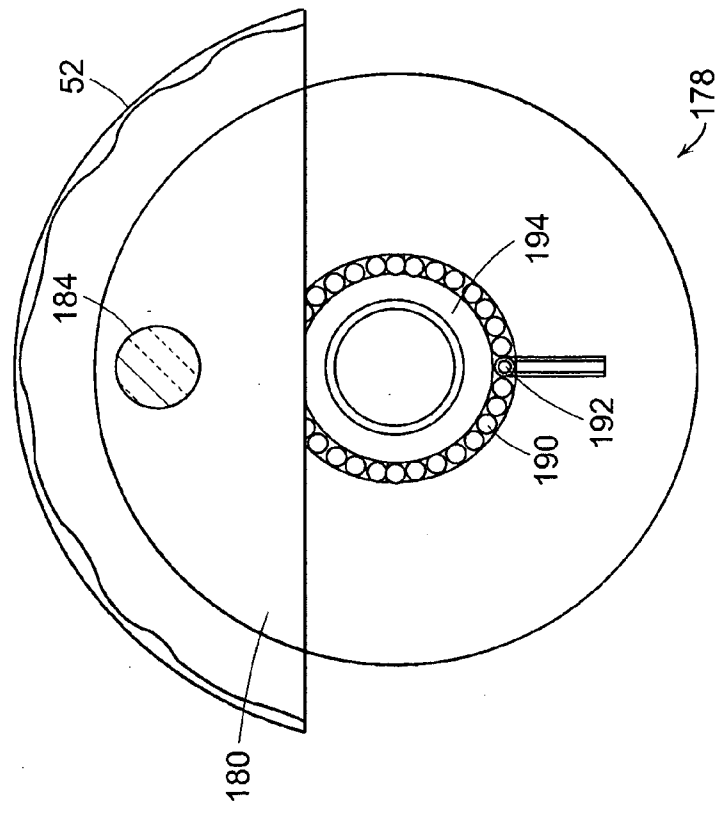


FIG. 16A

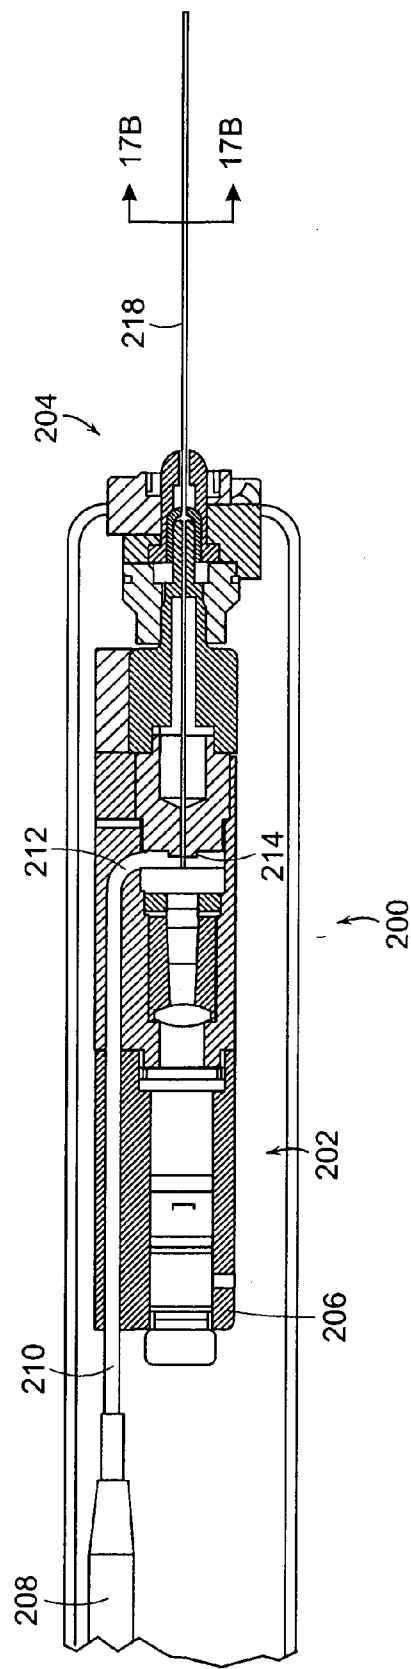


FIG. 17A

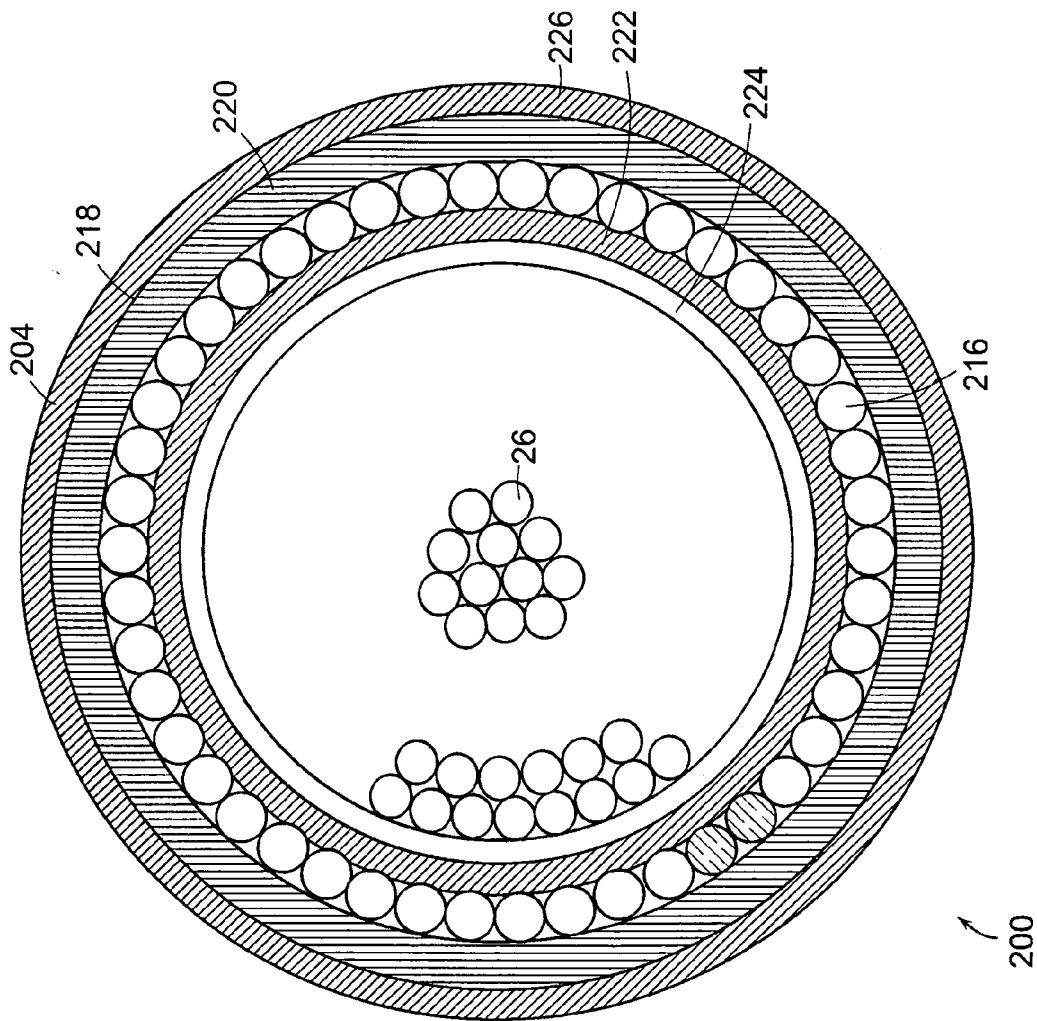
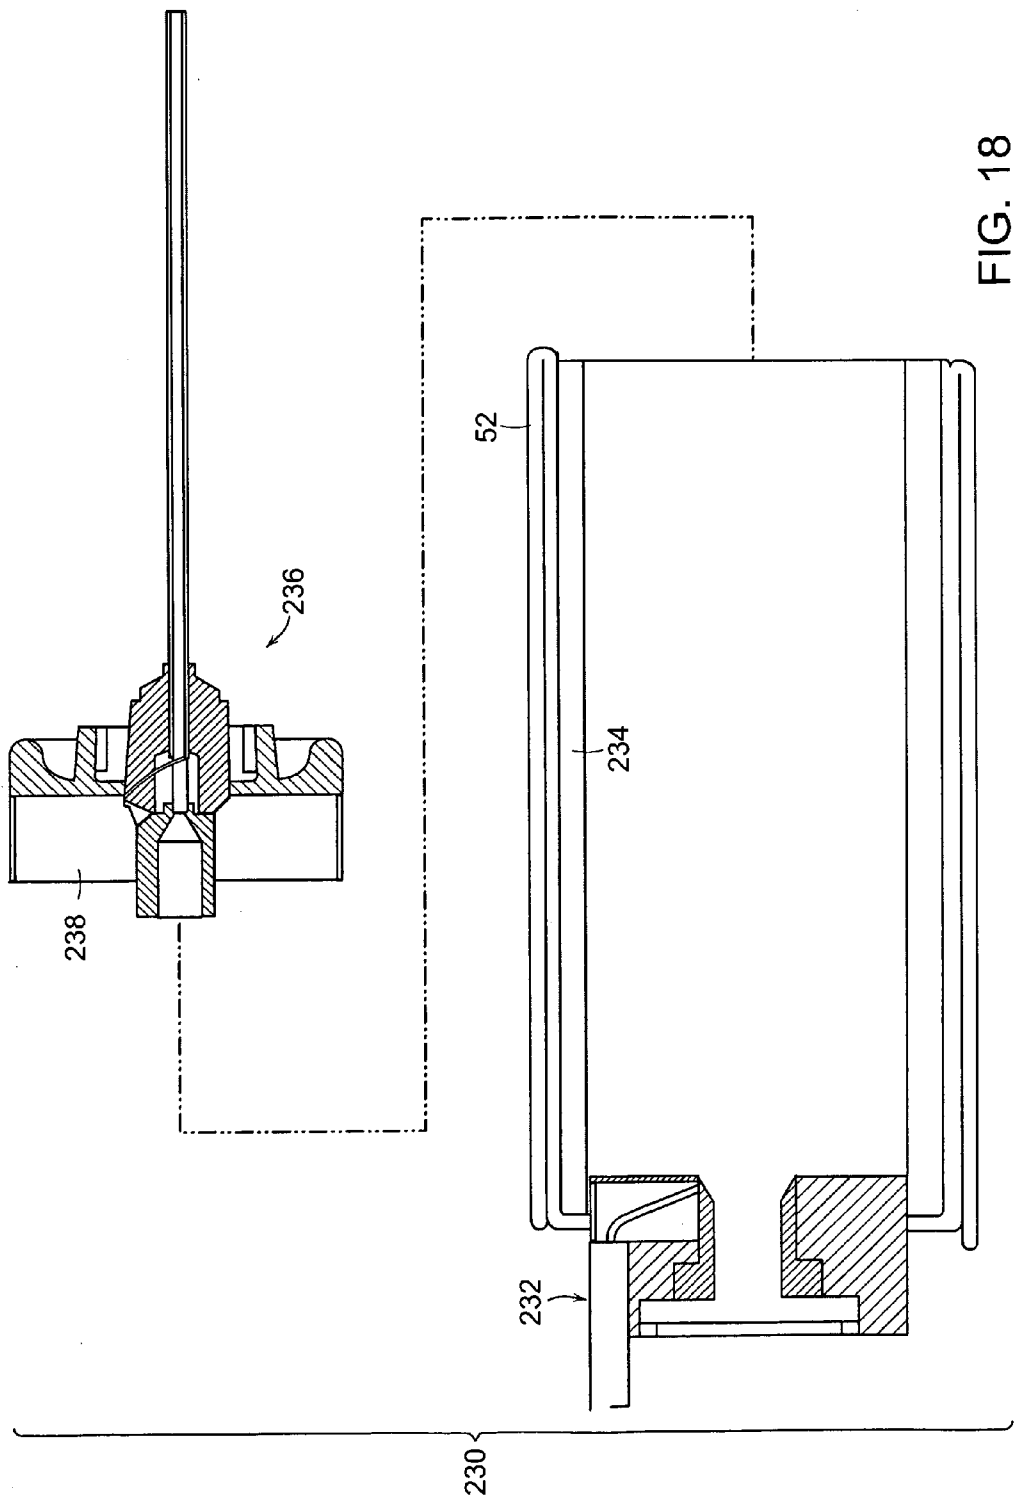


FIG. 17B



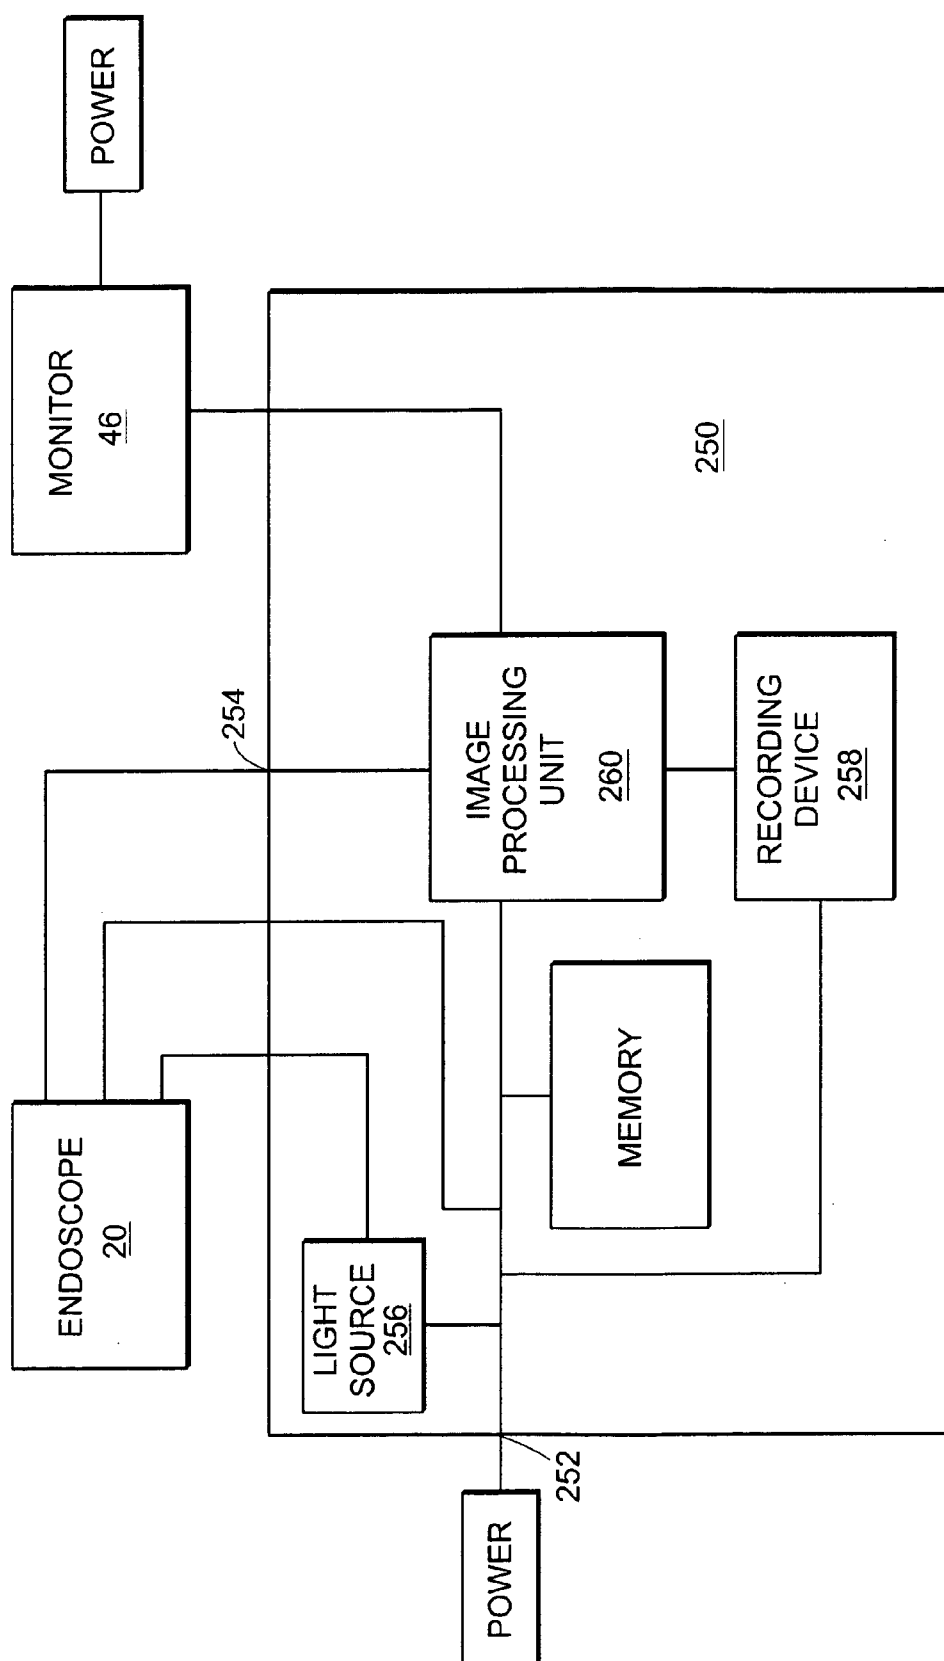


FIG. 19

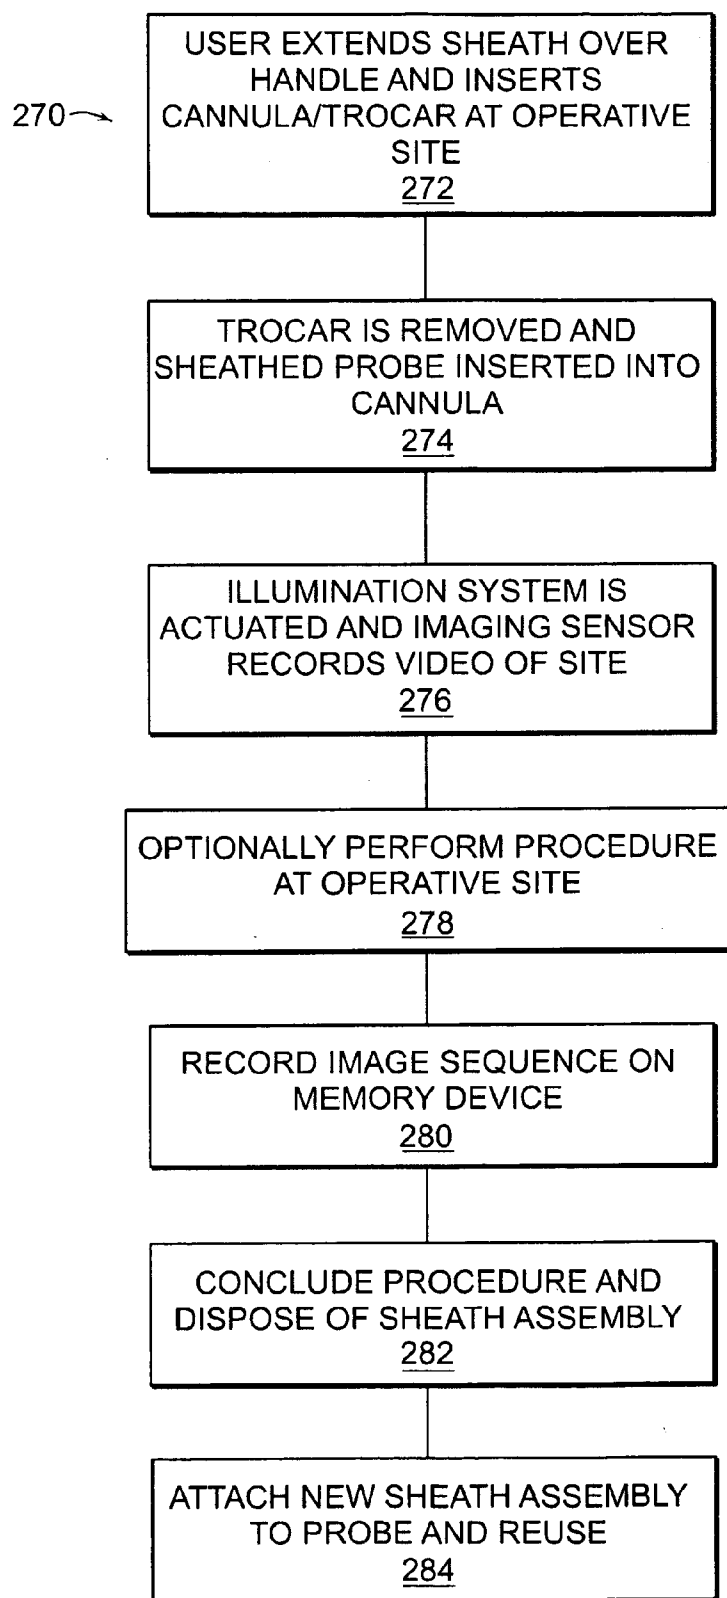


FIG. 20

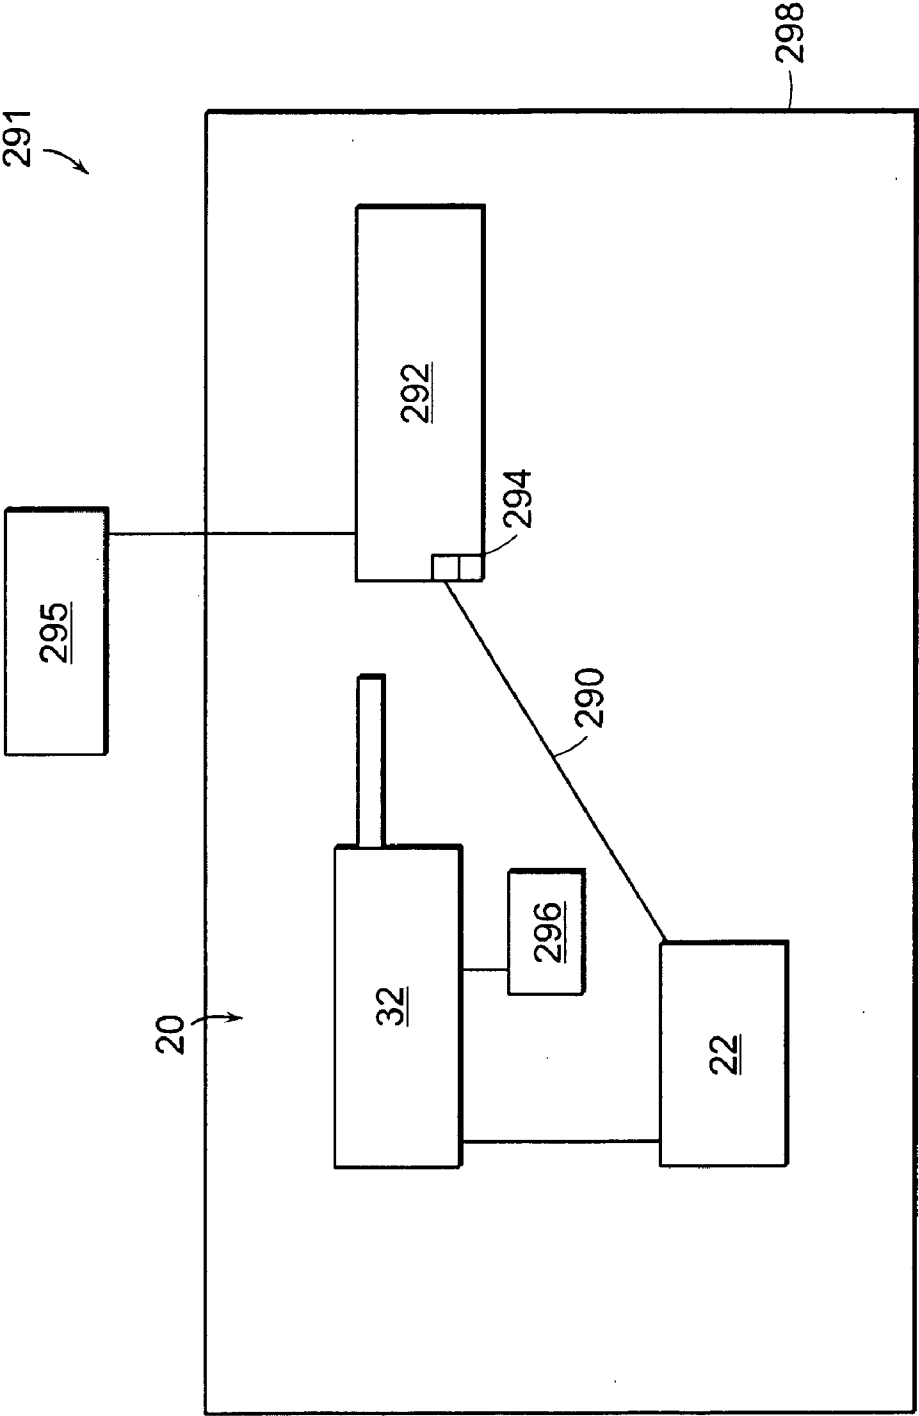
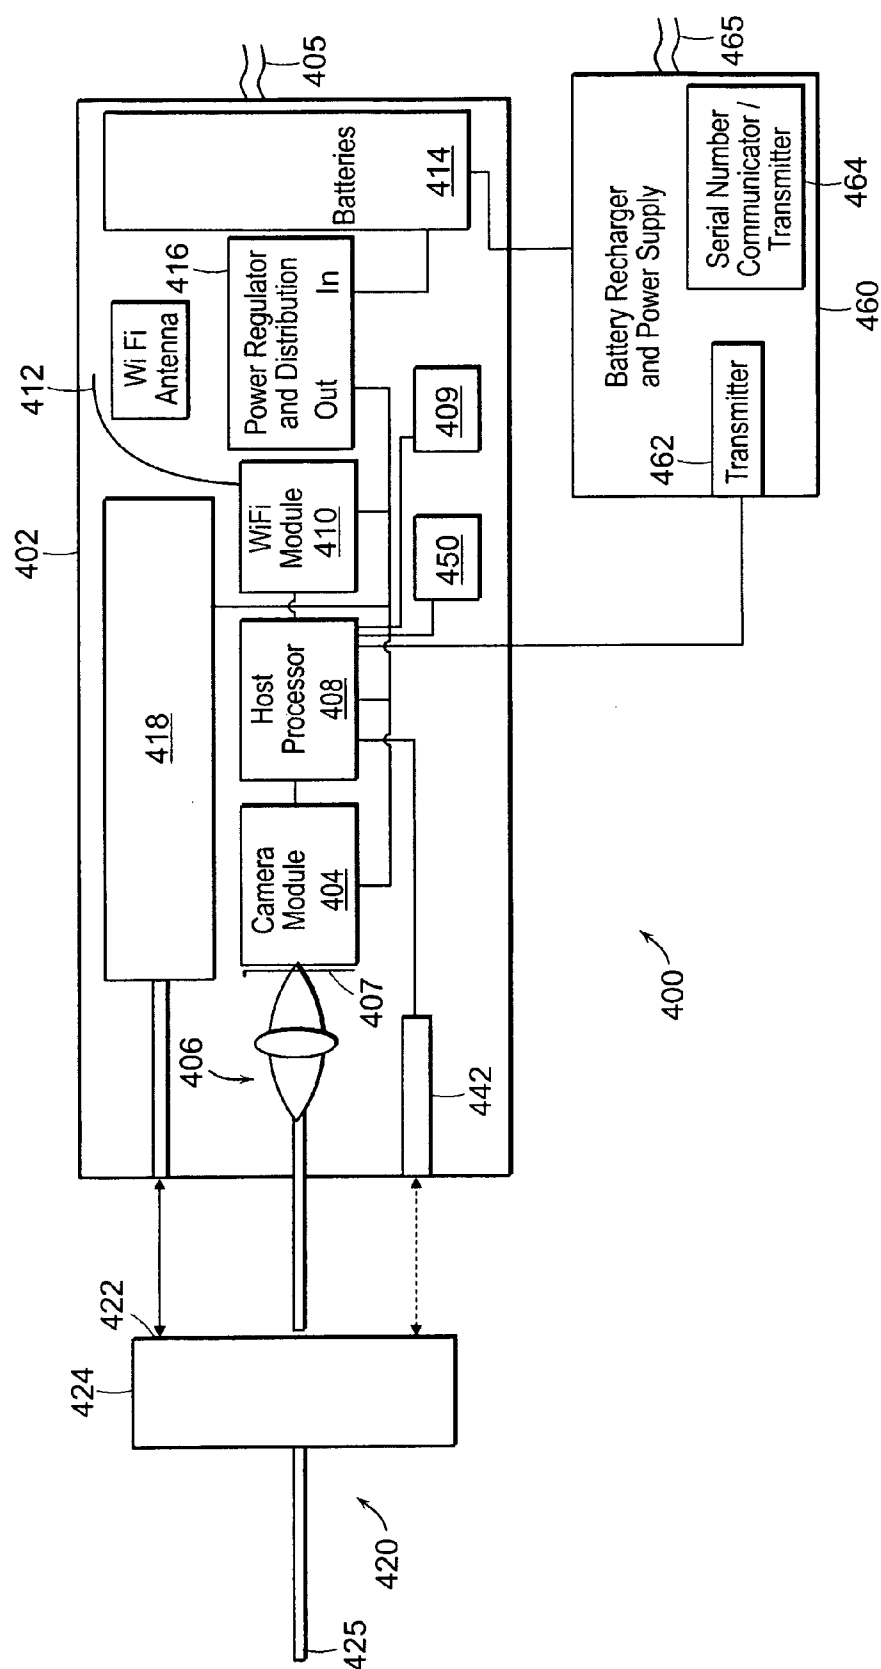


FIG. 21



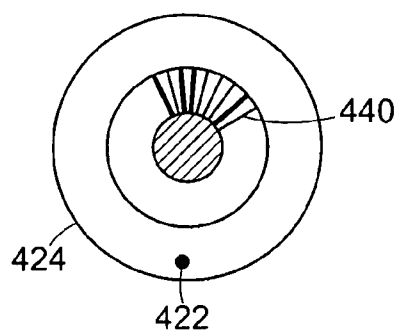


FIG. 23

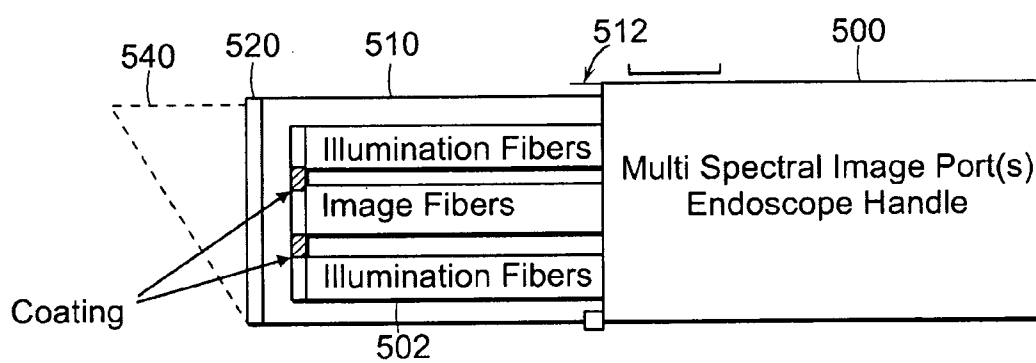


FIG. 24A

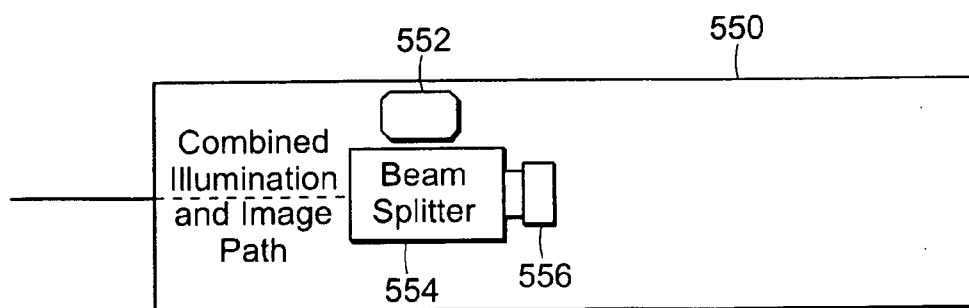


FIG. 25

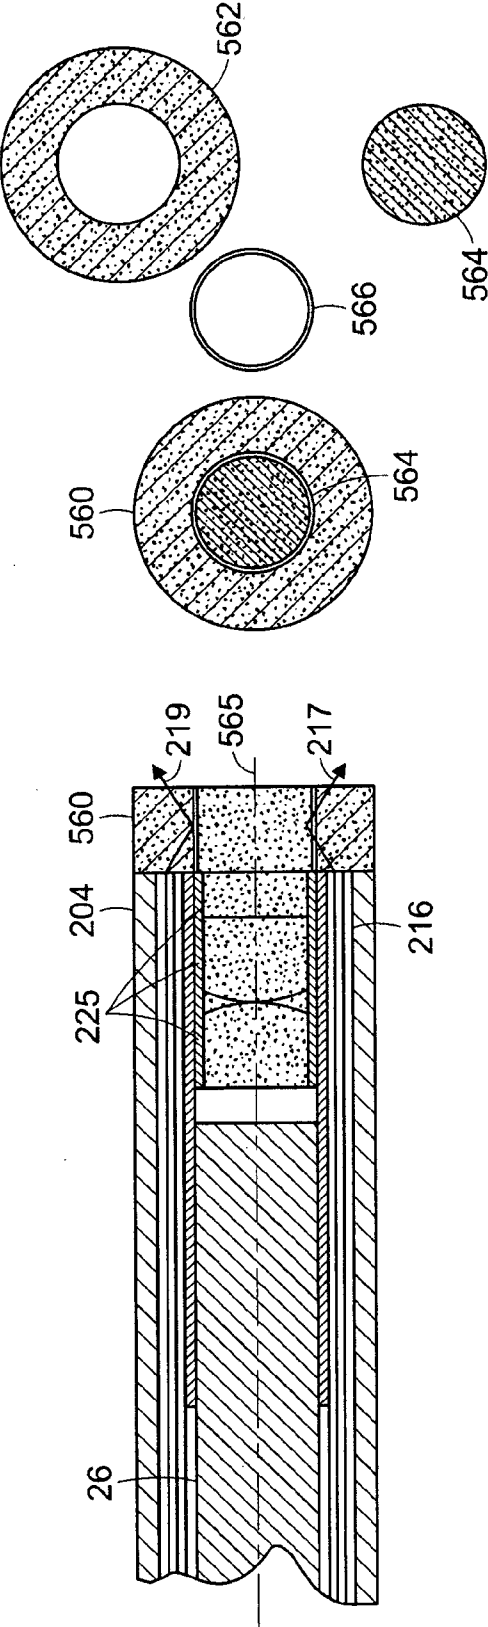


FIG. 24B

PORTABLE IMAGING SYSTEM EMPLOYING A MINIATURE ENDOSCOPE

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] The present application is a continuation-in-part of co-pending International Application No. PCT/US06/008342, filed Mar. 8, 2006 which is a continuation-in-part of U.S. patent application Ser. No. 11/075,827 filed on Mar. 8, 2005 which is a continuation-in-part of U.S. patent application Ser. No. 10/042,126, filed Oct. 19, 2001. This application claims priority to an application entitled "Miniature Endoscope With Imaging Fiber System" filed Mar. 4, 2005, now U.S. application Ser. No. 11/072,685. The entire contents of the above applications are incorporated herein by reference.

BACKGROUND OF THE INVENTION

[0002] Endoscopes enable visual examination of structure inside cavities. In the field of medicine, the use of endoscopes permits inspection of organs for the purposes of diagnosis, viewing of a surgical site, sampling tissue, or facilitating the safe manipulation of other surgical instruments.

[0003] Laparoscopes, for example, are used particularly for examining organs in the abdominal area. Laparoscopes typically include a light pipe for illuminating the region to be viewed, at least one lens assembly for focusing and relaying the image of the illuminated object, and a housing for the entire assembly which is structured to minimize tissue damage during the surgical procedure. The light pipe can include a fiber optic element for illuminating the site. The laparoscope housing includes a distal section that can be inserted within a body cavity and a proximal section which can include a handle that a user grips to position the distal end near the surgical site.

[0004] Existing endoscopes can include an imaging device such as a charged coupled device (CCD). This device can capture an image of an object being viewed and convey it to a display device, such as a monitor. There is a continuing need to improve on the operational features and manufacturability of endoscope systems that improve imaging capability and reduce the risk to the patient.

SUMMARY OF THE INVENTION

[0005] The present invention relates to a small diameter imaging probe or endoscope having improved durability, resolution, and field of view. In a preferred embodiment of the invention, the distal end of the probe including a disposable sheath, can be inserted into the tissue under examination. The probe is less than 3 millimeters in diameter, and preferably less than 2 millimeters in diameter, to reduce trauma at the point of insertion and thereby provide access to sites that are otherwise unavailable for endoscopic procedures.

[0006] In a preferred embodiment, the endoscope has a fiber optic waveguide that transmits an image from a distal end to a proximal end. A lens system is positioned at the distal end of the fiber optic waveguide. An imaging device is optically coupled to the proximal end of fiber optic waveguide. A sheath extends about the fiber optic

waveguide, the sheath including illumination fibers. Although a preferred embodiment utilizes a probe and sheath assembly having an outer diameter of 2 mm or less, certain applications will accommodate a larger diameter instrument having a larger number of imaging fibers to provide a higher resolution image. These applications can utilize outer diameters in a range of 2-4 mm.

[0007] In one embodiment, the lens system having a first lens element, a second lens element and an aperture stop. The lens system couples light from any given position on the object to a plurality of optical fibers such that the numerical aperture of light varies as a function of the angle relative to the longitudinal axis of the lens system. This provides more efficient coupling to the fiber apertures. This is accomplished using a non-telecentric lens system.

[0008] A preferred embodiment of the lens system includes a pair of lenses and an aperture stop. The lenses are shaped to improve light collection around the periphery of the distal lens. This provides a clearer image across the entire field of view of the device. The aperture stop is positioned to provide efficient coupling to the array of fibers.

[0009] The imaging device can be a charged coupled device (CCD), a CMOS imaging device or other solid state imaging sensor having a two dimensional array of pixel elements. The imaging sensor is mounted on a circuit board in a handle assembly. The sensor can capture an image as an object being viewed and an image processing circuit mounted onto the circuit board transfers the image data over a video cable to a computer for storage, processing and/or display.

[0010] The miniature endoscope system can be used for orthopedic, rheumatologic, general laparoscopic, gynecological or ear, nose and throat procedures small and large joints, cardiac, oncology, lung, breast, brain GI and veterinary applications for example. Although many applications require a small diameter to reduce trauma, certain applications can accommodate larger diameters. The probe can include an open channel in either the sheath or the imaging probe to provide for the insertion of other operative elements to flush the site with fluid, direct light or other energy source onto a treatment site, or to remove a tissue sample.

[0011] The sheath assembly can include a concentric array of illumination fibers extending to a connector on a sheath hub assembly. Alternatively, the illumination fibers can couple to a fiber connector in the probe assembly that is coupled directly via fiber optic cable extending from the handle to a light source housing. The housing can include a video disk recorder that writes the video onto disk. For certain applications, an illumination bundle can be positioned within the probe such that the sheath is thinner or can accommodate a larger working channel.

[0012] The present system, has four preferred applications for orthopedic use: in-office diagnostics, operating room surgical resections/procedures, in office post-operative evaluation, and therapeutic usage for the delivery of medications into joints, while confirming their correct location under direct visualization.

[0013] In addition to its use in the office, the system can be used in the operating room instead of a standard arthroscope. By eliminating the need to use arthroscopic irrigation fluid or a large-bore camera, the amount of pain and swelling

following an arthroscopic procedure will be substantially reduced if not eliminated. The patient can return to the office or playing field the next day.

[0014] The system is used for the postoperative assessment of the healing process for tissue and bond graft procedures, which are not currently possible using conventional MRI techniques. Examples include: assessment of articular cartilage resurfacing procedures, meniscal repairs, labral repairs, rotator cuff repairs, fracture reductions of joint surfaces, ligament integrity, and other usages.

[0015] The system includes a computer (or other viewing system), camera, light source and reusable handle that does not require reprocessing between procedures and a sterile barrier and lens components that is single patient use and disposable. The system eliminates the space requirements, cost of reprocessing equipment, manpower and costs associated with the time sensitive endoscope re-sterilization.

BRIEF DESCRIPTION OF THE DRAWINGS

[0016] The foregoing and other objects, features and advantages of the invention will be apparent from the following more particular description of preferred embodiments of the invention, as illustrated in the accompanying drawings in which like reference characters refer to the same parts throughout the different views. The drawings are not necessarily to scale, emphasis instead being placed upon illustrating the principles of the invention.

[0017] FIG. 1 illustrates a schematic illustration of a miniature endoscope system according to the invention;

[0018] FIG. 2 is a cross-sectional view of cannula;

[0019] FIG. 3 is a cross-sectional view of a trocar within a cannula;

[0020] FIG. 4 is a perspective view of the miniature endoscope;

[0021] FIG. 5 is a sectional view of the miniature endoscope with a cannula overlying the disposable sheath;

[0022] FIG. 6A is a sectional view of the disposable sheath/illuminator unit;

[0023] FIG. 6B is an enlarged sectional view of the distal end to the disposable sheath;

[0024] FIG. 7A is a sectional view of the proximal end of the disposable sheath/illumination unit taken along line 7A-7A of FIG. 6A;

[0025] FIG. 7B is a front view of the distal end of the disposable sheath taken along the line 7B-7B of FIG. 6A and FIG. 6B;

[0026] FIG. 8 is a side view of the disposable sheath/illumination unit showing the illumination pigtail;

[0027] FIG. 9 is a sectional view of an imaging unit of the miniature endoscope;

[0028] FIG. 10A is an enlarged view of the distal end of the imaging unit as indicated by the portion defined 10A in FIG. 9;

[0029] FIG. 10B is a front view of the distal end of the imaging unit taken along the line 10B-10B of FIG. 10A;

[0030] FIG. 11 is a schematic of an enlarged partial sectional view of the imaging unit taken along the line 11-11 of FIG. 10A;

[0031] FIG. 12 is an enlarged view of the distal lens system;

[0032] FIG. 13 is a graph of the sine of the maximum ray angle versus normalized image height for different lens systems for the distal end of the endoscope;

[0033] FIG. 14 is an enlarged view of another embodiment of a distal lens system;

[0034] FIG. 15 is a sectional view of another embodiment of an endoscope;

[0035] FIG. 16A is a sectional view of the endoscope taken along line 16A-16A of FIG. 15;

[0036] FIG. 16B is a sectional view of the endoscope taken along line 16B-16B of FIG. 15;

[0037] FIG. 16C is an enlarged sectional view of the imaging unit as indicated by the portion defined by 10C in FIG. 16B;

[0038] FIG. 17A is a sectional view of another embodiment of an endoscope;

[0039] FIG. 17B is a sectional view of the endoscope taken along the line 17B-17B of FIG. 17A;

[0040] FIG. 18 is a side view of a two-part disposable sheath/illuminator unit;

[0041] FIG. 19 is a schematic of a control unit for a preferred embodiment of the invention;

[0042] FIG. 20 illustrates a preferred method of using the invention;

[0043] FIG. 21 illustrates a preferred embodiment of a portable endoscopic system in accordance with the invention;

[0044] FIG. 22 illustrates a preferred embodiment of an endoscopic in accordance with the invention;

[0045] FIG. 23 is an end view of a sheath;

[0046] FIG. 24A is a schematic view of a preferred endoscopic device;

[0047] FIG. 24B is a cross-sectional view of the insertion portion of the probe; and

[0048] FIG. 25 is a schematic view of another preferred endoscopic device.

DETAILED DESCRIPTION OF THE INVENTION

[0049] An embodiment of the invention is illustrated in FIG. 1 that shows a miniature endoscope 20. The endoscope 20 has an imaging unit 22 and a sheath/illuminator unit 24. The endoscope 20 has an image transmission path such as a plurality of optical fibers 26, as best seen at fibers 146 in FIGS. 11 and 12, in an elongated tube 28 of a rod tip 29 used to view objects to be examined. The optical fibers 26 are optically coupled to an imaging device 30, such as a charged coupled device as seen in FIG. 9, or other pixilated flat panel sensor, in a handle 32. A disposable sheath 34 of the sheath/illuminator unit 24 overlies the elongated tube 28 of

the rod tip 29, which contains the optical fibers 26. The disposable sheath 34 has at the proximal end a base 35 with a mounting mechanism 36 for securing to the handle 32. In one embodiment, the disposable sheath 34 of the sheath/illuminator unit 24 has a plurality of optical fibers for transmitting light to the distal end of the disposable sheath 34 and the distal probe 29. The distal end of the disposable sheath/illuminator unit 24 has a connection 38 to connect to a light source 40.

[0050] The handle 32 can house a power input 41, used to provide power to the endoscope 20. It is recognized that the light source 40 and/or power source can be mounted within the handle 32.

[0051] The handle 32 can also house an image output 42. The image output 42 provides a connection between an imaging device in the imaging unit 22 of the endoscope 20 and an electronic storage and/or display device. In one embodiment, the storage device is a computer 44, which is connected to a monitor 46. A control unit 250 is described in greater detail with respect to FIG. 19.

[0052] As explained below in greater detail the imaging unit 22 does not need to be sterilized in that the imaging unit 22 does not contact or is in direct exposure to the body. The sheath/illuminator unit 24 has the disposable sheath 34 that is a sleeve assembly 52 that is carried by the base 35 secured to the imaging unit 22 that overlies the elongated tube 28 to create a sterilized barrier. In addition, the sheath/illumination unit 24 has a sterilized drape 52 which is mounted to the base 35 of the sheath/illuminator unit 24 and is positioned to overlie the remaining portion of the imaging unit 22 to provide a sterile environment.

[0053] Endoscopes and endoscopes with disposable sheaths are described in PCT Application PCT/US00/25107 filed on Sept. 13, 2000 and U.S. patent application Ser. No. 09/518,954 filed on Mar. 6, 2000. The entire contents of the above applications are incorporated herein by reference in their entirety.

[0054] Prior to discussing the endoscope 20 in further detail, in order to use the endoscope 20, the endoscope 20 needs to be positioned in the body to view the desired location. One such method is to insert a cannula 60 into the body and thread the endoscope 20 through the cannula 60. One method of inserting the cannula 60 into the body and then inserting the endoscope 20 into a body using the cannula 60 is described below.

[0055] During an insertion procedure, a cannula 60 such as seen in FIG. 2, is first inserted into a site within a body. The cannula 60 has a base 62 and a tube 64. The tube 64 has a shaft 66 which extends from the distal end 68 to a void 70 in the base 62. In one embodiment, the tube 64 is made of a flexible material such as plastic or thin wall stainless steel. The cannula 60 has a luer 72 for insertion of medications or fluids or for attachment to a suction device.

[0056] For insertion of the cannula 60 into the body, a trocar 76, as seen in FIG. 3, is inserted into cannula 60 with a rigid shaft 78 of the trocar 76 received within the shaft 66 of the cannula 60. The rigid shaft 78 of the trocar 76 extends slightly beyond the distal end of the tube 64 of the cannula 60 and has a stylet 80 to cut into the tissue at the surgical site if necessary. Once the cannula 60 is positioned at the surgical site, the trocar 76 is removed from the cannula 60

and the endoscope 20 is installed. The cannula 60 is positioned by the user's hands feeling the location.

[0057] While the cannula 60 and trocar 76 are of a relative minimal cost and can be reused after sterilization or disposed of after use, because of several components in the endoscope 20 such as components in the imaging unit 22, it is not desirous to dispose of the entire endoscope 20. The endoscope 20 uses a disposable sleeve or sheath 34 to aid in maintaining a sterile environment and reduce or eliminate the sterilization requirements prior to reuse.

[0058] With the method of inserting the endoscope 20 into the cannula 60 to have the distal end of the endoscope 20 at the proper location, previously described, the endoscope 20 is described in further detail. Referring to FIG. 4, a perspective view of the endoscope 20 is shown. The endoscope 20 has the reusable imaging unit 22 and the disposable sheath/illuminator unit 24. The disposable sheath/illuminator unit 24 has an elongated tube for overlying and encircling the elongated tube 28 of the imaging unit 22. The elongated tube of the sheath/illuminator unit 24 has a sealed distal end 84 and several embodiments includes fiber optics for transmitting the illumination from an external light source 40, such as seen in FIG. 1, to the distal end 84. At the proximal end of the sheath/illuminator unit 24 is a base 35 with a mounting mechanism 36 for securing to the imaging unit 22 of the endoscope 20. An optical pigtail 88 projects from the base 35 for connecting to the light source 40. In addition, the sheath/illuminator unit 24 has a drape 52 which is mounted to the base 35 and is extended over the handle 32 of the imaging unit 22. The handle 32 of the imaging unit 22 contains optics and the imaging device 32 to receive the image transmitted through the optical fibers 26 located in the elongated tube 28 of the imaging unit 22 as described in further detail below with respect to FIGS. 9-11.

[0059] FIG. 5 is a sectional view of the miniature endoscope 20 including the reusable imaging unit 22 with imaging an optical fiber 26 and the disposable sheath/illuminator unit 24. The cannula 60 is shown overlying the disposable sheath 34 of the sheath/illuminator unit 24, which overlies the probe 29 of the imaging unit 22.

[0060] As seen in FIG. 5, the reusable imaging unit 22 of the endoscope 20 is encircled by the disposable sterile sheath/illuminator unit 24. The disposable/sheath illuminator unit 24 has the disposable sheath 34 that is sealed at the distal end 84 and encircles and surrounds the elongated tube 28 carrying the optical fibers 26 of the imaging unit 22. The mounting mechanism 36 on the base 35 of the sheath/illuminator unit 24 is secured to a mounting mechanism 92 on the imaging unit 22.

[0061] The disposable sheath/illuminator unit 24 has the drape 52 which surrounds the handle of the imaging unit 22. In addition, the sheath/illuminator unit 24 has the illumination pigtail connecting to a light source 40 as seen in FIG. 1. The illumination pigtail 88 is optically coupled to the optical fibers in the sheath as explained in further detail below.

[0062] Referring to FIG. 6A, a side view of the sheath/illuminator unit 24 is shown. The sheath unit 24 has the disposable sheath 34 with an elongated outer sheath 98 which extends from the base 35 to the distal end 84. The illuminator pigtail 88 extends from the base and is optically

coupled to illumination fibers within the sheath 34 as seen in FIG. 7A. The drape 52 is carried by the base 35 of the sheath/illuminator unit 24 for overlying the handle 35 of the imaging unit 22 when the two units 22 and 24 are combined.

[0063] FIG. 6B is an enlarged view of the distal end 84 of the disposable sheath 34 of the sheath/illuminator unit 24. The disposable sheath 34 has the outer sheath 98 which extends from within the base 35, as seen in FIG. 6A, and serves as protective covering and a sterile barrier for the sheath unit 24. Spaced and collinear with the outer sheath 98 is an inner tube 100 of the disposable sheath 34. The inner tube 100 defines a cylindrical void on space 102 for receiving the elongated tube 28 of the probe 29 of the imaging unit 22. The inner tube 100 likewise from the distal end 84 of the disposable sheath 34 to the base 35 of the sheath/illuminator unit 22. The inner tube 100 extends further than the outer sheath 98 to create a channel 106 to receive a plurality of illumination fibers 108 as best seen in FIG. 6A and 7A. At the distal end, of the inner tube 100 is located a window 110 which is secured to the inner tube 100 to make a sterile 84 barrier between the airspace 102 for receiving the elongated tube 28 of the image unit 22 and the outer portion of the sheath/illuminator unit 24 which is in contact with the body.

[0064] In a preferred embodiment, the outer sheath 98 of the disposable sheath 34 of the sheath/illuminator unit 24 is made of a stainless steel material and has an outer diameter of about 0.038 inches. The inner tube 100 is likewise made of a stainless steel material. The illumination fibers 108 are made of a glass or plastic fiber. Depending on the size of the device, the maximum number of illumination fibers 108 used to fill channel 106. In one example, the disposable sheath 34 extends 2.246 inches from the base 35 of the sheath/illuminator unit 24.

[0065] Interposed between the outer sheath 98 and the inner tube is the plurality of illumination fibers 108 which encircle the inner tube 100 as best seen in FIG. 7A and 7B. FIG. 7A is a sectional view through the base 35 of the disposable sheath 24. The outer sheath 98 is shown in the lower half of FIG. 7A and terminates prior to the portion sectioned in the upper half of FIG. 7A. The inner tube 100, however, which defines the airspace 102 to receive the elongated tube 28 of the imaging unit 22 extends to a receiving chamber 114 as seen in FIG. 6A and therefore is shown in both the upper and lower portions of FIG. 7A. The light is transmitted from the illumination pigtail 88 through fibers 108, as seen in FIG. 6A, to a transmission unit 118 as seen in the upper half of FIG. 7A which abuts the illumination fibers 108 located between the outer sheath 98 and the inner tube 100 of the disposable sheath 34 of the sheath/illuminator unit 24.

[0066] FIG. 7B shows the distal end 84 of the disposable sheath/illumination unit 24. The window 110 overlies and seals the airspace 102 that receives the imaging unit 22 and is encircled by the inner tube 100. Interposed between the outer sheath 98 and the inner tube 100 is the plurality of illumination fibers 108. In the embodiment shown, the distal end of the illumination fibers 108 are not protected and exposed to the body.

[0067] FIG. 8 is similar to FIG. 6A in that it shows the disposable sheath/illumination unit 24. In addition, FIG. 8 shows the entire illumination pigtail which is broken away in FIG. 6A.

[0068] The illumination pigtail 88 has a connection 38 for connecting to a connector on the light source 40. The illumination pigtail 88 has a plurality of optical fibers which run from the connection 38 to the fibers 108 which transmit the light received from the light source 40 to the transmission unit 118 shown in FIG. 7A and exit at 84.

[0069] Referring to FIG. 9, a sectional view of the imaging unit of the endoscope 20 is shown. The imaging unit 22 has the probe 29 with the elongated tube 28 that extends from the handle 32. At the proximal end of the handle 32, is the imaging device. In this embodiment, a charged coupled device (CCD) 30B which converts the optical image into an electrical image is carried in the detachable housing 120A of the handle 32. Interposed between the optical fiber or fibers 26 which extend in the elongated tube 28 and the CCD 30B is a plurality of lenses 122A for projecting the image of the proximal end 124 of the optical fiber or fibers 26 to the CCD 30B. The glass window 122B is attached to housing 120B and provides a seal to the scope. It also protects the lenses from contamination.

[0070] The imaging unit 22 enlarges the image from the end of the fiber optic 26 and couples it to the charged coupled device 30B. As indicated above, the charged coupled device is connected to a electronic storage and/or display device such as a computer 44 which is connected to a monitor 46 as seen in FIG. 1.

[0071] The handle 32 of the imaging unit 22 has a mounting mechanism 128 for coupling with the mounting mechanisms 36 of the sheath illuminator unit 24. The mounting mechanism 128 has slots 130 for receiving pins located on the mounting mechanisms 36. In addition, the mounting mechanism 128 has a projection 134, from which the probe 29 projects, that is received by the receiving chamber 114 of the sheath/illuminator unit 24 as seen in FIG. 6A.

[0072] An enlarged view of the distal end of the imaging unit 22 is shown in FIG. 10A. The rod tip 29 of the imaging unit 22 has the elongated tube 28 that extends from the distal end 126 to the housing 120 of the handle 32. At the distal end 126 of the rod tip 29 there is in addition a tube 138 which extends a slight distance from the distal end 126 and just a slight distance beyond the ends of the optical or image fibers 26. The tube 138 is commonly referred to as the long tube in that a shorter and smaller diameter tube 140 which is collinear with the long tube 138 is received within the long tube 138 and extends a lens system 142 at the distal end 126. The elongated or outer tube 128, long tube 138 and small tube 140 are mounted so that their distal ends are flush and are secured by an adhesive such as a medical grade epoxy. At the end of the elongated tube 28 of the imaging unit 22 is the lens system 142 that is described in further detail below. The elongated tube 28 of the imaging unit 22 is received within the disposable sheath/illumination unit 24 and therefore does not need to be sterilized prior to the first use.

[0073] FIG. 10B is an end-view of the distal end 126 of the imaging unit 22. The lens system 142, the small tube 140, the long tube 138 and the outer or elongated tube 28 are shown and are all collinear.

[0074] Referring to FIG. 11, a sectional view of the imaging unit 22 of the endoscope 20 is shown. The probe 29 of the imaging unit 22 has a plurality of fibers 146 for transmitting the image from the distal end 126 of the rod tip

29 to the handle 32. Encircling the fiber 146 at the distal end of the rod tip 29 is the long tube 138 for holding the fibers 146 of the image fibers 26 in position. The outer or elongated tube 28 encircles the long tube 138 and protects the fibers 146 of the image fibers 26 from their beginning near the distal end 126 of the rod tip 29 to the other end within the handle 32. There are typically thousands of fibers 146 as shown in FIG. 11 that are fused together. The loading of the image into them is done by the distal end lens system 142 which as described below arranges the light levels of the image in a relationship to the location of the image fiber bundle 26.

[0075] In addition, the fibers are in a disorder pack method. This disorder pack method limits transmission of images/light from one lens 142 to another as the image fiber bundle 26 extends from near the distal end 126 of the imaging unit 22 towards the proximal end of the fibers located within the handle 32. The disorder packing of fibers is achieved by varying the doping of the fibers, which is the area to be examined.

[0076] Referring to FIG. 12, a sectional view of the distal end of the rod tip 29 of the imaging unit 22 within the disposable sheath 34 of the sheath/illuminating unit 24 is shown. The disposable sheath 34 has the outer sheath 98 collinear with the inner tube 100. Interposed between the outer sheath 98 and the inner tube 100 is the plurality of illumination fibers 108 as best seen in FIG. 7B for illumination. At the distal end of the disposable sheath is the window that is secured, such as by cementing, to create a boundary to the air space or inner channel 102 that receives the rod tip 29 of the imaging unit 22. The imaging unit 22 has the elongated or outer tube 28 that extends from the distal end 126 to within the handle 32 as shown in FIG. 9. Located in the distal end 126 of the rod tip 29 are two additional tubes or sleeves, the shorter inner sleeve, referred to as the small tube 140, that retains and holds the lens

have a convex surface 156 that faces each other. The second lens 152, closer to the distal end 126, has a planar surface 158 which abuts the optical aperture stop 154. The aperture stop 154 and the lenses 150 and 152 are designed so that the sine of the maximum ray angle approaches the fibers at N.A. (numerical aperture).

[0078] The ray tracings 160 in FIG. 12 illustrate the projection of an image off the page to the right at the proper focal length and how this image is translated through the aperture stop 154 and through the lenses 152 and 150 to the plurality of fibers 146 in the image fibers 26. The lens system is non-telecentric.

[0079] Referring to FIG. 13 a graph of the sign of the maximum ray angle versus the normalized image height for three different lens systems including a prior art lens system is shown. As discussed below, the field of view is dependent upon the lens configuration. The graph in FIG. 13 shows a line for the maximum sign of a ray angle for a 50 degree lens system and a second line for a maximum sign of ray angle of a 70 degree lens system. In the 70 degree system, the maximum sign is approximately 0.32. Therefore, the N.A. (numerical aperture) of the fiber is approximately the same. In contrast, the 50 degree field of view system has an sign of a maximum ray angle of approximately 0.25. Therefore, the fibers have this numerical aperture. The system can provide a field of view at any selected level from 30-80 degrees, for example.

[0080] In one embodiment, the endoscope 20 has 10,000 fiber elements. In this embodiment, each fiber element 146 has a diameter of 4.4 microns. The overall diameter of the fiber 26 is 0.46 mounting mechanism. The elongated or outer tube 28 of the imaging unit is made from stainless steel. It is recognized, that the scope can be formed in many sizes, the following table is merely an illustration of various intervening size scopes.

	3k	10k	30k	50k	100k
Sheath/Illumination unit outer diameter	1-4 mm				
Imaging Unit rod tip outer diameter	0.5-3.5 mm				
No. of fiber elements	3,000	10,000	30,000	50,000	100,000
Fiber image diameter		0.46 mm	0.75 mm		
Fiber pixel size (individual fiber)	4.4 microns	4.4 microns	4.4 microns		
Lens Type	Achromatic or Selfoc Grin	Achromatic or Selfoc Grin	Achromatic	Achromatic	Achromatic
Depth of Field (DOF)		3 mm-20 mm			
Field of View (FOV)	Dependent on Lens 50°-70°				

elements of the distal lens system 142. A larger longer sleeve, referred to as the long tube 138, encircles the tube 140 and the beginning of the fibers 146 of the image fibers 26.

[0077] The distal lens system 142 as shown in FIG. 12 is an achromatic lens system having a pair of lenses 150 and 152 and an aperture stop 154. The lenses 150 and 152 each

[0081] As can be seen from table above, an alternative to an acromat lens described above with respect to FIG. 12 and 13 is a selfoc grin lens. FIG. 14 shown an alternative embodiment of the rod tip 29 of the imaging unit 22 of the endoscope 20 with a grin lens 168. The grin lens 168 as shown in FIG. 14 is a single element gradient index lens. The rod tip 29 of the image unit 22 as shown in FIG. 14 has

an elongated or outer tube **28** that extends from the distal end **126** to the handle **32**, not shown in FIG. **14**. In addition, similar to that of FIG. **10A**, a tube **138** extends a slight distance from the distal end **126**. This tube **138** is commonly referred to as the long tube, it extends just slightly beyond the ends of the optical image fibers **26**. In contrast to the embodiment shown in FIG. **10A** in that the lens **170** is a single lens there is no need for a small tube **140** for retaining the elements of a lens system.

[0082] The grin lens **168** in general does not provide as good of image quality as that of the acromat lens system **142** described above in that the image becomes less clear (i.e., blurry and distorted) towards the edge of the image. In addition, the color correction, changes in intensity as a function of wavelength, is not as good as in the acromat lens system. However, the GRIN lens system **168** maybe desirable in situations where cost is a higher factor than the overall image quality. In addition, because of the grin lens **170** being a single element lens the depth of fields may be limited. While only 2 different degrees of freedom are shown, it is recognized that lens systems with other fields of view can be made.

[0083] FIG. **15** is a sectional view of alternative endoscope **170**. In this embodiment of the endoscope **170**, the illuminator pigtail **172** is a part of the handle **174** of the imaging unit **176** and is therefore not part of a disposable sheath/illuminator unit **178**. An optical fiber bundle **180** is used for transmitting the illumination light from the pigtail **172** to a handle interface **182** in the handle **184** where the light is transferred to a light interface **184** on the sheath/illuminator unit **178** to transmit light from the handle **184** to the disposable sheath **186**.

[0084] FIG. **16A** is a sectional view showing the interface. FIG. **16A** is a sectional view of the base **188** of the disposable/sheath illuminator unit **178**. The upper portion of FIG. **16A** shows the drape **52** spaced from the base **188**. The base **188** has a light interface **184** that receives light from the handle interface **182** carried on the handle **174**.

[0085] In addition in the embodiment of the endoscope **170** shown in FIGS. **16A-16C**, the sheath/illuminator unit **178** has one of the illumination fibers **190** replaced by a tube or channel **192**. The tube **192** which is seen in FIGS. **15** and **16A-16C** is capable of receiving a laser fiber. The user passes a laser fiber through the tube **190** from the proximal end of the illumination unit **178** in the base **188** as seen in FIG. **15**, to the distal end of the illumination unit so that the user while viewing the image through the imaging fibers and CCD can complete a process using the laser fiber.

[0086] The lower half of FIG. **16A** shows a cross-sectional view through the base **188** of the sheath/illuminator unit **178** shows the tube **192** extending through the base into the annular ring containing the illumination fibers **190**. Similar to that shown in FIG. **7A**, FIG. **16A** shows an inner tube **194** around which the illumination fibers **190** are located. The inner tube **194** defines an airspace through which the probe **29** of the imaging unit **176** of the endoscope **170** passes.

[0087] FIG. **16B** is a sectional view of the disposable sheath **186** showing an outer tube **196** of the disposable sheath **186** and circling the illumination fibers **190** and a signal hypotube **192**. The inner tube **194** surrounds the airspace **102** which receives the probe **29** of the imaging unit

176. FIG. **16C** is an enlarged view showing the hypertube **192** with its opening to receive the laser fiber in the annular ray containing the illumination fibers **190** between the inner tube **194** and outer sheath **196**.

[0088] While FIGS. **15-16C** do not show a cannula **60**, it is recognized in most uses of the endoscope **20** or **170**, a cannula **60** can be used for extra protection of the endoscope **20** or **170**.

[0089] Referring to FIG. **17A**, a sectional view of an alternative endoscope **200** is shown. The endoscope **200** has an imaging unit **202** and a sheath unit **204**. In contrast to the previous embodiments, the sheath **204** that is disposable does not include any part of the illumination unit. Referring to FIG. **17A**, the illumination source **40** is connected to the handle **206** of the imaging unit **202** by an illumination pigtail **208** similar to that shown in FIG. **15**. But in contrast, there is no coupling such that that the light is transmitted to the disposable sheath **204**. Rather, as seen in FIG. **17A**, the illuminator pigtail **208** is a part of the handle **206** of the imaging unit **202**. An optical fiber **210** is used for transmitting the illumination light from the pigtail **208** to an interface **212** in the handle **206**. The interface **212** is located within the handle **206** and transfer the light to an annular ring **214** of a plurality of illumination fiber **216**.

[0090] Referring to FIG. **17B**, the probe **218** has an outer tube **220** and an inner tube **222**. Interposed between the tubes **220** and **222** is the annular space for receiving the plurality of illumination fibers **216**. Located in the inner tube **222**, which is similar to the elongated tube **28** in the first embodiment, is the image fiber bundle **26**. The fiber bundle **26** is spaced from the inner tube **222**. A long tube **224**, which extends for a slight distance from the distal end **126** to just beyond the ends of the image fiber bundle **26**, is interposed between the fibers **26** and the inner tube **222**.

[0091] In that the sheath is not required to carry illumination to the distal end of the rod tip **218** in the embodiment shown in FIGS. **17B**, the sheath **204** has a single outer layer **226**. A window curved to avoid retroreflection is secured to the distal end of the single outer layer **226**.

[0092] Referring to FIG. **18**, a two piece disposable sheath/illuminator unit **230** is shown. The endoscope has a first unit **232** of the two piece disposable sheath/illumination unit **230**, a mounting and cover unit **232**, that is mounted to the handle **32** of the imaging unit **22**. The mounting and cover unit **232** has a drape **52** that extends over the handle **32** of the imaging unit **22** and the illumination pigtail **88** when used. The drape **52** is retained on a disposable sleeve **234** to hold the drape **52** until positioned over the handle **32**. The second unit **236** of the disposable sheath/illumination unit **230**, a disposable sheath **236**, contains the elongated tube that covers the probe **29**. This second unit **236** has a mounting mechanism **238** to secure to the first unit **232**. It is therefore possible to remove the disposable sheath, the second unit, **236** and replace it with a new one while keeping the drape **52** that is mounted to the mounting and cover unit **232** over the handle.

[0093] FIG. **19** is a schematic of a control unit **250** for the endoscope. This control unit **250** has a power source output **252**, an input **254** for the image from the CCD and a light source **256**. In addition to a processing unit **260** for processing the image data, the unit has a recording device **258**

such as a CD writer to create a storable medium to retain data such as a baseline for the patient.

[0094] The endoscope is used as shown generally in the process sequence 270 of FIG. 20. The patient comes to the user/physician's office. The physician or technician uses a double gloved technique where two sterilized gloves are placed on each of the physician's hands. The physician takes the handle/illuminator unit which is not sterilized in one hand and secure the sterilized sheath/illuminator unit with the other hand. The physician then takes the lighting cord and secure the light cord to the pigtail on the disposable sheath/illuminator unit. The power and image output are likewise connected to the control unit. With the endoscope connected to the control unit, the drape portion of the sheath assembly is extended 272 over the handle and down the cords to such a length to provide a sterile field. With this completed, the physician takes off the first pair of gloves and is ready to begin the procedure.

[0095] After medicating the site, the cannula with the trocar is inserted into the body by a standard technique of probing with the physician's hand. Once the cannula is in position, the trocar is removed 274 and the tip of the endoscope is placed into the cannula. The endoscope is secured to the cannula using a screw or other attachment mechanism. The system is actuated 276 and video recording is initiated so that the physician is able to move the cannula in and out and around to position the probe for viewing of the desired site or a monitor. The physician can perform a procedure 278 at the site using other instruments such as a laser scalpel or cautery tool, or electrosurgical tool and/or the operative channel in the probe or sheath assembly. The entire examination or operative procedure can be recorded 280 on a video disk or other memory device. The procedure is concluded and the sheath assembly can be disposed 282 of and another sterile sheath assembly can be attached 284 to the probe for another procedure.

[0096] A preferred embodiment provides multi spectral imaging capability. This embodiment includes the use of a light source and a detector to provide images over the wavelength range of 700 nm-1200 nm. This allows the user to see through blood to observe tissue.

[0097] Another embodiment uses the ultraviolet (UV) region of the electromagnetic spectrum (10 nm-380 nm) to be able to treat tissue. Ultraviolet light in the range of 325-250 nm can pull together and cauterize. Lasers or conventional broadband light sources can be used to provide light to the illumination system. The imaging fiber bundle can also be used for illumination with a beam splitter in the handle to couple light from one or more sources individually or simultaneously to the fiber bundle.

[0098] Embodiments of the invention can be employed in office-based settings for performing diagnostic imaging of interior surfaces of a body. Office-based as used herein refers to locations other than essentially sterile environments such as, by way of example, hospital operating rooms, hospital procedure rooms, rooms proximate to sterilization means such as autoclaves, and the like. Examples of office locations are, but are not limited to, examination rooms at a physician's office, training rooms adjacent to locker rooms in sporting complexes, ambulances, residences, field hospitals, hospital corridors, examination rooms, emergency rooms, office buildings, stores, and the like.

[0099] On site sterilization of the entire miniature endoscope 20 is avoided by making all surfaces that directly contact a patient's skin in the vicinity of the insertion site disposable. The disposable portions are retained in sterile packaging until they are utilized for a single procedure. The use of disposable components allows the miniature endoscope 20 to be employed following accepted standards-of-care guidelines such as those used for routine arthrocentesis.

[0100] In addition, the miniature endoscope 20 operates as a fluidless system, although fluid can be used if desired. A fluidless system refers to the fact that no liquid media, irrigation or distention fluid (e.g., saline solution) has to be injected into a patient's body in the vicinity of the target area, i.e. the area that will be viewed using the invention. In other words, the miniature endoscope can simply be inserted through a patient's skin, and used to view a target area without requiring additional instruments, injection means, consumable substances and without generating excess hazardous waste, other than the disposable portion, such as would be generated if irrigation fluids were injected into and removed from the target area.

[0101] The disposable portion 20 may comprise a disposable needle covering employing a transparent window in its distal end. The transparent window prevents fluids from a patient's body from coming into contact with non-disposable portions (e.g., 32) of the system. Nondisposable portions operating in conjunction with the disposable portion 20 may include a thin shaft which slides inside the introducer and contains a fiber optic illumination system for conducting images of the target area to a miniature camera located in a handle 32. The fiber optic illumination system may comprise a protective window and high resolution fiber optics and lens transmission means for conveying images to the camera. The disposable portion may also include a slide port for introduction of surgical instruments or for evacuation of fluids by suction or for introduction of medications to the target area.

[0102] In an embodiment of the invention, a highly portable miniature endoscopic imaging system is provided. The system shown in FIG. 21 is man-portable, in that it can be transported or carried by a person. FIG. 21 illustrates exemplary embodiments of a portable endoscopic system 291 comprising, among other things, miniature endoscope 20, handle 32, imaging unit 22, cable 290 and laptop 292. In FIG. 21, the endoscopic unit and imaging unit 22 are connected directly to laptop 292 by way of cable 290. For example, imaging unit 22 may output a video signal that is sent to a video in jack on laptop 292. Laptop 292 is then used to enter patient information, session details, and is used to display real-time image data as the procedure is carried out.

[0103] An embodiment of the portable endoscopic system employs a personal computer memory card international association (PCMCIA) card for facilitating coupling of image data to laptop 292. PCMCIA card may be an industry standard card as known in the art, or it may be specially adapted for use with the miniature endoscope. A specially adapted PCMCIA card may include hardware for receiving and processing video signals received from the imaging unit. The output of PCMCIA card 294 may be an industry standard data format for conveying processed image data to a display associated with laptop.

[0104] A portable endoscopic system 291 that includes imaging unit or an interface box 32 and an interface box

cable 290 for conveying data to laptop 292. Interface box may include more sophisticated imaging, image processing, and data communication hardware and/or software than can be employed in PCMCIA card 294 or directly inside laptop 292. The interface box 296 may be configured to perform real-time image enhancement on data received through the distal end of miniature endoscope 20. Image enhancement may be used to produce images suitable for performing diagnostics while making use of less costly components in miniature endoscope 20. By way of example, a GRIN lens may be employed in miniature endoscope 20 to provide image data to interface box. Interface box may employ image processing algorithms for enhancing the image quality produced by the edges of GRIN lenses. Interface box may then convey image data to laptop 292 in an industry standard format by way of cable. The system can also include mounting on a cart 298 for transport, as display 295 and a light source system 296. The system can include a standard lamp for visible light imaging as well as infrared or ultraviolet light sources for imaging or treatment.

[0105] A generalized architecture can be used including a central processing unit (CPU), which is typically comprised of a microprocessor associated with random access memory (RAM) and read-only memory (ROM). Often, CPU is also provided with cache memory and programmable FlashROM. The interface between the microprocessor and the various types of CPU memory is often referred to as a local bus, but also may be a more generic or industry standard bus. CPU processes and interprets machine-readable, or function-executable, instructions associated with an operating system, user-developed applications, diagnostic tools, patient data hospital servers, health provider computers, and computers associated with remote experts. A graphical user interface (GUI) can be used for patient data entry and display as well as image viewing.

[0106] Many computing platforms are also provided with one or more storage drives, such as a hard-disk drives (HDD), floppy disk drives, compact disc drives (CD, CD-R, CD-RW, DVD, DVD-R, etc.), and proprietary disk and tape drives (e.g., Iomega Zip™ and Jaz™, etc.). Additionally, some storage drives may be accessible over a computer network such as network-based storage system. The RAM is capable of storing machine-readable instructions and information necessary to operate software applications for processing and displaying image data received from miniature endoscope.

[0107] Many computing platforms are provided with one or more communication interfaces, according to the function intended of the computing platform. For example, a personal computer, laptop, or belt-wearable computer is often provided with a high speed serial port (RS-232, RS-422, etc.), an enhanced parallel port (EPP), and one or more universal serial bus (USB) ports. The computing platform may also be provided with a local area network (LAN) interface, such as an Ethernet card, and other high-speed interfaces such as the High Performance Serial Bus IEEE-1394.

[0108] Computing platforms such as wireless telephones and wireless networked PDA's may also be provided with a radio frequency (RF) interface with antenna, as well. In some cases, the computing platform may be provided with an infrared data arrangement (IrDA) interface, too.

[0109] Computing platforms are often equipped with one or more internal expansion slots, such as Industry Standard

Architecture (ISA), Enhanced Industry Standard Architecture (EISA), Peripheral Component Interconnect (PCI), Personal Computer Memory Card International Association (PCMCIA), or proprietary interface slots for the addition of other hardware, such as sound cards, memory boards, and graphics accelerators.

[0110] Additionally, many units, such as laptop computers and PDA's, are provided with one or more external expansion slots allowing the user the ability to easily install and remove hardware expansion devices, such as PCMCIA cards, SmartMedia cards, and various proprietary modules such as removable hard drives, CD drives, and floppy drives.

[0111] Often, the storage drives, communication interfaces, internal expansion slots and external expansion slots are interconnected with the CPU via a standard or industry open bus architecture, such as ISA, EISA, or PCI.

[0112] A computing platform is usually provided with one or more user input devices, such as a keyboard or a keypad, and mouse or pointer device, and/or a touch-screen display. In the case of a personal computer, a full size keyboard is often provided along with a mouse or pointer device, such as a track ball or TrackPoint™. In the case of a web-enabled wireless telephone, a simple keypad may be provided with one or more function-specific keys. In the case of a PDA, a touch-screen is usually provided, often with handwriting recognition capabilities, and in the case of a laptop, a small keyboard and touch-sensitive display may be provided.

[0113] Additionally, a microphone, such as the microphone of a web-enabled wireless telephone or the microphone of a personal computer, is supplied with the computing platform. This microphone may be used for entering user choices, such as voice navigation of web sites, user menus associated with operating miniature endoscope 20, conveying data to remote locations, or auto-dialing telephone numbers. Voice recognition capabilities normally in the form of software may be employed for facilitating speech based interaction with the computer.

[0114] Many computing platforms are also equipped with a camera device, such as a still digital camera or full motion video digital camera which can be used for facilitating collaboration between the person performing the endoscopic procedure and a remote expert that may be guiding the procedure and interpreting results in essentially real-time by way of a networked display device.

[0115] One or more user output devices, such as a display, are also provided with most computing platforms. The display may take many forms, including a Cathode Ray Tube (CRT), a Thin Flat Transistor (TFT) array, a simple set of light emitting diodes (LED), liquid crystal display (LCD) indicators, a heads-up (i.e. hands free) display, or a projection display.

[0116] One or more speakers and/or annunciators are often associated with computing platforms, too. The speakers may be used to reproduce audio instructions. Annunciators may take the form of simple beep emitters or buzzers, commonly found on certain devices such as PDAs and PIMs. Annunciators may be used to alert the operator of system that an error has occurred. These user input and output devices may be directly interconnected to the CPU via a proprietary bus structure and/or interfaces, or they may be interconnected through one or more industry open buses such as ISA, EISA,

PCI, etc. The computing platform is also provided with one or more software and firmware programs to implement the desired functionality of the computing platforms.

[0117] A generalized organization of software and firmware on this range of computing platforms. One or more operating system (OS) native application programs may be provided on the computing platform, such as word processors, spreadsheets, contact management utilities, address book, calendar, email client, patient tracking, user menus for operating system, etc. Additionally, one or more portable or device-independent programs may be provided, which must be interpreted by an OS-native platform-specific interpreter, such as Java™ scripts and programs.

[0118] Often, computing platforms are also provided with a form of web browser or micro-browser, which may also include one or more extensions to the browser such as browser plug-ins and configured to facilitate transmission and reception of image data over network.

[0119] The computing device is often provided with an operating system, such as Microsoft Windows™, UNIX®, IBM OS/2™, or AIX®, LINUX, MAC OS™, Sun Solaris™, or other platform specific operating systems. Smaller devices such as PDA's and wireless telephones may be equipped with other forms of operating systems such as real-time operating systems (RTOS) or Palm Computing's PalmOS™.

[0120] A set of basic input and output functions (BIOS) and hardware device drivers 356 are often provided to allow the operating system and programs to interface to and control the specific hardware functions provided with the computing platform. Additionally, one or more embedded firmware programs 358 are commonly provided with many computing platforms, which are executed by onboard or "embedded" microprocessors as part of the peripheral device, such as a microcontroller or a hard drive, a communication processor, network interface card, or sound or graphics card.

[0121] Various hardware components, software and firmware programs of a wide variety of computing platforms, including but not limited to personal computers, laptops, workstations, servers, web-enabled telephones, and other like appliances can be used. It will be readily recognized by those skilled in the art that the following methods and processes may be alternatively realized as hardware functions, in part or in whole, without departing from the spirit and scope of the invention.

[0122] An exemplary system uses portable system operating in conjunction with a network. A doctor's office containing portable system, a network, a health insurance provider having data storage associated therewith, a hospital server having data storage, a remote expert computer and a network-based storage system.

[0123] The doctor's office employs portable system for performing diagnostic evaluations of one or more patients. Image data obtained from a session may be stored on laptop and conveyed to one or more remote locations by way of network. Network may be any type of network running any kind of network protocol. By way of example, network may be an intranet such as a local area network (LAN) operating within a corporate location or university campus, a metropolitan area network (MAN) operating within a geographic

region such as a city and its surrounding suburbs, or a wide area network (WAN) such as the world wide web. In addition, network may run any type of networking protocol such as, for example, transmission control protocol and Internet protocol (TCP/IP), asynchronous transfer mode (ATM), synchronous optical network (Sonet), frame relay, integrated services digital network (ISDN), open shortest path first (OSPF), etc. Network may employ a plurality of links for coupling network elements and locations. Links may be comprised of hardwired links and/or wireless links. Examples of hardwired links are, but are not limited to, coaxial cable, twisted pair cable, optical fibers, etc.; and examples of wireless links are, but are not limited to, radio frequency (RF) such as IEEE 802.11 based links, or free space optical links. Network may also comprise gateways and/or firewalls for providing access to network and for providing protection against undesirable network traffic such as denial-of-service attacks as well as network traffic containing malicious code such as computer worms and viruses.

[0124] Data conveyed from portable system to network may be directed to a health insurance provider. The health insurance provider may archive received data on data storage by way of link for future use. Health insurance provider may employ its own experts, alone or in combination with automated analysis systems, to review data obtained during an endoscopic procedure using the invention. Portable system may also convey data to a hospital server. The hospital server may further include data storage coupled thereto by link. Hospital server may serve as a pooling resource for maintaining data associated with patients having an affiliation therewith. By way of example, if a patient required surgery based on a diagnosis obtained using portable system, the image data could be reviewed by a surgeon prior to, or during, surgery to ensure that proper and complete treatment is rendered in an efficient manner.

[0125] Data obtained using portable system may further be sent to a remote expert computer by way of network. A remote expert, using remote expert computer, may review image data post mortem or in quasi-real-time. The remote expert may provide a second opinion prior to scheduling more invasive procedures or the remote expert may provide the primary diagnosis in situations where a skilled operator is performing the procedure with miniature endoscope 20. For example, disaster relief personnel may be on scene at a remote location and performing a diagnostic procedure on a disaster victim. A remote expert may be viewing image data received over a free space satellite network in real-time to direct the on-scene personnel with respect to the diagnostic procedure. The remote expert may then direct an on-scene person to mark an insertion location on a victim/patient, to introduce the needle covering, to maneuver the endoscope 20, and then may use real-time data to recommend accurate treatment for the victim without having to be on site. Data from portable system may further be conveyed to network-based storage system. Network-based storage system may serve as secure and redundant storage for image data resident on laptop. In addition, network-based storage system may serve to keep image data in a location that is more readily accessed for replay than if the data were kept solely on laptop. The system and other remote entities may be communicated with using portable system without departing from the spirit of the invention.

[0126] A preferred method for using the miniature endoscope 20 in conjunction with portable system to perform diagnostic procedures. In which the transport by cart into an examination room or other site where the procedure will be performed. Then a camera is coupled to the viewing system. Next, an insertion site is prepared on a patient's body. Preparation of the insertion site may include, among other things, marking the site using a medically approved writing instrument, cleansing the area with an antiseptic solution, etc. A disposable needle covering may be coupled to the imaging and viewing system. As previously discussed herein, only disposable portions of miniature endoscope 20 contact the patient so no special sterilization processes need be applied on site. The needle covering of miniature endoscope 20 is then inserted into a target area of a patient. After the needle point is in the vicinity of the target, the imaging and viewing system may be activated. Image data is viewed and recorded using laptop during the diagnostic procedure. When the diagnosis is complete, the needle is withdrawn from the target area. After needle withdrawal, the insertion location may be dressed using sutures, liquid adhesives approved for topical wound dressing, butterfly closures, or conventional small wound dressings such as gauze or bandages.

[0127] Recorded image data can be reviewed by the diagnostician and shown to the patient in the procedure room. After review, recorded data can be archived locally on laptop, on removable storage media, or by way of network-based storage system. In addition, image data long with alphanumeric and/or voice annotations may be sent to one or more remote locations using network. Then the portable system may be returned to its storage location, and the patient immediately discharged after the procedure, since no complex anesthesia was required.

[0128] While exemplary embodiments of the invention have been described and illustrated hereinabove, the invention is not limited thereto. Many alternative embodiments and implementations are possible in light of the disclosure without departing from the spirit of the invention. For example, the portable system may be deployed in a distributed architecture where the user is located at a first geographic location, with a patient and the miniature endoscope comprising elements 20, 21 and 22 while the laptop display is located a distance away and is coupled to the miniature endoscope by way of a wireless network. In another alternative embodiment, the invention may be deployed in a ruggedized configuration for use in battlefield triage and/or for responding to disasters in remote and rugged locations. In still other embodiments, the portable endoscopic system may be integrated into mechanized conveyances such as trains, ambulances, air planes, ships, vehicles, etc. In yet other embodiments, images generated using the portable endoscopic system may be replayed and used for training purposes. In still further embodiments, the portable endoscopic system may comprise a belt-wearable computer having a short range high bandwidth link to handle for receiving image data. In this embodiment, handle may comprise a self-contained power source such as a rechargeable battery. This embodiment may further utilize a heads-up display worn on a user's head. Such a configuration provides the user with maximum mobility and minimum weight. The belt-wearable embodiment may further communicate with network by way of a wireless link.

[0129] In yet another alternative embodiment, laptop can be replaced with a customized processing device that can take on essentially any form factor and user interface configuration. For example, it may be desirable to have a dedicated processing module having only an on/off switch. When switched on, the customized processing device may gather image data and store it for later review or it may automatically transmit data to a remote location using a wireless RF or free space optical link.

[0130] FIG. 22 illustrates another preferred embodiment of a portable endoscope 400 in accordance with the invention including a handle 402 having a camera module 404, an optical coupler 406, a processor 408, a wireless communications module 410, a wireless antenna 412, a battery 414 and a power regulator 416. Also included in the portable system is a light source 418 within handle 402. The light source 418 preferably comprises an LED assembly such as an EOSTTMLED fiber optic illuminator available from Edmund Optics, Barrington, N.J. The light source can also comprise one or more laser diodes or a combination of laser diodes and LEDs, a laser or laser diode in the ultraviolet portion of the spectrum can be used to induce fluorescence in tissue for diagnostic purposes or for cautery. The handle can have a control panel 409 with buttons that the user employs to electrically operate the handle.

[0131] The camera 404 can a CCD or CMOS imaging sensor such as the TC7040 two megapixel CMOS imaging sensor device available from TransChip Israel Research Center, Ltd. This device includes a 1600×1200 pixel color sensor array that is packaged with a clock, controller, image processor and local SRAM memory in a single chip package. The camera preferably has sensitivity in the infrared portion of the spectrum (750-1000 nm) as well as the visible. For certain applications it is preferable to use an infrared imaging sensor that can detect light in the range of 1500 nm to 1900 nm, for example, as this improves imaging of tissue through blood. An infrared light source as well as spectral or cutoff filters 407 for the detector may be needed for certain spectral imaging applications.

[0132] The disposable 420 as described previously herein has a port 422 for coupling light from the light source into the fiber optic illumination bundle within the coupler 424 of the disposable. The distal end of the sheath can have a cutting element 425 that can be recessed during insertion and imaging and mechanically actuated by wire or other means to cut a tissue sample from a region of interest within the body.

[0133] The handle 402 can also include a bar code reader 442 or other device that uniquely identifies the disposable component being attached thereto. The bar code 440 can be imprinted on the proximal end of the disposable coupler 424 shown in FIG. 23. This bar code can have a radial or rectangular array. A radial array can be scanned past the reader 442 while the coupler 424 rotates into the locked position with the handle 402. Alternatively some other electronic identifying and recording device such as a radio frequency identification (RFID) system can be used or a chip with a serial number can be in the disposable. This can be used for safety and record/inventory purposes.

[0134] The wireless module provides for delivery of video from the handle to a receiver in communication with a desktop or laptop computer. A cable 405 can also optionally

be connected to the handle **402** to provide a connection to the computer and associated display. A display **450** can also be integrated directly into the handle **402** for viewing by the user. The video or still images taken with the camera can also be recorded onto removable media such as a compact flash card, CD, DVD, mini DVD or SD card. Compact media can be inserted into a slot in the handle **402**.

[0135] For certain applications it can be desirable to use the imaging waveguide to deliver light onto the tissue as well. A beam splitter within the handle can be used for this purpose as described previously.

[0136] The handle **402** can also be configured to dock with a base unit **460** that can transmit and receive images and data from the processor **408** with a transceiver **462**. The base **460** can also be used as a recharger for the battery **414** and can include a communications circuit for a network or internet connection, a facsimile device or standard telephone data connection.

[0137] The disposable can also include a lens at the distal end, or a prism or mirror for side-viewing applications. The disposable can have a length of between 20 mm and 2500 mm depending on the application. For small joints or bones such as the hand or foot smaller lengths are used. For applications such as the hip, longer lengths up to 2500 mm may be used. For imaging applications such as the breast or brain, imaging in the visible portion of the spectrum can be supplemented by imaging in the near infrared or infrared portions of the spectrum. This can be used to supplement mammographic screening. A biopsy can also be used to collect a tissue sample, if needed. Dyes or tissue autofluorescence can also be used with a narrowband light source such as a laser diode emitting at a wavelength in a range of 300 nm to 500 nm, for example. Gallium nitride diode lasers can be used for this purpose.

[0138] FIG. 24A shows a preferred embodiment in which the illumination fibers **502** are rigidly attached to the handle **500**. The disposable **510** is connected with connector **512** to the handle and can include a lens **520** or a mirror or prism **540** for angled or side viewing. A cross-sectional side view of such an embodiment is illustrated in FIG. 24B which is also seen in the sectional view of FIG. 17B. This embodiment employs a distal window **560** on the end of the disposable sheath **204** that is fluidly sealed to the sheath. In this embodiment the window has an outer transparent element or illumination window **562** that transmits the illuminating light from the fibers **216** in a distal direction as shown by light rays **217**, **219**. The window **560** can have a separate inner element or light collection window **564** which receives light returning from the illuminated region of interest. The outer and inner window elements are optically decoupled by a light barrier **566** that can be a stainless steel spacer that is attached to both the outer and inner elements **562**, **564** using an adhesive, for example. The imaging fibers **26** receive light collected through element **564** and focused by lens system **225** onto the imaging fibers generally along longitudinal axis **565**.

[0139] FIG. 25 illustrates an embodiment in which a beam splitter **554** in the handle **550** optically couples both the light source **552** and the imaging device **556** to a single fiber bundle. This provides for illumination and light collection through a single light channel. The light source can be LED source and/or a laser as described previously herein.

[0140] Many changes in the details, materials and arrangements of parts, herein described and illustrated, can be made by those skilled in the art in light of teachings contained hereinabove. Accordingly, it will be understood that the following claims are not to be limited to the embodiments disclosed herein and can include practices other than those specifically described, and are to be interpreted as broadly as allowed under the law.

What is claimed:

1. A fiber optic probe for viewing within a mammalian body comprising:

a handle having an image device, an optical coupler and a connector; and

a disposable sheath that encloses a fiber optic device, the sheath being connected to the handle with the connector and having a diameter of less than 3 mm.

2. The fiber optic probe of claim 1 further comprising a battery within the handle.

3. The fiber optic probe of claim 1 further comprising a processor connected to the imaging device.

4. The fiber optic probe of claim 1 further comprising a light source within the handle.

5. The fiber optic probe of claim 4 wherein the light source comprises a light emitting diode (LED).

6. The fiber optic probe of claim 5 further comprising red, green and blue light emitting diodes.

7. The fiber optic probe of claim 4 wherein the light source comprises a laser.

8. The fiber optic probe of claim 7 wherein the laser comprises a gallium nitride diode laser.

9. The fiber optic probe of claim 1 further comprising a wireless transmitter that transmits video images to a control unit.

10. The fiber optic probe of claim 9, further comprises a wireless transmitter circuit module and an antenna.

11. The fiber optic device of claim 1 further comprising a wireless receiver.

12. The fiber optic device of claim 2 further comprising of power regulation circuit connected to the battery, a light source, a processor and the imaging devices.

13. The fiber optic device of claim 1 wherein the disposable sheath comprises a concentric fiber array having a diameter less than 2 mm.

14. The fiber optic device of claim 1 wherein the fiber optic device comprising an imaging fiber bundle that is rigidly connected to the handle, a proximal end of the imaging fiber bundle being optically coupled to the optical coupler.

15. The fiber optic probe of claim 14 further comprising a lens at a distal end of the imaging fiber bundle.

16. The fiber optic probe of claim 1 wherein the disposable sheath is detachably connected to the handle and the fiber optic device.

17. The fiber optic device of claim 1 wherein the disposable sheath includes the fiber optic device that is detachable from the handle.

18. The fiber optic device of claim 17 wherein the detachable fiber optic device comprises an imaging bundle and an illumination fiber optic device connected to a light source.

19. The fiber optic device of claim 1 wherein the sheath is insertable into a body lumen without a distending fluid.

20. The fiber optic device of claim 1 further comprising a base unit that is connectable to the handle.

21. The fiber optic device of claim 20 wherein the handle locks with the base unit such that the handle is electrically connected to the base unit.

22. The fiber optic device of claim 20 wherein the base unit comprises a battery charger.

23. The fiber optic device of claim 20 wherein the base unit comprises a network connection.

24. The fiber optic device of claim 20 wherein the base unit comprises a transmitter.

25. The fiber optic device of claim 20 wherein the base unit is connected to a facsimile device.

26. The fiber optic device of claim 20 wherein the base unit is connected to a computer.

27. The fiber optic device of claim 1 further comprising a cable connecting the handle to a computer.

28. The fiber optic probe of claim 9 wherein the control unit comprises a computer.

29. The fiber optic device of claim 28 wherein the computer comprises a laptop computer and a display.

30. The fiber optic device of claim 1 wherein the imaging device comprises a CMOS imaging device.

31. The fiber optic device of claim 1 wherein the imaging device detects light in a range of 300 nm to 1900 nm.

32. The fiber optic device of claim 1 further comprising an identification circuit that identifies the sheath.

33. The fiber optic device of claim 32 wherein the identification circuit comprises a bar code reader that reads a bar code on the sheath.

34. The fiber optic device of claim 32 wherein the identification circuit comprises a radio frequency identification system.

35. The fiber optic probe of claim 32 wherein the identification circuit is on the handle.

36. The fiber optic probe of claim 32 wherein the sheath comprises an electronic identifier.

37. The fiber optic probe of claim 32 wherein the sheath has a serial number.

38. The fiber optic probe of claim 1 further comprising a light source that induces fluorescence in tissue that is detected with the imaging device.

39. The fiber optic probe of claim 1 wherein the imaging device detects infrared light in a range of 700 nm to 1000 nm.

40. The fiber optic device of claim 1 further comprising a cart for transport of a computer display and the probe.

41. The fiber optic device of claim 1 further comprising an achromatic lens at a distal end of the fiber optic device.

42. The fiber optic device of claim 1 wherein the imaging device detects light in a visible and a near infrared range.

43. The fiber optic device of claim 1 further comprising a cutting element to collect tissue sample.

44. The fiber optic device of claim 1 wherein the sheath includes a lens, a mirror or a prism at a distal end for side viewing.

45. The fiber optic device of claim 1 wherein the sheath is between 50 mm and 2500 mm in length.

46. The fiber optic device of claim 1 further comprising a fluid delivery channel for delivering medication or imaging dye to a region of interest in a body lumen or cavity.

47. The fiber optic device of claim 1 further comprising a display device on the handle.

48. The fiber optic device of claim 1 further comprising a control panel on the handle.

49. The fiber optic device of claim 1 further comprising a spectral filter coupled to the imaging device.

50. A method of performing body imaging comprising:

providing a handle having an imaging device;

attaching the handle to a disposable sheath, the sheath enclosing a fiber optic imaging device;

inserting the sheath into the patient; and

viewing a site within the patient without insertion of a fluid at the site.

51. The method of claim 50 further comprising providing an illumination source having a wavelength in the range of 700 nm-1200 nm.

52. The method of claim 50 further comprising providing a light source having a wavelength in a range of 10 nm to 380 nm to treat tissue in the patient.

53. The method of claim 50 further comprising providing a cart for transport of a system including a computer, a display, and a probe storage.

54. The method of claim 50 further comprising providing a laptop computer having a graphical user interface to display one or more images and enter patient data.

55. The method of claim 50 further comprising providing a light source in the handle.

56. The method of claim 50 further comprising viewing the site without a distending fluid

57. The method of claim 55 wherein the light source comprises an LED array.

58. The method of claim 50 further comprising transmitting image data from the handle to a computer with a wireless connection.

59. The method of claim 50 further comprising locking the handle with a base having a battery charger.

60. The method of claim 50 further comprising providing a battery, a processor, a wireless transmitter and a light source in the handle, the light source being coupled to a fiber optic array in the sheath.

61. A fiber optic probe for viewing within a mammalian body comprising:

a handle having an imaging device, an optical coupler that optically couples a fiber optic imaging channel to the imaging device, a fiber optic illumination channel, and a connector; and

a disposable sheath that encloses the fiber optic imaging channel, the sheath being connected to the handle with the connector and having a diameter of less than 3 mm the sheath further comprising a distal window.

62. The fiber optic probe of claim 61 further comprising a battery within the handle.

63. The fiber optic probe of claim 61 further comprising a processor connected to the imaging device.

64. The fiber optic probe of claim 61 further comprising a light source within the handle.

65. The fiber optic probe of claim 64 wherein the light source comprises a light emitting diode (LED).

66. The fiber optic probe of claim 61 wherein the window further comprises an illumination window and a light collection window.

67. The fiber optic probe of claim 66 wherein the illumination window is optically decoupled from the collection window.

68. The fiber optic probe of claim 67 wherein the sheath is fluidly sealed to the window.

69. The fiber optic probe of claim 68 wherein the collection window is decoupled from the illumination window with an optical barrier.

70. The fiber optic probe of claim 69 wherein the optical barrier comprises a spacer attached with an adhesive.

* * * * *