



## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 5 :  A61F 2/06	A1	(11) International Publication Number: WO 93/22986 (43) International Publication Date: 25 November 1993 (25.11.93)
---	----	--

(21) International Application Number: PCT/US93/01966

(22) International Filing Date: 10 March 1993 (10.03.93)

(30) Priority data:  
880,435 8 May 1992 (08.05.92) US

(71) Applicant: SCHNEIDER (USA) INC. [US/US]; 5905 Nathan Lane, Plymouth, MN 55442 (US).


(72) Inventors: JOHNSON, Liann, M. ; 8335 Patsy Lane, Minneapolis, MN 55427 (US). THOMPSON, Richard, J. ; 804 Southview Street Southeast, Watertown, MN 55388 (US). SCHOLL, John, A. ; 427 Orchard Court, Danville, CA 94526 (US).

(74) Agents: RICHARDSON, Peter, C. et al.; Pfizer Inc., 235 East 42nd Street, New York, NY 10017 (US).

(81) Designated States: AU, CA, DE (Utility model), JP, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).

Published  
With international search report.

(54) Title: ESOPHAGEAL STENT AND DELIVERY TOOL

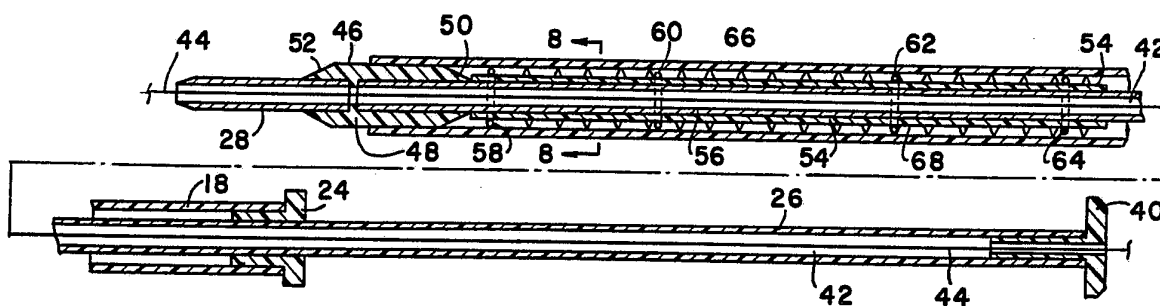

## (57) Abstract

A radially self-expanding stent (90) particularly suited for treating esophageal strictures, includes a medial region (92) and proximal and distal cuffs (94, 96) having diameters greater than the medial region (92) diameter when the stent (90) is in the relaxed state. A silicone coating circumscribes the medial region (92), but the cuffs (94, 96) are not coated and retain their open weave construction. As a result, the cuffs (94, 96) remain particularly well suited to immediately contact esophageal wall tissue and resist stent migration, while the silicone coated medial region (92) provides a barrier to tumor ingrowth, and has an enhanced radial restoring force to maintain an open passageway in the esophagus. A deployment device (16) for the stent (90) includes an interior catheter (26) surrounded by the stent (90) and having an esophageal dilation feature (28), along with an exterior catheter (18) that radially compresses the stent (90). A low durometer sleeve (54), fixed to the interior tube (26) and in surface engagement with the compressed stent (90), tends to fix the axial position of the stent (90) relative to the interior catheter (26) whenever the exterior catheter (18) is moved axially relative to the inner catheter (26). Consequently, precision in stent placement and the ability to recapture a partially deployed stent are enhanced.

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	FR	France	MR	Mauritania
AU	Australia	GA	Gabon	MW	Malawi
BB	Barbados	GB	United Kingdom	NL	Netherlands
BE	Belgium	GN	Guinea	NO	Norway
BF	Burkina Faso	GR	Greece	NZ	New Zealand
BG	Bulgaria	HU	Hungary	PL	Poland
BJ	Benin	IE	Ireland	PT	Portugal
BR	Brazil	IT	Italy	RO	Romania
CA	Canada	JP	Japan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SK	Slovak Republic
CI	Côte d'Ivoire	LJ	Liechtenstein	SN	Senegal
CM	Cameroon	LK	Sri Lanka	SU	Soviet Union
CS	Czechoslovakia	LU	Luxembourg	TD	Chad
CZ	Czech Republic	MC	Monaco	TG	Togo
DE	Germany	MG	Madagascar	UA	Ukraine
DK	Denmark	ML	Mali	US	United States of America
ES	Spain	MN	Mongolia	VN	Viet Nam
FI	Finland				

-1-

**ESOPHAGEAL STENT AND DELIVERY TOOL****BACKGROUND OF THE INVENTION**

The present invention relates to body implantable treatment devices, and more particularly to stents and other prostheses intended for fixation in body lumens especially including the esophagus.

Carcinomas in the esophagus lead to progressive dysphagia, i.e. difficulty in swallowing, and the inability to swallow liquids in the most severe cases. While surgical removal is sometimes effective, the majority of patients have tumors that can not be surgically removed. Repeated dilations of the esophagus provide only temporary relief.

Difficult or refractory cases often are treated by intubation using rigid plastic prostheses, or laser therapy with an Nd:YAG laser. These techniques, while often effective, have disadvantages. Rigid plastic prostheses are large, for example having a diameter of 10-12 mm and larger (25-29 mm) outer end flanges. Placement of rigid plastic stents is traumatic, and too frequently causes perforation of the esophageal wall. These prostheses further are subject to migration, obstruction with food or tumor ingrowth, and late pressure necrosis.

Laser therapy is expensive, typically requiring several treatment sessions. Tumor recurrence is frequent, in the range of 30-40 percent. Submucosal tumors, and certain pulmonary and breast tumors causing dysphagia by esophageal compression, can not be treated by laser therapy.

The search for a more suitable prosthesis has lead to experiments with Gianturco stents, also known as Z-stents. U.S. Patent No. 4,800,882 (Gianturco)

-2-

describes such a device employed as an endovascular stent. Such stents for the esophagus have been constructed of 0.018 inch stainless steel wire, and provided with a silicone cover to inhibit tumor  
5 ingrowth. It was found necessary, however, to provide a distal silicone bumper to prevent trauma to the esophageal mucosa.

Self-expanding mesh stents also have been considered for use as esophageal prostheses. U.S.  
10 Patent No. 4,655,771 (Wallsten) discloses a mesh stent as a flexible tubular braided structure formed of helically wound thread elements. Mesh stents appear unlikely to lead to pressure necrosis of the esophageal wall. With its inherent pliability the  
15 mesh stent, as compared to a rigid plastic stent, is insertable with much less trauma to the patient. Further, the stent can mold itself to and firmly fix itself against the esophageal wall, to resist migration. However, the stent is subject to tumor  
20 ingrowth because of the spaces between adjacent filaments.

A further difficulty with self-expanding stents, concerns their accurate placement and deployment. Typically a tube surrounds the self-expanding stent  
25 and radially compresses the stent into a reduced-radius delivery configuration. With the stent positioned at a treatment site, the outer tube is axially withdrawn, permitting the stent to radially self-expand. However, the larger size of an  
30 esophageal stent (as compared to biliary and vascular applications, for example) gives rise to substantial friction at the stent/outer tubing interface. As a result, it is difficult to precisely maintain the position of the stent during deployment, and

-3-

practically impossible to retract the stent after partial deployment.

Therefore, it is an object of the present invention to provide a stent delivery device  
5 including exterior tubing surrounding the stent and movable axially to release the stent for radial self-expansion without a tendency in the stent to follow the axial movement of the exterior tubing.

Another object is to provide a stent deployment  
10 device capable of retracting a radially self-expanding stent for repositioning of the stent, even though the stent has been partially deployed and is radially expanded over the majority of its axial length.

15 Another object is to provide a device for delivering and deploying a prostheses to a treatment site within a body lumen, with means for dilating the body lumen at the treatment site prior to stent deployment.

20 A further object of the invention is to provide a radially self-expanding stent including a freely radially self-expanding fixation region in combination with a barrier region to inhibit tumor ingrowth.

25 Yet another object is to provide an esophageal prostheses deployable with reduced trauma to the patient, having more resistance to migration, and providing a barrier to tumor ingrowth as effective as conventional rigid plastic prostheses.

30 To achieve these and other objects, there is provided an apparatus for deploying a radially self-expanding stent within a body lumen. The apparatus includes a stent confining means for elastically compressing a radially self-expanding stent into a

-4-

delivery configuration in which the self-expanding stent has a reduced radius along its entire axial length. The apparatus includes an elongate and flexible stent delivery device having a proximal end, a distal end and a distal region near the distal end. The distal region is used in delivering the radially self-expanding stent into a body lumen, and in positioning at a treatment site within the body lumen with the stent surrounding the delivery device along the distal region. The proximal end of the delivery device remains outside of the body. An axial restraining means is disposed along the distal region of the delivery device. A control means is operably associated with the delivery device and the confining means. The control means moves the confining means axially relative to the delivery device toward and away from a confinement position in which the confining means compresses the self-expanding stent into the delivery configuration, and urges the stent into a surface engagement with the axial restraining means. The restraining means, due to the surface engagement, tends to maintain the self-expanding stent axially aligned with the deployment device as the confining means is moved axially away from the confinement position to release the stent for radial self-expansion.

Preferably the stent delivery device is an elongate and flexible length of interior tubing, with a central lumen for accommodating a guidewire. The stent confining means can be an elongate and flexible length of tubing, having a lumen for containing the interior tubing. The second (or outer) tubing surrounds the stent to confine it.

-5-

The preferred axial restraining means is a low durometer sleeve surrounding the interior tubing along the distal region. If desired, an adhesive can be applied to an exterior surface of the sleeve.

- 5 Alternatively, the axial restraining means can consist of several elongate strips disposed along the distal region, with adhesive applied to radially outward surfaces of the strips, if desired.

10 In either event, so long as the exterior tubing surrounds the stent to radially compress the stent, it also maintains the stent in surface engagement with the sleeve or strips. As the exterior tubing is axially withdrawn to allow part of the stent to radially self-expand, the rest of the stent remains  
15 confined against the sleeve or the strips. As a result, the stent does not travel axially with the exterior tubing. Rather, the stent remains substantially fixed in the axial direction with respect to the interior tubing. This structure  
20 affords several advantages. First, the interior tubing can be used as a means to positively maintain the radially self-expanding stent in the desired axial position during deployment. The interior tubing can itself be employed as a reliable indicator  
25 of stent position, both prior to and during deployment. Further, should the need arise to retract the stent after a partial deployment, the outer tubing can be moved back into the confinement position, without tending to carry the stent along  
30 with it.

Another aspect of the present invention is a device for fixation in a body lumen. The device includes a tubular stent of open weave construction having a predetermined normal configuration. The

-6-

stent is radially compressible to a reduced-radius configuration to facilitate an axial insertion of the stent into a body lumen for delivery to a treatment site within the body lumen. A continuous film is  
5 formed axially along the stent and circumscribes the stent over a barrier region of the stent. The continuous film substantially prevents growth of tissue through the stent along the barrier region. A portion of the stent is substantially free of the  
10 continuous film to provide a fixation region of the stent for positively fixing the stent within the body lumen at the treatment site. Fixation is achieved by radial expansion of the stent into a surface engagement with a tissue wall segment defining the  
15 body lumen.

The preferred stent comprises a mesh formed of braided helical strands. The fixation region can comprise a proximal cuff and a distal cuff, with the barrier region being a medial sleeve of the stent  
20 positioned between the cuffs. Also, the barrier region preferably has a diameter less than the fixation region diameter when the stent is in its normal or relaxed configuration. A preferred material for the film is silicone. When properly  
25 controlled as to thickness, the silicone film provides a gradual self-expansion. More particularly, while the fixation region self-expands virtually instantaneously upon release of the stent, the medial barrier region, upon encountering a tumor  
30 or other stricture, can take up to 24 hours to achieve a substantially complete radial self-expansion against the tumor.

This feature is particularly advantageous in connection with treating esophageal strictures, where



-7-

tissue at the stricture may be severely weakened, and where normal convulsions of the esophagus tend to cause stent migration. More particularly, the rapidly expanding fixation regions contact normal esophageal tissue on either side of a stricture, and are sufficiently pliable to adjust to esophageal convulsions. Meanwhile, the barrier region of the stent experiences a gradual radial expansion, thus causing minimal disruption to tissue along the stricture.

A further feature of the invention is a system for treating a stricture within a body lumen. The system includes a radially self-expanding stent, and an elongate and flexible stent delivery device having a proximal end and distal end. The device further has a distal region for delivering the radially self-expanding stent into the body lumen and positioning the stent at a treatment site within the body lumen, with the stent surrounding the delivery device along the distal region. A first elongate and flexible length of tubing, having a lumen running the length of thereof, contains the stent delivery device within the lumen. The first tubing also elastically compresses the stent into a delivery configuration in which the stent has a reduced radius along its entire axial length. The first tubing is movable proximally relative to the delivery device and the stent, to allow the stent to radially self-expand into a surface engagement with body tissue defining the lumen. A distal tip is provided at the distal end of the stent delivery device for initially dilating a stricture at the treatment site. An enlargement feature is provided near the distal end of the stent delivery device. The enlargement feature has a

-8-

diameter substantially equal to an interior diameter of the first tubing. The enlargement feature further has a distal transition region that diverges proximally from the tip to a mid-portion of the enlargement feature. The transition region further dilates the stricture to facilitate a positioning of the distal region of the first tubing along the stricture.

Preferably the distal region of the delivery device has a diameter less than the diameter of the enlargement feature mid-portion, and the enlargement feature further includes proximal transition region that converges in the proximal direction from the enlargement feature mid-portion. The proximal transition region facilitates withdrawal of the delivery device after deployment of the stent.

Thus, in accordance with the present invention, a radially self-expanding stent can be positioned accurately at a desired treatment site within a body lumen, based on an accurate positioning of the interior tubing or other stent delivery means. The stent may be allowed to radially self-expand over the majority of its axial length, and yet be retracted if necessary or desired, all while its axial position with respect to the delivery tool is maintained.

#### IN THE DRAWINGS

For a further appreciation of the above and other features and advantages, reference is made to the following detailed description and to the drawings, in which:

Figure 1 is a side elevational view of a stent deployment device constructed in accordance with the present invention;

Figure 2 is an end elevation of the device;

-9-

Figure 3 is a sectional view taken along the line 3-3 in Figure 2;

Figure 4 is a side elevation of the stent in a relaxed configuration;

5        Figures 5-8 are sectional views similar to Figure 3, showing the device at several stages of deploying a radially self-expanding stent;

10       Figure 9 is a sectional view taken along the line 8-8 in Figure 3, showing a stent retaining layer;

Figure 10 is a sectional view similar to Figure 9, but showing an alternative embodiment device utilizing stent retaining strips in lieu of the retaining layer shown in Figure 9;

15       Figure 11 is a schematic view of an esophageal prosthesis constructed in accordance with the present invention;

Figures 12 and 13 illustrate alternative braid angle configurations for self-expanding prostheses;

20       Figure 14 is a side elevational showing a mandrel used in forming the prosthesis of Figure 11;

Figure 15 schematically illustrates the prostheses of Figure 11 in an esophagus, a short time after its deployment;

25       Figure 16 schematically illustrates the prosthesis one day after its deployment; and

Figure 17 illustrates an alternative prostheses constructed according to the present invention, and deployed in an esophagus, with a distal end of the prostheses protruding into the stomach.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

Turning now to the drawings, there is shown in Figure 1 a deployment device 16 for delivering a stent or other prostheses to an intended fixation

-10-

location within a body cavity, and then controllably releasing the stent for radial self-expansion to a fixation within the body cavity.

The device includes an elongate exterior catheter or tubing 18 constructed of a biocompatible polymer, e.g. polypropylene, FEP or Teflon, with an outside diameter of about 12 mm or less. A central lumen 20 runs the length of catheter 18. On the outside of catheter 18 are visible markings 22 designating cm. When using the device, e.g. in deploying a radially self-expanding prostheses within the esophagus, a physician can determine the extent of insertion into the esophagus based upon these markings. Throughout deployment, the proximal end of exterior catheter 18 remains outside the patient. A hub or handle 24 at the proximal end of the exterior catheter, facilitates manipulation of exterior catheter 18 by hand.

An interior catheter or tubing 26 runs through lumen 20, contained within the exterior catheter. Interior catheter 26 has an outside diameter of approximately 6 mm or less, and is constructed of a biocompatible polymer, e.g. polypropylene, FEP, Hytrel or nylon.

At the distal end of interior catheter 26 is a distal tip 28. The distal tip is flexible, yet sufficiently rigid to be self-supporting rather than pliable when encountering tissue. As a result, distal tip 28 can be used to dilate the esophagus along regions where a tumor or other stricture is present. Over the majority of its length, distal tip 28 has a diameter substantially equal to the interior tubing diameter, with a distal converging end 30 formed as part of the tip.

-11-

A proximal region 32 of interior catheter 26 extends proximally beyond hub 24. Visible markings on the outer surface of catheter 26 define three adjacent segments of the proximal region, as indicated at 34, 36 and 38, respectively. These segments can be different colors if desired, to enhance their recognition. These segments, and more particularly the position of hub 24 along them, indicate the axial position of exterior catheter 18 relative to interior catheter 26. The segments further indicate the stages of stent deployment, as is later explained.

At the proximal end of interior catheter 26 is a hub or handle 40, which facilitates manipulation of the interior catheter by hand. A lumen 42 (Figure 3) runs the length of interior catheter 26, to accommodate a guidewire 44.

Figure 3 reveals further features of interior catheter 26, including a distal enlargement feature 46 positioned just proximally of tip 28. Enlargement feature 46 is cylindrical, and includes a mid-portion or medial region 48 having an outside diameter of about 11-12 mm, substantially equal to the diameter of lumen 20. Thus the enlargement feature is in surface engagement with exterior catheter 18 as shown in Figure 3, and can slide relative to the exterior catheter.

Enlargement feature 46 also includes proximal and distal transition regions at 50 and 52, respectively. Distal transition region 52 diverges proximally from the distal tip to the mid-portion of the enlargement feature. The proximal transition region converges proximally from the mid-portion to the interior catheter.

-12-

An annular restraining sleeve 54 surrounds a distal region 56 of the interior catheter. The sleeve is formed by wrapping double sided adhesive tape around the interior catheter so that the sleeve  
5 adheres to the inner catheter and also exhibits a tackiness over its exterior surface. Radiopaque markers 58, 60, 62 and 64 surround the sleeve. These markers can be surrounded by sleeve 54 if desired.

Surrounding sleeve 54 is a radially self-  
10 expanding stent 66. The stent preferably is of open weave or mesh construction, formed of multiple helically wound strands or filaments of a flexible material such as body compatible stainless steel. The durometer of sleeve 54 is substantially less than  
15 the durometer of catheters 18 and 26. Retaining sleeve 54 is sized such that whenever exterior catheter 18 radially compresses stent 66, the catheter also is pressing the stent into a surface engagement with the retaining sleeve, to the point of  
20 at least slightly elastically deforming the sleeve. As a result, friction between the stent and sleeve 54 substantially exceeds friction between the stent and the interior surface of catheter 18. Given the length and positioning of retaining sleeve 54, stent  
25 66 when compressed contacts the sleeve over its entire axial length. In any event, the stent should contact sleeve 54 over at least its entire medial region. Thus, there is no tendency in the stent to travel with exterior catheter 18 as this catheter  
30 moves axially relative to catheter 26. Rather, the stent remains essentially fixed in the axial direction relative to catheter 26. As a result, the axial position of interior catheter 26 serves as a reliable indication of the location of stent 66, not

-13-

only before deployment, but throughout most of the deployment procedure.

An adhesive layer 68 on the exterior surface of retaining sleeve 54 of course further insures that  
5 stent 66 remains axially fixed relative to the interior catheter. It has been found that adhesive is not necessary when deploying a stent of open weave or mesh construction over its entire length. Friction due to the lower durometer of the retaining  
10 sleeve, alone, has been found sufficient to anchor the stent. However, when a silicone or other polymeric film covers the stent medial region, the adhesive is a key factor, in combination with the low durometer, in retaining the stent during external  
15 catheter withdrawal.

As shown in Figure 3, stent 66 is in a reduced-radius and axially elongated configuration. The stent is compressed into this configuration due to the external radial force provided by exterior  
20 catheter 18. When the exterior catheter is withdrawn, thus removing the external force, stent 66 assumes a normal or relaxed configuration shown schematically in Figure 4. More particularly, a medial region 70 of the stent assumes a diameter of  
25 about 20 mm, and opposite end regions 72 and 74 of the stent assume a diameter of about 30 mm.

Hub 24 is fixed to exterior catheter 18, and has an opening to accommodate interior catheter 26 such that the interior catheter is slidable axially  
30 relative to hub 24. Hub 40 has an opening formed therethrough, to accommodate guidewire 44.

An annular sleeve detent 76 surrounds the proximal region of interior catheter 26, between hubs 24 and 40. When positioned as shown in Figure 1,

-14-

retaining sleeve 76 surrounds the interior catheter and abuts the hubs to prevent any substantial movement of the interior catheter axially relative to exterior catheter 18. Sleeve 76 thus functions as a safety detent, preventing premature deployment of the stent. Sleeve detent 76 has a lengthwise slit, and thus is easily removed from proximal region 32 for stent deployment.

Deployment of stent 66 within the esophagus is considered appropriate when a tumor, lesion or other stricture has constricted the esophageal passageway to a diameter less than about 15 mm. This represents a severe constriction in light of the normal passageway diameter of about 22 mm. Deployment begins by oral insertion and positioning of guidewire 44, using an endoscope (not shown) in a manner well known in connection with treating not only the esophagus but other body lumens, e.g. arteries. The guidewire catheter has a diameter of about 0.035-0.042 inches. Once the guidewire has been properly positioned, the endoscope is withdrawn.

Next, deployment device 16, including stent 66 radially compressed as shown in Figure 3, is inserted over guidewire 44 and thus is directed toward the desired treatment location as it is moved distally. Eventually, distal tip 28 of the device encounters the esophageal stricture. At this point, the deployment device is firmly but carefully moved further in the distal direction, to utilize distal tip 28 to dilate the region of the stricture. Once the distal tip has entered the region, distal transition region 52 and mid-portion 48 of the enlargement feature are used to further dilate the region of the stricture, eventually to the point



-15-

where the distal region of exterior catheter 18 is passed through the region of the stricture. Thus, according to one feature of the present invention, the stent delivery device also dilates the region of the esophageal stricture and no separate dilating tool is required.

With the distal end of the exterior catheter past the stricture, stent deployment is initiated. More particularly, with interior catheter 26 held substantially fixed, hub 24 is manipulated by hand to withdraw exterior catheter 18 in the proximal direction. When hub 24 encounters segments 34 along the proximal region 32 of the interior catheter, the distal end of the exterior catheter is near the distal end of stent 66, meaning that deployment is about to begin. Before further withdrawal of the exterior catheter, it is advisable to re-examine the stent position, to insure that medial region 70 of the stent is aligned with the stricture, represented in Figure 5 by a tumor 78 in esophageal wall tissue 80. With stent 66 properly aligned, exterior catheter 18 is withdrawn proximally until hub 24 encounters segment 36. As shown in Figure 5, by the time the hub encounters segment 36, distal end region 72 of stent 66 is released from the exterior catheter and radially self-expands until it encounters tissue 80.

Figure 6 illustrates further withdrawal of exterior catheter 66, to the point where hub 24 encounters marked segment 38. This corresponds to release of stent 66 over its distal region and medial region, i.e. roughly two-thirds deployment. One of the advantages of retaining sleeve 54 is that even at this advanced stage, it remains possible to recover

-16-

or retract stent 66 by moving exterior catheter 18 distally relative to interior catheter 26. Such stent recapture occasionally is necessary, in order to reposition stent 66 relative to the esophageal  
5 stricture. More generally, the stent is virtually always retractable, even when a majority of its axial length is released. With the stent retaining means of the present invention, stents have been found to be retractable after up to 80 percent deployment.

10 Figure 7 illustrates full withdrawal of exterior catheter 18 to completely release stent 66, corresponding to proximal movement to the point where hub 24 is at the proximal end of proximal segment 38. Stent 66 is radially expanded (and axially shortened)  
15 over its entire length, although not expanded to its normal, relaxed configuration. Rather, the stent expands only until the constraining force of esophageal tissue 80 and the remaining residual force in the stent reach an equilibrium. In the  
20 equilibrium state, stent 66 has a diameter substantially larger than the diameter of enlargement feature 46, in particular its mid-portion. Accordingly, interior catheter 26 can be withdrawn proximally through the expanded stent. Proximal  
25 transition region 50 further insures against the possibility of enlargement feature 46 being caught during attempted withdrawal, either by stent 66 or a stricture in the esophagus. However, as a precaution against this event, the physician can advance  
30 exterior tubing 18 distally through the deployed stent until its distal end once again surrounds the enlargement feature as shown in Figure 1.

Figure 8 illustrates a proximal withdrawal of enlargement feature 46 and distal tip 28 past stent

-17-

66. Withdrawal of the delivery tool is followed by withdrawal of guidewire 44, unless the guidewire is retained for guiding another tool, e.g. an endoscope, into the esophagus.

5        Figure 9 illustrates the radial compression of stent 66 by exterior catheter 18 to press the stent into surface engagement with restraining sleeve 54. Figure 10 is a view similar to Figure 9, but showing an alternative deployment device in which several  
10 strips 82, elongate in the axial direction, are spaced apart angularly in an array about an interior catheter 84. Like sleeve 54, the strips are constructed of a material having a substantially lower durometer than the catheters. The strips are  
15 secured to the interior catheter and, if desired, are provided with adhesive coatings along their radially outward surfaces, as indicated at 86.

While stent 66 is satisfactory in many respects, it is unsuitable for treatment of certain cancerous  
20 tissue in the esophagus. Such tissue is not as strong as healthy esophageal tissue, and thus is subject to rupture or other damage from an excessively rapid and forceful expansion of a conventional open weave stent. The stent is subject  
25 to tumor ingrowth due to its open weave construction. Further, points or edges at the opposite ends of the stent may perforate the esophageal wall.

A prostheses or stent 90, shown in Figure 11, is constructed to address all of these concerns. Like  
30 stent 66, stent 90 is of mesh or open weave construction, comprised of multiple braided and helically wound strands. Stent 90 has a medial sleeve or region 92, a distal cuff 94 and proximal cuff 96. The proximal and distal ends of the stent

-18-

are directed radially inward, as indicated at 98 and 100. When stent 90 is in its relaxed or normal configuration as shown in the figure, medial region 92 has a diameter of about 20 mm, and the cuffs have  
5 a diameter of about 30 mm. The filaments forming the stent, preferably of a body compatible stainless steel, are about 0.22 mm or less in diameter.

While cuffs 94 and 96 are open, medial region 92 is circumscribed, i.e. completely covered, with a  
10 continuous polymeric film, preferably silicone. The silicone film is applied by dip coating of stent 90, in which event the film initially covers one of the cuffs, and is removed from that cuff prior to using the stent. The preferred thickness of the silicone  
15 film is in the range of 0.003 - 0.01 inches (0.075 - 0.25 mm), and is controlled primarily by the number of dip coating applications. More specifically, from three to five dip coatings result in a thickness within the preferred range.

20 The silicone film is elastic, and thus is radially self-expanding like the remainder of stent 90. However, the silicone reinforces the medial region such that it has a much greater restoring force than the open weave portions of the stent. In  
25 particular, while cuffs 94 and 96 tend to recover virtually instantaneously from a radially compressed configuration, a tumor would inhibit their recovery. Medial region 92 recovers against a tumor, although it has been observed to take 24 hours for recovery.  
30 It has been found that the recovery rate of the medial region 92 can be controlled by controlling the thickness of the silicone film.

The gradual recovery rate of the medial region against tumors affords several advantages which make

-19-

stent 90 particularly well suited for treating esophageal strictures. Certain advantages arise from the coated medial region itself, and other advantages arise from the combination of the medial region with cuffs 94 and 96. Considered alone, medial region 92 provides an effective barrier to tissue ingrowth, because of the continuous silicone film. The gradual recovery of medial sleeve 92, from the radially compressed state when the stent is deployed, substantially reduces the chance that weakened cancerous tissue will be harmed during stent radial self-expansion. While a recovery rate of about one hour would significantly reduce most of the risk, the observed recovery rate of 24 hours is highly preferred. A further advantage arises from the fact that the residual force along the medial region is greater than the residual force along the more rapidly expanding cuffs. As a result, the maximum radial dilating force is provided along that portion of stent 90 aligned with the esophageal stricture.

As mentioned above, cuffs 94 and 96 radially expand rapidly upon their release from a stent confining means such as exterior catheter 18. Thus, the cuffs rapidly contact and reach equilibrium with healthy tissue of the esophageal wall. Residual force in the cuffs at equilibrium is much less than the residual force along medial region 92. As a result, cuffs 94 and 96 readily conform to changes in the esophageal wall during swallowing and other convulsions of the esophagus. Thus, the cuffs are particularly effective in resisting either proximal or distal migration the stent. The open weave construction of the cuffs does not give rise to the problem of tumor ingrowth, since medial region 92 is

-20-

aligned with the stricture, while the cuffs engage healthy tissue.

Yet another advantage of the silicone film is that it provides reinforcement along medial region 5 92, enabling the stent to be constructed with a reduced braid angle. The braid angle is measured, based on the filament incline from the axial dimension of the stent. Figures 12 and 13 illustrate a high braid angle and a low braid angle, 10 respectively. In each case, the stent is oriented with its axial length in the horizontal direction. Heretofore, 90 degrees has been considered a lower practical limit for the braid angle of a mesh or open weave stent. Employing the silicone film, however, 15 enables a reduction of the braid angle to as low as 70 degrees, as illustrated in Figure 13. The advantage of a lower braid angle resides in the fact that the braid angle determines the ratio of stent axial shortening to radial increase, as the stent 20 self-expands. With a reduced braid angle, there is less axial shortening for a given radial expansion. Due to the reduced axial "drift", the stent can be more accurately positioned within body lumens during its deployment.

25 Figure 14 illustrates a mandrel 102 particularly well suited for forming stent 90. Mandrel 102 includes a central shank 104, enlargements 106 and 108 on opposite sides of the shank, and end portions 110 and 112. To form the stent, the individual 30 filaments or strands are wound in helical fashion to form an open weave cylinder. The cylinder is placed upon mandrel 102 and heated to a temperature in the range of from about 800-1,000 degrees F. The filaments, when cooled, retain the shape of the

-21-

mandrel. Portions of the stent formed along the outer ends of the mandrel are trimmed, leaving the inwardly directed ends 98 and 100.

Figures 15 and 16 schematically illustrate stent 90 after its deployment in the esophagus. An esophageal wall 114 includes a tumor 116. Using a device such as device 16, stent 90 is deployed as above explained. Medial region 92 of the stent is aligned with the tumor, and cuffs 94 and 96 are aligned with healthy portions of the esophageal wall 114 proximally and distally of tumor 116. The cuffs expand into engagement and equilibrium with esophageal wall 114 substantially immediately after deployment. Medial region 92, while it may engage tumor 116, remains radially reduced.

Figure 16 illustrates stent 90 one day after deployment. Medial region 92 has recovered, and presses against tumor 116 to maintain the esophageal passage along the stricture. The diameter of medial region 92 at equilibrium is likely to be greater than two-thirds of the cuff diameter at equilibrium, because of the greater residual force due to the silicone film.

Figure 17 illustrates another alternative stent 120 particularly suited for esophageal placement near the stomach, more particularly when a flared distal end or lower end 122 of the stent is near or protruding into the stomach, e.g. to treat a stricture near the stomach. Accordingly, stent 120 includes a distal region 124 circumscribed with a continuous silicone film, and a proximal cuff 126 of mesh or open weave construction. The proximal end 128 of the stent is inclined inward, to avoid the chance for esophageal perforation. Stent 120 can be

-22-

deployed with a tool substantially identical to deployment device 16.

Thus, in accordance with the present invention, a radially self-expanding stent includes a barrier  
5 region circumscribed by a silicone film to reduce tumor ingrowth, in combination with a fixation region of open weave construction. The stent is resistant to migration and to tumor ingrowth, and can be configured to recover gradually along its barrier  
10 region after deployment, to minimize harm to weakened, cancerous tissue. The device for deploying the stent incorporates a dilation tip and a further dilation feature proximally of the tip, to eliminate the need for a separate esophageal dilating tool.  
15 During delivery and deployment, the stent surrounds and is radially compressed against a low durometer stent restraining sleeve. This fixes the stent axially with respect to an interior catheter of the deployment device, for enhanced accuracy in stent  
20 positioning and enhanced ability to recover or retract a partially deployed stent.

What is claimed is:



-23-

## CLAIMS

1. An apparatus (16) for deploying a radially self-expanding stent (66) within a body lumen, including:

5 a stent confining means (18) for elastically compressing a radially self-expanding stent (66) into a delivery configuration in which the self-expanding stent (66) has a reduced radius along its entire axial length;

10 an elongate and flexible stent delivery device (26) having a proximal end, a distal end and a distal region near the distal end for use in delivering the radially self-expanding stent (66) into a body lumen and in positioning the stent (66) at a treatment site within the body lumen with the  
15 stent (66) surrounding the delivery device (26) along the distal region, while the proximal end of the flexible delivery device (26) remains outside of the body;

20 an axial restraining means (54) disposed along the distal region of the delivery device (26); and

a control means (24, 40) operably associated with the delivery device (26) and the confining means (18), for moving the confining means  
25 (18) axially relative to the delivery device (26) toward and away from a confinement position in which the confining means (18) compresses the self-expanding stent (66) into the delivery configuration and urges the stent (66) into a surface engagement  
30 with the axial restraining means (54);

wherein the axial restraining means (54), due to said surface engagement, tends to maintain the self-expanding stent (66) axially aligned with the

-24-

35 deployment device (16) as the confining means (18) is moved axially away from the confinement position to release the stent (66) for radial self-expansion.

2. The apparatus of Claim 1 wherein:

the stent delivery device (26) comprises a first elongate and flexible length of tubing (26).

3. The apparatus of Claim 2 further including: a central lumen (42) running the axial length of the first tubing (26), for accommodating a guidewire (44).

4. The apparatus of Claim 2 further including: a distal tip (28) at the distal end of the first tubing (26), for dilating a malignant stricture at the treatment site.

5. The apparatus of Claim 2 wherein:

the stent confining means (18) comprises a second elongate and flexible length of tubing (18) having a lumen (20) running the length thereof, and  
5 wherein the first length of tubing (26) is contained within the lumen (20) with a proximal portion of the first tubing (26) extended proximally of the second tubing (18) when the second tubing (18) is in the confinement position.

6. The apparatus of Claim 5 wherein:

the control means (24, 40) comprises a first hub (40) at the proximal end of the first tubing (26) and a second hub (24) at the proximal end  
5 of the second tubing (18).

7. The apparatus of Claim 5 wherein:

the axial restraining means (54) comprises a sleeve (54) surrounding the first tubing (26) along the distal region, said sleeve (54) having a lower  
5 durometer than the second tubing (18).

8. The apparatus of Claim 7 further including:

-25-

an adhesive (68) applied to an exterior surface of the sleeve (54).

9. The apparatus of Claim 5 wherein:

the axial restraining means (54) comprises a plurality of elongate strips (82) disposed along the distal region.

10. The apparatus of Claim 9 wherein:

the strips (82) are oriented axially and spaced apart angularly from one another to form a set of the strips (82) surrounding the first tubing (26).

11. The apparatus of Claim 10 further including:

an adhesive layer (86) along a radially outward surface of each of the strips (82).

12. The apparatus of Claim 5 further including:

visible indicia along the proximal portion of the first tubing (26) for indicating the position of a distal end of the second tubing (18) with  
5 respect to the distal region of the first tubing (26).

13. The apparatus of Claim 12 wherein:

said indicia further measure the extent to which the radially self-expanding stent (66) is deployed.

14. The apparatus of Claim 5 further including:

visible markings (22) along at least a proximal region of the second tubing (18) for indicating the extent of insertion of the second  
5 tubing (18) into the body lumen.

15. The apparatus of Claim 5 further including:

a detent device (76) removably mounted to the first tubing (26) along the proximal portion, for preventing any substantial axial movement of the  
5 first tubing (26) relative to the second tubing (18),

-26-

to maintain the second tubing (18) in the confinement position.

16. A device for fixation in a body lumen, including:

a tubular stent (90) of open weave construction having a predetermined normal configuration and being radially compressible to a reduced-radius configuration to facilitate an axial insertion of the stent into a body lumen for delivery to a treatment site within the body lumen; and

a continuous film formed axially along the stent (90) and circumscribing the stent (90) over a barrier region (92) of the stent (90) to substantially prevent growth of tissue through the stent (90) along the barrier region (92); and

wherein a portion (94, 96) of the stent (90) is substantially free of the continuous film to provide a fixation region of the stent (90) for positively fixing the stent (90) within the body lumen at the treatment site, by radial expansion of the stent (90) into a surface engagement with a tissue wall segment defining the body lumen.

17. The device of Claim 16 wherein:

the stent (90) is elastic, tending to assume the reduced-radius configuration in response to the application of an external force, and tending to assume the normal configuration in the absence of the external force.

18. The device of Claim 17 wherein:

the film is an elastic polymer that reinforces the stent (90) along the barrier region (92).

19. The device of Claim 18 wherein:

the film is formed of silicone.

-27-

20. The device of Claim 18 wherein:  
the fixation region (94, 96) of the stent (90) tends to exert a lower restoring force in its return toward the normal configuration, as compared to the barrier region (92) of the stent (90), upon removal of the external force.

21. The device of Claim 20 wherein:  
the barrier region (92) requires at least one hour to return toward the normal configuration when encountering a tumor.

22. The device of Claim 17 wherein:  
the stent (90) comprises a mesh formed of braided helical strands.

23. The device of Claim 22 wherein:  
a braid angle, defined as the angle between two intersecting helical strands and encompassing a longitudinal axis of the stent, is approximately 70 degrees.

24. The device of Claim 16 wherein:  
the barrier region (92) has a diameter less than the diameter of the fixation region when the stent (90) is in the normal configuration.

25. The device of Claim 17 wherein:  
said fixation region (94, 96) is comprised of a proximal cuff and a distal cuff, and the barrier region (92) is comprised of a medial sleeve of the stent between the proximal and distal cuffs.

26. The device of Claim 25 wherein:  
the stent (90) is formed of braided helical strands, with opposite ends of the strands at proximal and distal ends of the stent bent radially inward.

FIG. 1

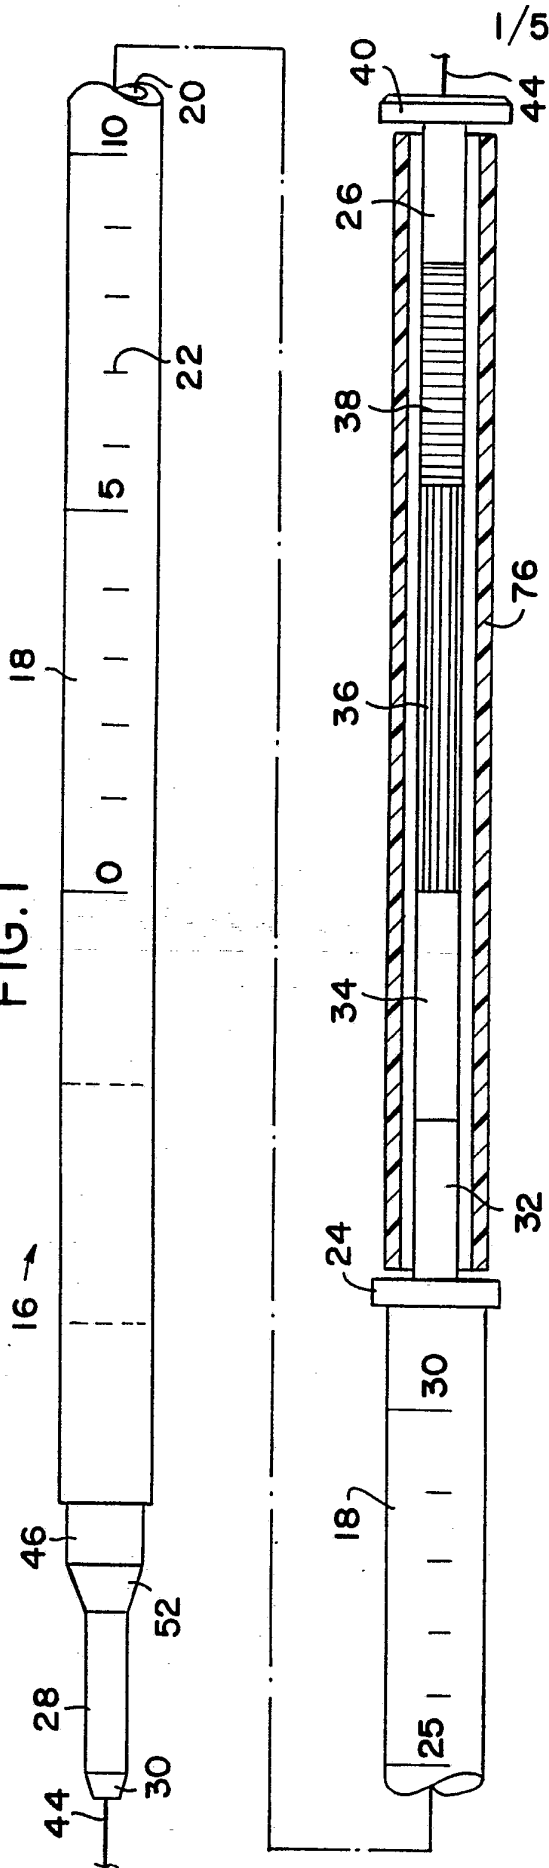


FIG. 2





FIG. 3

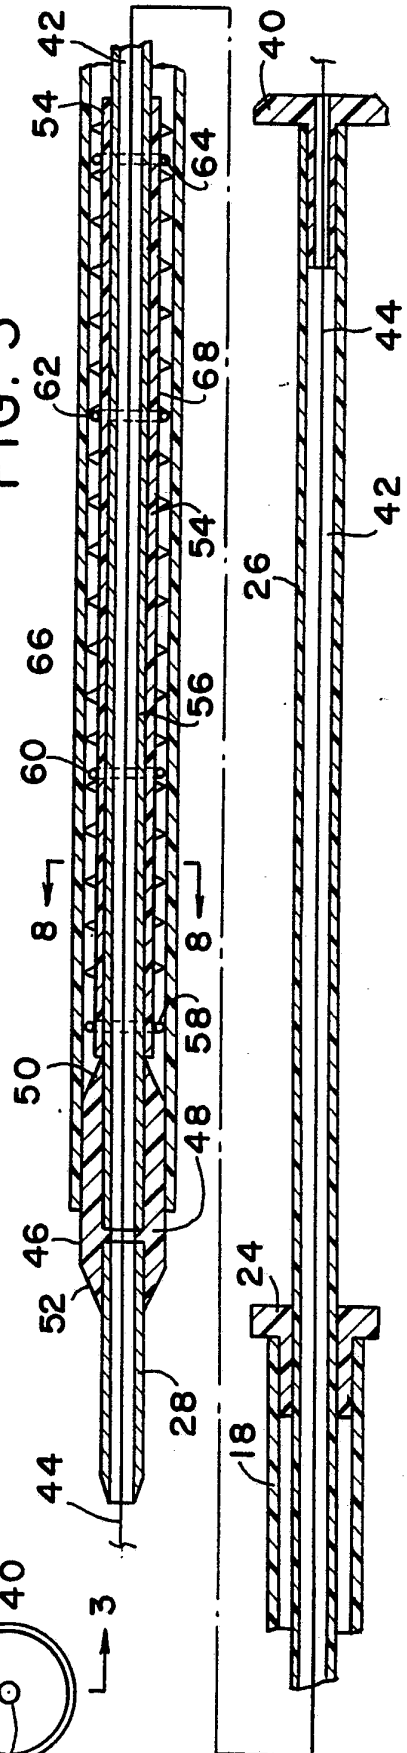

2 / 5

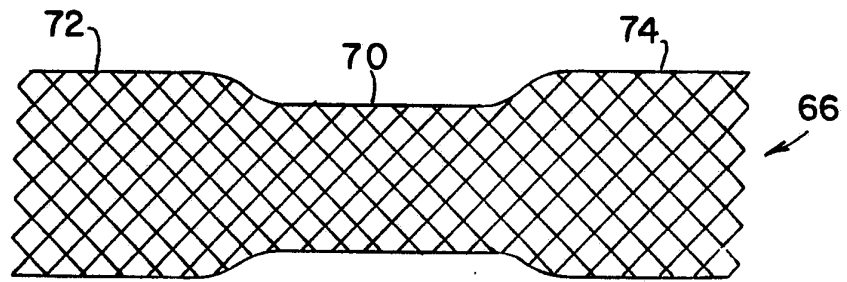


FIG. 4

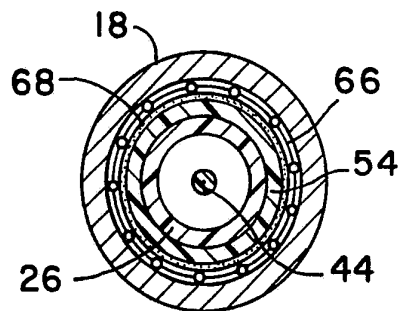


FIG. 9

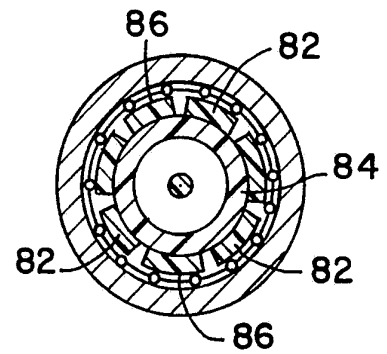


FIG. 10

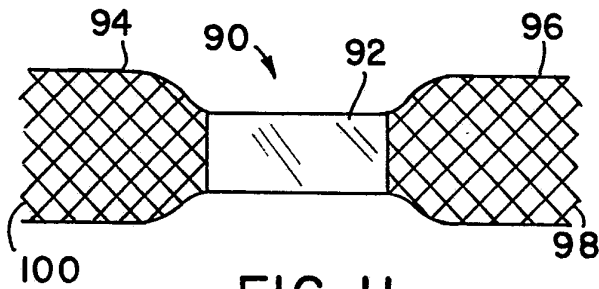


FIG. 11

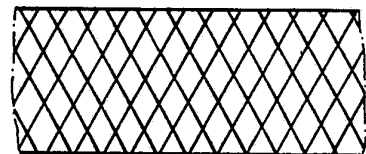


FIG. 12

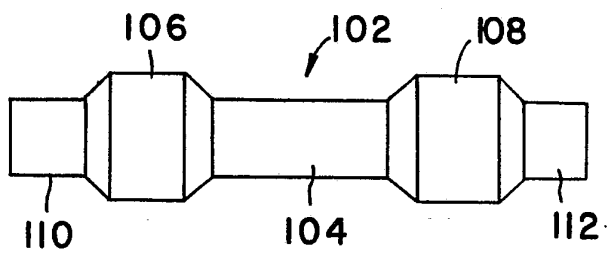


FIG. 14





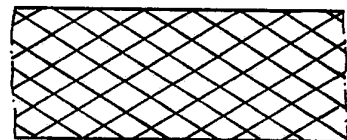


FIG. 13

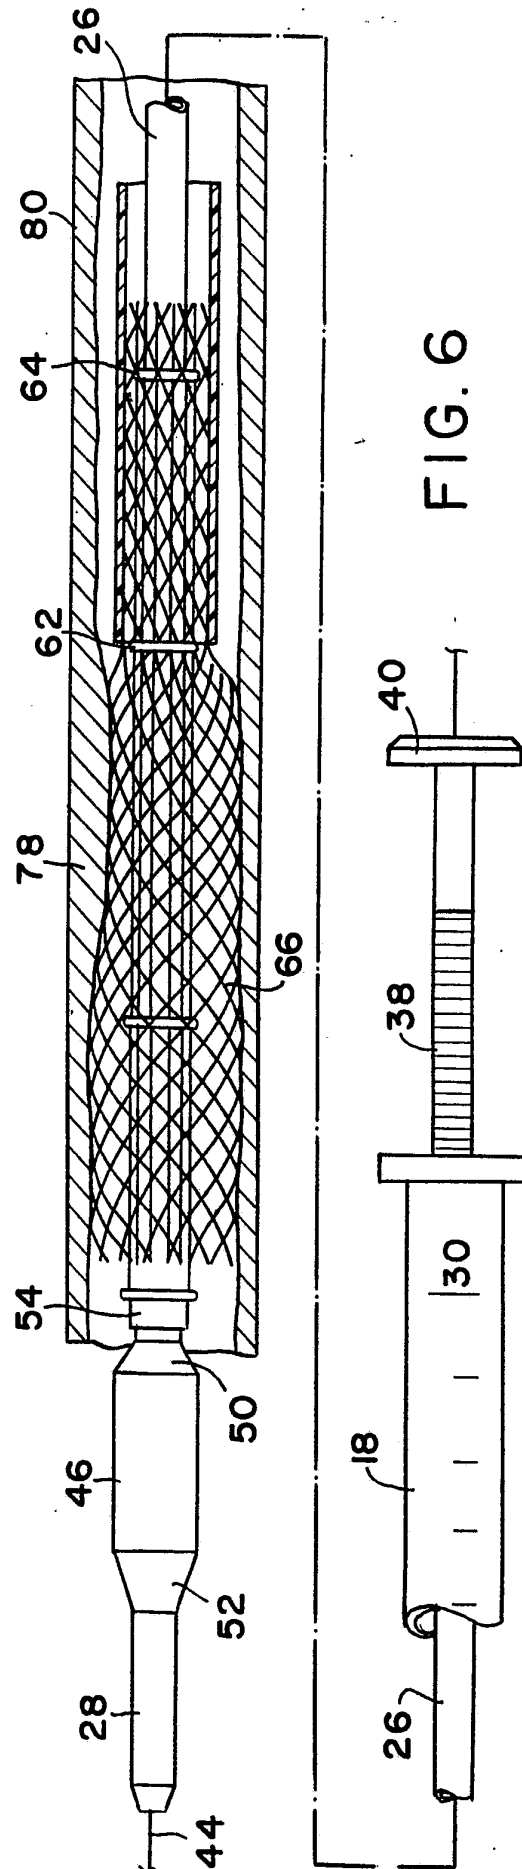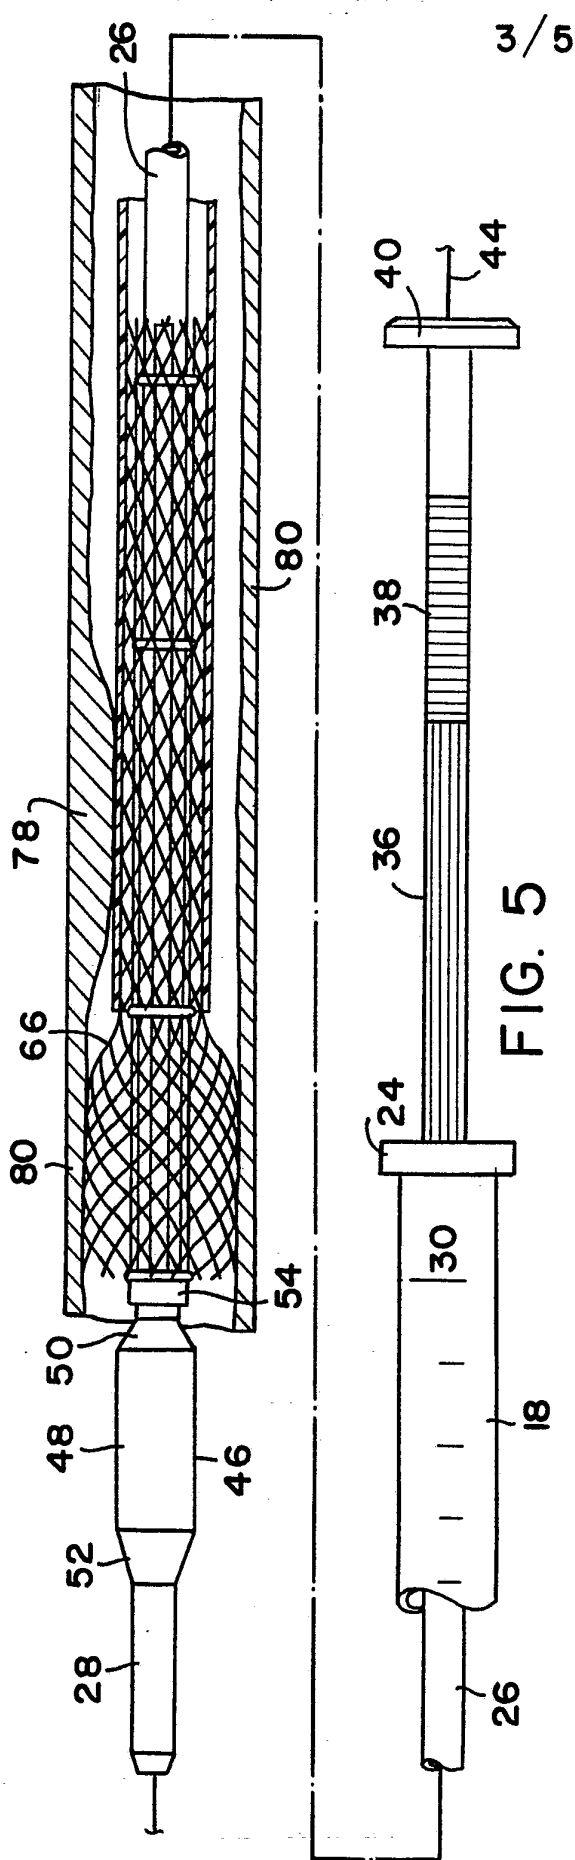

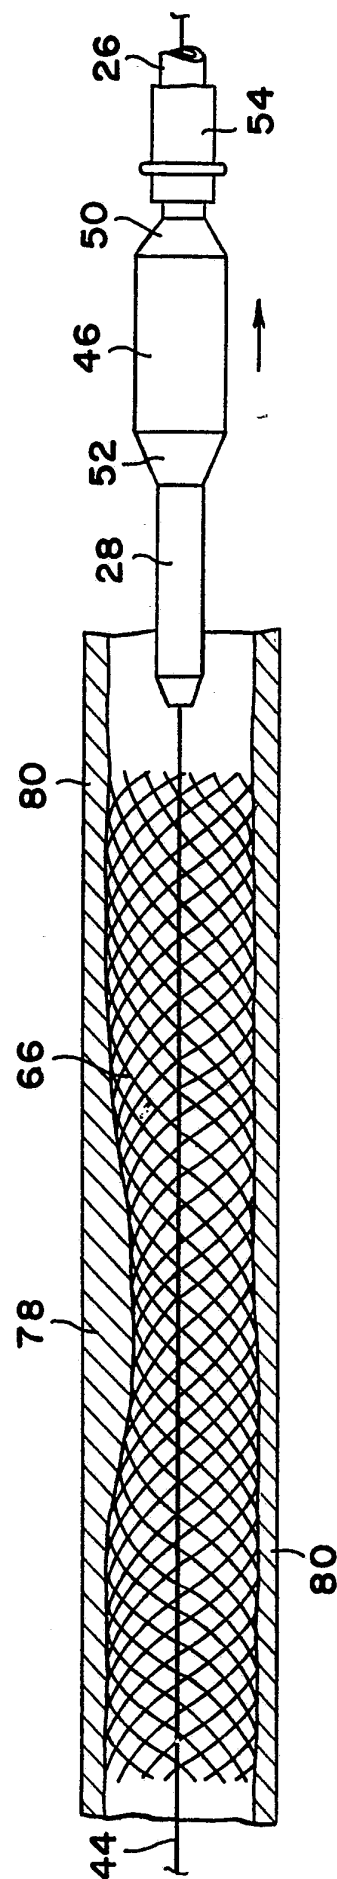

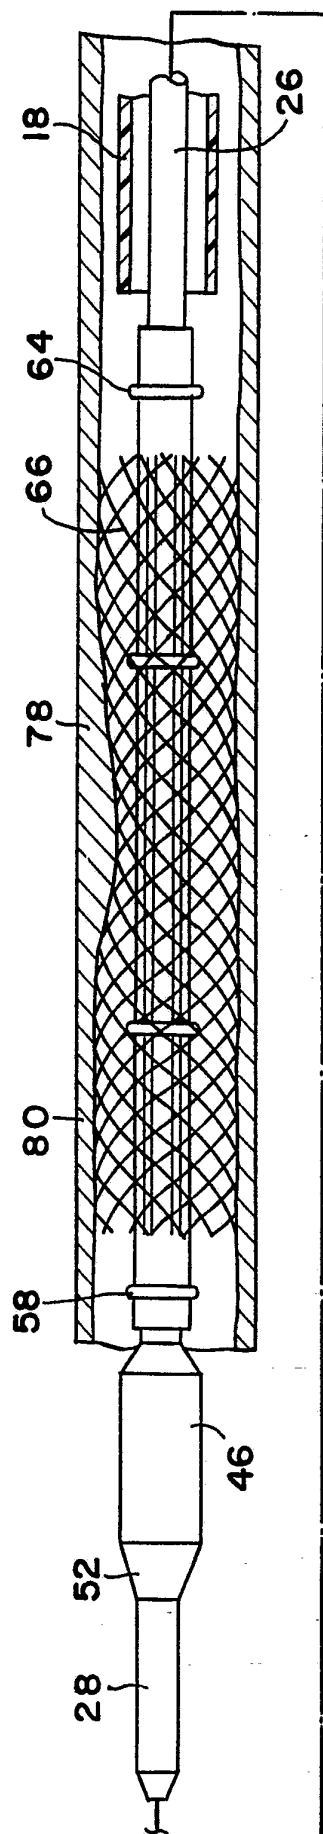

5/5

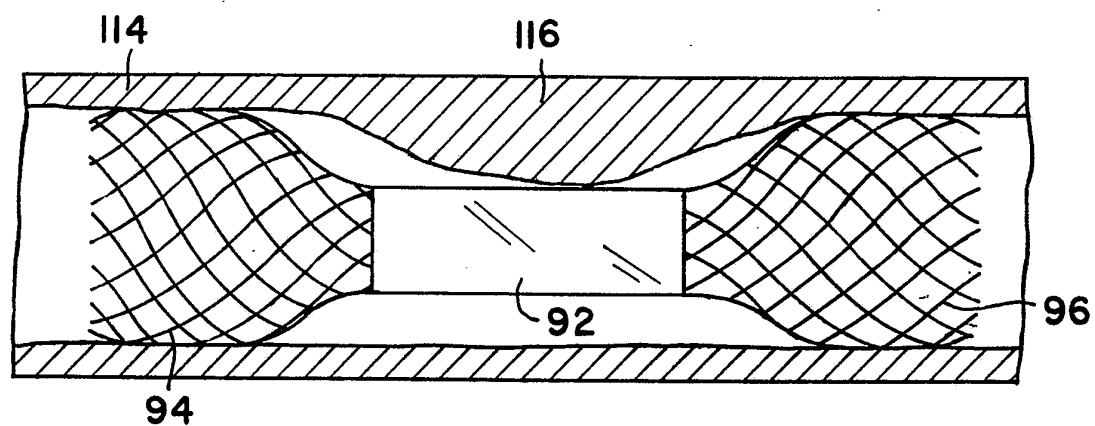


FIG. 15

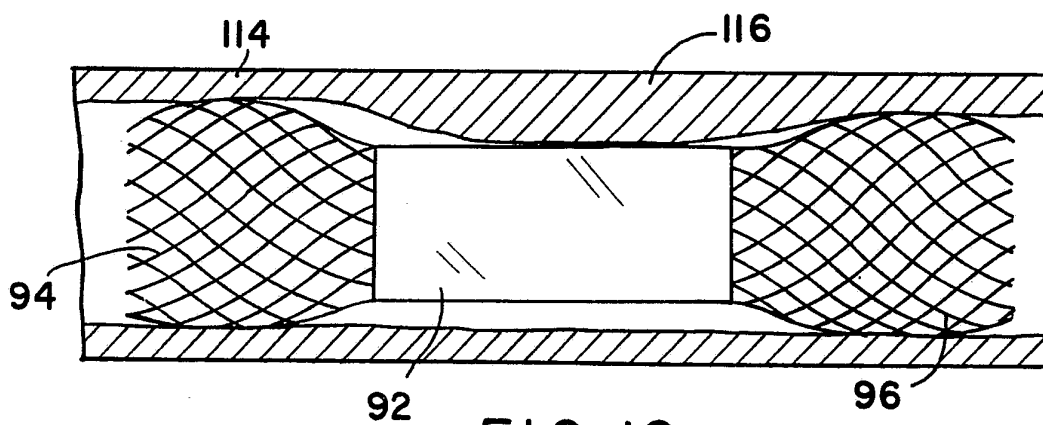


FIG. 16

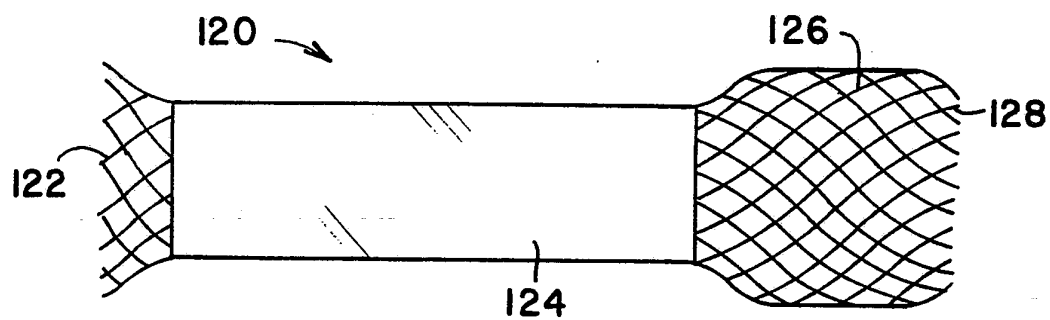


FIG. 17

# INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 93/01966

<b>I. CLASSIFICATION OF SUBJECT MATTER</b> (if several classification symbols apply, indicate all) <sup>6</sup>		
According to International Patent Classification (IPC) or to both National Classification and IPC Int.C1.5                      A 61 F      2/06		
<b>II. FIELDS SEARCHED</b>		
Minimum Documentation Searched <sup>7</sup>		
Classification System	Classification Symbols	
Int.C1.5	A 61 F	
Documentation Searched other than Minimum Documentation to the Extent that such Documents are Included in the Fields Searched <sup>8</sup>		
<b>III. DOCUMENTS CONSIDERED TO BE RELEVANT<sup>9</sup></b>		
Category <sup>10</sup>	Citation of Document, <sup>11</sup> with indication, where appropriate, of the relevant passages <sup>12</sup>	Relevant to Claim No. <sup>13</sup>
X	EP,A,0408245 (AMERICAN MEDICAL SYSTEMS) 16 January 1991	1-8, 12-14
Y	see the whole document ---	11
X	US,A,5089006 (F.B. STILES) 18 February 1992	1-3, 5, 6, 9, 10
Y	see the whole document ---	11
X	WO,A,8704935 (R.E. FISCHHELL ET AL.) 27 August 1987 see abstract ---                      -/-	1-3, 5, 6
<div style="display: flex; justify-content: space-between;"> <div style="width: 45%;"> <p><sup>10</sup> Special categories of cited documents :</p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier document but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> </div> <div style="width: 45%;"> <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.</p> <p>"&amp;" document member of the same patent family</p> </div> </div>		
<b>IV. CERTIFICATION</b>		
Date of the Actual Completion of the International Search		Date of Mailing of this International Search Report
27-05-1993		07. 09. 93
International Searching Authority		Signature of Authorized Officer
EUROPEAN PATENT OFFICE		

III. DOCUMENTS CONSIDERED TO BE RELEVANT (CONTINUED FROM THE SECOND SHEET)		
Category *	Citation of Document, with indication, where appropriate, of the relevant passages	Relevant to Claim No.
A	<p>US,A,4973301 (I. NISSENKORN) 27  November 1990  see column 3, line 27 - line 37 see column 4,  line 17 - line 36; figures 4-6  -----</p>	12-14

# INTERNATIONAL SEARCH REPORT

International application No.

PCT/US 93/01966

## Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:  
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:  
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:  
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

## Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

For further information see Form PCT/ISA/206 sent on 22.06.93.

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

1-15

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☒ No protest accompanied the payment of additional search fees.

**ANNEX TO THE INTERNATIONAL SEARCH REPORT  
ON INTERNATIONAL PATENT APPLICATION NO.**

US 9301966

SA 71368

This annex lists the patent family members relating to the patent documents cited in the above-mentioned international search report. The members are as contained in the European Patent Office EDP file on 01/09/93  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP-A- 0408245	16-01-91	CA-A- 2020957	14-01-91
		DE-U- 9010130	13-09-90
		JP-C- 1718137	14-12-92
		JP-A- 3057465	12-03-91
		JP-B- 3079023	17-12-91
		US-A- 5026377	25-06-91
US-A- 5089006	18-02-92	CA-A- 2030196	30-05-91
WO-A- 8704935	27-08-87	EP-A, B 0257091	02-03-88
		EP-A- 0556940	25-08-93
		US-A- 4768507	06-09-88
US-A- 4973301	27-11-90	None	