

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
19 February 2009 (19.02.2009)

PCT

(10) International Publication Number
WO 2009/023622 A1

- (51) International Patent Classification:
H01J 49/04 (2006.01) **B01D 59/44** (2006.01)
- (21) International Application Number:
PCT/US2008/072754
- (22) International Filing Date: 11 August 2008 (11.08.2008)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
11/893,308 15 August 2007 (15.08.2007) US
- (71) Applicant (for all designated States except US): **VARIAN, INC.** [US/US]; 3120 Hansen Way, D-102, Palo Alto, CA 94304 (US).
- (72) Inventors; and
- (75) Inventors/Applicants (for US only): **WANG, Mingda** [US/US]; 42103 Camino Santa Barbara, Fremont, CA 94539 (US). **FANCHER, Charles, A.** [US/US]; 222 Kingston Street, San Francisco, CA 94110 (US). **MUNTEAN, Felician** [RO/US]; 119 Plaza Circle, Danville, CA 94526 (US). **STEINER, Urs** [US/US]; 784 Pear Avenue, Sunnyvale, CA 94087 (US).
- (74) Agents: **FISHMAN, Bella** et al.; Varian, Inc., Legal Department, 3120 Hansen Way, D-102, Palo Alto, CA 94304 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

- with international search report
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

(54) Title: SAMPLE IONIZATION AT ABOVE-VACUUM PRESSURES

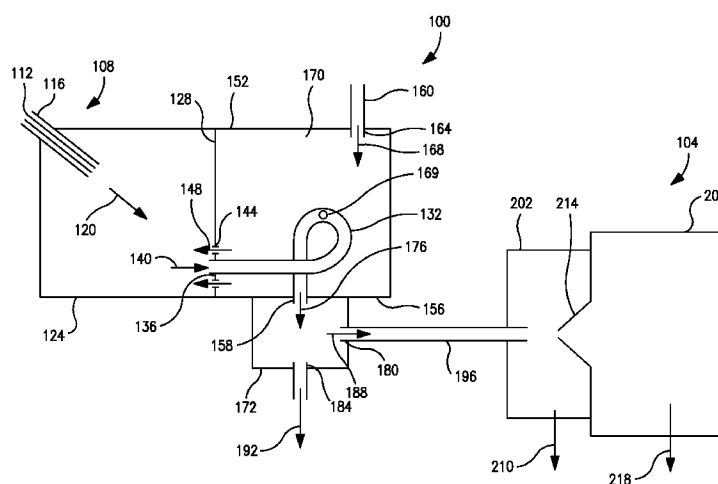


FIG. 1

(57) Abstract: Sample material ionized in a sample receiving chamber is flowed into a sample conduit. Drying gas may also flow into the sample conduit and may be heated. The pressure and length of the sample conduit may be provided according to the product 50 or greater Torr-cm. The sample conduit may include a turn. The sample conduit may lead to an ion extraction chamber at which a sampling orifice may lead to a mass spectrometer. The diameter of the sample conduit may be larger than the diameter of the sampling orifice. An electrical field may be applied in the ion extraction chamber to slow incoming ions. A voltage jump may be applied to the sample conduit.

WO 2009/023622 A1

SAMPLE IONIZATION AT ABOVE-VACUUM PRESSURES

FIELD OF THE INVENTION

[0001] The present invention relates generally to ionization of sample material performed at pressures above vacuum. This type of ionization may be performed, for example, for providing ions for introduction into an analytical instrument such as a mass spectrometer.

BACKGROUND OF THE INVENTION

[0002] Certain techniques, such as in analytical chemistry, require that components of a sample be ionized prior to analysis. Mass spectrometry (MS) is an example of such analytical techniques. Generally, MS encompasses a variety of instrumental methods of qualitative and quantitative analysis that enable ionized species of analytes (i.e., sample molecules of interest) to be resolved according to their mass-to-charge ratios. For this purpose, an MS system converts the components of a sample into ions, sorts or separates the ions based on their mass-to-charge ratios, and processes the resulting ion output (e.g., ion current, flux, beam, etc.) as needed to produce a mass spectrum. Typically, a mass spectrum is a series of peaks indicative of the relative abundances of charged components as a function of mass-to-charge ratio.

[0003] A typical MS system includes a sample inlet system, an ion source or ionization device, a mass analyzer, an ion detector, a signal processor, a readout/display means, and an electronic controller such as a computer. The MS system also includes a vacuum system to enclose the mass analyzer(s) in a controlled, evacuated environment. In addition to the mass analyzer(s), depending on design, all or part of the sample inlet system, ion source, and ion detector may also be enclosed in the evacuated environment. One broad class of ion sources, however, ionizes sample material at or near atmospheric pressure in a region necessarily distinct from the vacuum or low-pressure regions of the mass analyzer. Atmospheric-pressure ionization (API) thus requires a structural interface to transport ions produced in the atmospheric-pressure environment of the API source to the evacuated environment of the mass spectrometer. API techniques are particularly useful when it is desired to couple mass spectrometry with an analytical separation technique such as liquid chromatography (LC). For instance, the output or effluent from an LC column may serve as the sample source or input into an API interface. Typically, the effluent consists of a liquid-phase matrix of analytes and mobile-phase material (e.g., solvents, additives, matrix components, etc.).

[0004] Examples of API techniques include electrospray ionization (ESI), atmospheric-pressure chemical ionization (APCI), atmospheric-pressure photoionization (APPI), and

atmospheric-pressure matrix-assisted laser desorption/ionization (AP-MALDI). API techniques such as these are known and therefore need not be described in detail. As appreciated by persons skilled in the art, ESI is a desorption ionization technique characterized by the use of an electrically conductive electrospray needle. APCI is a gas-phase ionization technique
5 characterized by the use of a corona discharge needle. APPI is characterized by the use of a photon source such as an ultraviolet (UV) lamp. AP-MALDI is characterized by the use of a pulsed laser beam and laser radiation-absorbing organic molecules.

[0005] Each technique typically employs an ionizing device extending into a chamber held at atmospheric pressure. The atmospheric-pressure chamber is physically separated from one or
10 more vacuum or low-pressure regions of the mass spectrometer in which ion-guiding and mass-analyzing components reside. The ionizing device receives an analyte-bearing sample material from which the ionizing device produces a gaseous stream or spray that may comprise analyte ions, ion clusters, charged droplets, and neutral droplets. An inert nebulizing gas such as nitrogen (N₂) may be utilized to assist in forming this sample spray. The resulting sample spray
15 is directed through the interior of the atmospheric-pressure chamber to a sampling orifice that leads to the mass spectrometer. One or more electrical fields may be generated in the atmospheric-pressure chamber to guide the sample spray toward the sampling orifice.

[0006] Ideally in conventional techniques, only the analyte ions enter the mass spectrometer, and not the other components of the spray such as neutral solvated droplets. In addition to the
20 above-mentioned optional nebulizing gas, a stream of an inert drying gas such as nitrogen may be introduced into the atmospheric-pressure chamber to assist in the evaporation of solvent and/or sweep the solvent away from the sampling orifice. The drying gas may be heated prior to introduction into the chamber. The drying gas may be introduced through an annular opening formed by a tube that is coaxial with the sampling orifice, in counter-flow relation to the spray
25 as the spray approaches the sampling orifice. Alternatively, the drying gas may be introduced as a curtain in front of the sampling orifice.

[0007] A recurring problem in API techniques such as those noted above is the entry of unwanted droplets and other non-analytical material into the sampling orifice that serves as the entry into the evacuated regions of the mass spectrometer. Such unwanted components may
30 degrade the performance of the mass spectrometer and/or the quality of the mass spectral data produced thereby through contamination, reduction in sensitivity, reduction in robustness, peak tailing, etc. These problems can be exacerbated as the flow rate of sample material introduced into the ion source is increased. As previously noted, the API ion source has conventionally been provided with a counterflow or a curtain of a heated, dry inert gas such as nitrogen to

protect the sampling orifice by evaporating and blowing away the unwanted components. These previous approaches, however, have failed to adequately prevent the entry of unwanted components into the sampling orifice, and do not provide a sufficient degree of contact between the drying gas and the spray of sample material. In addition, in the previous approaches, desolvation of entrained sample cluster ions and evaporation of liquid droplets are incomplete, and the efficiency with which ions are extracted into the mass spectrometer is less than desirable. It is desirable to increase collisions of solvated ions or cluster ions prior to their entering the mass spectrometer to thereby increase the signal-to-noise (S/N) ratio.

[0008] In addition, the sampling orifice conventionally employed as the exit from the atmospheric-pressure ionization chamber to the mass spectrometer typically serves as the direct interface between the ionization chamber and the first stage of the mass spectrometer. This sampling orifice is typically the inlet of a small-diameter, long capillary that drops the fluid pressure from atmospheric down to about 1 – 20 mTorr. The inside diameter of the sampling orifice (and associated length of capillary) is determined by the pumping system provided with the ionization/mass spectrometry apparatus. Because it is not practical to pump gaseous fluid in these types of systems at a flow rate much greater than 60 CFM, the inside diameter of the sampling orifice is typically held to around 5 μm . The small diameter of the sampling orifice and its use for sampling the ion-bearing stream directly from the ionization chamber into the mass spectrometer result in a large portion of the ions produced in the ionization chamber not being collected in the sampling orifice for analysis by the mass spectrometer.

[0009] The foregoing problems attending conventional systems employing API interfaces may result in less than desirable performance parameters, such as low sensitivity, low S/N ratio, low ion signal strength, insufficient separation of analyte ions from liquid droplets and matrix background components, insufficient evaporation of liquid droplets, insufficient collisions of solvated ions or cluster ions and thus insufficient desolvation, and high chemical background. Accordingly, there continues to be a need for improving ionization techniques that require environments of higher pressure than, and thus an interface with, the associated low-pressure/vacuum analytical instrument receiving the as-produced ions such as a mass spectrometer.

SUMMARY OF THE INVENTION

[0010] To address the foregoing problems, in whole or in part, and/or other problems that may have been observed by persons skilled in the art, the present disclosure provides apparatus,

devices, systems and/or methods relating to proportional valves, as described by way of example in implementations set forth below.

[0011] According to one implementation, an ionization apparatus includes an interface chamber defined by a plurality of boundaries, and a heated sample conduit extending through the interface chamber. The sample conduit includes an inlet and an outlet, each of which is positioned within at least one of the boundaries. The sample conduit establishes a sample material flow path separated from an interface chamber interior. Within the sample conduit, a drying gas is mixed with the sample material flow and the product of the pressure times the length of said conduit is equal or greater than 50 torr x cm.

[0012] According to another implementation, an ionization apparatus includes an interface chamber including a plurality of boundaries defining an interface chamber interior, a drying gas inlet communicating with the interface chamber interior, and a sample conduit extending through the interface chamber and including a sample conduit inlet and a sample conduit outlet. The sample conduit inlet and the sample conduit outlet are positioned at at least one of the boundaries whereby the sample conduit establishes a sample material flow path separated from the interface chamber interior. The boundary at which the sample conduit inlet is positioned including a drying gas outlet proximate to the sample conduit inlet and communicating with the interface chamber interior, whereby the interface chamber establishes a drying gas flow path from the drying gas inlet, around the sample conduit and to the drying gas outlet.

[0013] According to another implementation, an ionization apparatus includes a sample receiving chamber including a boundary defining a sample receiving chamber interior, an ion extraction chamber separate from the sample receiving chamber and including an ion exit aperture and an exhaust aperture, and a sample conduit. The sample conduit includes an inlet communicating with the sample receiving chamber, an outlet communicating with the ion extraction chamber, and a length extending between the inlet and the outlet outside the sample receiving chamber. The sample conduit further includes a nonlinear section located in the length whereby the sample conduit establishes a sample material flow path that includes a turn.

[0014] According to another implementation, an ionization apparatus includes a sample receiving chamber including a boundary defining a sample receiving chamber interior, an ion extraction chamber separate from the sample receiving chamber and including an ion exit aperture and an exhaust aperture, a sample conduit communicating with the sample receiving chamber and the ion extraction chamber, and a device for applying an electrical field in the ion extraction chamber of a polarity opposite to the polarity of ions entering the ion extraction chamber from the sample conduit outlet.

[0015] According to another implementation, an ionization apparatus includes a sample receiving chamber including a boundary defining a sample receiving chamber interior, a sample conduit, and a device for accelerating or decelerating ions in the sample conduit. The sample conduit includes an inlet communicating with the sample receiving chamber, an outlet
5 communicating with the ion extraction chamber, and a length extending between the inlet and the outlet outside the sample receiving chamber.

[0016] According to yet other specific implementations the ionization apparatus comprises the following features.

[0017] The drying gas within the sample conduit is mixed with the sample material flow and
10 the product of the pressure times the length of the conduit is in a range between 100 and 10,000 Torr x cm or the product of the pressure times the length of the conduit is in a range between 200 and 2000 Torr x cm.

[0018] The sample conduit further comprises a nonlinear section whereby the sample material flow path includes a turn. The nonlinear section may include a bend or a coiled section.

15 [0019] An axis of the sample conduit inlet is parallel to an axis of the sample conduit outlet or an axis of the sample conduit inlet is oriented at a non-zero angle relative to an axis of the sample conduit outlet.

[0020] The ion extraction chamber of the ionization apparatus communicates with the sample conduit outlet and comprises an ion exit aperture and an exhaust aperture. The ionization
20 apparatus further comprises a device for applying an electrical field in the ion extraction chamber of a polarity opposite to the polarity of ions entering the ion extraction chamber from the sample conduit outlet.

[0021] According to another implementation, a method for extracting ions from a sample material includes ionizing sample material in a sample receiving chamber. A sample conduit is
25 provided within an interface chamber. Drying gas is flowed into the sample conduit for mixing an ionized sample material with the drying gas for obtaining within the sample conduit the product of the pressure times the length of the conduit being equal or greater than 50 torr x cm.

[0022] According to another implementation, a method for extracting ions from a sample material includes ionizing sample material in a sample receiving chamber. Heated drying gas is
30 flowed into an interface chamber separate from the sample receiving chamber, around a sample conduit disposed in the interface chamber, and into the sample receiving chamber via a drying gas outlet. At least a portion of the ionized sample material and the drying gas is flowed from the sample receiving chamber into the sample conduit via a sample conduit inlet disposed

proximate to the drying gas outlet. The heated drying gas in the interface chamber is utilized to heat the ionized sample material and the drying gas flowing through the sample conduit.

[0023] According to another implementation, a method for extracting ions from a sample material includes ionizing sample material in a sample receiving chamber, and flowing at least a portion of the ionized sample material along with drying gas from the sample receiving chamber, through a sample conduit and into an ion extraction chamber. The sample conduit defines a flow path for the ionized sample material and drying gas that includes a sample conduit inlet communicating with the sample receiving chamber, an outside section of the sample conduit disposed outside the sample receiving chamber, and a turn in the sample conduit located in the outside section.

[0024] According to another implementation, a method for extracting ions from a sample material includes ionizing sample material in a sample receiving chamber, flowing at least a portion of the ionized sample material along with drying gas from the sample receiving chamber to an ion extraction chamber, and applying an electrical field in the ion extraction chamber having a polarity opposite to the polarity of ions of the ionized sample material flowing into the ion extraction chamber to slow the flow rate of the ions as the ions enter the ion extraction chamber.

[0025] According to another implementation, a method for extracting ions from a sample material includes ionizing sample material in a sample receiving chamber, flowing at least a portion of the ionized sample material along with drying gas from the sample receiving chamber into a sample conduit extending outside the sample receiving chamber, and applying a voltage jump to the ionized sample material flowing through the sample conduit whereby charged species of the ionized sample material are accelerated or decelerated relative to uncharged species of the ionized sample material and the drying gas.

[0026] According to another implementation, an ionization apparatus includes a sample receiving chamber, a sample ionizing device communicating with the sample receiving chamber, a drying gas outlet communicating with the sample receiving chamber, a sample conduit communicating with the sample receiving chamber and including a sample conduit inlet and a sample conduit outlet, and an ion extraction chamber receiving the sample conduit outlet. The ion extraction chamber includes an ion exit orifice spaced from the sample conduit outlet by a gap. An inside diameter of the ion exit orifice is less than an inside diameter of the sample conduit outlet. A central axis of the ion exit orifice is substantially coincident with a central axis of the sample conduit outlet.

[0027] According to another implementation, a method for extracting ions from a sample material includes ionizing sample material in a sample receiving chamber at a pressure above atmospheric pressure, and flowing at least a portion of the ionized sample material along with drying gas from the sample receiving chamber, through a sample conduit and to an ion

5 extraction chamber, the ion extraction chamber being at atmospheric pressure.

BRIEF DESCRIPTION OF THE DRAWINGS

[0028] The invention can be better understood by referring to the following figures. The components in the figures are not necessarily to scale, emphasis instead being placed upon illustrating the principles of the invention. In the figures, like reference numerals designate corresponding parts throughout the different views.

[0029] Figure 1 is a schematic view of an example of an ionization apparatus according to one implementation.

[0030] Figure 2 is a schematic view of an example of an ionization apparatus according to another implementation.

[0031] Figure 3 is a schematic view of an example of an ionization apparatus according to another implementation.

[0032] Figure 4 is a schematic view of an example of an ionization apparatus according to another implementation.

[0033] Figure 5 is a schematic view of an example of an ionization apparatus according to another implementation.

[0034] Figure 6 is a schematic view of an example of an ion extraction chamber according to one implementation.

[0035] Figure 7 is a schematic view of an example of a sample conduit according to one implementation.

[0036] Figure 7A is a schematic view of an example of a portion of a sample conduit according to another implementation.

[0037] Figure 7B is a schematic view of an example of a portion of a sample conduit according to another implementation.

[0038] Figure 8 is a schematic view of an example of an ionization apparatus according to another implementation.

[0039] Figure 9 is a schematic view of an example of an ionization apparatus according to another implementation.

DETAILED DESCRIPTION OF THE INVENTION

[0040] In general, the term “communicate” (for example, a first component “communicates with” or “is in communication with” a second component) is used herein to indicate a structural, functional, mechanical, electrical, optical, magnetic, ionic or fluidic relationship between two or more components or elements. As such, the fact that one component is said to communicate with a second component is not intended to exclude the possibility that additional components

may be present between, and/or operatively associated or engaged with, the first and second components.

[0041] In the context of the present disclosure, the term “atmospheric pressure” is not limited to an exact value for atmospheric pressure such as 1 atmosphere (760 Torr) at sea level.

5 Instead, the term “atmospheric pressure” also generally encompasses any pressure that is substantially at (i.e., about, approximately, or near) atmospheric pressure. Accordingly, “atmospheric pressure” generally encompasses a range of pressures from about 100 Torr to about 7,000 Torr (or about 0.1 atm to about 10 atm). In addition, implementations of ionization apparatus and methods disclosed herein are not limited to operation at atmospheric pressure, but
10 instead generally include ionization at any above-vacuum pressure, i.e., any pressure not normally considered to be a vacuum pressure, as well as pressures significantly higher than atmospheric and near-atmospheric pressure. Accordingly, in the context of the present disclosure, the term “above-vacuum pressure” generally encompasses any pressure within a range of about 10 Torr (or about 0.01 atm) or greater.

15 [0042] For convenience, the term “mass spectrometer” is used herein in a general, non-limiting sense to refer to a mass analyzing/sorting device and any associated components typically operating within an evacuated or low-pressure space that receives an input of analyte ion-bearing sample material from an API interface or other type of ionization interface operating at above-vacuum pressures.

20 [0043] The subject matter disclosed herein generally relates to systems, apparatus, devices, instruments, processes and methods related to ionization of samples typically for the purpose of sample analysis. Examples of implementations relating to the invention are described in more detail below with reference to Figures 1-9. These examples are provided in the context of mass spectrometry (MS), but it will be recognized that the broad aspects of the invention may be
25 applicable to other types of analytical instrumentation. Generally, any process in which the production of ions is desired, including the use of analytical instruments other than mass spectrometers, may fall within the scope of this disclosure.

[0044] Figure 1 is a schematic view of an example of an ionization apparatus or system **100** according to one implementation. The ionization apparatus **100** may, for example, be
30 operatively associated with a mass spectrometer **104**. The ionization apparatus **100** includes a sample ionization device **108** for ionizing a sample. The sample ionization device **108** may be any suitable ionization device such as, but not limited to, an ionization device utilized in conjunction with ESI, APCI, APPI, or AP MALDI as briefly summarized above. It will be noted, however, that in multi-mode implementations the illustrated sample ionization device **108**

may represent two or more of the foregoing types of ionization devices provided in the same sample receiving chamber **124** and operated concurrently or sequentially. In practice, the utilization of different types of ionization techniques, such as ESI, APCI, APPI or AP MALDI, may be complementary and thus highly useful. Moreover, while such devices are

5 conventionally associated with atmospheric-pressure ionization (API), implementations of the subject matter taught herein are not limited to operation at atmospheric pressure, as noted above.

[0045] Depending on the specific ionization technique being implemented, the sample ionization device **108** may include a conduit (e.g., capillary, needle, small tube, etc.) **112** in which a sample material to be ionized flows and, optionally, a coaxially disposed outer conduit
10 **116** in which an inert nebulizing gas such as nitrogen (N₂) flows. Other components, such as a vaporizing device, an electrical or electromagnetic energy input device (e.g., voltage source, counter-electrode, electrospray needle, corona discharge electrode, photon source, laser, etc.), and the like, may be included as needed for implementing a particular ionization technique as understood by persons skilled in the art. For simplicity, such other components are not
15 illustrated. In all such ionization techniques, sample material typically is emitted from the sample ionization device **108** as a stream of gas and vapor components (e.g., jet, spray, electrospray, aerosol, etc.), which for convenience will be referred to as a sample droplet stream or ionized sample material **120** regardless of form or composition.

[0046] For purposes of the present disclosure, no specific limitations are placed on the
20 composition of the sample material, the manner in which the sample material is provided to the sample ionization device **108**, or fluid dynamic parameters such as flow rate, pressure, viscosity, and the like. In a typical implementation, the sample material provided to the sample ionization device **108** is predominantly a fluid but in other implementations may be a solid or a multi-phase mixture. In many implementations involving API, the fluid is predominantly in a liquid phase.
25 For example, the sample material may be a solution in which analyte components are initially dissolved in one or more solvents or carried by other types of components. In addition to solvents, other auxiliary components (that is, components for which analysis is not necessary but enhanced) may be present, such as excipients, buffers, additives, dopants, reagents, or the like. As another example, the sample material may be the eluent from a chromatographic,
30 electrophoretic or other analytical separation process, in which case the sample material may be a matrix composed of analyte and mobile-phase components. Depending on the location of a given portion of sample material in the ionization apparatus **100** or the procedural stage at which ionization is occurring, the sample material may comprise primarily ions alone or ions in combination with other components such as charged and/or neutral droplets, vapor, gas, or the

like. Accordingly, the term “sample material” as used herein is not limited by any particular phase, form, or composition. Moreover, the sample material flowing through the sample ionization device **108** may originate from any suitable source or sample inlet system (not shown), such as a batch volume, a sample probe, or an upstream instrument or process. For example, the inlet into the sample ionization device **108** may comprise or communicate with the outlet of an analytical separation system or device such as a chromatographic column. As other examples, the sample material may be supplied to the sample ionization device **108** from a liquid handling system, a reservoir, a syringe or other sample moving device, or a dissolution testing system. The flow of the sample material to or through the sample ionization device **108** may be induced by any means, such as pumping, moving boundary, pressure differential, capillary action, or electrically-related techniques.

[0047] As illustrated in Figure 1, the sample droplet stream **120** flows into the interior of a sample receiving chamber (or ionization chamber) **124**. The sample receiving chamber **124** may be defined by any suitable housing or enclosing structure, including a wall or other boundary or structure **128**. The sample receiving chamber **124** provides an enclosed region in which full or partial ionization of a sample material may occur as part of a desired analytical procedure such as detecting analyte ions in mass spectrometry. At least one wall or portion of a wall of the sample receiving chamber **124**, for example the boundary **128**, includes an opening for receiving a sample interface conduit **132** having an inlet **136**. The sample conduit inlet **136** serves as a sample outlet orifice of the sample receiving chamber **124**, whereby sample material exits the sample receiving chamber **124** and enters the sample conduit **132** via the inlet **136** generally in the direction indicated by a flow arrow **140**. The sample conduit inlet **136** may be flush or substantially flush with (or register with) the corresponding opening of the sample receiving chamber **124**, or alternatively the inlet end of the sample conduit **132** may extend into the sample receiving chamber **124**. In all such cases, the sample conduit inlet **136** may be characterized as being positioned or located at the boundary **128**. The same boundary **128** of the sample receiving chamber **124** may also include a drying gas outlet **144** by which drying gas is admitting into the sample receiving chamber **124**. The drying gas outlet **144** may be flush or substantially flush with the surface of the boundary **128** facing the sample receiving chamber **124**, or alternatively may extend into the sample receiving chamber **124**. The drying gas outlet **144** may include one or more drying gas orifices, slits, arcuate slots, or the like located proximate to the sample conduit inlet **136**. Accordingly, in the implementation illustrated in Figure 1, drying gas is introduced into the sample receiving chamber **124** via the drying gas outlet **144** generally in the direction(s) indicated by a flow arrow or arrows **148**. At least the

initial flow **148** of drying gas may be generally counter to or in reverse to the flow **140** of exiting sample material. However, the initial direction of the flow **148** of drying gas may be in any direction, e.g., the same direction as the flow **148** of sample material. Moreover, drying gas may constitute a component of the exiting flow **140** in combination with the sample material

5 provided in the sample droplet stream **120**.

[0048] The ionization apparatus **100** may also include an interface or intermediate chamber **152**. The interface chamber **152** may be defined by any suitable housing or enclosing structure. One or more walls, boundaries or other structures of the interface chamber **152** may be shared with the sample receiving chamber **124** and thus serve as a partition between the sample
10 receiving chamber **124** and the interface chamber **152**, for example the boundary **128** as illustrated in Figure 1. The boundary **128**, as well as other boundaries described in the present disclosure, generally encompass one distinct side of a given chamber, and thus may include not only a single planar wall or surface but also other structural features associated with that wall or surface. In the example illustrated in Figure 1, the interface chamber **152** provides an enclosed
15 interior through which most or all of the length of the sample conduit **132** runs. At least one wall or portion of a wall of the interface chamber **152**, for example a boundary **156**, includes an opening for receiving an outlet **158** of the sample conduit **132**.

[0049] The sample conduit **132** serves as a distinct interface or stage intermediately positioned between the sample receiving chamber **124** and the low-pressure/vacuum regions of
20 the mass spectrometer **104**. In some implementations, the sample conduit **132** includes at least one nonlinear section (structure, feature, etc.) such that the internal flow path defined by the sample conduit **132** includes at least one turn. That is, when considering at least two given points along the length of the sample conduit **132**, the center axis of the internal cross-section of the sample conduit **132** at the one point will be oriented at a non-zero angle relative to the center
25 axis of the internal cross-section at the other point. In this manner, at one or more points along the length of the sample conduit **132**, the center axis of the internal cross-section encounters and passes through the inside surface of the sample conduit **132**, such that liquid droplets or other heavier components of the sample material flowing along this axis will impinge on the inside surface. The nonlinear section(s) may be provided to increase the energy exchange between the
30 sample conduit wall, the drying gas, and the sample material, resulting in desolvation of sample cluster ions and evaporation of liquid droplets.

[0050] For example, the sample conduit **132** may include one or more bends or turns between the inlet **136** and outlet **158**, thereby establishing a non-linear (e.g., single-bend, multi-bend, convoluted, serpentine, etc.) flow path of extended length along which the sample material

and drying gas are transported from the sample receiving chamber **124** toward the mass spectrometer **104**. The turn or bend in the sample conduit **132** may range from being sharp or abrupt to being curved with a relatively large radius of curvature, as appropriate for the flow rate through the sample conduit **132**, the pressure in the sample conduit **132**, and the expected composition of the sample material. In the example illustrated in Figure 1, a significant portion of the length of the sample conduit **132** turns along a loop, spiral, or helix. This type of nonlinear feature results in a curved flow path with many centerline axes angled relative to one another, thus providing many opportunities for sample components to encounter the inner wall of the sample conduit **132**. In other examples, the sample conduit **132** may include an elbow or L-shaped section, a U-shaped section, etc.

[0051] The ionization apparatus **100** also includes a drying gas source **160** for supplying a suitable drying gas to the ionization apparatus **100**. The drying gas may be, for example, nitrogen (N_2). The drying gas source **160** includes one or more drying gas source inlets **164** by which one or more flows **168** of drying gas are introduced into the ionization apparatus **100**.

The drying gas source **160** may also include a means or device (not specifically shown) for heating the drying gas prior to its introduction into the ionization apparatus **100**, as well as a means for flowing the drying gas and regulating the flow rate or pressure of the drying gas such as a pump and associated components. One of the boundaries of the interface chamber **152**, for example the boundary **170** as illustrated in Figure 1, may include an opening, fitting, feed-through or the like for accommodating a conduit of the drying gas source **160** that terminates at the drying gas inlet **164**, in which case the drying gas source **160** communicates with the interface chamber **152**. The drying gas source outlet **164** may be flush or substantially flush with the corresponding opening of the boundary **170** of the interface chamber **152**, or may extend into the interface chamber **152**.

[0052] Accordingly, in the example illustrated in Figure 1, the ionization apparatus **100** is configured to establish a flow path for the heated drying gas into the interface chamber **152** via one or more drying gas source inlets **164** as indicated by the flow arrow **168**, through the interior of the interface chamber **152**, and from the interface chamber **152** into the sample receiving chamber **124** via a drying gas outlet **144** (e.g., one or more drying gas orifices) as indicated by the flow arrow(s) **148**. The flow of drying gas through the interface chamber **152** is physically separate from the flow of sample material and drying gas through the sample conduit **132**. However, as the drying gas travels through the interior of interface chamber **152**, the drying gas may flow around and in thermal contact with the outer surface of the sample conduit **132**, thereby heating the sample material flowing through the sample conduit **132** as well as

maintaining an elevated temperature of the drying gas flowing with the sample material through the sample conduit **132**. The sample conduit **132**, including the sample conduit inlet **136** and outlet **158**, may be positioned in the interface chamber **152** relative to the drying gas source inlet **164** and drying gas outlet **144** as needed to heat the sample material flowing through the sample conduit **132**. Likewise, the drying gas source inlet **164**, including the angle or orientation of the initial direction of the drying gas flow **168**, and drying gas outlet **144** may be positioned relative to the sample conduit **132** as needed to effectively heat the sample material flowing through the sample conduit **132**. With the foregoing considerations in mind, it will be understood that the relative positions and orientations of the drying gas source inlet **164**, the drying gas outlet **144**, and the sample conduit **132** have been illustrated in Figure 1 arbitrarily and by way of example only.

[0053] If needed or desired, additional components (not shown) may be utilized to optimize the transfer of thermal energy from the drying gas introduced into the interface chamber **152** and the sample conduit **132**. For example, the drying gas source **160** may include a plenum or manifold that routes the drying gas to two or more appropriately positioned drying gas source inlets **164**. As another example, plenums, baffles or other structures may be provided in the interface chamber **152** to modify the drying gas flow path in the interface chamber **152** in a desired manner.

[0054] As an alternative or in addition to utilizing the drying gas to heat the sample conduit **132**, other means for heating the sample conduit **132** may be employed. For example, resistive heating means (not shown) may be employed, such as by running electrical current through a conductive layer or section of the sample conduit **132**. In another example, an electrical cartridge may be employed to heat the sample conduit **132**. The use of means other than the drying gas to heat the sample conduit **132** may be desirable for independently controlling the heating of the sample conduit **132** and the flow of the drying gas.

[0055] As an alternative or in addition to the use of one or more drying gas outlets **144** to allow drying gas to be admitted into the sample conduit **132** at the sample conduit inlet **136**, one or more apertures **169** may be formed through the wall of the sample conduit **132** at more or more points along the length of the sample conduit **132** for the same purpose of establishing contact between the heated drying gas and the sample material flowing through the sample conduit **132**. As an example, Figure 1 illustrates a drying gas inlet aperture **169** located at or near the middle-length of the sample conduit **132**. The pressure differential between the interface chamber **152** and the interior of the sample conduit **132** is sufficient to draw the drying gas into the sample conduit **132** at the desired location along its length. The size of the aperture

169 and/or the number of apertures **169** provided may be selected so as to attain the desired flow characteristics of the drying gas into the sample conduit **132**.

[0056] The ionization apparatus **100** may also include an ion extraction or exit chamber **172**. The ion extraction chamber **172** may be defined by any suitable housing or enclosing structure.

5 One or more walls, boundaries or other structures of the interface chamber **152** may be shared with other chambers or regions of the ionization apparatus **100**. For example, the boundary **156** illustrated in Figure 1 may serve as a partition or common side between the interface chamber **152** and the ion extraction chamber **172**. As noted above, this boundary **156** may include an opening for receiving the sample conduit outlet **158**. The sample conduit outlet **158** may be
10 flush or substantially flush with this opening, or the outlet end of the sample conduit **152** may extend into the ion extraction chamber **172**. The ion extraction chamber **172** provides an enclosed interior into which sample material flows from the sample conduit outlet **158**, as generally indicated by a flow arrow **176**, in preparation for separation of analyte ions from non-analytical material and introduction of the analyte ions into the mass spectrometer **104**. The ion
15 extraction chamber **172** also provides openings for accommodating a sampling orifice **180** for receiving ions and an exhaust port **184** for receiving non-analytical material.

[0057] Unlike conventional ionization interfaces that are limited to operating at or close to atmospheric pressure, the interior of the sample receiving chamber **124** according to implementations presently disclosed may be at atmospheric (or ambient) pressure, near
20 atmospheric pressure, or significantly above or below atmospheric pressure. Generally, the pressure in the sample receiving chamber **124** may range from 100 Torr to 15,200 Torr, or 0.013 to 20 atmospheres, and should be higher than the pressure in the ion extraction chamber **172**. The drying gas, or both the drying gas and nebulizing gas such as may be provided by the sample ionizing device **108**, may be utilized to pressurize the sample receiving chamber **124** to a
25 desired background pressure for ionization. Pressurizing the sample receiving chamber **124** to an above-atmospheric pressure may assist in driving both drying gas and sample material into the sample conduit **132**.

[0058] The pressure in the interface chamber **152** may generally be any value. However, when the interface chamber **152** is utilized to direct a flow of drying gas to heat the sample
30 conduit **132**, the pressure in the interface chamber **152** may largely be dictated by the drying gas introduced from the drying gas source outlet **164**, in which case the pressure in the interface chamber **152** should be such as to facilitate or at least not impair this thermal energy-transferring function of the drying gas. Generally, the pressure in the interface chamber **152** may be at ambient or atmospheric pressure, may be the same or about the same as the pressure in the

sample receiving chamber **124**, or may be higher than the pressure in the sample receiving chamber **124**, for example about 5-40 Torr above the pressure in the sample receiving chamber **124**.

[0059] The pressure in the ion extraction chamber **172** may be any pressure suitable for extracting ions from the incoming sample flow **176** as well for maintaining a pressure differential between the sample receiving chamber **124** and the ion extraction chamber **172** so as to drive sample material and drying gas through the sample conduit **132**. In one example, the pressure in the ion extraction chamber **172** is on the order of a hundred or hundreds of Torr, a further example being about 200 Torr. In other examples, the pressure in the ion extraction chamber **172** may range up to an above-atmospheric pressure. It follows that the pressure in the interface itself, i.e., the sample conduit **132**, is lower than the pressure in the sample receiving chamber **124**. It will be noted, however, that the means by which sample material exits the sample receiving chamber **124** is the sample conduit **132** taught in the present disclosure, whereas in conventional ionization apparatus the exit means is the sampling orifice, i.e., the capillary or skimmer that leads directly into the low-pressure/vacuum pump stages of a mass spectrometer.

[0060] The pressure in the sample conduit **132**, including in the region of the inlet **136**, is higher than the pressure of a conventionally positioned sampling orifice. This higher pressure and longer time of contact between the sample material and the drying gas result in more efficient transfer of thermal energy between the heated drying gas and the solvent droplets and clustered ions of the sample material produced from the sample ionizing device **108**.

[0061] In operation, sample material is directed toward the sample conduit inlet **136** in the sample droplet stream **120** emitted from the sample ionizing device **108**. In addition, the charged components of the sample droplet stream **120** may be attracted toward the sample conduit inlet **136** by applying a suitably directed electrical field in the sample receiving chamber **124**. For example, a potential difference may be established between a component of the sample ionizing device **108** such as an electrospray needle, a corona discharge electrode, a photon source or other conductive element, and the sample conduit inlet **136** or other conductive element proximate to the sample conduit inlet **136**. Sample material is drawn into the sample conduit inlet **136** as a result of the pressure difference between the sample receiving chamber **124** and the sample conduit **132**. The flow **140** of sample material into the sample conduit inlet **136** may be assisted through application of an electrical field as noted above or an additional electrical field. In addition, if the sample receiving chamber **124** is pressurized to a relatively

high level above atmospheric pressure, such pressurization may act to push sample material into the sample conduit inlet **136**.

[0062] The sample material flows into the sample conduit inlet **136**. In implementations that provide the drying gas outlet(s) **144** in the illustrated location, the sample material initially flows against the counter-flow **148** of drying gas. The drying gas thus contacts the sample material in the region in front of the sample conduit inlet **136**, where the drying gas assists in evaporating liquid droplets and/or sweeping solvent droplets away from the sample conduit inlet **136**. Liquid droplets not evaporated or swept away as a result of this initial encounter with the drying gas then enter the sample conduit inlet **136** along with ions, charged clusters and other components of the sample material. Unlike conventional techniques, drying gas is also deliberately permitted to exit the sample receiving chamber **124** with the sample material and/or enter the sample conduit **132** via the aperture(s) **169** as described previously. As noted above, in conventional ionization apparatus, the exit for sample material from an ionization chamber is the sampling orifice (e.g., a capillary or skimmer) that leads directly into a mass spectrometer. In conventional techniques, the ideal process would be for only analyte ions to exit the sample receiving chamber **124**. These conventional techniques thus seek to maximize the evaporation and sweeping away of liquid droplets in the sample receiving chamber **124** and minimize entrainment of drying gas with the flow of sample material exiting the sample recovering chamber **124**. By contrast, in the implementation illustrated in Figure 1, the exit for sample material from the sample receiving chamber **124** is the inlet **136** into the sample conduit **132**, which provides an interface formed so as to significantly increase the degree of contact between the heated drying gas and the sample material as well as improve other performance criteria such as discussed below.

[0063] One or more features of the ionization apparatus **100** according to implementations such as the above-described example may be implemented to provide improved desolvation of sample ions, evaporation of droplets, and separation of sample ions from liquid droplets and matrix background components, thus enabling acquisition of a higher ion signal, lower chemical background, higher signal-to-noise ratio (S/N), higher sensitivity, and less contamination of the downstream analytical instrument such as a mass spectrometer **104**. The interface provided by the ionization apparatus **100**, in particular the sample conduit **132**, is operated at an elevated temperature by means such as described above, thus enhancing desolvation of the sample ions. Additionally, the sample ions, droplets and other components introduced into the sample receiving chamber **124** by the sample ionization device **108** are entrained into the sample conduit **132** together with the drying gas emanating from the drying gas outlet **144**. Collisions

between these components within the interior of the sample conduit **152** further enhance desolvation of the sample ions. Moreover, the drying gas remains in thermal contact with the droplets of the sample material for a longer time as compared with conventional ionization interfaces, resulting in more thermal energy being transferred to the droplets and thus enhancing evaporation of the droplets. By the time the sample material reaches the ion extraction chamber **172** as indicated by the flow **176**, most or all of the liquid-phase components have evaporated and the clustered and solvated ions have been liberated. Thermal energy transfer is also improved because the ionization apparatus **100** is configured to enable the interface to be operated at a relatively higher pressure as compared with conventional ionization interfaces. As indicated above, depending on path length, the interface may be operated from a couple of tens of Torr to several atmospheres. Also, the nonlinear path of sample material as established by a nonlinear (e.g., bent, spiral, convoluted, etc.) sample conduit **132** provides more collisions between sample ions and drying gas and forces larger liquid droplets to impinge on the inside surface of the sample conduit **132** due to momentum, centrifugal force, or the like. Each bent or turned section of the sample conduit **132** may have any angle and radius of curvature suitable for this purpose.

[0064] One indication or measurement of the total number of collisions occurring in the sample conduit **132** is to consider the product of the pressure within the sample conduit **132** and the length of the sample conduit **132** (Torr x cm, or Torr-cm). In one example, this pressure-length product ranges from 50 Torr-cm or greater. In another example, the pressure-length product ranges from 100 to 10,000 Torr-cm. In another example, the pressure-length product ranges from 200 to 2,000 Torr-cm. Depending on the length of the sample conduit **132**, the pressure in the sample conduit **132** may range from 20 Torr to 7,000 Torr. In another example, the pressure in the sample conduit **132** ranges from about 100 Torr to about 7,000 Torr. In another example, the pressure in the sample conduit **132** is about 200 Torr and the length of the sample conduit **132** is about 10 cm, giving a pressure-length product of 2,000 Torr-cm in this particular example. It will be noted that the pressure within the sample conduit **132** may be taken to be an average value, although it will be further noted that in typical implementations the change in pressure through the length of the sample conduit **132** is minimal. In many implementations, the pressure in the sample conduit **132** depends primarily on pumping speed.

[0065] Continuing with the present example of operation, after the sample material reaches the ion extraction chamber **172**, desolvated ions are extracted from the incoming flow **176** and enter the sampling orifice **180** as generally indicated by an arrow **188**, while neutral components and other non-analytical material are directed into the exhaust port **184** as generally indicated by

an arrow **192**. For this purpose, the exhaust port **184** may communicate with a suitable vacuum source such as a pump (not shown). In other implementations described below, the exhaust port may serve as a vent to an atmospheric environment. In the implementation illustrated in Figure 1, the axis of the sample conduit outlet **158** is generally aligned with the axis of the exhaust port **184** and the sampling orifice **180** is oriented in off-axis relation to the sample conduit outlet **158**. In other implementations described below, the axis of the sample conduit outlet **158** is generally aligned with the axis of the sampling orifice **180** and the exhaust port **184** is oriented in off-axis relation to the sample conduit outlet **158**. One or more voltage sources may be connected in electrical communication with conductive elements in the ion extraction region, such as the sample conduit **152**, the sampling orifice **180**, and one or more walls of the ion extraction chamber **172**, as needed to assist in extracting the desired analyte ions from the incoming flow **176**. In many implementations, however, the pressure differential between the ion extraction chamber **172** and the low-pressure or evacuated side of the sampling orifice **180** provides an adequate driving force for directing ions into the sampling orifice **180**. As further discussed below, appropriate voltages may applied so as to slow or retard the flow of ions flowing into the extraction chamber **172**.

[0066] The sampling orifice **180** serves as an ion inlet leading to the lower pressure and evacuated regions of the mass spectrometer **104**. Depending on the length of the ion passage into the mass spectrometer **104**, the sampling orifice **180** may constitute the inlet of a small-bore tube or capillary **196** such as illustrated by example in Figure 1. Continuing with this example, the mass spectrometer **104** may include one or more intermediate chambers or pump stages **202** and a mass analyzing stage **206**. The pump stage **202** illustrated in Figure 1 may be pumped down by a suitable pump, as represented by an arrow **210**, to a suitable sub-atmospheric pressure such as, for example, about 1 Torr. Ions transported by the capillary **196** flow through the pump stage **202** and into the mass analyzing stage **206** via an orifice such as may be provided in a skimmer plate **214**. The mass analyzing stage **206** may be pumped down by a suitable pump, as represented by an arrow **218**, to a suitable low vacuum pressure such as, for example, about 1 or 2 mTorr. The mass analyzing stage **206** may include various components associated with implementing mass spectrometry as appreciated by persons skilled in the art, such as ion guides and mass sorting devices. The pressure within the mass sorting device may be further reduced to a very low vacuum pressure such as, for example, 10^{-5} Torr or less. Various mass spectrometric techniques are known. The implementations taught by the present disclosure do not require any particular type of mass spectrometer **104**.

[0067] Figure 2 is a schematic view of another example of an interface structure of an ionization apparatus **250**. This implementation includes a coiled or helical sample conduit **232** that provides several turns in the flow path of the sample material. The sample conduit **232** includes an inlet **256** and an outlet **260**. The sample conduit inlet **256** is surrounded by several circumferentially spaced drying gas orifices **264** formed in a wall **268** of the interface chamber. This wall **268** may constitute a boundary shared with the sample receiving chamber into which the drying gas enters from the drying gas orifices **264**. The drying gas orifices **264** are radially spaced from the sample conduit inlet **256** by a small distance, thus enabling the drying gas to perform its conventional evaporating and sweeping functions in the sample receiving chamber as well as become entrained with the sample material into the sample conduit inlet **256**. The sample conduit outlet **260** registers with or extends through another wall **272** that adjoins the wall **268** at a common border. Other components illustrated in Figure 2 may be configured similar to like components described above and illustrated in Figure 1.

[0068] Figure 3 is a schematic view of another example of an interface structure of an ionization apparatus **300**. This implementation includes a sample conduit **332** having an inlet **336** and an outlet **358**. The sample conduit **332** includes a single bend or L-shaped feature. The angle of the bend may be 90 degrees or about 90 degrees as illustrated in Figure 3, or may be any other angle sufficient to provide a nonlinear sample material flow path in which large droplets may impinge against the inside surface of the sample conduit **332**.

[0069] Figure 4 is a schematic view of another example of an interface structure of an ionization apparatus **400**. This implementation includes a sample conduit **432** having an inlet **436** and an outlet **458**. The sample conduit **432** establishes a sample material flow path that turns 180 degrees such as by including two bends or L-shaped features, or a U-shaped feature. One boundary or side **428** provides openings for both the inlet end and outlet end of the sample conduit **432**. This boundary or side **428** may be shared by not only the sample receiving chamber **124** but also the ion extraction chamber **172**. In one example illustrated in Figure 4, the U-shaped feature includes a straight or substantially straight section **470** between two legs. In another example, also illustrated in Figure 4, the sample conduit **432** alternatively includes a curved section **471** between the two legs.

[0070] Figure 5 is a schematic view of another example of an interface structure of an ionization apparatus **500**. This implementation includes a sample conduit **532** having an inlet **536** and an outlet **558**. The sample conduit **532** includes two or more bends or L-shaped features. One boundary or side **528** provides an opening for the inlet end of the sample conduit **532**. Another boundary or side **530** provides an opening for the outlet end of the sample conduit

532. The boundary or side **530** is opposite to the boundary or side **528**, or at least is spaced from the boundary or side **528** by an intervening boundary or side **556**. In another alternative of the implementation illustrated in Figure 5, the sample conduit **532** again includes multiple bends but in the form of a coil or helix similar to configuration illustrated in Figure 2.

5 [0071] Regarding the examples described above and illustrated in Figures 2-5, the sample conduits **232**, **332**, **432** and **532** may include one or more apertures similar to the aperture **169** alternatively or additionally provided with the sample conduit **132** illustrated in Figure 1.

Moreover, the pressure within and length of the sample conduits **232**, **332**, **432** and **532**, and thus the pressure-length product obtained by these implementations, may be as provided above
10 in connection with the implementation corresponding to Figure 1.

[0072] The several implementations of nonlinear sample conduits illustrated in Figures 1-5 are given by way of example and not as limitations. The invention encompasses additional implementations for providing a nonlinear sample material flow path in which large droplets may impinge against the inside surface of the sample conduit.

15 [0073] In other implementations, as alternatives to the examples of ionization apparatus such as described above and illustrated in Figures 1-5, the drying gas source **160** or at least its outlet **164** may reside directly in the sample receiving chamber **124**. In this case, the drying gas source outlet **164** may be positioned at an orientation and proximity to the sample conduit inlet **136** whereby, similar to the above-described implementations, the drying gas interacts with the
20 sample material in the sample receiving chamber **124** and becomes entrained with the sample material into the sample conduit inlet **136**. As in the above-described implementations, heat from the drying gas is transferred to the sample material in front of the sample conduit inlet **136** as well as while both the drying gas and sample material travel through the sample conduit **132**. In another specific example, the drying gas may be introduced directly into the sample receiving
25 chamber **124** at a desired angle relative to the flow **120** of sample material emitted from the sample ionization device **108**, similar to the technique described in U.S. Patent No. 5,412,208. In the present invention, however, this technique results in the flows of drying gas and sample material intersecting in a region in front of the sample conduit inlet **136**. If needed to ensure maintenance of the sample material flowing through the sample conduit **132** at an elevated
30 temperature, a secondary or auxiliary source of heated gas may be provided to introduce heated gas into the interface chamber **152** to direct the auxiliary heated gas into thermal contact with the sample conduit **132**. That is, such implementations may include both a drying gas source inlet and an auxiliary heating gas source inlet.

[0074] Figure 6 is a schematic view of one example of an ion extraction chamber **600** that may be utilized in conjunction with any of the foregoing implementations. As represented by a flow arrow **604**, sample material is directed into the ion extraction chamber **600** via a sample conduit **608**. As represented by a flow arrow **612**, ions are extracted from the sample flow **604** and directed into an entrance **616** to a mass spectrometer via a sampling orifice **620**. As represented by a flow arrow **624**, neutrals and other non-analytical components of the sample material are directed out of the ion extraction chamber **600** via an exhaust port **628**, typically under the influence of a low-pressure or vacuum pump or, in other implementations, under atmospheric conditions.

[0075] In some implementations, the ion extraction chamber **600** provides a means for applying a retarding direct-current (DC) electric field across the ion extraction region to increase the efficiency of the process of ion extraction. The resultant force of this applied electrical field is (or may generally be) in the opposite direction to the incoming sample flow **604**, thus slowing down the ion flow in the extraction region. As a result, when a steady state is reached, ion density in the ion extraction region will be higher than in other areas. The retarding DC field applied at the ion extraction chamber **600** may be implemented by applying one or more appropriate voltages to one or more conductive surfaces associated with the ion extraction chamber **600**. For example, as illustrated in Figure 6, a conductive wall or wall section **632** of the ion extraction chamber **600** is electrically isolated from other conductive elements by insulating elements **636** and **640**. Another conductive wall or wall section **642** of the ion extraction chamber **600** is electrically isolated from the first wall **632** and other conductive elements by insulating elements **636** and **646**. The structure defining the sampling orifice **620** is electrically isolated from the walls **632** and **642** by the insulating elements **640** and **646**.

Voltage sources **650**, **654** and **658** or other suitable means are employed to apply voltages V1, V2 and V3 to the first wall **632**, second wall **642** and sampling orifice **620**, respectively. For positive ions, the voltage V1 is positively biased and is higher in magnitude than the voltage V2 to generate the retarding DC field. The potential difference $\Delta V = V1 - V2$ may range, for example, between approximately 200 V to approximately 2 kV. For extraction of positive ions into the sampling orifice **620**, the voltage V3 should be less than the voltage V2 and typically is 0 V or simply represents a ground state.

[0076] Figure 7 is a perspective view of an implementation in which one or more DC or radio-frequency (RF) voltage jumps are applied to a sample conduit **700** to promote collisions between sample ions and drying gas (and/or other neutrals). The sample conduit **700** includes an inlet **704** and an outlet **708**. The sample conduit **700** further includes two or more electrically

conductive segments, for example three segments **712**, **716** and **720**. The open ends of adjacent segments are separated by a gap and enclosed by a hollow insulating element. For example, the open ends of adjacent segments **712** and **716** are separated by a gap **724** enclosed by an insulating element **728**, and the open ends of adjacent segments **716** and **720** are separated by a gap **732** enclosed by an insulating element **736**. Voltage sources or other suitable means are placed in electrical communication with adjacent segments to generate voltage jumps across the gaps. For example, voltage sources **740** and **744** communicate with the adjacent segments **712** and **716** to apply a potential difference $V_4 - V_5$ across the gap **724**, which may be pulsed. The potential difference applied across each gap **724** or **732** may range, for example, between approximately 500 V to approximately 2 kV. The polarity of the applied electric field may be in either direction, regardless of the whether the ions traveling in the sample conduit **700** are positive or negative, or may be alternating. Depending on the polarity of the applied electric field relative to the polarity of the ions, the voltage jumps cause the ions and other charged components of the sample material to accelerate or decelerate relative to the electrically neutral components and the drying gas. The acceleration or deceleration of the ions is relative because the flow rate of the electrically neutral components and the drying gas remains dependent on non-electrical factors, such as the pressure differential between the sample conduit inlet **704** and the sample conduit outlet **708**, the expansion due to evaporation of liquid droplets, etc. Thus, as a result of the applied voltage jumps, collisions are promoted between accelerating charged species and drying gas molecules initially in front of the accelerating charged species and/or between decelerating charged species and drying gas molecules initially in back of the decelerating charged species.

[0077] Alternatively, Figure 7A illustrates a length or portion of a sample conduit **750** that has been split or segmented lengthwise into lengthwise segments **754** and **758** separated by a lengthwise or elongated gap **762**. The gap **762** in the sample conduit **750** may be enclosed by a hollow insulating element (not shown, but see similar insulating element **728** and **736** in Figure 7). Respective voltage sources **766** and **770** are placed in electrical communication with these lengthwise segments **754** and **758** to enable application of a potential difference $V_6 - V_7$ across the gap **762**, which may be pulsed. By this configuration an RF voltage jump may be applied transversely to the general direction of flow of sample material through the sample conduit **750**, thereby transversely shaking or perturbing the ions and other charged components to promote collisions with the drying gas molecules and/or other neutrals.

[0078] As a further alternative, Figure 7B illustrates a length or portion of a sample conduit **774** that has been split or segmented cross-wise into two (or more) cross-wise segments **776** and

778 separated by a cross-wise gap 780. Each cross-wise segment 776 and 778 is further split or segmented lengthwise into respective lengthwise segments 782, 783, 784 and 785, which are separated by corresponding lengthwise or elongated gaps 788 and 790. The gaps may be enclosed by hollow insulating elements (not shown) as needed. Respective voltage sources 792, 793, 794 and 795 are placed in electrical communication with the lengthwise segments 782, 783, 784 and 785 to enable application of a potential difference $V_6 - V_7$ across the corresponding lengthwise gaps 788 and 790, which may be pulsed. As illustrated in Figure 7B, the polarity of the potential difference may be reversed from one cross-wise segment 776 to another adjacent cross-wise segment 778 such that the electrical field applied to the ions alternates as the ions flow through successive cross-wise segments 776 and 778. By this configuration, DC voltage jumps may be applied transversely to the general direction of flow of sample material through the sample conduit 774, thereby transversely shaking or perturbing the ions and other charged components to promote collisions with the drying gas molecules and/or other neutrals. Note also that RF voltage jumps may also be applied in this implementation.

[0079] Figure 8 is a schematic view of another example of an ionization apparatus or system 800. As in the foregoing implementations, the ionization apparatus 800 includes a sample ionization device 108 for ionizing a sample and thus producing a sample droplet stream 120. The sample droplet stream 120 flows into the interior of a sample receiving chamber (or ionization chamber) 824. The sample receiving chamber 824 may be defined by any suitable housing or enclosing structure, including one or more walls or other types of structural boundaries. At least one wall or boundary 828, or portion of such wall or boundary 828, includes an opening for receiving a sample interface conduit 832 having an inlet 836 and an outlet 858. The sample conduit inlet 836 serves as a sample outlet orifice of the sample receiving chamber 824, whereby sample material exits the sample receiving chamber 824 and enters the sample conduit 832 via the inlet 836 generally in the direction indicated by a flow arrow 840. The sample conduit inlet 836 may thus be positioned or located at the boundary 828. That is, the sample conduit inlet 836 may be flush or substantially flush with the corresponding opening provided by the boundary 828, or the inlet end of the sample conduit 832 may extend into the sample receiving chamber 824. The sample conduit outlet 858 is disposed outside the sample receiving chamber 824 at some distance from the boundary 828. The same boundary 828 of the sample receiving chamber 824 may also include a drying gas outlet 844 (e.g., one or more drying gas orifices) located proximate to the sample conduit inlet 836. Accordingly, drying gas is introduced into the sample receiving chamber 824 via the drying gas outlet 844 generally in the direction(s) indicated by a flow arrow or arrows 848. At least the initial flow

848 of drying gas may be generally counter to or in reverse to the flow **840** of exiting sample material. Moreover, drying gas may constitute a significant component of the exiting flow **840** in combination with the sample material. The drying gas is supplied by a suitable drying gas source **860** via an inlet **864**. The drying gas source **860** may include a device (not specifically shown) for heating the drying gas. As an alternative or in addition to the use of the drying gas outlet **844**, drying gas may be introduced into the sample conduit **832** via one or more apertures (not shown) in the sample conduit **832** as described above in connection with the implementation illustrated in Figure 1.

[0080] The ionization apparatus **800** also includes an ion extraction or exit chamber **872**.

The ion extraction chamber **872** may be defined by any suitable housing or enclosing structure, which in turn may be defined by one or more walls, boundaries or other structures. One boundary **856** of the ion extraction chamber **872** may include an opening for receiving the sample conduit outlet **858**. The sample conduit outlet **858** may thus be positioned or located at the boundary **828**. That is, the sample conduit outlet **858** may be flush or substantially flush with the corresponding opening provided by the boundary **856**, or the outlet end of the sample conduit **832** may extend into the ion extraction chamber **872**. The ion extraction chamber **872** provides an enclosed interior into which sample material flows from the sample conduit outlet **856**, as generally indicated by a flow arrow **876**, in preparation for separation of analyte ions from non-analytical material and introduction of the analyte ions into the mass spectrometer **104**. The ion extraction chamber **872** also provides openings for accommodating a sampling orifice **180** and an exhaust port **884**. In the implementation illustrated in Figure 8, the sample conduit outlet **858** is aligned with the sampling orifice **180**, and the exhaust port **884** is oriented at an angle (off-axis) to the sample conduit outlet **858**.

[0081] The sample conduit **832** serves as a distinct interface or stage intermediately positioned between the sample receiving chamber **124** and the low-pressure/vacuum regions of the mass spectrometer **104** (see, e.g., Figure 1). In the implementation illustrated in Figure 8, the internal diameter of the sample conduit **832** is large relative to the diameter of sampling orifices, capillaries and other openings conventionally utilized for transferring sample material from an atmospheric-pressure ionization interface to evacuated regions of a mass spectrometer such as the illustrated sampling orifice **180**. The sample conduit **832** may also be relatively short. For example, the internal diameter of the sample conduit **832** may range from about 0.05 cm to about 1 cm, and the length from the sample conduit inlet **836** to the sample conduit outlet **858** may range from about 0.5 cm to about 5 cm. In another example, the length of the sample conduit **832** ranges from about 3 to about 4 cm. In another example, the internal diameter of the

sample conduit **832** may range from about 0.5 % to about 10 % of the length of the sample conduit **832**. In another example, the internal diameter of the sample conduit **832** may range from about 100 % to about 10,000 % of the internal diameter of the sampling orifice **180**.

[0082] In the implementation illustrated in Figure 8, the sample conduit **832** remains straight or linear along its length from the sample conduit inlet **836** to the sample conduit outlet **858**. In other implementations, similar to those described above, the sample conduit **832** may include at least one nonlinear structure or feature such as one or more bends or turns between the inlet **836** and outlet **858**, thereby establishing a non-linear flow path along which the sample material and drying gas are transported from the sample receiving chamber **124** to the mass spectrometer **104**. Whether the sample conduit **832** is entirely linear or includes one or more nonlinear features, the sample conduit outlet **858** is aligned or substantially aligned with the sampling orifice **180** in the implementation illustrated in Figure 8. For instance, the central axis of the sample conduit **858** may be collinear or substantially collinear with the central axis of the sampling orifice **180**.

[0083] In the implementation illustrated in Figure 8, the sample receiving chamber **824** may be maintained at an above-atmospheric pressure and the ion extraction chamber **872** may be maintained at an atmospheric or near-atmospheric pressure. The drying gas, or the drying gas in combination with a nebulizing gas such as may be provided by the ionizing device **108**, may be utilized to pressurize the sample receiving chamber **824** to the desired above-atmospheric pressure. The exhaust port **884** serves to vent the interior of the ion extraction chamber **872** to an ambient or near-ambient environment as indicated by an arrow **892**, thereby maintaining the ion extraction chamber **872** at the atmospheric or near-atmospheric pressure. As an example, the pressure in the sample receiving chamber **824** may range from approximately 1000 Torr to approximately 15,200 Torr, and the pressure in the ion extraction chamber **872** may range from approximately 500 Torr to approximately 1400 Torr. The resulting pressure differential between the inlet and outlet sides of the sample conduit **832** may be utilized to draw sample material from the sample droplet stream **120** and drying gas from the incoming drying gas flow **848** into the sample conduit inlet **836** as indicated by the flow arrow **840**. Because in this implementation the ion extraction chamber **872** may operate at or near atmospheric pressure, a large pump at this pump stage is not required, thus reducing costs.

[0084] The large-diameter sample conduit **832** functions as a gas restrictor tube that drops the gas pressure to at or near atmospheric pressure at its outlet end. Accordingly, sample flow **840** into the sample conduit inlet **836** may be increased by increasing the pressure in the sample receiving chamber **824** to above atmospheric as noted above. This configuration enables a much larger portion of the sample-bearing gas produced by the ionizing device **108**, and particularly

the desired analyte ions, to be directed toward the mass spectrometer **104**, as compared to conventional ionization apparatus in which a very small-diameter sampling orifice leading to evacuated regions is provided directly at the exit of the sample receiving chamber **824**. The ability to sample a much larger portion of the ionized plume produced in the sample receiving chamber **824** may be utilized to increase the sensitivity of the mass spectrometer **104**. The relatively high pressure and large volume within the sample conduit **832** enhances the collisions and thermal contact between the drying gas and the sample material. Moreover, the configuration results in a high concentration of sample material at the sample conduit outlet **858**, which in turns allows a large portion of the analyte ions to be collected in the sampling orifice **180**. The junction of the sample conduit outlet **858**, the sampling orifice **180**, and the intervening gap in the ion extraction chamber **872** may act as a momentum separator, whereby heavier ion-bearing sample material flows straight into the sampling orifice **180** as indicated by the flow arrow **888** and lighter material such as non-analytical solvent are vented through the exhaust port **884** as indicated by the flow arrow **892**. This action of momentum separation may be enhanced by providing a sample conduit **832** that is electrically conductive and applying a voltage to the sample conduit **832**, whereby charged components of the sample material accumulate on and near the centerline of the sample conduit **832**. As a further means for directing ions into the sampling orifice **180**, a conductive element **898** such as an aperture-containing plate, cylinder, or grid may be positioned between the sample conduit outlet **858** and the sampling orifice **180**.

[0085] Figure 9 is a schematic view of another example of an ionization apparatus or system **900**. The ionization apparatus **900** is similar to the ionization apparatus **800** described above and illustrated in Figure 8. Figure 9, however, illustrates that other features described earlier in this disclosure in connection with Figures 1-7 may also be applied to the ionization apparatus **800** or **900** illustrated in Figures 8 or 9. For instance, Figure 9 illustrates a large-diameter sample conduit **932** that includes a nonlinear feature. Figure 9 also illustrates an interface chamber **952** between a sample receiving chamber **924** and an ion extraction chamber **972**. The drying gas source inlet **164** of the drying gas source **160** is positioned relative to the sample conduit **932** and a drying gas outlet (e.g., one or more orifices) **944** so as to provide effective thermal energy transfer from the drying gas introduced into the interface chamber **952** to the sample conduit **932**.

[0086] In the implementations illustrated in Figures 8 and 9, the sample conduits **832** and **932** may include one or more apertures similar to the aperture **169** alternatively or additionally provided with the sample conduit **132** illustrated in Figure 1. Moreover, the pressure-length

product (Torr-cm) characterizing the sample conduit **832** or **932** may be as provided above in connection with the implementation corresponding to Figure 1.

[0087] It will be further understood that various aspects or details of the invention may be changed without departing from the scope of the invention. Furthermore, the foregoing

5 description is for the purpose of illustration only, and not for the purpose of limitation—the invention being defined by the claims.

WHAT IS CLAIMED IS:

1. An ionization apparatus comprising:

an interface chamber defined by a plurality of boundaries; and

a heated sample conduit extending through the interface chamber, the sample conduit

comprising an inlet and an outlet, each positioned within at least one of the boundaries and
establishing a sample material flow path separated from an interface chamber interior,

wherein within the sample conduit a drying gas is mixed with the sample material flow
and the product of the pressure times the length of said conduit is equal or greater than 50 Torr x
cm.

2. The ionization apparatus of claim 1, further comprising a drying gas outlet

communicating with the interface chamber interior and having a plurality of drying gas outlet
orifices arranged around the sample conduit inlet.

3. The ionization apparatus of claim 2, wherein the sample conduit comprises at least one
opening for introducing drying gas therein.

4. The ionization apparatus of claim 1, further comprising a device for accelerating or
decelerating ions in the sample conduit.

5. The ionization apparatus of claim 1, further comprising:

a sample receiving chamber including a boundary defining a sample receiving chamber
interior;

an ion extraction chamber separate from the sample receiving chamber and comprising
an ion exit aperture and an exhaust aperture;

the inlet of the sample conduit communicating with the sample receiving chamber, the
outlet communicating with the ion extraction chamber, and a length of the sample conduit
extending between the inlet and the outlet outside the sample receiving chamber, the sample
conduit further including a nonlinear section located in the length; and

a drying gas inlet communicating with the interface chamber, wherein the sample
material flow path runs from the sample receiving chamber to the ion extraction chamber
separate from the interface chamber interior, and the interface chamber establishes a drying gas
flow path from the drying gas inlet, around the sample conduit and to the drying gas outlet.

6. The ionization apparatus of claim 1, further comprising:
a sample receiving chamber communicating with the sample conduit inlet;
a sample ionizing device communicating with the sample receiving chamber;
a drying gas outlet communicating with the sample receiving chamber; and
5 an ion extraction chamber receiving the sample conduit outlet, the ion extraction chamber including an ion exit orifice spaced from the sample conduit outlet by a gap, an inside diameter of the ion exit orifice being less than an inside diameter of the sample conduit outlet, and a central axis of the ion exit orifice being substantially coincident with a central axis of the sample conduit outlet.

10 7. The ionization apparatus of claim 6, wherein the sample conduit has a substantially straight cross-section from the sample conduit inlet to the sample conduit outlet, whereby the sample conduit establishes a substantially straight sample material flow path from the sample receiving chamber to the ion extraction chamber.

15 8. The ionization apparatus of claim 6, wherein the sample conduit includes a nonlinear section located between the sample conduit inlet and the sample conduit outlet, whereby the sample conduit establishes a sample material flow path that includes a turn.

20 9. The ionization apparatus of claim 6, further including means for maintaining the pressure in the sample receiving chamber to an above-atmospheric pressure, and means for maintaining the pressure in the ion extraction chamber at atmospheric pressure.

25 10. A method for extracting ions from a sample material comprising:
ionizing sample material in a sample receiving chamber;
providing a sample conduit within an interface chamber;
flowing drying gas into the sample conduit for mixing an ionized sample material with the drying gas for obtaining within the sample conduit the product of the pressure times the length of the conduit being equal or greater than 50 Torr x cm.

30 11. The method of claim 10, further comprising flowing the ionized sample material from the sample conduit into an ion extraction chamber, and applying an electrical field in the ion extraction chamber having a polarity opposite to the polarity of ions of the ionized sample

material flowing into the ion extraction chamber to slow the flow rate of the ions as the ions enter the ion extraction chamber.

12. The method of claim 10, further comprising applying a voltage jump to the ionized sample material flowing through the sample conduit whereby charged species of the ionized sample material are accelerated or decelerated relative to uncharged species of the ionized sample material and the drying gas.

13. The method of claim 10, further comprising:

ionizing sample material in a sample receiving chamber at a pressure above atmospheric pressure; and

flowing at least a portion of the ionized sample material along with drying gas from the sample receiving chamber, through the sample conduit and to an ion extraction chamber, the ion extraction chamber being at atmospheric pressure.

14. The method of claim 10, further including flowing ions of the ionized sample material received in an ion extraction chamber into a sampling orifice communicating with a sub-atmospheric region of an analytical instrument.

15. The method of claim 14, wherein the ionized sample material is received in the ion extraction chamber via an outlet of the sample conduit having a central axis substantially coincident with the central axis of the sampling orifice, and the ions are flowed into the sampling orifice along a substantially linear flow path.

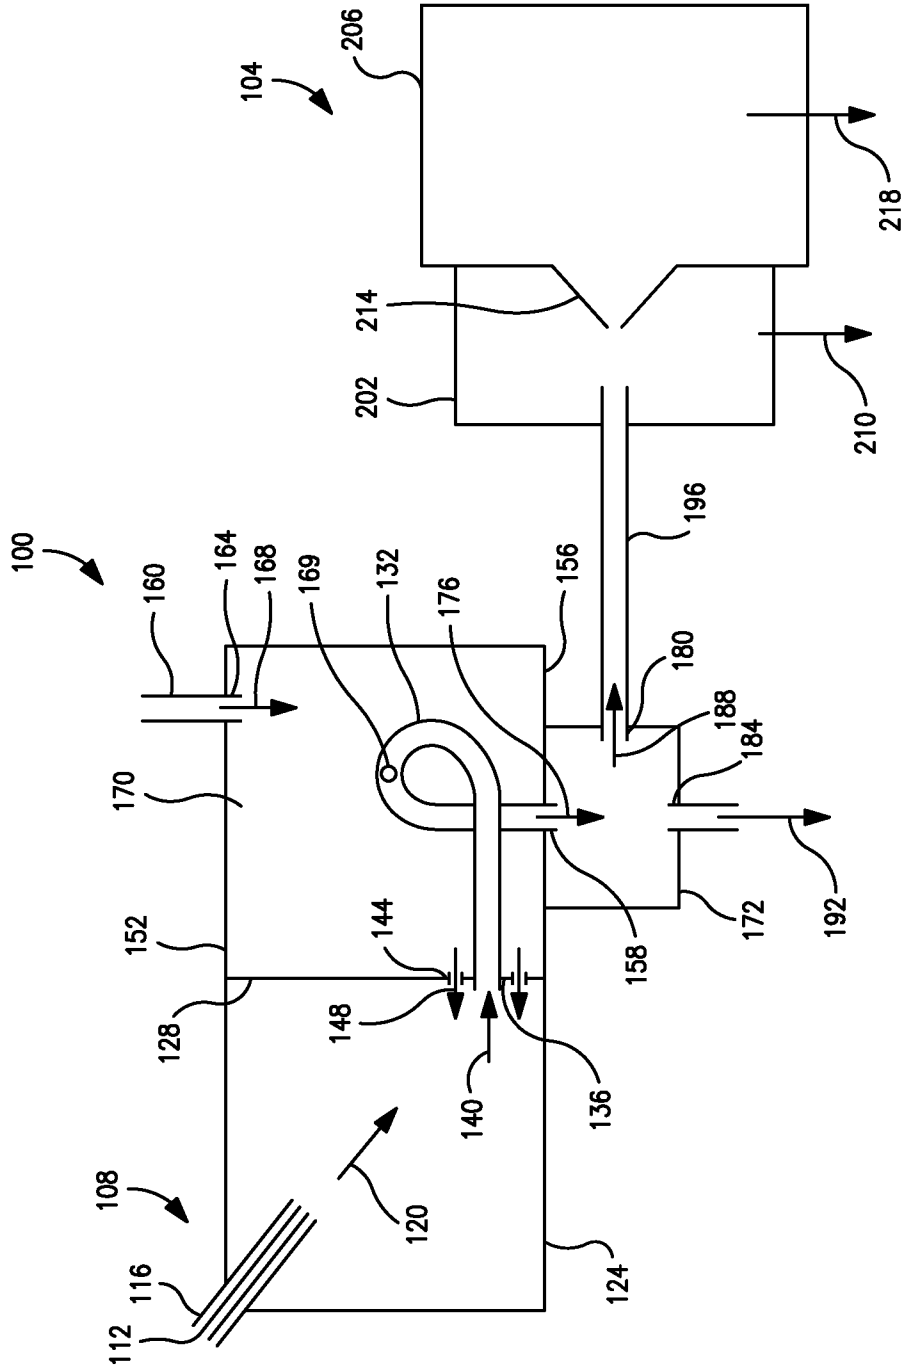


FIG. 1

2/11

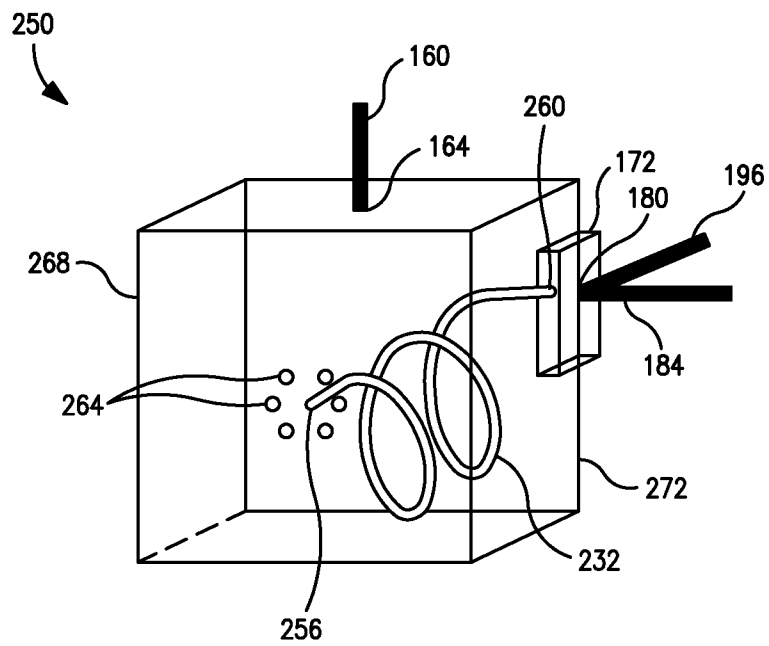
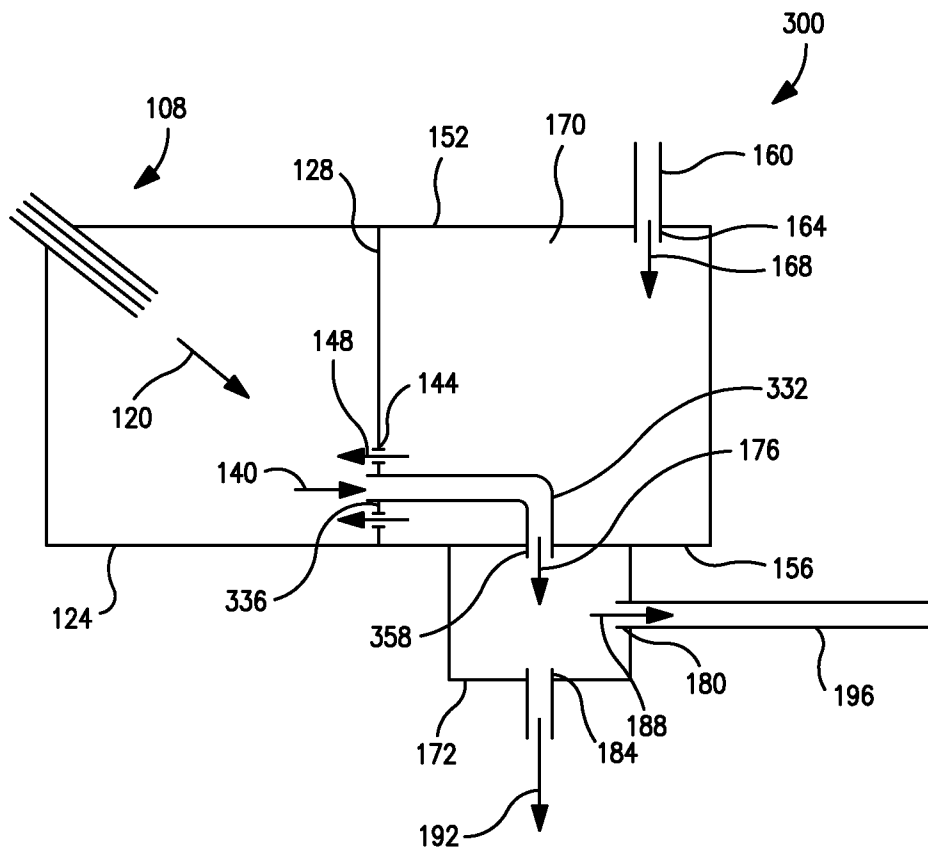
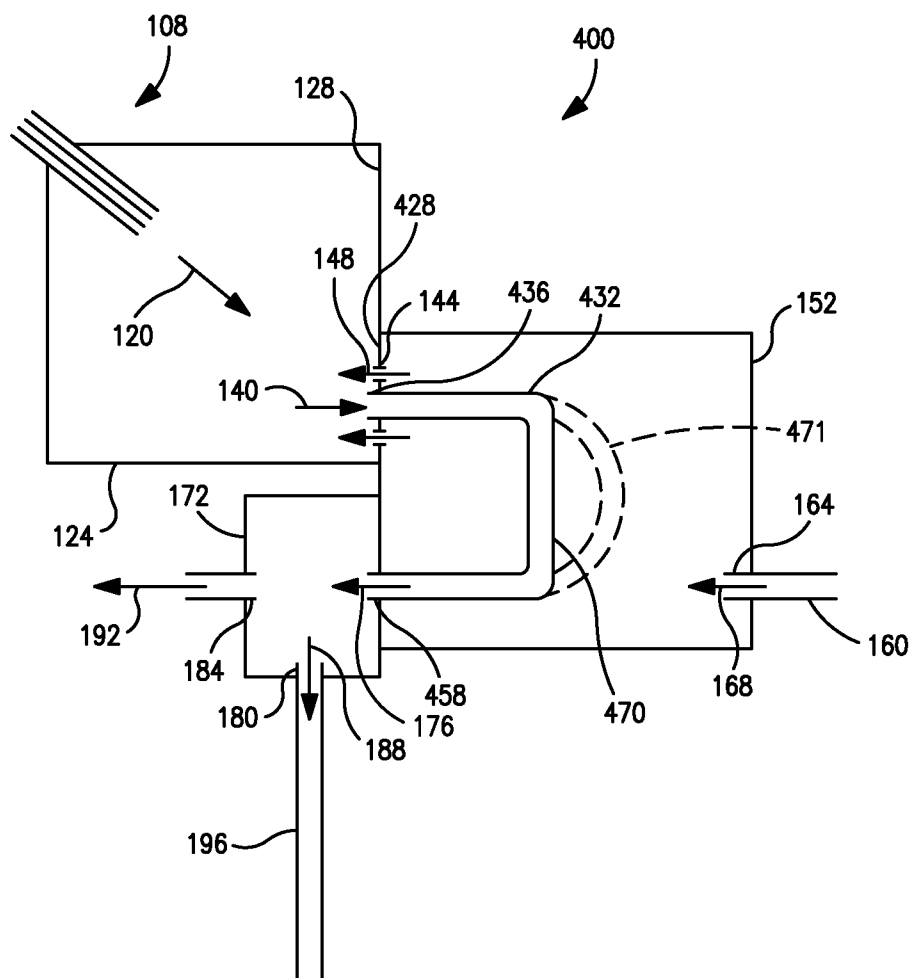


FIG. 2

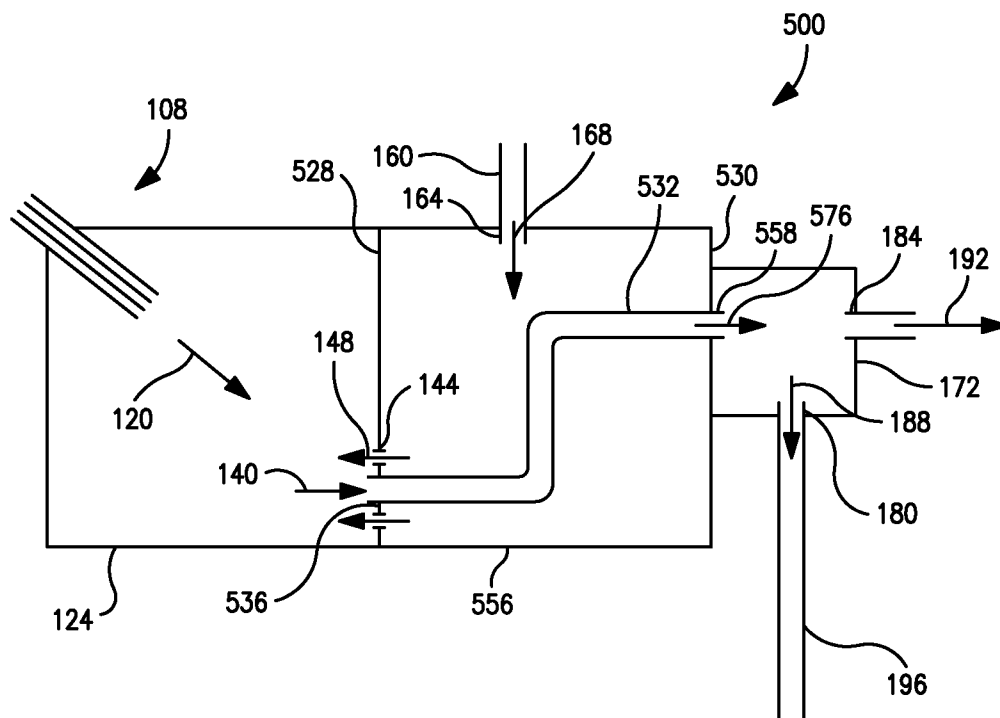
3/11

**FIG. 3**

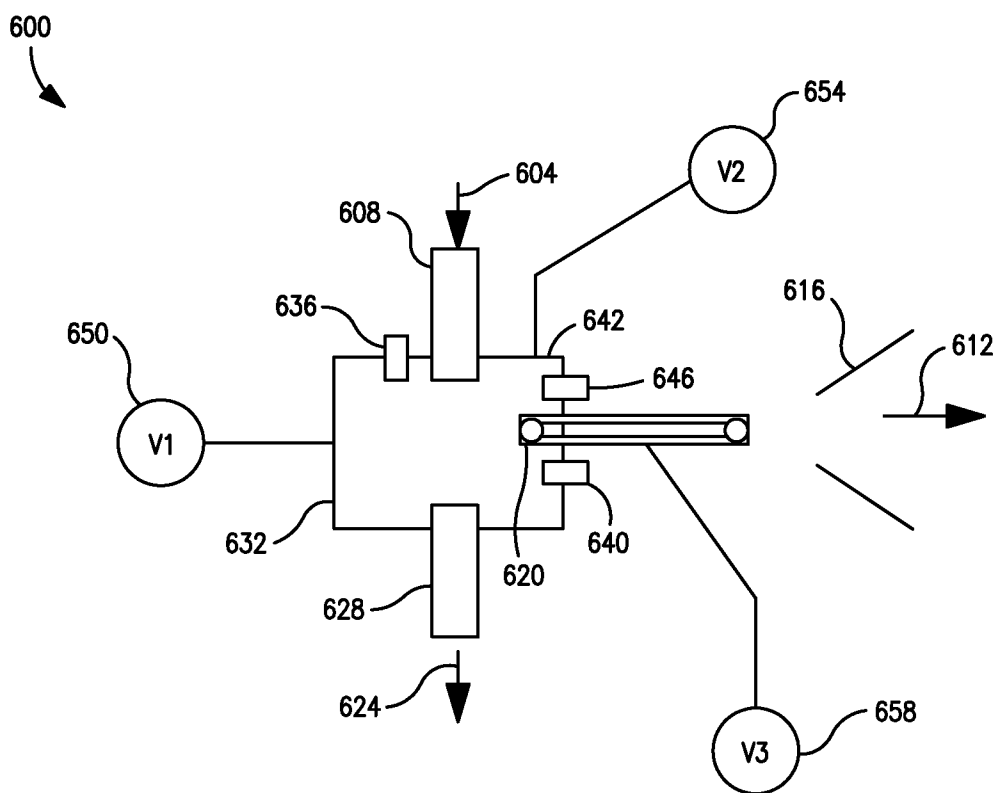
4/11

**FIG. 4**

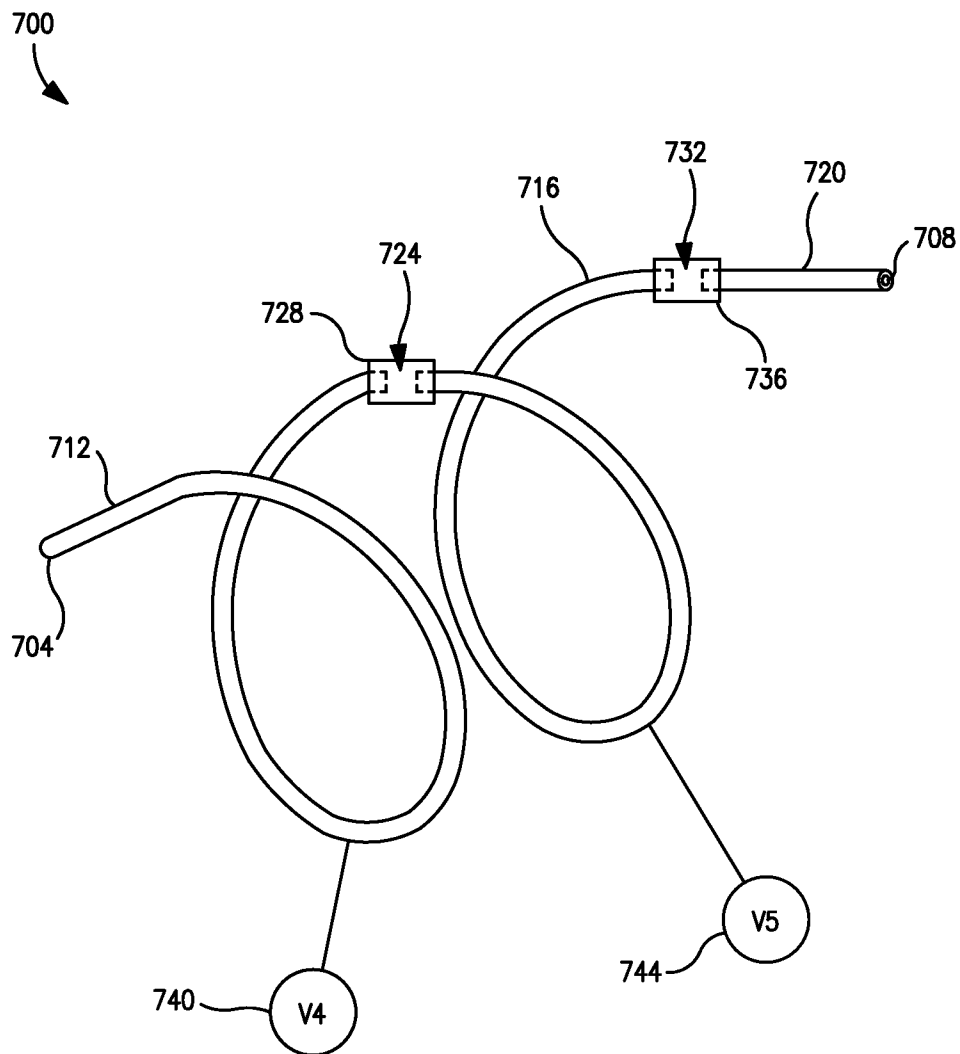
5/11

**FIG. 5**

6/11

**FIG. 6**

7/11

**FIG. 7**

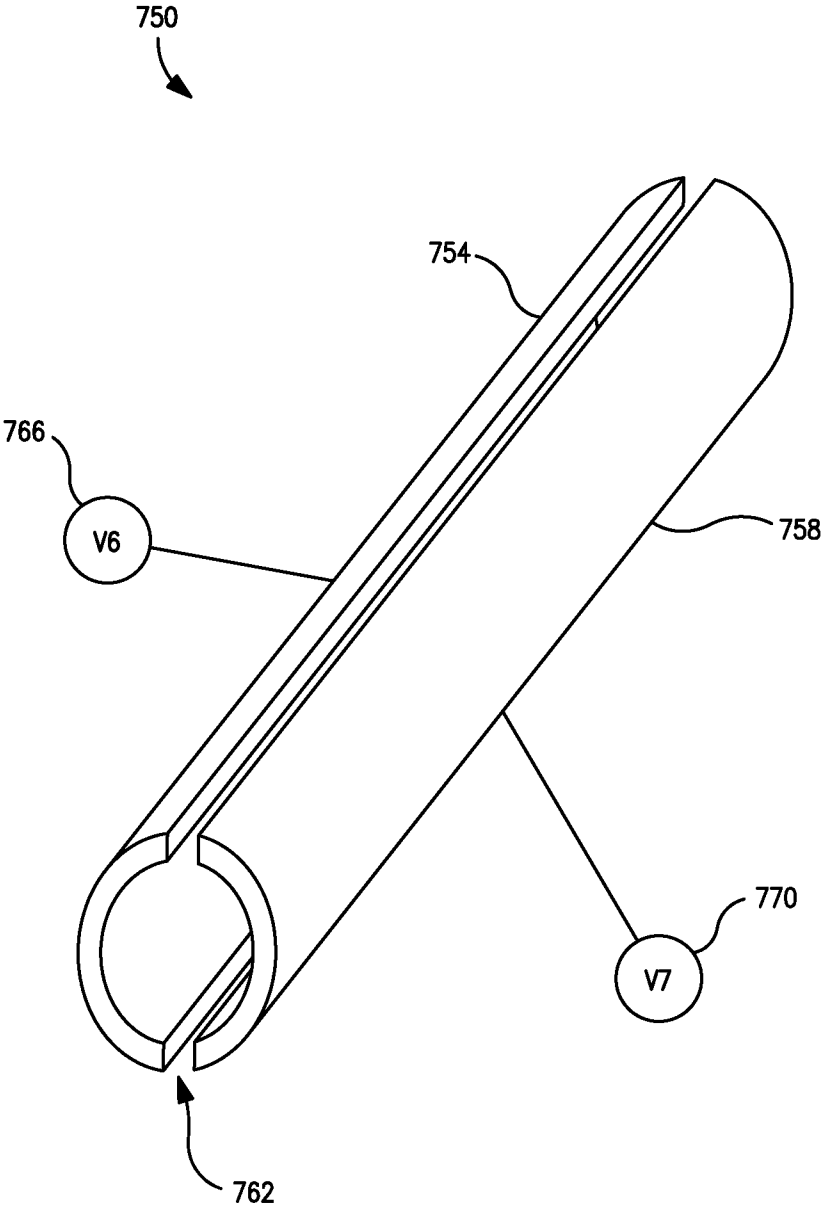
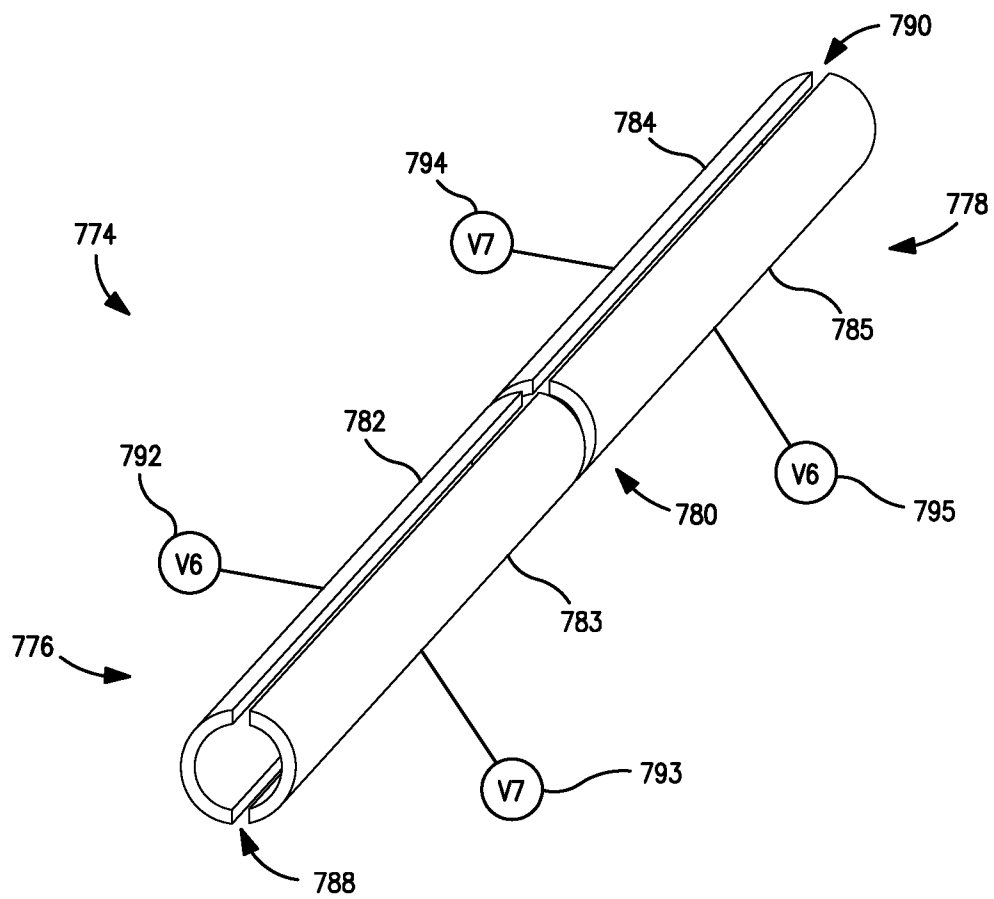


FIG. 7A

9/11

**FIG. 7B**

10/11

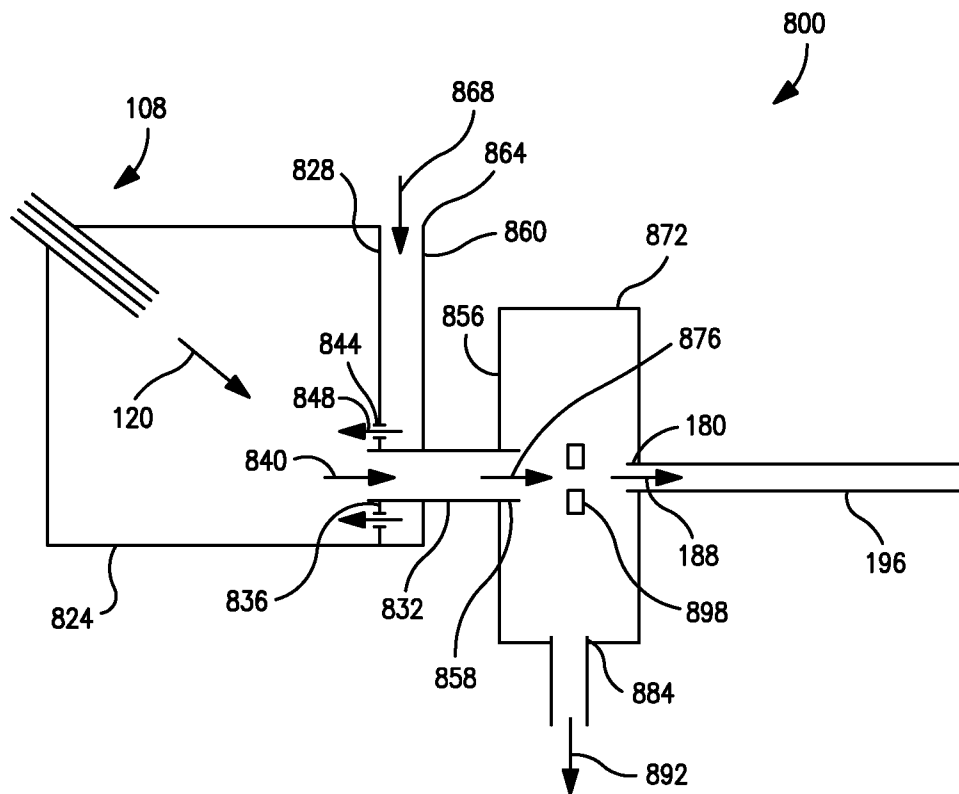


FIG. 8

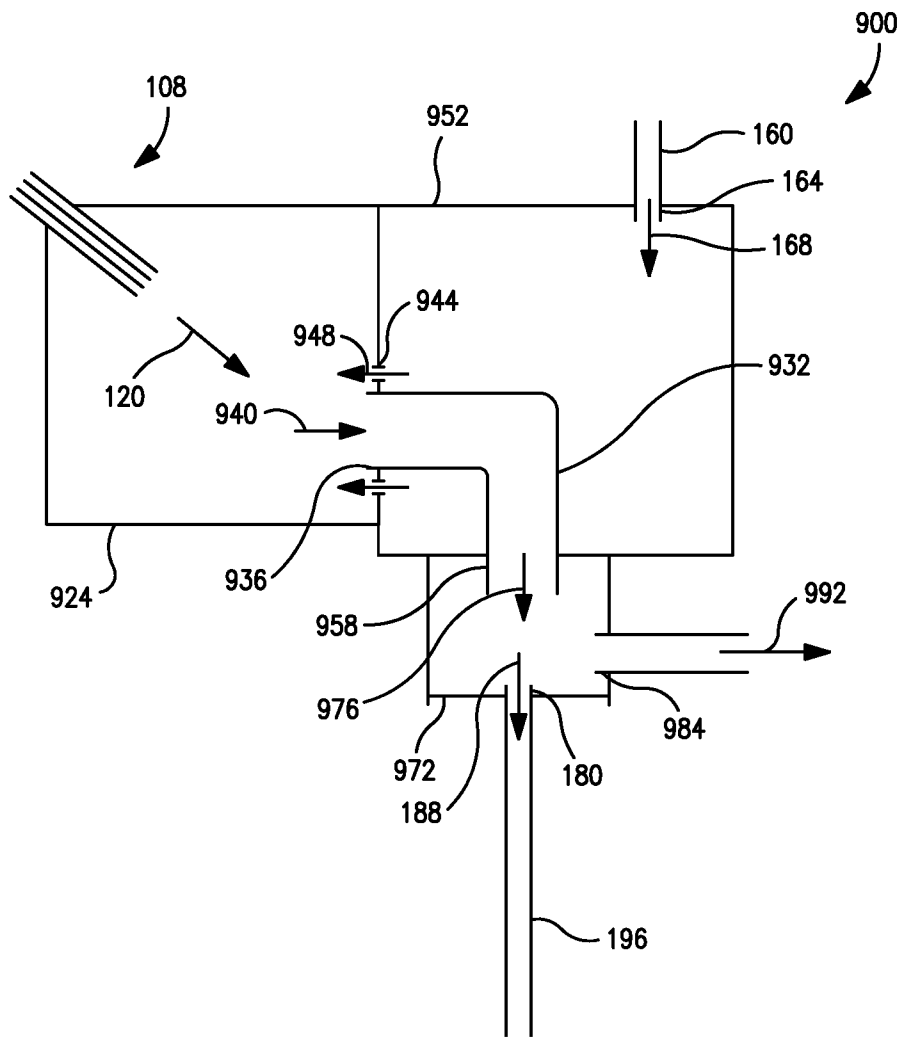


FIG. 9

A. CLASSIFICATION OF SUBJECT MATTER***H01J 49/04(2006.01)i, B01D 59/44(2006.01)i***

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC8: H01J, G01N, B01J

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean Utility models and applications for Utility models since 1975

Japanese Utility models and applications for Utility models since 1975

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKIPASS(KIPO internal) "Keywords: ionization apparatus, interface chamber, conduit, drying gas, pressure, inlet, outlet, ion extraction chamber, mass spectrometer"

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 6429426 B1 (HANS-RUDIGER DORING) 06 August 2002 see abstract, claims 1-43, col. 2 line 46 - col. 10 line 67, figures 1-3.	1-15
A	WO 00-62054 A2 (THE REGENTS OF THE UNI. OF CALIFORNIA) 19 October 2000 see abstract, claims 1-20, page 2 line 15 - page 12 line 26, figures 1-2.	1-15
A	US 6426226 B1 (SELIM MEHMET SENKAN) 30 JULY 2002 see abstract, claims 1-18, col. 5 line 65 - col. 28 line 17, figures 29-32.	1-15



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

16 DECEMBER 2008 (16.12.2008)

Date of mailing of the international search report

16 DECEMBER 2008 (16.12.2008)

Name and mailing address of the ISA/KR

Korean Intellectual Property Office
Government Complex-Daejeon, 139 Seonsa-ro, Seo-
gu, Daejeon 302-701, Republic of Korea

Facsimile No. 82-42-472-7140

Authorized officer

KIM, Sung Hoon

Telephone No. 82-42-481-8505



INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2008/072754

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US6429426 B1	06.08.2002	AT334387 T	15.08.2006
		CA2313729 A1	17.01.2001
		DE19933650 C1	08.03.2001
		DE50013217 D1	07.09.2006
		EP1070960 A2	24.01.2001
		JP2001068053 A	16.03.2001
		KR20010015374 A	26.02.2001
WO 00-62054 A2	19.10.2000	AU 2000-42291 A1	14.11.2000
		AU 4229100 A	14.11.2000
		CN 1242265 C	15.02.2006
		CN 1367874 A	04.09.2002
		JP 2003-527563 T	16.09.2003
		KR 10-2001-0108487 A	07.12.2001
		KR 10-2007-0009743 A	18.01.2007
US 6426226 B1	30.07.2002	AU 1064200 A	05.06.2000
		AU 1998-94494 B2	03.05.1999
		AU 2000-10642 A1	05.06.2000
		BR 9915268 A	07.08.2001
		CA 2306256 A1	22.04.1999
		CA 2347697 A1	25.05.2000
		CN 1333871 A	30.01.2002
		EP 1019713 A1	19.07.2000
		EP 1129348 A1	05.09.2001
		ID 24631 A	27.07.2000
		ID 29172 A	09.08.2001
		JP 2002-530647 T	17.09.2002
		KR 10-2001-0031021 A	16.04.2001
		KR 10-2001-0092734 A	26.10.2001
		PA 01004785 A	06.05.2002
		NZ 503731 A	25.05.2001
		NZ 511228 A	31.01.2003
		PL 339834 A1	02.01.2001
		PL 348157 A1	06.05.2002
		US 6426226 B1	30.07.2002
		WO 00-29844 A1	25.05.2000
		WO 99-19724 A1	22.04.1999