



(51) International Patent Classification:
G01K 15/00 (2006.01)

(21) International Application Number:
PCT/EP2019/054725

(22) International Filing Date:
26 February 2019 (26.02.2019)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
18163982.4 26 March 2018 (26.03.2018) EP

(71) Applicant: AMS INTERNATIONAL AG [CH/CH]; Rietstrasse 4, 8640 Rapperswil (CH).

(72) Inventors: SUY, Hilco; Koolwitjelaan 18, 5691 RN Son en Breugel (NL). DE JONG, Frans; c/o ams International AG, Rietstrasse 4, 8640 Rapperswil (CH). SAKIC, Agata; Ekkerstraat 14, 5616 SP Eindhoven (NL). NE-


NADOVIC, Nebojsa; De Gamert 2207, 6605 WE Wijchen (NL). CALAERTS, Geert; c/o ams International AG, Rietstrasse 4, 8640 Rapperswil (CH). TEN CATE, Hans; c/o ams International AG, 8640 Rapperswil (CH). DE KOK, Renie; c/o ams International AG, 8640 Rapperswil (CH). VALTER, Andreis; c/o ams International AG, 8640 Rapperswil (CH).

(74) Agent: EPPING HERMANN FISCHER PATENTANWALTSGESELLSCHAFT MBH; Schloßschmidstr. 5, 80639 München (DE).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,

(54) Title: ARRANGEMENT AND METHOD FOR CALIBRATING TEMPERATURE SENSORS

FIG. 1

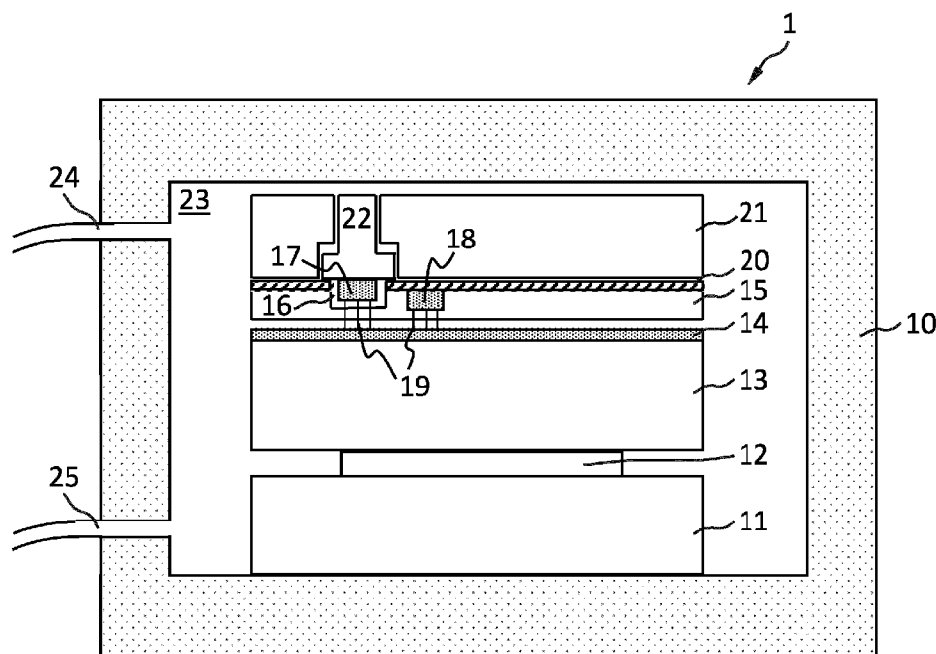

(57) Abstract: A calibration arrangement (1) has a sealable and thermally - isolated chamber (10) comprising a socket mount (15) having a number of reference samples (18) in thermal contact with the socket mount (15) and a number of sample sockets (16) for devices-under test, DUTs (17), with each sample socket (16) being arranged in proximity to and associated to at least one of the reference samples (18). The arrangement (1) further comprises a thermal chuck (13) and a circuit board (14), which is configured to provide electrical connection to the reference samples (18) in the socket mount (15) and DUTs (17) in the sample sockets (16). The thermal chuck (13) is configured to thermalize the socket mount (15) and the circuit board (14) to a temperature set point.



SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

Description

ARRANGEMENT AND METHOD FOR CALIBRATING TEMPERATURE SENSORS

- 5 The present disclosure relates to an arrangement and a method for calibrating sensors.

High-accuracy temperature sensors are utilized in a large variety of applications in which it is required to monitor
10 the temperature with high accuracy. For example, reliable body temperature measurements require an accuracy of less than 100 mK. To provide temperature sensors with this high level of accuracy, a reliable way of calibrating newly fabricated temperature sensors is required. The calibration
15 process of high accuracy temperature sensors typically involves several hours of stabilization in a highly-controlled temperature-stable environment.

It is an object of the invention to provide an improved
20 concept for calibrating temperature sensors.

This object is achieved with the subject-matter of the independent claims. Embodiments and developments of the improved concept are defined in the dependent claims.
25

The improved concept is based on the idea of a calibration arrangement featuring fast thermalization of devices-under-test, DUTs, while avoiding temperature gradients to achieve a more accurate calibration. To this end, the improved concept
30 is realized by a calibration arrangement that is characterized by having a sufficiently small distance between the DUTs, for example CMOS temperature sensors, that are to be calibrated and reference samples used for the calibration

process. With such an arrangement the calibration process of temperature sensors can be performed with high accuracy within short time periods, for example within several seconds, and with high parallelism, i.e. simultaneous
5 calibration of a large number of sensors, for example several hundreds of sensors at once.

In particular, the improved concept proposes a calibration arrangement comprising a sealable and thermally isolated
10 chamber, in which a socket mount, a circuit board and a thermal chuck are arranged.

The socket mount comprises a number of temperature reference samples, which are in thermal contact with the socket mount.
15 The socket mount further comprises a number of sample sockets for DUTs, wherein each sample socket is arranged in proximity to and associated to at least one of the reference samples. In such an arrangement each of the DUTs can be calibrated by means of N reference samples, with N being an integer number
20 leading to a ratio 1:N between the number of DUTs and the number of reference samples. Typically, N is between one and four.

The circuit board is configured to provide electrical
25 connection to the DUTs in the sample sockets and the reference samples in the socket mount. For example, the electrical connection is configured to provide a connection of the DUTs and the reference samples to a power supply and/or a readout circuit. The thermal chuck is arranged in
30 thermal contact with the socket mount and the circuit board, and is configured to thermalize the socket mount and the circuit board to a temperature set point.

The improved concept further comprises a method for calibrating temperature sensors in such a calibration arrangement.

- 5 In various embodiments of the calibration arrangement according to the improved concept, the socket mount comprises additional sample sockets for DUTs, wherein each of the additional sample sockets is arranged in proximity to and associated to the at least one of the reference samples.

10

Analogous to having multiple reference samples for each of the DUTs, conversely a number M of DUTs, with M being an integer number, may be calibrated by means of a single reference sample. In this case, the sample arrangement is

- 15 described by a ratio M:1 between the number of DUTs and the number of reference samples. Likewise, M is typically between one and four.

In some embodiments, the arrangement of multiple DUTs per reference sample is combined with the converse case, leading to a ratio of M:N. For example, an arrangement of 2:2 can be chosen, in which two DUTs can each be calibrated by means of two reference samples.

- 20 In various embodiments of the calibration arrangement according to the improved concept, each of the sample sockets is arranged at a distance of less than 10 mm, in particular less than 5 mm, from the associated at least one of the reference samples.

30

Moreover, in preferred embodiments each of the sample sockets is arranged at the same distance from the associated at least one of the reference samples.

The proximity between the DUTs placed in the sample sockets and the reference samples ensures a short thermal path between them and hence allows for a reliable and accurate calibration of DUTs. The underlying principle for this is that, due to the proximity, each of the DUTs thermalizes to the same temperature as the at least one associated reference sample. Such a configuration therefore also compensates calibration errors due to possible temperature gradients across the calibration arrangement and offsets compared to the set point of the thermal chuck.

Having the same distance between each of the reference samples and each of the associated sample sockets further guarantees a consistent calibration of all DUTs placed in the sample sockets in terms of accuracy.

In some embodiments the reference samples are of the same type as the DUTs to be placed into the sample sockets.

The advantage of such embodiments is that the DUTs and the reference samples show the same behavior, for example by means of thermalization behavior. In this way, the accuracy of the calibration process can be further enhanced. Moreover, in this case reference samples can easily be swapped with DUTs that are pre-calibrated in a lab setting against a very accurate and NIST-traceable reference.

In a preferred embodiment the socket mount is made from a material with high thermal conductivity. Suitable materials include metals, such as, for instance, stainless steel or aluminum.

Especially for industrial production it is desirable to perform the calibration of temperature sensors not only with high parallelism but also within short time periods. To this end, a socket mount with high thermal conductivity

5 substantially reduces the thermalization time of both DUTs placed in the sample sockets and the reference samples in the arrangement. In particular, the thermalization time can be reduced to a timescale of a few seconds, after which meaningful results of the calibration process can be
10 obtained.

In some embodiments the calibration arrangement comprises a gas surrounding the socket mount. The calibration arrangement is further configured to thermalize the gas to the
15 temperature set point in these embodiments. The arrangement may further be configured to operate at the given set point of the gas by means of pressure and/or relative humidity.

Operating the calibration arrangement with a gas surrounding
20 DUTs placed in the sample sockets allows for the temperature calibration according to the designed purpose of the sensors regarding, for example, type of the gas, pressure and/or relative humidity.

25 Beyond that, in many cases DUTs feature more than one sensor per unit. Besides a temperature sensor, a DUT may for example comprise a gas sensor, relative humidity sensor and/or a pressure sensor. In such an embodiment the calibration of the DUTs by means of temperature can be extended by a calibration
30 of gas sensing, relative humidity measurements and/or pressure measurements without the need for modifying the arrangement or disturbing its temperature equilibrium. In addition, accurate calibration of the DUTs by means of gas,

relative humidity and/or pressure relies on the knowledge of the precise temperature, which can be obtained with the DUTs according to this embodiment.

5 In preferred embodiments the calibration arrangement further comprises an evaluation circuit, which is configured to generate, based on a temperature-dependent quantity, respective sets of measurement signals for each of the DUTs placed in the associated sample sockets. Each set of
10 measurement signals hereby comprises a test measurement signal from a distinct one of the DUTs, and a reference measurement signal from the associated at least one of the reference samples.

15 The acquisition of measurement sets allows for the calibration of the DUTs by means of the associated reference samples via comparison of the test measurement signal and the reference measurement signals of the respective set of measurement signals.

20 In some embodiments the evaluation circuit is further configured to generate a calibration signal for each set of measurement signals. The calibration signal is hereby based on the result of the comparison between the test measurement
25 signal and the reference measurement signals of the respective set of measurement signals.

Under the assumption that each of the DUTs in the sample sockets is thermalized to the same temperature as the
30 associated at least one of the reference samples, the result of the comparison of the test measurement signal and the reference measurement signals can be used by means of the evaluation circuit to calibrate the respective DUT. The use

of multiple reference samples for the calibration of each DUT can hereby further enhance the accuracy of the calibration process. On the other hand, having multiple DUTs associated to each reference samples allows for a larger number of DUTs
5 that can be simultaneously calibrated in the arrangement.

In a preferred embodiment the evaluation circuit is configured to generate the sets of measurement signals within a timeframe of less than 10 seconds.

10

Besides a fast thermalization of DUTs placed in the sample sockets, it is further desirable to likewise perform the actual calibration process in short timeframes, in particular within timeframes of less than 10 seconds.

15

In some embodiments the calibration arrangement further comprises an apparatus configured to exert a force on the DUTs in the sample sockets. The force vector hereby points in the direction of the sample sockets.

20

The apparatus in such an embodiment acts as a push mechanism forcing the DUTs into the sample sockets. This both enhances the thermal contact between the DUTs and the sample mount as well as ensures a sufficient electrical contact between
25 contacts of the DUTs and contacts on the circuit board.

The aforementioned object is further solved by a method of calibrating temperature sensors in a calibration arrangement, for example according to one of the embodiments described
30 above.

The method comprises arranging a number of devices under test, DUTs, in a sealable and thermally isolated chamber of

the calibration arrangement such that each of the DUTs is in proximity to, associated to and in thermal contact with at least one of a number of reference samples. The method further comprises controlling the calibration arrangement to
5 thermalize the DUTs and the reference samples to a temperature set point, and generating, based on a temperature-dependent quantity, sets of measurement signals for each of the DUTs. Each set of measurement signals comprises a test measurement signal from a distinct one of
10 the DUTs and a reference measurement signal from each of the associated at least one of the reference samples.

In some embodiments the method further comprises the generation of a calibration signal for each pair of
15 measurement signals based on a result of a comparison of the test measurement signal and the reference measurement signals of the respective set of measurement signals.

In some embodiments of the method each set of measurement
20 signals is generated simultaneously or within a given timeframe.

Further embodiments of the method become apparent to the skilled reader from the embodiments of the calibration
25 arrangement described above.

The following description of figures of example embodiments may further illustrate and explain aspects of the improved concept. Elements and parts of the arrangement with the same
30 structure and the same effect, respectively, appear with equivalent reference symbols. In so far as elements and parts of the arrangement correspond to one another in terms of

their function in different figures, the description thereof is not repeated for each of the following figures.

Figure 1 shows an exemplary embodiment of a calibration
5 arrangement according to the improved concept;

Figure 2 shows a further exemplary embodiment of a
calibration arrangement according to the improved
concept;

10 Figure 3 shows an exemplary embodiment of a sample mount
according to the improved concept;

Figure 4 shows a cross-section of the exemplary embodiment
15 shown in figure 3;

Figure 5 shows a second exemplary embodiment of a sample
mount according to the improved concept;

20 Figure 6 shows a third exemplary embodiment of a sample
mount according to the improved concept;

Figure 7 shows a fourth exemplary embodiment of a sample
mount according to the improved concept; and

25 Figure 8 shows an exemplary result of a temperature sensor
calibration according to the improved concept,
validated in a lab setup against an independent
NIST-traceable reference probe.

30 Figure 1 shows the cross-section of an exemplary embodiment
of a calibration arrangement 1 comprising a sealable and
thermally isolated chamber 10. Components inside the chamber

10 are arranged in a stacked manner. In this example, the stack comprises from bottom to top: a thermal mass 11, a Peltier element 12, a thermal chuck 13 and circuit board 14. In other examples the stack might comprise additional
5 components. The sample mount 15 with the sample sockets 16 is arranged above the circuit board 14. Also shown is a device-under-test, DUT, 17 placed inside the sample socket 16 as well as a reference sample 18. The reference samples are for example of the same type as the DUTs 17 and are calibrated
10 with NIST-traceability. In this embodiment the reference samples are fixated and covered by a cover plate 20. A pushdown mechanism 22 provides thermal contact for the DUTs 17 as well as electrical contact between pogo pins 19 of the DUTs 17 and the circuit board 14. Additionally, a pushdown
15 housing 21 thermally couples the pushdown mechanism 22 to the cover plate 20 and the sample mount 15. In this example, the chamber 10 further comprises a gas 23 surrounding the stack of components, in particular the DUTs 17 and reference samples 18. The gas is introduced for example by means of a
20 temperature controlled gas inlet 24. The chamber further comprises a gas outlet 25.

The components of the arrangement 1, in particular the sample mount 15, the circuit board 14 and the surrounding gas 23,
25 are thermalized to a temperature set point. The thermalization can for example be achieved by means of temperature control of heated walls of the chamber 10, the Peltier element 12 and a temperature controlled gas inlet 24. To ensure thermalization to the same temperature, the
30 aforementioned components may be thermalized by a single temperature control. For example, the walls of the chamber 10 and the temperature controlled gas inlet 24 may be

temperature controlled by means of a coolant liquid supplying both components.

For a reliable calibration process a large degree of

5 temperature stability of the sample sockets 16 and the reference samples 18 is required. This is achieved by means of the thermal chuck 13, which is in thermal contact with the socket mount 15 and the circuit board 14. The thermal chuck is preferably made of a material with high thermal
10 conductivity, for example a metal such as stainless steel or aluminum, and provides a large thermal mass in comparison to the DUTs 17. Due to the high thermal conductivity, DUTs 17 that are placed into the sample sockets 16 and pushed down by means of the pushdown mechanism 22 quickly thermalize to the
15 temperature set point of the arrangement 1, for example within seconds. Due to their close proximity of a few millimeters causing a short thermal path and small thermal resistance, it is guaranteed that each of the DUTs 17 thermalizes to the same temperature as the associated
20 reference sample 18. This condition holds true also in case of a temperature gradient across the individual components of the arrangement 1, which can for example be caused by a long thermal path and high thermal resistance between the sample sockets 16 and the Peltier element 12.

25

After the DUTs 17 and the reference samples 18 are thermalized, the actual calibration process can be performed. For example, an evaluation circuit which is electrically connected to the circuit board 14 generates, based on a
30 temperature-dependent quantity, respective sets of measurement signals for each of the DUTs 17. In particular, each set of measurement signals comprises a test measurement signal from a distinct one of the DUTs 17 and a reference

measurement signal from the associated at least one of the reference samples 18.

The evaluation circuit may comprise a memory, containing for example a look-up table for converting the test measurement signal and the reference measurement signals of each measurement set into units of temperature.

The evaluation circuit may further generate a calibration signal for each set of measurement signals, wherein each calibration signal corresponds to a result of a comparison of the test measurement signal and the reference measurement signals of the respective set of measurement signals. Each calibration signal can hence be used for calibrating the corresponding DUT 17 for accurate absolute temperature measurements. The achievable accuracies are below 100 mK, in particular below 50 mK at the temperature set point, and within 200 mK in a temperature range of ± 50 K around the temperature set point.

In particular, the evaluation circuit is configured to generate each set of measurement signals simultaneously or within a given timeframe, for example within seconds. Preferably, also the calibration signals are generated within short time periods, i.e. within seconds.

In some applications, the DUTs 17 contain additional sensors in addition to a temperature sensor. Hence, a calibration of the additional sensors of the DUTs 17 in the calibration arrangement 1 may be desired without the need for modifying the arrangement or disturbing its temperature equilibrium.

Therefore, the arrangement 1 may be further configured to calibrate the additional sensors of the DUTs 17 by means of gas, relative humidity and/or pressure analogous to the temperature calibration. To this end, the temperature
5 controlled gas inlet 24 is further configured to provide an active gas flow for introducing a specific gas 23 into the chamber and stabilize the gas 23 by means of relative humidity and/or pressure.

10 Figure 2 shows an exemplary embodiment of the arrangement 1 featuring the pairwise arrangement of the DUTs 17 and the reference samples 18 on the sample mounts 15. In particular, the chamber 10 may comprise more than one sample mount 15. In such an embodiment, the arrangement 1 may host a large number
15 of DUTs 17, and a likewise large number reference samples 18, at the same time. For example the number of DUTs 17 that can be placed in the chamber may be in the order of 100.

Figure 3 shows a schematic top view of an exemplary sample
20 mount 15. The sample mount 15 in this example features a 1:1 arrangement of each of a number of reference samples 18 and a sample socket 16 in its proximity, in which a DUT 17 can be placed. The distance between each of the reference samples 18 and the associated sample socket 16 is the same across the
25 entire sample mount 15. For example, this distance is less than 10 mm, in particular less than 5 mm. Assuming that the sample mount 15 is made from a material with high thermal conductivity, this setup allows for the fast thermalization of each reference sample 18 and a DUT 17 to the same
30 temperature.

Figure 4 shows a cross section of the exemplary sample mount 15 shown in figure 3. In this cross-section, the cover plate

20 becomes apparent, covering the reference samples 18. This cover plate 20 has the effect of protecting the reference samples 18 and ensuring that the latter remain thermalized to the temperature set point while the chamber is exposed to the environment, for example during insertion of new DUTs 17 into the sample sockets 16.

Figure 5 shows a schematic top view of a further exemplary sample mount 15. In this case the ratio between reference samples 18 and sample mounts 16 is 1:2, leading to a situation in which two DUTs 17 placed into the respective sample sockets 16 can be calibrated by means of one single reference sample 18.

Other sample arrangements not shown may feature more than two sample sockets being associated to a reference sample, described by a ratio of 1:N. Typically, ratios of up to 1:4 are realized.

In further sample arrangements not shown more than one reference sample 18 may be associated to each of the DUTs 17 in the sample sockets 16, leading to a ratio of M:1, whereas typical ratios are as large as 4:1.

Figure 6 shows a schematic top view of a further exemplary sample mount 15. In this sample arrangement, the ratio between reference samples 18 and DUTs 17 in the respective sample sockets 16 is 2:2. This leads to the fact that each of the DUTs 17 is arranged at an equal distance from the associated two reference samples 18. In such an arrangement, each of the DUTs 17 can be calibrated by means of two reference samples 18, leading to a more accurate calibration while maintaining a small footprint of each group of two DUTs 17 and two reference samples 18.

Figure 7 shows a further exemplary sample mount 15. This linear sample arrangement likewise allows for calibrating each of the DUTs 17 by means of multiple reference samples 18. Due to the constant distance between each of the sample sockets 16 and their adjacent reference samples 18, DUT 17a for example is associated to reference samples 18a and 18b, while DUT 17b is associated to reference samples 18b and 18c. This pattern continues accordingly across the entire sample mount 15.

Figure 8 shows the result of an exemplary calibration of 252 DUTs 17 calibrated at a temperature set point of 25°C of the calibration arrangement 1. The graph shows the accuracy of the newly calibrated devices versus the temperature in a verification chamber. The temperature inside the chamber is determined via an independent NIST-traceable reference probe. For this, the deviation between the DUTs 17 and the temperature reference is evaluated for a temperature range between -40°C and 100°C. The lowest standard deviation is expectedly observed at the calibration set point of 25°C, resulting in an accuracy of the calibrated temperature sensors of less than 100 mK.

Reference numerals

	1	sensor arrangement
	10	sealable and thermally isolated chamber
5	11	thermal mass
	12	Peltier element
	13	thermal chuck
	14	circuit board
	15	socket mount
10	16	sample socket
	17	device-under-test
	18	reference sample
	19	pogo pins
	20	cover plate
	21	push-down housing
	22	push-down mechanism
15	23	gas
	24	gas inlet
	25	gas outlet

Claims

1. A calibration arrangement (1) for temperature sensors comprising

- 5 - a sealable and thermally isolated chamber (10);
- a socket mount (15) comprising
- a number of reference samples (18) with each of the reference samples (18) being in thermal contact with the socket mount (15); and
- 10 - a number of sample sockets (16) for devices-under test, DUTs (17), with each sample socket (16) being arranged in proximity to and associated to at least one of the reference samples (18);
- a circuit board (14) configured to provide electrical
- 15 connection to the sample sockets (16) and the reference samples (18) in the socket mount (15); and
- a thermal chuck (13) in thermal contact with the socket mount (15) and the circuit board (14), the thermal chuck (13) being configured to thermalize the socket mount (15)
- 20 and the circuit board (14) to a temperature set point.

2. The calibration arrangement (1) according to claim 1, wherein the socket mount (15) comprises additional sample sockets (16) for DUTs (17), wherein each of the additional

25 sample sockets (16) is arranged in proximity to and associated to the at least one of the reference samples (18).

3. The calibration arrangement (1) according to claim 1 or 2, wherein each of the sample sockets (16) is arranged at a

30 distance of less than 10 mm, in particular less than 5 mm, from the associated at least one of the reference samples (18).

4. The calibration arrangement (1) according to one of claims 1 to 3, wherein each of the sample sockets (16) is arranged at the same distance from the associated at least one of the reference samples (18).

5

5. The calibration arrangement (1) according to one of claims 1 to 4, wherein the socket mount (15) is made from a material with high thermal conductivity.

10 6. The calibration arrangement (1) according to one of claims 1 to 5, wherein the arrangement (1) comprises a gas (20) surrounding the socket mount (15) and is configured to thermalize the gas (20) to the temperature set point.

15 7. The calibration arrangement (1) according to claim 6, wherein the arrangement (1) is configured to operate at a given set point of the gas (20) by means of pressure and/or relative humidity.

20 8. The calibration arrangement (1) according to one of claims 1 to 7, wherein the arrangement (1) comprises an evaluation circuit configured to generate, based on a temperature-dependent quantity, a respective set of measurement signals for each of the DUTs (17) placed in the sample sockets (16),
25 with each set of measurement signals comprising

- a test measurement signal from a distinct one of the DUTs (17); and
- a reference measurement signal from each of the associated at least one of the reference samples (18).

30

9. The calibration arrangement (1) according to claim 8, wherein the evaluation circuit is configured to generate a calibration signal for each set of measurement signals based

on a result of a comparison of the test measurement signal and the reference measurement signals of the respective set of measurement signals.

5 10. The calibration arrangement (1) according to claim 8 or 9, wherein the evaluation circuit (1) is configured to generate the sets of measurement signals within a timeframe of less than 10 seconds.

10 11. The calibration arrangement (1) according to one of claims 1 to 10, wherein the arrangement (1) is further configured to calibrate the DUTs (17) in terms of a gas-dependent parameter, in particular in terms of pressure and/or relative humidity.

15

12. The calibration arrangement (1) according to one of claims 1 to 11, further comprising an apparatus (19) configured to exert a force on the DUTs (17) in the sample sockets (16) in the direction of the sample sockets (16), in particular for creating thermal contact between the DUTs (17) and the socket mount (15) and electrical contact between contacts of the DUTs (17) and contacts on the circuit board (14).

25 13. A method for calibrating temperature sensors, the method comprising

- arranging devices-under-test, DUTs (17), in a sealable and thermally isolated chamber (10) of a calibration arrangement (1) such that each of the DUTs is in proximity to, associated to and in thermal contact with at least one of a number of reference samples (18);

30

- controlling the calibration arrangement (1) to thermalize the DUTs (17) and the reference samples (18) to a temperature set point; and
- generating, based on a temperature-dependent quantity, a set of measurement signals for each of the DUTs (17), with each set of measurement signals comprising
 - a test measurement signal from a distinct one of the DUTs (17); and
 - a reference measurement signal from each of the associated at least one of the reference samples (18).

14. The method according to claim 13, further comprising the generation of a calibration signal for each set of measurement signals based on a result of a comparison of the test measurement signal and the reference measurement signals of the respective set of measurement signals.

15. The method according to claim 13 or 14, wherein each set of measurement signals is generated simultaneously or within a given timeframe.

FIG. 1

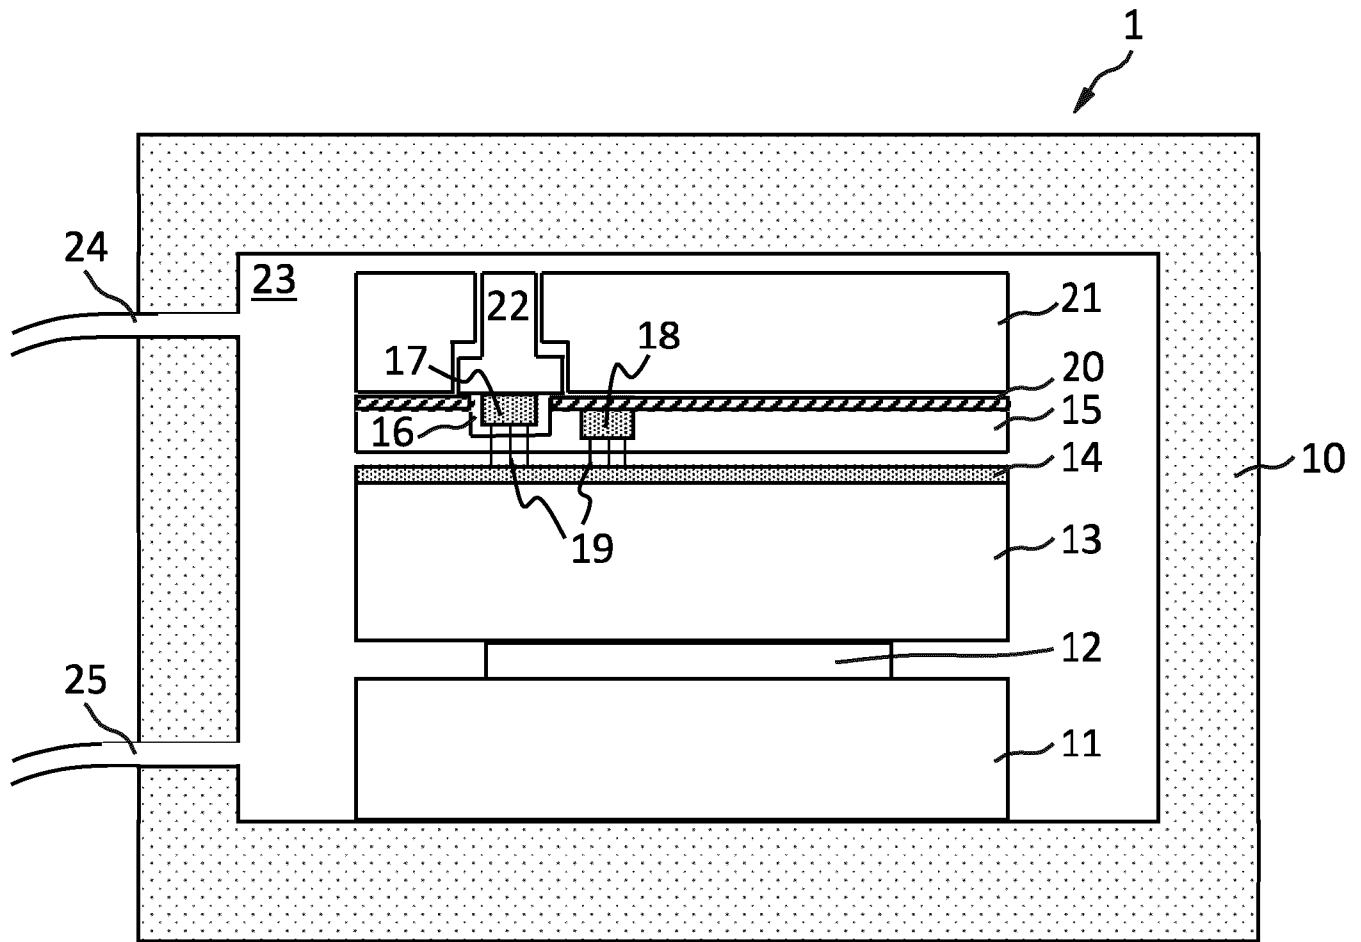


FIG. 2

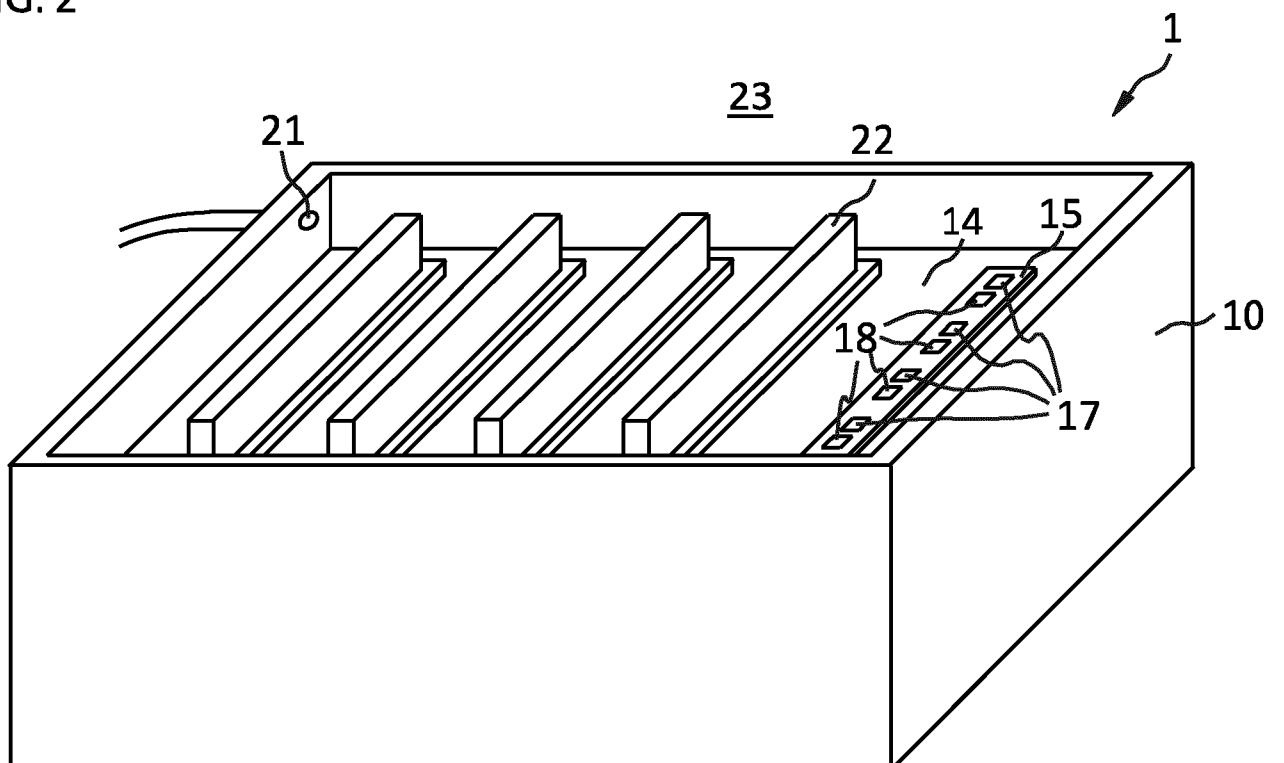


FIG. 3

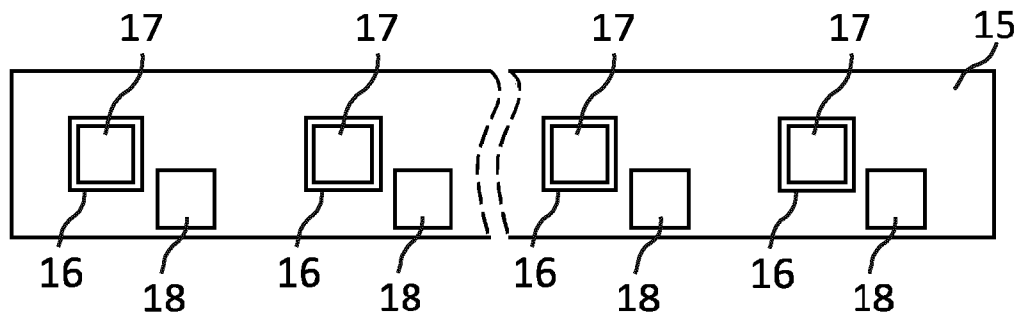


FIG. 4

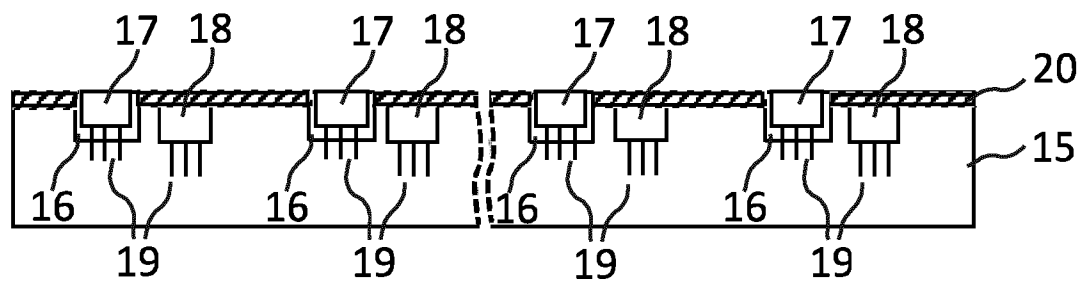


FIG. 5

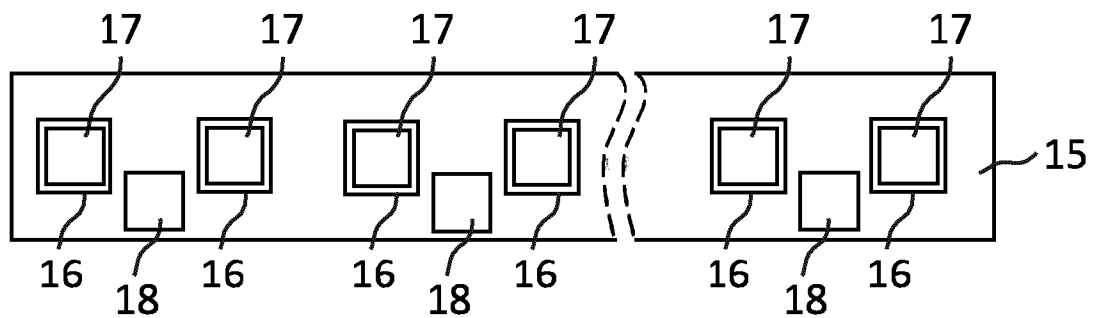


FIG. 6

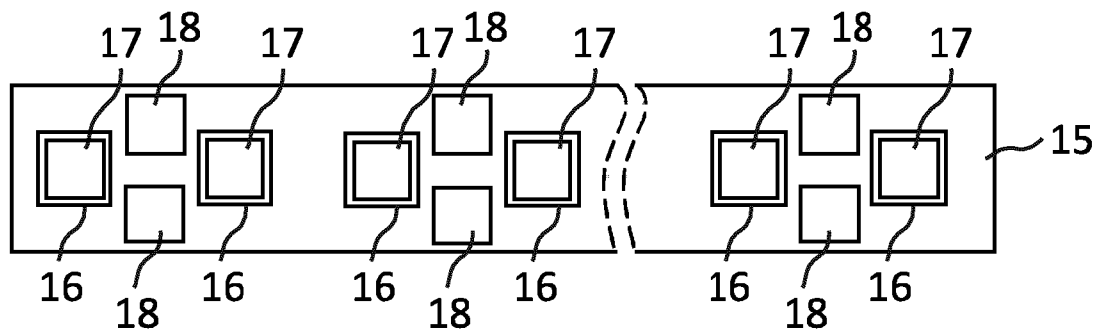


FIG. 7


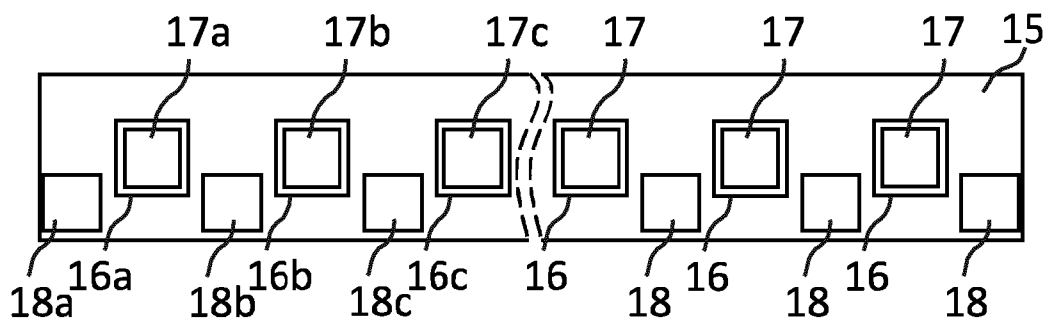


FIG. 8

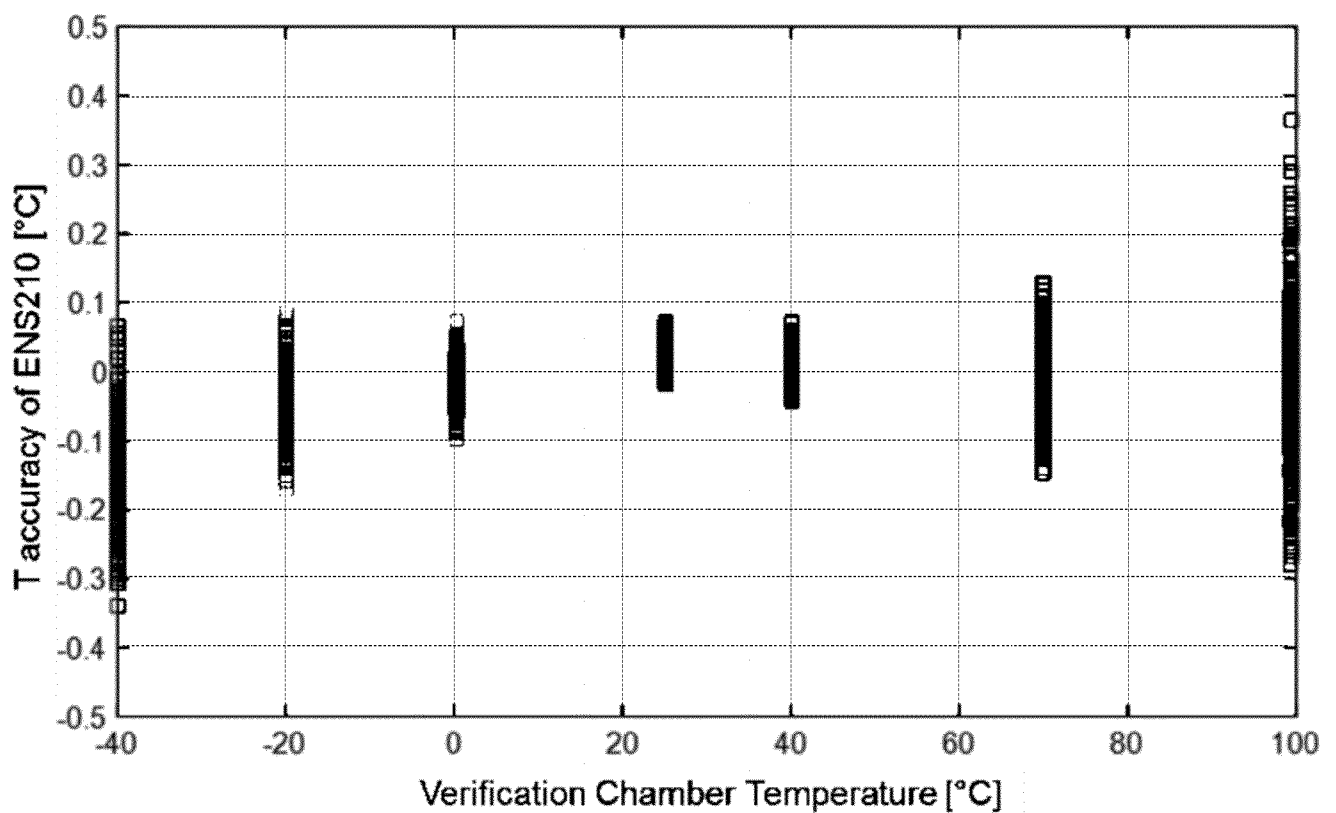

INTERNATIONAL SEARCH REPORT

International application No

PCT/EP2019/054725

A. CLASSIFICATION OF SUBJECT MATTER

INV. G01K15/00

ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

G01K

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	CN 102 539 018 B (SHANGHAI MICROELECTRONICS EQUI) 18 December 2013 (2013-12-18) paragraphs [0001], [0007] - [0015], [0020], [0050], [0052], [0060], [0062]; figures 1,2 -----	1-15
A	CN 102 435 351 B (WUHAN HITRUSTY ELECTRONICS CO LTD) 20 November 2013 (2013-11-20) paragraphs [0001], [0005], [0013], [0022] -----	1-15
A	US 2015/338289 A1 (FRIEDRICHS RENÉ [DE]) 26 November 2015 (2015-11-26) paragraphs [0001], [0004], [0007], [0020] -----	1-15



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

10 May 2019

Date of mailing of the international search report

20/05/2019

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Phleps, Stefanie

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/EP2019/054725

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
CN 102539018	B	18-12-2013	NONE

CN 102435351	B	20-11-2013	NONE

US 2015338289	A1	26-11-2015	CN 105094168 A 25-11-2015
			DE 102014007786 A1 26-11-2015
			DK 2947439 T3 09-10-2017
			EP 2947439 A1 25-11-2015
			ES 2642120 T3 15-11-2017
			US 2015338289 A1 26-11-2015
