

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
26 August 2010 (26.08.2010)

PCT

(10) International Publication Number
WO 2010/096824 A1

(51) International Patent Classification:
A61F 2/28 (2006.01)

(21) International Application Number:
PCT/US20 10/025093

(22) International Filing Date:
23 February 2010 (23.02.2010)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
61/154,734 23 February 2009 (23.02.2009) US

(72) Inventors; and

(71) Applicants : **BARTEE, Barry, K.** [US/US]; 4620 71st Street, Lubbock, TX 79424 (US). **BARTEE, Chaddick, M.** [US/US]; 4620 71st Street, Lubbock, TX 79424 (US).

(74) Agents: **SMYTH, Anthony, G.** et al; Pillsbury Winthrop Shaw Pittman LLP, P.o. Box 10500, Mclean, VA 22102 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).


Published:

— with international search report (Art. 21(3))



WO 2010/096824 A1

(54) Title: REINFORCED PTFE MEDICAL BARRIER

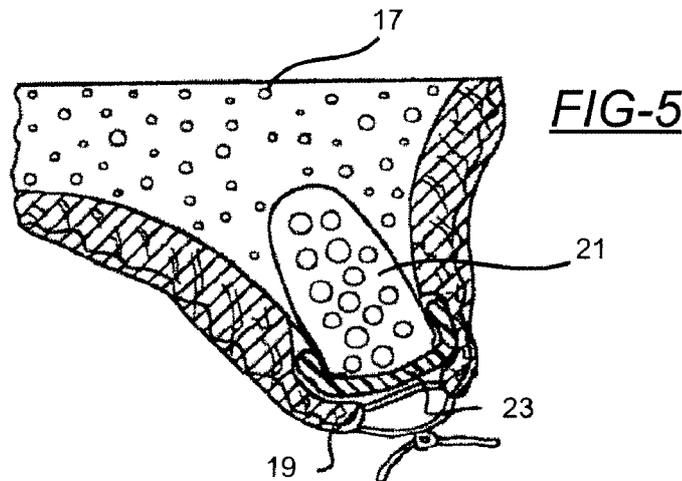

(57) Abstract: Systems, methods and devices usable in the repair of a bone defect are described. A portion of a bone defect is covered with a multilayered membrane that includes a reinforcing layer. A member of the reinforcing member is fastened to an area of bone and soft tissue is secured about the membrane. The membrane facilitates healing of the defect. One membrane comprises a plurality of layers that includes a binding layer and a PTFE layer which has a textured surface and a substantially smooth surface. The textured surface provides a top surface of the membrane and the substantially smooth surface contacts bone.

REINFORCED PTFE MEDICAL BARRIER

Cross-Reference to Related Applications

[0001] The present Application claims priority from United States Provisional Patent Application No. 61/154,734, filed February 23, 2009, which application is incorporated herein by reference for all purposes.

[0002] The present Application is related to copending United States Patent Application Serial No. 11/941,060 entitled "Hydrophilic High Density PTFE Medical Barrier," filed November 15, 2007 which is a continuation of United States Patent Application No. 10/947,066, filed September 21, 2004, which issued as United States Patent No. 7,296,998 and United States Patent Application Serial No. 08/971,390, filed November 17, 1997 entitled "Textured High Density PTFE Medical Barrier," which issued as United States Patent No. 5,957,690, each related application being expressly incorporated by reference herein.

BACKGROUND OF THE INVENTION

Field of the Invention

[0003] The present invention relates generally to repair of bone defects and more particularly, to systems, apparatus and methods of assisting growth of bone and tissue after trauma and surgery.

Description of Related Art

[0004] Regeneration of bone defects remains a significant clinical problem. For example, in oral reconstructive surgery, bone defects may occur as a result of tooth extraction, cyst formation, surgery, trauma, or destruction by periodontal or peri-implant disease. Some synthetic membrane materials have been used for guided tissue regeneration, including cellulose acetate filter, perforated Teflon®, mantle leaf, expanded polytetrafluoroethylene (PTFE), and resorbable polymers. Naturally derived membranes such as bovine collagen and lyophilized dura mater have also been used.

[0005] Membrane-assisted guided tissue regeneration techniques are based on the hypothesis that during wound healing, cells adjacent to the bone defect migrate to repopulate the defect at various rates. By placing a barrier such as a biocompatible membrane over the defect, the rapidly migrating connective tissue cells will be mechanically prevented from entering the defect. Theoretically, this

allows the slower-migrating mesenchymal cells from the surrounding bone and marrow, having osteogenic potential, to repopulate the defect selectively.

[0006] A common feature of earlier synthetic membrane systems is macroporosity, which was believed to enhance regeneration by improving wound stability through tissue integration and allowing diffusion of extra-cellular nutrients across the membrane. However, in some applications, the use of macroporous biomaterials in the oral cavity can result in early bacterial contamination of the material. Bacterial contamination of macroporous biomaterials can result in antibiotic-resistant infection, which can require early removal of the device.

[0007] Additionally, a common feature of macroporous biomaterials is the ingrowth of surrounding tissues, which was thought to be necessary for stabilization of the implant. In macroporous biomaterials, cells readily incorporate into the material and connective tissue is manufactured. While this incorporation into the material slows the migration of cells, it presents a difficult problem to the patient and the surgeon during the removal process. The incorporated cells and fibrous connective material may make removal of the barrier painful and traumatic to the patient and very time consuming and difficult for the surgeon.

[0008] It has been discovered that the use of a flexible high-density polytetrafluoroethylene (PTFE) sheet material is useful in guided tissue regeneration. High density PTFE is substantially nonporous or microporous so as not to incorporate cells or attach to fibrous adhesions. By presenting a smooth surface to the biological materials, a high density PTFE barrier is easily inserted and removed following extended implantation periods. An example of a high density PTFE barrier material is disclosed in U.S. Pat. No. 5,480,711.

[0009] While high density PTFE medical barriers provide advantages over macroporous barriers, the smooth surface of the high density PTFE barriers sometimes leads to dehiscence of the soft tissue overlying the barrier. The dehiscence problem is caused by the fact that the smooth surface of high density PTFE will not incorporate cells and will not attach to fibrous adhesions. Thus, over the course of healing, the incision will occasionally split open over the high density PTFE barrier.

BRIEF SUMMARY OF THE INVENTION

[0010] Certain embodiments of the invention comprise systems and methods for repairing bone defects that can include covering a portion of a bone defect using a reinforced membrane and securing soft tissue about the membrane, whereby the membrane facilitates healing of the defect. In certain embodiments, the membrane may comprise a plurality of layers, including a binding layer and a polytetrafluoroethylene polymer (PTFE) layer, the PTFE layer having a textured surface and a substantially smooth surface. In certain embodiments, the textured surface provides a top surface of the membrane. In certain embodiments, the substantially smooth surface contacts the bone. In certain embodiments, the textured surface is made of unsintered PTFE. In certain embodiments, the substantially smooth surface is made of expanded PTFE. In certain embodiments, the binding layer is a titanium binder.

[0011] Certain embodiments of the invention provide a medical barrier that includes a reinforced material which is a titanium binder configured to span a bone cavity and adapted for fixation to bone surrounding the bone cavity and a PTFE membrane attached at one or more points to the titanium binder, with the titanium binder having one or more elongate members; wherein the titanium binder can be formed in a desired shape and/or deformed to obtain the desired shape. In certain embodiments, the elongate members have one or more predrilled holes suitable for securing a fastener to an area of bone. In certain embodiments, the fastener is a surgical screw. In certain embodiments, the fastener is a surgical pin. In certain embodiments, at least one of the elongate members is free to move independently of the PTFE membrane. In certain embodiments, the PTFE membrane is attached to a portion of a bottom layer of the PTFE membrane.

[0012] Certain embodiments provide a medical barrier that includes a sheet of unsintered substantially unexpanded polytetrafluoroethylene (PTFE) polymer material having a density in a range of about 1.2 gm/cc to about 2.3 gm/cc, and preferably in the range of about 1.45 gm/cc to about 1.55 gm/cc, and having at least one textured surface. Preferably, the sheet has one textured surface and one substantially smooth surface, and has substantially uniform strength in all directions.

[0013] In certain embodiments, the sheet of the medical barrier has a thickness in a range of about 0.125 mm to about 0.25 mm. The textured surface can be formed by a plurality of indentations formed in the surface of the sheet. The indentations

can have a depth less than the thickness of the sheet and each indentation can have a preferred width of about 0.5 mm. The indentations can be distributed substantially uniformly over the surface of the sheet. In certain embodiments, the indentations are distributed over the surface of the sheet at about 196 indentations per square centimeter.

[0014] The medical barrier of the present invention can be particularly well adapted for use in guided tissue regeneration in the repair of bone defects, and particularly in the repair of alveolar bone defects. The barrier prevents the entry of rapidly migrating gingival tissue cells into the defect and allows the alveolar bone to regenerate. During healing, the gingival tissue adheres somewhat to the textured surface of the barrier to anchor the gingival tissue over the barrier, thereby preventing dehiscence or splitting open of the tissue covering the material. However, the high density unexpanded substantially non-porous nature of the medical barrier of the present invention can prevent gingival tissue from growing into or through the barrier and the barrier may be removed with a minimum of trauma to the gingival tissue after the bone defect has healed.

BRIEF DESCRIPTION OF THE DRAWINGS

[0015] FIG. 1 is a perspective view showing the textured surface of the medical barrier of the present invention.

[0016] FIG. 2 is a perspective view showing the untextured surface of the medical barrier of the present invention.

[0017] FIG. 3 is an enlarged view of the textured surface of the medical barrier of the present invention.

[0018] FIG. 4 is a lateral cross-sectional view of a maxillary bony defect resulting from the extraction of a tooth.

[0019] FIG. 5 is a lateral cross-sectional view of the maxillary bony defect of FIG. 4 showing the placement of the medical barrier of the present invention to cover the bony defect with the mucoperiosteal flap sutured over the medical barrier.

[0020] FIG. 6 is a lateral cross-sectional view showing the healed maxillary bony defect of FIGS. 4 with the gingival tissue healed over the medical barrier of the present invention.

[0021] FIG. 7 depicts a first example of a titanium reinforcement binder.

[0022] FIG. 8 depicts a first example of a titanium reinforced bi-layered membrane.

[0023] FIG. 9 depicts a second example of a titanium reinforcement binder.

[0024] FIG. 10 depicts a second example of a titanium reinforced bi-layered membrane.

[0025] FIG. 11 depicts an assembly drawing for a third example of a reinforced bi-layered membrane.

[0026] FIG. 12 depicts an assembly drawing for a fourth example of a reinforced bi-layered membrane.

[0027] FIG. 13 depicts an assembly drawing for a fifth example of a reinforced bi-layered membrane.

DETAILED DESCRIPTION OF THE INVENTION

[0028] Embodiments of the present invention will now be described in detail with reference to the drawings, which are provided as illustrative examples so as to enable those skilled in the art to practice the invention. Notably, the figures and examples below are not meant to limit the scope of the present invention to a single embodiment, but other embodiments are possible by way of interchange of some or all of the described or illustrated elements. Wherever convenient, the same reference numbers will be used throughout the drawings to refer to same or like parts. Where certain elements of these embodiments can be partially or fully implemented using known components, only those portions of such known components that are necessary for an understanding of the present invention will be described, and detailed descriptions of other portions of such known components will be omitted so as not to obscure the invention. In the present specification, an embodiment showing a singular component should not be considered limiting; rather, the invention is intended to encompass other embodiments including a plurality of the same component, and vice-versa, unless explicitly stated otherwise herein. Moreover, applicants do not intend for any term in the specification or claims to be ascribed an uncommon or special meaning unless explicitly set forth as such. Further, the present invention encompasses present and future known equivalents to the components referred to herein by way of illustration.

[0029] The term sintered is a term well known in the art and is used herein consistent with that understanding. The term unsintered is used herein to describe

PTFE polymer that has not been subjected to the sintering process. Unsintered PTFE is substantially unexpanded and typically contains no substantially defined intermodal distance, which substantially reduces its porosity relative to e-PTFE. The limited porosity of the unsintered, substantially unexpanded d-PTFE substantially reduces tissue adhesions to the d-PTFE or migration of tissue into the d-PTFE. However, the limited porosity allows for the passage of ions and other small molecules necessary for cellular nourishment and waste transport.

[0030] Certain aspects of the invention will be described with reference to the example depicted in Figs. 1 and 2. Certain embodiments of the invention employ a medical barrier 11. Barrier 11 may comprise a sheet of unsintered substantially unexpanded polytetrafluoroethylene (PTFE) polymer. Barrier 11 includes a textured surface 13 and an untextured surface 14. In one example, barrier 11 has a sheet thickness in the range of about 0.125 mm to about 0.25 mm and a density in the range of about 1.2 gm/cc to about 2.3 gm/cc. In another example, the density lies in the range of about 1.45 gm/cc to about 1.55 gm/cc. With reference to Fig. 3, the textured surface can be formed by a plurality of indentations 15 formed in surface 13 of barrier 11. Indentations 15 may be hexagonal in shape, although other shapes are contemplated and fall within the scope of the invention. The indentations can have a depth less than the thickness of the sheet and, in certain embodiments, indentations 15 can be about 0.15 mm deep. The indentations 15 may be dimensioned based on application and the width can be greater or smaller, including for example, dimensions of about 0.5 mm wide.

[0031] The distribution of indentations 15 can be substantially uniform over surface 13 of barrier 11. In one example, approximately 150 indentations are provided per square centimeter over surface 13 of sheet 11. In another example 250 indentations are provided per square centimeter over surface 13 of sheet 11.

[0032] Figs. 4-6, show an example of the manner of use of the barrier of the present invention. Fig. 4 is a lateral cross-sectional view of an adult human maxilla after a tooth extraction showing the bone of the alveolar process 17. Soft tissue gingiva 19 covers bone 17. A tooth socket 21 provides an example of a bone defect. Other examples of bone defects are those caused by periodontal disease, cyst formation, surgery, or trauma. Normal healing of a defect includes migration of foreign cells such as fibroblasts and gingival epithelial cells. As the cells proliferate into the defect, they inhibit bone cell regeneration, which results in overall loss of

bone mass. In the case of extractions, the loss of bone mass results in a loss of alveolar ridge profile.

[0033] Fig. 5 is an example of a method for using the barrier of the present invention. Socket 19 is packed with granular particles of hydroxyapatite as a precursor to bone. Other materials and/or articles, such as endosseous type dental implants, may be placed into socket 21. The packed socket 21 can be covered with a layer 23 of the barrier of the present invention. The smooth side of the barrier can be placed over socket 21 and bone 17. Thus, the textured side of the barrier can be positioned adjacent the gingival tissue 19. The material provides substantially uniform strength in all directions, thereby allowing the surgeon to shape layer 23 over socket 21 and bone 17. After layer 23 is placed over socket 21 and bone 17, the gingival flaps 19 are sutured over layer 23. Layer 23 holds the hydroxyapatite particles in place in socket 21 during healing and prevents migration of cells and connective tissue into socket 21. However, connective tissue typically forms a weak attachment with the textured surface of layer 23, without growing through the material. The attachment is weak enough that the layer may be removed after healing without significant trauma but is strong enough to prevent the dehiscence.

[0034] Fig. 6 shows a typical extraction site after healing, but prior to removal of layer 23. As shown in Fig. 6, the alveolar ridge profile 25 can be preserved and the gingival tissue 19 can be completely healed over ridge 25. Layer 23 may be removed by making a small incision (not shown) in gingival tissue 19 to expose a portion of layer 23. The layer 23 may then be pulled out with forceps or the like. The material can typically be easily pulled out without trauma to the patient because the attachment of the connective tissue to the textured surface is typically weak.

[0035] In certain embodiments, a multilayer reinforced material configured to span a bone cavity and adapted for fixation to bone surrounding the bone cavity can be used. The multilayer material can comprise various materials forming one or more layers to provide qualities such as: strength in substantially all directions, inertness, pliability, malleability, resistance to compressive forces, and adhesiveness, such that the materials used to form each layer can be selected to impart different functional capabilities. For example, the layers can optionally be made of PTFE, such as expanded PTFE, unsintered PTFE, high density PTFE, which typically provide strength, flexibility and inertness. In certain embodiments, a titanium binder forms a layer of the multi-layered material. The titanium binder is typically bendable

and can have one or more elongate members such that the titanium binder can be formed to obtain a desired shape and/or can be deformed, reformed to obtain the desired shape prior to placement about the bone defect and maintain the formed shape upon placement. In one example, portions or all of the binder can be bent, twisted and/or stretched as necessary to obtain the desired shape. In certain embodiments, other malleable or flexible inert materials can be used to form a binding layer. The titanium binding layer typically has one or more holes suitable for securing a fastener such as a surgical pin or screw to the bone repair site. In certain embodiments, the fastener secures the multilayered reinforced material to the surgical site.

[0036] In certain embodiments, layers of the multilayered reinforced material can be attached at one or more points. The layers may be fixed or attached using any suitable means, including use of an adhesive layer for attachment or bonding the layers. The PTFE layers partially cover the titanium binder. According to certain aspects of the invention, the PTFE layers can substantially envelope the titanium binder. Certain embodiments can include a bi-layered titanium reinforced material, as described in more detail below.

[0037] Fig. 7 shows an example of a titanium reinforcement binder for use in the bi-layered titanium reinforced membrane of Fig. 8 (described below). In certain embodiments, the titanium reinforcement binder has a frame 70 or body suitable for placement over a bone cavity, such as an alveolar cavity. The frame 70 which can have a first elongate member 71, for placement over the cavity toward a lingual side of the cavity, and two elongate members 72 and 73 in a "Y-shaped configuration" at an opposite end of the titanium binder, each having perforations or holes 74 and 75 for securing a fastener, such as a surgical screw to an area of bone, typically at a surgical site, for example on the buccal side of the jaw, or upper alveolar arch, in the repair of alveolar defects or maxillofacial defects.

[0038] In the example of Fig. 7, dimensions of the binder are selected based on the application. Similarly, the physical and mechanical properties of the binder are selected according to application. In the depicted examples, surgical grade titanium is used to provide malleability, strength and low weight. It will be appreciated that Titanium possesses strength and weight characteristics that, together with the biologically inert nature of the metal offers advantages in many applications. It is contemplated that some applications may indicate that other dimensions, ratios of

dimensions and materials may be employed. For example, repair of bone material in a pelvis or hip may require the use of steel or other materials.

[0039] The structural configuration of the binder may be selected as desired to facilitate ease of placement and use in reconstructive repair of bone defects of various sizes, related soft tissue repair or skeletal surgery. The structural configuration of the binder can be selected to provide one or more appendages, or elongate members, suitable for placement about bone or surrounding tissues. The overall shape of the binder may be selected to achieve a desired strength, load distribution, barrier support, placement of fasteners, comfort, ease of insertion and/or removal and so on. The binder can also comprise bendable non-toxic materials. Moreover, certain embodiments employ materials coated, layered or encased in non-toxic materials. Binders can comprise titanium, stainless steel, platinum, ceramics, composites, carbon fiber materials and customized micro- or nano-material-based materials.

[0040] Fig. 8 depicts an example of a bi-layered titanium reinforced membrane which is reinforced with the titanium binder shown in Fig 7. In this example, the bi-layered titanium reinforced membrane can have a body 80 with tapered or rounded edges which covers or encloses the titanium frame 81 on either side, such that the titanium frame 81 is placed within or enveloped between the layers of the membrane. The body 80 of the bi-layered reinforced membrane can have a narrowed portion 82 along one end and a wider portion 83 along an opposite end, such that the narrow portion 82 and wider portion 83 substantially covers and outlines the shape of the body of the titanium frame 81. The bi-layered titanium reinforced membrane of FIG. 8 can have a textured surface and a substantially smooth surface and can comprise two layers or sheets of PTFE. A first layer or sheet comprised of unsintered high density PTFE (dPTFE) having a density of about 1.2 gm/cc to about 2.3 gm/cc (as described in U.S. Patent No. 5,957,690) can be used to form the textured surface. A second layer or sheet which can be used to form the substantially smooth surface can be comprised of expanded PTFE (ePTFE) and have a measurable intermodal distance; Table 1 provides exemplary specifications for the intermodal distance and density.

	Characteristics	Value	Tolerance	Units	Sampling Plan	Level	AQL
1	Inside Diameter	20.00	+1.00/-1.50	mm	ANSI/ASQC Z1.9	GLII	2.5
2	Wall Thickness	0.25	± 0.04	mm	ANSI/ASQC Z1.9	GLII	2.5
3	Internodal Distance	65.0	± 15.0	Microns	ANSI/ASQC Z1.9	GLII	4.0

Table 1

[0041] Specifically, the d-PTFE material which may be implemented as the first layer or sheet of material forming the textured surface can be made from a high density PTFE with a density in a range of about 1.2 grams/cc to about 2.3 grams/cc; for some applications, the density of d-PTFE may be in a range of about 1.45 grams/cc to about 1.55 grams/cc. As set forth above, the d-PTFE material may be unsintered and unexpanded with a nominal pore channel size of less than about 5 micrometers. In some embodiments, the unsintered, unexpanded d-PTFE may have a nominal pore channel size of less than 2 micrometers. In some embodiments, the unsintered, unexpanded d-PTFE may have a nominal pore channel size of less than 0.5 micrometers. In some embodiments, the unsintered, unexpanded d-PTFE may have a nominal pore channel size of less than 0.2 micrometers. This small pore channel size may allow a composite multi-layer material employing d-PTFE to exhibit superior functional characteristics, resulting clinically in reduced host response (inflammation), soft tissue in-growth, and resultant adhesions.

[0042] The textured surface of the first layer or sheet of material forming the textured surface of the present invention can be made by first forming a thin sheet of unsintered PTFE and then embossing the sheet with indentations. PTFE resin is mixed with a lubricant such as mineral spirits to form a paste. The paste is then calendered between rollers to form a thin flat sheet of the desired thickness in the range of about 0.125 mm to 0.25 mm. The calendering is performed to reduce the thickness of the sheet and to impart substantially uniform strength in all directions to the sheet. The lubricant is removed by drying the sheet at temperature somewhat above the boiling point of the mineral spirit lubricant, but well below the sintering temperature of PTFE, which is about 327 degrees C. The foregoing process steps result in a flat sheet of unsintered PTFE about 0.125 to 0.25 mm thick, having a density in the range of about 1.2 gm/cc to about 2.3 gm/cc, and having substantially uniform strength in all directions. The resulting flat sheet has two substantially smooth surfaces.

[0043] After the sheet has been dried, the sheet can be embossed to form the indentations in one of its surfaces. In the certain embodiments, the embossing step can be performed by placing a sheet of patterned polymer mesh on top of the unembossed sheet of unsintered PTFE. The patterned polymer sheet material, such as polyethylene or polypropylene, is typically harder and has more compressive strength than the unsintered PTFE material. In some embodiments the polymer sheet can be a suitable commercially available fine pore-size sheet filter material. The polymer sheet can have a pattern that is embossed. The polymer sheet and the unsintered PTFE sheet can be passed together between a pair of rollers, which emboss the pattern of the polymer sheet into one surface of the unsintered PTFE sheet. After embossing, the polymer sheet may be discarded. After embossing, the embossed unsintered PTFE sheet may be cut into smaller sheets of various shape and size for formation of the titanium reinforced bi-layered membrane.

[0044] In some embodiments of the composite bi-layered titanium reinforced membrane, the sheet of unsintered, textured d-PTFE forming the first layer may be laminated or otherwise combined with the sheet of substantially smooth, expanded e-PTFE forming the second layer, to surround or envelope or at least partially surround or envelope, the titanium binder creating the titanium reinforced bi-layered membrane. The shape and size of the sheets forming the layers can vary such that each sheet is partially attached to the titanium binder. In certain embodiments, each sheet may partially cover or fully cover the titanium binder. Typically the sheets of the layers will be attached, at least partially. It will be appreciated that such attachment may be accomplished by stitching layers of material, exertion of hydraulic or other pressure, application of a biocompatible adhesive or heat, or some combination of the foregoing. One or more combinations may be used in the laminating process. The composite bi-layered titanium reinforced material constructed and operative in accordance with the present disclosure may have utility in applications related to the regeneration of soft tissue defects and surgical reconstruction of bone and skeletal defects throughout the body, including reconstruction to correct maxillofacial defects, such as alveolar defects and orbital defects.

[0045] In certain embodiments, the titanium binder can be attached at a point or at least partially attached to one the PTFE sheets forming the layers. The binder can be attached by such methods as bonding, or by adhesive or mechanical fasteners.

The attachment of the titanium binder can form a patch, such that a sheet forming a first layer or a top layer can be bonded to a sheet forming a second layer, or bottom layer.

[0046] Fig. 9 shows an example of a titanium reinforcement binder. The titanium reinforcement binder can have a frame 90 or body suitable for placement over a bone cavity, such as an alveolar cavity. Frame 90 in the example has a plurality of elongate members including a pair of members 91 and 92 in an X-shaped configuration with two parallel elongate members 93 and 94 traversing the frame 90. Each of the plurality of elongate members 91-94 may be provided with a perforation or pilot hole. For example, elongate member 94 has a hole 95 located at a distal end of the member 94. Holes can be used for securing the frame 90 at one or more points using a fastener, such as a surgical screw or pin, to an area of bone at a surgical site. Pilot holes can be provided based on the application and/or dimensions of the defect to be repaired. In some embodiments, a plurality of predrilled pilot holes may be provided in the frame. Pilot holes enable a surgeon to more rapidly place and attach the fastener relative to the defect.

[0047] Fig. 10 shows a bi-layered titanium reinforced membrane reinforced by the titanium binder shown in Fig 9. The bi-layered titanium reinforced membrane can have a body 100 with tapered or rounded edges which can cover or encloses the titanium frame 101 on either side, such that the titanium frame 101 can be bonded within or enveloped between the layers of the membrane. The body 100 of the bi-layered reinforced membrane can be rectangular such that it covers the titanium binder.

[0048] The bi-layered titanium reinforced membrane of Fig. 10 can have a textured surface and a substantially smooth surface and can comprise two layers or sheets of PTFE. A first layer or sheet, which may comprise unsintered high density PTFE (dPTFE) having a density of about 1.2 gm/cc to about 2.3 gm/cc (as described in U.S. Patent No. 5,957,690), forms the textured surface. A second layer or sheet which can be used to form the substantially smooth surface is comprised of expanded PTFE (ePTFE) which has a measurable intermodal distance; the intermodal distance and the density are provided in the product specifications set forth in Table i .

[0049] Specifically, the d-PTFE material which may be implemented as the first layer, or sheet of material forming the textured surface can be a high density PTFE

with a density in a range of about 1.2 grams/cc to about 2.3 grams/cc; for some applications, the density of d-PTFE may be in a range of about 1.45 grams/cc to about 1.55 grams/cc. As set forth above, the d-PTFE material may be unsintered and unexpanded having a nominal pore channel size of less than about 5 micrometers. In some embodiments, the unsintered, unexpanded d-PTFE may have a nominal pore channel size of less than 2 micrometers. In some embodiments, the unsintered, unexpanded d-PTFE may have a nominal pore channel size of less than 0.5 micrometers. In some embodiments, the unsintered, unexpanded d-PTFE may have a nominal pore channel size of less than 0.2 micrometers. This small pore channel size may allow a composite multi-layer material employing d-PTFE to exhibit superior functional characteristics, resulting clinically in reduction of: host response (inflammation), soft tissue in-growth, and resultant adhesions.

[0050] In some embodiments, the textured surface of the first layer or sheet of material used to form the textured surface can be made by first forming a thin sheet of unsintered PTFE and then embossing the sheet with indentations as described above.

[0051] In accordance with some embodiments, the sheet of unsintered, textured d-PTFE which can be used to form the first layer may be laminated or otherwise combined with the sheet of substantially smooth, expanded e-PTFE which can be used to form the second layer, such that the layers surround, envelope, or at least partially attach. It will be appreciated that such attachment may be accomplished by stitching layers of material, exertion of hydraulic or other pressure, application of a biocompatible adhesive or heat, or some combination of the foregoing. One or more combinations may be used in the laminating process. The composite bi-layered titanium reinforced material constructed and operative in accordance with the present disclosure may have utility in applications related to the regeneration of soft tissue defects and surgical reconstruction of bone and skeletal defects throughout the body, including reconstruction to correct maxillofacial defects, such as alveolar defects and orbital defects.

[0052] The bilayered titanium reinforced membrane as shown in Fig. 10 can be used in the repair of larger areas of bone or skeletal defects, for example on the alveolar arch or other craniofacial defects such as those to the orbit of the eye. The unsintered, textured d-PTFE surface which can form the first layer can be placed such that it faces or is adjacent to the soft tissue, for example the gingival tissue, and

the substantially expanded e-PTFE forming the second layer can be placed such that it faces, or is adjacent to the bone or skeletal area or cavity. It is contemplated that different configurations and sequences of layers may be employed in various applications. The material of the membrane has a substantially uniform strength in all directions and allows the surgeon to shape the membrane to a desired configuration for placement at the surgical site. The titanium frame 101 may also be shaped or formed by bending prior to placement at the site. The titanium binder can be made from such materials that it holds its shape when bent. The bilayered titanium reinforced membrane is placed over or about a bone cavity or, the desired surgical site with the unsintered, textured d-PTFE forming the first layer facing the soft tissue, or for example the gingival tissue, and the with the sheet of substantially smooth, expanded e-PTFE forming the second layer facing or adjacent to the bone or skeletal cavity. The titanium reinforced bilayered membrane can then be fixed or fastened to the bone by surgical pins or screws secured to the surgical site by placement through, for example the pilot hole 102, along the distal end of the elongate member 103, of the titanium frame 101.

[0053] Figures 11-13 depict components used in the manufacture of reinforced bilayered membranes. In each of these drawings, a multilayer reinforced component 110, 120 and 130 is formed using a plurality of layers. In the examples depicted, a strength member 112, 122 and 132 is formed in a desired shape from a material suited to the application. Suitable materials can include titanium, stainless steel, composite, carbon fiber and customized micro- or nano-material based materials. First and second layers of membranes 114 and 116, 124 and 126 and 134 and 136 may be provided above, below or around strength member 112, 122 and 132. First and second layers of membranes 114 and 116, 124 and 126 and 134 and 136 may be bonded to strength member 112, 122 and 132 using adhesive and/or mechanical fasteners.

[0054] From the foregoing, it may be seen that the medical barrier of the present invention overcomes the shortcomings of the prior art, and is particularly well adapted for use in guided tissue regeneration in the repair of bone defects, as for example in the repair of alveolar bone defects. The barrier prevents the entry of rapidly migrating gingival tissue cells into the defect and allows the alveolar bone to regenerate. During healing, the gingival tissue adheres somewhat to the textured surface of the barrier to anchor the gingival tissue over the barrier, thereby

preventing dehiscence or splitting open of the tissue covering the material. However, the high density unexpanded substantially non-porous nature of the medical barrier of the present invention prevents gingival tissue from growing into or through the barrier. Thus, after the bone defect has healed, the barrier may be removed with a minimum of trauma to the gingival tissue.

Additional Descriptions of Certain Aspects of the Invention

[0055] The foregoing descriptions of the invention are intended to be illustrative and not limiting. For example, those skilled in the art will appreciate that the invention can be practiced with various combinations of the functionalities and capabilities described above, and can include fewer or additional components than described above. Certain additional aspects and features of the invention are further set forth below, and can be obtained using the functionalities and components described in more detail above, as will be appreciated by those skilled in the art after being taught by the present disclosure.

[0056] Certain embodiments of the invention provide methods of repairing bone defects. Some of these embodiments comprise covering a portion of a bone defect using a reinforced membrane. Some of these embodiments comprise securing soft tissue about the membrane, whereby the membrane facilitates healing of the defect. In some of these embodiments, the membrane comprises a plurality of layers, including a binding layer and a polytetrafluoroethylene polymer (PTFE) layer, the PTFE layer having a textured surface and a substantially smooth surface. In some of these embodiments, the textured surface provides a top surface of the membrane. In some of these embodiments, the substantially smooth surface contacts the bone. In some of these embodiments, the textured surface comprises unsintered PTFE. In some of these embodiments, the substantially smooth surface comprises expanded PTFE. In some of these embodiments, the binding layer comprises a titanium binder.

[0057] Some of these embodiments comprise filling the bone defect with particulate grafting material prior to placing the reinforced layered membrane. In some of these embodiments, the unsintered PTFE has a density of about 1.2 gm/cc to about 2.3 gm/cc. In some of these embodiments, the expanded PTFE has a measurable internodal distance. In some of these embodiments, the binding layer is positioned between a top and bottom PTFE layer.

[0058] Certain embodiments of the invention provide reinforced materials. Some of these embodiments comprise a titanium binder configured to span a bone cavity

and adapted for fixation to bone surrounding the bone cavity. Some of these embodiments comprise a PTFE membrane attached at one or more points to the titanium binder. In some of these embodiments, the titanium binder has one or more elongate members and wherein the titanium binder may be formed to obtain a desired shape. In some of these embodiments, the elongate members have one or more predrilled holes suitable for securing a fastener to an area of bone. In some of these embodiments, the fastener is a surgical screw. In some of these embodiments, the fastener is a surgical pin. In some of these embodiments, at least one of the elongate members is free to move independently of the PTFE membrane. In some of these embodiments, the PTFE membrane is attached to a portion of a bottom layer of the PTFE membrane.

[0059] Certain embodiments of the invention provide systems, methods and devices for repairing a bone defect. Some of these embodiments comprise covering a portion of a bone defect using a membrane that includes a reinforcing member. Some of these embodiments comprise fastening the reinforcing member to an area of bone. Some of these embodiments comprise securing soft tissue about the membrane. In some of these embodiments, the membrane facilitates healing of the defect. In some of these embodiments, the membrane comprises a plurality of layers, including a binding layer and a polytetrafluoroethylene polymer (PTFE) layer, the PTFE layer having a textured surface and a substantially smooth surface.

[0060] In some of these embodiments, the textured surface provides a top surface of the membrane. In some of these embodiments, the substantially smooth surface contacts the bone. In some of these embodiments, the textured surface comprises unsintered PTFE. In some of these embodiments, the unsintered PTFE has a density of between 1 gm/cc to about 4 gm/cc. In some of these embodiments, the substantially smooth surface comprises expanded PTFE. In some of these embodiments, expanded PTFE has a measurable internodal distance. In some of these embodiments, the reinforcing member is embodied in the binding layer. In some of these embodiments, the binding layer comprises a titanium binder. In some of these embodiments, the binding layer is positioned between a top and bottom PTFE layer. Some of these embodiments comprise filling the bone defect with particulate grafting material prior to covering the portion of the bone defect with the membrane.

[0061] In some of these embodiments, the plurality of layers comprise a first layer formed from unsintered, substantially unexpanded polytetrafluoroethylene polymer having no measurable, repeatable intermodal distance. In some of these embodiments, the unsintered substantially unexpanded polytetrafluoroethylene polymer has a density in a range of about 1.2 gm/cc to about 2.3 gm/cc. In some of these embodiments, the unsintered substantially unexpanded polytetrafluoroethylene polymer has a plurality of pores having a nominal channel size of less than 5 micrometers. In some of these embodiments, the plurality of layers comprise a second layer formed from an open structured material. In some of these embodiments, surfaces of the first and second layers are attached at a common interface.


[0062] Although the present invention has been described with reference to specific exemplary embodiments, it will be evident to one of ordinary skill in the art that various modifications and changes may be made to these embodiments without departing from the broader spirit and scope of the invention. Accordingly, the specification and drawings are to be regarded in an illustrative rather than a restrictive sense.

WHAT IS CLAIMED IS:

1. A method of repairing a bone defect, comprising:
covering a portion of a bone defect using a membrane that includes a reinforcing member;
fastening the reinforcing member to an area of bone; and
securing soft tissue about the membrane, whereby the membrane facilitates healing of the defect.
2. The method of claim 1, wherein the membrane comprises a plurality of layers, including a binding layer and a polytetrafluoroethylene polymer (PTFE) layer, the PTFE layer having a textured surface and a substantially smooth surface.
3. The method of claim 2, wherein the textured surface provides a top surface of the membrane.
4. The method of claim 2, wherein the substantially smooth surface contacts the bone.
5. The method of claim 2, wherein the textured surface comprises unsintered PTFE.
6. The method of claim 5, wherein the unsintered PTFE has a density of about 1.2 gm/cc to about 2.3 gm/cc.
7. The method of claim 2, wherein the substantially smooth surface comprises expanded PTFE.
8. The method of claim 6, wherein the expanded PTFE has a measurable internodal distance.
9. The method of claim 2, wherein the reinforcing member is embodied in the binding layer, and wherein the binding layer comprises a titanium binder.
10. The method of claim 9, wherein the binding layer is positioned between a top and bottom PTFE layer.
11. The method of claim 1, further comprising filling the bone defect with particulate grafting material prior to covering the portion of the bone defect with the membrane.


12. A reinforced material comprising:
 - a titanium binder configured to span a bone cavity and adapted for fixation to bone surrounding the bone cavity; and
 - a PTFE membrane attached at one or more points to the titanium binder,wherein
 - the titanium binder has one or more elongate members and wherein the titanium binder may be formed into a desired shape.
13. The reinforced material of claim 12, wherein the elongate members have one or more predrilled holes suitable for securing a fastener to an area of bone.
14. The reinforced material of claim 13, wherein the fastener is a surgical screw.
15. The reinforced material of claim 13, wherein the fastener is a surgical pin.
16. The reinforced material of claim 12, wherein at least one of the elongate members is free to move independently of the PTFE membrane.
17. The reinforced material of claim 12, wherein the PTFE membrane is attached to a portion of a bottom layer of the PTFE membrane.

FIG-1

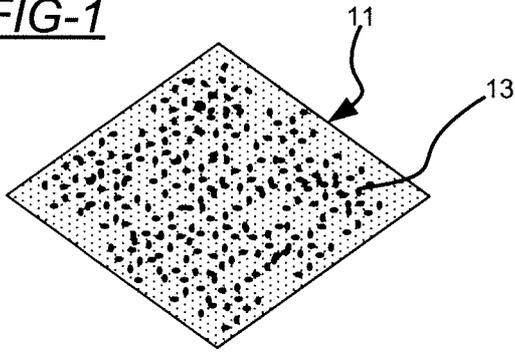


Textured Surface




FIG-2

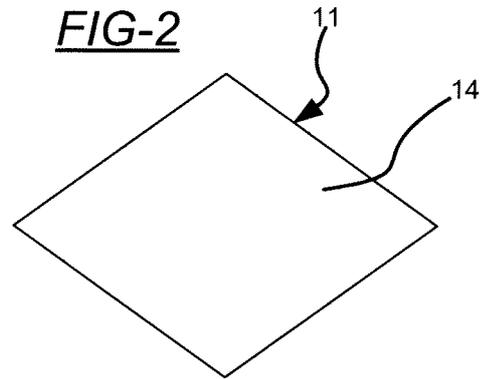





Untextured Surface

FIG-3

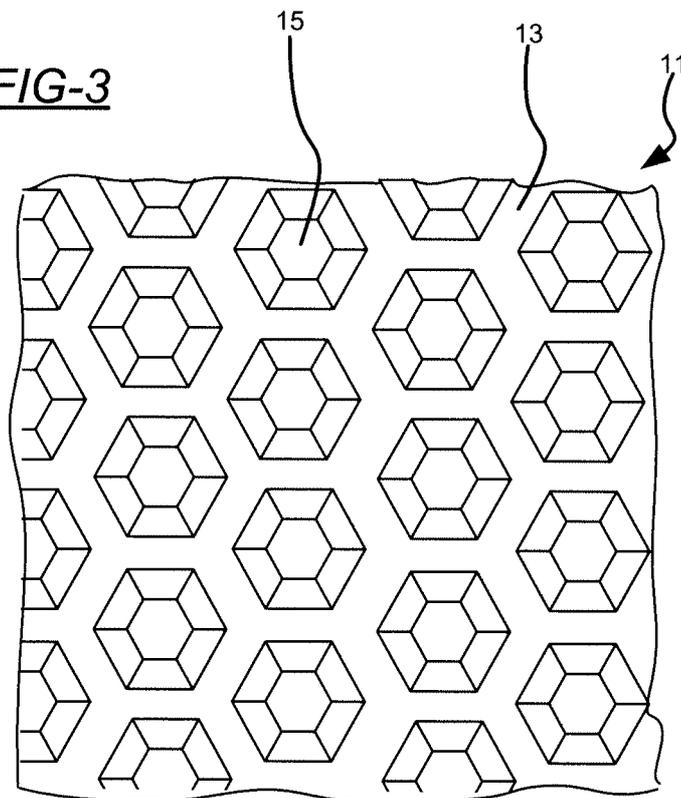

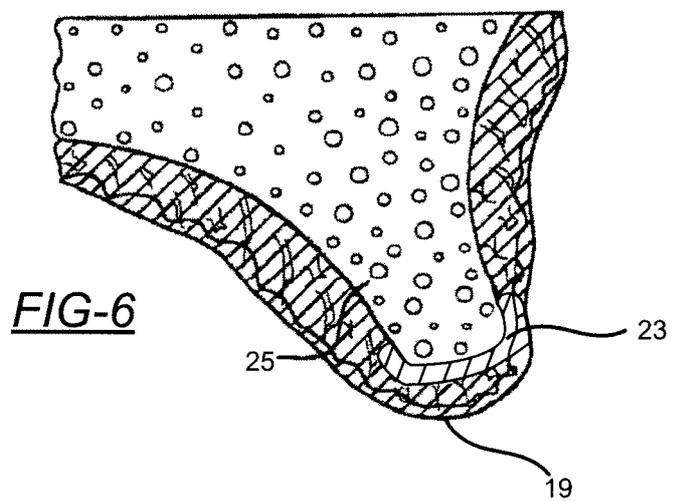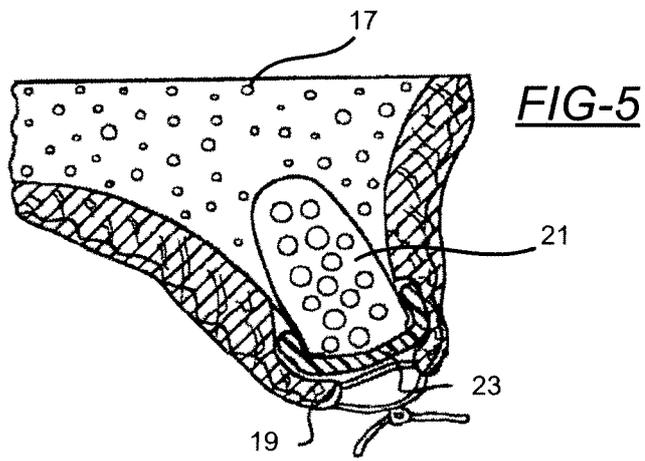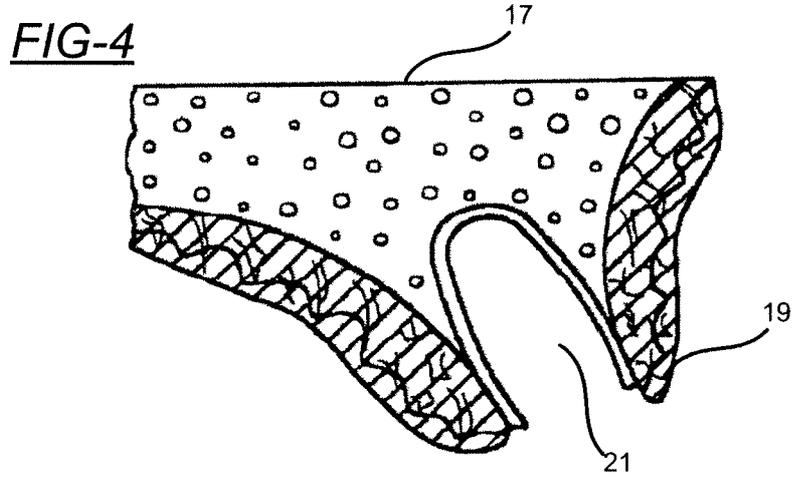

BUCCAL

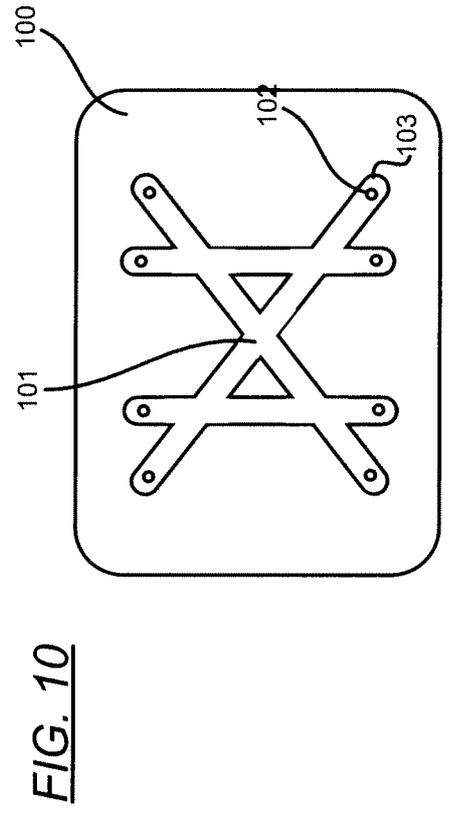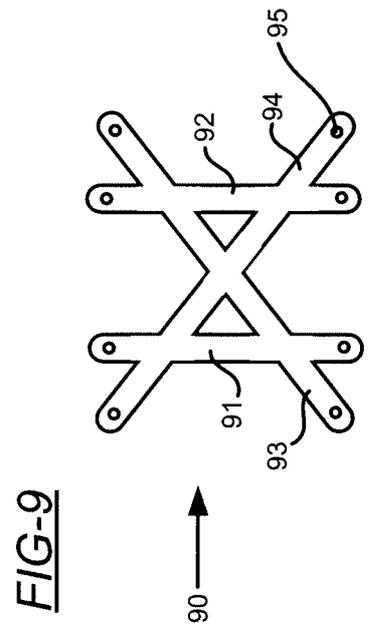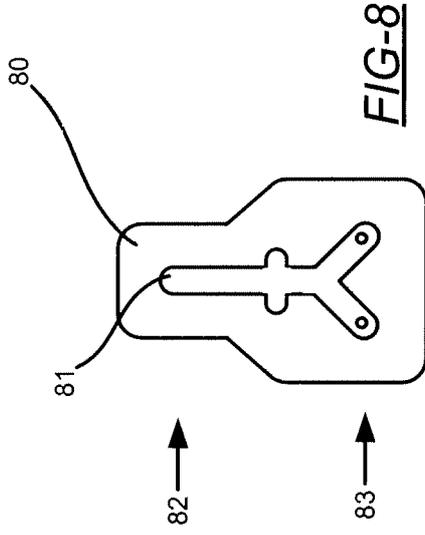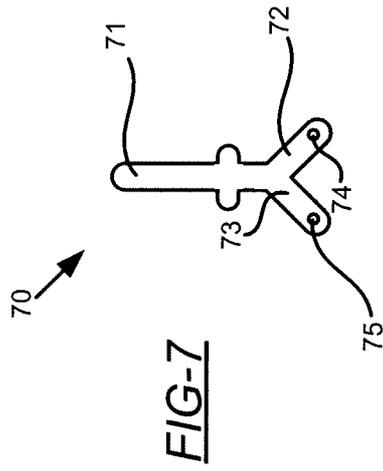

4/6



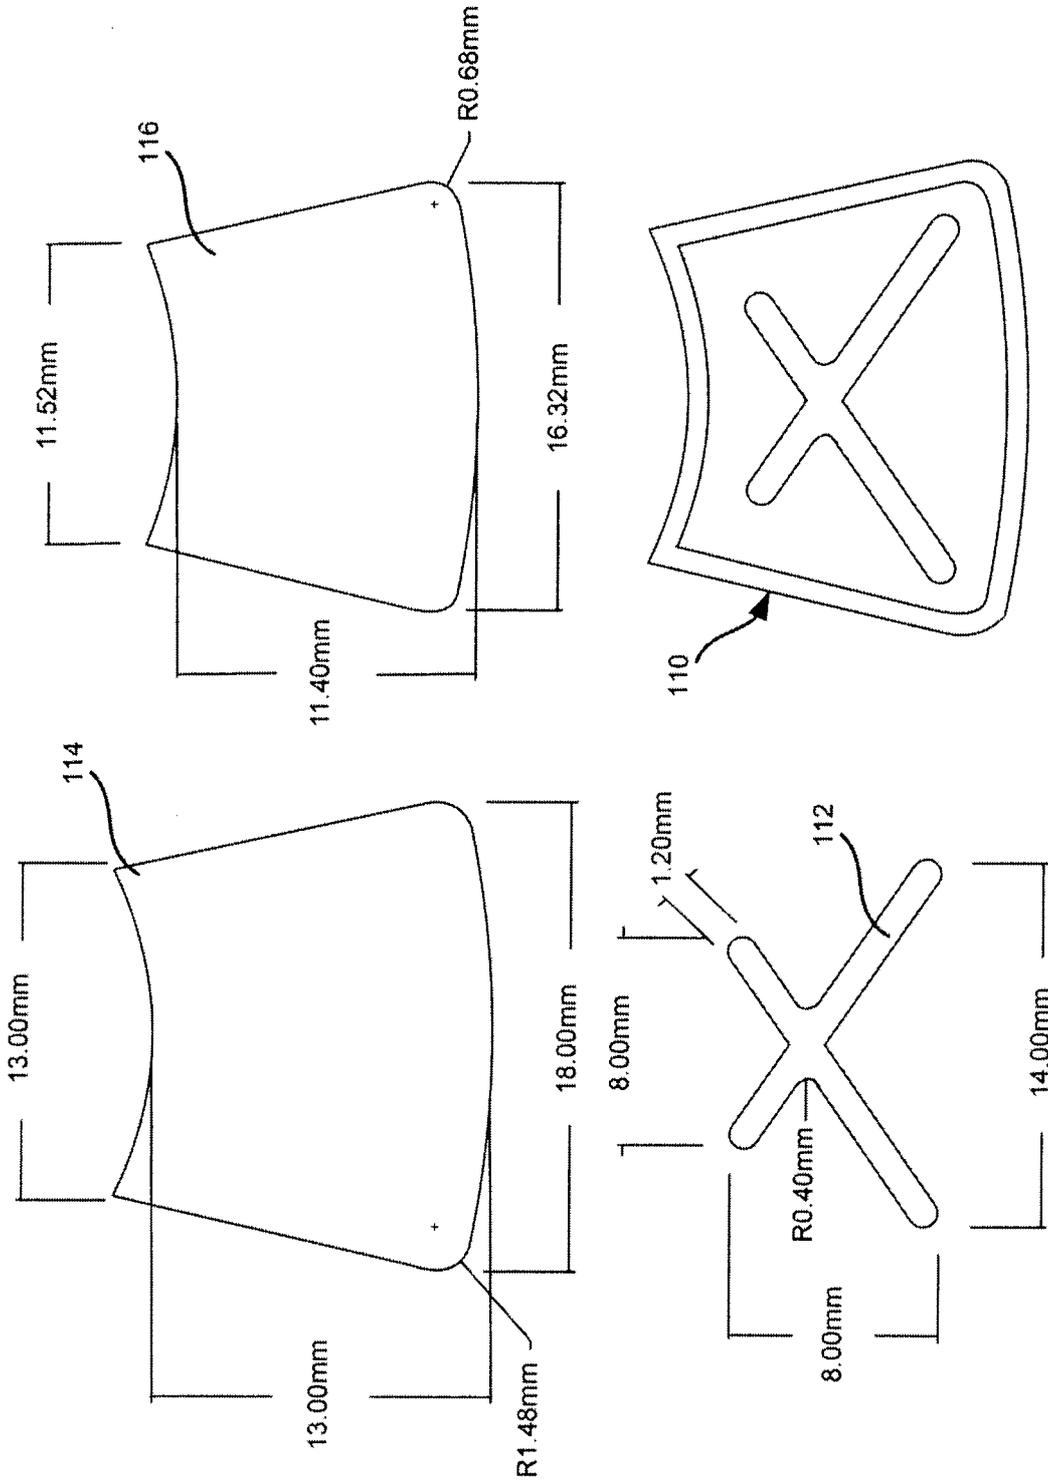


FIG-11

Perio/Furcation Posterior



5/6

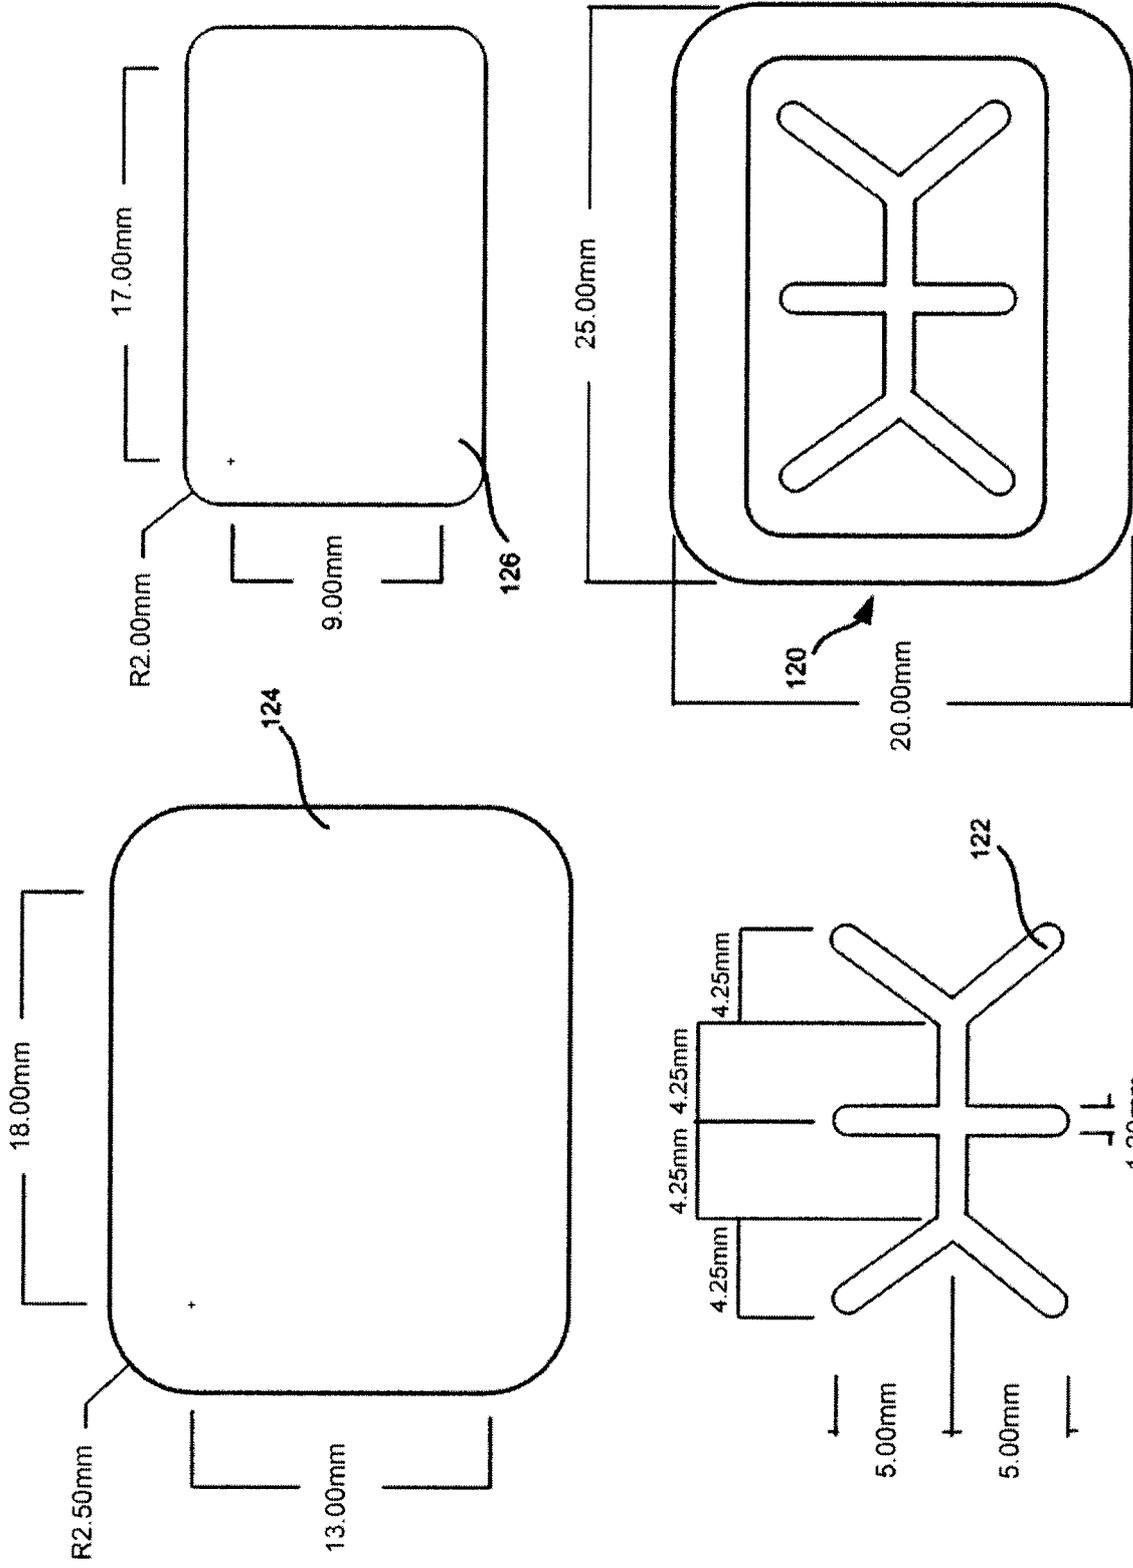

Posterior Single FIG-12

6/6




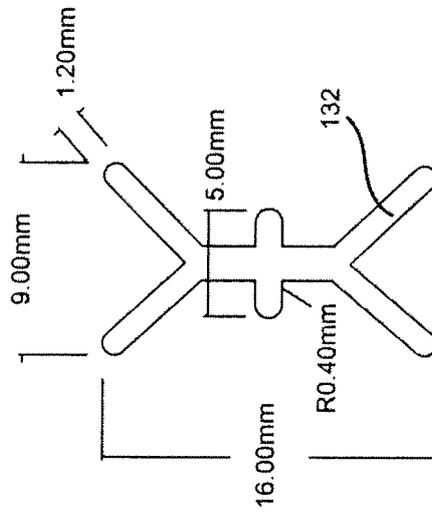


FIG-13

Anterior Single

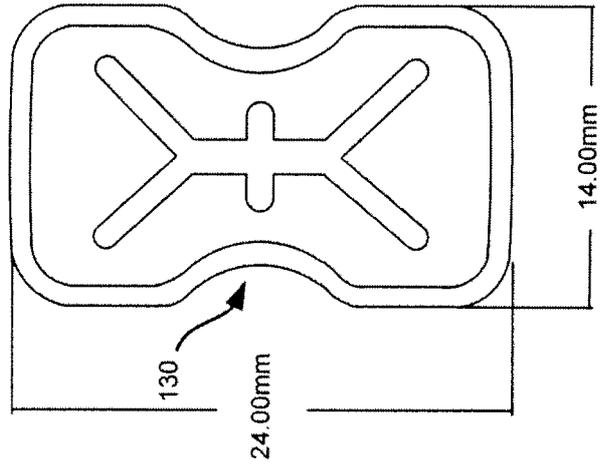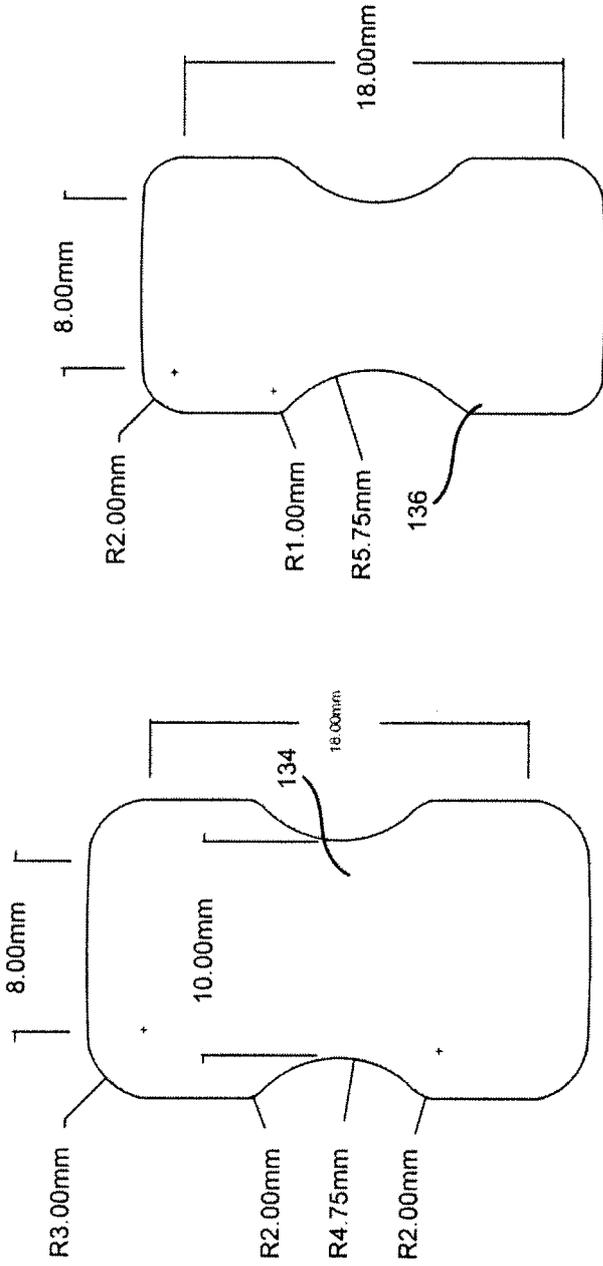

INTERNATIONAL SEARCH REPORT

International application No

PCT/US2010/025093

A CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61 F 2/28 (201 0.01)

USPC - 623/23.76

According to International Patent Classification (IPC) or to both national classification and IPC

B FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC(B) - A61F 2/28 (2010 01)

USPC - 623/23 76, 623/17 19, 623/23 5

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

MicroPatent, Fr̄patentsonhn β, Google, Google Patent, Science Direct, Google Scholar

C DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No
Y	US 2006/0224242 A1 (SWORDS et al) 05 October 2006 (05 10 2006) see entire document	1-17
Y	US 2005/0102036 A1 (BARTEE et al) 12 May 2005 (12 05 2005) see entire document	1-17
Y	VANDANA et al 'Preliminary Study Of The Guided Tissue Regeneration Procedures For Adjacent Buccal Root Coverage Using Single Gtam-Tr6t Membrane' Journal of Clinical and Diagnostic Research (serial online) 2008 February (cited 2009 February 2) Vol 3, pg 1365-1 369, Accessed at http //www jcdr net/back_ issues asp? issn=0973-709x&year=2009&month=February &volume=3& issue=1 &page=1 365-1 369& id=341	12-17
A	US 5,093,179 A (SCANTLEBURY et al) 03 March 1992 (03 03 1992) see entire document	1-17
A	US 2007/0061015 A1 (JENSEN et al) 15 March 2007 (15 03 2007) see entire document	1-17

 Further documents are listed in the continuation of Box C

* Special categories of cited documents	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be of particular relevance	"X" document of particular relevance, the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier application or patent but published on or after the international filing date	"Y" document of particular relevance, the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

12 April 2010

Date of mailing of the international search report

22 APR 2010

Name and mailing address of the ISA/US

Mail Stop PCT, Attn ISA/US, Commissioner for Patents
P O Box 1450, Alexandria, Virginia 22313-1450

Facsimile No 571-273-3201

Authorized officer

Blame R Copenheaver

PCT Helpdesk 571 272-4300
PCTOSP 571-272 7774