



US00D846138S

(12) **United States Design Patent** (10) **Patent No.:** **US D846,138 S**
Masuda et al. (45) **Date of Patent:** **** Apr. 16, 2019**

(54) **CLINICAL ANALYZER**

Primary Examiner — Anhdao Doan

(71) Applicant: **Hitachi High-Technologies Corporation**, Minato-ku, Tokyo (JP)

(74) *Attorney, Agent, or Firm* — Crowell & Moring LLP

(72) Inventors: **Ai Masuda**, Tokyo (JP); **Hiroyuki Noda**, Tokyo (JP); **Mitsuru Oonuma**, Tokyo (JP); **Tetsuji Kawahara**, Tokyo (JP); **Takamichi Mori**, Tokyo (JP)

(57) **CLAIM**

The ornamental design for a clinical analyzer, as shown and described.

(73) Assignee: **Hitachi High-Technologies Corporation**, Tokyo (JP)

DESCRIPTION

(**) Term: **15 Years**

This application contains subject matter related to the following co-pending U.S. design patent applications:

(21) Appl. No.: **29/627,767**

Application Ser. No. 29/627,777, filed herewith and entitled “Clinical Analyzer”;

(22) Filed: **Nov. 29, 2017**

Application Ser. No. 29/627,778, filed herewith and entitled “Clinical Analyzer”;

(30) Foreign Application Priority Data

Application Ser. No. 29/627,780, filed herewith and entitled “Clinical Analyzer”;

May 31, 2017 (JP) 2017-011783

Application Ser. No. 29/627,764, filed herewith and entitled “Clinical Analyzer”;

(51) **LOC (11) Cl.** **24-01**

Application Ser. No. 29/627,774, filed herewith and entitled “Clinical Analyzer With Graphical User Interface”; and

(52) **U.S. Cl.**

Application Ser. No. 29/627,781, filed herewith and entitled “Clinical Analyzer With Graphical User Interface”.

USPC **D24/216**

(58) Field of Classification Search

FIG. 1 is a front, top and right side perspective view of a clinical analyzer according to the design;

USPC D24/107, 169, 185, 186, 216–219, D24/231–234; D10/81

FIG. 2 is a front elevational view thereof;

CPC G01N 2035/00306; G01N 2035/00326; G01N 2035/00336; G01N 2030/027; G01N 21/76

FIG. 3 is a right side elevational view thereof;

See application file for complete search history.

FIG. 4 is a left side elevational view thereof;

FIG. 5 is a top plan view thereof;

FIG. 6 is a bottom plan view thereof;

FIG. 7 is a rear elevational view thereof;

(56) References Cited

FIG. 8 is a front, top and right side perspective view thereof shown in an opened position;

U.S. PATENT DOCUMENTS

FIG. 9 is an enlarged cross-sectional view taken in the direction of line 9-9 of FIG. 2; and,

D643,936 S * 8/2011 Oonuma D24/232

FIG. 10 is an enlarged cross-sectional view taken in the direction of line 10-10 of FIG. 2.

D653,765 S * 2/2012 Oonuma D24/216

The broken lines illustrate portions of the clinical analyzer that form no part of the claimed design.


D740,435 S * 10/2015 Oonuma D24/216

D740,956 S 10/2015 Oonuma et al.

D740,957 S * 10/2015 Oonuma D24/216

(Continued)

1 Claim, 6 Drawing Sheets

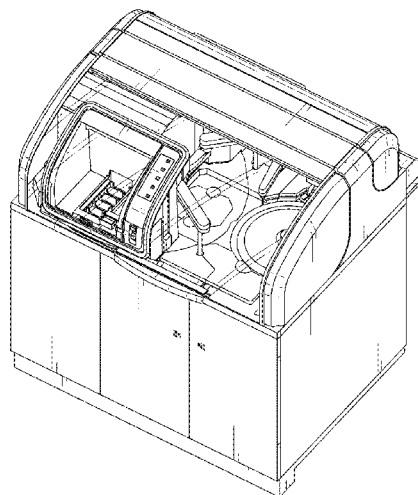

(56)

References Cited

U.S. PATENT DOCUMENTS

D810,956	S *	2/2018	LiCalzi	D24/216
D812,241	S *	3/2018	LiCalzi	D24/216
2014/0329270	A1 *	11/2014	Favaloro	G01N 1/312
				435/30
2014/0342358	A1 *	11/2014	Dockrill	G01N 1/312
				435/6.11
2017/0234898	A1 *	8/2017	Luoma, II	G01N 35/0095
				436/48
2017/0269114	A1 *	9/2017	Bryant	G01N 35/04

* cited by examiner

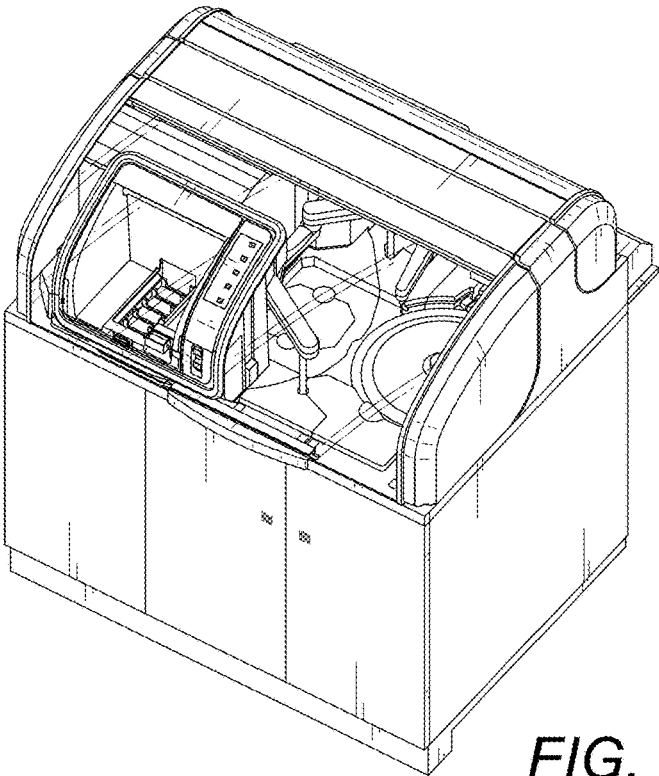


FIG. 1

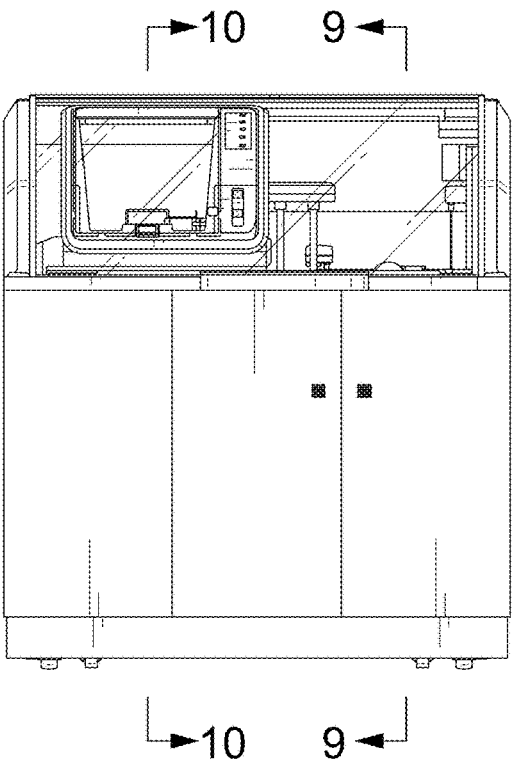


FIG. 2

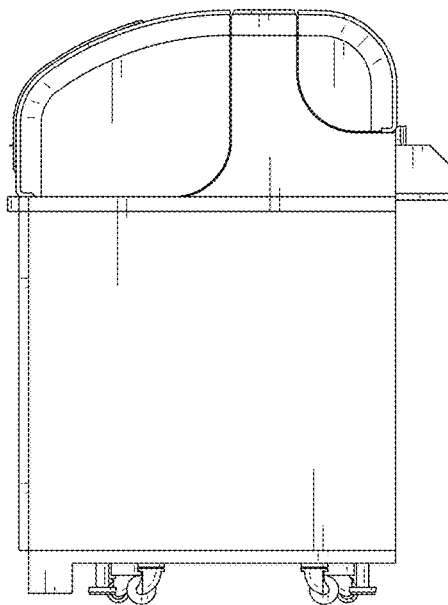


FIG. 3

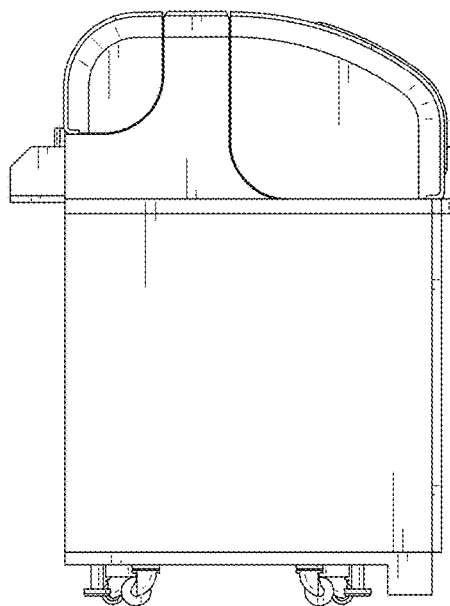


FIG. 4

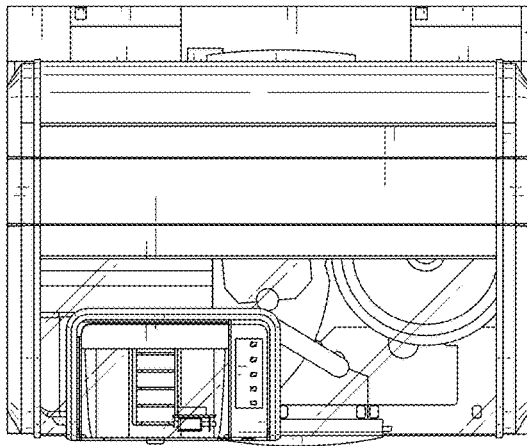


FIG. 5

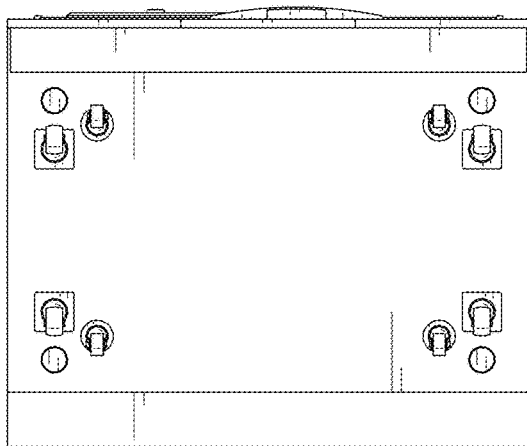


FIG. 6

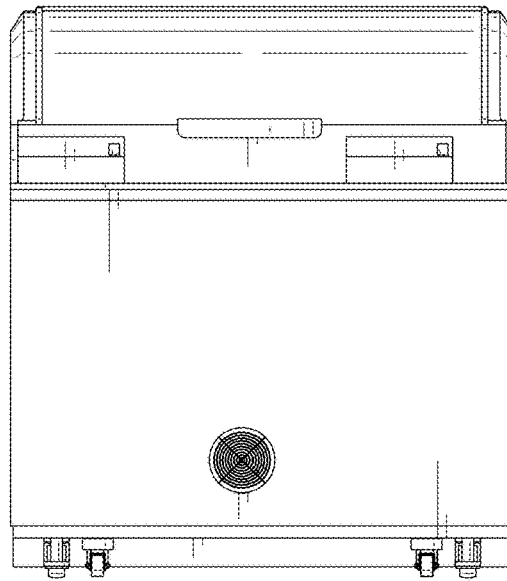


FIG. 7

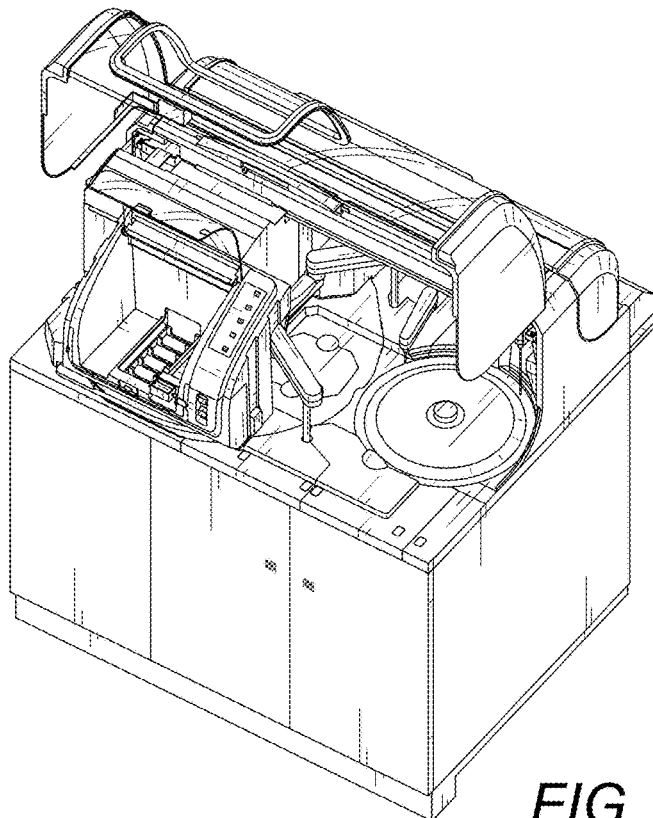


FIG. 8

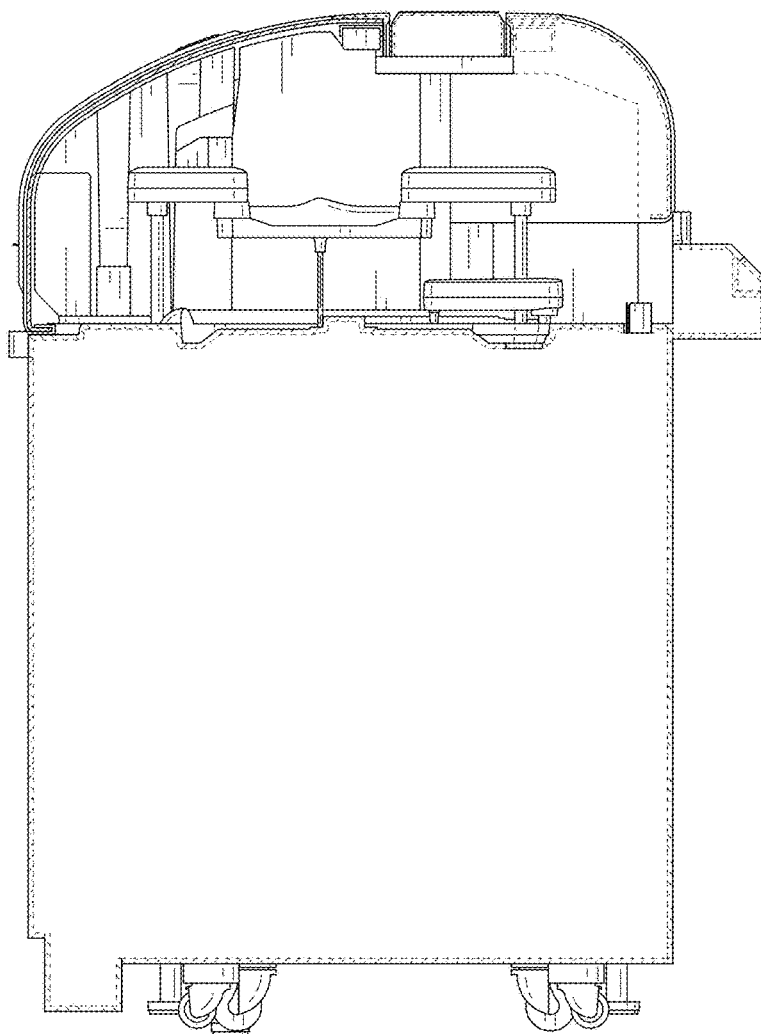


FIG. 9

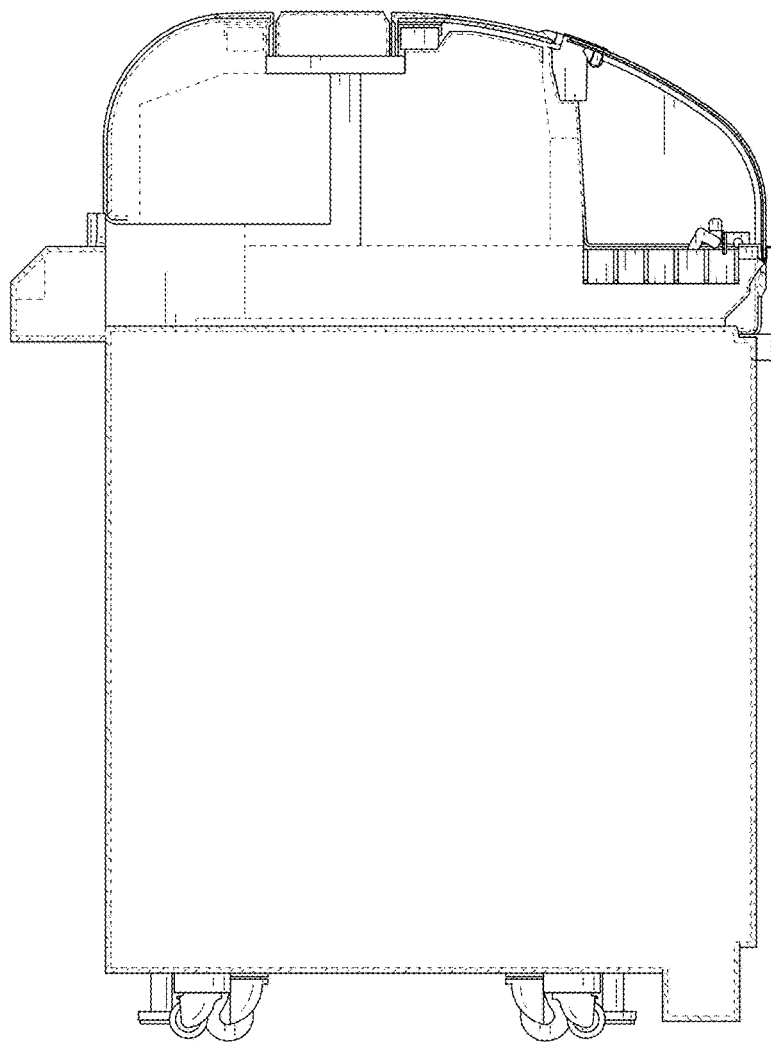


FIG. 10