

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
4 November 2004 (04.11.2004)

PCT

(10) International Publication Number
WO 2004/093679 A1

(51) International Patent Classification⁷: **A61B 5/0484**, 5/04

(21) International Application Number:
PCT/GB2004/001565

(22) International Filing Date: 13 April 2004 (13.04.2004)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
0309049.5 22 April 2003 (22.04.2003) GB

(71) Applicants (for all designated States except US): **THE VICTORIA UNIVERSITY OF MANCHESTER** [GB/GB]; Oxford Road, Manchester M13 9PL (GB). **UMIST VENTURES LIMITED** [GB/GB]; P.O. Box 88, Manchester M60 1QD (GB).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **POMFRETT, Christopher, John, Douglas**; 17 Manifold Close, Elworth, Sandbach, Cheshire CW11 1XP (GB). **MCCANN, Hugh**; 44 Patch Lane, Bramhall, Stockport, Cheshire SK7 1HX (GB).

(74) Agent: **ALLMAN, Peter, John**; Marks & Clerk, Sussex House, 83-85 Mosley Street, Manchester M2 3LG (GB).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Declaration under Rule 4.17:


— of inventorship (Rule 4.17(iv)) for US only

Published:

— with international search report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: NERVOUS SYSTEM MONITORING METHOD

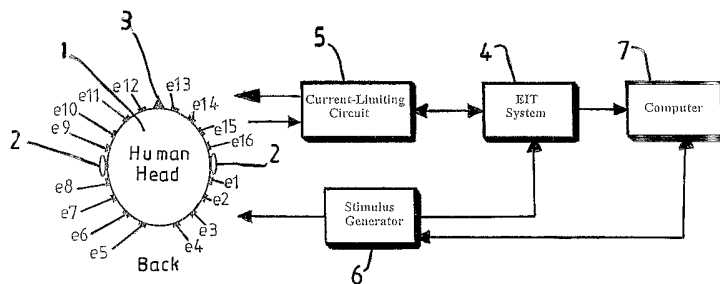

(57) Abstract: A method for monitoring the response of a nervous system of a body to a stimulus. The method comprises collecting a set of voltage measurements between selected areas on a surface of the body whilst current is being passed between selected regions of the surface of the body. The set of voltage measurements is collected over a predetermined measurement period, the predetermined measurement period is initiated at a predetermined time after application of the stimulus, and the collected voltage measurements are compared with reference to determine normal or abnormal response of the nervous system.

WO 2004/093679 A1

NERVOUS SYSTEM MONITORING METHOD

The present invention relates to a method for monitoring the response of a nervous system of a body to a defined stimulus, such as a flash of light before a subject's eyes or an audible sound adjacent to a subject's ears, or another event or sequence of events.

There is a well-known requirement for a method capable of imaging the activity of a nervous system such as a human brain which is sufficiently fast to capture neural activity with sub-second resolution. For example, Susan Greenfield, a professor of pharmacology at Oxford University, England, giving the Andrew Olle Memorial Trust lecture in Sydney, Australia in May 2000 stated that "I think that there is the plausible prospect in this century of being able to devise very good imaging techniques that enable us to catch that which we can't catch at the moment because the imaging techniques are too slow". The present invention is concerned with delivering a method which is capable of imaging the human brain to sub-second resolution.

As described by Pomfrett C.J.D. and Healy T.E.J. (1995), "Awareness and the Depth of Anaesthesia", Healy T.E.J and Cohen P.J. (eds) "A Practice of Anaesthesia", Edward Arnold, pages 864-878, it is well known that activity within the human brain can be monitored using standard EEG approaches. For example auditory, visual and somatosensory evoked responses can be generated which show that there is a latency after the occurrence of a stimulating event such as an audible sound or a light flash before sensory pathways in the brain respond. Typically there is a delay of at least several tens of milliseconds after a stimulating event before the evoked response can be detected by EEG equipment. Furthermore, although EEG equipment is capable of picking up signals showing that some response has been generated, the location of the source of such signals within the brain cannot be accurately determined from the detected signals.

It is known to use MRI and PET techniques to produce images of cerebral activity, but such techniques respond to haemodynamic and/or metabolic recovery processes which occur over time periods of typically many seconds or minutes and cannot therefore be used to image short term neural activity.

Electrical impedance tomography (EIT) has also been proposed as a method of imaging neurological functions within a body. US patent number 5919142 describes various EIT systems which have been proposed for measuring changes in impedance taking place within the brain and using those measurements to image the progress of information along circuits within the brain. It is stated that the brain may be stimulated by for example a visual signal and EIT images subsequently reconstructed for each millisecond or so of the recording "window", thus enabling the resultant action potential processes to be tracked along their pathways in the subject's brain. Although such a theoretical reconstruction to a resolution of milliseconds is discussed, it is conceded in US 5919142 that there is no established technique to permit accurate imaging of neuronal depolarisation with millisecond or sub-millisecond time resolution. It is stated that impedance changes associated with action potentials are generally very small and very rapid and the impedance of the tissue as a whole which is interposed between locations at which impedance measuring electrodes must be positioned may not change in proportion to changes in local action potentials.

Individual impedance measurements (or voltage measurements during current injection) take a finite length of time, typically measured in milliseconds, and in order to build up a sufficient number of impedance measurements to enable the generation of a single image of local impedance distributions within the brain a number of individual impedance measurements must be taken. Typically therefore it takes a few hundred milliseconds to collect sufficient impedance measurements to produce a single image of the brain, although it is feasible to measure voltages in parallel during current injection, thus reducing the measurement period to a few tens of milliseconds.

A further problem encountered with EIT systems when used for brain imaging is that changes of impedance resulting from neural activity within the brain are thought to be relatively small, for example between 0.1 and 1% of baseline impedance. If true, this makes it very difficult to distinguish impedance fluctuations resulting from changes in neural activity from background noise. The approach suggested in US patent 5919142 seeks to improve sensitivity to changes in impedance resulting from neural activity by taking a first set of impedance measurements whilst a first electrical input signal is being applied to the brain for a period of for example

100 milliseconds or more, taking a second set of impedance measurements when a second electrical input signal that is the reverse of the first is applied to the brain, calculating the difference between the two sets of measurements, and generating an image on the basis of the calculated difference. The application of the first and second input signals can be synchronised with the application of separate stimulus signals to the body. The problem with this approach is that there is a 100 millisecond delay between the generation of the two sets of signals which are compared so as to generate the data from which an image is subsequently generated. It is quite clear therefore that such a system cannot be sensitive to changes in impedance resulting from cerebral activity occurring over periods of only a few milliseconds.

US patent 5919142 dates from a priority date of 22nd June 1995. Since that date the same research group has continued with research into the use of electric impedance tomography for studying human brain activity. This is indicated by the paper "3-Dimensional Electrical Impedance Tomography of Human Brain Activity", Tidswell T., Gibson A., Bayford R.H. and Holder D.S., *Neuro Image* 13, 283-294 (2001). That paper describes the use of EIT to detect local changes in cerebral blood flow and blood volume. The data measurement for each impedance image was recorded over a period of 25 seconds. Before recording measurements, the neural stimulation process was initiated and remained active for several minutes. It is stated that reproducible impedance changes of about 0.5% lasted from 6 seconds after the onset of a stimulus to 41 seconds after stimulus cessation. The described system was however looking at the side-effects of brain activity, that is changes in blood flow and blood volume, rather than the neurological activity of which such changes are merely side effects. Furthermore, although some interesting results were generated, the paper itself concedes that problems of low resolution and reconstruction error remain which must be overcome if EIT is to be used as a fast neuro imaging tool with clear clinical applications. It is stated that a faster EIT system is being tested which will allow more measurements to be made per image but however many measurements are made, it still cannot be expected that the above technique will be sensitive to neuronal or synaptic phenomena occurring over a period of for example only one or a few milliseconds.

It is an object of the present invention to obviate or mitigate at least one of the problems outlined above.

According to a first aspect of the present invention, there is provided a method for monitoring the response of a nervous system of a body to an applied stimulus, comprising applying the stimulus, and collecting a set of voltage measurements between selected areas on a surface of the body whilst current is being passed between selected regions of the surface of the body, wherein the set of voltage measurements is collected over a predetermined measurement period, the predetermined measurement period is initiated a predetermined time after application of the stimulus, and the collected voltage measurements are compared with reference measurements to determine normal or abnormal response of the nervous system.

If a single set of measurements is taken, that set may be compared with predetermined data to assess neurological behaviour. If a series of sets of measurements are taken, neurological behaviour may be assessed by comparing different sets, and images representative of that behaviour may be generated.

The stimulus may be applied by the system, or alternatively may occur spontaneously. Occurrence of the stimulus may be detected, and this detection may start computation of the predetermined time. The stimulus may be a feature of an environment in which the body is located.

According to a second aspect of the present invention, there is provided a method for monitoring the response of a predetermined part of a nervous system of a body to an applied stimulus, comprising identifying the predetermined part of the nervous system, applying the stimulus, passing current between selected regions of the surface of the body, and collecting a set of voltage measurements between selected areas on the surface of the body, wherein the said regions and/or areas are selected on the basis of a neurological model of the nervous system and the applied stimulus such that sensitivity of the derived impedance measurements to changes in the predetermined part of the nervous system is maximised.

For example, if activity of the Lateral Geniculate Nucleus (LGN) is of interest, current may be passed between regions at the front and rear of the head to maximise the effect of activity in the LGN on the voltage measurements.

Embodiments of the present invention will now be described, by way of example, with reference to the accompanying drawings, in which:

Figure 1 is a schematic representation of an apparatus used in accordance with the method of the present invention;

Figure 2 represents current signals applied and voltage signals measured by the apparatus of Figure 1; and

Figure 3 shows six impedance images generated at various times after the application of a visual stimulus.

Figure 1 illustrates an apparatus for putting the invention into effect. A subject's head 1 has adhered to it sixteen electrodes e1 to e16 distributed in a plane around the head. In some circumstances it may be preferred to have a non-planar distribution of electrodes as described in Polydorides N., Lionheart W.R.B., and McCann, H.: "Krylov Subspace Iterative Techniques: On the detection of brain activity with electrical impedance tomography" IEEE Transactions on Medical Imaging, Volume 21, No 6, June 2002 pages 596-603. The subject's ears 2 and nose 3 are schematically illustrated to indicate the orientation of the subject's head. Calibrated headphones (not shown) are provided to deliver an auditory evoked response (AER) stimulus to the subject's ears and goggles (not shown) are provided which include light emitting diodes for generating a visually evoked response (VER) stimulus. Each of the sixteen electrodes is a silver-silver chloride EEG electrode of type, which present a relatively small contact impedance in the scalp.

An EIT system 4 is provided to deliver current to selected pairs of electrodes via a current limiting circuit 5 and to perform voltage measurements between other selected pairs of electrodes. A stimulus generator 6 also provides an input for the EIT system 4 such that EIT measurement can be effected at appropriate times relative to application of a stimulus. A computer 7 is provided to control the overall operation of the system and to log experimental results.

The equipment illustrated in Figure 1 is essentially conventional and will not therefore be described in further detail here. Characteristics of such equipment are well known and details may be derived for example from the documents referred to above.

In use, a stimulus such as a VER stimulus or an AER stimulus is applied to the subject. At a predetermined time after application of the stimulus a current is passed between a first pair of electrodes for a predetermined period. Thereafter current is injected between each pair of electrodes in turn. For each current injection a series of voltage measurements are taken between pairs of electrodes. Figure 2 comprises three parts, an upper part indicating application of the stimulus (represented by a vertical bar), a central part indicating periods during which current is passed between selected pairs of electrodes, and a lower part indicating periods during which voltage measurements are made between selected pairs of electrodes. Thus, after a time period denoted t_i after application of the stimulus, a start signal is sent from the stimulus generator 6 to the EIT system 4 of Figure 1. Thus, measurement is triggered at a predetermined time delay after stimulus application. Some embodiments of the EIT system may be configured to commence measurement at a delayed time after receipt of the start signal, and in such cases the time at which the stimulus generator 6 applies the start signal is adjusted accordingly.

After the start signal is received by the EIT system 4, current is passed between electrodes e1 and e9 for a period of 38 milliseconds. There is then a delay of 0.3 milliseconds, followed by a period of 38 milliseconds during which current is passed between electrodes e2 and e10. During the generation of a single set of measurements, this pattern of current injection is repeated for the following electrode pairs: e1-e9, e2-e10, e3-e11, e4-e12, e5-e13, e6-e14, e7-e15 and e8-e16. During application of current between electrodes e1 and e9, twelve voltage values are measured between adjacent electrodes in sequence, that is electrodes e2-e3, e3-e4, e4-e5, e5-e6, e6-e7, e7-e8, e10-e11, e11-e12, e12-e13, e13-e14, e14-e15, and e15-e16. Some of these measurements are illustrated in the lower part of figure 2. No measurements are made between electrode pairs including either of the electrodes (e1 and e9) between which current is passed. Each of the voltage measurements is taken over a period of 3.0 milliseconds with a delay of 0.18 milliseconds between successive measurements.

During the first current injection period, the first voltage measurement is taken between electrodes e2 and e3, (electrode e1 being used for current injection) whereas the first voltage measurement during the second current injection period is taken

between electrodes e3 and e4 (electrode e2 being used for current injection). The same rolling pattern of electrode selections continues through the full series of eight current injection periods. The EIT system applies a delay of 2 milliseconds between receipt of a signal from the stimulus generator, and initiation of current injection. Thus a full series of measurements is accumulated over a period of $2+8 \times 38 + 7 \times 0.3 = 308.1$ ms.

By applying a stimulus and obtaining a complete set of voltage measurements as described above, an image of the impedance distribution in the brain can be created using known image reconstruction algorithms (see for example "Krylov Subspace Iterative Techniques: on the detection of brain activity with electrical impedance tomography" as referred to above). Such an image can then be viewed by a medical practitioner to determine whether or not the brain has responded to the application of the stimulus in a normal manner. That is, it is known from neurological models which part of the brain should be active at a predetermined t_l value (Figure 2) after application of a particular type of stimulus, and thus the image can be analysed to determine whether or not activity is present as expected in the brain.

The time delay t_l between application of the stimulus and initiation of the EIT measurement process may be variable by a user, using functionality provided by the computer 7 (Figure 1). Thus, a plurality of images may be generated, by presenting a plurality of stimuli to the user, and initiating EIT measurement at a different t_l value after application of each stimulus. Using this method a plurality of images can be created which can be arranged in order of increasing t_l to represent changing brain activity at different times following application of a stimulus.

In some applications, the computer 7 may be programmed to control the stimulus generator 6 to present the plurality of stimuli, take the necessary measurements at various times after stimulus application, and present the results to the user. In other applications, the computer may be programmed so as to expect a user specified t_l value, apply a stimulus, initiate EIT measurement after the user specified time delay, and create an image using the measurements obtained. Upon reviewing the created image, the user may determine that further images need to be generated at different specific t_l values, and thus further single images can be created.

If the computer 7 is programmed to apply a plurality of stimuli, and generate a plurality of images at different t_i values, delays between successive stimuli are varied in a random manner so as to avoid the subject's brain being "trained" to expect stimuli at particular times. Furthermore, the delay times between different stimuli and the initiation of EIT measurement can be varied in a random manner. Thus images are not generally generated in order of increasing time delay.

Referring to Figure 3, there are illustrated six impedance measurements generated at different delays after the application of a visual stimulus. The top left hand image of Figure 3 was generated by starting EIT measurement at approximately 80 milliseconds after the application of a visual stimulus. The lateral geniculate nucleus (LGN) 8 is shown as being active at the time at which this image was generated. At this time, the LGN was receiving information on brightness and location of the visual stimulus, originating from the rods of the retina. The LGN receives an input from the optic nerve. The LGN is active through most visual processing as can be seen from the six images of Figure 3.

The upper centre image of Figure 3 was generated by starting EIT measurement at approximately 105 milliseconds after the application of a visual stimulus. The LGN 8 is still active but at this time neurological modelling shows that information on the colour of the visual stimulus is being processed, originating from the cones of the retina. Brightness and contour information is processed in an area 9 (known as area V1), at the back of the brain. The area 9 is brighter in this image, indicating the expected activity.

The upper right image was generated by starting EIT measurement at 137 milliseconds after the application of a visual stimulus. It can be seen that activity in the area 9 has increased considerably with this part of the brain working to integrate colour stereo and texture information, ready for relay to higher brain regions. In addition, feedback information is being relayed back to the LGN 8 in order to fine tune its processing of future information. Intense activity in LGN area 8 and increased activity in V1 area 9 is indicated in this image.

The lower left image of Figure 3 was generated by starting EIT measurement at 186 milliseconds after the application of a visual stimulus. It can be seen that information is now being passed to other visual centres 10, 11 at either side of the

brain. These areas 10, 11 are responsible for colour processing and the identification of objects.

The lower centre image of Figure 3 was generated by starting EIT measurement at 201 milliseconds after the application of a visual stimulus. Large dark areas 12, 13, 14 correspond to activity in the left anterior cingulate gyrus and connected regions of the limbic system. These regions are responsible for many things, but most relevant here is the emotion accompanying the recognition of an object. These same regions 12, 13, 14 are responsible for deciding whether a noxious stimulus is actually painful. In the present circumstance, we can assume that these areas of the brain are determining information of the form "that was another flash". It is not surprising that imaging using this technique is able to directly visualise human emotions arising as a result of the sensory stimulus.

The lower right image of figure 3 was generated by starting EIT measurement at 248 milliseconds after the application of a visual stimulus. Most visual processing is complete by this stage and higher brain regions are determining the action to be taken in response to the received information. Large parts of the brain are preparing for any subsequent flash, and thus there is a need for random sequences of flashes to eliminate habituation as described above.

The described system could be used to assist in the diagnosis of a patient presenting with blindness. Possible reasons for blindness, caused for example by a blow to the head, include a detached retina or brain damage. Application of a visual stimulus to the patient and examination of an image or images of the patient's brain created using the above-described EIT technique will allow analysis of the cause of blindness. In such examination, a medical practitioner will know where in the brain activity can be expected at particular delay times after stimulus application. If any brain activity is observed, clearly the retina is not detached as signals are being sent to the brain, thus indicating that the blindness may be caused by brain damage. If however no response is observed in the brain to the stimulus, the cause could either be a detached retina, or more serious brain damage. If some brain activity is observed, images can be taken at different delay times after stimulus application, such that images created after a particular time delay do not show expected behaviour. The

medical practitioner is therefore provided with an indication of the location of the brain damage.

As a further example, if a patient presents with symptoms of a stroke, an embodiment of the present invention may be used to image brain condition. Electrodes are applied to the patient's head as illustrated in figure 1 and as described above. Stimuli are then presented to the patient and response monitored. A nerve stimulator is placed on the patient's leg, and triggered to provide a number of unequally temporally spaced stimuli; at a predetermined time after each stimulus, an EIT measurement is taken creating an image as described above.

When this imaging process is complete, an audio stimulus is provided and a series of images is again created. Similarly, a visual stimulus is provided and a number of images created. The three sets of images created, each in response to a different type of stimulus, allow a thorough assessment of brain function to be made, thus allowing evaluation of the severity of the stroke.

The imaging apparatus required for this procedure is relatively small in size, and relatively cheap to provide. Thus the apparatus may be provided to a general practitioner, allowing him to quickly and easily assess the need for a patient to be referred to a neurologist.

It will be appreciated that although in the described embodiment of the invention each set of measurements is accumulated after a respective stimulating event, all the sets of measurements could be accumulated after a single stimulating event. If the invention is to be implemented in this way, EIT techniques must be used which allow relatively fast current injection and voltage measurement so as to allow images to be captured with the required temporal resolution.

In some embodiments of the present invention, for example those concerned with diagnosing the cause of blindness, only specific parts of the brain need be imaged. By referring to a known neurological model of the brain, the specific parts of the brain that need to be imaged can be identified. Using this information, the number of current injections required can be reduced from the eight injections described with reference to Figure 2 to one or two carefully selected injections. For example, when imaging the visual pathway current may be passed between regions at the front and the back of the head. That is, injection is parallel to the visual pathway which

generally runs from the eyes to the back of the brain. If response to an auditory stimulus is to be monitored, the pathway from the ears to auditory cortex at the side of the brain needs to be monitored, and so electrodes must be placed at least at the side of the head. A parallel voltage measurement protocol may be used. This makes it possible to dramatically reduce the time taken to capture the required measurement data. In alternative embodiments, all current injections described with reference to Figure 2 may be used, but only a limited number of voltage measurements taken for each injection. Alternatively, both the injections and measurements may be selected on the basis of a neurological model and the applied stimulus.

In the described embodiments, each stimulating event is of short duration. A stimulating event could however be relatively prolonged, extending into a subsequent period during which impedance measurements are made.

It may be desired to use other stimuli occurring in the patient's environment, the application of which cannot be controlled, in place of the deliberate application of stimuli as described above. This is possible, providing accurate timing between occurrence of the stimulus and the beginning of EIT frame acquisition process is available.

The measurement data may be processed to reduce sensitivity to effects such as noise and the temporal variation of impedance within the brain during the measurement sequence. For example, a Kalman filter may be used in a conventional manner. In some embodiments of the invention, a plurality of stimulus may be applied, and a number of sets of voltage measurements collected at a particular time after application of each respective stimulus. Sets of voltage measurements collected in this way can then be averaged so as to provide greater accuracy.

CLAIMS

1. A method for monitoring the response of a nervous system of a body to a stimulus, comprising collecting a set of voltage measurements between selected areas on a surface of the body whilst current is passed between selected regions of the surface of the body, wherein the set of voltage measurements is collected over a predetermined measurement period, the predetermined measurement period is initiated a predetermined time after application of the stimulus, and the collected voltage measurements are compared with reference measurements to determine normal or abnormal response of the nervous system.
2. A method according to claim 1, wherein the set of voltage measurements is used to produce an image representing the distribution of impedance within the body.
3. A method according to claim 1 or 2, wherein the stimulus comprises a series of stimuli, a set of voltage measurements is collected during current injection periods initiated after the application of each stimulus, the collection of voltage measurements related to each stimulus is initiated at a time delayed relative to the respective stimulus, the time delay differs for each stimulus, and differences between collected sets of voltage measurements are interpreted as representing changes in nervous system activity over the time difference between the respective time delays.
4. A method according to claim 3 as dependent upon claim 2, wherein the images are compared to identify changes in nervous system activity.
5. A method according to any preceding claim, wherein the applied stimulus is a visual or an auditory stimulus.
6. A method according to any preceding claim, wherein measured voltage measurements are filtered using a Kalman filter.

7. A method according to any preceding claim, further comprising applying the stimulus.
8. A method according to any one of claims 1 to 6 wherein application of the stimulus is detected, and said detection starts computation of the said predetermined time.
9. A method according to claim 8, wherein the stimulus occurs spontaneously.
10. A method according to claim 9, wherein the stimulus is a feature of an environment in which the body is located.
11. A method for monitoring the response of a predetermined part of a nervous system of a body to an applied stimulus, comprising identifying the predetermined part of the nervous system, applying the stimulus, passing current between selected regions of a surface of the body, and collecting a set of voltage measurements between selected areas on the surface of the body whilst current is being passed, wherein the said regions and/or areas are selected on the basis of a neurological model of the nervous system and the applied stimulus such that sensitivity of the derived impedance measurements to changes in the predetermined part of the nervous system is maximised.
12. A method according to claim 11, wherein the derived impedance measurements are compared with reference measurements to determine normal or abnormal response of the nervous system.
13. A method according to claim 11 or 12, wherein the stimulus is a visual or auditory stimulus.
14. A method according to any one of claims 1 to 10, used in combination with a method according to any one of claims 11 to 13.

15. An apparatus for monitoring the response of a nervous system of a body to an applied stimulus comprising means for applying the stimulus to the body, and means for collecting a set of voltage measurements between selected areas on a surface of the body whilst current is being passed between selected regions of the surface of the body, wherein the set of voltage measurements is collected over a predetermined measurement period, the predetermined measurement period is initiated at a predetermined time after application of the stimulus, and means are provided to compare the collected voltage measurements with reference measurements to determine normal or abnormal response of the nervous system.

16. An apparatus for monitoring the response of a predetermined part of a nervous system of a body to an applied stimulus, comprising means for applying the stimulus, means for passing current between selected regions of the surface of the body, and means for collecting a set of voltage measurements between selected areas on the surface of the body whilst current is being passed, wherein the said regions and/or areas are selected on the basis of a neurological model of the nervous system and the applied stimulus such that the sensitivity of the derived impedance measurements to changes in the predetermined part of the nervous system is maximised.

17. A method of diagnosing a brain dysfunction, comprising applying a stimulus to a patient, and collecting a set of voltage measurements between selected areas on a surface of the patient's head while current is being passed between selected regions of the surface of the body, wherein the set of voltage measurements is collected over a predetermined measurement period, the predetermined measurement period is initiated at a predetermined time after application of the stimulus, and the collected voltage measurements are compared with reference measurements to determine normal or abnormal response of the nervous system.

18. A data carrier carrying computer program code means to cause a computer to execute procedure in accordance with the method of any one of claims 1 to 14.

19. A computer apparatus comprising:

a memory for storing processor readable instructions;
a processor for reading and executing instructions from said memory;
wherein said memory comprises instructions to cause the processor to execute the method of any one of claims 1 to 14.

20. A method substantially as herein fore described with reference to the accompanying drawings.

21. An apparatus substantially as hereinbefore described with reference to the accompanying drawings.

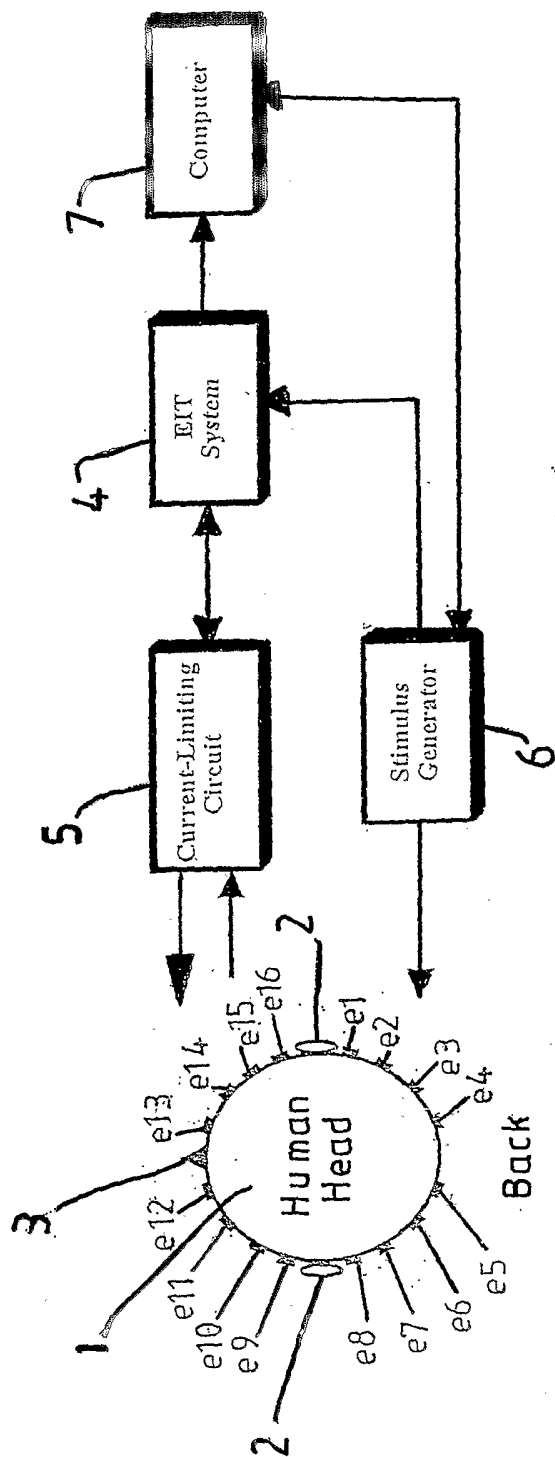


FIG. 1

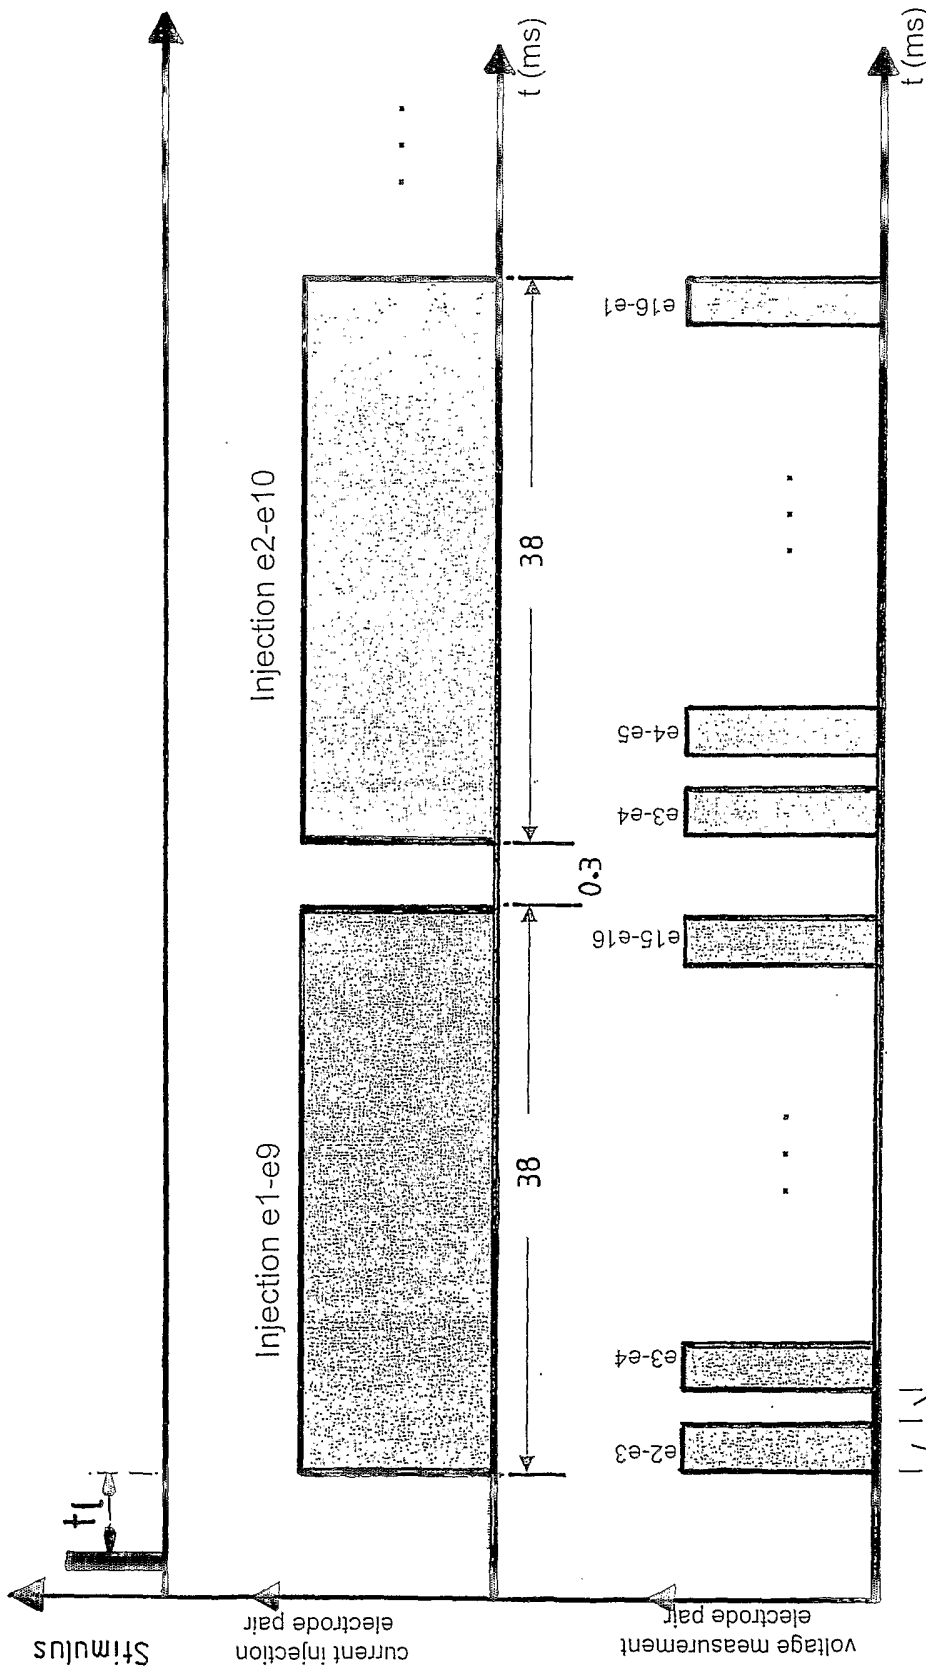


FIG. 2

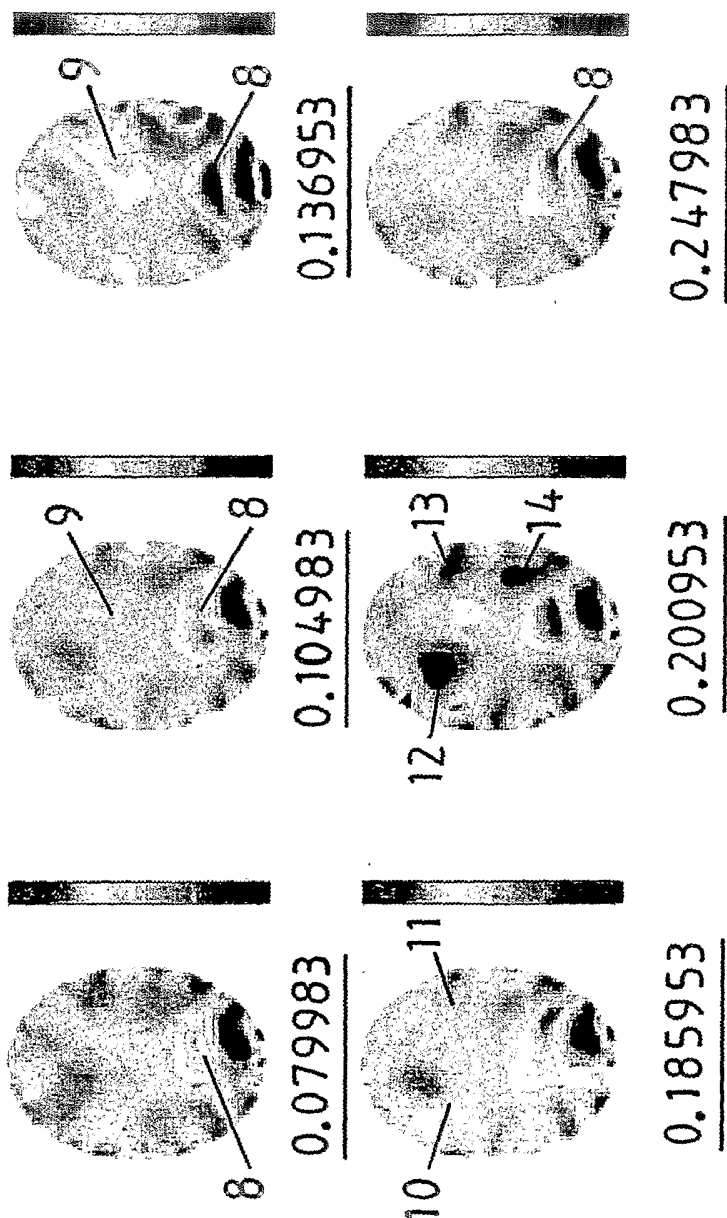


FIG. 3

INTERNATIONAL SEARCH REPORT

PCT/GB2004/001565

A. CLASSIFICATION OF SUBJECT MATTER
 IPC 7 A61B5/0484 A61B5/04

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
 IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data, PAJ

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5 143 081 A (YOUNG WISE ET AL) 1 September 1992 (1992-09-01) column 1, line 30 -column 20, line 26; figure 8	15, 16
X	US 2003/009111 A1 (CORY JOAN M ET AL) 9 January 2003 (2003-01-09) paragraph '0002! - paragraph '0070!; figures 1,2,6	15, 16
A	DE 101 04 153 A (SIEMENS AUDIOLOGISCHE TECHNIK) 6 June 2002 (2002-06-06) paragraph '0009! - paragraph '0023! -/--	15, 16

Further documents are listed in the continuation of box C.

Patent family members are listed in annex.

° Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- "&" document member of the same patent family

Date of the actual completion of the international search

28 July 2004

Date of mailing of the international search report

06/08/2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
 NL - 2280 HV Rijswijk
 Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
 Fax: (+31-70) 340-3016

Authorized officer

Kurze, V

INTERNATIONAL SEARCH REPORT

PCT/GB2004/001565

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 919 142 A (BOONE KEVIN GRAHAM ET AL) 6 July 1999 (1999-07-06) cited in the application column 2, line 65 -column 7, line 59; figure 1 -----	15,16
A	HOLDER D S: "IMPEDANCE CHANGES DURING THE COMPOUND NERVE ACTION POTENTIAL: IMPLICATIONS FOR IMPEDANCE IMAGING OF NEURONAL DEPOLARISATION IN THE BRAIN" MEDICAL AND BIOLOGICAL ENGINEERING AND COMPUTING, PETER PEREGRINUS LTD. STEVENAGE, GB, vol. 30, no. 2, 1 March 1992 (1992-03-01), pages 140-146, XP000271685 ISSN: 0140-0118 the whole document -----	15,16

INTERNATIONAL SEARCH REPORT

PCT/GB2004/001565

Box II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. Claims Nos.: 1-14, 17
because they relate to subject matter not required to be searched by this Authority, namely:
see FURTHER INFORMATION sheet PCT/ISA/210

2. Claims Nos.: 18-21
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
see FURTHER INFORMATION sheet PCT/ISA/210

3. Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.

2. As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.

3. As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:

4. No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- The additional search fees were accompanied by the applicant's protest.
- No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

Continuation of Box II.1

Claims Nos.: 1-14,17

Rule 39.1(iv) PCT - Diagnostic method practised on the human or animal body: The claimed methods encompass the steps of data collection (voltage measurements), the comparison with reference measurements and a deductive step for diagnosis (determine normal or abnormal response of the nervous system). Therefore, these methods are considered to constitute a diagnostic method in the sense of Rule 39.1(iv) PCT.

Continuation of Box II.2

Claims Nos.: 18-21

Claims 18 and 19: The claimed subject-matter (data carrier or computer) is defined merely by certain method steps. Because there are no apparatus features defined within these claims which enable the device to carry out the method steps, it is unclear (Article 6 PCT) which apparatus features might be involved. Therefore, these claims are so unclear that a meaningful search cannot be carried out (Article 17(2)(a)(ii) PCT).
Claims 20 and 21: The claims may not rely on references to the description and drawings (Rule 6.2(a) PCT), because such references render the claims unclear as to which method steps or apparatus features are meant (Article 6 PCT). Therefore a meaningful search of these claims is impossible (Article 17(2)(a)(ii) PCT).

The applicant's attention is drawn to the fact that claims, or parts of claims, relating to inventions in respect of which no international search report has been established need not be the subject of an international preliminary examination (Rule 66.1(e) PCT). The applicant is advised that the EPO policy when acting as an International Preliminary Examining Authority is normally not to carry out a preliminary examination on matter which has not been searched. This is the case irrespective of whether or not the claims are amended following receipt of the search report or during any Chapter II procedure.

INTERNATIONAL SEARCH REPORT

Information on patent family members

PCT/GB2004/001565

Patent document cited in search report	A	Publication date	Patent family member(s)	Publication date
US 5143081	A	01-09-1992	NONE	
US 2003009111	A1	09-01-2003	CA 2449567 A1 EP 1401332 A2 WO 02100247 A2	19-12-2002 31-03-2004 19-12-2002
DE 10104153	A	06-06-2002	DE 10104153 A1	06-06-2002
US 5919142	A	06-07-1999	DE 69603729 D1 DE 69603729 T2 EP 0833585 A1 WO 9700642 A1 JP 11507858 T	16-09-1999 27-01-2000 08-04-1998 09-01-1997 13-07-1999