



US007201762B2

(12) **United States Patent**  
**Greene, Jr. et al.**

(10) **Patent No.:** **US 7,201,762 B2**  
(45) **Date of Patent:** **\*Apr. 10, 2007**

(54) **VASCULAR EMBOLIZATION WITH AN EXPANSIBLE IMPLANT**

FOREIGN PATENT DOCUMENTS

WO WO 89/11257 11/1989

(Continued)

(75) Inventors: **George R. Greene, Jr.**, Costa Mesa, CA (US); **Robert F. Rosenbluth**, Laguna Nigel, CA (US); **Brian J. Cox**, Laguna Nigel, CA (US)

OTHER PUBLICATIONS

Radiology "eMOBOLIZATION with rAIOOPAQUE Microbeads of Polyacrylonitrile Hydrogel: Evaluation in Swine" Y. Pierre gobin.\*

(73) Assignee: **Microvention, Inc.**, Aliso Viejo, CA (US)

(Continued)

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

*Primary Examiner*—Suzette J. Gherbi  
(74) *Attorney, Agent, or Firm*—Klein, O'Neill & Singh, LLP; Howard J. Klein

This patent is subject to a terminal disclaimer.

(57) **ABSTRACT**

(21) Appl. No.: **10/320,033**

A vascular implant formed of a compressible foam material has a compressed configuration from which it is expansible into a configuration substantially conforming to the shape and size of a vascular site to be embolized. Preferably, the implant is formed of a hydrophilic, macroporous foam material, having an initial configuration of a scaled-down model of the vascular site, from which it is compressible into the compressed configuration. The implant is made by scanning the vascular site to create a digitized scan data set; using the scan data set to create a three-dimensional digitized virtual model of the vascular site; using the virtual model to create a scaled-down physical mold of the vascular site; and using the mold to create a vascular implant in the form of a scaled-down model of the vascular site. To embolize a vascular site, the implant is compressed and passed through a microcatheter, the distal end of which has been passed into a vascular site. Upon entering the vascular site, the implant expands in situ substantially to fill the vascular site. A retention element is contained within the microcatheter and has a distal end detachably connected to the implant. A flexible, tubular deployment element is used to pass the implant and the retention element through the microcatheter, and then to separate the implant from the retention element when the implant has been passed out of the microcatheter and into the vascular site.

(22) Filed: **Dec. 16, 2002**

(65) **Prior Publication Data**

US 2003/0088311 A1 May 8, 2003

**Related U.S. Application Data**

(63) Continuation of application No. 09/730,071, filed on Dec. 5, 2000, now Pat. No. 6,500,190, which is a continuation of application No. 09/110,816, filed on Jul. 6, 1998, now Pat. No. 6,165,193.

(51) **Int. Cl.**  
*A61B 19/00* (2006.01)  
*A61F 2/06* (2006.01)

(52) **U.S. Cl.** ..... **606/191**; 623/903

(58) **Field of Classification Search** ..... 623/11.11, 623/1.4, 1.39, 1.21, 1.11; 606/191  
See application file for complete search history.


(56) **References Cited**

U.S. PATENT DOCUMENTS

3,709,842 A 1/1973 SToy et al.

(Continued)

**15 Claims, 3 Drawing Sheets**

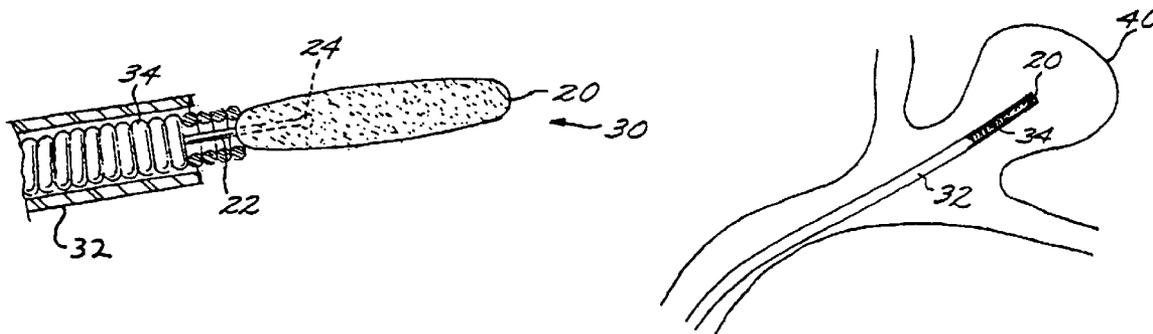

U.S. PATENT DOCUMENTS

4,365,621 A 12/1982 Brundin  
 4,436,684 A 3/1984 White  
 4,506,393 A 3/1985 Murphy  
 4,509,504 A 4/1985 Brundin  
 4,529,739 A 7/1985 Scott et al.  
 4,551,132 A 11/1985 Pasztor et al.  
 4,663,358 A 5/1987 Hyon et al.  
 4,673,539 A \* 6/1987 Hammar et al. .... 264/1.1  
 4,795,741 A 1/1989 Leschiner et al.  
 4,819,637 A 4/1989 Dormandy, Jr. et al.  
 4,873,707 A 10/1989 Robertson  
 4,940,412 A 7/1990 Blumenthal  
 4,994,069 A 2/1991 Ritchart et al.  
 5,007,936 A 4/1991 Woolson  
 5,133,731 A 7/1992 Butler et al.  
 5,156,777 A 10/1992 Kaye  
 5,184,306 A 2/1993 Erdman et al.  
 5,226,911 A 7/1993 Chee et al.  
 5,258,042 A 11/1993 Mehta  
 5,274,565 A 12/1993 Reuben  
 5,312,415 A 5/1994 Palermo  
 5,320,639 A 6/1994 Rudnick  
 5,350,397 A 9/1994 Palermo et al.  
 5,354,290 A 10/1994 Gross  
 5,360,446 A 11/1994 Kennedy  
 5,365,996 A 11/1994 Crook  
 5,382,259 A 1/1995 Phelps et al.  
 5,382,260 A 1/1995 Dormandy, Jr. et al.  
 5,448,489 A 9/1995 Reuben  
 5,452,407 A 9/1995 Crook  
 5,456,693 A 10/1995 Conston et al.  
 5,460,621 A \* 10/1995 Gertzman et al. .... 604/358  
 5,476,472 A 12/1995 Dormandy, Jr. et al.  
 5,525,334 A 6/1996 Ito et al.  
 5,541,234 A \* 7/1996 Unger et al. .... 521/66  
 5,573,994 A 11/1996 Kabra et al.  
 5,578,074 A 11/1996 Mirigian  
 5,580,568 A 12/1996 Greff et al.  
 5,582,619 A 12/1996 Ken  
 5,624,461 A 4/1997 Mariant  
 5,624,685 A 4/1997 Takahashi et al.  
 5,645,558 A 7/1997 Horton  
 5,658,308 A 8/1997 Snyder  
 5,718,711 A 2/1998 Berenstein et al.  
 5,738,667 A \* 4/1998 Solar ..... 604/523  
 5,750,585 A \* 5/1998 Park et al. .... 521/143  
 5,752,974 A 5/1998 Rhee et al.  
 5,762,125 A 6/1998 Mastrorio  
 5,823,198 A \* 10/1998 Jones et al. .... 128/899  
 5,826,587 A 10/1998 Berenstein et al.  
 5,911,731 A 6/1999 Pham et al.  
 5,916,235 A \* 6/1999 Guglielmi ..... 606/200

5,935,148 A 8/1999 Villar et al.  
 5,957,948 A 9/1999 Mariant  
 6,015,424 A \* 1/2000 Rosenbluth et al. .... 606/200  
 6,063,070 A \* 5/2000 Eder ..... 606/1  
 6,066,325 A \* 5/2000 Wallace et al. .... 424/400  
 6,096,034 A \* 8/2000 Kupiecki et al. .... 606/32  
 6,113,629 A 9/2000 Ken  
 6,177,095 B1 \* 1/2001 Sawhney et al. .... 424/426  
 6,299,619 B1 \* 10/2001 Greene et al. .... 606/108  
 6,383,174 B1 \* 5/2002 Eder ..... 606/1  
 6,463,317 B1 \* 10/2002 Kucharczyk et al. .... 600/411  
 6,605,294 B2 \* 8/2003 Sawhney ..... 424/426  
 2003/0134032 A1 \* 7/2003 Chaouk et al. .... 427/2.24

FOREIGN PATENT DOCUMENTS

WO WO 97/26939 7/1997  
 WO WO 98/16266 4/1998  
 WO WO 99/23954 5/1999  
 WO WO 99/56783 11/1999

OTHER PUBLICATIONS

Hawley's Twelfth Editin condensed chemical dictionary pp. 351-352.\*  
 Chirila, Traian et al.; "Poly[2-hydroxyethyl methacrylate]. . ." Biomaterials 1993, vol. 14, No. 1.  
 Horak, Daniel et al.; "Hydrogels in endovascular embolizatin . . ." Biomateroals 1986, vol. 7 November.  
 Horak, D. et al.; "New radiopaque poly-HEMA-based hydrogel particles Journal of Biomedical Materials Research vol. 34, 183-188 (1997).  
 Latchaw, richard E. et al.; "Polyvinyl Foam Embolization of Vascular . . ." Radiology 131:669-678, Jun. 1979.  
 Chithambara Thanoo, B. et al.; "Radiopaque hydrogel microspheres" J. Microencapsulation, 1989, vol. 6, No. 2, 233-244.  
 McGurk, M. et al.; "Rajid prototyping techniques for anatomical modeling in medicine" Ann R Coll Surg Engl 1997; 79:169-174.  
 Rao, Vrk et al.; "Hydrolyzed mCrospheres from cross-linked . . ." J. Neurodiol, 1991, 18, 61-69.  
 Robertson, Douglas D. et al.; "Design of Custom Hip Stem Prostheses . . ." Journal of Computer Assisted Tomography 11(5):804-809 Sep./Oct. 1987.  
 McPherson, David D.; "Three-Dimensional Arterial Imaging" Scientific American, Science and Medicine March/April pp. 22-33.  
 MacDonald, Warren et al.; "Designing an Implant by CT Scanning and solid Modeling" Journal of Bone and Joint Surgery vol. 68-B, No. 2, Mar. 1986, pp. 208-212.  
 Wake, Conley M. et al.; "Dynamic of Fibrovascular Tissue . . ." Cell Transplantation, vol. 4, No. 3, pp. 275-279 1995.  
 Woerly, S. et al.; "Intracerebral implantation of synthetic . . ." Biomaterials Mar. 1990; 11(2): 97-107.

\* cited by examiner

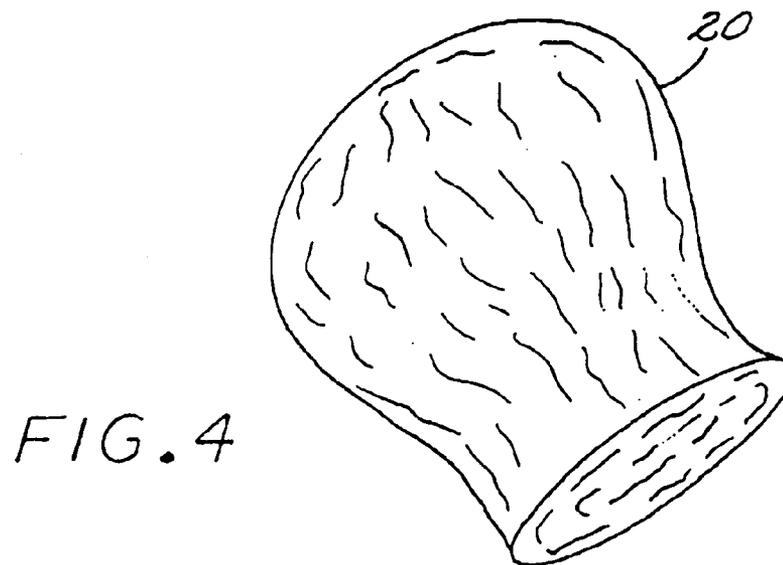


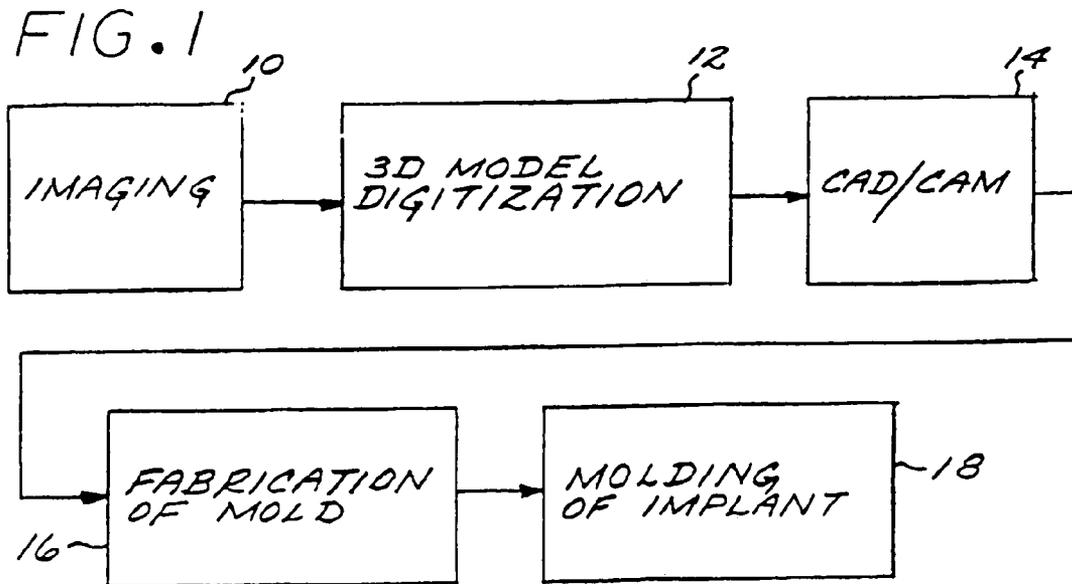


FIG. 5

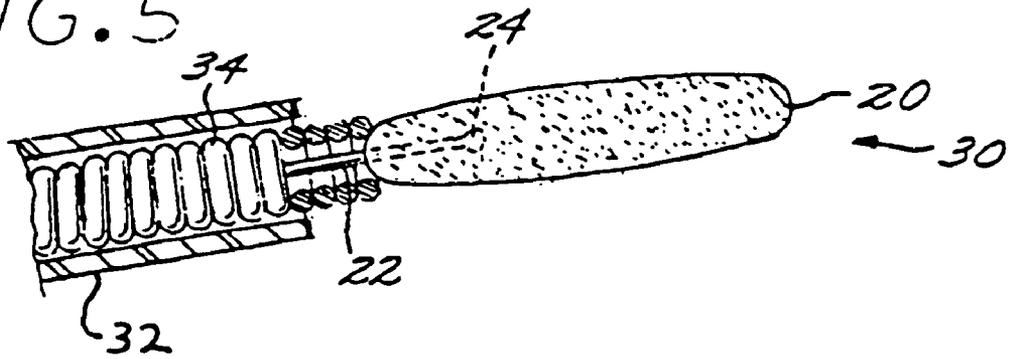


FIG. 6

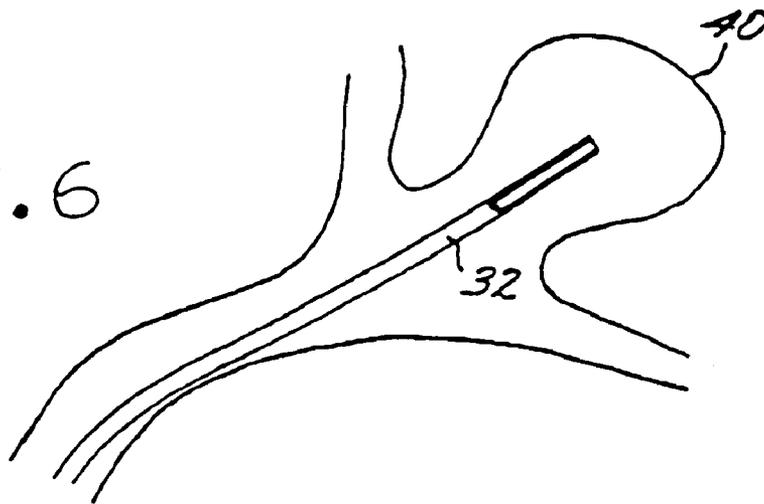


FIG. 7

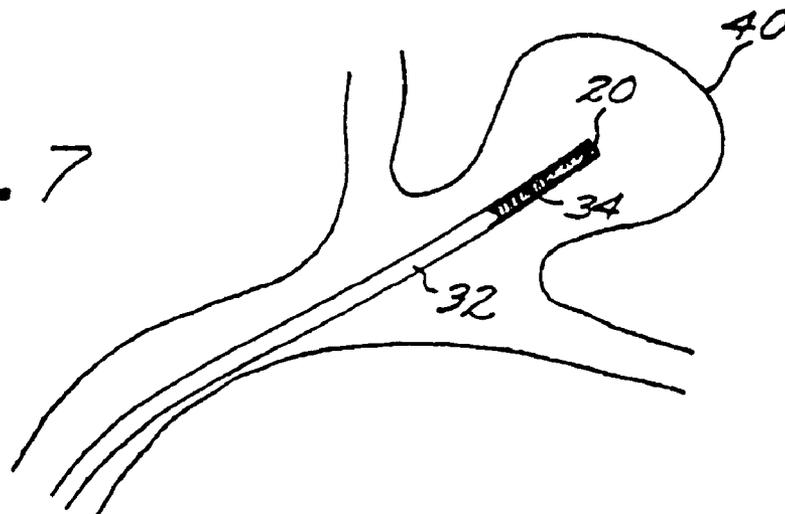


FIG. 8

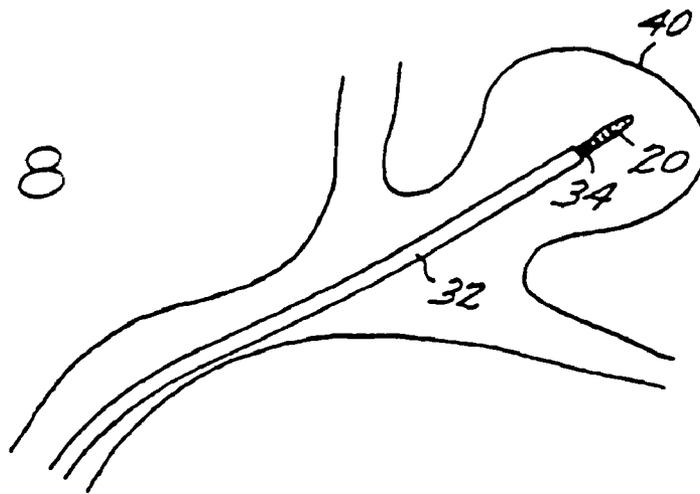


FIG. 9


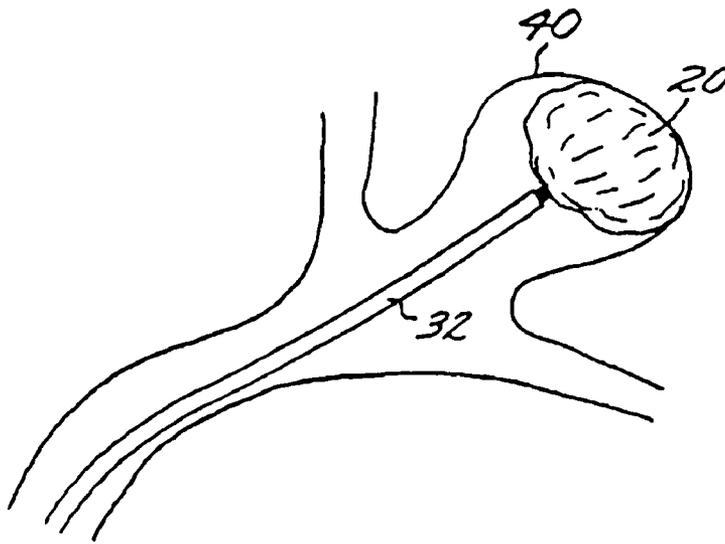


FIG. 10

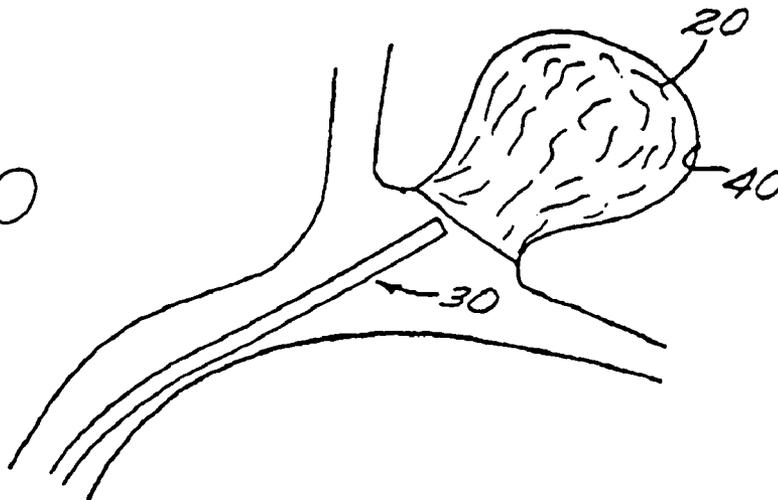

## VASCULAR EMBOLIZATION WITH AN EXPANSIBLE IMPLANT

### CROSS REFERENCE TO RELATED APPLICATION

This application is a Continuation of application Ser. No. 09/730,071; filed Dec. 5, 2000 now U.S. Pat. No. 6,500,190, which is a Continuation of application Ser. No. 09/110,816; filed Jul. 6, 1998, now U.S. Pat. No. 6,165,193.

### FEDERALLY SPONSORED RESEARCH OR DEVELOPMENT

Not applicable

### BACKGROUND OF THE INVENTION

The present invention relates to the field of methods and devices for the embolization of vascular aneurysms and similar vascular abnormalities. More specifically, the present invention relates to (a) an expansible vascular implant that is inserted into a vascular site such as an aneurysm to create an embolism therein; (b) a method of making the expansible implant; and (c) a method and an apparatus for embolizing a vascular site using the implant.

The embolization of blood vessels is desired in a number of clinical situations. For example, vascular embolization has been used to control vascular bleeding, to occlude the blood supply to tumors, and to occlude vascular aneurysms, particularly intracranial aneurysms. In recent years, vascular embolization for the treatment of aneurysms has received much attention. Several different treatment modalities have been employed in the prior art. U.S. Pat. No. 4,819,637—Dormandy, Jr. et al., for example, describes a vascular embolization system that employs a detachable balloon delivered to the aneurysm site by an intravascular catheter. The balloon is carried into the aneurysm at the tip of the catheter, and it is inflated inside the aneurysm with a solidifying fluid (typically a polymerizable resin or gel) to occlude the aneurysm. The balloon is then detached from the catheter by gentle traction on the catheter. While the balloon-type embolization device can provide an effective occlusion of many types of aneurysms, it is difficult to retrieve or move after the solidifying fluid sets, and it is difficult to visualize unless it is filled with a contrast material. Furthermore, there are risks of balloon rupture during inflation and of premature detachment of the balloon from the catheter.

Another approach is the direct injection of a liquid polymer embolic agent into the vascular site to be occluded. One type of liquid polymer used in the direct injection technique is a rapidly polymerizing liquid, such as a cyanoacrylate resin, particularly isobutyl cyanoacrylate, that is delivered to the target site as a liquid, and then is polymerized in situ. Alternatively, a liquid polymer that is precipitated at the target site from a carrier solution has been used. An example of this type of embolic agent is a cellulose acetate polymer mixed with bismuth trioxide and dissolved in dimethyl sulfoxide (DMSO). Another type is ethylene glycol copolymer dissolved in DMSO. On contact with blood, the DMSO diffuses out, and the polymer precipitates out and rapidly hardens into an embolic mass that conforms to the shape of the aneurysm. Other examples of materials used in this "direct injection" method are disclosed in the following U.S. Pat. No. 4,551,132—Pásztor et al.; U.S. Pat.

No. 4,795,741—Leshchiner et al.; U.S. Pat. No. 5,525,334—Ito et al.; and U.S. Pat. No. 5,580,568—Greff et al.

The direct injection of liquid polymer embolic agents has proven difficult in practice. For example, migration of the polymeric material from the aneurysm and into the adjacent blood vessel has presented a problem. In addition, visualization of the embolization material requires that a contrasting agent be mixed with it, and selecting embolization materials and contrasting agents that are mutually compatible may result in performance compromises that are less than optimal. Furthermore, precise control of the deployment of the polymeric embolization material is difficult, leading to the risk of improper placement and/or premature solidification of the material. Moreover, once the embolization material is deployed and solidified, it is difficult to move or retrieve.

Another approach that has shown promise is the use of thrombogenic microcoils. These microcoils may be made of a biocompatible metal alloy (typically platinum and tungsten) or a suitable polymer. If made of metal, the coil may be provided with Dacron fibers to increase thrombogenicity. The coil is deployed through a microcatheter to the vascular site. Examples of microcoils are disclosed in the following U.S. Pat. No. 4,994,069—Ritchart et al.; U.S. Pat. No. 5,133,731—Butler et al.; U.S. Pat. No. 5,226,911—Chee et al.; U.S. Pat. No. 5,312,415—Palermo; U.S. Pat. No. 5,382,259—Phelps et al.; U.S. Pat. No. 5,382,260—Dormandy, Jr. et al.; U.S. Pat. No. 5,476,472—Dormandy, Jr. et al.; U.S. Pat. No. 5,578,074—Mirigian; U.S. Pat. No. 5,582,619—Ken; U.S. Pat. No. 5,624,461—Mariant; U.S. Pat. No. 5,645,558—Horton; U.S. Pat. No. 5,658,308—Snyder; and U.S. Pat. No. 5,718,711—Berenstein et al.

The microcoil approach has met with some success in treating small aneurysms with narrow necks, but the coil must be tightly packed into the aneurysm to avoid shifting that can lead to recanalization. Microcoils have been less successful in the treatment of larger aneurysms, especially those with relatively wide necks. A disadvantage of microcoils is that they are not easily retrievable; if a coil migrates out of the aneurysm, a second procedure to retrieve it and move it back into place is necessary. Furthermore, complete packing of an aneurysm using microcoils can be difficult to achieve in practice.

A specific type of microcoil that has achieved a measure of success is the Guglielmi Detachable Coil ("GDC"). The GDC employs a platinum wire coil fixed to a stainless steel guidewire by a solder connection. After the coil is placed inside an aneurysm, an electrical current is applied to the guidewire, which heats sufficiently to melt the solder junction, thereby detaching the coil from the guidewire. The application of the current also creates a positive electrical charge on the coil, which attracts negatively-charged blood cells, platelets, and fibrinogen, thereby increasing the thrombogenicity of the coil. Several coils of different diameters and lengths can be packed into an aneurysm until the aneurysm is completely filled. The coils thus create and hold a thrombus within the aneurysm, inhibiting its displacement and its fragmentation.

The advantages of the GDC procedure are the ability to withdraw and relocate the coil if it migrates from its desired location, and the enhanced ability to promote the formation of a stable thrombus within the aneurysm. Nevertheless, as in conventional microcoil techniques, the successful use of the GDC procedure has been substantially limited to small aneurysms with narrow necks.

Still another approach to the embolization of an abnormal vascular site is the injection into the site of a biocompatible

hydrogel, such as poly (2-hydroxyethyl methacrylate) (“pHEMA” or “PHEMA”); or a polyvinyl alcohol foam (“PAF”). See, e.g., Horák et al., “Hydrogels in Endovascular Embolization. II. Clinical Use of Spherical Particles”, *Bio-materials*, Vol. 7, pp. 467–470 (November, 1986); Rao et al., “Hydrolysed Microspheres from Cross-Linked Polymethyl Methacrylate”, *J. Neuroradiol.*, Vol. 18, pp. 61–69 (1991); Latchaw et al., “Polyvinyl Foam Embolization of Vascular and Neoplastic Lesions of the Head, Neck, and Spine”, *Radiology*, Vol. 131, pp. 669–679 (June, 1979). These materials are delivered as microparticles in a carrier fluid that is injected into the vascular site, a process that has proven difficult to control.

A further development has been the formulation of the hydrogel materials into a preformed implant or plug that is installed in the vascular site by means such as a microcatheter. See, e.g., U.S. Pat. No. 5,258,042—Mehta and U.S. Pat. No. 5,456,693—Conston et al. These types of plugs or implants are primarily designed for obstructing blood flow through a tubular vessel or the neck of an aneurysm, and they are not easily adapted for precise implantation within a sack-shaped vascular structure, such as an aneurysm, so as to fill substantially the entire volume of the structure.

There has thus been a long-felt, but as yet unsatisfied need for an aneurysm treatment device and method that can substantially fill aneurysms of a large range of sizes, configurations, and neck widths with a thrombogenic medium with a minimal risk of inadvertent aneurysm rupture or blood vessel wall damage. There has been a further need for such a method and device that also allow for the precise locational deployment of the medium, while also minimizing the potential for migration away from the target location. In addition, a method and device meeting these criteria should also be relatively easy to use in a clinical setting. Such ease of use, for example, should preferably include a provision for good visualization of the device during and after deployment in an aneurysm.

#### SUMMARY OF THE INVENTION

Broadly, a first aspect of the present invention is a device for occluding a vascular site, such as an aneurysm, comprising a conformal vascular implant, formed of an expansible material, that is compressible from an initial configuration for insertion into the vascular site by means such as a microcatheter while the implant is in a compressed configuration, and that is expansible in situ into an expanded configuration in which it substantially fills the vascular site, thereby to embolize the site, wherein the initial configuration of the implant is a scaled-down model of the vascular site.

In a preferred embodiment, the implant is made of a hydrophilic, macroporous, polymeric, hydrogel foam material, in particular a water-swallowable foam matrix formed as a macroporous solid comprising a foam stabilizing agent and a polymer or copolymer of a free radical polymerizable hydrophilic olefin monomer cross-linked with up to about 10% by weight of a multiolefin-functional cross-linking agent. The material is modified, or contains additives, to make the implant visible by conventional imaging techniques.

Another aspect of the present invention is a method of manufacturing a vascular implant, comprising the steps of: (a) imaging a vascular site by scanning the vascular site to create a digitized scan data set; (b) using the scan data set to create a three-dimensional digitized virtual model of the vascular site; and (c) forming a vascular implant device in

the form of a physical model of the vascular site, using the virtual model, the implant being formed of a compressible and expansible biocompatible foam material. In a specific embodiment, the forming step (c) comprises the substeps of: (c)(1) using the virtual model to create a scaled-down, three-dimensional physical mold of the vascular site; and (c)(2) using the mold to create a vascular implant in the form of a scaled-down physical model of the vascular site.

In the preferred embodiment of the method of manufacturing the implant, the imaging step is performed with a scanning technique such as computer tomography (commonly called “CT” or “CAT”), magnetic resonance imaging (MRI), magnetic resonance angiography (MRA), or ultrasound. Commercially-available software, typically packaged with and employed by the scanning apparatus, reconstructs the scan data set created by the imaging into the three-dimensional digitized model of the vascular site. The digitized model is then translated, by commercially-available software, into a form that is useable in a commercially available CAD/CAM program to create the scaled-down physical mold by means of stereolithography. A suitable implant material, preferably a macroporous hydrogel foam material, is injected in a liquid or semiliquid state into the mold. Once solidified, the hydrogel foam material is removed from the mold as an implant in the form of a scaled-down physical model of the vascular site.

A third aspect of the present invention is a method for embolizing a vascular site, comprising the steps of: (a) passing a microcatheter intravascularly so that its distal end is in a vascular site; (b) providing a vascular implant in the form of a scaled-down physical model of the vascular site, the implant being formed of a compressible and expansible biocompatible foam material; (c) compressing the implant into a compressed configuration dimensioned to pass through a microcatheter; (d) passing the implant, while it is in its compressed configuration, through the microcatheter so that the implant emerges from the distal end of the microcatheter into the vascular site; and (e) expanding the implant in situ substantially to fill the vascular site.

The apparatus employed in the embolization method comprises an elongate, flexible deployment element dimensioned to fit axially within an intravascular microcatheter; a filamentous implant retention element disposed axially through the deployment element from its proximal end to its distal end; and an implant device removably attached to the distal end of the retention element.

The implant device, in its preferred embodiment, is formed of a moldable, hydrophilically expansible, biocompatible foam material that has an initial configuration in the form of a scaled-down physical model of the vascular site, that is compressible into a compressed configuration that fits within the microcatheter, and that is hydrophilically expansible into an expanded configuration in which it is dimensioned substantially to conform to and fill the vascular site. Alternatively, the implant device may be formed of a non-hydrophilic foam material having an initial configuration that is substantially the same size and shape as the vascular site, and that restores itself to its initial configuration after it is released from its compressed configuration.

The retention element is preferably a flexible wire having a distal end configured to releasably engage the implant device while the implant device is in its compressed configuration, thus to retain the implant device within the distal end of the microcatheter while the distal end of the microcatheter is inserted into the vascular site. The wire is movable axially with the deployment element in the distal direction to expose the implant from the distal end of the

microcatheter, and is movable proximally with respect to the deployment element to urge the implant device against the distal end of the deployment element, thereby push the implant device off of the wire. Thus released into the vascular site, the implant device expands into an expanded configuration in which it substantially conforms to and fills the vascular site.

The present invention provides a number of significant advantages. Specifically, the present invention provides an effective vascular embolization implant that can be deployed within a vascular site with excellent locational control, and with a lower risk of vascular rupture, tissue damage, or migration than with prior art implant devices. Furthermore, the implant device, by being modelled on the actual vascular site in which it is to be implanted, effects a conformal fit within the site that promotes effective embolization, and yet its ability to be delivered to the site in a highly compressed configuration facilitates precise and highly controllable deployment with a microcatheter. In addition, the method of fabricating the implant device, by modeling it on each individual site, allows implant devices to be made that can effectively embolize vascular sites having a wide variety of sizes, configurations, and (in the particular case of aneurysms) neck widths. These and other advantages will be readily appreciated from the detailed description that follows.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a flow chart showing a method of manufacturing a vascular implant in accordance with a preferred embodiment of the manufacturing method aspect of the present invention;

FIG. 2 is a perspective view of a vascular implant in accordance with a preferred embodiment of the vascular implant device aspect of the present invention, showing the implant in its initial configuration;

FIG. 3 is an elevational view of the implant of FIG. 2, showing the implant in its compressed configuration;

FIG. 4 is a perspective view of the implant of FIG. 2, showing the implant in its expanded configuration;

FIG. 5 is a cross-sectional view of an implanting apparatus employed in a method of embolizing a vascular site in accordance with a preferred embodiment of the embolizing method aspect of the present invention; and

FIGS. 6 through 10 are semischematic views showing the steps in a method of embolizing a vascular site (specifically, an aneurysm) in accordance with a preferred embodiment of the embolizing method aspect of the present invention.

#### DETAILED DESCRIPTION OF THE INVENTION

##### The Method of Manufacturing a Vascular Implant.

A first aspect of the present invention is a method of manufacturing a vascular implant device. The steps of a preferred embodiment of the manufacturing method are shown as a sequence of descriptive boxes in the flow chart of FIG. 1.

The first step, shown in box 10 of FIG. 1, is the step of creating an image of a vascular site, such as an aneurysm, in which an embolizing implant is to be installed. This imaging step is performed by scanning the site using any of several conventional imaging techniques, such as computer tomography, magnetic resonance imaging (MRI), magnetic resonance angiography (MRA), or ultrasound.

The result of the imaging step is a digitized scan data set that is stored in a computer memory, from which the data set is retrieved for operation of the next step: computerized reconstruction of a three-dimensional digitized virtual model of the vascular site (box 12 of FIG. 1). This step of creating a three-dimensional digital model is typically performed by software designed for this purpose that is packaged with and employed by the imaging apparatus.

The digitized, three-dimensional virtual model is then translated into a form in which it can be employed in a commercially-available CAD/CAM program (box 14) which controls a stereolithography process (box 16) to create a mold for forming an implant device. The translation of the virtual model is performed by software that is commercially available, for example, from Cyberform International, Inc., of Richardson, Tex., and from Stratasys, Inc., of Minneapolis, Minn. The mold (not shown) is preferably scaled-down from the dimensions of the vascular site, with a scale of about 1:2 to about 1:6, with about 1:4 being preferred. Alternatively, the mold may be made "life size" (i.e., 1:1); that is, a full-size or nearly full-size replica of the vascular site. The mold is used in the fabrication of a vascular implant device by conventional molding techniques (box 18).

##### The Implant Device.

A vascular implant device 20, in accordance with the present invention, is shown in FIG. 2 as it appears in its uncompressed or precompressed initial configuration after withdrawal from the mold. Preferably, the implant device 20 is molded directly onto the distal end portion of an elongate, flexible, filamentous retention element, such as a retention wire 22, for purposes to be described below. The retention wire 22 preferably has a distal end that terminates in a knob 24 (FIG. 5) for better retention of the implant device 20 thereon.

In the preferred embodiment, the implant device 20 is made of a biocompatible, macroporous, hydrophilic hydrogel foam material, in particular a water-swelling foam matrix formed as a macroporous solid comprising a foam stabilizing agent and a polymer or copolymer of a free radical polymerizable hydrophilic olefin monomer cross-linked with up to about 10% by weight of a multiolefin-functional cross-linking agent. A suitable material of this type is described in U.S. Pat. No. 5,570,585—Park et al., the disclosure of which is incorporated herein by reference. Another suitable material is a porous hydrated polyvinyl alcohol foam (PAF) gel prepared from a polyvinyl alcohol solution in a mixed solvent consisting of water and a water-miscible organic solvent, as described, for example, in U.S. Pat. No. 4,663,358—Hyon et al., the disclosure of which is incorporated herein by reference. Still another suitable material is PHEMA, as discussed in the references cited above. See, e.g., Horák et al., supra, and Rao et al., supra. The foam material preferably has a void ratio of at least about 90%, and its hydrophilic properties are such that it has a water content of at least about 90% when fully hydrated.

In a preferred embodiment, the implant device 20, in its initial, precompressed configuration, will have the same configuration as the vascular site, but it will be smaller, by a factor of approximately two to approximately six. The material of the implant device 20, and its initial size, are selected so that the implant device 20 is swellable or expandable to approximately the size of the vascular site, primarily by the hydrophilic absorption of water molecules from blood plasma, and secondarily by the filling of its pores with blood. The result is an expanded configuration for the

implant device **20**, as shown in FIG. **4**, that is large enough substantially to fill the vascular site.

Alternatively, the implant **20** device can be molded so that in its initial, precompressed configuration, it is “life size”, i.e., approximately the same size as the vascular site. In this case, the preferred material is a compressible, non-hydrophilic polymeric foam material, such as polyurethane. In actual clinical practice, a non-hydrophilic implant device **20** would advantageously be made slightly smaller than actual life size, to accommodate swelling due to the filling of the pores.

The foam material of the implant device **20**, whether hydrophilic or non-hydrophilic, is advantageously modified, or contains additives, to make the implant **20** visible by conventional imaging techniques. For example, the foam can be impregnated with a water-insoluble radiopaque material such as barium sulfate, as described by Thanoo et al., “Radiopaque Hydrogel Microspheres”, *J. Microencapsulation*, Vol. 6, No. 2, pp. 233–244 (1989). Alternatively, the hydrogel monomers can be copolymerized with radiopaque materials, as described in Horák et al., “New Radiopaque PolyHEMA-Based Hydrogel Particles”, *J. Biomedical Materials Research*, Vol. 34, pp. 183–188 (1997).

Whatever the material from which the implant device **20** is made, the implant device **20** must be compressible to a fraction of its initial size, preferably into a substantially cylindrical or lozenge-shaped configuration, as shown in FIG. **3**. Compression of the implant device **20** can be performed by squeezing it or crimping it with any suitable fixture or implement (not shown), and then “setting” it in its compressed configuration by heating and/or drying, as is well-known. The purpose for this compression will be explained below in connection with the method of using the implant device **20** to embolize a vascular site.

The Method and Apparatus for Embolizing a Vascular Site.

The method of embolizing a vascular site using the implant device **20** is performed using an implanting apparatus **30**, a preferred embodiment of which is shown in FIG. **5**. The implanting apparatus **30** comprises the retention element or wire **22**, a microcatheter **32**, and an elongate, flexible, hollow, tubular element **34** (preferably a coil) that functions as an implant deployment element, as will be described below. With the implant device **20** attached to the distal end of the retention wire **22**, the proximal end of the retention wire **22** is inserted into the distal end of the implant deployment element **34** and threaded axially through the implant deployment element **34** until the proximal end of the implant device **20** seats against, or is closely adjacent to, the distal end of the implant deployment element **34**. The implant deployment element **34** is dimensioned for passing axially through the microcatheter **32**. Thus, the implant deployment element **34**, with the implant device **20** extending from its proximal end, may be inserted into the proximal end (not shown) of the microcatheter **32** and passed axially therethrough until the implant device **20** emerges from the distal end of the microcatheter **32**, as shown in FIG. **5**.

The implant device **20**, in its compressed configuration, has a maximum outside diameter that is less than the inside diameter of the microcatheter **32**, so that the implant device **20** can be passed through the microcatheter **32**. The implant device **20** is preferably compressed and “set”, as described above, before it is inserted into the microcatheter **32**.

FIGS. **6** through **10** illustrate the steps employed in the method of embolizing a vascular site **40** using the implant device **20**. The vascular site **40** shown in the drawings is a

typical aneurysm, but the invention is not limited to any particular type of vascular site to be embolized.

First, as shown in FIG. **6**, the microcatheter **32** is threaded intravascularly, by conventional means, until its distal end is situated within the vascular site **40**. This threading operation is typically performed by first introducing a catheter guidewire (not shown) along the desired microcatheter path, and then feeding the microcatheter **32** over the catheter guidewire until the microcatheter **32** is positioned substantially as shown in FIG. **6**. The catheter guidewire is then removed.

The implant deployment element **34**, with the implant device **20** extending from its distal end, is then passed through the microcatheter **32**, as described above, until the implant device **20** emerges from the distal end of the microcatheter **32** into the vascular site **40**, as shown in FIGS. **7** and **8**. When inserting the implant device **20** into the microcatheter **32**, a biocompatible non-aqueous fluid, such as polyethylene glycol, may be injected into the microcatheter **32** to prevent premature expansion of the implant device **20** due to hydration, and to reduce friction with the interior of the microcatheter **32**. The implant device **20** thus being exposed from the microcatheter **32** into the interior of the vascular site **40**, the pores of the implant device **20** begin to absorb aqueous fluid from the blood within the vascular site **40** to release its “set”, allowing it to begin assuming its expanded configuration, as shown in FIG. **9**. Then, if the implant device **20** is of a hydrophilic material, it continues to expand due to hydrophilic hydration of the implant material, as well as from the filling of its pores with blood. If the implant device **20** is of a non-hydrophilic material, its expansion is due to the latter mechanism only.

Finally, when the expansion of the implant device **20** is well underway (and not necessarily when it is completed), the retention wire **22** is pulled proximally with respect to the implant deployment element **34**, causing the implant device to be pushed off the end of the installation wire **22** by means of the pressure applied to it by the distal end of the implant deployment element **34**. The implant device **20**, now free of the implanting apparatus **30**, as shown in FIG. **10**, may continue to expand until it substantially fills the vascular site **40**. The implanting apparatus **30** is then removed, leaving the implant device **20** in place to embolize the vascular site **40**.

While a preferred embodiment of the invention has been described above, a number of variations and modifications may suggest themselves to those skilled in the pertinent arts. For example, instead of custom-fabricating the implant device for each patient, implant devices in a variety of “standard” sizes and shapes may be made, and a particular implant device then selected for a patient based on the imaging of the vascular site. In this case, the fabrication method shown in FIG. **1** would be modified by first creating a three-dimensional digital model for each standardized implant, (box **12**), and then proceeding with the subsequent steps shown in boxes **14**, **16**, and **18**. Imaging (box **10**) would be performed as an early step in the embolization procedure, followed by the selection of one of the standardized implant devices. This and other variations and modifications are considered within the spirit and scope of the invention, as described in the claims that follow.

What is claimed is:

1. A method of embolizing a vascular site comprising the steps of:
  - (a) providing a vascular implant comprising a hydrophilic hydrogel and having an initial compressed configuration, wherein the implant is releasably attached, in its

- initial configuration, to the distal end of a flexible, elongate deployment element that includes a coiled element;
- (b) providing a microcatheter having a distal end, and passing the microcatheter intravascularly until its distal end is situated closely adjacent to or within the vascular site;
  - (c) passing the implant and the deployment element through the microcatheter until the implant emerges from the distal end of the microcatheter;
  - (d) controllably releasing the implant from the deployment element; and
  - (e) expanding the implant in situ in the vascular site from its initial configuration to an expanded configuration that substantially fills the vascular site, primarily by hydrophilic hydration.
2. A method of embolizing a vascular site, comprising the steps of:
- (a) providing a vascular implant attached to the distal end of an elongate filamentous retention element, the implant comprising a macroporous hydrophilic hydrogel foam implant and having an initial compressed configuration, from which it is expansible into an expanded configuration substantially conforming to the vascular site;
  - (b) passing the implant and the retention element through a coiled deployment element having a distal end until the implant emerges from the distal end of the deployment element;
  - (c) passing a microcatheter intravascularly until its distal end is situated within the vascular site;
  - (d) passing the deployment element through the microcatheter, while the implant is in its initial configuration, until the implant emerges from the distal end of the microcatheter into the vascular site;
  - (e) controllably detaching the implant from the retention element; and
  - (f) expanding the implant in situ primarily by hydrophilic hydration substantially to fill the vascular site.
3. The method of claim 2, wherein the detaching step is performed by pulling the retention element proximally with respect to the deployment element, so that the implant is pushed off the end of the retention element by means of the pressure applied to it by the distal end of the deployment element.
4. Apparatus for embolizing a vascular site, comprising: a deployment element having a distal end and comprising a flexible elongate coil; and

- an expansile embolizing element, comprising a hydrophilic hydrogel and having an initial compressed configuration, wherein the embolizing element is releasably attached to the distal end of the deployment element, and wherein the embolizing element expands in situ, after being controllably released from the deployment element in the vascular site, from its initial configuration to an expanded configuration primarily by hydrophilic hydration.
- 5. The apparatus of claim 4, wherein the hydrogel is a hydrophilic polymer selected from the group consisting of olefins, polyvinyl alcohol, and PHEMA.
  - 6. The apparatus of claim 4, wherein the embolizing element is formed of a molded hydrogel.
  - 7. The apparatus of claim 4, wherein the hydrogel is porous.
  - 8. The apparatus of claim 4, wherein the hydrogel includes a radiopaque material.
  - 9. The apparatus of claim 4, wherein the hydrogel includes a drug that is releasable into the vascular site.
  - 10. Apparatus for embolizing a vascular site, comprising: a deployment element having a distal end and comprising a flexible, elongate coil; an expansile embolizing element, comprising a hydrophilic hydrogel and having an initial compressed configuration, wherein the embolizing element is releasably attached to the distal end of the deployment element, and wherein the embolizing element expands in situ, after being controllably released from the deployment element in the vascular site, from its initial configuration to an expanded configuration primarily by hydrophilic hydration, wherein the hydrogel has a water content of a least about 90% when fully hydrated.
  - 11. The apparatus of claim 10, wherein the hydrogel is a hydrophilic polymer selected from the group consisting of olefins, polyvinyl alcohol and PHEMA.
  - 12. The apparatus of claim 10, wherein the embolizing element is formed of a molded hydrogel.
  - 13. The apparatus of claim 10, wherein the hydrogel is porous.
  - 14. The apparatus of claim 10, wherein the hydrogel includes a radiopaque material.
  - 15. The apparatus of claim 10, wherein the hydrogel includes a drug that is releasable into the vascular site.

\* \* \* \* \*