



(51) International Patent Classification:

A61M 25/10 (2013.01) *A61B 18/24* (2006.01)
A61B 17/3205 (2006.01)

(21) International Application Number:

PCT/US2013/026994

(22) International Filing Date:

21 February 2013 (21.02.2013)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/602,653 24 February 2012 (24.02.2012) US

(71) Applicant: **ISOLASE, LTD.** [—/IL]; 22a Nitzanim Street,
34354 Haifa (IL).

(72) Inventors; and

(71) Applicants (for US only): **PELED, Omer** [IL/IL]; 22a
Nitzanim Street, 34354 Haifa (IL). **MIRABITO, A., Jason**
[US/US]; 129 North Shore Road, Derry, NH 03038 (US).

(74) Agents: **MIRABITO, A, Jason** et al.; Mintz Levin Cohn
Ferris Glovsky And Popeo, P.C., One Financial Center,
Boston, MA 02111 (US).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,


AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP,
KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD,
ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI,
NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU,
RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ,
TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA,
ZM, ZW.

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
ML, MR, NE, SN, TD, TG).

Published:

- with international search report (Art. 21(3))
- with amended claims (Art. 19(1))

(54) Title: IMPROVEMENTS IN ABLATION TECHNIQUES FOR THE TREATMENT OF ATRIAL FIBRILLATION

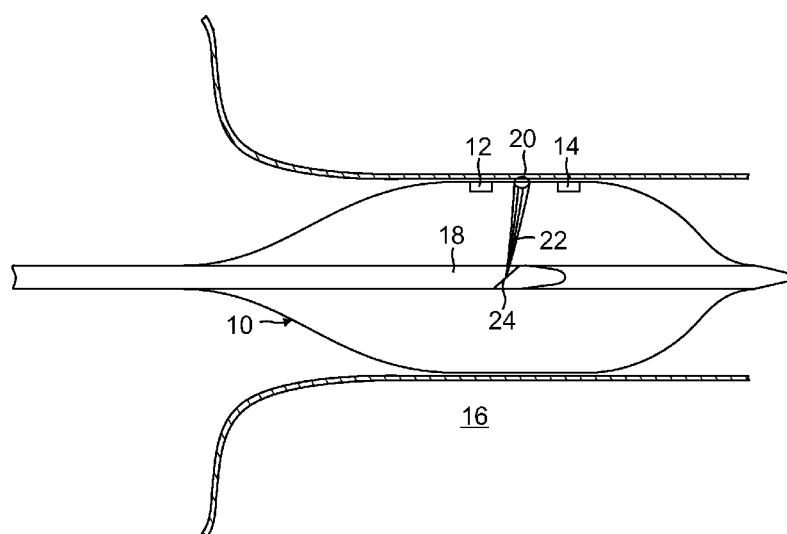

(57) Abstract: A catheter device provides a balloon structure and a side-firing laser lumen within the balloon to create lesions in the pulmonary vein (PV) in the treatment of atrial fibrillation. Mounted on the balloon so as to contact the PV when the balloon is inflated are one or more electrodes which may be used in a measurement mode, a treatment mode, or both.



IMPROVEMENTS IN ABLATION TECHNIQUES FOR THE TREATMENT OF ATRIAL FIBRILLATION

5 RELATED APPLICATIONS

This application claims priority to Serial No. 61/602,653, filed February 24, 2012, which is incorporated herein by reference in its entirety.

FIELD OF THE INVENTION

10

This invention relates to improvements in the field of atrial fibrillation, including devices and methods for the treatment of atrial fibrillation using new and improved apparatus.

BACKGROUND OF THE INVENTION

15

Pulmonary vein ablation is a known surgical treatment for atrial fibrillation (AF). Current solutions are based on a single energy source e.g. RF, cryogenic, ultrasound, laser or microwave. Each modality has its own advantages and disadvantages both in terms of tissue interaction or delivery method.

20

In order to optimize the treatment, a uniform transmural lesion must be created in the target tissue. Overtreatment may result in irreversible collateral thermal or mechanical damage to surrounding tissue which may lead to perforation or other complications while insufficient lesion creation may not electrically isolate the PV from the left atrium wall. With some of the technologies available today, due to the nature of the treatment modality, it is difficult to determine at what point the treatment desired is sufficiently administered.

25

For example, in a known treatment technique using a cryogenic fluid, the fluid is introduced into a balloon catheter which may be positioned within the pulmonary vein (PV). From experience and prior knowledge the operating doctor may have determined the length of time the fluid should be in contact with the tissue to achieve the desired ablation and creation of a lesion in the tissue. However, this may be imprecise and can vary from doctor to doctor and with the patient's tissue makeup. Further, introduction of the cryogenic fluid, its withdrawal, and stopping the creation of the lesion is imprecise given that the cooling of the tissue is gradual and to some extent not precisely controllable. Thus, there remains a need to provide an ablation system that permits more precise control of the creation of a lesion and for controllably halting the extent of the damage created by the lesion.

30

Another example is the creation of a lesion using radio frequency (RF) energy. Typically, unlike a cryogenic solution, in the treatment of AF using a RF source, a balloon is not used, but rather a catheter with one or more electrodes is introduced into the PV and the electrodes activated. Again, as in the example of the cryogenic treatment, the duration of treatment and the extent of damage caused by the application of RF may be imprecise and only loosely controllable. Thus, there is a need to provide a RF ablation system that permits more precise control and monitoring of a lesion created by the application of RF energy.

SUMMARY OF THE INVENTION

One aspect of the invention in the present application is to create a system which combines different modalities in a unique structure. Based on its nature, some modalities can be used for treatment or for measuring and diagnostic purposes in order to monitor the lesion dimension and quality and to feedback the system in order to optimize the treatment.

The present invention provides a device suitable for insertion into the pulmonary vein for the treatment of atrial fibrillation and in particular may include at least one aperture lumen having distal and proximal ends as well as an inflatable balloon in the vicinity of the distal end of the lumen. An optical fiber may be positioned at least partially within the at least one lumen; and there may be at least one opening in the vicinity of the distal end and within the inflatable balloon. An optical device may be placed in the lumen in the vicinity of the distal end and within the balloon to deflect a laser beam introduced in the vicinity of the proximal end and exiting in the vicinity of the distal end of the lumen. At least one electrode may be formed on the balloon, and the at least one electrode may be suitable for one or both of measurement and treatment of the pulmonary vein. A controller may be operatively connected to the at least one electrode, such that, when the inflatable balloon is inflated, the at least one electrode comes into contact with the pulmonary vein wall for one or more of measurement and treatment of atrial fibrillation.

BRIEF DESCRIPTION OF THE DRAWINGS

In the drawings, in which like reference numerals indicate related parts are elements of the embodiments of the present invention throughout the several views:

5

FIG. 1 is a diagram of a laser ablation balloon device in accordance with the present invention.

10

FIG. 2 is another embodiment of the invention of FIG. 1 in which there are a plurality of arrays of measuring elements.

FIG. 3 is an alternative embodiment to that of FIG. 1 which includes a number of treatment electrodes.

15

FIG. 4 is a variation of the embodiment of FIG. 3 and includes a number of cross related RF electrodes.

20

FIG. 5 is an alternative embodiment of FIG. 1 and includes 2 lumens, a laser lumen and a viewing lumen.

FIG. 5A is an alternative embodiment of FIG. 5 including a laser lumen and a viewing lumen.

25

FIG. 6 is an embodiment related to FIG. 5 illustrating the ability of the laser viewing lumens to rotate about an axis within the balloon.

FIG. 7 is an alternative to the side firing laser of FIG. 1 and includes a conical shape reflector.

30

FIG. 8 is an improved cryogenic balloon device which provides heat and cooling control as well as RF sensors.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

RF is presently the dominant technology for PV ablation and, as mentioned, does not require a balloon at all. RF is delivered directly to the target tissue by coil electrodes, in a variety of shapes, and delivered through a catheter.

Known laser ablation systems deliver the laser energy through a side firing fiber located in a fixation balloon. Laser ablation systems have the advantage that the interaction of tissue to various types and wavelengths of laser beams is well-known in the art, in terms of absorption of the heat generated by the beam and the extent and timing of cooling of the irradiated tissue. In addition, the use of laser beams to ablate tissue has the advantage that the beam can be instantly turned on and off, allowing a more precise control of the creation of a lesion and ablation than with either the cryogenic or RF modalities. The beam may be delivered from the inner volume of a balloon, through its wall, to the target tissue. The beam may exit the balloon along a strip which acts as a window. The optical window in the balloon material is, of course, chosen so as to be transparent to the laser beam so that balloon integrity is maintained during ablation. An example of a laser treatment system suitable for the treatment of AF but without measuring features or functionality is given in US Patent No. 7,137,395 entitled "Circumferential Pulmonary Vein Ablation Using a Fiberoptic Balloon Catheter", the entire disclosure of which is herein incorporated by reference in its entirety.

One aspect of the present invention is to create a balloon which has at least one, but perhaps more than one, measuring element on either side of the area of the balloon through which the laser beam passes, called herein the treatment strip. In one configuration, two or more arrays of such elements can be positioned from both sides of the laser treatment strip. Each array may have one or more rows of elements.

Each measuring element may be an RF electrode or an Ultrasound transducer, and is embedded on the outer surface of the balloon's wall and is wired with flexible wires also embedded on or in the balloon. Each element has an outer surface which is configured to create a direct contact with the tissue when the balloon is inflated.

Turning now to the Figures, Fig 1 shows one aspect of the invention in which a balloon 10 with measuring elements 12 and 14 is positioned within the PV 16. A side firing fiber 18 located in the balloon targets a tissue region 20 within a treatment strip through the balloon. As illustrated in FIG. 1, a surface 24 is used to deflect the beam spot from along the length axis of the catheter to an angle to impact the surface of the PV. While FIG. 1 shows this to be approximately 90 degrees, it is to be understood that any suitable angle may be

utilized. One structure to deflect the beam may be to angle the face of the firing fiber to totally internally reflect the beam out of the face of the fiber in a direction transverse to the length axis of the catheter, although any suitable desired angle may be chosen, as disclosed in U.S. Patent No. 5,772,657, entitled "Side Firing Fiber Optic Laser probe", the entirety of which is herein incorporated by reference. An angled mirror facing the exit of the laser fiber may be utilized to deflect the beam. The beam spot 22 can manually or automatically scan (by rotation) the treatment strip to ablate the PV wall. Measuring elements 12 and 14 from both sides of the strip can also treat tissue located between active pair of elements. It is known in the art that electrodes of the radio-frequency type and the ultrasonic type can be used alternatively in a measuring mode or a treatment mode, thus enabling the ablation device of the present invention to both measure the degree of success of ablation as well as to operate in conjunction with the side firing laser to provide treatment to the PV. Bipolar RF electrodes can be activated by a system controller (not shown) in a variety of sequences (measuring and/or treatment) to generate treatment and/or measuring vectors. In one example, illustrated in FIG. 4, the vectors 30 can crisscross each other and generate multiple adjacent X shapes from RF electrodes 32 (A1-A7, B1-B7) in addition to the laser treatment. In yet another embodiment, the multiple electrodes 32 can measure tissue impedance changes resulting from the laser treatment or any other treatment and to assess the size, depth or electrical quality of a lesion. This information can be feedback to the system controller for further treatment.

In yet in another configuration, the RF electrodes 32 may be replaced by ultrasound transducers which in the embodiments of FIGS. 1, 3 and 4 may measure changes in the mechanical properties of the tissue by measuring changes of sound velocity, absorption or reflection in different energies or frequencies of the target tissue. Multiple elements can be used to focus ultrasound energy in order to also achieve therapeutic threshold and to ablate tissue ultrasonically rather than use RF energy.

Turning now to FIG. 2. Figure 2 shows the side firing balloon catheter 40 including a laser ablation strip 46 through which laser energy is focused upon the PV. In the embodiment shown in FIG. 2, two rows of measuring and/or treating elements 42 and 44 are positioned on either side of the laser ablation strip 46 in order to measure and/or treat the PV in conjunction with or in lieu of the laser beam 48 from the side firing laser 50.

In addition to measuring changes in the tissue, the ultrasound elements may be used for measuring, for example, the thickness of the PV wall, which may aid the operating doctor to determine the extent of treatment applied to the tissue. The ultrasound elements may be

used to measure the overall dimensions of not only the PV but also the dimensions of the lesion(s) created by the treatment.

In another configuration illustrated in FIG. 3, the RF electrode array may include more than one row of electrodes in each side of the treatment strip. As shown in FIG. 3, the inner pair 60, 62 can create an electric field which then pushes the electric field 70 created by pair 64, 66 deeper into the target tissue 68. A third pair (not illustrated) may be used to push the electric field even deeper. More pairs can be utilized in order to fully cover the PV wall. A pair of the RF electrodes, for example, can be configured to deliver energy fluence to ablate a tissue in a certain depth in conjunction with the laser ablation beam 72 or in lieu of such beam or alternatively between energization of the laser ablation beam 72 and RF electrodes 60, 62, 64 and 66. The same pair of electrodes can then be configured to deliver non-ablative energy and to only push deeper the ablative energy of the next pair. Using this sequence of events can create a homogenous lesion across the PV wall to achieve the best electrical isolation safely.

Turning now to FIG. 5, this figure is similar to that shown in FIG. 1 but includes a second fiber viewing lumen 80 arranged in parallel “over-under” relationship to the side firing fiber lumen 82 for the laser beam. In this embodiment, the second side-viewing fiber lumen 80 is incorporated that views the inside of the balloon with an 180 degree offset from that of the side-firing fiber 82 lumen (as shown, although other angular offsets may be utilized). However, one way to visualize the extent of lesion creation immediately after the laser firing is to orient the firing and viewing lumens “side-by-side” rather than in the “over-under” relationship of FIG. 5. This is illustrated in FIG. 5A, in which the lumens 92 and 94 sit side-by-side, the firing laser lumen being 92 and the viewing lumen being 94. When the lumen 92, 94 combination is rotated in direction 96, the laser fires through lumen 92 and the results are viewable through lumen 94. Of course, lumens 92 and 94 may be “in line” with one another, as shown in FIG. 5 or “offset” from one another, as shown in FIG. 6, to be discussed below. However, any suitable angle or orientation between the firing and viewing lumens may be utilized.

For both of FIGS. 5 and 5A, it is to be understood that with both the side-firing lumens and the side-viewing lumens that the light beams are reoriented from along the lumens axis to an angle from such axis using any number of devices described above with respect to the embodiment of FIG. 1. As shown in FIG. 5, the second side-viewing fiber lumen 80 includes a opening 88 in the lumen 80 which allows the light from the viewing fiber to be angled from a position along the longitudinal axis length of the lumen to one at an

angle with respect to the lumen longitudinal axis. While the operating doctor may wish to move the side firing laser 84 around the periphery of the balloon in a circular motion while firing the laser, there are at least two visualization problems. The first is knowing where the laser is in fact firing and whether areas of the PV sought to be treated are either not treated or treated too much. The second is that while the operating doctor may rotate the proximal end of the side-firing 84 fiber a given number of degrees, due to torsional forces within the fiber itself, the same given degrees of rotation may not translate precisely with the working distal end of the side-firing fiber 84, again potentially providing either over or under treatment.

While the viewing lumen may be of a conventional type, instead an optical coherence tomography (OCT) device may be incorporated in the viewing lumen as well or instead of the conventional type.

Thus, we have provided, in addition to the second viewing fiber lumen 80, a series of markings 86, shown as lines in FIG. 5 for illustration only, either on the inside or the outside of the balloon 90, that may be viewed through the viewing fiber, again accounting for the 180 (or other) degree offset. Thus, the operating doctor will not only be able to view the extent of the lesion made by the use of the laser energy but will also know the precise position of the side-firing fiber and the areas of the lesion within the PV that require further (or less) ablation. The markings may be marked from 0 degrees to 360 degrees or with any other suitable scale. In addition, as shown in FIG. 6, the side-firing laser fiber 100 opening and the viewing fiber 102 opening may be offset from one another so that the markings do not interfere with the window within which the laser beam 104 operates. The combined side-firing and viewing fibers may be rotated in either direction, as illustrated by arrow 108.

In addition, due to the extent of miniaturization of electronic elements, it may be useful to incorporate positioning determining elements within the balloon itself. One possible technology is MediGuide's (now St. Jude Medical) MPS imagery technology on the distal end of the side-firing fiber to give the operating doctor a 3D perspective of the balloon position vis-à-vis the PV.

A further peripheral that may be utilized is a suitable sensor such as sensor 110 shown in FIG. 6 located at the distal tip of the side-firing fiber 120 which can interact with the circumferentially disposed RF or ultrasound electrodes 112, 114 to determine the location or orientation of the side-firing fiber tip within the balloon and relative to a treatment window or within the PV.

Yet another embodiment, illustrated in FIG. 6, to assure accurate positioning and orientation of the side-firing fiber 120 and the treatment area is to equip the fiber with an

electromagnetically actuated manipulator 122 that controls rotation and/or displacement of the side-firing fiber's distal end. Suitable electrical connections may be made to a manipulation device/toggle at the proximal end of the fiber which may be manipulated by the operating doctor. While the electromagnetically manipulator 122 is shown in FIG. 6 to be located just outside the balloon 124 it is understood that it is within the scope of the invention that the actuator 122 may be located within the balloon 124. This may be combined with the direct visualization or the sensor 110 described above to give the operating doctor direct positional orientation information of the side-firing fiber.

Turning now to FIG. 7, this figure illustrates another form of a laser fiber treatment device. While the lasers shown in Figs. 1, 5 and 6 are side-firing devices, the laser fiber structure shown in FIG. 7 is a 360 degree firing laser. In lieu of the flat but angled mirror surface shown (24 in FIG. 1) in Figs. 1, 5 and 6, at the distal end of the fiber 200 is installed a conically shaped mirror or reflector 202, with the apex 204 of the cone disposed to face the laser-firing fiber 200. In this manner, when the laser beam is directed to the mirror, the beam will be reflected 90 degrees to the laser beam axis and reflected in a 360 degree circular beam. In order to accomplish this, between the distal end of the fiber and conical mirror is disposed a tube-like window 208 of a suitable material around the entire circumference of the tube containing the fiber to allow the laser beam reflected from the conical mirror to pass out of the catheter. The material chosen for the window preferably is a material transparent to the laser beam itself. While FIG. 7 illustrates a 90 degree reflection from the conically shaped mirror or reflector, it is to be understood that the cone shape or height may be chosen to reflect the laser beam at other than 90 degrees depending on the desired orientation.

Turning now to FIG. 8, that figure illustrates improvements to a cryogenic-based ablation system. As discussed above, one problem with known cryogenic systems is the lack of precision that may result in either undertreatment or overtreatment of the PV in terms of lesion creation. In FIG. 8, to a presently-known cryogenic balloon catheter 300, such as that made by Medtronic, two improvements are added. The first is a series of RF or other (such as ultrasonic) sensors 302 of the type as previously described in connection with FIG. 2. The second is the addition of a source 312 of a heated fluid which may be introduced either through the same lumen 304 as the cold fluid is introduced or through a second lumen 306. In addition, a third lumen 308 may be provided to remove cold and/or heated fluid from the balloon and return it to the system. In operation, cold fluid from source 314 is introduced into the balloon 300 as is presently known through lumen 306. The RF or other sensors 302 are activated to assess the lesion caused in the PV by the application of cold fluid. Once the

desired lesion has been created or is the process of creation, the RF sensors which are operatively connected to a system controller 310 will signal the system controller to provide heated fluid to the catheter and thus to the balloon to halt the ablation of the PV. The third lumen 308 may be utilized at this juncture to remove all the fluid within the balloon return to
5 a volume 316 in which it may be reused or discarded. It is to be understood that the terms “Cold fluid” and “heated fluid” are used relatively herein, inasmuch as the temperatures of cold fluid being introduced are well established in cryogenic devices being marketed presently. In particular, the term “heated fluid” means fluid which is of a temperature greater than, to any degree, to that of the “cold fluid”. The ability to control the introduction of both
10 cooled and heated fluid also allows for treatments in which the tissue may be alternatively cooled and heated in order to achieve the desired treatment effect. In lieu of a heated fluid being introduced into the balloon, the second lumen 304 may be constructed of a resistive-type heating element to heat the cold fluid already present within the balloon. One or more thermocouples 320 may be provided with the balloon itself and on the balloon outside surface
15 to determine tissue and fluid temperatures operatively connected to and in conjunction with the controller apparatus 310. It is further to be understood that only the first improvement discussed above or the second improvement discussed above may be provided on the cryogenic balloon catheter 300.

It is further to be understood that the RF or other (ultrasound) sensors may be
20 reversed in their function and operate as further sources for causing ablation. For example, the PV may be subjected to both a cryogenic treatment followed by an RF treatment of the type discussed in connection with FIGS. 1- 4 above, or vice versa, or even an alternate cryogenic/RF treatment repeated a desired number of times.

Finally, as mentioned, in a typical RF ablation device, a balloon is not utilized, but
25 rather, typically, coils with electrodes are positioned in the PV or other desired location. Mounting RF electrodes on the outer surface of a balloon, as shown in various figures herein, allows direct and precise contact between the electrodes and tissue. In addition, in such a balloon RF ablation device, a side-viewing optical fiber of the type described with reference to FIG. 5 may be utilized to provide visual inspection of lesion created by the RF ablation
30 coil.

The advantages of the invention described in this application have been set forth in the foregoing description and in the appended drawings. It will be understood, however, that this disclosure is, in any number of respects, only illustrative. Changes may be made in details including such matters as shape, size, arrangement of parts without departing from the

scope of the present invention. The scope of the invention herein is defined by the appended claims now following.

What we claim is:

1. A device suitable for insertion into the pulmonary vein for the treatment of atrial fibrillation, the device comprising:

5 at least one apertured lumen having distal and proximal ends;
 an inflatable balloon in the vicinity of the distal end of the lumen;
 an optical fiber at least partially within the at least one lumen;
 at least one opening in the vicinity of the distal end and within the
 inflatable balloon;
10 an optical device in the lumen in the vicinity of the distal end and within
 the balloon to deflect a laser beam introduced in the vicinity of the
 proximal end and exiting in the vicinity of the distal end of the lumen;
 at least one electrode formed on the balloon, wherein the at least one
 electrode is suitable for one or both of measurement and treatment of the
15 pulmonary vein,
 a controller operatively connected to the at least one electrode;
 wherein, when the inflatable balloon is inflated, the at least one electrode
 comes into contact with the pulmonary vein wall for one or more of
 measurement and treatment.

AMENDED CLAIMS**received by the International Bureau on 12 August 2013(12.08.2013)**

What we claim is:

1. A device suitable for insertion into the pulmonary vein for the treatment of atrial fibrillation, the device comprising:
 - at least one apertured lumen having distal and proximal ends;
 - an inflatable balloon in the vicinity of the distal end of the lumen;
 - an optical fiber at least partially within the at least one lumen and disposed along the axis of the lumen, the optical fiber being suitable for conveying a beam of laser energy;
 - at least one opening in the vicinity of the distal end and within the inflatable balloon;
 - an optical device in the lumen in the vicinity of the distal end and within the balloon to deflect a laser beam introduced in the vicinity of the proximal end and exiting in the vicinity of the distal end of the lumen at angles other than along the lumen axis, the lumen being rotatable around the lumen axis while the inflatable balloon remains stationary;
 - at least one electrode formed on the balloon, wherein the at least one electrode is suitable for one or both of measurement and treatment of the pulmonary vein wall,
 - a controller operatively connected to the at least one electrode;
 - wherein, when the inflatable balloon is inflated, the at least one electrode comes into contact with the pulmonary vein wall and is operable for one or more of measurement and treatment, the controller also being operatively connected to a source of laser energy and being operable to cause laser energy to be conveyed along the lumen axis to the optical device, the optical device deflecting the laser beam to impinge on the pulmonary vein wall.
2. The device of claim 1, wherein the optical device is a surface which deflects the laser beam from along the lumens axis to the pulmonary vein wall.
3. The device of claim 2, wherein the optical device is an angled mirror.

4. The device of claim 1, wherein the deflected laser energy impinges on the pulmonary vein wall through a laser beam treatment area within the inflated balloon.
5. The device of claim 4, further comprising a plurality of electrodes formed at least partially around the periphery of the balloon, the electrodes being located outside the laser beam treatment area.
6. The device of claim 1, wherein the at least one electrode is one or more of an electrode for applying RF or ultrasound energy to the pulmonary vein wall.
7. The device of claim 1, further comprising at least a second apertured lumen, the second lumen being positioned parallel to and adjacent to the first aperture lumen, the second lumen having at least one opening in the vicinity of the distal end of the first lumen and having a viewing optical fiber within the second lumen, an optical device in the second lumen in the vicinity of the distal end of the second lumen, the optical device of the first and the second lumens being offset from one another, wherein the optical fiber of the second lumen is positioned to convey viewed images of the pulmonary vein wall to a user.
8. The device of claim 7, further comprising one or more markings on the balloon and viewable by the viewing optical fiber to convey lumen position information to the user.
9. The device of claim 8, wherein the lumen position information comprises angular markings.
10. The device of claim 2, wherein the deflecting surface is a conically shaped reflecting surface, whereby a laser beam impinging the conically shaped surface is deflected in a substantially 360 degree circular beam.
11. The device of claim 1, wherein the controller is operable to one or more of:
controlling the source of laser energy to cause laser energy to impinge on the pulmonary vein wall while operating the at least one electrode for measurement;

operating the at least one electrode for measurement after the laser energy has impinged on the pulmonary vein wall;
operating the at least one electrode for treatment after the laser energy has impinged on the pulmonary vein wall; and
operating both the laser energy and the at least one electrode simultaneously for treatment.

12. The device of claim 5 wherein the plurality of electrodes are arranged in two or more rings and wherein the controller activates the plurality of electrodes in a crisscross manner for treatment of the pulmonary vein wall.
13. The device of claim 5, wherein the plurality of electrodes is suitable for measurement of pulmonary vein wall tissue impedance changes after one or more of a laser energy and an electrode treatment, the measurement being fed back to the controller to determine the extent of treatment.
14. A device for insertion in the pulmonary vein for the treatment of atrial fibrillation, the device comprising;
 - a plurality of substantially parallel apertured lumens having distal and proximal ends;
 - an inflatable balloon in the vicinity of the distal ends of the lumens, the apertured lumens having openings in the distal ends of the lumens within the inflatable balloon;
 - at least one electrode formed on the balloon, wherein the at least one electrode is suitable for one or both of measurement and treatment of the pulmonary vein;
 - the plurality of lumens being suitable for the introduction and the evacuation of a cryogenic fluid into the balloon;
 - a controller operatively connected to the at least one electrode and to a source of cryogenic fluid wherein, when the inflatable balloon is inflated, the at least one electrode comes into contact with the pulmonary vein wall; and

the controller being further operable to introduce cryogenic fluid into the inflated balloon to treat the pulmonary vein wall.

15. The device of claim 14, wherein the controller is operable to control the treatment of the pulmonary vein wall with one or both of the at least one electrode and the cryogenic fluid.
16. The device of claim 15, wherein the controller is further operable to operate the at least one electrode to measure treatment parameters after treatment by one or both of cryogenic fluids and the at least one electrode.

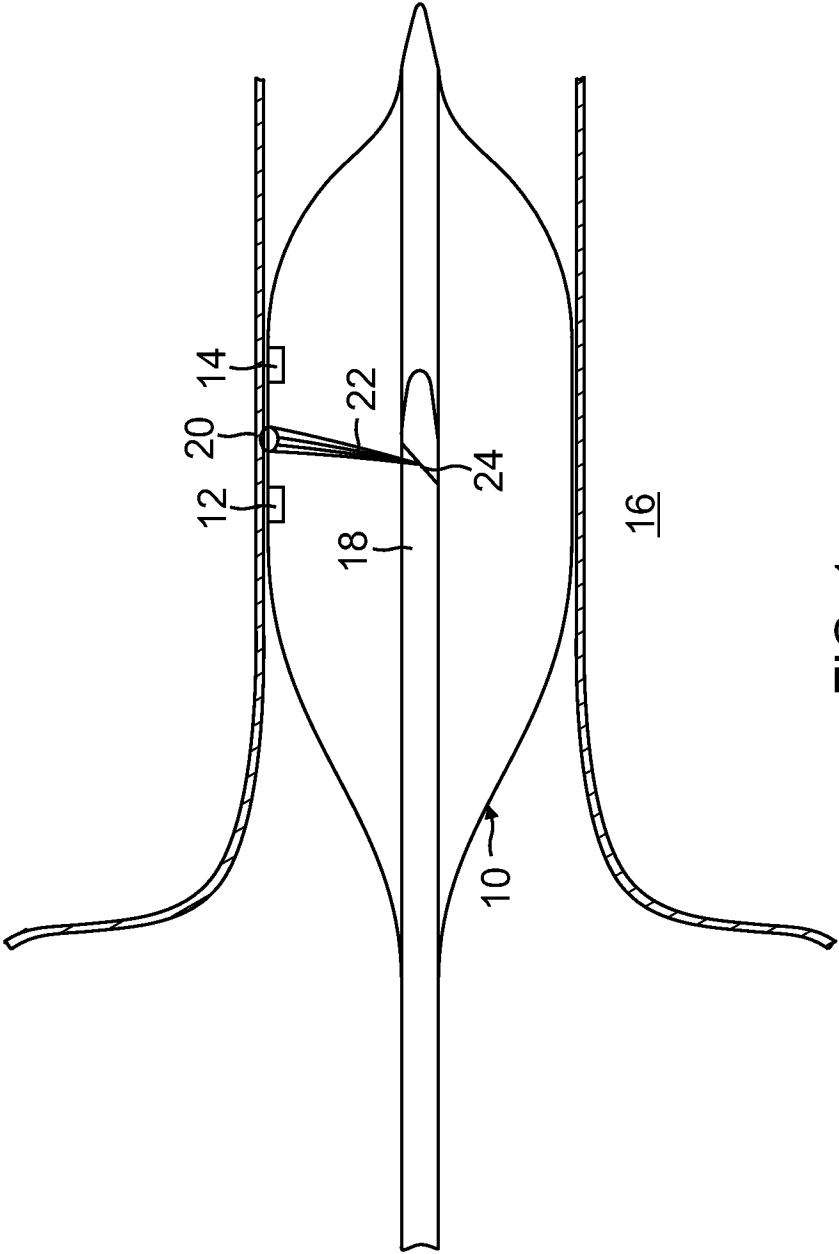


FIG. 1

2/6

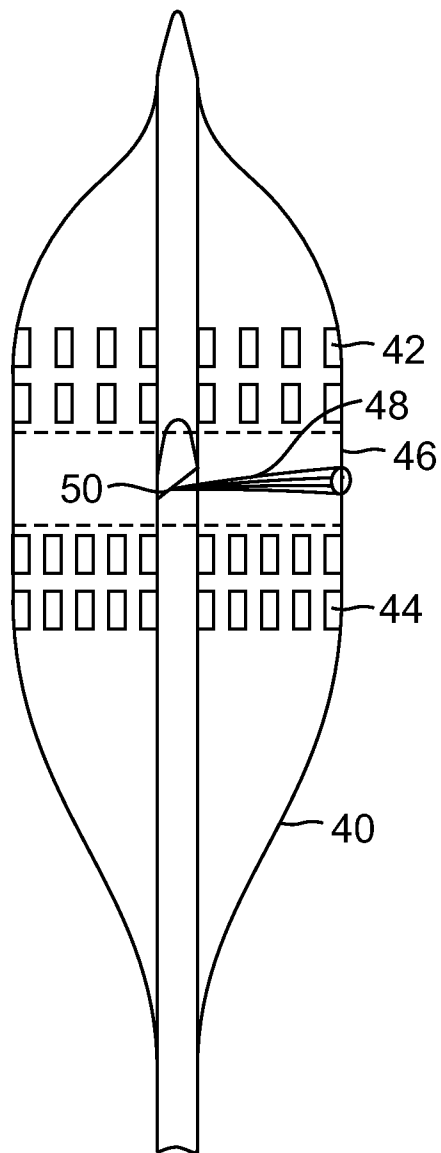


FIG. 2

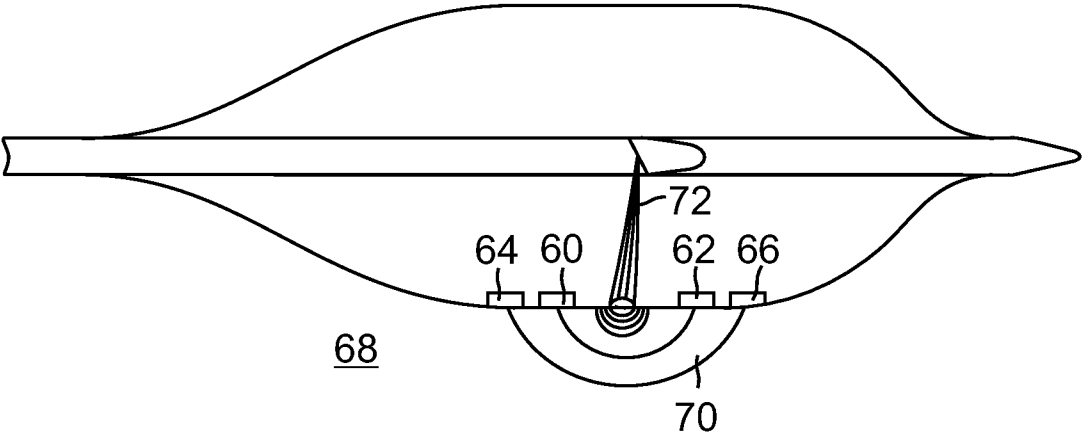


FIG. 3



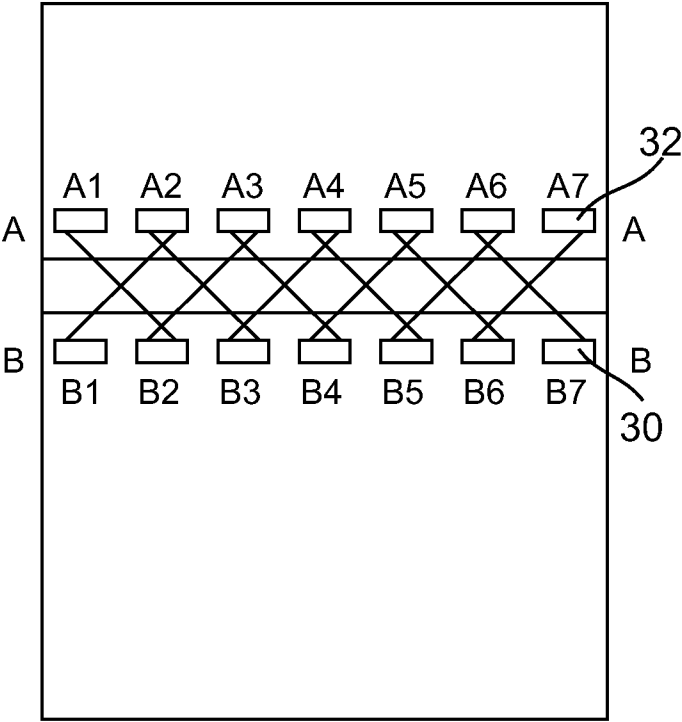


FIG. 4

4/6

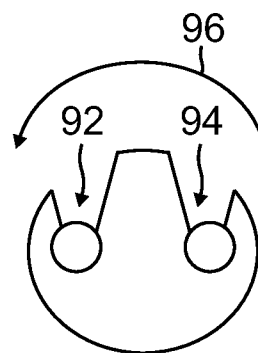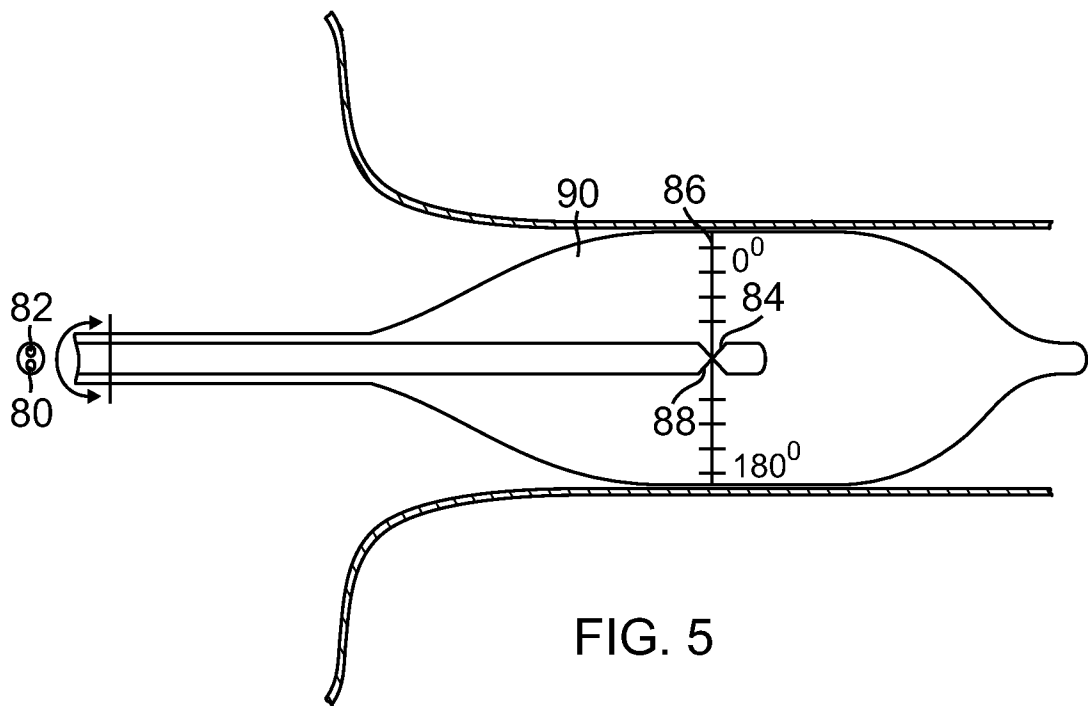

5/6

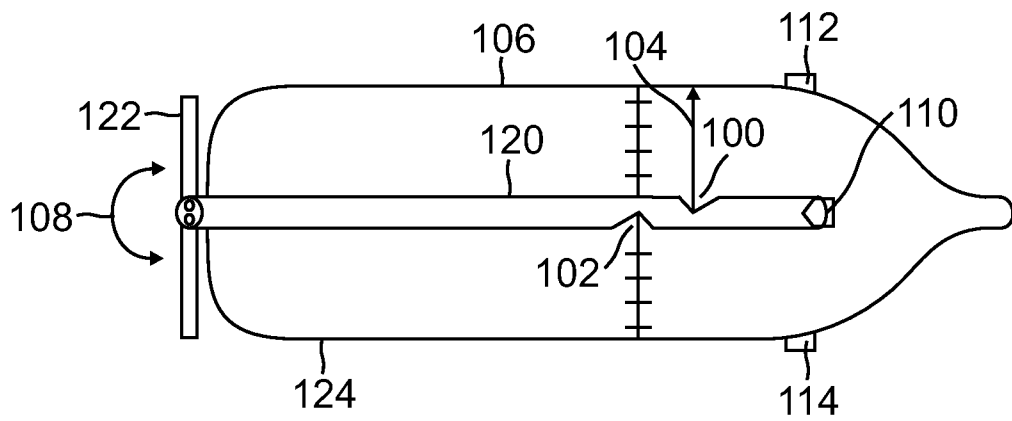


FIG. 6

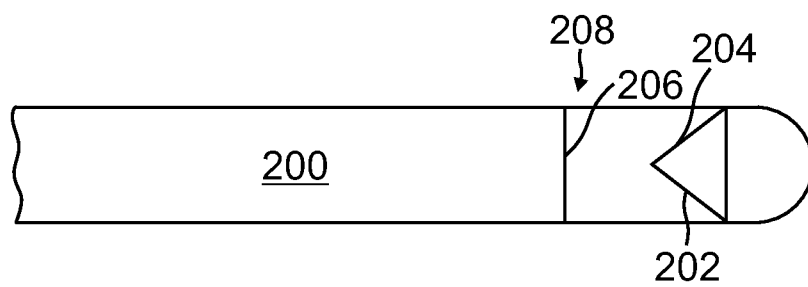


FIG. 7

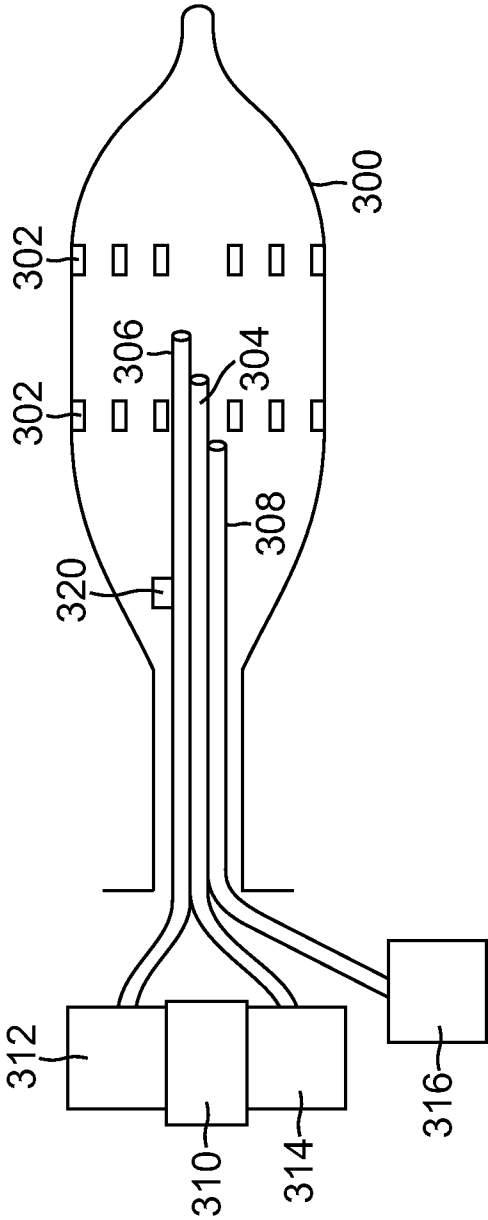


FIG. 8

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2013/026994**A. CLASSIFICATION OF SUBJECT MATTER****A61M 25/10(2006.01)i, A61B 17/3205(2006.01)i, A61B 18/24(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61M 25/10

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & Keywords: atrial fibrillation, AF, pulmonary vein, PV, ablation, radio frequency, RF, lumen, balloon, optical fiber, electrode, controller

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 7137395 B2 (FRIED, N. M. et al.) 21 November 2006 See abstract; claims 1, 35; column 4, lines 61-62; column 5, lines 1-7; figures 4, 6.	1
Y	WO 2005-112812 A1 (MEDTRONIC, INC.) 1 December 2005 See abstract; paragraph [0053]; figures 6, 15.	1
A	US 7399300 B2 (BERTOLERO, A. A. et al.) 15 July 2008 See abstract; column 22, lines 4-41; figures 6-7.	1
A	US 2006-0106375 A1 (WERNETH, R. L.) 18 May 2006 See abstract; claim 1; figure 7.	1
A	US 2005-0059965 A1 (EBERL, G. R. et al.) 17 March 2005 See abstract; claims 13, 29; figure 4.	1



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

12 June 2013 (12.06.2013)

Date of mailing of the international search report

13 June 2013 (13.06.2013)

Name and mailing address of the ISA/KR

Korean Intellectual Property Office
189 Cheongsu-ro, Seo-gu, Daejeon Metropolitan City,
302-701, Republic of Korea

Facsimile No. 82-42-472-7140

Authorized officer

HAN, In Ho

Telephone No. 82-42-481-3362



INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/026994

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 7137395 B2	21.11.2006	US 2002-052621 A1	02.05.2002
WO 2005-112812 A1	01.12.2005	AU 2003-209600 A1	16.09.2003
		AU 2003-209600 B2	02.07.2009
		AU 2003-287205 A1	07.06.2004
		AU 2003-291353 A1	03.06.2004
		AU 2005-244868 A1	01.12.2005
		AU 2005-245432 A1	01.12.2005
		CA 2434149 A1	18.07.2002
		CA 2569413 A1	01.12.2005
		CA 2569701 A1	01.12.2005
		CN 101370554 A	18.02.2009
		CN 101948233 A	19.01.2011
		EP 1361816 A2	19.11.2003
		EP 1361816 B1	04.11.2009
		EP 1423053 A1	02.06.2004
		EP 1490306 A1	29.12.2004
		EP 1558331 A1	03.08.2005
		EP 1558331 B1	18.02.2009
		EP 1560527 A2	10.08.2005
		EP 1560527 B1	15.10.2008
		EP 1585446 A1	19.10.2005
		EP 1589879 A1	02.11.2005
		EP 1592349 A1	09.11.2005
		EP 1592349 B1	17.06.2009
		EP 1750605 A1	14.02.2007
		EP 1750605 B1	07.03.2012
		EP 1750804 A1	14.02.2007
		EP 1750804 B1	02.07.2008
		EP 1830720 A1	12.09.2007
		EP 1830720 B1	07.04.2010
		EP 1919378 A2	14.05.2008
		EP 1980212 A1	15.10.2008
		EP 1980212 B1	18.05.2011
		EP 2092285 A2	26.08.2009
		EP 2292563 A2	09.03.2011
		EP 2292563 A3	18.05.2011
		EP 2292564 A2	09.03.2011
		EP 2292564 A3	11.05.2011
		EP 2292565 A2	09.03.2011
		EP 2292565 A3	25.05.2011
		GB 2363392 A	19.12.2001
		JP 2002-129445 A	09.05.2002
		JP 2004-526479 A	02.09.2004
		JP 2005-526682 A	08.09.2005
		JP 2007-537011 A	20.12.2007
		JP 2007-537013 A	20.12.2007
		JP 2010-132548 A	17.06.2010
		JP 2010-512507 A	22.04.2010

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/026994

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		US 2001-0049869 A1	13.12.2001
		US 2002-0095067 A1	18.07.2002
		US 2002-0095139 A1	18.07.2002
		US 2002-0138109 A1	26.09.2002
		US 2003-0167799 A1	11.09.2003
		US 2004-0055125 A1	25.03.2004
		US 2004-0082830 A1	29.04.2004
		US 2004-0087831 A1	06.05.2004
		US 2004-0088035 A1	06.05.2004
		US 2004-0138522 A1	15.07.2004
		US 2004-0138526 A1	15.07.2004
		US 2004-0138527 A1	15.07.2004
		US 2004-0138531 A1	15.07.2004
		US 2004-0138621 A1	15.07.2004
		US 2004-0267303 A1	30.12.2004
		US 2005-0209564 A1	22.09.2005
		US 2005-0235697 A1	27.10.2005
		US 2005-0261673 A1	24.11.2005
		US 2005-0267454 A1	01.12.2005
		US 2005-0273129 A1	08.12.2005
		US 2006-0025756 A1	02.02.2006
		US 2006-0041243 A1	23.02.2006
		US 2006-0162383 A1	27.07.2006
		US 2006-0200002 A1	07.09.2006
		US 2006-0229594 A1	12.10.2006
		US 2007-0049863 A1	01.03.2007
		US 2008-0190144 A1	14.08.2008
		US 2008-0190145 A1	14.08.2008
		US 2008-0202168 A1	28.08.2008
		US 2008-0209944 A1	04.09.2008
		US 2008-0209948 A1	04.09.2008
		US 2008-0217539 A1	11.09.2008
		US 2008-0223081 A1	18.09.2008
		US 2008-0229785 A1	25.09.2008
		US 2008-0264105 A1	30.10.2008
		US 2008-0271492 A1	06.11.2008
		US 2008-0314087 A1	25.12.2008
		US 2009-0143638 A1	04.06.2009
		US 2010-0063475 A1	11.03.2010
		US 2010-0069844 A1	18.03.2010
		US 2010-0198346 A1	05.08.2010
		US 2010-0294935 A1	25.11.2010
		US 6447443 B1	10.09.2002
		US 6595934 B1	22.07.2003
		US 6676597 B2	13.01.2004
		US 6786898 B2	07.09.2004
		US 6837848 B2	04.01.2005
		US 6890295 B2	10.05.2005
		US 6918908 B2	19.07.2005
		US 6936046 B2	30.08.2005

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/026994

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		US 7024887 B2	11.04.2006
		US 7063693 B2	20.06.2006
		US 7073352 B2	11.07.2006
		US 7100253 B2	05.09.2006
		US 7146225 B2	05.12.2006
		US 7326173 B2	05.02.2008
		US 7338434 B1	04.03.2008
		US 7438680 B2	21.10.2008
		US 7494460 B2	24.02.2009
		US 7507235 B2	24.03.2009
		US 7610776 B2	03.11.2009
		US 7628780 B2	08.12.2009
		US 7706882 B2	27.04.2010
		US 7721573 B2	25.05.2010
		US 7740623 B2	22.06.2010
		US 7744562 B2	29.06.2010
		US 7779650 B2	24.08.2010
		US 7788950 B2	07.09.2010
		US 7793520 B2	14.09.2010
		US 7800066 B2	21.09.2010
		US 7827826 B2	09.11.2010
		US 8221402 B2	17.07.2012
		US 8241274 B2	14.08.2012
		US 8273072 B2	25.09.2012
		WO 02-054937 A2	18.07.2002
		WO 02-054937 A3	18.07.2002
		WO 02-102252 A1	27.12.2002
		WO 03-074433 A2	12.09.2003
		WO 2004-041349 A1	21.05.2004
		WO 2004-043267 A2	27.05.2004
		WO 2004-064645 A1	05.08.2004
		WO 2004-064646 A1	05.08.2004
		WO 2004-064647 A1	05.08.2004
		WO 2005-113068 A1	01.12.2005
		WO 2006-060431 A1	08.06.2006
		WO 2007-002227 A2	04.01.2007
		WO 2007-005297 A1	11.01.2007
		WO 2007-067945 A2	14.06.2007
		WO 2007-067945 A8	14.06.2007
		WO 2008-073261 A2	19.06.2008
		WO 2011-041123 A2	07.04.2011
US 7399300 B2	15.07.2008	AU 2003-293403 A1	23.06.2004
		EP 1575421 A2	21.09.2005
		EP 1689285 A2	16.08.2006
		US 2003-0120268 A1	26.06.2003
		US 2003-0158464 A1	21.08.2003
		US 2004-0102771 A1	27.05.2004
		US 2005-0149069 A1	07.07.2005
		US 2005-0149152 A1	07.07.2005

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/026994

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		US 2005-0240175 A1	27.10.2005
		US 2005-0288666 A1	29.12.2005
		US 2006-0015165 A1	19.01.2006
		US 2007-0156185 A1	05.07.2007
		US 2007-0239155 A1	11.10.2007
		US 2009-0076503 A1	19.03.2009
		US 2009-0076537 A1	19.03.2009
		US 2010-0016851 A1	21.01.2010
		US 2011-0009853 A1	13.01.2011
		US 6849075 B2	01.02.2005
		US 7226448 B2	05.06.2007
		US 7542807 B2	02.06.2009
		US 7591818 B2	22.09.2009
		US 7749157 B2	06.07.2010
		US 7819867 B2	26.10.2010
		US 7951069 B2	31.05.2011
		US 7957820 B2	07.06.2011
		US 8096990 B2	17.01.2012
		US 8419729 B2	16.04.2013
		WO 2004-049971 A2	17.06.2004
		WO 2004-091373 A2	28.10.2004
		WO 2005-046456 A2	26.05.2005
US 2006-0106375 A1	18.05.2006	AU 2005-306826 A1	26.05.2006
		AU 2005-306826 B2	01.03.2012
		CA 2587331 A1	26.05.2006
		EP 1824405 A2	29.08.2007
		EP 1824405 A4	20.08.2008
		EP 1824405 B1	12.01.2011
		WO 2006-055286 A2	26.05.2006
		WO 2006-055286 A3	06.07.2006
US 2005-0059965 A1	17.03.2005	US 7736362 B2	15.06.2010
		WO 2005-032636 A1	14.04.2005