

(12) 特許協力条約に基づいて公開された国際出願

(19) 世界知的所有権機関
国際事務局

(43) 国際公開日
2018年5月3日(03.05.2018)



(10) 国際公開番号

WO 2018/079321 A1

(51) 国際特許分類:

A61B 5/04 (2006.01) A61B 5/0408 (2006.01)
A61B 5/0402 (2006.01) A61B 5/0478 (2006.01)

(21) 国際出願番号: PCT/JP2017/037344

(22) 国際出願日: 2017年10月16日(16.10.2017)

(25) 国際出願の言語: 日本語

(26) 国際公開の言語: 日本語

(30) 優先権データ:

特願 2016-207639 2016年10月24日(24.10.2016) JP

(71) 出願人: 日本電信電話株式会社 (NIPPON TELEGRAPH AND TELEPHONE CORPORATION) [JP/JP]; 〒1008116 東京都千代田区大手町一丁目5番1号 Tokyo (JP). 東レ株式会社(TORAY INDUSTRIES, INC.) [JP/JP]; 〒1038666 東京都中央区日本橋室町2丁目1番1号 Tokyo (JP).


(72) 発明者: 石原 隆子 (ISHIHARA, Takako); 〒1808585 東京都武蔵野市緑町3丁目9-1

1 NTT 知的財産センタ内 Tokyo (JP). 高河原 和彦(TAKAGAHARA, Kazuhiko); 〒1808585 東京都武蔵野市緑町3丁目9-1 1 NTT 知的財産センタ内 Tokyo (JP). 宝田 博美(TAKARADA, Hiromi); 〒1038666 東京都中央区日本橋室町2丁目1番1号 東レ株式会社東京事業場内 Tokyo (JP). 石川 恵美子(ISHIKAWA, Emiko); 〒5308222 大阪府大阪市北区中之島3丁目3番3号 東レ株式会社大阪事業場内 Osaka (JP). 佐藤 雅伸(SATO, Masanobu); 〒1038666 東京都中央区日本橋室町2丁目1番1号 東レ株式会社東京事業場内 Tokyo (JP). 村上 康晴(MURAKAMI, Yasuharu); 〒5308222 大阪府大阪市北区中之島3丁目3番3号 東レ株式会社大阪事業場内 Osaka (JP).

(74) 代理人: 山川 茂樹, 外(YAMAKAWA, Shigeki et al.); 〒1006104 東京都千代田区永田町2丁目11番1号 山王パークタワー4階 山川国際特許事務所内 Tokyo (JP).

(54) Title: WEARABLE ELECTRODE

(54) 発明の名称: ウェアラブル電極

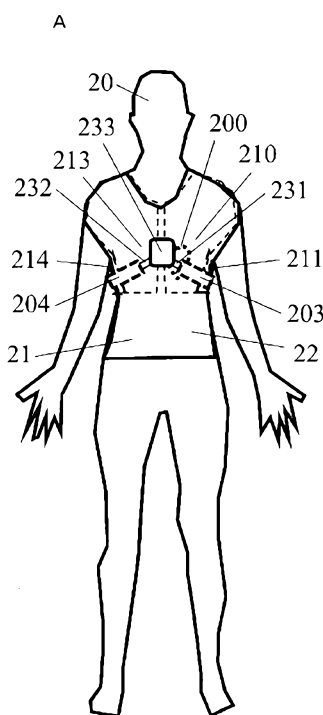

(57) Abstract: Provided is a wearable electrode, which is configured from an electrode (203) which is anchored to an article of clothing (21) so as to be capable of simultaneously making contact with all sites of skin from the ventral side to the dorsal side of the upper left-hand part of the body of a wearer (20), and an electrode (204) which is anchored to the article of clothing (21) so as to be capable of simultaneously making contact with all sites of skin from the ventral side to the dorsal side of the upper right-hand part of the body of the wearer (20). The electrodes (203, 204) are installed such that, with the wearer (20) in an upright standing state, the positions in which said electrodes (203, 204) are worn gradually descend from the ventral side to the dorsal side, or else, with the wearer (20) in the upright standing state, the positions in which said electrodes (203, 204) are worn gradually ascend from the ventral side to the dorsal side.

(57) 要約: ウェアラブル電極は、着用者(20)の左上半身の腹側から背側にかけての各部位の皮膚に同時に接触し得るように衣服(21)に固定された電極(203)と、着用者(20)の右上半身の腹側から背側にかけての各部位の皮膚に同時に接触し得るように衣服(21)に固定された電極(204)とから構成される。電極(203, 204)は、着用者(20)が直立の状態で腹側から背側にかけて装着位置が漸次下がるように、あるいは着用者(20)が直立の状態で腹側から背側にかけて装着位置が漸次上がるように設置される。

(81) 指定国(表示のない限り、全ての種類の国内保護が可能): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) 指定国(表示のない限り、全ての種類の広域保護が可能): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), ユーラシア (AM, AZ, BY, KG, KZ, RU, TJ, TM), ヨーロッパ (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

添付公開書類:

一 国際調査報告(条約第21条(3))

Specification
Wearable Electrode

Technical Field

5 [0001] The present invention relates to a wearable electrode to be used to acquire a bioelectric signal such as an electrocardiographic waveform on a daily basis.

Background Art

10 [0002] Recently, the importance of daily self-care of health is pointed out. One method of personal healthcare like this is to record and analyze bioelectric signals such as electrocardiographic waveforms for long time periods. This method is known
15 to be able to find disturbances of autonomic nerves and symptoms of heart diseases in early stages, and effective in preventive medicine. A garment to which a biological electrode is attached (a wearable electrode) in order to acquire bioelectric signals for long periods
20 of time is attracting attention (see non-patent literature 1).

Related Art Literature

Non-Patent Literature

[0003] Non-Patent Literature 1: David M.D. Riberio,
25 et al., "A Real time, Wearable ECG and Continuous Blood Pressure Monitoring System for First Responders", 33rd Annual International Conference of the IEEE EMBS, pp.

6894 - 6898, 2011

Disclosure of Invention

Problem to be Solved by the Invention

[0004] Figs. 7A to 7C are schematic views showing the
5 way a conventional wearable electrode is put on a human
body. Fig. 7A is a human body front view, Fig. 7B is a
human body side view, and Fig. 7C is a human body rear
view. In the conventional wearable electrode as shown
in Figs. 7A to 7C, biological electrodes 101 and 102 are
10 often installed in two, left and right portions of the
chest at the height of the heart muscle of a heart 100
of a wearer 110 (this height is near the central line of
the left ventricle, which is near the lower line of the
nipple in the case of a male).

15 [0005] Such a conventional wearable electrode,
however, has the following problems. That is, the
biological electrodes 101 and 102 are sometimes detached
from the body of the wearer when the wearer bends
forward, so that measurement of bioelectric signals
20 cannot be measured, or, the wearer feel unpleasant when
the biological electrodes 101 and 102 are fastened on
the body of the wearer by a flexible material so that
the biological electrodes 101 and 102 do not leave the
body.

25 [0006] It is an object of the present invention to
provide a wearable electrode capable of reducing the
unpleasant feeling of a wearer, and acquiring

bioelectric signals even when the wearer takes various postures.

Means of Solution to the Problem

[0007] According to the present invention, a wearable
5 electrode for detecting a bioelectric signal of a wearer
of a garment is characterized by including one or more
first electrodes fixed to the garment such that the
first electrodes can simultaneously come in contact with
skin of respective parts from a ventral side to a dorsal
10 side of an upper left part of a body of the wearer, and
one or more second electrodes fixed to the garment such
that the second electrodes can simultaneously come in
contact with skin of respective parts from a ventral
side to a dorsal side of an upper right part of the body
15 of the wearer, wherein the first electrodes and the
second electrodes are installed such that attaching
positions gradually descend from the ventral side to the
dorsal side with the wearer standing upright, or the
attaching positions gradually ascend from the ventral
20 side to the dorsal side with the wearer standing
upright.

Effect of the Invention

[0008] The present invention includes the first
electrodes fixed to the garment such that the first
25 electrodes can simultaneously come in contact with the
skin of respective parts from the ventral side to the
dorsal side of the upper left part of the body of the

wearer, and the second electrodes fixed to the garment such that the second electrodes can simultaneously come in contact with the skin of respective parts from the ventral side to the dorsal side of the upper right part of the body of the wearer. Even when the wearer bends forward, therefore, the bioelectric signal of the wearer can be acquired because at least a part of each of the first and second electrodes come in contact with the body of the wearer. Also, the present invention can reduce the unpleasant feeling of the wearer because it is unnecessary to tighten the body of the wearer by the first and second electrodes. Furthermore, in the present invention, the first and second electrodes are installed such that the attaching positions gradually descend from the ventral side to the dorsal side with the wearer standing upright, or the attaching positions gradually ascend from the ventral side to the dorsal side with the wearer standing upright. Accordingly, it is possible to reduce an impediment to expansion and compression of the garment around the waist of the wearer caused by the first and second electrodes, and further reduce the unpleasant feeling of the wearer.

Brief Description of Drawings

[0009] Figs. 1A to 1C are schematic views showing the way a wearable electrode according to the first embodiment of the present invention is put on a human body;

Fig. 2 is a graph showing the tension per unit width of the chest, which is necessary to measure the heartbeat, when using the wearable electrode according to the first embodiment of the present invention and a
5 conventional wearable electrode;

Fig. 3 is a view for explaining an example of a method of putting the wearable electrode according to the first embodiment of the present invention on a human body;

10 Fig. 4 is a graph showing the tension per unit width of the chest, which is necessary to measure the heartbeat, when using the wearable electrode according to the first embodiment of the present invention and a wearable electrode in which electrodes are horizontally
15 arranged;

Fig. 5 is a view for explaining the wearable electrode in which the electrodes are horizontally arranged;

Figs. 6A to 6C are schematic views showing the
20 way a wearable electrode according to the second embodiment of the present invention is put on a human body; and

Figs. 7A to 7C are schematic views showing the way a conventional wearable electrode is put on a human
25 body.

Best Mode for Carrying Out the Invention

[0010] The present invention will be explained below

by referring to preferred embodiments, but the present invention is not limited to these embodiments.

[0011] [First Embodiment]

Figs. 1A to 1C are schematic views showing the way a wearable electrode according to the first embodiment of the present invention is put on a human body. Fig. 1A is a front view of a human body, Fig. 1B is a side view of the human body, and Fig. 1C is a rear view of the human body. As shown in Figs. 1A to 1C, the wearable electrode of this embodiment includes a garment 21, one or more belt-like electrodes 203, and one or more belt-like electrodes 204. The electrodes 203 are fixed to the inside of the garment 21 (the side in contact with the skin of a wearer 20 (a living body) of the garment 21), so that the electrodes 203 simultaneously come in contact with the skin of a left breast 210 of the wearer 20 of the garment 21, the skin of at least one (211 in Fig. 1A) of the left side chest, the left hypochondriac region, and the left armpit of the wearer 20, and the skin of at least one (212 in Fig. 1C) of the dorsal side of the left side chest, the dorsal side of the left hypochondriac region, and the lower portion of the left scapular region of the wearer 20, and the attaching positions gradually descend from the ventral side to the dorsal side with the wearer 20 standing upright. The electrodes 204 are fixed to the inside of the garment 21, so that the electrodes 204

simultaneously come in contact with the skin of a right breast 213 of the wearer 20 of the garment 21, the skin of at least one (214 in Fig. 1A) of the right side chest, the right hypochondriac region, and the right armpit of the wearer 20, and the skin of at least one (215 in Fig. 1C) of the dorsal side of the right side chest, the dorsal side of the right hypochondriac region, and the lower portion of the right scapular region of the wearer 20, and the attaching positions gradually descend from the ventral side to the dorsal side with the wearer 20 standing upright. Figs. 1A to 1C also depict a heart 200 of the wearer 20.

[0012] Note that the armpit means a so-called underarm region, the side chest means a region below the armpit, and the hypochondriac region means a region below the side chest. Note also that the lower portion of the scapular region means a region below the scapular region having the scapula. The names of the individual parts of the human body are disclosed in, e.g., reference literature 'Shoji Hashimoto, "Introduction to Nursing 1 Mechanism and Work of Human Body", pp. 3 - 8, 2013'.

[0013] The electrodes 203 and 204 are respectively connected to a biological signal acquisition apparatus 233 by interconnections 231 and 232. Of the one or more electrodes 203 and the one or more electrodes 204, some of them are positive electrodes, and the rest are

negative electrodes.

[0014] A material of the electrodes 203 and 204 is not particularly limited, and it is possible to unlimitedly use a carbon filler mixed resin, Ag cloth, 5 conductive polymer impregnated fabric, and fabric impregnated with an electrolyte. The conductive polymer impregnated fabric is favorable because stimulation to the skin in a tight contact state is low and the durability is high. Also, the size of the electrodes 10 203 and 204 is not particularly limited as long as the installation conditions explained with reference to Figs. 1A to 1C are met.

[0015] Note that a reference potential often used when receiving a bioelectric signal may also be obtained 15 by installing an additional reference electrode on the garment 21 so that the reference electrode does not come in contact with the abovementioned positive and negative electrodes, and connecting the reference electrode to the biological signal acquisition apparatus 233 via an 20 interconnection. In this case, of the one or more electrodes 203 separated from each other and the one or more electrodes 204 separated from each other, some are positive electrodes, and some are negative electrodes, and the electrode 203 or the electrode 204 other than 25 the electrodes that function as the positive electrodes and the negative electrodes is the reference electrode.

Furthermore, the reference potential may also

be an intermediate potential obtained from signals received by the positive electrode and the negative electrode, or the GND potential of the circuit of the biological signal acquisition apparatus 233.

5 [0016] The garment 21 is not particularly limited as long as the electrodes 203 and 204 can be installed, and it is possible to take forms such as a stomach band, a belt, and a corset, in addition to a shirt shown in Figs. 1A to 1C.

10 When the garment 21 is a shirt as shown in Figs. 1A to 1C, the body including a part below the neck and the scapular regions is wrapped up, so the electrodes 203 and 204 are arranged and maintained in more appropriate positions.

15 [0017] The electrodes 203 and 204 are arranged on the inside of a front body 22 of the garment 21. The electrodes 203 and 204 extend from the ventral side to the dorsal side so as to go round nearly the half of the body surface of the wearer 20. Accordingly, a part from
20 the armpit to the abdomen of the front body 22 is extended toward the dorsal side from a center 26 of the armhole of the garment 21 so as to accommodate the dorsal-side distal ends of the electrodes 203 and 204. In accordance with this extension of the front body 22,
25 therefore, a part from the armpit to the abdomen of a back body 23 of the garment 21 to be sewed up to the front body 22 is restricted in the direction of the

posterior median line of the wearer 20 from the center
26 of the armhole, so a width W2 of this part is smaller
than a body width W1. Consequently, sewing lines 24 and
25 of the front body 22 and the back body 23 are
5 arranged nearer the dorsal side than the body-side
barycentric line of the wearer 20.

[0018] As the material of the garment 21, it is
possible to unlimitedly use natural fiber materials such
as cotton and wool and synthetic fiber materials such as
10 polyester and nylon used in ordinary clothes. However,
the present invention is not limited to the shapes and
materials of the garment 21 as described above.

[0019] Examples of the method of fixing the
electrodes 203 and 204 to the garment 21 are a method of
15 sewing the electrodes 203 and 204 to the garment 21, a
method of adhering the electrodes 203 and 204 to the
garment 21, and a method of impregnating the garment 21
with the electrodes 203 and 204. Of these methods, the
adhesion method is particularly easy. It is also
20 possible to bond the electrodes 203 and 204 to the front
body 22 or the back body 23 of the garment 21 by
thermocompression bonding by using an iron or a hot
press machine before sewing the garment 21, and sew the
front body 22 and the back body 23 after that.

25 [0020] As the interconnections 231 and 232, although
well-known wiring materials can unlimitedly be used, it
is more desirable to use a flexible wiring material

(e.g., conductive rubber), or a material having a flexible structure or layout such as a spring, since the interconnections 231 and 232 are installed on the garment 21 which deforms in accordance with the motion
5 of the wearer 20.

[0021] Also, the interconnections 231 and 232 are desirably covered with an insulator so as not to acquire signals from, e.g., the human body other than the electrode installation portions. Like the electrodes
10 203 and 204, the interconnections 231 and 232 are fixed to the front body 22 of the garment 21 such that the attaching positions gradually descend from the end portions on the side of the biological signal acquisition apparatus 233 to the end portions on the
15 side of the electrodes 203 and 204, with the wearer 20 standing upright. Examples of the method of fixing the interconnections 231 and 232 to the garment 21 are a method of sewing the interconnections 231 and 232 to the garment 21, and a method of adhering the
20 interconnections 231 and 232 to the garment 21.

[0022] In this embodiment, the electrodes 203 and 204 do not cross the sewing lines 24 and 25 because the electrodes 203 and 204 and the interconnections 231 and 232 are fixed to the front body 22 of the garment 21.
25 As a consequence, the garment 21 fits the three-dimensional body structure, and the electrodes 203 and 204 hardly get out of positions. In addition, the

electrodes 203 and 204 and the interconnections 231 and 232 can be installed on the front body 22 before sewing the garment 21, and this facilitates the sewing step.

[0023] The biological signal acquisition apparatus 233 acquires and processes a bioelectric signal (in this embodiment, an electrocardiographic waveform) detected by the electrodes 203 and 204. As the biological signal acquisition apparatus 233, it is possible to unlimitedly use a well-known apparatus that acquires an electrocardiographic waveform and detects an R wave. The biological signal acquisition apparatus 233 has a function of detecting the heartbeat from the electrocardiographic waveform, various display functions, and a function of wirelessly transmitting the acquired bioelectric signal and heartbeat information to the outside. Also, the biological signal acquisition apparatus 233 can be fixed on either the inside or the outside (the side opposite to the side in contact with the skin of the wearer 20) of the garment 21.

[0024] In this embodiment as described previously, however, the positions of the end portions of the interconnections 231 and 232 on the side of the electrodes 203 and 204 must be obliquely below the positions of the end portions of the interconnections 231 and 232 on the side of the biological signal acquisition apparatus 233, with the wearer 20 standing upright. Therefore, the position of the biological

signal acquisition apparatus 233 must be determined so as to implement the layout of the interconnections 231 and 232 like this.

[0025] Fig. 2 shows the results of measurement of the tension of the chest necessary to measure the heartbeat, when the same wearer wore the conventional wearable electrode (Fig. 7) in which electrodes were installed in two, left and right portions of the chest at the height of the heart of the wearer and the wearable electrode of this embodiment in turn, and walked at 4 km per hour. In Fig. 2, the lowest value of the tension per unit width (1 cm) around the waist when normal heartbeat measurement was successful is taken as the measurement result. Also, as shown in Fig. 3, the electrodes 203 and 204 of the wearable electrode of this embodiment made an angle θ of 30° with a horizontal plane 27 when the wearer 20 was standing upright.

[0026] Referring to Fig. 2, tension 300 was necessary to measure the heartbeat when using the conventional wearable electrode, and tension 301 was necessary to measure the heartbeat when using the wearable electrode of this embodiment. As shown in Fig. 2, compared to the conventional wearable electrode, this embodiment reduces the tension of the chest necessary to measure the heartbeat, and hence can reduce the unpleasant feeling of the wearer.

[0027] Fig. 4 shows the results of measurement of the

tension of the chest when the same wearer wore the wearable electrode in which the electrodes 203 and 204 were horizontally arranged on the garment 21 and the wearable electrode of this embodiment in turn. In Fig. 4, the tension per unit width (1 cm) around the waist when the around-the-waist dimension of the chest on which the electrodes 203 and 204 were arranged was extended by 20% is taken as the measurement result. As shown in Fig. 3, the electrodes 203 and 204 of the wearable electrode of this embodiment made an angle θ of 30° with the horizontal line 27 when the wearer 20 was standing upright. As shown in Fig. 5, the wearable electrode in which the electrodes 203 and 204 are horizontally arranged is an electrode in which the horizontal plane 27 and the extending direction of the electrodes 203 and 204 are parallel (θ is 0°) when the wearer 20 was standing upright.

[0028] Referring to Fig. 4, tension 400 was obtained when using the wearable electrode in which the electrodes 203 and 204 were horizontally arranged, and tension 401 was obtained when using the wearable electrode of this embodiment.

Fig. 4 shows that this embodiment can reduce the tension of the chest and the unpleasant feeling of the wearer by obliquely installing the electrodes 203 and 204, compared to the wearable electrode in which the electrodes 203 and 204 are horizontally installed.

[0029] In this embodiment as described above, the electrode 203 is so installed as to simultaneously come in contact with the skin in respective parts from the ventral side to the dorsal side of the upper left part of the body of the wearer, and the electrode 204 is so installed as to simultaneously come in contact with the skin in respective parts from the ventral side to the dorsal side of the upper right part of the body of the wearer. Even when the wearer is bending forward, therefore, at least a part of each of the electrodes 203 and 204 comes in contact with the body of the wearer, so the bioelectrical signal of the wearer can be acquired. Also, this embodiment does not adopt a structure that tightens the body of the wearer by the electrodes 203 and 204, and hence can reduce the unpleasant feeling of the wearer. Furthermore, the electrodes 203 and 204 and the interconnections 231 and 232 are installed obliquely to the horizontal plane with the wearer standing upright. Therefore, even when materials having flexibility lower than that of the material of the garment 21 are used as the electrodes 203 and 204 and the interconnections 231 and 232, it is possible to reduce an impediment to expansion and contraction of the garment 21 around the waist caused by the electrodes 203 and 204 and the interconnections 231 and 232, and reduce the unpleasant feeling of the wearer.

[0030] [Second Embodiment]

Next, the second embodiment of the present invention will be explained. Figs. 6A to 6C are schematic views showing the way a wearable electrode according to the second embodiment of the present invention is put on a human body. Fig. 6A is a human body front view, Fig. 6B is a human body side view, and Fig. 6C is a human body rear view. As shown in Figs. 6A to 6C, the wearable electrode of this embodiment includes a garment 21a, one or more belt-like electrodes 203a, and one or more belt-like electrodes 204a. The electrodes 203a are fixed to the inside of the garment 21a, so that the electrodes 203 simultaneously come in contact with the skin of at least one of the ventral side of the left side chest and the ventral side of the left hypochondriac region of a wearer 20 of the garment 21a, the skin of at least one (211 in Fig. 6A) of the left side chest, the left hypochondriac region, and the left armpit of the wearer 20, and the skin of at least one (216 in Fig. 6C) of the dorsal side of the left side chest and the left scapular region of the wearer 20, and the attaching positions gradually ascend from the ventral side to the dorsal side with the wearer 20 standing upright. The electrodes 204a are fixed to the inside of the garment 21a, so that the electrodes 204a simultaneously come in contact with the skin of at least one of the ventral side of the right side chest and the ventral side of the right hypochondriac region of the

wearer 20 of the garment 21a, the skin of at least one (214 in Fig. 6A) of the right side chest, the right hypochondriac region, and the right armpit of the wearer 20, and the skin of at least one (217 in Fig. 6C) of the dorsal side of the right side chest and the right scapular region of the wearer 20, and the attaching positions gradually ascend from the ventral side to the dorsal side with the wearer 20 standing upright.

[0031] The electrodes 203a and 204a are respectively connected to a biological signal acquisition apparatus 233 by interconnections 231a and 232a. When using a reference electrode, the electrode 203a or 204a other than the electrodes 203a and 204a that function as positive electrodes and negative electrodes can be used as the reference electrode, as in the first embodiment.

[0032] The electrodes 203a and 204a are made of the same material as the electrodes 203 and 204 of the first embodiment, but are arranged on the inside of a back body 23a of the garment 21a. In this embodiment, the electrodes 203a and 204a extend from the dorsal side to the ventral side so as to go round nearly the half of the body surface of the wearer 20. Accordingly, a part from the armpit to the abdomen of the back body 23a is extended toward the ventral side from a center 26 of the armhole of the garment 21a so as to accommodate the ventral-side distal ends of the electrodes 203a and 204a. In accordance with this extension of the back

body 23a, therefore, a part from the armpit to the abdomen of a front body 22a of the garment 21a to be sewed up to the back body 23a is restricted in the direction of the anterior median line of the wearer 20

5 from the center 26 of the armhole, so a width W3 of this part is smaller than a body width W1. Consequently, sewing lines 24a and 25a of the front body 22a and the back body 23a are arranged nearer the ventral side than the body-side barycentric line of the wearer 20.

10 [0033] Like the electrodes 203a and 204a, the interconnections 231a and 232a are fixed to the back body 23a of the garment 21a such that the attaching positions gradually descend from the end portions on the side of the biological signal acquisition apparatus 233

15 to the end portions on the side of the electrodes 203a and 204a, with the wearer 20 standing upright.

[0034] In this embodiment, the electrodes 203a and 204a do not cross the sewing lines 24a and 25a because the electrodes 203a and 204a and the interconnections

20 231a and 232a are fixed to the back body 23a of the garment 21a. As a consequence, the garment 21a fits the three-dimensional body structure, and the electrodes 203a and 204a hardly get out of positions. In addition, the electrodes 203a and 204a and the interconnections

25 231a and 232a can be installed on the back body 23a before sewing the garment 21a, and this facilitates the sewing step. Furthermore, in this embodiment, the

interconnections 231 and 232 and the biological signal acquisition apparatus 233 need not be installed on the ventral side. Accordingly, the garment 21a can be front-open garment, and this can facilitate dressing and undressing.

[0035] In the first embodiment and this embodiment, the method of fixing the electrodes 203, 203a, 204, and 204a and the interconnections 231, 231a, 232, and 232a to the front body 22 or the back body 23a is not particularly limited, and an arbitrary method can be used. Especially when performing fixation by thermocompression bonding, if the electrodes 203, 203a, 204, and 204a and the interconnections 231, 231a, 232, and 232a do not cross the sewed portions as in the first embodiment and this embodiment, the compression-bonding surface is flat, so the front body or back body before sewing in which members to be compression-bonded are arranged can be placed on the plate of a hot press machine normally used in thermocompression bonding.

This not only facilitates forming the garment 21 and 21a, but also improves the durability of adhesion because the electrodes 203, 203a, 204, and 204a and the interconnections 231, 231a, 232, and 232a can evenly be adhered on the entire surface.

[0036] The function of the biological signal acquisition apparatus 233 is the same as explained in the first embodiment. In this embodiment, however, the

positions of the end portions of the interconnections 231a and 232a on the side of the electrodes 203a and 204a must be obliquely below the positions of the end portions of the interconnections 231a and 232a on the side of the biological signal acquisition apparatus 233, with the wearer 20 standing upright. Therefore, the position of the biological signal acquisition apparatus 233 must be so determined as to be able to implement the layout of the interconnections 231a and 232a as described above.

[0037] The rest of the arrangement is the same as explained in the first embodiment. Thus, this embodiment can achieve the same effect as that of the first embodiment.

[0038] Note that in the first and second embodiments, the electrode shape is an almost rectangular shape in planar view when the electrode is not fixed to a garment but stretched flat. However, the present invention is not limited to this, and it is also possible to adopt an electrode shape that is an almost elliptical shape when the electrode is stretched flat.

Note also that the biological signal acquisition apparatus 233 may also have a structure that can detachably be attached to the garment 21 and 21a. In this case, the biological signal acquisition apparatus 233 and the interconnections 231, 231a, 232, and 232a are electrically connected via connectors.

Industrial Applicability

[0039] The present invention is applicable to a technique of acquiring a bioelectric signal.

Explanation of the Reference Numerals and Signs

5 [0040] 20...wearer, 21, 21a...garment, 22, 22a...front body of a garment, 23, 23a...back body of garment, 24, 24a, 25, 25a...sewing line of front or back body, 26...center of armhole, 200...heart, 203, 203a, 204, 204a...electrode, 210...left breast, 211...at least
10 one of left side chest, left hypochondriac region, and left armpit, 212...at least one of dorsal side of left side chest, dorsal side of left hypochondriac region, and lower portion of left scapular region, 213...right breast, 214...at least one of right side chest, right
15 hypochondriac region, and right armpit, 215...at least one of dorsal side of right side chest, dorsal side of right hypochondriac region, and lower portion of right scapular region, 216...at least one of dorsal side of left side chest and left scapular region, 217...at least
20 one of dorsal side of right side chest and right scapular region, 231, 231a, 232, 232a...interconnection, 233...biological signal acquisition apparatus

C L A I M S

1. A wearable electrode for detecting a
2 bioelectric signal of a wearer of a garment,
3 characterized by comprising:
4 one or more first electrodes fixed to the
5 garment such that the first electrodes can
6 simultaneously come in contact with skin of respective
7 parts from a ventral side to a dorsal side of an upper
8 left part of a body of the wearer; and
9 one or more second electrodes fixed to the
10 garment such that the second electrodes can
11 simultaneously come in contact with skin of respective
12 parts from a ventral side to a dorsal side of an upper
13 right part of the body of the wearer,
14 wherein the first electrodes and the second
15 electrodes are installed such that attaching positions
16 gradually descend from the ventral side to the dorsal
17 side with the wearer standing upright, or the attaching
18 positions gradually ascend from the ventral side to the
19 dorsal side with the wearer standing upright.

2. The wearable electrode according to claim
2 1, characterized in that
3 the first electrodes are fixed to the garment
4 such that the first electrodes can simultaneously come
5 in contact with skin of a left breast of the wearer,
6 skin of at least one of a left side chest, a left
7 hypochondriac region, and a left armpit of the wearer,

8 and skin of at least one of the dorsal side of the left
9 side chest, the dorsal side of the left hypochondriac
10 region, and a lower portion of a left scapular region of
11 the wearer, and the attaching positions gradually
12 descend from the ventral side to the dorsal side with
13 the wearer standing upright, and

14 the second electrodes are fixed to the garment
15 such that the second electrodes can simultaneously come
16 in contact with skin of a right breast of the wearer,
17 skin of at least one of a right side chest, a right
18 hypochondriac region, and a right armpit of the wearer,
19 and skin of at least one of the dorsal side of the right
20 side chest, the dorsal side of the right hypochondriac
21 region of the wearer, and a lower portion of a right
22 scapular region, and the attaching positions gradually
23 descend from the ventral side to the dorsal side with
24 the wearer standing upright.

3. The wearable electrode according to claim
2 2, characterized by further comprising a first
3 interconnection and a second interconnection configured
4 to electrically connect a biological signal acquisition
5 apparatus for acquiring the bioelectric signal of the
6 wearer and the first electrodes and the second
7 electrodes,

8 wherein the first interconnection and the
9 second interconnection are fixed to the garment such
10 that when the biological signal acquisition apparatus is

11 fixed to the ventral side of the garment, the attaching
12 positions gradually descend from end portions on a side
13 of the biological signal acquisition apparatus to end
14 portions on a side of the first electrodes and the
15 second electrodes, with the wearer standing upright.

4. The wearable electrode according to claim
2 3, characterized in that the first electrodes, the
3 second electrodes, the first interconnection, and the
4 second interconnection are fixed to a front body of the
5 garment.

5. The wearable electrode according to claim
2 1, characterized in that
3 the first electrodes are fixed to the garment
4 such that the first electrodes can simultaneously come
5 in contact with skin of at least one of the ventral side
6 of the left side chest and the ventral side of the left
7 hypochondriac region of the wearer, skin of at least one
8 of the left side chest, the left hypochondriac region,
9 and the left armpit of the wearer, and skin of at least
10 one of the dorsal side of the left side chest and the
11 left scapular region of the wearer, and the attaching
12 positions gradually ascend from the ventral side to the
13 dorsal side with the wearer standing upright, and
14 the second electrodes are fixed to the garment
15 such that the second electrodes can simultaneously come
16 in contact with skin of at least one of the ventral side
17 of the right side chest and the ventral side of the

18 right hypochondriac region of the wearer, skin of at
19 least one of the right side chest, the right
20 hypochondriac region, and the right armpit of the
21 wearer, and skin of at least one of the dorsal side of
22 the right side chest and the right scapular region of
23 the wearer, and the attaching positions gradually ascend
24 from the ventral side to the dorsal side with the wearer
25 standing upright.

6. The wearable electrode according to claim
2 5, characterized by further comprising a first
3 interconnection and a second interconnection configured
4 to electrically connect a biological signal acquisition
5 apparatus for acquiring the bioelectric signal of the
6 wearer and the first electrodes and the second
7 electrodes,

8 wherein the first interconnection and the
9 second interconnection are fixed to the garment such
10 that when the biological signal acquisition apparatus is
11 fixed to the dorsal side of the garment, the attaching
12 positions gradually descend from end portions on a side
13 of the biological signal acquisition apparatus to end
14 portions on a side of the first electrodes and the
15 second electrodes, with the wearer standing upright.

7. The wearable electrode according to claim
2 6, characterized in that the first electrodes, the
3 second electrodes, the first interconnection, and the
4 second interconnection are fixed to a back body of the

5 garment.

8. The wearable electrode according to any
2 one of claims 1 to 7, characterized in that, some of one
3 or more of the first electrodes separated from each
4 other and one or more of the second electrodes separated
5 from each other, are positive electrodes, some of the
6 other are negative electrodes, and the first electrode
7 and the second electrodes which are other than the
8 electrodes that function as the positive electrodes or
9 the negative electrodes functions are reference
10 electrodes.

FIG.1A

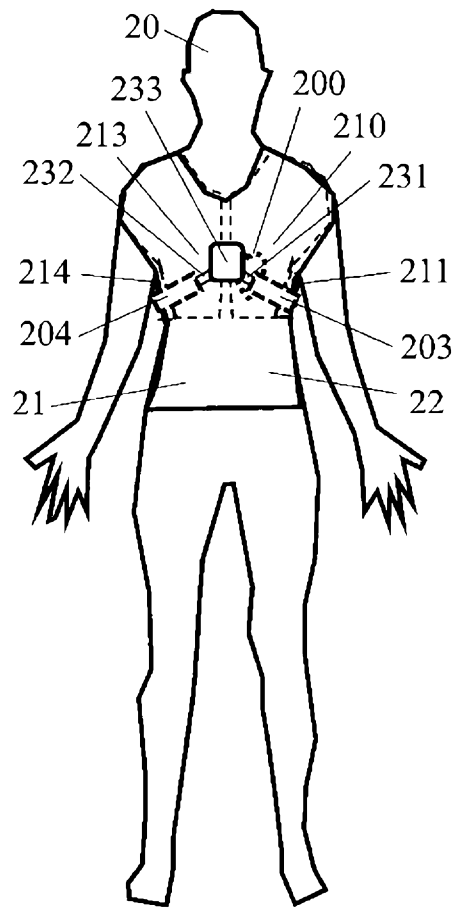


FIG.1B

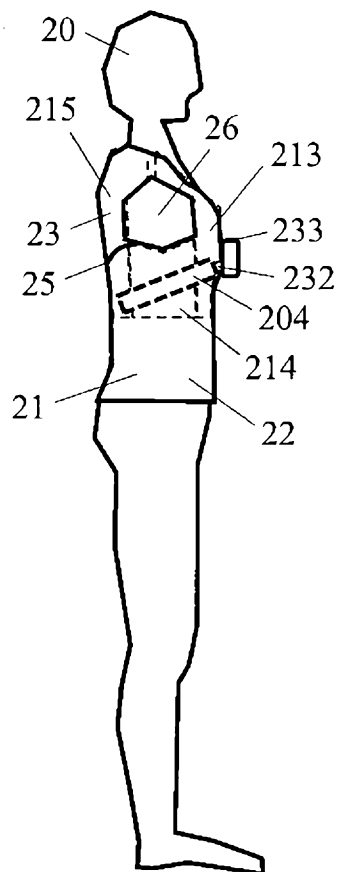
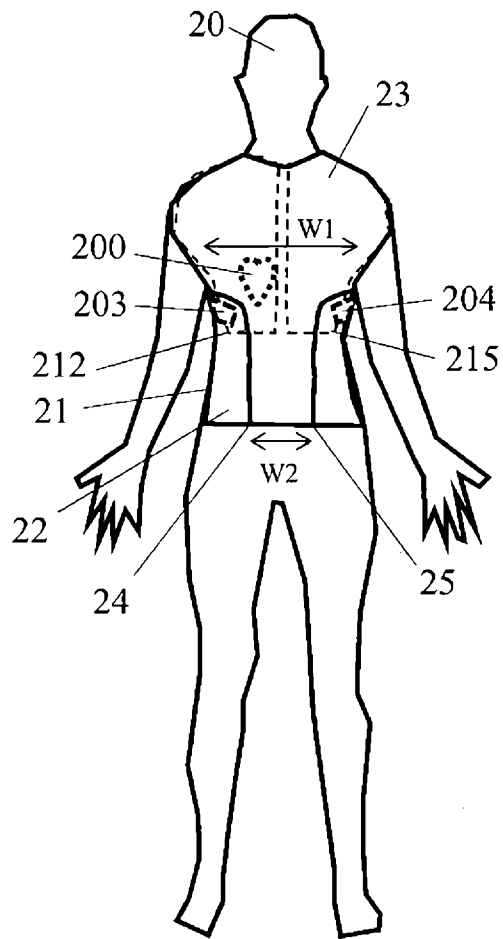


FIG.1C



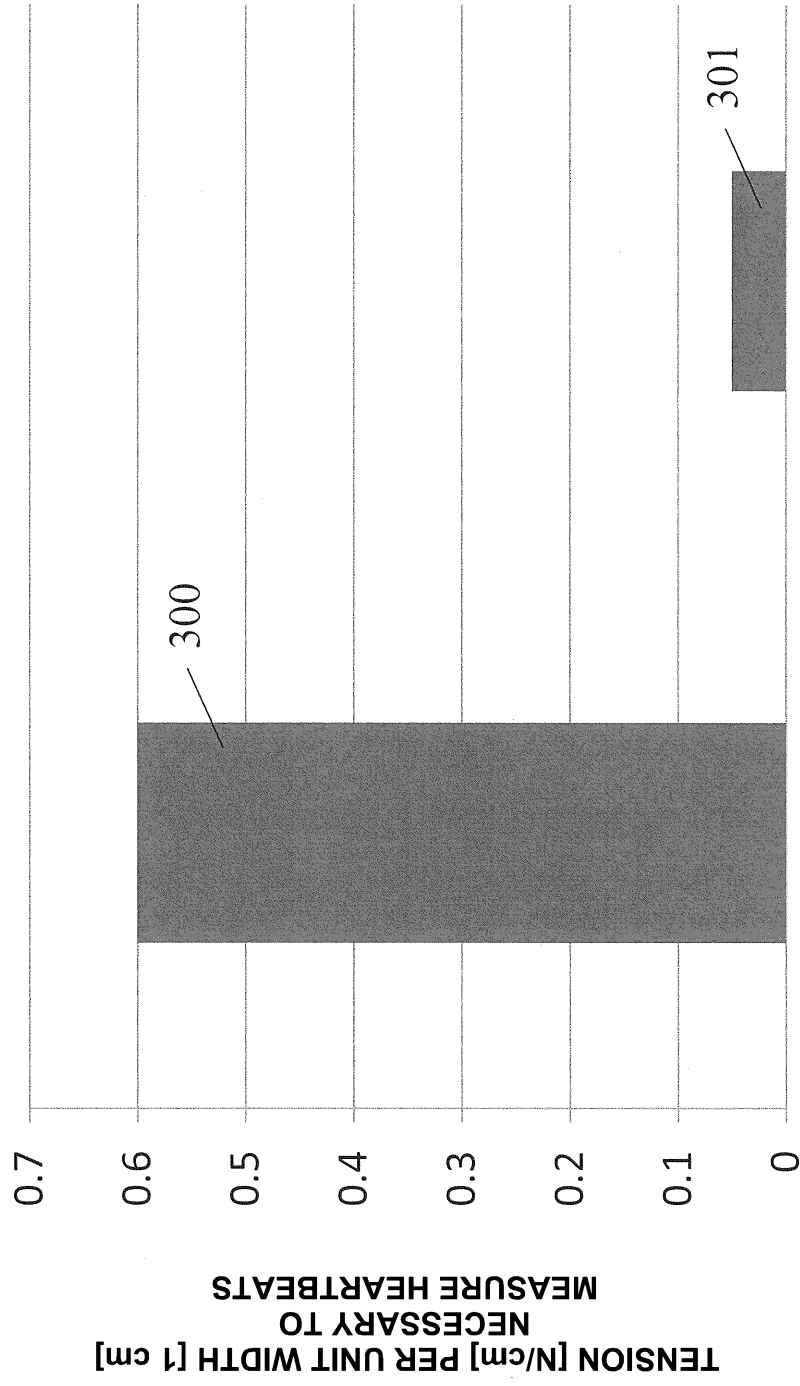
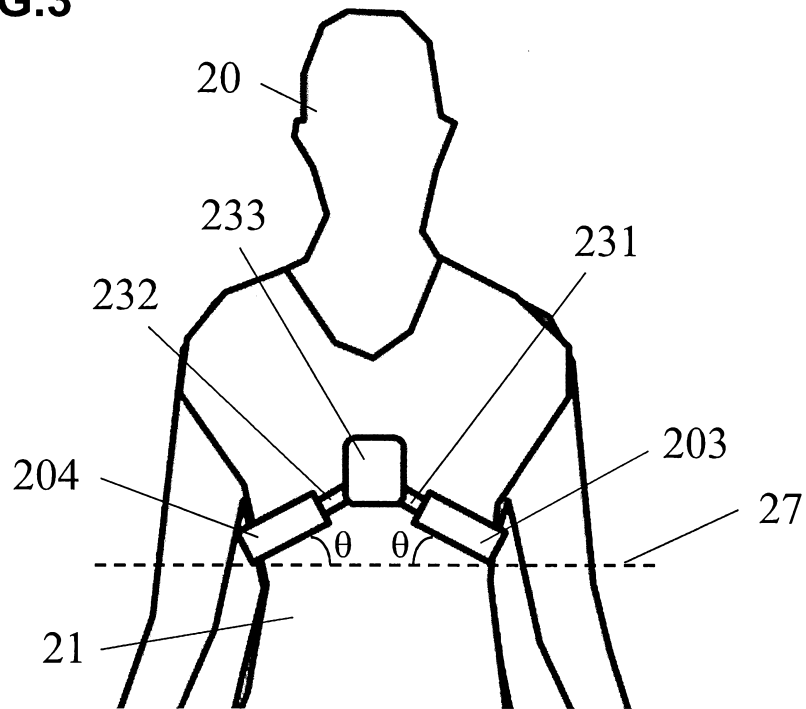


FIG.2

FIG.3



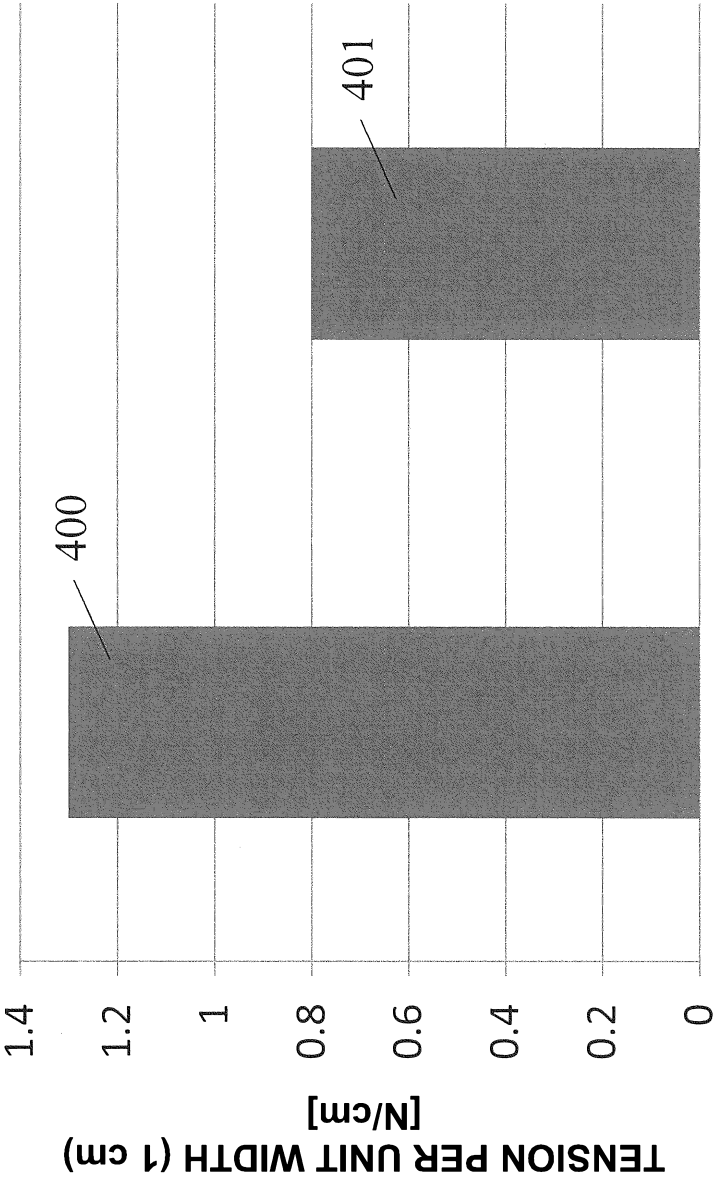


FIG.4

FIG.5

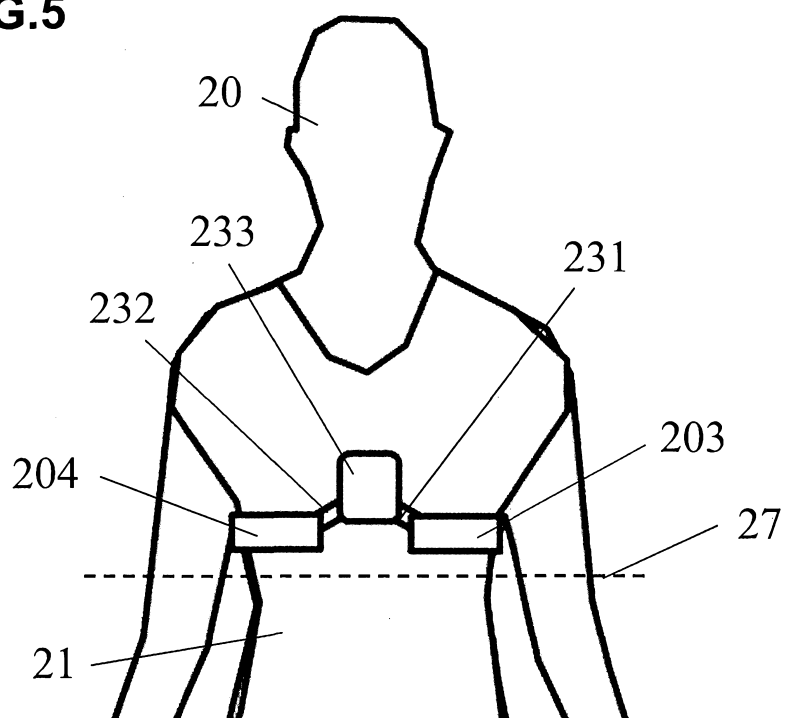


FIG.6A

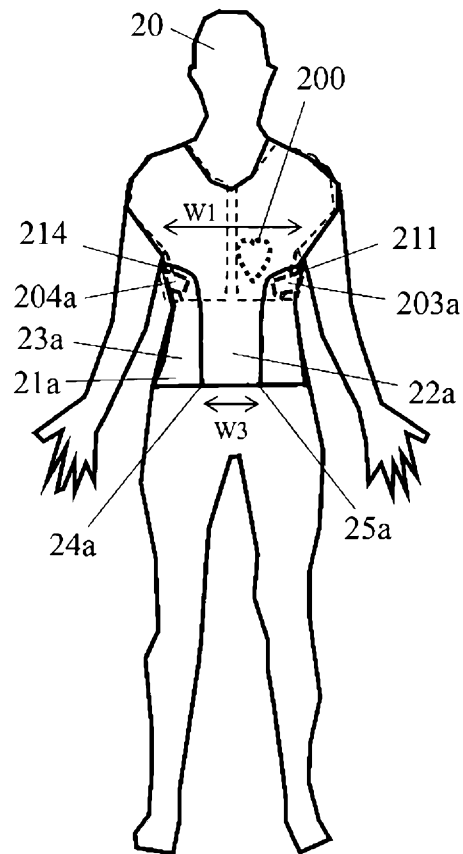


FIG.6B

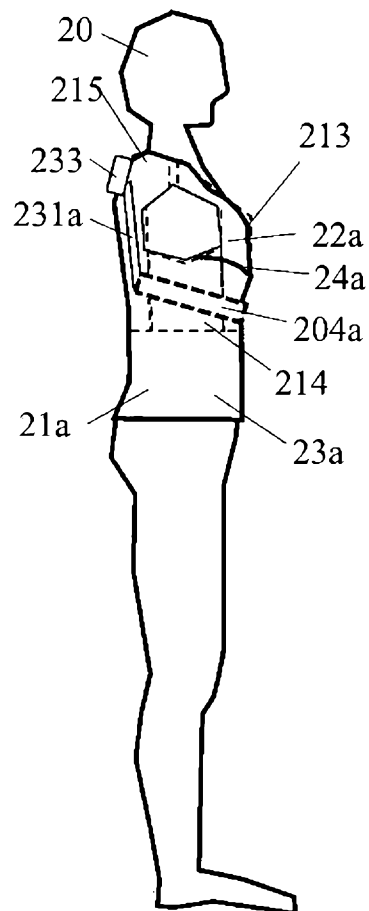


FIG.6C

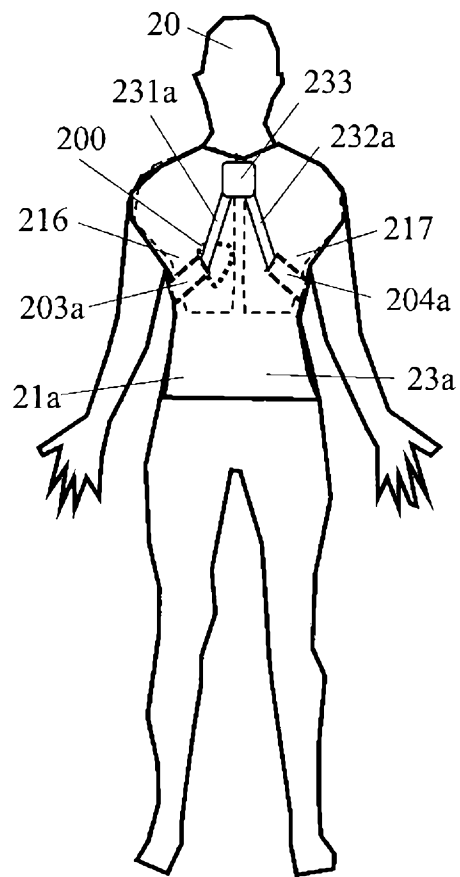


FIG.7A

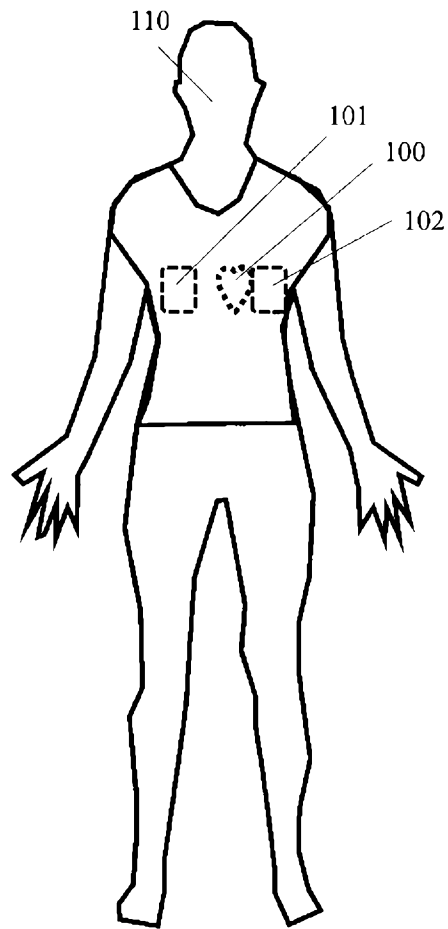


FIG.7B



10/10

FIG.7C

