



US00D942012S

(12) **United States Design Patent**
Nacev et al.

(10) **Patent No.:** US D942,012 S
(45) **Date of Patent:** ** Jan. 25, 2022

- (54) **ANALYTICAL DEVICE**
- (71) Applicant: **Promaxo, Inc.**, Oakland, CA (US)
- (72) Inventors: **Aleksandar Nacev**, San Francisco, CA (US); **Amit Vohra**, Rocklin, CA (US); **Ryan Hilaman**, Oakland, CA (US); **Said Ijanaten**, Bethesda, MD (US)
- (73) Assignee: **Promaxo, Inc.**, Oakland, CA (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/744,371**
- (22) Filed: **Jul. 28, 2020**

D639,948 S	6/2011	Personnelli	
D658,294 S	4/2012	Awad	
D665,911 S	8/2012	Laukkanen	
D726,917 S	4/2015	Kim	
D742,523 S	11/2015	Sui	
D757,939 S	5/2016	Tsujita et al.	
D783,830 S	4/2017	Baba	
D804,031 S	11/2017	Hsu et al.	
D817,494 S	5/2018	Apetauer et al.	
D857,203 S	8/2019	Kim et al.	
D890,927 S *	7/2020	Chong	D24/158
D893,725 S *	8/2020	You	D24/158
2017/0325763 A1	11/2017	Hoernig et al.	
2018/0252782 A1*	9/2018	You	G01R 33/34007

* cited by examiner

Primary Examiner — Anhdao Doan
(74) *Attorney, Agent, or Firm* — K&L Gates LLP

Related U.S. Application Data

- (62) Division of application No. 29/681,014, filed on Feb. 21, 2019, now Pat. No. Des. 895,803.
- (51) **LOC (13) Cl.** **24-01**
- (52) **U.S. Cl.**
USPC **D24/158**
- (58) **Field of Classification Search**
USPC D24/107, 158–160, 185–187
CPC G01N 2223/1016; G01N 2223/301; G01N 2223/031; G01N 2223/419; G01N 23/046; G01R 33/48; A61B 5/055
See application file for complete search history.

References Cited

U.S. PATENT DOCUMENTS

- D557,418 S 12/2007 Onuma et al.
- D591,862 S * 5/2009 Taniguchi D24/158

(57) **CLAIM**

The ornamental design for an analytical device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an analytical device of our new design.

FIG. 2 is a front view of the analytical device of FIG. 1.

FIG. 3 is a back view of the analytical device of FIG. 1.


FIG. 4 is a side view of the analytical device of FIG. 1.

FIG. 5 is another side view of the analytical device of FIG. 1.

FIG. 6 is a top view of the analytical device of FIG. 1; and, FIG. 7 is a bottom view of the analytical device of FIG. 1.

The broken lines illustrate portions of the analytical device that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

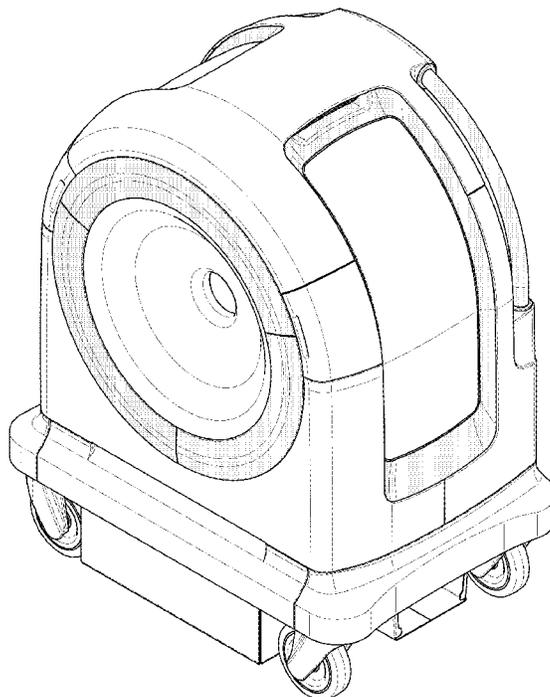

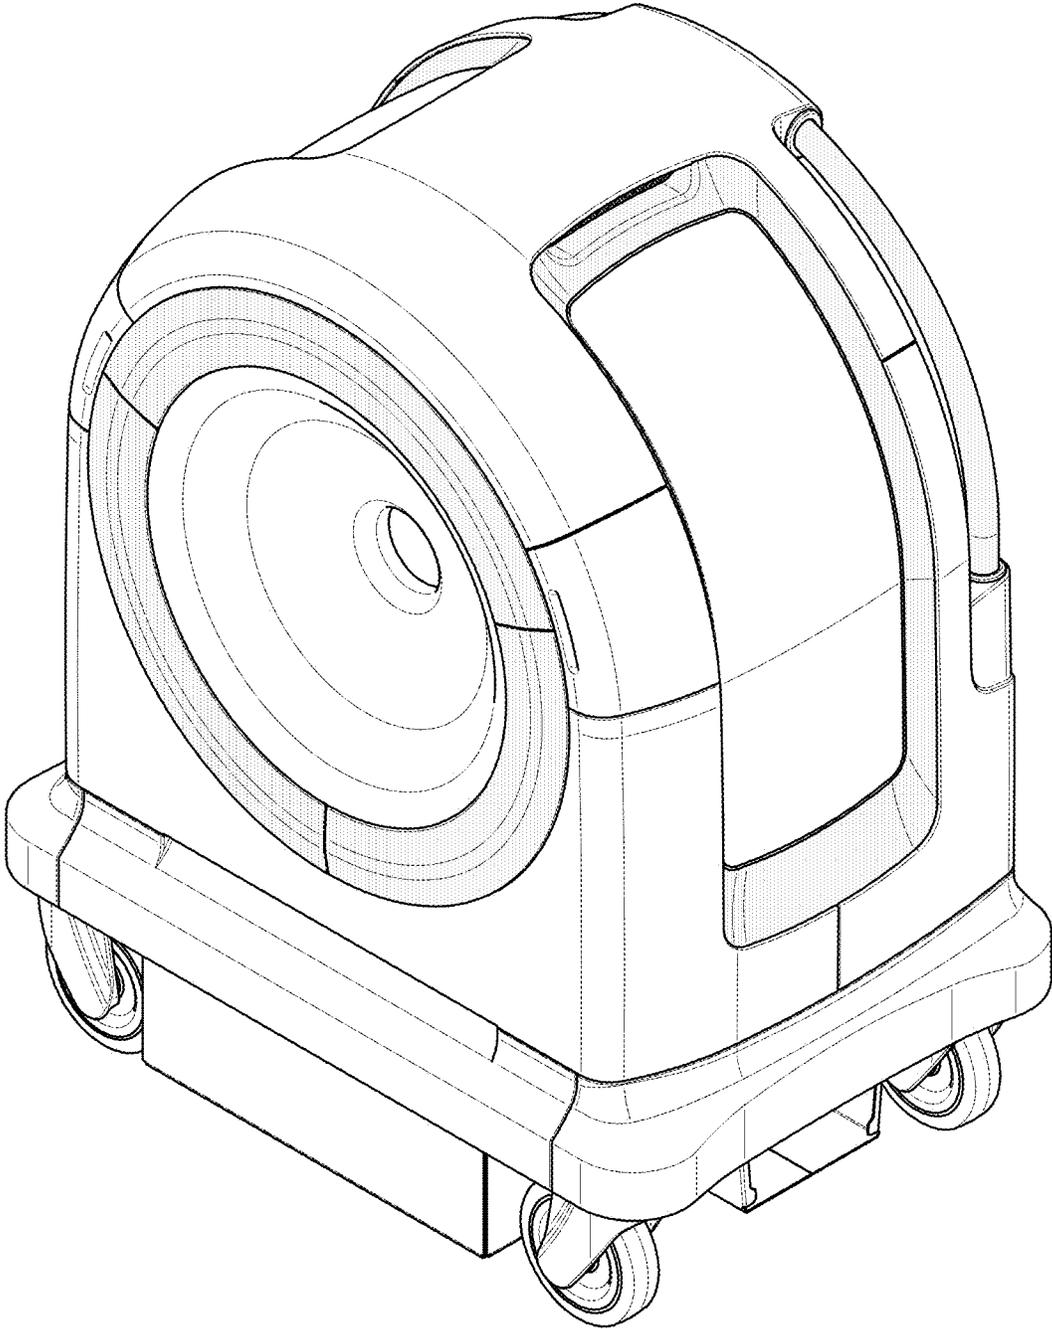


FIG. 1

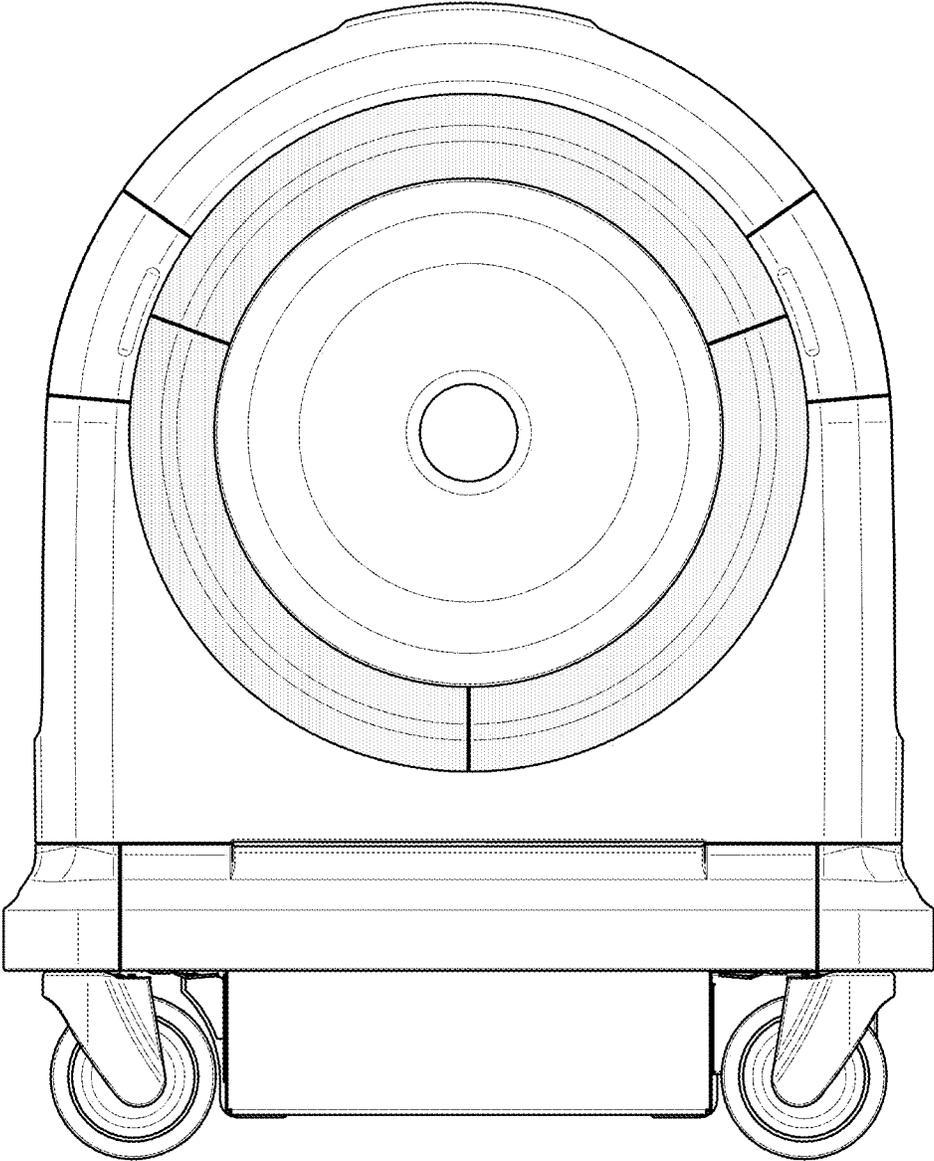


FIG. 2

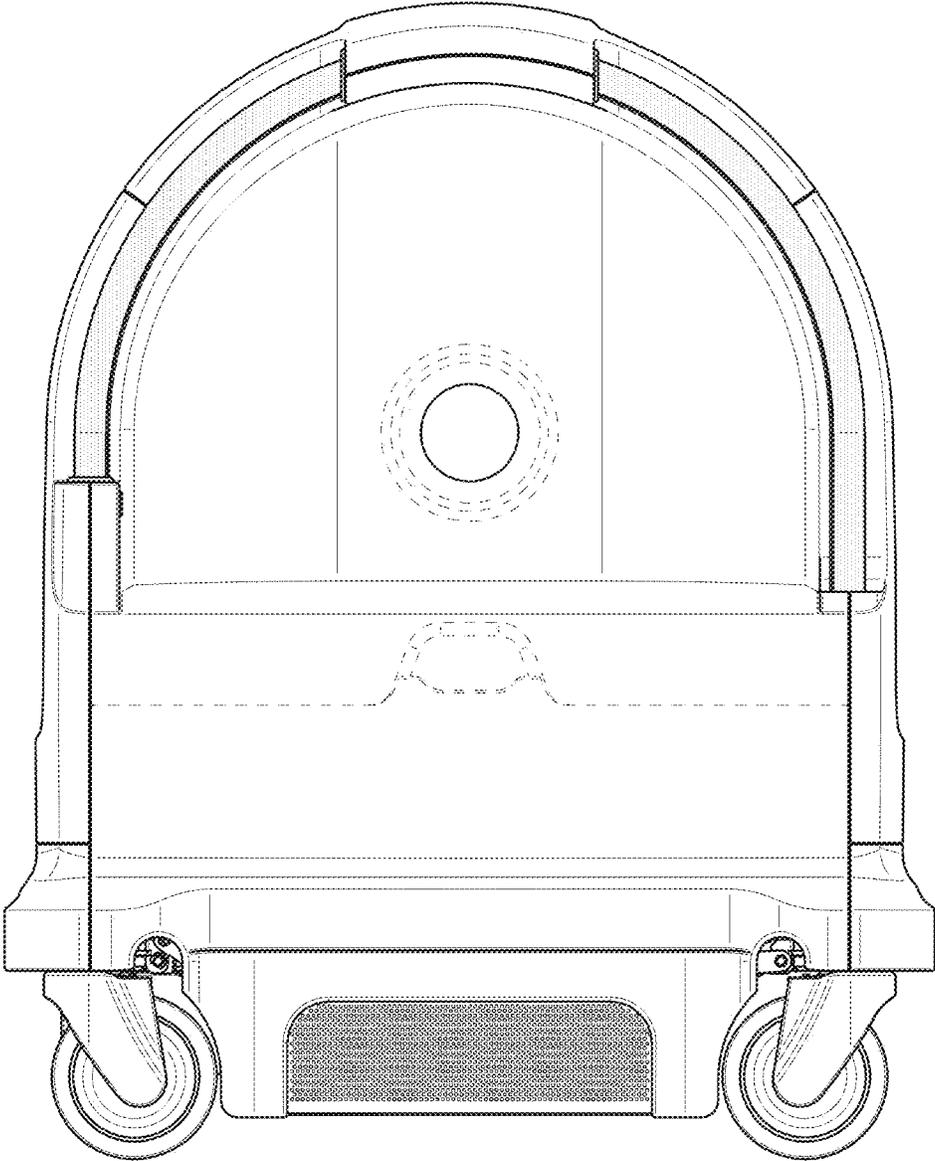


FIG. 3

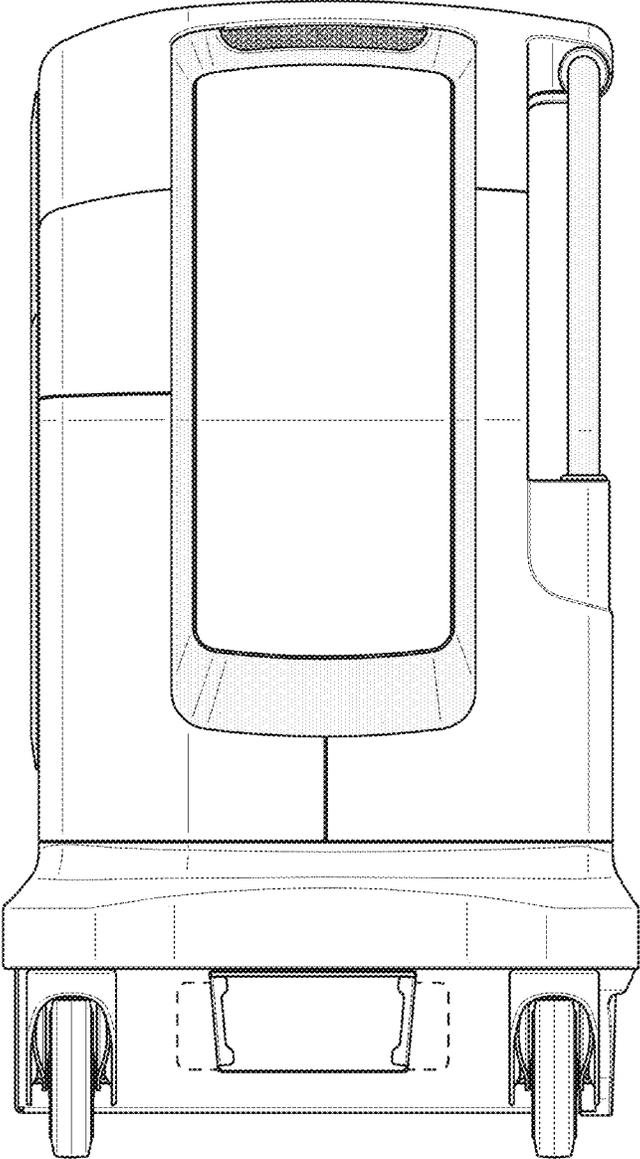


FIG. 4

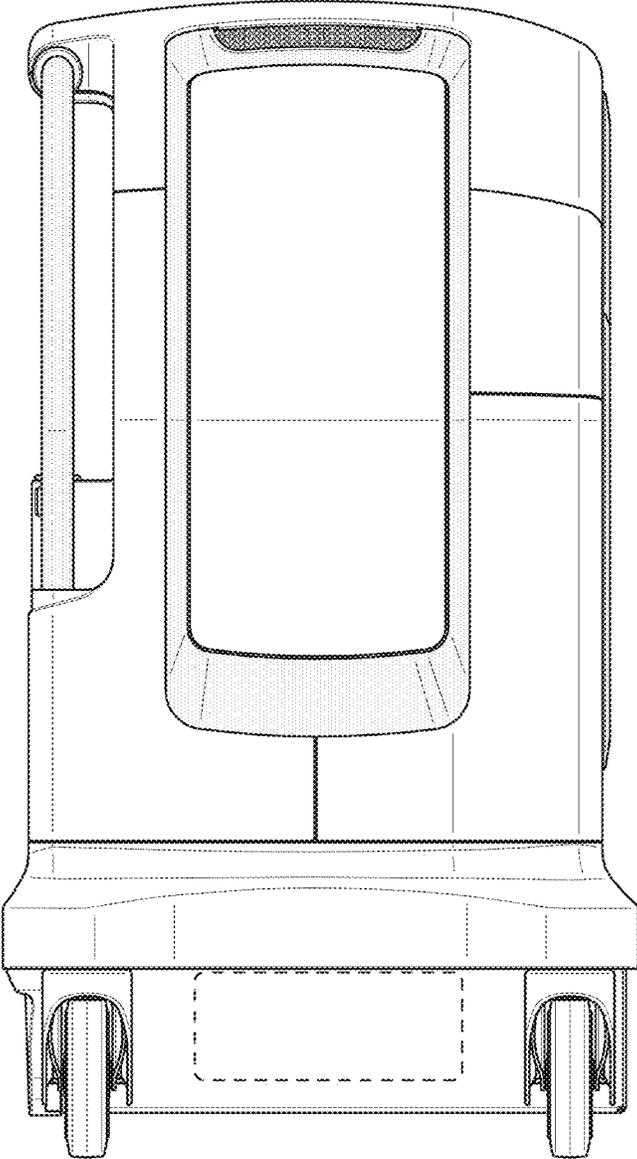


FIG. 5

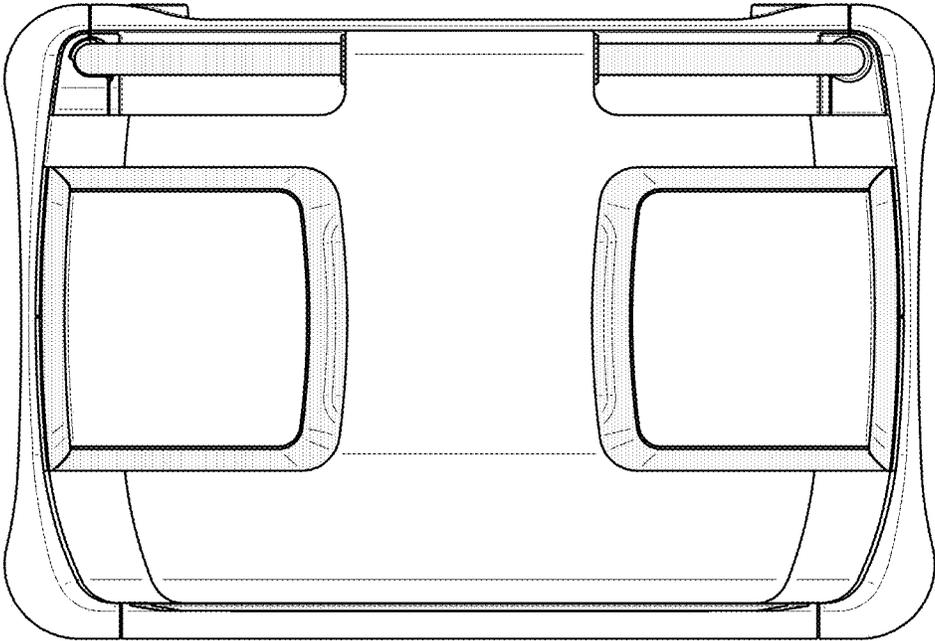


FIG. 6

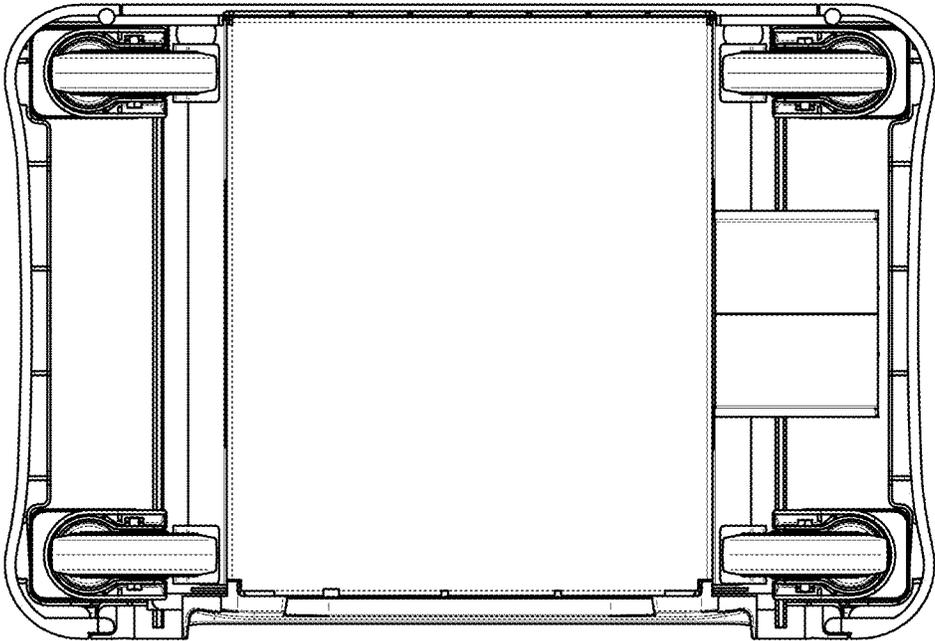


FIG. 7