



(22) Date de dépôt/Filing Date: 2004/07/01

(41) Mise à la disp. pub./Open to Public Insp.: 2005/01/13

(45) Date de délivrance/Issue Date: 2014/01/21

(62) Demande originale/Original Application: 2 527 667

(30) Priorité/Priority: 2003/07/02 (US60/485.015)

(51) Cl.Int./Int.Cl. *A61M 1/36* (2006.01),
A61K 35/14 (2006.01)


(72) Inventeurs/Inventors:
CARTER, LEE F., US;
KOLENBRANDER, JEREMY P., US;
LADTKOW, JAMES R., US;
SCIBONA, JOSEPH A., US;
STEWART, JEFFREY A., US;
FLETCHER, CHRISTOPHER, US

(73) Propriétaire/Owner:
TERUMO BCT, INC., US

(74) Agent: ROBIC

(54) Titre : SYSTÈME DE SURVEILLANCE ET DE COMMANDE POUR LE FRACTIONNEMENT DU SANG

(54) Title: MONITORING AND CONTROL SYSTEM FOR BLOOD PROCESSING

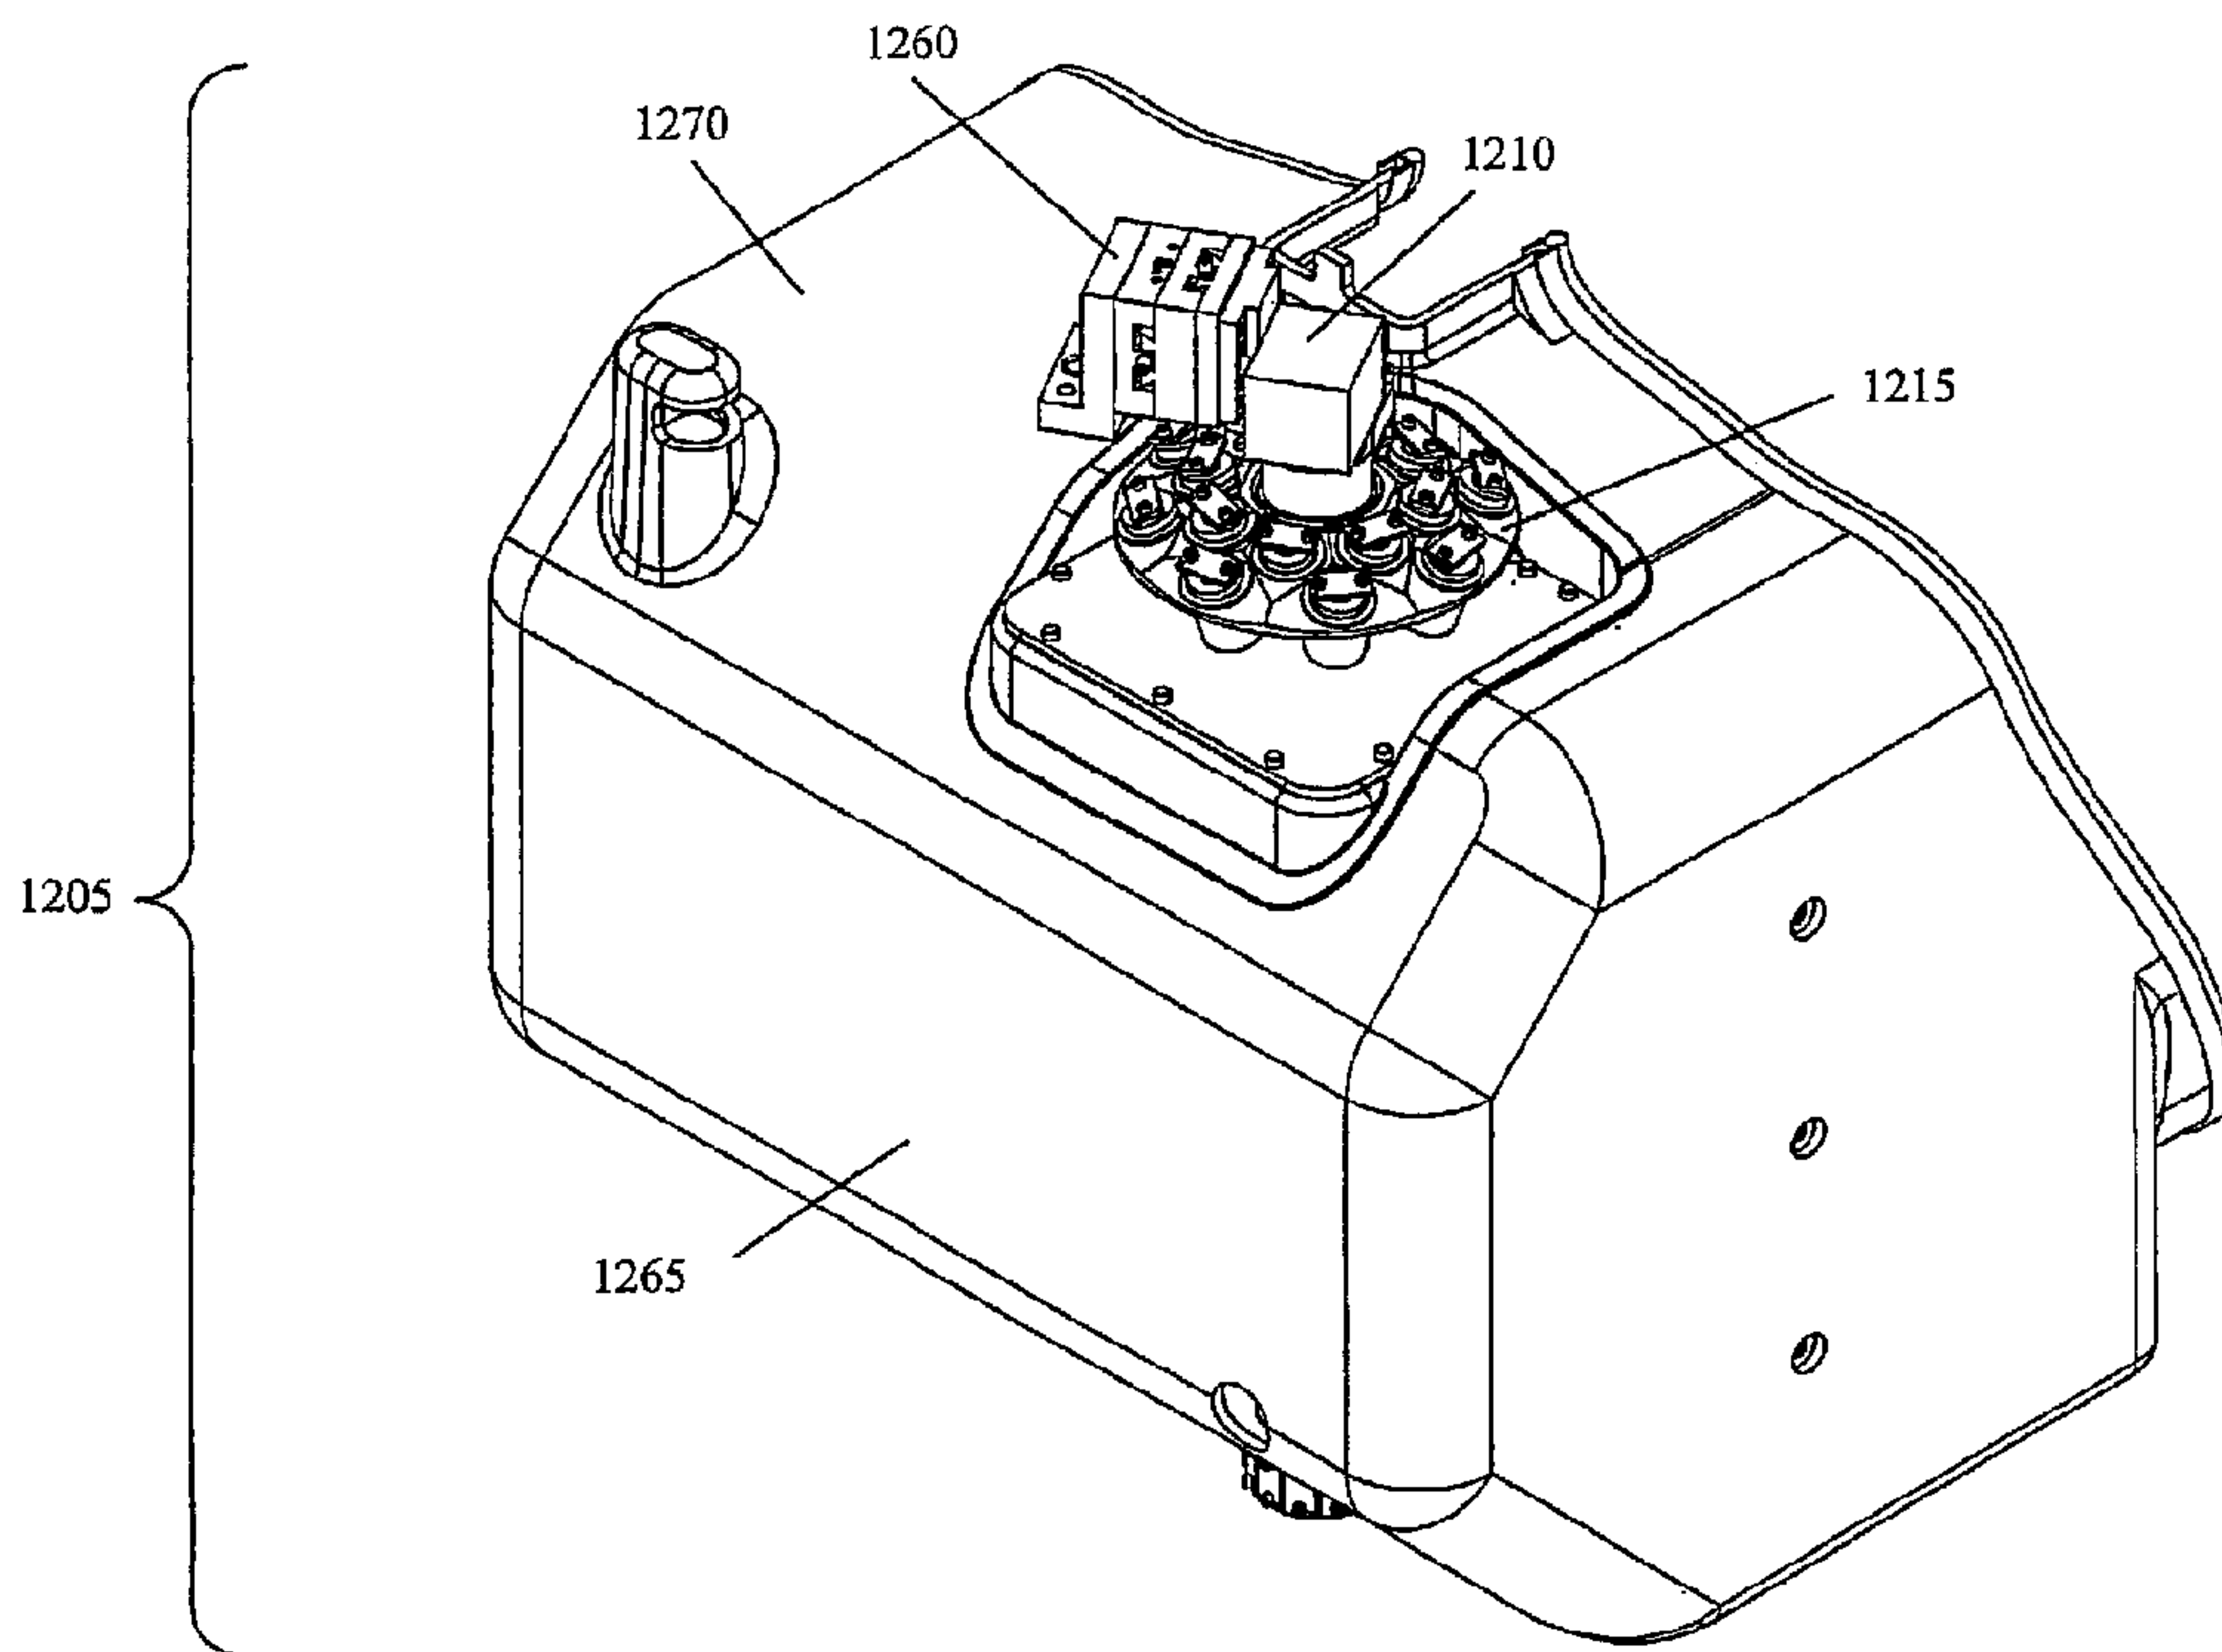

(57) Abrégé/Abstract:

The invention relates generally to methods of monitoring and controlling the processing of blood and blood samples, particularly the separation of blood and blood samples into its components with a two-dimensional optical measurement and control device. The method may comprise the steps of providing a blood processing system comprising a density centrifuge blood processing system and an elutriation blood processing system; filling the elutriation blood processing system with a desired component; measuring a cellular flux of cells entering the elutriation blood processing system with a two-dimensional optical control system; and flushing the elutriation blood processing system.

ABSTRACT

The invention relates generally to methods of monitoring and controlling the processing of blood and blood samples, particularly the separation of blood and blood samples into its components with a two-dimensional optical measurement and control device. The method may comprise the steps of providing a blood processing system comprising a density centrifuge blood processing system and an elutriation blood processing system; filling the elutriation blood processing system with a desired component; measuring a cellular flux of cells entering the elutriation blood processing system with a two-dimensional optical control system; and flushing the elutriation blood processing system.

MONITORING AND CONTROL SYSTEM FOR BLOOD PROCESSING

FIELD OF THE INVENTION

This priority invention relates to a monitoring and control system for blood processing.

BACKGROUND OF THE INVENTION

Large scale blood collection and processing play important roles in the worldwide health care system. In conventional large scale blood collection, blood is removed from a donor or patient, separated into its various blood components via centrifugation, filtration and/or elutriation and stored in sterile containers for future
10 infusion into a patient for therapeutic use. The separated blood components typically include fractions corresponding to red blood cells, white blood cells, platelets and plasma. Separation of blood into its components can be performed continuously during collection or can be performed subsequent to collection in batches, particularly with respect to the processing of whole blood samples. Separation of blood into its various components under highly sterile conditions is critical to most therapeutic applications.

Recently, apheresis blood collection techniques have been adopted in many large scale blood collection centers wherein a selected component of blood is collected and the balance of the blood is returned to the donor during collection. In
20 apheresis, blood is removed from a donor and immediately separated into its components by on-line blood processing methods. Typically, on-line blood processing is provided by density centrifugation, filtration and/or diffusion-based separation techniques. One or more of the separated blood components are collected and stored in sterile containers, while the remaining blood components are directly re-circulated to the donor. An advantage of this method is that it allows more frequent donation from an individual donor because only a selected blood component is collected and purified. For example, a donor undergoing

plateletpheresis, whereby platelets are collected and the non-platelet blood components are returned to the donor, may donate blood as often as once every fourteen days.

Apheresis blood processing also plays an important role in a large number of therapeutic procedures. In these methods, blood is withdrawn from a patient undergoing therapy, separated, and a selected fraction is collected while the remainder is returned to the patient. For example, a patient may undergo leukapheresis prior to radiation therapy, whereby the white blood cell component of his blood is separated, collected and stored to avoid exposure to radiation.

10 Alternatively, apheresis techniques may be used to perform red blood cell exchange for patients with hematological disorders such as sickle cell anemia and thalassemia, whereby a patient's red blood cell component is removed and donated packed red blood cells are provided to the patient along with his remaining blood components. Further, apheresis may be used to perform therapeutic platelet depletion for patients having thrombocytosis and therapeutic plasma exchange for patients with autoimmune diseases.

20 Both conventional blood collection and apheresis systems typically employ differential centrifugation methods for separating blood into its various blood components. In differential centrifugation, blood is circulated through a sterile separation chamber which is rotated at high rotational speeds about a central rotation axis. Rotation of the separation chamber creates a centrifugal force directed along rotating axes of separation oriented perpendicular to the central rotation axis of the centrifuge. The centrifugal force generated upon rotation separates particles suspended in the blood sample into discrete fractions having different densities. Specifically, a blood sample separates into discrete phases corresponding to a higher density fraction comprising red blood cells and a lower density fraction comprising plasma. In addition, an intermediate density fraction comprising platelets and leukocytes forms an interface layer between the red blood

cells and the plasma. Descriptions of blood centrifugation devices are provided in U.S. Patent No. 5,653,887 and U.S. Patent No. 7,033,512.

To achieve continuous, high throughput blood separation, extraction or collect ports are provided in most separation chambers. Extraction ports are capable of withdrawing material from the separation chamber at adjustable flow rates and, typically, are disposed at selected positions along the separation axis corresponding to discrete blood components. To ensure the extracted fluid exiting a selected extraction port is substantially limited to a single phase, however, the phase boundaries between the separated blood components must be positioned along the separation axis such that an extraction port contacts a single phase. For example, if the fraction containing white blood cells resides too close to the extraction port corresponding to platelet enriched plasma, white blood cells may enter the platelet enriched plasma stream exiting the separation chamber, thereby degrading the extent of separation achieved during blood processing. Although conventional blood processing via density centrifugation is capable of efficient separation of individual blood components, the purities of individual components obtained using this method is often not optimal for use in many therapeutic applications. For example, centrifugation separation of blood samples is unable to consistently (99% of the time) produce separated platelet components which have less than 1×10^6 white blood cells per every 3×10^{11} platelets collected. The presence of white blood cells in platelet products increases the risks of viral exposure and immunological complications upon infusion into a patient.

As a result of the inability to achieve optimal purity levels using centrifugation separation alone, a number of complementary separation techniques based on filtration, elutriation and affinity-based techniques have been developed to achieve the optimal purities needed for use of blood components as therapeutic agents. These techniques, however, often reduce the overall yield realized and may reduce the therapeutic efficacy of the blood components collected. Exemplary methods

and devices of blood processing via filtration, elutriation and affinity based methods are described in U.S. Patent Serial No. 6,334,842 and International Patent Application Serial No. PCT/US03/117764.

The purity of extracted blood components using density centrifugation is currently limited by the control of the position of phase boundary layers between separated components provided by conventional centrifugation devices and methods. The position of phase boundaries along the separation axis depends on a number of variables. First, phase boundary positions depend on the relative flow rates of individual blood components out of the separation chamber. Second, phase
10 boundary positions depend on the rotational velocity of the separation chamber about the central rotation axis and the temperature of the blood undergoing separation. Third, phase boundary positions vary with the composition of the blood undergoing processing. Blood sample composition may vary considerably from donor to donor and/or from patient to patient. In addition, blood composition may vary significantly as function of time for a given donor or patient, especially as blood is recycled through the separation chamber multiple times. Given the sensitivity of the phase boundary position to many variables which change from person to person and during processing, it is important to monitor the position of the phase
20 boundaries during blood processing to ensure optimal separation conditions are maintained and the desired purity of selected blood components is achieved. In addition, accurate characterization of the positions of phase boundaries allows for separation conditions to be adjusted and optimized for changes in blood composition during processing.

Although capable of measuring the position of one or more phase boundaries, conventional optical monitoring and control methods for blood processing have substantial limitations. First, conventional optical monitoring systems and methods, such as those discussed in U.S. Patents 5,316,667 and 5,260,598, utilize one-dimensional optical detection or one-dimensional optical

scanning. Accordingly, these methods are unable to characterize the intensities of transmitted and/or scattered light from a two-dimensional or three-dimensional region of a blood processing device. Moreover, these methods are unable to measure the flux or purities of cellular material exiting the separation chamber through a selected extraction port. Second, conventional optical monitoring methods lack the signal-to-noise ratios needed for many blood processing applications because light intensities characterized are limited to a single optical axis. For example, conventional optical monitoring methods lack the sensitivity needed to accurately resolve the position of the phase boundaries between white
10 blood cells and other blood components because white blood cells comprise less than 1% of total blood volume. Therefore, these methods are not capable of providing blood components, such as platelets and red blood cells, with white blood cell levels reduced to the extent needed to avoid immunological complications and viral transmission. Third, conventional optical monitoring methods are limited to fixed optical geometries and are incapable of monitoring regions of the density centrifuge device located on a plurality of different optical axes. As a result, the functional capabilities of conventional optical methods for monitoring and controlling separation by density centrifugation are substantially limited to monitoring the position of phase boundaries in the separation chamber.

20 It will be appreciated from the foregoing that a need exists for methods and devices for monitoring and controlling the processing of whole blood samples and blood component samples. Particularly, optical monitoring methods and devices are needed which are capable of accurately characterizing the separation, extraction and collection of blood components processed by density centrifugation. In addition, multifunctional optical monitoring and control systems for blood processing are needed which are capable of simultaneously monitoring a plurality of regions corresponding to a separation region, sample identification region and a blood component extraction region. Accordingly, it is an object of the present invention to

provide methods, devices and device components for blood processing which are capable of high throughput separation, characterization and collection of individual blood components, particularly red blood cells, white blood cells, platelet enriched plasma and plasma.

SUMMARY OF THE INVENTION

This invention provides methods, devices and device components for improving the processing of fluids comprising fluid components, such as blood, components of blood and fluids derived from blood. Methods, devices and device components of the present invention are capable of monitoring and controlling
10 separation of blood into discrete components and subsequent collection of selected components. The present invention includes methods, devices and device components for optically monitoring blood processing via a wide range of separation techniques, including density centrifugation, centrifugal elutriation, size and shape filtration, affinity chromatography or any combination of these techniques. The methods, devices and device components of the present invention are capable of characterizing the composition and purity of a collected blood component and capable of measuring the rate in which a blood component is extracted and collected. In addition, the methods, devices and device components of the present invention are capable of controlling blood processing by optimizing
20 separation and extraction conditions to reproducibly achieve a desired selected purity and/or composition of a blood component. The present invention improves processing of static blood samples or flowing blood samples.

In accordance with an aspect of the invention, there is provided a method of processing blood comprising the steps of:

providing a two stage blood processing system comprising a density centrifuge blood processing system and an elutriation blood processing system;

flowing blood into said two stage blood processing system, wherein the blood is separated into a plurality of components in the density centrifuge blood processing system including at least one desired component and a plasma containing component;

filling the elutriation blood processing system with said desired component until the elutriation blood processing system is in a filled operating state;

measuring a cellular flux of cells entering the elutriation blood processing system with a two-dimensional optical control system; and

10 flushing the elutriation blood processing system when in the filled operating state by flowing the plasma containing component into the elutriation blood processing system, thereby processing said blood.

The invention is further illustrated by the following description, examples, drawings and claims.

BRIEF DESCRIPTION OF THE DRAWINGS

Fig.1 is a schematic drawing showing an optical monitoring and control system of the present invention.

Fig. 2 is a schematic drawing showing a side view of a light collection element and two-dimensional detector useable in the present invention.

20 Fig. 3 is a schematic drawing showing a front cut-away view of a light collection element and two-dimensional detector useable in the present invention.

Fig. 4 is a schematic drawing showing a top plan view of a mounting configuration providing for selective adjustment of the position of the light collection element and two-dimensional detector.

Fig. 5 is a schematic drawing showing observation regions of monitoring systems of the present invention.

Figure 6 is a top plan view of an optical cell of a separation chamber showing an expanded region illustrated in Figures 6A and 6B. Figures 6A and 6B show schematics of images generated by the methods of the present invention of the expanded region shown in Figure 6 having a human blood sample therein separated into blood components. The images in Figs. 6A and 6B illustrate the ability of the methods and devices of the present invention to monitor and control the position of phase boundaries between separated blood components. In Figures 10 6A and 6B, triangles schematically represent white blood cells and platelets, circles schematically represent red blood cells and areas having lines schematically represent plasma.

Fig. 7 shows images of the rotating separation chamber of a density centrifuge generated by the methods of the present invention. The image in Figure 7 includes a phase boundary monitoring region and a white blood cell extraction port monitoring region. Analysis of the image in Fig. 7 provides a measurement of the composition and flux of cellular material out of the separation chamber. In figure 7, triangles schematically represent white blood cells and platelets, circles represent red blood cells and areas having lines represent plasma.

20 Fig. 8 shows the temporal behavior of the measured phase boundary positions (bottom two curves) and transmitted light intensities through the extraction port monitoring region (top two curves) during white blood cell collection. Figure 8A show corresponding 50 point moving averages. Solid diamonds (designated as RBC Pixels) correspond to the position of the phase boundary between the red blood cell containing component and the buffy coat layer, open squares (designated as Platelet Pixels) correspond to the position of the phase boundary between the platelet containing component and the buffy coat layer, solid triangles

(designated as Extraction Port Tool #1) correspond to median transmitted intensities through a first flux monitoring region and X markers (designated as Extraction Port Tool #2) correspond to median transmitted intensities through a second flux monitoring region.

Fig. 9 shows a series of plots of the observed white blood cell concentrations as a function of the median intensity of light transmitted through the second flux monitoring region (X markers, + markers and - markers) corresponding to the rotational velocities (RPM) indicated in the legend. Also shown in Figure 9, are plots of the hematocrit of the extracted material as a function of the median intensity of light transmitted through the second flux monitoring region (diamond markers, square markers and triangle markers) corresponding to the rotational velocities (RPM) indicated in the legend.

Fig. 10 shows a plot of the concentration of white blood cells in the extracted material as a function of the position of the phase boundary (in terms of pixel height of the collected image) between the red blood cell containing component and the buffy coat layer corresponding to the rotational velocities (RPM) indicated in the legend.

Fig. 11 shows a schematic of an exemplary master-smart slave control system of the present invention capable of controlling blood processing.

Figure 12 provides a schematic flow diagram illustrating an automated, computer controlled process control system for a density centrifuge blood processing device.

Figure 13 is a schematic diagram showing exemplary Control Driver and APC Sub-System architectural relationships useful in the methods of the present invention.

Figure 14 is a schematic diagram showing exemplary Procedure Control and APC Sub-System architectural relationships useful in methods of the present invention.

Figure 15 shows exemplary architectural relationships of the APC Executive with the APC Driver, Image Data List Container, and the APC components within the Control Sub-System useful in the methods of the present invention.

Figure 16 is a schematic diagram providing a state chart for the image data analyzer task.

Figure 17 shows an exemplary architecture of the APC Driver component of the present invention.

Figure 18 shows an exemplary high level state diagram for a APC Driver task useful for the methods of the present invention.

10 Figure 19 shows an exemplary architecture of a APC Image Processing Engine component of the present invention.

Figure 20 provides an exemplary state chart for an image analyzer task useful in the methods of the present invention.

Fig. 21A provides a schematic diagram of a rotated side view of an optical cell of the present invention useful for monitoring blood processing via density centrifugation. Fig. 21B provides a cross sectional view of an exemplary extraction port design of the present invention. Fig. 21C provides a cross sectional view of an alternative extraction port design of the present invention, wherein first extraction port and second extraction port each have axial bores having a rectangular cross
20 sectional profile.

Fig. 22 is a top view of an optical monitoring and control system of the present invention well suited for blood processing via density centrifugation.

Fig. 23 is a cut away view corresponding to cut away axis **1200** indicated in Figure 22.

Fig. 24 is a side view of the optical monitoring and control system illustrated in Figures 22 and 23.

Fig. 25 provides a schematic diagram of an exploded, side view of a bottom pulsed LED source useful in the methods and devices of the present invention.

Fig. 26 shows a functional flow diagram representing a method of synchronizing light pulses generated by top and bottom pulsed LED light sources trigger and trigger delay settings.

- 10 Fig. 27 provides plots of measurements of the white blood cell concentration (square markers) and hematocrit (diamond markers) of a separated blood component passing through an extraction port as function of the measured average intensity of light transmitted through the extraction port.

DETAILED DESCRIPTION OF THE INVENTION

Referring to the drawings, like numerals indicate like elements and the same number appearing in more than one drawing refers to the same element. In addition, hereinafter, the following definitions apply:

- 20 The terms "light" and "electromagnetic radiation" are used synonymously and refer to waves of electric and magnetic fields that also exhibit particle-like behavior. Light useful for the methods of the present invention includes gamma rays, X-rays, ultraviolet light, visible light, infrared light, microwaves, radio waves or any combination of these.

"Depth of field" refers to the zone of acceptable sharpness in a picture and/or image extending in front of and behind the plane of the subject. Depth of field may be quantitatively characterized as the range of distances reproduced in a picture and/or image over which the image is not unacceptably less sharp than the sharpest part of the image. The term "depth of field" is intended to be interpreted consistently with the mean of this term as understood by those having skill in the art. A light collection element may be characterized in terms of its depth of field.

"Optically differentiable" refers to differences in the optical characteristics of two or more illuminated materials. Optically differentiable materials can have different
10 absorption coefficients, extinction coefficients, scattering cross sections, fluorescence excitation wavelengths, phosphorescence excitation wavelengths, emission wavelengths or any combinations of these characteristics. As the optical characteristics of most materials depend on wavelength, materials can be optically differentiable when illuminated by light having a selected wavelength range. Exemplary optically differentiable materials useable in the present invention include, but are not limited to, erythrocytes, eosinophils, basophils, monocytes, lymphocytes, granulocytes, platelets (thrombocytes), plasma proteins, and plasma. Exemplary optically differentiable materials further include the materials comprising a blood processing device or blood sample container, such as polymeric materials
20 such as plastics, metals, and glass.

"Flux of cellular material exiting the separation chamber" refers to the amount of cells, such as erythrocytes, leukocytes, thrombocytes or any combination of these, which cross a defining area, such as the cross-sectional area of an extraction port of blood processing device, such as a density centrifuge, elutriation separation chamber or filtration separation device, per unit time. Flux of cellular material can be expressed in units of: (number of cells) $\text{cm}^{-2} \text{ s}^{-1}$.

"Optical communication" refers to the orientation of two or more elements such that light is capable of propagating from one element to another element. Elements can be in optical communication via one or more additional elements such as reflectors, lenses, fiber optic couplers, wave guides or any combinations of these. In one embodiment of the present invention, one or more light sources and a light collection element can be positioned in optical communication with an observation region on a blood processing device, such as a density centrifuge. In this embodiment, at least a portion of light from one or both of the light sources is directed onto an observation region and the light collection element is positioned
10 such that it is capable of collecting at least a portion of light scattered transmitted, or both from the observation region.

"Light collection element" refers to a device or device component which collects light and distributes the collected light in a desired way. Light collection elements useable in the present invention are capable of collecting at least a portion of transmitted light, scattered light or both generated upon illumination of an observation region on a blood processing device. Exemplary light collection elements of the present invention are capable of collecting light in a manner generating an image of an observation region on a two dimensional detector. Light collection elements of the present invention include, but are not limited to, fixed
20 focus lenses, spherical lenses, cylindrical lenses, aspheric lenses, wide angle lenses, zoom lenses, concave lenses, convex lenses, biconcave lenses, biconvex lenses, lens systems comprising a plurality of lenses, wave guides, fiber optic couplers, reflectors, spherical mirrors, aspherical mirrors, prisms, apertures, lenses, or any combination or equivalents of these. Light collection elements of the present invention are capable of directing collected light onto another optical device or device component, such as a two-dimensional detector. Light collection elements include at least one lens system having a selectively adjustable field of view and/or

focal length. Light collection elements can be translatable along a detection axis, which is perpendicular to a central rotation axis.

"Field of view" refers to the angular distribution of light rays which are collected and detected by an optical detection system, such as a light collection element in optical communication with a two dimensional detector. The field of view of a two dimensional imaging system of the present invention is the portion of an illuminated object or plurality of objects which is represented in a two dimensional image. Optical detection systems of the present invention can have a fixed field of view or a field of view which is selectively adjustable.

- 10 "Blood processing" refers to the manipulation of a blood sample or component thereof, to realize a change in composition. Blood processing includes methods of separating blood or a component thereof into components or subcomponents, leukoreduction, pathogen inactivation, blood filtering, oxygenating blood and blood components, dialysis, blood purification or clearing, pathogen removal, blood and blood component warming, blood component washing, and red blood cell deglycerolization. The present invention provides improved methods of blood processing wherein a blood sample or component thereof is separated into components or subcomponents on the basis of density, size, diffusion rate, sedimentation velocity, surface chemistry properties or combinations of these
- 20 characteristics.

"Observation region" refers to an illuminated portion of an object or plurality of objects which generates transmitted light, scattered light or both at least a portion of which that is collected by a light collection element and detected by a two-dimensional detector. In preferred embodiments of the present invention, the observation region is positioned on a blood processing device, component of a blood processing device, such as an optical cell, or a blood sample container. The size and position of the observation region is determined by the field of view of the

light collection element, the position of the light collection element from the blood processing device, the area of the two-dimensional detector and the position of the two-dimensional detector with respect to the light collection element. In an embodiment, the size, shape and position of the observation region is selectively adjustable by controlling the position of the light collection element with respect to the blood processing device and the field of view of the light collection element. In an embodiment of the present invention, one or more phase boundaries between optically differentiable components are viewable in the observation region. In another preferred embodiment, at least one separated component is viewable in the observation region. In another preferred embodiment, at least one extraction port is viewable in the observation region.

"Interface region" refers to a region of the a blood separation device wherein two or more optically differentiable phases are viewable. For example, in one embodiment the interface area is defined by a region of the separation chamber wherein the phase boundary between a red blood cell containing component and a plasma containing component is viewable. In another embodiment, the interface area is defined by a region of the separation chamber wherein the phase boundary between a red blood cell containing component and a mixed-phase white blood cell and platelet containing component and the phase boundary between the mixed-phase white blood cells and platelet containing component and plasma containing component are viewable. In another embodiment, the phase boundary between a white blood cell containing component and a platelet containing component are viewable. In the present invention, a two-dimensional distribution of scattered and/or transmitted light intensities of light from an interface region provides a measurement of the position of one or more boundary layers along a plurality of separation axes. In an exemplary embodiment, the interface region is an optical cell of a separation chamber.

"Composition-monitoring region" refers to portion of a blood processing device occupied by at least one separated phase. For example, the composition-monitoring region can be defined by a region of a separation chamber in a density centrifuge wherein light is transmitted through one or more discrete phase in the separation chamber upon illumination by an incident light beam. As the transmission of light through a separated compound depends on identity and concentration of cellular and non-cellular material, monitoring scattered light, transmitted light, or both, from a composition-monitoring region provides a measurement of the identity, concentration, cell type, purity of at least one component or any combination of these. In an exemplary embodiment, the composition monitoring region is an extraction port in an optical cell of a separation chamber.

"Blood sample" and "blood" are used synonymously to refer to whole blood, one or more blood component, one or more blood products, or any combination of these. "Blood component" and "blood product" as used herein include cellular components, noncellular components of blood and combinations of cellular and noncellular components of blood. Exemplary cellular components include but are not limited to erythrocytes (red blood cells), leukocytes (white blood cells), and thromobocytes (platelets) and combinations of these materials. Leukocytes comprise monocytes, granulocytes, agranulocytes, lymphocytes. Exemplary noncellular components include but are not limited to plasma, dissolved salts and minerals and plasma proteins. A blood component can be further fractionated into blood sub-components.

"Two-dimensional detector" refers to any detector capable of measuring a two-dimensional distribution of scattered and/or transmitted light intensities, such as a two-dimensional distribution of scattered and/or transmitted light intensities corresponding to an image of a portion or component of a blood processing system. Exemplary two-dimensional detectors measure two-dimensional distributions of

scattered and/or transmitted light intensities comprising images of an observation region on a separation chamber of a blood processing system. Optionally, two-dimensional detectors generate one or more output signals which are received by another device component as input. Preferred two-dimensional detectors of the present invention include, but are not limited to, a charge coupled device (CCD), a two-dimensional photodiode array, a two-dimensional photoconductive array, a two-dimensional pyroelectric array, a digital camera, a complimentary metal oxide semiconductor (CMOS) detector, a plurality of photodiodes and a plurality of photomultiplier tubes. Two dimensional detectors may measure two-dimensional
10 distribution of scattered and/or transmitted light intensities corresponding to a monochrome image or a color image. In one embodiment, two dimensional-detectors of the present invention have the ability to selectively detect light corresponding to a selected wavelength range. In one embodiment, two dimensional-detectors of the present invention measure a plurality of two-dimensional distribution of scattered and/or transmitted light intensities corresponding to a plurality of selected wavelength ranges, such as wavelength ranges corresponding to red light, green light and blue light.

"Separation axis" refers to the axis along which blood components having different densities are separated in a density centrifuge. As a separation chamber is rotated
20 about a central rotation axis in a density centrifuge, the centrifugal force is directed along separation axes. Accordingly, a plurality of axes rotates about the central rotation axis of a density centrifuge. In a preferred embodiment, the optical monitoring methods of the present invention are capable of measuring the positions of one or more phase boundaries between optically differentiable components along the separation axis.

"Flux" refers to the rate at which cellular material, non-cellular material, or both, crosses a defining plane. Flux can be expressed by the following unit: (number of X) $\text{cm}^{-2} \text{s}^{-1}$, where in X is a cellular component or non-cellular component of blood.

In a preferred embodiment, the optical monitoring methods of the present invention are capable of measuring the flux of cellular components including, but not limited to, red blood cells, neutrophils, esinophils, basophils, monocytes, lymphocytes, platelets or any combination of these, through an extraction port of a separation chamber.

"Image" refers to a visual representation of one or more patterns of light originating from an observation region. Images of the present invention can be two dimensional images or three dimensional images. The present invention provides methods and devices whereby a measured two-dimensional distribution of scattered and/or transmitted light intensities provides an image corresponding to an observation region, such as an observation region positioned on a separation chamber an/or optical cell of a density centrifuge. In one embodiment, images generated by the methods and devices of the present invention correspond to light scattered, transmitted, or both, from one or more components undergoing density centrifugation, such as components of a blood sample. Alternatively, images generated by the methods and devices of the present invention correspond to light scattered, transmitted, or both, from a region of the density centrifuge itself, such as the optical cell of a separation chamber. Two-dimensional distributions of scattered and/or transmitted light intensities and images measured by the methods and devices of the present invention can be used to determine the position of phase boundaries between optically differentiable components along a separation axis, the composition of selected components, the flux and composition of cellular or non-cellular materials out of the separation chamber, the identity of a blood sample and the identity of the kit or container containing a blood sample.

"Resolution" refers generally to the ability of an optical measurement to illustrate an image comprising patterns of light originating from an observation region. The greater the resolution the sharper the image. Resolution of a two-dimensional

optical measurement is commonly expressed in terms of number of pixels on the horizontal and vertical axis by the following equations:

$$\text{horizontal resolution} = \frac{\left(P_h \right)}{L_h}$$

$$\text{vertical resolution} = \frac{\left(P_v \right)}{L_v}$$

(I)

(II)

wherein P_h and P_v , are the number of pixels extending along the horizontal and vertical axes, respectively, and L_h and L_v are the lengths of the image along the horizontal and vertical axes, respectively. Optical monitoring systems of the present invention are capable of generating high resolution images of an observation region.

10 "Epi-illumination" refers to the illumination of an object and generation of scattered light. In epi-illumination, light is directed to the object along an axis of illumination which is different than the optical axis whereby scattered light is collected and detected.

"Parallel" refers to a geometry in which two surfaces are equidistant from each other at all points and have the same direction or curvature. Substantially parallel refers to a geometry in which angular deviations from absolute parallelism are less than 10 degrees, and preferably less than 0.5 degrees for some applications. The present invention includes optical cells for blood processing comprising a plurality of optical surfaces positioned in substantially parallel planes.

In the following description, numerous specific details of the devices, device components and methods of the present invention are set forth in order to provide a thorough explanation of the precise nature of the invention. It will be apparent, however, to those of skill in the art that the invention can be practiced without these specific details. Reference in the specification to "a preferred embodiment," "a more preferred embodiment" or "an exemplary embodiment" means that a particular feature, structure, or characteristic set forth or described in connection with the embodiment is included in at least one embodiment of the invention. Reference to "preferred embodiment," "a more preferred embodiment" or "an exemplary embodiment" in various places in the specification do not necessarily refer to the same embodiment.

This invention provides methods, devices and device components for monitoring and controlling blood processing, preferably by density centrifugation, centrifugal elutriation and/or filtration. In particular, the present invention provides a multifunctional optical monitoring system capable of measuring two-dimensional distributions of scattered and/or transmitted light intensities comprising images corresponding to an observation region, which is particularly useful for achieving effective separation of blood into individual components and subsequent collection of separated components.

Figure 1 schematically illustrates an exemplary embodiment of the optical monitoring system of the present invention capable of measuring a two-dimensional distribution of scattered and/or transmitted light intensities corresponding to patterns of light originating from an observation region on a separation chamber. The illustrated monitoring system **100** comprises light source **110**, light collection element **120**, and two-dimensional detector **130**. Light source **110** is in optical communication with a density centrifuge **140** comprising separation chamber **150** which rotates about central rotation axis **160**. Rotation about central rotation axis **160** results in separation of a blood sample in the separation chamber into discrete

blood components along a plurality of rotating separation axes oriented orthogonal to the central rotation axis **160**. In a preferred embodiment, separation chamber **150** is held in a circular filler (not shown in Figure 1), which is also capable of rotation about central rotation axis **160**. In one embodiment of the present invention, a filler comprises a disc having an internal, circular groove wherein the separation chamber is positioned and fastened. During operation of the density centrifuge, the filler is operationally connected to a rotating means such that both filler and separation chamber are rotated about the central rotation axis **160**. In the schematic shown in Figure 1, the blood sample is separated into an outer higher
10 density phase corresponding to a red blood cell component **170**, an intermediate density phase corresponding to a white blood cell and platelet-containing component (e.g. buffy coat) **180** and a lower density inner phase corresponding to a platelet enriched plasma component **190**.

Light source **110** provides incident light beam **200**, which illuminates an observation region **220** on separation chamber **150**, preferably in a manner generating scattered and/or transmitted light from the blood sample undergoing separation. In one embodiment, light source **110** is capable of generating an incident light beam, a portion of which is transmitted through at least one blood component undergoing separation in separation chamber **150**. At least a portion of
20 scattered and/or transmitted light **210** from the observation region **220** is collected by light collection element **120**. Light collection element **120** is capable of directing at least a portion of the collected light **210** onto two-dimensional detector **130**. The two-dimensional detector **130** detects patterns of scattered and/or transmitted light **210** from the observation region, thereby measuring two-dimensional distributions of scattered and/or transmitted light intensities. In an exemplary embodiment, two-dimensional distributions of scattered and/or transmitted light intensities comprise images corresponding to patterns of light originating from the observation region **220**. In one embodiment, images of the present invention are monochrome images,

which provide a measurement of the brightness of separated blood components along the separation axis. Alternatively, images of the present invention are color images, which provide a measurement of the colors of separated blood components along the separation axis.

Observation region **220** is positioned on a portion of the density centrifuge **140**, preferably on the separation chamber **150**. In the exemplary embodiment illustrated in Figure 1, separated blood components and phase boundaries between optically differentiable blood components are viewable in observation region **220**. In one embodiment, the observation region is positioned on an optical cell of the
10 separation chamber having windows for transmitting the incident beam through the blood sample undergoing processing. In an alternative preferred embodiment, one or more extraction ports (not shown in Figure 1) are viewable in observation region **220**. In another embodiment, observation region **220** is positioned on the top of the separation chamber **150** such that leaks of the blood sample and/or improper alignment of the separation chamber or filler are viewable. In another alternative embodiment, the observation region **220** is positioned on a portion of the separation chamber such that the composition of a separated blood component can be directly monitored. For example, a monitoring system of the present invention provides a method of characterizing the type of cellular component collected and counting the
20 amount of cells extracted from the separation chamber as a function of time. Alternatively, the monitoring system is arranged such that the concentration of non-cellular blood components, such as blood plasma proteins, is directly measured. In one embodiment, the observation region **220** is arranged such that a plurality of measurements are obtained from every measured two-dimensional distribution of scattered and/or transmitted light intensities.

Optionally, the observation region **220** can also be illuminated by epi-illumination light source **230**, which is positioned on the same side of the separation chamber as the light collection element and two-dimensional detector. Epi-

illumination light source **230** is positioned such that it generates an incident beam **240** which is scattered by the blood sample and/or centrifuge. A portion of the light from Epi-illumination light source **230** scattered by the separation chamber and is collected by light collection element **120** and detected by two-dimensional detector **130**, thereby measuring a two-dimensional distribution of scattered and/or transmitted light intensities.

In one embodiment, two-dimensional detector **130** is also capable of generating output signals corresponding to the measured two-dimensional distributions of scattered and/or transmitted light intensities and/or images. In the
10 exemplary embodiment shown in Figure 1, two-dimensional detector **130** is operationally connected to a centrifugation device controller **225** capable of receiving the output signals. In one embodiment, centrifugation device controller **225** displays the measured intensity distributions, stores the measured intensity distributions, processes measured intensity distributions in real time, transmits control signals to various optical and mechanical components of the monitoring system and centrifuge or any combination of these. In a preferred embodiment, centrifugation device controller **225** is operationally connected to centrifuge **140** and is capable of adjusting selected operating conditions of the density centrifuge, such as the flow rates of cellular and non-cellular components out of the separation
20 chamber, the position of one or more phase boundaries along the separation axes, rotational velocity of the separation chamber about central rotation axis **160**, the infusion of anticoagulation agents or other blood processing agents to the blood sample, or any combination of these.

As shown in Figure 1, centrifugation device controller **225** can also be operationally connected to light source **110** and/or epi-illumination light source **230**. In this embodiment, centrifugation device controller **225** and/or two-dimensional detector **130** are capable of generating output signals for controlling illumination conditions. For example, output signals from two-dimensional detector can be used

to control the timing of illumination pulses, illumination intensities, the distribution of illumination wavelengths and/or position of light source **110** and/or epi-illumination light source **230**. As also shown in the embodiment illustrated in Figure 1, centrifugation device controller and two-dimensional detector are two way communication. In this embodiment, centrifuge device controller sends control signals to two-dimensional detector **130** to selectively adjust detector exposure time, detector gain and to switch between monochrome and color imaging.

Figure 2 shows a schematic drawing of a side view of a light collection element **120** and two-dimensional detector **130** of the present invention. Two-dimensional detector comprises a digital camera **300**, aperture **310**, and a close focus lens system **312**, which are disposed along optical axis **313**. Light originating from the observation region, for example light propagating substantially parallel to optical imaging axis **313**, is collected by close focus lens system **312** and directed onto digital camera **300**. In the exemplary embodiment shown in Figure 2, the close focus lens system **312** comprises zoom lens element **315**, close focus lens element **320**, and focus lens element **325**. Use of a close focus lens system **312** is beneficial due to the large range of fields of view provided. Optionally, light collection element **120** and two-dimensional detector **130** further comprises one or more spacers **330**.

Use of an aperture **310** in this embodiment is beneficial because it allows the exposure of the camera to transmitted or scattered light to be selectively gated on and off as the separation chamber is rotated. Further, use of an aperture is beneficial because it is useful for controlling the light exposure time of the detector. Aperture size can be varied in the present invention. Because the separation chamber is rotating at a known, rotational velocity, proper selection of the aperture timing allows the position of the observation area on the separation chamber to be selectively adjusted with great accuracy, preferably to within 0.1 mm or better. Use of an aperture is also beneficial because it provides precise control over the detector exposure times needed to measure two dimensional distributions of

transmitted and/or scattered light intensities comprising high quality images of an observation region.

Referring again to the embodiment illustrated in Fig. 1, light collection element **120**, two-dimensional detector **130**, or both, can be arranged such that they are moveable, for example moveable along a first detection axis **250**, which is oriented orthogonal to the central rotation axis of the centrifuge. Movement of light collection element **120** in a direction along detection axis **250** adjusts the position of observation region **220** on the density centrifuge. In another embodiment, light collection element **120** is also capable of movement in a direction along a second
10 detection axis (not shown) which is orthogonal to the first detection axis **250**. The present invention also includes an embodiment wherein light source **110**, epi-illumination light source **230**, or both, are also capable of movement in a manner to optimize illumination and subsequent detection of transmitted and/or scattered light from the selectively adjustable observation region.

Figure 3 (not drawn to scale), shows a cut away view of an exemplary embodiment having a light collection element **120** and two-dimensional detector **130** which are capable of translation along detection axis **250**. In the embodiment illustrated in Figure 3, two-dimensional detector **130** and light collection element **120** are supported by motorized flying crane assembly **400**. The monitoring system
20 **395** has slide rails **405** for mounting to a density centrifuge and is equipped with a transmissive glass bottom plate **407** separating components of the monitoring system from the density centrifuge. Optical glass bottom plate **407** is substantially transparent to light originating from the observation region and protects light collection element **120** and two-dimensionally detector **130** from dust, debris and leaked blood components. Optionally, mounting collar **397** can be provided to dampen vibrations originating from rotation of the centrifuge, which can lead to misalignment of two-dimensional detector **130** and light collection element **120**.

Incorporation of motorized flying crane assembly **400** allows translation of two-dimensional detector **130** and light collection element **120** along detection axis **250**. As shown in Figure 3, crane assembly **400** rides on wheel guide support rails **410**, which are mounted on top of divider walls **420**. Divider walls **420** provide a support for crane assembly **400** and also serve to minimize the unwanted detection of background light. The crane assembly **400** is driven by a selectively adjustable stepping motor **430** and digital rotational encoder **435** capable of providing high resolution positional increments, for example increments of about 10 micrometers or less.

10 The monitoring system is also equipped with illumination light source **110** for illuminating the density centrifuge. In the embodiment shown in Figure 3, light source **110** is supported by flying crane assembly **400**. An incident light beam is generated by the light source **110** and directed through glass bottom pane **407** toward the density centrifuge. Alternatively, light source **110** further include one or more reflectors (not shown) to provide illumination from below the density centrifuge. The incident light beam is transmitted and/or scattered by the density centrifuge and a portion of light translating substantially parallel to optical imaging axis **313** is collected by the light collection element **120** and detected. In a preferred embodiment, light source **110** comprises a plurality of light emitting diode sources.

20 Figure 4 illustrates another mounting configuration providing movement of the light collection element **120** and two-dimensional detector **130**. As illustrated in Fig. 4, light collection element **120** and two-dimensional detector **130** are mounted on arm **600**, which is operationally connected to actuator **610**. Arm **600** is capable of rotation along arc path **620** upon action of actuator **610**. As shown in Fig. 4, movement along arc path **620** translates light collection element **120** and two-dimensional detector **130** past a range of regions of separation chamber **150**. Optionally, light collection element **120** and two-dimensional detector **130** can be supported by a low friction support surface operationally connected to the filler (not

shown) which holds the separation chamber in place. Mounting on the filler or bucket or container is particularly advantageous for batch processing or for separation in bags or other containers. The light collection element **120** and two-dimensional detector **130** can also be mounted on a cover of the centrifuge. An advantage of the mounting configuration shown in Figure 4 is that it is less susceptible to vibrations and spatial distortions introduced upon translation than other monitoring systems providing for translation of the light collection element and detector.

Figure 5 shows a plurality of observation regions provided by an optical monitoring system of the present invention having a light collection element and two-dimensional detector capable of translation along a detection axis **313** oriented perpendicular to the central rotation axis of a density centrifuge **700**. The squares shown in Figure 5 represent various fields of view provided by the present invention corresponding to a variety of light collection element and two-dimensional detector positions along detection axis **313**. Squares having the same areas but different center points correspond to different positions of the light collection element and detector along the detection axis. Squares having different areas but same center points corresponding to different fields of view for a selected light collection element and detector position along the detection axis. A smaller field of view is preferred for some applications because it provides higher resolution images of an observation region. Alternatively, a larger field of view is preferred for some applications because of the more expansive observation region it provides. Hatched region **704** represents additional regions of density centrifuge **700** which can be optically characterized by selectively adjusting the illumination timing and detector exposure time upon rotation of the separation chamber about the central rotation axis.

Squares **705**, **706** and **707** represent different fields of view achievable for first detection configuration wherein light collection element and two-dimensional

detector are positioned distal to the center **710** of density centrifuge **700**. While field of view **705** provides images capturing a small area of density centrifuge **700**, field of view **705** provides images having higher resolution than wider fields of view **706** and **707**. Squares **711**, **712** and **713** are fields of view corresponding to a second detection configuration wherein light collection element and two-dimensional detector are positioned proximate to the center **710** of density centrifuge **700**. Squares **715**, **716** and **717** are fields of view corresponding to a third detection configuration wherein light collection element and two-dimensional detector are positioned along detection axis **313** and located at an intermediate distance from center **710** of density centrifuge **700**.

Selection of the appropriate detector light exposure timing, field of view position and field of view area provides selective control over the position of the observation region on the blood processing device. Reference to detector exposure timing refers to the time over which the detector is exposed to transmitted and/or scattered light. The detector light exposure timing determines the angular orientation of the rotating separation chamber at the time in which a two dimensional distribution of transmitted and/or scattered light intensities is measured. In one embodiment, the exposure timing of the detector is controlled by triggering the opening and closing of an aperture, by triggering pulsed illumination and/or by detector gate settings in the digital camera itself. As shown in figure 5, use of a two-dimensional detector provides monitoring systems capable of monitoring large regions of a density centrifuge.

Light sources of the present invention comprise any device capable of generating one or more incident beams for illuminating an observation region on the density centrifuge. Exemplary light sources of the present invention comprise a single lamp or a plurality of lamps positioned to illuminate a single side or multiple sides of a density centrifuge. Light sources useable in the present invention include, but are not limited to, light emitting diodes and arrays of light emitting diode light

sources, xenon flash lamps, filament lamps, pulsed lasers, continuous wave lasers and fluorescent lamps. Use of light emitting diode light sources is preferred for some applications because they are capable of generating precisely timed illumination pulses. Use of a xenon flash lamp is preferred for some applications because it provides very high light intensities. Preferred light sources generate an incident light beam having a substantially uniform intensity. In one embodiment, light sources of the present invention generate an incident beam having a selected wavelength range and selected intensity. In one embodiment, light sources of the present invention further comprise fiber optical light pipes or waveguides capable of
10 controlling the illumination area on the blood processing device.

In a preferred embodiment, the optical monitoring system of the present invention comprises a plurality of light sources, each capable of generating an incident light beam having a different wavelength range. In one embodiment, for example, the optical monitoring system of the present invention comprises a combination of any of the following: white light source, red light source, green light source and blue light source. Use of a combination of light sources having different wavelength ranges is beneficial for discriminating and characterizing separated blood fractions because absorption constants and scattering coefficients of cellular and non-cellular components of blood vary with wavelength. For example, a red
20 blood cell containing component is easily distinguished from platelet enriched plasma containing component by illumination with light having wavelengths selected over the range of about 500 nm to about 600 nm because the red blood cell component absorbs light over this wavelength significantly more strongly than the platelet enriched plasma containing component. In addition, use of multiple colored light sources for illumination provides a means of characterizing the white blood cell type in an extracted blood component. As different white blood cell types have different absorption and scattering cross sections at different wavelengths, monitoring transmitted and/or scattered light from a white cell-containing blood

component provides a means of distinguishing the various white blood cell types in a blood component and quantifying the abundance of each cell-type.

Light sources of the present invention provide a continuous incident light beam or a pulsed incident light beam. Pulsed light sources are capable of being switched on and off in a manner synchronous with the rotation of the separation chamber to provide two dimensional distributions of transmitted and/or scattered light intensities corresponding to an observation region having a substantially fixed position using sensors, switches or other types of known cooperation. Alternatively, pulsed light sources of the present invention can be configured such that they can
10 be switched on and off in a manner asynchronous with the rotation of the separation chamber providing two dimensional distributions of transmitted and/or scattered light intensities corresponding to different observation regions for each full rotation. This alternative embodiment provides a method of selectively adjusting the location of the observation region and, thereby, probing different regions of the separation chamber. In one embodiment, triggering of illumination pulses is based on the rotational speed of the centrifuge or can be based on the angular position of the separation chamber as detected by optical or electronic methods well known in the art. In a preferred embodiment, triggering is provided by trigger pulses generated by the centrifuge device controller and/or two-dimensional detector.

20 An illumination system of the present invention also includes one or more aperture plates capable of providing a selected illumination area on a blood processing device or component thereof. In a preferred embodiment, an aperture plate is positioned between the light source and the blood sample undergoing separation. In this embodiment, the aperture plate masks areas of the separation chamber where exposure to light causes unwanted scattered light. In some instances, the reduction of unwanted scattered light detected by the two-dimensional detector reduces noise and, therefore, improves signal to noise ratio and image quality. Aperture plates are typically integrated into a filler which holds

the separation chamber in place during rotation. In this embodiment, the aperture plate rotates with the separation chamber. Optical filters and polarizers can also be incorporated into the illumination system of the present invention to provide illumination beams having selected optical properties, such as intensity, power, wavelength range and polarization state. Diffusers can also be incorporated into the illumination system of the present invention to provide spatially uniform illumination beams as is well known in the art.

Light collection elements of the present invention include any device capable of collecting and transmitting light in a manner generating a two dimensional distribution of transmitted and/or scattered light intensities of light from an observation region. Preferred light collection elements collecting and transmitting light in a manner generating a two dimensional distribution of transmitted and/or scattered light intensities comprising an image of the observation region. In an embodiment, the light collection element includes at least one fixed focus lens system. Alternatively, the light collection element includes at least one variable focal length lens system providing a selectively adjustable focal length, thereby, providing a selectively adjustable field of view. Light collection with a lens system providing an adjustable focal length provides monitoring systems wherein the size and shape of observation region can be selectively adjusted. In an exemplary embodiment, light collection elements of the present invention are capable of providing a field of view selectable over the range of about 1 cm² to about 10 cm². The ability to adjust the field of view provides optical monitoring systems wherein the resolution of the image generated can be changed and optimized for a given application or measurement.

Two-dimensional detectors of the present invention comprise any device or device component capable of detecting one or more patterns of light originating from a two-dimensional area or three-dimensional region. At the most fundamental level, two-dimensional detectors of the present invention comprise a plurality of

discrete light detectors distributed over a two-dimensional area. In a preferred embodiment, a two-dimensional detector of the present invention is capable of measuring two-dimensional distributions of transmitted and/or scattered light intensities comprising high quality images. Reference to a high quality images in the present invention relates to the ability to generate with good reproducibility high resolution, preferably for some applications greater than 20 pixels per millimeter and more preferably for some applications greater than 50 pixels per millimeter, images of an observation region, which exhibit high signal to noise ratio, preferably for some applications greater than 10 and more preferably for some applications greater than 100. In one embodiment, image quality is optimized in the present invention by selective adjustment of the illumination intensities, detector exposure time, detector gain and the position of the light source, light collection element and detector.

In one embodiment, a two-dimensional detector of the present invention is capable of generating a monochrome image corresponding to the brightness of an observation region on a density centrifuge, or other blood processing device or device component. In an exemplary embodiment, the two-dimensional detector is capable of detecting light over the entire wavelength range used for illumination. Alternatively, detectors of the present invention further comprise one or more optical filters capable of transmitting light of a selected wavelength distribution and capable of preventing transmission of light having other wavelengths. Use of optical filtering is beneficial for decreasing the effect of unwanted background scattered light and differentiating and/or characterizing separated blood components. The present invention includes methods wherein imaging is provided using photosensitive films.

In one embodiment, two-dimensional detectors of the present invention are capable of generating a color image corresponding to an observation on a density centrifuge or other blood processing device. For example, color imaging is the

useful for characterizing the extent of hemolysis during blood processing because hemoglobin has a strong, characteristic absorption over the wavelength range of 500 nm - 600 nm. In addition, color imaging is be useful in determining the concentration of red blood cells or white blood cells in a separated and/or extracted blood component. In one embodiment, the two-dimensional detector of the present invention is capable of switching between color and monochrome imaging, preferably for some applications on a frame-to-frame basis.

Exemplary centrifuge separation chambers of the present invention are continuous flow through chambers or static, disposable chambers of a constant
10 volume. Exemplary flow through separation chambers have an optical cell with one or more optical surfaces for transmitting light and can have one or more extraction ports for extracting a selected blood component. Optimally, extraction ports of the present invention reside close to or in the focal plane of the light collection element. Positioning of extraction ports in the focal plane is preferred because it improves measurement of the fluxes of cellular and noncellular material out of the separation chamber. Separation chambers of the present invention can include one or more dams positioned proximate to the extraction ports to facilitate selective extraction of separated blood components having reduced impurities arising from adjacent
20 components. The use of dams in blood processing via density centrifugation is well known in the art and described in U.S. Patents 6,053,856; 6,334,842 and 6,514,189.

Separation chambers of the present invention can further include one or more calibration markers for quantifying the absolute position of phase boundaries along the separation axis. Calibration markers are preferably located in the focal plane of the light collection element and can be any object or surface capable of easy recognition and characterization when imaged onto the two-dimensional detector. Use of a calibration marker can correct changes in optical alignment caused by rotation induced vibration and instrument jitter. Calibration markers of

the present invention facilitate image processing by enabling a computer algorithm to determine the precise location and physical dimensions of an observation region corresponding to a generated image or elements of an observation region. For example, calibration markers indicate the absolute position of phase boundaries between separated blood components in an observation region. Calibration markers also provide a means of establishing and maintaining correct focusing of the light collection element to ensure high quality images are obtained. Additionally, calibration markers also provide a means of calibrating the absolute brightness or color of pixels in a two dimensional image. In an exemplary embodiment, the
10 calibration marker is the edge of the separation chamber or the edge of a filler device component which secures the separation chamber in place. Alternatively, the calibration marker is a series of bars having a known thickness, brightness and/or color.

Separation chambers usable in the present invention can be made from any material sufficiently transparent to allow efficient illumination of a sample undergoing centrifugation. Separation chambers useful for some applications comprise an optical cell having one or more optical surfaces for transmitting light. In a preferred embodiment, the separation chamber is made of a polymeric material such as polyvinylchloride. Preferred separation chambers have highly polished
20 optical surfaces, such as windows capable of transmitting an illumination beam with great spatial uniformity. Separation chambers can also be flexible containers or annular disposable separation vessels.

In another embodiment of the present invention, the optical monitoring system includes a plurality of light collection elements and two-dimensional detectors. For example, in an exemplary embodiment, pairs of light collection elements and detectors are positioned to monitor different observation regions. Alternatively, pairs of light collection elements and detectors can be configured to

detect light having different wavelength ranges originating from the same observation region.

In one embodiment, centrifugation device controllers of the present invention comprise a device or device component such as a computer or processor capable of receiving an output signal from the two-dimensional detector and affecting the separation conditions of the density centrifuge. In a preferred embodiment, centrifugation device controllers are capable of selective adjustment of the position of one or more phase boundaries along the separation axes. In one embodiment, for example, centrifugation device controllers of the present invention adjust the
10 position of phase boundaries by varying the flow rates of one or more selected blood components out of the separation chamber. This can be achieved through the use of pumps, such as peristaltic pumps, to effectuate movement through tubing. Inlet pumps can be provided which are capable of forcing material out of the separation chamber. In another embodiment, the centrifugation device controller is capable of shutting down the centrifuge upon receiving a two-dimensional distribution of light intensities comprising a image indicating a leak of blood components out of the separation chamber, a misalignment of the separation chamber, a clot in the extraction ports or similar condition. In another embodiment, the centrifuge controller is capable of regulating the infusion of a blood agent, such
20 as an anti-coagulating agent, to the blood sample undergoing processing. Alternatively, the centrifugation device controller comprises a means for controlling the pumping rate of material out of the separation chamber in a manner capable of blowing out clots in the extraction ports. For example, upon receiving an output signal corresponding to a two-dimensional distribution of light intensities comprising a image indicating a platelet clot in a plasma extraction port, a centrifuge device controller of the present invention is capable of automatically clearing the clot by lowering the red blood cell level by reducing the pumping rate of the plasma pump and then rapidly accelerating the pumping rate of the plasma pump to force the clot

out of the extraction port. Alternatively, the centrifuge controller is be capable of selectively adjusting the rotational velocity of the centrifuge.

The optical monitoring system of the present invention can be integrated into a blood processing system, such as the systems described in U.S. Patent Serial No. 5,653,887. In an embodiment, the monitoring system acts to provide the system controller with the information relevant to the blood processing or a therapeutic procedure in real time. A monitoring system of the present invention is capable of adjusting illumination and detection conditions necessary to achieve two-dimensional distributions of light intensities corresponding to the highest optical quality images. In one embodiment, the monitoring system is in two-way communication with the device controller and is capable of receiving input data defining a selected blood processing procedure or a patient undergoing treatment. Such data can included the purity of blood components to be separated and extracted, the identity of blood components to be collected, the identity of blood components to be returned to the patient, the amount of a particular blood component to be collected or any combination of these. Inlet fluid composition data can also be used to calculate other desired information such as predicted yields and anticipated time for a desired collection or process.

The present invention provides optical monitoring and control systems for blood processing devices, especially useful for processing blood via density centrifugation. As will be recognizable to those having skill in the art, all devices, device elements and device equivalents are within the scope of the present invention. The invention provides exemplary methods, devices and device components for monitoring and controlling the position of phase boundaries in a rotating separation chamber with improved sensitivity over conventional one-dimensional optical monitoring methods. In addition, the present invention provides multi-functional optical monitoring and control systems capable of monitoring and controlling diverse operating conditions of a density centrifuge. These and other

variations of the present optical monitoring and control systems are within the spirit and scope of the claimed invention. Accordingly, it must be understood that the detailed description, embodiments, drawings and examples set forth here are intended as illustrative only and in no way represent any limitations on the scope of the invention.

It will be apparent to one of ordinary skill in the art that methods, devices, device elements, materials, procedures and techniques other than those specifically described herein can be applied to the practice of the invention as broadly disclosed herein without resort to undue experimentation. All art-known functional equivalents of methods, devices, device elements, materials, procedures and techniques specifically described herein are intended to be encompassed by this invention.

Example 1: Monitoring the position of phase boundaries between optically differentiable blood components undergoing density centrifugation.

The ability of the methods and devices of the present invention to monitor and control the position of phase boundaries between optically differentiable blood components was verified by experimental studies. Specifically, it is a goal of the present invention to provide optical monitoring and control systems capable of accurately measuring the position of one or more phase boundaries along the separation axes of a separation chamber of a density centrifuge blood processing apparatus. Further, it is a goal of the present invention to provide optical monitoring and control systems capable of selectively adjusting the position of one or more phase boundaries along the separation axis of a separation chamber to achieve optimal separation and extraction of blood components.

To achieve the aforementioned goals, two-dimensional distributions of transmitted and/or scattered light intensities comprising images of an optical cell containing human blood undergoing density centrifugation were measured for a variety of extraction flow conditions. The optical monitoring and control system evaluated comprises a light source, a close focus lens system, and a digital camera, arranged as illustrated in Figures 1 and 2. The light source is a combination of a xenon lamps and light emitting diodes which provides incident beams comprising white light which is directed through a windowed optical cell of the separation chamber. This configuration provided illumination of both the top and
10 bottom of the windowed optical cell. The digital camera is an industry standard 1/3 inch DVT camera manufactured by DVT. The digital camera and lens set are positioned above the separation chamber such that phase boundaries between optically differentiable blood components are viewable as the optical cell is rotated into the observation region. Two dimensional distributions of transmitted and scattered light comprising two-dimensional color images were acquired upon every other rotation of the separation chamber. The illumination and detector configuration employed provided a horizontal field of view of approximately 32 mm, a vertical field of view of approximately 24 mm, a horizontal resolution of approximately 19.4 pixels mm⁻¹ and a vertical resolution of approximately
20 19.4 pixels mm⁻¹. As will be evident to a person of ordinary skill in the art, the exemplary optical components and configurations described above are but one means of generating, collecting and detecting patterns of light corresponding to a observation region and functionally equivalent lens and detector arrangements are intended to be within the scope of the present invention.

The centrifuge is equipped with a single stage separation chamber with an optical cell having a plurality of transmissive extraction ports. It is understood that the separation chamber could also be dual stage with extraction ports in different positions on separation chamber. Also the separation chamber could be formed of

multiple chambers connected by tubing. As will be clear to one skilled in the art, other known centrifuge apparatus could be used. The separation chamber is also equipped with calibration markers for quantifying absolute phase boundary positions along the separation axes and for quantifying transmitted light intensities corresponding to separated blood components. The separation chamber is held in place by a circular filler which rotates about the central axis of the density centrifuge. The filler is also provided with calibration markers. The optical cell is equipped with three extraction ports, which terminate in the separation chamber at selected distances along the separation axis. The three extraction ports correspond

10 to a plasma component, a buffy coat layer and a red blood cell component. First and second extraction ports corresponding to the plasma component and the buffy coat layer, respectively, are operationally connected to peristaltic pumps which are capable of establishing an extraction flow rate out of the separation chamber selected over the range of about $0.1 \text{ cm}^3 \text{ m}^{-1}$ to about $250 \text{ cm}^3 \text{ m}^{-1}$. Peristaltic pumps connected to the density centrifuge are controlled by a computer, which is in two-way communication with the digital camera. Red blood cells exit the extraction port via a flow established by the centrifugal force and inlet pump.

Figure 6 is a top plan view of an optical cell **1100** of a separation chamber showing an expanded region **1101** illustrated in Figures 6A and 6B. Figure 6A

20 shows a schematic of an image generated by the methods of the present invention of expanded region **1101** having a human blood sample therein separated into blood components. The inlet flow rate of blood sample to the separation chamber was 75 ml min^{-1} and the flow rates of red blood cells and plasma components out of the separation chamber were $53 \text{ cm}^3 \text{ min}^{-1}$ and $20 \text{ cm}^3 \text{ min}^{-1}$, respectively. The image in Figure 6A includes a phase boundary monitoring region **725**, a calibration region **726** and extraction port **865** having orifice **727**. Visible in the phase boundary monitoring region **725** are a red blood cell containing component **730**, a plasma component **732** and a mixed phase buffy coat layer **734** having both white blood

cells and platelets. A first stable phase boundary **736** between red blood containing component **730** and an buffy coat layer **734** and a second stable phase boundary **738** between the buffy coat layer **734** and a low density plasma component **732** are both viewable in phase boundary monitoring region **725**. Visible in calibration region **726** is the first calibration marker comprising the edge **740** of the optical cell and a second calibration marker **742** comprising a series of bars 1 mm in thickness and having a known absorption and scattering characteristics. First and second calibration markers provide references for optimizing focusing of the light collection element, indicating the positions and physical dimensions of portions of the phase boundary monitoring region **725** and measuring the positions of phase boundaries between the red blood cell containing component, the buffy layer and the plasma component.

Analysis of the image in Figure 6A was performed in real time and provided measurements of the position of first and second boundary layers. The average intensities of transmitted light corresponding to each blood component were also determined and analyzed with respect to the intensities of transmitted red light, green light and blue light. The position of first stable phase boundary **736** between red blood cell containing component **730** and an intermediate buffy coat layer **734** was determined to be 9.8 ± 0.1 mm, relative to first calibration marker **740**. The position of second stable phase boundary **738** between the buffy coat layer **734** and a low density plasma component **732** was determined to be 7.7 ± 0.1 mm, relative to first calibration marker **740**. Average transmitted light intensities corresponding to each blood component were determined using a 0-100 relative intensity scale for red light, green light and blue light components of the transmitted light wherein a value of 0 indicates no detected light and a value of 100 corresponds to transmitted light intensities which saturate the detector. The average transmitted light intensity levels of the red blood cell containing component **730** were determined to be 9, 7, and 8 for red light, green light and blue light

components, respectively. The average transmitted light intensity levels of the buffy coat layer **734** were 26, 23 and 19 for red light, green light and blue light components, respectively. The average transmitted light intensity levels of the plasma component **732** were 63, 48 and 27 for red light, green light and blue light components, respectively.

Figure 6B shows a schematic of an image of the separation chamber upon increasing the flow rate of the plasma component out of the separation chamber to equal 22 ml min^{-1} and decreasing the flow rate of the red blood cell containing component out of the separation chamber to equal 51 ml min^{-1} . The inlet flow rate of blood sample to the separation chamber was held constant at 75 ml min^{-1} . Analysis of the image in Figure 6B was performed in real time and provided measurements of the position of first and second boundary layers and the average intensities of transmitted red light, green light and blue light for the modified flow conditions. The position of first stable phase boundary **736** between red blood containing component **730** and an intermediate buffy coat layer **734** was determined to be $9.2 \pm 0.1 \text{ mm}$, relative to first calibration marker **740**. The position of second stable phase boundary **738** between the intermediate buffy coat layer **734** and a low density plasma component **732** was determined to be $7.4 \pm 0.1 \text{ mm}$, relative to the to first calibration marker **740**. The average transmitted light intensity levels of the red blood cell containing component **730** were determined to be 11, 8, and 6 for red light, green light and blue light components, respectively. The average transmitted light intensity levels of the buffy coat layer **734** were 24, 20 and 17 for red light, green light and blue light components, respectively. The average transmitted light intensity levels of the plasma component **732** were 63, 46 and 27 for red light, green light and blue light components, respectively.

Figures 6A and 6B show that the present invention is capable of monitoring the position of phase boundaries between separated blood components in real time. In addition, a comparison of Figs. 6A and 6B demonstrates that adjustment of

the flow rate of one or more selected blood components out of the separation chamber results in a change in the positions of phase boundaries between separated blood components along the separation axes. Specifically, increasing the flow rate of the plasma component out of the separation chamber and decreasing the flow rate of the red blood cell containing component out of the separation chamber resulted in a shift of the position of the first phase boundary between the red blood cell containing component and the buffy coat layer toward the first calibration marker.

10 The images shown in Figures 6A and 6B illustrate the ability of the optical monitoring and control system to resolve the position of a plurality of phase boundaries between separated blood components. In addition, the images shown in Figures 6A and 6B also illustrate the ability of the optical monitoring and control system to adjust the flow rates of extracted blood components in a manner providing control over the position of phase boundaries between separated blood components. The ability of the monitoring and control system of the present invention to selectively adjust the position of phase boundaries between separated blood components allows phase boundary positions to be optimized to provide extracted components having a desired composition and purity. Specifically, the present invention provides a means of controlling the position of phase boundaries
20 between optically differentiable components such that only a single blood component is proximate to the terminus of a selected extraction port.

Example 2: Measurement of the composition and flux of cellular material out of a density centrifuge.

It is a goal of the present invention to provide multifunctional optical monitoring systems capable of monitoring a plurality of operating conditions of a blood processing device. Specifically, it is a goal of the present invention to provide monitoring and control systems providing simultaneous measurements of phase boundary positions and the fluxes of cellular materials, such as white blood cells,

platelets and red blood cells, out of a separation chamber of a density centrifuge. Further, it is a goal of the present invention to provide optical monitoring systems capable of characterizing the cell-type of material separated, extracted and collected. The ability of optical monitoring systems of the present invention to simultaneously monitor the position of phase boundaries in the separation chamber and the composition and flux of cellular blood components through an extraction port was verified by experimental studies.

To achieve the aforementioned goals, two-dimensional distributions of transmitted and scattered light intensities comprising two-dimensional images of separation and extraction regions of an optical cell of a rotating separation chamber in a density centrifuge were measured and analyzed in real time to provide simultaneous measurements of the positions of boundary layers between optically differentiable blood components and the compositions and fluxes of cellular materials out of the separation chamber. The optical monitoring and control system evaluated comprises a light source, a close focus lens system, and a digital camera, arranged as illustrated in Figures 1 and 2 and as described in Example 1. Illumination is provided by a light source positioned beneath the separation chamber which is capable of directing light through a white blood cell extraction port of the optical cell. Illumination is also provided to the top of the optical cell. Light transmitted through and scattered by the optical cell was collected by the close focus lens system and detected by the digital camera. Two dimensional distributions of transmitted and scattered light were acquired for every other rotation of the separation chamber at a rotational velocity of 1490 revolution min.⁻¹.

Figure 7 shows an image generated by the methods of the present invention corresponding to the separation of a human blood sample and extraction of a separated white blood cell-containing blood component. The image in Figure 7 includes a phase boundary monitoring region **800** and a white blood cell extraction port monitoring region **805** of the optical cell. Visible in phase boundary monitoring

region **800** are a red blood cell containing component **810**, a plasma component **820** and a mixed phase buffy coat layer **830** having both white blood cells and platelets. Several calibration markers are also apparent in the image in Figure 7. The edge **840** of the optical cell comprises a first calibration marker for determining the absolute position of phase boundaries between optically differentiable blood components. A series of bars **850** having a thickness of 1 mm and known scattering and absorption characteristics comprises a second calibration marker useful for optimizing the focusing of the light collection element and indicating the positions and physical dimensions of the phase boundary monitoring region **800** and the
10 white blood cell extraction port monitoring region **805**. Light intensities transmitted through the phase boundary monitoring region **800** were acquired as a function of time and analyzed in real time to provide measurements of the position of the phase boundary **855** between red blood cell component **810** and buffy coat layer **830** and the phase boundary **857** between the buffy coat layer **830** and plasma components **820**. All boundary layer positions were measured relative to the edge of the optical cell **840**.

White blood cell extraction port monitoring region **805** includes a first flux monitoring region **860** and a second flux monitoring region **863** positioned on white blood cell extraction port **865** of the optical cell. In this example, extraction port **865**
20 having orifice **727** is configured to collect white blood cells in the human blood sample and extends a distance along the separation axis of such that it terminates proximate to the buffy coat layer in the rotating separation chamber. The two-dimensional distribution of light intensities of light transmitted through the first and second flux monitoring regions **860** and **863** depends on the concentration, and spatial distribution and cell-type of cellular material exiting the separation chamber. Light intensities transmitted through first and second flux monitoring regions **860** and **863** were acquired as a function of time and analyzed to characterize the composition and flux of cellular material out of the separation chamber. As cellular

material, such as white blood cells and red blood cells, absorbs and scatters light from the light sources, passage of cellular material through the extraction port was observed to decrease the observed transmitted light intensities.

Figures 8 shows the temporal behavior of the phase boundary layer positions in the optical cell and transmitted light intensities through the extraction port monitoring region during white blood cell collection. The position of the phase boundary separating the red blood cell containing component **810** and the buffy coat layer **830** as a function of time is indicated by solid diamond markers (and designated as RBC Pixels in Figure 8) and the position of the phase boundary separating buffy coat layer from the plasma layer as a function of time is indicated by open square markers (and designated as Platelet Pixels in Figure 8). Figure 8A shows 50-point moving averages corresponding to the position of the phase boundary separating the red blood cell containing component and the buffy coat layer (designated as RBC Pixels in Figure 8A) and the position of the phase boundary separating buffy coat layer from the plasma layer (designated as Platelet Pixels in Figure 8A) to better illustrate the temporal behavior of these parameters. As shown in Figures 8 and 8A, plots corresponding to the different phase boundaries do not intersect. This observation indicates that separation of the blood sample was maintained throughout extraction and collection. As shown in Figures 8 and 8A, plots corresponding to different boundary layers exhibit similar periodic behavior with maxima occurring at approximately the same times. The periodic nature of the plots shown in Figures 8 and 8A arises from the pumping characteristics of the peristaltic pumps and the surface tension of cellular material exiting the separation chamber.

A plot of the median transmitted intensities through the first flux monitoring region as a function of time is also shown in Figure 8 as solid triangle markers (and designated as Extraction Port Tool #1 in Figures 8 and 8A) and a plot of the median transmitted intensities through the second flux monitoring region as a function of

time is also shown in Figure 8 as X markers (and designated as Extraction Port Tool #2 in Figures 8 and 8A). Figure 8A shows the corresponding 50-point moving averages for first and second flux monitoring regions. Both plots of the median transmitted intensities exhibit periodic behavior similar to that shown in the phase boundary measurements. The correlation between the maxima and minima in each of the plots in Figures 8 and 8A suggests that the separation was effective and maintained throughout extraction and collection.

Integration of the plots in Figure 8 of the median transmitted intensities through the first and second flux monitoring regions as a function of time provides a measurement of the net amount of cellular material collected during the extraction period. To verify this aspect of the present invention, aliquots of blood components passing through the white blood cell extraction port were analyzed to provide complementary measurements of the composition of the extracted material. Aliquots of extracted material were collected over 3 minute sampling intervals and were subsequently analyzed using flow cytometry methods well known in the art. Figure 9 shows a series of plots (X markers, + markers and - markers) of the observed white blood cell concentrations as a function of the median intensity of light transmitted through the second flux monitoring region. As shown in Fig. 9, the concentration of white blood cells collected for a given aliquot is inversely correlated to the observed median transmitted light intensity. The inverse correlation in Figure 9 provides an experimental verification that methods of the present invention provides real time measurements of the cellular composition of material extracted from the separation chamber. Also shown in Figure 9, are plots (diamond markers, square markers and triangle markers) of the hematocrit of the extracted material as a function of the median intensity of light transmitted through the second flux monitoring region.

Figure 10 shows a plot of the concentration of white blood cells in the extracted material as a function of the position of the phase boundary between the

red blood cell containing component and the buffy coat layer for the rotational velocities (RPM) indicated in the legend. The linear relationship shown in Figure 10, provides a useful index to allow the operator of the monitoring and control system to set the phase boundary between the red blood cell containing component and the buffy coat layer in a manner providing a desired concentration of extracted white blood cells.

Example 3: Methods of real-time image processing and device control.

10 The present invention also includes a variety of methods for processing data from an optical monitoring system corresponding to two dimensional distributions of transmitted and/or scattered light intensities to provide real time measurements of important operating parameters. Methods of organizing, processing and analyzing optical data are used in the present invention to generate input signals useful for monitoring and controlling blood processing. The present invention includes several computational approaches to managing and synchronizing data acquisition, data analysis and device control processes.

A. Master - Smart Slave Process Control System for Controlling Blood Processing.

20 Using computer science terminology for information transfer, a process control system of the present invention can be conceptualized as a data "Client" as it requests specific information from the optical robot / smart sensor. Similarly, the optical robot / smart sensor can be conceptualized as a data "Server" as it provides the specific information that the process control system requests. Therefore, the present invention includes certain aspects of a "Client / Server" design. Using engineering terminology for command and control, the process control system can be conceptualized as a "Master" component since it commands the optical robot / smart sensor, and the optical robot / smart sensor can be conceptualized as a "Slave" component since it responds to process control system commands.

In one aspect, the present invention provides a blood processing controller having a master - smart slave process control system, which is particularly useful for providing automated control of a blood processing device or a blood processing procedure. Use of the term "master - smart slave control system" in the present invention refers to a hardware and software architecture wherein a master Procedure Control system generates control signals requesting specific information from a smart slave data acquisition and analysis system. A smart slave data acquisition and analysis system of the present invention is capable of performing measurements to ascertain information requested from the master Procedure Control system. Furthermore, a smart slave data acquisition and analysis system of the present invention is also capable of optimizing measurement conditions to achieve the best information to return to the master Procedure Control system. At any time during the procedure, however, the master Procedure Control system can switch modes and command the smart slave data acquisition and analysis system to examine a different set of parameters. This ability to dynamically change what area or parameters are being monitored, utilizing different reference points and delivering different examination sets, is beneficial because it provides better error detection and device management.

A primary advantage of the master - smart slave process control system of the present invention is that it provides the ability to extract and analyze optical measurements of important operating parameters of a blood processing device on a very short time scale, preferably on a time scale of less than about 50 milliseconds. Exemplary data analysis methods of the present invention provide control systems capable of correlating a plurality of measurements in real time to provide the best measurement of the composition of blood sample undergoing processing and/or to optimize a selected blood processing procedure. In addition, data analysis methods of the present invention also include predictive data analysis algorithms capable of monitoring trends in important measurements in real time

which enables the process control system to respond to changes in blood processing conditions or sample composition quickly. Furthermore, data analysis methods of the present invention are capable of evaluating uncertainties in optical measurements in real time, which provides an important index for product validation and quality control assessments.

Figure 11 shows a schematic of an exemplary master - smart slave process control system of the present invention capable of controlling blood processing. The exemplary control system **900** illustrated in Figure 11 comprises master Procedure Control system **905** in two way communication with a smart slave data acquisition and analysis system **910**. Master Procedure Control system **905** is capable of receiving input signals corresponding to a selected blood processing procedure, a sample undergoing processing and/or a patient undergoing treatment. Based on these input signals, master Procedure Control system **905** generates and transmits procedure requests and procedure commands **915** to the smart slave data acquisition and analysis system **910**. In a preferred embodiment, master Procedure Control system **905** also generates and transmits a series of test commands **920** to smart slave data acquisition and analysis system **910**. Smart slave data acquisition and analysis system **910** is capable of receiving test commands **920** and generating test response signals **922** which verify that control system **900** is fully functional and that the patient or blood sample identified by the smart slave data acquisition and analysis system **910** is correctly associated with the selected blood processing procedure or therapy.

Smart slave data acquisition and analysis system **910** has a distributed processing architecture and comprises a first computer processor **924** in two-way communication with a second computer processor **926**. First computer processor **924** is configured to receive procedure requests and procedure commands **915** from master Procedure Control system **905** and transmit processing commands **932** to second computer processor **926**. Second computer processor **926** analyzes

the processing commands **932** and transmits camera setting commands **934** to the CCD camera and light collection element **928** which provide information related to establishing the proper exposure time, camera and light collection element position, field of view, color or monochrome imaging and other parameters necessary for acquiring high quality images of the blood processing device. First computer processor **924** is also configured to transmit illumination control and triggering commands **936** to light source and camera triggering hardware **937**. Using centrifuge positional encoder data, triggering hardware **937** transmits electronic trigger signals to the light source driver circuits **939** and camera trigger **940**.

10 Camera and light collection element **928** measure two dimensional distributions of transmitted and/or scattered light intensities comprising images of an observation region on a blood processing device or blood sample undergoing processing. The raw image data **941** is transmitted to the second computer processor **926** for image formatting and real time image processing. In an exemplary embodiment wherein the process control system is operationally connected to a density centrifuge, an image is acquired upon every other rotation of the separation chamber. For a rotational velocity of 3000 rotations per minute, this corresponds to acquisition of an image every 40 milliseconds.

The formatted image data is operated on by second computer processor **926**

20 using one or more image-processing algorithms, each of which correspond to a different desired measurement or plurality of measurements. Image-processing algorithms extract measurements from the image data and determine critical and salient information about physical and chemical characteristics of the blood components undergoing processing and the operation of the blood processing device itself. Image-processing algorithms examine and quantify the image data in both the spatial and frequency domains. Image-processing methods include the following industry standard techniques: 2D-convolutions, 2D-transforms, histograms, thresholding, edge / line detection, segmentation, mensuration,

morphological filters, spatial filters, frequency domain filters, nonlinear filters, adaptive filters, bayesian filters, graphics and color image processing algorithms. Operation of an image-processing algorithm on the formatted image data generates numerical measurement data **943**, which is used to populate data fields of derived image objects. Therefore, at least one image data object is created every time new image data is received by the image data acquisition algorithms. In addition, a corresponding time stamp is be fed in to the image data object upon its instantiation. Time stamp information is used to track the rotational velocities of the centrifuge and to generate sampling rate information utilized in calculating velocity and acceleration values for the parameters of interest. Additional time stamps can be assigned to image data objects corresponding to different states in the data acquisition, analysis and handling process. It is important to note, however, that the image data object does not contain the actual graphical image data. Rather, the image data object contains one or more measurements extracted by operation of the image-processing algorithms.

Immediately after creation of a new image data object, it is placed onto a linked list of image data objects designated as the image data list **944**. This list stores and enqueues image data information backwards in time. For an acquisition rate of 25 frames per second, 25 image data objects are inserted onto the image data list every second. Maintaining an image data list limited to a finite set of image data objects is beneficial because it prevents over-consumption of the system memory and avoids system failure due to over-consumption of computational resources. Therefore, the image data list acts as a managed circular buffer by deleting the oldest image data off the tail end of the list while inserting newly acquired image date at the head of the list. In an exemplary embodiment, a cooperative list manager algorithm manages the storage and removal of image data objects in the image data list. Importantly, an input - output bottleneck is avoided by using the dual processor design of the present invention because the

image data objects are stored in memory and periodically examined by the first computer processor **924**. This aspect of the process control system allows data processing, analysis and evaluation on a very short time scale, preferably for some applications less than 50 milliseconds.

Image data objects in the image data list are periodically examined by the first computer processor **924** and provide key data sets for monitoring and controlling blood processing. First computer processor **924** operates on image data objects in the image data list using multiple-image-data object analysis and evaluation algorithms. For example, applied image-data analysis algorithms can
10 evaluate a single image data object or a short series of image data objects to determine the resolution of the acquired image, the brightness levels of an acquired image, the field of view of the observation area or other aspects of the monitoring and control system. Measurements generated from the operation of the image-data analysis algorithms establish the basis of image information output signals **948** sent to the master Procedure Control system **905**. Image information output signals provide information requested by the master Procedure Control system **905**. For example, information output signals **948** can be related to the purity of extracted blood components or the amount of collected materials. Image information output signals can also provide alarm signals indicating that the blood processing system
20 or image processing system is not working as expected or indicating a rapid change in the composition of the blood sample undergoing processing.

Measurements generated from the operation of the image-data analysis algorithms and process control algorithms also serve as the basis of output signals sent to the camera and light collection element **928**, light source and camera triggering hardware **937** to optimize the quality of the images acquired and analyzed. For example, output signals can adjust in the intensity of the illumination beam, change the color of the illumination beam, or adjust the camera's gain or exposure time. In this manner, smart slave data acquisition and analysis system **910** acts as

a smart sensor capable of dynamically optimizing the quality of the measurements requested by the master Procedure Control system **905**.

In one embodiment, list manager algorithms communicate with process control and image data analysis algorithms to determine how long the link-list should be. The list manager algorithms can also manage simultaneous access to the list by utilizing either mutexes, semaphores or critical sections. This is an important feature since the algorithms inserting image data objects onto the list and those reading a series of frames of image data objects are generally asynchronous multiple threads.

10 In an exemplary embodiment, first computer processor **924** operates on the image data list using predictive image data analysis algorithms to examine one or more trends in the image data parameters. The specific predictive algorithms read the object data list periodically, examine a series of image data objects acquired during a given time interval and analyze the series for changes in a plurality of selected parameters of interest. For example, a specific predictive control algorithm can examine changes in the position of a phase boundary along the separation axis and/or the composition of a blood component exiting the separation chamber. In an exemplary embodiment, a predictive image data analysis algorithm analyzes the object data list every time a new image is acquired and the object data list is then
20 analyzed as pair of chronologically ordered frames for the purpose of comparative analysis. These frames are denoted as current frame and previous frame. The current frame contains the most recently acquired image data object, and a specified number chronologically ordered data objects that immediately preceded the most recently acquired data object. The previous frame contains a matching number of chronologically ordered image data objects, starting with the image data object sequenced immediately before the oldest image data object in the current frame. Predictive image data analysis algorithms compare and correlate a plurality of parameters from the two frames to derive positional, directional, characteristic,

and associated rates of change information relating to the desired extracted image data information. Discrete magnitudes of changes in a plurality of parameters as a function of corresponding discrete time intervals are used to derive velocity and acceleration information for the specific parameters of interest. This rate information, along with specific associated positional or quantitative characteristic data is used to generate Image Information data packets **948** sent to the master Procedure Control system **905**. In an exemplary embodiment, master Procedure Control system **905** uses the Image Information data sent on a periodic basis by first computer processor **924** along with discrete extraction pump flow data as
10 inputs to a discrete data closed loop transfer function. In turn, the output values of the discrete data transfer functions are used to automatically manipulate the operating conditions of the centrifuge, such as plasma flow rate out of the separation chamber, rotational velocity, collect flow rates.

The primary goal of the image processing and control systems of the present invention is to provide automatic tracking and maintenance of optimal separation conditions for a particular blood processing application or therapy. For example, a exemplary data processing system is designed to maximize the efficiency of white blood cell collection by allowing the system to skim off the specific, desired types of cells, while minimizing contamination by collecting unwanted cell types. A
20 significant advantage of the automated data processing methods of the present invention is that they free up time of the nurse or physician operating the blood processing apparatus to concentrate on patient care. In addition, the automated data processing methods of the present invention improves consistency and quality of the collected blood components.

In one embodiment, the data processing methods of the present invention are capable of monitoring and tracking the position of the phase boundary between red blood cells and less dense blood components along the separation axis. In an exemplary embodiment, a predetermined control value can be established, wherein

the measured position of the phase boundaries exceeds the predetermined control value, a signal is generated which rapidly de-accelerates the plasma flow rate in a manner capable of restoring the red blood cell level to below the control value.

In another preferred embodiment, the data processing methods of the present invention characterize and track the cells flowing up and out of a given extraction port. In this method images corresponding to one or more extraction port are acquired and processed provide real time measurements of the number and cell-type of cellular material exiting the separation chamber.

10 A key advantage of the optical monitoring system and data processing method of the present invention is that a plurality of key operating parameters are simultaneously monitored and dynamic adjustments based on the combination of these measurements can be made in real time. Artificial intelligence algorithms can take the data generated and utilize it in a dynamic multi-variable decision making matrix. Importantly, the system perform different correlations on the different data sets to optimize and manage a blood component collection process and quality of the blood components collected. For example, in an exemplary embodiment, the red blood cell level and collected blood component concentration are concurrently examined using the methods of the present invention. The combination of both measurements provides a description of the blood processing process far more
20 complete than conventional systems for controlling blood processing. For example, detection of an acceptable red blood cell level in the separation chamber and a very low concentration of collect red blood cells can be indicative of the presence of a clot in the red blood cell extraction port. Therefore, upon observing this combination of measurements, an output signal can be generated which reduces the plasma pump and then rapidly accelerated the plasma and collect pumps to blow the clot out of the extraction port.

In another embodiment, the thickness of a buffy coat layer comprising white blood cells is monitored in real time. As white blood cells are removed from the blood sample, the buffy coat layer gets thinner and thinner, thereby change the position of phase boundaries relative to the inlet of an extraction port. The ability of the present invention to track these changes in real time allows for better collection and higher purity of the removed white blood cell fraction. For example, statistical models can be applied to adjust the control value associate with the position of the phase boundary between a red blood cell component and a buffy coat layer to optimize collection of white blood cells while minimizing the unwanted collection of red blood cells.

In a preferred embodiment, the smart slave data acquisition and analysis system serves as a slave robot to the master Procedure Control system. The master Procedure Control system selects a specific therapeutic procedure that an operator has requested. Next, the master Procedure Control system loads the corresponding software module for that procedure and starts the procedure. At this time the specific procedure will establish communication with the smart slave data acquisition and analysis system. Then the procedure within the master Procedure Control system will query the smart slave data acquisition and analysis system and determine if it has an imaging procedure algorithm that is a suitable match for the therapeutic procedure loaded into the master Procedure Control system. If a suitable match is found, then the master Procedure Control system will command the smart slave data acquisition and analysis system to load the appropriate software module and start running it. Once the therapeutic procedure in master Procedure Control system links up with the imaging procedure in the smart slave data acquisition and analysis system, it will command the imaging procedure to go into the specific monitoring and data analysis routines associated with the specific procedure. The master Procedure Control system will also command the smart slave data acquisition and analysis system to report back image information and

data packets at a pre-configured periodic rate. The image information and data packets contain critical information pertaining to control parameters relevant to the specific procedure. The master Procedure Control system can utilize image data information as long as necessary for certain measurement.

B. Partially Distributed Software Executed Methods for Controlling Blood Processing.

The present invention provides software executed methods for monitoring and controlling blood processing via density centrifugation. Methods of the present invention include fully automated control systems comprising a partially distributed
10 software system running on a single processor or multiprocessor computing system. Exemplary methods of the present invention optimize the amount of information extracted from one or more two dimensional distributions of transmitted and/or scattered light intensities comprising images of a blood processing device or device component. In addition these methods provide real time data analysis, error detection and device control based on a plurality of predictive system control algorithms. The ability of methods of the present invention to effectively analyze large amounts of optical data and selectively adjust operating conditions in real time is particularly beneficial for processing blood samples exhibiting a highly variable
20 compositions, such as those commonly encountered in patients undergoing therapy, and therapeutic applications wherein significant changes in a patient's blood composition commonly occur during processing.

3B(i). Control System Overview

Figure 12 provides a schematic flow diagram illustrating an automated, computer controlled process control system for a density centrifuge blood processing device. The illustrated process control system is a digital imaging based smart sensor that monitors blood component processing within a separation chamber of a density centrifuge. The overview provided in Figure 12 indicates

major software components and important data paths of the process control system useful for providing device monitoring and control in real time.

The illustrated process control system comprises a Control Subsystem and an Automated Process Control (APC) Sub-System. As the process control system employs a software architecture having some components that are executed on a Control Sub-System, it can be conceptualized as a partially distributed software model. Use of a partially distributed software model in the present invention is preferred for some applications because it provides an efficient way of acquiring, processing, analyzing and using large amounts of image data.

10 The physical boundary between the APC Sub-System and the Control Sub-System is indicated by the dashed line in Figure 12. Additional device components are also indicated in Figure 12, such as the digital camera and synchronization timing controller (STC), to illustrate how elements of the process control system are interfaced with additional device components useful in the methods and devices of the present invention. These additional device components can be viewed as stand alone elements in communication with the process control system or as integral parts of the APC Sub-System. For example, the digital camera and STC can comprise embedded type (firmware-based) micro-controllers that are controlled and monitored through the APC Driver component of the APC Sub-System.

20 Referring again to Figure 12, there are two main data loops within the process control system software architecture. First, an Image Analysis Loop is provided which is contained completely within the APC Sub-System. This data loop is responsible for acquisition, processing and analysis of image data provided by a CCD camera in optical communication with a density centrifuge blood separation device. Second, a Control Loop is provided which is distributed between the APC subsystem and the Control Sub-Systems. This data loop is responsible for using

the analyzed image data to control and optimize a procedure running on a blood processing system.

In the Image Analysis Loop, the APC Executive determines the type of image analysis to be performed, and sends APC processing orders to the APC Driver. These processing orders contain selected information including, but not limited to, camera exposure settings, STC trigger settings, and image processing orders for the sequence of one or more images required for a selected analysis. In one embodiment, once a set of orders is sent to the APC Driver, it will normally continuously execute the orders until another set of orders is received. The APC Driver provides key hardware components with initialization and command information which appropriately prepares the hardware for the acquisition of a desired image or plurality of images. The APC Driver then receives the resulting image data and forwards this data along with a copy of the STC and camera settings, and the image processing orders to the Image Processing Engine. Packaging by annotating the image data with complementary command and device setting data allows the APC Driver to handle all of the time-critical operations required to synchronize the image data with settings used to generate the image and the orders necessary to process the image. In addition, packaging in this manner eliminates requirements for tight time-coupling among the other APC software and hardware components. The Image Processing Engine performs the requested operations for each image, and inserts analyzed data for each image frame into a Image Data List Container. The processing provided by the Image Processing Engine effectively reduces the large amount of data contained in the image itself to a small set of measured parameters. The APC Executive obtains the analyzed data from the Image Data List Container and copies this data into local buffers as necessary, allowing it to perform analysis operations requiring multiple frames of data. This aspect of the invention allows trends in several frames of data to be extracted and used as input in important predictive device control algorithms.

In regard to the Image Analysis Loop, it is important to note that listing the operations in this order does not imply that a single image frame is processed to completion, and only then is the next frame started. Rather, each step runs concurrently, allowing higher image throughput rates. This functional capability of the present control system can be conceptualized as operation of a computation pipeline capable of performing a large number of independent computations on different data sets. For example, while the Image Processing Engine is busy analyzing one image, the APC Driver can be reading the data for the next image from the camera and preparing the next data packet for the image processing engine.

In the Control Loop, The APC Executive sends analyzed image data and status to the Control Driver. The Control Driver uses the image data to determine appropriate operating setting of the density centrifuge including but not limited to, inlet and extraction pump flow rates, valve positions, and rotational velocity of the density centrifuge. The Control Driver also makes this status available to Procedure Control through the Machine State Data. Procedure Control uses information on the current procedure as well as APC status information and data to determine one or more APC orders, and to adjust parameters used by the Control Driver. The APC Executive receives orders and procedure status from Procedure Control, and uses this information to determine the appropriate APC processing orders for a selected blood processing procedure or device configuration.

To further illustrate the capabilities of the present control system and not intending to imply any limitations on its design and uses, an example is presented below to further clarify the operations of the process control system of the present invention. For this example, the APC Sub-System is in steady-state measurement mode for a mononuclear cell (MNC) collection. Upon first entering this mode, the APC Executive writes the orders for the frame sequence required and the APC Driver will repeat the sequence until ordered otherwise. Assuming that the APC

Executive has ordered a series of eleven image frames corresponding to two dimensional distributions of transmitted or scattered light intensities to be collected. The first ten frames specify measuring the red-cell interface position and optical density of the fluid in an extraction port corresponding to a collection port. The final frame specifies a somewhat more lengthy image analysis, intended to monitor image data relating to the quality of the images being collected, and thus relating to the reliability of the measurements collected in the other frames.

In this example, the APC Driver collects each of the frames in sequence, forwarding image data and image processing orders to the Image Processing Engine. The Image Processing Engine analyzes each of the frames and places the analyzed data for each image frame in the Image Data List Container. The APC Executive receives the analyzed data and splits it into two data streams: a first data stream for the measurement frames and a second data stream for the image quality assessment frames.

Information from the quality assessment frames is used by the APC Executive to determine the reliability of the measurements. The reliability information is sent to the Control Sub-System along with the measurement data. The quality assessment frames can also be used by the APC Executive to fine-tune device parameters to improve image quality. However, the APC Executive is only allowed to autonomously adjust parameters that do not potentially introduce measurement bias. For example, increasing the amount of light used for the images can make the red-blood cell interface more distinct, but can also cause an apparent shift in the interface position. In one embodiment, significant adjustments to improve image quality (such as re-calibrating the lighting and exposure to re-optimize image quality) must be ordered by Procedure Control.

The optical density measurements are then processed to determine the current efficiency of the collection. The measurements are sent to the Control

Driver, and then sent to the Machine State Data. Procedure Control uses these measurements to adjust the commanded interface position used by the Control Driver to optimize the collection. In one embodiment, the current interface position measurement is filtered by the APC Executive, and the APC Executive reports the filtered value along with trend information to the Control Driver. This data is used internally by the Control Driver to adjust operating parameters, such as peristaltic pump flow rates and the rotational velocity of the centrifuge, as necessary to maintain the commanded interface position.

10 The exemplary control system illustrated in Figure 12 can be executed using a multiprocessor computing system. Selected components of control systems of the present invention can be run in a distributed fashion on separate processors. In one embodiment, the Procedure Control and the Control Driver run on a first processor, the Image Processing Engine runs on a second processor and the APC Executive runs on a third processor. Use of multiple processing computing methods in the present invention allows measurements to be extracted from a large amount of raw image data, and allows the measurements to be used to provide flexible dynamic device control on very short time scales, such as a time scale less than 50 milliseconds.

20 APC Sub-System and Control Sub-System can be configured in two-way communication via any means known in the art, such as an Ethernet connection. Components of either the APC Sub-System or the Control Sub-System can be configured to be in two-way or one-way communication via use of shared memory. In an exemplary embodiment, however, the APC Sub-System and the Control Sub-System do not communicate using shared memory.

The process control system of the present invention can also be configured to provide for effective data archiving of raw image data, processed image data and device settings. This functionality of the present invention allows a user to review

blood processing data after a selected procedure to extract additional information, such as information related to the composition of collected blood components or the effectiveness of a given therapy. In the present invention, data archiving can be achieved by the APC Sub-System, the Control Sub-System or both. At least a portion of data extracted from acquired two-dimensional distributions of transmitted light intensities, such as measured operating parameters, are optionally also displayed to an operator or service technician.

2B(ii) Control Driver and APC Sub-System relationship.

10 Figure 13 is a schematic diagram showing exemplary Control Driver and APC Sub-System architectural relationships useful in the methods of the present invention. For the sake of clarity, only APC relevant message paths and objects are included in Figure 13.

In the embodiment illustrated in Figure 13, APC proxy task within the Control Driver contains closed loop transfer functions that dynamically determine important centrifuge device settings including, but not limited to, pump flow rates, valve positions, and rotational velocity of the centrifuge, to achieve process control targets specified by Procedure Control. The transfer function performs hardware adjustments to minimize the difference between the error signals and the desired reference parameters. Procedure Control uses the APC status information to verify
20 the operation of the APC and uses the APC data to obtain overall processing, predictive or trending information. Procedure Control periodically analyzes the trending data for specific patterns, and use the results of the analysis as the basis of adaptive process control decisions.

3B(iii) Procedure Control and APC Sub-System relationship.

Figure 14 is a schematic diagram showing exemplary Procedure Control and APC Sub-System architectural relationships useful in methods of the present

invention. For the sake of clarity, only APC relevant message paths and objects are included in Figure 14.

Procedure Control utilizes the APC Sub-System as a smart real-time information server and has supervisory control over the APC Sub-System. In the embodiment illustrated in Figure 14, Procedure Control selects operational modes of the APC Sub-System. According to the mode of operation, the APC transmits back to the Control Driver and Procedure Control, periodic sensor data analysis packets. In conjunction with commanding the APC Sub-System into a specific analysis mode, Procedure Control commands the Control Driver to enter into a
10 specific type of closed-loop transfer function mode. The Control Driver is configured to receive the time-critical APC sensor data as an error-signal input to its closed looped feedback transfer functions. Procedure Control performs adaptive process control by analyzing the trending or statistical behavior data over longer time periods and adjusting the Control Driver's transfer function set points to achieve a desired procedure performance.

3B(iv) **APC Executive**

The APC Executive is configured to manage the APC Sub-System while providing real-time process control information to the Control Sub-System. Figure 15 shows exemplary architectural relationships of the APC Executive with the APC
20 Driver, Image Data List Container, and the APC components within the Control Sub-System useful in the methods of the present invention.

The APC Executive task is responsible for controlling the image acquisition, image analysis, and streaming-data output of the APC Sub-System in accordance with a selected Procedure Control's orders. The executive task evaluates the APC orders and determine an appropriate course of action. If Procedure Control is requesting that the APC Sub-System change its blood component processing monitoring or analysis modes, then the executive task can perform the following

operations: (1) send APC processing (image acquisition / processing) orders to APC Driver component via the processing commands object, (2) send image analysis and data-feed orders to the Image Data Analyzer, (3) monitor the Image Data Analyzer's status and data-feed output, and then send APC (change-mode) status back to Procedure Control. After establishing the desired mode of operation, the APC Executive can automatically monitor and control the APC Sub-System to maintain the flow of requested information back to the Control Sub-System. The orders sent to the Image Data Analyzer specify the type of multivariable real-time analysis that the snapshot analyzer should perform and the type of data packets that the Image Data Analyzer should spool back to the Control Driver. The orders can also specify the type and level of error management and data filtering that the Image Data Analyzer should perform. When the Image Processing Engine inserts new data onto the list, the Image Data Container notifies the Image Data Analyzer. Then the Image Data Analyzer snapshot analyze the new image data object along with a number of preceding objects. Figure 16 is a schematic diagram providing a state chart for the image data analyzer task.

The APC Executive is also be responsible for calibration and error handling within the APC Sub-System. In one embodiment, the APC Executive autonomously manages its calibration and error handling up until predetermined non-recovery limits. Alternatively, the APC Executive is configured to always respond to error recovery and calibration orders from Procedure Control. In either the directed or autonomous error recovery / calibration cases, the Control Sub-System is configured to receive the appropriate status information. Procedure Control receives error status messages from the APC Executive once it has recognized an error condition, while the Control Driver is simultaneously receiving trending packets with both data and error or degraded performance information. The APC Sub-System can manage calibration and error handling using predetermined validation parameters in orders that the APC Executive sends the Image Data

Analyzer. In an embodiment of the present invention, the Procedure Control is the final arbitrator for the determining whether the APC Sub-System is working correctly and sending the Control Driver the requested control loop and adaptive process control information.

3B(v) **APC Driver**

Figure 17 shows an exemplary architecture of the APC Driver component of the present invention. As shown in Figure 17, the APC Driver consists of two active tasks. The APC Driver task is responsible for the interface to the APC Executive and is configured to read processing commands from the APC Executive, and set
10 the camera and STC properly for executing those commands. It also is configured to write back status associated with the APC Driver operation for use by the APC Executive.

The image conversion task is responsible for receiving the raw image data from the camera and for generating a packet of information to the Image Processing Engine which includes this image data, the STC and camera settings, and the processing orders associated with the particular image. When a new image is available, a signal is sent to the Image Processing Engine to notify it of the availability of the new image data. The image conversion task is also be responsible for managing the buffers used to receive raw image data from the
20 camera and the buffer used to send data to the image processing engine. The Image Processing Engine is be responsible for signaling when it no longer needs a particular object.

Figure 18 shows an exemplary high level state diagram for a APC Driver task useful for the methods of the present invention. Table 1 describes each of the states provided in Figure 18.

Table 1 — APC Driver Task States Description

State	Description
Idle	Waiting for wakeup event. Wakeup events can be generated from new orders sent from the APC Executive, or from a wakeup time scheduled on a previous scan through the APC Driver task state machine.
Update Centrifuge Status	The APC Driver task monitors centrifuge position and speed through the STC. This data is used to compute timing for when trigger events are expected and to determine if new hardware settings can be safely written before a pending trigger event.
Check for New Processing Commands	This state checks for new processing commands from the APC Executive. If new commands are available, the APC Driver task generates a new set of internal orders to be used for image acquisition.
Check for New Orders Needed for Next Image	The APC Executive can command a sequence of one or more images to be processed. For example, it might command 10 images for tracking blood interface position, followed by an image used to periodically assess image quality. During this state, the driver determines if the next image to be acquired requires any change in the current STC and camera settings.

State	Description
Process New Orders	If new hardware settings are required for the next image, the driver must then determine if a sufficient time is available to write these settings before the next trigger event. This determination uses the current centrifuge position and speed, the position of the next trigger event, and the particular hardware settings that must be modified (e.g. changing only strobe duration on the STC can be faster than changing camera exposure settings).
Write New Settings to Hardware	New settings are written to the hardware, and the CurrentImageSettings object is updated so that when the image is received by the image conversion task, the correct settings corresponding to that image are available.
Check for Expected Trigger Event	In order to ensure correct synchronization between image settings and image data, the APC Driver task must check that image data is received by the image conversion task at the specified time. Either a false camera trigger (image data sent when none was expected) or a missed camera trigger (no image data sent when a new image should have been acquired) can cause the synchronization of the CurrentImageSettings data and the image data received from the camera to be lost.

State	Description
Error Handling	If a synchronization error is detected, the hardware must be reset to a known state, and the driver task resynchronized with the incoming image data.
Schedule Wakeup Next	The APC Driver task schedules the next wakeup event for the time to the next expected trigger event (based on current centrifuge position and speed). However, if this time exceeds 10 msec, the next wakeup is scheduled for 10 msec instead, to ensure that centrifuge speed changes are tracked appropriately.

3B(vi) Image Processing Engine

Figure 19 shows an exemplary architecture of a APC Image Processing Engine component of the present invention. For the sake of clarity, not all data and message paths are included in this diagram and only those data and message paths relevant to the following are included.

10 In one embodiment, the image analyzer task is responsible for the real-time analysis of continuously streaming still-type digital images (frames). For a new image frame, the image analyzer task applies a suite of sensor algorithms (image analyzer tools) to extract specific blood component processing measurements from the image. After each frame has been analyzed, the extracted sensor measurements, image exposure parameters (camera, STC settings), and time / sequence stamps are used to construct a new image data object. The image analyzer then inserts the new data object onto the Image Data List Container (chronologically ordered circular buffer). The analyzer task is be configured to

receive each new image frame from the APC Driver component. For each new frame cycle the APC Driver loads an analyzable image structure into a designated memory buffer, update the analyzer commands object, and then notify the image analyzer task that a new image is ready to be processed with an image buffer ready signal. The architecture of the Image Analyzer partially decouples the asynchronous real-time image exposure and processing intervals defined by the centrifuge rpm from the executive task. The APC Executive indirectly controls and monitor the Image Analyzer through the APC Driver and the Image Data List Container. When the APC Executive task sends processing orders to the APC
10 Driver, the APC Driver redirects the image processing orders contained within the APC Executive's processing orders to the analyzer commands object. Image processing orders are used to determine the analyzer's mode of operation and the type of analysis that it performs. The APC Executive is configured to monitor the analyzer's image processing status by evaluating its output to the Image Data List Container. Figure 20 provides an exemplary state chart for an image analyzer task useful in the methods of the present invention.

In an embodiment, the analyzer task receives its processing orders from the read buffer of the analyzer commands objects for each frame. When the analyzer task is signaled by the APC Driver that a new image is ready to be processed it
20 obtains the image buffer location, image processing orders, and image exposure setting from the analyzer commands read buffer. It then selects the image analysis tools specified by the analyzer commands object and analyze the image. After the analysis, the analyzer task uses the extracted measurement data, image time stamps, image sequence count, and STC / camera exposure event settings, to create a new image data object. After creating the new image data object, the analyzer task then inserts it onto the Image Data List Container. If analyzer commands object orders enabled image data logging, it copies the image structure

into the image log buffer and signal the logging proxy that new logging data is available.

3B(vii) Image Data List Container

The Image Data List Container is configured to provide managed access to chronologically ordered sequences (circular buffer) of extracted image sensor data. The Image Processing Engine inserts image data objects into the Image Data List Container each time it processes a new image frame. The APC Executive is configured to receive notification of new data being inserted onto the list container from the Image Data List Container.

10 C. Image Processing Algorithms.

In one aspect, the present invention provides image processing algorithms useful for extracting measurements from two-dimensional distributions of transmitted and/or scattered light intensities comprising images of components of a blood processing system and/or a blood sample undergoing processing. Useful image processing algorithms for the methods of the present invention can be classified in several fundamental measurement categories including (1) direct measurements, (2) statistical measurements and (3) frequency based measurements.

20 Direct measurements refer to evaluation of the distances from known device components in a blood processing system and performing best fit algorithms to determine important features, such as the position of phase boundaries between optically differentiable separated blood components. Exemplary direct measurements and corresponding image processing algorithms useful for the methods of the present invention include, but are not limited to, (1) a measurement vector along the detected edge regions relative to the phase boundaries between separated blood components; (2) adaptive thresholding edge detection and/or gradient-based edge detection techniques to automatically determine accurate

measurements of the positions of phase boundaries between separated blood components; (3) pattern matching algorithms for determining the position, orientation and physical dimensions of a known device component or element of a known device component; (4) a distance measurement from a known device component or element of a known device component, such as the distance from the top of a rib on an optical cell to the RBC — Buffy coat layer phase boundary, buffy coat layer — plasma phase boundary or platelet — plasma phase boundary; (5) a distance measurement from a known device component or element of a known device component to a region of interest.

- 10 Statistical measurements refer to measurements which probe intensity values over a region of interest and use statistical tools to determine average light intensities and/or spatial distribution of light intensities of light transmitted and/or scattered from observation regions corresponding to important device components, such as light transmitted and/or scattered from one or more extraction ports or inlets. In this manner, fluxes and compositions of separated blood components in a region of interest, such as an extraction port, are determined in real time. Exemplary statistical measurements and corresponding image processing algorithms useful for the methods of the present invention include, but are not limited to: (1) a measurement of the mean intensity of transmitted and/or scattered
- 20 light from a region of interest (e.g. extraction port); (2) a measurement of the median intensity of transmitted and/or scattered light from a region of interest (e.g. extraction port); (3) a measurement of the minimum and/or maximum intensity of transmitted and/or scattered light from a region of interest (e.g. extraction port); (4) a measurement of the percentage contrast in an image of a region of interest (e.g. extraction port); (5) measurements of variance and standard deviation of observed transmitted and/or scattered light intensities of light from a region of interest (e.g. extraction port); (6) entropy distributions of measured transmitted and/or scattered light intensities of light from a region of interest (e.g. extraction port).

Frequency measurements translate measured light intensities of a two dimensional distribution of light intensities to identify the difference between high frequency and low frequency components. In one embodiment, for example, fast Fourier transform (FFT) or a power spectral series (FFT)² are used to evaluate the homogeneous or inhomogeneous nature of the flux of cellular material through an extraction port useful for evaluating the composition of extracted, separated blood components. Exemplary frequency measurements and corresponding image processing algorithms useful for the methods of the present invention include, but are not limited to: (1) determination of the minimum frequency resolution provide by
 10 the equation:

$$\text{minimum frequency resolution} = \frac{1}{(\text{length of the region of interest})}$$

(III)

(2) determination of the frequency resolution provided by the equation:

$$\text{frequency resolution} = \frac{(\text{number of frequency samples})}{(\text{length of the region of interest})}$$

(IV)

(3) determination of the ratio of the maximum frequency to minimum frequency within a selected range; (4) determination of the distribution or other characteristics of the power spectrum as a function of the radius of the power spectrum.

Image processing algorithms operate on a single two-dimensional distribution of transmitted and/or scattered light intensities corresponding to an image of a device component and/or blood sample to determine operating
 20 conditions useful for controlling a blood processing device. Measurements that can be extracted from a single frame of image data include, but are not limited to, the positions of phase boundaries between optically differentiable separated blood components, the composition and flux of extracted, separated blood components passing through an extraction port, and the composition of blood passing through

an inlet on a separation chamber. Uncertainties in these measurements can also be ascertained in real time from a single frame of image data analyzed by image processing algorithms of the present invention. Evaluating uncertainties in measured parameters is important in the present methods because it provides important data relevant to the data should be used in trending.

Alternatively, image processing algorithms can operate on a plurality of two-dimensional distributions of transmitted and/or scattered light intensities corresponding to multiple images of a device component and/or blood sample. Image processing algorithms that operate on multiple frames of image data are
10 useful for analyzing and predicting the temporal behavior of important operating conditions, such as the positions of phase boundaries between optically differentiable separated blood components and the compositions and fluxes of extracted, separated blood components passing through an extraction port. Exemplary Image processing algorithms that operate on multiple frames of image data comprise predictive data analysis algorithms capable of monitoring trends in important measurements in real time. Such predictive data analysis algorithms provide process control systems capable of very quickly adjusting one or more device settings in response to changes in blood processing conditions or sample composition for optimizing a given procedure or therapy.

20 Image processing algorithms of the present invention can be determined empirically by correlating measured parameters, such as average intensities of transmitted and/or scattered light or two dimensional distribution of intensities of transmitted and/or scattered light, with observed compositions of extracted separated blood components. in one embodiment, such correlations are determined by operation of fitting algorithms to individual image data sets or multiple image data sets. Appropriate correlations for image processing algorithms of the present invention can depend on the composition of the blood undergoing processing or other characteristics of a donor or a patient undergoing treatment.

Alternatively, in another embodiment correlations are determined using neural networks and machine learning algorithms known in the art. For example, such machine learning algorithms are used to continually refine image processing algorithms by operation on archived image data.

An exemplary method for controlling a blood processing device comprises the steps of: (1) performing a first measurement of an operating condition of said blood processing device corresponding to a first time; (2) performing a second measurement of said operating condition of said blood processing device corresponding to a second time; (3) analyzing said first and second measurements of said operating condition using a predictive data analysis algorithm, wherein operation of said predictive data analysis algorithm generates a predicted operating condition of said blood processing device at a future time; and (4) adjusting at least one setting of said blood processing device based on said predicted operating condition of said blood processing device at said future time, thereby controlling said blood processing device.

Example 4: Optical Cell for Monitoring and Controlling Blood Processing.

The present invention includes optical cells for use in monitoring and controlling blood processing using a wide variety of blood processing techniques. Optical cells of the present invention are capable of transmitting at least a portion of an incident light beam and/or light scattered by one or more fluid components in the optical cell. Optionally, optical cells of the present invention may comprises selectively absorbing, reflecting, scattering, collimating and/or focusing regions capable of selectively manipulating an incident light beam or light scattered by one or more fluid components in the optical cell. Moreover, optical cells of the present invention maximize regions of a blood separation system which are viewed and optically characterized using a fixed position CCD OR CMOS camera equipped with a fixed focus lens system. This feature of optical cells of the present invention provides for multifunctional blood processing systems which are capable of

simultaneously monitoring and controlling a plurality of blood processing operating conditions, including composition of separated blood components, fluxes of extracted, separated blood components and positions of phase boundaries between optically differentiable separated components.

Figure 21A provides a schematic diagram of a rotated side view of an optical cell of the present invention useful for monitoring blood processing via density centrifugation. The illustrated optical cell **1100** comprises a blood component extraction chamber **1105**, a first extraction port **1110**, a second extraction port **1115** and a third extraction port **1117**. Extraction chamber **1105** comprises a first side wall **1120** and a second side wall **1125** which define a blood separation region **1126**, wherein blood components are separated along separation axis **1127** on the basis of density upon formation of a centrifugal field by a density centrifuge. In the embodiment shown in Figure 21A, extraction chamber **1105**, first extraction port **1110** and second extraction port **1115**, are each capable of passing at least a portion of incident light, such as light propagating along an optical axis which is substantially parallel to the incident light beam axis **1140** and light scattered by blood or blood components in blood separation region **1126**, first extraction port **1110**, and/or second extraction port **1115**. Optionally, optical cell **1100** can further comprise ribs **1141** to enhance structural integrity and provide good mechanical ruggedness.

As shown in Figure 21A, first extraction port **1110**, second extraction port **1115** and third extraction port **1117** are tubular elements in fluid communication with blood separation region **1126**. In an embodiment of the present invention, first extraction port **1110** terminates at an orifice positioned about midway between first side wall **1120** and second side wall **1125**, second extraction port **1115** terminates at an orifice positioned proximate to first side wall **1120** and third extraction port **1117** terminates at an orifice positioned proximate to second side wall **1125**. This arrangement allows blood components of different densities to be extracted through

different extraction ports because first, second and third extraction ports **1110**, **1115** and **1117** are in fluid communication with different regions of blood separation region **1126** during blood processing. In one embodiment of the present invention, optical cell **1100** is configured such that white blood cells can be extracted through first extraction port **1110**, plasma and/or platelets can be extracted through second extraction port **1115**, and red blood cells can be extracted through third extraction port **1117**.

Optical cell **1100** is configured such that it can be coupled to a blood separation chamber (not shown in Figure 21A) such that blood undergoing
10 processing is flowed through optical cell **1100**, and discrete fractions corresponding to selected blood components are extracted through first, second and third extraction ports **1110**, **1115** and **1117**. In one embodiment, optical cell **1100** is an integrated element of a blood processing chamber. In another embodiment, optical cell **1100** is a separate component of a blood processing system in fluid communication with a separation chamber. In one embodiment, optical cell **1100** is configured such that it is periodically rotated into and out of an observation region of an optical monitoring and control system of the present invention as the separation chamber of a density centrifuge rotates. In this manner, two dimensional distributions of intensities of transmitted light, scattered light or both comprising
20 images of optical cell **1100** are measured for each rotation or for selected rotations. Optical cell **1100** can comprise a disposable component of a blood processing system or can be a reusable component.

Extraction chamber **1105**, first extraction port **1110**, second extraction port **1115** and third extraction port **1117** can further comprise one or more optical surfaces capable of transmitting light, such as an incident optical beam or light scattered from blood or blood components. Optical surfaces of extraction chamber **1105**, first extraction port **1110**, second extraction port **1115** and third extraction port **1117** can be external optical surfaces that are not in contact with blood

undergoing processing and are exposed to the ambient surroundings. Alternatively, optical surfaces of extraction chamber **1105**, first extraction port **1110** second extraction port **1115** and third extraction port **1117** can be internal optical surfaces that are in contact with blood undergoing processing and not exposed to the ambient surroundings. In an exemplary embodiment, optical surfaces of extraction chamber **1105** are positioned such that a high quality optical image of at least a portion of the optical cell **1100** is generated upon illumination with a first collimated light beam directed on the top **1113** of optical cell **1100** and a second collimated light beam directed on the bottom **1114** of optical cell **1100**. This configuration
10 allows two dimensional distributions of light intensities comprising images of optical cell **1100** to be measured and analyzed in real time.

Use of the term optical surface in the present invention refers to surfaces capable of efficiently transmitting incident light, such as collimated, incident light beams having a selected distribution of wavelengths, such as wavelengths in the visible and/or infrared regions of the electromagnetic spectrum, and/or light scattered from blood or blood components undergoing processing. Optical surfaces of the present invention preferred for some applications of the present invention do not significantly alter the intensities, wavelength distribution and spatial characteristics of incident light, such as propagation direction and extent of
20 collimation. Optical surfaces of the present invention can be substantially optically flat, such as the degree of flatness provided by a diamond polish, for example a degree of flatness exhibiting deviations from absolute flatness less than about 0.001 inch. Use of optically flat optical surfaces in optical cells of the present invention is beneficial because they are capable of efficiently transmitting a collimated light beam without substantially distorting the spatial characteristics of the beam, such as transmitting a collimated beam without significant focusing and without significantly increasing beam divergence. Optical surfaces of the present invention can also be optically smooth surfaces, such as the degree of smoothness

provided by a diamond polish, for example a degree of smoothness provided by a diamond polish exhibiting deviations from a absolutely smooth surface of less than about 3 microinches. Use of optically smooth surfaces in optical cells of the present invention is beneficial because they are capable of providing highly transmissive surfaces wherein scattering of incident light from the optical surface is minimized. The present invention also include embodiments wherein optical cell **1100** comprises a plurality of optical surfaces that are positioned in substantially parallel planes. Use of parallel optical surfaces is beneficial for providing good transmission of light through optical cell **1100**.

- 10 In the embodiment shown in Figure 21A, extraction chamber **1105** has a first external optical surface **1130** and a second external optical surface **1135**, capable of efficiently transmitting one or more collimated light beams propagating along optical axis substantially parallel incident light beam axis **1140** and/or light scattered from blood or blood components in blood separation region **1126**. Optionally, extraction chamber **1105** can also comprise a first internal optical surface, second internal optical surface or both (not shown in Figure 21A) positioned opposite to first optical surface **1130** and/or second optical surface **1135**, respectively, and in contact with the blood separation region **1126**. Preferable for some applications of the present invention, external and/or internal optical surfaces of extraction
- 20 chamber **1105** are flat and oriented in substantially parallel planes to increase transmission of an incident light beam. External and/or internal optical surfaces of extraction chamber **1105** are preferably highly transmissive, optically flat and optically smooth, such that they are capable of providing a flat, undistorted image of at least a portion of top **1113** of optical cell **1100** to a CCD or CMOS camera positioned in optical communication with the extraction chamber.

As shown in Figure 21A, first extraction port **1110** and second extraction port **1115** have external optical surfaces **1146** and **1147**, respectively, capable of efficiently transmitting one or more collimated light beams propagating along optical

axis substantially parallel incident light beam axis **1140** and/or light scattered from blood or blood components in the extraction ports. Figure 21B provides a cross sectional view of an exemplary extraction port design of the present invention. As shown in Figure 21B, first extraction port **1110** and second extraction port **1115** each have an axial bore **1150** having a square cross sectional profile. In this embodiment, first extraction port **1110** and second extraction port **1115** have internal optical surfaces **1155**, which are capable of efficiently transmitting one or more collimated light beams propagating along an optical axis which is substantially parallel to incident light beam axis **1140**. Optionally, first extraction port **1110** and second extraction port **1115** can have additional internal optical surfaces **1160** positioned opposite optical surfaces **1155** to further increase transmission and minimize unwanted beam distortion affects, such as focusing and increasing beam divergence. In addition, first extraction port **1110** and second extraction port **1115** can have additional external optical surfaces **1161** to enhance transmission of light through first and second extraction ports **1110** and **1115**. Internal and/or external optical surfaces of first extraction port **1110** and second extraction port **1115** are preferably highly transmissive, optically flat and optically smooth, such that they are capable of providing a flat, undistorted image of at least a portion of the extraction ports to a CCD or CMOS camera positioned in optical communication with the extraction chamber. Monitoring the transmission of light through first and second extraction ports **1110** and **1115** while blood components are extracted from blood separation region **1126** provides a means of measuring the composition of extracted blood components.

The present invention also includes optical cell configurations having extraction ports with axial bores having cross sectional profiles other than square profiles, such as rectangular profiles, trapezoidal profiles and curved profiles. Figure 21C provides a cross sectional view of an alternative extraction port design of the present invention, wherein first extraction port **1110** and second extraction

port **1115** each have an axial bores **1150** having a rectangular cross sectional profile. Use of extraction ports having a rectangular cross sectional profiles with lengths **1157** of internal optical surfaces **1155** larger than the width **1158** of side walls **1165** is preferred for some applications because it provides for better measurements of the composition and/or flux of cellular and/or noncellular materials in the extraction port. For example, use of rectangular cross sectional profiles providing a very thin axial bore **1150** (i.e. having length **1157** significantly larger than width **1158**) is beneficial because it distributes absorbing material, such as cellular blood components, in a layer having a larger cross sectional area positioned orthogonal to the propagation axes of the incident beam, which allows the spatial distribution of such absorbing material to be more accurately characterized. Further, use of a thin axial bore **1150** is beneficial because it decreases the optical path length of the beam through the extracted component, which is useful for avoiding substantially complete absorption of an incident beam directed onto the extraction ports. In one embodiment, extraction ports **1110** and **1115** have rectangular cross sectional profile characterized by an aspect ratio (aspect ratio = (width) / (length)) selected over the range of about 0.1 to about 0.4. For example, an extraction port of the present invention has a length **1157** equal to about 0.080 inches and a width **1158** equal to about 0.030 inches. Selection of the cross sectional profile and physical dimensions of axial bores **1150** of extraction ports of the present invention can be made on the basis of the flow rates through the extraction ports desired, optical transmission considerations and light imaging considerations.

Referring again to Figure 21A, in one embodiment of the present invention second external optical surface **1135** of extraction chamber **1105** and external optical surfaces of first extraction port **1110** and second extraction port **1115** are positioned such that that are in the depth of field provided by a light collection element and two-dimensional detector (no shown in Figure 21A). Exemplary

second external optical surface **1135** of extraction chamber **1105** and external optical surfaces of first extraction port **1110** and second extraction port **1115** occupy substantially the same plane **1170**. In this context the expression "substantially the same plane" includes deviations from an absolutely coplanar orientation less than or equal to about 0.1 inches. Preferably for some applications, second external optical surface **1135** of extraction chamber **1105** and external optical surfaces **1146** and **1147** of extraction port **1110** and second extraction port **1115** can be positioned in a common plane corresponding to the focal plane of a fixed position CCD or CMOS camera equipped with a fixed focus lens system in optical communication with optical cell **1100**. This optical configuration allows for simultaneous imaging and sensitive optical characterization of the blood separation region **1126**, first extraction port **1110** and second extraction port **1115**. An advantage of this optical configuration is that it allows simultaneous measurements of the position of phase boundaries in the blood separation region **1126** and the composition of blood components extracted through first and second extraction ports **1110** and **1115**.

Optical cell **1100** can also comprise additional elements to facilitate a number of optical measurements. First, optical cell **1100** can be provided with a variety of calibration markers. Calibration markers and optical surfaces **1135**, **1146** and **1147** can be positioned in common plane **1170**, such as a plane corresponding to the focal plane of a fixed position CCD or CMOS camera equipped with a fixed focus lens in optical communication with optical cell **1100**. Calibration markers can be positioned on optical cell **1100** itself, for example on the closest of ribs **1141** to plane **1170**, or on a device or device component for holding optical cell **1100** in a density centrifuge, such as a filler device component. In one embodiment, calibration markers comprise markers for calibrating the physical dimensions and spatial orientation of a collected image, for example one or more two dimensional shapes such as bars having selected physical dimensions and spacing. In one

embodiment, calibration markers comprise markers for calibrating intensities of collected images, for example one or more two dimensional forms having selected absorption, scattering and reflection characteristics. In one embodiment, calibration markers comprise markers for calibrating the colors of collected images, for example one or more colored forms such as a color wheel.

Optical cells of the present invention may further comprise one or more selectively absorbing, reflecting, scattering, focusing and/or collimating regions. In one embodiment, optical cells of the present invention have one or more masked regions that are capable of substantially preventing transmission of light by
10 absorbing, scattering and/or reflecting an incident beam. In one embodiment, optical cells of the present invention have one or more curved surfaces for selectively adjusting the spatial characteristics of an incident beam, for example by focusing or collimating an incident beam.

Optical cells of the present invention can be fabricated from a wide range of at least partially transmissive materials including but not limited to polymers, plastics, thermosets and thermoplastics. Optical cells comprising one or more amorphous polymers are preferred in some embodiments because they provide for better transmission of incident light than corresponding crystalline materials. Exemplary materials useful for fabricating optical cells of the present invention
20 include, but are not limited to, amorphous polyvinyl chloride, polycarbonate, and polyethylene terephthalate glycol (PETG) and polyethylene terephthalate (PET thermoplastic).

Example 5: System for Monitoring and Controlling Blood Processing via Density Centrifugation.

The present invention includes systems for monitoring and controlling blood processing via density centrifugation that are capable of providing simultaneous

real time measurements of the positions of phase boundaries between optically differentiable blood components relative to calibration markers and the compositions and/or fluxes of separated and extracted blood components. A system of the present invention exhibiting excellent sensitivity, mechanical ruggedness and reliability comprises a fixed position CCD camera equipped with a fixed focus lens, a top pulsed LED (light emitting diode) light source and a bottom pulsed LED light source. Use of a fixed position CCD camera equipped with a fixed focus lens system provides a system exhibiting high mechanical stability with respect to maintaining optical alignment, which avoids the need for periodic
10 adjustments of the optical path lengths illumination and detection beams. In addition, use of top and bottom pulsed LED light sources provides considerable flexibility in the wavelength distributions and intensities of illumination light beams directed onto the blood processing system and subsequently detected. Further, use of top and bottom pulsed LED light sources also provides accurate and reproducible temporal characteristics of illumination pulses useful for generating high optical quality images of a rotating optical cell of a separation chamber.

Figure 22 is a top view of an optical monitoring and control system of the present invention well suited for blood processing via density centrifugation. Figure 23 is a cut away view corresponding to cut away axis **1200** indicated in Figure 22.
20 Figure 24 is a side view of the optical monitoring and control system illustrated in Figures 22 and 23. The illustrated optical monitoring and control system **1205** comprises CCD camera equipped with a fixed focus lens system **1210**, an optical cell **1220**, a top pulsed LED light source **1215**, and a bottom pulsed LED light source **1225**. As illustrated in Figure 23, CCD camera with a fixed focus lens system **1210** is in optical communication with optical cell **1220** and positioned to intersect optical axis **1230**. Top pulsed LED light source **1215** is in optical communication with optical cell **1220** and is positioned such that it is capable of directing a plurality of collimated upper illumination light beams **1235**, propagating

along propagation axes that intersect optical axis **1230**, onto the top side **1239** of optical cell **1220**. Bottom pulsed LED light source **1225** is also in optical communication with optical cell **1220** and is positioned such that it is capable of directing a plurality of collimated bottom illumination light beams **1240**, propagating along a propagation axis parallel to optical axis **1230**, onto the bottom side **1250** of optical cell **1220**. Optionally, the top pulsed LED light source, bottom pulsed LED light source or both can be replaced with one or more pulsed xenon lamps for generating upper illumination light beams **1235**, bottom illumination light beams **1240** or both. Use of pulsed xenon lamps is desirable for application requiring very
10 intense upper and lower illumination light beams.

Optical cell **1220** is an integral component of a separation chamber of a density centrifuge and is held in position a selected distance from the density centrifuge's central rotational axis by filler **1255**. Filler **1255** and optical cell **1220** are configured in a manner such that both are capable of free rotation about the central rotational axis of the density centrifuge. In the embodiment shown in Figures 22, 23, 24, filler **1255** has an aperture **1256** of selected dimensions for passing at least a portion of bottom illumination light beams **1240**. Alternatively, aperture **1256** can comprise a stand alone optical element positioned along optical axis **1230** between bottom pulsed LED light source **1225** and optical cell **1220** or can be a
20 integral component of optical cell **1220** itself. Aperture **1256** can be any shape including, but not limited to, circular, square, rectangular, polygonal, romboidal, ellipsoidal or any combination of these shapes. Use of aperture **1256** in the present invention is useful for preventing detector saturation cause by too much light impinging on the sensing surface of the CCD camera and is useful for enhancing contrast with respect to areas of interest. Optionally, filler **1255** can also be equipped with other optical elements (not shown) for adjusting the spatial characteristics or wavelength distribution of bottom illumination light beams **1240**, such as optical filters, band pass filters, cut off filters and/or diffusers.

In an exemplary embodiment, top pulsed LED light source **1215** is positioned about 4.26 inches from the top **1239** of optical cell **1220**, and bottom pulsed LED light source **1225** is positioned about 7.47 inches from the top **1239** of optical cell **1220**. In the exemplary embodiment shown in Figure 23, CCD camera with fixed focus lens system **1210** is positioned such that the focal plane of fixed focus lens system is substantially co-planar with selected optical surfaces of optical cell **1220**, such as optical surfaces corresponding to an interface monitoring region, calibration markers, one or more extraction ports and one or more inlets. In this embodiment, the CCD camera is also separated from the center of the fixed focus lens system by
10 a distance along optical axis **1230** such that an image corresponding to selected optical surfaces of optical cell **1220** is provided on the sensing surface of the CCD camera. An advantage of this optical configuration is that it allows two dimensional distributions of light intensities comprising images of top **1239** of rotating optical cell **1100** to be measured and analyzed in real time.

CCD camera with fixed focus lens system **1210** is held in a fixed position a selected distance along optical axis **1230** from top **1239** of optical cell **1220** by mounting assembly **1260**. The mounting assembly **1260**, shown in Figures 22 - 24, comprises a bracket capable of maintaining a fixed position and orientation of CCD camera with fixed focus lens system **1210**. Mounting assembly **1260** can also
20 comprise a 2 — axis locking translation stage, optionally with a 2 axis titling mechanism, capable of selectively adjusting the relative orientation and position of the camera and fixed focus lens system with respect to optical cell **1220**.

As shown in Figures 22 - 24, optical monitoring and control system **1205** is integrated directly into a density centrifuge blood processing device **1265**. To provide good mechanical stability of optical monitoring and control system **1205**, mounting assembly **1260** is directly affixed to a frame member (not shown in Figs 22 - 24) supporting housing **1270** of density centrifuge blood processing device **1265**. In one embodiment, bottom pulsed LED light source **1225** is also be affixed

to a frame member (not shown in Figs 22 - 24) supporting housing **1270** of density centrifuge blood processing device **1265** by means of an additional mounting assembly **1261**. Top pulsed LED light source **1215** is secured to CCD camera with fixed focus lens system **1210**, as shown in Figures 22 - 24. Alternatively, top pulsed LED light source **1215** can be directly affixed to a frame member (not shown in Figs 22 - 24) supporting housing **1270** of density centrifuge blood processing device **1265** by means of an additional mounting assembly. Mounting assemblies useful in the present invention comprise any fastening means known in the art, such as clamps, brackets, connectors, couplers, additional housing elements and all known equivalents, and can be affixed to frame members supporting housing **1270** by any means known in the art including the use of bolts, fasteners, clamps, screws, rivets, seals, joints, couplers or any equivalents of these known in the art.

Referring to the cross section shown in Figure 23, first transparent plate **1275** is provided between CCD camera with a fixed focus lens system **1210** and optical cell **1220**, and second transparent plate **1280** is provided between bottom pulsed LED light source **1225** and optical cell **1220**. First and second transparent plates **1275** and **1280** physically isolate CCD camera with a fixed focus lens system **1210**, top pulsed LED light source **1215** and bottom pulsed LED light source **1225** from optical cell **1220** so that these components will not contact a sample undergoing processing in the event of sample leakage from the separation chamber. In addition, first and second transparent plates **1275** and **1280** minimize degradation of CCD camera with a fixed focus lens system **1210**, top pulsed LED light source **1215** and bottom pulsed LED light source **1225** due to unwanted deposition of dust and other contaminants that can be introduced to the system upon rotation of the separation chamber and filler. Further, first and second transparent plates **1275** and **1280** also allow a user to optimize the alignment of the camera with fixed focus lens system, top pulsed LED light source and bottom pulsed LED light source without exposure to a blood sample in the separation

chamber. First and second transparent plates **1275** and **1280** can comprise any material capable of transmitting at least a portion of upper and bottom illumination light beams **1235** and **1240**. Exemplary materials for first and second transparent plates **1275** and **1280** include, but are not limited to, glasses such as optical quality scratch resistant glass, transparent polymeric materials such as transparent plastics, quartz and inorganic salts.

Top pulsed LED light source **1215** and bottom pulsed LED light source **1225** in the optical monitoring and control system illustrated in Figures 22 — 24 each comprise a plurality of LEDs, such as a LED array light source. Top pulsed LED
10 light source **1215** comprises 12 LEDs each equipped with parabolic reflectors to provide beam collimation. Bottom pulsed LED light source **1225** also comprises 12 LEDs and a collimating optical element, such as one or more lenses, parabolic reflectors or a combination of these elements. Figure 25 provides a schematic diagram of an exploded, side view of a bottom pulsed LED source **1225** useful in the methods and devices of the present invention. The illustrated pulsed LED light source comprises a collimating optical element **1310** in optical communication with elements **1314** of a LED array. As shown in Figure 25, collimating optical element
20 **1310** is a multifaceted parabolic reflecting and collimating element comprising a plurality of contoured reflective surfaces **1312**, each of which is positioned in optical communication with a LED light element **1314**. Contoured reflective surfaces **1312** have a modified parabolic contour profile in one embodiment of the present invention useful for monitoring and controlling blood processing. Depending on the contour profile selected for contoured reflective surfaces **1312**, collimating optical element **1310** may be configured to provide a plurality of incident beam propagating along propagation axes that are approximately parallel or a plurality of incident beam propagating along propagation axes which are not parallel. The embodiment illustrated in Figure 25 is useful for generating a plurality of incident beams that may be directed onto the bottom side **1250** surface of the optical cell **1220**.

LEDs useful for the top and bottom pulsed LED sources **1215** and **1225** can be red LEDs, green LEDs, white LEDs or any combination of these. In an exemplary embodiment, top and bottom pulsed LED source **1215** and **1225** each comprise 4 red LEDs, 4 green LEDs and 4 white LEDs. LEDs useful in the present invention provide collimated beams having intensities large enough allow measurement of two dimensional intensity distributions comprising to images of optical cell **1220**. In an embodiment of the present invention, LED drive circuitry is optionally positioned proximate to top and/or bottom LED sources to optimize device performance.

10 Top pulsed LED light source **1215** and bottom pulsed LED light source **1225** are capable of providing synchronized light pulses having accurately selectable temporal characteristics. Pulse widths of light pulses useable in the present invention depend on the rotational velocity of the density centrifuge. Typically, the smaller the pulse width of the light pulse the less blurring of the optical image corresponding to the acquired two dimensional distribution of light intensities. However, larger pulse widths allow more photons to be detected by the camera and, thus, provide enhanced signal to noise ratios. For a rotational velocity equal to about 3000 RPM, pulse widths less than about 8 microseconds are useful for minimizing blurring of the image of the optical cell generated. Exemplary light
20 pulses useful for some applications of the present invention have pulse widths selected over the range of about 1 microsecond to about 50 microseconds.

In one embodiment, CCD camera with a fixed focus lens system **1210** comprise a monochrome or color CCD camera positioned a fixed, selected distance from a fixed focus lens system. CCD camera and fixed focus lens system can be contained in a housing **1285** capable of maintaining the selected separation distance between these elements and also capable of minimizing detection of unwanted scattered light. Housing **1285** can be equipped with one or more fixed spacers or selectively adjustable spacers for establishing and maintaining a

selected distance between the CCD camera and the fixed focus lens system. An exemplary fixed focus lens system comprises a plurality of spherical lenses, cylindrical lenses, spacers or any combination of these elements. An exemplary CCD camera is the "Flea[®] camera" manufactured by Point Grey Research, Inc. and has a pixel area equal to about 1024 pixels by 768 pixels. An exemplary lens comprises a F 2.8 fixed focal length lens system having a focal length of 28 millimeters manufactured by Schneider Optics, Inc. This combination of exemplary optical components provides a field of view equal to about 3/8 inch by 1/2 inch and a depth of field selected over the range of about 1/16 inch to about 1/2 inch. This field of view and depth of field allows for measurement of two dimensional distributions of light intensities comprising images of optical cell **1220** useful for monitoring and controlling the positions of phase boundary positions in an interface region and the compositions of cellular material exiting one or more extraction port. Use of a CCD camera equipped with a fixed focus lens system enhances the mechanical stability of the system and is useful for maintaining selected relative orientations and positions of the CCD camera, fixed focus lens system and the optical cell. This aspect of the present invention provides the system with the ability to make highly reproducible measurements of the positions of phase boundary layers between optically differentiable, separated blood components in an interface region and the compositions of separated blood components exiting the optical cell through one or more extraction ports.

Figure 23 also shows the optical path lengths provided by the present optical geometry. Top pulsed LED light source **1215** generates a plurality of pulsed collimated upper illumination light beams **1235** which propagate along propagation axes that intersect optical axis **1230**. At least a portion of upper illumination light beams **1235** passes through transparent plate **1275** and are directed onto the top side **1239** of optical cell **1220**. A portion of upper illumination light beams **1235** is scattered by optical cell **1220**, one or more separated blood components therein

and/or filler **1255**. Bottom pulsed LED source **1215** generates a collimated bottom illumination light beams **1240** which propagates along a propagation axis substantially parallel to optical axis **1230**. At least a portion of bottom illumination light beams **1240** passes through transparent plate **1280** and is directed onto the bottom side **1250** of optical cell **1220**. A portion of bottom illumination light beams **1240** is transmitted through optical cell **1220** and one or more separated blood components therein. Light transmitted through optical cell **1220** can correspond to an interface monitoring region, one or more inlets, one or more extraction ports, one or more calibration markers or any combination of these.

10 Light **1290** transmitted and/or scattered by optical cell **1220** is collected by fixed focal length lens system and imaged onto the sensing surface of the CCD camera. In this manner, a two dimensional distribution of light intensities is measured by CCD camera that corresponds to an image of at least a portion of optical cell **1220**, such as the top **1239** of optical cell **1220**. Detection of scattered light corresponding to the upper illumination light beams **1235** is primarily used for system calibration, proximity identification and translational sensor tracking. Detection of transmitted light corresponding to the bottom illumination light beams **1240** is primarily used for measurement of the position of one or more phase boundary layers of optically differentiable separated blood components in optical
20 cell **1220** and for measurement of the composition and flux of separated blood components exiting one or more extraction ports of optical cell **1220**. Detecting transmitted and scattered light arising from both top and bottom illumination maximizes the amount of information that can be extracted from an acquired two dimensional distribution of light intensities and enhances the multifunctional capabilities of optical monitoring and control systems of the present invention.

Optionally, optical monitoring and control system **1205** may further comprise one or more additional light detectors useful for optimizing the light levels of top and bottom pulsed LED light sources **1215** and **1225**. In one embodiment, an additional

light detector comprising a photodiode is provided which is capable of measuring scattered light from bottom pulsed LED light source **1225**. Use of an additional light detector capable of scattered light from bottom pulsed LED light source **1225** is useful for trouble shooting and error handling aspects of the present invention.

The COD camera is capable of generating one or more output signals corresponding to the measured two dimensional distribution of light intensities. Output signals are sent to one or more centrifuge device controllers (not shown in Figures 22 - 24), such as a computer or processor, capable of analyzing the acquired two dimensional distributions of transmitted and/or scattered light intensities and adjusting important operating conditions which affect separation conditions and the composition of extracted blood components. Selectively adjustable operating conditions include, but are not limited to, the rotational velocity of the centrifuge, the flow rates of one or more inlet pumps, and the flow rates of one or more extraction pumps, or any combination of these.

The optical monitoring and control system **1205** depicted in Figures 22 - 24 is a pulsed optical system, whereby two dimensional intensity distributions corresponding to optical cell **1220** are acquired as it is rotated about the central rotational axis of the density centrifuge **1265**. Two dimensional intensity distributions can be acquired for every full rotation of optical cell **1220** or can be acquired for selected rotations of optical cell **1220**, such as every other full rotation. Acquiring two dimensional intensity distributions for every other rotation of optical cell **1220** is beneficial for some applications because it avoids the need for costly CCD cameras capable of collecting more than about 30 frames per second and also minimizes spatial indication, calibration and optical imaging problems associated with reproducible instrument jitter observed upon rotation of the separation chamber.

To generate two dimensional intensity distributions corresponding to good images of optical cell **1220**, top and bottom illumination pulse, camera shutter and gating settings and the rotation of optical cell **1220** of a separation chamber of a density centrifuge must be accurate synchronized. Accurate synchronization of these elements allows two dimensional images of transmitted and/or scattered light intensities comprising high optical quality images of the optical cell may be measured for each full rotation or for selected rotations. In the present invention, the rotational position of components of the density centrifuge and/or monitoring and control system, such as the optical cell or separation chamber, is accurately
10 measured using an encoded motor system, as well known in the art. In an exemplary embodiment, density centrifuge **1265** is provided with any optical sensor capable of reading a plurality of markers on a rotating element of the density centrifuge. This configuration allows for real time measurements of the rotational position of the optical cell, preferably measurements of rotational position accurate to about 0.09 degrees. This configuration also provides real time measurements of the rotational position of the optical cell when the rotational velocity changes, such as during spin up or spin down of the density centrifuge.

The encoded motor system is also capable of generating output signals in real time corresponding to the rotational position of components of the density
20 centrifuge and/or monitoring and control system, such as the optical cell or separation chamber. In an exemplary embodiment, these output signals are provided as input to a synchronization and timing controller capable of sending one or more trigger signals to the top pulsed LED light source, bottom pulsed LED light source and the CCD camera. Trigger signals provided by the synchronization and timing controller to these device components include the trigger location (i.e. the time or rotational position for initiating to a light pulse), the trigger frequency (i.e. for which rotations should light pulses be generated), the pulse width setting (duration of light pulse) and the delay setting (i.e. time between when the trigger signal is

received and when the light pulse is to be initiated). LED elements in top and bottom pulsed LED light sources and camera shutter and gate setting can be accurately triggered at times corresponding to a desired rotational position of the density centrifuge using trigger signals generated by the synchronization and timing controller. Selection of the rotational position corresponding to the trigger signal allows the observation region to be selectively adjusted in the present invention. In this manner, a plurality of selected regions of the optical cell, separation chamber and other components of the density centrifuge are optically probed.

10 In an exemplary embodiment, the exposure time of the CCD camera is determined by the pulse width of the light pulses generated by the top and bottom pulsed LED light sources, rather than by the gating setting or shutter of the CCD camera. In one embodiment, the shutter of the CCD camera is open a few orders of magnitude longer than the light pulse duration without having significant background noise affects. As the pulse widths of light pulses generated by LED light sources can be controlled very accurately, this aspect of the present invention eliminates the need of costly CCD cameras providing very accurate gating corresponding to short exposure times.

20 Figure 26 shows a functional flow diagram representing a method of synchronizing light pulses generated by top and bottom pulsed LED light sources and camera shutter and gate settings. As illustrated in Figure 26, encoded motor system **1350** generates one or more output signals **1355** corresponding to the rotational position of the optical cell. Output signals **1355** are received as input to the synchronization and timing controller **1360**. Synchronization and timing controller **1360** is also configured to receive control signals **1365** from a device controller. Control signals **1365** and output signals **1355** are processed by synchronization and timing controller **1360**, and serve as the basis of a plurality of trigger signals **1370** which are sent to the top pulsed LED light source, the bottom pulsed LED light source and the CCD camera. Optionally, one or more trigger

signals are also be used to adjust the lighting in the density centrifuge chamber to allow a user to visually assess the state of the density centrifuge during processing. An advantage of this aspect of the present invention is that timing and synchronization of light pulses and camera settings are handled by the synchronization and timing controller 1360 without expenditure of other system resources, such as processing time of the device controller.

Use of LED light sources in the present invention is beneficial because these light sources are small, light weight and have relatively low power consumptions compared to many conventional non-LED light sources. LED light sources also exhibit long operating lifetimes and uniform radiant outputs. In addition, LED light sources are capable of pulse operation generating discrete pulse having accurately selectable temporal characteristics such as pulse width and initiation time. Pulse LED sources also are capable of generating pulses having substantially uniform intensities and wavelength distributions. Use of LED is also preferred for some applications of the present invention because it provides good control of the wavelength distribution of the upper and/or lower illumination beams. The present invention includes embodiments, wherein the wavelength distribution of top and bottom illumination beams is selectively adjustable by blending the output of LEDs having different colors, such as red, green and white LEDs. In these embodiments, the wavelength distributions of top and bottom illumination beams are be independently selected on a shot per shot basis to optimize a desired optical measurement, such as the measurement of the position of phase boundaries between optically differentiable blood components and/or the compositions of extracted blood components passing through an extraction port.

Optical monitoring and control systems of the present invention having a fixed position camera and fixed focus lens system are capable of providing very sensitive measurements of the positions of phase boundaries between optically differentiable separated blood components. For example, systems of the present

invention having a fixed position camera and fixed focus lens system are capable of measuring the position of the phase boundary between red blood cell containing components and a buffy coat layer and the position of the phase boundary between a plasma containing components and a buffy coat layer to within 0.0005 ± 0.0002 inches.

Optical monitoring and control systems of the present invention having a fixed position camera and fixed focus lens system are capable of providing very sensitive measurements of the compositions and fluxes of separated blood components through an extraction port. Systems of the present invention having a
 10 fixed position camera and fixed focus lens system are capable of measuring the hematocrit of an extracted blood component, such as a white blood cell containing component, passing through an extraction port to within about 1%. In addition, the two dimensional distribution of the intensities of light transmitted through an extraction cell also provides an accurate measurement of the cellular composition of an extracted blood component. Figure 27 provides plots of the white blood cell concentration (square markers) and hematocrit (star markers) of a separated blood component passing through an extraction port as function of the measured average
 20 intensity of light transmitted through an observation region position on the extraction port. As illustrated by the plots the average intensity of transmitted light is strongly inversely correlated with both the white blood cell concentration and the hematocrit. Statistical analysis of the plots in Figure 27 yields the following algorithms relating the average intensity of transmitted light to the white blood cell concentration and the hematocrit:

$$\text{Hct}(\%) = 297.8 \times (I)^{-1.0666};$$

(V)

$$\text{Conc. WBC} = 8796 \times (I)^{-1.3988}$$

(VI)

wherein Hct(%) is the hematocrit, conc. WBC is the concentration of white blood cells multiplied by a factor of 1000 in units of number per microliter and I is the average intensity of light transmitted through the extraction port.

Example 6: Density Centrifugation Methods for Processing Blood.

The present invention provides methods for processing blood and blood components. Methods of the present invention are applicable for processing blood and blood components having a wide range of compositions, which make them especially well suited for therapeutic procedures for patient pools that often exhibit a large range of blood compositions. In addition, the methods of the present invention are particularly well suited for blood processing applications wherein the composition of a patient's extracted blood undergoes significant variation during a selected procedure.

1. **Blood Processing Based on Optical Characterization of the Composition of Extracted Blood Components**

In one embodiment, the present invention provides a method of processing blood capable of providing extracted blood components having a selected composition. In the context of this description the term "composition" relates to the purity, cell-type, concentration and/or speciation of cellular and/or noncellular blood components in an extracted blood component. An advantage of this aspect of the present invention is that it is capable of optimizing a particular blood processing therapy, such as a blood component reduction therapy (e.g. leukapheresis therapy or therapeutic platelet depletion) or capable of providing blood components having compositions optimized for a particular therapeutic application, such as an infusion therapy.

In one embodiment, a user selects a desired blood component to be separated and extracted, and selects an optimal composition or range of compositions of the extracted blood component for an intended therapeutic

application. The selected type of blood component and composition is then provided to a device controller of the present invention as input. The device controller configures and adapts the blood processing device to achieve separation and extraction conditions necessary for producing a blood component having the desired composition. In the context of blood processing via density centrifugation, for example, the optical monitoring and control system measures the concentration and type of an extract blood component in real time and iteratively adjust operating conditions, such as the flow rates of the inlet pump, flow rates of extraction pumps and rotational velocity of the centrifuge, to achieve and maintain the desired composition of an extracted blood component. The methods of this aspect of the present invention, however, are not limited to blood processing via density centrifugation and, are also applicable to processing via a range of filtration and diffusion-based separation techniques.

This aspect of the present invention is particularly useful for separating and extracting a white blood cell component of blood using density centrifugation. Using the present methods, images of an extraction port corresponding to a separated white blood cell component are be acquired and analyze in real time to provide a measurement of the purity of the extracted component. The measured composition is then be compared to the user selected composition, such as a selected concentration or purity of white blood cells. If the measured composition is within a desired range of the selected composition, operating conditions of the density centrifuge are maintained as long as the composition of the extract portion does not change so as to be outside of the desired range. If the measured composition is not within a desired range of the selected composition, the operating conditions are iteratively adjusted in a manner bringing the observed composition closer to the selected composition. In one embodiment, the concentration of red blood cells in the extracted white blood cell component is measured in real time and compared to a calculated red blood cell concentration corresponding to the selected white blood

cell concentration. This exemplary method exploits well known relationships between the abundance of red blood cells in a white blood cell containing component generated by density centrifugation and the observed white blood cell concentration. In another method, the concentration of white blood cells is directly measured using the present optical monitoring methods and used to control blood processing. To facilitate direct monitoring and characterization of white bloods cells in the absence of red blood cells, operation conditions of the centrifuge can be modified to provide a buffy coat layer extending a larger thickness along the separation axes, such as by the addition of an intermediate density fluid or by
10 selection of appropriate rotational velocities.

2. Coarse and Fine Control of Blood Processing via Density Centrifugation

In another aspect of the present invention, simultaneous measurements of (1) the position of phase boundaries between two or more optically differentiable blood components and (2) the composition of an extracted blood component are used in combination to establish, optimize and maintain blood processing conditions in a density centrifuge blood processing system. In an exemplary method, the position of phase boundaries between two or more optically differentiable blood components is directly measured using the present methods and used to selectively adjust and establish a set of initial operating conditions of
20 the density centrifuge corresponding to the flow rate of the inlet pump, the flow rates of one or more extraction pumps, the rotational velocity of the centrifuge or any combination of these. These initial conditions provide a composition of the extracted component within a first range of the selected composition corresponding to a coarse optimization of the composition.

Upon achieving a composition within the first range of the selected composition, direct measurements of the composition of the extracted component(s) flowing through an extraction port are acquired and used to selectively adjust the operating conditions of the density centrifuge. Particularly, the

system operating conditions are iteratively adjusted to provide a composition of the extracted component with in a second range of the selected composition corresponding to a fine optimization of the composition. In this embodiment of the present invention, the second range is narrower than the first range. Upon achieving a composition within the second range of the selected composition, direct measurements of the composition of the extracted component(s) flowing through an extraction port are continuously acquired and compared to the selected composition. If necessary, the operating conditions are readjusted to maintain the composition of the extracted component within the first range. If for some reason
10 the composition of the extracted component exceeds both first and second ranges, the coarse optimization procedure is repeated and followed by the fine optimization procedure.

3. Bias Collection Methods of Collecting White Blood Cells

The optical monitoring and control methods of the present invention are capable of very accurately measuring the position of phase boundaries in an interface region and optically characterizing separated blood components exiting a separating chamber via one or more extraction ports. As most classes of cellular blood components, such as white blood cells, red blood cells and platelets, can be further differentiated on the basis of density into sub-classes, methods of the
20 present invention are also be capable of biased collection of blood components, wherein a blood component substantially enriched with a selected component sub-class is extracted and collected. In one embodiment, sub-classes of a given separated blood component are differentiated on the basis of their spatial distribution within a given separation layer in a separation chamber. Alternatively, specific sub-classes of cellular material are be selectively photoluminescently labeled to allow for optical differentiation, for example by fluorescent or phosphorescent labeling.

For example, white blood cells comprise a plurality of optically differentiable sub-classes, such as erythrocytes, eosinophils, basophils, monocytes, lymphocytes and granulocytes. These sub-classes can be differentiated on the basis of the distribution of these cell types in a separated buffy coat layer in a rotating density centrifuge. The large signal-to-noise ratios and high sensitivities for measuring the position of phase boundaries provided by the present optical monitoring methods allow very accurate positioning of selected regions of a given separated layer, such as a top region corresponding to a higher density sub-component or a bottom region corresponding to a lower density sub-component, relative to an extraction port. This functional capability in turn allows extracted components corresponding to fluid components enriched in selected sub-classes of white blood cells types to be extracted and collected using the present methods. For example, positioning the extraction port proximate to the top of the buffy layer results in a white blood cell containing component enriched in lymphocytes, and positioning the extraction port proximate to the bottom of the buffy layer results in a white blood cell containing component enriched in granulocytes.

Using the present methods, for example, the position of phase boundaries between optically differentiable white blood cell sub-classes can be directly measured and controlled to within about 0.005 inch. Thus, the positions of phase boundary layers may be selectively adjusted to achieve a position relative to an extraction port proximate for providing an extract component enriched in a desired white blood cell sub-class. Further, in some embodiments, the composition of the extracted white blood cell component is directly monitored and optically classified with respect to the populations of various sub-classes. Iterative adjustment of centrifuge operating conditions on the basis of the optical characterization of the material passing through the extraction port also allows for extraction and collection of a white blood cell component enriched with a selected white blood cell sub-component.

This aspect of the present invention is also applicable to red blood cell containing components and platelet containing components. For example, red blood cells or platelets in separated blood components having atypical shapes and sizes which gives rise to different densities of these materials. Accordingly, selective positioning of an extraction port in a separated red blood cell containing layer or platelet containing layer allow for extraction and collection of fluid components enriched in red blood cells or platelets in separated blood components having atypical shapes and sizes. Further, this concept may also be used to collect plasma containing components enriched in plasma proteins having selected densities and/or molecular weights.

4. Methods of Monitoring the Extent of Hemolysis During Blood Processing.

Hemolysis occurs when red blood cells are damaged and release at least a portion of their hemoglobin. Hemolysis occurs when blood components are subjected to stresses induced by centrifugal blood processing, such as stresses induced by pumping blood components, flowing blood components into, through and out of a separation chamber and/or applying a centrifugal field. When hemolysis occurs during centrifugal blood processing at least a portion of the free hemoglobin migrates to the separated, lower density plasma blood component.

The present invention provides a means for directly monitoring and controlling the extent of hemolysis occurring during blood processing via density centrifuge techniques. In this method, the intensity of light transmitted by the separated plasma component is monitored as a function of time. If appreciable hemolysis occurs the free hemoglobin that migrates to the separated plasma component will absorb light, particularly in the 500 nm to 600 nm region of the electromagnetic spectrum. Measurements of the decrease in transmitted light intensity, particularly over the wavelength range of 500 nm to 600 nm, are used to quantify the extent of hemolysis that has occurred during blood processing. In some embodiments, use of incident light beams having a wavelength distribution with a

peak between 500 nm to 600 nm, such as light provided by one or more green LEDs or using of selectively transmissive optical filters, enhances the sensitivity of these measurements. The present invention also includes methods of controlling the extent of hemolysis during blood processing whereby the inlet and extraction flow rates are lowered upon observation of an appreciable extent of hemolysis.

5. Enhanced Separation Protocols.

10 The optical monitoring and control methods and devices of the present invention are particularly well suited for blood processing methods wherein the rotational velocity of a density centrifuge is selectively adjusted as a function of time. Enhanced separation protocols include protocols that require a level of control that is not possible using algorithm-based systems because of the complex steps that require precise operating conditions and trigger points. An exemplary embodiment includes multiple protocol stages, each requiring different image analysis data and different areas of interest. For example, the methods of the present invention provide simultaneous measurements of the changes in the positions of phase boundaries between optically differentiable blood components caused by changes in the rotational velocity of the centrifuge and/or changes in the subject's incoming blood.

20 In an embodiment of the present invention, an enhanced separation protocol comprises three major stages. In the first stage, the blood processing system primes the optical cell and its associated secondary separation chamber with fluid.

In the protocol's second stage, the buildup stage, the monitoring and control system measures the position of the phase boundary between a red blood cell containing and a buffy coat layer and the position of a phase boundary between a buffy coat layer and plasma containing component. In addition, the monitoring and control system establishes a position of the buffy coat layer proximate to the orifice of an extraction port of an optical cell. After the monitoring and control system

establishes the positions of the buffy coat layer proximate to the orifice of an extraction port, the platelets, plasma, white blood cells and few red blood cells contained in the buffy coat layer are all extracted and passed into a secondary chamber, such as an elutriation chamber, to further separate the extracted blood components and enhance the purity of the selected components. Unselected components are returned to the patient, while the selected components, such as white blood cells, are collected in the secondary chamber. During the second stage, the monitoring and control system simultaneously measures the cellular flux of cells entering the secondary chamber, the position of the phase boundary between the buffy coat layer and the plasma containing layer, the position of the phase boundary between the buffy coat layer and the red blood cell containing layer, and the position of the buffy coat layer relative to the extraction port in order to maintain optimal performance and separation conditions. As a result of the ability of the monitoring and control system to view and optically characterize a plurality of areas of interest, the system can collect two-dimensional images of scattered or transmitted light from the secondary chamber itself, to help determine if the chamber is full and ready to enter the system's third stage.

In the protocol's third stage, the monitoring and control system evaluates the status of the secondary chamber. If the secondary chamber is full of a selected material, the optical monitoring and control system triggers a flush out of the secondary chamber. To flush the secondary chamber, for example, the monitoring and control system can simultaneously adjust the position of the phase boundary between the buffy coat layer and the plasma containing layer to a position wherein the extraction port is exclusively in contact with the plasma layer. This procedure ensures that the flux of cellular matter through the extraction port is minimized. The monitoring and control system also lowers the rotational velocity of the centrifuge and changes a valve position to flush the selected cells from the secondary chamber into a collection container. The synchronization and timing control

provided by the present methods allows the system to maintain precise interface positions required to achieve the flush step of the protocol. The monitoring and control system is also important for determining when the chamber is sufficiently flushed to return to another buildup stage by monitoring the intensities of transmitted and/or scattered light from the secondary processing chamber.

In one embodiment, the blood processing system repeats alternating buildup and flush stages to achieve a desired endpoint, at least partially based on the cellular flux measurements.

Enhanced blood separation protocols of the present invention may be used
10 to separate and collect a range of cellular and noncellular blood components including but not limited to, white blood cells, platelets, and plasma proteins. In one embodiment, the present invention provides a method of processing blood comprising the steps of: (1) providing a two stage blood processing system comprising a density centrifuge blood processing system and an elutriation blood processing system; (2) flowing blood into the two stage blood processing system, wherein the blood is separated into a plurality of components in the density centrifuge blood processing system including at least one desired component and a plasma containing component; (3) filling the elutriation blood processing system with the desired component until the elutriation blood processing system is in a
20 filled operating state; and (4) flushing the elutriation blood processing system when in the filled operating state by flowing the plasma containing component into the elutriation blood processing system, thereby processing the blood. Methods of this aspect of the present invention may further comprise the step of collecting at least a portion of the desired component in a container.

Methods of this aspect of the present invention may further comprise additional steps wherein device components and/or fluid components undergoing processing are optically characterized in real time using the present methods and

devices. Optionally, the method of the present invention further comprises the step of optically measuring the composition of blood components passing through an extraction port of the density centrifuge blood processing system into the elutriation blood processing system. Optionally, the method of the present invention further comprises the step of optically measuring the position of the desired component in a separation chamber of the density centrifuge blood processing system and an extraction port of the density centrifuge blood processing system. Optionally, the method of the present invention further comprises the step of optically measuring the composition and/or position of fluid components in the elutriation blood processing system.

Methods of this aspect of the present invention further comprises additional steps wherein the operating state of the elutriation blood processing system is directly evaluated via optical measurements. Optionally, the method of the present invention further comprises the step of determining when the elutriation blood processing system is in the filled operating state by optically measuring the composition and/or position of fluid components in the elutriation blood processing system. Optionally, the method of the present invention further comprises the step of determining when the elutriation blood processing system is in the filled operating state by optically measuring the composition, flux or both of blood components passing through an extraction port of the density centrifuge blood processing system into the elutriation blood processing system.

WHAT IS CLAIMED IS:

1. A method of processing blood comprising the steps of:
providing a two stage blood processing system comprising a density centrifuge blood processing system and an elutriation blood processing system;
flowing blood into said two stage blood processing system, wherein the blood is separated into a plurality of components in the density centrifuge blood processing system including at least one desired component and a plasma containing component;
filling the elutriation blood processing system with said desired component
10 until the elutriation blood processing system is in a filled operating state;
measuring a cellular flux of cells entering the elutriation blood processing system with a two-dimensional optical control system; and
flushing the elutriation blood processing system when in the filled operating state by flowing the plasma containing component into the elutriation blood processing system, thereby processing said blood.
2. The method of claim 1, further comprising the step of optically measuring the composition of blood components passing through an extraction port of the density centrifuge blood processing system into the elutriation blood processing system.
3. The method of claim 1, further comprising the step of optically measuring the
20 position of the desired component in a separation chamber of the density centrifuge blood processing system and an extraction port of the density centrifuge blood processing system.
4. The method of claim 1, further comprising the step of optically measuring the composition of fluid components in the elutriation blood processing system.

5. The method of claim 1, further comprising the step of optically measuring the position of fluid components in the elutriation blood processing system.

6. The method of claim 1, further comprising the step of determining when the elutriation blood processing system is in the filled operating state by optically measuring the composition of fluid components in the elutriation blood processing system.

7. The method of claim 1, further comprising the step of determining when the elutriation blood processing system is in the filled operating state by optically measuring the position of fluid components in the elutriation blood processing system.

8. The method of claim 1, further comprising the step of determining when the elutriation blood processing system is in the filled operating state by optically measuring the composition, flux or both of blood components passing through an extraction port of the density centrifuge blood processing system into the elutriation blood processing system.

9. The method of claim 1, wherein said desired component is a white blood cell containing component.

10. The method of claim 1, wherein said desired component is a platelet containing component.

20 11. The method of claim 1, further comprising the step of collecting at least a portion of said desired component in a container.

12. The method of claim 1, further comprising simultaneously measuring cellular flux entering the elutriation blood processing system, the position of a phase boundary between a buffy coat layer and a plasma containing layer, the position of

a phase boundary between the buffy coat layer and a red blood cell containing layer; and the position of the buffy coat layer relative to an extraction port.

13. The method of claim 12, where the simultaneous measuring is performed by a single optical monitoring and control system.

14. The method of claim 13, wherein said single optical monitor and control signal causes the blood processing system to flush the elutriation blood processing system by simultaneously adjusting the position of the phase boundary between the buffy coat layer and the plasma containing layer.

15. The method of claim 1, wherein the blood processing system repeats
10 alternating build-up and flush stages, at least partially based on cellular flux measurements.

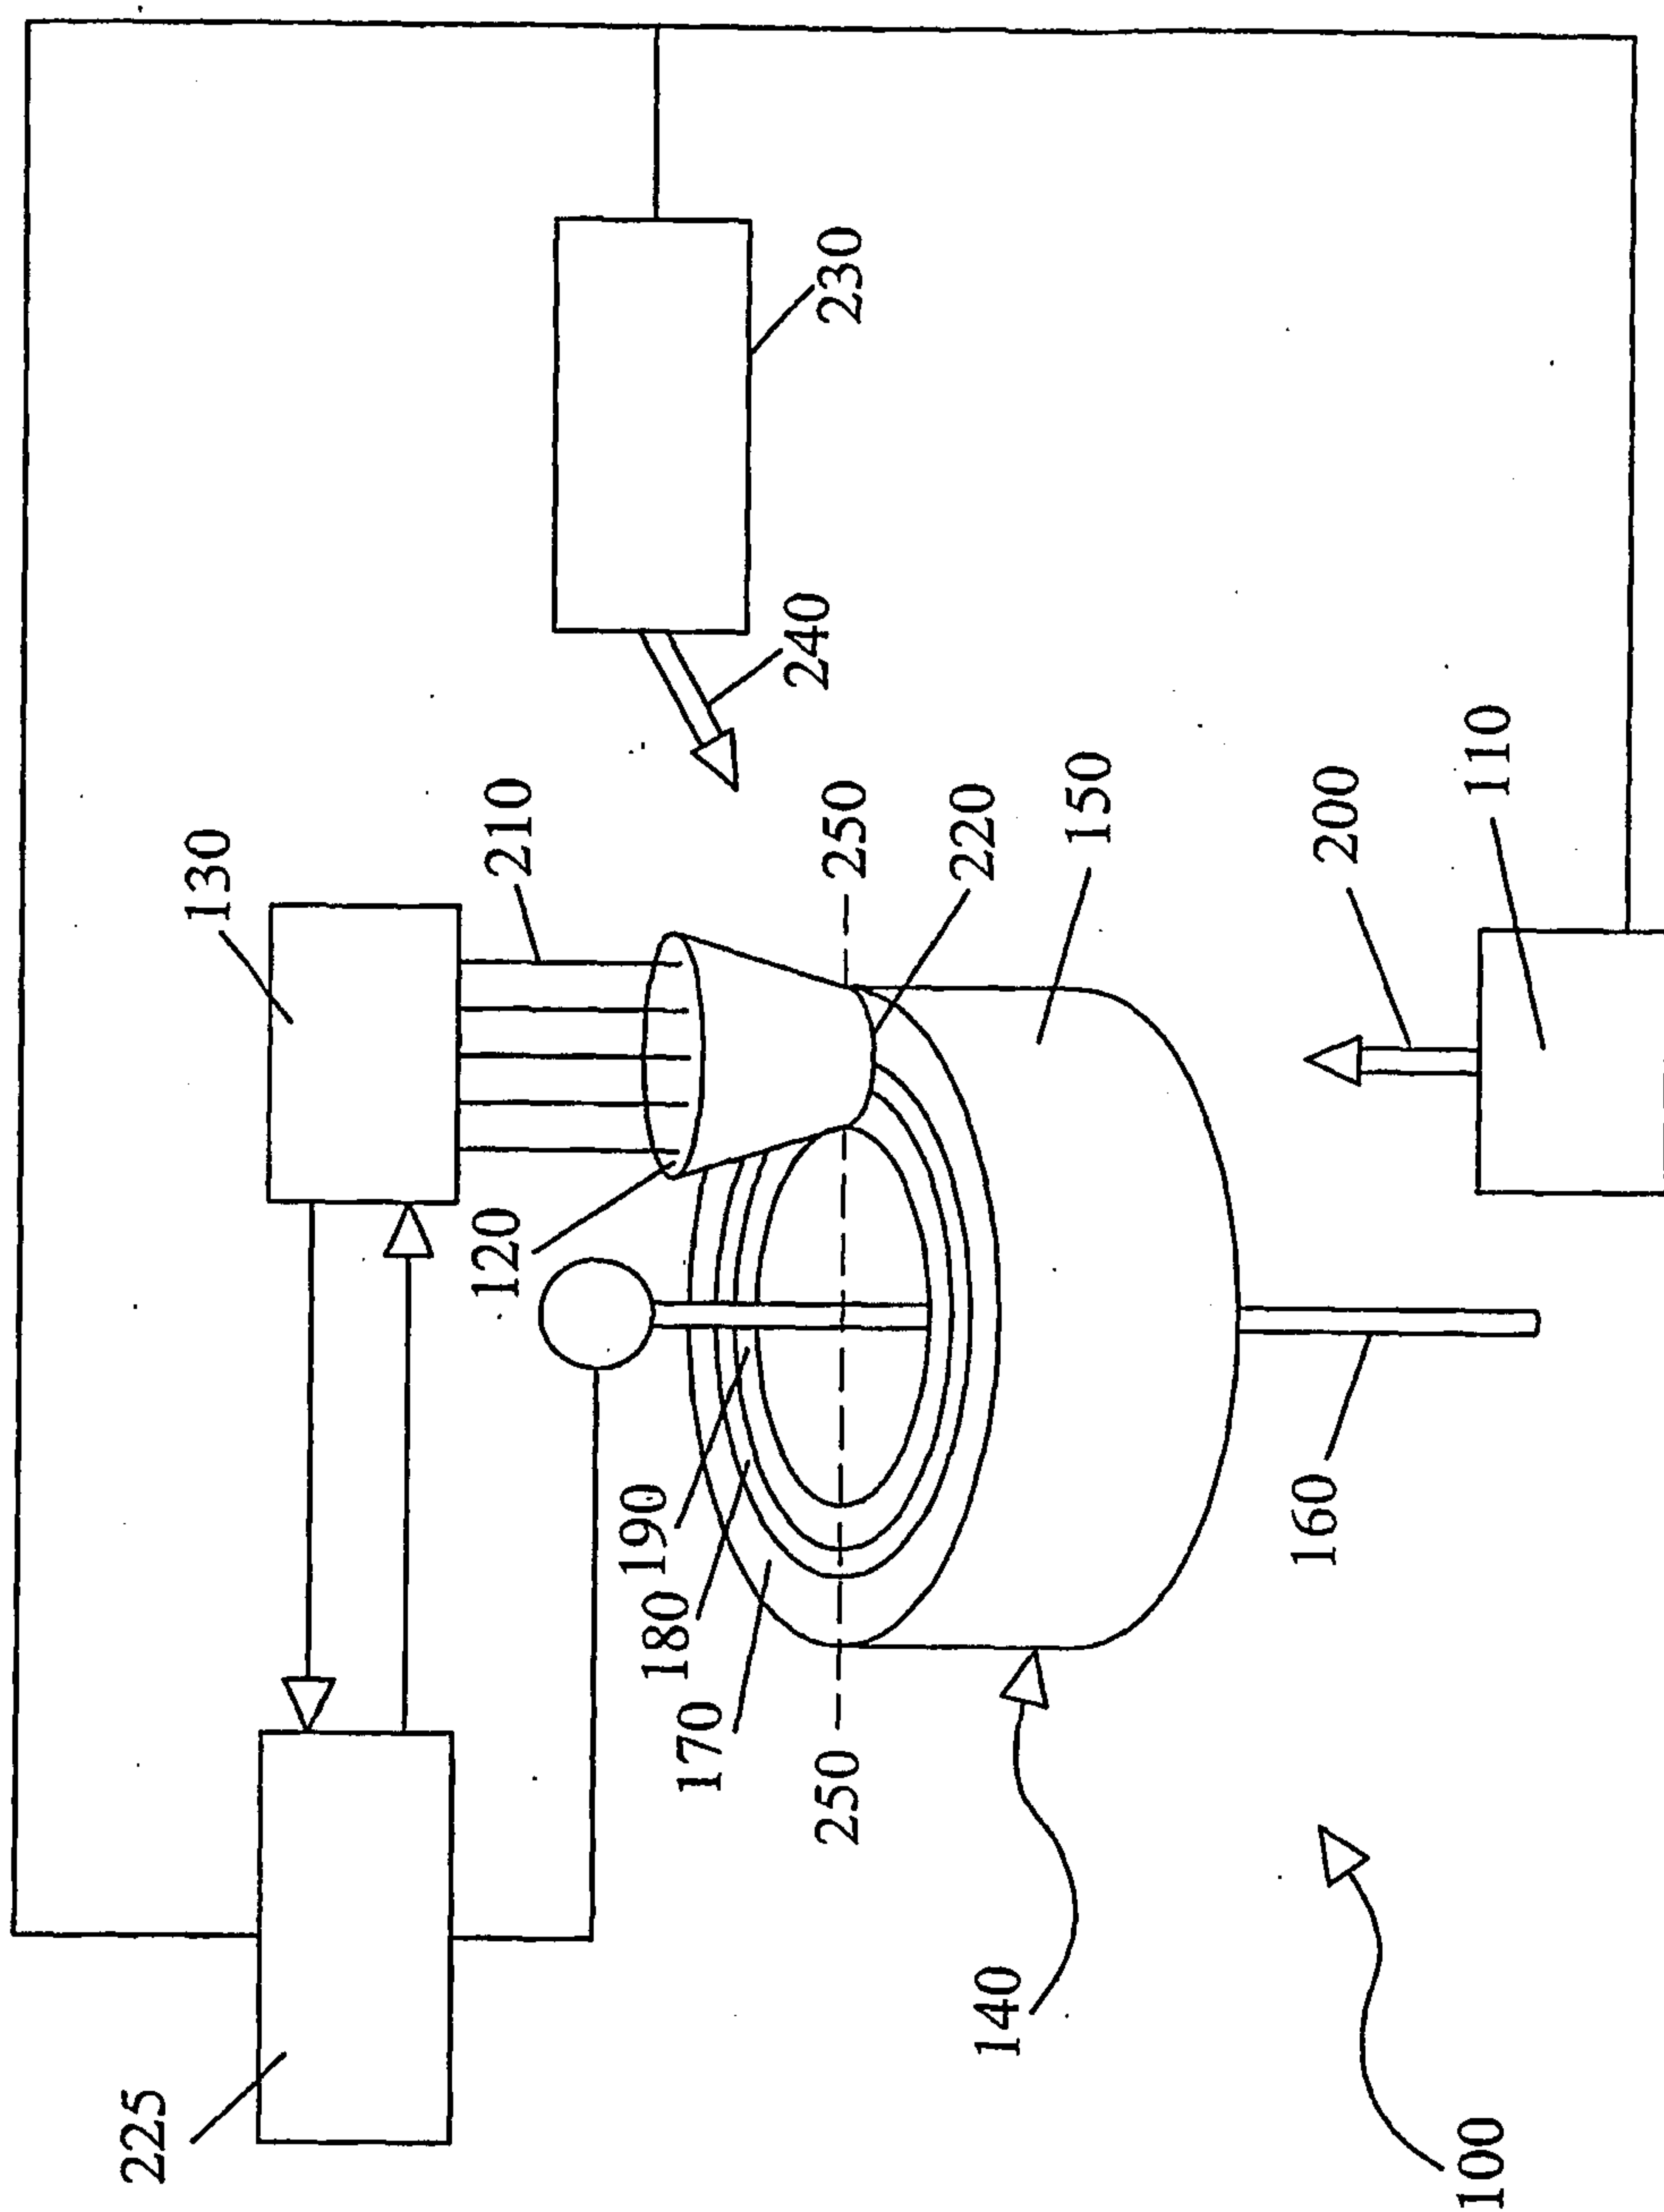


Figure 1

2 / 29

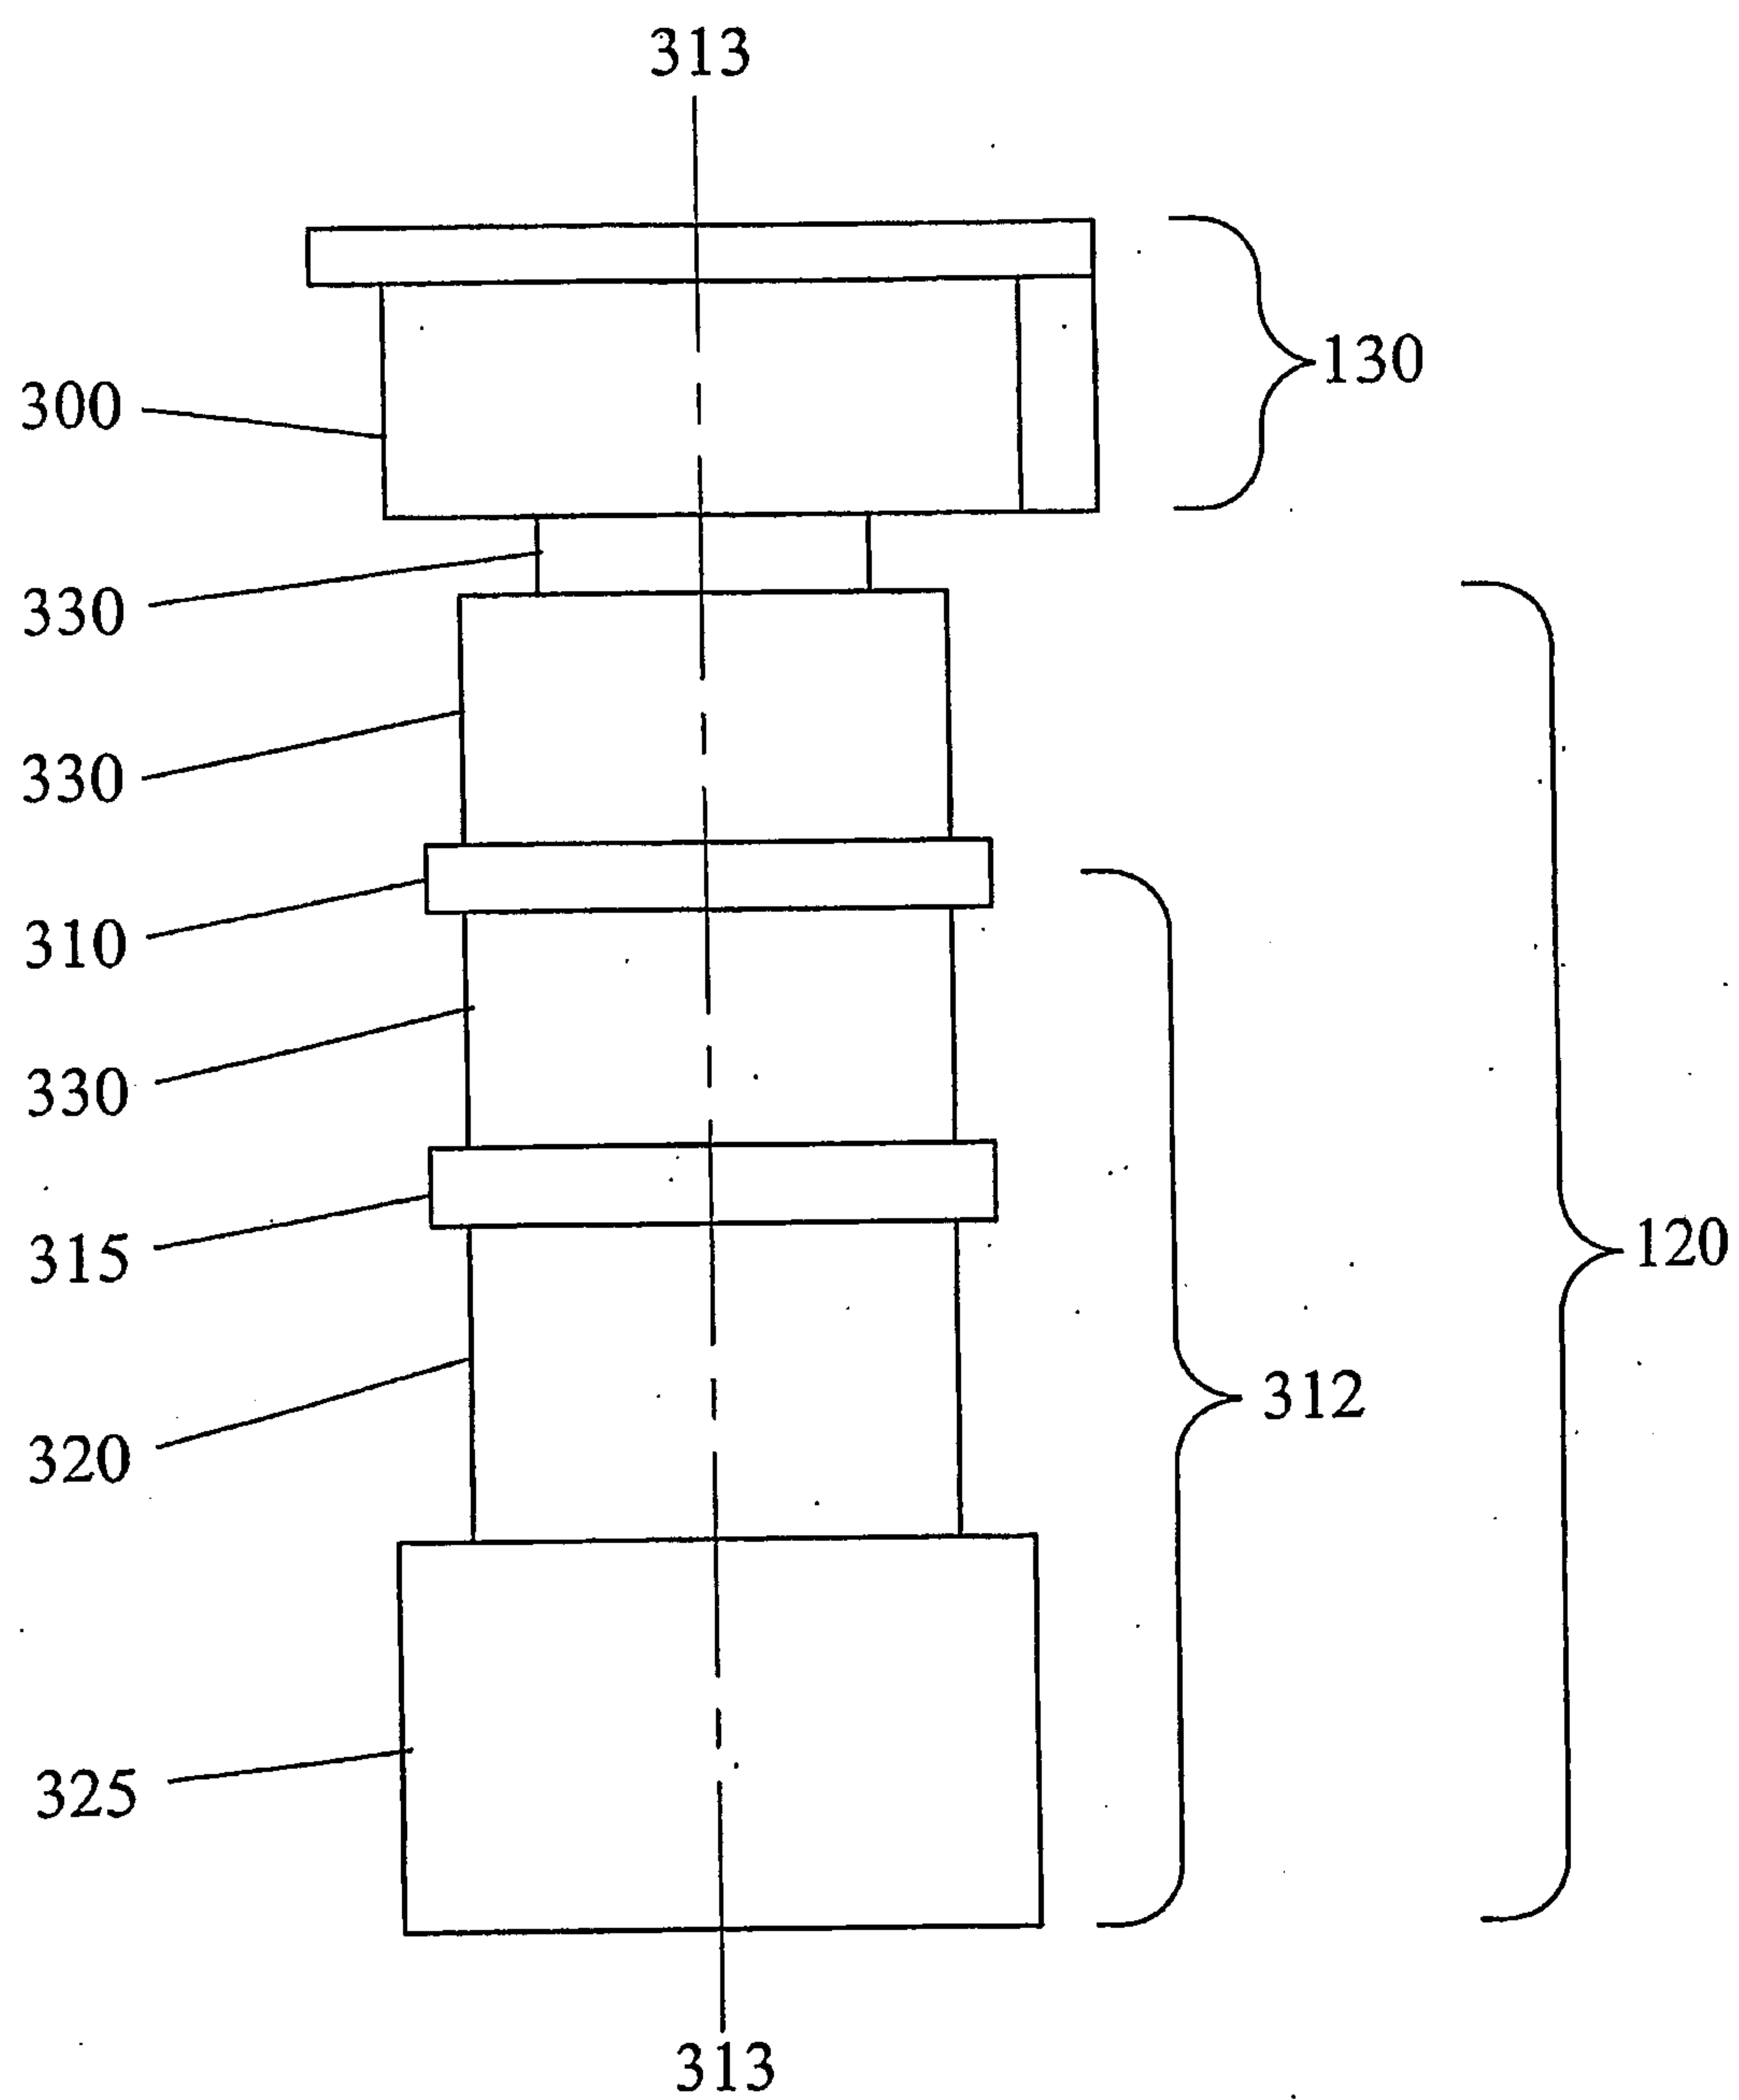


Figure 2

3 / 29

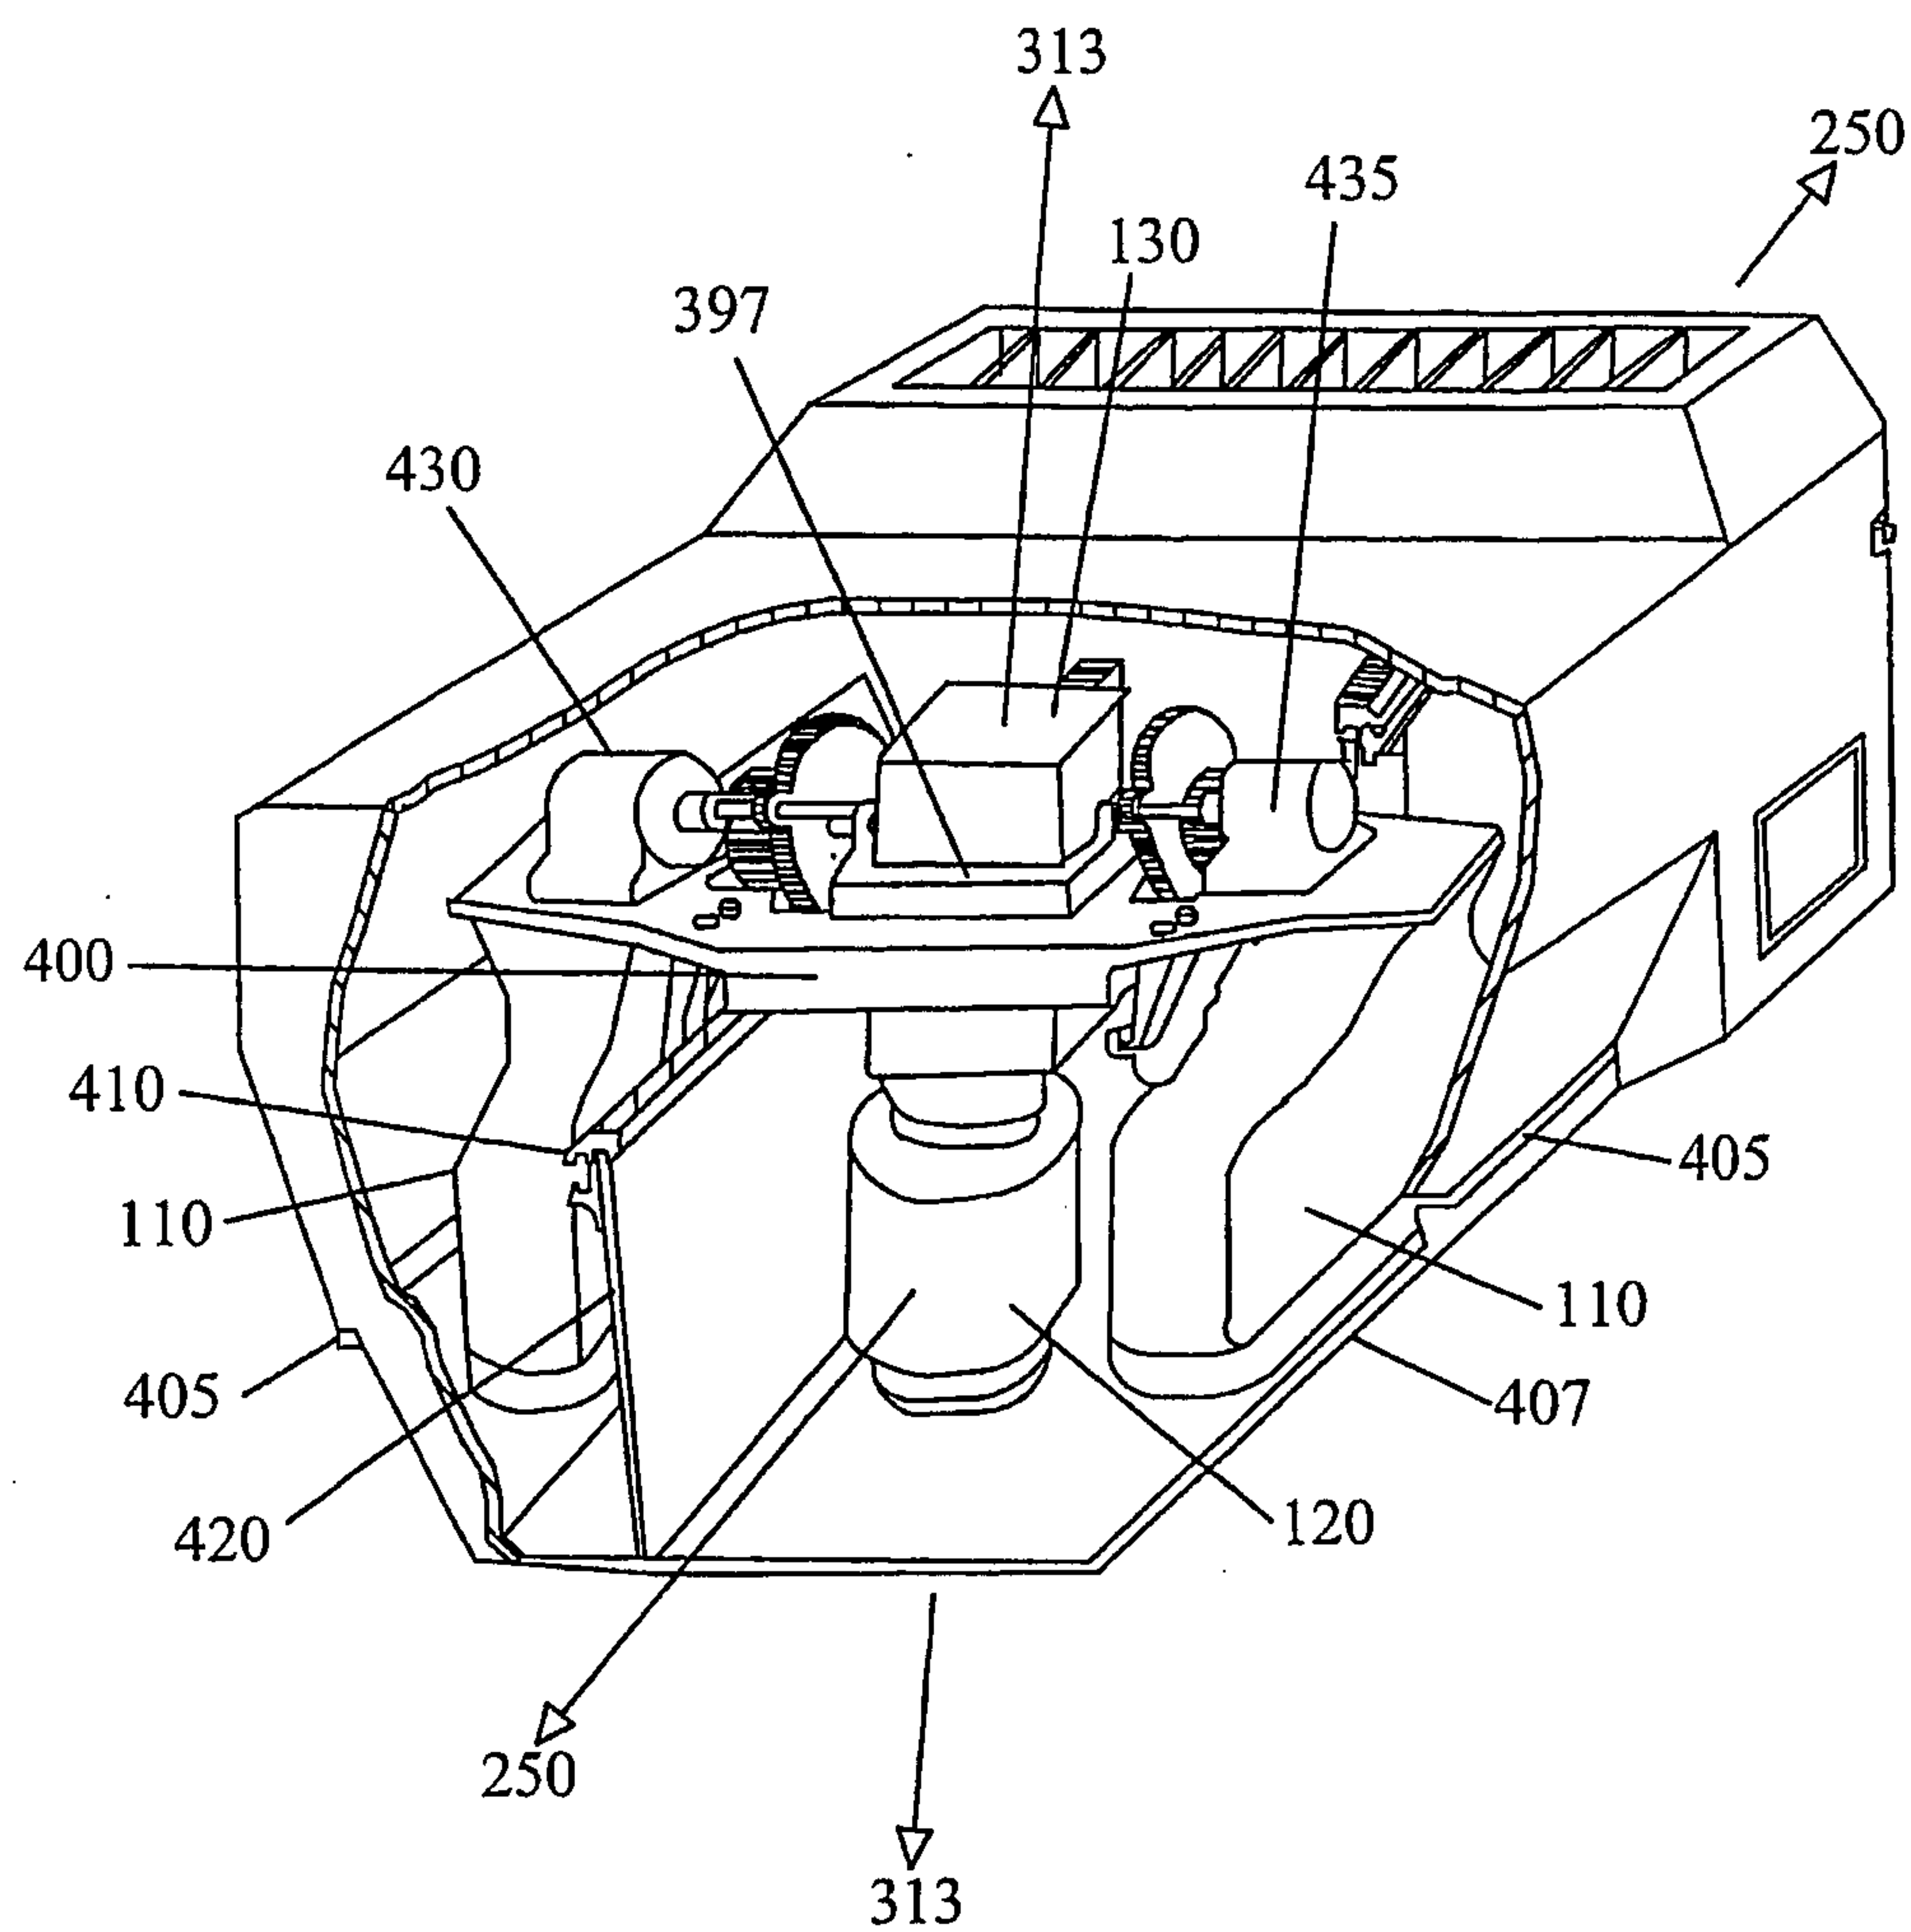


Figure 3

4 / 29

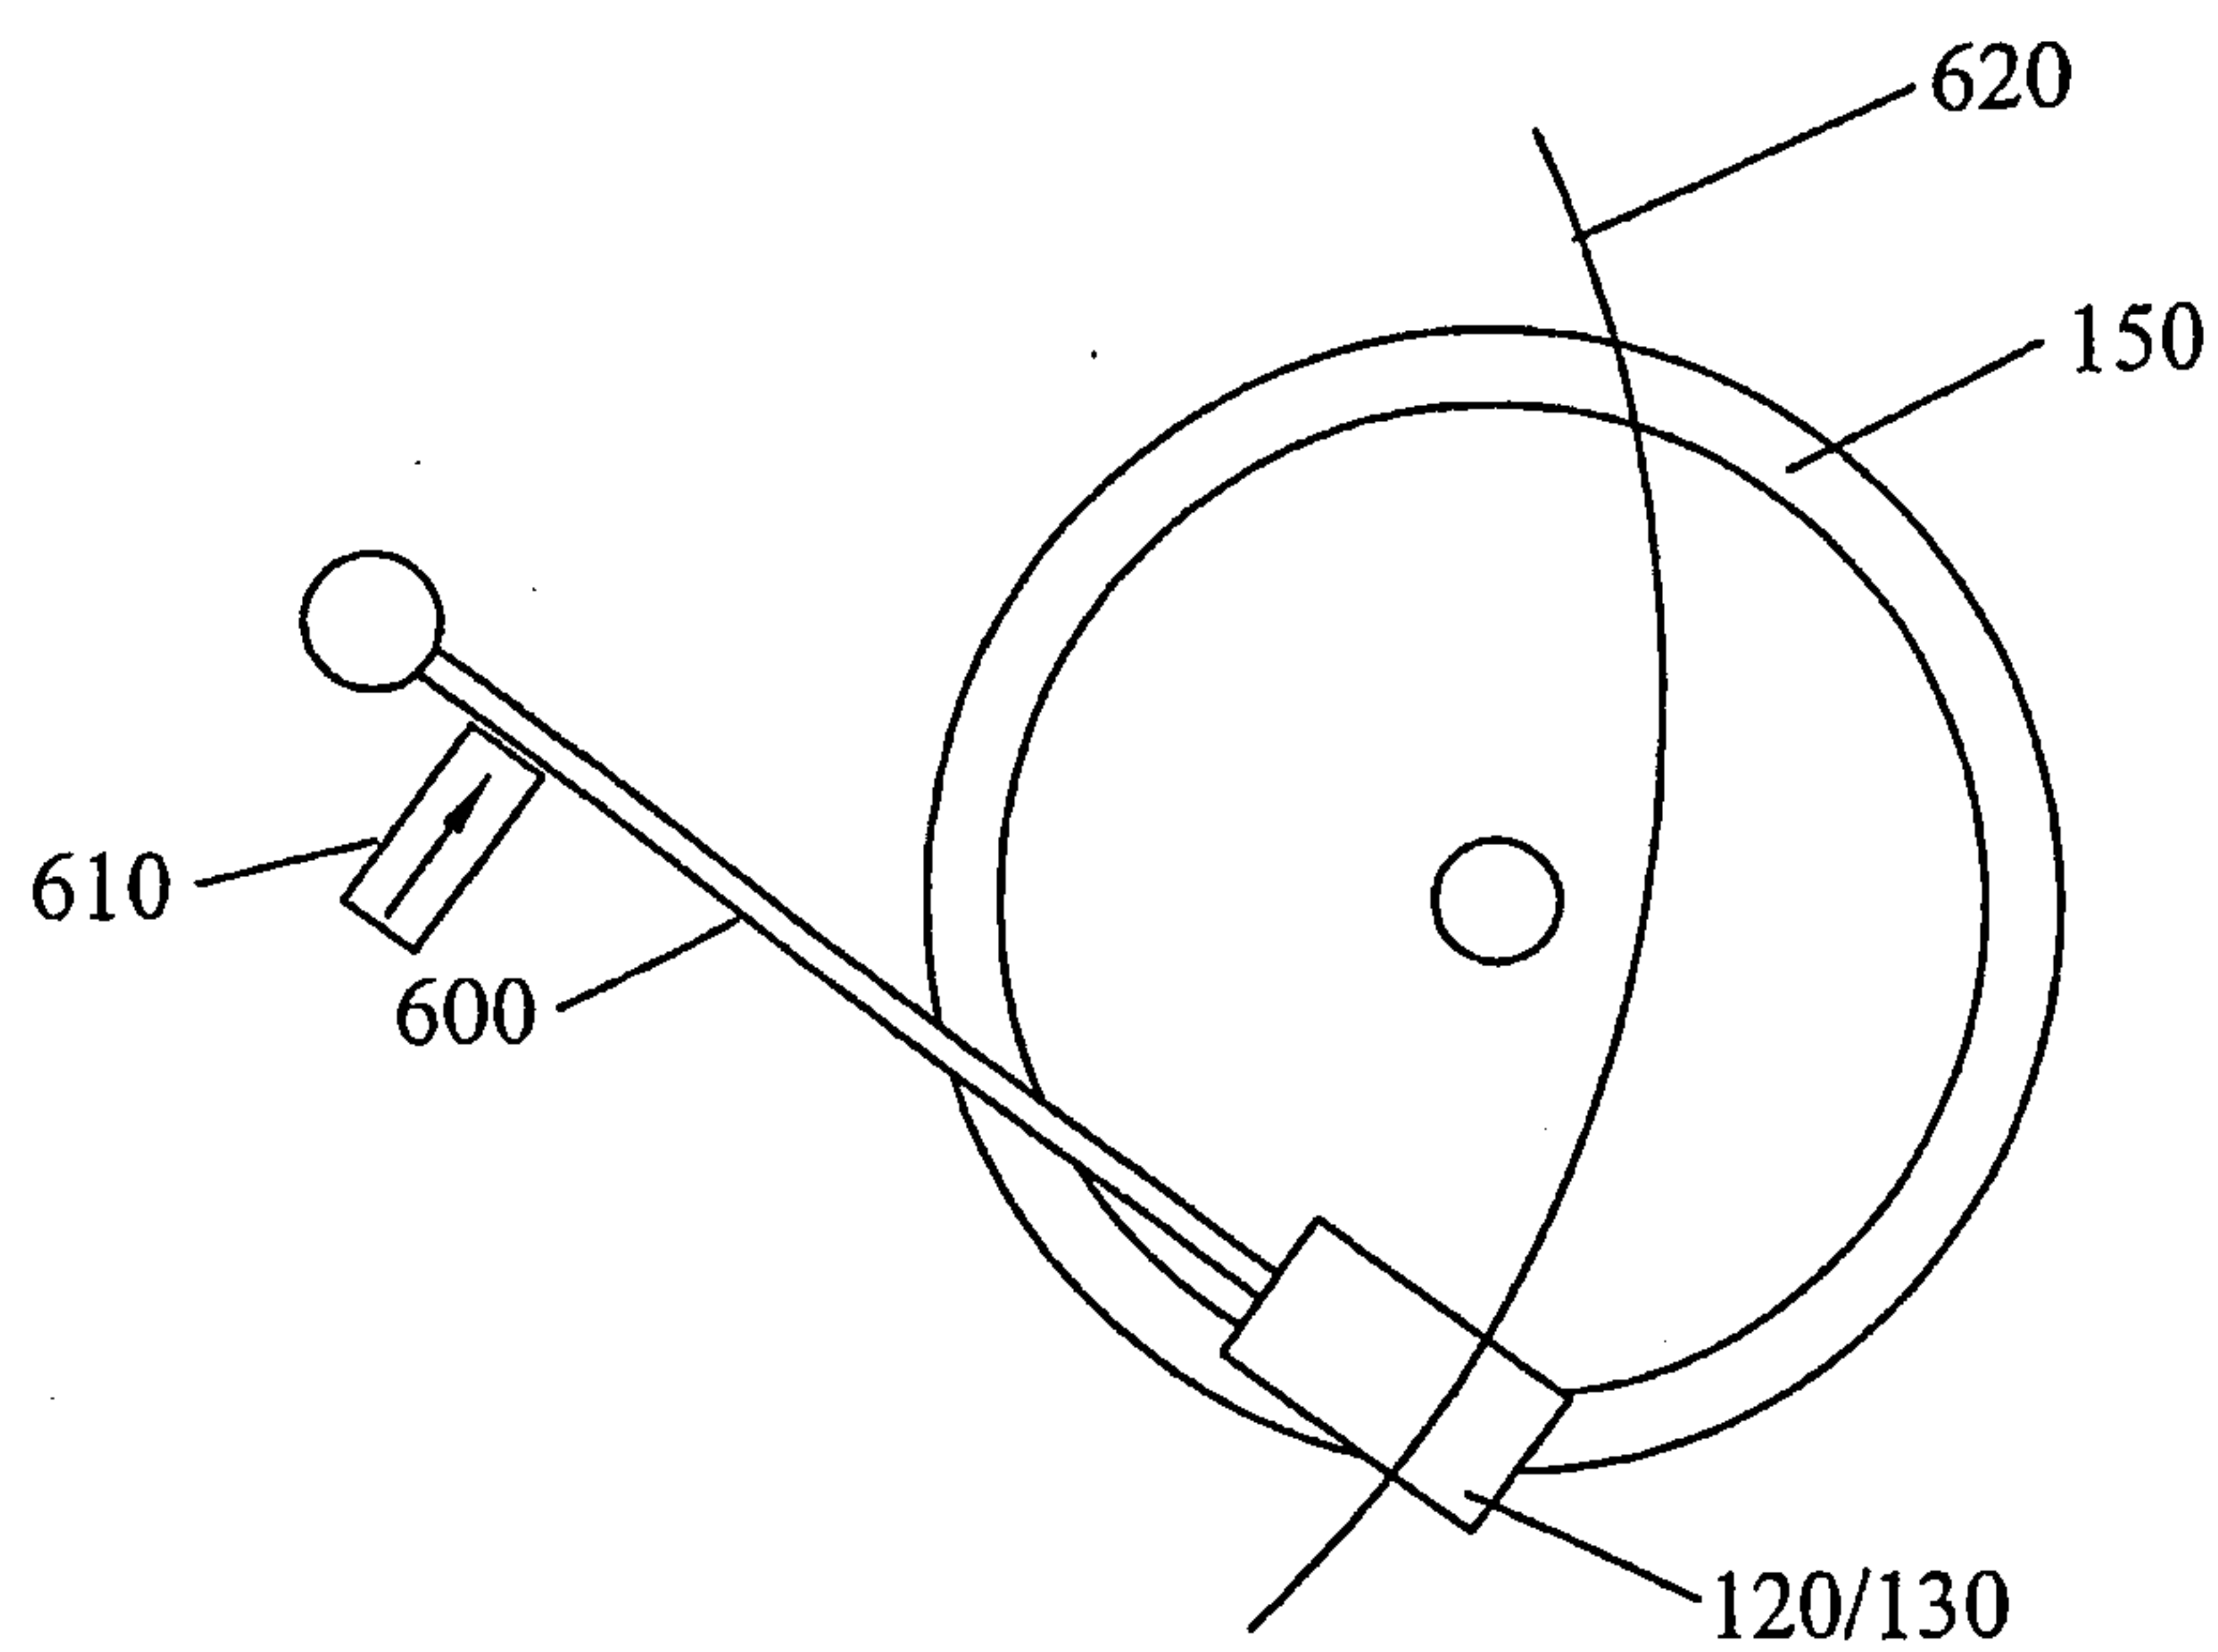


Figure 4

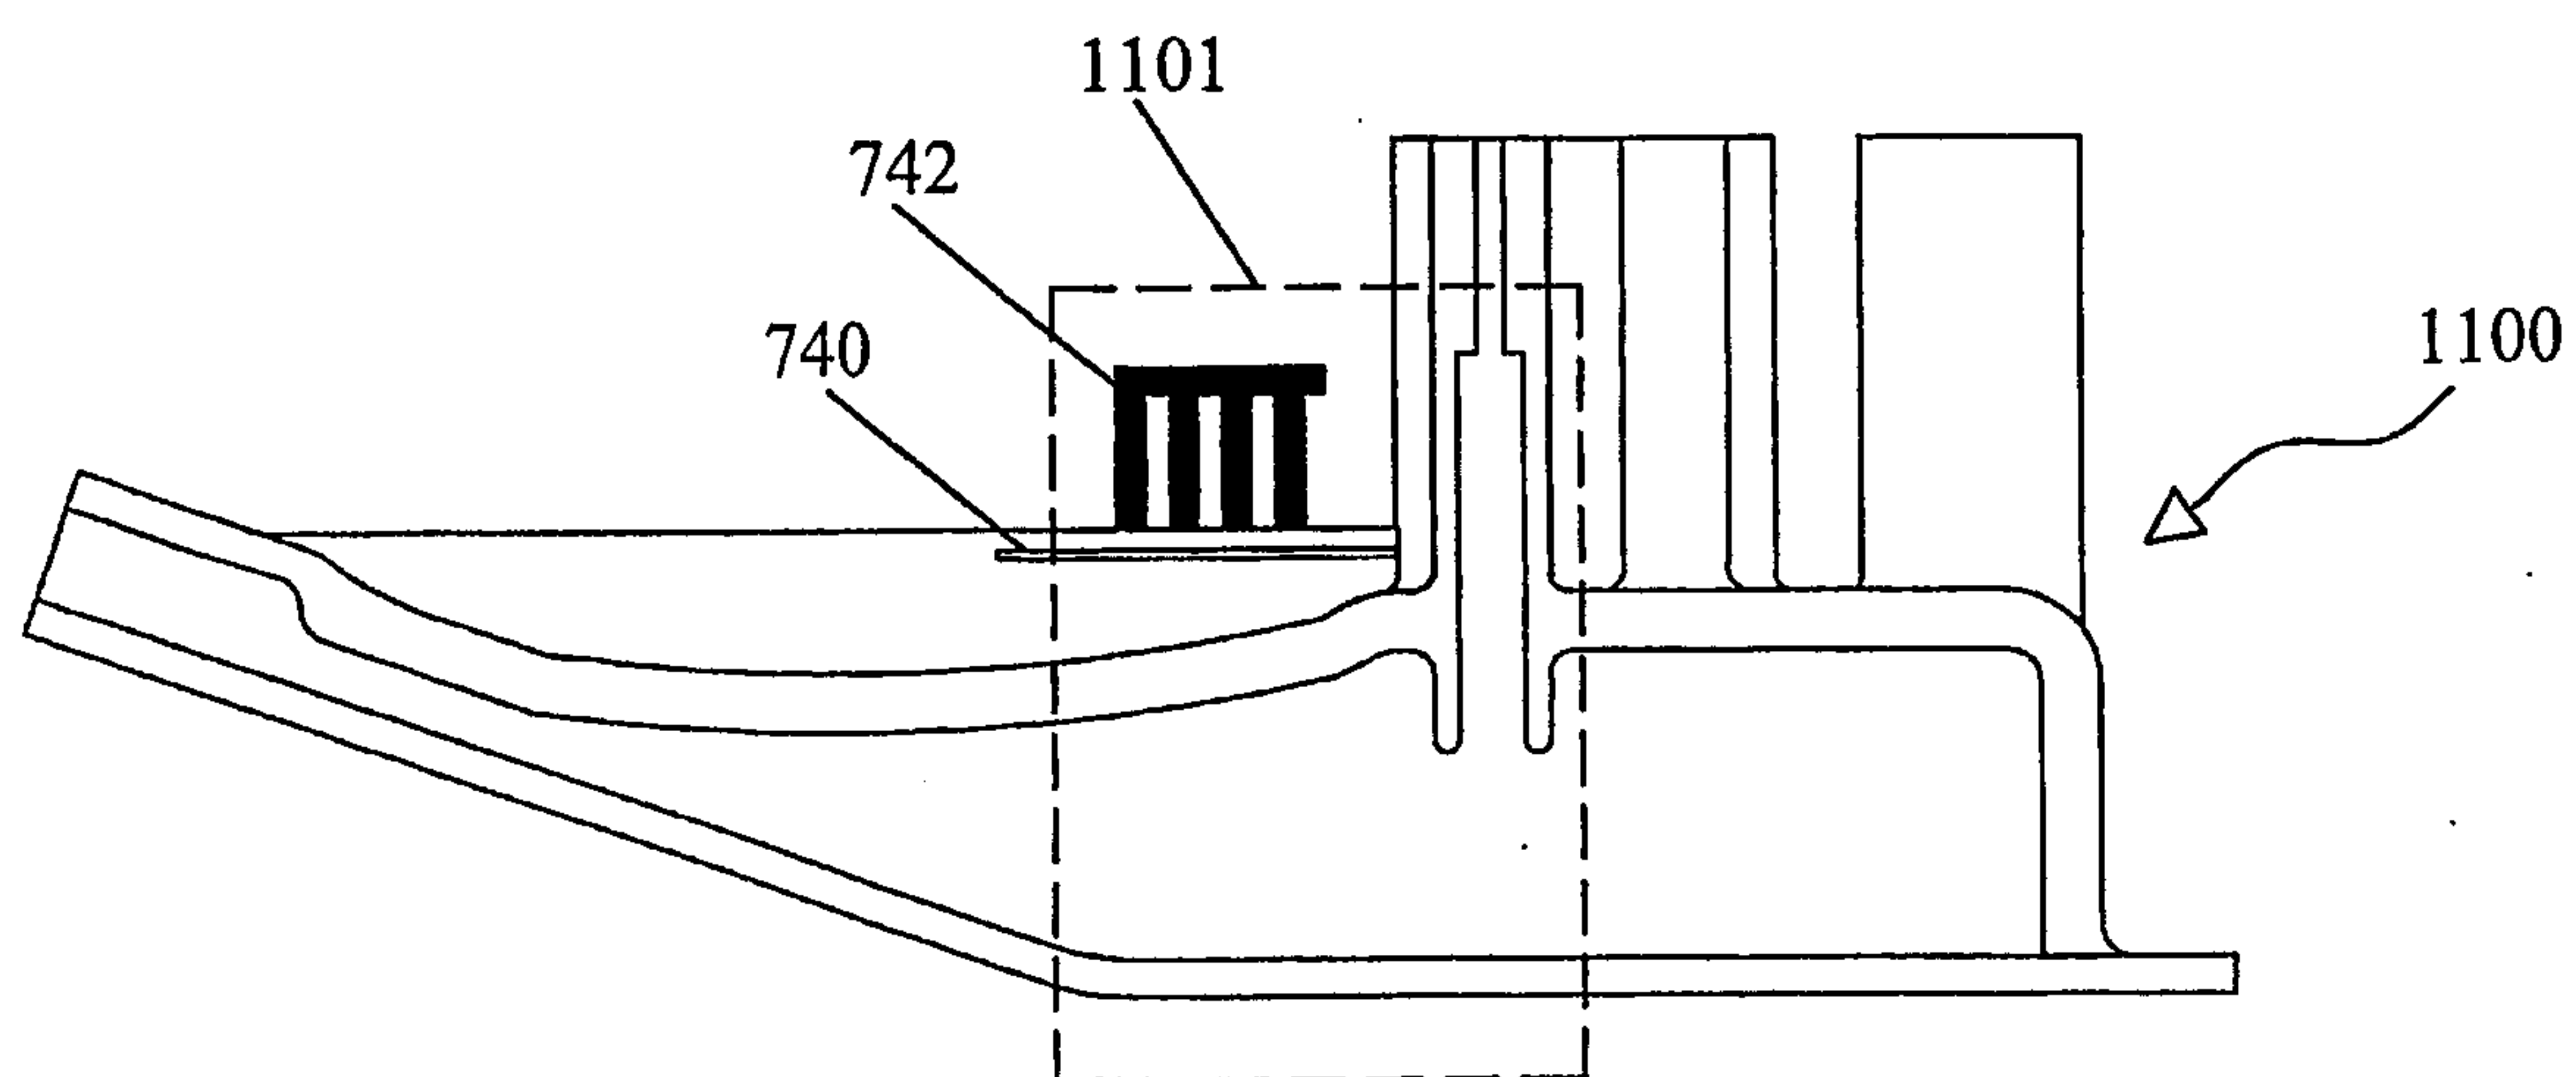


Figure 6

REPLACEMENT SHEET

5 / 29

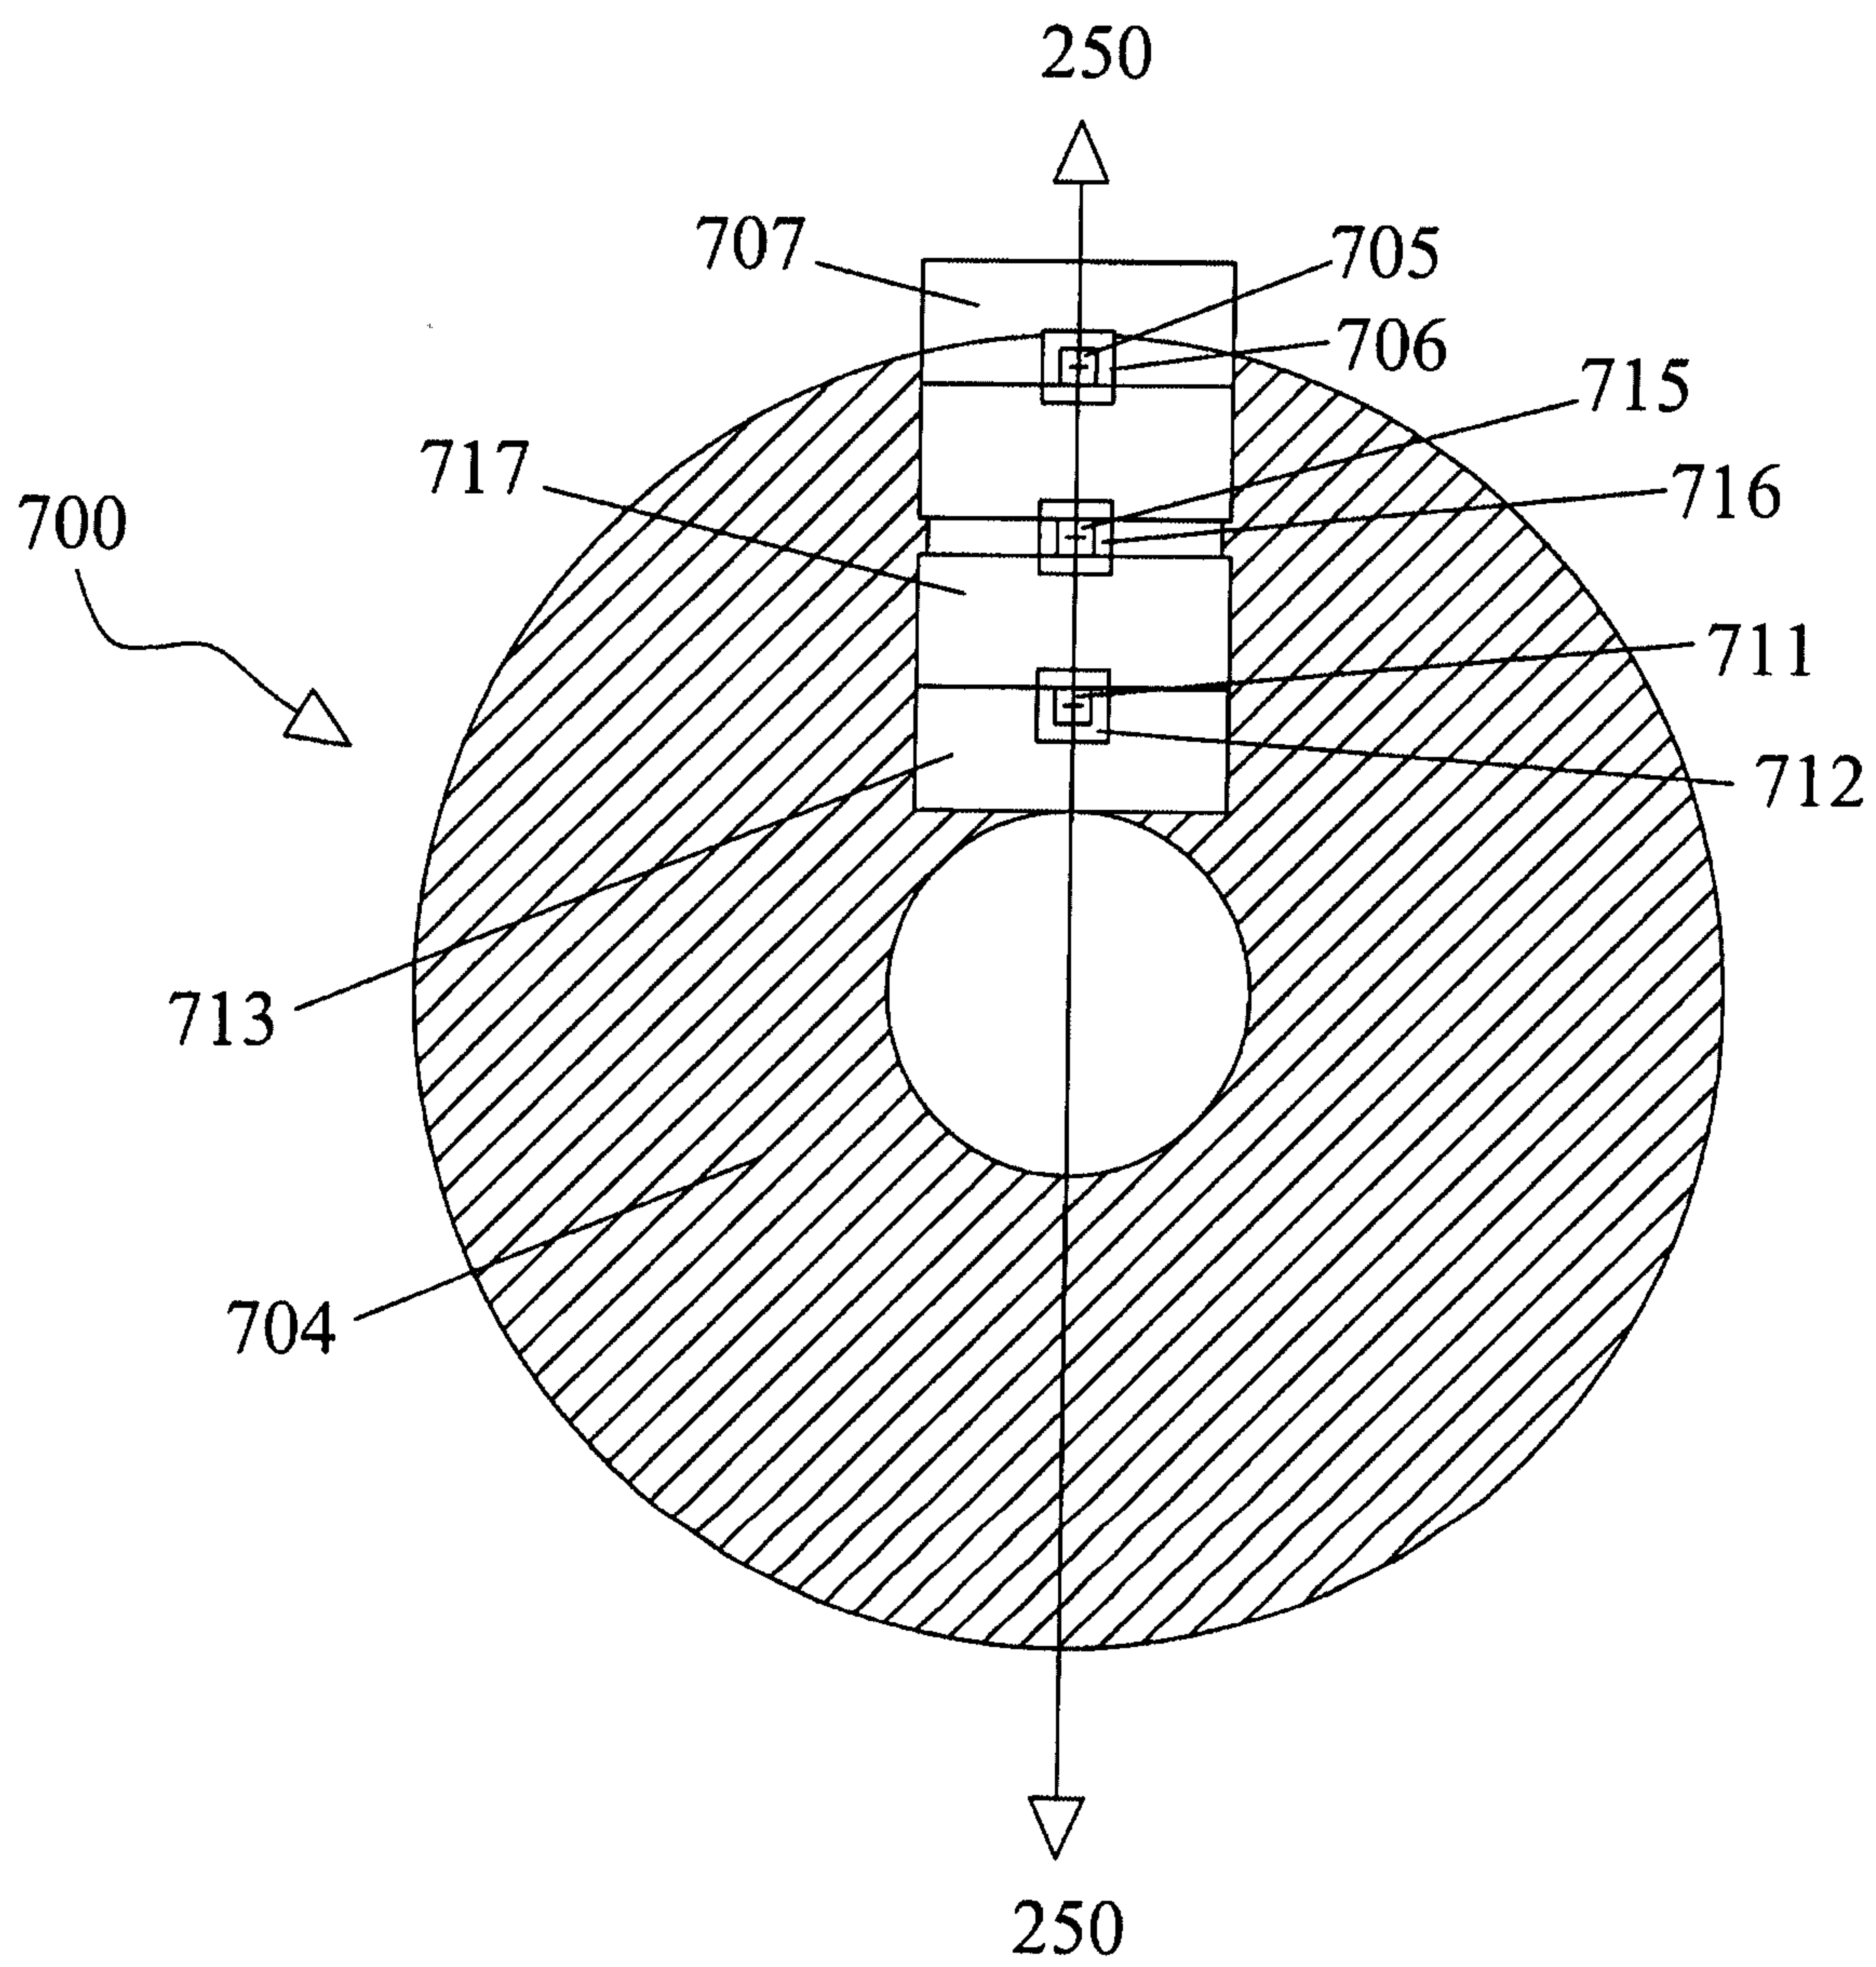


Figure 5

6 / 29

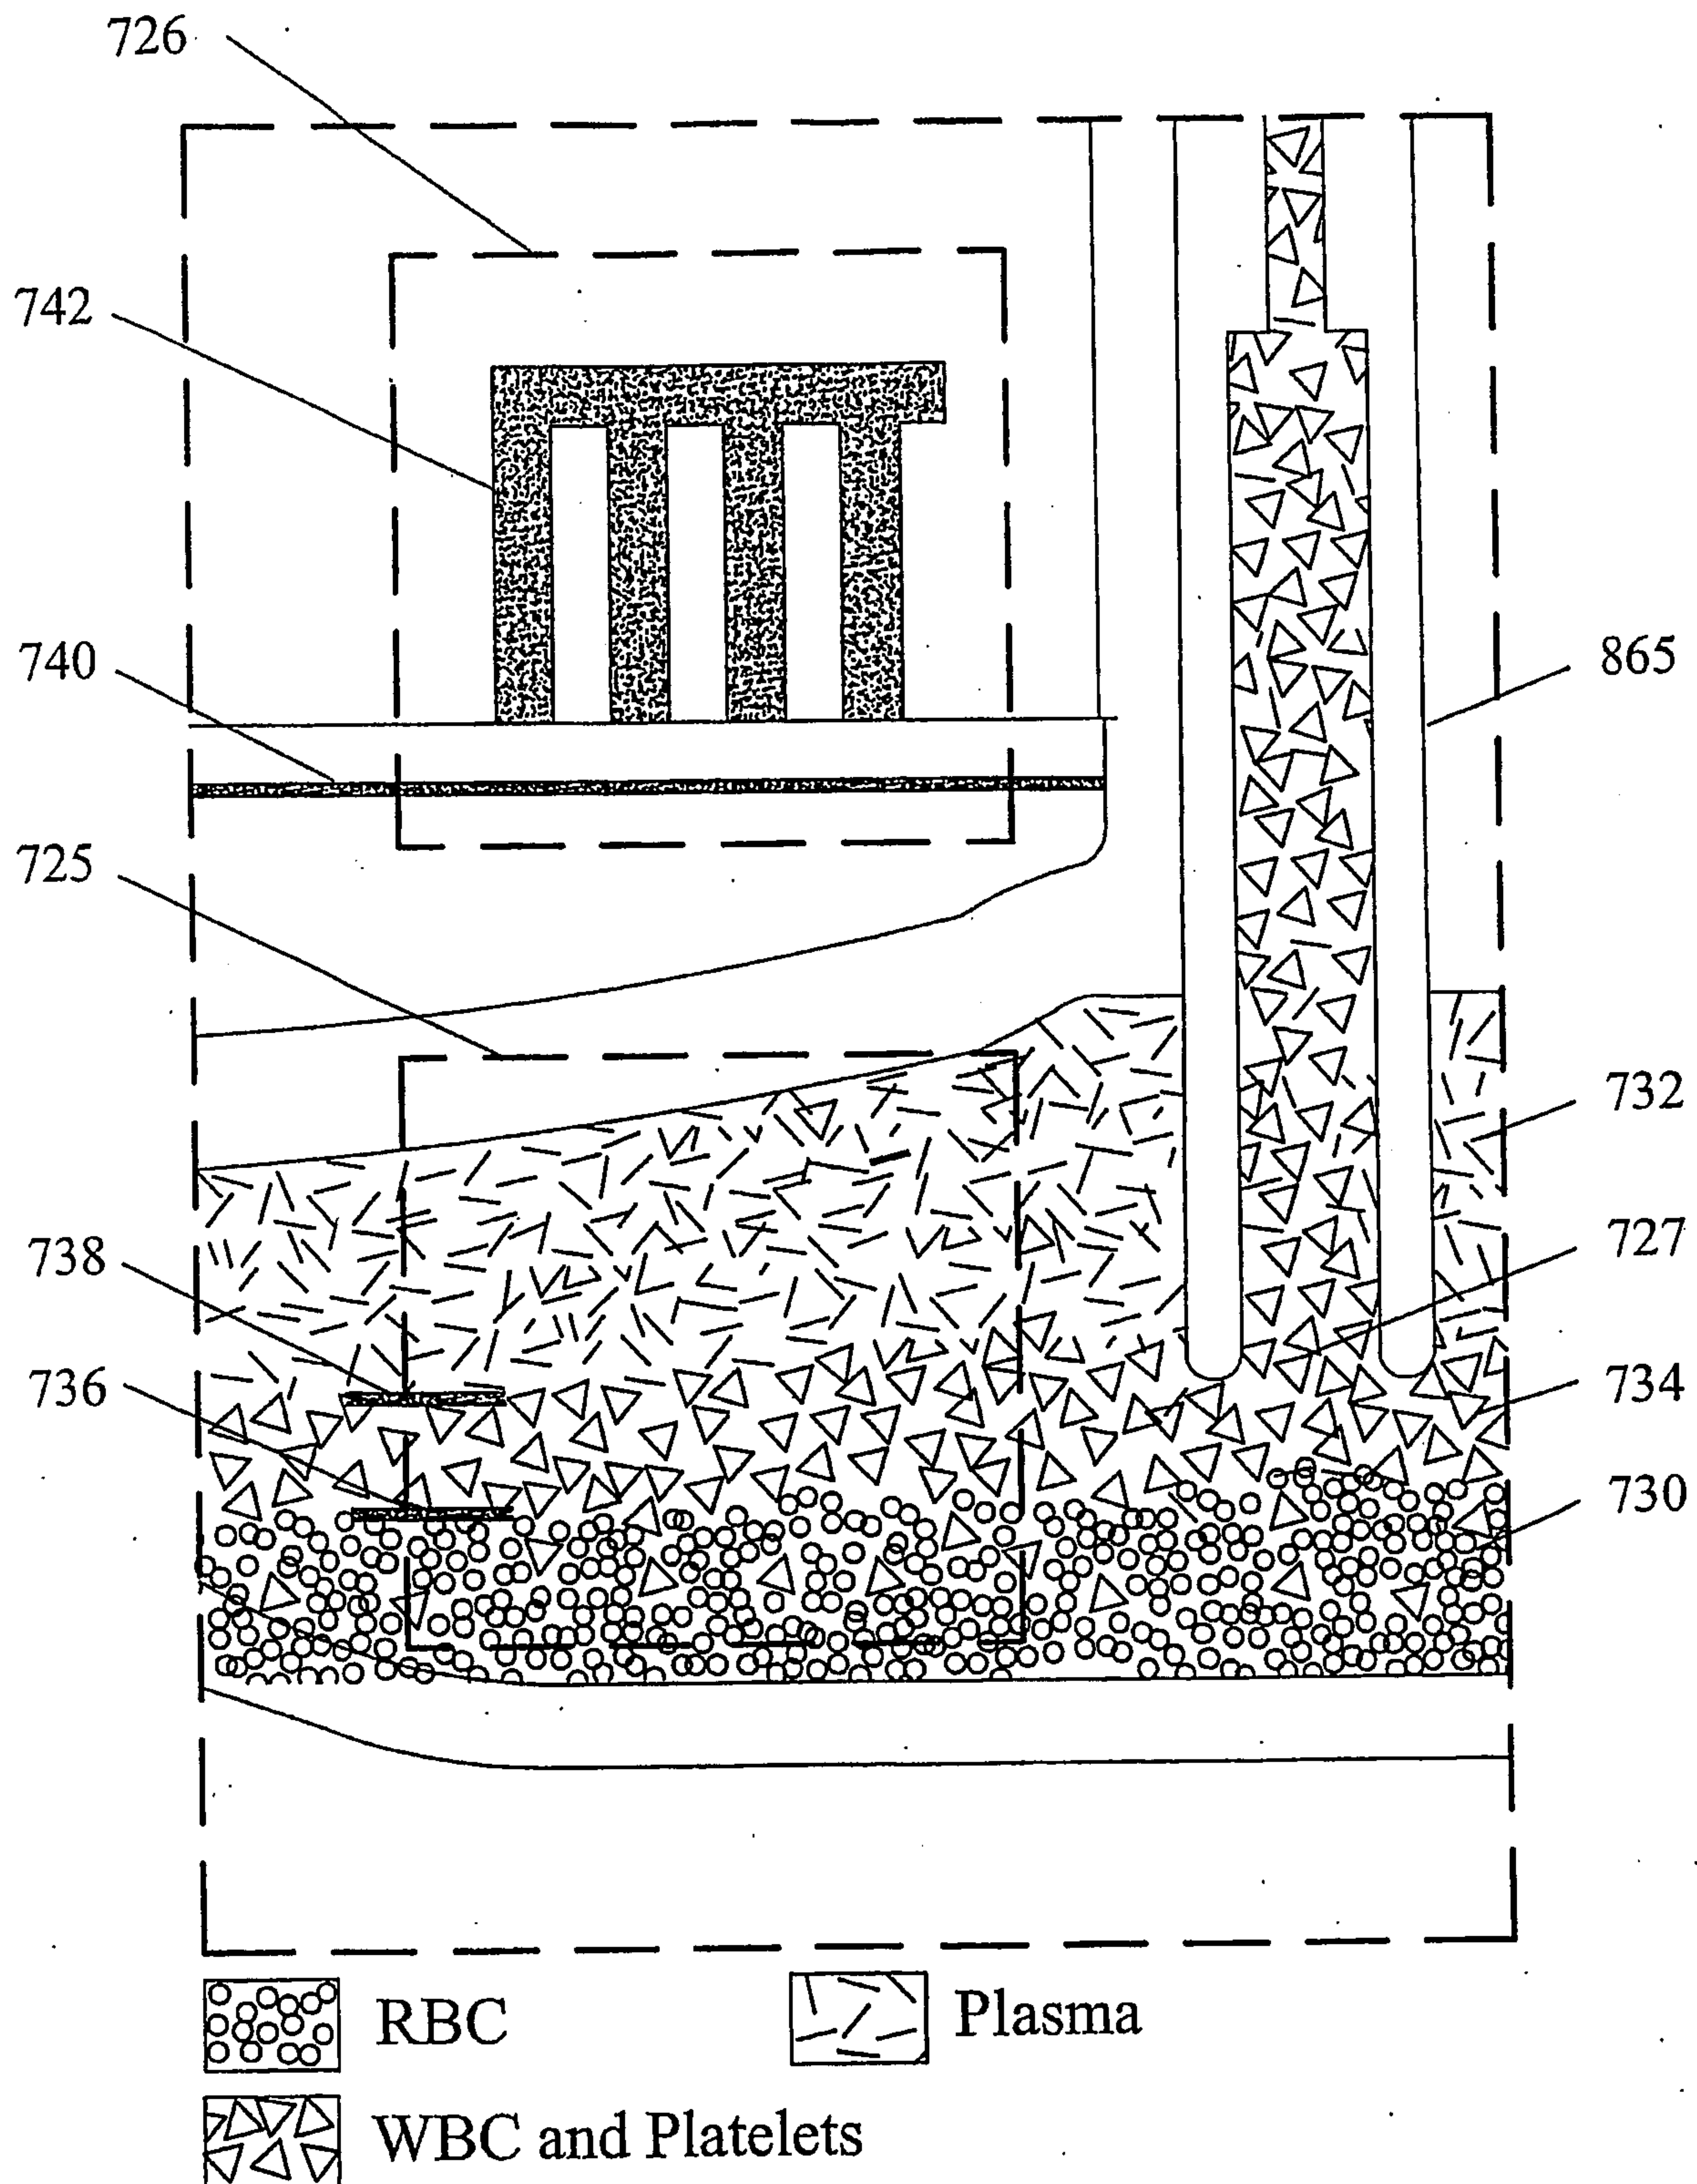


Figure 6A

7 / 29

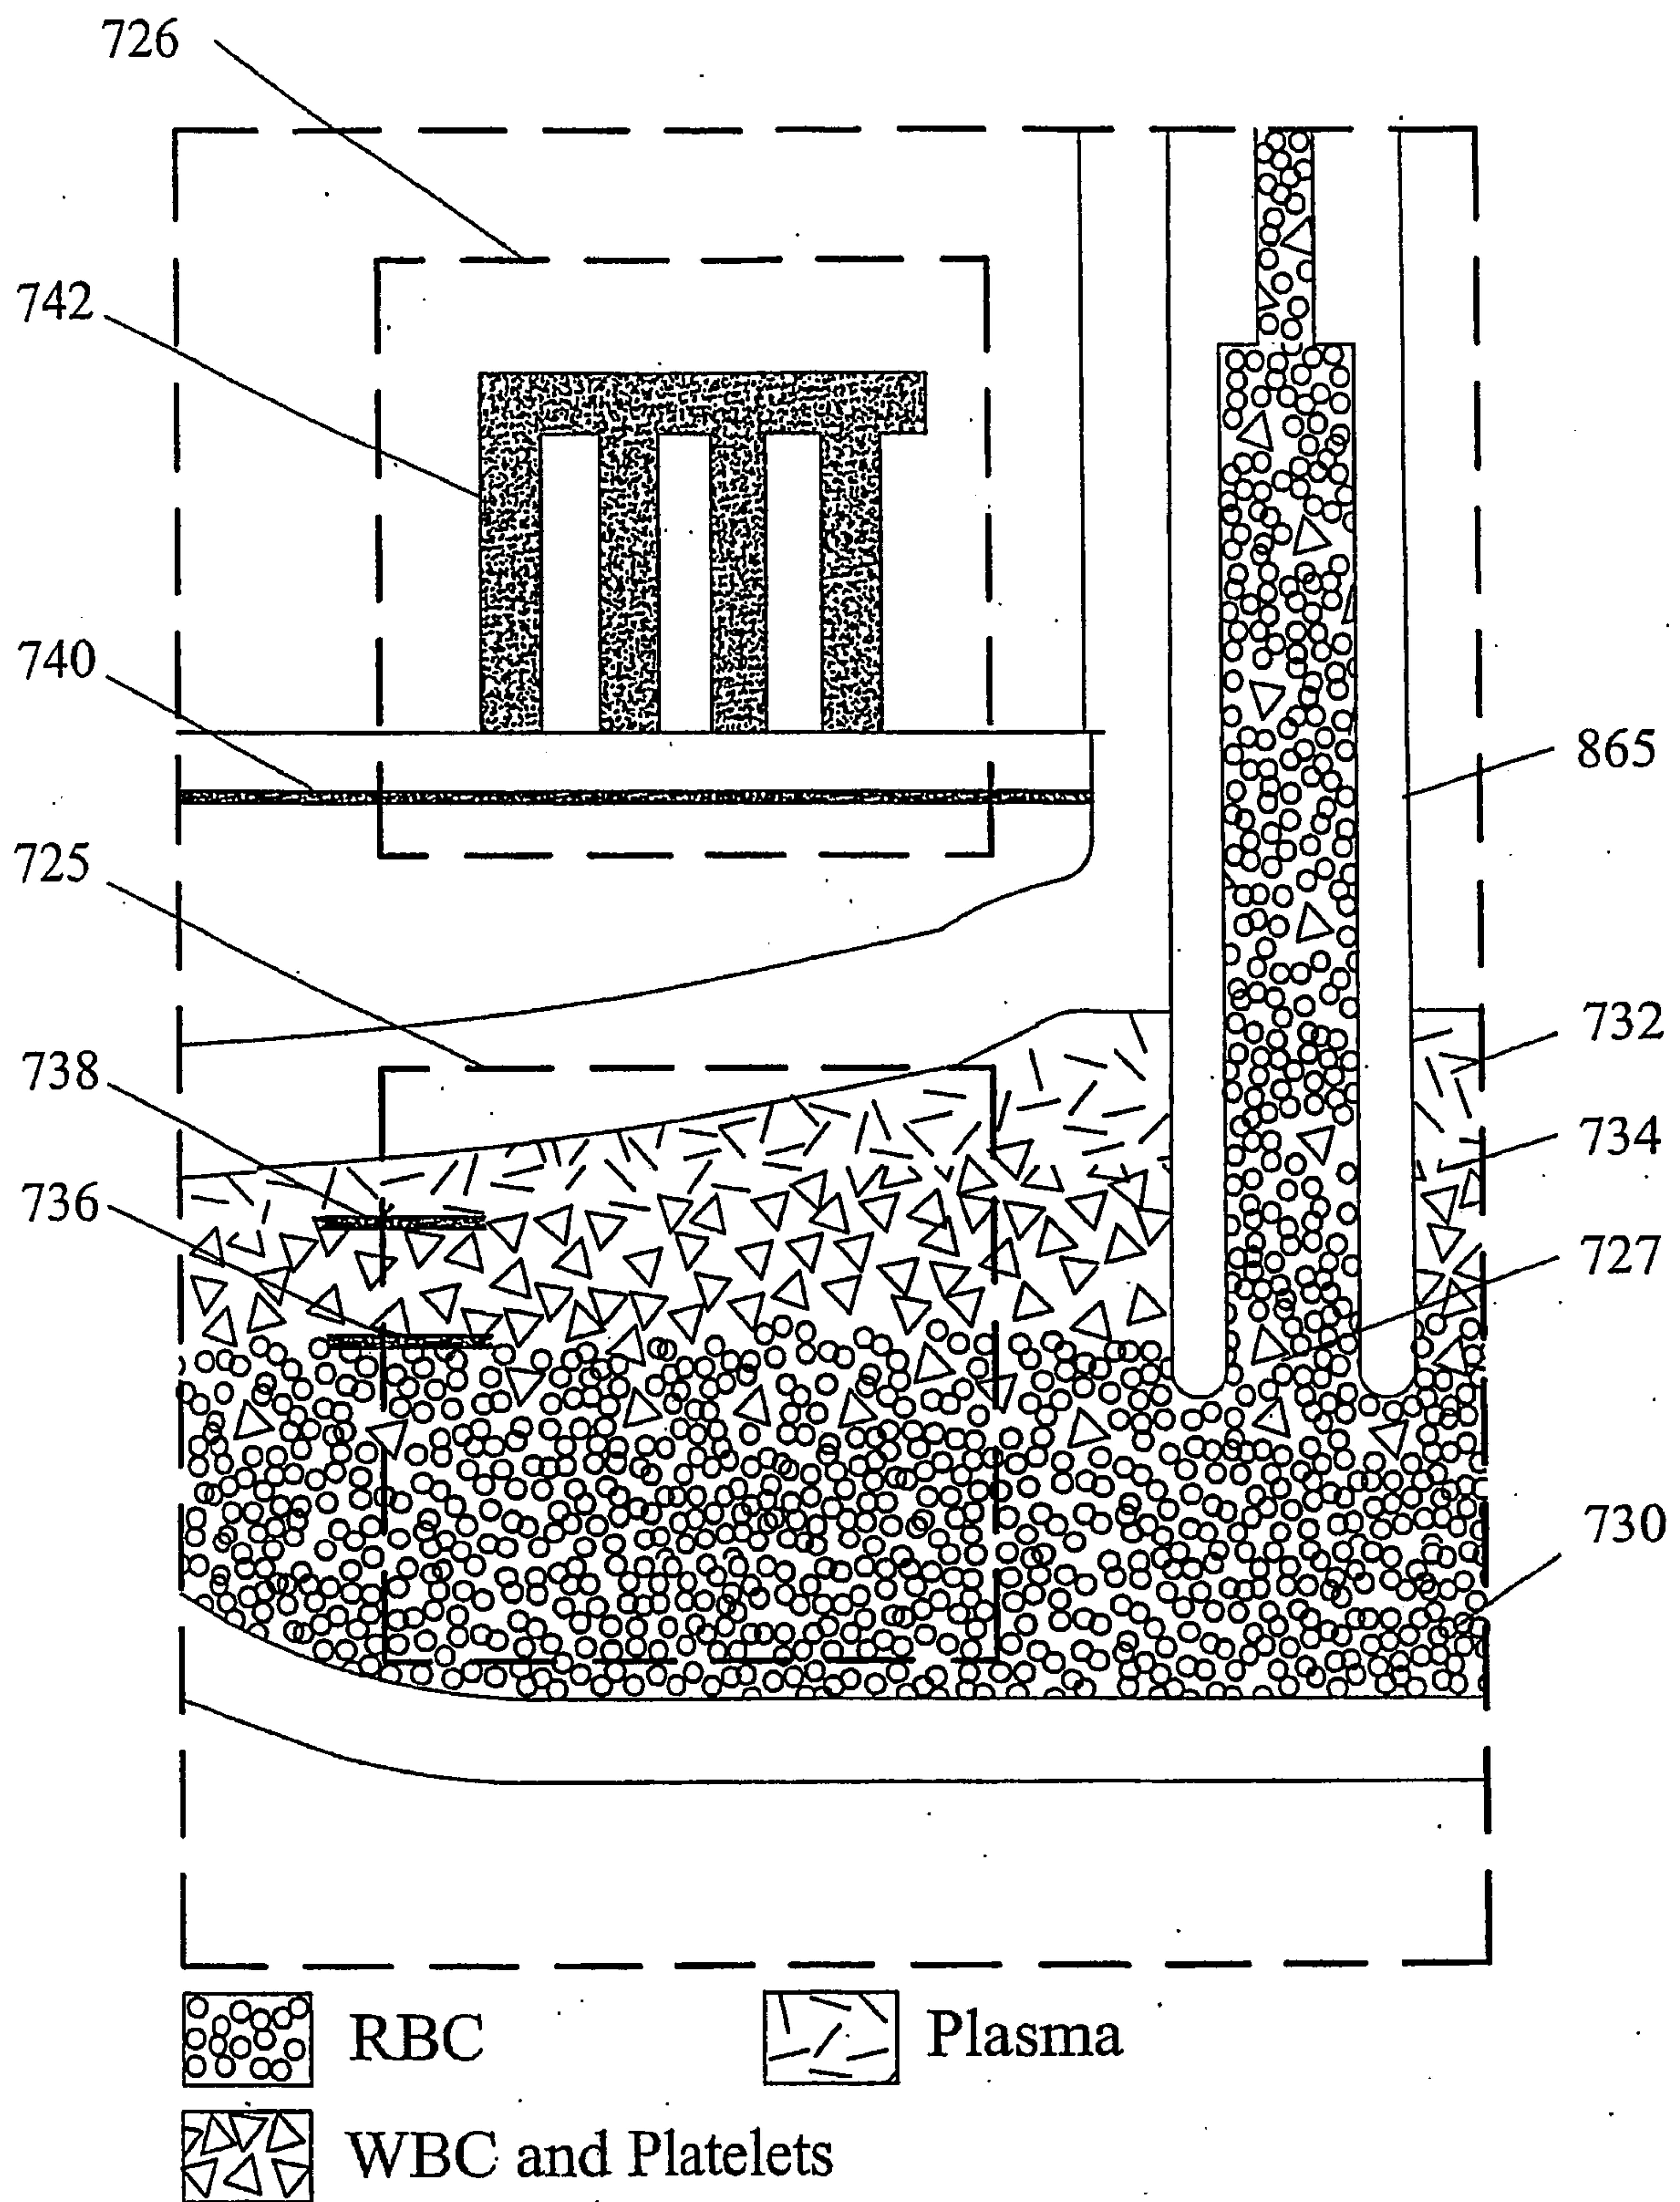


Figure 6B

8 / 29


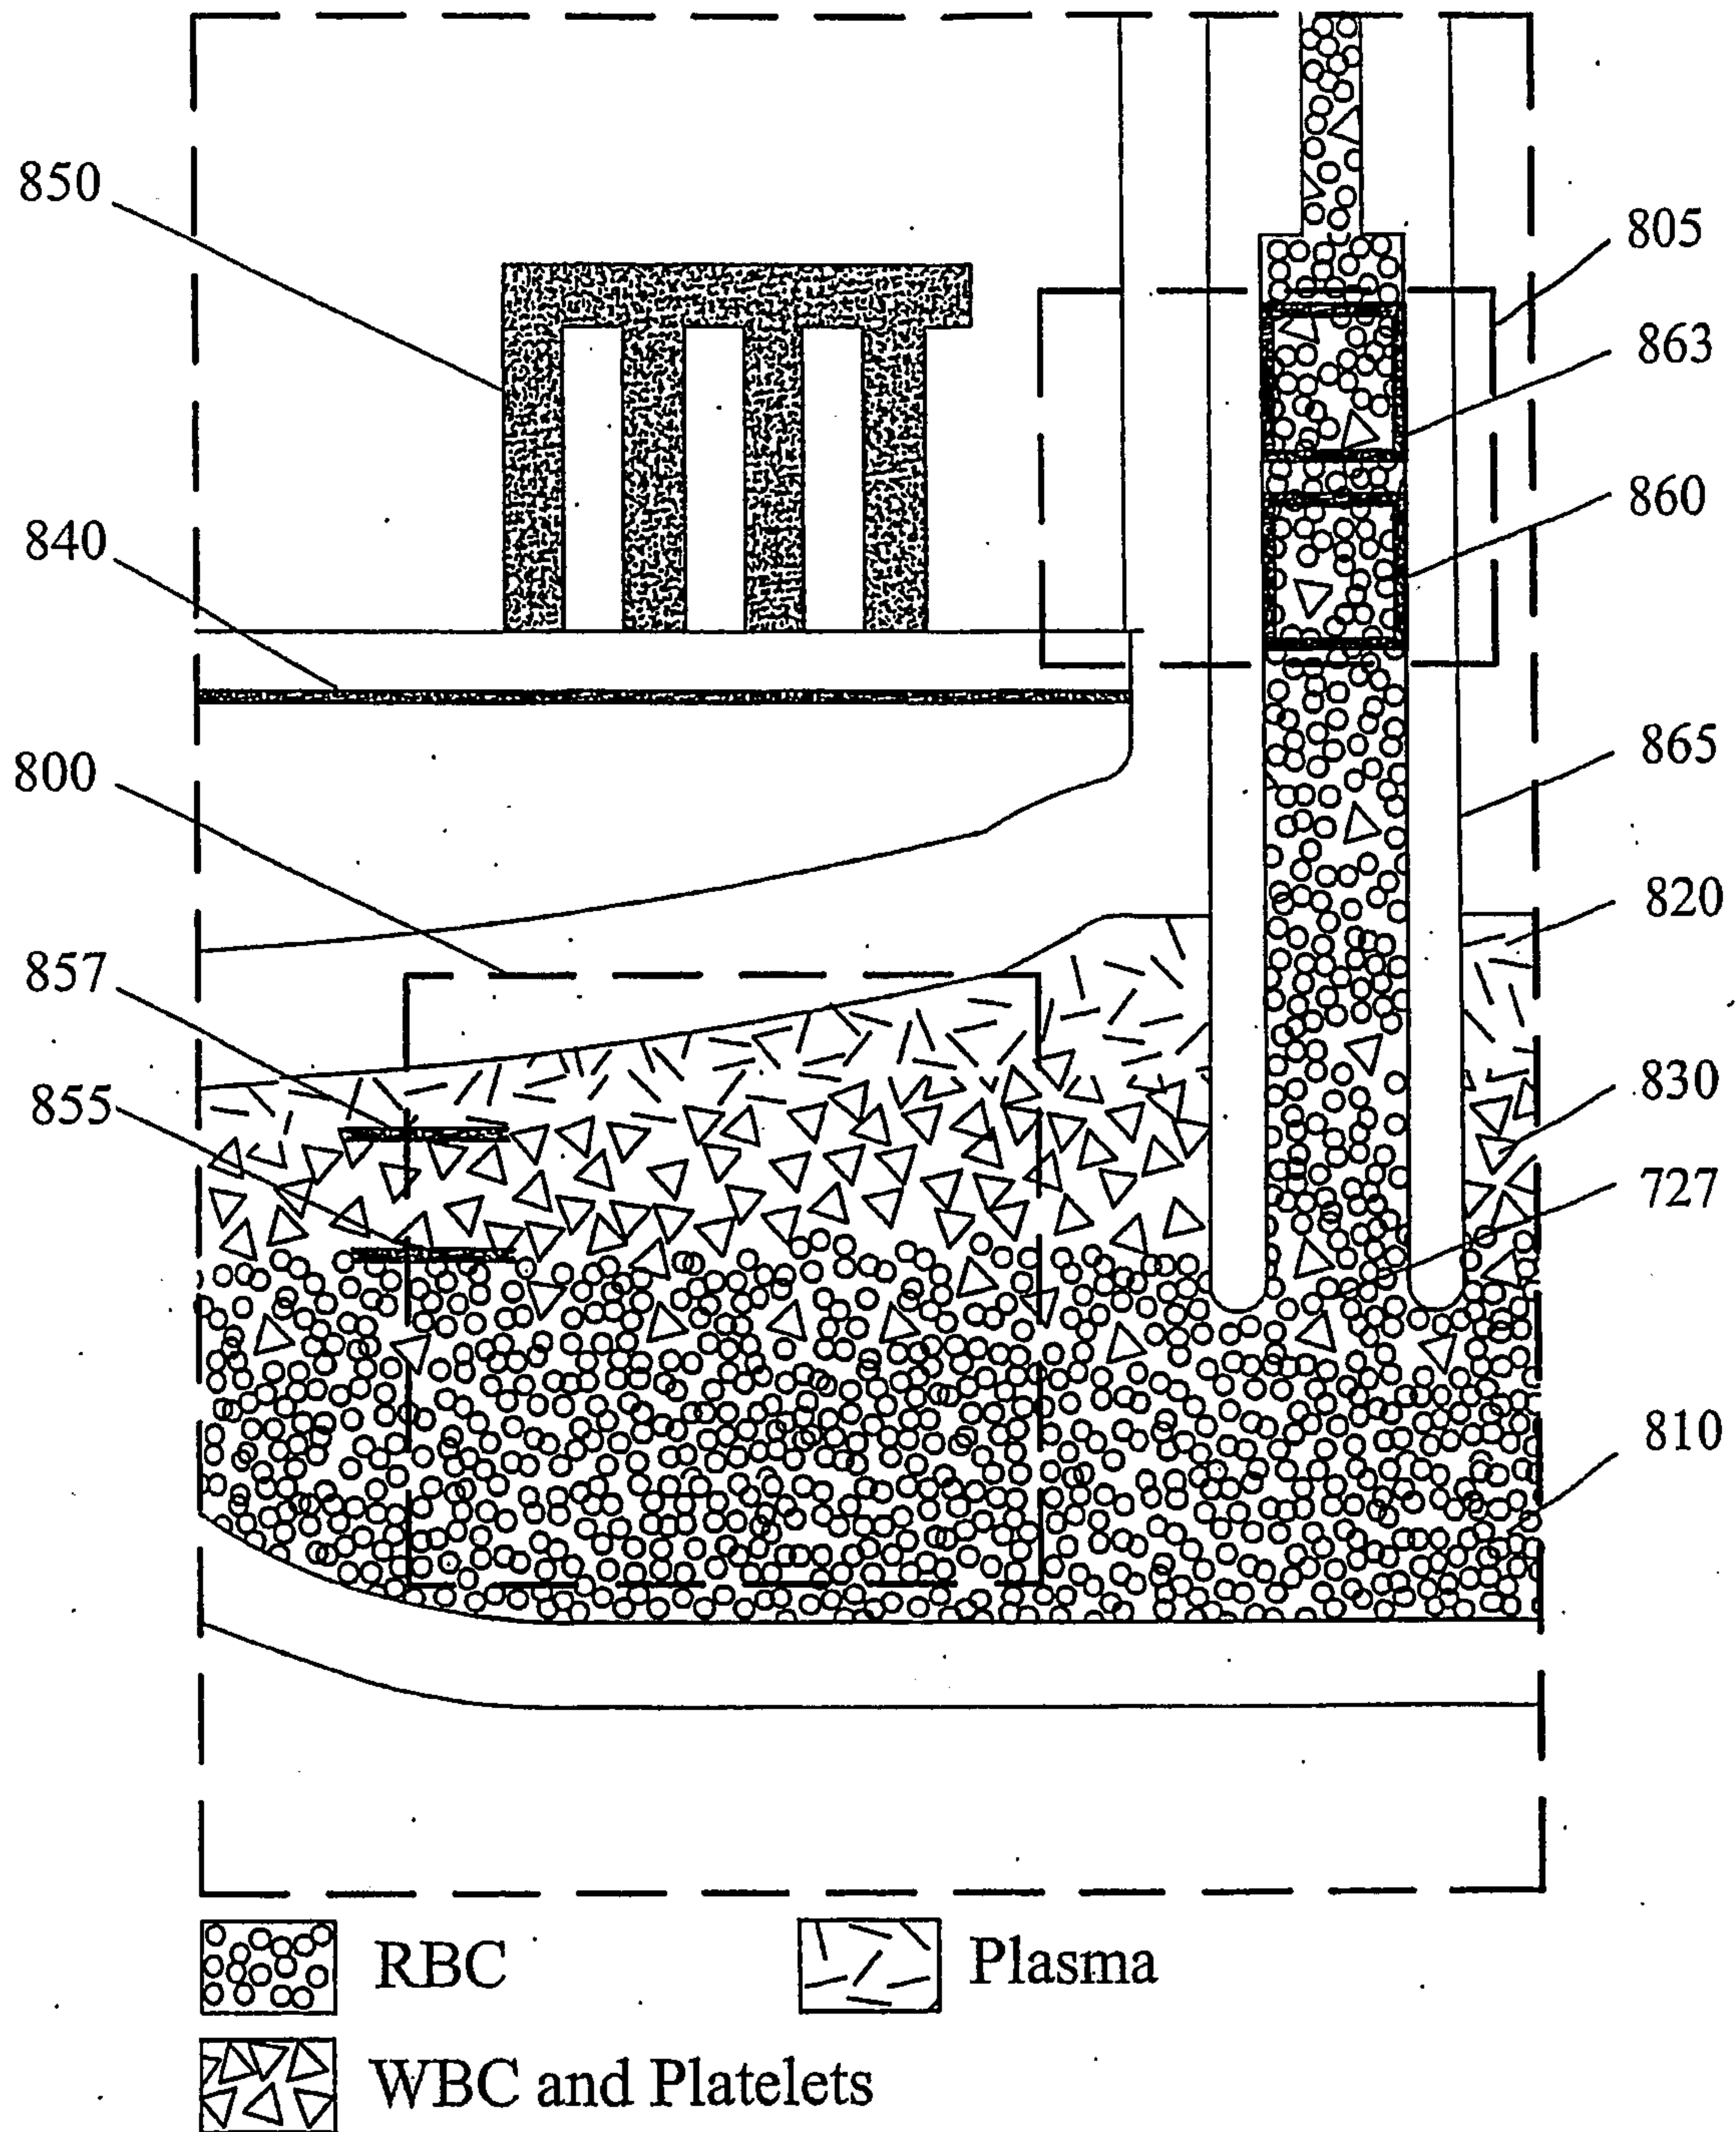


Figure 7

Relative Intensity at Extraction Port

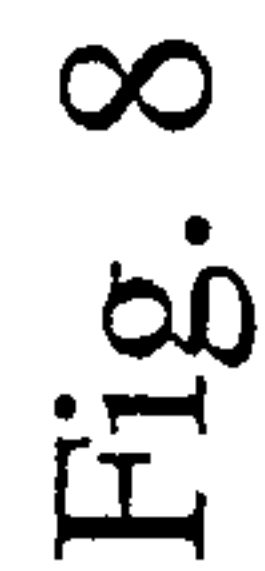

Fi. 8

Example Filtered Data from a Human Blood Experiment
(50 point moving averages)

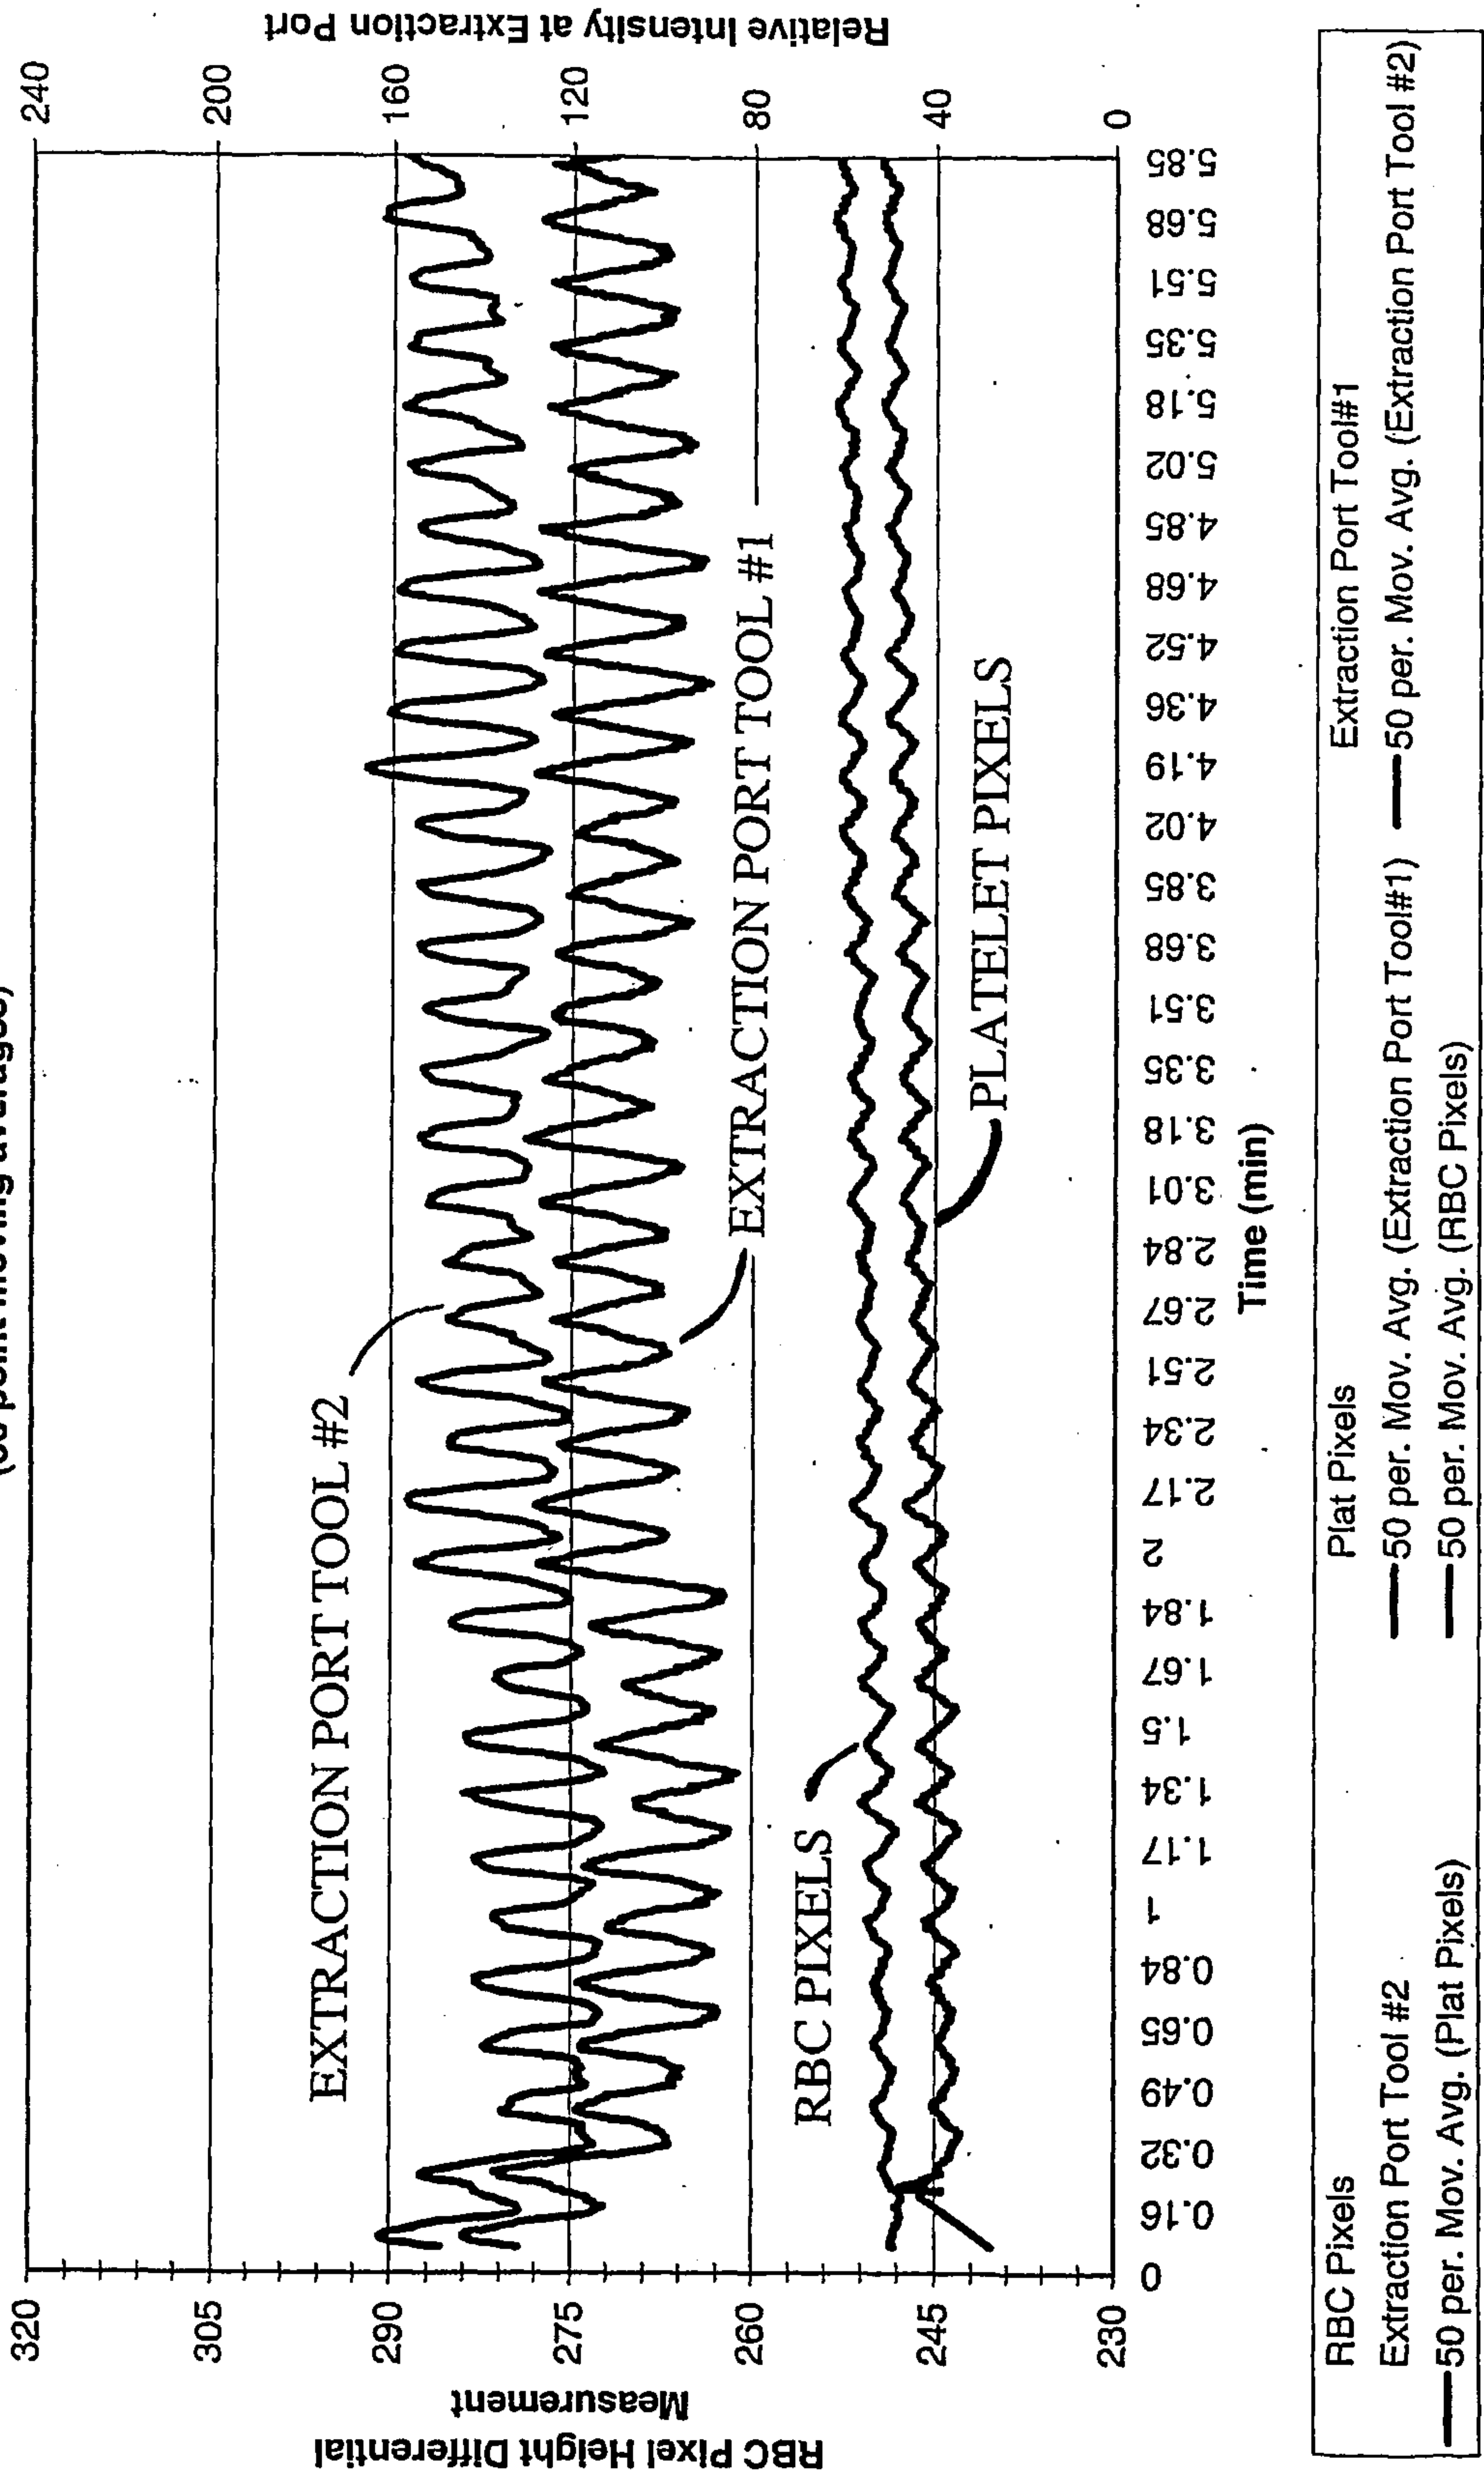


Fig. 8A

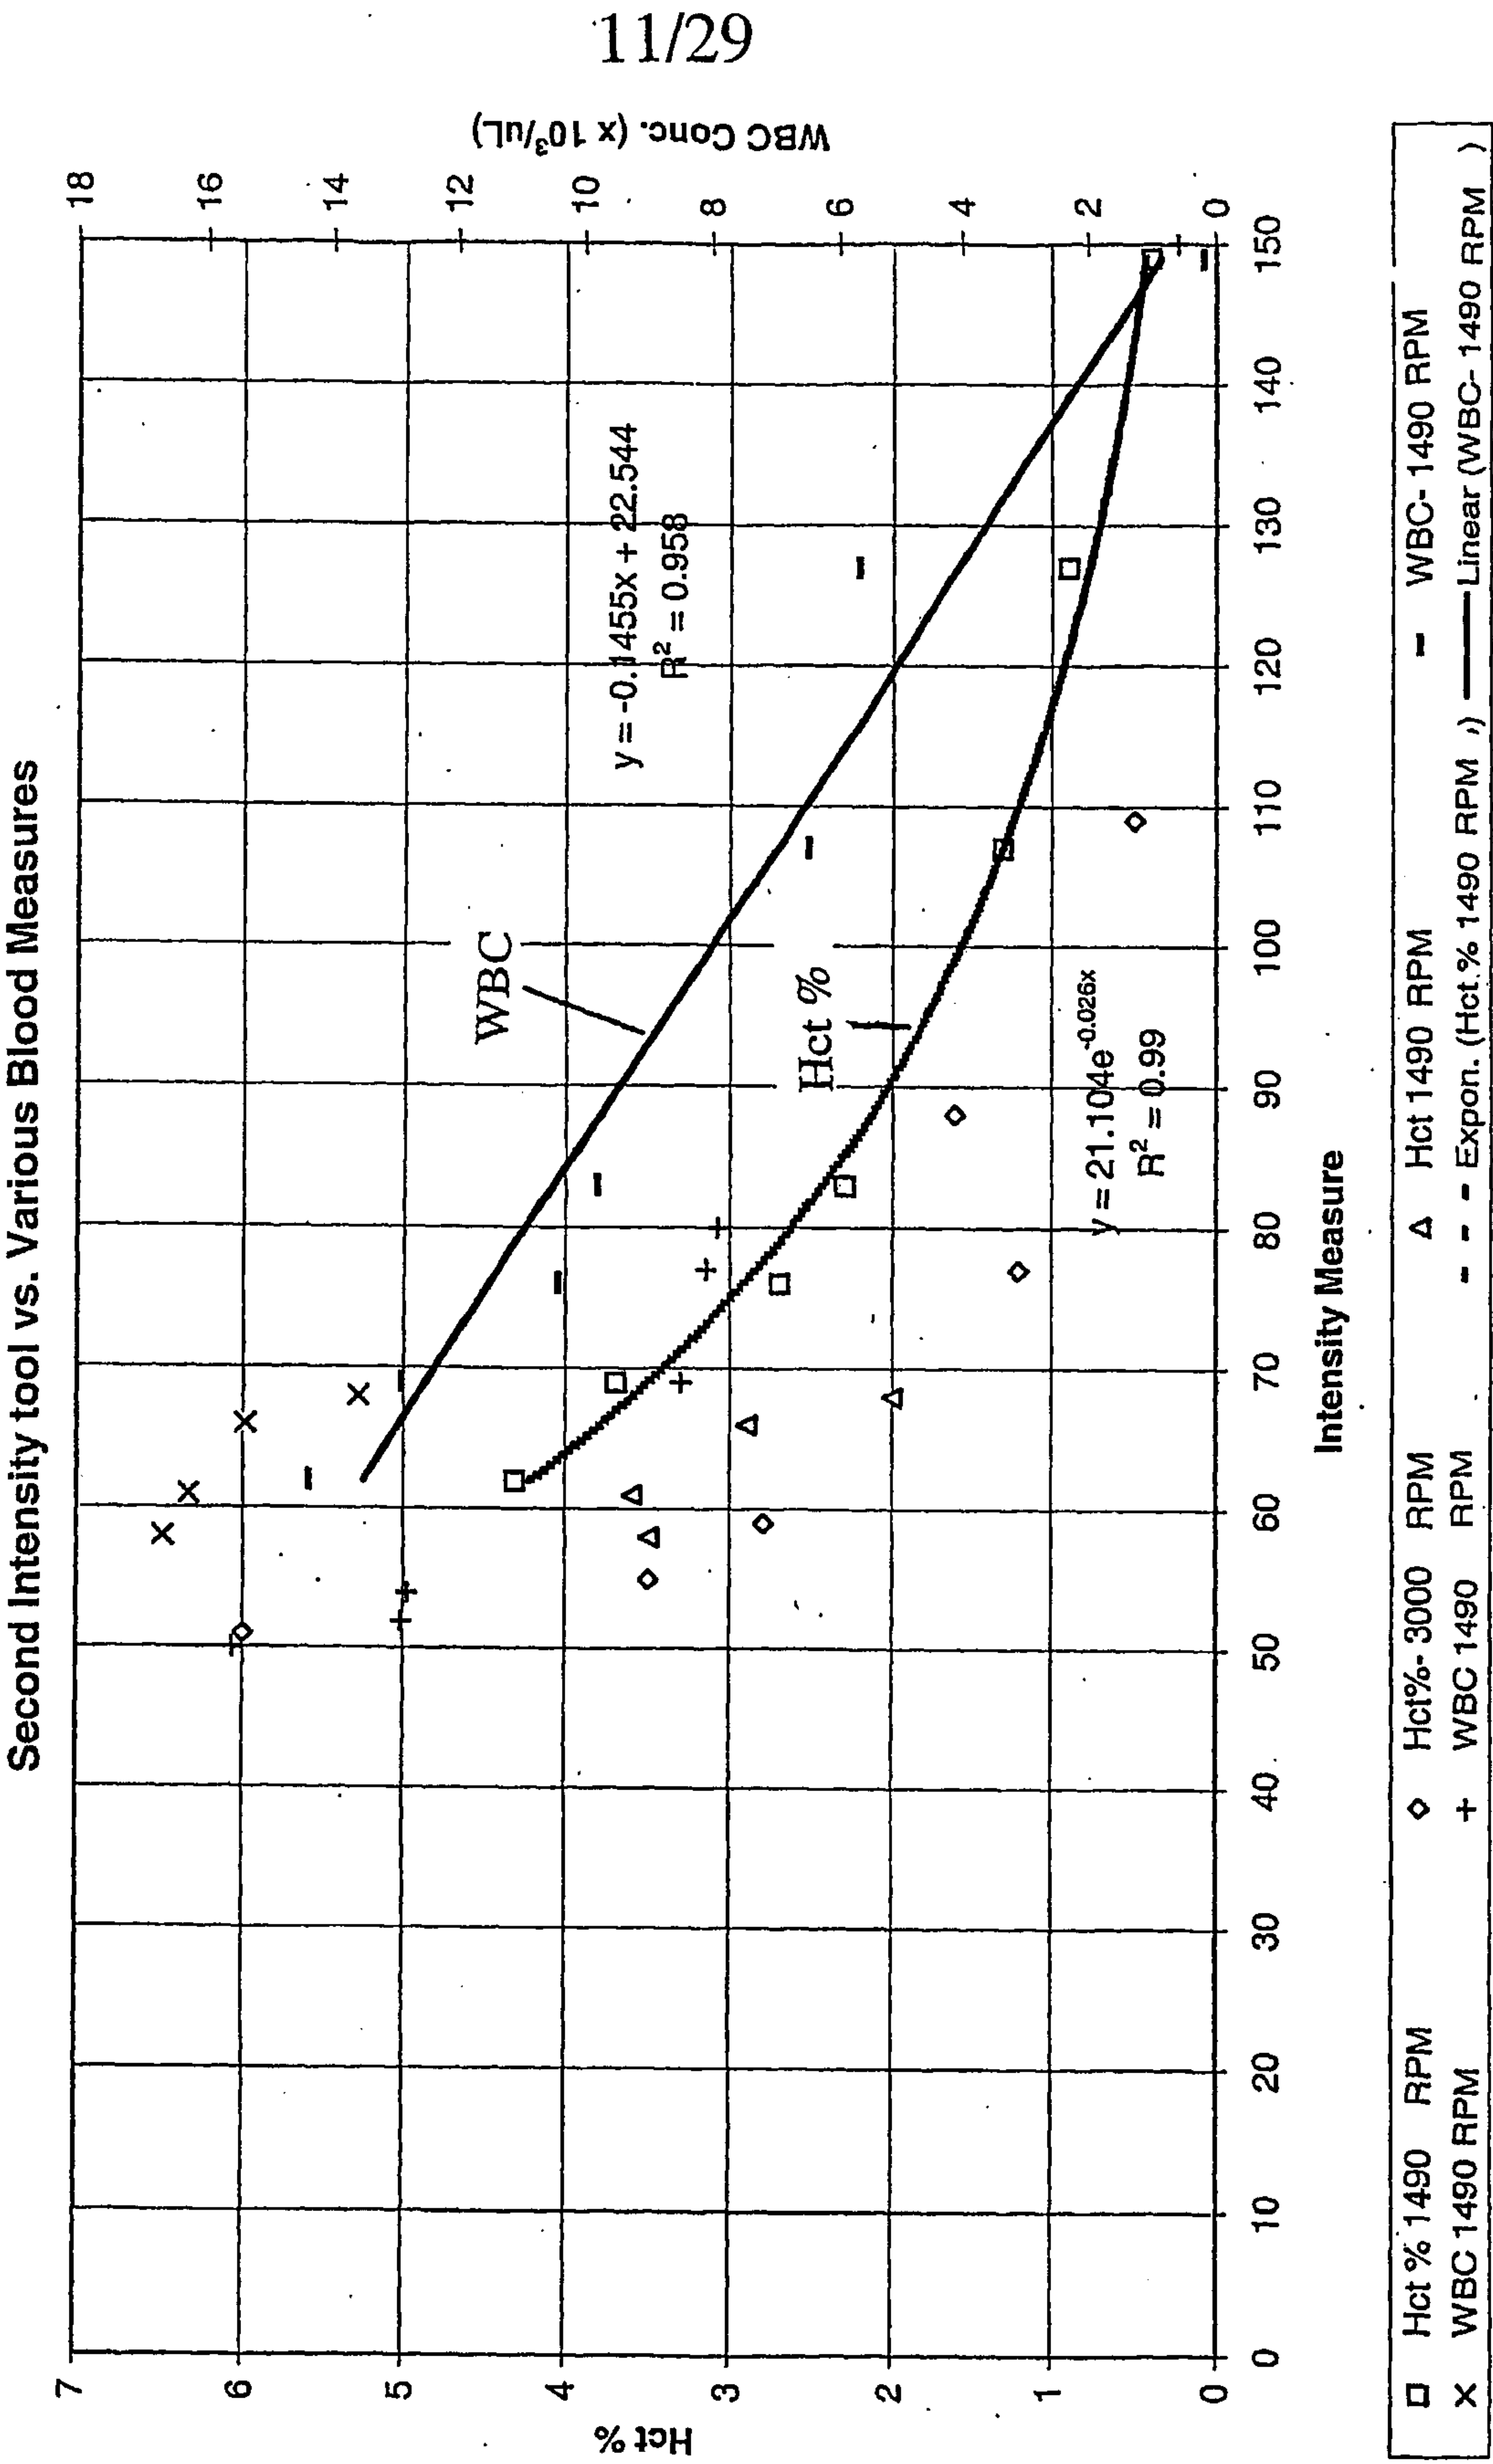


Fig. 9

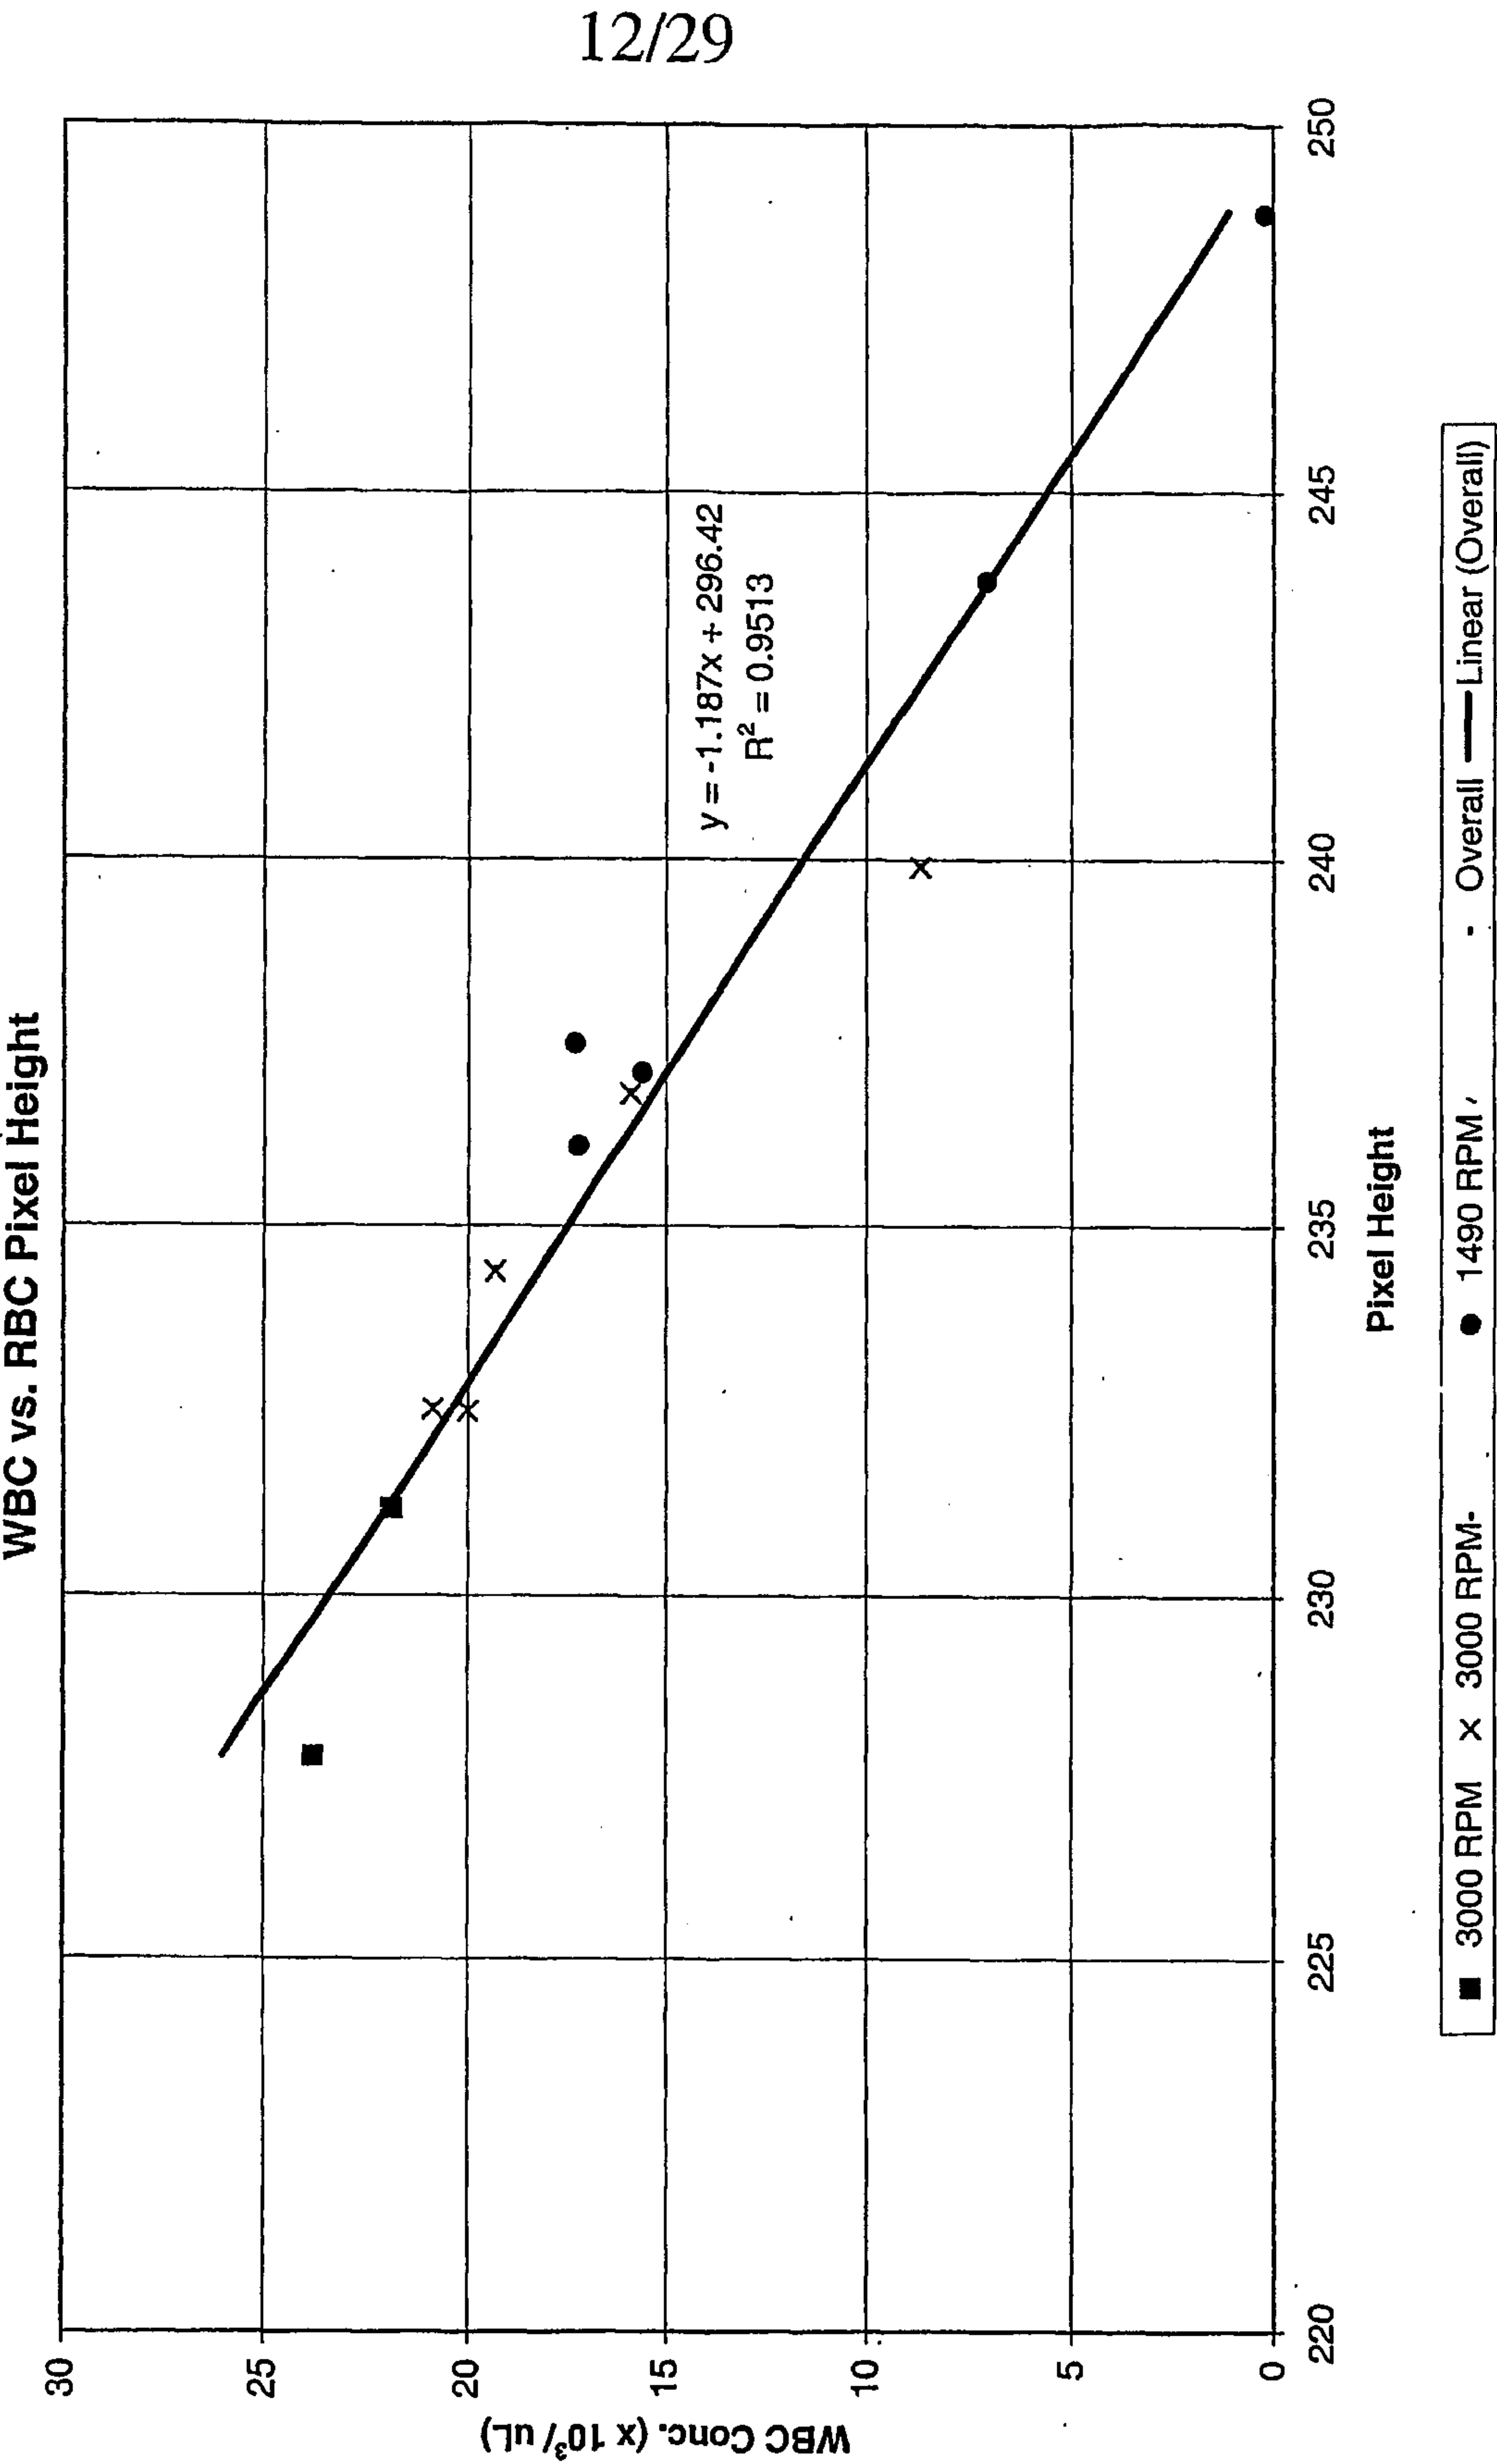


Fig. 10

REPLACEMENT SHEET

13 / 29

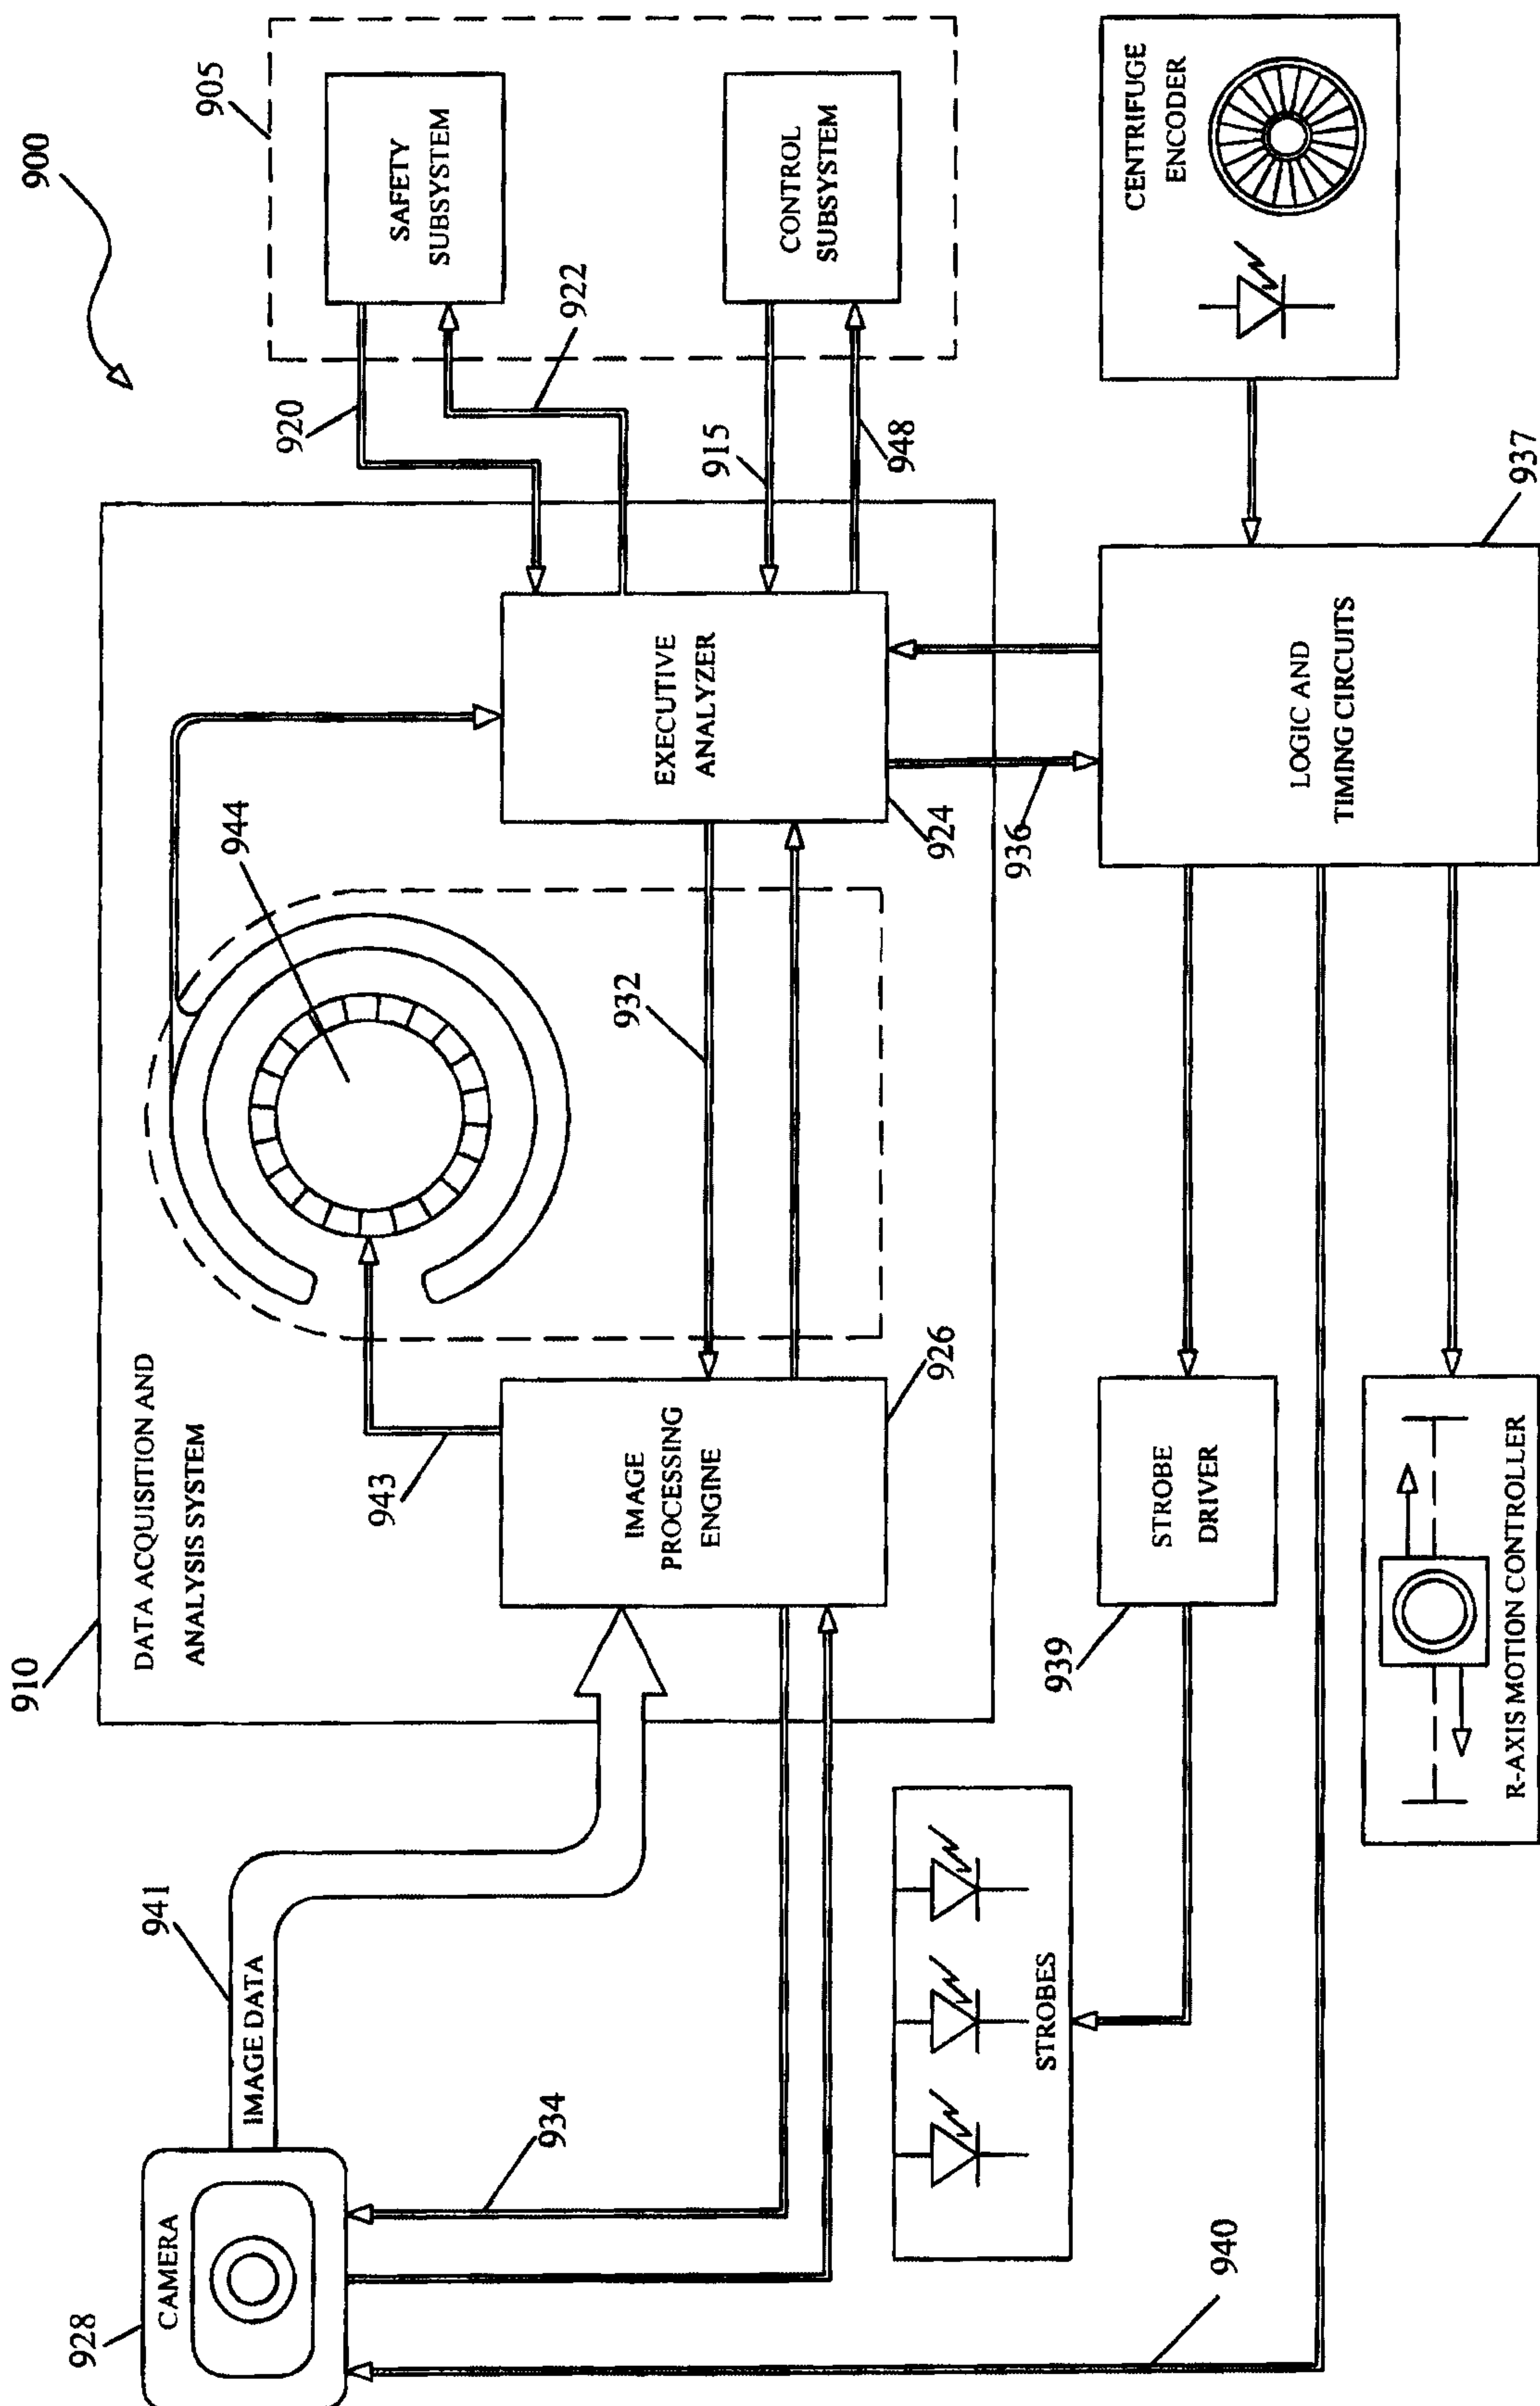


Figure 11

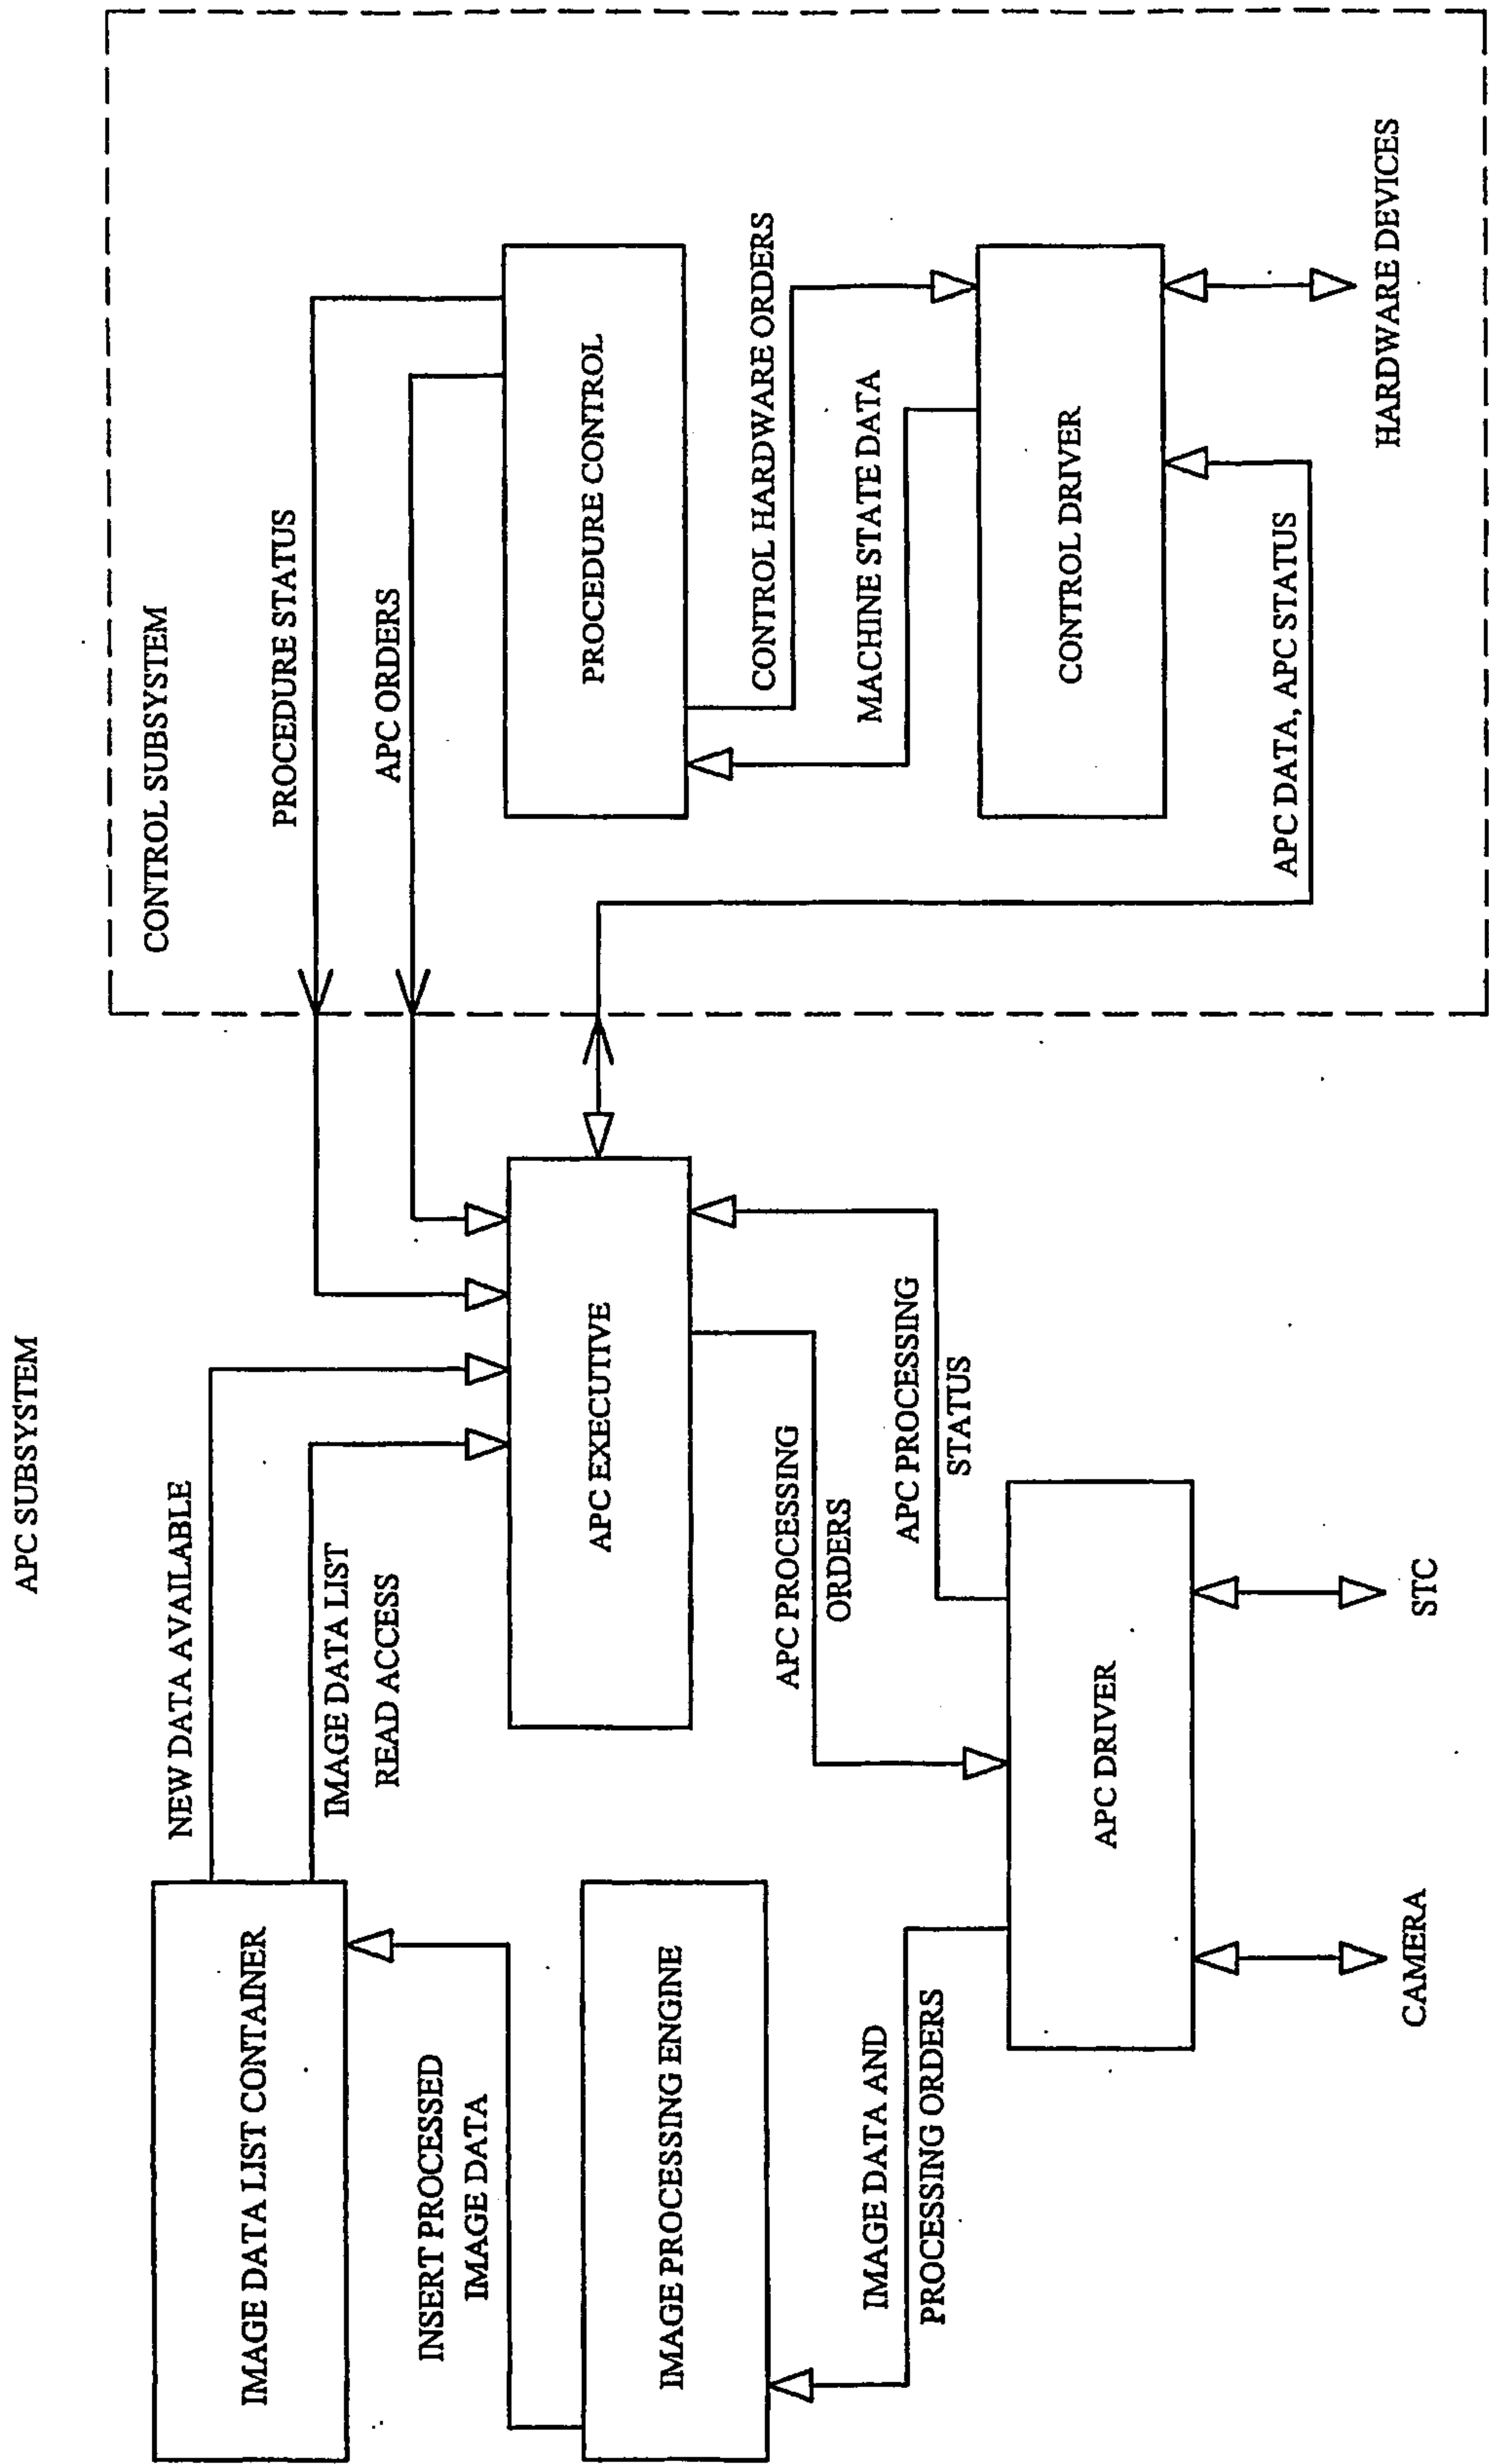


Figure 12

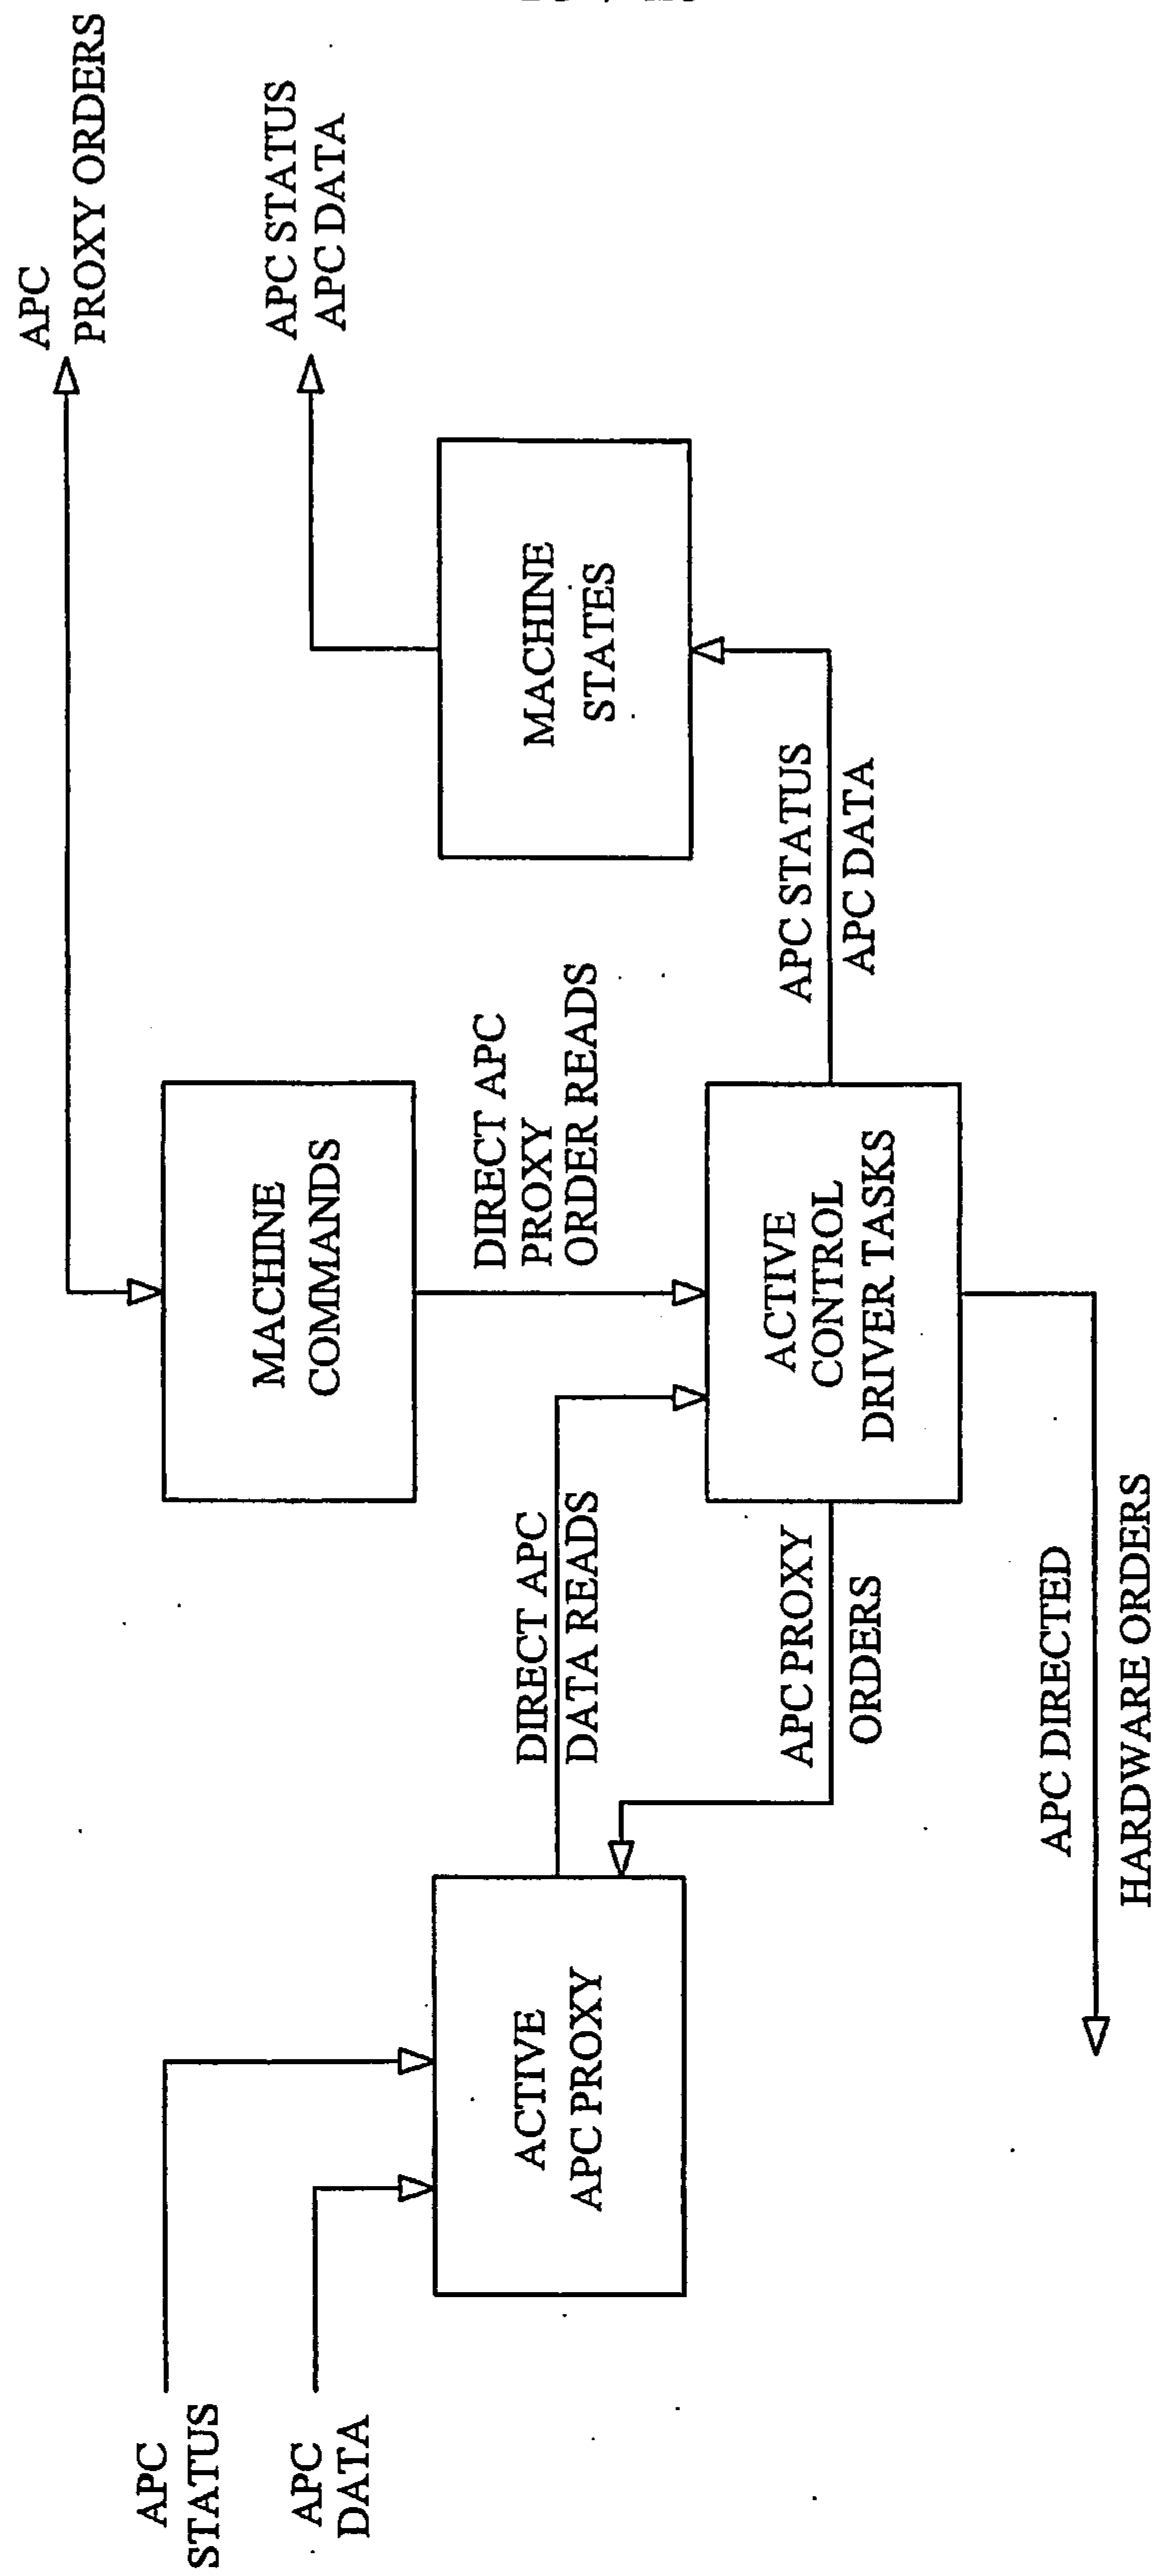


Figure 13

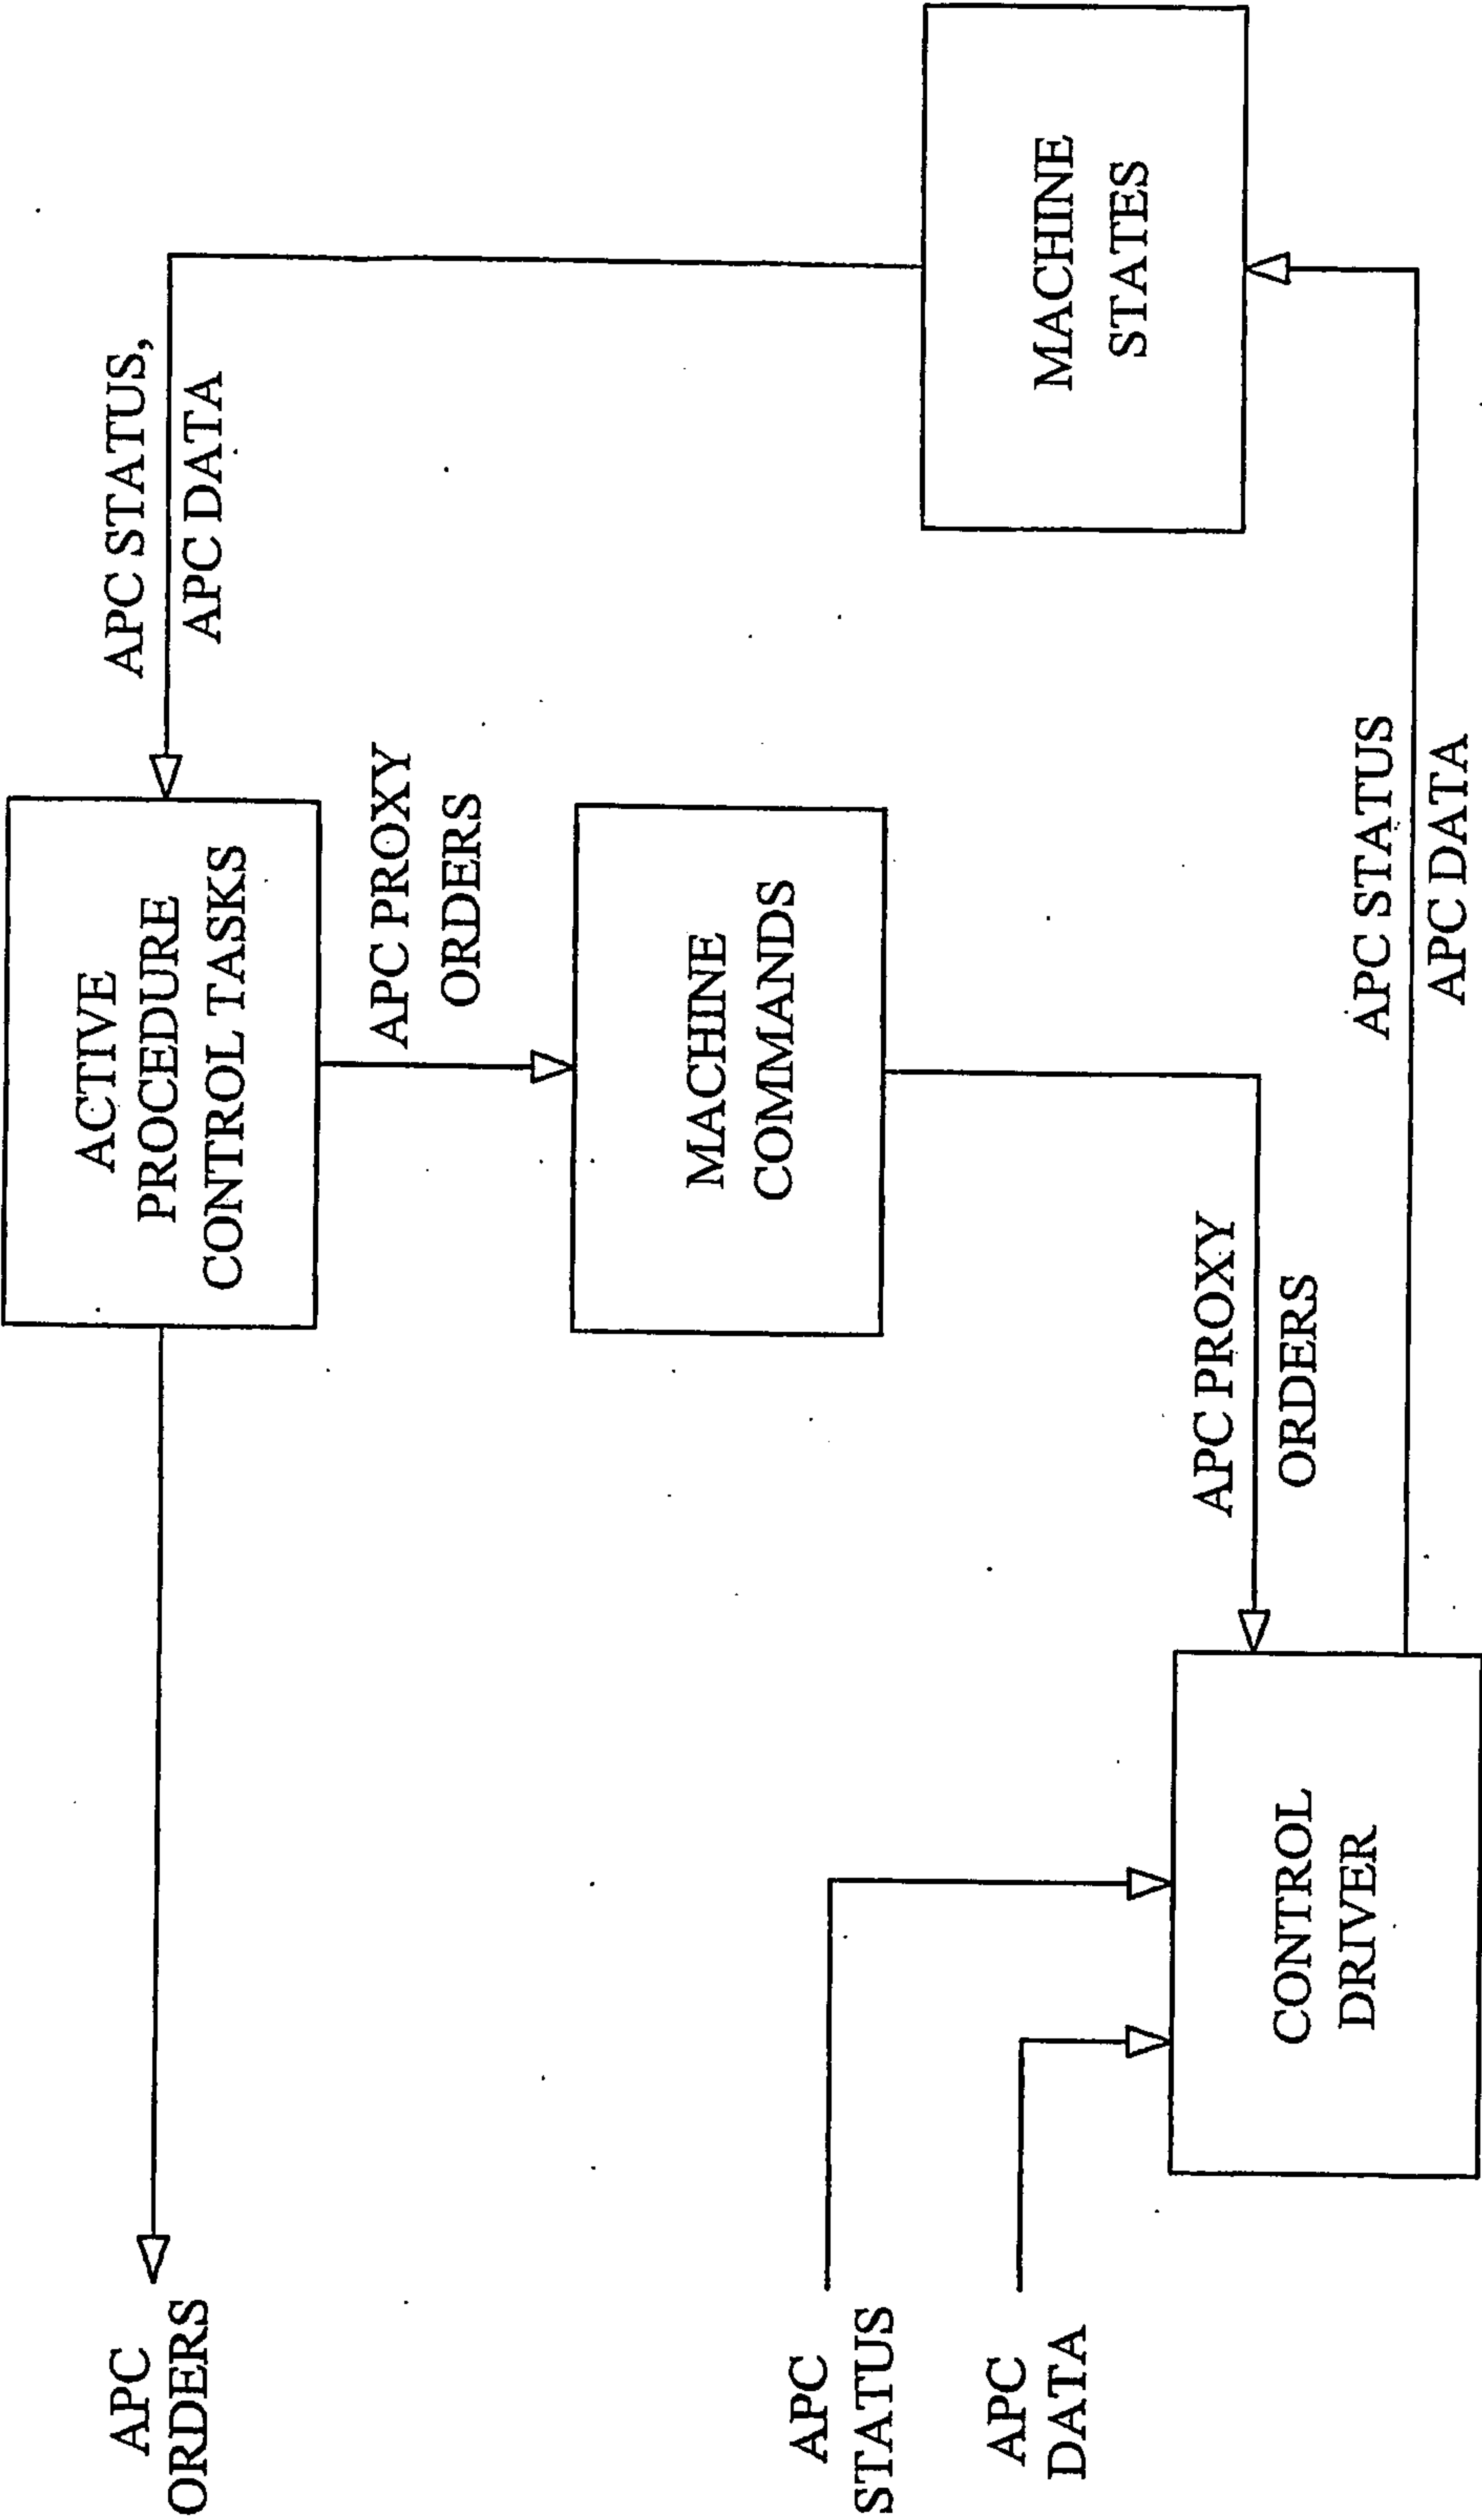


Figure 14

17 / 29

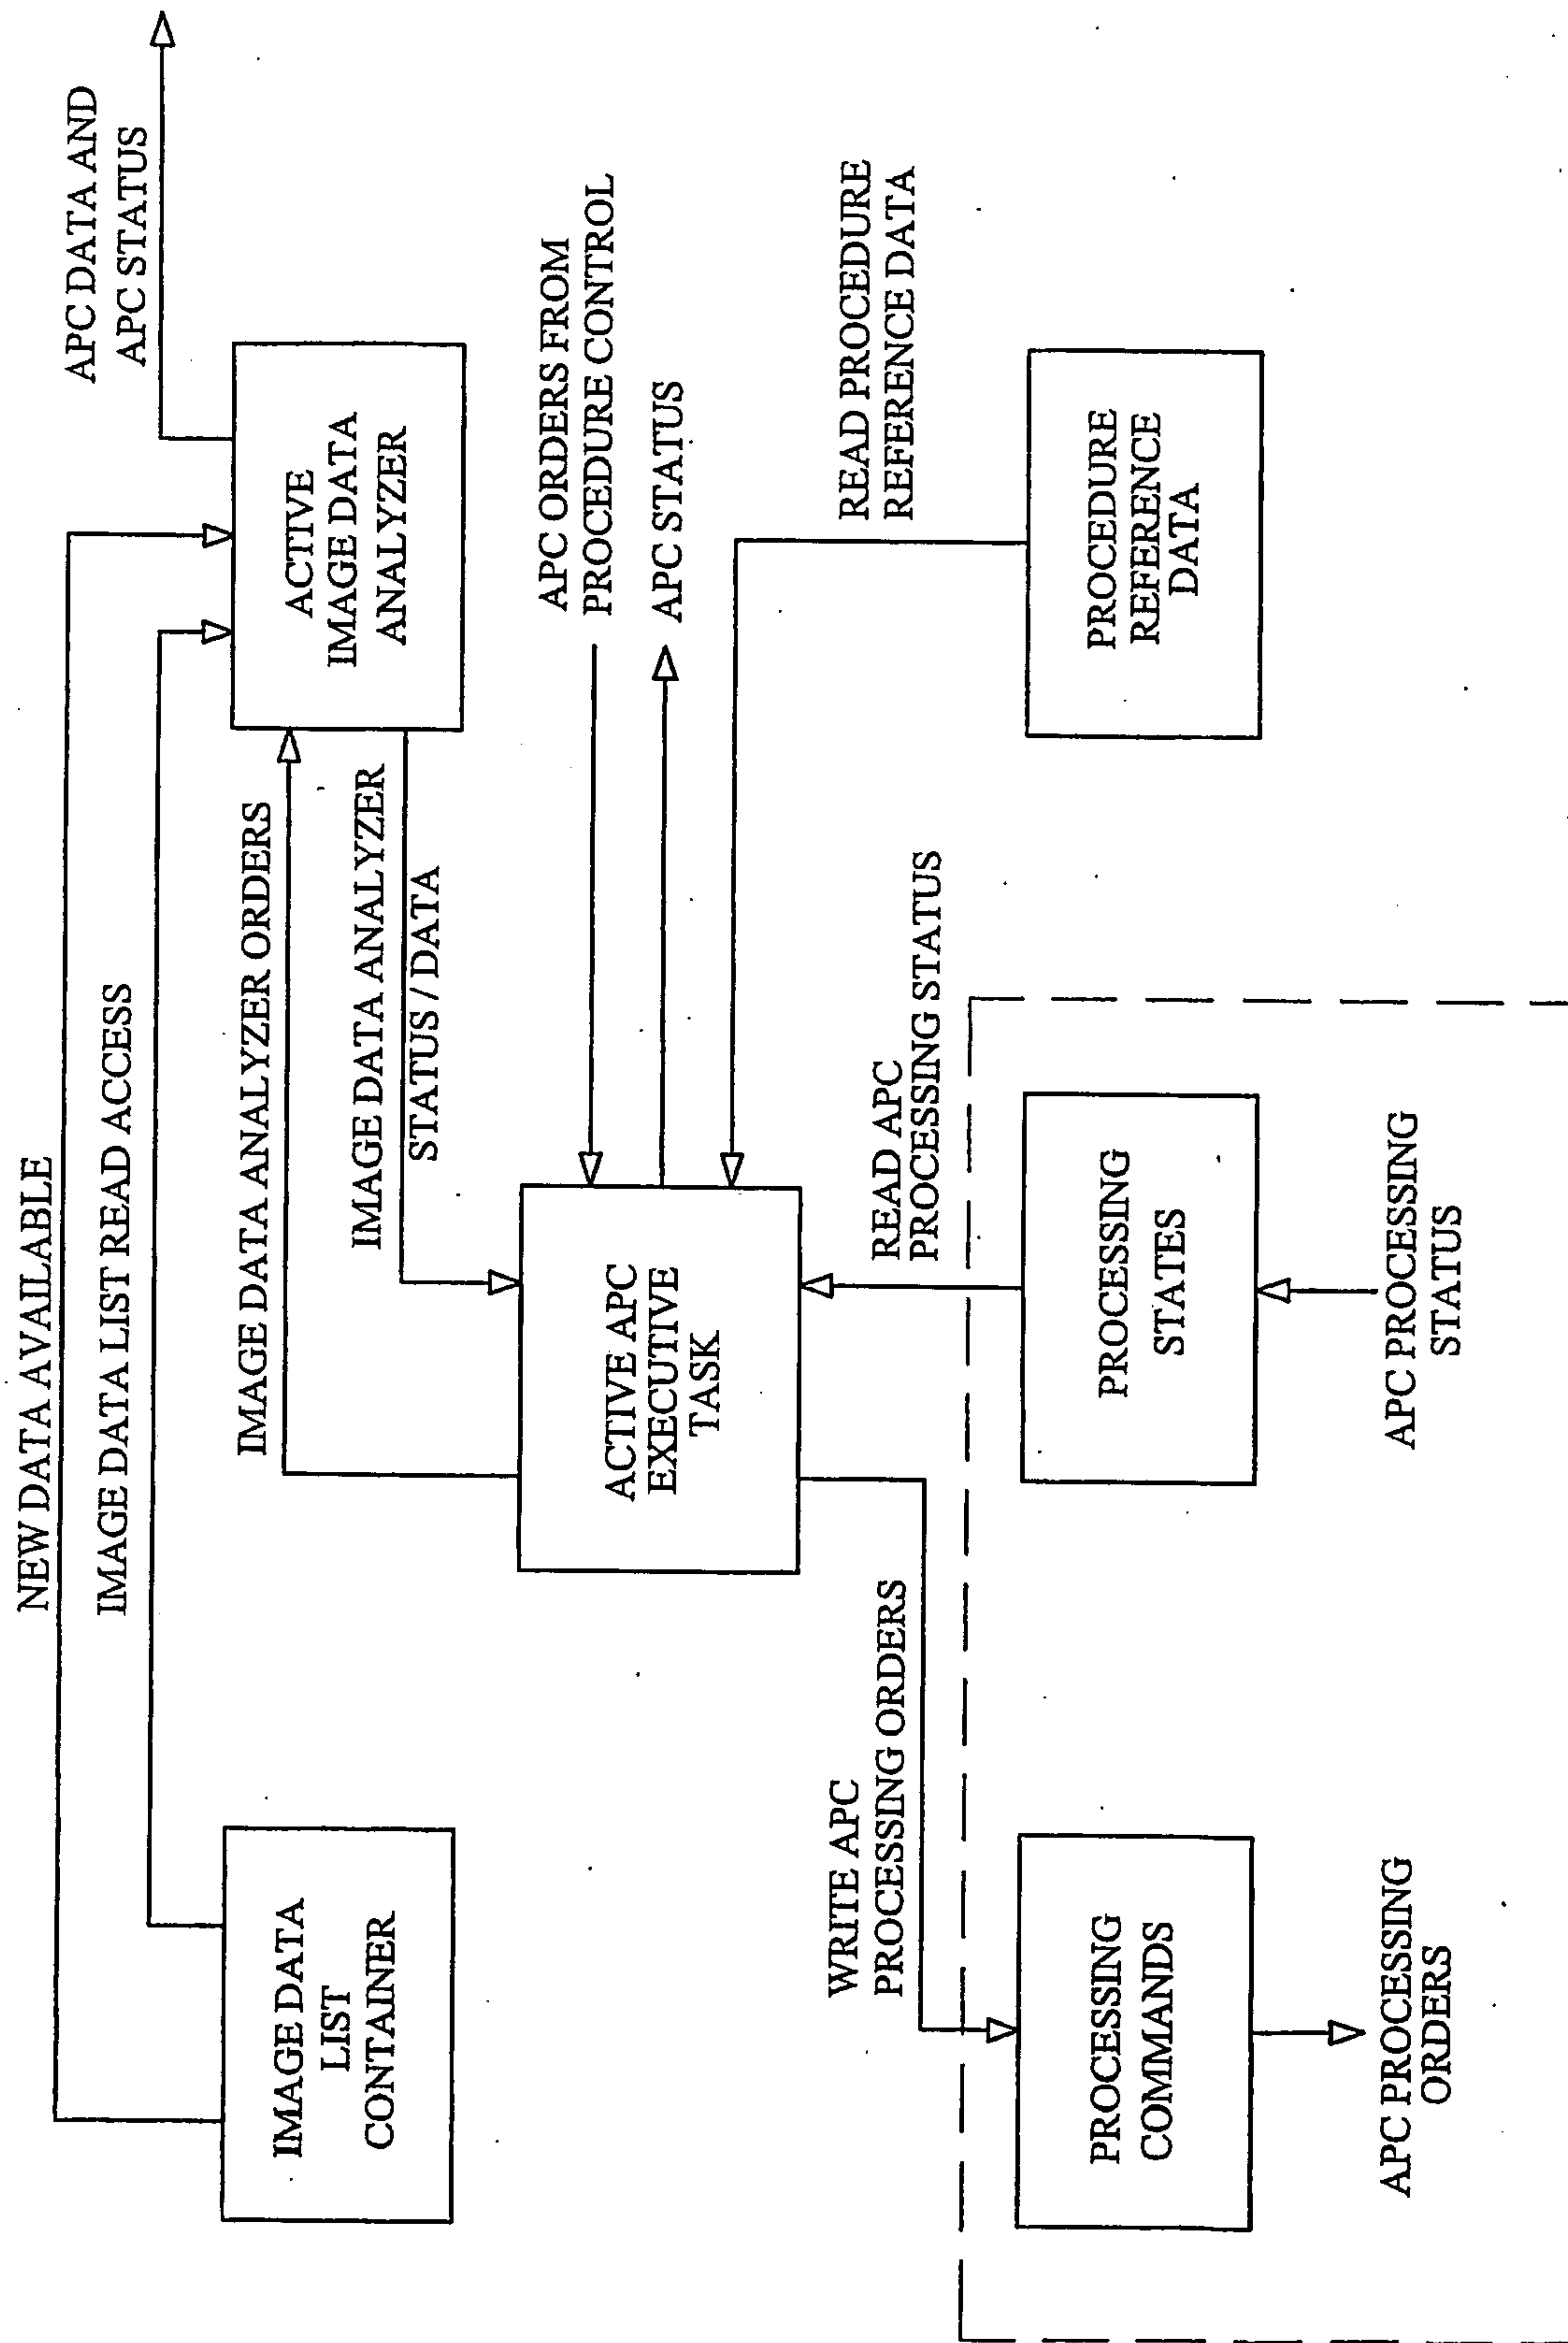


Figure 15

18 / 29

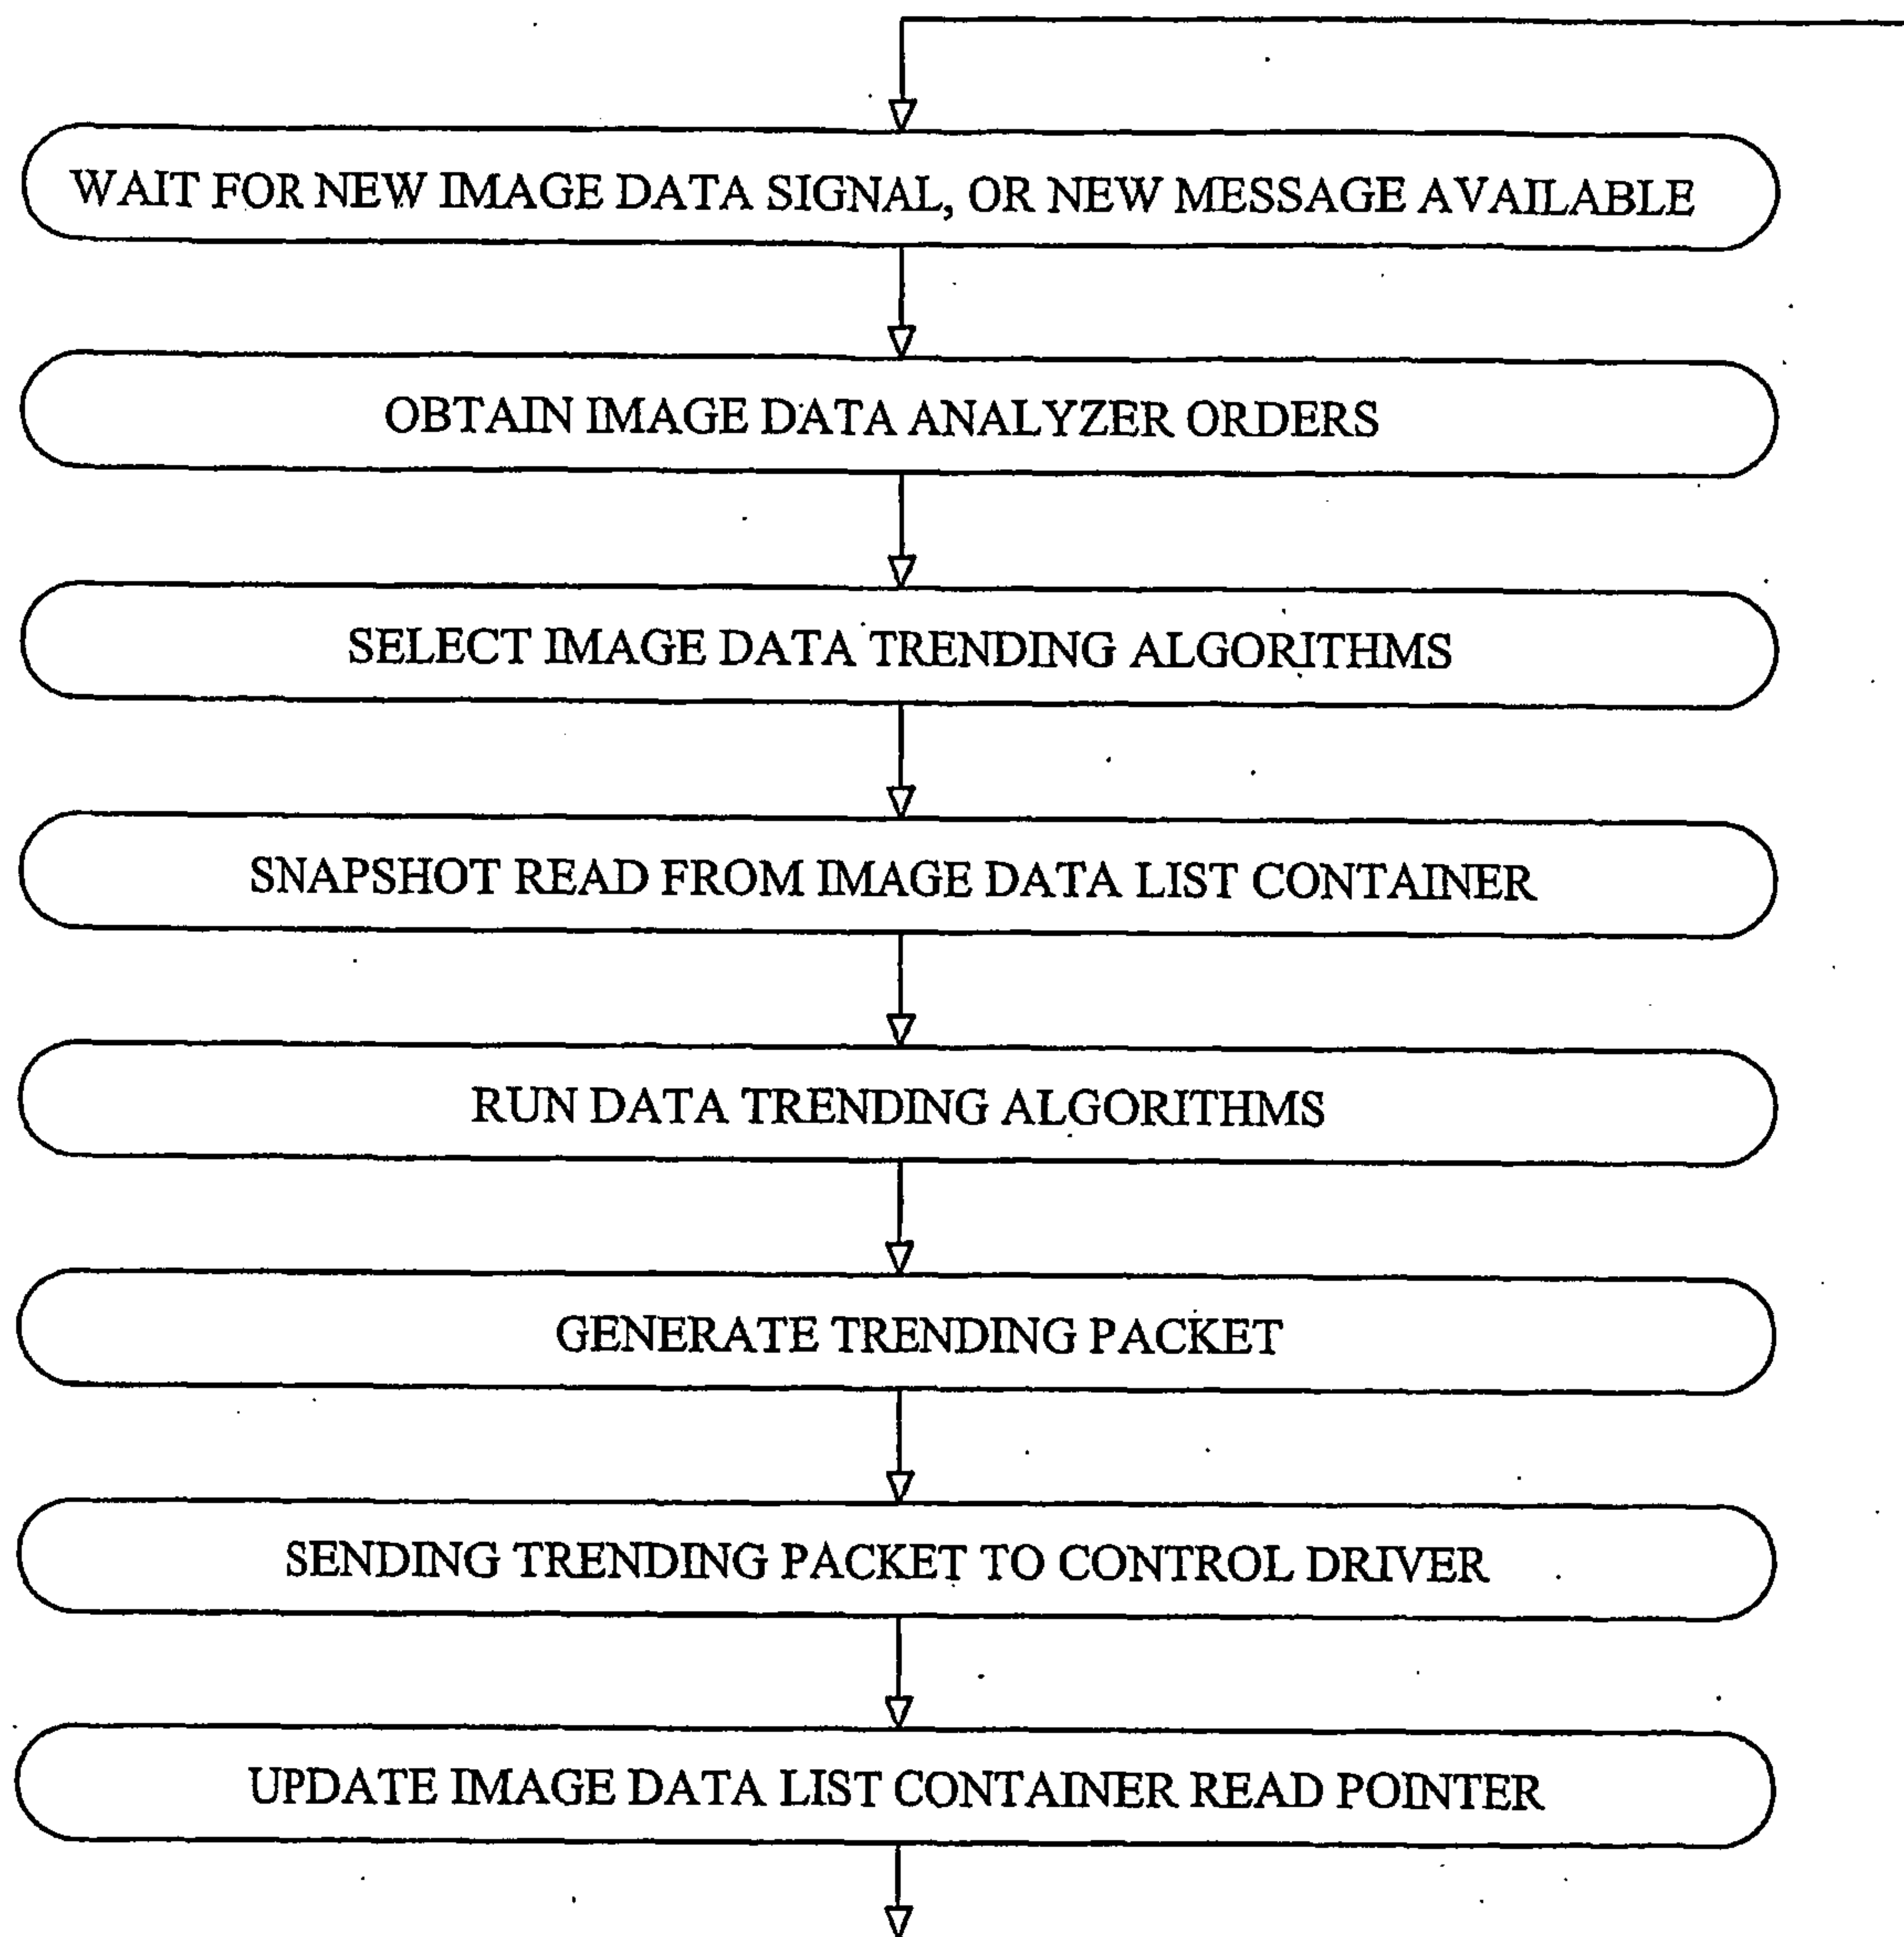


Figure 16

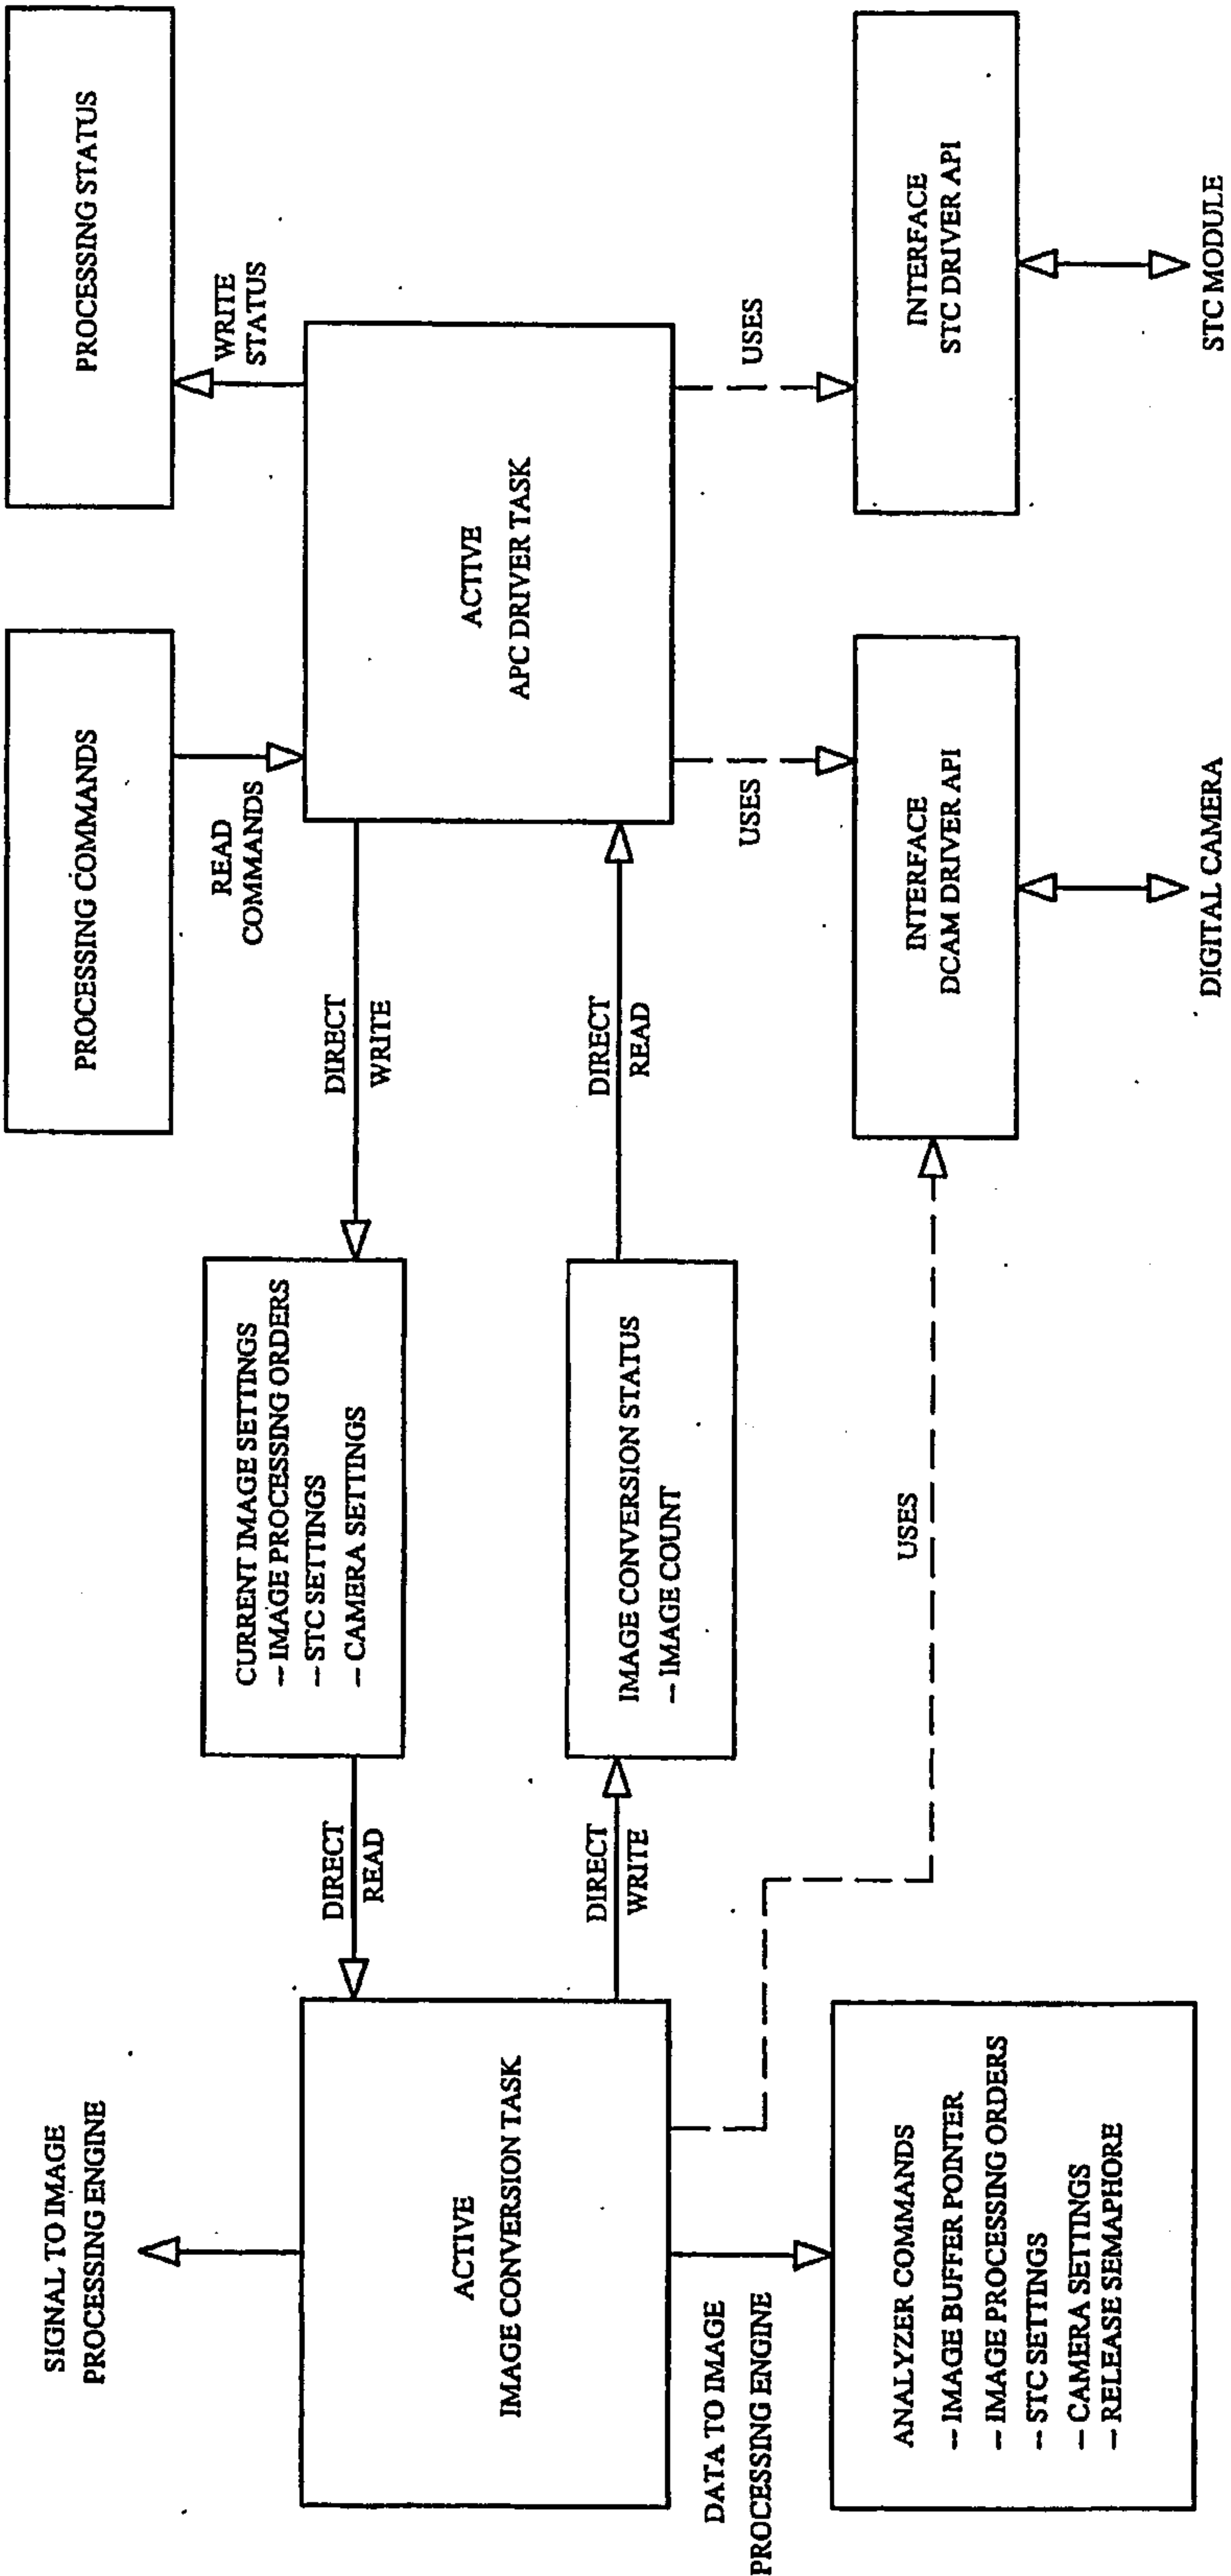


Figure 17

20 / 29

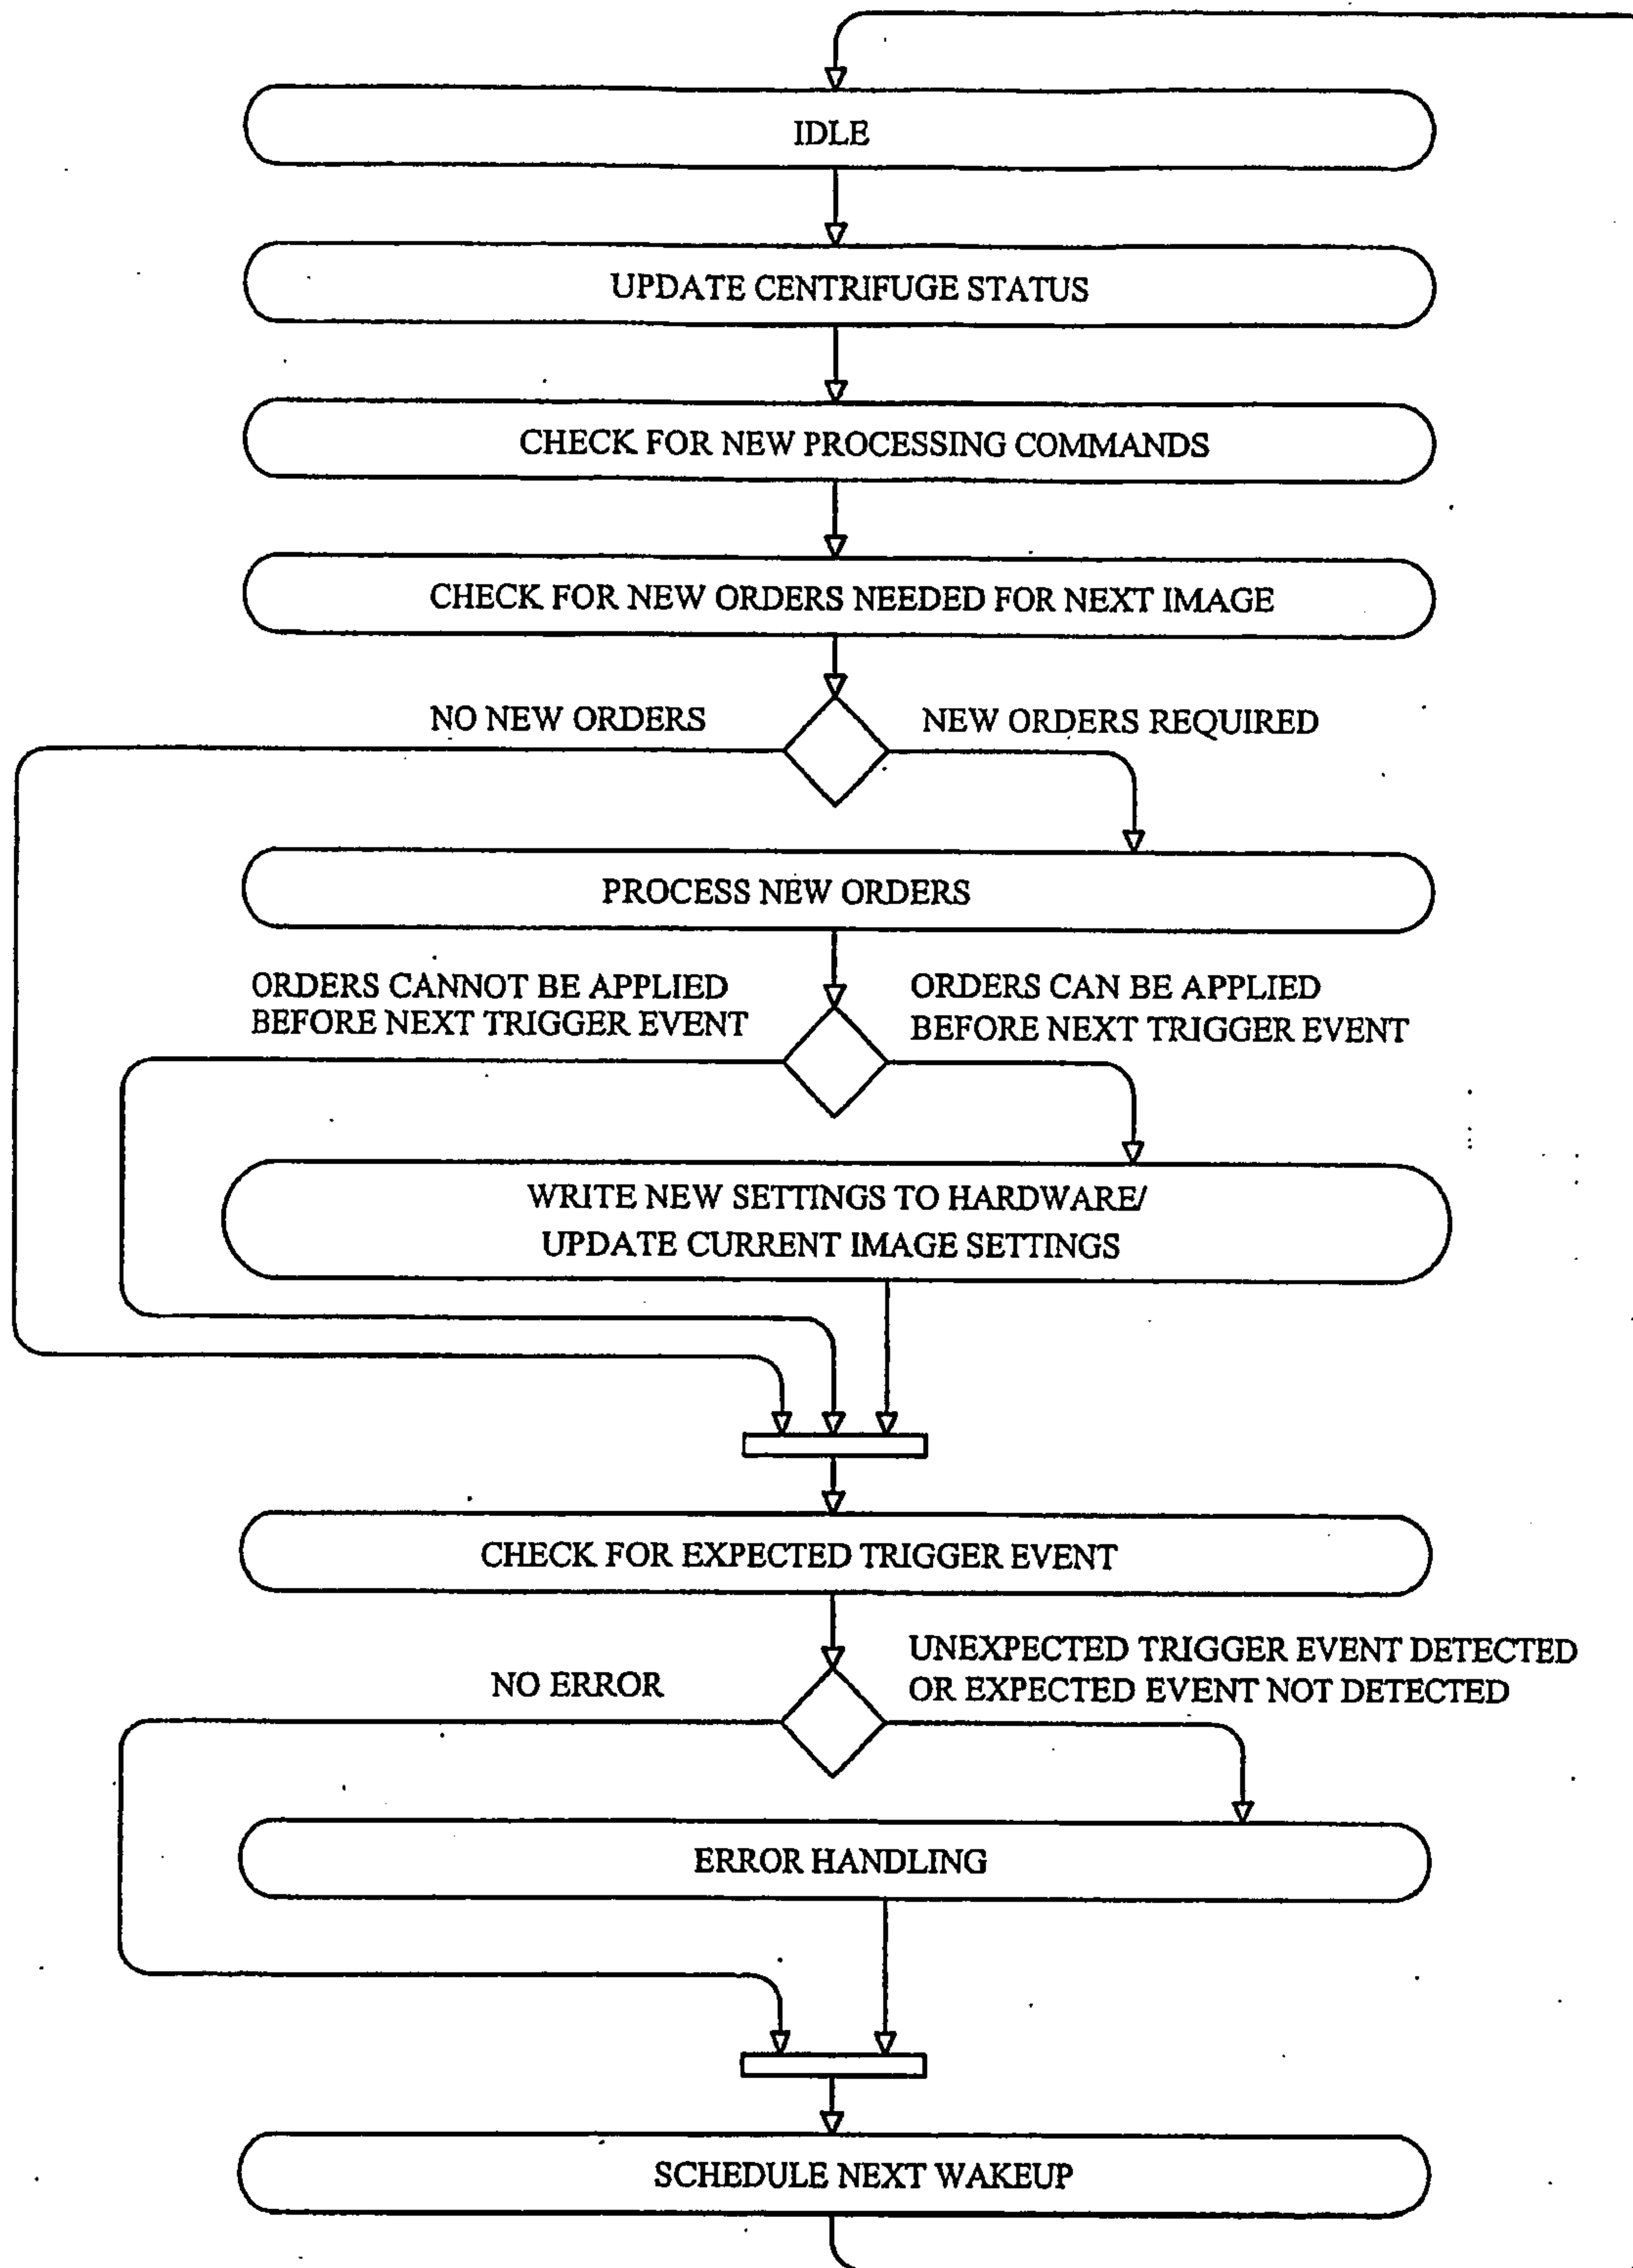


Figure 18

21 / 29

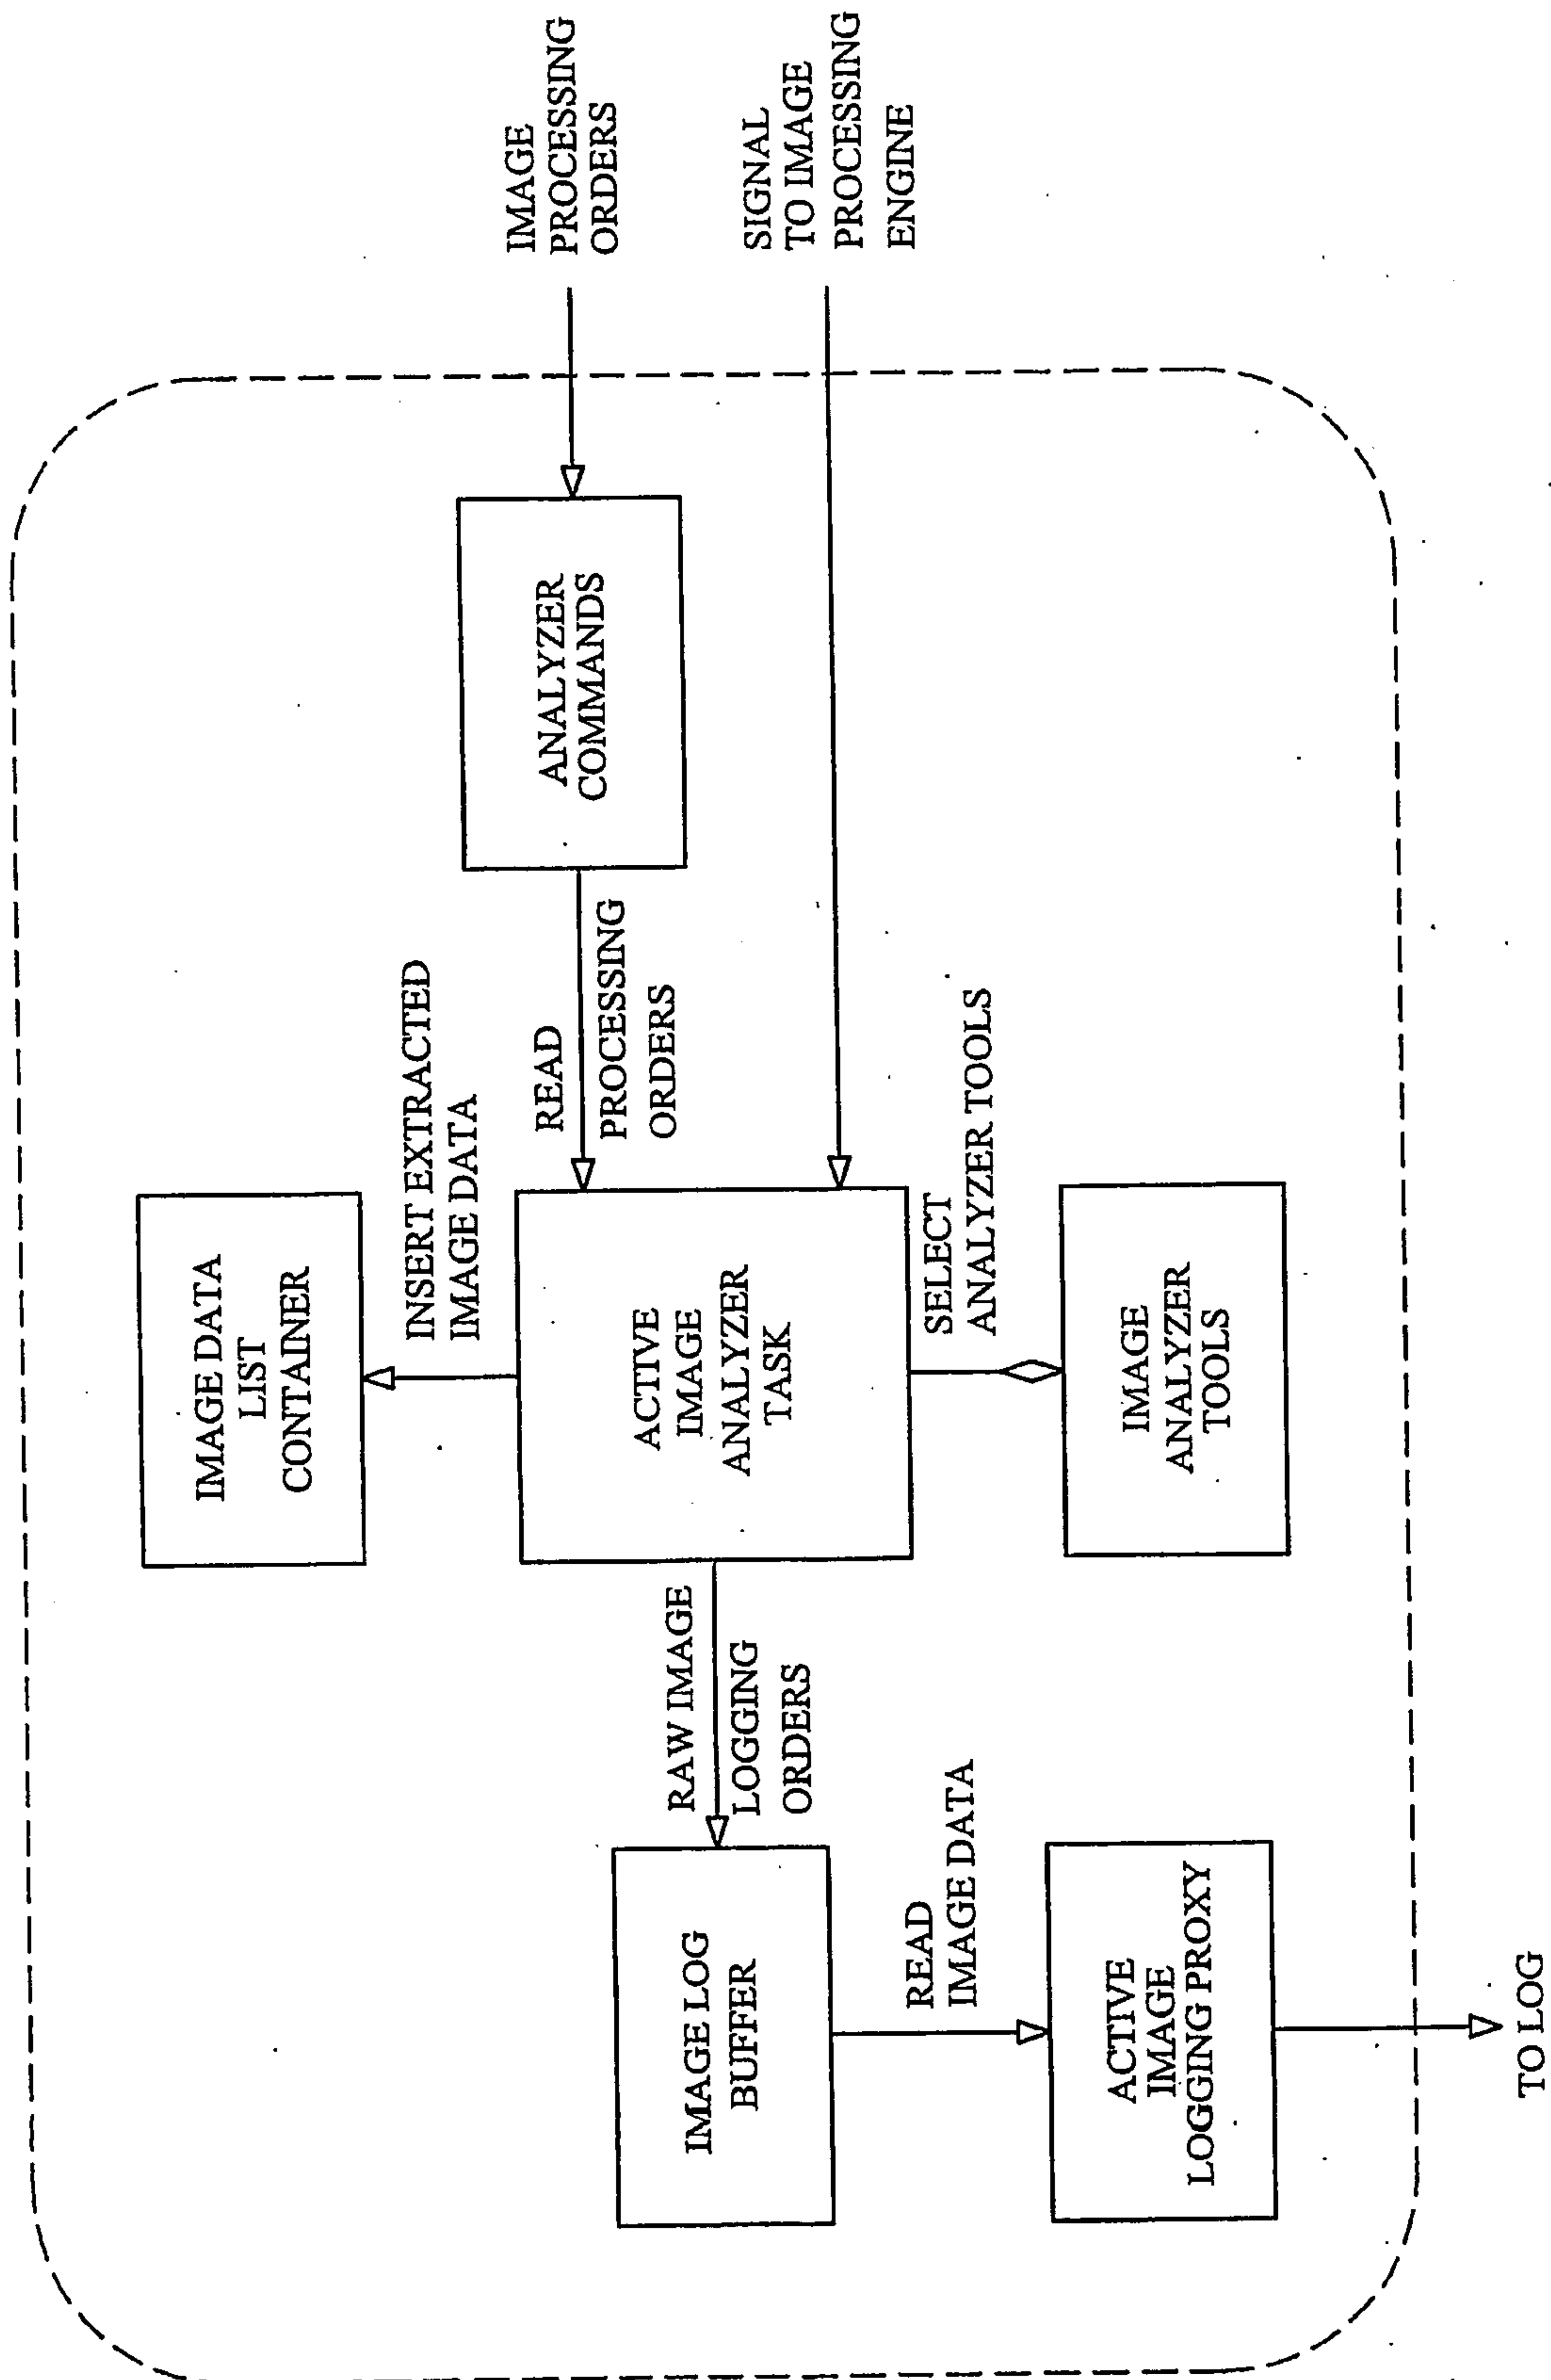


Figure 19

22 / 29

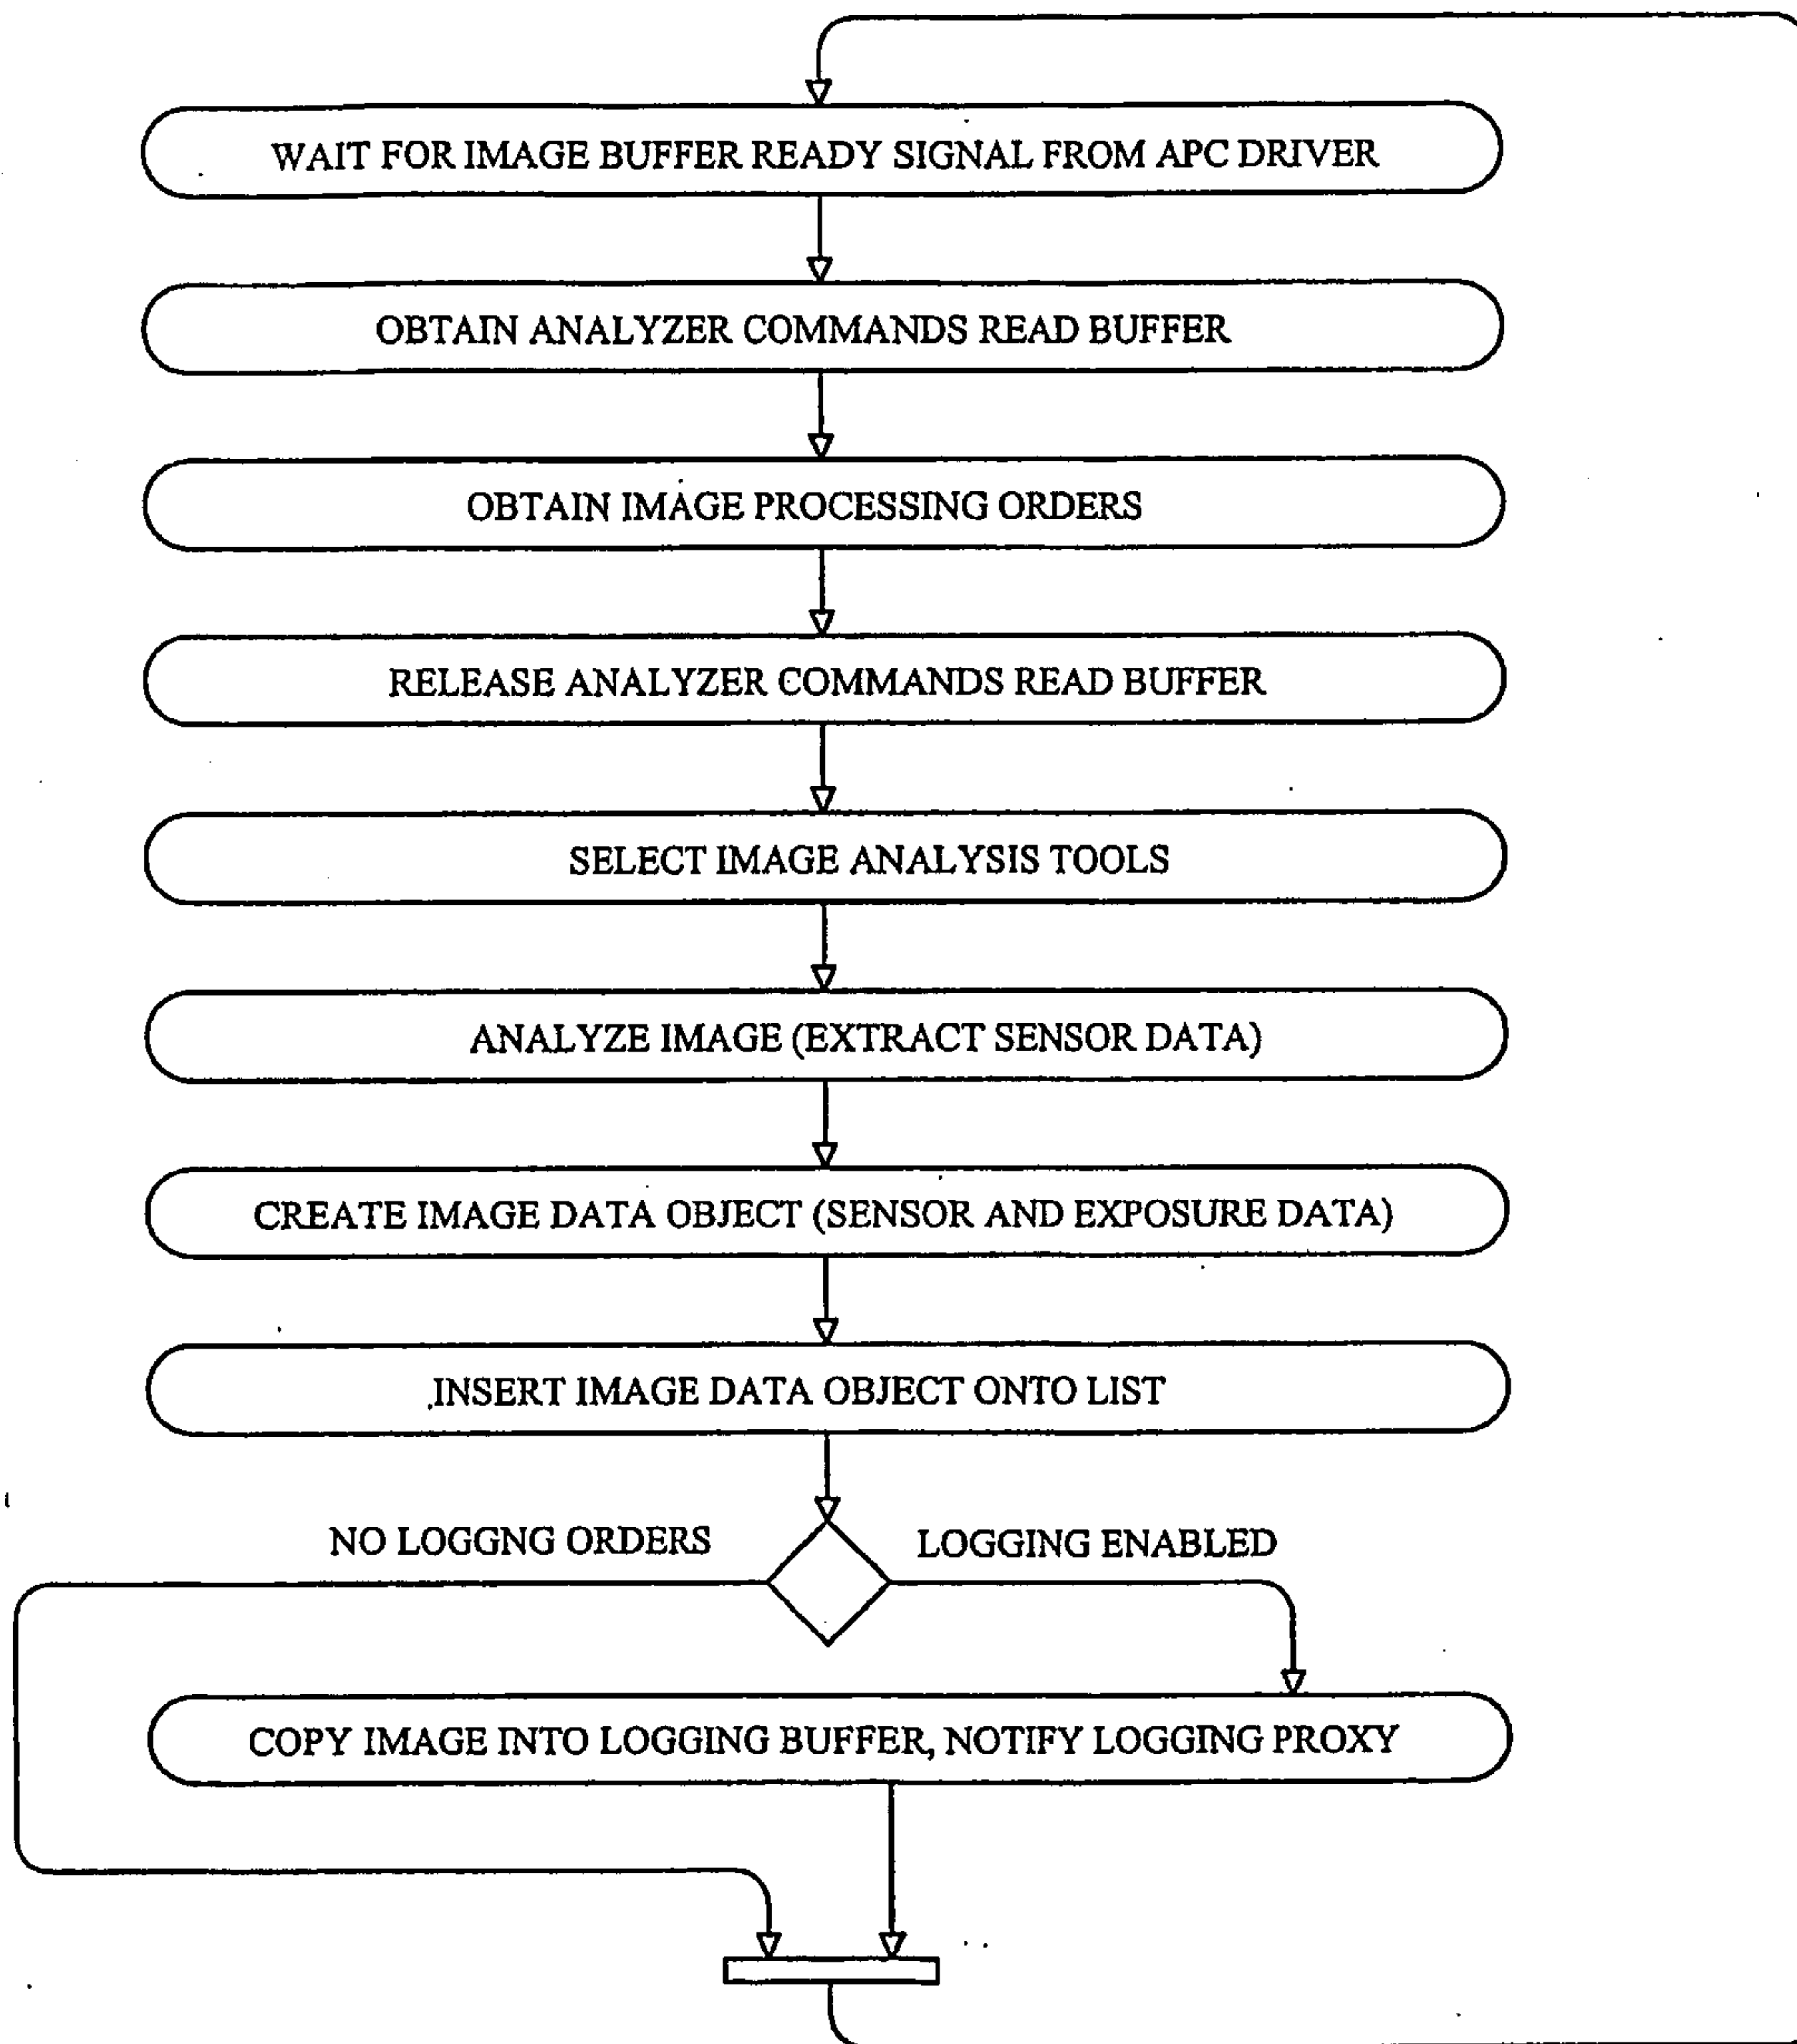


Figure 20

23 / 29

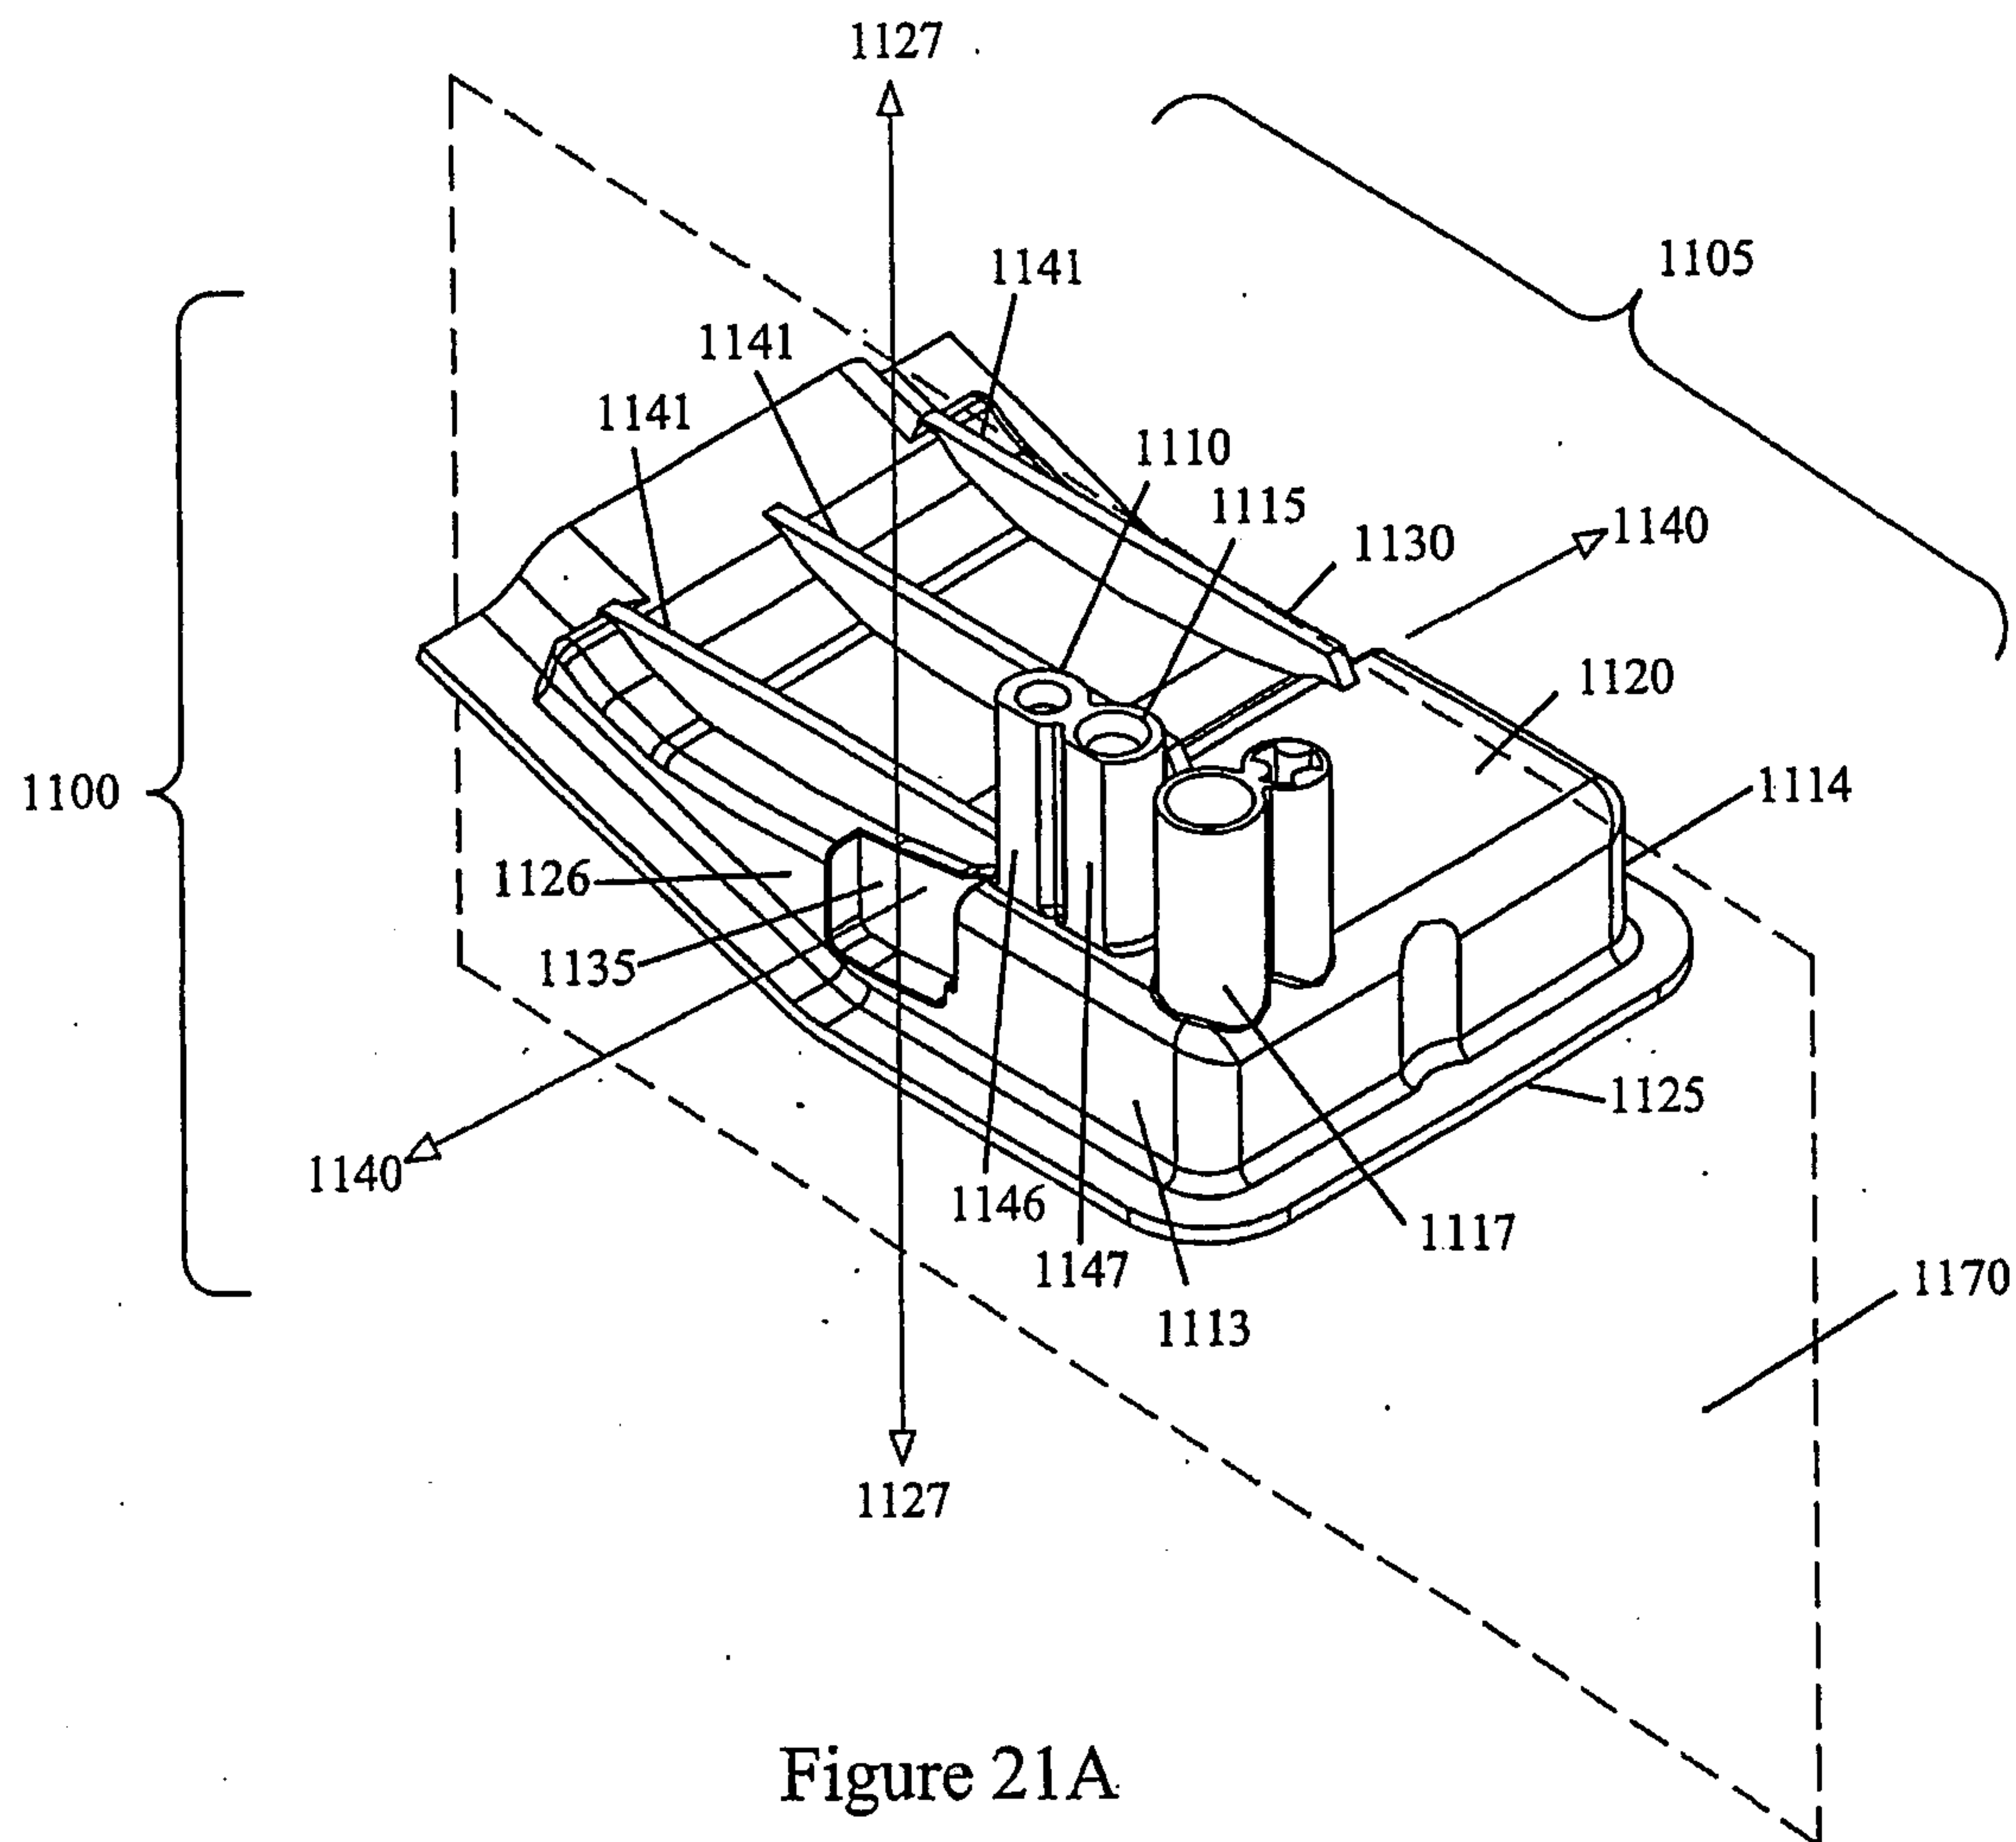


Figure 21A

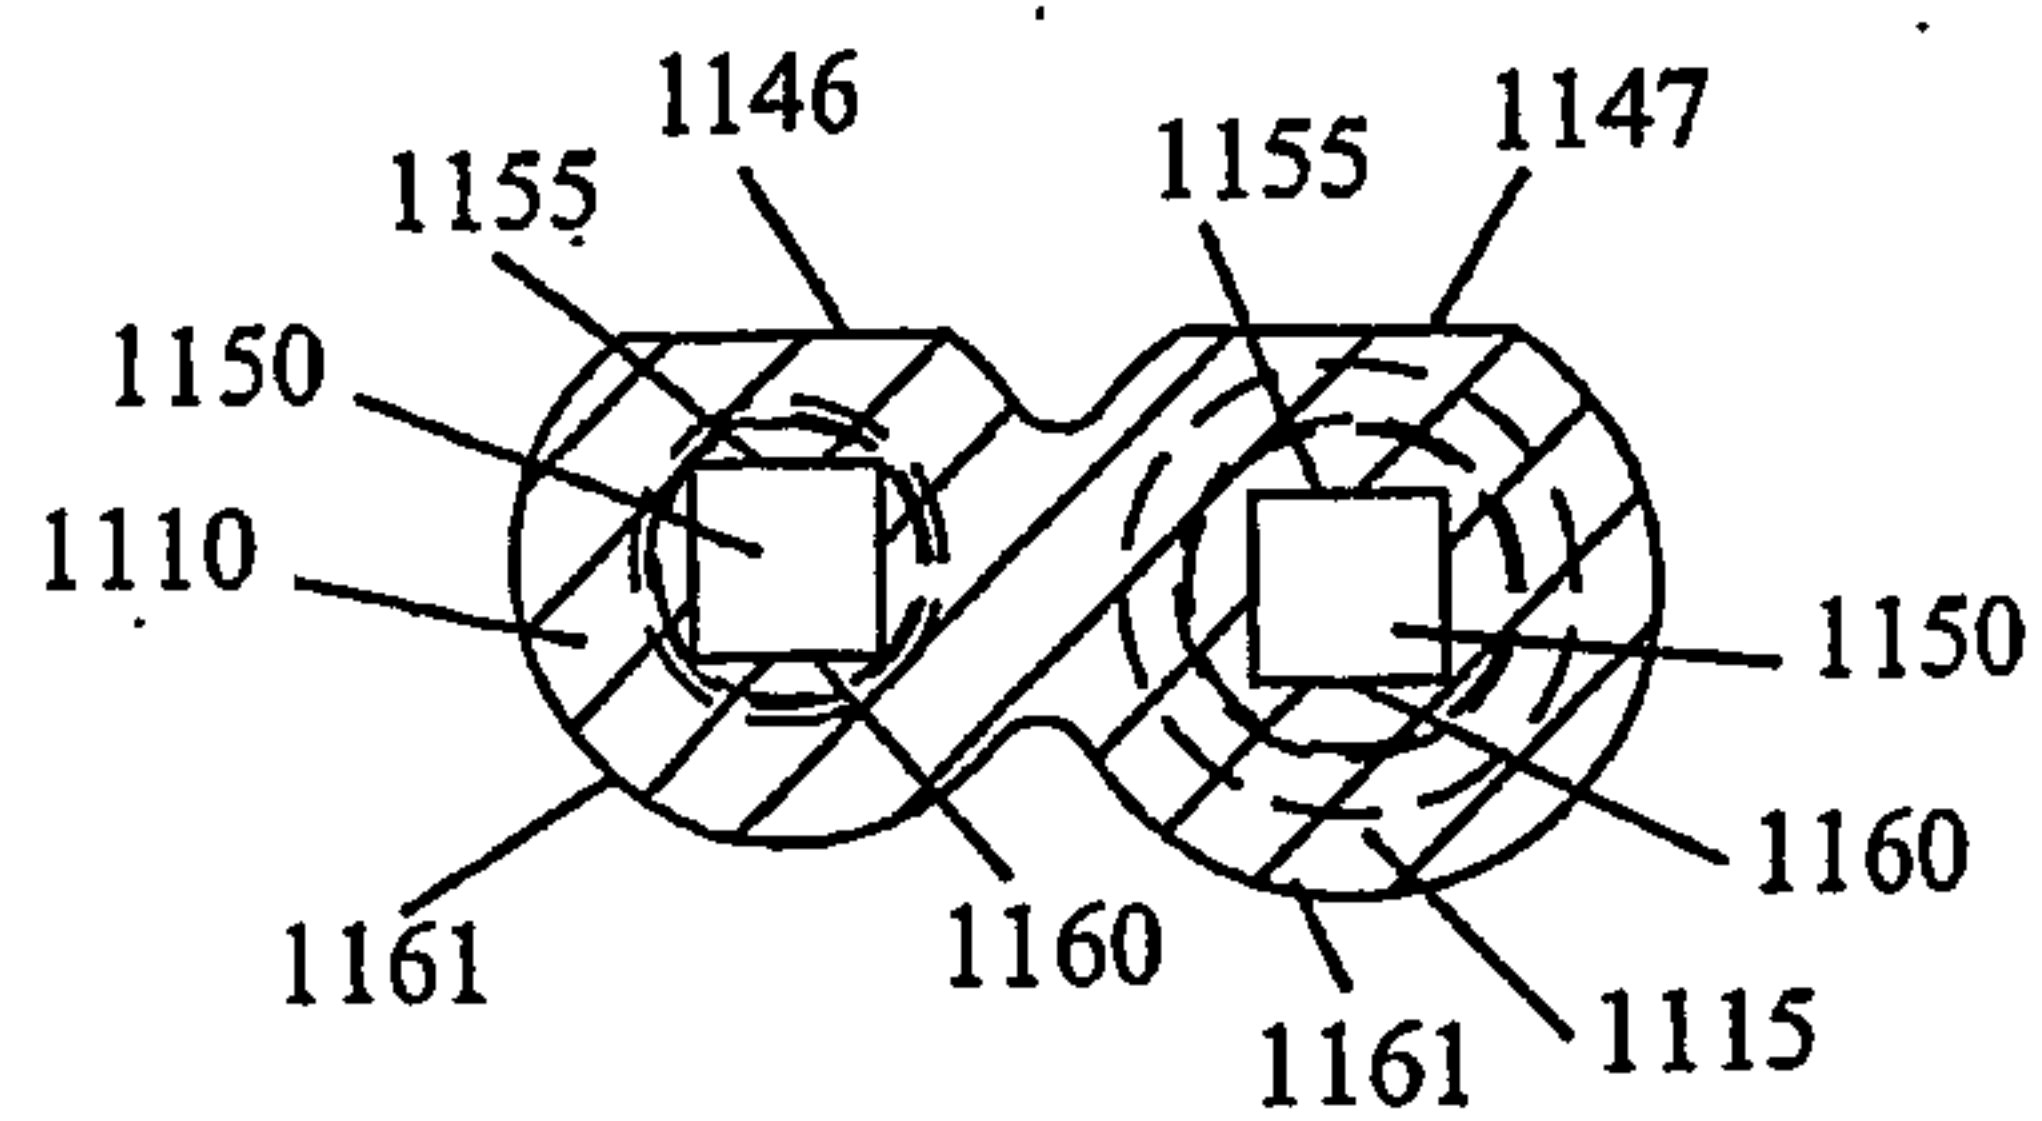


Figure 21B

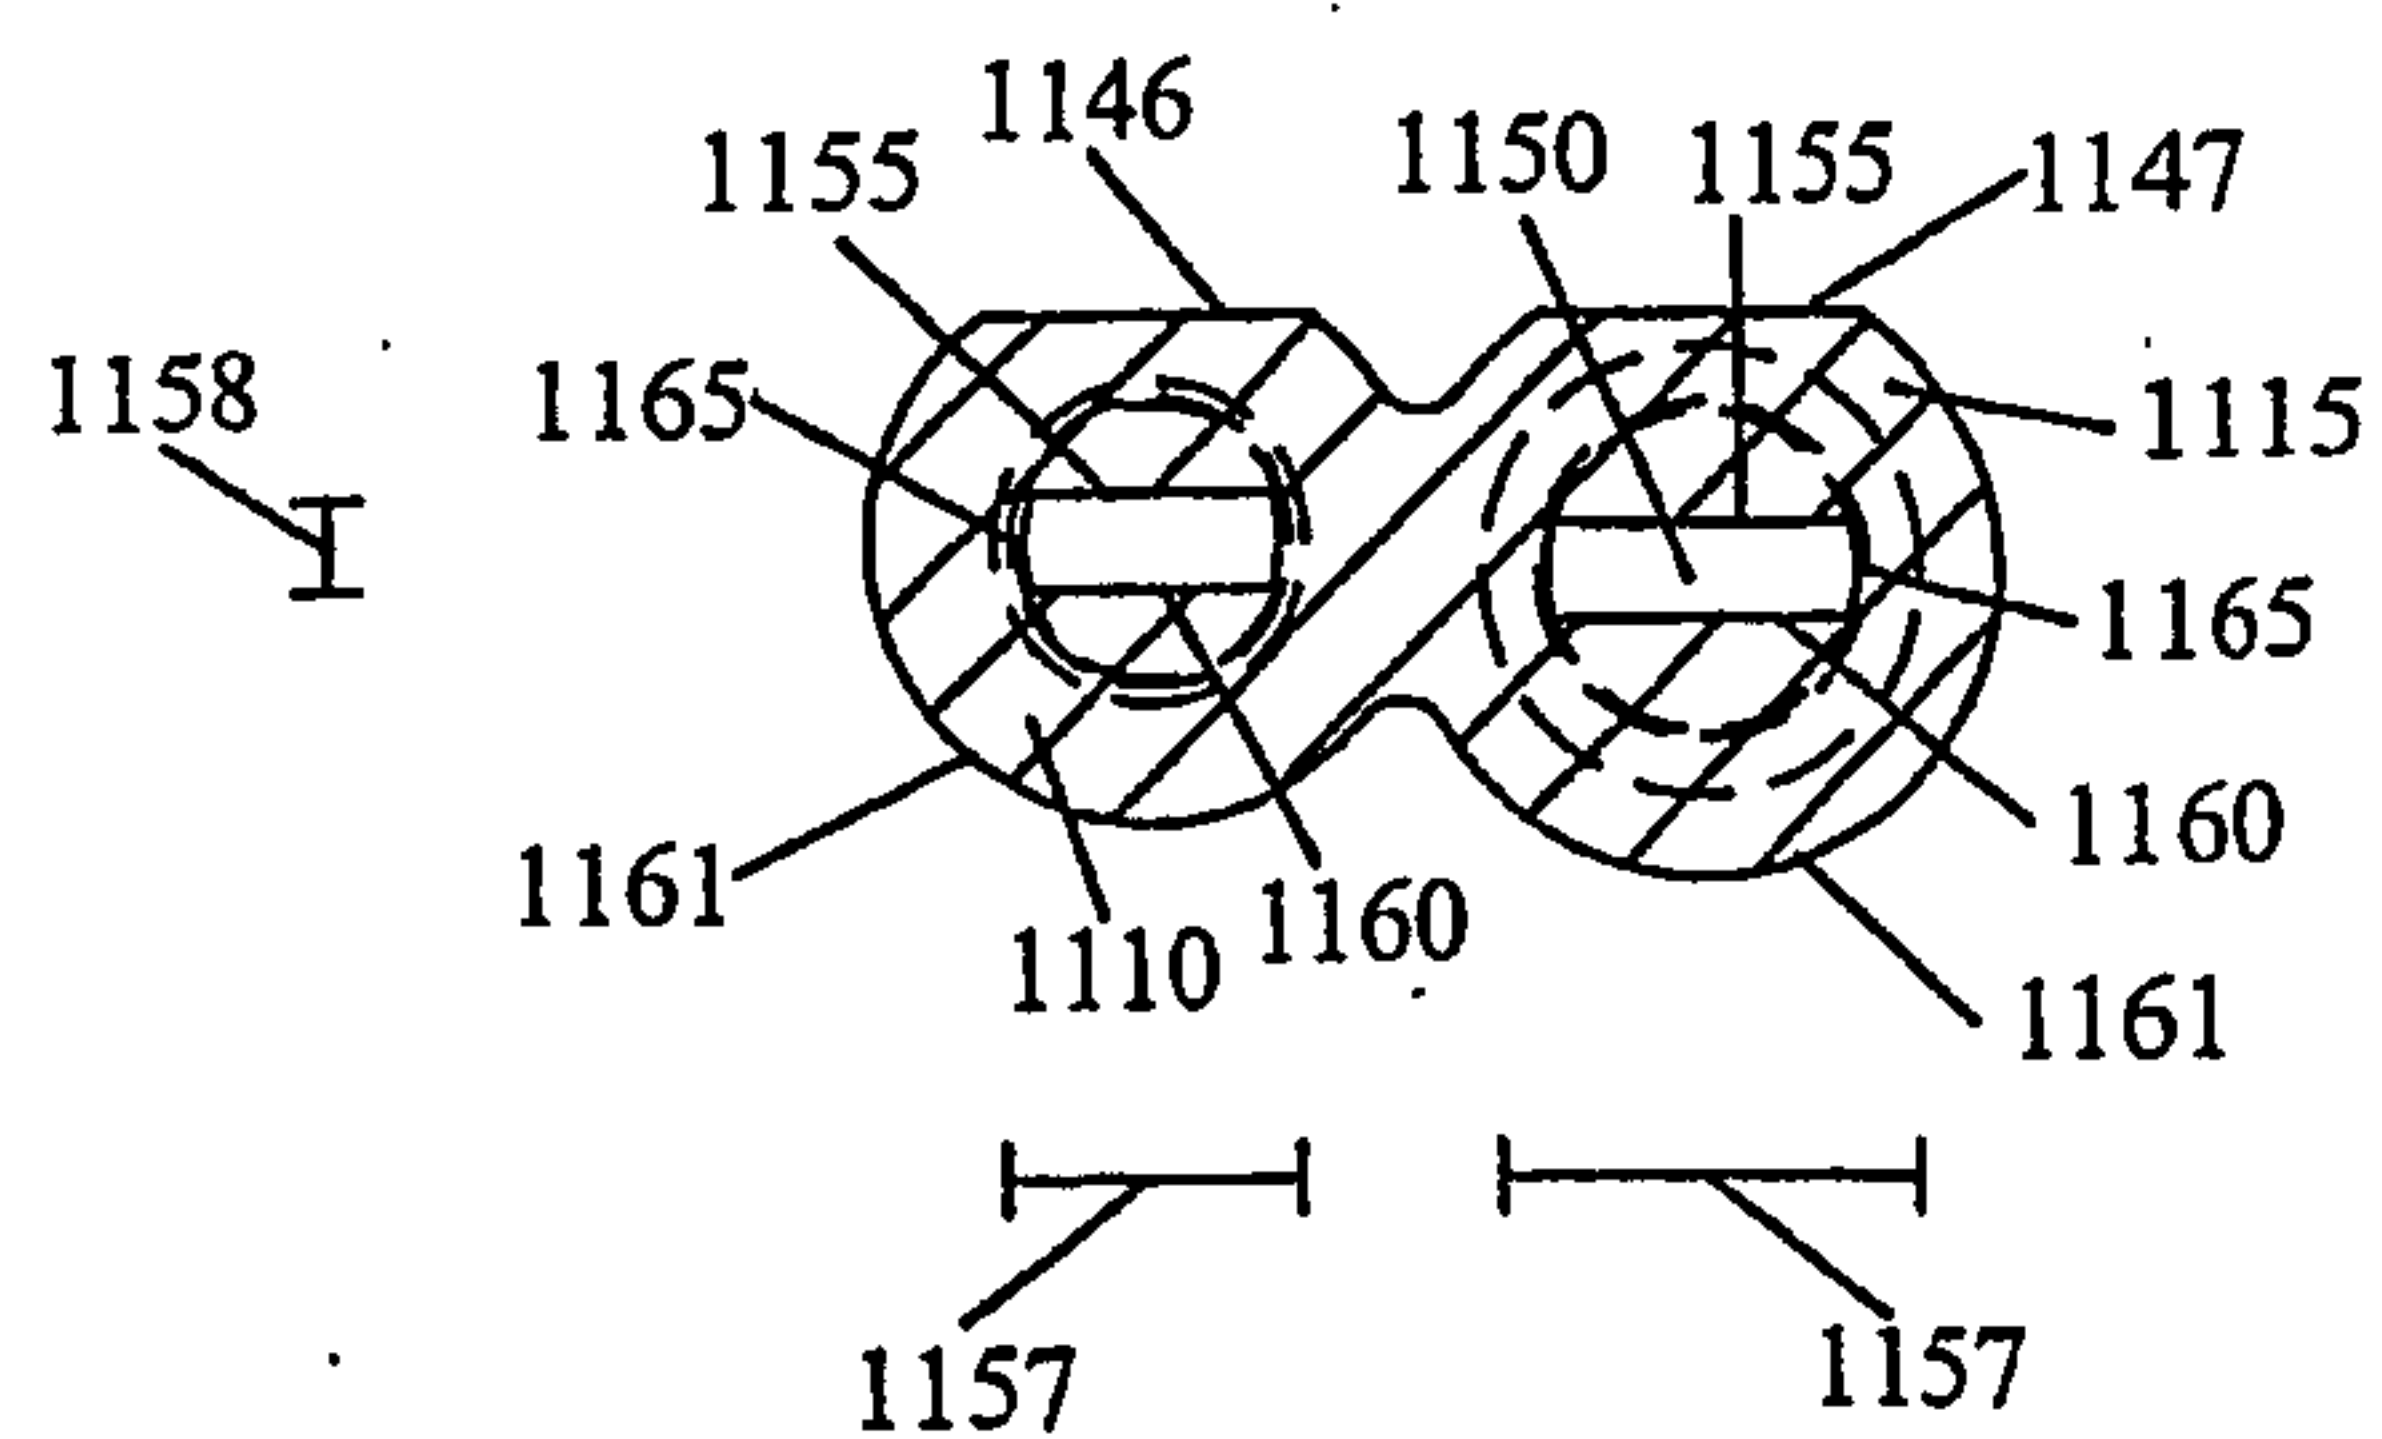


Figure 21C

24 / 29

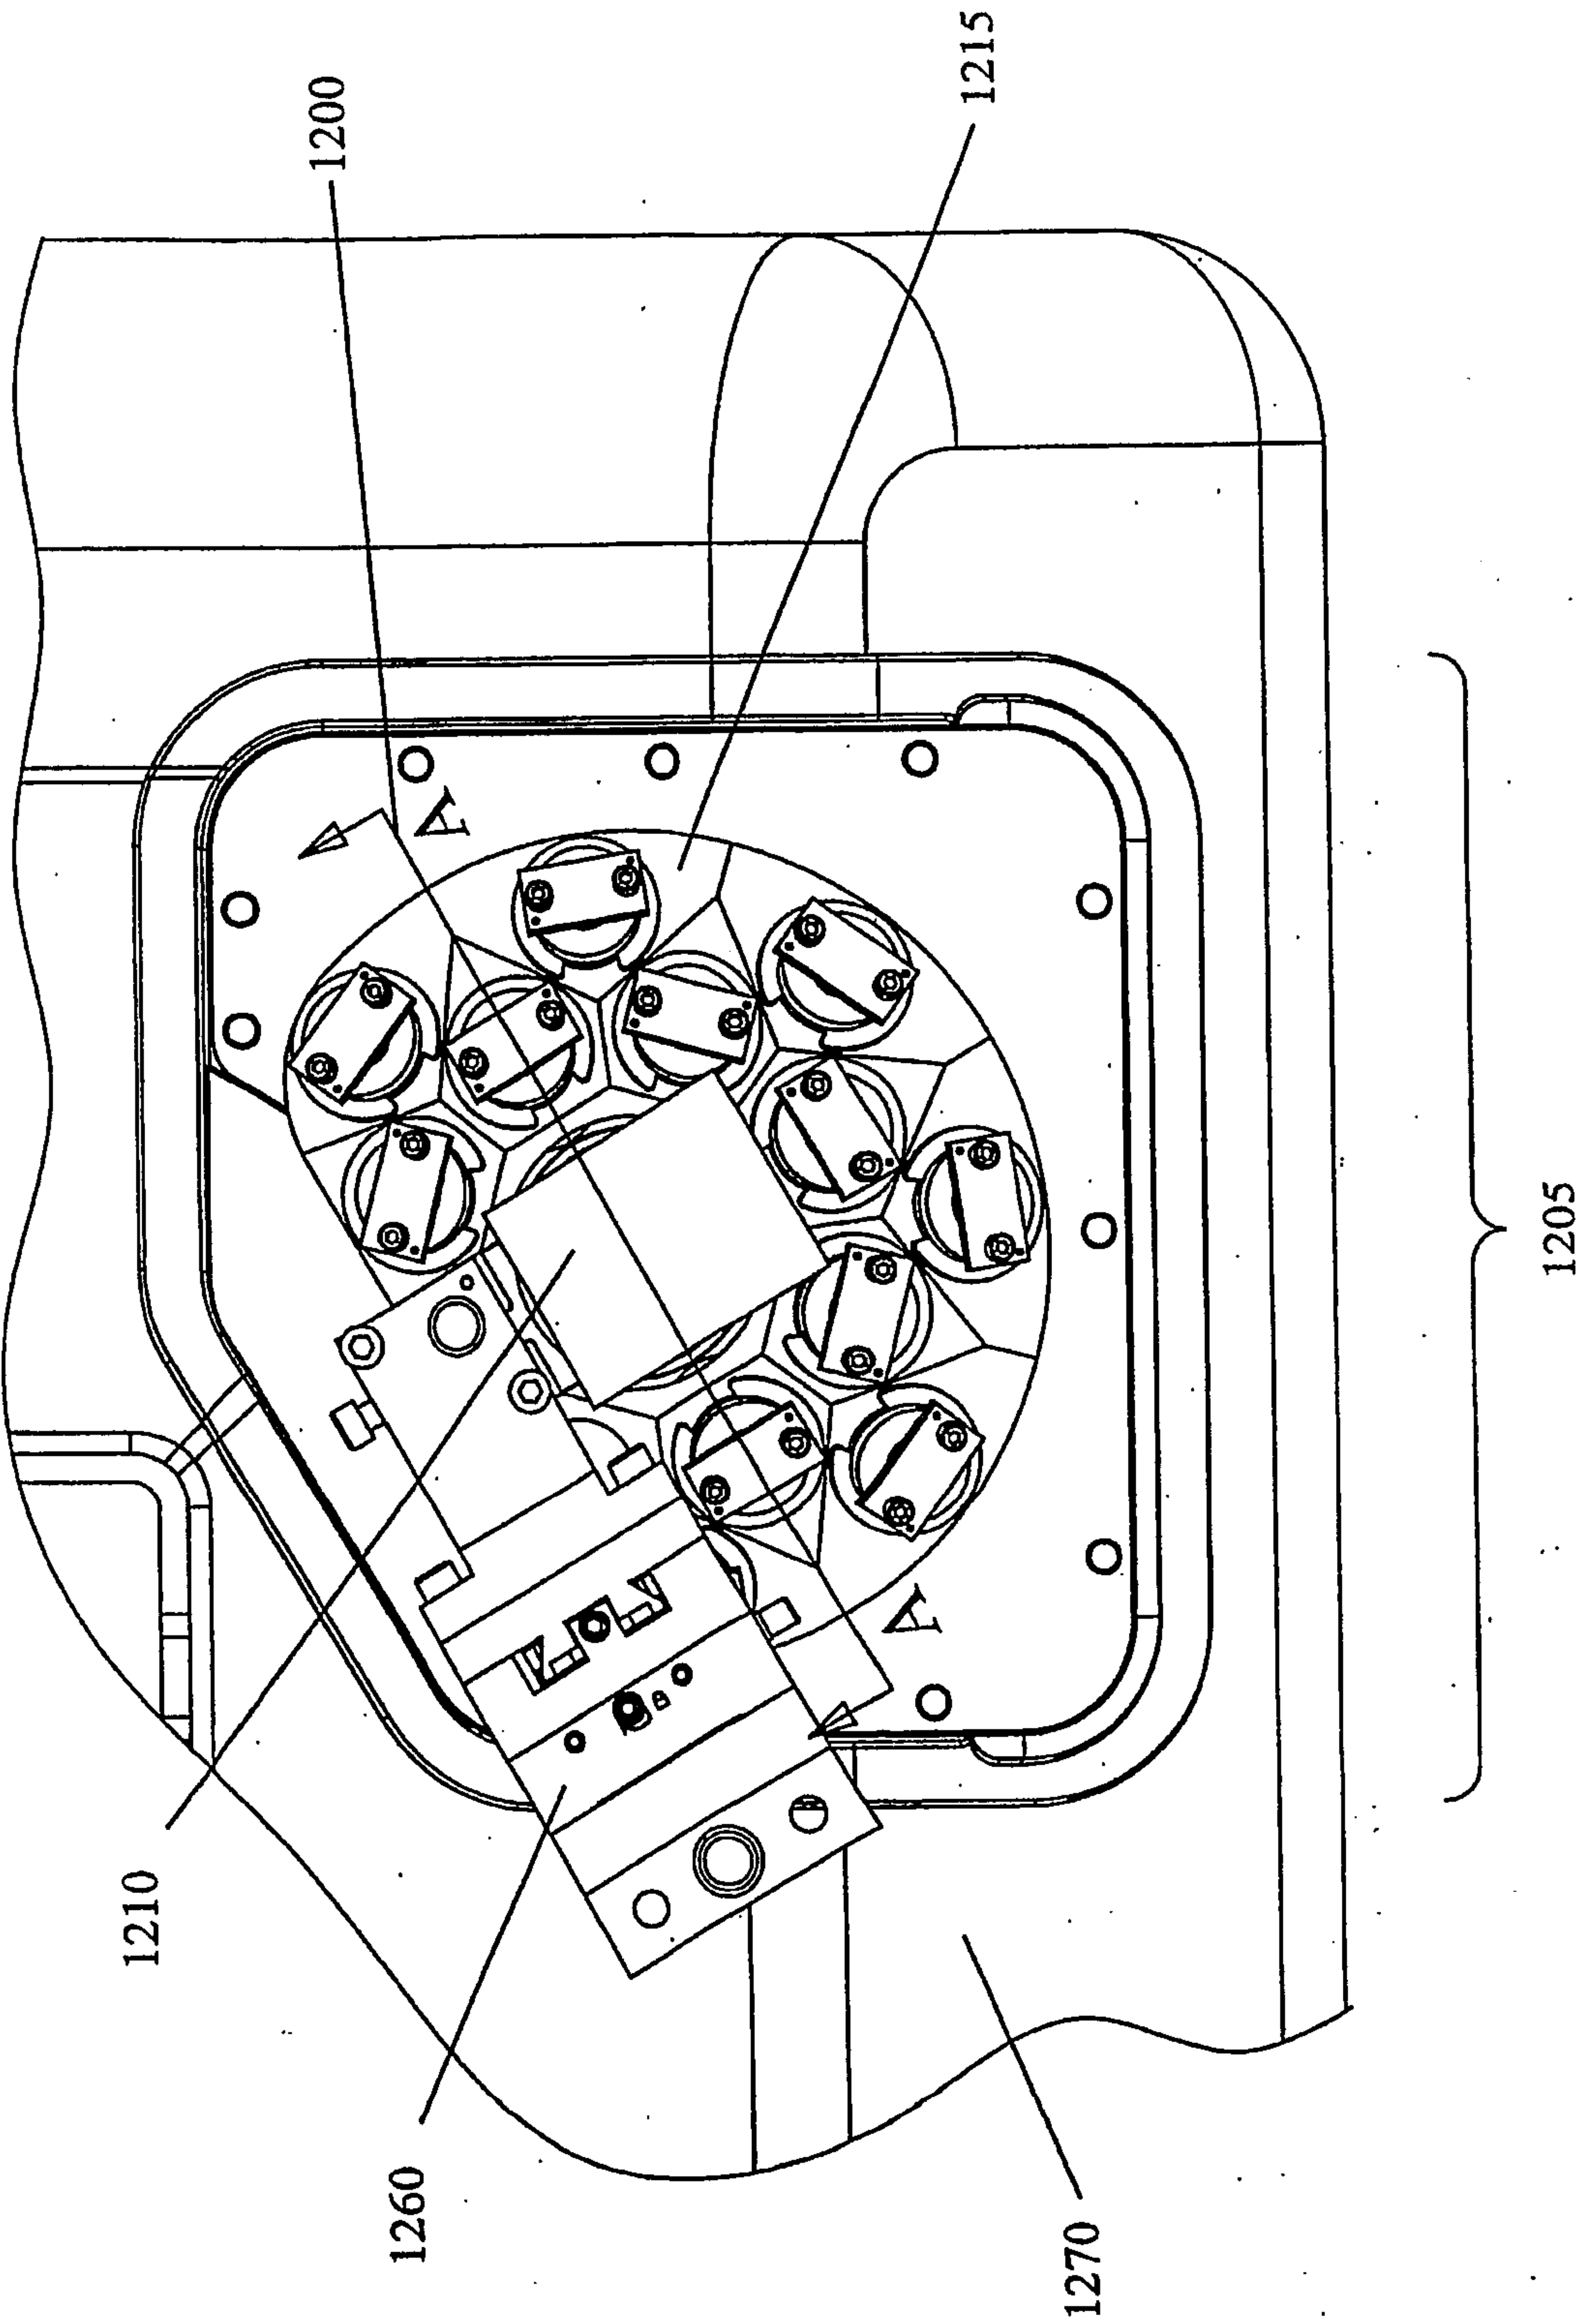


Figure 22

25 / 29

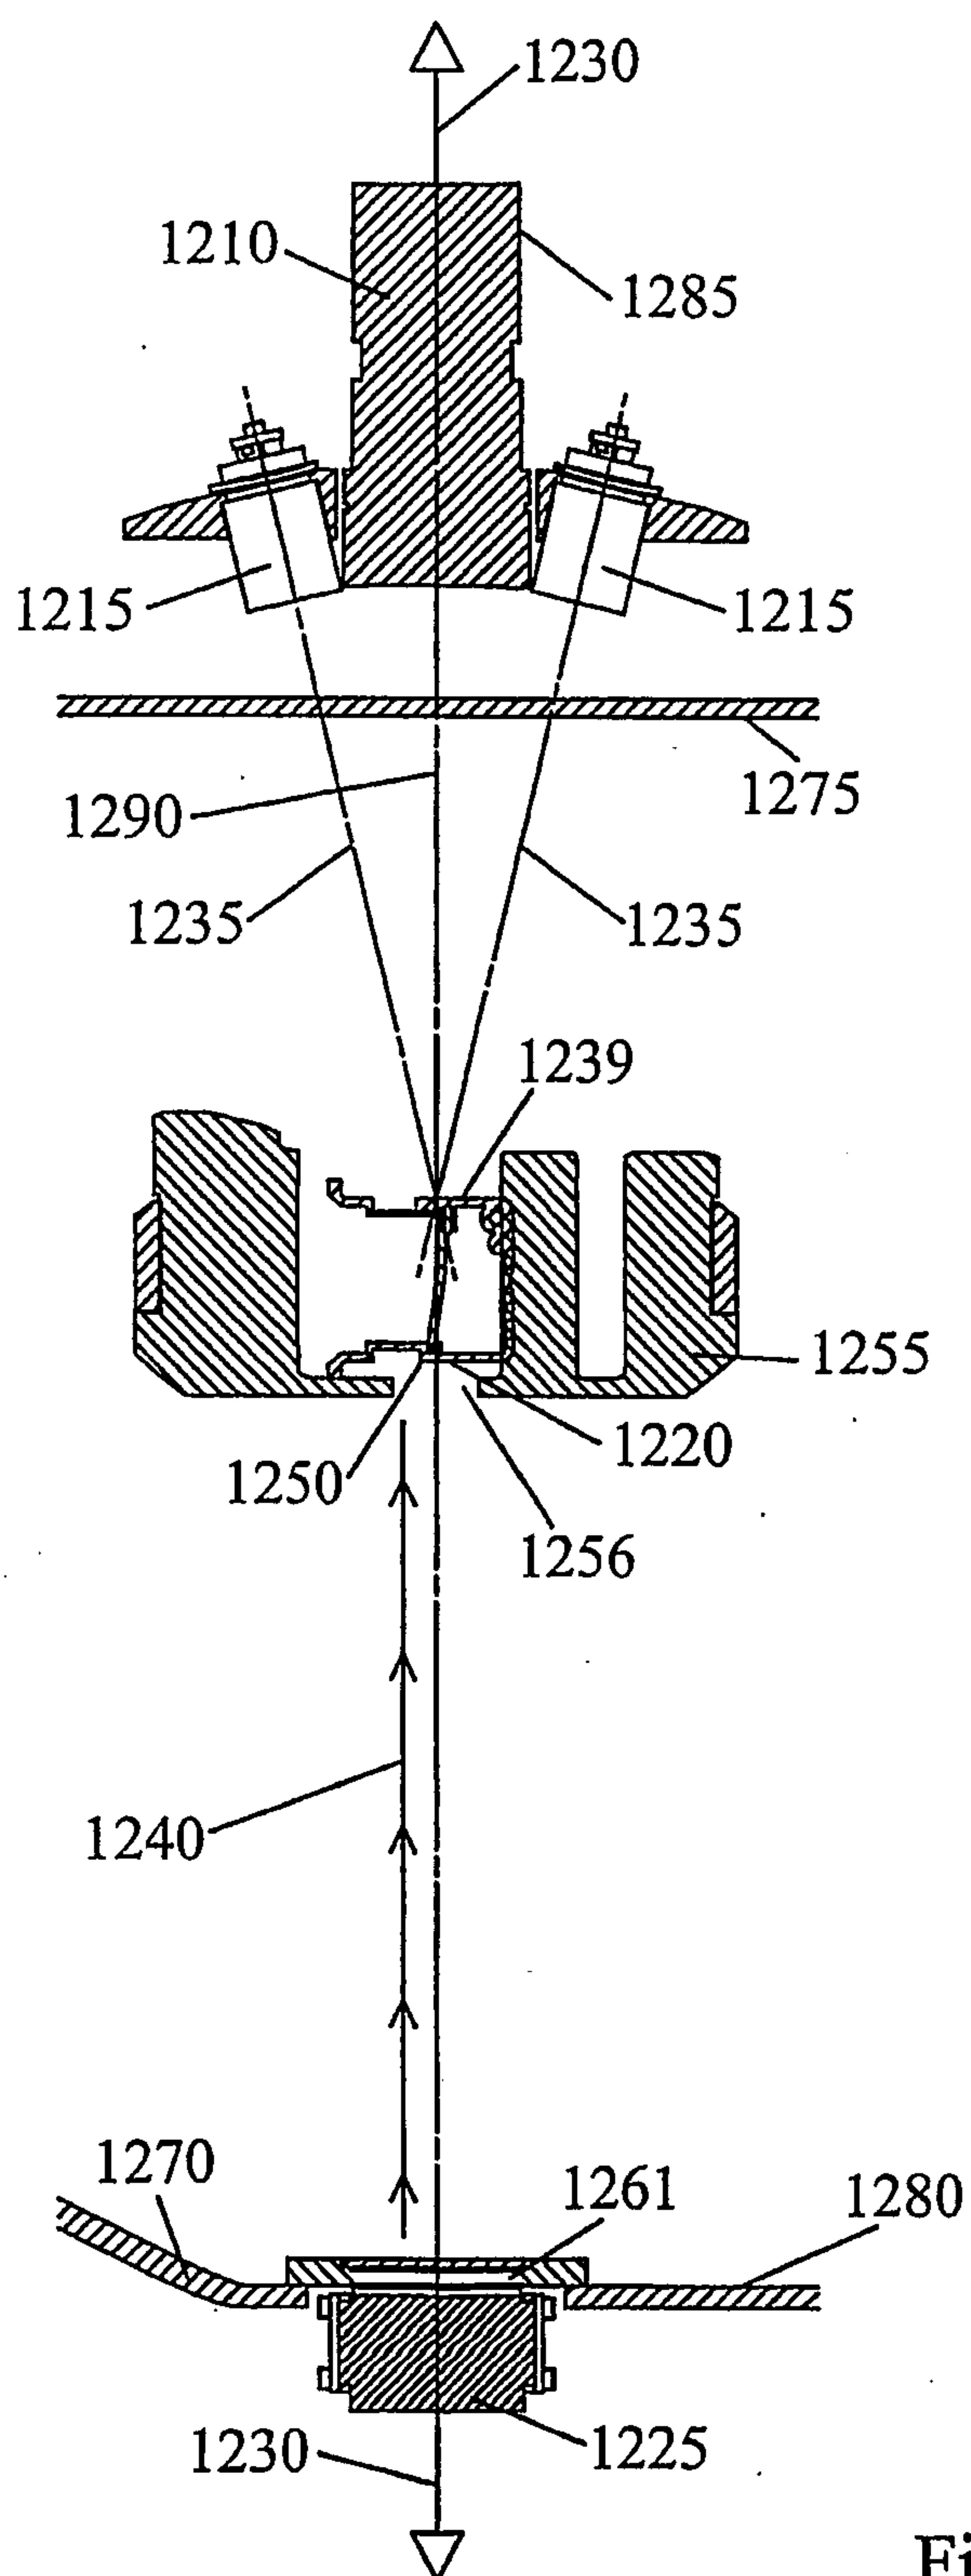


Figure 23

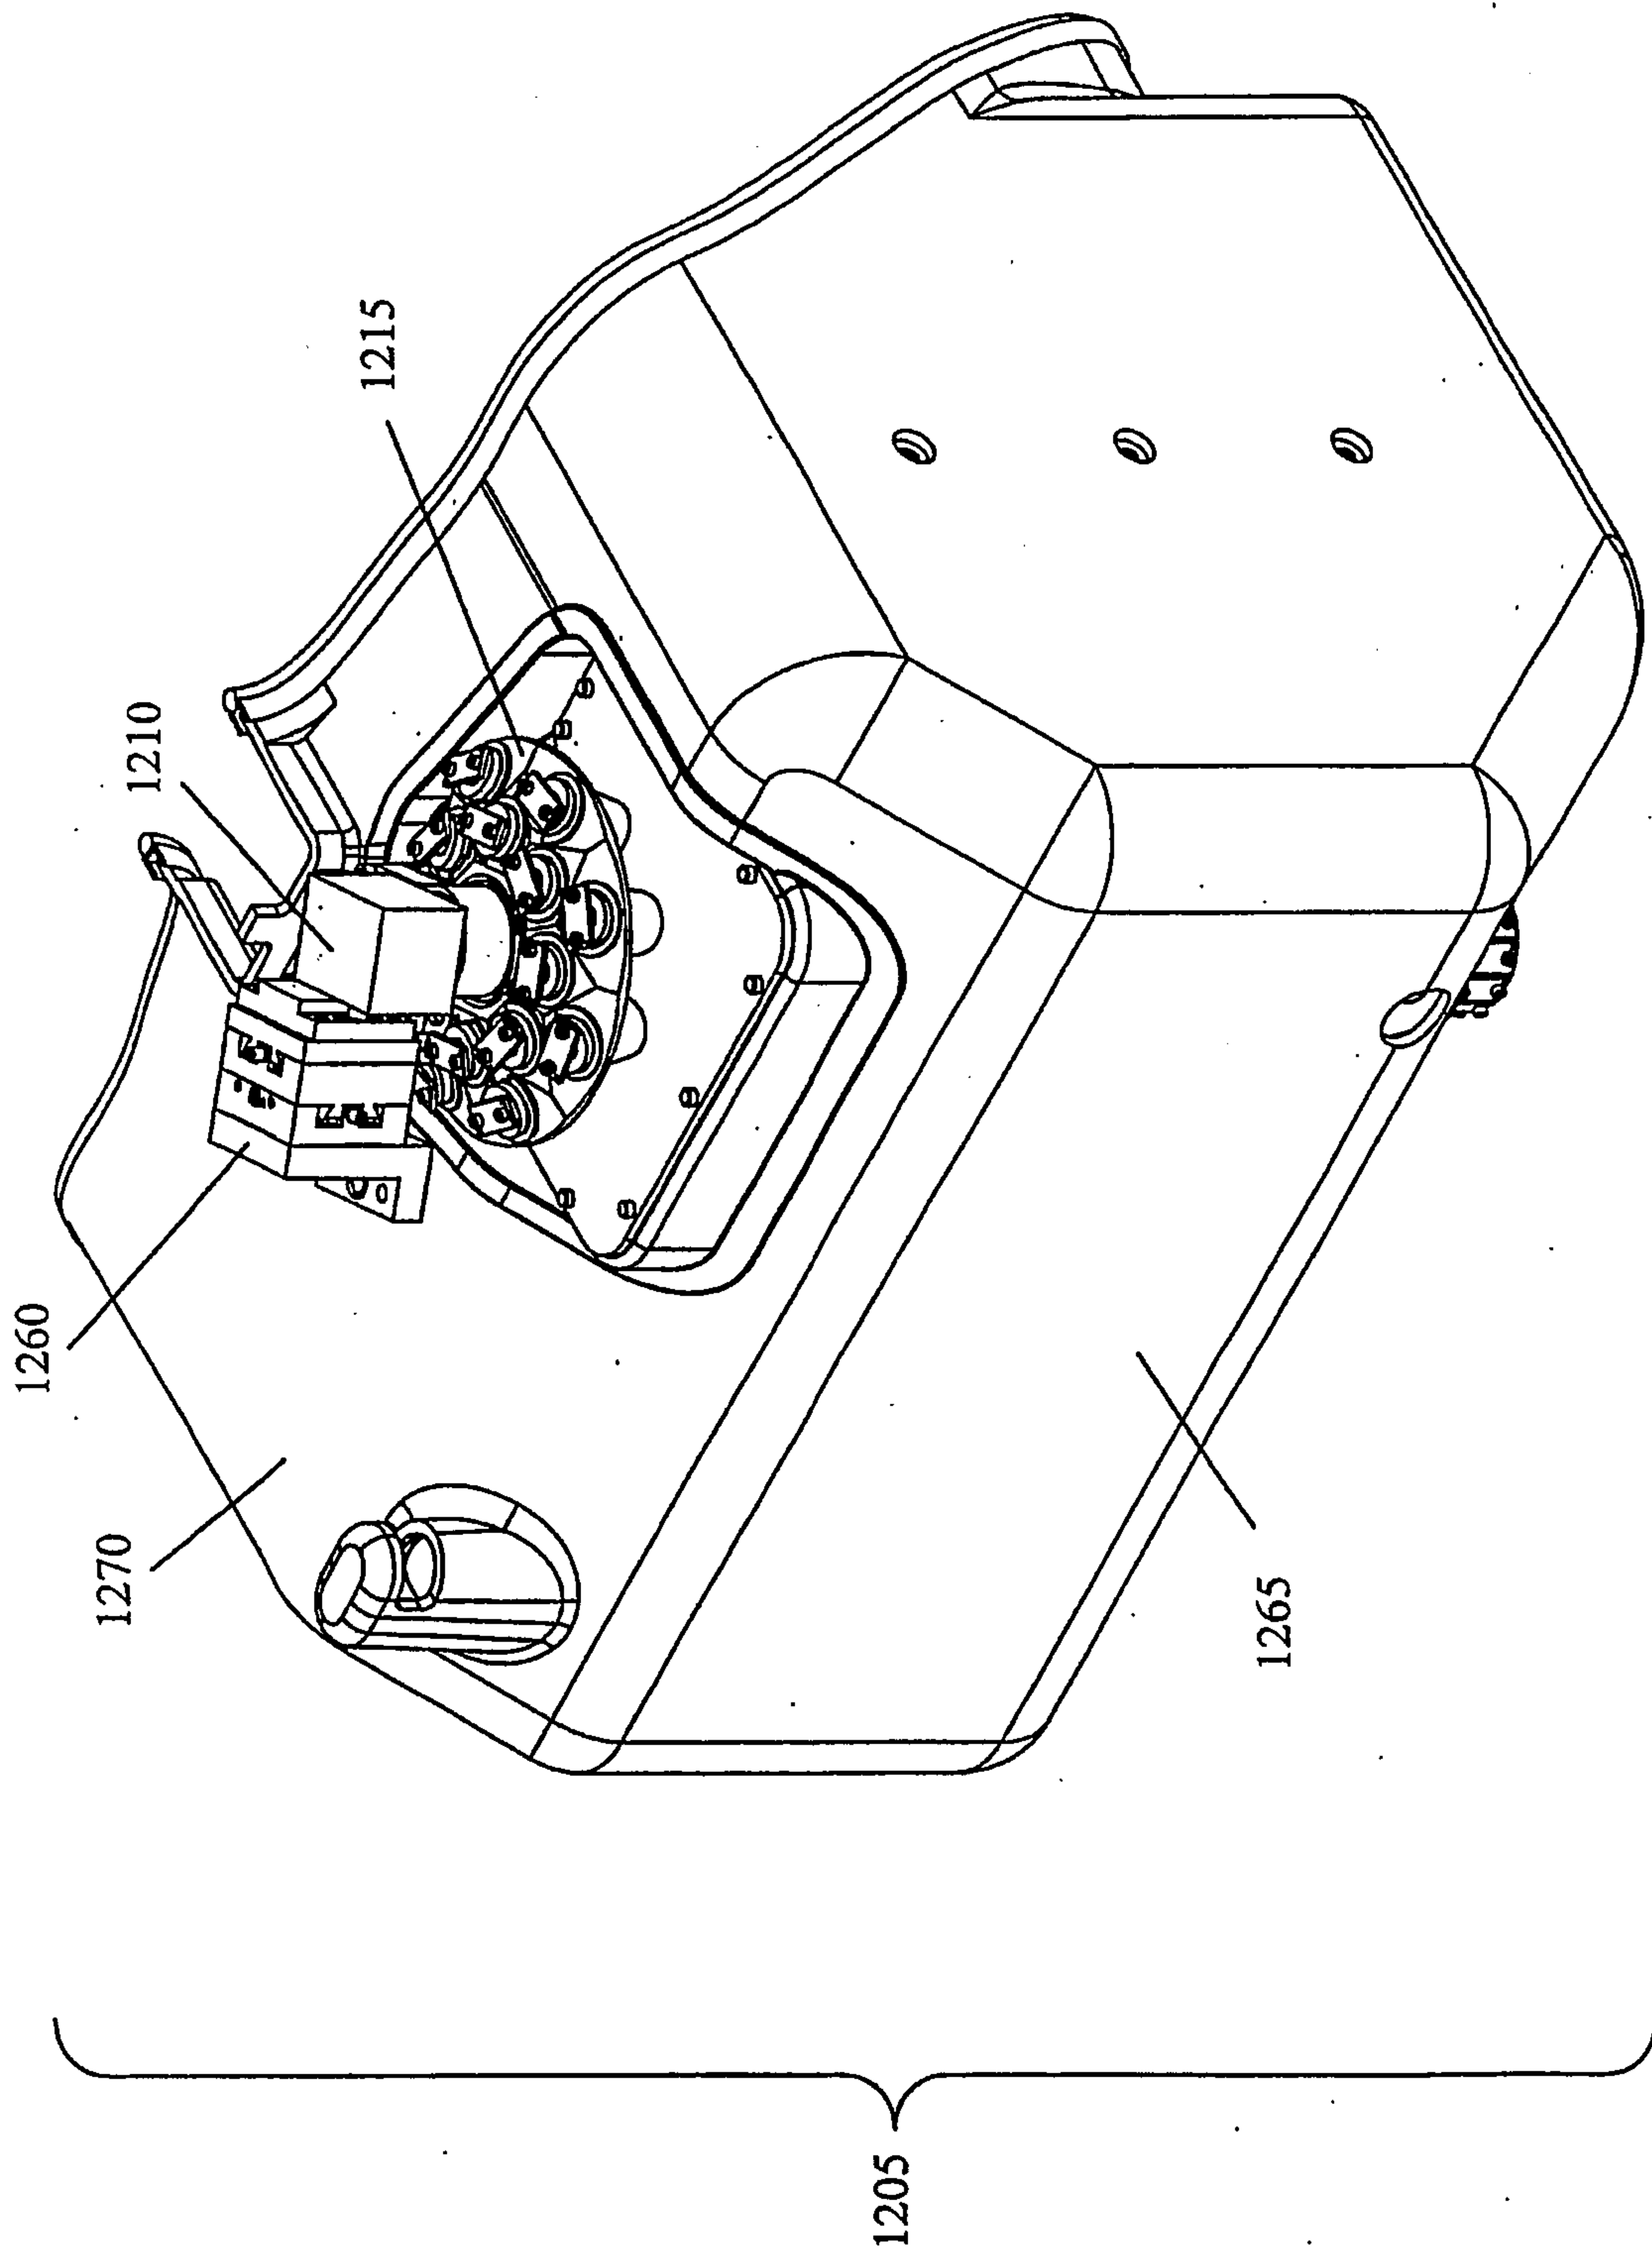


Figure 24

27 / 29

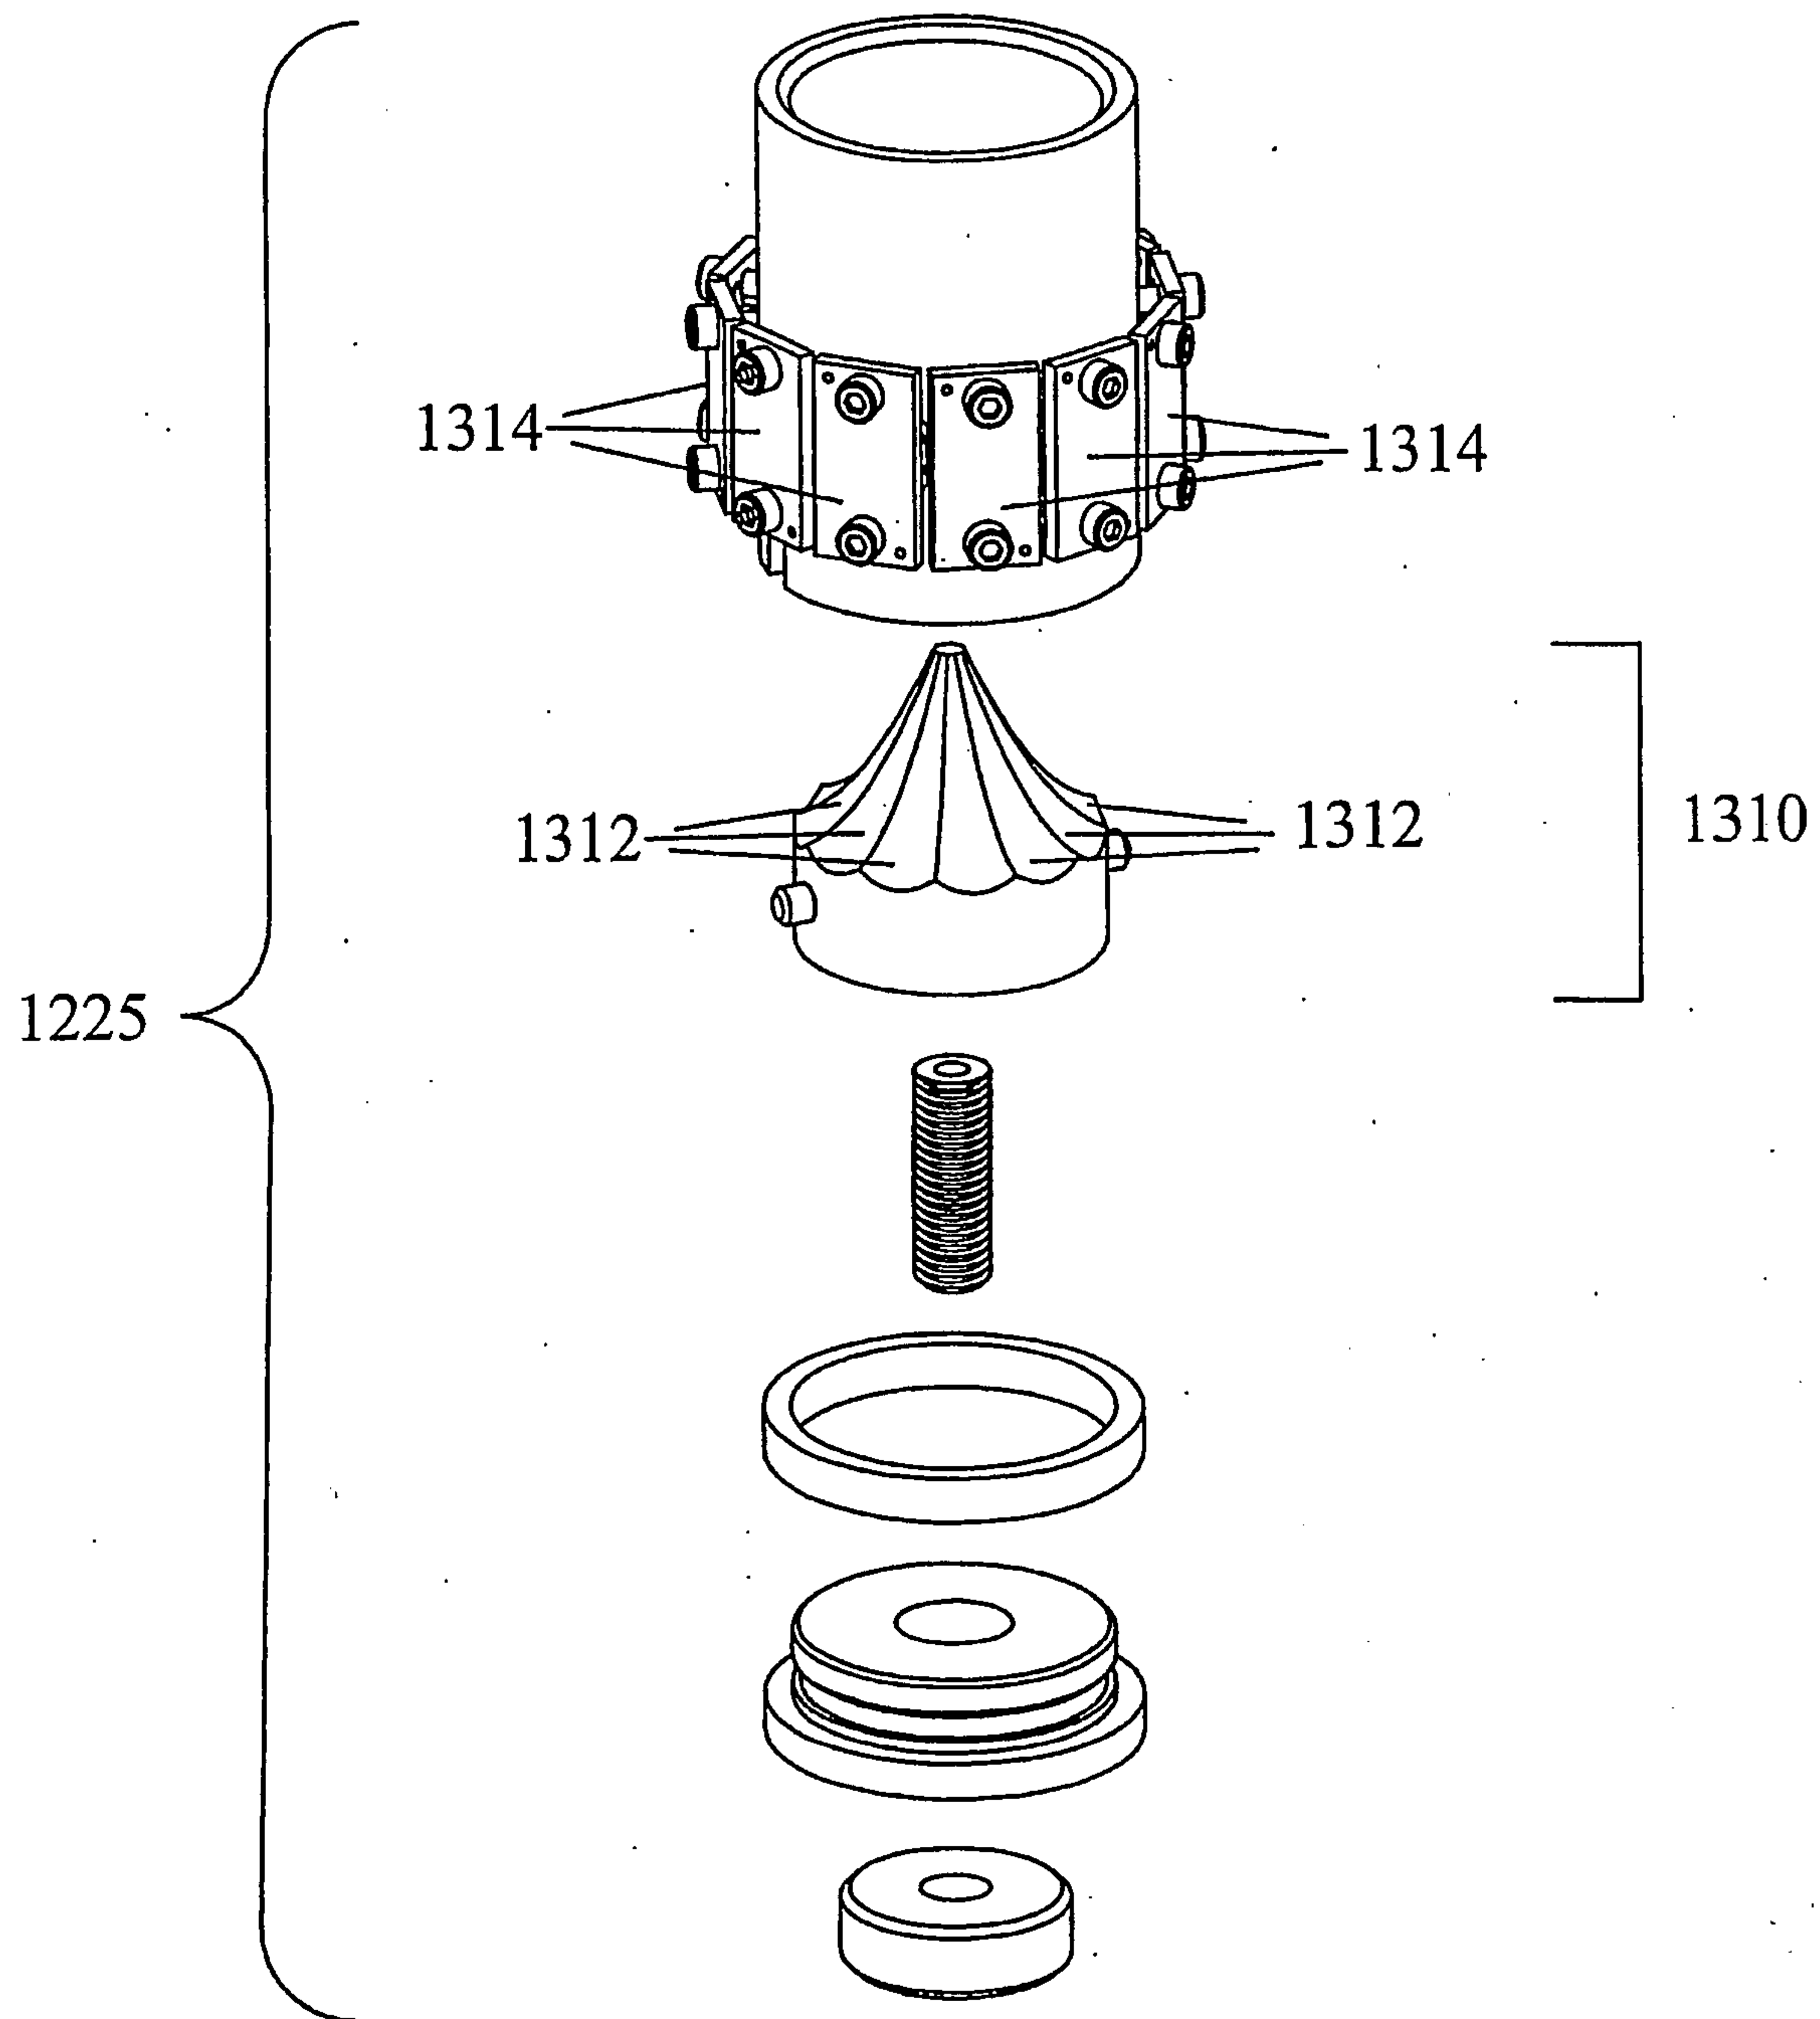


Figure 25

REPLACEMENT SHEET

28 / 29

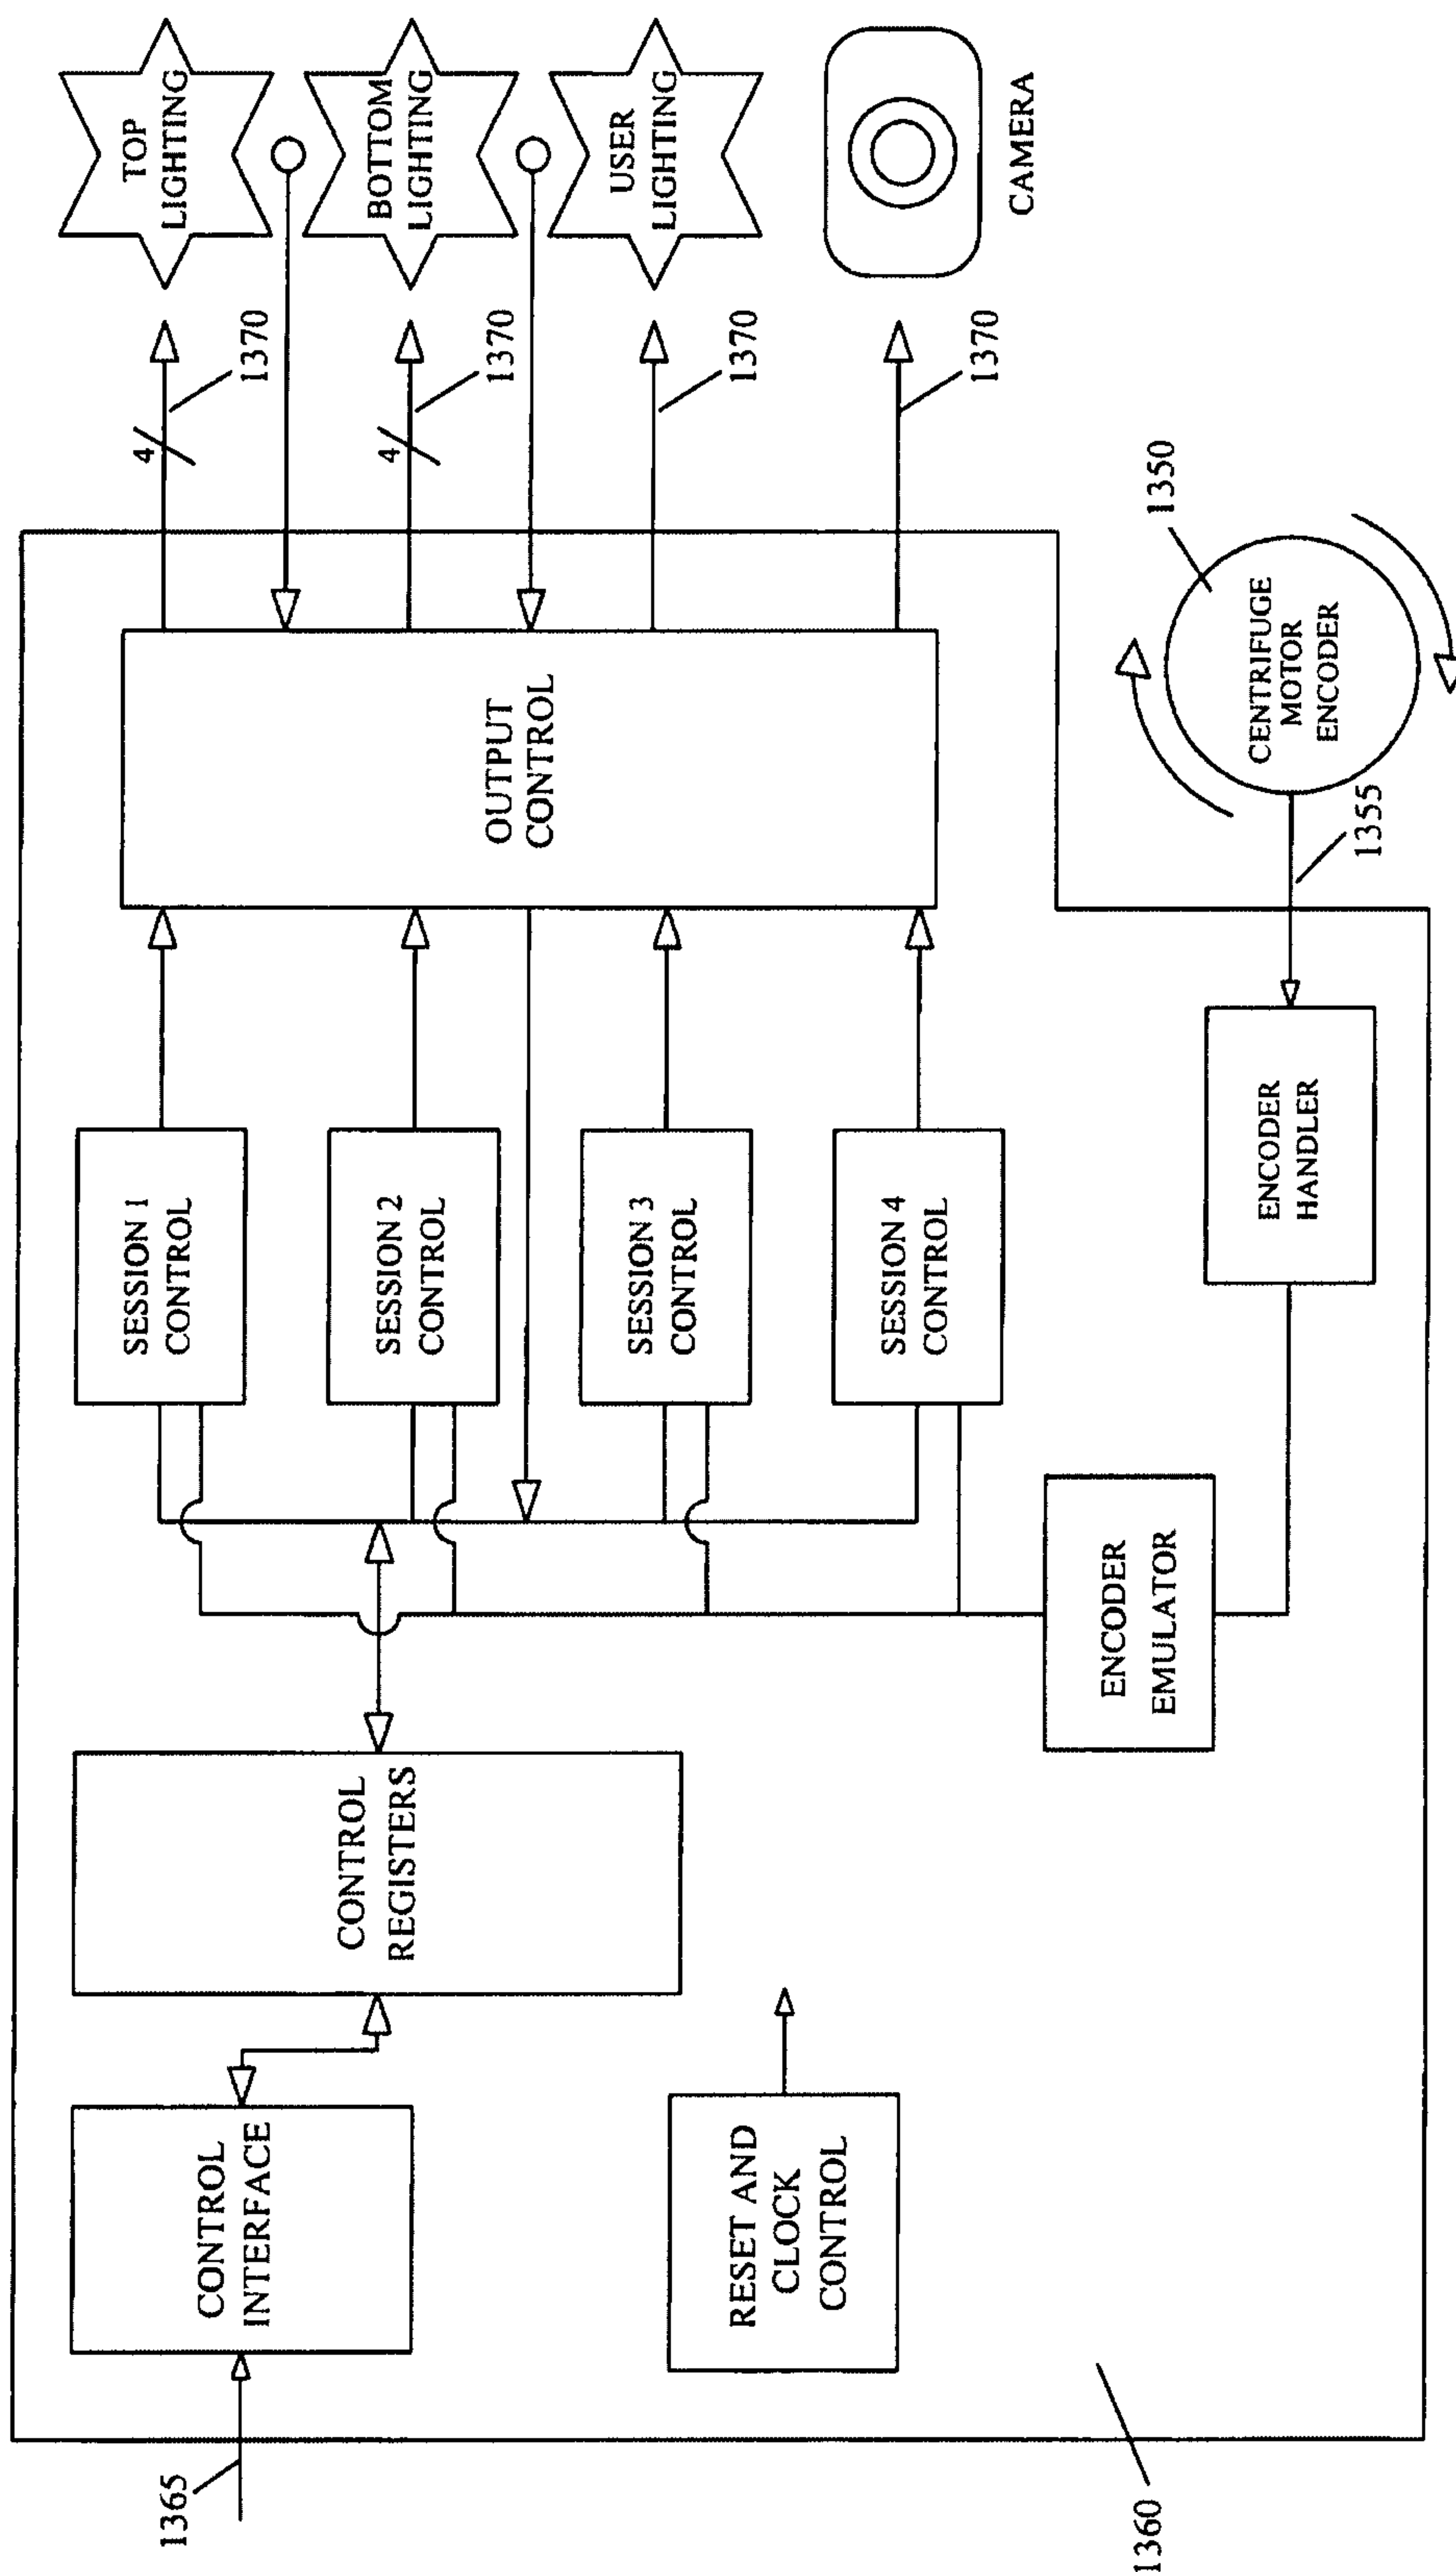


Figure 26

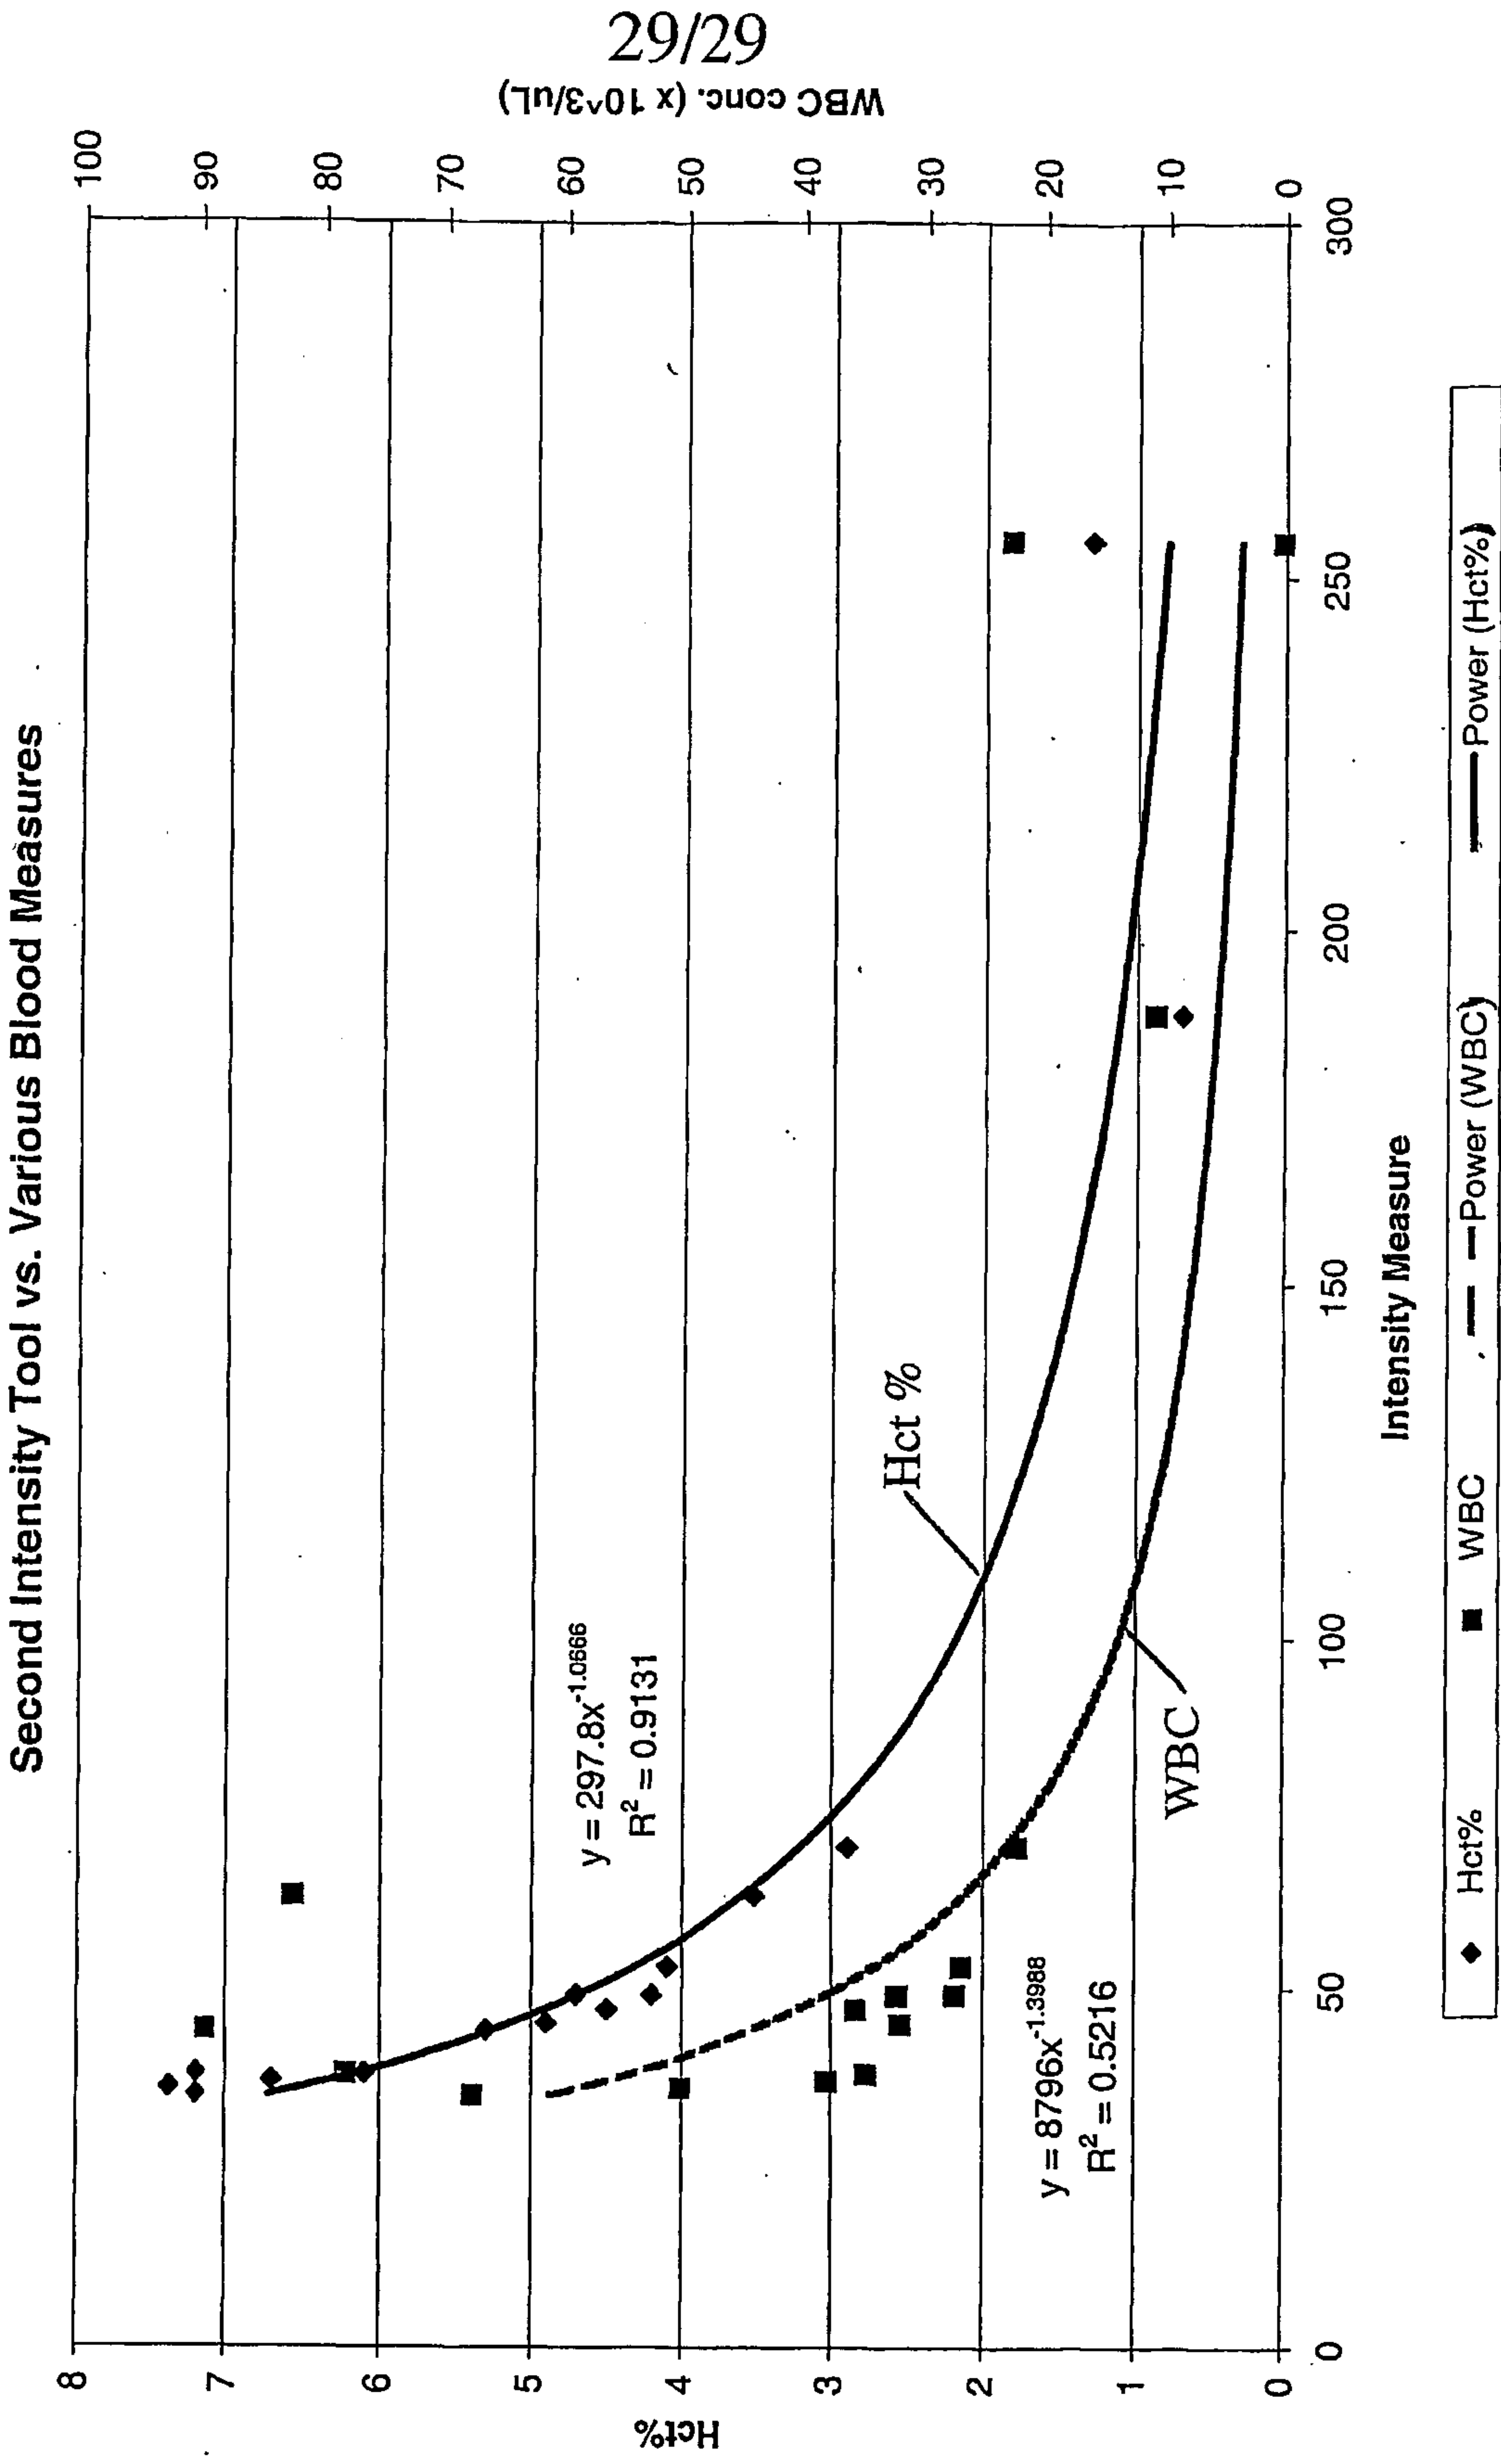


Fig. 27

1205

