



US00D910182S

(12) **United States Design Patent** (10) **Patent No.:** **US D910,182 S**
Dacosta et al. (45) **Date of Patent:** **** Feb. 9, 2021**

- (54) **HANDHELD MULTI-MODAL IMAGING DEVICE**
- (71) Applicant: **SBI Alapharma Canada, Inc.**, Toronto (CA)
- (72) Inventors: **Ralph S. Dacosta**, Etobicoke (CA); **Kathryn Ottolino-Perry**, Toronto (CA); **Christopher Gibson**, Toronto (CA); **Nayana Thalanki Anantha**, Toronto (CA); **Simon Treadwell**, Toronto (CA); **Connor Wright**, Toronto (CA); **Kimberlyn Dampitan**, Mississauga (CA); **Todd Daynes**, Aurora (CA); **Todd Meaney**, Thornhill (CA)
- (73) Assignees: **SBI ALAPHARMA CANADA, INC.**, Toronto (CA); **UNIVERSITY HEALTH NETWORK**, Toronto (CA)

(**) Term: **15 Years**

(21) Appl. No.: **29/677,154**

(22) Filed: **Jan. 17, 2019**

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.** **D24/158; D24/187**
USPC **D24/158; D24/187**

(58) **Field of Classification Search**
USPC D10/78; D24/133, 137, 158, 186, 187, D24/138, 152, 176
CPC A61B 8/445; A61B 8/4455; A61B 8/4461; A61B 8/12
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D515,214 S * 2/2006 Jackson, III D24/176
D701,606 S * 3/2014 Ohmukai D24/187
D703,331 S * 4/2014 Kitayama D24/187

D703,333 S * 4/2014 Saeki D24/187
D724,234 S * 3/2015 Hagege D24/187
D748,808 S * 2/2016 Matsumura D24/187
D750,260 S * 2/2016 Sauer D24/186
D810,293 S * 2/2018 Peel D24/152
D862,697 S * 10/2019 Kenworthy D24/158
D866,764 S * 11/2019 Pukall D24/152

(Continued)

FOREIGN PATENT DOCUMENTS

WO 2019148268 A1 8/2019

OTHER PUBLICATIONS

International Patent Application No. PCT/IB2020/050383, dated Jan. 17, 2020.

(Continued)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Jones Robb, PLLC

(57) **CLAIM**

The ornamental design for a handheld multi-modal imaging device, as shown and described.

DESCRIPTION

FIG. 1 is a top, left side perspective view of an embodiment of a handheld multi-modal imaging device showing our new design.

FIG. 2 is a bottom, left side perspective view thereof.

FIG. 3 is a left side view thereof.

FIG. 4 is a right side view thereof.

FIG. 5 is a top view thereof.


FIG. 6 is a bottom view thereof.

FIG. 7 is a front view thereof; and,

FIG. 8 is a back view thereof.

The broken lines on the handle member represent environment and the remaining broken lines illustrate portions of the handheld multi-modal imaging device that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

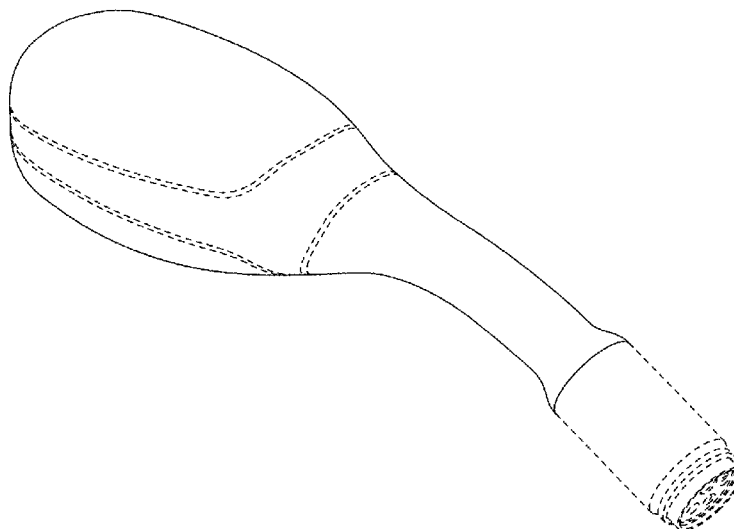

(56)

References Cited

U.S. PATENT DOCUMENTS

2016/0045114 A1 2/2016 Dacosta et al.
2017/0290515 A1 10/2017 Butte et al.

OTHER PUBLICATIONS

International Search Report and Written Opinion from International Patent Application No. PCT/CA2019/000015, dated Jun. 4, 2019.
Gao et al., "Fluorescent chemical probes for accurate tumor diagnosis and targeting therapy," The Royal Society of Chemistry, Mar. 20, 2017, <https://www.researchgate.net/publication/315469453_Fluorescent_chemical_probes_for_accurate_tumor_diagnosis_and_targeting_therapy>.

Ntziachristos et al., "Current concepts and future perspectives on surgical optical imaging in cancer", Journal of Biomedical Optics, vol. 15(6), Nov./Dec. 2010, <<https://www.spiedigitallibrary.org/journals/Journal-of-Biomedical-Optics/volume-15-issue-6-1066024/Current-concepts-and-future-perspectives-on-surgical-optical-imaging-n/10.1117/1.3523364.full?SSO=1>>.

* cited by examiner

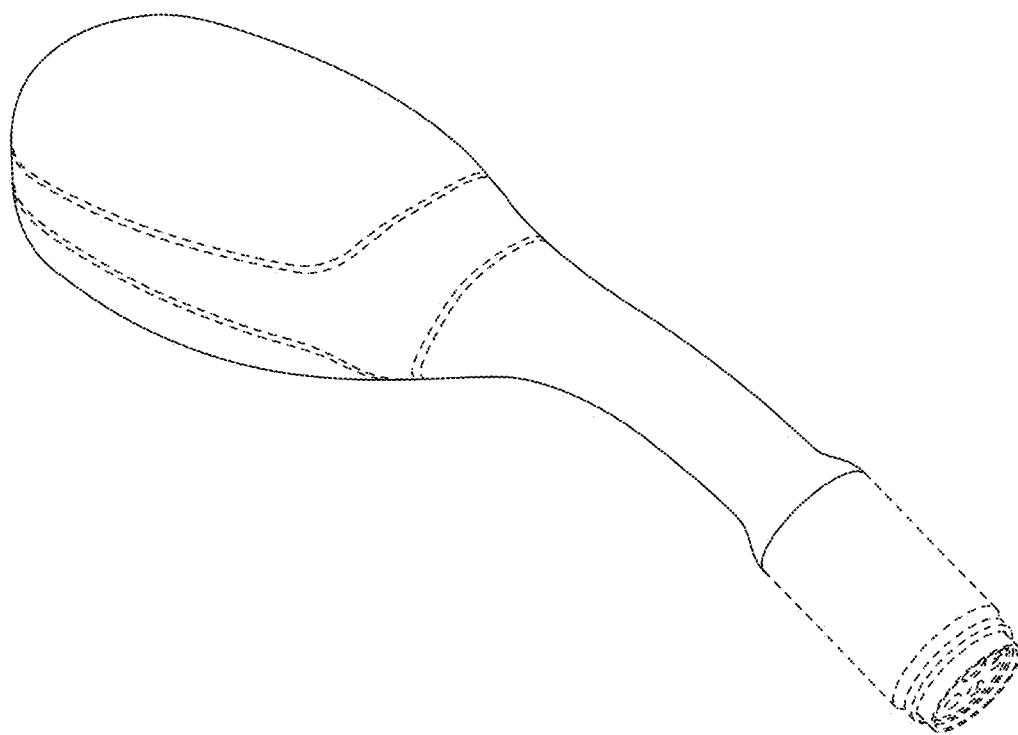


FIG. 1

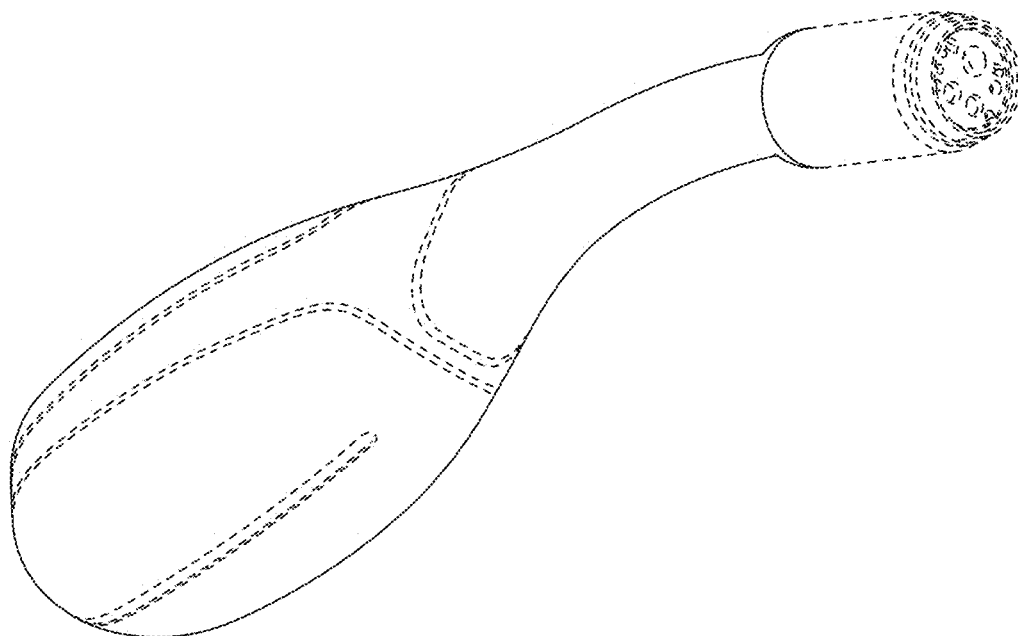


FIG. 2

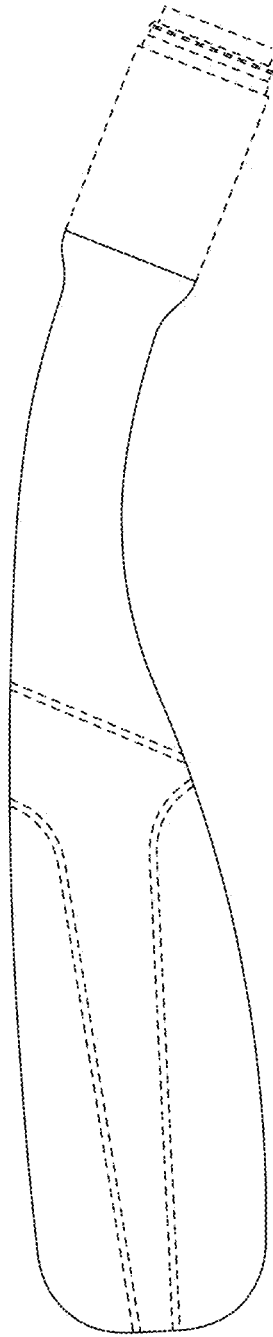


FIG. 3

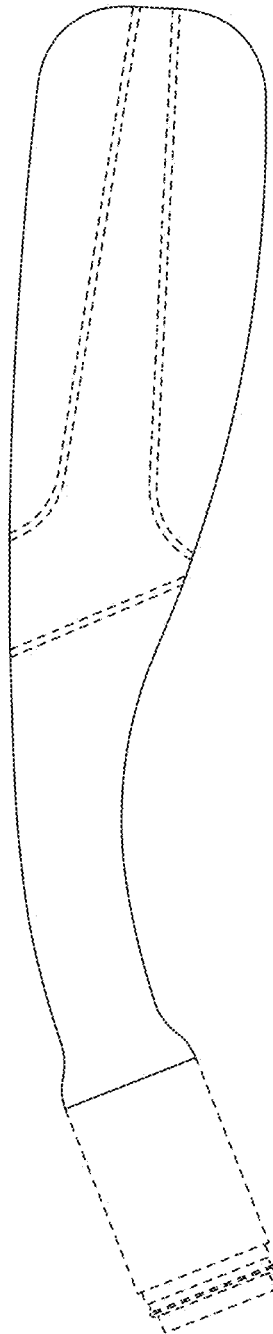


FIG. 4

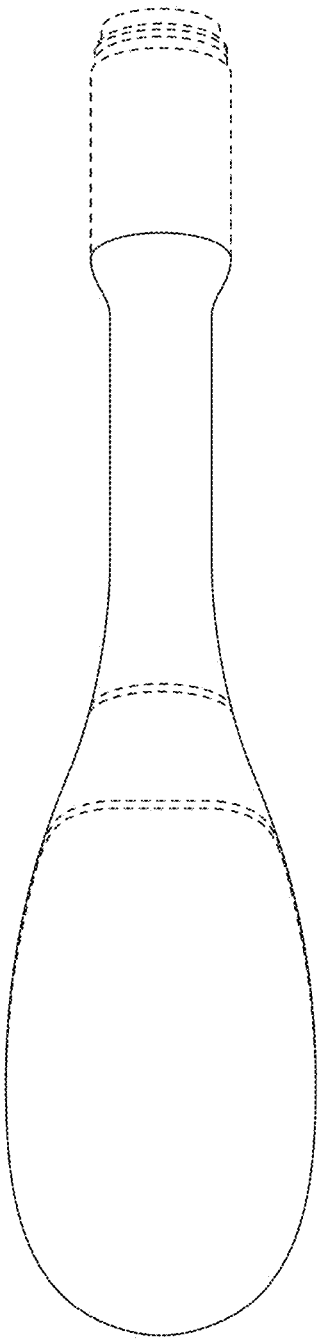


FIG. 5

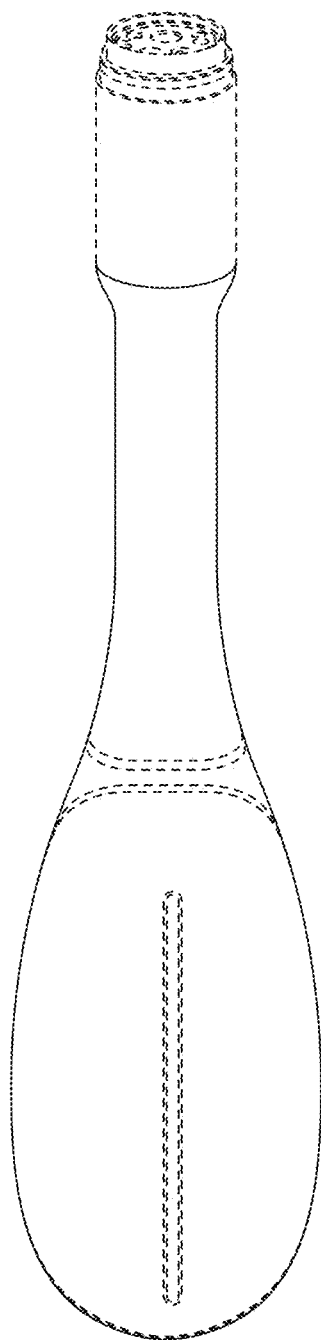


FIG. 6

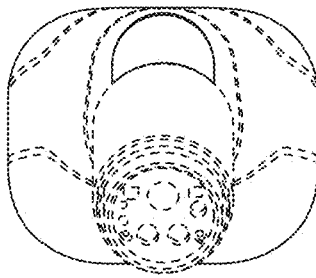


FIG. 7

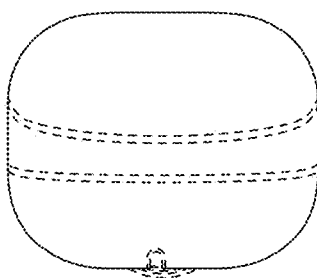


FIG. 8