

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
7 May 2009 (07.05.2009)

PCT

(10) International Publication Number  
WO 2009/059220 A1

(51) International Patent Classification:  
A61M 25/00 (2006.01)

(74) Agent: WIGHT, Todd, W.; Rutan & Tucker LLP, 611 Anton Boulevard, Suite 1400, Costa Mesa, CA 92626 (US)

(21) International Application Number:  
PCT/US2008/082106

(22) International Filing Date: 31 October 2008 (31.10.2008)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:  
12/262,820 31 October 2008 (31.10.2008) US  
60/984,661 1 November 2007 (01.11.2007) US

(71) Applicant (for all designated States except US): C.R. BARD, INC. [US/US]; 730 Central Avenue, Murray Hill, NJ 07974 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): MOEHLE, Ryan, T. [US/US]; 1036 East 4895 South, Salt Lake City, UT 84117 (US). BARRON, William, R. [US/US]; 12124 South 4250 West, Riverton, UT 84065 (US). SANDERS, Scott, W. [US/US]; 955 East 1960 North, Lehi, UT 84043 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with international search report



WO 2009/059220 A1

(54) Title: CATHETER ASSEMBLY INCLUDING TRIPLE LUMEN TIP

(57) Abstract: A catheter assembly for use in accessing a vasculature of a patient during renal replacement or other therapies is disclosed. The catheter assembly includes a catheter body that defines first and second lumens. The catheter body defines a distal tip region that includes a venous lateral opening that is in fluid communication with the first lumen and includes a distal-facing portion. The distal tip region further includes an arterial lateral opening that is in fluid communication with the second lumen, includes a distal-facing portion, and is substantially un-staggered with respect to the venous lateral opening. A distal end opening is defined on the distal tip region and is sized to pass a fluid therethrough. In one embodiment, the distal end opening is in fluid communication with a third lumen of the catheter body that can withstand high fluid flow rates associated with power injection of contrast media.

**CATHETER ASSEMBLY INCLUDING TRIPLE LUMEN TIP****CROSS-REFERENCE TO RELATED APPLICATIONS**

**[01]** This application claims the benefit of priority to U.S. Patent Application No. 12/262,820, filed October 31, 2008, and entitled “Catheter Assembly Including Triple Lumen Tip,” as well as to U.S. Provisional Patent Application No. 60/984,661, filed November 1, 2007, and entitled “Catheter Assembly Including Triple Lumen Tip,” each of which is incorporated herein by reference in its entirety.

**BRIEF SUMMARY**

**[02]** Briefly summarized, embodiments of the present invention are directed to a catheter assembly for use in accessing a vasculature or other vessel of a patient during renal replacement or other suitable therapies. In one embodiment, the catheter assembly includes a catheter body that defines at least first and second lumens. The catheter body defines a distal tip region that includes at least one venous lateral opening that is in fluid communication with the first lumen and includes a distal-facing portion, and at least one arterial lateral opening that is in fluid communication with the second lumen and includes a distal-facing portion. The at least one arterial lateral opening is opposingly positioned in a substantially un-staggered configuration with respect to the at least one venous lateral opening. A distal end opening is defined on the distal tip region and is sized to pass a fluid therethrough. In one embodiment, the distal end opening is in fluid communication with a third lumen of the catheter body that can withstand high fluid flow rates associated with power injection of contrast media, for instance.

**[03]** In another embodiment, a catheter assembly including a catheter body defining a first lumen and a second lumen is disclosed. The catheter body includes a distal tip region, which in turn includes a nose portion that defines a distally converging outer surface. A venous lateral opening, in fluid communication with the first lumen, is partially defined on the distally converging outer diameter. An arterial lateral opening, in fluid communication with the second lumen, is also partially defined on the distally converging outer diameter. The venous and arterial lateral openings are symmetrically disposed in a substantially un-staggered position with respect to one another. The distal tip portion further includes a distal end opening in fluid communication with one of the venous and arterial lumens and is sized to pass a guidewire therethrough.

[04] These and other features of the present invention will become more fully apparent from the following description and appended claims, or may be learned by the practice of the invention as set forth hereinafter.

#### **BRIEF DESCRIPTION OF THE DRAWINGS**

[05] To further clarify the above and other advantages and features of the present invention, a more particular description of the invention will be rendered by reference to specific embodiments thereof that are illustrated in the appended drawings. It is appreciated that these drawings depict only typical embodiments of the invention and are therefore not to be considered limiting of its scope. The invention will be described and explained with additional specificity and detail through the use of the accompanying drawings in which:

[06] FIG. 1 is a perspective view of a catheter assembly incorporating various features of an embodiment of the present invention;

[07] FIG. 1A is a perspective view of another example of a catheter assembly configured according to one embodiment;

[08] FIG. 2 is a perspective view of a distal tip region of the catheter assembly shown in FIG. 1, configured according to one embodiment;

[09] FIG. 3 is a side view of the catheter distal tip region of FIG. 2;

[010] FIG. 4 is a top view of the catheter distal tip region of FIG. 2;

[011] FIG. 5 is an end view of the catheter distal tip region of FIG. 2;

[012] FIG. 6 is a perspective view of the catheter distal tip region of FIG. 2, depicting various details of lateral openings defined therein;

[013] FIG. 7A is a cross sectional view of the catheter assembly and distal tip region of FIG. 2, showing the flow of blood therethrough in a “forward” flow configuration;

[014] FIG. 7B is a cross sectional view of the catheter assembly and distal tip region of FIG. 2, showing the flow of blood therethrough in a “reverse” flow configuration;

[015] FIG. 8A is a cross sectional view of the catheter assembly, taken along the line 8A—8A in FIG. 4;

[016] FIG. 8B is another cross sectional view of the catheter tip, taken along the line 8B—8B in FIG. 4;

[017] FIG. 8C is yet another cross sectional view of the catheter tip, taken along the line 8C—8C in FIG. 4;

[018] FIG. 8D is yet another cross sectional view of a distal tip region of the catheter assembly showing positioning of a third lumen thereof in accordance with one embodiment;

[019] FIGS. 9A-9F depict various views of a catheter assembly including a distal tip region configured in accordance with one embodiment;

[020] FIGS. 10A-10D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment;

[021] FIGS. 11A-11D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment;

[022] FIGS. 12A-12D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment;

[023] FIGS. 13A-13D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment;

[024] FIGS. 14A-14D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment;

[025] FIGS. 15A-15D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment;

[026] FIGS. 16A-16D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment;

[027] FIGS. 17A-17D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment;

[028] FIGS. 18A-18D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment;

[029] FIGS. 19A-19D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment; and

[030] FIGS. 20A-20D are perspective, front, side, and top views, respectively, of a catheter including a distal tip region configured in accordance with one embodiment.

#### **DETAILED DESCRIPTION OF SELECTED EMBODIMENTS**

[031] Reference will now be made to figures wherein like structures will be provided with like reference designations. It is understood that the drawings are diagrammatic and schematic representations of example embodiments, and are not limiting of the embodiments nor are they necessarily drawn to scale.

[032] FIGS. 1-20D depict various features of embodiments of the present invention, which are generally directed to an acute catheter assembly for use in accessing a vasculature or other vessel of a patient during renal replacement therapies such as hemodialysis or blood purification, though the principles of the present invention may be extended to other catheters employed in other uses in addition to these. Such acute catheters are typically employed in short-term placement scenarios such as a placement of less than 30 days, though the principles to be described herein can also apply to mid-term and long term catheter placements as well.

[033] In accordance with one example embodiment, the catheter assembly includes a distal tip region defining separate venous and arterial lateral openings, in fluid communication with corresponding venous and arterial lumens that are employed for simultaneously infusing and aspirating blood from a vein or other vessel of a patient's vasculature during hemodialysis treatments. The venous and arterial lateral openings are disposed in a substantially equivalent, non-staggered position with respect to one another so as to enable positioning thereof in a predetermined region of the vasculature. This notwithstanding, the lateral openings are configured to reduce the likelihood of recirculation by the arterial segment of treated blood just returned to the vessel by the venous segment, thus increasing catheter efficiency. Moreover, the lateral openings can be operated in a reverse flow configuration without significantly impacting catheter efficiency during hemodialysis.

**[034]** Embodiments of the catheter assembly to be described herein further include a distal end opening in fluid communication with a lumen of the catheter configured to withstand relatively high pressure and flow rates typically associated with power injection. This enables aspiration or infusion of fluids to occur via this lumen independently of the venous and arterial lumens. “Power injection” is defined herein to include fluid infusion under relatively high flow rates and/or relatively high pressures. For instance, in one embodiment power injection includes fluid infusion through a catheter lumen at a flow rate of between about three and about eight milliliters per second, and/or at a pressure of between about 50 and about 250 psi.

**[035]** For clarity it is to be understood that the word “proximal” refers to a direction relatively closer to a clinician using the device to be described herein, while the word “distal” refers to a direction relatively further from the clinician. For example, the end of a catheter placed within the body of a patient is considered a distal end of the catheter, while the catheter end remaining outside the body is a proximal end of the catheter. Further, the words “including,” “has,” and “having,” as used herein, including the claims, shall have the same meaning as the word “comprising.”

**[036]** Reference is first made to FIG. 1, which depicts various features of a hemodialysis catheter assembly, generally designated at 10, according to one example embodiment. As shown, the catheter 10 includes an elongate catheter body 11 including a proximal end 11A and a distal end 11B. The elongate catheter body 11 defines a first lumen 12, a second lumen 14, and a third lumen 15 (FIG. 7A) that longitudinally extend from the proximal end 11A to the distal end 11B thereof. The lumens 12, 14, and 15 can have one or more cross sectional shapes along their respective lengths, including round, oval, D-cross sectional shapes, or any combination thereof. In one embodiment, the first and second lumens 12, 14 are sized so as to accommodate fluid flow rates required for hemodialysis, *i.e.*, about 300 milliliters/min. at about 250 millimeters Hg pressure. In one embodiment, the third lumen is sized with a diameter of about .035 to about .038 inch to accommodate blood draws and fluid aspiration/infusion therethrough.

**[037]** A trifurcating hub 20 is included at the catheter body proximal end 11A, providing fluid communication between the first, second, and third lumens 12, 14, 15 and arterial extension leg 16, venous extension leg 18, and power extension leg 19, respectively. The extension legs 16, 18, 19 each include a luer connector 16A, 18A,

19A, and a clamp 16B, 18B, 19B. So configured, the extension legs 16, 18 provide fluid communication with the first and second lumens 12 and 14 so as to enable the infusion or aspiration of fluids from the central venous system of a patient. As such, fluid infusion or aspiration devices, such as a hemodialysis apparatus for example, may be connected to the catheter assembly 10 via the luer connectors 16A, 18A, thus providing intravascular access to the patient. Similarly, the extension leg 19 provides fluid communication with the third lumen 15 to enable fluid infusion/aspiration from the vein when a corresponding device is connected thereto via the connector 19A. Note that the respective positions and configurations of the extension legs detailed here can change according to a particular catheter assembly design and therefore not be viewed as limiting. The catheter body 11 further includes a suture wing 21 for providing securement of the catheter body to the patient.

**[038]** FIG. 2 shows the catheter assembly 10 according to another example embodiment, wherein the extension legs 16, 18 each include a pre-curved portion 16C, 18C. The pre-curved portions 16C, 18C enable the extension legs 16, 18 of the catheter assembly 10 to extend downward against the patient's body once the distal portion of the catheter assembly has been placed in the vasculature to provide patient comfort.

**[039]** In greater detail, the power extension leg 19 of FIGS. 1 and 2 fluidly connects to the third lumen 15 via the trifurcating hub 20. In particular, the power extension leg 19 is configured in one embodiment to enable rapid infusion, *i.e.*, power injection, of contrast media, useful for contrast-enhanced CT scan imaging, or other fluids into the patient vessel via the third lumen 15. Specifically, in one embodiment, the power extension leg 19 and third lumen 15 are configured to infuse fluids at a rate of between about 3 milliliters and about 8 milliliters per second and at a fluid pressure of between about 50 and 250 psi, though other flow rates and fluid pressures may also be possible. The power extension leg 19 and third lumen 15 can also be used to remove blood or other fluids alone or during simultaneous use of the first and second lumens 12 and 14, and to monitor central venous pressure with the assistance of a transducer. The power extension leg 19 and third lumen 15 are also sufficiently sized to receive a guidewire therethrough to enable insertion of the catheter assembly over the guidewire. Note that the components of the power extension leg 19 are colored purple in one embodiment to indicate power injectability. Other colors could also be used.

**[040]** Both FIGS. 1 and 2 further include a distal tip region, generally designated at 50, that is configured in accordance one example embodiment of the present invention, the details of which are given below. It should be appreciated that the distal tip region to be described below can be included with hemodialysis catheters, such as those shown in FIGS. 1 and 2, or with other catheters, such as central venous catheters, for example. Indeed, the catheter assembly according to embodiments of the present invention can be adapted for use in other applications, such as chronic dialysis treatment, or where access is desired to be gained to a vessel, such as the internal jugular, subclavian, or femoral vessels, or other body lumen of a patient. Examples of such other applications include apheresis, hemoperfusion, etc.

**[041]** Reference is now made to FIGS. 2-6, which show various views of a distal tip region, generally designated at 50, of the catheter assembly 10 and configured according to one example embodiment. In detail, the distal tip region 50 generally includes a terminal catheter portion 50A and a nose portion 50B disposed distally of the terminal catheter portion to define a distal end of the catheter assembly 10. The terminal catheter portion 50A, as part of the more proximal portion of the catheter body 11, is composed of suitable material(s) that exhibit qualities, such as suitable softness to allow for ease of insertion without causing vessel trauma, and biocompatibility for enabling the catheter to operate as intended. In one embodiment, the catheter body 11 is composed of material(s) including a thermoplastic polyurethane-based resin material, specifically a polyether-based, aliphatic thermoplastic polyurethane sold under the trademark TECOFLEX, namely TECOFLEX EG-60D-B20, having a Shore D hardness of approximately 60, where “B20” refers to the radiopacifier loading, *i.e.*, barium sulfate loading at 20%. Other suitable materials can also be employed.

**[042]** In contrast, the nose portion 50B includes a material relatively softer than that of the terminal catheter portion 50A so as to prevent the tip portion from damaging the vessel or other vasculature during vessel entry or transit. In one embodiment, the nose portion 50B is composed of material(s) including TECOFLEX EG-85A-B20 having a Shore A hardness of approximately 85. Notwithstanding the above description, it should be appreciated that the terminal catheter portion and the nose portion can include other materials having the desired properties as described herein and as appreciated by one skilled in the art. One non-limiting example of material that can be used for the terminal catheter portion and nose portion is silicone.

**[043]** Note that in the illustrated embodiment, the nose portion 50B is joined to the terminal catheter portion 50A via a molding process during manufacture of the catheter assembly 10. In other embodiments, however, other processes for joining the nose portion to the catheter body can be employed, including for instance RF fusion (RF tipping), bonding via adhesive, integrally forming the nose portion with the catheter body, etc.

**[044]** As best seen in FIGS. 3 and 4, the nose portion 50B is distally converging. In the present embodiment, the nose portion 50B is tapered so as to ease entry and passage of a distal portion of the catheter body 11 into the vasculature or other internal cavity of a patient. The nose portion 50B may be colored differently from the remainder of the catheter body 11 to indicate that the catheter assembly 10 can be employed for relatively rapid fluid aspiration and infusion via the third lumen 15 and corresponding power extension leg 19, as was described further above.

**[045]** The distal tip region 50 includes various openings for enabling the infusion and aspiration of fluids while the catheter assembly 10 is placed for use within the patient vasculature. Specifically, and in accordance with one embodiment, the distal tip region includes a venous lateral opening 60, an arterial lateral opening 62, and a distal end opening 64.

**[046]** In greater detail, the venous and arterial lateral openings 60 and 62 are positioned opposite one another proximate the catheter body distal end 11B and are defined in a lateral portion of an outer wall of the catheter body 11 so as to be in fluid communication with first lumen 12 and the second lumen 14, respectively, thus enabling blood or other fluids to flow via the openings to/from the lumens when the catheter assembly 10 is positioned within the patient's vasculature. The venous and arterial lateral openings 60 and 62 are defined by perimeters 60A and 62A, respectively, as best seen in FIG. 4 and described further below.

**[047]** Note that each of the lateral openings 60 and 62 distally extends from the terminal catheter portion 50A into the nose portion 50B. Of course, the exact placement of the lateral openings 60 and 62 along the longitudinal length of the catheter body 11 can vary according the needs of a particular application.

**[048]** FIG. 4 shows that in the present embodiment the venous and arterial lateral openings 60 and 62 are substantially un-staggered, *i.e.*, equally placed with respect to one another along the longitudinal length of the catheter body 11 such that each is substantially disposed an equal distance from the distal catheter end 11B. Such un-staggered disposal of the lateral openings 60 and 62 enables both openings to be placed proximate a desired location within the vasculature and ensures that the recirculation rate of already treated blood through the catheter assembly 10 is held relatively constant regardless the respective directions of blood travel in/out of the lateral openings. This feature is useful should reversal of blood flow directions through the catheter be necessary. In one embodiment, the recirculation rate in either direction is less than or equal to about five percent. In another embodiment, the venous and lateral openings can be staggered.

**[049]** FIGS. 2-6 further show the manner in which the venous and lateral openings 60 and 62 are defined in the distal tip region 50. The lateral openings 60 and 62 can take various shapes and configurations as will be shown further below, but in the present embodiment the lateral openings are defined by angled cross-drilled cuts through the outer wall of the catheter body 11 to establish communication with the respective first or second lumens 12, 14. In one embodiment, such cuts are referred to as “skive” cuts.

**[050]** In one embodiment, a long axis of each cross-drilled cut of the lateral openings 60, 62 defines in one embodiment an angle  $\theta_1$  of about 35 degrees with a longitudinal axis of the catheter body 11, though this angle can vary in one embodiment from about greater than zero to about 90 degrees. This angular character imparts both a lateral and distal directional component to fluid flow out of either lateral opening 60, 62, as represented by the flow arrows in FIG. 4, which assists in enabling low-recirculation fluid flow out of or into either lateral opening. Each lateral opening 60 and 62 in the present embodiment is defined by identical cross cuts having the same angle  $\theta_1$  with respect to the longitudinal axis 70, though it is also possible to vary the angle generally, or to vary the angle differently for each opening.

**[051]** In one embodiment, the lateral openings can be defined by a compound-angle cross cut, wherein the long axis of each lateral opening defines an angle with the catheter body longitudinal axis and with a plane dividing the first lumen and the second lumen,

*i.e.*, coplanar with the septum separating the first and second lumens proximal of the distal tip region.

**[052]** An end view of the cross cut, depicted in FIG. 6, shows that the cross cut of each opening 60 and 62 in the illustrated embodiment is made so as to generally define a semicircular cavity through a peripheral portion of the distal tip region 50. This cavity is defined by a portion of a circle 72 having a radius “R,” shown in FIG. 6. In the present embodiment, the cross cut that defines the lateral openings 60 or 62 is achieved via use of a cylindrical drill bit or coring tool having a radius equal to the radius R of the circle 72 and cutting through the distal tip region 50 set at the angle  $\theta_1$ . For instance, in one embodiment a drill bit having a radius of 1/16 inch is used to diagonally cross cut the venous and arterial lateral openings 60 and 62 through a catheter body defining an oblong cross section, wherein the average of the major and minor diameters is approximately 0.173 inches. Note that the catheter body size in one embodiment can vary from 7-16 Fr., though other French sizes are also possible. Though shown in connection with the venous lateral opening 60, the above description applies to the arterial opening 62 as well. Note here that, though identically sized and shaped in the present embodiment, the first and second openings could have respectively differing dimensions if desired or needed for a particular application.

**[053]** As a result of defining the cross cuts as just described, the venous and arterial openings 60 and 62 are defined by their respective perimeters 60A and 62A discussed above. The angle at which the cross cuts are made, together with the shape of the catheter body 11 at the point of the cuts, results in the perimeters 60A and 62A shaped as seen in the accompanying figures. As best seen in FIG. 4, each perimeter 60A and 62A defines in the present embodiment a figure-eight shape, or analemma, when viewed in a two-dimensional perspective and an elongate saddle shape when viewed in a three-dimensional perspective. Further, because a distal portion of each opening 60 and 62 is defined on a portion of the tapered nose portion 50B (best seen in FIGS. 4 and 5), each opening has a distal-facing component, best seen in FIG. 5, wherein a portion each lateral opening is distally visible.

**[054]** The configuration of the venous and arterial lateral openings 60 and 62 described above provides various aspects for the catheter assembly 10. First, because of their saddle shapes, the lateral openings 60 and 62 partially extend circumferentially

about the outer perimeter of the catheter body 11. This helps to prevent undesired suctioning of the distal tip region 50 to the vessel wall when one of the openings is removing blood from the vessel as the negative flow pressure of the opening is distributed about a portion of the catheter body circumference. If vessel suck-up does occur, the lateral openings 60, 62 are shaped so as to nonetheless provide acceptable fluid flow in and out of the catheter assembly 10. The relatively large size of the lateral openings 60 and 62 also assists in the prevention of occlusion or sheath formation and provides a fanned-out or wide distribution of fluid flowing out therefrom. Recirculation efficiency rates are improved as a result.

**[055]** Second, the distal-facing aspect of each lateral opening 60 and 62 assists in imparting a distal direction to fluids being ejected therefrom. This enables the ejected fluid to distally flow away from one respective lateral opening and distal-to proximal flow into the other lateral opening even when the catheter body 11 is positioned against a vessel wall. In addition, the lateral openings 60, 62 are symmetrically opposed, in direction from one another, *i.e.*, a 180-degree separation as best shown in FIG. 4, so as to ensure fluid entry and exit from the lateral openings occurs on opposite sides of catheter assembly 10, further reducing recirculation. Furthermore, this symmetric positioning produces a “criss-cross” relationship between the lateral openings 60 and 62, as best seen in FIG. 3, which assists in reducing recirculation. Moreover, similar fluid flow characteristics are realized even when fluid flow through the catheter assembly 10 is reversed, as discussed further below. In addition, the lateral opening configuration described herein minimizes radical redirection of the fluid upon exiting the catheter body 11 via either of the lateral openings 60 or 62, which in turn prevents fluid turbulence and possible clotting or hemolysis.

**[056]** As shown in FIGS. 2-6, the distal end opening 64 is distally located at the distal end of the distal tip region nose portion 50 and is in fluid communication with the third lumen 15 so as to enable high flow rate infusion, *i.e.*, power injection of contrast media or other fluids such as TPN nutritional fluid and medications into the vessel, as well as the removal of blood from the vessel during catheter use. In the case of infusion of contrast media or medications into the vessel, placement of the distal end opening 64 distally of the first and second openings 60 and 62 advantageously results in minimization of contrast media/medication intake into either of the first or second

openings if the infusion takes place simultaneously with fluid passage through the venous and arterial openings 60 and 62, such as during hemodialysis or other treatments.

**[057]** Note that, in one embodiment a guidewire can be inserted through the distal end opening 64, the third lumen 15, and the power extension leg 19 during initial or exchange catheter placement in the patient vasculature. Also note that the relatively proximate placement of the three openings 60, 62, and 64 in the distal portion of the catheter body 11 enables each opening to be placed near desired location within the vasculature, such as the superior vena cava (“SVC”).

**[058]** Reference is now made to FIGS. 7A and 7B in describing flow characteristics with respect to the configuration of the distal tip region 50 of the catheter assembly 10 according to the present embodiment. FIGS. 7A and 7B show the distal tip region 50 after the catheter assembly 10 has properly positioned within a vessel of a patient. Arrow 84 shows the direction of blood flow past the distal tip region 50 within the patient’s vessel.

**[059]** In greater detail, FIG. 7A shows fluid flow through the distal tip region 50 in a “forward” direction, wherein blood is aspirated by the second lumen 14, or “uptake” lumen, for removal from the body and treatment by a hemodialysis apparatus or for some other suitable purpose. Aspirated blood enters the second lumen 14 via the arterial lateral opening 62 of the distal tip region 50. Similarly, blood is infused, or returned, to the vessel by the first lumen 12, or “return” lumen, after treatment by a hemodialysis apparatus or some other suitable purpose. Infused blood exits the first lumen 12 from the venous lateral opening 60. Note that the lateral orientation of the venous and arterial lateral openings 60, 62 provides for low recirculation of already-treated blood within the vessel, recirculation being defined as already-treated blood that is returned to the bloodstream via the venous lumen being immediately aspirated by the arterial lumen to be re-treated. Such recirculation is undesirable as it results in lower treatment efficiency, resulting in longer treatment time.

**[060]** During hemodialysis procedures, it is sometimes necessary to reverse the blood flow through the catheter assembly 10. FIG. 7B shows fluid flow through the distal tip region 50 during such a “reverse” flow situation. In contrast to the forward flow conditions of FIG. 7A, the second lumen 14 in FIG. 7B is employed to infuse blood into the vessel while the first lumen 12 aspirates blood from the vessel. In this

configuration, the infused blood enters the vessel via the arterial lateral opening 62, while the aspirated blood is removed via the venous lateral opening 60. Again, the lateral orientation of the venous and arterial lateral openings 60, 62 provides for low recirculation of already-treated blood within the vessel. Thus, it is seen that low recirculation results regardless of the direction in which the catheter is operating.

**[061]** FIGS. 7A and 7B further show that fluid can be aspirated or infused via the distal end opening 64 in fluid communication with the third lumen 15 before, after, or during infusion/aspiration by the venous and arterial lateral openings 60, 62. As mentioned, the third lumen 15 and distal end opening 64 are configured so as to withstand relatively high pressurized fluid flow infusion into the vessel. It is appreciated that in other embodiments, more than one of the catheter lumens can be configured for high pressurized fluid flow infusion, if desired.

**[062]** It should be appreciated that the labels “venous” and “arterial” as used above in describing the various components of the present catheter assembly are employed for sake of convenience in describing aspects of present embodiments. Indeed and as just described, though the arterial lateral opening is normally employed in hemodialysis procedures for aspirating blood from the blood vessel in which the catheter is disposed and the venous lateral opening for returning already treated blood to the vessel, this can be reversed such that blood is returned via the arterial lateral opening and aspirated by the venous lateral opening. As such, embodiments of the present invention should not be considered limited by the use of this and other descriptive terminology herein.

**[063]** Reference is now made to FIGS. 8A-8C, which depict various details regarding the catheter body 11. In detail, FIG. 8A shows a cross sectional view of the catheter body 11 at a point proximal to the distal tip region 50, showing the first lumen 12, the second lumen 14, and the third lumen 15. The three lumens 12, 14, 15 are defined along the longitudinal length of the catheter body 11 and bounded by an outer perimeter or wall 86. The outer wall 86 of the catheter body 11 in the present embodiment defines an oblong shape and includes a transverse axis 88 that intersects the first and second lumens 12, 14 and spans the width of the catheter body. Placement of the first and second lumens 12, 14 adjacent one another, with the third lumen 15 positioned therebelow, provides a robust lumen configuration that resists inadvertent closure of lumens via kinking of the catheter body 11. In addition, the oblong cross

sectional configuration of the catheter body 11 enables circular cross sectional shapes to be employed for the lumens 12, 14, and 15, which are relatively more efficient than “D”-shaped or other shaped lumens in terms of fluid flow.

**[064]** As seen in FIG. 8B and as previously described, the venous lateral opening 60 is defined so that it intercepts the first lumen 12, while the arterial lateral opening is defined so that it intercepts the second lumen 14. As such, the first lumen 12 establishes fluid communication between the venous extension leg 18 and the venous lateral opening 60, while the second lumen 14 establishes fluid communication between the arterial extension leg 16 and the arterial lateral opening 62. In one embodiment, the angled cross cuts that define the venous and arterial openings 60 and 62 are made tangentially with respect to a septum 90 separating the first and second lumens 12, 14 such that the septum wall remains intact as a barrier between the two lumens.

**[065]** FIGS. 8A-8C successively depict the manner in which the third lumen is raised from a bottom-central location along the length of the catheter body 11 to a central position upon its exit at the distal end opening 64, as shown in FIG. 5. Of course, other lumen position configurations are also possible.

**[066]** It is appreciated that various modifications may be made to the catheter assembly configurations described above. It is noted that for purposes of clarity, only selected differences between the foregoing and following embodiments are described. For instance, FIGS. 9A-9F depict a distal tip region 150 including a terminal catheter portion 150A integrally formed with the catheter body 11 and a nose portion 150B including a relatively low hardness, *e.g.*, soft, material and joined to the terminal catheter portion 150A in a manner similar to that already described above in connection with FIGS. 2-6.

**[067]** The distal tip region 150 defines a venous lateral opening 160 in fluid communication with the first lumen 12 and an arterial lateral opening 162 in fluid communication with the second lumen 14. A distal end opening 164 is also defined at a distal end of the nose portion 150B. The catheter assembly as configured in FIGS. 9A-9F is a dual lumen device in that it includes only two lumens 12 and 14 (FIG. 9E). As best seen in FIG. 9F, therefore, the distal end opening 164 does not communicate with a third lumen, but rather with a guidewire channel 164A defined by the nose portion 150B, which in turn communicates with the first lumen 12. In this way, a guidewire pathway is

established through the catheter body 11 and distal tip region 150 to enable the catheter assembly to be inserted over a guidewire during initial placement and catheter exchange procedures.

**[068]** FIG. 9E depicts a cross sectional view of the catheter body proximal of the distal tip region 150. As shown, top and bottom portions of an outer wall 186 of the catheter body 11 include thickened regions 186A, which provide added kink resistance to the catheter body.

**[069]** By virtue of its communication with the first lumen 12, the guidewire channel 164A provides an added fluid outlet/inlet for the first lumen via the distal end opening 164, thus providing an additional fluid pathway that further reduces recirculation during operation of the catheter. This fluid communication also maintains the guidewire channel 164A patent via the flow of blood therethrough so as to prevent occlusion thereof. Further note that, though it is centrally located at the distal end of the nose portion 150B, the venous lateral opening 164 can be positioned such that it and the corresponding guidewire channel 164A are in longitudinal linear alignment with the first lumen 12. Further, the venous lateral opening and the corresponding guidewire channel can be configured as to be in communication with the second lumen or both the first and second lumens, if desired.

**[070]** FIGS. 10A-10D and 11A-11D are further examples of a dual lumen catheter assembly configuration, in accordance with example embodiments thereof. The distal tip regions 250/350 each include a terminal catheter portion 250A/350A and a nose portion 250B/350B at which are defined a venous lateral opening 260/360, an arterial lateral opening 262/362, and a distal end opening 264/364. A guidewire channel 264A/364A is defined between the distal end opening 264/364 to the first lumen 12 so as to be in communication therewith. As can be seen in comparison, the lateral openings 260, 262 of FIGS. 10A-10D are differently shaped from corresponding lateral openings 360, 362 of FIGS. 11A-11D. Further, the nose portion 250B (FIG. 10A) is distally converging in a tapered configuration, whereas the nose portion 350B (FIG. 11A) distally converges in a rounded configuration to define a bullet-shape. Note also that the venous and arterial lateral openings of the dual lumen embodiments describe herein include distal-facing portions, as best seen in FIGS. 10B and 11B, offering characteristics similar to those outlined above in connection with the discussion relating to FIGS. 2-6.

[071] FIGS. 12A-20D depict possible configurations of a catheter assembly distal tip region including three lumens, according to additional example embodiments. As they share aspects with the embodiment described above in connection with FIGS. 2-7B, only selected aspects of the embodiments to follow will be discussed below.

[072] FIGS. 12A-12D depicts a catheter assembly distal tip region 450, including a terminal catheter portion 450A and a nose portion 450B. The distal tip region 450 further includes a venous lateral opening 460 in fluid communication with the first lumen 12 and an arterial lateral opening 462 in fluid communication with the second lumen 14. A distal end opening 464 is also defined at a distal end of the nose portion 450B. In the present embodiment, the lateral openings 460 and 462 each define a trapezoidal perimeter when viewed from the perspective of FIG. 12D, and are symmetrically opposed from one another.

[073] FIGS. 13A-13D depicts a catheter assembly distal tip region 550, including a terminal catheter portion 550A and a nose portion 550B. The distal tip region 550 further includes a venous lateral opening 560 in fluid communication with the first lumen 12 and an arterial lateral opening 562 in fluid communication with the second lumen 14. A distal end opening 564 is also defined at a distal end of the nose portion 550B. In the present embodiment, the lateral openings 460 and 462 each define a stepped perimeter when viewed from the perspective of FIG. 13D, and are symmetrically opposed from one another.

[074] FIGS. 14A-14D depict a catheter assembly distal tip region 650, including a terminal catheter portion 650A and a nose portion 650B. The distal tip region 650 further includes a venous lateral opening 660 in fluid communication with the first lumen 12 and an arterial lateral opening 662 in fluid communication with the second lumen 14. A distal end opening 664 is also defined at a distal end of the nose portion 650B and is axially offset from a central axis of the catheter body 11. In the present embodiment, the lateral openings 660 and 662 each define an oval perimeter when viewed from the perspective of FIG. 12C, and are symmetrically opposed from one another, as best seen in FIG. 14D.

[075] FIGS. 15A-15D depict a catheter assembly distal tip region 750, including a terminal catheter portion 750A and a nose portion 750B. The distal tip region 750 further includes a venous lateral opening 760 in fluid communication with the first lumen

12 and an arterial lateral opening 762 in fluid communication with the second lumen 14. A distal end opening 764 is also defined at a distal end of the nose portion 750B and is axially offset from a central axis of the catheter body 11. In the present embodiment, the lateral openings 760 and 762 each define an oval perimeter when viewed from the perspective of FIG. 15C, and are symmetrically opposed from one another, as best seen in FIG. 15D.

**[076]** FIGS. 16A-16D depict a catheter assembly distal tip region 850, including a venous lateral opening 860 in fluid communication with the first lumen 12 and an arterial lateral opening 862 in fluid communication with the second lumen 14. A distal end opening 864 is also defined at a distal end of the distal tip region 850 and is axially offset from a central axis of the catheter body 11. In the present embodiment, the lateral openings 860 and 862 are separated by a septum 890, and each defines a partial oval perimeter when viewed from the perspective of FIG. 16C, and are symmetrically opposed from one another, as best seen in FIG. 16D.

**[077]** FIGS. 17A-17D depict a catheter assembly distal tip region 950, including a venous lateral opening 960 in fluid communication with the first lumen 12 and an arterial lateral opening 962 in fluid communication with the second lumen 14. A distal end opening 964 is also defined at a distal end of the distal tip region 850 and is axially offset from a central axis of the catheter body 11. In the present embodiment, the lateral openings 960 and 962 are separated by a septum 990, and each defines an acute angle-shaped perimeter together with a portion of an outer catheter body wall 986 when viewed from the perspective of FIG. 16C. As before, the lateral openings 960, 962 are symmetrically opposed from one another, as best seen in FIG. 17D.

**[078]** FIGS. 18A-18D depict a catheter assembly distal tip region 1050, including a terminal catheter portion 1050A and a nose portion 1050B. The distal tip region 1050 further includes a venous lateral opening 1060 in fluid communication with the first lumen 12 and an arterial lateral opening 1062 in fluid communication with the second lumen 14. A distal end opening 1064 is also defined at a distal end of the distal tip region nose portion 1050B and is centrally disposed with respect to a central axis of the catheter body 11. In the present embodiment, the lateral openings 1060 and 1062 are separated by a septum 1090, and each defines a partial oval perimeter when viewed from

the perspective of FIG. 18C. As before, the lateral openings 1060, 1062 are symmetrically opposed from one another, as best seen in FIG. 18D.

**[079]** FIGS. 19A-19D depicts a catheter assembly distal tip region 1150, including a nose portion 1150B. The distal tip region 1150 further includes a venous lateral opening 1160 in fluid communication with the first lumen 12 and an arterial lateral opening 1162 in fluid communication with the second lumen 14. A distal end opening 1164 is also defined at a distal end of the nose portion 1150 and is axially offset from a central axis of the catheter body 11. In the present embodiment, the lateral openings 1160 and 1162 each define a triangular perimeter when viewed from the perspective of FIG. 19D, and are symmetrically opposed from one another as best seen in FIG. 19D.

**[080]** FIGS. 20A-20D depict a catheter assembly distal tip region 1250, including a terminal catheter portion 1250A and a nose portion 1250B. The distal tip region 1250 further includes a venous lateral opening 1260 in fluid communication with the first lumen 12 and an arterial lateral opening 1262 in fluid communication with the second lumen 14. A distal opening 1264 is also defined on the nose portion 1250B and is axially offset from a central axis of the catheter body 11. In the present embodiment, the lateral openings 1260 and 1262 are separated by a septum 1290, and each defines a frustoconical perimeter when viewed from the perspective of FIG. 20C. As before, the lateral openings 1260, 1262 are symmetrically opposed from one another, as best seen in FIG. 20D. In addition to the lateral openings 1260, 1262, the terminal catheter portion 1250A further includes a plurality of venous openings 1260A and a plurality of arterial openings 1262A. The openings 1260A, 1262A are relatively smaller than the lateral openings 1260, 1262, and are distributed about the perimeter of the catheter body so as to further reduce the possibility of vessel wall suck-up.

**[081]** Embodiments of the present invention may be embodied in other specific forms without departing from its spirit or essential characteristics. The described embodiments are to be considered in all respects only as illustrative, not restrictive. The scope of the embodiments of the present invention is, therefore, indicated by the appended claims rather than by the foregoing description. All changes that come within the meaning and range of equivalency of the claims are to be embraced within their scope.

What is claimed is:

## CLAIMS

1. A catheter assembly, comprising:  
a catheter body defining at least a first lumen and a second lumen, the catheter body including a distal tip region, the distal tip region including:  
at least one venous lateral opening in fluid communication with the first lumen, the at least one venous lateral opening including a distal-facing portion;  
at least one arterial lateral opening in fluid communication with the second lumen, the at least one arterial lateral opening including a distal-facing portion, the at least one arterial lateral opening being opposingly positioned in about an un-staggered configuration with respect to the at least one venous lateral opening; and  
a distal end opening sized to pass a fluid therethrough.
2. The catheter assembly as defined in claim 1, wherein the at least one venous lateral opening and the at least one arterial lateral opening are symmetrically positioned with respect to one another.
3. The catheter assembly as defined in claim 1, wherein the distal end opening is in communication with a third lumen defined by the catheter body.
4. The catheter assembly as defined in claim 1, wherein the distal end opening is in communication with the first lumen.
5. The catheter assembly as defined in claim 4, wherein a guidewire is passable from the first lumen through the distal end opening via a guidewire channel, the guidewire channel in communication with both the first lumen and the distal end opening.
6. The catheter assembly as defined in claim 1, wherein the at least one venous lateral opening and the at least one arterial lateral opening are defined by an angled cross cut through an outer perimeter of the catheter body.

7. The catheter assembly as defined in claim 1, wherein the first and second lumens define circular cross sectional shapes, wherein the distal end opening is in fluid communication with a third lumen defined by the catheter body, the third lumen defining a circular cross sectional shape, and wherein an outer perimeter of the catheter body defines an oblong cross sectional shape.

8. The catheter assembly as defined in claim 7, wherein the third lumen can withstand a flow rate therethrough of between about three and about eight milliliters per second.

9. The catheter assembly as defined in claim 1, wherein the at least one venous lateral opening and the at least one arterial lateral opening provide substantially equal recirculation rates in a forward flow direction and in a reverse flow direction.

10. The catheter assembly as defined in claim 1, wherein the distal tip region further defines a tapered nose portion, a portion of both the at least one venous lateral opening and the at least one arterial lateral opening being defined on the nose portion, the distal end opening defined at a distal end of the nose portion.

11. The catheter assembly as defined in claim 10, wherein the distal end opening is centrally defined on the nose portion.

12. The catheter assembly as defined in claim 10, wherein the nose portion includes a material having a low hardness relative to a material from which the catheter body is defined.

13. The catheter assembly as defined in claim 12, wherein the catheter body includes a material having a Shore D hardness of approximately 60, and wherein the nose portion includes a material having a Shore A hardness of approximately 85.

14. The catheter assembly as defined in claim 13, wherein the nose portion includes a polyurethane-based resin.

15. By a catheter assembly, a method of treating blood of a patient, the method comprising:

- a) aspirating blood from the patient through a first opening defined in a first lumen of the catheter assembly;
- b) treating the blood outside the body of the patient;
- c) infusing the treated blood to the patient through a second opening defined in a second lumen of the catheter assembly;
- d) infusing a fluid through a third lumen of the catheter assembly; and
- e) reversing the flow of blood within the first and second lumens so as to infuse blood through the first lumen and aspirate blood through the second lumen, a recirculation rate after reversal of the flow of blood being less than or equal to about five percent.

16. The method of treating blood as defined in claim 15, wherein infusing the fluid further comprises:

infusing the fluid through the third lumen such that the fluid exits the catheter assembly via a distal end opening defined distally of the first and second openings.

17. The method of treating blood as defined in claim 15, wherein a recirculation rate of treated blood during stages a-c is less than or equal to about five percent.

18. The method of treating blood as defined in claim 15, wherein infusing the fluid further comprises:

infusing the fluid through the third lumen at a flow rate of between about three and about eight milliliters per second.

19. The method of treating blood as defined in claim 15, wherein infusing the fluid further comprises:

infusing the fluid through the third lumen at a fluid pressure of between about 50 and about 250 psi.

20. A catheter assembly, comprising:  
a catheter body defining a first lumen, a second lumen, and a third lumen,  
the catheter body including a distal tip region, the distal tip region  
including:  
a tapered nose portion;  
a venous lateral opening in fluid communication with the first  
lumen and defined on a portion of the nose portion so as to  
define a distal-facing portion;  
an arterial lateral opening in fluid communication with the second  
lumen and defined on a portion of the nose portion so as to  
define a distal-facing portion, the venous and arterial  
lateral openings symmetrically opposed in substantially  
un-staggered position with respect to one another; and  
a distal end opening defined on a distal end of the nose portion,  
the distal end opening in fluid communication with the  
third lumen.

21. The catheter assembly as defined in claim 20, wherein the third  
lumen can withstand a flow rate therethrough of between about three and about eight  
milliliters per second and a fluid pressure of between about 50 and about 250 psi.

22. The catheter assembly as defined in claim 21, wherein the venous  
and arterial lateral openings are shaped as to impart a lateral and a distal direction to  
fluid flowing out therefrom.

23. The catheter assembly as defined in claim 22, wherein the nose  
portion is joined to a distal end of the catheter body, the nose portion including a material  
having a lower hardness relative to a hardness of the catheter body.

24. The catheter assembly as defined in claim 23, wherein the nose  
portion is joined to the distal end of the catheter body by RF fusion.

25. The catheter assembly as defined in claim 23, wherein the venous  
and arterial lateral openings are defined by an angled cross cut.

26. The catheter assembly as defined in claim 25, wherein the venous and arterial lateral openings are defined about at least a portion of a circumference of the catheter body so as to protect against vessel wall suck-up.

27. The catheter assembly as defined in claim 24, wherein both of the distal-facing portions of the venous and arterial lateral openings can provide a distal flow of fluid during catheter assembly operation when the distal tip region is positioned against a vessel wall.

28. The catheter assembly as defined in claim 27, wherein the venous and arterial lateral openings are defined by a perimeter defining a figure-eight shape.

29. The catheter assembly as defined in claim 28, wherein a recirculation rate of fluids infused via the venous lateral opening by the arterial lateral opening is less than or equal to about five percent.

30. The catheter assembly as defined in claim 20, further comprising:  
a first pre-curved extension leg in fluid communication with the first lumen of the catheter body; and  
a second pre-curved extension leg in fluid communication with the second lumen of the catheter body.

31. The catheter assembly as defined in claim 20, wherein both of the venous segment and the arterial segment can be employed for blood aspiration and blood infusion when the catheter is inserted in a vasculature of a patient.

32. The catheter assembly as defined in claim 20, wherein when inserted into a vasculature of a patient:  
in a first operational configuration state blood is aspirated from the vasculature via the arterial lateral opening and blood is infused into the vasculature via the venous distal opening; and  
in a second operational configuration state blood is aspirated from the vasculature via the venous lateral opening and blood is infused into the vasculature via the arterial distal opening.

33. The catheter assembly as defined in claim 20, wherein the venous and arterial lateral openings are defined such that a long axis of each lateral opening defines an acute angle with respect to a longitudinal axis of the catheter body such that a lateral and distal flow direction is imparted to fluid outflow therefrom.

34. A catheter assembly, comprising:

a catheter body defining a first lumen and a second lumen, the catheter body including a distal tip region, the distal tip region including:  
a nose portion defining a distally converging outer surface;  
a venous lateral opening in fluid communication with the first lumen, the venous lateral opening being at least partially defined on the distally converging outer diameter;  
an arterial lateral opening in fluid communication with the second lumen, the arterial lateral opening being at least partially defined on the distally converging outer diameter, the venous and arterial lateral openings being symmetrically disposed in a substantially un-staggered position with respect to one another; and  
a distal end opening in fluid communication with one of the venous and arterial lumens and sized to pass a guidewire therethrough.

35. The catheter assembly as defined in claim 34, wherein each of the venous and arterial lateral openings include a distal-facing portion.

36. The catheter assembly as defined in claim 34, wherein a guidewire channel provides the fluid communication between the distal end opening and the respective one of the first and second lumens.

37. The catheter assembly as defined in claim 36, wherein the distal end opening is in fluid communication with the first lumen and wherein the guidewire channel and the distal end opening are axially aligned with the first lumen.


38. The catheter assembly as defined in claim 34, wherein fluid is passable from the first lumen to exit via the distal end opening.


39. The catheter assembly as defined in claim 34, wherein a portion of each of the venous and arterial lateral openings is further defined on a terminal catheter portion of the distal tip region, the terminal catheter portion being proximal to the nose portion.


40. The catheter assembly as defined in claim 34, wherein the nose portion defines one of a bullet shape and a tapered shape.

41. The catheter assembly as defined in claim 34, wherein the catheter body defines an oblong cross sectional shape and wherein an outer wall of the catheter body is thickened on opposing sides thereof.

1 / 33

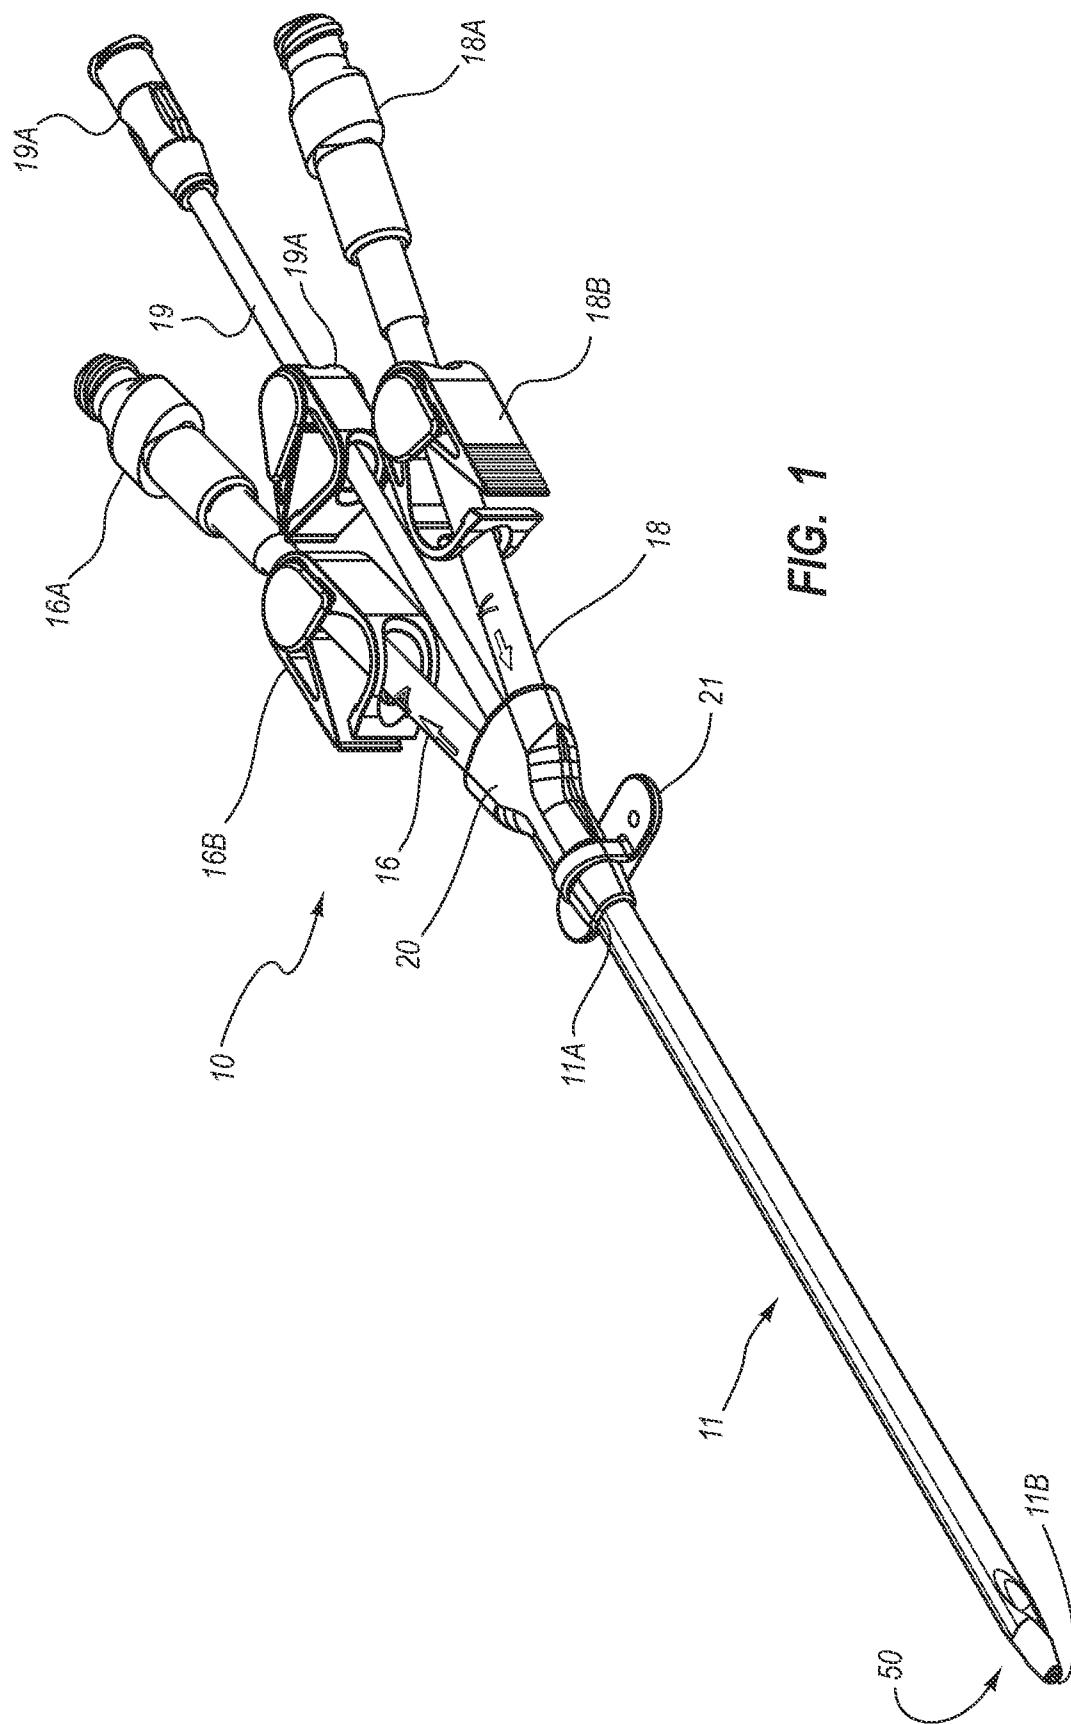

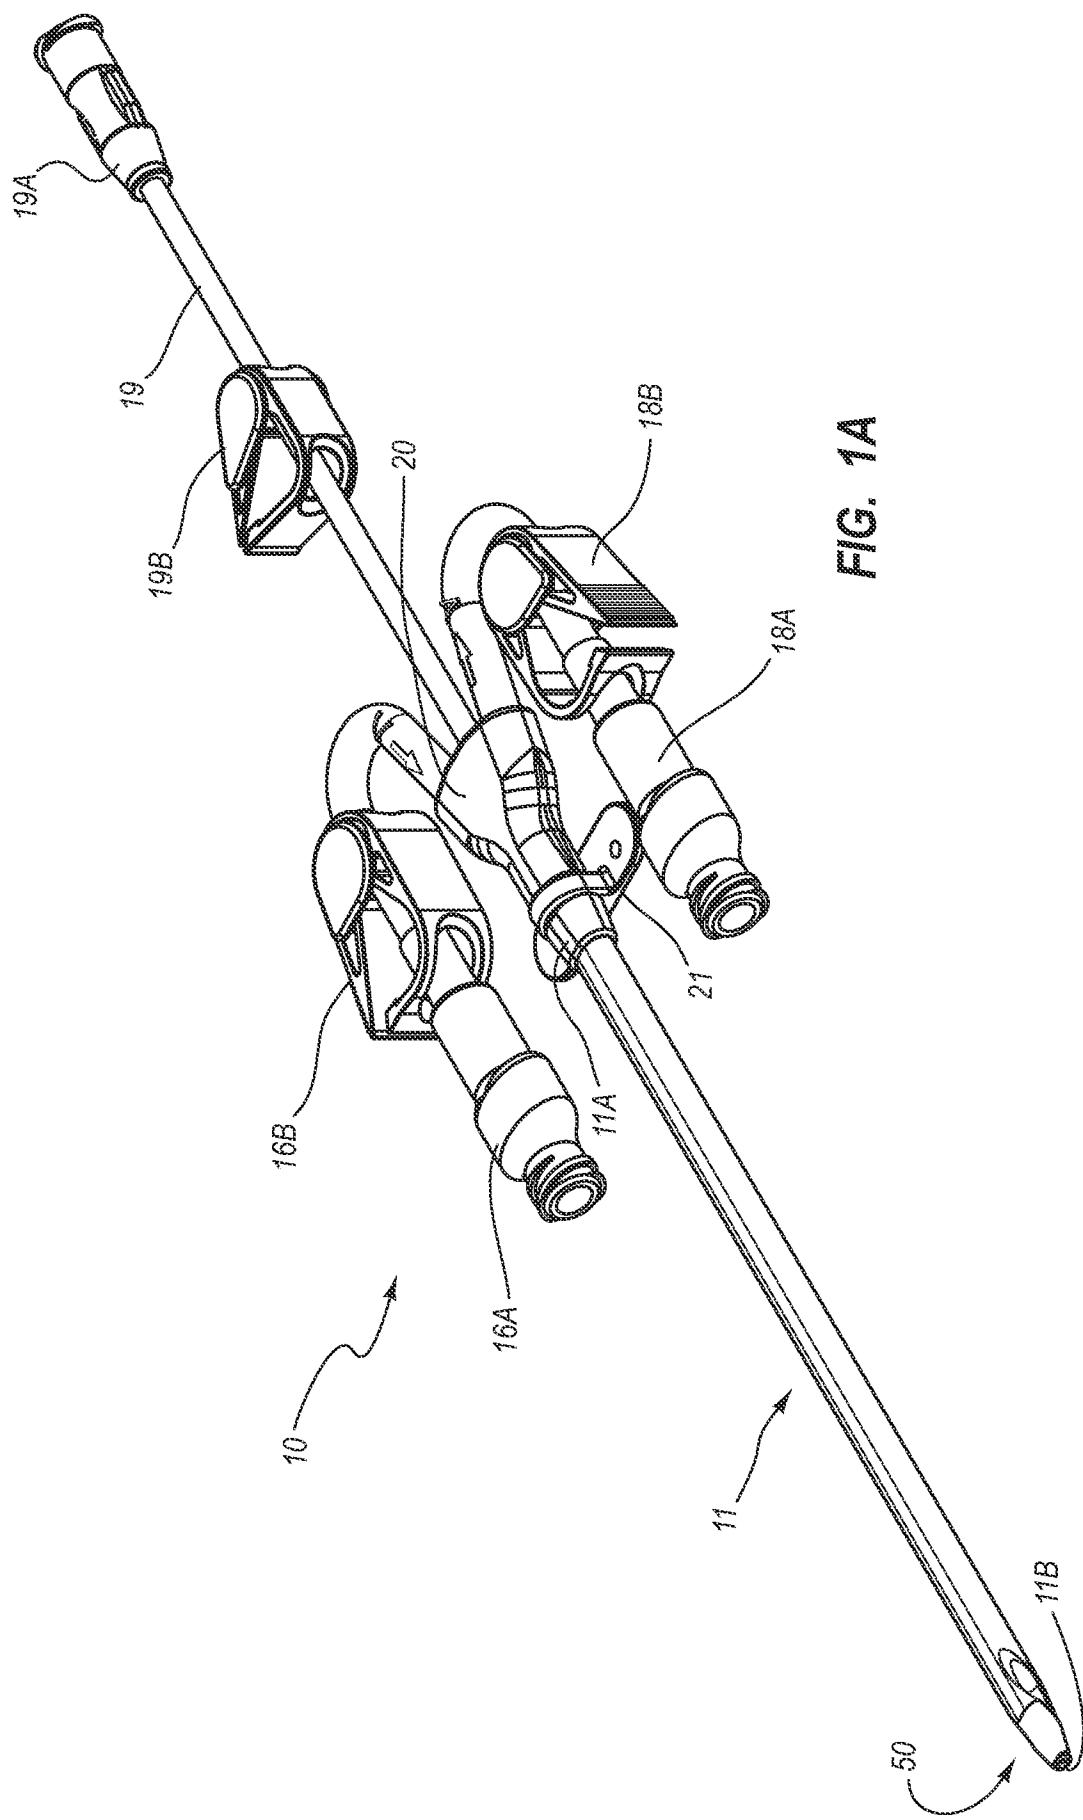

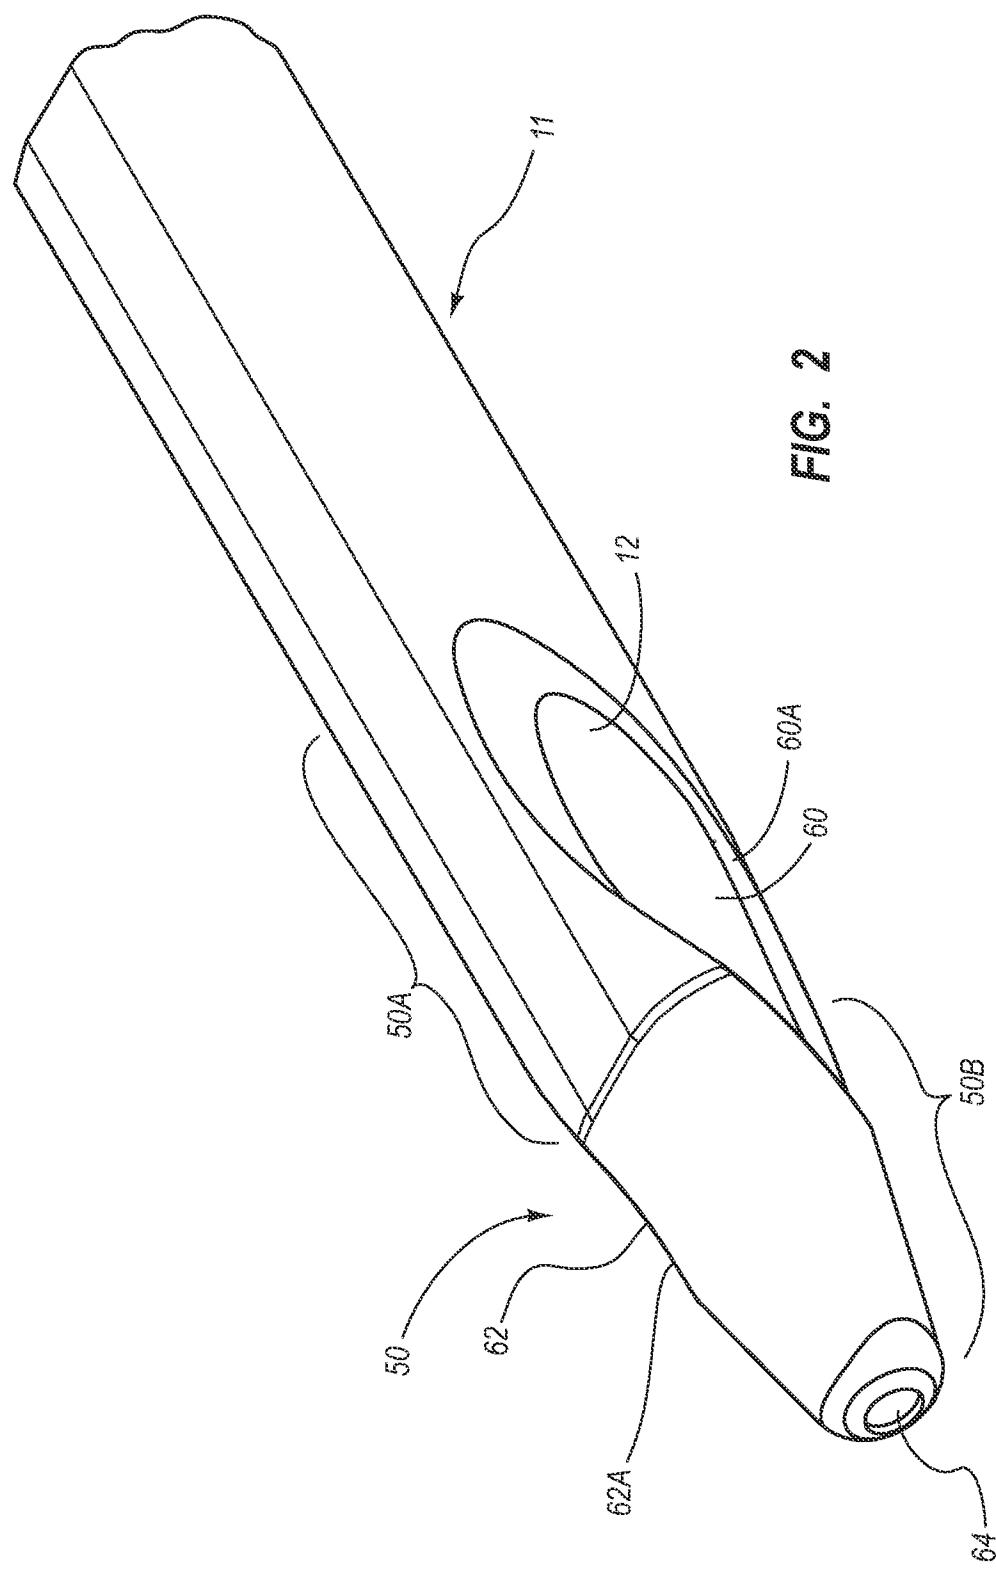

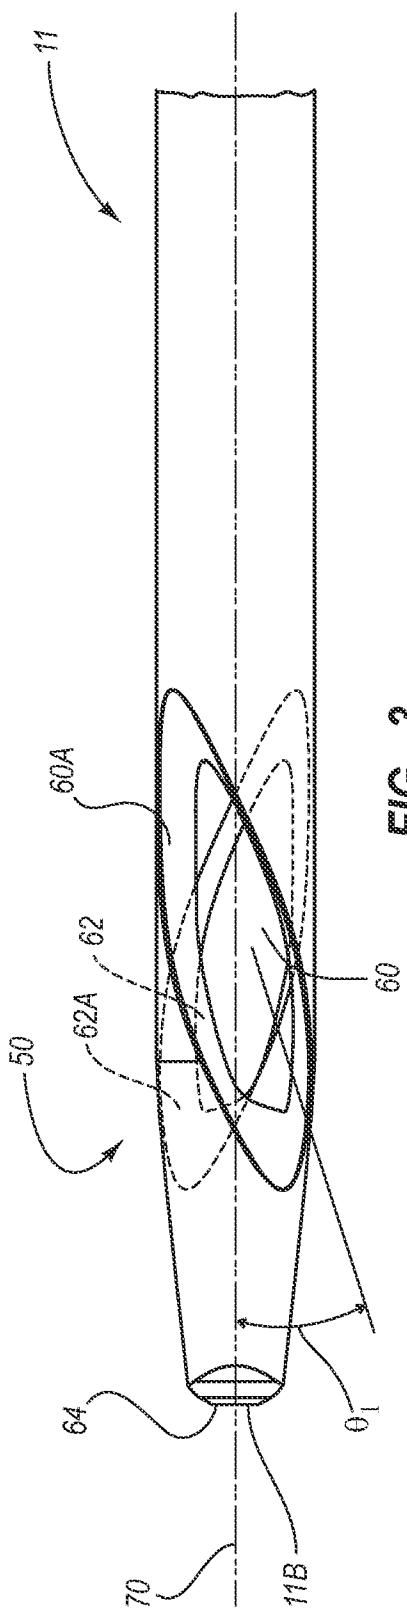


FIG. 3

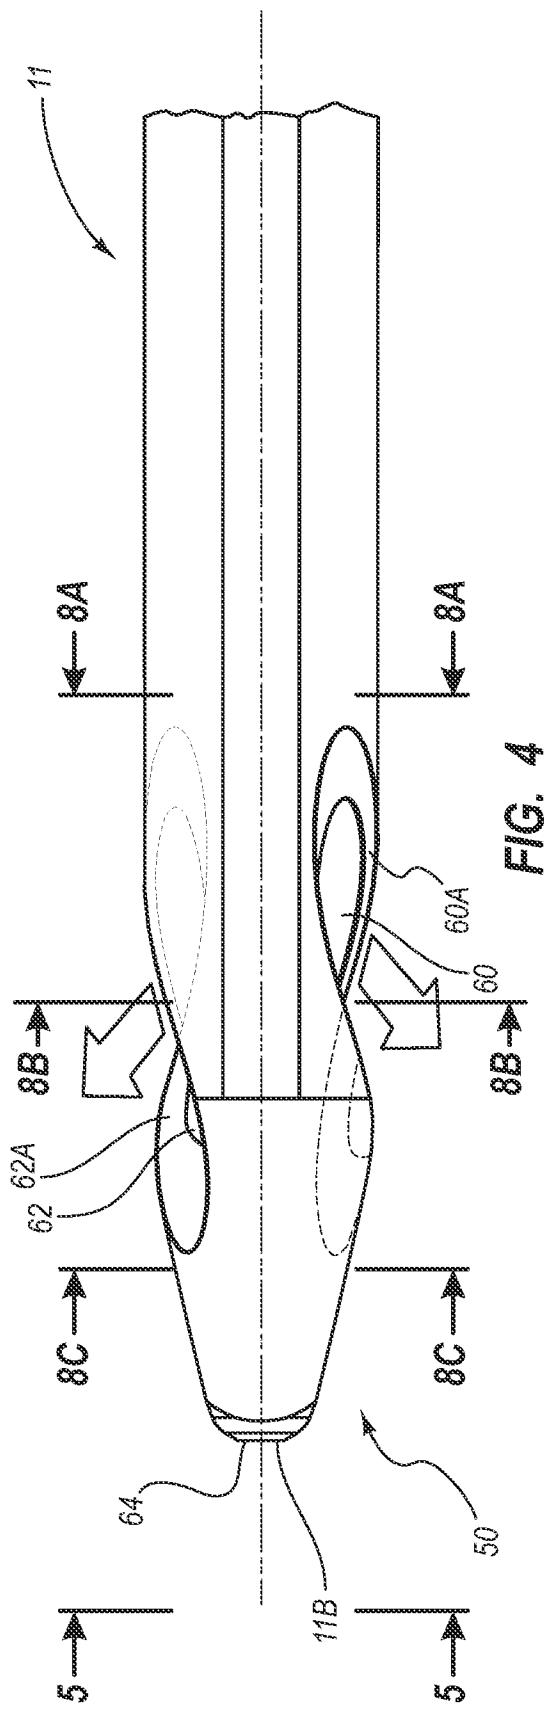


FIG. 4

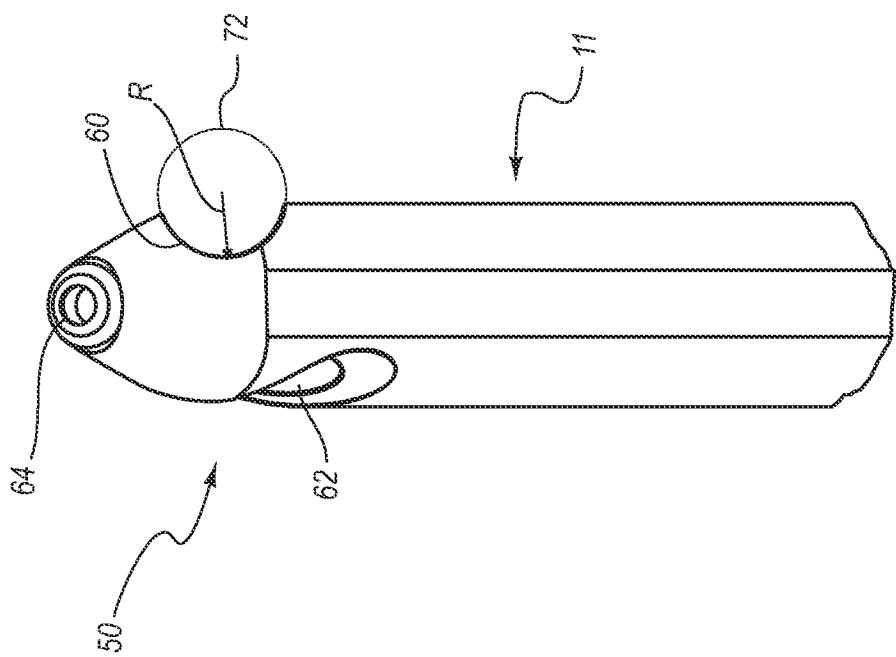


FIG. 6

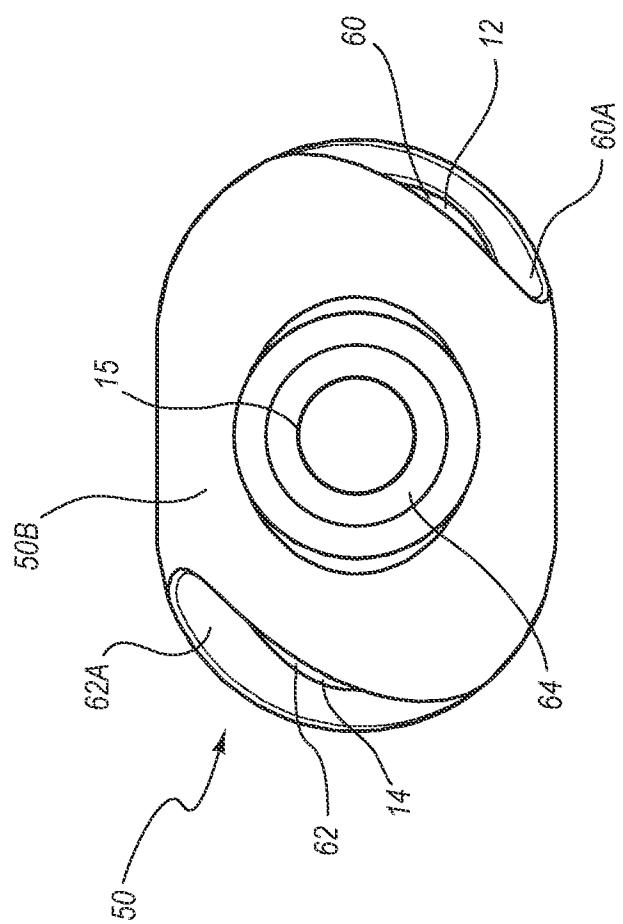


FIG. 5

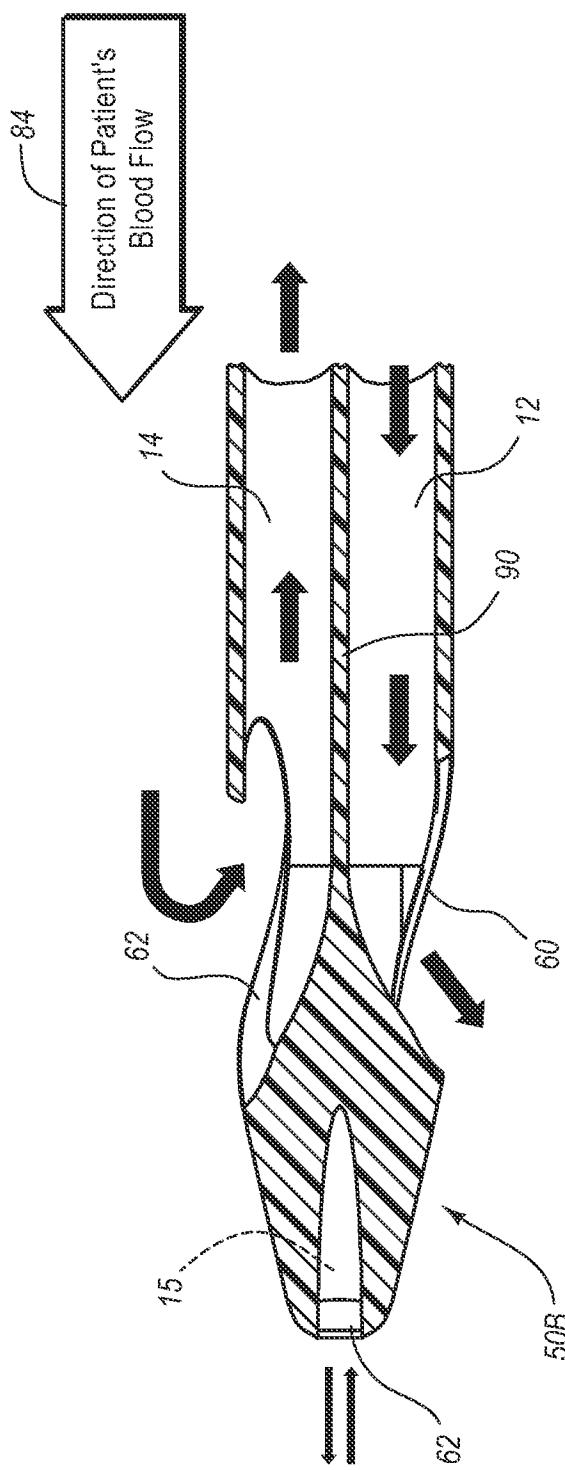


FIG. 7A

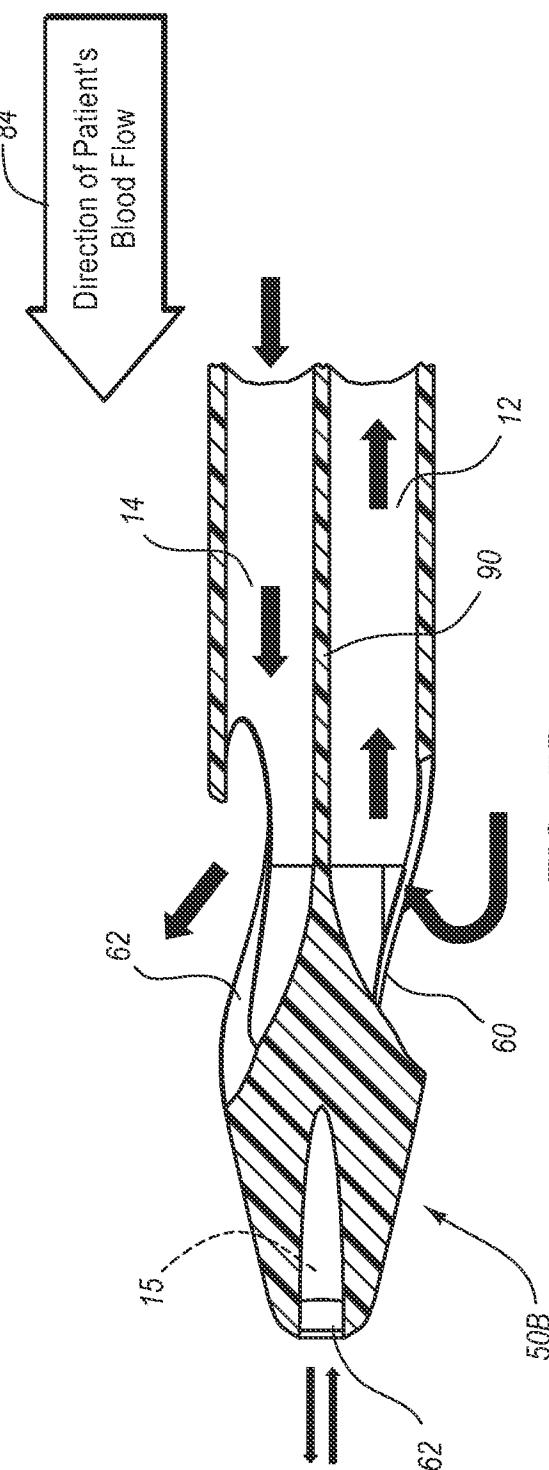


FIG. 7B

7 / 33

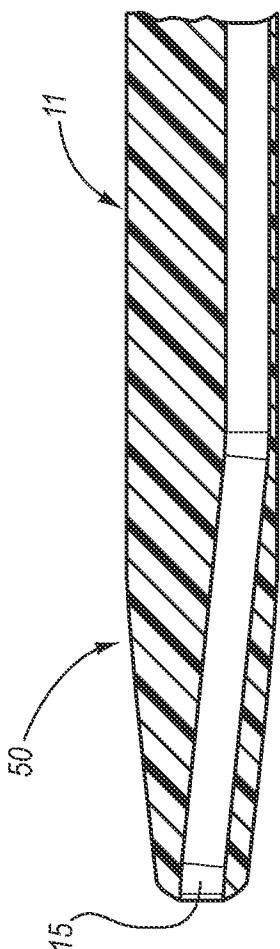
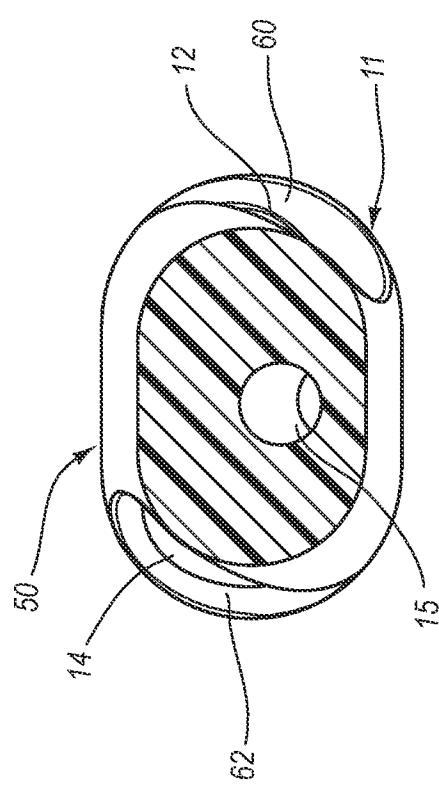
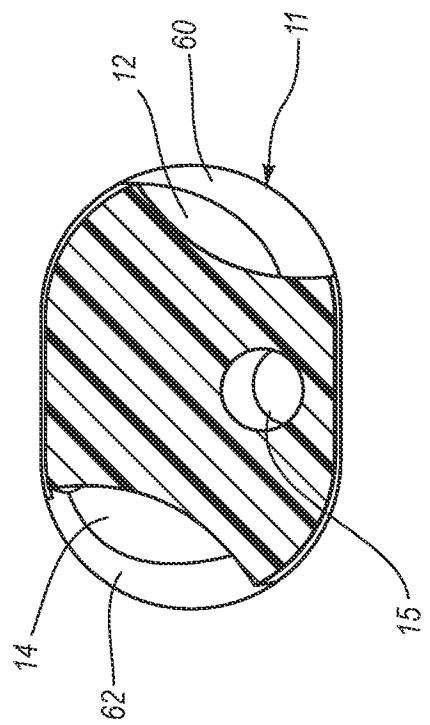
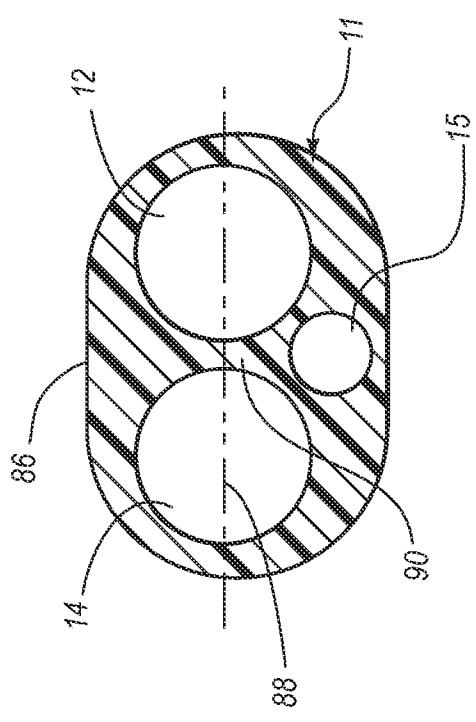
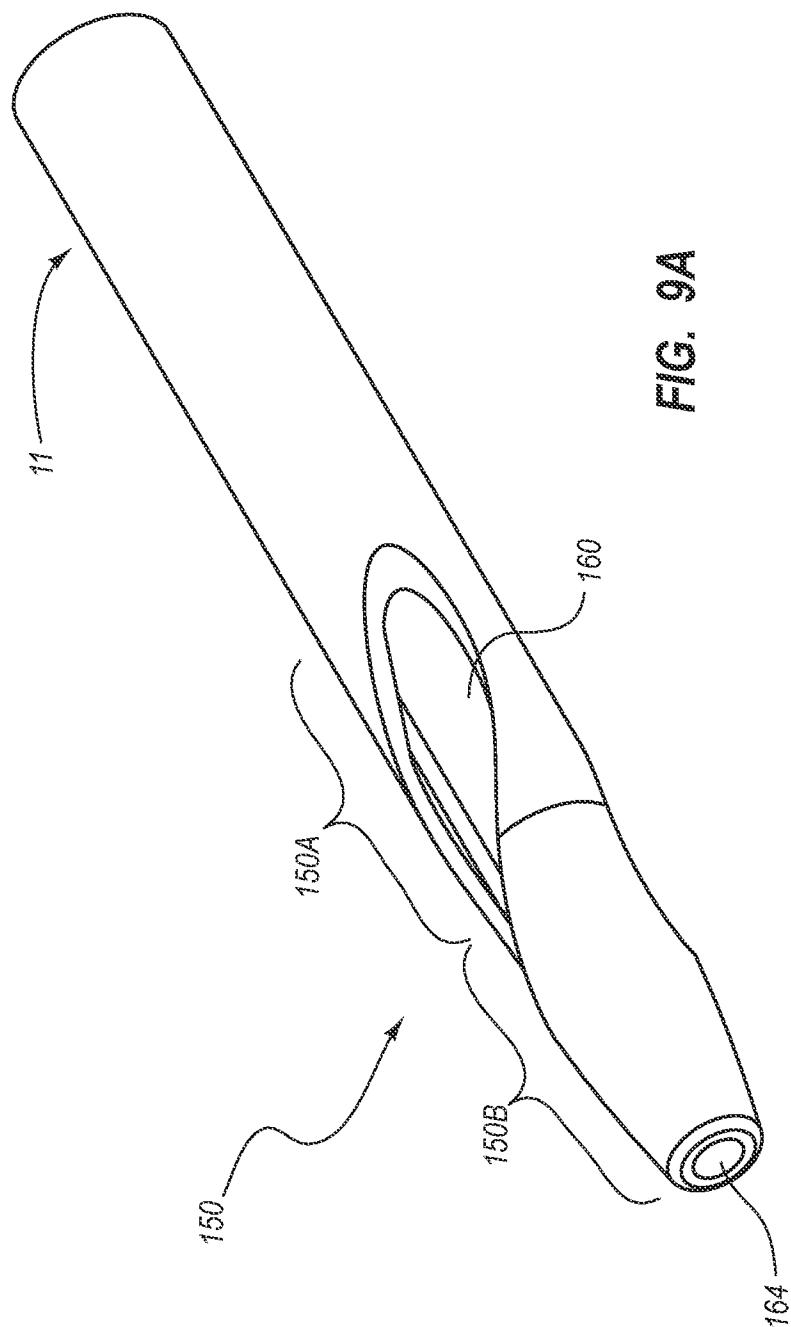


FIG. 9A



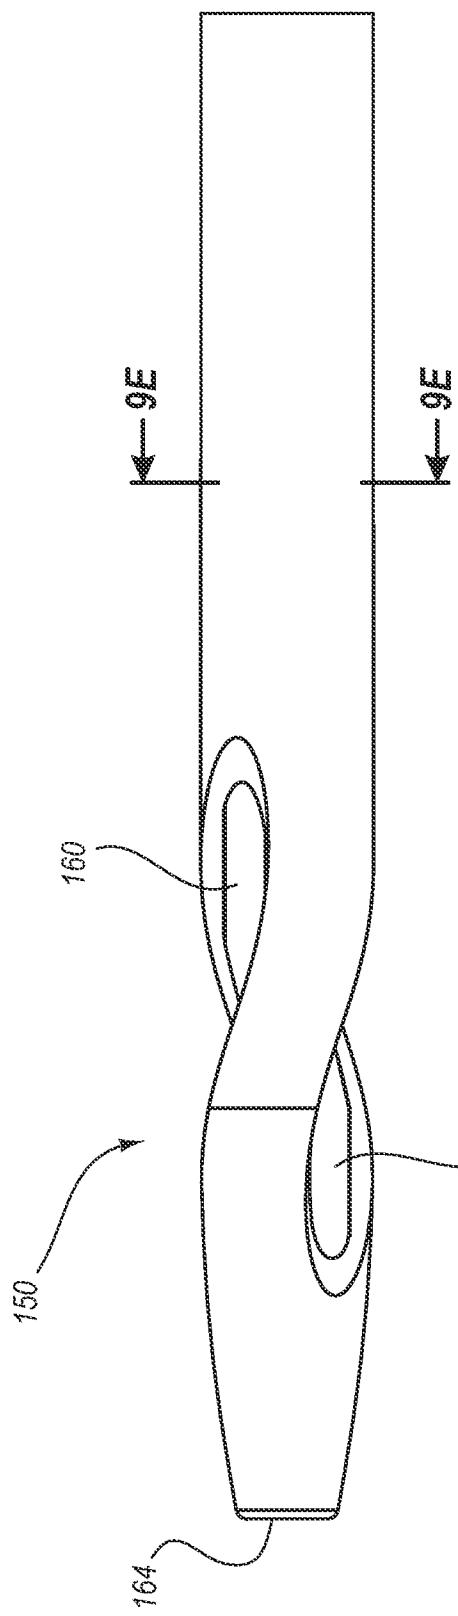


FIG. 9B

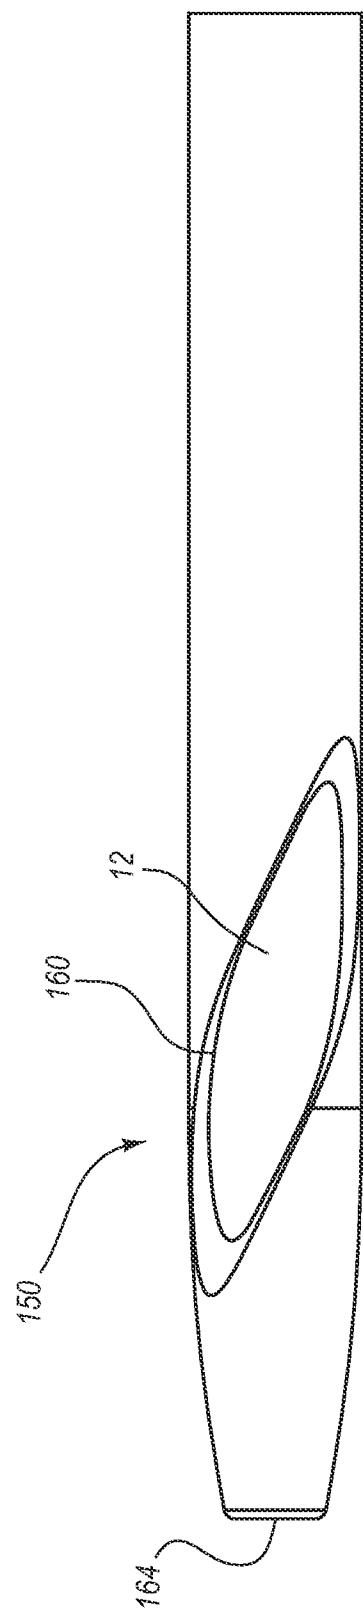


FIG. 9C

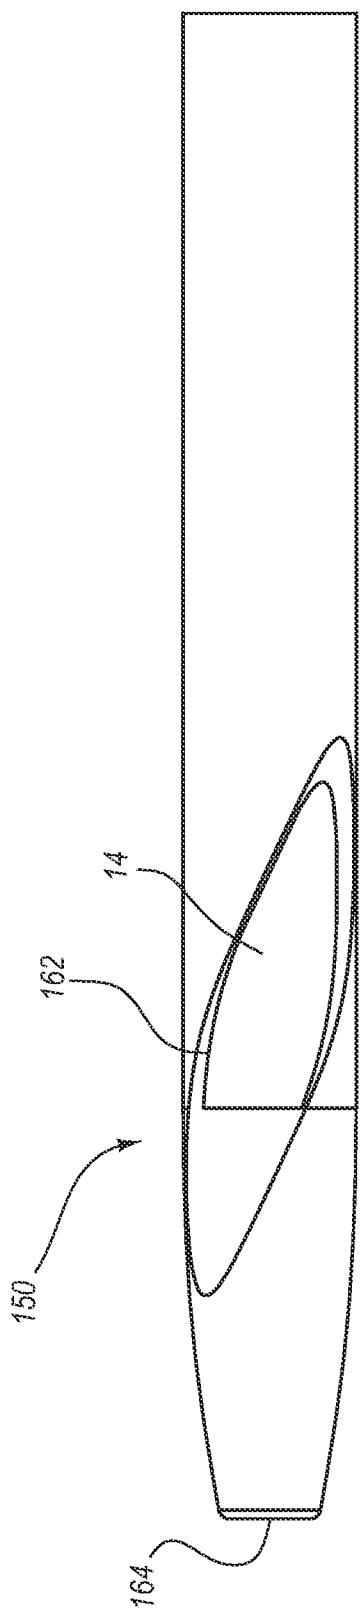


FIG. 9D

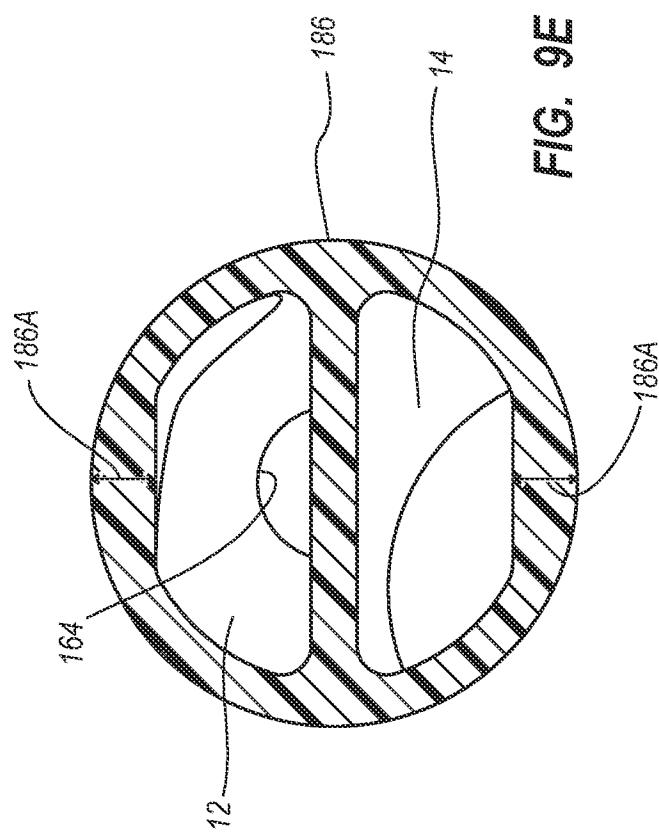


FIG. 9E

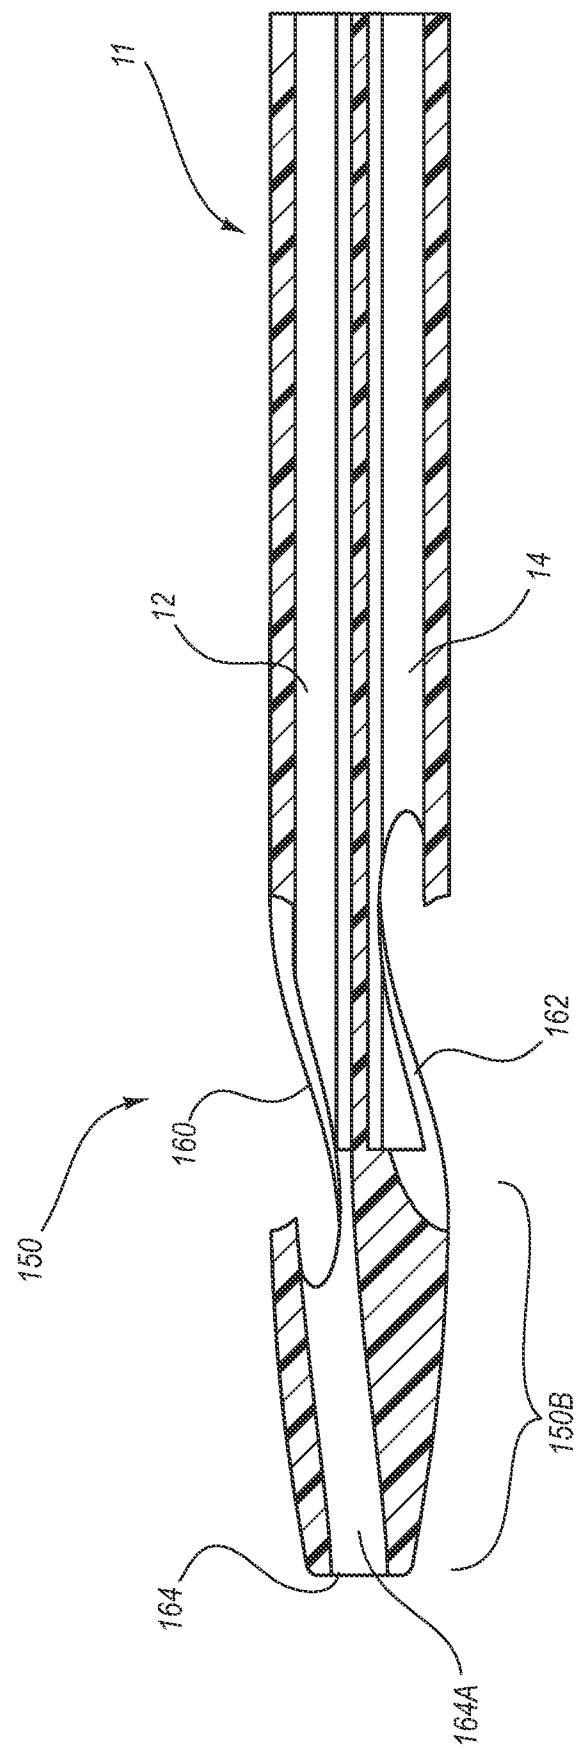


FIG. 9F

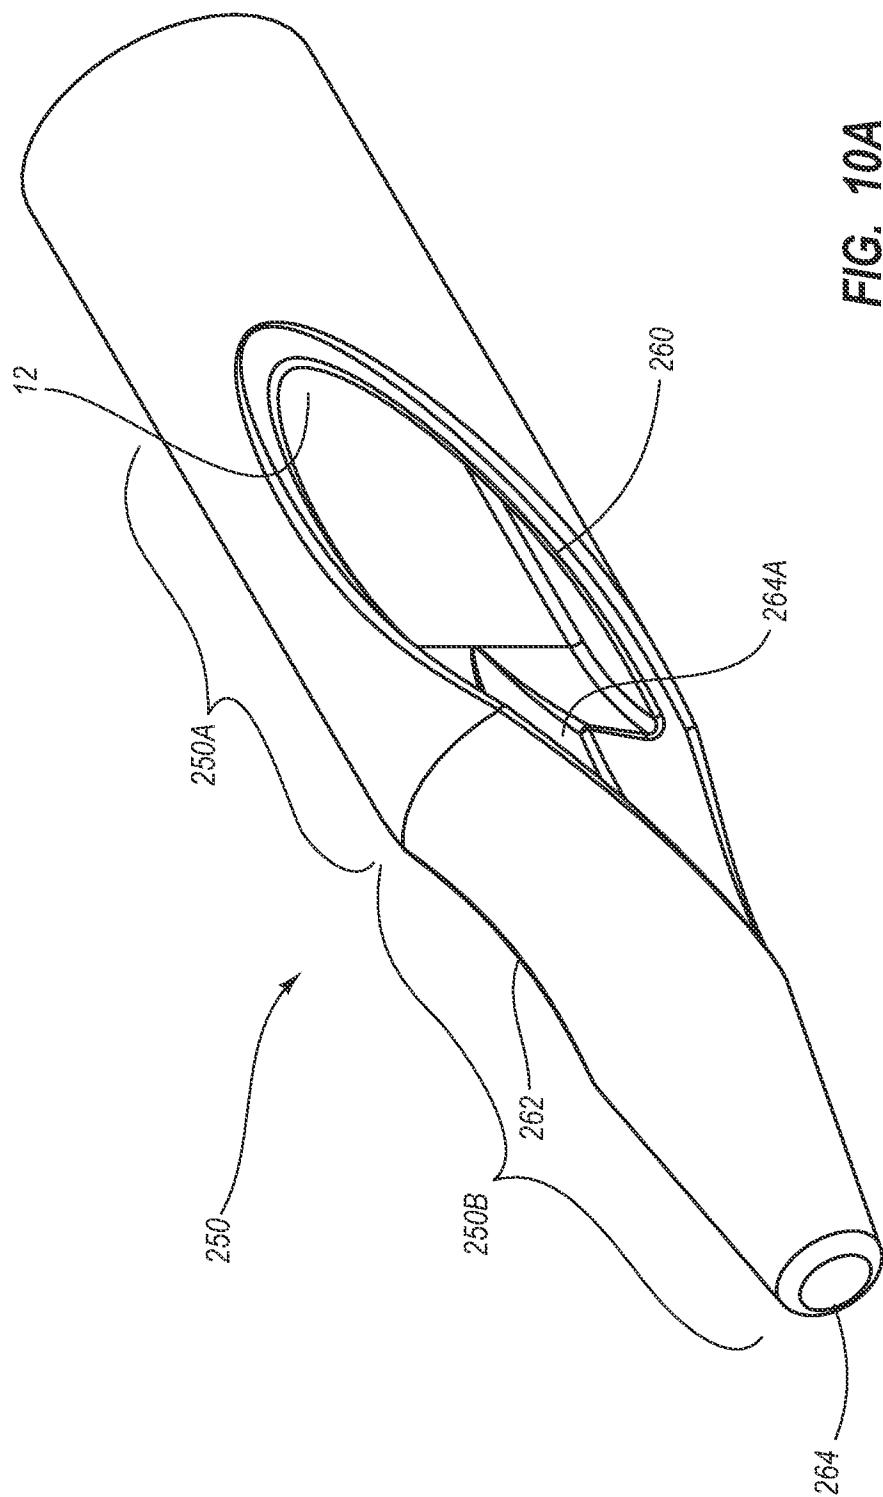


FIG. 10A

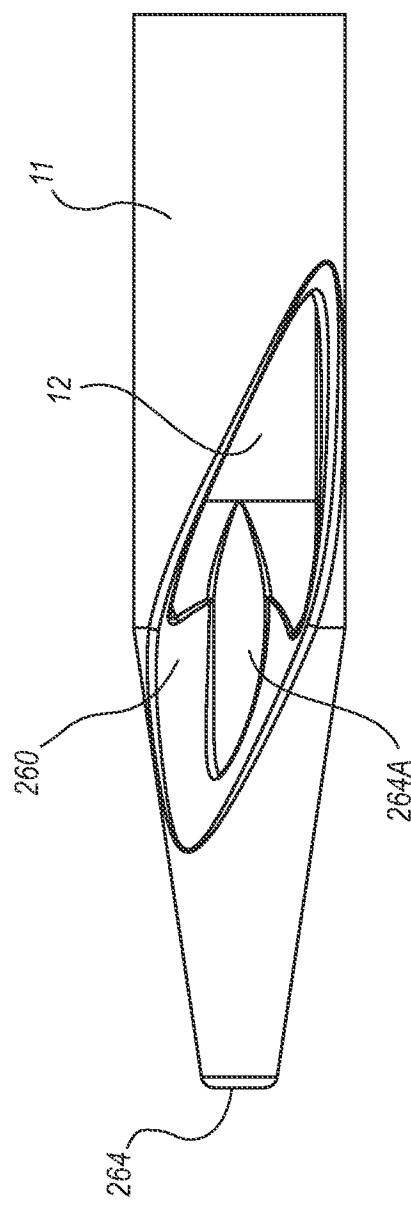


FIG. 10C

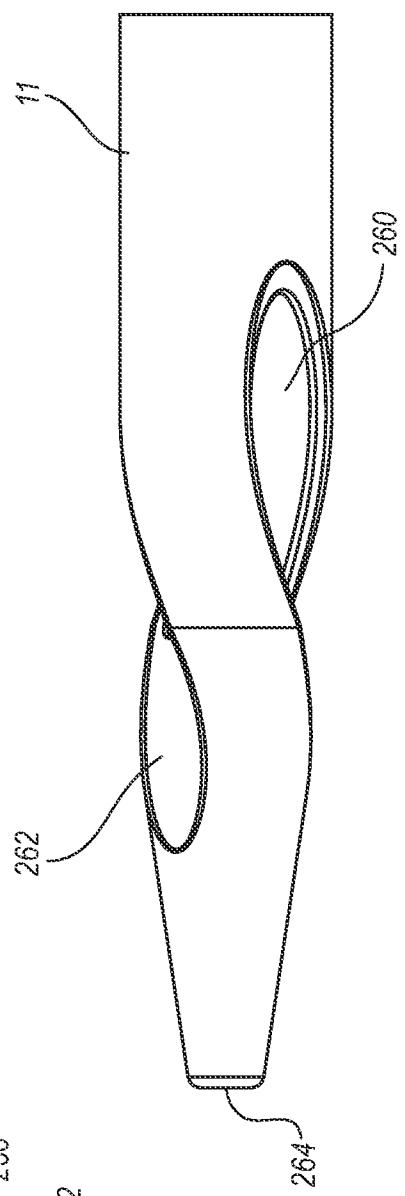


FIG. 10D

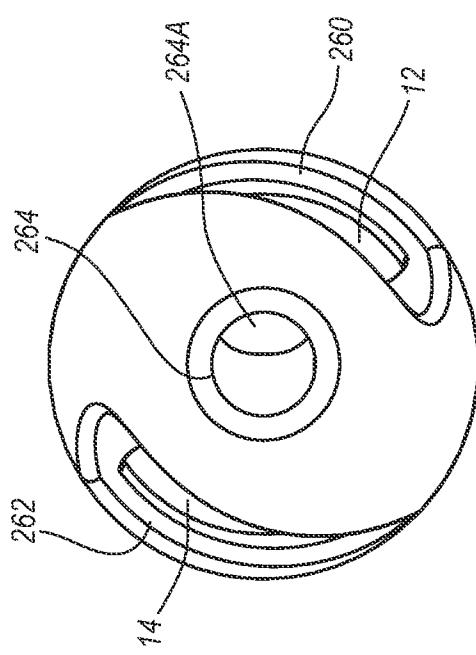
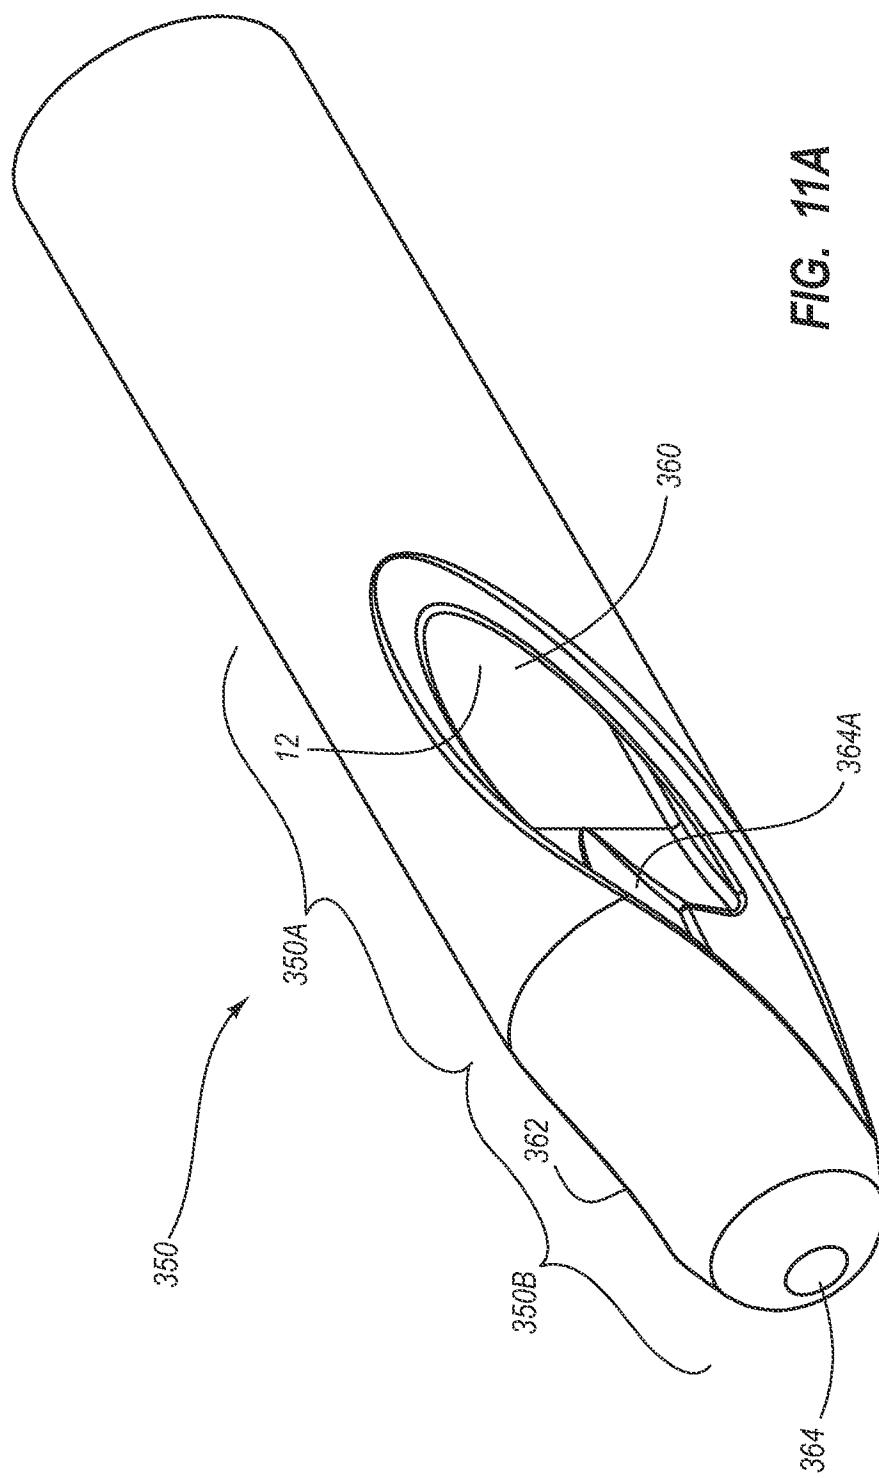


FIG. 10B



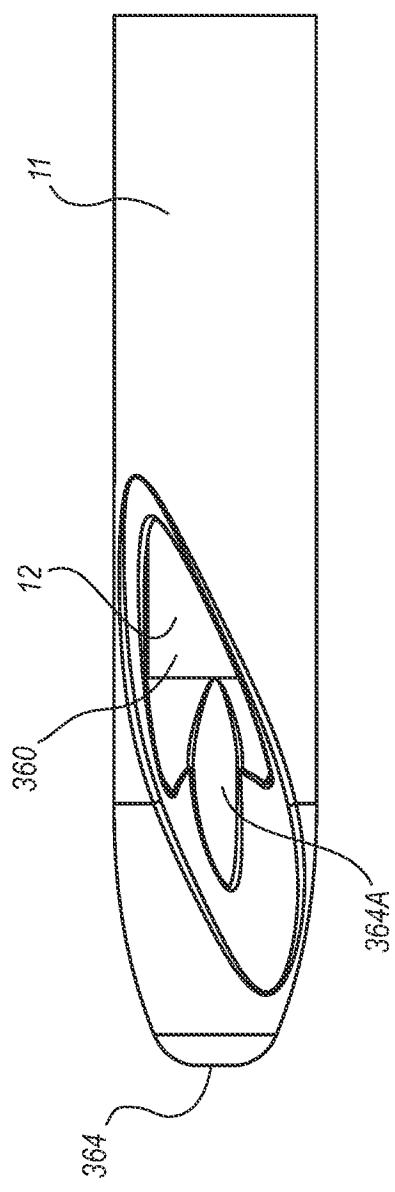


FIG. 11C

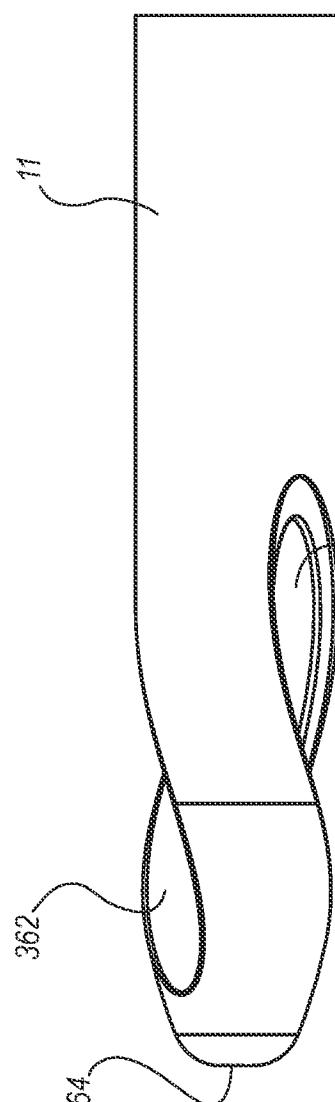


FIG. 11D


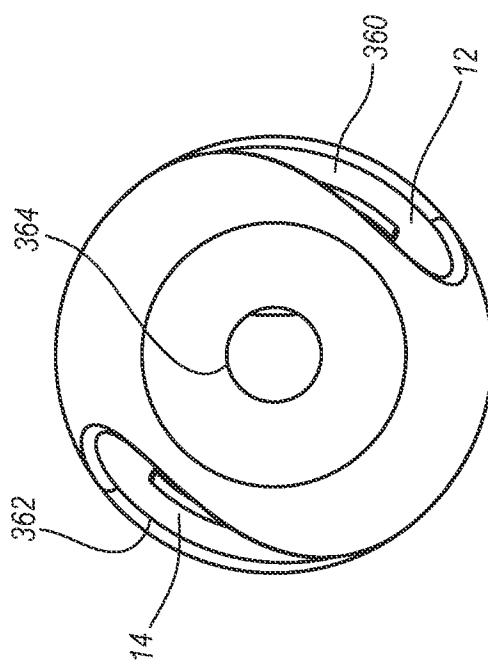


FIG. 11B

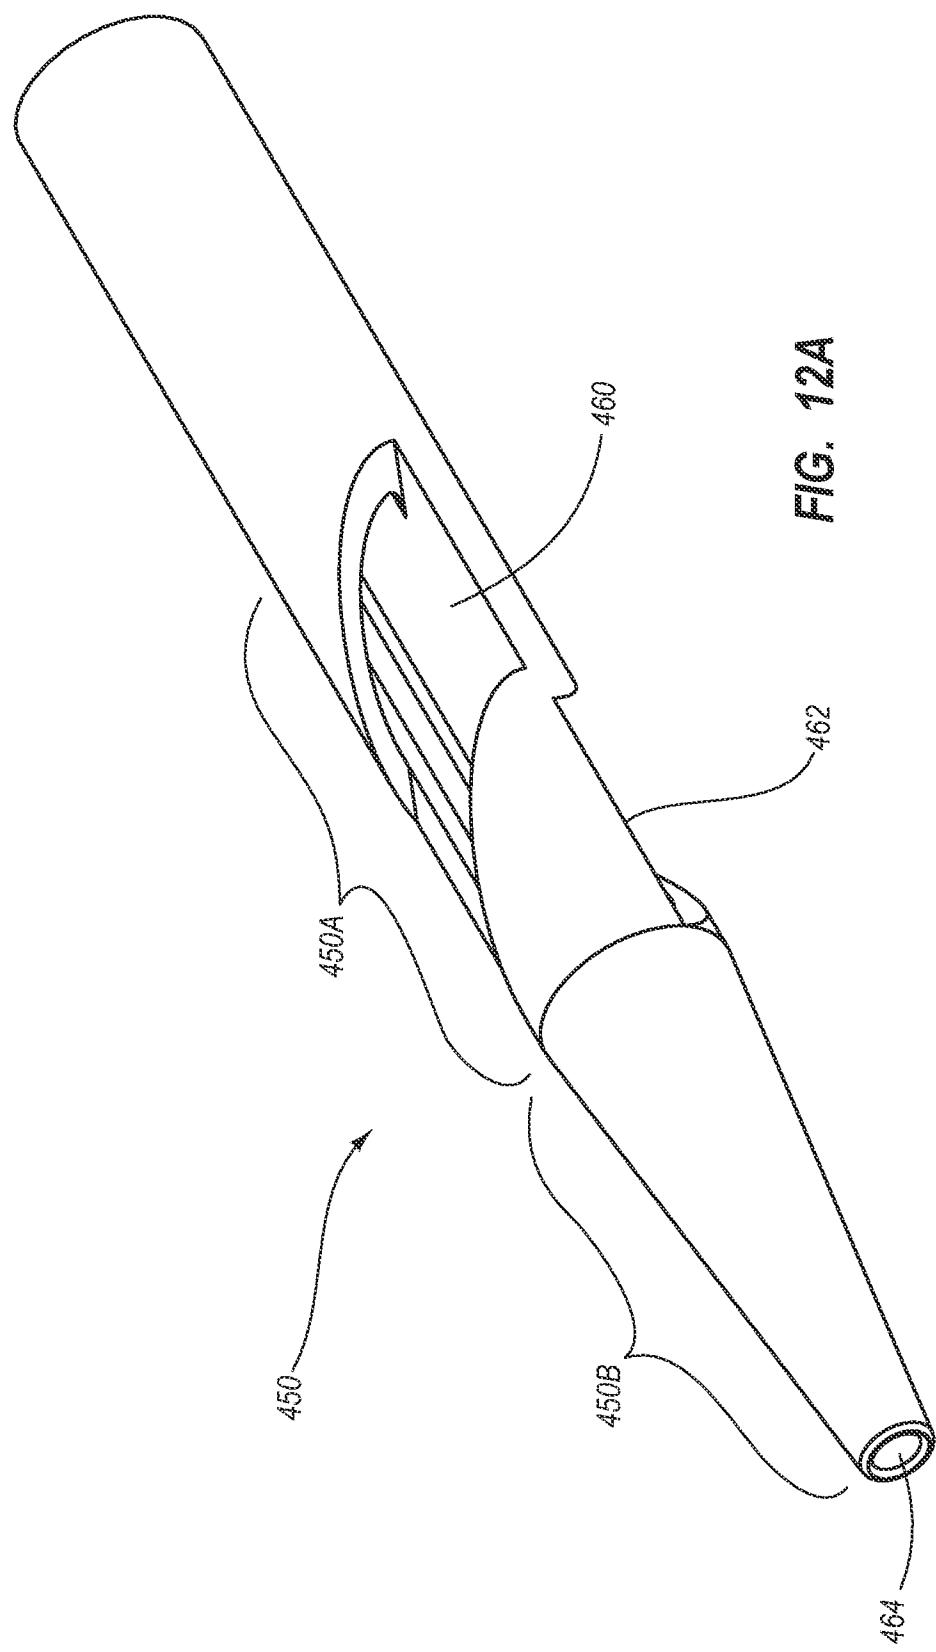

17 / 33

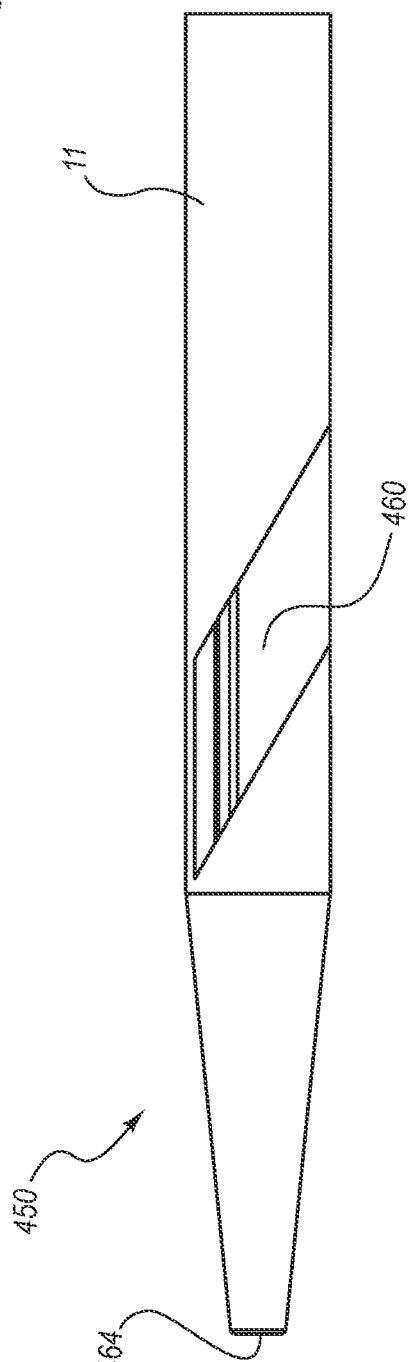
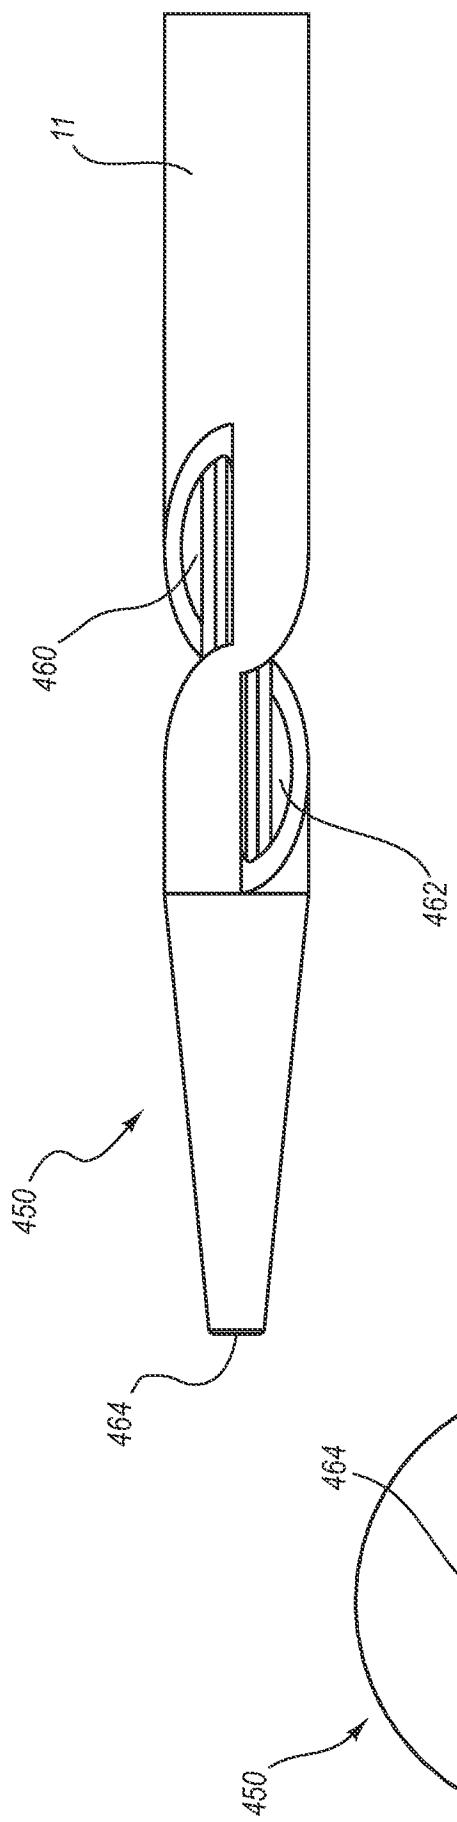
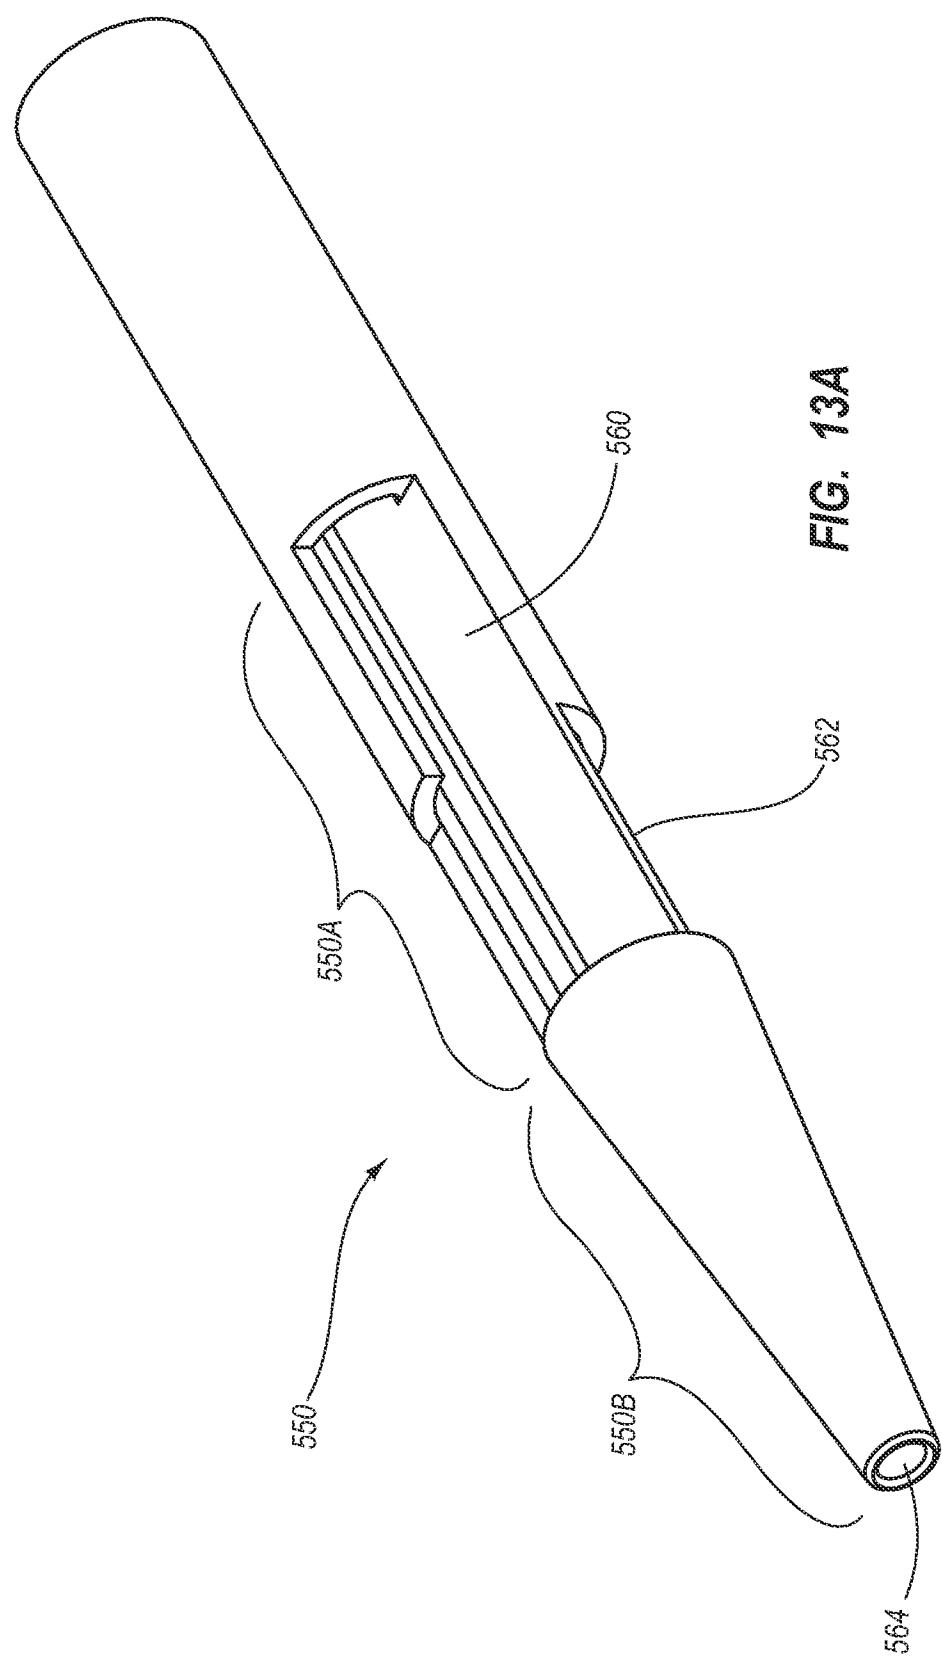


FIG. 12B



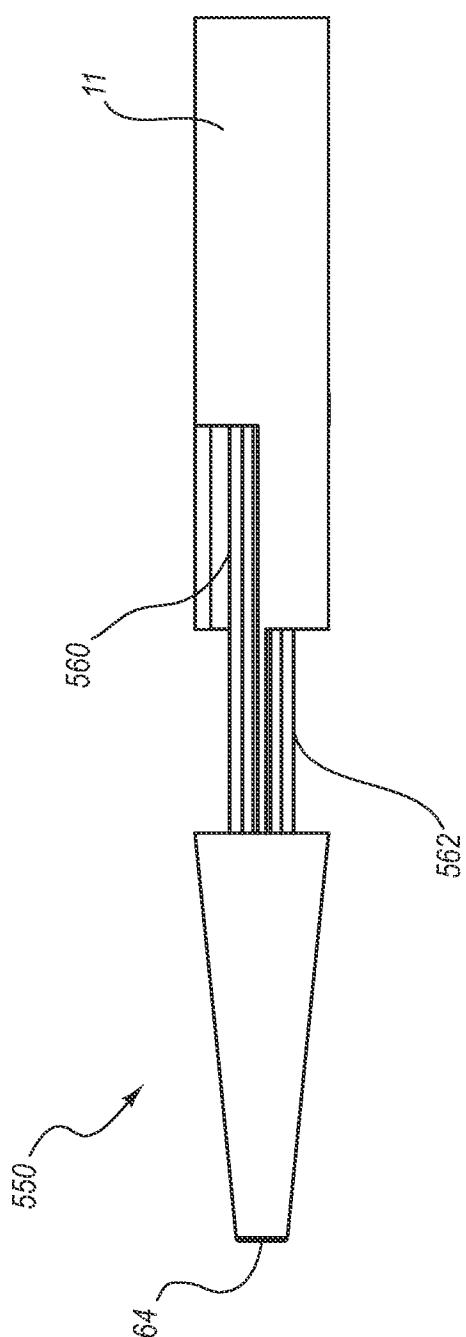


FIG. 13C

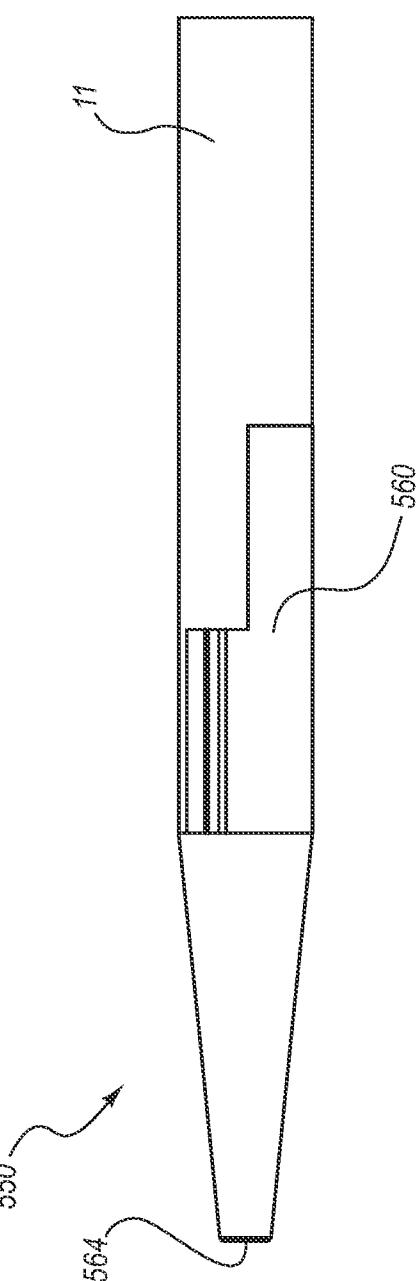


FIG. 13D

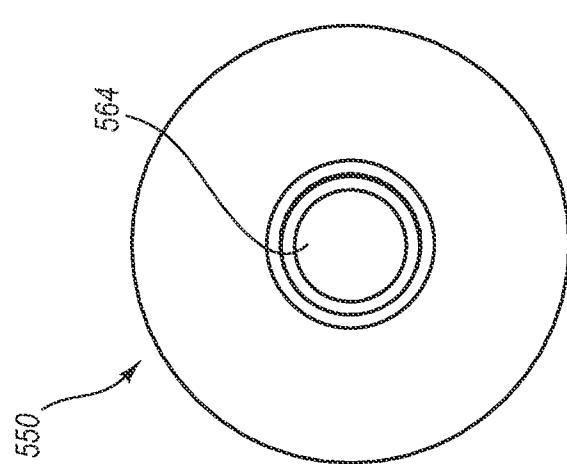


FIG. 13B

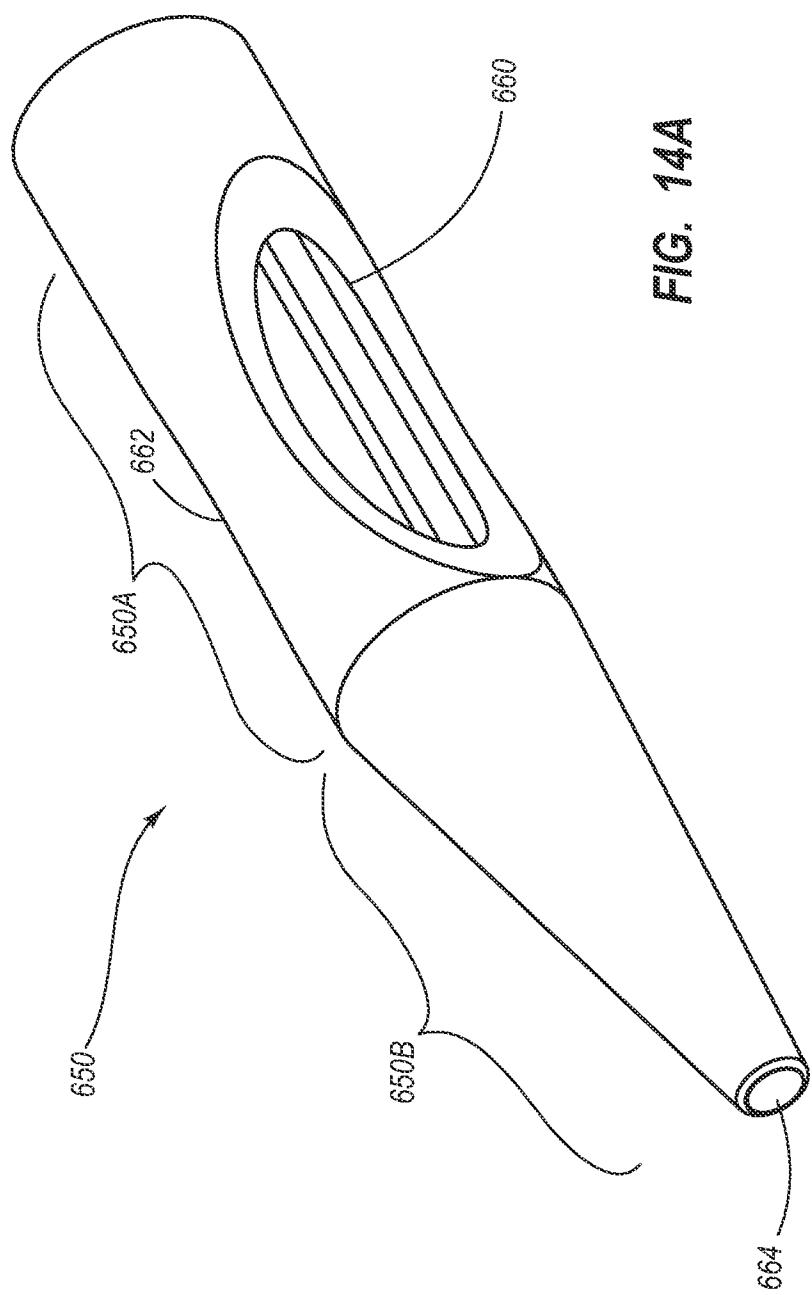
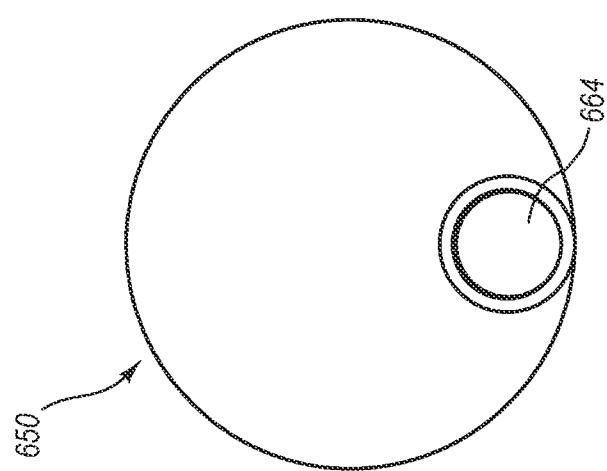
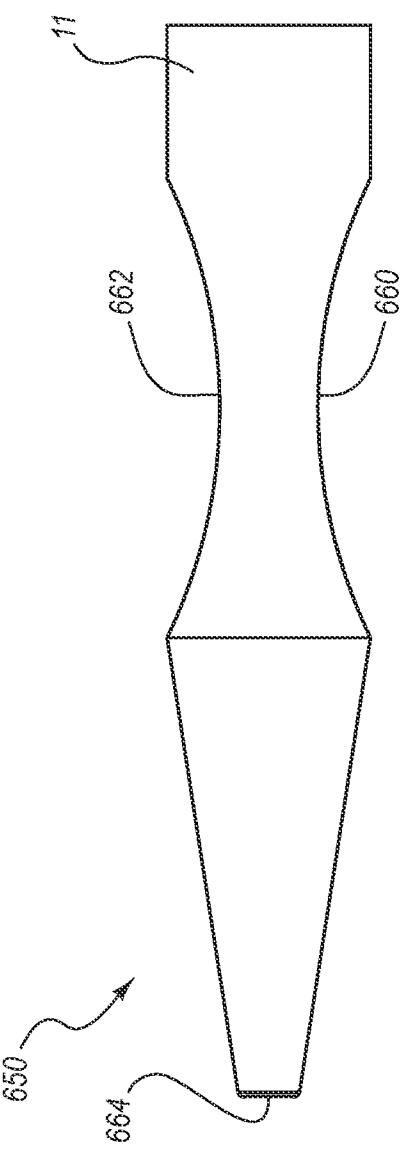
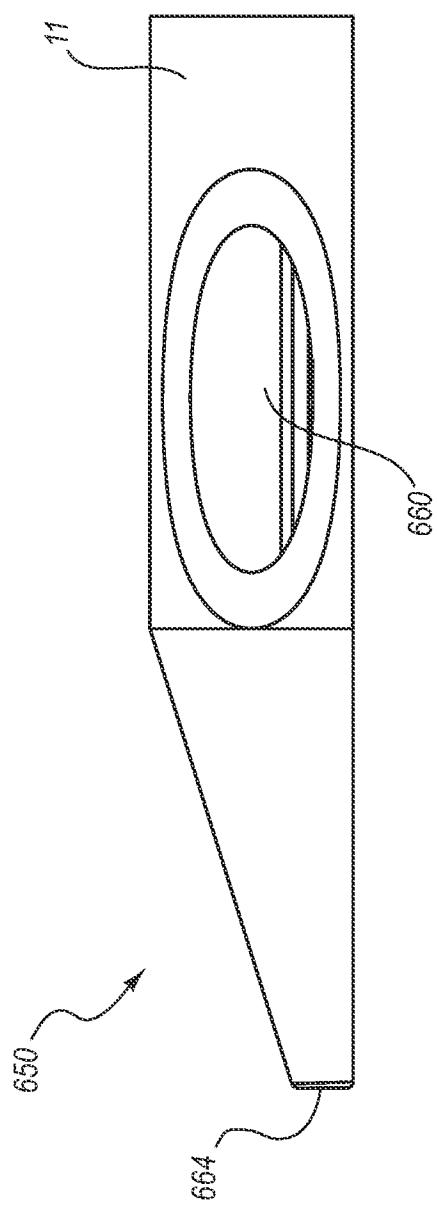
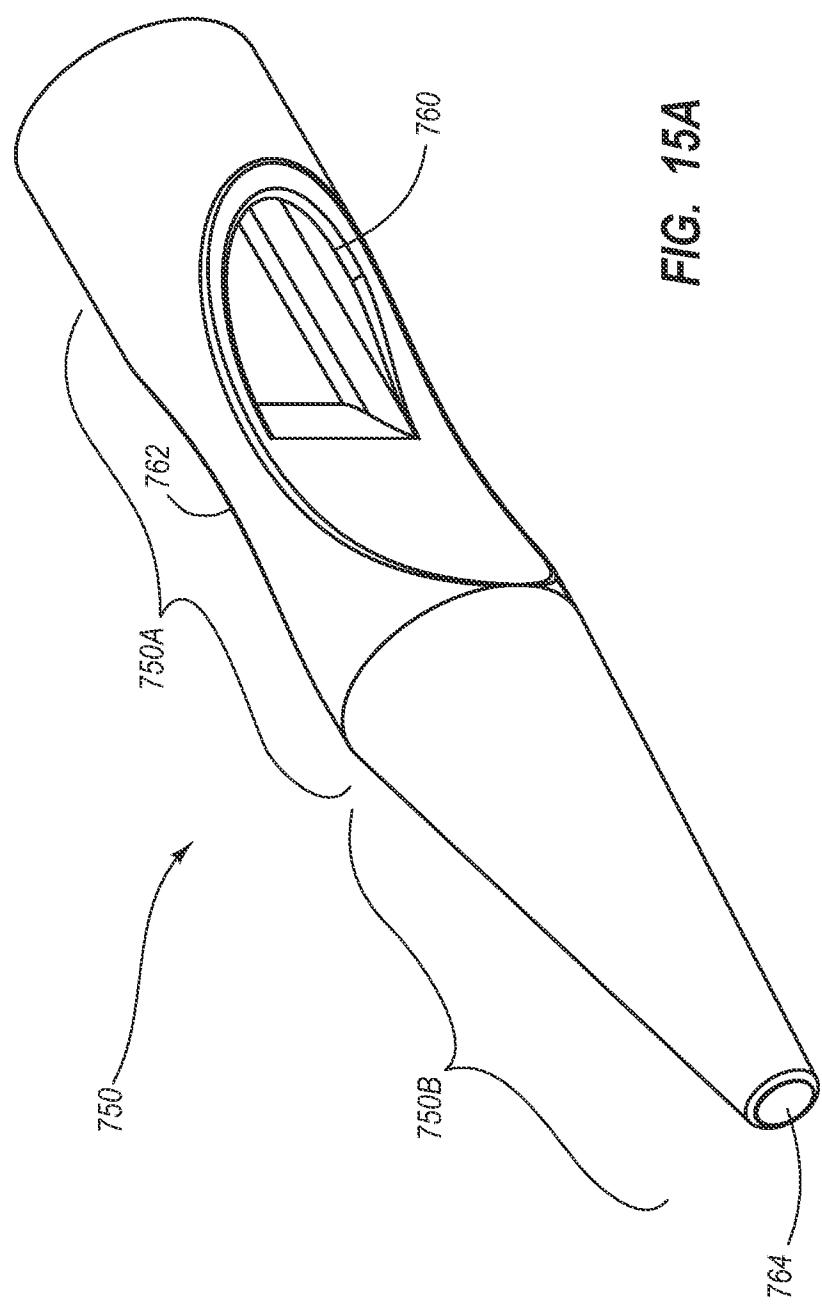
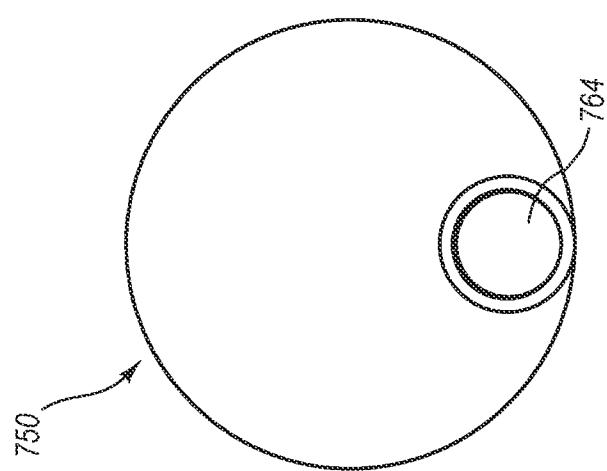
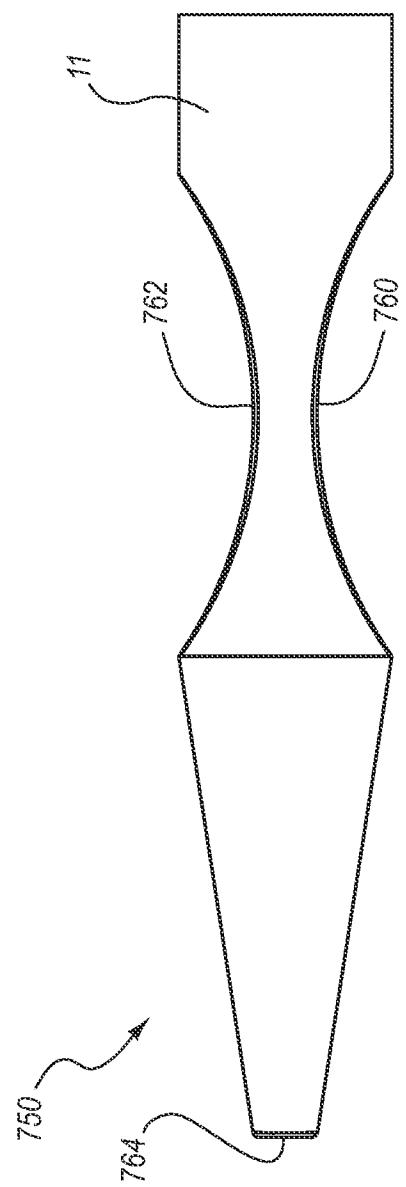
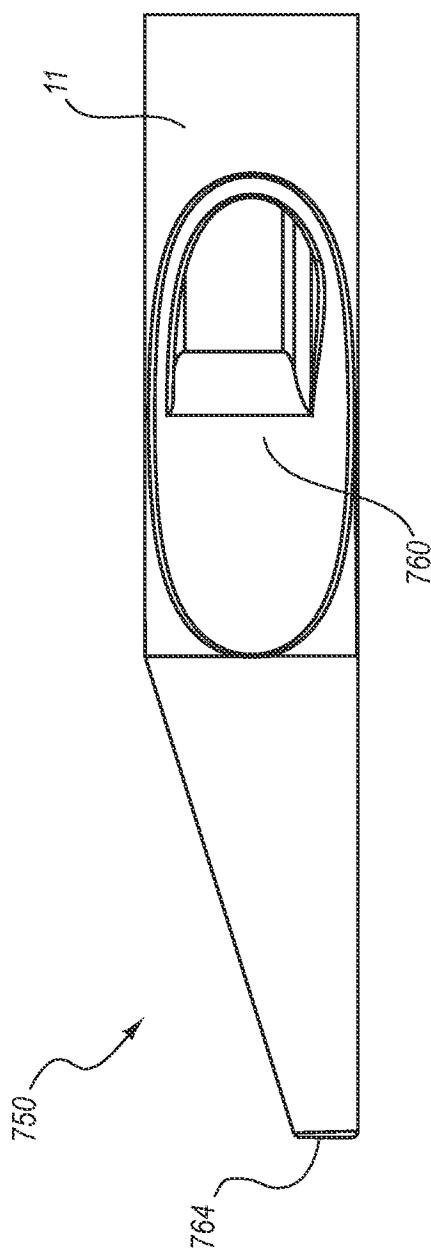
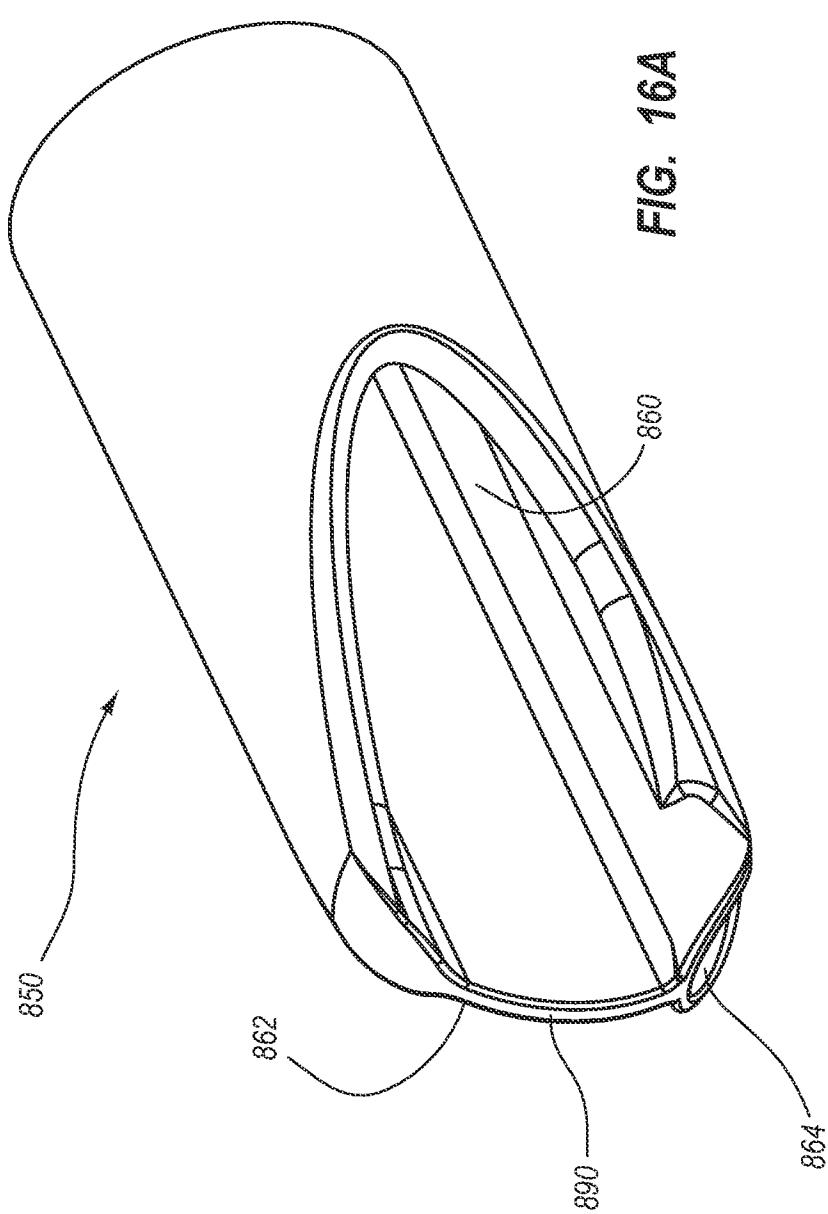


FIG. 14A









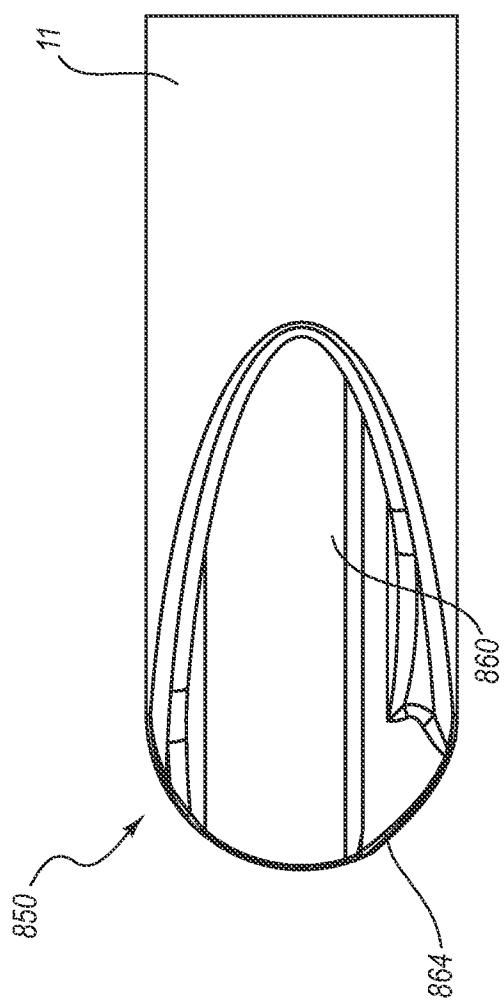


FIG. 16C

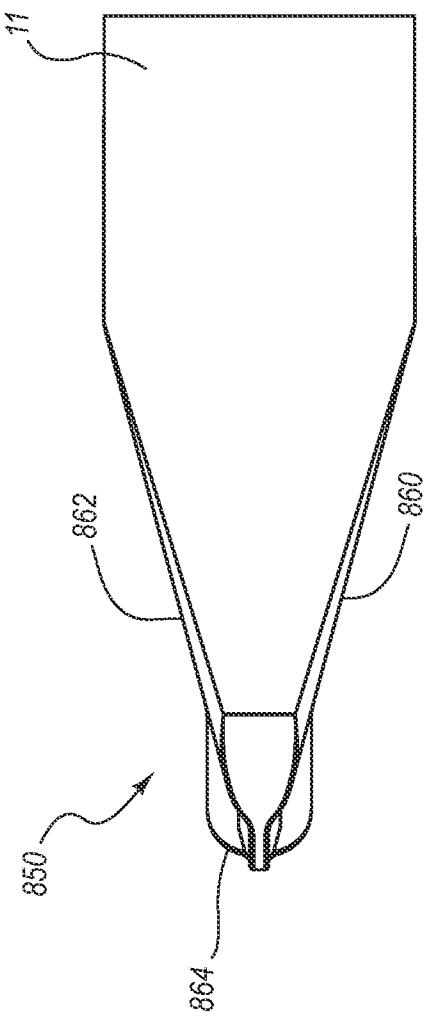


FIG. 16D







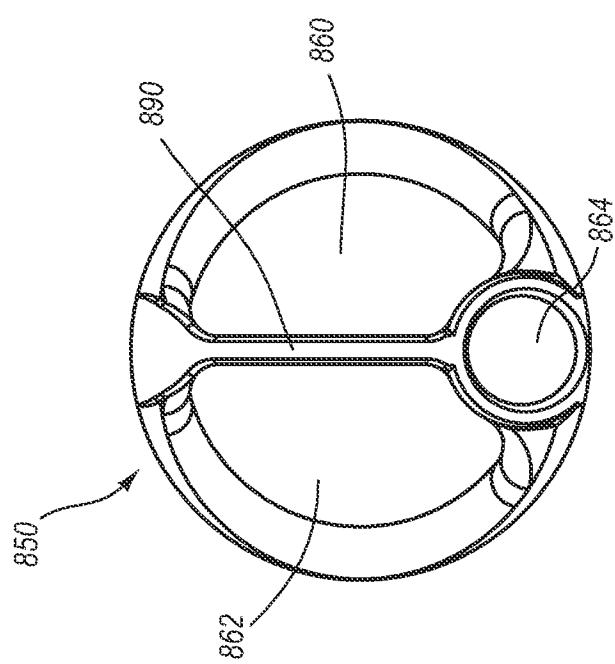



FIG. 16B

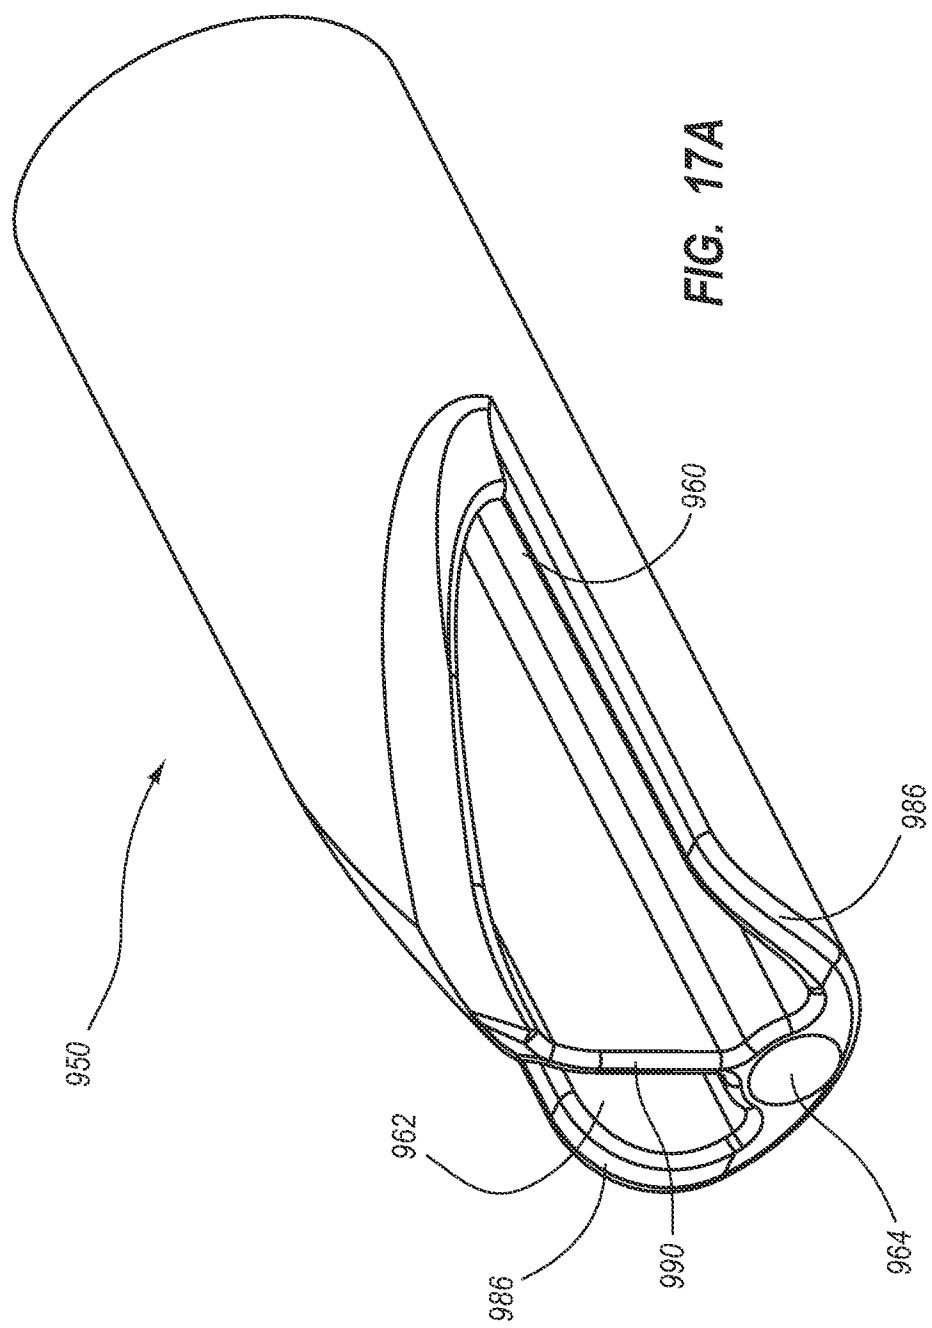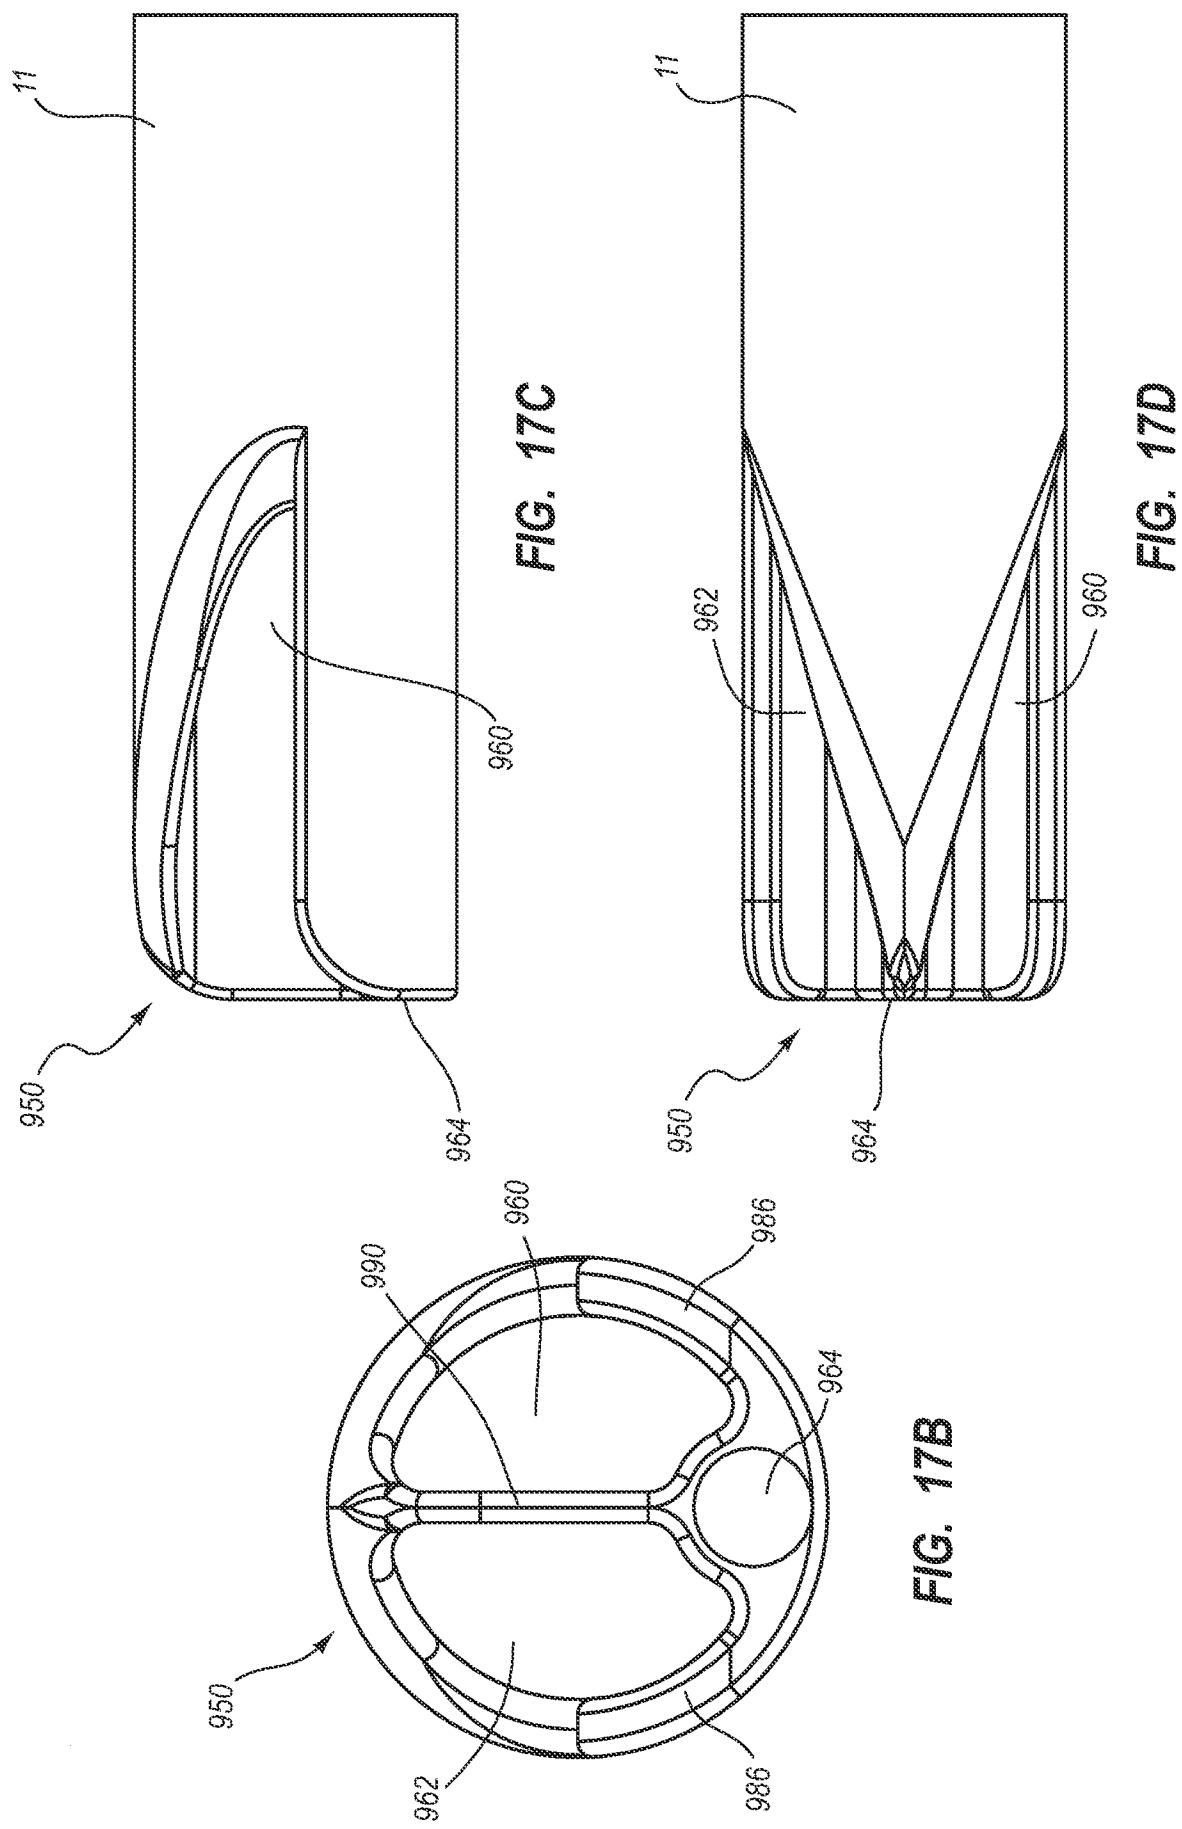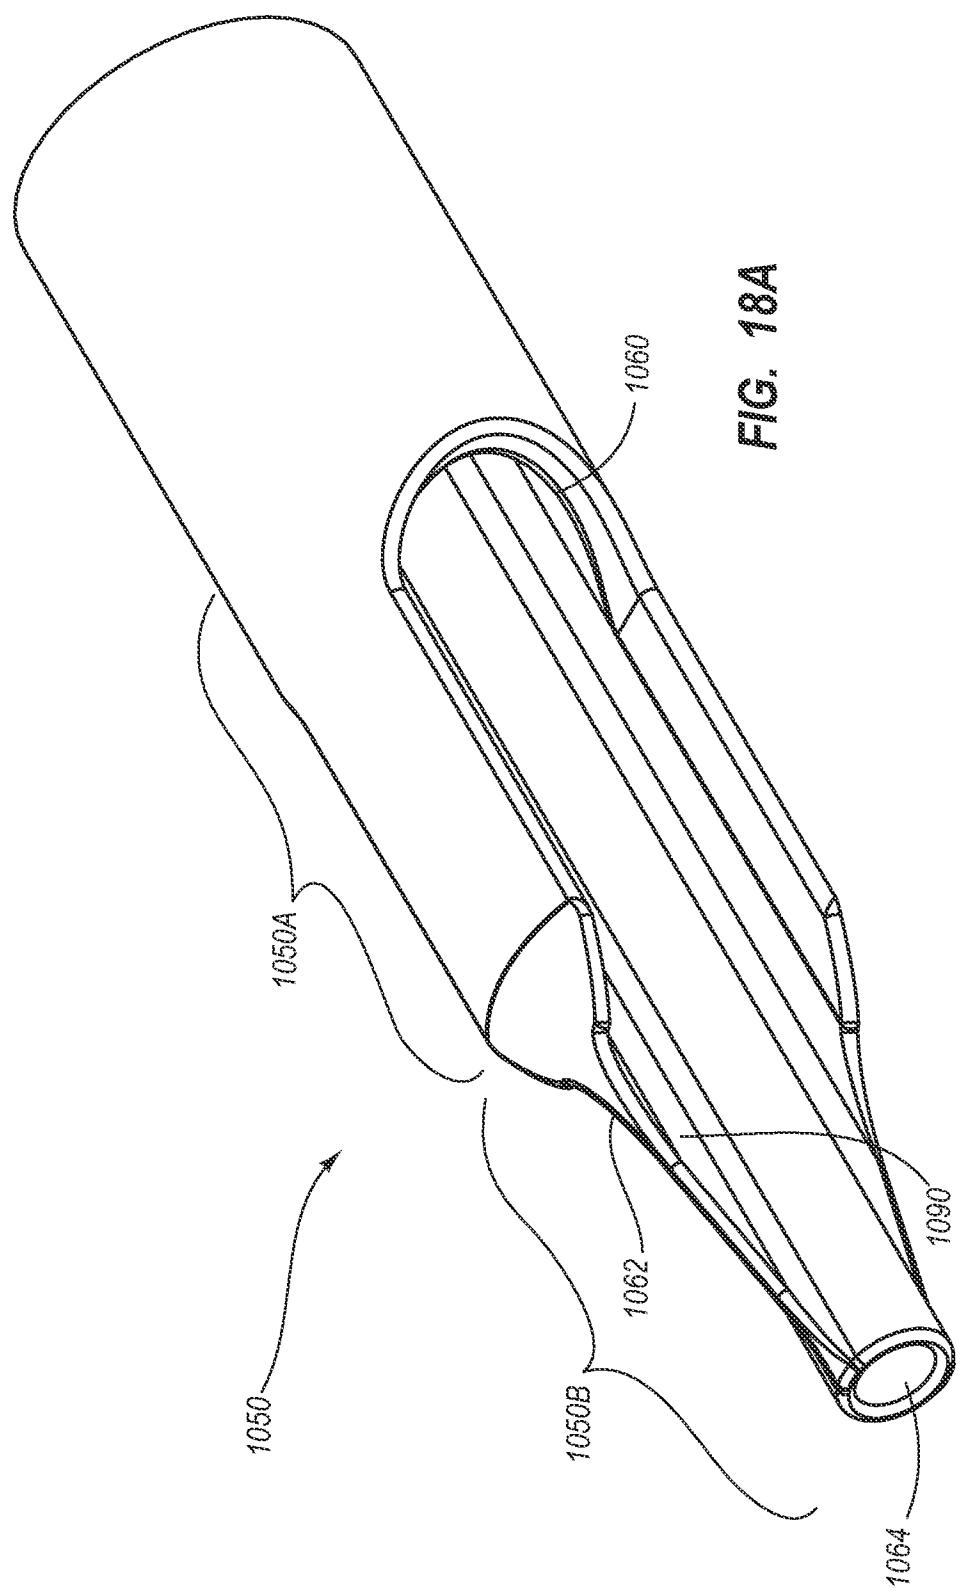


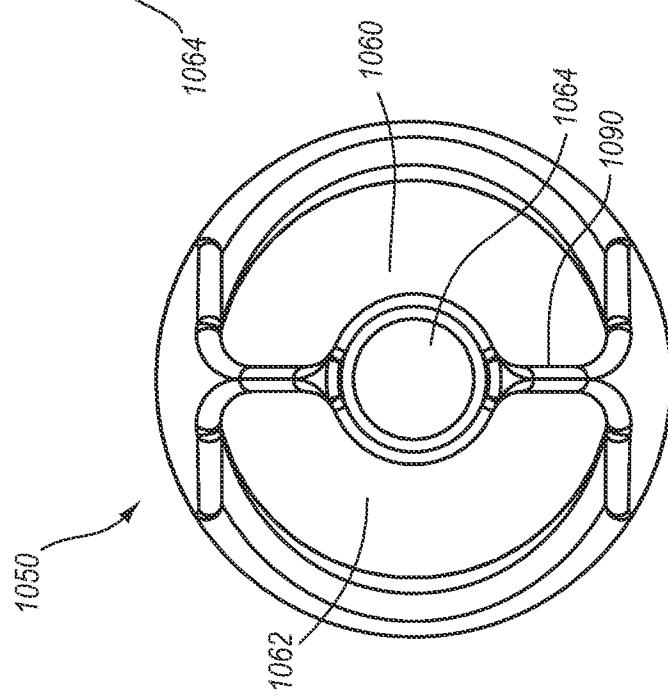


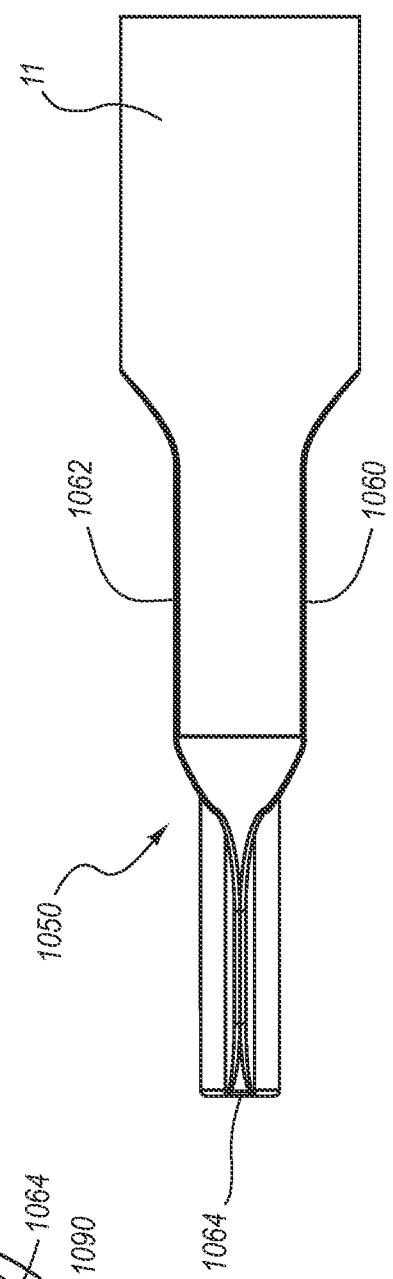




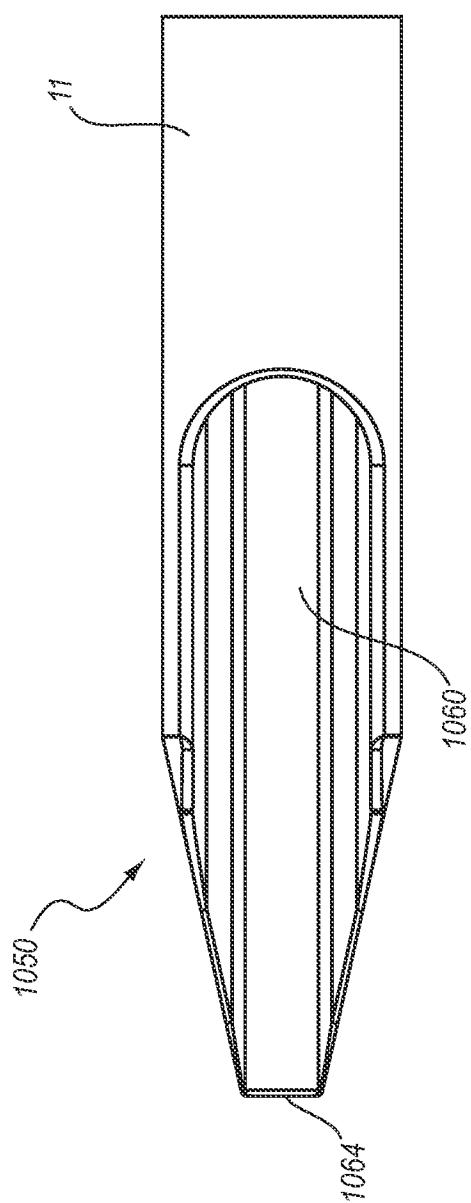


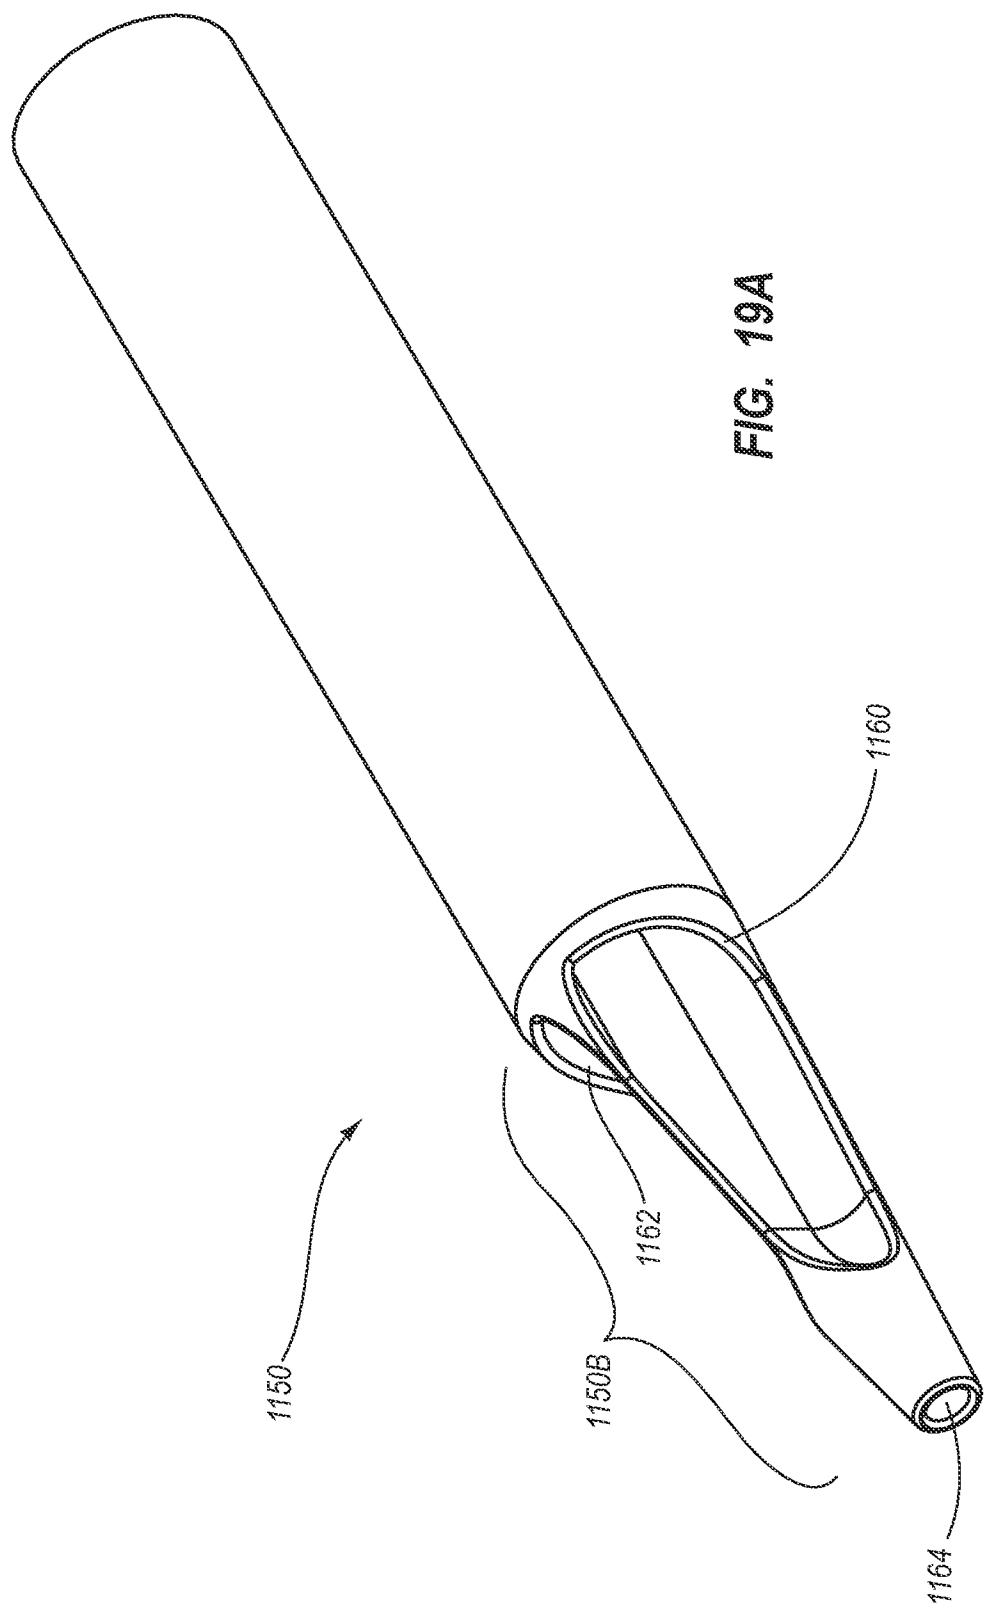

31 / 33

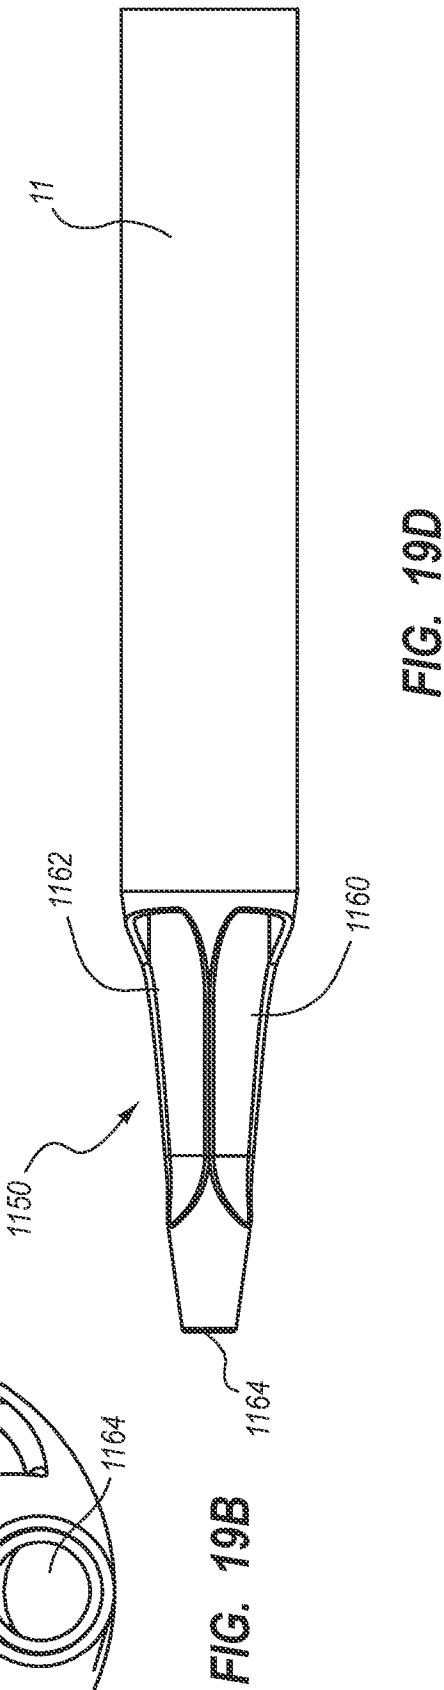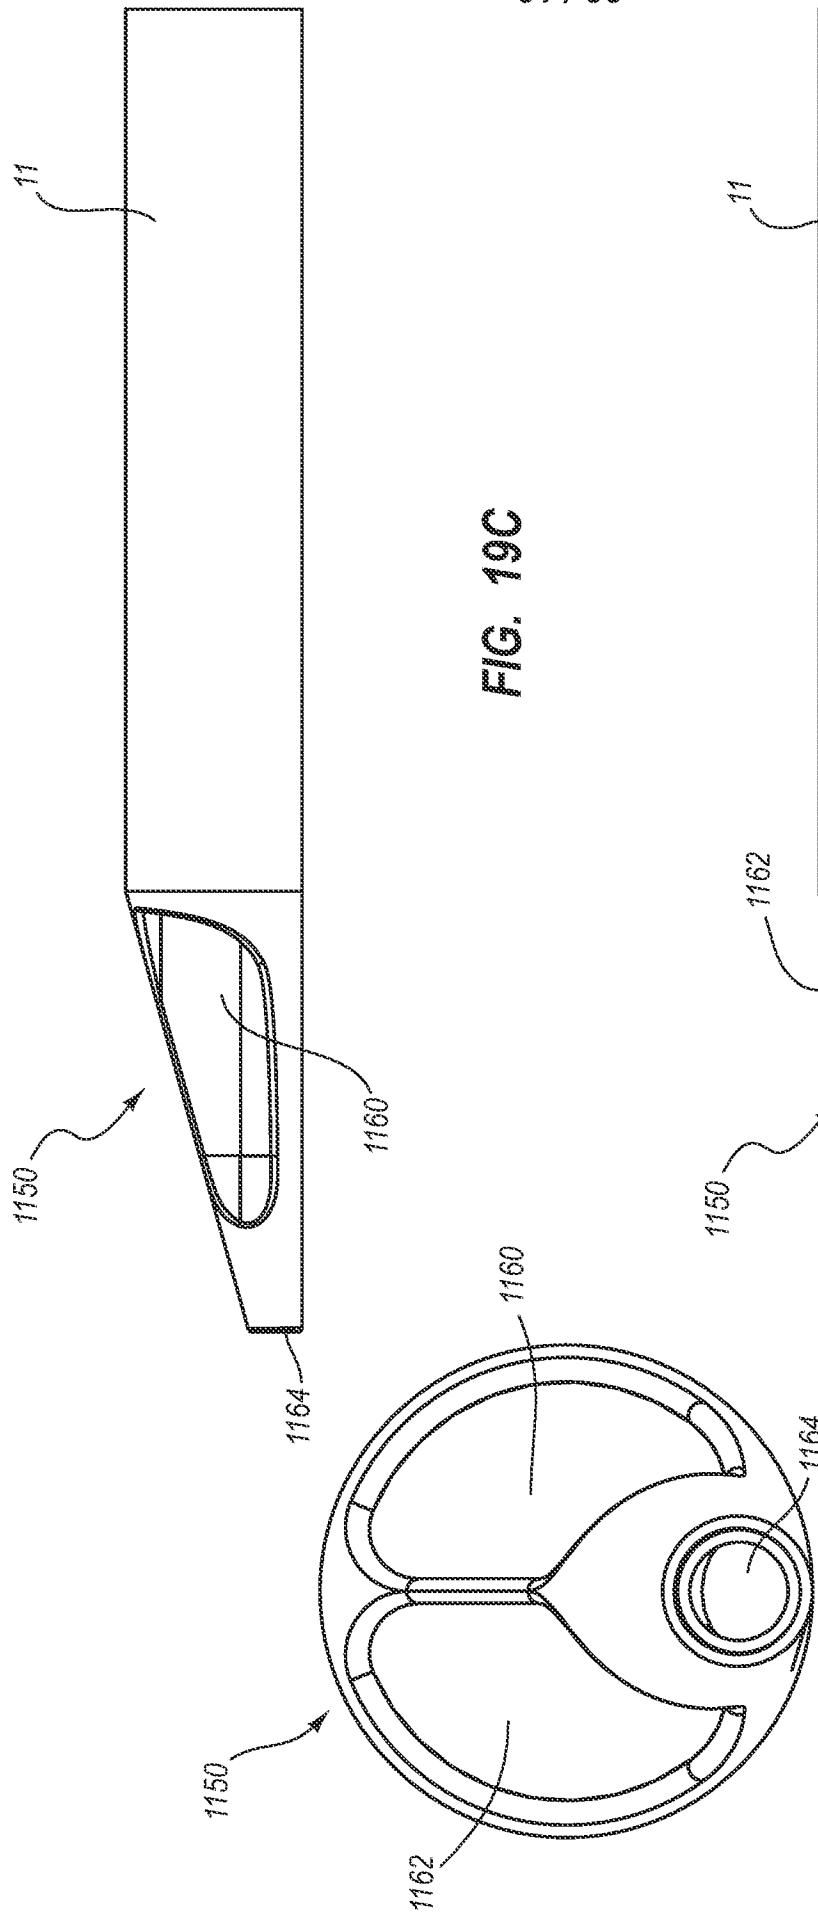

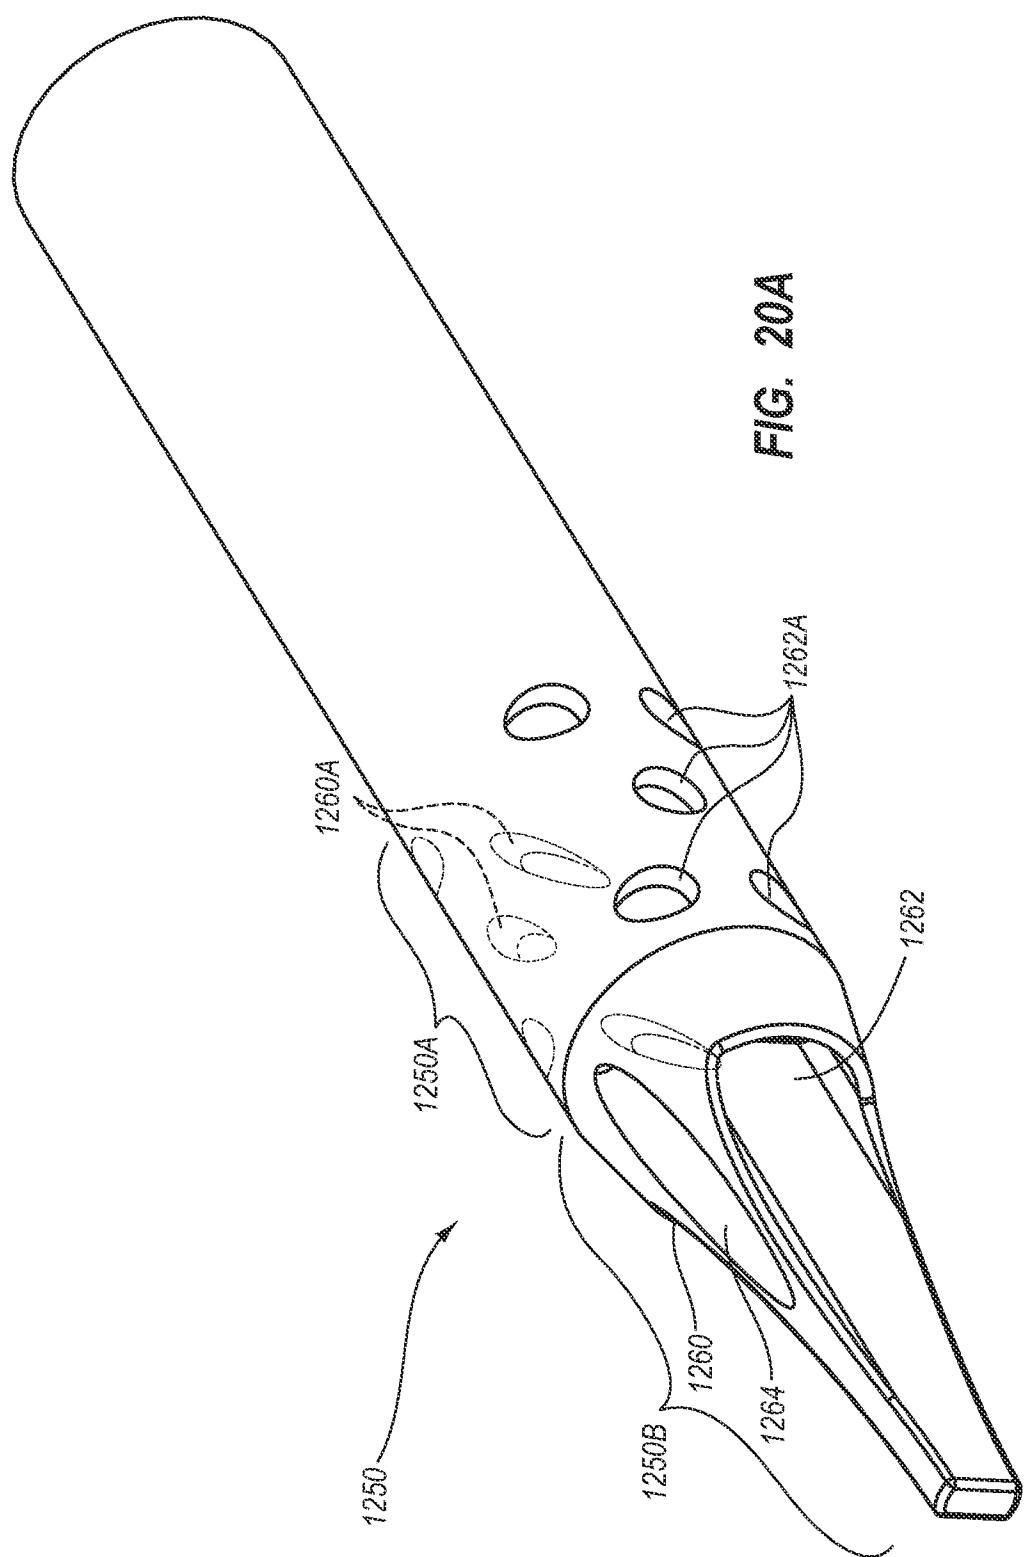

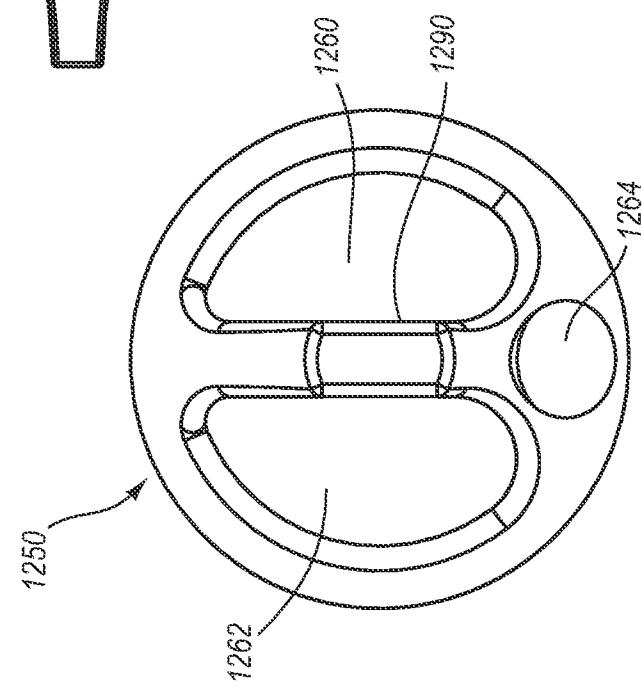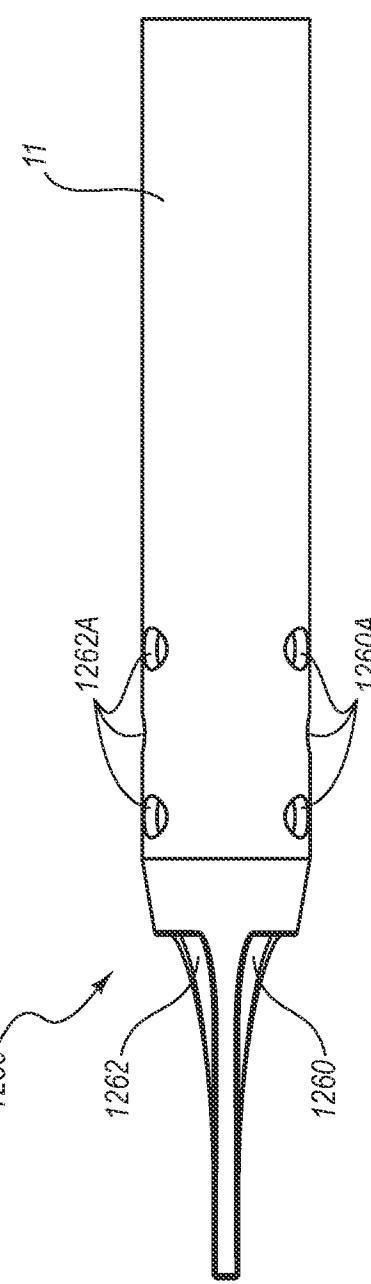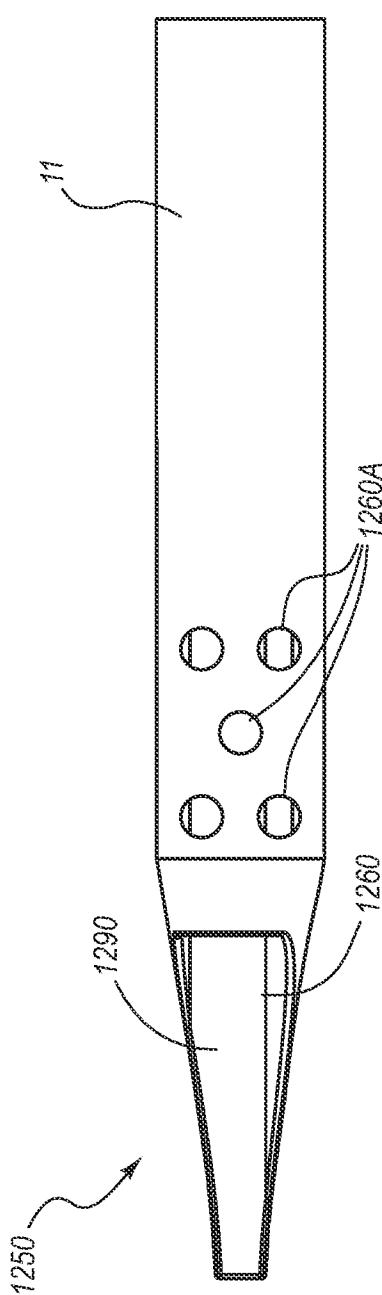

# INTERNATIONAL SEARCH REPORT

International application No.

PCT/US 08/82106

## A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61M 25/00 (2008.04)

USPC - 604/272

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

USPC: 604/272

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched  
USPC:604/4.01,48,93.01,264

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

PubWEST(USPT,PGPB,EPAB,JPAB), Google patent, Google Scholar

Search Terms: catheter assembly, renal replacement, first and second lumens, distal tip, venous, arterial, lateral opening, un-staggered, fluid communication, third lumen,RF fusion

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5,451,206 A (YOUNG) 19 September 1995 (29.09.1995) entire document, especially col 4, In 54-60; col 4, In 65- col 5, In 3; col 5, In 7-15; col 5, In 44-52; col 7, In 18-22, In 31-34; col 7, In 40-42; col 7, In 43-54; col 7, In 55-63; col 7, In 64-col 8, In 4; col 8, In 5-16; col 8, In 32-37; col 8, In 44-55; col 8, In 59-63; col 11, In 51-66; col 11, In 67-col 12, In 9; col 12, In 47-60; col 12, In 61 -col 13, In 6; col 13, In 13-34; col 13, In 44-49; col 13, In 55-62; col 14,In 32-36; FIG.1	1-14, 20-23, 30, 32-41 ----- 19, 24-29, 31
Y	US 2005/0256461 A1 (DIFIORE) 17 November 2005 (17.11.2005) para[0074],[0094],[0097] claim 88, 89	15-19
Y	US 2007/0129704 A1 (O'MAHONY et al) 07 July 2007 (07.07.2007) para[0039]	15-19, 29
Y	US 2005/0027289 A1 (CASTELLANU et al) 03 February 2005 (03.02.2005) para[0043]	24, 27-29
Y	US 5,489,278 A (ABRAHAMSON) 06 February 1996 (06.02.1996) col 5,In 54-65;col 6, In15-19	25-26, 28, 29
Y	US 6,428,513 B1 (ABRAHAMSON) 06 August 2002 (06.08.2002) col 3, In 40-55; col 7, In 23-28	16, 31
Y	US 2005/0261663 A1 (PATTERSON et al) 24 November 2005 (24.11.2005) para[0239]	18

Further documents are listed in the continuation of Box C.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search	Date of mailing of the international search report
01 January 2009 (01.01.2009)	12 JAN 2009
Name and mailing address of the ISA/US Mail Stop PCT, Attn: ISA/US, Commissioner for Patents P.O. Box 1450, Alexandria, Virginia 22313-1450 Facsimile No. 571-273-3201	Authorized officer: Lee W. Young PCT Helpdesk: 571-272-4300 PCT OSP: 571-272-7774 