



(51) International Patent Classification:

G09B 9/00 (2006.01) *G09B 23/30* (2006.01)
G09B 23/28 (2006.01)

(21) International Application Number:

PCT/CA2016/050389

(22) International Filing Date:

5 April 2016 (05.04.2016)

(25) Filing Language:

English

(26) Publication Language:

English

(71) Applicant: **SYNAPTIVE MEDICAL (BARBADOS) INC.** [BB/BB]; Chancery House High Street, Bridgetown (BB).

(72) Inventors; and

(71) Applicants : **GMEINER, Timotheus Anton** [CA/CA]; 555 Richmond St. W., 8th Floor, Toronto, Ontario M5V 3B1 (CA). **KERINS, Fergal** [CA/CA]; 555 Richmond St. W., 8th Floor, Toronto, Ontario M5V 3B1 (CA). **CH-EUNG, Aaron Yu Lai** [CA/CA]; 555 Richmond St. W., 8th Floor, Toronto, Ontario M5V 3B1 (CA). **HOANG, Kimberly Bojanowski** [US/CA]; 555 Richmond St. W., 8th Floor, Toronto, Ontario M5V 3B1 (CA).

(74) Agent: **ROWAND LLP**; Suite 900, 357 Bay Street, Toronto, Ontario M5H 2T7 (CA).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: MULTI-METRIC SURGERY SIMULATOR AND METHODS

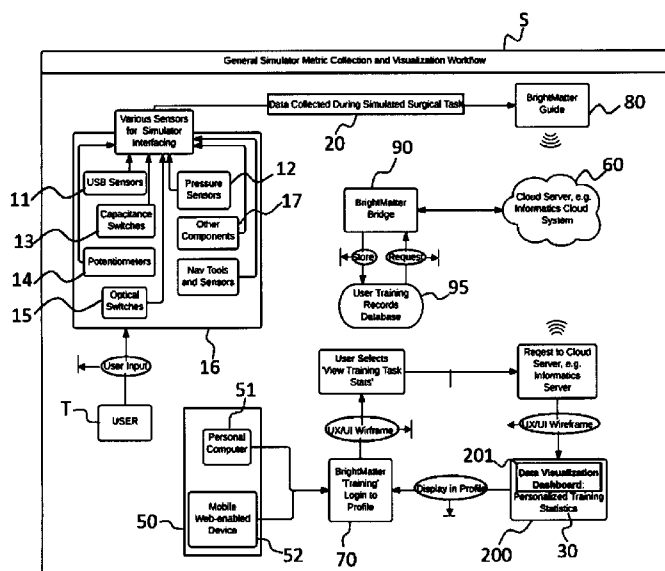


FIG. 1

(57) Abstract: Multi-metric surgery simulator devices, systems, and methods, involving at least one sensor configured to collect surgical training performance data relevant to at least one surgical task, the at least one sensor configured to operate with a surgical navigation system comprising a processor, the processor configurable, by way of a set of executable instructions storable in relation to a non-transitory medium, to perform at least one of analyze collected data, transform the collected data, and provide feedback in relation thereto; and at least one surgery simulator apparatus operatively coupled with the at least one sensor, the at least one surgery simulator apparatus configured to operate with a tracking system, whereby collected data is obtainable and clinical performance in relation to the at least one surgical task is quantitatively evaluable and progressively improvable.

MULTI-METRIC SURGERY SIMULATOR AND METHODS

TECHNICAL FIELD

5 [0002] The subject matter of the present disclosure generally relates to the field of surgery simulators. More particularly, the subject matter of the present disclosure technically relates to the field of surgery simulators in relation to image guided medical procedures. Even more particularly, the subject matter of the present disclosure technically relates to the field of surgery simulators in relation to image guided medical procedures with surgical navigation.

BACKGROUND

10 [0003] In the related art, surgery, such as neurosurgery, for example, brain tumors are typically excised through an open craniotomy approach guided by imaging. The data collected in these solutions typically consists of CT scans with an associated contrast agent, such as iodinated contrast agent, as well as MRI scans with an associated contrast agent, such as gadolinium contrast agent. Also, optical imaging is often used in the form of a microscope to differentiate
15 the boundaries of the tumor from healthy tissue, known as the peripheral zone. Tracking of instruments relative to the patient and the associated imaging data is also often achieved by way of external hardware systems such as mechanical arms, radiofrequency, or optical tracking devices. As a set, these devices are commonly referred to as surgical navigation systems and are often cumbersome and provide inaccurate tracking.

20 [0004] Port-based surgery is a minimally invasive surgical technique where a port is introduced to access a surgical region of interest using surgical tools. Unlike other minimally invasive techniques, such as laparoscopic techniques, a port diameter is larger than a tool diameter. Hence, the tissue region of interest is visible through the port, wherein exposed tissue in a region of interest, at a depth few centimetres below the skin surface, is accessible through a narrow
25 corridor in the port.

[0005] Several related art problems generally preclude or impair the ability to perform port-based navigation in an intra-operative setting. For example, the position of the port axis relative to a typical tracking device (TD) is a free and uncontrolled parameter that prohibits the determination of access port orientation. Further, the limited access which is available, due to

the required equipment for the procedure, causes indirect access port tracking to be impractical and unfeasible. Also, the requirement for angulation of the access port to access many areas within the brain during a procedure makes navigation of the access port a difficult and challenging problem that has not yet been addressed.

5 [0006] Additionally, the climbing costs of healthcare, coupled with alarming rates of malpractice suits, have highlighted the need for an efficient and effective method of surgical training in the related art, e.g., in relation to neurosurgery. Gross malpractice payments aside, surgical errors increase hospitalization time and adversely affect the health of patients, resulting in death or injury. The majority of these errors have been attributed to lack of skill and experience on the
10 part of medical personnel. A number of simulation tools have been used in the related art.

[0007] For instance, U.S. Patent Publication No. 20150347682 involves simulation by acquiring 2-D images, optionally including using X-rays, to generate 3-D or 4-D imaging. U.S. Patent Publication No. 20150347682 involves simulation by acquiring medical imaging data encoded in a standard video format. U.S. Patent Publication No. 20150086955 involves simulation of a
15 tissue model configured so that one or more of the layers are in the form of a lattice structure rather than fully solid layers using silicone with 3-D printing.

[0008] In another example, U.S. Patent Publication No. 20140378995 involves a simulator having a surgeon's console with a software suite to simulate a surgical instrument and a training environment. This related art simulator has training exercises corresponding to difficulty levels,
20 wherein, upon completion of a task, the user receives a report describing performance metrics and a composite score is calculated from these metrics in relation to the user's own performance.

[0009] In addition, in the related art, phantoms or simulators are used in surgical training. Certain sub-anatomical features present a development / manufacturing challenge in the related art. For example, brain ventricles are negative spaces within the brain that allow cerebral spinal
25 fluid (CSF) to circulate and nourish the brain and provide protection against compression. A number of related art methods for preparing these structures have experienced many challenges, such as a related art method of creating voids or negative spaces, wherein balloons are inflated within a liquid hydrogel and subsequently cooled. After one freeze-thaw cycle (FTC), the

balloon is removed from the hydrogel, whereby a scar is formed on the surface, thereby necessitating post-processing, such as back-filling with water and removal of air pockets that develop.

5 [0010] Accordingly, challenges experienced in the related art include inaccuracy in training surgeons to perform neurosurgery, especially in relation to situations involving real-time registration of a surgical trajectory in relation to the unique characteristics of a particular tissue types or sub-types, such as in relation to cerebral tissue. Therefore, a need exists for a surgery simulator that provides feedback in relation to the user's own performance, other users; performance, other statistical data, and ultimate performance goals, by way of a variety of
10 metrics.

BRIEF SUMMARY

[0011] In accordance with embodiments of the present disclosure, a variety of solutions address at least the related art challenges, in multi-metric devices, apparatuses, systems, and methods that provides feedback in relation to the user's own performance, other users; performance, other
15 statistical data, and ultimate performance goals, by way of a variety of metrics that include, that provides training in conjunction with surgical navigation systems for improving minimally invasive surgical procedures, such as an improved system and method for mapping navigation space to patient space modeling in relation to a given medical procedure, and that provides modeling of the unique characteristics of a particular tissue types or sub-types, for example,
20 cerebral tissue, as well as modeling of pathological tissue, wherein simulated tissue samples comprises a 3-D print or a rapid-prototype. By capturing the metrics of surgical training in relation to a variety of other metrics, as well as the user's metrics (multi-metric approach), data, and information, a surgeon's skill can be objectively evaluated in the embodiments of the present disclosure. The multi-metric devices, apparatuses, systems, and methods ensure that training
25 sessions are more than just simulated "experiences" as multi-metric simulation provides a quantitatively validated clinical function. To date, such capabilities have been hitherto unknown in the related art.

[0012] In accordance with an embodiment of the present disclosure, a multi-metric surgery simulator system, comprises: at least one sensor configured to collect surgical training performance data relevant to at least one surgical task, the at least one sensor configured to operate with a surgical navigation system comprising a processor, the processor configurable, by way of a set of executable instructions storable in relation to a non-transitory medium, to perform at least one of analyze collected data, transform the collected data, and provide feedback in relation thereto; and at least one surgery simulator apparatus operatively coupled with the at least one sensor, the at least one surgery simulator apparatus configured to operate with a tracking system, whereby collected data is obtainable and clinical performance in relation to the at least one surgical task is quantitatively evaluable and progressively improvable.

[0013] In accordance with another embodiment of the present disclosure, a method of fabricating a multi-metric surgery simulator system, comprises: providing at least one sensor, providing the at least one sensor comprising: configuring the at least one sensor to collect surgical training performance data relevant to at least one surgical task, and configuring the at least one sensor to operate with a surgical navigation system comprising a processor, the processor configurable, by way of a set of executable instructions storable in relation to a non-transitory medium, to perform at least one of analyze collected data, transform the collected data, and provide feedback in relation thereto; and providing at least one surgery simulator apparatus, providing the at least one surgery simulator apparatus comprising: operatively coupling the at least one surgery simulator apparatus with the at least one sensor, configuring the at least one surgical simulator to operate with a tracking system, whereby collected data is obtainable and clinical performance in relation to the at least one surgical task is quantitatively evaluable and progressively improvable.

[0014] In accordance with yet another embodiment of the present disclosure, a method of quantitatively evaluating and progressively improving clinical performance of at least one surgical task by way of a multi-metric surgery simulator system, comprises: providing the metric surgery simulator system, comprising: providing at least one sensor, providing the at least one sensor comprising: configuring the at least one sensor to collect surgical training performance data relevant to at least one surgical task, and configuring the at least one sensor to operate with a surgical navigation system comprising a processor, the processor configurable, by way of a set of executable instructions storable in relation to a non-transitory medium, to perform

at least one of analyze collected data, transform the collected data, and provide feedback in relation thereto; and providing at least one surgery simulator apparatus, providing the at least one surgery simulator apparatus comprising: operatively coupling the at least one surgery simulator apparatus with the at least one sensor, configuring the at least one surgical simulator to operate
5 with a tracking system, whereby collected data is obtainable and clinical performance in relation to the at least one surgical task is quantitatively evaluable and progressively improvable; and using the metric surgery simulator system, thereby collecting surgical training performance data relevant to the at least one surgical task, obtaining the collected data, analyzing the collected data, transforming the collected data, providing the feedback in relation thereto, and
10 quantitatively evaluating and progressively improving the clinical performance.

[0015] Benefits of the multi-metric devices, apparatuses, systems, and methods of the present disclosure, using a multi-metric performance characterization, include, but are not limited to, establishing a benchmark level of proficiency for which a trainee must demonstrate at least competence, and preferably proficiency, before proceeding to further training. The multi-metric
15 approach ensures that in graduating trainees have a homogeneous skill-set; and the multi-metric approach is applicable to any level of training and any surgical procedure as the multi-metric simulator devices, system, and methods are reconfigurable for a plurality of tools and sensing or tracking devices in relation to the tools for quantifying relevant training milestones. Prospective, randomized, and blind clinical studies relating to the multi-metric approach of the present
20 disclosure have shown that trainees acquiring skills thereby perform significantly better *in vivo* as compared to traditionally trained colleagues using related art simulators.

[0016] Some of the features in the present disclosure are broadly outlined in order that the section entitled Detailed Description is better understood and that the present contribution to the art may be better appreciated. Additional features of the present disclosure are described
25 hereinafter. In this respect, understood is that the present disclosure is not limited in its application to the details of the components or steps set forth herein or as illustrated in the several figures of the being carried out in various ways. Also, understood is that the phraseology and terminology employed herein are for the purpose of the description and should not be regarded as limiting.

BRIEF DESCRIPTION OF THE DRAWING

[0017] The above, and other, aspects, features, and advantages of several embodiments of the present disclosure will be more apparent from the following Detailed Description as presented in conjunction with the following several figures of the Drawing.

5 [0018] FIG. 1 is a schematic diagram illustrating a multi-metric surgery simulator system, comprising at least one of an optical task training apparatus and a Raman spectroscopic identification training apparatus, configured to perform at least one of multi-metric data collection and data visualization, in accordance with an embodiment of the present disclosure.

[0019] FIG. 2 is a schematic diagram illustrating workflow relating to five visuomotor tasks
10 related to a given surgical procedure in relation to an optical task training apparatus, by example only, in accordance with an embodiment of the present disclosure.

[0020] FIG. 3 is a schematic diagram illustrating a multi-metric surgery simulator system, comprising an optical task training apparatus, as shown in FIG. 2, configured to perform at least one of multi-metric data collection and data visualization, in accordance with an
15 embodiment of the present disclosure.

[0021] FIG. 4 is a schematic diagram illustrating workflow relating to three visuomotor tasks, such as a craniotomy, a cannulation, and a resection, related to a given surgical procedure in relation to a Raman spectroscopic identification training apparatus, by example only, in accordance with an embodiment of the present disclosure.

20 [0022] FIG. 5 is a schematic diagram illustrating a multi-metric surgery simulator system, comprising Raman spectroscopic identification training apparatus, as shown in FIG. 4, configured to perform at least one of multi-metric data collection and data visualization, in accordance with an embodiment of the present disclosure.

[0023] FIG. 6A is a diagram illustrating a 2-D spiral training feature incorporable as an initial
25 exercise feature and/or reconfigurable in relation to a simple surgical task portion as included in a surgery simulator apparatus of a multi-metric surgery simulator system, showing a user's tracing by way of a pen-tipped tool or stylus, by example only, in accordance with an

embodiment of the present disclosure.

[0024] FIG. 6B is a diagram illustrating a 2-D spiral training feature incorporable as an initial exercise feature and/or reconfigurable in relation to a simple surgical task portion as included in a surgery simulator apparatus of a multi-metric surgery simulator system, showing another user's tracing by way of a pen-tipped tool or stylus, by example only, in accordance with an embodiment of the present disclosure.

[0025] FIG. 7 is a diagram illustrating an exploded perspective view of a surgery simulator apparatus of a multi-metric surgery simulator system, the surgery simulator apparatus comprising at least one of a simple surgical task portion and a complex surgical task portion, in accordance with an embodiment of the present disclosure.

[0026] FIG. 8A is a diagram illustrating a side view of a surgery simulator apparatus of a multi-metric surgery simulator system, as shown in FIG. 7, in accordance with an embodiment of the present disclosure.

[0027] FIG. 8B is a diagram illustrating a front view of a surgery simulator apparatus of a multi-metric surgery simulator system, as shown in FIG. 7, in accordance with an embodiment of the present disclosure.

[0028] FIG. 9 is a diagram illustrating a cross-sectional view of a surgery simulator apparatus of a multi-metric surgery simulator system, as shown in FIG. 7, in accordance with an embodiment of the present disclosure.

[0029] FIG. 10 is a diagram illustrating an exploded side view of a surgery simulator apparatus of a multi-metric surgery simulator system, the multi-metric surgery apparatus comprising at least one of a simple surgical task portion and a complex surgical task portion, in accordance with an embodiment of the present disclosure.

[0030] FIG. 11 is a diagram illustrating a top perspective view of a guide training feature having threaded eyebolts for guiding loops, as included in a simple surgical task portion shown in FIG. 10, by example only, in accordance with an embodiment of the present disclosure.

[0031] FIG. 12 is a diagram illustrating a top perspective view of a target training feature having pin holders, as included in a simple surgical task portion shown in FIG. 10, by example only, in accordance with an embodiment of the present disclosure.

5 [0032] FIG. 13 is a diagram illustrating a top perspective view of an incision training feature, as included in a complex surgical task portion shown in FIG. 10, by example only, in accordance with an embodiment of the present disclosure.

[0033] FIG. 14 is a diagram illustrating a top perspective view of a task cup configured to accommodate a suture training feature, as included in a complex surgical task portion shown in FIG. 10, by example only, in accordance with an embodiment of the present disclosure.

10 [0034] FIG. 15 is a diagram illustrating a top view of a simple surgical task portion comprising at least one of a 3-D spiral training feature, as included in a multi-metric surgery apparatus of a multi-metric surgery simulator system, in accordance with an embodiment of the present disclosure.

15 [0035] FIG. 16 is a diagram illustrating a top view of a simple surgical task portion comprising at least one of a 3-D spiral training feature, as included in a multi-metric surgery apparatus of a multi-metric surgery simulator system, in accordance with an embodiment of the present disclosure.

20 [0036] FIG. 17 is a diagram illustrating an alternative cut-away interior perspective view of a simple surgical task portion comprising at least one of a 3-D spiral training feature, as included in a multi-metric surgery apparatus of a multi-metric surgery simulator system, in accordance with an embodiment of the present disclosure.

[0037] FIG. 18 is a diagram illustrating several alternative color-code features, such as effected by way of 3-D printing or rapid-prototyping, relating to the simple surgical task portion, as shown in FIG. 15, in accordance with an embodiment of the present disclosure.

25 [0038] FIG. 19 is a diagram illustrating perspective views of color-code features, such as effected by way of 3-D printing, relating to the simple surgical task portion or any other

component of the multi-metric surgery apparatus, as shown in FIG. 10, by examples only, in accordance with alternative embodiments of the present disclosure.

[0039] FIG. 20 is a diagram illustrating a perspective view of a component comprising color-code features, such as effected by way of 3-D printing, relating to another component of the multi-metric surgery apparatus, as shown in FIG. 10, by example only, in accordance with alternative embodiments of the present disclosure.

[0040] FIG. 21 is a flow diagram illustrating a method of fabricating a multi-metric surgery simulator system, in accordance with an embodiment of the present disclosure

[0041] FIG. 22 is a flow diagram illustrating a method of quantitatively evaluating and progressively improving clinical performance of at least one surgical task by way of a multi-metric surgery simulator system, in accordance with an embodiment of the present disclosure.

[0042] Corresponding reference numerals or characters indicate corresponding components throughout the several figures of the Drawing. Elements in the several figures are illustrated for simplicity and clarity and have not necessarily been drawn to scale. For example, the dimensions of some of the elements in the figures may be emphasized relative to other elements for facilitating understanding of the various presently disclosed embodiments. Also, common, but well-understood, elements that are useful or necessary in commercially feasible embodiment are often not depicted in order to facilitate a less obstructed view of these various embodiments of the present disclosure.

20

DETAILED DESCRIPTION

[0043] The multi-metric simulator devices, apparatuses, systems, and methods of the present disclosure enhance the acquisition and maintenance of surgical skills in the realm of surgical training, wherein learning is optimized by way of the multi-metric feedback. The multi-metric feedback unambiguously characterizes a plurality of important aspects corresponding to each procedure of a plurality of surgical procedures. The multi-metric feedback is generated by analyzing each surgical task of each surgical procedure for a given training session or training curriculum. Further, the multi-metric simulator devices, system, and methods involve a self-

reconfiguring feature, wherein the multi-metric feedback and/or the analysis related thereto also configure or reconfigure a given simulation in terms of visible presentation as well as function.

[0044] The subject matter described herein are useful in the field neurosurgery as well as the training thereof, including oncological care, neurodegenerative disease, stroke, brain trauma, and orthopedic surgery. However, the subject matter of the present disclosure may extend or apply to other conditions or fields of medicine; and such extensions or applications are encompassed by the present disclosure. The systems and methods described herein encompass surgical processes that are applicable to surgical procedures for brain, spine, knee, and any other region of the body that will benefit from the use of an access port or small orifice to access the interior of an animal body, such as a human body.

[0045] Various systems, apparatuses, devices, or processes are below-described and provide examples of the navigation systems and methods embodiments, in accordance with embodiments of the present disclosure. None of the below-described embodiments limits any claimed embodiment; and any claimed embodiment may also encompass systems, apparatuses, devices, or processes which may differ from below-described examples. The claimed embodiments are not limited to systems, apparatuses, devices, or processes having all of the features of any one of the below-described systems, apparatuses, devices, or processes or to features common to some or all of the below-described systems, apparatuses, devices, or processes.

[0046] Furthermore, this Detailed Description sets forth numerous specific details in order to provide a thorough understanding of the various embodiments described throughout the present disclosure. However, understood is that the embodiments described herein may be practiced without these specific details. In other instances, conventional methods, procedures, and components have not been described in detail to prevent obscuring the embodiments of the present disclosure.

[0047] Referring to FIG. 1, this schematic diagram illustrates a multi-metric surgery simulator system **S**, comprising at least one surgery simulator apparatus **100**, the at least one surgery simulator apparatus **100** comprising at least one of an optical task training apparatus and a Raman spectroscopic identification training apparatus, the Raman spectroscopic identification training apparatus comprising a modular Raman training feature, configured to perform at least one of multi-metric data collection, whereby collected data **20** is obtainable, and data visualization, whereby a data visualization dashboard **200** is displayable, e.g., via a display device (not shown), in accordance with an embodiment of the present disclosure. The optical task training apparatus comprises an Optical Task Trainer (OTT) or Clinical Skills Trainer (CST); and the Raman spectroscopic identification training apparatus comprising a modular Raman training feature, such as a Raman Spectroscopic Identification Trainer (RSIT). By using the OTT, the multi-metric surgery simulator system **S** is configured to educate surgical trainees, further educate practicing neurosurgeons, and other healthcare professionals on the specific utility of the optics system, such as the Synaptive® brightmatter™ guide system. The OTT comprises a tabletop tool configured to operate with the Synaptive® brightmatter™ navigation system **250**, the Synaptive® brightmatter™ drive system, and the Synaptive® brightmatter™ optics systems for synergistically combining the features thereof.

[0048] Still referring to FIG. 1, a multi-metric surgery simulator system **S**, comprises: at least one sensor **10** configured to collect surgical training performance data relevant to at least one surgical task, the at least one sensor **10** configured to operate with a surgical navigation system, such as Synaptive® brightmatter™ navigation system, comprising a processor, the processor configurable, by way of a set of executable instructions storable in relation to a non-transitory medium, to perform at least one of analyze collected data **20**, transform the collected data **20**, and provide feedback **30** in relation thereto; and at least one surgery simulator apparatus **100** operatively coupled with the at least one sensor **10**, the at least one surgery simulator apparatus **100** configured to operate with a tracking system, such as the Synaptive® brightmatter™ guide system, whereby the collected data **20** is obtainable, and whereby clinical performance in relation to the at least one surgical task is quantitatively evaluable and progressively improvable, in accordance with an embodiment of the present disclosure.

[0049] Still referring to FIG. 1, the multi-metric surgery simulator system **S** further comprises a tracking feature **40** (FIGS. 7-10) coupled with the at least one surgery simulator apparatus **100** and configured to receive at least one signal from the at least one sensor **10** and to transmit at least one signal to the at least one processor (not shown), the tracking feature **40** comprising at least one of an optical tracking feature operable with a pointer tool and a Raman spectroscopic tracking feature operable with a Raman probe tool, e.g., the RSIT, by example only.

[0050] Still referring to FIG. 1, the processor (not shown) is further configured to transmit at least one of the collected data **20**, the transformed collected data, and the feedback **30** to at least one of a user interface **50** and a storage medium. The user interface **50** is configured to provide access to at least one of the collected data **20**, the transformed collected data, and the feedback **30** by at least one of at least one trainee **T**, at least one trainer (not shown), and at least one peer (not shown) via at least one of a server-based application, an Internet-based application, a cloud-based application, a mobile application, and a social media application.

[0051] Still referring to FIG. 1, the user interface **50** comprises a display device, such as a portable electronic device, e.g., a laptop **51** and a handheld device **52**, e.g., a cellular phone and a smart phone. The storage medium comprises an informatics cloud, such as a non-transient memory device (not shown) and a cloud server, e.g., an informatics cloud server **60**. The feedback **30** further comprises a plurality of feedback cycles, the plurality of feedback cycles comprising consultation information from at least one of the at least one trainer and the at least one peer after a training session, whereby convergent training is facilitated.

[0052] Still referring to FIG. 1, the at least one sensor **10** comprises at least one of at least one USB sensor **11**, at least one pressure sensor **12**, at least one capacitance switch **13**, at least one potentiometer **14**, at least one optical switch **15**, at least one navigation tool sensor **16**, and the like. The at least one surgery simulator apparatus **100** is further operable with a spectral biopsy probe (not shown), a broadband probe (not shown), a near-infrared probe (not shown), a fluorescent probe (not shown), a parallel imaging probe (not shown), a magnetic resonance imaging probe (not shown), a structured light scanning probe (not shown), and an augmented reality tool (not shown).

[0053] Still referring to FIG. 1, the processor is further configured to transmit information to the user interface, the information comprising: a prompt for a user's login information; a dashboard for facilitating visualization of data; a display of a user's profile; a display of a trainee's visuomotor training task statistics; a display of a trainee's training records; and a display of a trainee's current training session data in relation to at least one dataset of: initial threshold data relating to the surgical task, a trainee's past training session data, at least one other trainee's past training session data, and transformed threshold data relating to the surgical task, the transformed threshold data comprising an iterative computation relating to at least one of the initial threshold data relating to the surgical task, the trainee's past training session data, and the at least one other trainee's past training session data, wherein the at least one dataset comprises at least one parameter of a merit point, a demerit point, and a task completion time.

[0054] Still referring to FIG. 1, the multi-metric surgery simulator system **S** is configured to provide improved surgical fidelity in relation to a plurality of imaging tools or visualization tools, wherein surgical fidelity comprises the ability of a visualization tool to provide a trainee or a surgeon with visual input that results in the precise performance of a motor task in relation to initial exercise using basic endoscopes and basic microscopes, and in relation to subsequent exercises using the plurality of imaging tools. The multi-metric surgery simulator system **S** is configured to provide surgical training my way of a series of approximately six (6) exercises, by example only, whereby performance data is collected (collected data **20**) and transformed in relation to a trainee or a surgeon. The collected data **20** is transformed for generating conclusions relating to surgical fidelity as a function of experience level and imaging tool type. The collected data **20** is transformed to generate the feedback **30**, the feedback **30** comprising at least one demerit for inaccuracy in surgical tool positioning and a period of time for completion of each respective surgical task.

[0055] Still referring to FIG. 1, the feedback **30** further facilitates development of surgical skills by providing information to a user relating to visuomotor skills for surgical accuracy improvement over time regarding a trainee or a surgeon and by providing information to a user relating to the manner in which the skill improvement differs regarding a trainee or a surgeon, e.g., in relation to the trainee or surgeon, in relation to other trainees or surgeons, and/or in relation to historical data from at least one database. The feedback **30** further facilitates

updating of planned trajectories, e.g., during an actual surgical procedure as well as a simulation thereof. The multi-metric surgery simulator system **S**, being configured to provide improved surgical fidelity in relation to a plurality of imaging tools, improves a trainee's or a surgeon's ability to use indirect cues, such as motion parallax, relative size of structures, in-and-out movements, familiarity with image distortion, and the like, to compensate for lack of true three-dimensional perception, thereby decreasing learning curves.

[0056] Still referring to FIG. 1, the multi-metric simulator devices, apparatuses, and systems, are configurable and/or reconfigurable for a specific medical or surgical procedure. The multi-metric simulator system **S** comprises sensors **10** that collect data relevant to specific tasks being performed by a surgical trainee, such as the trainee **T**. The collected data **20** are stored, e.g., in cloud storage, such as via a Synaptive® system's informatics-cloud; and feedback based on the collected data **20** is visible (displayable) to a user, e.g., a trainee **T** and/or other relevant party at his/her convenience. After a training session, through feedback **30** from the Synaptive® system's ecosystem during a training session, reference to a user's training performance data, and consultation with at least one of at least one trainer and at least one peer, a trainee **T** experiences significantly more feedback cycles relating to his/her training than provided by related art simulators. By coupling this type of infrastructure with Synaptive® surgical simulators, e.g., the system **S**, of various kinds, e.g., using Synaptive® surgical navigation systems, Synaptive® tracking systems, and the like, the trainee **T** would be able to see progressive improvement in key visuomotor skills before *in vivo* skill testing and at significantly more convenience and lower cost than by using cadavers.

[0057] Still referring to FIG. 1, the multi-metric simulator system **S** of the present disclosure is used as a skill development tool for training surgeons and obtaining quantitative metrics on their progress in conjunction with a Synaptive® technology suite, whereby the multi-metric simulator system **S** is configured to link thereto via the Synaptive® brightmatter™ Guide **80** to the Synaptive® brightmatter™ Bridge **90** for facilitating storing performance data in a database **95**, e.g., a web-app-accessible database. This linking feature enables users, training centers, and clinical administrators to log-in, evaluate, and share performance statistics for better understanding as to the manner in which a trainee's performance compares with a trainee's previous performance as well as with peers or to historical averages, whereby social components

are incorporable into the multi-metric simulator system **S**, e.g., via competition features and prize features to motivate surgical residents to strive for the utmost in surgical proficiency.

[0058] Still referring to FIG. 1, the multi-metric simulator system **S** of the present disclosure is configured to demonstrate all Synaptive® hardware/software and could scale for integration with magnetic resonance (MR), combined Raman Spectroscopy (RS) and Optical Coherence Tomography (OCT) ("Raman-OCT"), and a myriad of other current and future devices. The datasets generated by the multi-metric simulator system **S** are useable for collecting historical statistical data on how surgeons use our tool which could aid in verification and validation (V&V) procedure, generation marketing, the manner in which a surgeon's performance is improvable by reconfiguration or self-reconfiguration of the multi-metric simulator system via additional product variables, e.g., feature offerings, that are identifiable via operation of the multi-metric simulator system. The multi-metric simulator devices, apparatuses, systems, and methods of the present disclosure encompass general workflow application, wherein the multi-metric simulator apparatus comprises at least one of optical task trainer (OTT) and a Raman-Spectroscopy identification trainer (RSIT).

[0059] Referring to FIG. 2, this schematic diagram illustrates workflow **WF** relating to five visuomotor tasks related to a given surgical procedure in relation to a surgery simulator apparatus **100** comprising an optical task training apparatus having an optical tracking feature, by example only, in accordance with an embodiment of the present disclosure. For a surgery simulator apparatus **100** comprising an optical task training apparatus having an optical tracking feature, the at least one surgical task comprises at least one training routine of a spiral target routine (FIGS. 6A and 6B), a fiducial marker point routine, a blind target routine, and a suturing routine (FIG. 14), by example only. The optical task training apparatus, having an optical tracking feature, is iteratively operable in relation to one through five of five tasks for generating two performance datasets, e.g., indicating total demerit points and task completion time, in accordance with an embodiment of the present disclosure. The optical task training apparatus **OTT** is configured to communicate with navigation system **250**; and the navigation system **250** is configured to communicate with a planning system **255**.

[0060] Still referring to FIG. 2 and ahead to FIGS. 15-17, by example only, the workflow WF relating to five visuomotor tasks comprises a first simple visuomotor task (Visuomotor Task 1), the first simple visuomotor task comprising: guiding or tracing, using a tool with a pen tip, along a 2-D spiral path of the 2-D spiral training feature 128; and observing the tracing via a microscope and subsequently an endoscope, wherein a demerit point is assigned for each instance that the tracing overlaps a designated boundary region of the 2-D spiral training feature 128, e.g., a darkened area, and wherein the number of demerit points is inversely related to a performance score, wherein a time period for completion of a surgical task is measured and recorded, and wherein the time period is inversely related to the performance score, and guiding (or tracing) (line series) a tool with a pen tip along a 3-D spiral path of the 3-D spiral training feature 128'; and observing the tracing via a microscope and subsequently an endoscope, wherein a demerit point is assigned for each instance that the tracing overlaps a designated boundary region of the 3-D spiral training feature 128', e.g., a darkened area, wherein the number of demerit points is inversely related to a performance score, wherein a time period for completion of a surgical task is measured and recorded, and wherein the time period is inversely related to the performance score.

[0060] Still referring to FIG. 2 and ahead to FIGS. 15-17, by example only, the workflow WF relating to five visuomotor tasks further comprises a second simple visuomotor task (Visuomotor Task 2), the second simple visuomotor task comprising: guiding or tracing a tool with a pen tip to locate a plurality of fiducial markers, wherein a portion of the plurality of fiducial markers are disposed deeper than another portion of fiducial markers, wherein at least a portion of the fiducial markers are disposed away from the trainee line of sight, wherein a demerit point is assigned for each instance that the tracing fails to coincide with fiducial markers, wherein the number of demerit points is inversely related to a performance score, and wherein a time period for completion of the second simple visuomotor task is measured and recorded.

[0061] Still referring to FIG. 2 and ahead to FIGS. 15-17, by example only, the workflow WF relating to five visuomotor tasks further comprises: a third simple visuomotor task (Visuomotor Task 3), the third simple visuomotor task comprising: guiding or tracing, using a tool with a pen tip, to locate a plurality 2-D, wherein at least a portion of the plurality 2-D lines

are disposed away from the trainee line of sight, wherein a demerit point is assigned for each instance that the tracing fails to coincide with the 2-D lines, and wherein a time period for completion of the third simple visuomotor task is measured and recorded; and a fourth simple visuomotor task (Visuomotor Task 4), the fourth simple visuomotor task comprising: guiding or tracing, using a tool with a pen tip, to locate a plurality 3-D, wherein at least a portion of the plurality 3-D lines are disposed away from the trainee line of sight, wherein a demerit point is assigned for each instance that the tracing fails to coincide with the 3-D lines, and wherein a time period for completion of the fourth simple visuomotor task is measured and recorded.

[0062] Still referring to FIG. 2 and ahead to FIGS. 15-17, by example only, the workflow WF relating to five visuomotor tasks further comprises: a fifth simple visuomotor task (Visuomotor Task 5), the fifth simple visuomotor task comprising: performing suturing exercises, using an untracked tool around two small parallel pillars disposed in a perpendicular orientation relative to the trainee's line of sight, wherein at least a portion of the plurality 2-D lines are disposed away from the trainee line of sight, wherein a time period for completion of the third simple visuomotor task is measured and recorded.

[0063] Referring to FIG. 3, this schematic diagram illustrates a multi-metric surgery simulator system S, comprising a surgery simulator apparatus 100 comprising an optical task training apparatus having an optical tracking feature, as shown in FIG. 2, configured to perform at least one of multi-metric data collection and data visualization, in accordance with an embodiment of the present disclosure. By using the optical tracking feature, such as the OTT, a merit point is determined for the pointer tool moved within a predetermined boundary, a demerit point is determined for the pointer tool moved outside the predetermined boundary, and a task completion time is determined for each at least one training routine, by example only.

[0064] Referring to FIG. 4, this schematic diagram illustrates Raman task workflow **RTWF** relating to three visuomotor tasks, such as a craniotomy, a cannulation, and a resection, related to a given surgical procedure in relation to a surgery simulator apparatus **100**, as included in a multi-metric surgery simulator system **S**, comprising a Raman spectroscopic identification training apparatus having a Raman spectroscopic identification feature, e.g., a Raman task trainer **RTT**, by example only, in accordance with an embodiment of the present disclosure. By using the Raman spectroscopic tracking feature, the at least one surgical task comprises at least one of incision, craniotomy, cannulation, resection, transplantation, suturing, decannulating, and closing for each data type, such as data relating to the mass of removed simulated tour, the mass of removed simulated healthy tissue, and the duration for task completion (FIG. 5).

[0065] Still referring to FIG. 4, the surgery simulator apparatus **100**, as included in a multi-metric surgery simulator system **S**, comprising a Raman spectroscopic identification training apparatus having a Raman spectroscopic identification feature comprises surface-enhanced Raman scattering (SERS) nanoparticles configured to generate distinct spectra and are potentially useful as bright contrast agents for molecular diagnostics, in accordance with an embodiment of the present disclosure. Similarly, large volume liquid tissue "phantoms" that simulate breast and prostate cancerous tissue for Raman identification have been made using an intralipid (scattering agent), Indian ink (absorption agent), and synthesized calcification powder (calcium hydroxyapatite) and are encompassed by the present disclosure. The system **S** is configured as a Raman tissue simulator to accommodate a large volume tissue "phantom" or simulated tumour inserts, e.g., simulated cancerous tissue inserts, that contain elements that are responsive to Raman spectroscopy tools in a manner that is quantitatively evaluable.

[0066] Still referring to FIG. 4, the simulated tissue, e.g., a PVA-hydrogel doped with SERS nanoparticles, such as in the form of simulated brain tissue, is modeled to incorporate simulated imbedded tumor targets comprising Raman-spectroscopy-tunable and responsive to a Raman spectroscopy instrument, such as a spectroscopy probe **400**, wherein the simulated brain tissue is cannulable, having an identifiable spectra, inspectable with the Raman-probe, and resectable. For example, the surgery simulator apparatus **100**, comprising a Raman spectroscopic

identification training apparatus having a Raman spectroscopic identification feature, e.g., a Raman task trainer **RTT**.

[0067] Referring to FIG. 5, this schematic diagram illustrates a multi-metric surgery simulator system **S** comprising a surgery simulator apparatus **100**, the surgery simulator apparatus **100** comprising a Raman spectroscopic identification training apparatus having a Raman spectroscopic identification feature, e.g., a Raman task trainer **RTT**, as shown in FIG. 4, configured to perform at least one of multi-metric data collection and data visualization, in accordance with an embodiment of the present disclosure. For surgery simulator apparatus **100**, comprising the Raman spectroscopic tracking feature, for each at least one surgical task, a merit point is determined for resection of the at least one simulated pathological tissue feature by using data **501** collected in relation to the mass of the simulated pathological tissue feature, e.g., a simulated tumour, a demerit point is determined for resection of any portion of the at least one simulated healthy tissue feature by using data **502** collected in relation to the mass of the simulated healthy tissue feature, and a task completion time is determined by using data **503** collected in relation thereto. As such, three types of data **500** are collected and transmitted as collected data **20** to the guidance system, such as the Synaptive® brightmatter™ guidance system **80.0**

[0068] Still referring to FIG. 5, the surgery simulator apparatus **100** comprises a Raman spectroscopic identification training apparatus having a Raman spectroscopic identification feature, e.g., a Raman task trainer **RTT**. The system **S**, comprising the surgery simulator apparatus **100**, is compatible with any data-generating input and is linkable to any and all Synaptive® hardware, firmware, or software tools and incorporable in relations to a plurality of training simulation programs. For example, the system **S** is linkable to at least the following tools or equipment: the Synaptive® Spectral Biopsy Probe, the Synaptive® Spectroscopy Probe (broadband, NIR, Raman, Fluorescence, etc.), the Synaptive® parallel imaging probe, MRI equipment, structured light scanning equipment, the Synaptive® Mixed-Medical Reality hardware/software tools, the Synaptive® laser-ablation phantom, the Synaptive® Hematoma Task Trainer Phantom, the Synaptive® tumor resection phantom, the Synaptive® deep brain stimulation phantom, the Synaptive® endonasal procedure phantom, the Synaptive® lower lumbar procedure phantom, the Synaptive® orthopedic procedure phantom, and the like. In the

embodiments of the present disclosure, the collected data is transformed for providing feedback comprising key surgical performance indicators, wherein the system S is reconfigurable and scalable for simulating and training any medical device-coupled procedure.

[0069] Referring to FIG. 6A, this diagram illustrates a 2-D spiral training feature 128 incorporable as an initial exercise feature and/or in relation to an upper surface 111a of a simple surgical task portion fastener 111 for the simple surgical task portion 110 (FIG. 7), as included in a surgery simulator apparatus 100 of a multi-metric surgery simulator system S, showing a user's tracing 129a by way of a pen-tipped tool (not shown) or stylus (not shown), by example only, in accordance with an embodiment of the present disclosure. Initially, training may commence with a simple visuomotor task performed under a microscope and subsequently performed via an endoscope. For example, a first simple visuomotor task comprises guiding (or tracing) (line series) a tool with a pen tip along a 2-D spiral path of the 2-D spiral training feature 128; and observing the tracing via a microscope and subsequently an endoscope, wherein a demerit point is assigned for each instance that the tracing overlaps a designated boundary region of the 2-D spiral training feature 128, e.g., a darkened area, and wherein the number of demerit points is inversely related to a performance score, wherein a time period for completion of a surgical task is measured and recorded, and wherein the time period is inversely related to the performance score.

[0070] Referring to FIG. 6B, this diagram illustrates a 2-D spiral training feature 128 incorporable as an initial exercise feature and/or in relation to an upper surface 111a of a simple surgical task portion fastener 111 for the simple surgical task portion 110 (FIG. 7), as included in a surgery simulator apparatus 100 of a multi-metric surgery simulator system S, showing another user's tracing 129b by way of a pen-tipped tool (not shown) or stylus (not shown), by example only, in accordance with an embodiment of the present disclosure. Initially, training may commence with a simple visuomotor task performed under a microscope and subsequently performed via an endoscope. For example, a first simple visuomotor task comprises guiding (or tracing) a tool with a pen tip along a 2-D spiral path; and observing the tracing via a microscope and subsequently an endoscope, wherein a demerit point is assigned for each instance that the tracing overlaps a designated boundary region of the 2-D spiral training feature 128, e.g., a darkened area, and wherein the number of demerit points is

inversely related to a performance score, wherein a time period for completion of a surgical task is measured and recorded, and wherein the time period is inversely related to the performance score.

[0071] Still referring to FIG. 6B and referring back to FIG. 6A, the 2-D spiral training feature 128 is incorporable in relation to the upper surface 111a of a simple surgical task portion fastener 111 for the simple surgical task portion 110 (FIG. 7) is configured to support at least one of at least one surgical task pattern (not shown) and at least one simulated tissue feature (not shown). The 2-D spiral training feature 128 may be modular and disposable within a recessed portion of the upper surface 111a. In the example shown in FIG. 6A, the at least one surgical task pattern optionally comprises a spiral configuration and may be incorporated into a modular member for coupling with the simple surgical task portion 110, such as by way of at least one clipping feature, by example only. Further, the at least one surgical task pattern comprises a modification of the 2-D spiral training feature 128 to provide a third dimension, e.g., depth, wherein the at least one surgical task pattern comprises a 3-D spiral training feature 128' configured to couple with the simple surgical task portion 110, as included in a surgery simulator apparatus 100 of a multi-metric surgery simulator system S, and provides training for following a surgical trajectory, such as would be defined by a surgical plan, e.g., for training an access port procedure. The 3-D spiral training feature 128' comprises a generally funnel shape (FIGS. 15-17) for disposition within the simple surgical task portion 110.

[0072] Still referring to FIG. 6B and referring back to FIG. 6A, the 2-D spiral training feature 128 and the 3-D spiral training feature 128' further provide training for: a second visuomotor task (point series) comprising touching a series of approximately eight (8) points with a tool having a pen tip, wherein a speed of execution is measured and recorded; a third visuomotor task (line/point series) comprising tracing a series of lines with the tool having the pen tip, wherein a speed of execution is measured and recorded, and wherein a demerit is assigned for each untouched dot disposed on the lines; a fourth visuomotor task (3D fidelity) comprising tracing two rows of five dots with the tool having the pen tip that scale the inside of the 3-D spiral training feature 128' (approximately 11 cm in height, approximately 9.5 cm, and approximately 5.2 cm in respective upper and base diameters), wherein the two rows of five dots are offset by approximately 2 cm from one another, and touching each of the dots from top

to bottom of the 3-D spiral training feature 128', wherein a speed of execution is measured and recorded, and wherein a demerit is assigned for each untouched dot on each row; a fifth visuomotor task (3D line/point series) comprising sequentially touching "thumb" tags pressed on the 3-D spiral training feature 128', moving from the deepest region to the shallowest region thereof, wherein a speed of execution is measured and recorded; and an optional sixth visuomotor task comprising moving four items from one cup to another using Adson pickups and tying a knot around pillars with a suture string at the lowest point of the OTT, e.g., at the complex surgical task portion 120, that accommodates a training feature comprising two cross pillars having an approximate 2 mm diameter and being disposed approximately 4 mm apart from one another, wherein a speed of execution is measured and recorded (FIG. 14).

[0073] Referring to FIG. 7, this diagram illustrates, in an exploded perspective view, a surgery simulator apparatus 100 of a multi-metric surgery simulator system S, the surgery simulator apparatus 100 comprising at least one of a simple surgical task portion 110 and a complex surgical task portion 120, by example only, in accordance with an embodiment of the present disclosure. Each at least one surgery simulator apparatus 100 comprises at least one of a simple surgical task portion 110 and a complex surgical task portion 120; and each of the simple surgical task portion 110 and the complex surgical task portion 120 is configured to support training of the at least one surgical task in at least one of two dimensions and three dimensions. Each at least one surgery simulator apparatus 100 further comprises a housing 130 for accommodating at least one of the simple surgical task portion 110 and the complex surgical task portion 120.

[0074] Still referring to FIG. 7, the simple surgical task portion 110 comprises and/or accommodates simple surgical procedure training features for developing fundamental surgical gestures or psychomotor actions for handling simple surgical tasks that are prerequisite to developing a coordination level sufficiently high for handling complex tasks. Simple surgical tasks comprise any visuomotor skill task, such as 2-D tasks, e.g., spiral tracings for training gross navigation skills, line tracing for training fine navigation skills, and dot drawing for training fine target skills, placing pegs in holes, placing rings over pegs for handling general fine motor skills, and transferring small items between microsurgical instruments for handling fine coordination skills, by examples only.

- [0075] Still referring to FIG. 7, the complex surgical task portion **120** comprises and/or accommodates complex surgical procedure training features for developing a coordination level for handling complex tasks, such as critical segments of a larger surgical procedure, e.g., having chronologically defined steps, wherein the complex surgical procedure training features
- 5 simulate the surgical environment for the complex surgical procedure, and wherein the complex surgical tasks comprise a plurality of simple surgical tasks and/or a plurality of complex surgical tasks relating to the large surgical procedure, e.g., a brain tumour removal procedure. Complex surgical tasks also comprise any involved fine motor skill task, such as 3-D tasks, e.g., isolated knot-tying for training fine motor and coordination skills, simulated tumor
- 10 removal for training resection skills, simulated aneurysm-clipping for training fine incision and suturing skills, simulated pedicle screw placement for training fine tapping, drilling, and turning skills, simulated spinal decompression with depth coloring features for training drilling, simulated inter-body fusion for training disk-fusing and the like, simulated fluid column use for verifying integrity of anastomosis or dural repair, by examples only.
- 15 [0076] Still referring to FIG. 7, each at least one surgery simulator apparatus **100** of a multi-metric surgery simulator system **S** further comprises at least one of: at least one simple surgical task portion fastener **111** for facilitating disposition of the at least one of the simple surgical task portion **110** in relation to the housing **130**; at least one complex surgical task portion fastener **121** for facilitating disposition of the complex surgical task portion **120** in relation to
- 20 the simple surgical task portion **110**; and at least one housing fastener **131** for facilitating disposition of the housing **130** in relation to a generally horizontal surface (not shown), such as a workbench, laboratory bench, and a tabletop. The at least one surgery simulator apparatus **100** is configured to couple with the tracking feature **40**, wherein the tracking feature **40** comprises at least one tracking marker **41**, trackable by a tracking system.
- 25 [0077] Still referring to FIG. 7, the housing **130** comprises a generally angled frusto-conical configuration for facilitating simulation of a clinical access port environment. The at least one simple surgical task portion fastener **111** comprises at least one of at least one retention ring and any other suitable fastener. The at least one complex surgical task portion fastener **121** comprises at least one of at least one retention ring and any other suitable fastener. The at least
- 30 one housing fastener **131** comprises at least one of a screw, a bolt, a nut, a threaded, a hook-

and-loop fastener, and any other suitable fastener. The simple surgical task portion 110 comprises at least one of a generally conical configuration, a plurality of pin surgical task features 112, and a plurality of loop surgical task features 113. At least one of the plurality of pin surgical task features 112 and the plurality of loop surgical task features 113 is operatively coupled with the at least one sensor 10.

[0078] Referring to FIG. 8A, this diagram illustrates, in a side view, a surgery simulator apparatus 100 of a multi-metric surgery simulator system S, as shown in FIG. 7, in accordance with an embodiment of the present disclosure. Each at least one surgery simulator apparatus 100 comprises at least one of a simple surgical task portion 110 and a complex surgical task portion 120; and each of the simple surgical task portion 110 and the complex surgical task portion 120 is configured to support training of the at least one surgical task in at least one of two dimensions and three dimensions. Each at least one surgery simulator apparatus 100 further comprises a housing 130 for accommodating at least one of the simple surgical task portion 110 and the complex surgical task portion 120. The system S further comprises a tracking apparatus 40, the tracking apparatus 40 comprising at least one tracking marker 41, such as at least one tracking sphere, by example only. The tracking apparatus 40 configured to track at least one tool used during training using the apparatus 100.

[0079] Referring to FIG. 8B, this diagram illustrates, in a front view, a surgery simulator apparatus 100 of a multi-metric surgery simulator system S, as shown in FIG. 7, in accordance with an embodiment of the present disclosure. Each at least one surgery simulator apparatus 100 comprises at least one of a simple surgical task portion 110 and a complex surgical task portion 120; and each of the simple surgical task portion 110 and the complex surgical task portion 120 is configured to support training of the at least one surgical task in at least one of two dimensions and three dimensions. Each at least one surgery simulator apparatus 100 further comprises a housing 130 for accommodating at least one of the simple surgical task portion 110 and the complex surgical task portion 120. The system S further comprises a tracking apparatus 40, the tracking apparatus 40 comprising at least one tracking marker 41, such as at least one tracking sphere, by example only. The tracking apparatus 40 configured to track at least one tool used during training using the apparatus 100.

[0080] Referring to FIG. 9, this diagram illustrates, in a cross-sectional view, a surgery simulator apparatus 100 of a multi-metric surgery simulator system S, as shown in FIG. 7, in accordance with an embodiment of the present disclosure. The plurality of pin surgical task features 112 comprises a plurality of pin holders 114 for accommodating a plurality of targets for facilitating training touching by at least one of at least one tool (not shown) and at least one instrument (not shown) in relation to the plurality of targets. The plurality of loop surgical task features 113 comprises a plurality of threaded eyebolts as guiding loops for facilitating training manipulation of at least one simulated elongated tissue feature therethrough.

[0081] Referring to FIG. 10, this diagram illustrates, in an exploded side view, a surgery simulator apparatus 100 of a multi-metric surgery simulator system S, the surgery simulator apparatus 100 comprising at least one of a simple surgical task portion 110 and a complex surgical task portion 120, in accordance with an embodiment of the present disclosure. The complex surgical task portion 120 comprises at least one of a generally cupped configuration, having a cap portion 124 and a cup portion 125, for facilitating simulation of a clinical subdural environment. The cup portion 125 accommodates the task cup 126. The cap portion 124 accommodates at least one simulated surface tissue feature (not shown) and facilitates training of the at least one surgical task in relation to the at least one simulated surface tissue feature (not shown). The cup portion 125 accommodates at least one simulated deep tissue feature (not shown) and facilitates training of the at least one surgical task in relation to the at least one simulated deep tissue feature (not shown).

[0082] Referring to FIG. 11, is a diagram illustrating a top perspective view of a guide training feature having threaded eyebolts, such as plurality of loop surgical task features 113, as included in a simple surgical task portion shown in FIG. 10, by example only, in accordance with an embodiment of the present disclosure. The plurality of loop surgical task features 113 comprises the plurality of threaded eyebolts as guiding loops for facilitating training manipulation of at least one simulated elongated tissue feature therethrough.

[0083] Referring to FIG. 12, is a diagram illustrating a top perspective view of a target training feature having pin holders, as included in a simple surgical task portion shown in FIG. 10, by example only, in accordance with an embodiment of the present disclosure. The plurality of

pin surgical task features **112** comprises a plurality of pin holders **114** for accommodating a plurality of targets for facilitating training touching by at least one of at least one tool (not shown) and at least one instrument (not shown) in relation to the plurality of targets.

5 [0084] Referring to FIG. 13, this diagram illustrates, in a top perspective view, an incision training feature **135** for facilitating training incising a bone cap and dura, as included in a complex surgical task portion **120** shown in FIG. 10, by example only, in accordance with an embodiment of the present disclosure. The at least one simulated surface tissue feature **135** comprises at least one of a simulated epidermal tissue feature (not shown), a simulated dermal tissue feature (not shown), a simulated sub-dermal tissue feature (not shown), a simulated
10 muscle tissue feature (not shown), a simulated cranial bone tissue feature **136**, and a simulated dura tissue feature **137**, by example only. At least one neurosurgical instrument **140**, such as a scalpel, may be used for training incising the at least one simulated surface tissue feature **135**. The simulated cranial bone tissue feature **136** comprises urethane or any material having properties that approximate that of natural bone, especially cranial tissue, by example only.

15 [0085] Still referring to FIG. 13, the incision training feature **135** facilitates training incising a bone cap and dura by providing training for approaching the surgical site, wherein training approaching comprises training commencing a craniotomy by forming a hole in a simulated cranium, thereby forming a cranial hole such as by forming a burr-hole, and a simulated bone portion, such as a simulated cranial flap, testing a range of motion of the port, and intra-
20 operatively adjusting the simulated trajectory if required, forming an opening in a simulated dura, thereby forming a simulated dural flap, stitching-back the simulated dural flap, inserting the port, along the simulated trajectory via navigation guidance, such as provided on the at least one display device, and coaxially positioning a surgical camera, such as the optical camera of an OTT feature, in relation to the port and the tracking feature **40**.

25 [0086] Referring to FIG. 14, this diagram illustrates, in a top perspective view, a task cup **126** configured to accommodate a suture training feature **127** for facilitating training suturing, as included in a complex surgical task portion **120** shown in FIG. 10, by example only, in accordance with an embodiment of the present disclosure. The complex surgical task portion **120** comprises at least one of a generally cupped configuration, having a cap portion **124** and a

cup portion **125**, for facilitating simulation of a clinical subdural environment. The cup portion **125** accommodates the task cup **126**, wherein the task cup **126** further accommodates at least one simulated deep tissue feature (not shown), such as a simulated vascular tissue feature (not shown), a simulated neural tissue feature (not shown), and a simulated cerebral tissue feature (not shown). At least one neurosurgical instrument **140** may be used for training incising the suture training feature **127**.

[0087] Referring to FIG. 15, this diagram illustrates, in a top view, a simple surgical task portion **110** comprising at least one of a 2-D spiral training feature **128** (FIGS. 6A and 6B) having at least one distinctive color-code feature **150**, at least one measurement feature **151**, guide training feature, such as the 2-D spiral training feature **128**, and a target training feature **152** having at least one distinctive color-code feature **153**, as included in a surgery simulator apparatus **100** of a multi-metric surgery simulator system **S**, in accordance with an embodiment of the present disclosure. In this example, the simple surgical task portion **110** may also accommodate at least one representation of at least one simulated tissue structure having at least one of at least two dimensions, at least one color, and at least one pattern (FIGS. 18-20). The representation of at least one simulated tissue structure comprises at least one simulated tissue feature **135**, wherein the at least one simulated tissue feature **135** comprises at least one of a simulated healthy tissue feature and a simulated pathological tissue feature. Laparoscopic training may be provided by way of a trainee touching the at least one distinctive color-code feature **153** using a pointer tool, a touch-pen, or a stylus (not shown). Such "touching" in terms of accuracy, pressure, and speed is measurable as part of the collected data **20**, e.g., via the OTT using the tacking apparatus **40** and effects an immediate response via the feedback **30** to the trainee.

[0088] Still referring to FIG. 15, at least one of the at least one surgical task pattern and the at least one simulated tissue feature **135** comprises at least one of a three-dimensional (3-D) color print and a surface-enhanced Raman Spectroscopy scattering material, wherein the surface-enhanced Raman Spectroscopy scattering material comprises a matrix material and a dopant, the matrix material comprising at least one of silicone and polyvinyl alcohol hydrogel, and the dopant comprising doped with at least one of a scattering agent, an absorption agent, and a calcification agent. The scattering agent comprises at least one of an intralipid and a

nanoparticle. The absorption agent comprises an India ink. The calcification agent comprises calcium hydroxyapatite. The surface-enhanced Raman Spectroscopy scattering material is tunable in relation to at least one of at least one pathological tissue type, at least one pathological tissue mass, and at least one pathological tissue density for simulation thereof.

- 5 The surface-enhanced Raman Spectroscopy scattering material comprises polyvinyl alcohol doped with at least one type of nanoparticle configured to simulate at least one of at least one disease state, at least one health condition, and the like. The simulator system S is configurable for use in virtual reality or augmented reality environments as well.

[0089] Still referring to FIG. 15, in accordance with the embodiments of the present disclosure,
10 the systems and methods comprise simulated anatomical features also include negative (fluid-filled) spaces as sub-anatomy features in anatomical simulators/phantoms and utilize printing 3D structures using materials which are dissolvable once the simulator has been produced. In an embodiment of the present disclosure, a method of fabricating a simulated anatomical feature comprises steps, such as 3D printing of the negative space required, e.g., brain ventricles with a
15 dissolvable material such as a PVA filament, to produce a printed 3D volume, and placing the printed 3D volume within a mold of an anatomical part, pouring a polyvinyl alcohol (PVA) formulation into a mold, thereby surrounding and encapsulating the printed 3D volume, exposing the encapsulated printed 3D volume to an appropriate number of freeze thaw cycles (FTC), thereby producing a tissue phantom with the desired biomechanical properties. The printed 3D
20 volume is then dissolved, at least in part, to produce a fluid filled void having the approximate size and approximate shape of the printed 3D volume, e.g., in the undissolved state.

[0090] Still referring to FIG. 15, in accordance with the embodiments of the present disclosure, the filament material that is used to print the 3D volume is configured to result in a 3D volume capable of maintaining structural integrity through a plurality of FTCs and of complete
25 dissolution for forming a negative space in the simulated tissue. The filament material comprises properties relating to a desired structural integrity. The filament material is also formable by printing the 3D volume and applying a protective layer of a water-resistant material to extend the filament material's life until the plurality of FTCs is complete.

[0091] Still referring to FIG. 15, in an embodiment of the present disclosure, a method of fabricating an anatomical feature that simulates the brain, the method comprises producing the ventricles and cerebral spinal fluid (CSF) by printing a PVA filament having a wall thicknesses, thereby providing a final solution having a targeted viscosity. This method ensures slowing the rate of equalization of concentrations of various materials, e.g., PVA and water, thereby preventing a change in shape of the structure or impinging on the shelf/usable life of the product. The method of fabricating an anatomical feature further comprises adding further materials, such as cornstarch, to a for facilitating water retention in the spaces, such as the ventricles and the spinal fluid areas.

[0092] Still referring to FIG. 15, in accordance with other embodiments of the present disclosure, the systems and methods comprise using alternative filaments, such as high impact polystyrene (HIPS) as a solute and limonene as dissolution agent. In accordance with other embodiments of the present disclosure, the systems and methods comprise using additives, such as salt, sugar, sand, and silicone may be used. In another embodiment, vascularity is presentable by 3D printing on a red plastic using a high resolution and PVA filament as scaffold, e.g., by placing the filament in a hydrogel contained in a silicone mold and immersing in the hydrogel formulation, thereby forming a simulator, optionally comprising a plurality of FTCs. The solution would dissolve the scaffold and form a cryogel supporting the printed structure.

[0093] Still referring to FIG. 15, in accordance with an embodiment of the present disclosure, a method of fabricating a simulated anatomical structure having at least one void comprises: 3D printing at least one simulated anatomical feature having at least one simulated sub-anatomical feature using a dissolvable material; supporting and enclosing the one or more structures in an interior of a mold of the anatomical phantom; filling a remaining internal volume in the interior of the mold between an outer surface of the one or more structures and an inner surface of the mold with a liquid precursor of a matrix material selected to mimic anatomical tissue and processing said liquid precursor to form a tissue mimic matrix material; and dissolving the one or more structures with a fluid selected to dissolve said dissolvable material to produce one or more internal cavities within the tissue mimic matrix material.

[0094] Still referring to FIG. 15, in accordance with an embodiment of the present disclosure, a method of fabricating a simulated void structure in a simulated anatomical structure comprises: printing, using 3D printing with silicone, one or more hollow structures of one or more desired sub-anatomical features, connecting the one or more hollow structures to a proximal end of an associated fluid flow channel; supporting and enclosing the one or more hollow structures and associated fluid flow channel in an interior of a mold of the anatomical phantom with a distal end of the associated fluid flow channel being located on an exterior of the mold; filling a remaining internal volume in the interior of the mold between an outer surface of both the one or more hollow structures and the associated vasculature and an inner surface of the mold with a liquid precursor of a matrix material selected to mimic anatomical tissue, the liquid precursor including at least polyvinyl alcohol, and curing the polyvinyl alcohol to produce a polyvinyl alcohol-based hydrogel to form a tissue mimic matrix material; and filling, through the access port, the one or more one hollow structures and their associated vasculature with liquid solutions selected to mimic preselected bodily fluids.

[0095] Referring to FIG. 16, this diagram illustrates, in a top view, a simple surgical task portion 110 comprising at least one of a 2-D spiral training feature 128 (FIGS. 6A and 6B) having a color-code feature 150, at least one measurement feature 151, guide training feature, such as the 2-D spiral training feature 128, and a target training feature 152 having a color-code feature 153, as (FIG. 15), as included in a surgery simulator apparatus 100 of a multi-metric surgery simulator system S, in accordance with an embodiment of the present disclosure. The at least one measurement feature 151 comprises a linear feature 151a and a plurality of graduated indicia 151b, e.g., for indicating depth. Each graduated indicia 151b of the plurality of graduated indicia 151b, comprises numeral indicia 151c for indicating a surgical depth.

[0096] Referring to FIG. 17, this diagram illustrates, in an alternative cut-away interior perspective view, a simple surgical task portion 110 comprising at least one of a 2-D spiral training feature 128 (FIGS. 6A and 6B) having a color-code feature 150, at least one measurement feature 151, guide training feature, such as the 2-D spiral training feature 128, and a target training feature 152 having a color-code feature 153 (FIG. 15), as included in a surgery simulator apparatus 100 of a multi-metric surgery simulator system S, in accordance with an embodiment of the present disclosure. The at least one measurement feature 151

comprises a linear feature **151a** and a plurality of graduated indicia **151b**, e.g., for indicating depth. Each graduated indicia **151b** of the plurality of graduated indicia **151b**, further comprises numeral indicia **151c** for indicating a surgical depth.

[0097] Referring to FIG. 18, this diagram illustrates several alternative color-code features **180**, such as effected by way of 3-D printing, e.g., a Stratasys® Polyjet® 3-D printing system, relating to the simple surgical task portion **110**, as shown in FIG. 15, in accordance with an embodiment of the present disclosure. The at least one simulated tissue feature **135**, comprising at least one of a three-dimensional (3-D) color print and a surface-enhanced Raman Spectroscopy scattering material, in embodiments of the present disclosure. The at least one simulated tissue feature **135** further comprises at least one of a polyvinyl alcohol (PVA) and a bio-compatible material.

[0098] Still referring to FIG. 18, in some embodiments of the present disclosure, the at least one of a three-dimensional (3-D) color print comprises a medical rapid-prototype material, such as a bio-compatible material or a simulated biological material. The medical rapid-prototype material enhances visualization and provides dimensional stability. The medical rapid-prototype material comprises a bio-compatible photopolymer, such as PolyJet® MED610, wherein bio-compatible photopolymer comprises a high dimensional stability and a colorless transparency in relation to other polymers and serves well as a simulated material, especially if combined with PVA.

[0099] Referring to FIG. 19, this diagram illustrates, in a close-up perspective view, a color-code features **180**, such as effected by way of 3-D printing, relating to the simple surgical task portion **110** or any other component of the surgery simulator apparatus **100**, as shown in FIG. 18, by examples only, in accordance with alternative embodiments of the present disclosure.

[0100] Referring to FIG. 20, this diagram illustrates, in a perspective view, a component **190** comprising color-code features **180**, such as effected by way of 3-D printing, relating to another component of the surgery simulator apparatus **100**, as shown in FIG. 18, by example only, in accordance with alternative embodiments of the present disclosure. [0101] Referring to FIG. 21, this flow diagram illustrates a method **M1** of fabricating a multi-metric surgery simulator

system **S**, in accordance with an embodiment of the present disclosure. The method **M1** comprises: providing at least one sensor, providing the at least one sensor comprising: configuring the at least one sensor to collect surgical training performance data relevant to at least one surgical task, and configuring the at least one sensor to operate with a surgical navigation system comprising a processor, the processor configurable, by way of a set of executable instructions storable in relation to a non-transitory medium, to perform at least one of analyze collected data, transform the collected data, and provide feedback in relation thereto, as indicated by block **2101**; and providing at least one surgery simulator apparatus, providing the at least one surgery simulator apparatus comprising: operatively coupling the at least one surgery simulator apparatus with the at least one sensor, configuring the at least one surgical simulator to operate with a tracking system, whereby collected data is obtainable and clinical performance in relation to the at least one surgical task is quantitatively evaluable and progressively improvable, as indicated by block **2102**.

[0102] Referring to FIG. 22, this flow diagram illustrates a method **M2** of quantitatively evaluating and progressively improving clinical performance of at least one surgical task by way of a multi-metric surgery simulator system **S**, in accordance with an embodiment of the present disclosure. The method **M2** comprises: providing the multi-metric surgery simulator system **S**, as indicated by block **2200**, providing the multi-metric surgery simulator system **S** comprising: providing at least one sensor **10**, providing the at least one sensor **10** comprising: configuring the at least one sensor **10** to collect surgical training performance data relevant to at least one surgical task, and configuring the at least one sensor **10** to operate with a surgical navigation system comprising a processor, the processor configurable, by way of a set of executable instructions storable in relation to a non-transitory medium, to perform at least one of analyze collected data, transform the collected data, and provide feedback in relation thereto, as indicated by block **2201**; and providing at least one surgery simulator apparatus **100**, providing the at least one surgery simulator apparatus **100** comprising: operatively coupling the at least one surgery simulator apparatus **100** with the at least one sensor **10**, configuring the at least one surgical simulator **100** to operate with a tracking system, whereby collected data **20** is obtainable and clinical performance in relation to the at least one surgical task is quantitatively evaluable and progressively improvable, as indicated by block **2202**; and using

the metric surgery simulator system **S**, thereby collecting surgical training performance data relevant to the at least one surgical task, obtaining the collected data **20**, analyzing the collected data **20**, transforming the collected data **20**, providing the feedback **30** in relation thereto, and quantitatively evaluating and progressively improving the clinical performance, as indicated by block **2203**. In the method **M2**, analyzing the collected data **20** comprises evaluating a trainee's current training session data in relation to at least one of initial threshold data relating to the surgical task, a trainee's past training session data, at least one other trainee's past training session data, and a historical average of at least one other trainee's past training session data.

[0103] Still referring to FIG. 22, transforming the collected data **20** in the method **M2** comprises at least one of: iteratively determining new threshold data using at least one of the trainee's current training session data in relation to at least one of the initial threshold data relating to the surgical task, the trainee's past training session data, the at least one other trainee's past training session data, and the historical average of at least one other trainee's past training session data; and incorporating at least one social component into the new threshold data, the at least one social component comprising at least one of a competitive award, a competitive prize, and the like, thereby providing historical statistical data for use in self-reconfiguring the at least one surgery simulator apparatus **100** for optimizing quantitative evaluation and progressive improvement of clinical performance and for optimizing integration with at least one of a plurality of tools, a plurality of instruments, a plurality of tracking systems, and a plurality of navigation systems.

[0104] Referring back to FIGS. 1-22, embodiments of the system **S** may be implemented using at least one processor with, or without, additional instructions stored in a memory, e.g., for execution by at least one general purpose microprocessor. Thus, the present disclosure is not limited to any specific configuration of hardware, firmware, and/or software. While some embodiments of the present disclosure are implementable in fully functioning computers and computer systems, various embodiments are capable of being distributed as a computing product in a variety of forms and are capable of being applied, regardless of the particular type of machine or computer readable media used to actually effect the distribution of the various embodiments. At least some aspects disclosed can be embodied, at least in part, in software. That is, the techniques may be carried out in a computer system or other data processing system

in response to a processor, such as a microprocessor, executing sequences of instructions contained in a memory, such as ROM, volatile RAM, non-volatile memory, cache, or a remote storage device. A computer readable storage medium can be used to store software and data which when executed by a data processing system causes the system to perform various methods. The executable software and data may be stored in various places including for example ROM, volatile RAM, nonvolatile memory and/or cache. Portions of this software and/or data may be stored in any one of these storage devices.

[0105] Still referring back to FIGS. 1-22, the preceding example embodiments involve systems and methods in which a device is intra-operatively configured based on the identification of a medical instrument. In other example embodiments, one or more devices may be automatically controlled and/or configured by determining one or more context measures associated with a medical procedure. A "context measure", as used herein, refers to an identifier, data element, parameter or other form of information that pertains to the current state of a medical procedure. In one example, a context measure may describe, identify, or be associated with, the current phase or step of the medical procedure. In another example, a context measure may identify the medical procedure, or the type of medical procedure, that is being performed. In another example, a context measure may identify the presence of a tissue type, or a simulated tissue type, during a medical procedure, or a surgical training session. In another example, a context measure may identify the presence of one or more fluids, such as biological fluids, simulated biological fluids, or non-biological fluids, e.g. wash fluids, during the medical procedure, and may further identify the type of fluid. Each of these examples relate to the image-based identification of information pertaining to the context of the medical procedure or simulated medical procedure.

[0106] Still referring back to FIGS. 1-22, examples of computer-readable storage media include, but are not limited to, recordable and non-recordable type media such as volatile and non-volatile memory devices, read only memory (ROM), random access memory (RAM), flash memory devices, floppy and other removable disks, magnetic disk storage media, optical storage media, e.g., compact discs (CDs), digital versatile disks (DVDs), etc. The instructions can be embodied in digital and analog communication links for electrical, optical, acoustical, or other forms of propagated signals, such as carrier waves, infrared signals, digital signals, and

the like. The storage medium may be the internet cloud, an informatics cloud server, or a computer readable storage medium such as a disc.

[0107] Still referring back to FIGS. 1-22, at least some of the methods described herein are capable of being distributed in a computer program product comprising a computer readable medium that bears computer usable instructions for execution by at least one processor to perform aspects of the methods described. The medium may be provided in various forms such as, but not limited to, one or more diskettes, compact disks, tapes, chips, USB keys, external hard drives, wire-line transmissions, satellite transmissions, internet transmissions or downloads, magnetic and electronic storage media, digital and analog signals, and the like. The computer useable instructions may also be in various forms, including compiled and non-compiled code.

[0108] While the present disclosure describes various embodiments for illustrative purposes, such description is not intended to be limited to such embodiments. On the contrary, the applicant's teachings described and illustrated herein encompass various alternatives, modifications, and equivalents, without departing from the embodiments, the general scope of which is defined in the appended claims. Except to the extent necessary or inherent in the processes themselves, no particular order to steps or stages of methods or processes described in this disclosure is intended or implied. In many cases the order of process steps may be varied without changing the purpose, effect, or import of the methods described.

[0109] Information as herein shown and described in detail is fully capable of attaining the above-described object of the present disclosure, the presently preferred embodiment of the present disclosure, and is, thus, representative of the subject matter which is broadly contemplated by the present disclosure. The scope of the present disclosure fully encompasses other embodiments which may become obvious to those skilled in the art, and is to be limited, accordingly, by nothing other than the appended claims, wherein any reference to an element being made in the singular is not intended to mean "one and only one" unless explicitly so stated, but rather "one or more." All structural and functional equivalents to the elements of the above-described preferred embodiment and additional embodiments as regarded by those of ordinary skill in the art are hereby expressly incorporated by reference and are intended to be

encompassed by the present claims. Moreover, no requirement exists for a system or method to address each and every problem sought to be resolved by the present disclosure, for such to be encompassed by the present claims. Furthermore, no element, component, or method step in the present disclosure is intended to be dedicated to the public regardless of whether the element, component, or method step is explicitly recited in the claims. However, that various changes and modifications in form, material, work-piece, and fabrication material detail may be made, without departing from the spirit and scope of the present disclosure, as set forth in the appended claims, as may be apparent to those of ordinary skill in the art, are also encompassed by the present disclosure.

INDUSTRIAL APPLICABILITY

[0110] The subject matter of the present disclosure industrially applies to the field of surgery simulators. More particularly, the subject matter of the present disclosure industrially applies to the field of surgery simulators in relation to image guided medical procedures. Even more particularly, the subject matter of the present disclosure industrially applies to the field of surgery simulators in relation to image guided medical procedures with surgical navigation.

CLAIMS

What is claimed:

1. A multi-metric surgery simulator system, comprising:

at least one sensor configured to collect surgical training performance data relevant to at least one surgical task, the at least one sensor configured to operate with a surgical navigation system comprising a processor, the processor configurable, by way of a set of executable
5 instructions storable in relation to a non-transitory medium, to perform at least one of analyze collected data, transform the collected data, and provide feedback in relation thereto; and

at least one surgery simulator apparatus operatively coupled with the at least one sensor, the at least one surgery simulator apparatus configured to operate with a tracking system, whereby collected data is obtainable and clinical performance in relation to the at least one
10 surgical task is quantitatively evaluable and progressively improvable.

2. The system of Claim 1, further comprising a tracking feature coupled with the at least one surgery simulator apparatus and configured to receive at least one signal from the at least one sensor and to transmit at least one signal to the at least one processor, the tracking feature comprising at least one of an optical tracking feature operable with a pointer tool and a Raman
5 spectroscopic tracking feature operable with a Raman probe tool.

3. The system of Claim 1,

wherein the processor is further configured to transmit at least one of the collected data, the transformed collected data, and the feedback to at least one of a user interface and a storage medium, and

5 wherein the user interface is configured to provide access to at least one of the collected data, the transformed collected data, and the feedback by at least one of at least one trainee, at least one trainer, and at least one peer via at least one of a server-based application, an Internet-based application, a cloud-based application, a mobile application, and a social media application.

4. The system of Claim 3, wherein the user interface comprises a display device.
5. The system of Claim 3, wherein the storage medium comprises an informatics cloud.
6. The system of Claim 5, wherein the feedback further comprises a plurality of feedback cycles, the plurality of feedback cycles comprising consultation information from at least one of the at least one trainer and the at least one peer after a training session, whereby convergent training is facilitated.
7. The system of Claim 1, wherein each at least one surgery simulator apparatus comprises at least one of a simple surgical task portion and a complex surgical task portion, each of the simple surgical task portion and the complex surgical task portion is configured to support training of the at least one surgical task in at least one of two dimensions and three dimensions,
- 5 the simple surgical task portion is configured to support training of the at least one simple surgical task prerequisite to handling a surgical procedure, and the complex surgical task portion is configured to support training of the at least one complex surgical task in the surgical procedure.
8. The system of Claim 7, wherein each at least one surgery simulator apparatus further comprises a housing for accommodating at least one of the simple surgical task portion and the complex surgical task portion.
9. The system of Claim 8, wherein each at least one surgery simulator apparatus further comprises at least one of:
- at least one simple surgical task portion fastener for facilitating disposition of the at least one of the simple surgical task portion in relation to the housing;
 - 5 at least one complex surgical task portion fastener for facilitating disposition of the complex surgical task portion in relation to the simple surgical task portion; and
 - at least one housing fastener for facilitating disposition of the housing in relation to a generally horizontal surface.

10. The system of Claim 8, wherein the housing comprises a generally angled frusto-conical configuration for facilitating simulation of a clinical access port environment.

11. The system of Claim 9,

wherein the at least one simple surgical task portion fastener comprises at least one of at least one retention ring and any other suitable fastener,

wherein the at least one complex surgical task portion fastener comprises at least one of
5 at least one retention ring and any other suitable fastener, and

wherein the at least one housing fastener comprises at least one of a screw, a bolt, a nut , a threaded, a hook and loop fastener, and any other suitable fastener.

12. The system of Claim 8,

wherein the simple surgical task portion comprises at least one of a generally conical configuration, a plurality of pin surgical task features, and a plurality of loop surgical task features, and

5 wherein at least one of the plurality of pin surgical task features and the plurality of loop surgical task features is operatively coupled with the at least one sensor.

13. The system of Claim 8, wherein the complex surgical task portion comprises at least one of a generally cupped configuration, having a cap portion and a cup portion, for facilitating simulation of a clinical subdural environment.

14. The system of Claim 13,

wherein the cap portion accommodates at least one simulated surface tissue feature and facilitates training of the at least one surgical task in relation to the at least one simulated surface tissue feature, and

5 wherein the cup portion accommodates at least one simulated deep tissue feature and facilitates training of the at least one surgical task in relation to the at least one simulated deep tissue feature.

15. The system of Claim 14,

wherein the at least one simulated surface tissue feature comprises at least one of a simulated epidermal tissue feature, a simulated dermal tissue feature, a simulated sub-dermal tissue feature, a simulated muscle tissue feature, a simulated cranial bone tissue feature, and a simulated dura tissue feature, and

wherein the at least one simulated deep tissue feature comprises at least one of a simulated vascular tissue feature, a simulated neural tissue feature, and a simulated cerebral tissue feature.

16. The system of Claim 12,

wherein the plurality of pin surgical task features comprises a plurality of pin holders as a plurality of targets for facilitating training touching by at least one of at least one tool and at least one instrument in relation to the plurality of targets, and

wherein the plurality of loop surgical task features comprises a plurality of threaded eyebolts as guiding loops for facilitating training manipulation of at least one simulated elongated tissue feature therethrough.

17. The system of Claim 7,

wherein at least one of the simple surgical task portion and the complex surgical task portion are configured to support at least one of at least one surgical task pattern and at least one simulated tissue feature,

wherein the at least one surgical task pattern optionally comprises a spiral configuration, wherein the at least one simulated tissue feature comprises a representation of at least one simulated tissue structure having at least one of at least two dimensions, at least one color, and at least one pattern, and

wherein the representation of at least one simulated tissue structure comprises at least one simulated tissue feature comprises at least one of a simulated healthy tissue feature and a simulated pathological tissue feature.

18. The system of Claim 17,

wherein at least one of the at least one surgical task pattern and the at least one simulated tissue feature comprises at least one of a three-dimensional color print and a surface-enhanced Raman Spectroscopy scattering material, and

- 5 wherein the surface-enhanced Raman Spectroscopy scattering material comprises a matrix material and a dopant, the matrix material comprising at least one of silicone and polyvinyl alcohol hydrogel, and the dopant comprising at least one of a scattering agent, an absorption agent, and a calcification agent.

19. The system of Claim 18, wherein the scattering agent comprises at least one of an intralipid and a nanoparticle.

20. The system of Claim 18, wherein the absorption agent comprises an India ink.

21. The system of Claim 18, wherein the calcification agent comprises calcium hydroxyapatite.

22. The system of Claim 17, wherein the surface-enhanced Raman Spectroscopy scattering material is tunable in relation to at least one of at least one pathological tissue type, at least one pathological tissue mass, and at least one pathological tissue density for simulation thereof.

23. The system of Claim 1, wherein the at least one sensor comprises at least one of at least one USB sensor, at least one pressure sensor, at least one capacitance switch, at least one potentiometer, at least one optical switch, at least one navigation tool sensor, and the like.

24. The system of Claim 1, wherein the at least one surgery simulator apparatus is further operable with a spectral biopsy probe, a broadband probe, a near-infrared probe, a fluorescent probe, a parallel imaging probe, a magnetic resonance imaging probe, a structured light scanning probe, and an augmented reality tool.

25. The system of Claim 17,

wherein, for an optical tracking feature, the at least one surgical task comprises at least one training routine of a spiral target routine, a fiducial marker point routine, a blind target routine, and a suturing routine,

5 wherein, for an optical tracking feature, for each at least one training routine, a merit point is determined for the pointer tool moved within a predetermined boundary, a demerit point is determined for the pointer tool moved outside the predetermined boundary, and a task completion time is determined,

10 wherein, for the Raman spectroscopic tracking feature, the at least one surgical task comprises at least one of incision, craniotomy, cannulation, resection, transplantation, suturing, decannulating, and closing, and

15 wherein, for the Raman spectroscopic tracking feature, for each at least one surgical task, a merit point is determined for resection of the at least one simulated pathological tissue feature, a demerit point is determined for resection of any portion of the at least one simulated healthy tissue feature, and a task completion time is determined.

26. The system of Claim 3, wherein the processor is further configured to transmit information to the user interface, the information comprising:

a prompt for a user's login information;

a dashboard for facilitating visualization of data;

5 a display of a user's profile;

a display of a trainee's visuomotor training task statistics;

a display of a trainee's training records; and

a display of a trainee's current training session data in relation to at least one dataset of:

initial threshold data relating to the surgical task,

10 a trainee's past training session data,

at least one other trainee's past training session data, and

transformed threshold data relating to the surgical task, the transformed threshold data comprising an iterative computation relating to at least one of the initial threshold data relating to the surgical task, the trainee's past training session data, and the at least one other trainee's past training session data, wherein the at least one dataset comprises at least one parameter of a merit point, a demerit point, and a task completion time.

15

27. A method of fabricating a multi-metric surgery simulator system, comprising:

providing at least one sensor, providing the at least one sensor comprising: configuring the at least one sensor to collect surgical training performance data relevant to at least one surgical task, and configuring the at least one sensor to operate with a surgical navigation system comprising a processor, the processor configurable, by way of a set of executable instructions storable in relation to a non-transitory medium, to perform at least one of analyze collected data, transform the collected data, and provide feedback in relation thereto; and

providing at least one surgery simulator apparatus, providing the at least one surgery simulator apparatus comprising: operatively coupling the at least one surgery simulator apparatus with the at least one sensor, configuring the at least one surgical simulator to operate with a tracking system, whereby collected data is obtainable and clinical performance in relation to the at least one surgical task is quantitatively evaluable and progressively improvable.

28. A method of quantitatively evaluating and progressively improving clinical performance of at least one surgical task by way of a multi-metric surgery simulator system, comprising:

providing the multi-metric surgery simulator system, comprising:

providing at least one sensor, providing the at least one sensor comprising: configuring the at least one sensor to collect surgical training performance data relevant to at least one surgical task, and configuring the at least one sensor to operate with a surgical navigation system comprising a processor, the processor configurable, by way of a set of executable instructions storable in relation to a non-transitory medium, to perform at least one of analyze collected data, transform the collected data, and provide feedback in relation thereto; and

providing at least one surgery simulator apparatus, providing the at least one surgery simulator apparatus comprising: operatively coupling the at least one surgery simulator apparatus with the at least one sensor, configuring the at least one surgical simulator to operate with a tracking system, whereby collected data is obtainable and clinical performance in relation to the at least one surgical task is quantitatively evaluable and progressively improvable; and

using the metric surgery simulator system, thereby collecting surgical training performance data relevant to the at least one surgical task, obtaining the collected data, analyzing

the collected data, transforming the collected data, providing the feedback in relation thereto, and
20 quantitatively evaluating and progressively improving the clinical performance.

29. The method of Claim 28, wherein analyzing the collected data comprises evaluating a trainee's current training session data in relation to at least one of initial threshold data relating to the surgical task, a trainee's past training session data, at least one other trainee's past training session data, and a historical average of at least one other trainee's past training session data.

30. The method of Claim 28, wherein transforming the collected data comprises at least one of:

iteratively determining new threshold data using at least one of the trainee's current training session data in relation to at least one of the initial threshold data relating to the surgical
5 task, the trainee's past training session data, the at least one other trainee's past training session data, and the historical average of at least one other trainee's past training session data; and

incorporating at least one social component into the new threshold data, the at least one social component comprising at least one of a competitive award, a competitive prize, and the like,

10 thereby providing historical statistical data for use in self-reconfiguring the at least one surgery simulator apparatus for optimizing quantitative evaluation and progressive improvement of clinical performance and for optimizing integration with at least one of a plurality of tools, a plurality of instruments, a plurality of tracking systems, and a plurality of navigation systems.

1/15

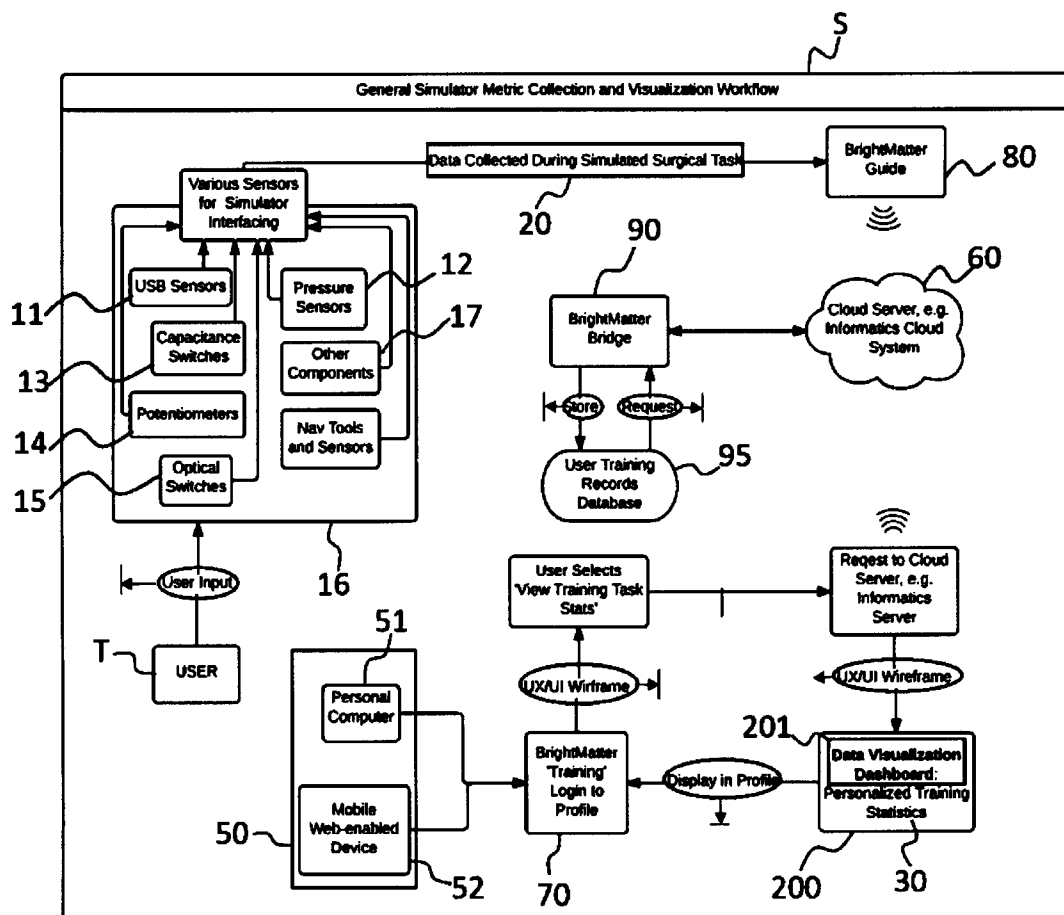


FIG. 1

2/15

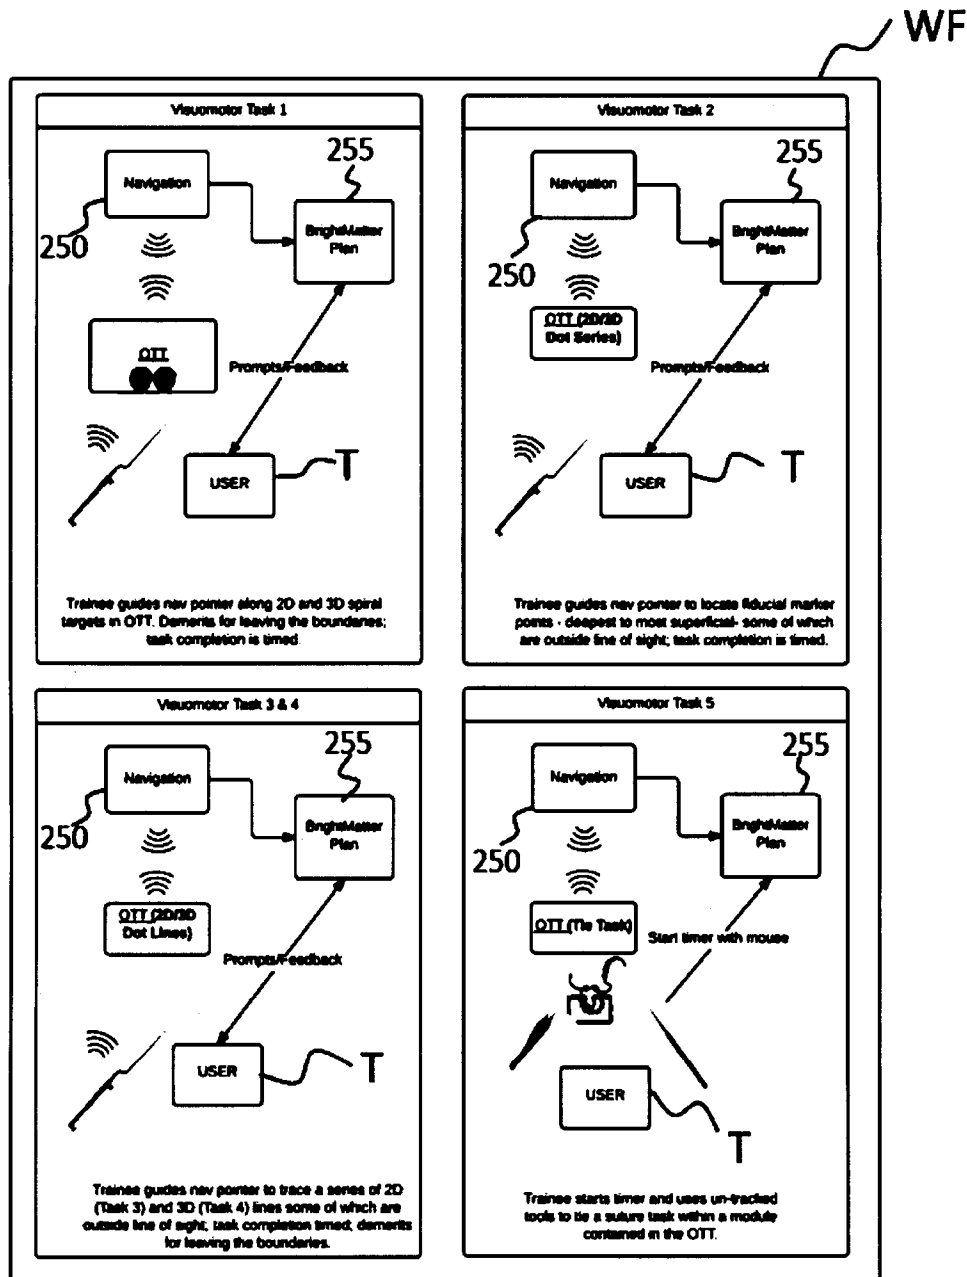


FIG. 2

3/15

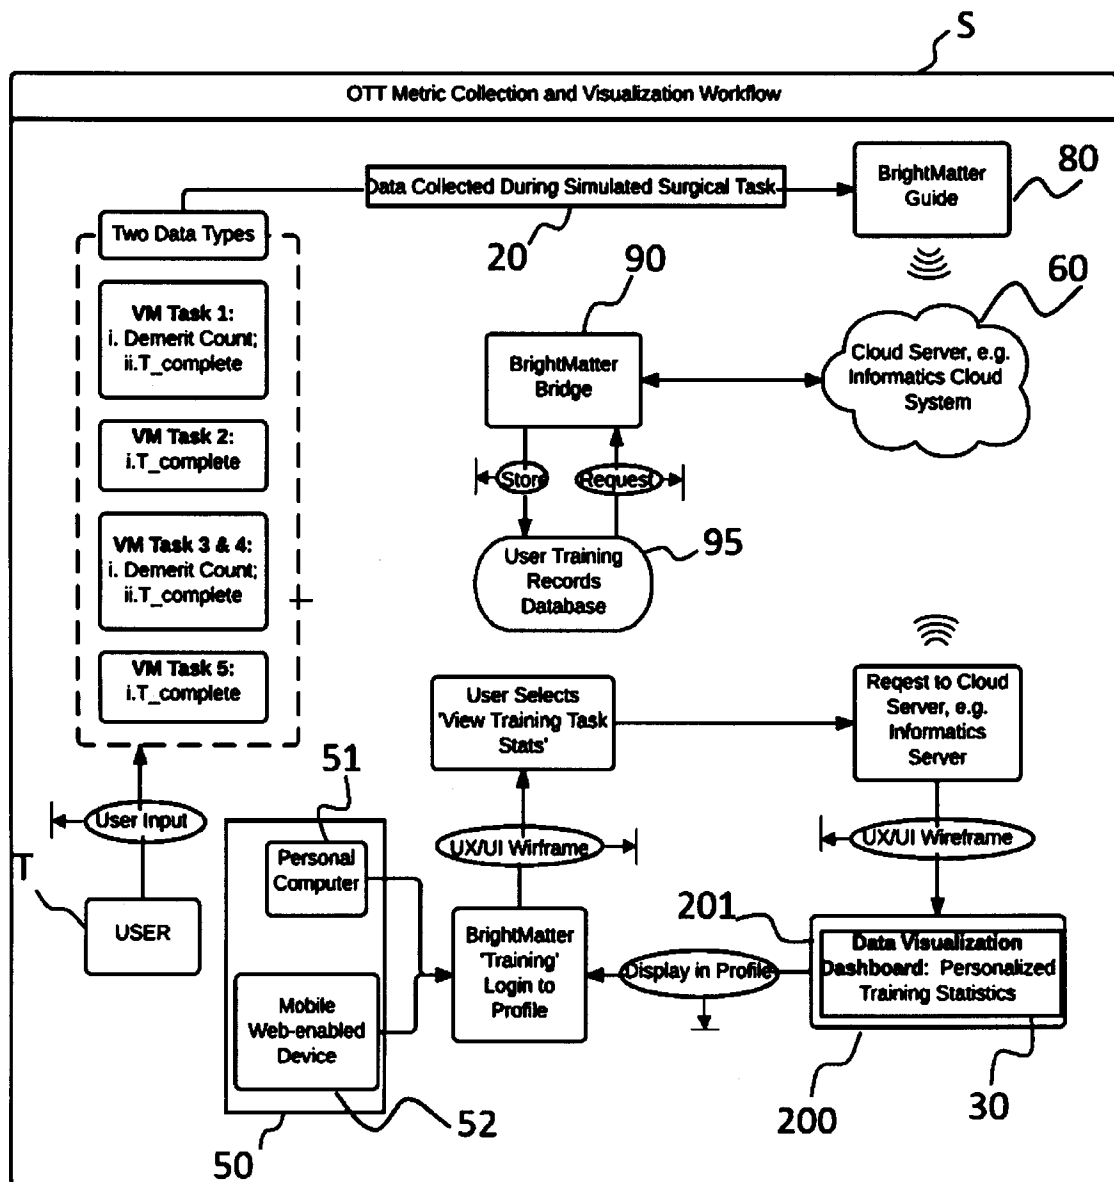


FIG. 3

4/15

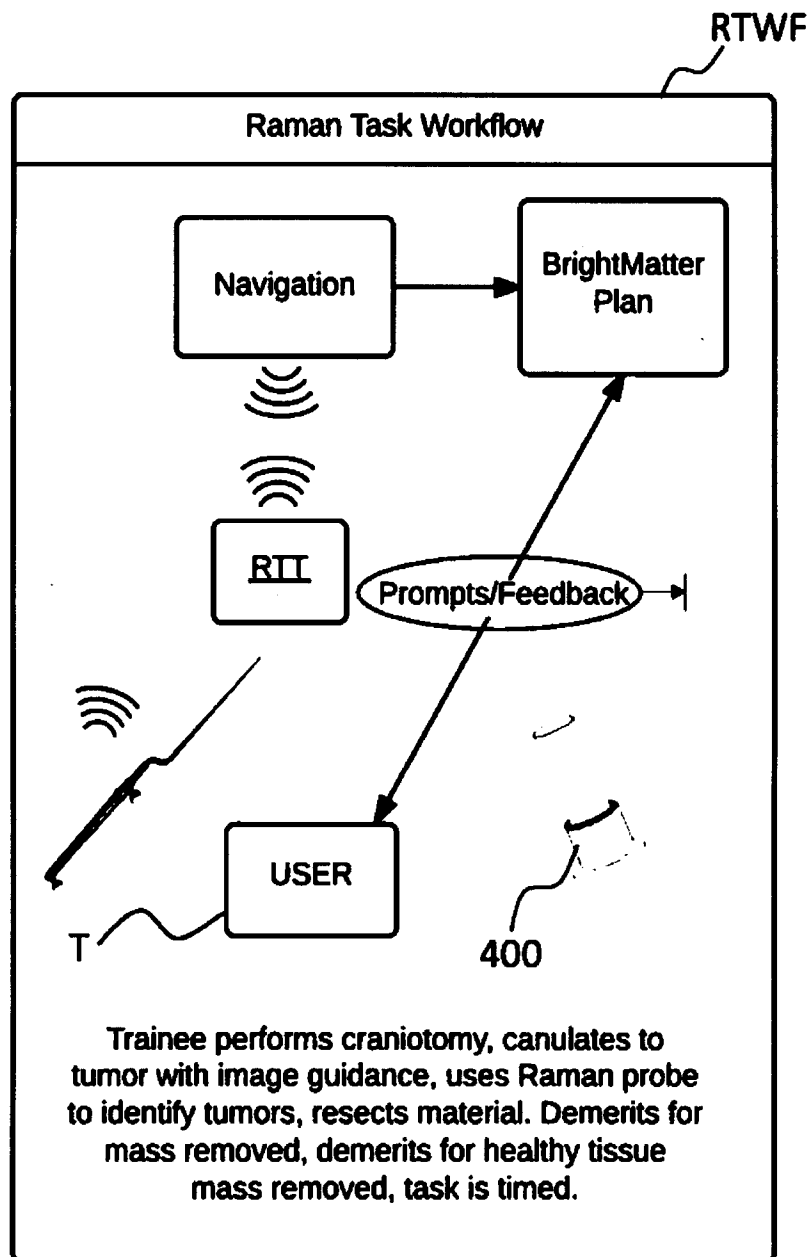


FIG. 4

5/15

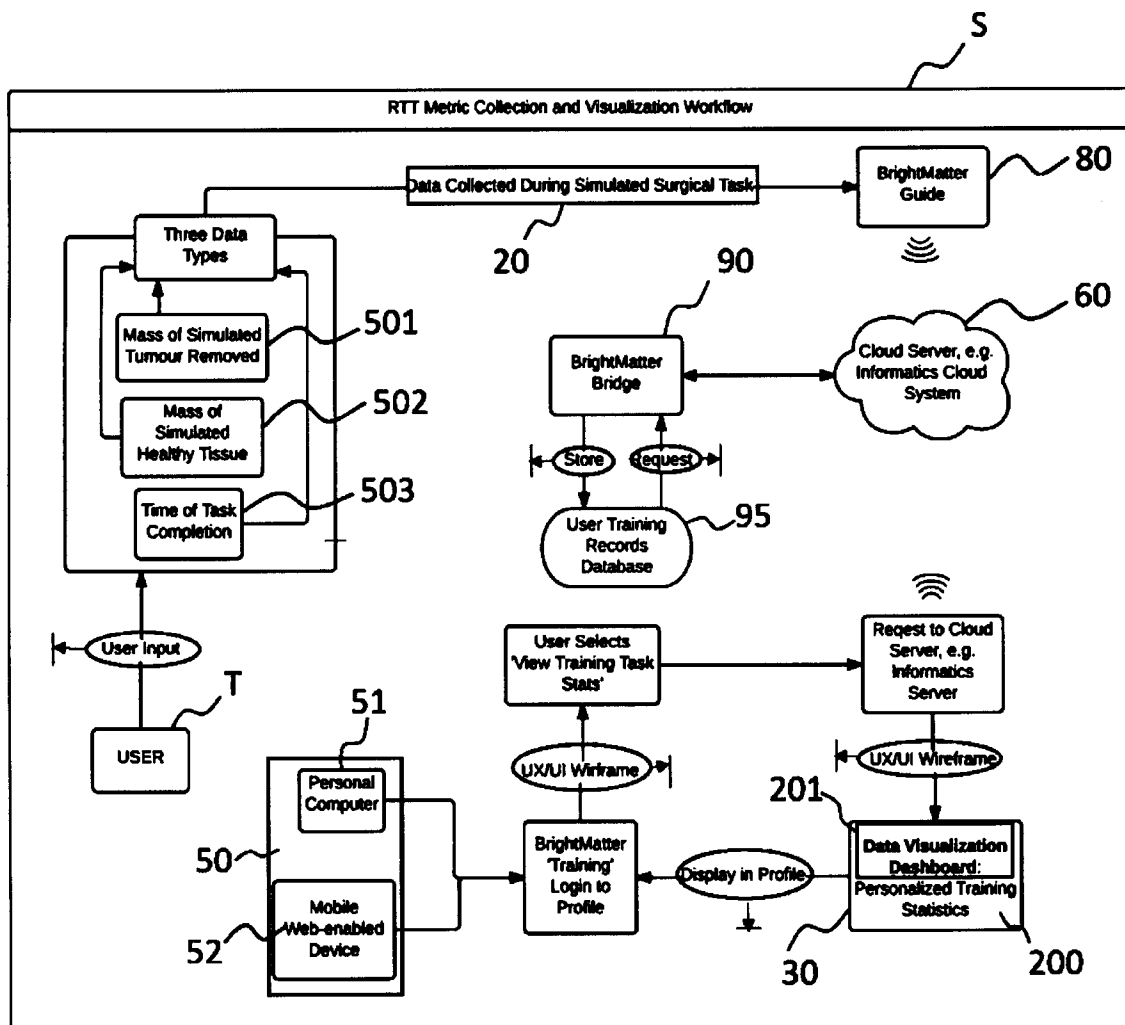


FIG. 5

6/15

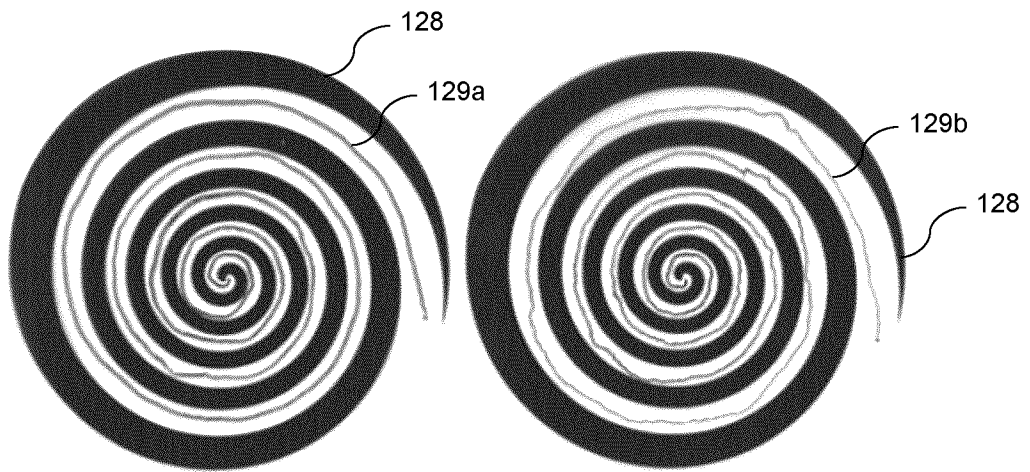


FIG. 6A

FIG. 6B

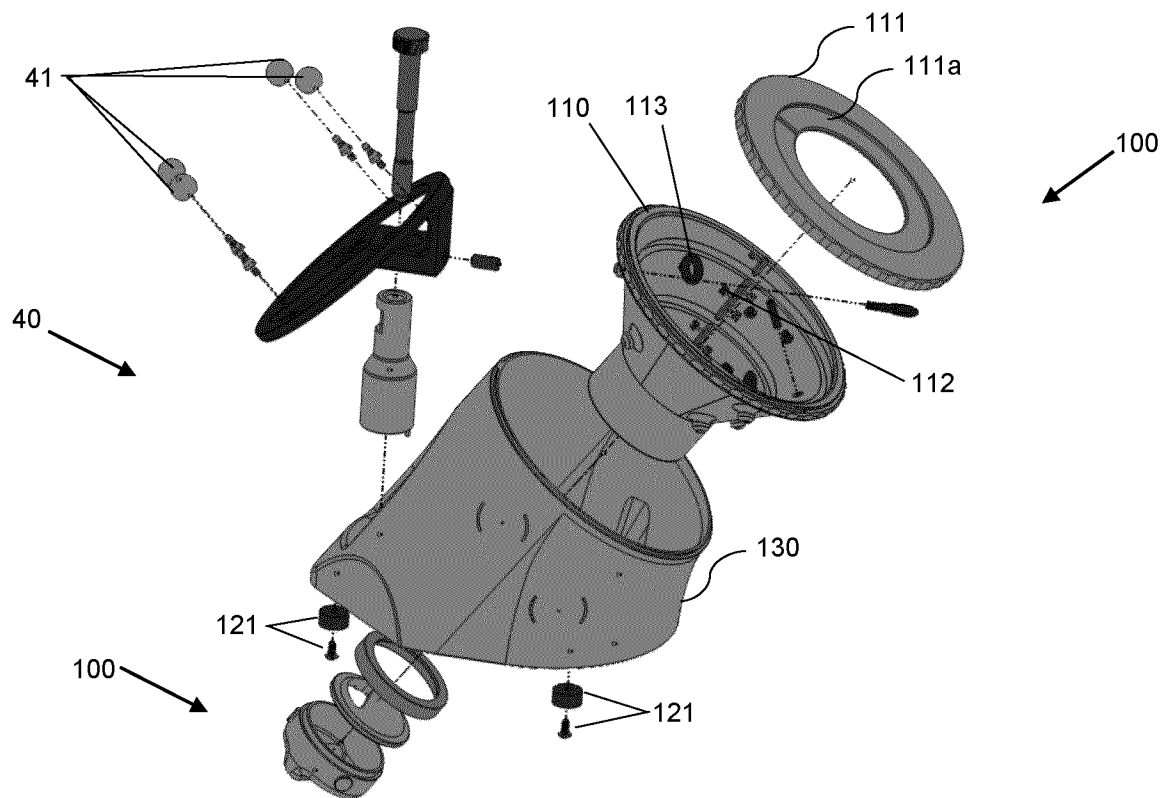


FIG. 7

7/15

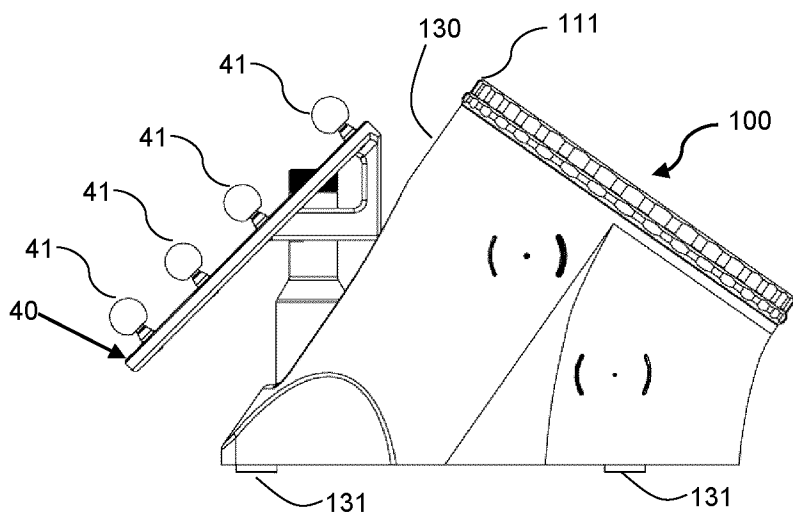


FIG. 8A

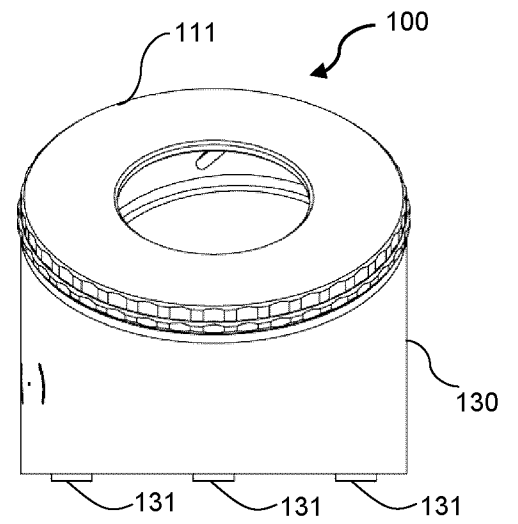


FIG. 8B

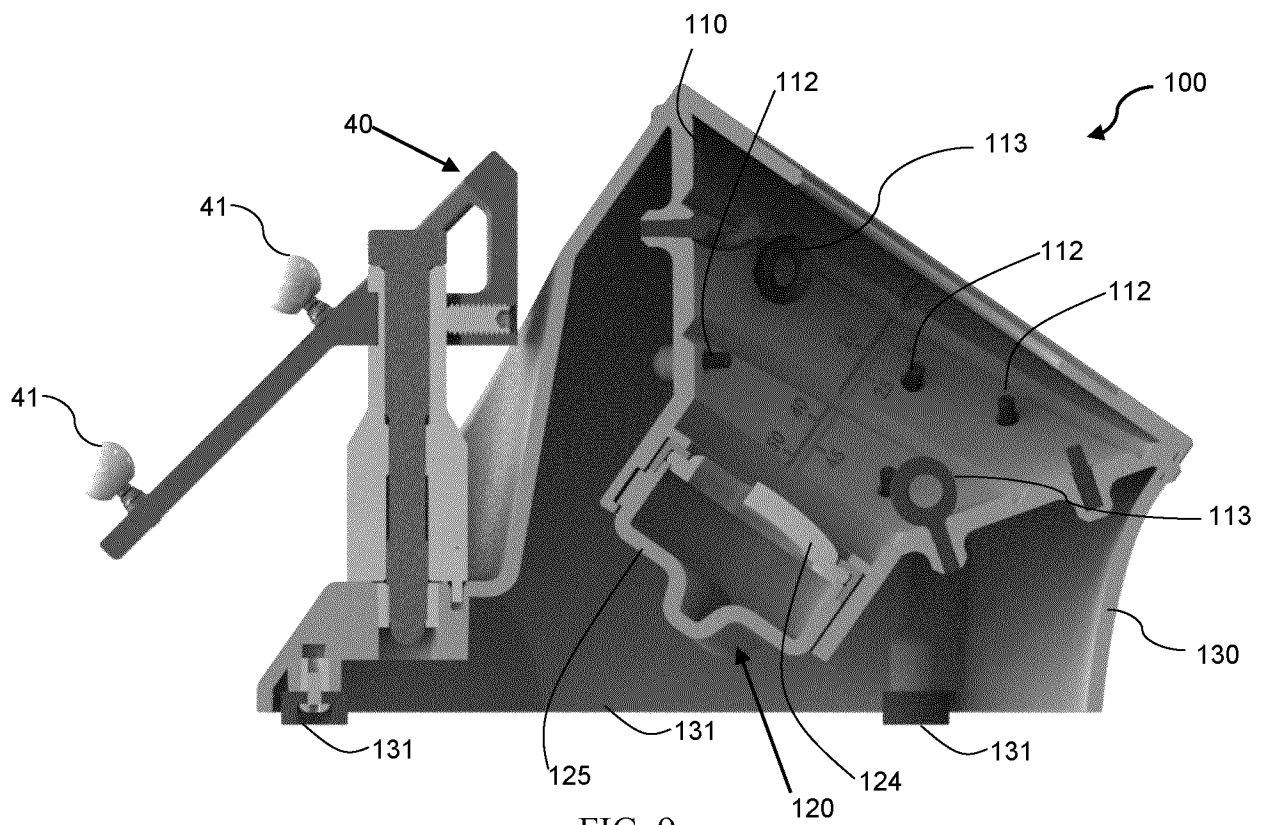


FIG. 9

8/15

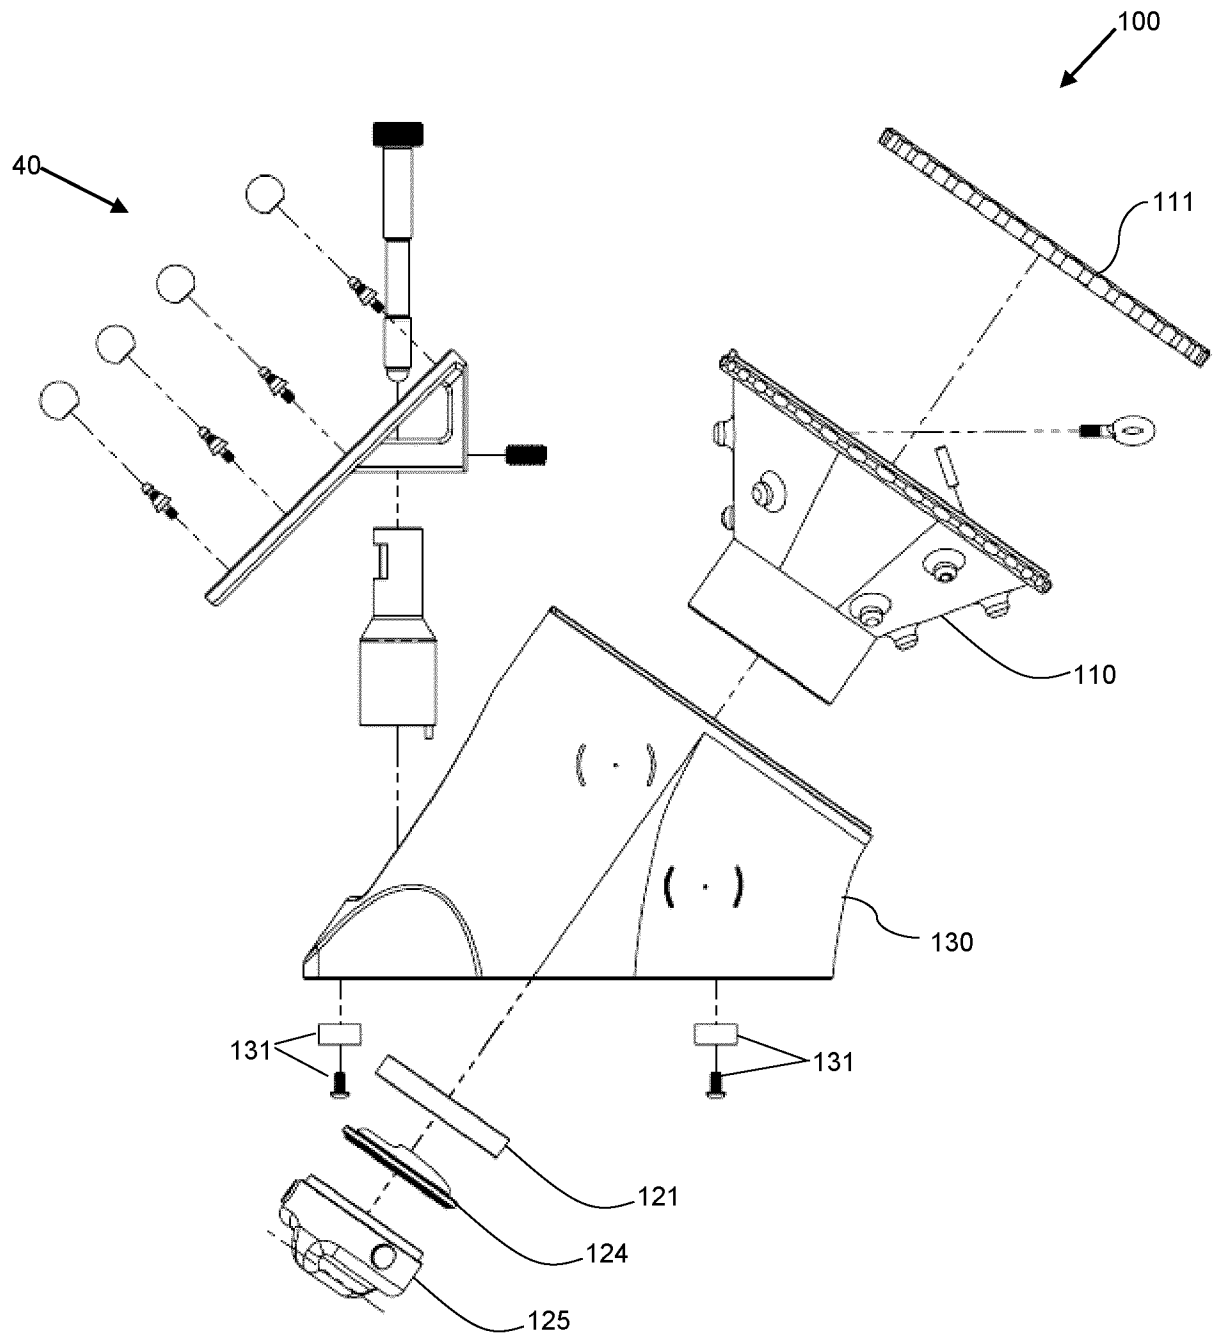


FIG. 10

9/15

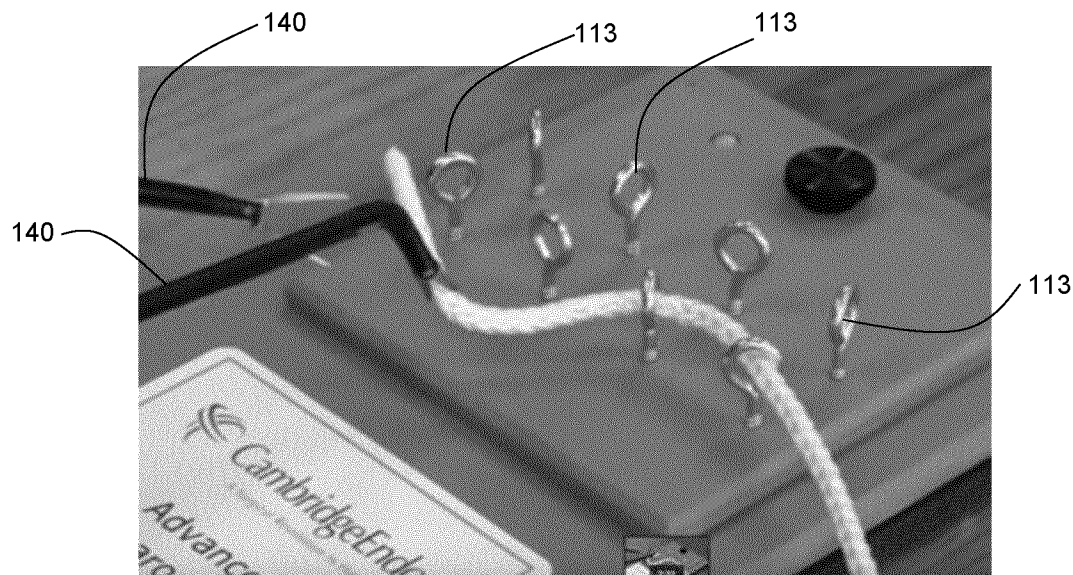


FIG. 11

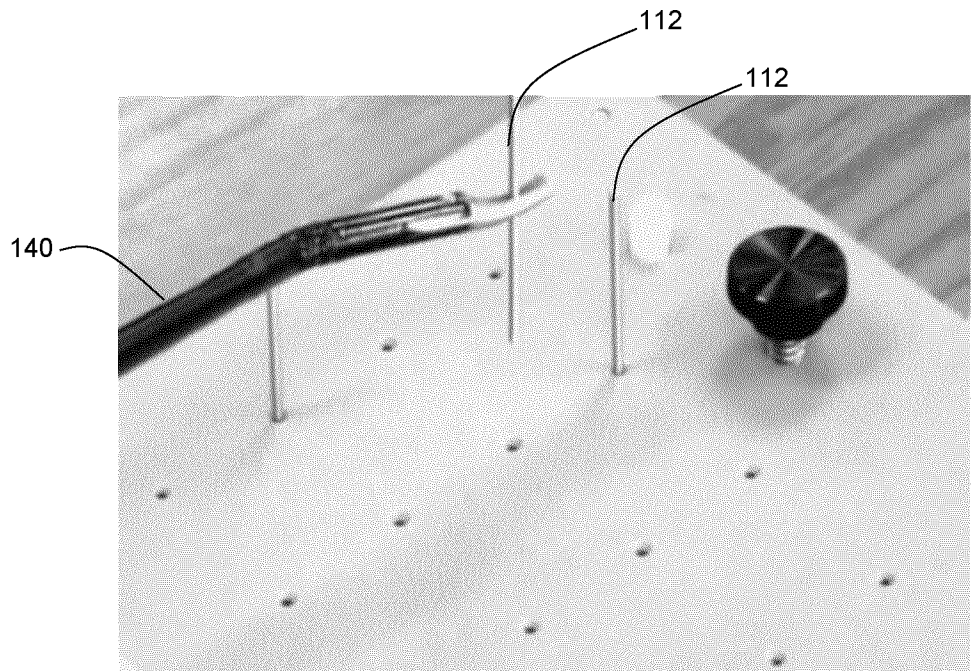


FIG. 12

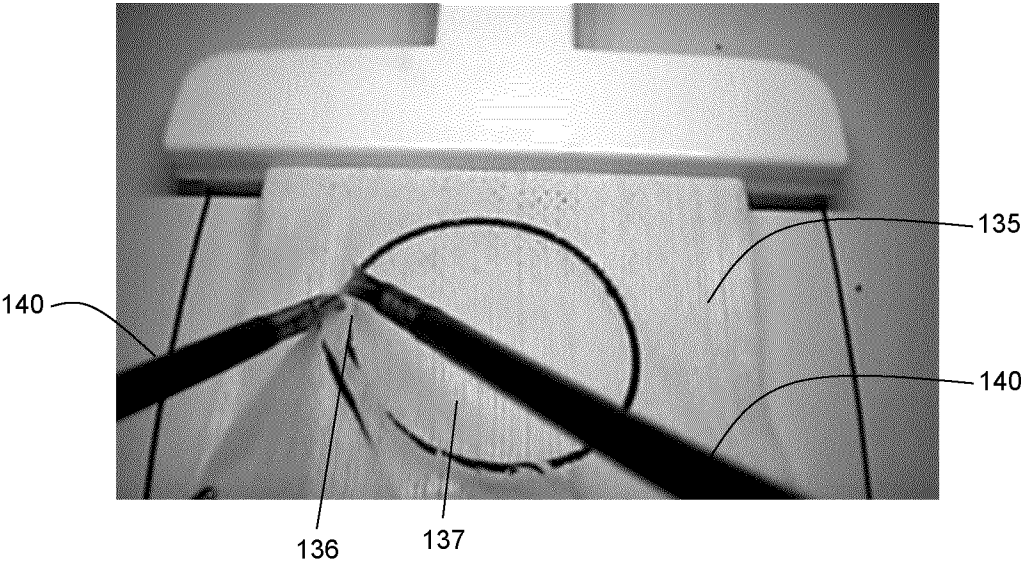


FIG. 13

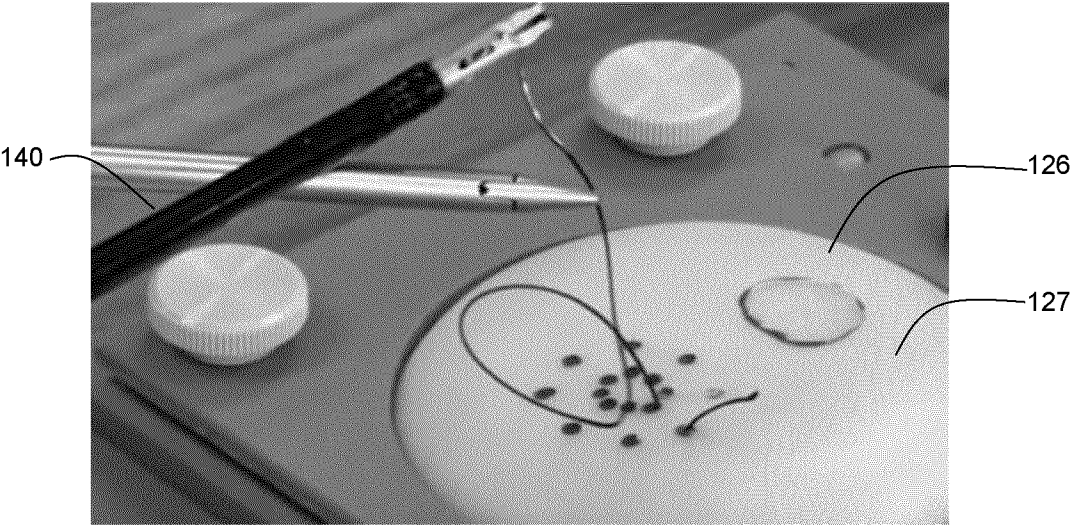


FIG. 14

11/15

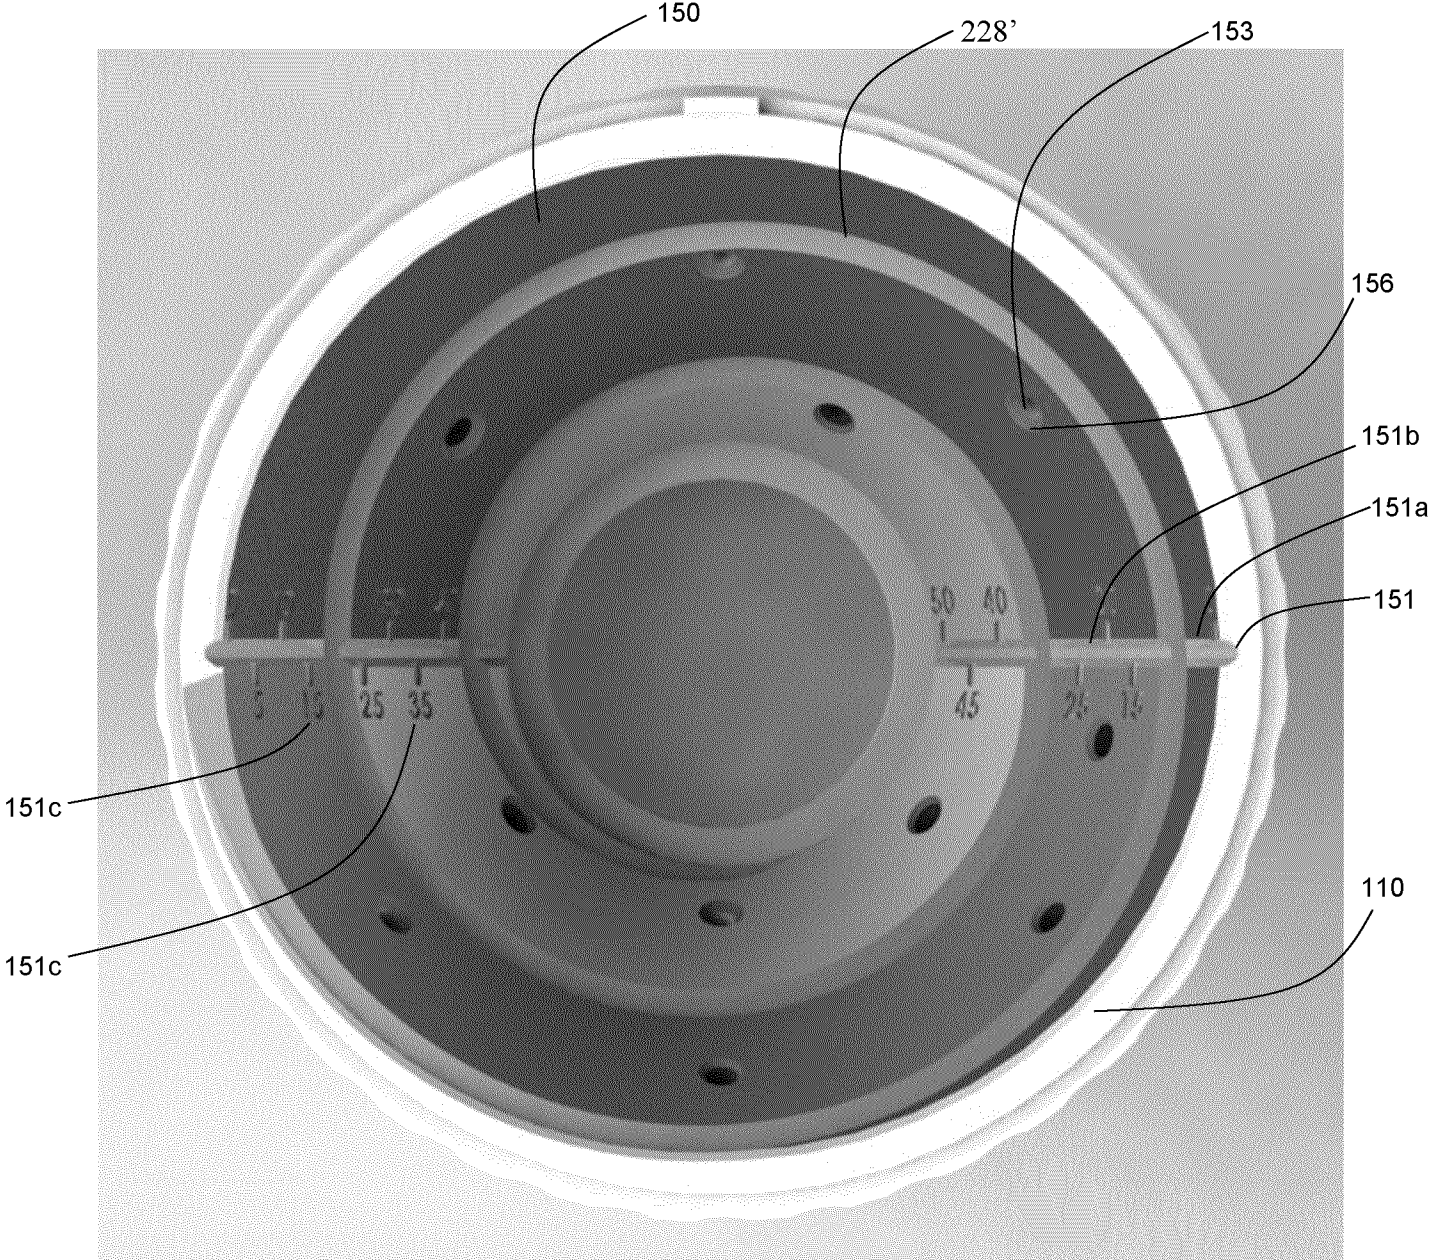


FIG. 15

12/15

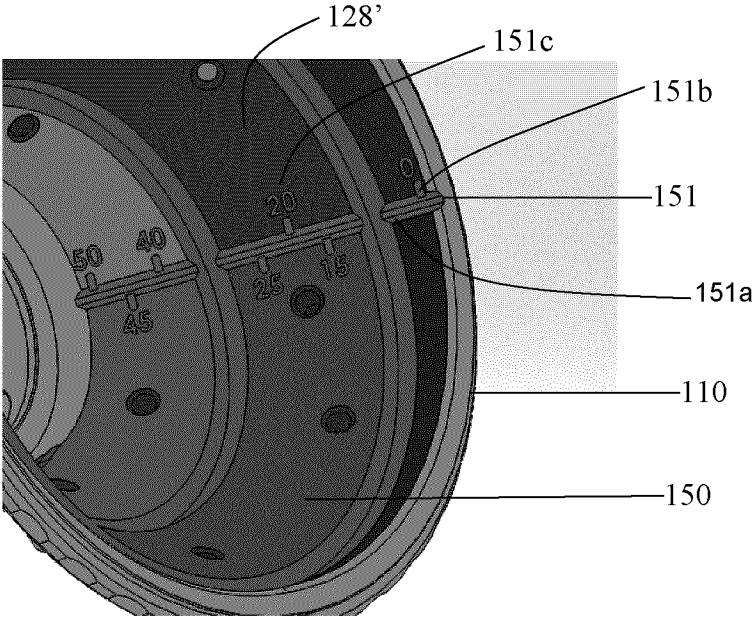


FIG. 16

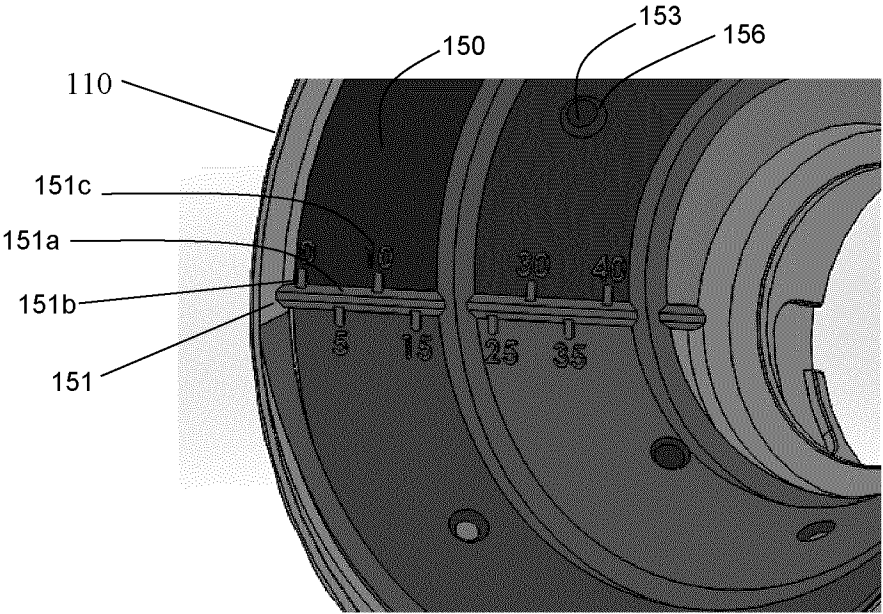


FIG. 17

13/15

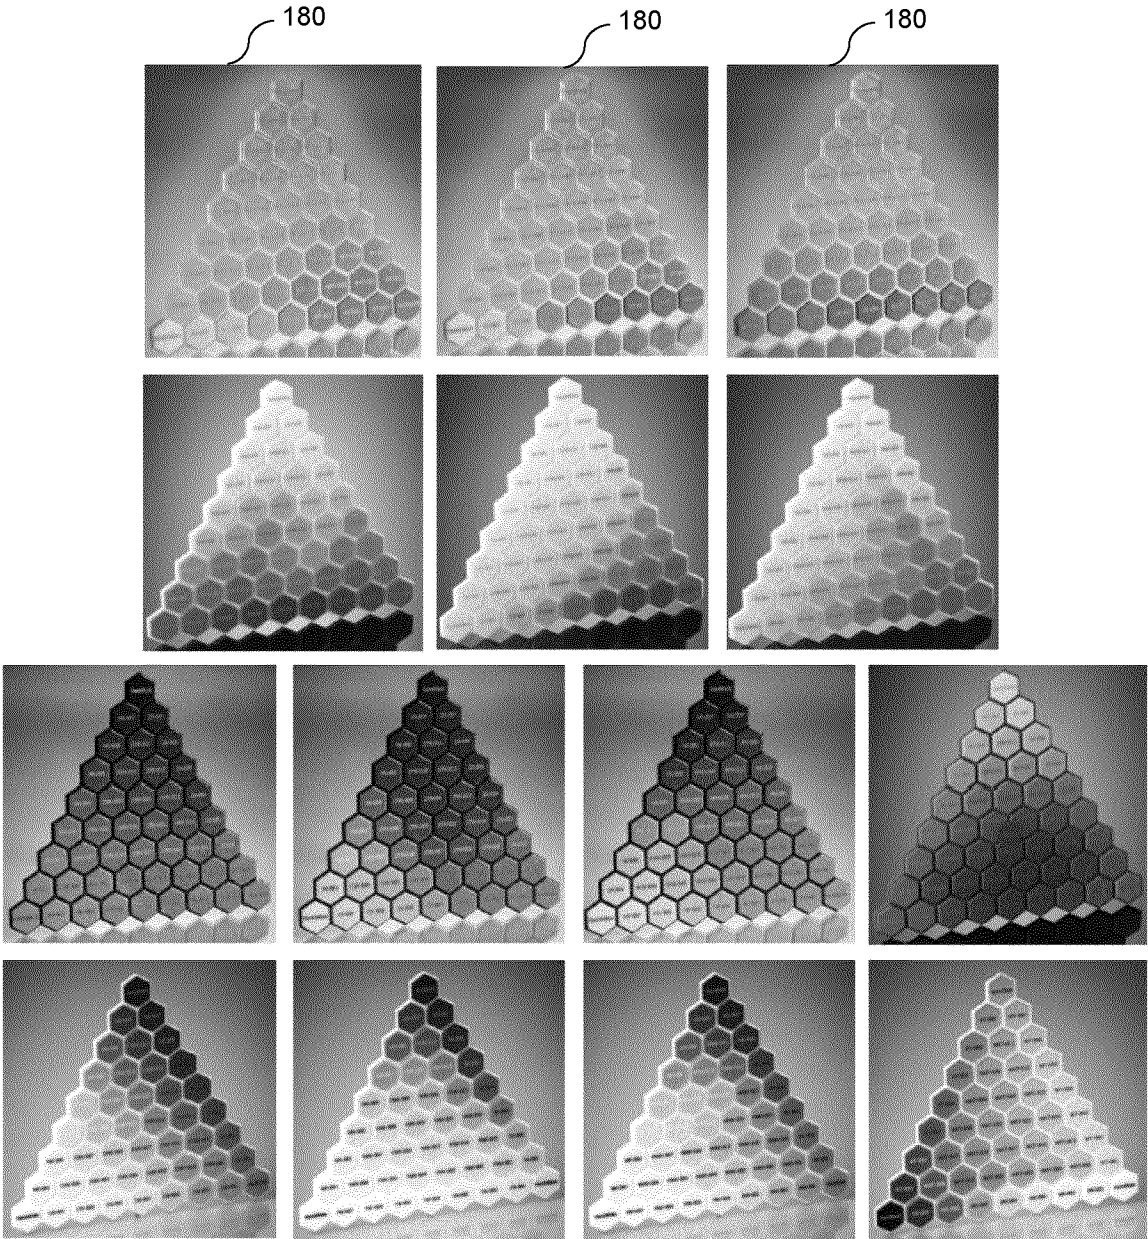


FIG. 18

14/15

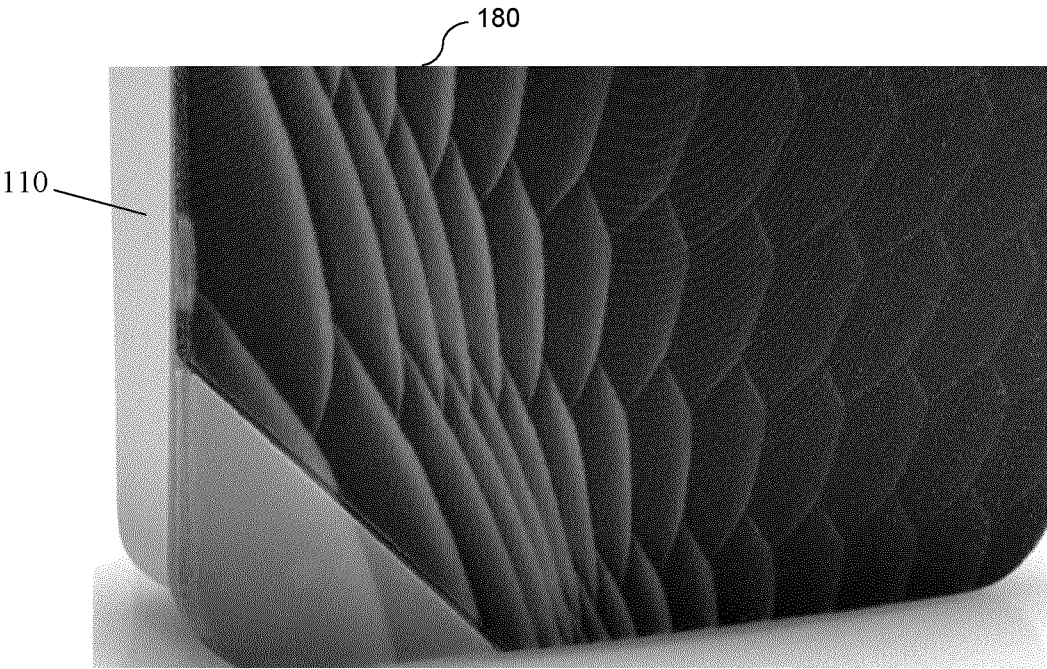


FIG. 19

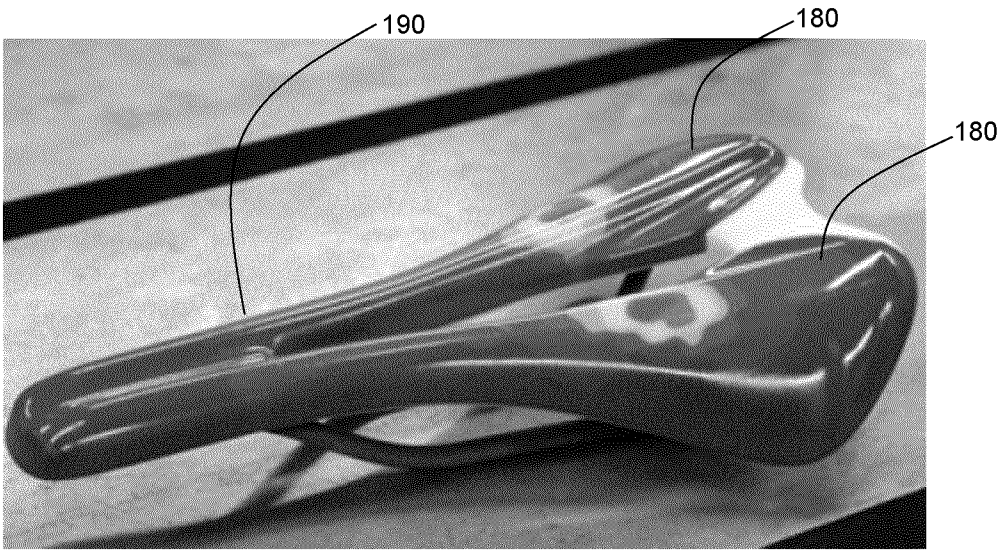


FIG. 20

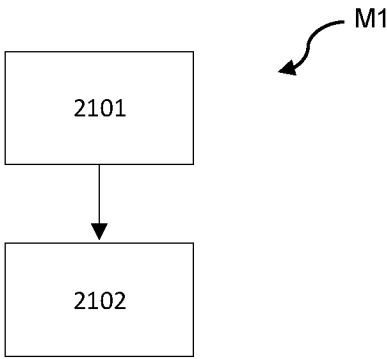


FIG. 21

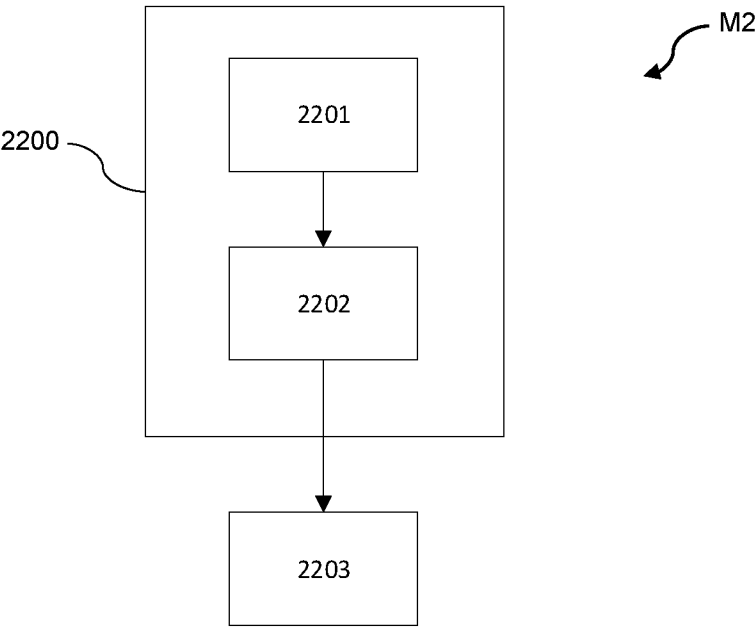


FIG. 22

INTERNATIONAL SEARCH REPORT

International application No.

PCT/CA2016/050389

A. CLASSIFICATION OF SUBJECT MATTER

IPC: **G09B 9/00** (2006.01), **G09B 23/28** (2006.01), **G09B 23/30** (2006.01)

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC: **G09B 9/00** (2006.01), **G09B 23/28** (2006.01), **G09B 23/30** (2006.01)

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic database(s) consulted during the international search (name of database(s) and, where practicable, search terms used)

Canadian Patent database and Orbit Patent database (search terms used: sensor, surgery, simulator, apparatus, system, navigation, screen, monitor, processor, data, feedback, tracking, Raman, optical, probe)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2013/0230837 A1 (DWIGHT A. MEGLAN, et al.) 5 September 2013 (05-09-2013) *whole document*	1 to 8, 23, 24 and 26 to 30
A	WO 02/070980 A1 (JAMES ANDERSON, et al.) 12 September 2002 (12-09-2002) *whole document*	1 to 30
A	US 2014/0220527 A1 (BAOXIN LI, et al.) 7 August 2014 (07-08-2014) *whole document*	1 to 30
A	WO 2007/068050 A1 (GLENN BRIEN, et al.) 21 June 2007 (21-06-2007) *whole document*	1 to 30
A	US 2015/0347682 A1 (YUANMING CHEN, et al.) 3 December 2015 (03-12-2015) *whole document*	1 to 30

Further documents are listed in the continuation of Box C.

See patent family annex.

* "A" "E" "L" "O" "P"	Special categories of cited documents: document defining the general state of the art which is not considered to be of particular relevance earlier application or patent but published on or after the international filing date document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) document referring to an oral disclosure, use, exhibition or other means document published prior to the international filing date but later than the priority date claimed	"T" "X" "Y" "&"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art document member of the same patent family
--------------------------------------	--	--------------------------	--

Date of the actual completion of the international search
05 January 2017 (05-01-2017)Date of mailing of the international search report
05 January 2017 (05-01-2017)Name and mailing address of the ISA/CA
Canadian Intellectual Property Office
Place du Portage I, C114 - 1st Floor, Box PCT
50 Victoria Street
Gatineau, Quebec K1A 0C9
Facsimile No.: 819-953-2476

Authorized officer

Jean-Francois Dufour (819) 639-7847

INTERNATIONAL SEARCH REPORT

International application No.
PCT/CA2016/050389

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2014/0378995 A1 (RAJESH KUMAR, et al.) 25 December 2014 (25-12-2014) *whole document*	1 to 30
A	US 2015/0086955 A1 (LAUREN PONIATOWSKI, et al.) 26 March 2015 (26-03-2015) *whole document*	1 to 30

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/CA2016/050389

Patent Document Cited in Search Report	Publication Date	Patent Family Member(s)	Publication Date
US 2013230837 A1	05 September 2013 (05-09-2013)	US 2013230837 A1 US 9092996 B2	05 September 2013 (05-09-2013) 28 July 2015 (28-07-2015)
WO 02070980 A1	12 September 2002 (12-09-2002)	WO 02070980 A1 AU 777746 B2 AU 4691100 A BR 0010297 A CA 2369830 A1 EP 1173604 A1 JP 2002542836 A MX PA01011182 A SG 142164 A1 US 2003027242 A1 US 6942989 B2 US 2006183183 A1 US 7326562 B2 US 2002137014 A1 US 7371067 B2 US 2002123089 A1 US 2002168618 A1 US 2004106167 A1 WO 0066763 A1 WO 02086797 A1	12 September 2002 (12-09-2002) 28 October 2004 (28-10-2004) 17 November 2000 (17-11-2000) 13 February 2002 (13-02-2002) 09 November 2000 (09-11-2000) 23 January 2002 (23-01-2002) 17 December 2002 (17-12-2002) 21 July 2003 (21-07-2003) 28 May 2008 (28-05-2008) 06 February 2003 (06-02-2003) 13 September 2005 (13-09-2005) 17 August 2006 (17-08-2006) 05 February 2008 (05-02-2008) 26 September 2002 (26-09-2002) 13 May 2008 (13-05-2008) 05 September 2002 (05-09-2002) 14 November 2002 (14-11-2002) 03 June 2004 (03-06-2004) 09 November 2000 (09-11-2000) 31 October 2002 (31-10-2002)
US 2014220527 A1	07 August 2014 (07-08-2014)	None	
WO 2007068050 A1	21 June 2007 (21-06-2007)	None	
US 2015347682 A1	03 December 2015 (03-12-2015)	US 2015347682 A1 US 2013085774 A1 US 9105200 B2	03 December 2015 (03-12-2015) 04 April 2013 (04-04-2013) 11 August 2015 (11-08-2015)
US 2014378995 A1	25 December 2014 (25-12-2014)	US 2014378995 A1 CN 103702631 A EP 2704658 A2 EP 2704658 A4 JP 2014520279 A KR 20140048128 A WO 2012151585 A2 WO 2012151585 A3	25 December 2014 (25-12-2014) 02 April 2014 (02-04-2014) 12 March 2014 (12-03-2014) 03 December 2014 (03-12-2014) 21 August 2014 (21-08-2014) 23 April 2014 (23-04-2014) 08 November 2012 (08-11-2012) 17 January 2013 (17-01-2013)
US 2015086955 A1	26 March 2015 (26-03-2015)	US 2015086955 A1 US 2013085736 A1 WO 2013165529 A2 WO 2013165529 A3	26 March 2015 (26-03-2015) 04 April 2013 (04-04-2013) 07 November 2013 (07-11-2013) 20 February 2014 (20-02-2014)