

(12) STANDARD PATENT
(19) AUSTRALIAN PATENT OFFICE

(11) Application No. **AU 2006270221 B2**

(54) Title
Polymer coatings containing drug powder of controlled morphology

(51) International Patent Classification(s)
B05D 3/00 (2006.01) **A61L 2/00** (2006.01)

(21) Application No: **2006270221** (22) Date of Filing: **2006.07.14**

(87) WIPO No: **WO07/011707**

(30) Priority Data

(31) Number	(32) Date	(33) Country
60/752,338	2005.12.20	US
60/745,733	2006.04.26	US
60/745,731	2006.04.26	US
60/699,650	2005.07.15	US
60/771,725	2006.02.08	US
60/771,066	2006.02.07	US

(43) Publication Date: **2007.01.25**

(44) Accepted Journal Date: **2012.01.19**

(71) Applicant(s)
Micell Technologies, Inc.

(72) Inventor(s)
Taylor, Doug;Cole, Mike;Deyoung, James;McClain, Jim;Smoke, Clint

(74) Agent / Attorney
Davies Collison Cave, 1 Nicholson Street, Melbourne, VIC, 3000

(56) Related Art
US 6669980
US 6368658
US 2003/0185964
US 2003/0222017

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
25 January 2007 (25.01.2007)

PCT

(10) International Publication Number
WO 2007/011707 A3

- (51) International Patent Classification:
B05D 3/00 (2006.01) *A61L 2/00* (2006.01)
- (21) International Application Number:
PCT/US2006/027321
- (22) International Filing Date: 14 July 2006 (14.07.2006)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
- | | | |
|------------|-------------------------------|----|
| 60/699,650 | 15 July 2005 (15.07.2005) | US |
| 60/752,338 | 20 December 2005 (20.12.2005) | US |
| 60/771,066 | 7 February 2006 (07.02.2006) | US |
| 60/771,725 | 8 February 2006 (08.02.2006) | US |
| 60/745,733 | 26 April 2006 (26.04.2006) | US |
| 60/745,731 | 26 April 2006 (26.04.2006) | US |

6231 Big Sandy Drive, Raleigh, NC 27616 (US). **COLE, Mike** [US/US]; 2609 Westmill Court, Raleigh, NC 27613 (US). **DEYOUNG, James** [US/US]; 9211 Garland Road, #6430b, Dallas, TX 75218 (US).

(74) Agents: **ELAMRANI, Samir** et al.; WILSON SONSINI GOODRICH & ROSATI, 650 Page Mill Road, Palo Alto, CA 94304-1050 (US).

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LV, LY, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(71) Applicant (*for all designated States except US*): **MICELL TECHNOLOGIES, INC.** [US/US]; 7516 Precision Drive, Raleigh, NC 27617 (US).

(72) Inventors; and


(75) Inventors/Applicants (*for US only*): **TAYLOR, Doug** [US/US]; 2008 Landmark Drive, Franklinton, NC 27525 (US). **MCCLAIN, Jim** [US/US]; 8008 Chadbourne Ct., Raleigh, NC 27613 (US). **SMOKE, Clint** [US/US];

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: POLYMER COATINGS CONTAINING DRUG POWDER OF CONTROLLED MORPHOLOGY

Rapid Expansion of Supercritical Solutions (RESS) Process Equipment

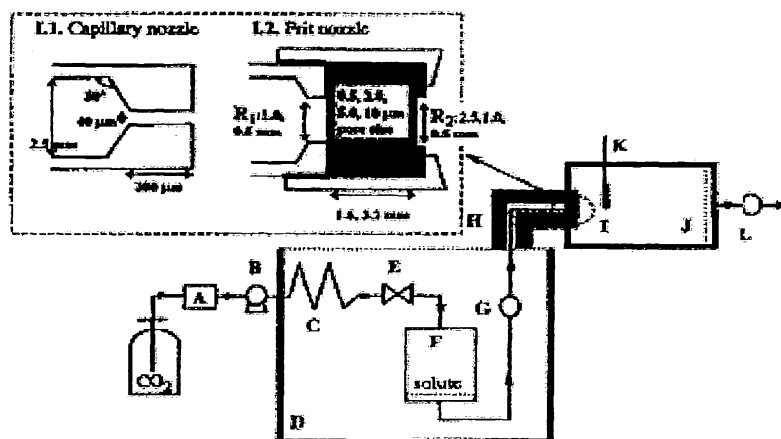

(57) Abstract: A method for depositing a coating comprising a polymer and pharmaceutical agent on a substrate, comprising the following steps: discharging at least one pharmaceutical agent in a therapeutically desirable morphology in dry powder form through a first orifice; discharging at least one polymer in dry powder form through a second orifice; depositing the polymer and/or pharmaceutical particles onto said substrate, wherein an electrical potential is maintained between the substrate and the pharmaceutical and/or polymer particles, thereby forming said coating; and sintering said coating under conditions that do not substantially modify the morphology of said pharmaceutical agent.



Published:

- with international search report
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(88) Date of publication of the international search report:

27 December 2007

**POLYMER COATINGS CONTAINING DRUG POWDER
OF CONTROLLED MORPHOLOGY**

CROSS-REFERENCE

5 [0001] This application claims the benefit of U.S. Provisional Application Nos. 60/699,650 filed July 15, 2005; 60/752,338 filed December 20, 2005; 60/771,066 filed February 7, 2006; 60/771,725 filed February 8, 2006; 60/745,731 filed April 26, 2006; and 60/745,733 filed April 26, 2006 which are incorporated herein by reference in its entirety.

BACKGROUND OF THE INVENTION

[0002] The present invention relates to methods for depositing a coating comprising a polymer and a pharmaceutical or biological agent in powder form onto a substrate.

15 [0003] It is often beneficial to provide coatings onto substrates, such that the surfaces of such substrates have desired properties or effects.

[0004] For example, it is useful to coat biomedical implants to provide for the localized delivery of pharmaceutical or biological agents to target specific locations within the body, for therapeutic or prophylactic benefit. One area of particular interest is drug eluting stents (DES) that has recently been reviewed by Ong and Serruys in Nat. Clin. Pract. Cardiovasc. Med., (Dec 2005), Vol 2, No 12, 647. Typically such pharmaceutical or biological agents are co-deposited with a polymer. Such localized delivery of these agents avoids the problems of systemic administration, which may be accompanied by unwanted effects on other parts of the body, or because administration to the afflicted body part requires a high concentration of pharmaceutical or biological agent that may not be achievable by systemic administration. The coating may provide for controlled release, including long-term or sustained release, of a pharmaceutical or biological agent. Additionally, biomedical implants may be coated with materials to provide beneficial surface properties, such as enhanced biocompatibility or lubriciousness.

25 [0005] Conventionally, coatings have been applied by processes such as dipping, spraying, vapor deposition, plasma polymerization, and electro-deposition. Although these processes have been used to produce satisfactory coatings, there are drawbacks associated therewith. For example it is often difficult to achieve coatings of uniform thicknesses and prevent the occurrence of defects (e.g. bare spots). Also, in many processes, multiple coating steps are frequently necessary, usually requiring drying between or after the coating steps.

35 [0006] Another disadvantage of most conventional methods is that many pharmaceutical or biological agents, once deposited onto a substrate, suffer from poor bioavailability, reduced shelf life, low in vivo stability or uncontrollable elution rates, often attributable to poor control of the

morphology and/or secondary structure of the agent. Pharmaceutical agents present significant morphology control challenges using existing spray coating techniques, which conventionally involve a solution containing the pharmaceutical agents being sprayed onto a substrate. As the solvent evaporates the agents are typically left in an amorphous state. Lack of or low degree of crystallinity of the spray coated agent can lead to decreased shelf life and too rapid drug elution. Biological agents typically rely, at least in part, on their secondary, tertiary and/or quaternary structures for their activity. While the use of conventional solvent-based spray coating techniques may successfully result in the deposition of a biological agent upon a substrate, it will often result in the loss of at least some of the secondary, tertiary and/or quaternary structure of the agent and therefore a corresponding loss in activity. For example, many proteins lose activity when formulated in carrier matrices as a result of the processing methods.

[0007] Conventional solvent-based spray coating processes are also hampered by inefficiencies related to collection of the coating constituents onto the substrate and the consistency of the final coating. As the size of the substrate decreases, and as the mechanical complexity increases, it grows increasingly difficult to uniformly coat all surfaces of a substrate.

[0008] What is needed is a cost-effective method for depositing inert polymers and pharmaceutical or biological agents onto a substrate, where the collection process is efficient, the coating produced is conformal, substantially defect-free and uniform, the composition of the coating can be regulated and the morphology and/or secondary structure of the pharmaceutical or biological agents can be controlled. The method would thus permit structural and morphological preservation of the agents deposited during the coating process.

SUMMARY OF THE INVENTION

[0009] In one aspect, the invention provides a coated coronary stent, comprising: a stent framework; and a rapamycin-polymer coating wherein at least part of rapamycin is in crystalline form.

[0010] In another aspect, the invention provides a coated coronary stent, comprising: a stent framework; and a macrolide immunosuppressive (limus) drug-polymer coating wherein at least part of the drug is in crystalline form. In one embodiment, the macrolide immunosuppressive drug comprises one or more of rapamycin, 40-O-(2-Hydroxyethyl)rapamycin (everolimus), 40-O-Benzyl-rapamycin, 40-O-(4'-Hydroxymethyl)benzyl-rapamycin, 40-O-[4'-(1,2-Dihydroxyethyl)]benzyl-rapamycin, 40-O-Allyl-rapamycin, 40-O-[3'-(2,2-Dimethyl-1,3-dioxolan-4(S)-yl)-prop-2'-en-1'-yl]-rapamycin, (2'E,4'S)-40-O-(4',5'-Dihydroxypent-2'-en-1'-yl)-rapamycin 40-O-(2-Hydroxy)ethoxycarbonylmethyl-rapamycin, 40-O-(3-Hydroxy)propyl-rapamycin 40-O-(6-Hydroxy)hexyl-rapamycin 40-O-[2-(2-Hydroxy)ethoxy]ethyl-rapamycin

2006270221 15 Dec 2011

4O-O-[(3S)-2,2-Dimethyldioxolan-3-yl]methyl-rapamycin, 4O-O-[(2S)-2,3-Dihydroxyprop-1-yl]-rapamycin, 4O-O-(2-Acetoxy)ethyl-rapamycin 4O-O-(2-Nicotinoyloxy)ethyl-rapamycin, 4O-O-[2-(N-Morpholino)acetoxy]ethyl-rapamycin 4O-O-(2-N-Imidazolylacetoxy)ethyl-rapamycin, 4O-O-[2-(N-Methyl-N'-piperazinyl)acetoxy]ethyl-rapamycin, 39-O-Desmethyl-39,40-O,O-ethylene-rapamycin, (26R)-26-Dihydro-40-O-(2-hydroxy)ethyl-rapamycin, 28-O-Methyl-rapamycin, 4O-O-(2-Aminoethyl)-rapamycin, 4O-O-(2-Acetaminoethyl)-rapamycin 4O-O-(2-Nicotinamidoethyl)-rapamycin, 4O-O-(2-(N-Methyl-imidazo-2'-ylcarbethoxamido)ethyl)-rapamycin, 4O-O-(2-Ethoxycarbonylaminoethyl)-rapamycin, 40-O-(2-Tolylsulfonamidoethyl)-rapamycin, 40-O-[2-(4',5'-Dicarboethoxy-1',2',3'-triazol-1'-yl)-ethyl]-rapamycin, 42-Epi-(tetrazolyl)rapamycin (tacrolimus), and 42-[3-hydroxy-2-(hydroxymethyl)-2-methylpropanoate]rapamycin (temsirolimus).

[0011] In yet another aspect, the invention provides a method for coating a substrate, said coating comprising

- at least one polymer; and
- at least one pharmaceutical agent in a therapeutically desirable morphology and/or at least one active biological agent;
- said method comprising the following steps:
 - discharging the at least one pharmaceutical agent and/or at least one active biological agent in dry powder form through a first orifice;
 - discharging the at least one polymer in dry powder form through a second orifice;
 - depositing the polymer and pharmaceutical agent and/or active biological agent particles onto said substrate, wherein an electrical potential is maintained between the substrate and the polymer and pharmaceutical agent and/or active biological agent particles, thereby forming said coating; and
 - sintering said coating under conditions that do not substantially modify the morphology of said pharmaceutical agent and/or the activity of said biological agent, wherein said sintering comprises treating said coated substrate with a compressed gas, compressed liquid or supercritical fluid that is a non-solvent for both the polymer and the pharmaceutical and/or biological agents.

2006270221 15 Dec 2011

[0012] In a further aspect, the invention provides a method for coating a substrate, said coating comprising

at least one polymer; and

at least one pharmaceutical agent in a therapeutically desirable morphology and/or

5 at least one active biological agent;

said method comprising the following steps:

discharging the at least one pharmaceutical agent and/or at least one active biological agent in dry powder form through a first orifice;

10 forming a supercritical or near supercritical fluid solution comprising at least one supercritical fluid solvent and at least one polymer and discharging said supercritical or near supercritical fluid solution through a second orifice under conditions sufficient to form solid particles of the polymer;

15 depositing the polymer and pharmaceutical agent and/or active biological agent particles onto said substrate, wherein an electrical potential is maintained between the substrate and the polymer and pharmaceutical agent and/or active biological agent particles, thereby forming said coating; and

20 sintering said coating under conditions that do not substantially modify the morphology of said pharmaceutical agent and/or the activity of said biological agent, wherein said sintering comprises treating said coated substrate with a compressed gas, compressed liquid or supercritical fluid that is a non-solvent for both the polymer and the pharmaceutical and/or biological agents.

[0013] A further aspect of the invention provides a method for depositing a coating onto a substrate, said coating comprising

25 at least one polymer; and at least one pharmaceutical agent in a therapeutically desirable morphology in dry powder form and/or at least one active biological agent;

said method comprising the following steps:

discharging the at least one pharmaceutical agent and/or at least one active biological agent through a first orifice;

30 forming a first stream of a polymer solution comprising at least one solvent and at least one polymer;

forming a second stream of a supercritical or near supercritical fluid comprising at least one supercritical fluid;

2006270221 15 Dec 2011

contacting said first and second streams, whereby said supercritical or near supercritical fluid acts as a diluent of said solution under conditions sufficient to form particles of said polymer;

5 depositing the polymer and pharmaceutical agent and/or active biological agent particles onto said substrate, wherein an electrical potential is maintained between the substrate and the polymer and pharmaceutical agent and/or active biological agent particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said pharmaceutical agent and/or the activity of said biological agent.

10 [0014] Yet another aspect of the invention provides a coated implantable medical device, comprising: a substrate; and

a coating having substantially uniform thickness disposed on said substrate, wherein said coating comprises at least one polymer and at least one pharmaceutical agent in a therapeutically desirable morphology and/or at least one active biological agent comprising an active secondary, tertiary or quaternary structure.

[0015] In one embodiment, the device is selected from the group consisting of stents, joints, screws, rods, pins, plates, staples, shunts, clamps, clips, sutures, suture anchors, electrodes, catheters, leads, grafts, dressings, pacemakers, pacemaker housings, cardioverters, cardioverter housings, defibrillators, defibrillator housings, prostheses, ear drainage tubes, ophthalmic implants, orthopedic devices, vertebral disks, bone substitutes, anastomotic devices, perivascular wraps, colostomy bag attachment devices, hemostatic barriers, vascular implants, vascular supports, tissue adhesives, tissue sealants, tissue scaffolds and intraluminal devices.

[0016] A further aspect of the invention provides a method for depositing a coating comprising a polymer and pharmaceutical agent on a substrate, wherein the method comprises the following steps:

forming a first supercritical or near critical fluid mixture that includes said at least one pharmaceutical agent;

forming a second supercritical or near critical fluid mixture that includes at least one polymer;

discharging the first supercritical or near critical fluid mixture through a first orifice under conditions sufficient to form solid particles of the pharmaceutical agent;

discharging the second supercritical or near critical fluid mixture through said first orifice or through a second orifice under conditions sufficient to form solid particles of the polymer;

depositing the solid pharmaceutical particles and/or polymer particles onto said substrate, wherein an electrical potential is maintained between the substrate and the pharmaceutical and/or polymer particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles.

[0017] Another aspect provides a method for depositing a coating comprising a polymer and a pharmaceutical agent on a substrate, comprising the following steps;

forming a first stream of a polymer solution comprising a first solvent and at least one polymer;

forming a second stream of a supercritical or near critical fluid mixture,

contacting said first and second streams, whereby said supercritical or near critical fluid acts as a diluent of said first solvent under conditions sufficient to form particles of the polymer;

forming a third stream of a solution comprising a second solvent and at least one pharmaceutical agent;

forming a fourth stream of a supercritical or near critical fluid mixture,

contacting said third and fourth streams, whereby said supercritical or near critical fluid

acts as a diluent of said second solvent under conditions sufficient to form particles of the pharmaceutical agent;

depositing the polymer and/or pharmaceutical particles onto said substrate, wherein an electrical potential is maintained between the substrate and the pharmaceutical and/or polymer particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles.

[0018] Yet another aspect of the invention provides a method for depositing a coating comprising a polymer and a pharmaceutical agent on a substrate, wherein the substrate is pre-coated with one or more polymers, the method comprising the following steps;

forming a first stream of a solution comprising a solvent and at least one pharmaceutical agent;

forming a second stream of a supercritical or near critical fluid mixture,

contacting said first and second streams, whereby said supercritical or near critical fluid acts as a diluent of said solvent under conditions sufficient to form particles of the pharmaceutical agent;

depositing the pharmaceutical particles onto said substrate, wherein an electrical potential is maintained between the substrate and the pharmaceutical particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles.

[0019] A further aspect provides a method for depositing a coating comprising a polymer and a pharmaceutical agent on a substrate, wherein the substrate is pre-coated with one or more pharmaceutical agents, the method comprising the following steps;

forming a first stream of a solution comprising a solvent and at least one polymer;

forming a second stream of a supercritical or near critical fluid mixture,

contacting said first and second streams, whereby said supercritical or near critical fluid acts as a diluent of said solvent under conditions sufficient to form particles of the polymer;

depositing the polymer particles onto said substrate, wherein an electrical potential is maintained between the substrate and the pharmaceutical particles, thereby forming said coating;

and

~~sintering said coating under conditions that do not substantially modify the morphology~~
of said solid pharmaceutical particles.

Yet another aspect of the invention provides a method for depositing a coating comprising a polymer and pharmaceutical agent on a substrate, wherein the method comprises the following steps:

co-introducing into a coaxial cylindrical spray tube an anti-solvent fluid mixture which is a supercritical or a near-critical fluid mixture and a solution or suspension of at least one pharmaceutical agent in a vehicle which is soluble or substantially soluble in the anti-solvent fluid mixture; contacting the anti-solvent fluid with said solution or suspension of at least one pharmaceutical agent to form a combined stream containing the supercritical or a near-critical fluid mixture, the vehicle and the pharmaceutical agent;

spraying the combined stream through an orifice of said tube into a vessel, wherein said vehicle is extracted from the solution or suspension and particles of the pharmaceutical agent substantially free of the vehicle are formed prior to deposition of said pharmaceutical particles on said substrate;

depositing the pharmaceutical particles onto a substrate pre-coated with particles of at least one polymer disposed into said vessel wherein an electrical potential is maintained between the substrate and the polymer particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles.

[0020] Still further aspect of the invention provides a method for depositing a coating comprising a polymer and pharmaceutical agent on a substrate, wherein the method comprises the following steps:

co-introducing into a coaxial cylindrical spray tube an anti-solvent fluid mixture which is a supercritical or a near-critical fluid mixture and a solution or suspension of at least one polymer in a vehicle which is soluble or substantially soluble in the anti-solvent fluid mixture; contacting the anti-solvent fluid with said solution or suspension of at least one polymer to form a combined stream containing the supercritical or a near-critical fluid mixture, the vehicle and the polymer;

spraying the combined stream through an orifice of said tube into a vessel, wherein said vehicle is extracted from the solution or suspension and particles of the polymer substantially free of the vehicle are formed prior to deposition of said polymer particles on said substrate;;

depositing the polymer particles onto a substrate pre-coated with particles of at least one pharmaceutical agent disposed into said vessel wherein an electrical potential is maintained between the substrate and the polymer particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles.

[0021] A further aspect provides a method for depositing a coating comprising a polymer and a biological agent on a substrate, comprising the following steps;

5 forming a first stream of a polymer solution comprising a first solvent and at least one polymer;

forming a second stream of a supercritical or near critical fluid mixture,

contacting said first and second streams, whereby said supercritical or near critical fluid acts as a diluent of said first solvent under conditions sufficient to form particles of the polymer;

10 forming a third stream of a solution comprising a second solvent and at least one biological agent;

forming a fourth stream of a supercritical or near critical fluid mixture,

contacting said third and fourth streams, whereby said supercritical or near critical fluid acts as a diluent of said second solvent under conditions sufficient to form particles of the

15 pharmaceutical agent;

depositing the polymer and/or biological agent particles onto said substrate, wherein an electrical potential is maintained between the substrate and the biological agent and/or polymer particles, thereby forming said coating; and

20 sintering said coating under conditions that do not substantially modify the structure of said biological agent particles.

[0022] Yet another aspect provides a method for depositing a coating comprising a polymer and a pharmaceutical agent on a substrate, comprising the following steps;

forming a first stream of a solution comprising a solvent and at least one pharmaceutical agent;

25 [0023] discharging said stream in a vessel containing said substrate and a supercritical or near critical fluid mixture, whereby said supercritical or near critical fluid acts as a diluent of said solvent under conditions sufficient to form particles of the pharmaceutical agent;

forming a second stream of a solution comprising a solvent and at least one polymer;

30 discharging said second stream in said vessel, whereby said supercritical or near critical fluid acts as a diluent of said solvent under conditions sufficient to form particles of the polymer

depositing the pharmaceutical and/or polymer particles onto said substrate, wherein an electrical potential is maintained between the substrate and the pharmaceutical and/or polymer particles, thereby forming said coating; and

35 sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles.

[0024] A further aspect provides a method for depositing a coating comprising a polymer and a pharmaceutical agent on a substrate, comprising the following steps;

providing a substrate pre-coated with at least one polymer;

forming a stream of a solution comprising a solvent and at least one pharmaceutical

agent;

discharging said stream in a vessel containing said substrate and a supercritical or near critical fluid mixture, whereby said supercritical or near critical fluid acts as a diluent of said solvent under conditions sufficient to form particles of the pharmaceutical agent;

depositing the pharmaceutical particles onto said substrate, wherein an electrical potential is maintained between the substrate and the pharmaceutical particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles.

[0025] Another aspect provides a method for depositing a coating comprising a polymer and a pharmaceutical agent on a substrate, comprising the following steps;

providing a substrate pre-coated with solid particles of at least one pharmaceutical agent;

forming a stream of a solution comprising a solvent and at least one polymer;

discharging said stream in a vessel containing said substrate and a supercritical or near critical fluid mixture, whereby said supercritical or near critical fluid acts as a diluent of said solvent under conditions sufficient to form particles of the polymer;

depositing the polymer particles onto said substrate, wherein an electrical potential is maintained between the substrate and the polymer particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles.

Yet another aspect provides a method for depositing a coating comprising a polymer and pharmaceutical agent on a substrate, wherein the method comprises the following steps:

contacting an anti-solvent fluid mixture which is a supercritical or a near-critical fluid mixture and a solution or suspension of at least one pharmaceutical agent in a vehicle which is soluble or substantially soluble in the anti-solvent fluid mixture to form a combined stream containing the supercritical or a near-critical fluid mixture, the vehicle and the pharmaceutical agent;

spraying the combined stream into a vessel, wherein said vehicle is extracted from the solution or suspension and particles of the pharmaceutical agent substantially free of the vehicle are formed prior to deposition of said pharmaceutical particles on a substrate pre-coated with particles of at least one polymer;

deposited the pharmaceutical particles onto said substrate disposed into said vessel wherein an electrical potential is maintained between the substrate and the pharmaceutical particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles.

[0026] A further aspect of the invention provides a method for depositing a coating comprising a polymer and pharmaceutical agent on a substrate, wherein the method comprises the following steps:

contacting an anti-solvent fluid mixture which is a supercritical or a near-critical fluid mixture and a solution or suspension of at least one pharmaceutical agent in a vehicle which is soluble or substantially soluble in the anti-solvent fluid mixture to form a combined stream containing the supercritical or a near-critical fluid mixture, the vehicle and the pharmaceutical agent;

spraying the combined stream into a vessel, wherein said vehicle is extracted from the solution or suspension and particles of the pharmaceutical agent substantially free of the vehicle are formed prior to deposition of said pharmaceutical particles on a substrate pre-coated with particles of at least one polymer; wherein said anti-solvent mixture and said solution or suspension of at least one pharmaceutical agent are supplied by first and second tubes, respectively, wherein said first and second tubes are disposed at an angle;

depositing the pharmaceutical particles onto said substrate disposed into said vessel wherein an electrical potential is maintained between the substrate and the polymer particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles

[0027] A further aspect of the invention provides a method for depositing a coating comprising a polymer and at least two pharmaceutical agents on a substrate, wherein the method comprises the following steps:

contacting an anti-solvent fluid mixture which is a supercritical or a near-critical fluid mixture, a solution or suspension of a first pharmaceutical agent in a first vehicle which is soluble or substantially soluble in the anti-solvent fluid mixture, and a solution or suspension of a second pharmaceutical agent in a second vehicle which is the same as the first vehicle or another vehicle soluble or substantially soluble in the anti-solvent fluid mixture to form a combined stream containing the supercritical or a near-critical fluid mixture, the vehicle or vehicles and the first and second pharmaceutical agents;

2006270221 15 Dec 2011

spraying the combined stream into a vessel, wherein said vehicle is extracted from the solution or suspension and particles of the first and second pharmaceutical agents substantially free of the vehicle or vehicles are formed prior to deposition of said pharmaceutical particles on a substrate pre-coated with particles of at least one polymer;

5 wherein said anti-solvent mixture, said solution or suspension of said first pharmaceutical agent, and said solution or suspension of said second pharmaceutical agent are supplied by first, second and third tubes, respectively, wherein said second and third tubes are each disposed at an angle from said first tube;

10 depositing the pharmaceutical particles onto said substrate disposed into said vessel wherein an electrical potential is maintained between the substrate and the polymer particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said solid pharmaceutical particles

15 **[0028]** Yet another aspect provides a coated implantable medical device, comprising: a substrate; and

a pharmaceutical agent-polymer coating having substantially uniform thickness disposed on the substrate, wherein the coating comprises at least one pharmaceutical agent all of the pharmaceutical agent or agents in the coating are substantially uniformly dispersed within the polymer coating.

20 **[0028A]** In another aspect of the invention there is provided a coated vascular stent, comprising:

a stent framework; and

a rapamycin-polymer coating wherein at least part of rapamycin is in crystalline form, wherein the coated coronary stent is formed by the following method:

25 discharging the rapamycin in dry powder form through a first orifice; discharging the polymer in dry powder form through a second orifice; depositing the polymer and rapamycin particles onto said stent framework, wherein an electrical potential is maintained between the stent framework and the polymer and rapamycin particles, thereby forming said coating; and sintering said coating under conditions that do not substantially
30 modify the morphology of said rapamycin, wherein said sintering comprises treating said coating with a compressed gas, compressed liquid or supercritical fluid that is a non-solvent for both the polymer and the rapamycin.

2006270221 15 Dec 2011

[0028B] In another aspect of the invention there is provided a coated vascular stent, comprising:

a stent framework; and

a rapamycin-polymer coating wherein at least part of rapamycin is in crystalline form, wherein the coated coronary stent is formed by the following method: discharging the rapamycin in dry powder form through a first orifice; forming a supercritical or near supercritical fluid solution comprising at least one supercritical fluid solvent and the polymer and discharging said supercritical or near supercritical fluid solution through a second orifice under conditions sufficient to form solid particles of the polymer; depositing the polymer and rapamycin particles onto said stent framework, wherein an electrical potential is maintained between the stent framework and the polymer and rapamycin particles, thereby forming said coating; and sintering said coating under conditions that do not substantially modify the morphology of said rapamycin, wherein said sintering comprises treating said coating with a compressed gas, compressed liquid or supercritical fluid that is a non-solvent for both the polymer and the rapamycin.

[0028C] In another aspect of the invention there is provided a coated vascular stent, comprising:

a stent framework; and

a rapamycin-polymer coating wherein at least part of rapamycin is in crystalline form, wherein the coated coronary stent is formed by the following method: discharging the rapamycin through a first orifice; forming a first stream of a polymer solution comprising at least one solvent and the polymer; forming a second stream of a supercritical or near supercritical fluid comprising at least one supercritical fluid; contacting said first and second streams, whereby said supercritical or near supercritical fluid acts as a diluent of said solution under conditions sufficient to form particles of said polymer; depositing the polymer and rapamycin particles onto said stent framework, wherein an electrical potential is maintained between the stent framework and the polymer and rapamycin particles, thereby forming said coating; and sintering said coating under conditions that do not substantially modify the morphology of said rapamycin, wherein said sintering comprises treating said coating with a compressed gas, compressed liquid or supercritical fluid that is a non-solvent for both the polymer and the rapamycin.

2006270221 04 Oct 2011

[0028D] In another aspect of the invention there is provided a coated coronary stent, comprising: a stent framework; and a macrolide immunosuppressive (limus) drug-polymer coating wherein at least part of the drug is in crystalline form, and wherein the coated
5 coronary stent is formed by one of the following methods:

discharging the drug in dry powder form through a first orifice; discharging the polymer in dry powder form through a second orifice; depositing the polymer and drug particles onto said stent framework, wherein an electrical potential is maintained between the stent framework and the polymer and drug particles, thereby forming said coating; and
10 sintering said coating under conditions that do not substantially modify the morphology of said drug;

discharging the drug in dry powder form through a first orifice; forming a supercritical or near supercritical fluid solution comprising at least one supercritical fluid solvent and the polymer and discharging said supercritical or near supercritical fluid
15 solution through a second orifice under conditions sufficient to form solid particles of the polymer; depositing the polymer and drug particles onto said stent framework, wherein an electrical potential is maintained between the stent framework and the polymer and drug particles, thereby forming said coating; and sintering said coating under conditions that do not substantially modify the morphology of said drug; and

20 discharging the drug through a first orifice; forming a first stream of a polymer solution comprising at least one solvent and the polymer; forming a second stream of a supercritical or near supercritical fluid comprising at least one supercritical fluid; contacting said first and second streams, whereby said supercritical or near supercritical fluid acts as a diluent of said solution under conditions sufficient to form particles of said
25 polymer; depositing the polymer and drug particles onto said stent framework, wherein an electrical potential is maintained between the stent framework and the polymer and drug particles, thereby forming said coating; and sintering said coating under conditions that do not substantially modify the morphology of said drug.

INCORPORATION BY REFERENCE

- 5 **[0029]** All publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

BRIEF DESCRIPTION OF THE DRAWINGS

- 10 **[0030]** The novel features of the invention are set forth with particularity in the appended claims. A better understanding of the features and advantages of the present invention will be obtained by reference to the following detailed description that sets forth illustrative embodiments, in which the principles of the invention are utilized, and the accompanying
15 drawings of which:

[0031] Figure 1. Rapid Expansion of Supercritical Solutions (RESS) process equipment.
See C. Domingo et al, Journal of Supercritical Fluids 10, 39-55 (1997)

[0032] Figure 2. Solution Enhanced Dispersion of Supercritical solutions (SEDS) process equipment.

[0033] Figure 3. SEDS nozzle design.

[0034] Figure 4. FTIR spectra of each individual component and the spray coating mixture. Individual peaks for each component are labeled.

[0035] Figure 5. Stents coated (a), (b) and sintered under different conditions (c), (d) with rapamycin, PEVA and PBMA (approximately 1:1:1). All stent surfaces are coated.

[0036] Figure 6. IR spectra of Si wafer chips coated with Rapamycin, PEVA and PBMA before and after sintering. No differences are observable between the two spectra. The baseline shift at larger wavenumber in the as deposited spectrum is due to light scattering caused by the large particle size.

[0037] Figure 7. Crystalline spray-coated rapamycin using a process of the present invention.

[0038] Figure 8. XRD spectra of rapamycin sprayed in two morphologies compared to an authentic sample.

[0039] Figure 9. Particle size control.

[0040] Figure 10. Further apparatus of the invention.

[0041] Figure 11. Cloud point isotherms for polyethylene-co-vinyl acetate (PEVA) and poly(butyl methacrylate) (PBMA) combined as discussed in examples 9, 10, 11 and 12.

[0042] Figure 12. Schematic Representation of the Coating and Sintering Process Apparatus, as discussed in example 9.

[0043] Figure 13. Detailed images of the coating and sintering process apparatus, as discussed in example 9.

[0044] Figure 14. Drug-Polymer coated coronary stent (a) immediately after deposition, (b) after annealing in a dense carbon dioxide environment at 40°C. The photographs correspond to the experiment discussed in example 10.

[0045] Figure 15. 40X Magnified Images of Rapamycin/PEVA/PBMA Coated Stents, Obtained From an Optical Microscope with Back and Side Lighting, Showing the Outside, Edge and Inside Surfaces, (a) before and (b) after sintering, as discussed in example 10.

[0046] Figure 16. 40X Magnified Images of Rapamycin/PEVA/PBMA Coated Stents, Obtained From an Optical Microscope with Back and Side Lighting, Showing the Outside and Inside Surfaces, (a) before and (b) after sintering, as discussed in example 10.

[0047] Figure 17. 100X Magnified Image of a Rapamycin/PEVA/PBMA Coated Stent, Obtained From an Optical Microscope. Crystalline drug is clearly visible embedded within a highly uniform polymer coating, as discussed in example 10.

[0048] Figure 18. Scanning Electron Microscope Images of Rapamycin/PEVA/PBMA Coated Stents, at (a) x30 magnification, (b) x250 magnification, (c) x1000 magnification and (d) x3000 magnification, as discussed in example 11.

[0049] Figure 19. Cross-sectional Scanning Electron Microscope Images of

Rapamycin/PEVA/PBMA Coated Stents at (a) x7000 magnification and (b) x20000

magnification. Four cross-sectional thicknesses measured: (1) $10.355\mu\text{M}$; (2) $10.412\mu\text{M}$; (3)

$10.043\mu\text{M}$ and (4) $10.157\mu\text{M}$, providing a calculated average thickness of $10.242\mu\text{M} \pm 2\%$, also

discussed in example 11.

[0050] Figure 20. Differential Scanning Calorimetry (DSC) of (a) PEVA Control, (b) PBMA

Control, (c) Rapamycin Control and (d) Coated Rapamycin, PEVA, PBMA Mixture. The

Rapamycin crystalline melt at $185\text{-}200^\circ\text{C}$ is indicated in (c) and (d), as discussed in example 12.

[0051] Figure 21. X-Ray Diffraction of (a) Microionized Rapamycin Powder (Control) and (b)

Coated Sintered Rapamycin/PEVA/PBMA Stents, as discussed in example 13.

[0052] Figure 22. Confocal Raman Analysis of Rapamycin/PEVA/PBMA Coated Stents (i.e.

Depth Profiling from Coating Surface to Metal Stent), highlighting (a) Rapamycin Depth Profile

Outside Circumference and (b) Polymer Depth Profile Outside Circumference, as discussed in example 14.

[0053] Figure 23. (a) Rapamycin UV-Vis Spectrum and (b) Calibration Curve at 277nm .

(c) PEVA/PBMA FT-IR Spectrum, (d) PEVA Calibration Curve at 1050nm and (e) PBMA Calibration Curve at 1285nm .

[0054] Figure 24. Quantification of Coating Components, (mean concentrations (3 stents each);

4 cell by 8mm parylene coated). (a) Rapamycin Quantification ($74 \pm 11\mu\text{g}$) Using UV-Vis

Method; (b) PEVA ($1060 \pm 190\mu\text{g}$) and (c) PBMA ($1110 \pm 198\mu\text{g}$) Quantification Using FT-IR Method, as discussed in example 15.

[0055] Figure 25. Optical Microscopy Showing the Outside Surface of a 3mm Guidant TriStar® Stent Coated with Paclitaxel-polymer composite, as discussed in example 16.

[0056] Figure 26. Paclitaxel Quantification After Coating on a 3mm Guidant TriStar® Stent

with Paclitaxel/PEVA/PBMA composite, as discussed in example 16. (a) Calibration Curve at 228nm in ethanol Using UV-Vis Standard Method and (b) Quantification ($148 \pm 14\mu\text{g}$) Using UV-Vis Method.

[0057] Figure 27. Quantification of Coating Components, (mean concentrations (3 stents each);

6 cell by 8mm parylene coated). (a) Rapamycin Quantification ($81 \pm 3\mu\text{g}$) Using UV-Vis

Method; (b) PEVA ($391 \pm 69\mu\text{g}$) and (c) PBMA ($268 \pm 64\mu\text{g}$) Quantification Using FT-IR Method, as discussed in example 17.

[0058] Figure 28. Shows a graphical summary of conditions employed in sintering experiments according to embodiments of the invention.

[0059] Figures 29 and 30 illustrate elution profiles for stents coated according to embodiments of the invention.

[0060] Figure 31 illustrates mechanical stability of stents coated according to embodiments of the invention.

DETAILED DESCRIPTION OF THE INVENTION

5 [0061] The present invention is explained in greater detail below. This description is not intended to be a detailed catalog of all the different ways in which the invention may be implemented, or all the features that may be added to the instant invention. For example, features illustrated with respect to one embodiment may be incorporated into other embodiments, and features illustrated with respect to a particular embodiment may be deleted from that
10 embodiment. In addition, numerous variations and additions to the various embodiments suggested herein will be apparent to those skilled in the art in light of the instant disclosure, which do not depart from the instant invention. Hence, the following specification is intended to illustrate some particular embodiments of the invention, and not to exhaustively specify all permutations, combinations and variations thereof.

15 [0062] Applicants specifically intend that all United States patent references cited herein be incorporated herein by reference in their entirety.

[0063] The present invention provides a cost-effective, efficient method for depositing a combination of an inert polymer or polymers and a pharmaceutical or biological agent or agents, onto parts or all surfaces of a substrate, to form a coating that is of a pre-determined, desired
20 thickness, conformal, substantially defect-free, and uniform and the composition of the coating can be regulated. In particular, the present invention addresses the problem of existing coating processes, which do not allow for structural and morphological preservation of the agents deposited during the coating process.

One aspect of the invention entails the deposition of the pharmaceutical or biological agents as
25 dry powders, using electrostatic capture to attract the powder particles to the substrate. Dry powder spraying is well known in the art, and dry powder spraying coupled with electrostatic capture has been described, for example in US Patents 5,470,603 6,319,541 or 6,372,246. The deposition of the polymer can be performed in any number of standard procedures, as the morphology of the polymer, so long as it provides coatings possessing the desired properties
30 (e.g. thickness, conformity, defect-free, uniformity etc), is of less importance. The function of the polymer is primarily one of inert carrier matrix for the active components of the coating.

[0064] In one aspect, the coating process involves taking the substrates that have been coated with pharmaceutical or biological agents and polymers and subjecting them to a sintering process that takes place under benign conditions, which do not significantly affect the structural and
35 morphological integrity of the pharmaceutical and biological agents. The sintering process as

used in the current invention refers to the process by which parts of the matrix or the entire polymer matrix becomes continuous (e.g., formation of a continuous polymer film). As discussed below, the sintering process is controlled to produce a fully conformal continuous matrix (complete sintering) or to produce regions or domains of continuous coating while producing voids (discontinuities) in the matrix. As well, the sintering process is controlled such that some phase separation is obtained between polymer different polymers (e.g., polymers A and B) and/or to produce phase separation between discrete polymer particles. The sintering process also improves the adhesion of the polymer coating. The sintering process involves treatment of the coated substrate with a compressed gas, compressed liquid, or supercritical fluid at conditions (e.g. temperature and pressure) such that it is a poor solvent or in some instances a non-solvent for the polymers, the pharmaceutical agents and the biological agents, but induces the formation of a continuous coating of polymer. The sintering process takes place under conditions (e.g. mild temperatures), and using benign fluids (e.g. a compressed gas, or supercritical fluid, the gas or fluid may comprise carbon dioxide, isobutylene or a mixture thereof for example) which will not significantly affect the structural and morphological integrity of the pharmaceutical and/or biological agents. It is noted that while under some situations better sintering results may be obtained by using supercritical or near critical fluids, in many embodiments according to the invention, treatment with compressed gas will provide the desired sintered polymer coating. Those of skill in the art will have no difficulty selecting a supercritical fluid, a near critical fluid or compressed gas in practicing the present invention. Sintering conditions may be adjusted such that the sintering process is not fully completed. That is, the sintering does not result in the formation of a fully continuous polymer matrix. When incomplete sintering is practiced according to the invention, some domains in the polymer matrix may be continuous, while other domains will define voids, cavities, pores, channels or interstices where the drug can be encapsulated or sequestered within the polymer matrix. Such a polymer matrix would be at a density less than the bulk density of the polymer; caused by micro or macroscopic voids in the polymer matrix. Alternatively, such a polymer matrix could retain phase separation of the polymer domains or in the case where multiple polymers are used, phase separation between the different polymer species. In most embodiments, whether the sintering process is complete or incomplete, the sintering conditions are selected to produce good adhesion of the coating to the substrate. For stents, adequate adhesion properties will generally reduce or prevent flaking or detachment of the coating from the stent during manipulation in use. [0065] One aspect of the invention is the combination of two or more of the dry powder, RESS and SEDS spraying techniques.

[0066] Another aspect of the invention involves the dry powder spraying of a pharmaceutical agent, in a preferred particle size and morphology, into the same capture vessel as a polymer that is also dry powder sprayed, whereby the spraying of the agent and the polymer is sequential or simultaneous.

5 [0067] Another specific aspect of the invention involves the dry powder spraying of an active biological agent, in a preferred particle size and possessing a particular activity, into the same capture vessel as a polymer that is also dry powder sprayed, whereby the spraying of the agent and the polymer is sequential or simultaneous.

[0068] Yet another aspect of the invention involves the dry powder spraying of a pharmaceutical agent, in a preferred particle size and morphology, into the same capture vessel as a polymer that is sequentially or simultaneously sprayed by the RESS spray process.

10 [0069] Yet another aspect of the invention involves the dry powder spraying of an active biological agent, in a preferred particle size and possessing a particular activity, into the same capture vessel as a polymer that is sequentially or simultaneously sprayed by the RESS spray process.

[0070] Yet another aspect of the invention involves the dry powder spraying of a pharmaceutical agent, in a preferred particle size and morphology, into the same capture vessel as a polymer that is sequentially or simultaneously sprayed by the SEDS spray process.

15 [0071] Yet another aspect of the invention involves the dry powder spraying of an active biological agent, in a preferred particle size and possessing a particular activity, into the same capture vessel as a polymer that is sequentially or simultaneously sprayed by the SEDS spray process.

[0072] Any combination of the above six processes is contemplated by this aspect of the invention.

20 [0073] In further aspects of the invention the substrates that have been coated with pharmaceutical or biological agents and polymers, as described in the above embodiments are then subjected to a sintering process. The sintering process takes place under benign conditions, which do not affect the structural and morphological integrity of the pharmaceutical and biological agents, and refers to a process by which the co-deposited pharmaceutical agent or biological agent-polymer matrix, becomes continuous and adherent to the substrate. This is achieved by treating the coated substrate with a compressed gas, compressed liquid or supercritical fluid at conditions such that it is a poor solvent of the polymers, a weak solvent of the polymers or a non-solvent for the polymers, the pharmaceutical agents and the biological agents, but an agent suitable for the treatment of polymer particles to form continuous polymer coatings. The sintering process takes place under conditions (e.g. mild temperatures), and using

benign fluids (e.g. supercritical carbon dioxide) which will not affect the structural and morphological integrity of the pharmaceutical and biological agents. Other sintering processes, which do not affect the structural and morphological integrity of the pharmaceutical and biological agents may also be contemplated by the present invention.

5 [0074] In further aspects of the invention, it is desirable to create coatings such that release of an active substance occurs with a predetermined elution profile when placed in the desired elution media. Coating properties can be modified in a variety of different ways in order to provide desirable elution profiles.

[0075] The chemical composition of the polymers can be varied, to provide greater or lesser
10 amounts of polymers that will allow or restrict the elution of active substance. For example, if the intended elution media contain water, a higher content of polymers that swell in water, will allow for a faster elution of active substance. Conversely, a higher content of polymers that do not swell in aqueous media will result in a slower elution rate.

[0076] The coating properties can also be controlled by alternating polymer layers. Layers of
15 polymers of different properties are deposited on the substrate in a sequential manner. By modifying the nature of the polymer deposited in each layer (e.g., depositing layers of different polymers) the elution profile of the coating is altered. The number of layers and the sequence in their deposition provide additional avenues for the design of coatings having controlled elution profiles.

20 [0077] The coating properties can also be modified by control of the macro and/or micro-structure of the polymer coating (diffusion pathways). This may be achieved by varying the coating process(es) or by using different sintering conditions.

[0078] The present invention provides several approaches for controlling the elution of a drug or several drugs. For example, in one embodiment, controlled elution is achieved by the
25 segregation of different polymers (e.g. PEVA / PBMA). In another embodiment, control of elution is achieved by controlling the conditions during the sintering process such that controlled incomplete sintering of the polymer matrix is obtained, whereby the coating would retain some of the particle-like structure of the polymer particles as deposited. Incomplete sintering would provide pores/voids in the coating and allow a additional pathways for elution of the drug ,
30 including drug elution around the polymer(s) instead of or in addition to elution through the polymer(s). The size of the pores or voids obtained through incomplete sintering of the polymer matrix may be obtained through several methods. For example, the rate of depressurization of a vessel in which the sintering process is carried out provides one avenue for controlling pore size. The size of the cavities or pores in the coating can be controlled by employing a porogen as an
35 excipient and subsequent removal of at least a portion of the porogen, for example by treatment

with a solvent of the porogen. Preferably, the porogen solvent comprises a densified gas (e.g.; carbon). In some embodiments the porogen is an SOA or other such hydrophobically derivatized carbohydrate. Removal of at least a portion of the porogen is preferably carried out during the sintering process.

5 [0079] In some aspects of the invention, the active substance elution profile is controllable by altering the polymer particle size. The method by which the polymer particles are deposited onto the substrate is thus varied to provide the desired elution rate. For example, for polymers released simultaneously through the same nozzle, RESS release from a supercritical solution would typically result in small polymer particles; RESS-like release from a mixture in a
10 compressed gas usually generates larger polymer particles. Using the SEDS process can result in variable polymer particle size, depending on the particular SEDS conditions employed.

[0080] In further aspects of the invention, the active substance elution profile is controllable by altering the polymer particle shape. One way to achieve variation in polymer particle shape is to alter the initial concentration of the polymers. At lower initial concentrations, polymers are
15 deposited as small particles. At increased concentrations, larger particles are formed. At higher concentrations, the formed particles become elongated, until at high concentrations the elongated features become fiber-like and eventually become continuous fibers.

[0081] In yet other aspects of the invention, the active substance elution profile is controllable by creating discrete domains of chemically different polymers. As described above, chemically
20 different polymers will allow or restrict the elution of active substance in different elution media. By changing the position of such polymers in discrete macroscopic domains within the coating, the elution profiles will be adjustable. For example during a process whereby two different polymers are released sequentially through the same nozzle, particles of either polymer could be deposited to position them, for example, closer to the outside, the inside or the middle of the
25 coating on the substrate. In another embodiment, the two polymers may be released simultaneously through two different nozzles at differing and/or alternating deposition rates, resulting in a similar effect. In a further embodiment, the deposition of eluting and non-eluting polymers is alternated to result in a fluctuating type of release. In yet other embodiments, the polymers are deposited to provide for a pulsatile release of active substance. Separation of the
30 polymer(s) providing different domains for drug diffusion is achieved, for example, by subsequent spray of the polymers through same nozzle or by using multiple nozzles. Also, as described above, controlling the elution of the active substance may be achieved by layering of different polymers across the depth of the coating. A combination of domain separation and cross-depth layering is also contemplated for the design of coatings having controlled elution
35 properties.

[0082] The deposition of active substance during any of these processes may be constant to provide even distribution throughout the coating, or the spraying of the active substance may be varied to result in differing amounts of active substance in the differing polymeric domains within the coating.

5 [0083] In further aspects of the invention, the active substance elution profile is controllable by varying the coating sintering conditions. For example, incomplete sintering will create open spaces, or pores in the interstitial spaces between the polymer particles, which will enable faster eluting of active substance from the coating. Another way to utilize the sintering conditions for elution control would be to deliberately create irregular coatings by foaming during the sintering
10 process. Rapid pressure release of a CO₂- or isobutylene-impregnated polymer film induces formation of foamed polymers which would create a coating with increased porosity and be very 'open' to diffusion/elution. Thus the elution profile would be controllable by manipulating the foaming conditions, which in turn controls the pore density and size.

15 Definitions

[0084] As used in the present specification, the following words and phrases are generally intended to have the meanings as set forth below, except to the extent that the context in which they are used indicates otherwise.

20 [0085] "Substrate" as used herein, refers to any surface upon which it is desirable to deposit a coating comprising a polymer and a pharmaceutical or biological agent, wherein the coating process does not substantially modify the morphology of the pharmaceutical agent or the activity of the biological agent. Biomedical implants are of particular interest for the present invention; however the present invention is not intended to be restricted to this class of substrates. Those of
25 skill in the art will appreciate alternate substrates that could benefit from the coating process described herein, such as pharmaceutical tablet cores, as part of an assay apparatus or as components in a diagnostic kit (e.g. a test strip).

[0086] "Biomedical implant" as used herein refers to any implant for insertion into the body of a human or animal subject, including but not limited to stents (e.g., vascular stents), electrodes,
30 catheters, leads, implantable pacemaker, cardioverter or defibrillator housings, joints, screws, rods, ophthalmic implants, femoral pins, bone plates, grafts, anastomotic devices, perivascular wraps, sutures, staples, shunts for hydrocephalus, dialysis grafts, colostomy bag attachment devices, ear drainage tubes, leads for pace makers and implantable cardioverters and defibrillators, vertebral disks, bone pins, suture anchors, hemostatic barriers, clamps, screws,

plates, clips, vascular implants, tissue adhesives and sealants, tissue scaffolds, various types of dressings (e.g., wound dressings), bone substitutes, intraluminal devices, vascular supports, etc.

[0087] The implants may be formed from any suitable material, including but not limited to organic polymers (including stable or inert polymers and biodegradable polymers), metals, inorganic materials such as silicon, and composites thereof, including layered structures with a core of one material and one or more coatings of a different material. Substrates made of a conducting material facilitate electrostatic capture. However, the invention contemplates the use of electrostatic capture in conjunction with substrate having low conductivity or which non-conductive. To enhance electrostatic capture when a non-conductive substrate is employed, the substrate is processed while maintaining a strong electrical field in the vicinity of the substrate.

[0088] Subjects into which biomedical implants of the invention may be applied or inserted include both human subjects (including male and female subjects and infant, juvenile, adolescent, adult and geriatric subjects) as well as animal subjects (including but not limited to dog, cat, horse, monkey, etc.) for veterinary purposes.

[0089] In a preferred embodiment the biomedical implant is an expandable intraluminal vascular graft or stent (e.g., comprising a wire mesh tube) that can be expanded within a blood vessel by an angioplasty balloon associated with a catheter to dilate and expand the lumen of a blood vessel, such as described in US Patent No. 4,733,665 to Palmaz Shaz.

[0090] "Pharmaceutical agent" as used herein refers to any of a variety of drugs or pharmaceutical compounds that can be used as active agents to prevent or treat a disease (meaning any treatment of a disease in a mammal, including preventing the disease, i.e. causing the clinical symptoms of the disease not to develop; inhibiting the disease, i.e. arresting the development of clinical symptoms; and/or relieving the disease, i.e. causing the regression of clinical symptoms). It is possible that the pharmaceutical agents of the invention may also comprise two or more drugs or pharmaceutical compounds. Pharmaceutical agents, include but are not limited to antirestenotic agents, antidiabetics, analgesics, antiinflammatory agents, antirheumatics, antihypotensive agents, antihypertensive agents, psychoactive drugs, tranquillizers, antiemetics, muscle relaxants, glucocorticoids, agents for treating ulcerative colitis or Crohn's disease, antiallergics, antibiotics, antiepileptics, anticoagulants, antimycotics, antitussives, arteriosclerosis remedies, diuretics, proteins, peptides, enzymes, enzyme inhibitors, gout remedies, hormones and inhibitors thereof, cardiac glycosides, immunotherapeutic agents and cytokines, laxatives, lipid-lowering agents, migraine remedies, mineral products, otologicals, anti parkinson agents, thyroid therapeutic agents, spasmolytics, platelet aggregation inhibitors, vitamins, cytostatics and metastasis inhibitors, phytopharmaceuticals, chemotherapeutic agents and amino acids. Examples of suitable active ingredients are acarbose, antigens, beta-receptor

blockers, non-steroidal antiinflammatory drugs (NSAIDs), cardiac glycosides, acetylsalicylic acid, virustatics, aclarubicin, acyclovir, cisplatin, actinomycin, alpha- and beta-sympatomimetics, (dmeprazole, allopurinol, alprostadil, prostaglandins, amantadine, ambroxol, amlodipine, methotrexate, S-aminosalicylic acid, amitriptyline, amoxicillin, anastrozole,

5 atenolol, azathioprine, balsalazide, beclomethasone, betahistine, bezafibrate, bicalutamide, diazepam and diazepam derivatives, budesonide, bufexamac, buprenorphine, methadone, calcium salts, potassium salts, magnesium salts, candesartan, carbamazepine, captopril, cefalosporins, cetirizine, chenodeoxycholic acid, ursodeoxycholic acid, theophylline and theophylline derivatives, trypsin, cimetidine, clarithromycin, clavulanic acid, clindamycin,

10 clobutinol, clonidine, cotrimoxazole, codeine, caffeine, vitamin D and derivatives of vitamin D, colestyramine, cromoglicic acid, coumarin and coumarin derivatives, cysteine, cytarabine, cyclophosphamide, ciclosporin, cyproterone, cytarabine, dapiprazole, desogestrel, desonide, dihydralazine, diltiazem, ergot alkaloids, dimenhydrinate, dimethyl sulphoxide, dimeticone, domperidone and domperidan derivatives, dopamine, doxazosin, doxorubizin, doxylamine,

15 dapiprazole, benzodiazepines, diclofenac, glycoside antibiotics, desipramine, econazole, ACE inhibitors, enalapril, ephedrine, epinephrine, epoetin and epoetin derivatives, morphinans, calcium antagonists, irinotecan, modafinil, orlistat, peptide antibiotics, phenytoin, riluzoles, risedronate, sildenafil, topiramate, macrolide antibiotics, oestrogen and oestrogen derivatives, progestogen and progestogen derivatives, testosterone and testosterone derivatives, androgen and

20 androgen derivatives, ethebamide, etofenamate, etofibrate, fenofibrate, etofylline, etoposide, famciclovir, famotidine, felodipine, fenofibrate, fentanyl, fenticonazole, gyrase inhibitors, fluconazole, fludarabine, flunarizine, fluorouracil, fluoxetine, flurbiprofen, ibuprofen, flutamide, fluvastatin, follitropin, formoterol, fosfomicin, furosemide, fusidic acid, gallopamil, ganciclovir, gemfibrozil, gentamicin, ginkgo, Saint John's wort, glibenclamide, urea derivatives as oral

25 antidiabetics, glucagon, glucosamine and glucosamine derivatives, glutathione, glycerol and glycerol derivatives, hypothalamus hormones, goserelin, gyrase inhibitors, guanethidine, halofantrine, haloperidol, heparin and heparin derivatives, hyaluronic acid, hydralazine, hydrochlorothiazide and hydrochlorothiazide derivatives, salicylates, hydroxyzine, idarubicin, ifosfamide, imipramine, indometacin, indoramine, insulin, interferons, iodine and iodine

30 derivatives, isoconazole, isoprenaline, glucitol and glucitol derivatives, itraconazole, ketoconazole, ketoprofen, ketotifen, lacidipine, lansoprazole, levodopa, levomethadone, thyroid hormones, lipoic acid and lipoic acid derivatives, lisinopril, lisuride, lofepramine, lomustine, loperamide, loratadine, maprotiline, mebendazole, mebeverine, meclozine, mefenamic acid, mefloquine, meloxicam, mepindolol, meprobamate, meropenem, mesalazine, mesuximide,

35 metamizole, metformin, methotrexate, methylphenidate, methylprednisolone, metixene,

metoclopramide, metoprolol, metronidazole, mianserin, miconazole, minocycline, minoxidil, misoprostol, mitomycin, mizolastine, moexipril, morphine and morphine derivatives, evening primrose, nalbuphine, naloxone, tilidine, naproxen, narcotine, natamycin, neostigmine, nicergoline, nicethamide, nifedipine, niflumic acid, nimodipine, nimorazole, nimustine, nisoldipine, adrenaline and adrenaline derivatives, norfloxacin, novamine sulfone, noscapine, nystatin, ofloxacin, olanzapine, olsalazine, omeprazole, omoconazole, ondansetron, oxaceprol, oxacillin, oxiconazole, oxymetazoline, pantoprazole, paracetamol, paroxetine, penciclovir, oral penicillins, pentazocine, pentifylline, pentoxifylline, perphenazine, pethidine, plant extracts, phenazone, pheniramine, barbituric acid derivatives, phenylbutazone, phenytoin, pimozide, pindolol, piperazine, piracetam, pirenzepine, piribedil, piroxicam, pramipexole, pravastatin, prazosin, procaine, promazine, propiverine, propranolol, propyphenazone, prostaglandins, protionamide, proxyphylline, quetiapine, quinapril, quinaprilat, ramipril, ranitidine, reproterol, reserpine, ribavirin, rifampicin, risperidone, ritonavir, ropinirole, roxatidine, roxithromycin, ruscogenin, rutoside and rutoside derivatives, sabadilla, salbutamol, salmeterol, scopolamine, selegiline, sertaconazole, sertindole, sertraline, silicates, sildenafil, simvastatin, sitosterol, sotalol, sparglumic acid, sparfloxacin, spectinomycin, spiramycin, spirapril, spironolactone, stavudine, streptomycin, sucralfate, sufentanil, sulbactam, sulphonamides, sulfasalazine, sulpiride, sultamicillin, sultiam, sumatriptan, suxamethonium chloride, tacrine, tacrolimus, talinolol, tamoxifen, taurolidine, tazarotene, temazepam, teniposide, tenoxicam, terazosin, terbinafine, terbutaline, terfenadine, terlipressin, tertatolol, tetracyclins, teryzoline, theobromine, theophylline, butizine, thiamazole, phenothiazines, thiotepa, tiagabine, tiapride, propionic acid derivatives, ticlopidine, timolol, tinidazole, tioconazole, tioguanine, tioxolone, tiropramide, tizanidine, tolazoline, tolbutamide, tolcapone, tolnaftate, tolperisone, topotecan, torasemide, antioestrogens, tramadol, tramazoline, trandolapril, tranlycypromine, trapidil, trazodone, triamcinolone and triamcinolone derivatives, triamterene, trifluoperidol, trifluridine, trimethoprim, trimipramine, tripeleminamine, triprolidine, trifosfamide, tromantadine, trometamol, tropalpin, troxerutine, tulobuterol, tyramine, tyrothricin, urapidil, ursodeoxycholic acid, chenodeoxycholic acid, valaciclovir, valproic acid, vancomycin, vecuronium chloride, Viagra, venlafaxine, verapamil, vidarabine, vigabatrin, viloazine, vinblastine, vincamine, vincristine, vindesine, vinorelbine, vinpocetine, viquidil, warfarin, xantinol nicotinate, xipamide, zafirlukast, zalcitabine, zidovudine, zolmitriptan, zolpidem, zopiclone, zotipine and the like. See, e.g., US Patent No. 6,897,205; see also US Patent No. 6,838,528; US Patent No. 6,497,729.

[0091] Examples of therapeutic agents employed in conjunction with the invention include, rapamycin, 40-O-(2-Hydroxyethyl)rapamycin (everolimus), 40-O-Benzyl-rapamycin, 40-O-(4'-Hydroxymethyl)benzyl-rapamycin, 40-O-[4'-(1,2-Dihydroxyethyl)]benzyl-rapamycin, 40-O-

Allyl-rapamycin, 40-O-[3'-(2,2-Dimethyl-1,3-dioxolan-4(S)-yl)-prop-2'-en-1'-yl]-rapamycin, (2':E,4'S)-40-O-(4',5'-Dihydroxypent-2'-en-1'-yl)-rapamycin 40-O-(2-Hydroxy)ethoxycarbonylmethyl-rapamycin, 40-O-(3-Hydroxy)propyl-rapamycin 40-O-(6-Hydroxy)hexyl-rapamycin 40-O-[2-(2-Hydroxy)ethoxy]ethyl-rapamycin 40-O-[(3S)-2,2-Dimethyldioxolan-3-yl]methyl-rapamycin, 40-O-[(2S)-2,3-Dihydroxyprop-1-yl]-rapamycin, 40-O-(2-Acetoxy)ethyl-rapamycin 40-O-(2-Nicotinoyloxy)ethyl-rapamycin, 40-O-[2-(N-Morpholino)acetoxy]ethyl-rapamycin 40-O-(2-N-Imidazolylacetoxy)ethyl-rapamycin, 40-O-[2-(N-Methyl-N'-piperazinyl)acetoxy]ethyl-rapamycin, 39-O-Desmethyl-39,40-O,O-ethylene-rapamycin, (26R)-26-Dihydro-40-O-(2-hydroxy)ethyl-rapamycin, 28-O-Methyl-rapamycin, 40-O-(2-Aminoethyl)-rapamycin, 40-O-(2-Acetaminoethyl)-rapamycin 40-O-(2-Nicotinamidoethyl)-rapamycin, 40-O-(2-(N-Methyl-imidazo-2'-ylcarbethoxamido)ethyl)-rapamycin, 40-O-(2-Ethoxycarbonylaminoethyl)-rapamycin, 40-O-(2-Tolylsulfonamidoethyl)-rapamycin, 40-O-[2-(4',5'-Dicarboethoxy-1',2',3'-triazol-1'-yl)-ethyl]-rapamycin, 42-Epi-(tetrazolyl)rapamycin (tacrolimus), and 42-[3-hydroxy-2-(hydroxymethyl)-2-methylpropanoate]rapamycin (temsirolimus).

[0092] The active ingredients may, if desired, also be used in the form of their pharmaceutically acceptable salts or derivatives (meaning salts which retain the biological effectiveness and properties of the compounds of this invention and which are not biologically or otherwise undesirable), and in the case of chiral active ingredients it is possible to employ both optically active isomers and racemates or mixtures of diastereoisomers.

[0093] "Stability" as used herein in refers to the stability of the drug in a polymer coating deposited on a substrate in its final product form (e.g., stability of the drug in a coated stent). The term stability will define 5% or less degradation of the drug in the final product form.

[0094] "Active biological agent" as used herein refers to a substance, originally produced by living organisms, that can be used to prevent or treat a disease (meaning any treatment of a disease in a mammal, including preventing the disease, i.e. causing the clinical symptoms of the disease not to develop; inhibiting the disease, i.e. arresting the development of clinical symptoms; and/or relieving the disease, i.e. causing the regression of clinical symptoms). It is possible that the active biological agents of the invention may also comprise two or more active biological agents or an active biological agent combined with a pharmaceutical agent, a stabilizing agent or chemical or biological entity. Although the active biological agent may have been originally produced by living organisms, those of the present invention may also have been synthetically prepared, or by methods combining biological isolation and synthetic modification. By way of a non-limiting example, a nucleic acid could be isolated from a biological source, or prepared by traditional techniques, known to those skilled in the art of nucleic acid

synthesis. Furthermore, the nucleic acid may be further modified to contain non-naturally occurring moieties. Non-limiting examples of active biological agents include peptides, proteins, enzymes, glycoproteins, nucleic acids (including deoxyribonucleotide or ribonucleotide polymers in either single or double stranded form, and unless otherwise limited, encompasses known analogues of natural nucleotides that hybridize to nucleic acids in a manner similar to naturally occurring nucleotides), antisense nucleic acids, fatty acids, antimicrobials, vitamins, hormones, steroids, lipids, polysaccharides, carbohydrates and the like. They further include, but are not limited to, antirestenotic agents, antidiabetics, analgesics, antiinflammatory agents, antirheumatics, antihypotensive agents, antihypertensive agents, psychoactive drugs, tranquilizers, antiemetics, muscle relaxants, glucocorticoids, agents for treating ulcerative colitis or Crohn's disease, antiallergics, antibiotics, antiepileptics, anticoagulants, antimycotics, antitussives, arteriosclerosis remedies, diuretics, proteins, peptides, enzymes, enzyme inhibitors, gout remedies, hormones and inhibitors thereof, cardiac glycosides, immunotherapeutic agents and cytokines, laxatives, lipid-lowering agents, migraine remedies, mineral products, otologicals, anti parkinson agents, thyroid therapeutic agents, spasmolytics, platelet aggregation inhibitors, vitamins, cytostatics and metastasis inhibitors, phytopharmaceuticals and chemotherapeutic agents. Preferably, the active biological agent is a peptide, protein or enzyme, including derivatives and analogs of natural peptides, proteins and enzymes.

[0095] "Activity" as used herein refers to the ability of a pharmaceutical or active biological agent to prevent or treat a disease (meaning any treatment of a disease in a mammal, including preventing the disease, i.e. causing the clinical symptoms of the disease not to develop; inhibiting the disease, i.e. arresting the development of clinical symptoms; and/or relieving the disease, i.e. causing the regression of clinical symptoms). Thus the activity of a pharmaceutical or active biological agent should be of therapeutic or prophylactic value.

[0096] "Secondary, tertiary and quaternary structure " as used herein are defined as follows. The active biological agents of the present invention will typically possess some degree of secondary, tertiary and/or quaternary structure, upon which the activity of the agent depends. As an illustrative, non-limiting example, proteins possess secondary, tertiary and quaternary structure. Secondary structure refers to the spatial arrangement of amino acid residues that are near one another in the linear sequence. The α -helix and the β -strand are elements of secondary structure. Tertiary structure refers to the spatial arrangement of amino acid residues that are far apart in the linear sequence and to the pattern of disulfide bonds. Proteins containing more than one polypeptide chain exhibit an additional level of structural organization. Each polypeptide chain in such a protein is called a subunit. Quaternary structure refers to the spatial arrangement of subunits and the nature of their contacts. For example hemoglobin consists of two α and two β

chains. It is well known that protein function arises from its conformation or three dimensional arrangement of atoms (a stretched out polypeptide chain is devoid of activity). Thus one aspect of the present invention is to manipulate active biological agents, while being careful to maintain their conformation, so as not to lose their therapeutic activity.

[0097] "Polymer" as used herein, refers to a series of repeating monomeric units that have been cross-linked or polymerized. Any suitable polymer can be used to carry out the present invention. It is possible that the polymers of the invention may also comprise two, three, four or more different polymers. In some embodiments, of the invention only one polymer is used. In some preferred embodiments a combination of two polymers are used. Combinations of polymers can be in varying ratios, to provide coatings with differing properties. Those of skill in the art of polymer chemistry will be familiar with the different properties of polymeric compounds. Examples of polymers that may be used in the present invention include, but are not limited to polycarboxylic acids, cellulosic polymers, , proteins, polypeptides, polyvinylpyrrolidone, maleic anhydride polymers, polyamides, polyvinyl alcohols, polyethylene oxides, glycosaminoglycans, polysaccharides, polyesters, polyurethanes, polystyrenes, copolymers, silicones, polyorthoesters, polyanhydrides, copolymers of vinyl monomers, polycarbonates, polyethylenes, polypropylenes, polylactic acids, polyglycolic acids, polycaprolactones, polyhydroxybutyrate valerates, polyacrylamides, polyethers, polyurethane dispersions, polyacrylates, acrylic latex dispersions, polyacrylic acid, mixtures and copolymers thereof. The polymers of the present invention may be natural or synthetic in origin, including gelatin, chitosan, dextrin, cyclodextrin, Poly(urethanes), Poly(siloxanes) or silicones, Poly(acrylates) such as poly(methyl methacrylate), poly(butyl methacrylate), and Poly(2-hydroxy ethyl methacrylate), Poly(vinyl alcohol) Poly(olefins) such as poly(ethylene), poly(isoprene), halogenated polymers such as Poly(tetrafluoroethylene) – and derivatives and copolymers such as those commonly sold as Teflon® products, Poly(vinylidene fluoride), Poly(vinyl acetate), Poly(vinyl pyrrolidone), Poly(acrylic acid), Polyacrylamide, Poly(ethylene-co-vinyl acetate), Poly(ethylene glycol), Poly(propylene glycol), Poly(methacrylic acid); etc. Suitable polymers also include absorbable and/or resorbable polymers including the following, combinations, copolymers and derivatives of the following: Polylactides (PLA), Polyglycolides (PGA), Poly(lactide-co-glycolides) (PLGA), Polyanhydrides, Polyorthoesters, Poly(N-(2-hydroxypropyl) methacrylamide), Poly(l-aspartamide), etc.

[0098] "Therapeutically desirable morphology" as used herein refers to the gross form and structure of the pharmaceutical agent, once deposited on the substrate, so as to provide for optimal conditions of ex vivo storage, in vivo preservation and/or in vivo release. Such optimal conditions may include, but are not limited to increased shelf life, increased in vivo stability,

good biocompatibility, good bioavailability or modified release rates. Typically, for the present invention, the desired morphology of a pharmaceutical agent would be crystalline or semi-crystalline or amorphous, although this may vary widely depending on many factors including, but not limited to, the nature of the pharmaceutical agent, the disease to be treated/prevented, the intended storage conditions for the substrate prior to use or the location within the body of any biomedical implant. Preferably at least 10%, 20%, 30%, 40%, 50%, 60%, 70%, 80%, 90% or 100% of the pharmaceutical agent is in crystalline or semi-crystalline form.

[0099] "Stabilizing agent" as used herein refers to any substance that maintains or enhances the stability of the biological agent. Ideally these stabilizing agents are classified as Generally Regarded As Safe (GRAS) materials by the US Food and Drug Administration (FDA). Examples of stabilizing agents include, but are not limited to carrier proteins, such as albumin, gelatin, metals or inorganic salts. Pharmaceutically acceptable excipient that may be present can further be found in the relevant literature, for example in the Handbook of Pharmaceutical Additives: An International Guide to More Than 6000 Products by Trade Name, Chemical, Function, and Manufacturer; Michael and Irene Ash (Eds.); Gower Publishing Ltd.; Aldershot, Hampshire, England, 1995.

[00100] "Compressed fluid" as used herein refers to a fluid of appreciable density (e.g., >0.2 g/cc) that is a gas at standard temperature and pressure. "Supercritical fluid", "near-critical fluid", "near-supercritical fluid", "critical fluid", "densified fluid" or "densified gas" as used herein refers to a compressed fluid under conditions wherein the temperature is at least 80% of the critical temperature of the fluid and the pressure is at least 50% of the critical pressure of the fluid.

[00101] Examples of substances that demonstrate supercritical or near critical behavior suitable for the present invention include, but are not limited to carbon dioxide, isobutylene, ammonia, water, methanol, ethanol, ethane, propane, butane, pentane, dimethyl ether, xenon, sulfur hexafluoride, halogenated and partially halogenated materials such as chlorofluorocarbons, hydrochlorofluorocarbons, hydrofluorocarbons, perfluorocarbons (such as perfluoromethane and perfluoropropane, chloroform, trichloro-fluoromethane, dichloro-difluoromethane, dichloro-tetrafluoroethane) and mixtures thereof.

[00102] "Sintering" as used herein refers to the process by which parts of the matrix or the entire polymer matrix becomes continuous (e.g., formation of a continuous polymer film). As discussed below, the sintering process is controlled to produce a fully conformal continuous matrix (complete sintering) or to produce regions or domains of continuous coating while producing voids (discontinuities) in the matrix. As well, the sintering process is controlled such that some phase separation is obtained between polymer different polymers (e.g., polymers A

and B) and/or to produce phase separation between discrete polymer particles. Through the sintering process, the adhesions properties of the coating are improved to reduce flaking of detachment of the coating from the substrate during manipulation in use. As described below, in some embodiments, the sintering process is controlled to provide incomplete sintering of the polymer matrix. In embodiments involving incomplete sintering, a polymer matrix is formed with continuous domains, and voids, gaps, cavities, pores, channels or, interstices that provide space for sequestering a therapeutic agent which is released under controlled conditions. Depending on the nature of the polymer, the size of polymer particles and/or other polymer properties, a compressed gas, a densified gas, a near critical fluid or a super-critical fluid may be employed. In one example, carbon dioxide is used to treat a substrate that has been coated with a polymer and a drug, using dry powder and RESS electrostatic coating processes. In another example, isobutylene is employed in the sintering process. In other examples a mixture of carbon dioxide and isobutylene is employed.

[00103] When an amorphous material is heated to a temperature above its glass transition temperature, or when a crystalline material is heated to a temperature above a phase transition temperature, the molecules comprising the material are more mobile, which in turn means that they are more active and thus more prone to reactions such as oxidation. However, when an amorphous material is maintained at a temperature below its glass transition temperature, its molecules are substantially immobilized and thus less prone to reactions. Likewise, when a crystalline material is maintained at a temperature below its phase transition temperature, its molecules are substantially immobilized and thus less prone to reactions. Accordingly, processing drug components at mild conditions, such as the deposition and sintering conditions described herein, minimizes cross-reactions and degradation of the drug component. One type of reaction that is minimized by the processes of the invention relates to the ability to avoid conventional solvents which in turn minimizes autoxidation of drug, whether in amorphous, semi-crystalline, or crystalline form, by reducing exposure thereof to free radicals, residual solvents and autoxidation initiators.

[00104] "Rapid Expansion of Supercritical Solutions" or "RESS" as used herein involves the dissolution of a polymer into a compressed fluid, typically a supercritical fluid, followed by rapid expansion into a chamber at lower pressure, typically near atmospheric conditions. The rapid expansion of the supercritical fluid solution through a small opening, with its accompanying decrease in density, reduces the dissolution capacity of the fluid and results in the nucleation and growth of polymer particles. The atmosphere of the chamber is maintained in an electrically neutral state by maintaining an isolating "cloud" of gas in the chamber. Carbon

dioxide or other appropriate gas is employed to prevent electrical charge is transferred from the substrate to the surrounding environment.

[00105] "Bulk properties" properties of a coating including a pharmaceutical or a biological agent that can be enhanced through the methods of the invention include for example: adhesion, smoothness, conformality, thickness, and compositional mixing.

[00106] "Solution Enhanced Dispersion of Supercritical Solutions" or "SEDS" as used herein involves a spray process for the generation of polymer particles, which are formed when a compressed fluid (e.g. supercritical fluid, preferably supercritical CO₂) is used as a diluent to a vehicle in which a polymer dissolved, (one that can dissolve both the polymer and the compressed gas). The mixing of the compressed fluid diluent with the polymer-containing solution may be achieved by encounter of a first stream containing the polymer solution and a second stream containing the diluent compressed fluid, for example, within one co-axial spray nozzle or by the use of multiple spray nozzles or by the use of multiple fluid streams co-entering into a mixing zone. The solvent in the polymer solution may be one compound or a mixture of two or more ingredients and may be or comprise an alcohol (including diols, triols, etc.), ether, amine, ketone, carbonate, or alkanes, or hydrocarbon (aliphatic or aromatic) or may be a mixture of compounds, such as mixtures of alkanes, or mixtures of one or more alkanes in combination with additional compounds such as one or more alcohols. (e.g., from 0 or 0.1 to 5% of a C₁ to C₁₅ alcohol, including diols, triols, etc.). See for example US Patent No. 6,669,785. The solvent may optionally contain a surfactant, as also described in (for example) US Patent No. 6,669,785.

[00107] In one embodiment of the SEDS process, a first stream of fluid comprising a polymer dissolved in a common solvent is co-sprayed with a second stream of compressed fluid. Polymer particles are produced as the second stream acts as a diluent that weakens the solvent in the polymer solution of the first stream. The now combined streams of fluid, along with the polymer particles, flow into a collection vessel. In another embodiment of the SEDS process, a first stream of fluid comprising a drug dissolved in a common solvent is co-sprayed with a second stream of compressed fluid. Drug particles are produced as the second stream acts as a diluent that weakens the solvent in the drug solution of the first stream. The now combined streams of fluid, along with the drug particles, flow out into a collection vessel. Control of particle size, particle size distribution, and morphology is achieved by tailoring the following process variables: temperature, pressure, solvent composition of the first stream, flow-rate of the first stream, flow-rate of the second stream, composition of the second stream (where soluble additives may be added to the compressed gas), and conditions of the capture vessel. Typically the capture vessel contains a fluid phase that is at least five to ten times (5-10x) atmospheric pressure.

~~PCT/US2006/027321~~

[00108] "Electrostatically charged" or "electrical potential" or "electrostatic capture" as used herein refers to the collection of the spray-produced particles upon a substrate that has a different electrostatic potential than the sprayed particles. Thus, the substrate is at an attractive
5 electronic potential with respect to the particles exiting, which results in the capture of the particles upon the substrate. i.e. the substrate and particles are oppositely charged, and the particles transport through the fluid medium of the capture vessel onto the surface of the substrate is enhanced via electrostatic attraction. This may be achieved by charging the particles and grounding the substrate or conversely charging the substrate and grounding the particles, or
10 by some other process, which would be easily envisaged by one of skill in the art of electrostatic capture.

[00109] "Open vessel" as used herein refers to a vessel open to the outside atmosphere, and thus at substantially the same temperature and pressure as the outside atmosphere.

[00110] "Closed vessel" as used herein refers to a vessel sealed from the outside
15 atmosphere, and thus may be at significantly different temperatures and pressures to the outside atmosphere.

[00111] Examples

[00112] The following examples are given to enable those skilled in the art to more clearly understand and to practice the present invention. They should not be considered as limiting the
20 scope of the invention, but merely as being illustrative and representative thereof.

[00113] **Example 1. Process Equipment**

[00114] The RESS process equipment used in the present studies is depicted in Figure 1. This is a common design for a RESS apparatus see C. Domingo et al, Journal of Supercritical Fluids 10, 39-55 (1997). The SEDS equipment used in the present studies is depicted in Figures
25 2 and 10. Figure 2 shows a common SEDS apparatus and Figure 10 shows a SEDS apparatus using a two-nozzle design with electrostatic capture of the sprayed particles. The nozzle orifice size can be used to control the particle size. Figure 3 depicts the nozzle design for the SEDS equipment shown in Figures 2 and 10. Figure 4 shows the FTIR spectra of a representative small molecule medically therapeutic agent, two polymers and the mixture of the components. IR
30 stretches specific to each molecule are identified and labeled. Figure 5 shows implantable medical devices coated with pharmaceutical agent and polymer under various sintering conditions. Figure 6 shows the infrared spectra of the 3-component coating before and after sintering. The spectra demonstrate that the sintering process does not adversely impact the coating since no new stretches appear in the after sintering spectrum. Figure 7 shows a wide
35 (left panel) and narrow (right panel) field view of sprayed rapamycin. Both crystalline and

amorphous rapamycin are visible in the images. Figure 8 shows XRD data taken for an authentic rapamycin sample, RESS sprayed rapamycin and SEDS sprayed rapamycin. The RESS sprayed rapamycin lacks any crystallinity indicated by the absence of diffraction peaks in the XRD.

SEDS sprayed rapamycin has diffraction peaks that are identical to the authentic sample

5 indicating that the two materials are the same. Figure 9 demonstrates particle size control using the SEDS process. In the upper left is an optical photograph of a view cell containing a substrate (horizontal line in bottom portion of the window) held at 2500 psi. An SEM micrograph is in the lower left image showing aggregated particles averaging approximately 35 nm in size. The upper right panel in figure 9 shows an optical photograph of a view cell pressurized at 1200 psi.

10 The particles are sufficiently large to scatter light as evidenced by the cloud of particles above the substrate in the image. The lower right panel in figure 9 shows that the particle size is approximately 20 microns. Figure 10 shows the SEDS spraying apparatus with a two-nozzle design and novel high voltage power supply used for the electrostatic collection of the SEDS sprayed particles. By operating at voltages below the component with the lowest ionization

15 potential, electrostatic collection of the SEDS sprayed particles can be achieved.

[00115] **Example 2. General Spray Coating 1**

[00116] A solution containing a therapeutic chemical compound that is saturated in a solvent or supersaturated in a solvent is sprayed at a flow rate sufficient to achieve flow into a chamber of known volume pressurized above ambient pressure and containing a medical device

20 substrate. The system temperature is held constant or allowed to vary so that any number of points in the phase diagrams of the solution or mixture or any of its individual components can be mapped in pressure-temperature, volume-pressure or pressure-volume space constituting liquid, gas or supercritical CO₂ conditions. CO₂ in any single phase or combination of phases flows through the chamber at a mass flow rate of 5 gm/min to some multiple of this flow rate.

25 After a period of time ranging from seconds to minutes or hours have elapsed, the solute and solvent flow that is a solution of the therapeutic compound and suitable solvent for the chosen solute or solutes cease but CO₂ flow continues for an additional period of time maintaining constant pressure during this period. After this time period, the pressure is dropped to atmospheric pressure. During the spray coating process the particles are attracted to the medical

30 substrate by charging the substrate oppositely to that of the sprayed particle charge by applying a voltage that is greater than 5000 V but less than the ionization potential of the most easily ionized component of the mixture. The particles may also traverse an electromagnetic field such that the field is used to guide the particle to a target.

[00117] Example 3. Spray Coating 2

[00118] A solution of equal parts of one solvent and another miscible solvent containing therapeutic chemical compound is prepared so that compound is not saturated. This solution is sprayed at a known flow rate ranging from 1mL/min to 100mL/min into a chamber of known volume and pressurized above ambient pressure. The system temperature is maintained at a constant level or allowed to vary so that any number of points in the phase diagrams of the solution or mixture or any of its individual components can be mapped in pressure –temperature, volume-pressure or pressure-volume space. CO₂ flows through the chamber at a known flow rate. Spraying is stopped after a period of time, but CO₂ flow continues for an additional period of time sufficient to ensure that the chamber volume has been turned over or replaced a sufficient number of times to remove any residual solvent or co-solvent from the chamber after which the pressure is reduced to atmospheric pressure. As in the above example, the particles generated in the spray process are collected on the medical substrate electrostatically as they are generated.

[00119] Example 4. Spray Coating 3

[00120] A therapeutic compound in a crystalline dry powder state is sprayed through a nozzle using dry powder coating process directed toward a stent. From a separate nozzle a CO₂ solution containing the polymer and a co-solvent or a polymer solution prepared in a suitable solvent such as dimethyl ether is sprayed toward the stent. The CO₂ flow rate is variable. The temperature of the stent and therapeutic chemical compound remain at room temperature or below room temperature in order to prevent degradation of thermally sensitive therapeutic compounds but the polymer solution temperature is maintained above the solvent critical temperature and pressure so that a supercritical solution or near supercritical solution exists. The particles are electrostatically captured during their generation or as they exit the dry powder spray nozzle as described in the previous examples.

[00121] Example 5. Uniform Surface Coating

[00122] The ability to uniformly coat arterial stents with controlled composition and thickness using electrostatic capture in a rapid expansion of supercritical solution (RESS) experimental series has been demonstrated. This technique involves spraying an equal part mixture of the therapeutic compound such as rapamycin and polymers such as PBMA and PEVA using a spray coating and collection technique described herein. To determine coating composition, infrared spectroscopy was used to collect the spectrum of a silicon wafer chip coated simultaneously with an arterial stent (Figure 4). Unique absorption bands were identified for each mixture component and band area was used as a metric to determine incorporation of each compound in the coating.

[00123] The individual bands used for compositional analysis were determined by spray coating Si wafer chips with each component separately. The coating thickness was determined gravimetrically and calculated from the density of the materials. It was assumed that the layer is fully dense. The thickness can be controlled by varying the spray time.

5 In the as sprayed state, the coating lacks strong adhesion to the substrate. Sintering the coated substrate (see Figure 5) dramatically improves coating adhesion while leaving the components unaltered as the infrared spectra shown in figure 6 confirm. The coating is sintered in a supercritical carbon dioxide environment allowing mild sintering conditions to be used with temperature below 80°C.

10 [00124] **Example 6. Spray Coating of Crystalline Rapamycin**

[00125] Several carbon dioxide based spray-coating methods were attempted to spray deposit rapamycin in crystalline form including RESS without successfully controlling rapamycin morphology. One SEDS coating method was successful in spray coating crystalline rapamycin as shown in figures 7 and 8. A solution of 10 parts hexane and 9 parts THF saturated
15 with Rapamycin is sprayed at a flow rate of 0.5 mL/min into a 25 mL chamber pressurized at 82 bar with carbon dioxide. The system temperature is held constant at 25°C constituting liquid CO₂ conditions. CO₂ flows through the pressurized chamber at a mass flow rate of 5 gm/min. After 5 minutes have elapsed, the drug and polymer spray cease but CO₂ flow continues for an additional 20 minutes maintaining constant pressure during this period. After this time period,
20 the pressure is dropped to atmospheric pressure. The particles are attracted to the substrate by charging the substrate oppositely to the particle charge by applying a voltage that is greater than 5000 V but less than the ionization potential of the most easily ionized component of the mixture.

[00126] As the SEM images show in Figure 7, crystalline rapamycin was deposited on the
25 substrate and the crystal size is approximately 2 microns (right panel in the figure) along its major axis with large crystalline aggregates distributed across the substrate surface (left panel).

[00127] The diffraction peaks in the XRD shown in Figure 8 confirm the identity of the crystals as rapamycin since the sprayed rapamycin (lowest spectrum) matches the as received rapamycin (middle spectrum) peak for peak. XRD results for other failed attempts (upper
30 spectrum) to spray crystalline rapamycin are included for comparative purposes. The amorphous diffraction pattern displayed in the top trace of figure 8 was obtained from a RESS sprayed sample and is also representative of failed attempts to spray crystalline rapamycin using SEDS based approaches using only polar or non-polar solvents. The goal of this experimental series was to demonstrate a carbon dioxide technique that could spray rapamycin in crystalline form.

35 No attempt was made to control crystal size, coverage uniformity, or aggregation

[00128] Example 7. Particle Size Control

[00129] Figure 9 shows optical and electron microscope comparison of the SEDS spraying process under different pressure conditions. Figure 9(a) shows an optical photograph taken of the view cell with CO₂ present at 1200 psi and 25°C. The nozzle appears as an angled line at approximately 11 o'clock originating from the left of the view cell. The substrate appears as a horizontal line in the bottom of the view cell. Figure 9(c) is a scanning electron micrograph of the particles deposited on the substrate that was removed from the view cell in 9(a). The scale of the scanning electron micrograph demonstrates the particle size.

[00130] Figure 9(b) shows an optical photograph taken of the view cell with CO₂ present at 2500 psi and 25°C. The nozzle appears as an angled line at approximately 11 o'clock originating from the left of the view cell. The substrate appears as a horizontal line in the bottom of the view cell. Figure 9(d) is a scanning electron micrograph of the particles deposited on the substrate that was removed from the view cell in 9(b). The scale of the scanning electron micrograph demonstrates the particle size. These images demonstrate an ability to control particle size and morphology. Both these features are important as elution rates can be affected by both parameters.

[00131] Example 8. Further Process Equipment

[00132] Further equipment is shown in Figure 10. This apparatus is used to spray rapamycin in crystalline form using a SEDS process with electrostatic capture. The unique features of this apparatus are the dual nozzle design and high voltage pass through permitting electrostatic capture of the sprayed particles. In other respects the design is similar to other SEDS equipment.

The dual nozzle separates polymer and drug spraying from each other which is important as it has been shown that polymers co-sprayed with another component can influence the ability of non polymer component to form particulate in the desired morphology. However, both the components are sprayed into the same chamber allowing the particles to be collected at a single point.

The high voltage pass through permits electrostatic capture of the sprayed components onto the desired substrate.

[00133] Example 9. Preparation of supercritical solution comprising, polyethylene-co-vinyl acetate (PEVA) and polybutyl methacrylate (PBMA) in isobutylene.

[00134] 75 mg of PEVA and 75 mg of PBMA are placed in a 25 mL view cell. The view cell is heated to 150 °C.

Isobutylene is added to a pressure of 3000 psig. Under these conditions, a clear solution is produced.

[00135] **Example 10.** Preparation of supercritical solution comprising polyethylene-co-vinyl acetate (PEVA) and polybutyl methacrylate (PBMA) in isobutylene.

150 mg of PEVA and 150 mg of PBMA are placed in a 25 mL view cell. The view cell is heated to 150 °C.

5 Isobutylene is added to a pressure of 4000 psig. Under these conditions, a clear solution is produced.

[00136] **Example 11.** Preparation of supercritical solution comprising polyethylene-co-vinyl acetate (PEVA) and polybutyl methacrylate (PBMA) in isobutylene and CO₂.

75 mg of PEVA and 75 mg of PBMA are placed in a 25 mL view cell and the cell is heated to 10 150°C.

Isobutylene is added to a pressure of 4000 psig, to produce a clear solution.

10 (v/v%) CO₂ is added. The addition of CO₂ at this volume percent does not precipitate the dissolved polymer.

[00137] **Example 12.** Preparation of supercritical solution comprising polyethylene-co-vinyl acetate (PEVA) and polybutyl methacrylate (PBMA) in isobutylene and CO₂.

15 150 mg of PEVA and 150 mg of PBMA are placed in a 25 mL view cell and the cell is heated to 150°C.

Isobutylene is added to a pressure of 4000 psig, to produce a clear solution.

10 (v/v%) CO₂ is added. The addition of CO₂ at this volume percent does not precipitate the dissolved polymer; however addition of CO₂ at higher volume fraction leads to polymer precipitation, under these conditions.

[00138] **Example 13.** Dry powder rapamycin coating on an electrically charged 316 stainless steel coupon.

[00139] A 1cm x 2cm stainless steel metal coupon serving as a target substrate for rapamycin coating was placed in a vessel and attached to a high voltage electrode. The vessel (V), of approximately 1500cm³ volume, was equipped with two separate nozzles through which rapamycin or polymers could be selectively introduced into the vessel. Both nozzles were grounded. Additionally, the vessel (V) was equipped with a separate port was available for purging the vessel. Upstream of one nozzle (D) was a small pressure vessel (PV) approximately 5cm³ in volume with three ports to be used as inlets and outlets. Each port was equipped with a valve which could be actuated opened or closed. One port, port (1) used as an inlet, was an addition port for the dry powdered rapamycin. Port (2), also an inlet was used to feed pressurized gas, liquid, or supercritical fluid into PV. Port (3), used as an outlet, was used to connect the pressure vessel (PV) with nozzle (D) contained in the primary vessel (V) with the target coupon. Dry powdered Rapamycin obtained from LC Laboratories in a predominantly

crystalline solid state, 50mg, milled to an average particle size of approximately 3 microns, was loaded into (PV) through port (1) then port (1) was actuated to the closed position. Gaseous carbon dioxide was then added to (PV) to a pressure of 400 to 600 psig at 20°C through port (2), then port (2) was closed to the source gas. The metal coupon was then charged to 40kV using a Glassman Series EL high-voltage power source. Port (3) was then actuated open allowing for the expansion of the pressurized carbon dioxide and rapamycin powder into the vessel (V) while the coupon remained charged. After approximately 60-seconds the voltage was eliminated and the coupon was isolated. Upon visual inspection of the coupon using an optical microscope it was determined that the entire surface area of the coupon, other than a small portion masked by the voltage lead, was covered in a relatively even distribution of powdered material. X-ray diffraction (XRD) confirmed that the powdered material was largely crystalline in nature as deposited on the metal coupon. UV-Vis and FTIR spectroscopy confirmed that the material deposited on the coupon was rapamycin.

[00140] Example 14. Dry powder rapamycin coating on a 316-stainless steel coupon with no electrical charge.

[00141] A coupon was coated in an identical fashion to what was described in Example 13. However, no voltage was applied to the coupon throughout the dry powder-coating run. After expansion of the carbon dioxide and the powdered rapamycin into vessel (V), and a period of roughly 60 seconds, the coupon was isolated and evaluated. The coupon was analyzed using an optical microscope and showed some dry powder material on much of the surface of the coupon. However, the coverage of drug on the surface was much lower than in example 1 and there was notably more variability in coverage at different locations on the coupon surface. The total powder coating was estimated to be about 1/3rd the amount determined to be crystalline rapamycin in example 1.

[00142] Example 15. Polymer coating on an electrically charged 316-stainless steel coupon using rapid expansion from a liquefied gas.

[00143] A coating apparatus as described in example 13 above was used in the foregoing example. In this example the second nozzle, nozzle (P), was used to feed precipitated polymer particles into vessel (V) to coat a 316-stainless steel coupon. Nozzle (P) was equipped with a heater and controller to minimize heat loss due to the expansion of liquefied gases. Upstream of nozzle (P) was a pressure vessel, (PV2), with approximately 25-cm³ internal volume. The pressure vessel (PV2) was equipped with multiple ports to be used for inlets, outlets, thermocouples, and pressure transducers. Additionally, (PV2) was equipped with a heater and a temperature controller. Each port was connected to the appropriate valves, metering valves, pressure regulators, or plugs to ensure adequate control of material into and out of the pressure

vessel (PV2). One outlet from (PV2) was connected to a metering valve through pressure rated tubing which was then connected to nozzle (P) located in vessel (V). In the experiment, 75 mg of polyethylene-co-vinyl acetate (PEVA) obtained from Aldrich Chemical Company with approximately 33-weight percent vinyl acetate and 75 mg of poly(butyl methacrylate) (PBMA) also obtained from Aldrich Chemical Company were added to pressure vessel (PV2).

Dichlorofluoromethane, 20.0 grams, was added to the pressure vessel (PV2) through a valve and inlet. Pressure vessel (PV2) was then heated to 40°C bringing the pressure inside the isolated vessel to approximately 40 psig. Nozzle (P) was heated to 120°C. After sufficient time to dissolve the two polymers in the liquefied gas inside (PV2), the vessel (PV2) was over-

pressurized with helium to approximately 200 psig using a source helium tank and a dual stage pressure regulator. See U.S. patent 6,905,555 for a description of Helium displacement art. A 1-cm x 2-cm 316-stainless steel coupon was placed into vessel (V) and attached to an electrical lead. Nozzle (P) was attached to ground. The coupon was charged to 40kV using a Glassman high-voltage power source at which point the metering valve was opened between (PV2) and nozzle (P) in pressure vessel (PV). Polymer dissolved in liquefied gas and over-pressurized with helium to 200 psig was fed at a constant pressure of 200 psig into vessel (V) maintained at atmospheric pressure through nozzle (P) at an approximate rate of 3.0 cm³/min. After approximately 5 seconds, the metering valve was closed discontinuing the polymer-solvent feed. Vessel (V) was purged with gaseous CO₂ for 30 seconds to displace chlorofluorocarbon. After approximately 30 seconds, the metering valve was again opened for a period of approximately 5 seconds and then closed. This cycle was repeated about 4 times. After an additional 1-minute the applied voltage to the coupon was discontinued and the coupon was removed from pressure vessel (V). Upon inspection by optical microscope, a polymer coating was evident as evenly distributed on all non-masked surfaces of the coupon. Dissolution of the polymer mixture from the surface of the coupon followed by quantification using standardized quantitative FT-IR methods determined a composition of approximately 1:1 PEVA to PBMA on the coupon.

[00144] **Example 16.** Dual coating of a metal coupon with crystalline rapamycin, and 1:1 mixture of polyethylene-co-vinyl acetate (PEVA) and poly(butyl methacrylate) (PBMA).

[00145] An apparatus described in example 13 and further described in example 15 was used in the foregoing example. In preparation for the coating experiment, 25 mg of crystalline powdered rapamycin with an average particle size of 3-microns was added to (PV) through port (1), then port (1) was closed. Then, (PV) was pressurized to 400-600 psig with gaseous carbon dioxide at 20°C through port (2), prior to closing port (2). Next, 75 mg of polyethylene-co-vinyl acetate (PEVA) with approximately 33-weight percent vinyl acetate and 75 mg of poly(butyl methacrylate) (PBMA) were added to pressure vessel (PV2). Dichlorofluoromethane, 20.0

granis, was added to the pressure vessel (PV2) through a valve and inlet. Pressure vessel (PV2) was then heated to 40°C bringing the pressure inside the isolated vessel (PV2) to approximately 40 psig. Nozzle (P) was heated to 120°C. After sufficient time to dissolve the two polymers in the liquefied gas, the vessel was over-pressurized with helium to approximately 200 psig using a source helium tank and a dual stage pressure regulator. A 1-cm x 2-cm 316-stainless steel coupon was added to vessel (V) and connected to a high-voltage power lead. Both nozzles (D) and (P) were grounded. To begin, the coupon was charged to 40kV after which port (3) connecting (PV) containing rapamycin to nozzle (D) was opened allowing expansion of carbon dioxide and ejection of rapamycin into vessel (V) maintained at ambient pressure. After closing port (3) and approximately 60-seconds, the metering valve connecting (PV2) with nozzle (P) inside vessel (V) was opened allowing for expansion of liquefied gas to a gas phase and introduction of precipitated polymer particles into vessel (V) while maintaining vessel (V) at ambient pressure. After approximately 5-seconds at a feed rate of approximately 3cm³/min., the metering valve was closed while the coupon remained charged. Port (1) was then opened and an additional 25-mg of powdered crystalline rapamycin was added to (PV), and then port (1) was closed. Pressure vessel (PV) was then pressurized with liquid carbon dioxide to 400-600 psig through port (2), after which port (2) was again closed. Maintaining the coupon at an applied voltage of 40kV, port (3) was again opened to nozzle (D) allowing for the expansion of carbon dioxide to a gas and the ejection of the powdered crystalline drug into the vessel (V). After and additional 60-seconds, the metering valve between (PV2) and nozzle (P) was again opened allowing for the expansion of the liquefied solvent to a gas into vessel (V) and the precipitation of polymer particles also in vessel (V). The sequential addition of drug followed by polymer or polymer followed by drug as described above was repeated for a total of four (4) cycles after which the applied potential was removed from the coupon and the coupon was removed from the vessel. The coupon was then examined using an optical microscope. A consistent coating was visible on all surfaces of the coupon except where the coupon was masked by the electrical lead. The coating appeared conformal but opaque and somewhat granular at high magnification.

[00146] **Example 17.** Dual coating of a metal coupon with crystalline rapamycin, and 1:1 mixture of polyethylene-co-vinyl acetate (PEVA) and poly(butyl methacrylate) (PBMA) followed by Supercritical Carbon Dioxide Annealing or Gaseous Carbon Dioxide Annealing.

[00147] After inspection of the coupon created in example 16, the coated coupon was carefully placed in a pressure vessel that was pressurized with carbon dioxide to a pressure of 4500 psig and at a temperature of 60°C. This CO₂ sintering process was done to enhance the physical properties of the film on the coupon. The coupon remained in the vessel under these conditions for approximately 3 hours after which the supercritical CO₂ was slowly vented from

the pressure vessel and then the coupon was removed and reexamined under an optical microscope. The coating was observed to be conformal, consistent, and semi-transparent as opposed to the opaque coating observed and reported in example 16 without dense carbon dioxide treatment. The coated coupon was then submitted for x-ray diffraction (XRD) analysis which confirmed the presence of crystalline rapamycin in the polymer matrix.

[00148] **Example 18.** Dual coating of a metal cardiovascular stent with crystalline rapamycin, and 1:1 mixture of polyethylene-co-vinyl acetate (PEVA) and poly (butyl methacrylate) (PBMA).

[00149] The apparatus described in examples 13, 15, and 16 above was used in the foregoing example. The metal stent used was a Tristar™ Coronary Stent of a nominal size of 3mm by 13mm. The stent was coated in an identical fashion to the coupon described in example 16 above. The stent was coated in an alternating fashion whereby the first coating layer of drug was followed by a thin layer of polymer. These two steps, called a drug/polymer cycle, were repeated 3-times so that the last applied coating layer was polymer. After completion of the coating step, the stent was removed from the vessel (V) and placed in a small pressure vessel where it was exposed to supercritical CO₂ as described above in example 16. After this low temperature annealing step, the stent was removed and examined using an optical microscope. The stent was then analyzed using a scanning electron microscope (SEM) equipped with a fast ion bombarding (FIB) device to provide cross-sectional analysis of the coated stent. The SEM micrograph at multiple locations on the stent indicated a completely conformal coating of between 6 and 15-microns in thickness. Evidence of rapamycin crystallites was also apparent in the micrographs.

[00150] **Example 19.** Layered coating of a cardiovascular stent with an anti-restenosis therapeutic and polymer in layers to control drug elution characteristics.

[00151] A cardiovascular stent is coated using the methods described in examples 17 and 18 above. The stent is coated in such as way that the drug and polymer are in alternating layers. The first application to the bare stent is a thin layer of a non-resorbing polymer, approximately 2-microns thick. The second layer is a therapeutic agent with anti-restenosis indication. Approximately 35 micrograms are added in this second layer. A third layer of polymer is added at approximately 2-microns thick, followed by a fourth drug layer which is composed of about 25 micrograms of the anti-restenosis agent. A fifth polymer layer, approximately 1- micron thick is added to stent, followed by the sixth layer that includes the therapeutic agent of approximately 15-micrograms. Finally, a last polymer layer is added to a thickness of about 2-microns. After the coating procedure, the stent is annealed using carbon dioxide as described in example 16 above. In this example a drug eluting stent (DES) is described with low initial drug

“burst” properties by virtue of a “sequestered drug layering” process, not possible in conventional solvent-based coating processes. Additionally, by virtue of a higher concentration of drug at the stent ‘inter-layer’ the elution profile is expected to reach as sustained therapeutic release over a longer period of time.

5 [00152] **Example 20.** Layered coating of a cardiovascular stent with an anti-restenosis therapeutic and an anti-thrombotic therapeutic in a polymer matrix.

[00153] A cardiovascular stent is coated as described in example 19 above. In this example, after a first polymer layer of approximately 2-microns thick, a drug with anti-thrombotic indication is added in a layer of less than 2-microns in thickness. A third layer
10 consisting of the non-resorbing polymer is added to a thickness of about 4-microns. Next another drug layer is added, a different therapeutic, with an anti-restenosis indication. This layer contains approximately 100 micrograms of the anti-restenosis agent. Finally, a polymer layer approximately 2-microns in thickness is added to the stent. After coating the stent is treated as described in example 16 to anneal the coating using carbon dioxide.

15 [00154] **Example 22.** Coating of stents with Rapamycin, polyethylene-co-vinyl acetate (PEVA) and polybutyl methacrylate (PBMA)

[00155] Micronized Rapamycin was purchased from LC Laboratories. PBMA (Mw = ~237k) and PEVA (33% vinyl acetate content) were purchased from Aldrich Chemicals. Two kinds of stents were used: 3mm TriStar® from Guidant and 6 cell x 8-mm, BX Velocity® from
20 Cordis. The stents were coated by dry electrostatic capture followed by supercritical fluid sintering, using 3 stents/coating run and 3 runs/data set. The coating apparatus is represented in figure 12. Analysis of the coated stents was performed by multiple techniques on both stents and coupons with relevant control experiments.

[00156] In this example a 1:1 ratio of PEVA and PBMA is dissolved in a
25 Dichlorofluoromethane (CCl_2FH), which is a compressed gas solvent known to be in the class of “Freon” chemicals. The physical properties of this particular Freon are as follows:

BP= 8.9 C

Tc=178.33 C

Pc=751.47 psig

30 Dc=0.526014 g/cc

[00157] A solution was formed by mixing 30 mg of the combined polymers per gram dichlorofluoromethane . The solution was then maintained at 60°C at vapor pressure (approx 28 psig) until the solution was ready to spray. The solution was then pressurized by adding an immiscible gas to the top of the vessel - typically Helium. Adding Helium compressed the
35 Freon-polymer solution up to 700 (+/-50 psig), which resulted in a compressed fluid. The

polymer-Freon solution was then pushed through a nozzle having an inner diameter of 0.005" by continuous addition of Helium into the vessel. The solvent (dichlorofluoromethane) is rapidly vaporized coming out of the nozzle (which is heated to 120°C), as its boiling point is significantly below room temperature.

5 The Drug is deposited by dry powder spray coating. Between 10-30 mg of drug are charged into a small volume of tubing, which is then pressurized with gaseous CO₂ to 400 psig. The mixture flows through a nozzle having an inner diameter of 0.187" into the coating vessel where the stents are held. During electrostatic deposition, the stent is charged and the nozzles are grounded. Figures 12 and 13 show the apparatus used for the coating and sintering process.

10 **[00158] Example 23. Optical Microscopy Analysis of Rapamycin/PEVA/PBM Coated Stents**

The stents produced in example 22 were examined by optical microscopy, at 40X magnification with back and side lighting. This method was used to provide a coarse qualitative representation of coating uniformity and to generally demonstrate the utility of the low-temperature CO₂

15 annealing step. The resulting photos shown in figure 14, demonstrate the differences in appearance (a) before and (b) after annealing in dense carbon dioxide at 40°C. Photos of the outside, edge and inside surfaces are presented in figure 15 (a), prior to sintering, which clearly shows nanoparticle deposition equally on all surfaces of the stent, and 15(b) after sintering, with the film showing a smooth and optically transparent polymer. Figure 16 shows additional 40X magnified images of Rapamycin/PEVA/PBMA coated stents, showing the outside and inside surfaces, (a) before sintering, further demonstrating the nanoparticle deposition equally on all surfaces of the stent and (b) after sintering, showing a smooth and optically transparent polymer film. Figure 17 shows a 100X magnified images of Rapamycin/PEVA/PBMA Coated Stents. Crystalline drug is clearly visible embedded within a highly uniform polymer coating.

25 **[00159] Example 24. Scanning Electron Microscopy Analysis of Rapamycin/PEVA/PBM Coated Stents**

[00160] The stents produced in example 21 were examined by scanning electron microscopy, and the resulting images presented in figure 18 at (a) x30 magnification, (b) x250 magnification, (c) x1000 magnification and (d) x3000 magnification. Clearly the nanoparticles have been sintered to an even and conformal film, with a surface topology of less than 5 microns, and demonstrate clear evidence of embedded crystalline rapamycin.

Cross-sectional (FIB) images were also acquired and are shown in figure 19(a) at 7000x and (b) 20000x magnification. An even coating of consistent thickness is visible. Four cross-sectional thicknesses were measured: (1) 10.355μM, (2) 10.412μM, (3) 10.043μM and (4) 10.157μM, to give an average thickness of 10.242μM, with only 2% (±0.2μM) variation.

[00161] **Example 25.** Differential Scanning Calorimetry (DSC) of

Rapamycin/PEVA/PBM Coated Stents

[00162] The stents produced in example 21 were examined by Differential Scanning Calorimetry (DSC). Control analyses of PEVA only, PBMA only and Rapamycin only are shown in figure 20 (a), (b) and (c) respectively. The DSC of the Rapamycin, PEVA and PBMA coated stent is shown in figure 20 (d). The rapamycin crystalline melt is clearly visible at 185-200°C and distinct from those of the polymers.

[00163] **Example 26.** X-Ray Diffraction (XRD) of Rapamycin/PEVA/PBM Coated Stents

[00164] The stents produced in example 21 were examined by X-Ray Diffraction (XRD). The control spectrum of micro-ionized Rapamycin powder is shown in figure 21 (a). The XRD of the Rapamycin, PEVA and PBMA coated, sintered stent is shown in figure 21 (b), showing that the Rapamycin remains crystalline (~64%) throughout the coating and sintering process.

[00165] **Example 27.** Confocal Raman Analysis of Rapamycin/PEVA/PBM Coated Stents

[00166] The stents produced in example 21 were examined by Confocal Raman Analysis, to provide depth profiling from the coating surface down to the metal stent. Figure 22 (a) shows the Rapamycin depth profile outside circumference (Rapamycin peak at ~1620) and 22 (b) shows the polymer depth profile outside circumference, clearly demonstrating that the drug is distributed throughout polymer coated stents. The highest drug content appears in the center of the polymer coating (~4μM from the air surface), which is controllable, via the coating and sintering conditions used. In certain embodiments of the invention, the drug would be close to the air surface of the coating. In other embodiments, the drug would be closer to the metal stent. In other embodiments, more than one drug would be deposited in the coating, wherein one drug would be closer to the air surface and another drug would be closer to the metal surface. In yet other embodiments, the drugs would be distributed together throughout the coating.

[00167] **Example 28.** UV-Vis and FT-IR Analysis of Rapamycin/PEVA/PBM Coated Stents for Quantification of Coating Components

[00168] A UV-VIS method was developed and used to quantitatively determine the mass of rapamycin coated onto the stents with poly(ethylene-co-vinyl acetate) (PEVA) and poly(butyl methacrylate) (PBMA). The UV-Vis spectrum of Rapamycin is shown in figure 23 (a) and a Rapamycin calibration curve was obtained, λ @ 277nm in ethanol, as shown in figure 23 (b). Rapamycin was dissolved from the coated stent in ethanol, and the drug concentration and mass calculated. An average mass of 74 ± 11μg Rapamycin was loaded onto the stents. The results in

figure 24 (a) show a consistent drug coating: (+/-) 15% stent-to-stent, (+/-) 12% run-to-run, (mean concentrations (3 stents each); 4 cell by 8mm parylene coated).

[00169] An FT-IR method was developed and used to quantitatively determine the mass of PEVA and PBMA coated onto stents with rapamycin. The FT-IR spectra of PEVA and PBMA is shown in figure 23 (c) and calibration curves were obtained using Beer's Law for PEVA $\lambda @ \sim 1050\text{cm}^{-1}$ and PBMA $\lambda @ \sim 1285\text{cm}^{-1}$, as shown in figures 23 (d) and (e), respectively. The polymers were dissolved from the coated stent in methylene chloride, and the polymer concentrations and the masses calculated accordingly. An average mass of $1060 \pm 190\mu\text{g}$ PEVA and $1110 \pm 198\mu\text{g}$ PBMA was loaded onto the stents. The results in figures 24 (b) and (c) show a consistent polymer coating: (+/-) 18% stent-to-stent, (+/-) 15% run-to-run, (mean concentrations (3 stents each); 4 cell by 8mm parylene coated).

[00170] **Example 29.** Coating of stents with with Paclitaxel/PEVA/PMBA

[00171] 3mm Guidant TriStar® Stents were coated with a Paclitaxel/PEVA/PMBA composite, by processes of the invention, as described herein. The coated stents were examined by optical microscopy, and photos of the outside surface of the stent (a) prior to sintering and (b) after sintering are shown in figure 25. Figure 26 (a) represents the UV-Vis calibration curve developed for Paclitaxel, $\lambda @ 228\text{ nm}$ in ethanol, using the methods of example 28, as described above. Rapamycin was dissolved from the coated stent in ethanol, and the drug concentration and mass calculated, to give an average mass of $148 \pm 14\mu\text{g}$ loaded Rapamycin, as shown in figure 26 (b).

[00172] **Example 30.** UV-Vis and FT-IR Analysis of Rapamycin/PEVA/PBM Coated Stents for Quantification of Coating Components

[00173] The UV-VIS and FT-IR methods, described in example 28, were used to determine the quantities of Rapamycin, PEVA and PBMA respectively, from stents coated with Rapamycin, PEVA and PBMA by processes of the invention, as described herein. The component quantifications are shown in figure 27 and calculated; (a) an average mass of $81 \pm 3\mu\text{g}$ Rapamycin was loaded onto the stents, (b) an average mass of $391 \pm 69\mu\text{g}$ PEVA and (c) $268 \pm 64\mu\text{g}$ PBMA was loaded onto the stents.

[00174] **Example 31.** Coating of stents with Rapamycin or Paclitaxel, polyethylene-co-vinyl acetate (PEVA) and polybutyl methacrylate (PBMA)

[00175] A 25 mL stainless steel reservoir is charged with $150.0 \pm 0.1\text{ mg}$ of poly(ethylene co-vinyl acetate) (PEVA) and $150.0 \pm 0.1\text{ mg}$ of poly(butyl methacrylate) (PBMA) to which is transferred $20.0 \pm 0.3\text{ grams}$ of dichlorofluoromethane. The pressure rises in the reservoir to approximately 28 psig. The reservoir is heated to 60°C after transferring dichlorofluoromethane to the reservoir. The reservoir is then pressurized with helium until the pressure reaches $700 \pm$

30 psig. Helium acts as a piston to push out the dichlorofluoromethane-polymer solution. The reservoir is isolated from the system by appropriate valving. A second stainless steel reservoir with volume of 15 ± 1 mL is charged with 13 mg of drug compound (rapamycin or Paclitaxel).

This reservoir is pressurized to 400 ± 5 psig with carbon dioxide gas. The temperature of the

5 drug reservoir is room temperature. The reservoir is isolated from the system by appropriate valving. A third reservoir is charged with tetrahydrofuran or dichloromethane solvent so that the polymer nozzle can be flushed between polymer sprays. This reservoir is also pressurized with helium to 700 psig and isolated from the system by appropriate valving. The polymer spray nozzle is heated to 120 ± 2 °C while the drug spray nozzle remains at room temperature. Stents

10 are loaded into the stent fixture and attached to a high voltage source via an alligator clamp. The alligator clamp enters the coating chamber via an electrically insulated pass through. Carbon dioxide gas is admitted into the coating vessel at 8 psig for a period of 5 minutes through a third gas flush nozzle to remove air and moisture to eliminate arcing between the nozzles and components held at high potential. After flushing the coating chamber with carbon dioxide gas, a

15 potential of 35kV is applied to the stents via a high voltage generator. This potential is maintained during each coating step of polymer and drug. The potential is removed when the polymer spray nozzle is flushed with tetrahydrofuran or dichloromethane. Polymer solution is sprayed for 7 secs from the polymer solution reservoir into the coating chamber. The applied potential is turned off and the polymer nozzle is removed from the coating chamber and flushed

20 with solvent for 2 minutes and then flushed with helium gas for approximately one minute until all solvent is removed from the nozzle. The coating chamber is flushed with carbon dioxide gas during the nozzle solvent flush to flush out dichlorofluoromethane gas. The polymer spray nozzle is placed back in the coating chamber and the carbon dioxide gas flush is stopped. A 35 kV potential is applied to the stents and the drug compound is rapidly sprayed into the coating chamber by opening appropriate valving. After one minute of rest time, polymer spray

25 commences for another seven seconds. The process can be repeated with any number of cycles.

[00176] The various analytical methods developed to examine the coated stents and the results they generated are summarized in the table below:

Analytical Method	To Provide	Result
Optical microscope	Visible images of the stents. Empirical survey of coating uniformity	Nanoparticles deposited evenly on all surfaces of stent Sintering to conformal film (with visual evidence of crystalline drug)
SEM	Top-down and cross-sectional images (electron micrographs) at various magnifications. Gross estimates of coating uniformity and thickness	Very smooth and conformal films at high magnification 10.2 ± 0.3 µm well-sintered films via cross-sectional analysis
X-ray diffraction (XRD)	Quantitative indication of drug morphology in coated films on proxy substrates	+65% crystalline rapamycin on proxy samples
Differential Scanning Calorimetry (DSC)	Qualitative evidence of crystalline rapamycin from proxy substrates (crystalline melt)	Demonstrated rapamycin crystalline melt (185-200°C)
Confocal Raman	Compositional data (drug, polymer A, Polymer B) at various depths in the film on the coated stents (i.e. surface, 2µm deep, 4-µm deep, etc.)	Drug distributed throughout polymer coated stents
UV-Vis Spectroscopy	Quantitative compositional information for drug loading on 'sacrificial' coated stents, BL method	74 ± 11µg drug loaded onto stents, run-to-run control within 12% deviation
FT-IR spectroscopy	Quantitative compositional information for loading of both polymers on 'sacrificial' coated stents, BL method	1060 ± 190µg PEVA loaded onto stents 1110 ± 198 µg PBMA loaded onto stents

]

[00177]

Example 32. (Figures 29 and 30) An elution medium was identified to produce elution profile under static conditions. SDS surfactant at 1% (v/v) in phosphate buffer at pH 7.0 was selected as the elution medium based upon comparison of the elution profiles generated with this medium to the desired elution profiles. The experiment showed that it was possible to generate an elution profile over a period of 30 hrs in a thermostatically controlled bath held at 37±1 °C over the time of the elution experiment (see figure 29). The samples used were sterilized at using an ethylene oxide process. Additional elution work was carried out to develop an elution method. The materials used were supplied by Aldrich (polymers) and LC Laboratories (Rapamycin). The elution profile is shown in figure 30. Another set of stents was analyzed. The set included 6 drug coated stents and two placebo stents. This set of stents showed no elution; however, the placebo stent was sintered simultaneously with the drug coated stent. Upon analysis, the placebo showed some rapamycin. These stents were subjected to stripping analysis to determine if any drug was present but simply did not elute. No drug was found.

[00178] Example 33: Mechanical stability of illustrative coated stents (Figure 31)

[00179] Balloon Inflation: stents were transferred onto a balloon dilation catheter via an “over the wire” transfer.

A stylet was inserted into the lumen of the catheter; the stent was picked up via the sterile
5 needle and transferred onto the stylet. The stent was manipulated on to the center of the balloon-
and the entire assembly was placed under the microscope. Due to the lack of crimping
equipment, the stent was adjusted in position by the use of a small vascular forceps placed on the
balloon to preclude the stent from shooting off during inflation and balloon expansion.

[00180] Inflation/(slow inflation)

10 The balloon was inflated using an inflator with an atmospheric pressure gauge- and expanded
in the same fashion that one would inflate a balloon / stent during an intervention. (rapid
expansion) – and the stents were observed at the completion of the “procedure”. The balloon
was taken up one atmosphere at a time – and the stent / balloon interface examined under the
microscope at each inflation. The balloon stent was placed on a clean microscope slide – to catch
15 any particulate. During the entire inflation process - no particulate/ no separation/ nor flaking
was evidenced on any of the stents. Materials on and around the abluminal area were seen to be
deformed and flattened by the balloon inflation – and were seen to be in approximation to the
stent struts. Any of the materials that were crossed or jumped from strut to strut were particularly
examined towards the effect of the expansion on the materials. In these experiments, the crossed
20 struted materials would break off – rather they elongated during the expansion – and never
separated from the main body.

[00181] Over Inflation

Each of the stents was inflated to its nominal expansion size for examination – and then
the stent was further expanded until balloon rupture – achieving in many cases a 75% increase in
25 size. Particular attention was paid to the inner and outer portions of the angled aspects of the
stent strut that provides the ability to expand. Where the nominal expanded angle might be on
the order of 20-25 degrees of deflection we were taking the stent to a point where these angles
were 45 plus degrees. None of the hyper expansion caused any deformation or flaking or
separation of the coating.

30 [00182] The materials showed good adhesion properties. The materials did not exhibit
any lack of adhesion even with excessive expansion. In the major areas of stent flex /
deformation during balloon inflation - no separation was seen. No particulate is evidenced in the
shipping vials. While some degree of strut-to-strut “cross talk” was seen – it was primarily as a
result of environmental contamination – which can be eliminated or reduce, for example, by

using clean room and laminar flow hoods and/or filtered gases. The polymer and drug combination appears to have excellent elongation properties.

[00183] In summary, in certain embodiments, the present invention provides a method for coating drug-eluting stents. Polymer(s) and drug(s) are applied in a controlled, low-temperature, solvent-free process. In one embodiment Rapamycin, PBMA and PEVA are applied to provide a conformal, consistent coating at target Rapamycin loading, in a 1:1 mixture of PBMA:PEVA, at a thickness of $\sim 10\mu\text{M}$, containing zero residual solvent. The Rapamycin is deposited in crystalline morphology ($\pm 50\%$). The Rapamycin/PEVA/PBMA film is applied using a method through which the stent is not exposed to solvents in the liquid state, wherein the drug and polymer content is highly controllable, and easily adaptable for different drugs, different (resorbable and permanent) polymers, multiple drugs on a single stent, and provides for a high degree of stent-to-stent precision. The absence of exposure of the stent to traditional liquid solvents during deposition enables control over drug content at variable film depths.

[00184] The foregoing is illustrative of the present invention, and is not to be construed as limiting thereof. While embodiments of the present invention have been shown and described herein, it will be obvious to those skilled in the art that such embodiments are provided by way of example only. Numerous variations, changes, and substitutions will now occur to those skilled in the art without departing from the invention. It should be understood that various alternatives to the embodiments of the invention described herein may be employed in practicing the invention. It is intended that the following claims define the scope of the invention and that methods and structures within the scope of these claims and their equivalents be covered thereby.

[00185] Throughout this specification and the claims which follow, unless the context requires otherwise, the word "comprise", and variations such as "comprises" and "comprising", will be understood to imply the inclusion of a stated integer or step or group of integers or steps but not the exclusion of any other integer or step or group of integers or steps.

[00186] The reference in this specification to any prior publication (or information derived from it), or to any matter which is known, is not, and should not be taken as an acknowledgment or admission or any form of suggestion that that prior publication (or information derived from it) or known matter forms part of the common general knowledge in the field of endeavour to which this specification relates.

2006270221 15 Dec 2011

THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:

1. A method for coating a substrate, said coating comprising
 at least one polymer; and
 5 at least one pharmaceutical agent in a therapeutically desirable morphology and/or
 at least one active biological agent;
 said method comprising the following steps:
 discharging the at least one pharmaceutical agent and/or at least one active
 biological agent in dry powder form through a first orifice;
 10 discharging the at least one polymer in dry powder form through a second orifice;
 depositing the polymer and pharmaceutical agent and/or active biological agent
 particles onto said substrate, wherein an electrical potential is maintained between the
 substrate and the polymer and pharmaceutical agent and/or active biological agent
 particles, thereby forming said coating; and
 15 sintering said coating under conditions that do not substantially modify the
 morphology of said pharmaceutical agent and/or the activity of said biological agent,
 wherein said sintering comprises treating said coated substrate with a compressed gas,
 compressed liquid or supercritical fluid that is a non-solvent for both the polymer and the
 pharmaceutical and/or biological agents.
 20
2. A method for coating a substrate, said coating comprising
 at least one polymer; and
 at least one pharmaceutical agent in a therapeutically desirable morphology and/or
 at least one active biological agent;
 25 said method comprising the following steps:
 discharging the at least one pharmaceutical agent and/or at least one active
 biological agent in dry powder form through a first orifice;
 forming a supercritical or near supercritical fluid solution comprising at least one
 supercritical fluid solvent and at least one polymer and discharging said supercritical or
 30 near supercritical fluid solution through a second orifice under conditions sufficient to
 form solid particles of the polymer;
 depositing the polymer and pharmaceutical agent and/or active biological agent
 particles onto said substrate, wherein an electrical potential is maintained between the

2006270221 15 Dec 2011

substrate and the polymer and pharmaceutical agent and/or active biological agent particles, thereby forming said coating; and

sintering said coating under conditions that do not substantially modify the morphology of said pharmaceutical agent and/or the activity of said biological agent,

5 wherein said sintering comprises treating said coated substrate with a compressed gas, compressed liquid or supercritical fluid that is a non-solvent for both the polymer and the pharmaceutical and/or biological agents.

3. A device comprising a substrate and a coating on the substrate formed by the
10 method of either claim 1 or claim 2.

4. The device of claim 3, wherein said substrate is a biomedical implant, and wherein said biomedical implant is selected from the group consisting of stents, joints, screws, rods, pins, plates, staples, shunts, clamps, clips, sutures, suture anchors, electrodes, catheters,
15 leads, grafts, dressings, pacemakers, pacemaker housings, cardioverters, cardioverter housings, defibrillators, defibrillator housings, prostheses, ear drainage tubes, ophthalmic implants, orthopedic devices, vertebral disks, bone substitutes, anastomotic devices, perivascular wraps, colostomy bag attachment devices, hemostatic barriers, vascular implants, vascular supports, tissue adhesives, tissue sealants, tissue scaffolds and
20 intraluminal devices.

5. The method of either claim 1 or claim 2, wherein the therapeutically desirable morphology of said pharmaceutical agent is crystalline or semi-crystalline.

25 6. The method of either claim 1 or claim 2, wherein following sintering, at least 70% of said pharmaceutical agent in the coating is crystalline or semi-crystalline.

7. The method of either claim 1 or claim 2, wherein said compressed gas, compressed liquid or supercritical fluid comprises carbon dioxide, isobutylene or a mixture thereof
30

8. The method of either claim 1 or claim 2, wherein the at least one polymer comprises two or more polymers, wherein the first polymer swells in aqueous media and the second polymer does not substantially swell in aqueous media.

2006270221 15 Dec 2011

9. The method of claim 8, wherein in aqueous media said pharmaceutical agent and/or active biological agent elutes from said first polymer, and substantially does not elute from second polymer.

5

10. The method of either claim 1 or claim 2, wherein said at least one pharmaceutical agent is selected from: Paclitaxel, Sirolimus, Everolimus, Zotarolimus, Dexamethasone, Tacrolimus, Biolimus, Leflunomide, M-Prednisolone, Cyclosporine, Mycophenolic Acid, Mizoribine, Tranilast, Angiopeptin, Methotrexate, Actinomycin, Abbott ABT-578, RestenASE, 2-choloro-deoxyadenosine Taxol and Taxol derivatives, Sirolimus and derivatives, Rituxan, Avastin, Herceptin, Activase, Caflo Activase, TNKase, Diclofenac, Indometacin, Ibuprofen, Sulindac, Abciximab, Heparin and derivatives such as Enoxaparin, Dalteparin, Nadroparin, Tinzaparin, and Hirudin, Hirolog, Warfarin and derivatives.

15

11. A coated vascular stent, comprising:

a stent framework; and

a rapamycin-polymer coating wherein at least part of rapamycin is in crystalline form, wherein the coated coronary stent is formed by the following method:

20 discharging the rapamycin in dry powder form through a first orifice; discharging the polymer in dry powder form through a second orifice; depositing the polymer and rapamycin particles onto said stent framework, wherein an electrical potential is maintained between the stent framework and the polymer and rapamycin particles, thereby forming said coating; and sintering said coating under conditions that do not substantially
25 modify the morphology of said rapamycin, wherein said sintering comprises treating said coating with a compressed gas, compressed liquid or supercritical fluid that is a non-solvent for both the polymer and the rapamycin.

12. A coated vascular stent, comprising:

30 a stent framework; and

a rapamycin-polymer coating wherein at least part of rapamycin is in crystalline form, wherein the coated coronary stent is formed by the following method:

2006270221 15 Dec 2011

discharging the rapamycin in dry powder form through a first orifice; forming a supercritical or near supercritical fluid solution comprising at least one supercritical fluid solvent and the polymer and discharging said supercritical or near supercritical fluid solution through a second orifice under conditions sufficient to form solid particles of the polymer; depositing the polymer and rapamycin particles onto said stent framework, wherein an electrical potential is maintained between the stent framework and the polymer and rapamycin particles, thereby forming said coating; and sintering said coating under conditions that do not substantially modify the morphology of said rapamycin, wherein said sintering comprises treating said coating with a compressed gas, compressed liquid or supercritical fluid that is a non-solvent for both the polymer and the rapamycin.

13. A coated vascular stent, comprising:
a stent framework; and
a rapamycin-polymer coating wherein at least part of rapamycin is in crystalline form, wherein the coated coronary stent is formed by the following method:

discharging the rapamycin through a first orifice; forming a first stream of a polymer solution comprising at least one solvent and the polymer; forming a second stream of a supercritical or near supercritical fluid comprising at least one supercritical fluid; contacting said first and second streams, whereby said supercritical or near supercritical fluid acts as a diluent of said solution under conditions sufficient to form particles of said polymer; depositing the polymer and rapamycin particles onto said stent framework, wherein an electrical potential is maintained between the stent framework and the polymer and rapamycin particles, thereby forming said coating; and sintering said coating under conditions that do not substantially modify the morphology of said rapamycin, wherein said sintering comprises treating said coating with a compressed gas, compressed liquid or supercritical fluid that is a non-solvent for both the polymer and the rapamycin.

14. The device of claim 3, wherein the substrate comprises a stent having a stent framework; wherein the pharmaceutical agent comprises rapamycin, and wherein at least part of the rapamycin is in crystalline form.

2006270221 15 Dec 2011

15. The coated vascular stent of any one of claims 11 to 13, wherein the stent framework is precoated with a primer layer of Parylene C and the rapamycin-polymer coating comprises polybutyl methacrylate (PBMA) and polyethylene-co-vinyl acetate (PEVA).
- 5 16. The coated vascular stent of any one of claims 11 to 13, wherein the stent framework is precoated with a primer layer of Parylene C and the rapamycin-polymer coating comprises one or more styrene based (co)polymer.
- 10 17. The coated vascular stent of any one of claims 11 to 13, wherein the stent framework is precoated with a primer layer of Parylene C and the rapamycin-polymer coating comprises one or more resorbable polymers.
- 15 18. The device of claim 3, wherein the coating comprises one or more resorbable polymers.
19. The coated vascular stent of any one of claims 11 to 13, wherein said rapamycin-polymer coating has substantially uniform thickness and rapamycin in the rapamycin-polymer coating is substantially uniformly dispersed within the coating.
- 20 20. The coated vascular stent of any one of claims 11 to 13, wherein said rapamycin is at least one of: at least 50% crystalline, at least 70% crystalline, and at least 90% crystalline.
- 25 21. The coated vascular stent of any one of claims 11 to 13, wherein the rapamycin in said stent has a shelf stability of at least 3 months, at least 6 months, and/or at least 9 months.
- 30 22. The coated vascular stent of any one of claims 11 to 13, wherein said stent provides an elution profile wherein about 10% to about 50% of rapamycin is eluted at week 1 after the stent is implanted in a subject under physiological conditions, about 25% to about 75% of rapamycin is eluted at week 2 and about 50% to about 100% of rapamycin is eluted at week 4.

2006270221 15 Dec 2011

The device of claim 3, wherein the pharmaceutical agent comprises a macrolide immunosuppressive drug which comprises one or more of rapamycin, 40-O-(2-Hydroxyethyl)rapamycin (everolimus), 40-O-Benzyl-rapamycin, 40-O-(4'-Hydroxymethyl)benzyl-rapamycin, 40-O-[4'-(1,2-Dihydroxyethyl)benzyl-rapamycin, 40-O-Allyl-rapamycin, 40-O[3'-(2,2-Dimethyl-1,3-dioxolan-4(S)-yl)-prop-2'en-1'-yl]-rapamycin, (2'E,4'S)-40-O-(4',5'-Dihydroxypent-2'en-1'-yl)-rapamycin 40-O-(2-Hydroxy)ethoxycarbonylmethyl-rapamycin, 40-O-(3-Hydroxy)propyl-rapamycin 4O-O-(6-Hydroxy)hexyl-rapamycin 40-O-[2-(2-Hydroxy)ethoxy]ethyl-rapamycin 4O-O-[(3S)-2,2-Dimethyldioxolan-3-yl)methyl-rapamycin, 4O-O-[(2S)-2,3-Dihydroxyprop-1-yl]-rapamycin, 4O-O-(2-Acetoxy)ethyl-rapamycin 4O-O-(2-Nicotinoyloxy)ethyl-rapamycin, 40-O-(N-Morpholino)acetoxylethy]-rapamycin 4O-O-(2-N-Imidazolylacetoxy)ethyl-rapamycin, 4O-O-[2-(N-Methyl-N'-piperazinyl)acetoxy]ethyl-rapamycin, 39-O-Desmethyl-39,40-O, O-ethylene-rapamycin, (26R)-26-Dihydro-40-O-(2-hydroxy)ethyl-rapamycin, 28-O-Methyl-rapamycin, 4O-O-(2-Aminoethyl)-rapamycin, 4O-O-(2-Acetaminoethyl)-rapamycin 4O-O-(2-Nicotinamidoethyl)-rapamycin, 4O-O-(2-(N-Methylimidazo-2'-ylcarbathoxamido)ethyl)-rapamycin, 4O-O-(2-Ethoxycarbonylaminoethyl)-rapamycin, 40-O-(2-Tolylsulfonylamidoethyl)-rapamycin, 40-O[2-(4',5'-Dicarboethoxy-1',2',3'-triazol-1'-yl)-ethyl]-rapamycin, 42-Epi-(tetrazoly)rapamycin (tacrolimus), and 42-

[3-hydroxy-2-(hydroxymethyl)-2-methylpropanoate]rapamycin (temsirolimus).

24. The device of claim 3, or the coated vascular stent of any one of claims 11 to 13, wherein said coating is substantially free of solvent residue.

25 25. The device of claim 3, wherein the pharmaceutical agent is selected from the group consisting of antirestenotic agents, antidiabetics, analgesics, antiinflammatory agents, antirheumatics, antihypotensive agents, antihypertensive agents, psychoactive drugs, tranquillizers, antiemetics, muscle relaxants, glucocorticoids, agents for treating ulcerative colitis or Crohn's disease, antiallergies, antibiotics, antiepileptics, anticoagulants, 30 antimycotics, antitussives, arteriosclerosis remedies, diuretics, proteins, peptides, enzymes, enzyme inhibitors, gout remedies, hormones and inhibitors thereof, cardiac glycosides, immunotherapeutic agents and cytokines, laxatives, lipid-lowering agents, migraine remedies, mineral products, otologicals, anti parkinson agents, thyroid therapeutic agents.

2006270221 15 Dec 2011

spasmolytics, platelet aggregation inhibitors, vitamins, cytostatics and metastasis inhibitors, phytopharmaceuticals, chemotherapeutic agents and amino acids. Examples of suitable active ingredients are acarbose, antigens, beta-receptor blockers, non-steroidal antiinflammatory drugs (NSAIDs), cardiac glycosides, acetylsalicylic acid, virustatics,

5 aclarubicin, acyclovir, cisplatin, actinomycin, alpha- and beta-sympatomimetics, (dimeprazole, allopurinol, alprostadil, prostaglandins, amantadine, ambroxol, amlodipine, methotrexate, S-aminosalicylic acid amitriptyline, amoxicillin, anastrozole, atenolol, azathioprine, balsalazide, beclomethasone, betahistine, bezafibrate, bicalutamide, diazepam and diazepam derivatives, budesonide, bufexamac, buprenorphine, methadone,

10 calcium salts, potassium salts, magnesium salts, candesartan, carbamazepine, captopril, cefalosporins, cetirizine, chenodeoxycholic acid, ursodeoxycholic acid, theophylline and theophylline derivatives, trypsins, cimetidine, clarithromycin, clavulanic acid, clindamycin, clobutinol, clonidine, cotrimoxazole, codeine, caffeine, vitamin D and derivatives of vitamin D, colestyramine, cromoglicic acid, coumarin and coumarin

15 derivatives, cysteine, cytarabine, cyclophosphamide, cyclosporin, cyproterone, cytabarine, dapiprazole, desogestrel, desonide, dihydralazine, diltiazem, ergot alkaloids, dimenhydrinate, dimethyl sulphoxide, dimeticone, domperidone and domperidan derivatives, dopamine, doxazosin, doxorubizin, doxylamine, dapiprazole, benzodiazepines, diclofenac, glycoside antibiotics, desipramine, econazole, ACE inhibitors, enalapril,

20 ephedrine, epinephrine, epoetin and epoetin derivatives, morphinans, calcium antagonists, irinotecan, modafinil, orlistat, peptide antibiotics, phenytoin, riluzoles, risedronate, sildenafil, topiramate, macrolide antibiotics, oestrogen and oestrogen derivatives, progestogen and progestogen derivatives, testosterone and testosterone derivatives, androgen and androgen derivatives, ethenzamide, etofenamate, etofibrate, fenofibrate,

25 etofylline, etoposide, famciclovir, famotidine, felodipine, fenofibrate, fentanyl, fenticonazole, gyrase inhibitors, fluconazole, fludarabine, fluarizine, fluorouracil, fluoxetine, flurbiprofen, ibuprofen, flutamide, fluvastatin, follitropin, formoterol, fosfomicin, furosemide, fusidic acid, gallopamil, ganciclovir, gemfibrozil, gentamicin, ginkgo, Saint John's wort, glibenclamide, urea derivatives as oral antidiabetics, glucagon,

30 glucosamine and glucosamine derivatives, glutathione, glycerol and glycerol derivatives, hypothalamus hormones, goserelin, gyrase inhibitors, guanethidine, halofantrine, haloperidol, heparin and heparin derivatives, hyaluronic acid, hydralazine, hydrochlorothiazide and hydrochlorothiazide derivatives, salicylates, hydroxyzine,

2006270221 15 Dec 2011

idarubicin, ifosfamide, imipramine, indometacin, indoramine, insulin, interferons, iodine
 and iodine derivatives, isoconazole, isoprenaline, glucitol and glucitol derivatives,
 itraconazole, ketoconazole, ketoprofen, ketotifen, lacidipine, lansoprazole, levodopa,
 levomethadone, thyroid hormones, lipoic acid and lipoic acid derivatives, lisinopril,
 5 lisuride, lofepramine, lomustine, loperamide, loratadine, maprotiline, mebendazole,
 mebeverine, meclozine, mefenamic acid, mefloquine, meloxicam, mepindolol,
 meprobamate, meropenem, mesalazine, mesuximide, metamizole, metformin,
 methotrexate, methylphenidate, methylprednisolone, metixene, metoclopramide,
 metoprolol, metronidazole, mianserin, miconazole, minocycline, minoxidil, misoprostol,
 10 mitomycin, mizolastine, moexipril, morphine and morphine derivatives, evening primrose,
 nalbuphine, naloxone, tilidine, naproxen, narcotine, natamycin, neostigmine, nicergoline,
 nicethamide, nifedipine, niflumic acid, nimodipine, nimorazole, nimustine, nisoldipine,
 adrenaline and adrenaline derivatives, norfloxacin, novamine sulfone, noscapine, nystatin,
 ofloxacin, olanzapine, olsalazine, omeprazole, omoconazole, ondansetron, oxaceprol,
 15 oxacillin, oxiconazole, oxymetazoline, pantoprazole, paracetamol, paroxetine, penciclovir,
 oral penicillins, pentazocine, pentifylline, pentoxifylline, perphenazine, pethidine, plant
 extracts, phenazone, pheniramine, barbituric acid derivatives, phenylbutazone, phenytoin,
 pimozide, pindolol, piperazine, piracetam, pirenzepine, piribedil, piroxicam, pramipexole,
 pravastatin, prazosin, procaine, promazine, propiverine, propranolol, propyphenazone,
 20 prostaglandins, protionamide, proxyphylline, quetiapine, quinapril, quinaprilat, ramipril,
 ranitidine, reproterol, reserpine, ribavirin, rifampicin, risperidone, ritonavir, ropinirole,
 roxatidine, roxithromycin, ruscogenin, rutoside and rutoside derivatives, sabadilla,
 salbutamol, salmeterol, scopolamine, selegiline, sertaconazole, sertindole, sertraline,
 silicates, sildenafil, simvastatin, sitosterol, sotalol, spaglumic acid, sparfloxacin,
 25 spectinomycin, spiramycin, spirapril, spironolactone, stavudine, streptomycin, sucralfate,
 sufentanil, sulbactam, sulphonamides, sulfasalazine, sulpiride, sultamicillin, sultiam,
 sumatriptan, suxamethonium chloride, tacrine, tacrolimus, taliolol, tamoxifen, taurolidine,
 tazarotene, temazepam, teniposide, tenoxicam, terazosin, terbinafine, terbutaline,
 terfenadine, tentertatolol, tetracyclins, teryzoline, theobromine, theophylline, butizine,
 30 thiamazole, phenothiazines, thiotepa, tiagabine, tiapride, propionic acid derivatives,
 ticlopidine, timolol, tinidazole, tioconazole, tioguanine, tioxolone, tiropamide, tizanidine,
 tolazoline, tolbutamide, tolcapone, tolinaftate, tolperisone, topotecan, torasemide,
 antioestrogens, tramadol, tramazoline, trandolapril, tranlycypromine, trapidil, trazodone,

2006270221 15 Dec 2011

triamcinolone and triamcinolone derivatives, triamterene, trifluoperidol, trifluridine, trimethoprim, trimipramine, tripeleminamine, triprolidine, trifosfamide, tromantadine, trometamol, tropalpin, troxerutine, tulobuterol, tyramine, tyrothricin, urapidil, ursodeoxycholic acid, chenodeoxycholic acid, valaciclovir, valproic acid, vancomycin, vecuronium chloride, Viagra, venlafaxine, verapamil, vidarabine, vigabatrin, vilazodone, vinblastine, vincamine, vincristine, vindesine, vinorelbine, vinpocetine, viquidil, warfarin, xantinol nicotinate, xipamide, zafirlukast, zalcitabine, zidovudine, zolmitriptan, zolpidem, zopiclone, and zotipine.

- 10 26. The device of claim 3, or the coated vascular stent of any one of claims 11 to 13, wherein said polymer is selected from poly(alkyl methacrylates) such as poly(methyl methacrylate) and poly(butyl methacrylate) (PBMA), polyethylene-co-vinyl acetate (PEVA), Polyethylene, polybutylene and polybutylene copolymers, Polyurethanes, polyanhydrides, Aliphatic polycarbonates, poly(3-hydroxybutyrate) and other
- 15 poly(hydroxyalkanoate)s, poly(alkyl siloxane)s such as Poly(dimethyl siloxane) (PDMS) and other silicone polymers, aliphatic polyesters, Polyglycolide (PGA), Polylactide (PLA) Poly(lactide-co-glycolide) (PLGA), Poly(ϵ -caprolactone) (PCL), Polytetrafluoroethylene, (PTFE) and PTFE copolymers, polystyrene and polystyrene copolymers, and poly(phosphazenes).

20

27. The method of either claim 1 or claim 2, the device of claim 3, or the stent of any one of claims 11 to 13, substantially as hereinbefore described.

1/31

Rapid Expansion of Supercritical Solutions (RESS) Process Equipment

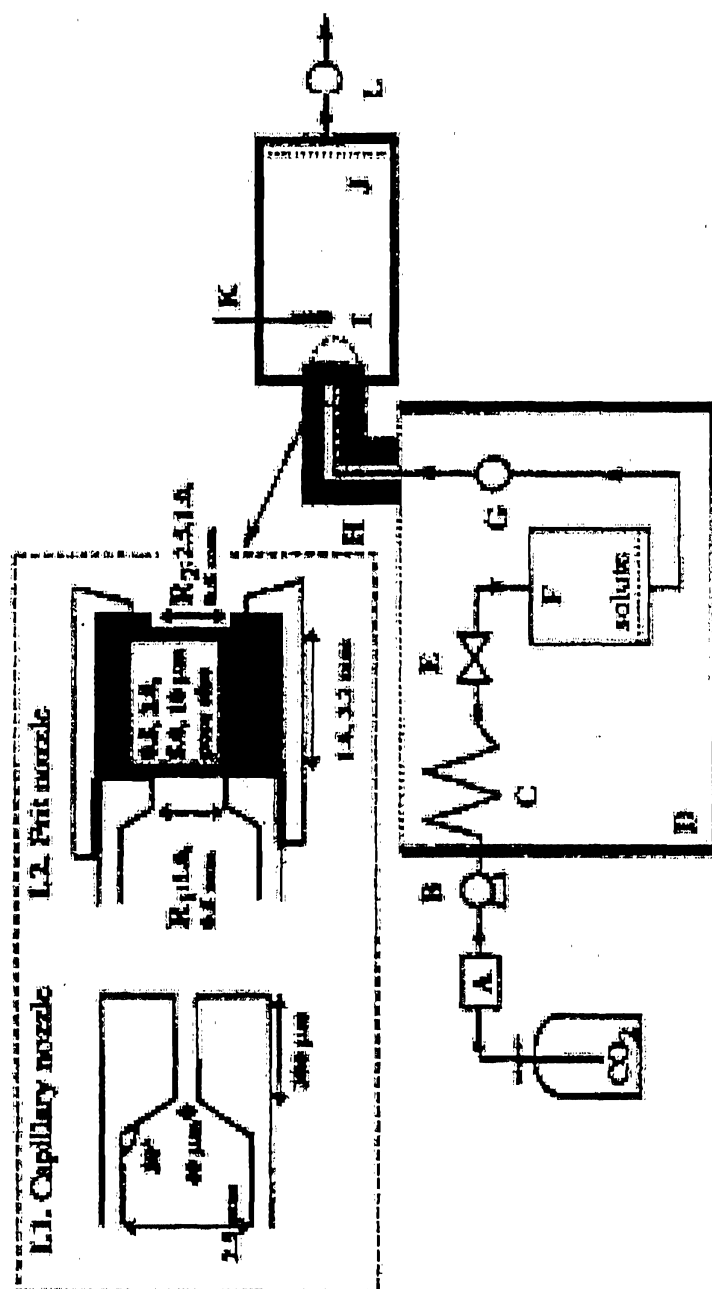


FIGURE 1

Solution Enhanced Dispersion of Supercritical Solutions (SEDS) Process Equipment

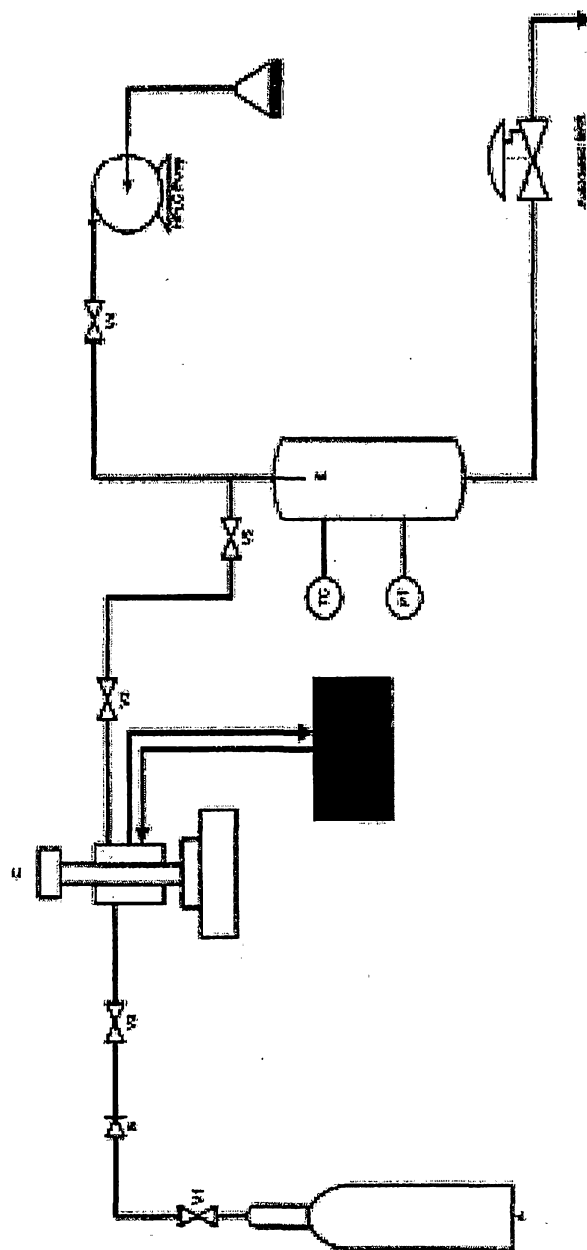


FIGURE 2

3/31

SEDS nozzle design

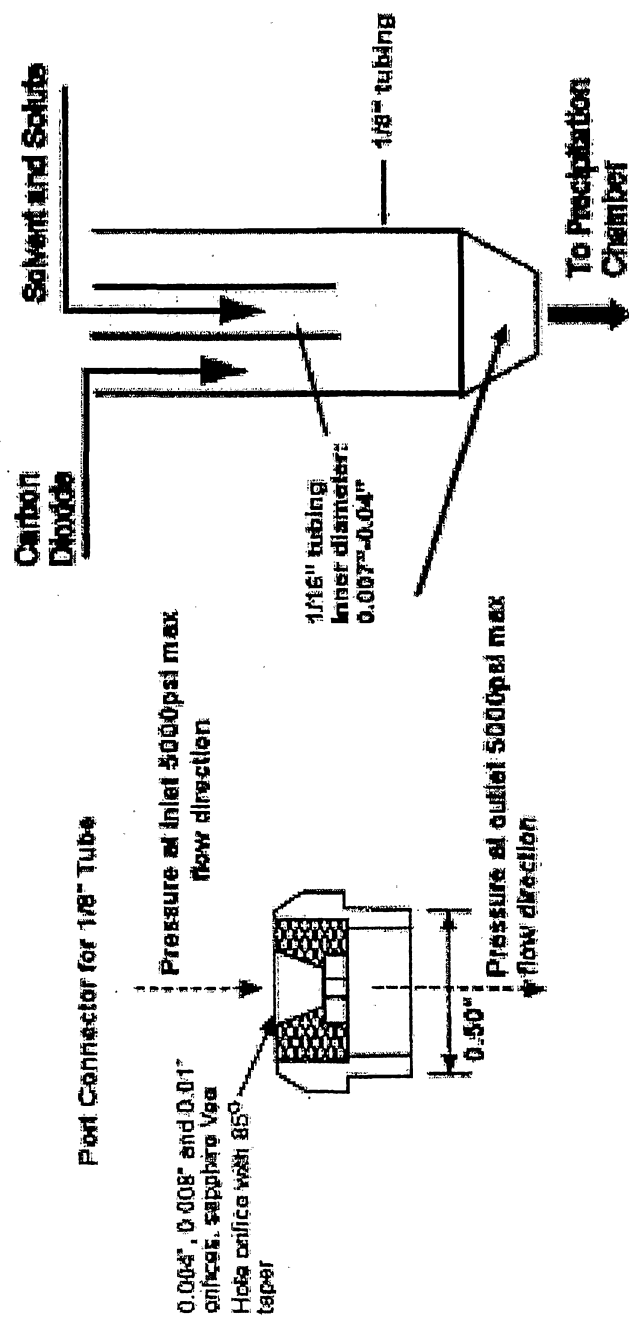


FIGURE 3

FTIR spectra of each component and
the spray coating mixture


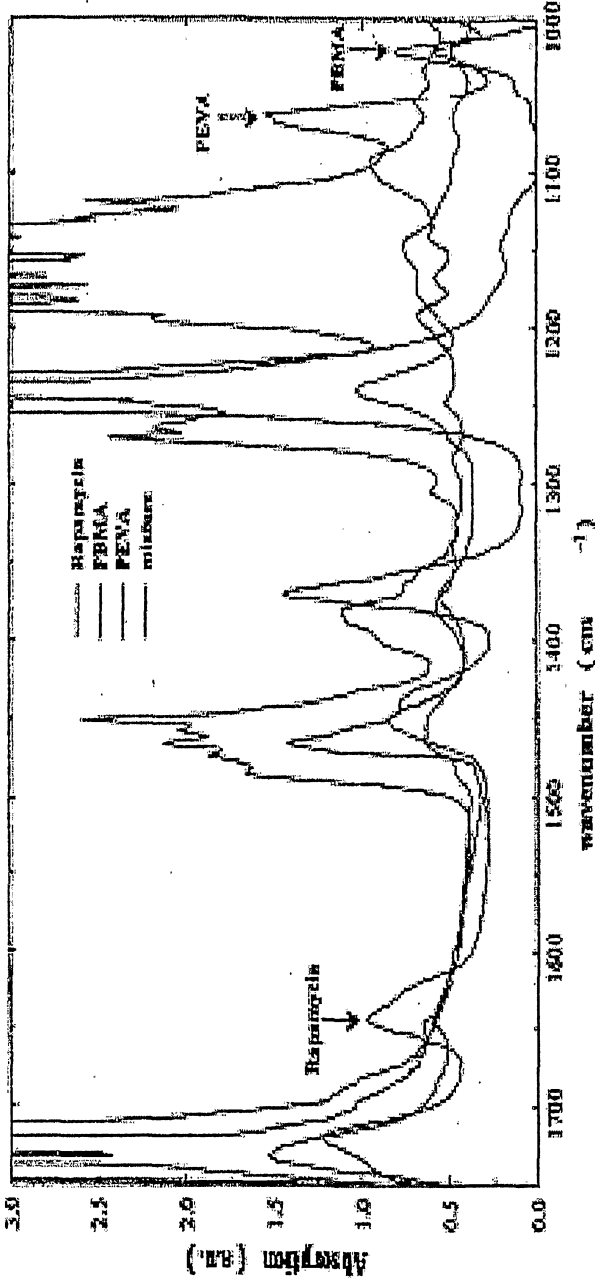


FIGURE 4

Stents coated with
Rapamycin, PEVA and PBMA (approx. 1:1:1)
No attempt was made to control morphology



(a) before sintering

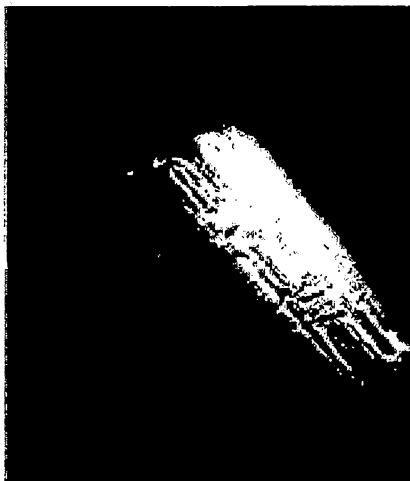

(b) after sintering



5/31

FIGURE 5

6/31

IR spectra of Si wafer chips coated with
Rapamycin, PEVA and PBMA

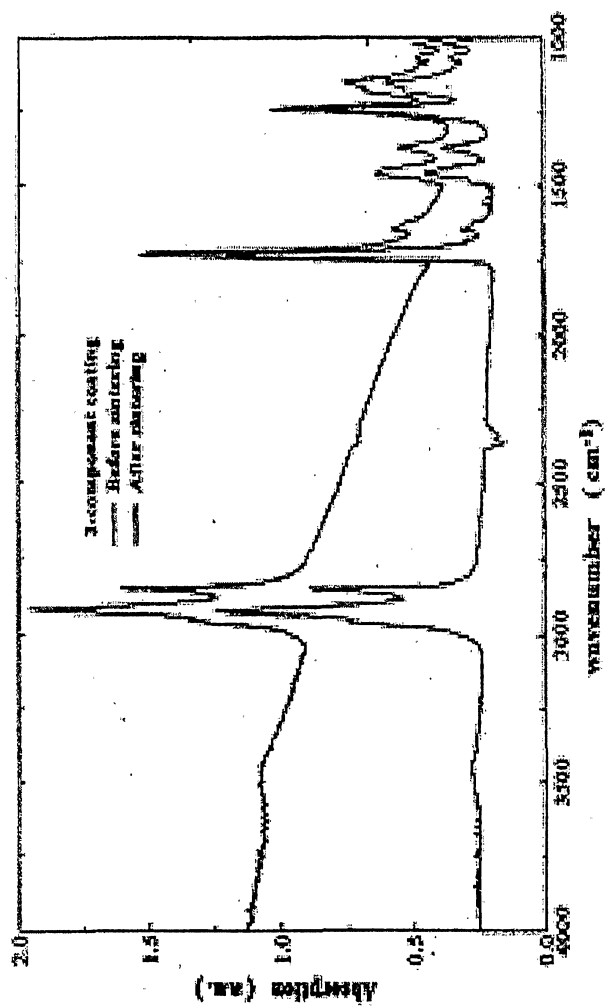


FIGURE 6

7/31

Crystalline spray-coated rapamycin

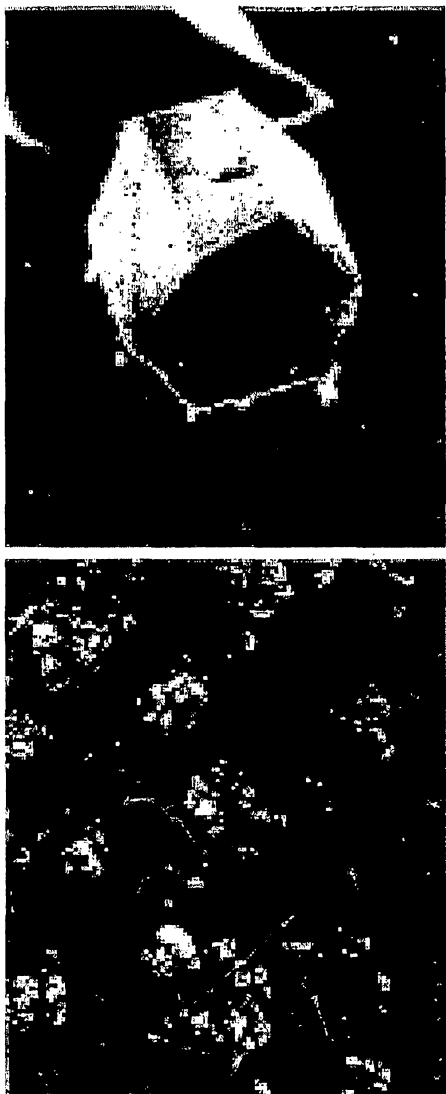


FIGURE 7

8/31

XRD spectra of rapamycin in Various Morphologies


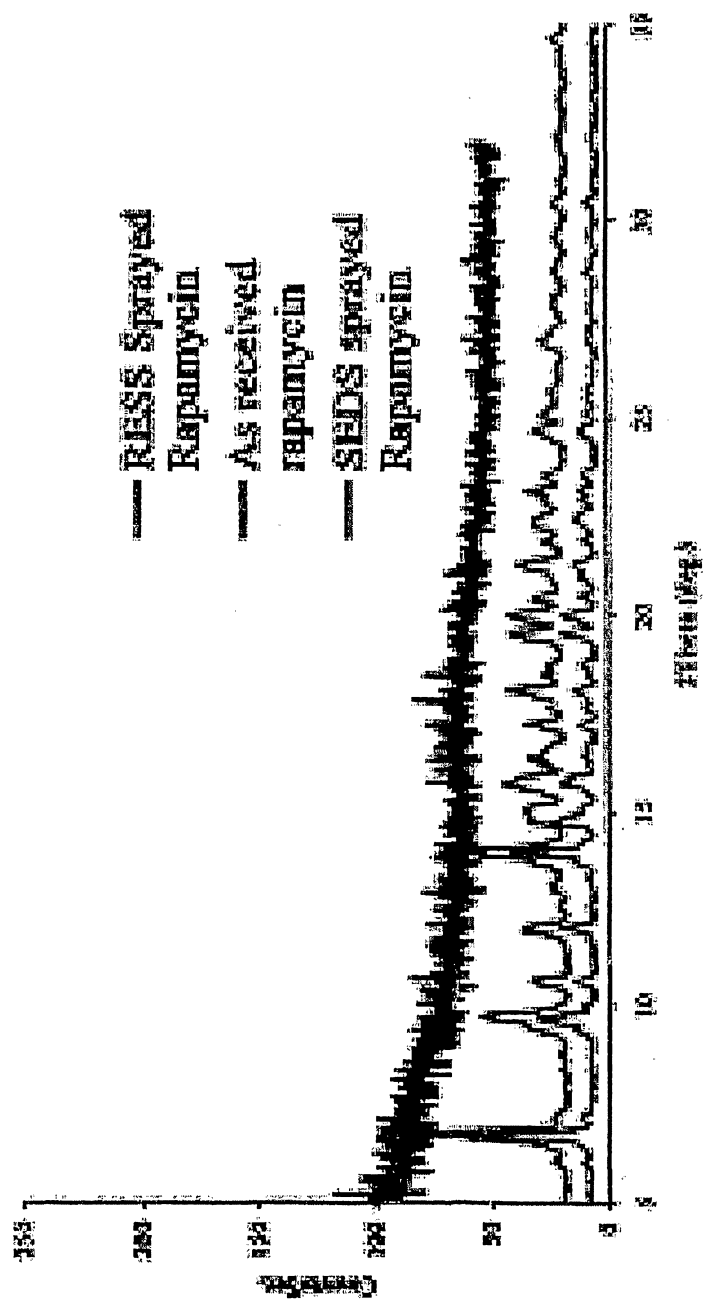


FIGURE 8

9/31

Optical and Electron Microscope Comparison of SEDS spraying process under different pressure conditions

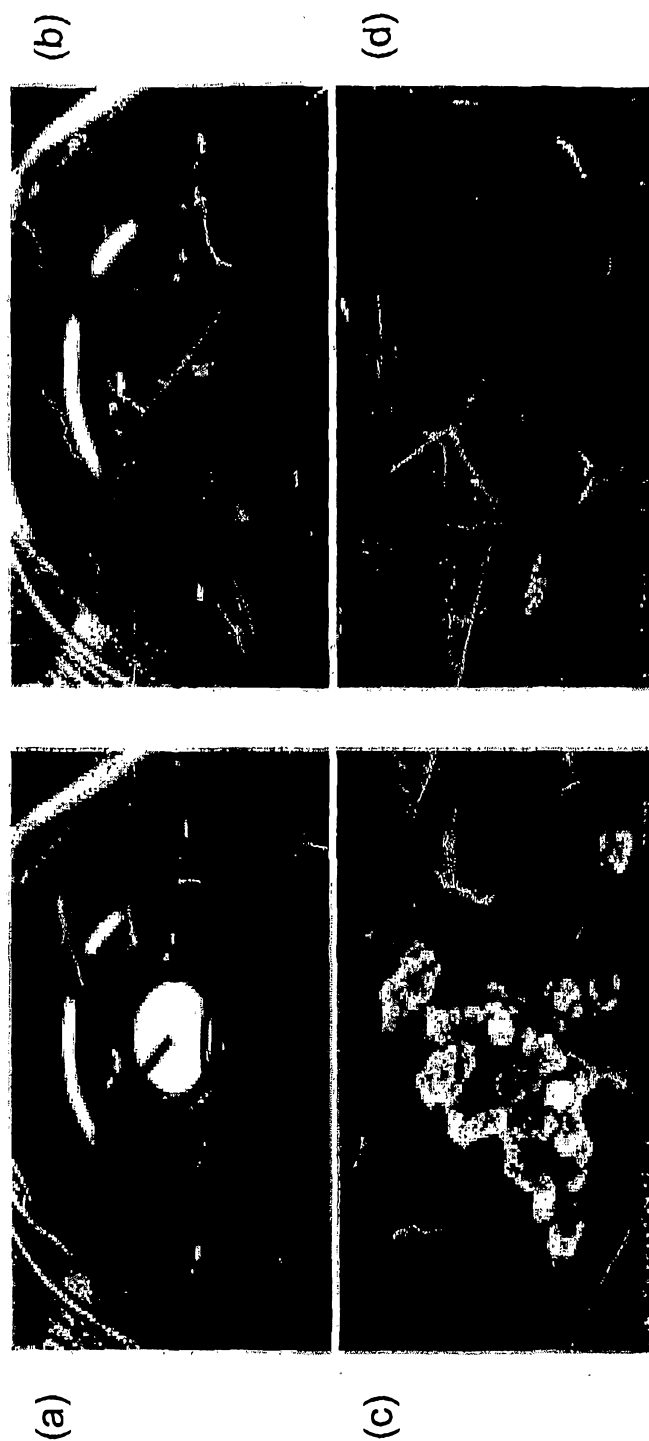

(a) Optical image of view cell. CO₂ at 1200psi, 25°C
(b) Optical image of view cell. CO₂ at 2500psi, 25°C
(c) SEM image of substrate from view cell in (a)
(d) SEM image of substrate from view cell in (b)

FIGURE 9

Crystalline Rapamycin Spray Apparatus

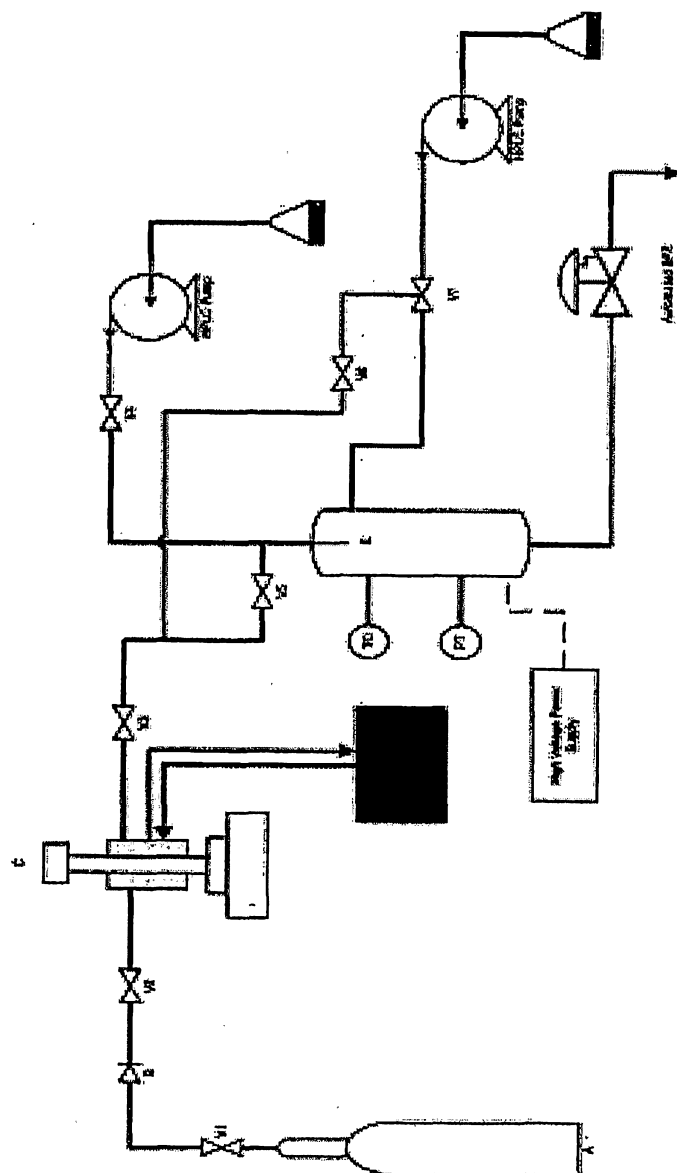


FIGURE 10

11/31

Cloud point isotherms for polyethylene-co-vinyl acetate (PEVA) and poly(butyl methacrylate) (PBMA) combined

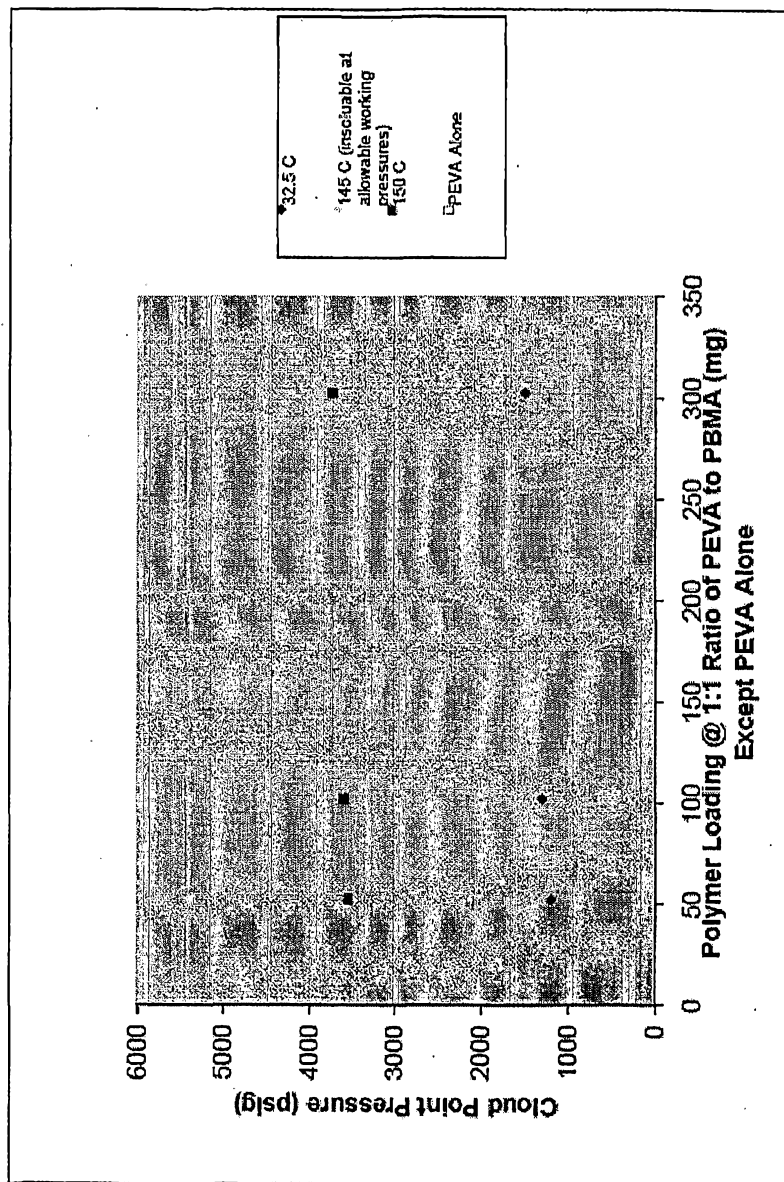


FIGURE 11

12/31

Schematic Representing the Coating and Sintering Process Apparatus

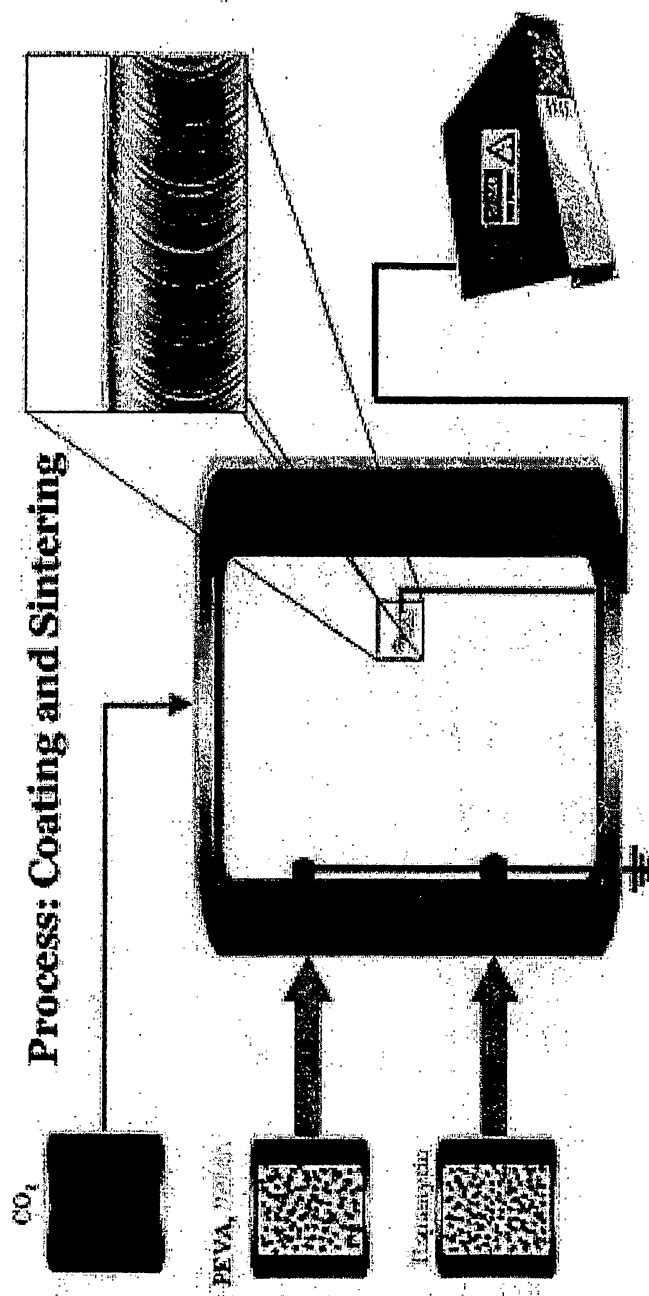


FIGURE 12

Coating and Sintering Process Apparatus



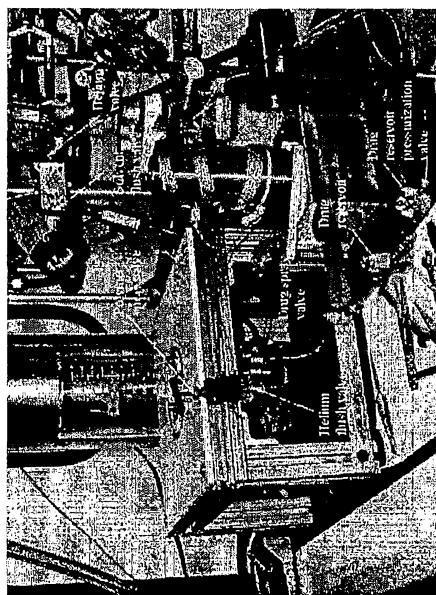


FIGURE 13

14/31

Drug-Polymer coated coronary stent

(a) immediately after deposition,

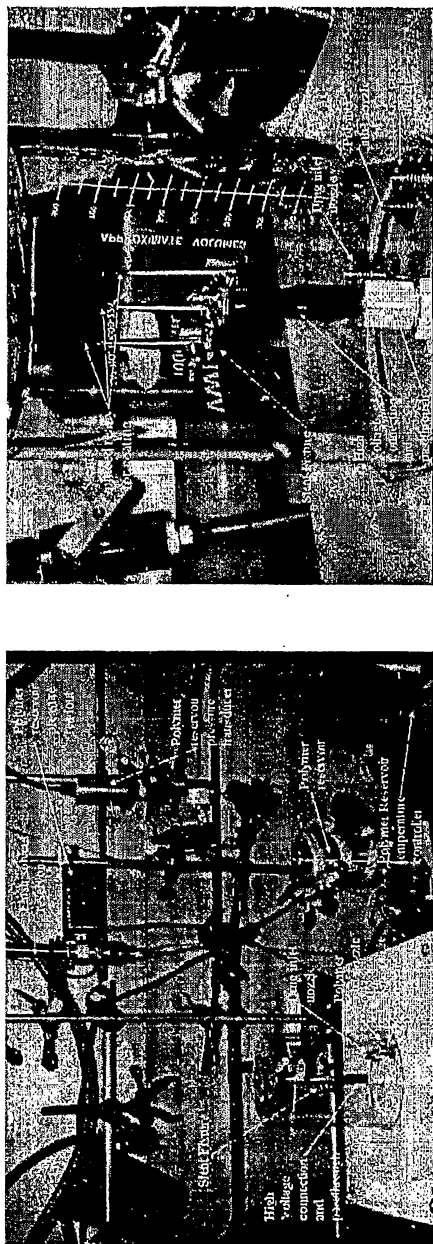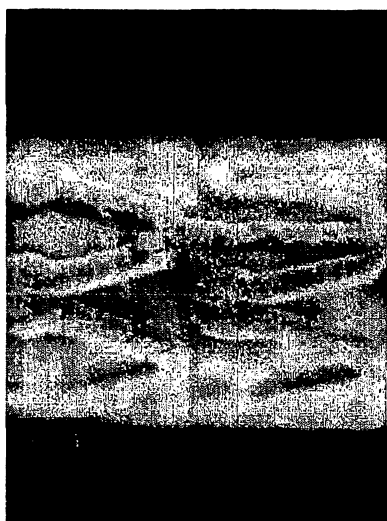

(b) after annealing in a dense carbon dioxide environment at 40°C

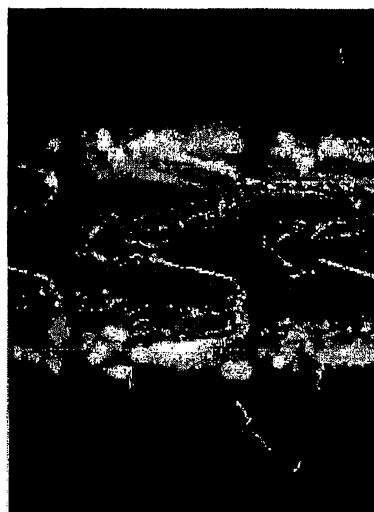


FIGURE 14

Optical Microscopy of Rapamycin/PEVA/PBMA Coated Stents

(a) Powder coated before sintering



Outside Surface




Edge Surface




Inside Surface


(b) Powder coated after sintering

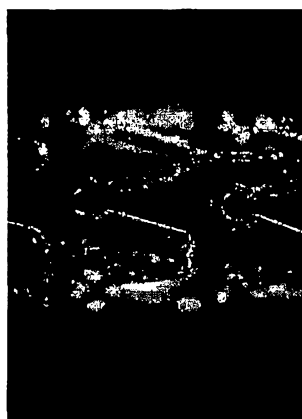

Outside Surface

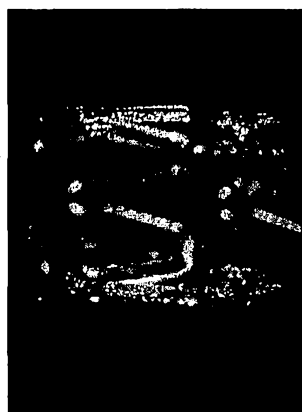

Edge Surface

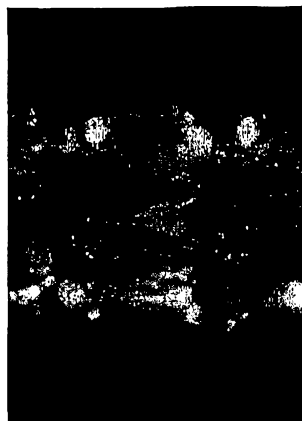

Inside Surface

Optical Microscopy of Rapamycin/PEVA/PBMA Coated Stents

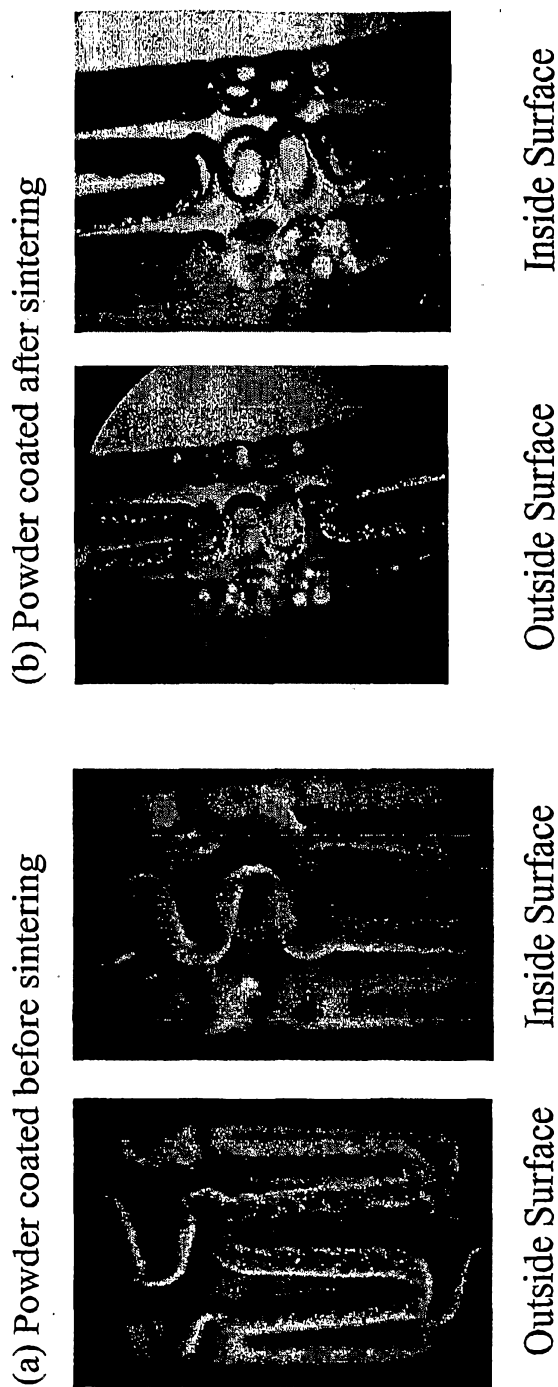


FIGURE 16

Optical Microscopy of Rapamycin/PEVA/PBMA Coated
Stents After Sintering at 100X magnification



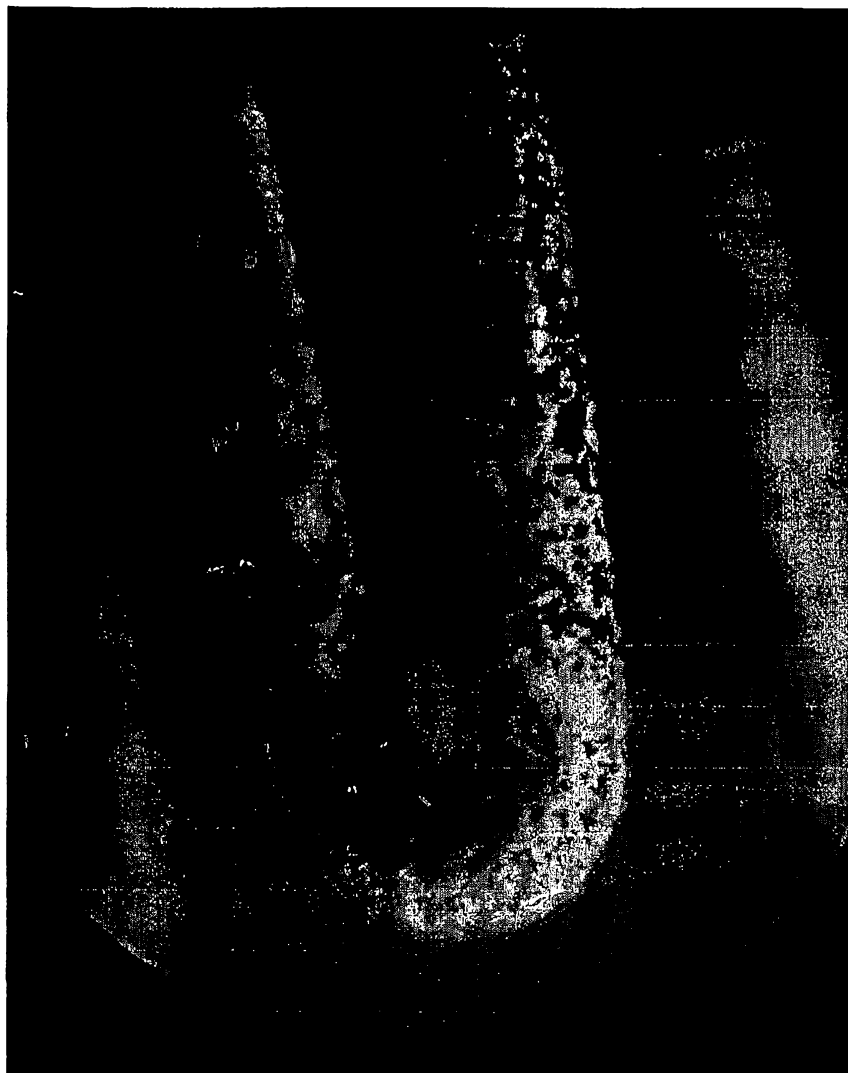


FIGURE 17


Scanning Electron Microscope Images of Rapamycin/PEVA/PBMA Coated Stents

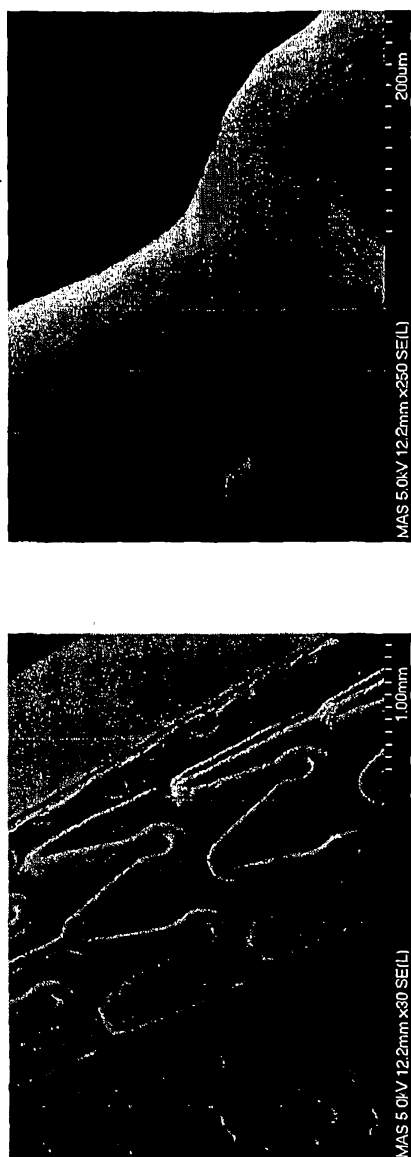


(a) x30 magnification

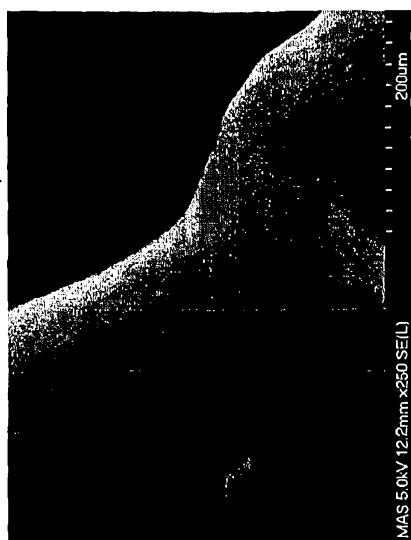

(b) x250 magnification

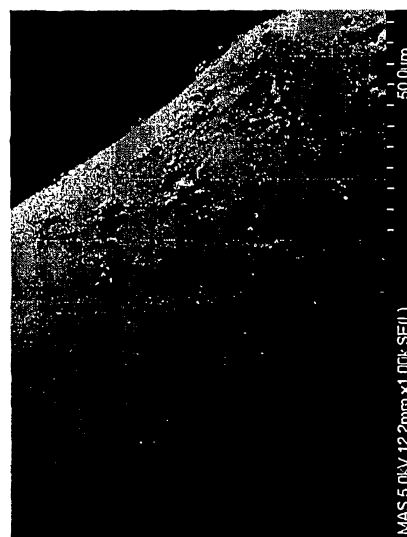


(c) x1000 magnification

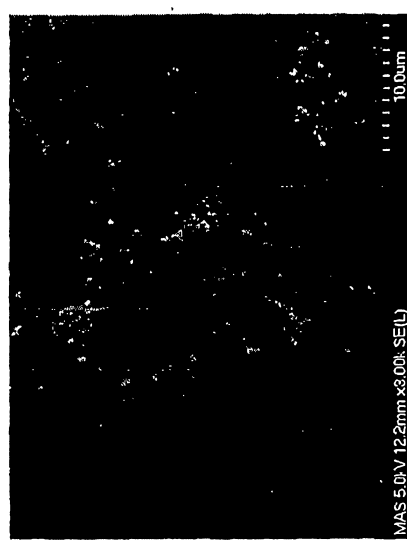

(d) x3000 magnification

FIGURE 18

Scanning Electron Microscope Images of Rapamycin/PEVA/PBMA Coated Stent (FIB Cross-sections)

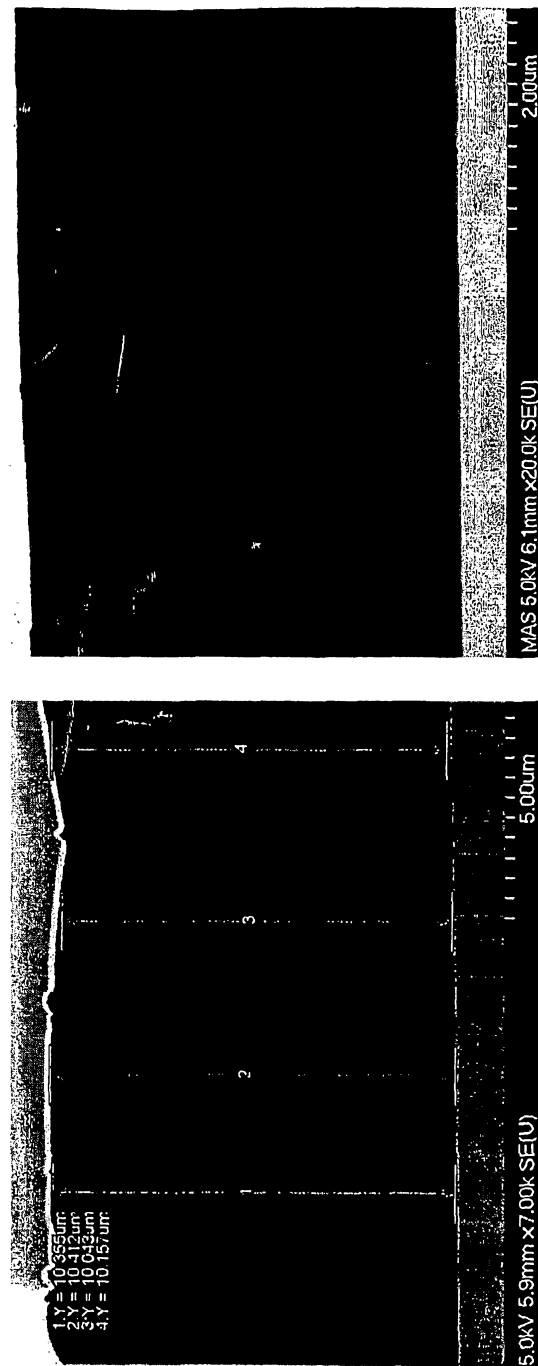

(a) x7000 magnification

(b) x20000 magnification

Four cross-sectional thicknesses measured:

- (1) 10.355 μ M; (2) 10.412 μ M; (3) 10.043 μ M; (4) 10.157 μ M

FIGURE 19

Differential Scanning Calorimetry Analysis of Rapamycin/PEVA/PBMA Coated Stents


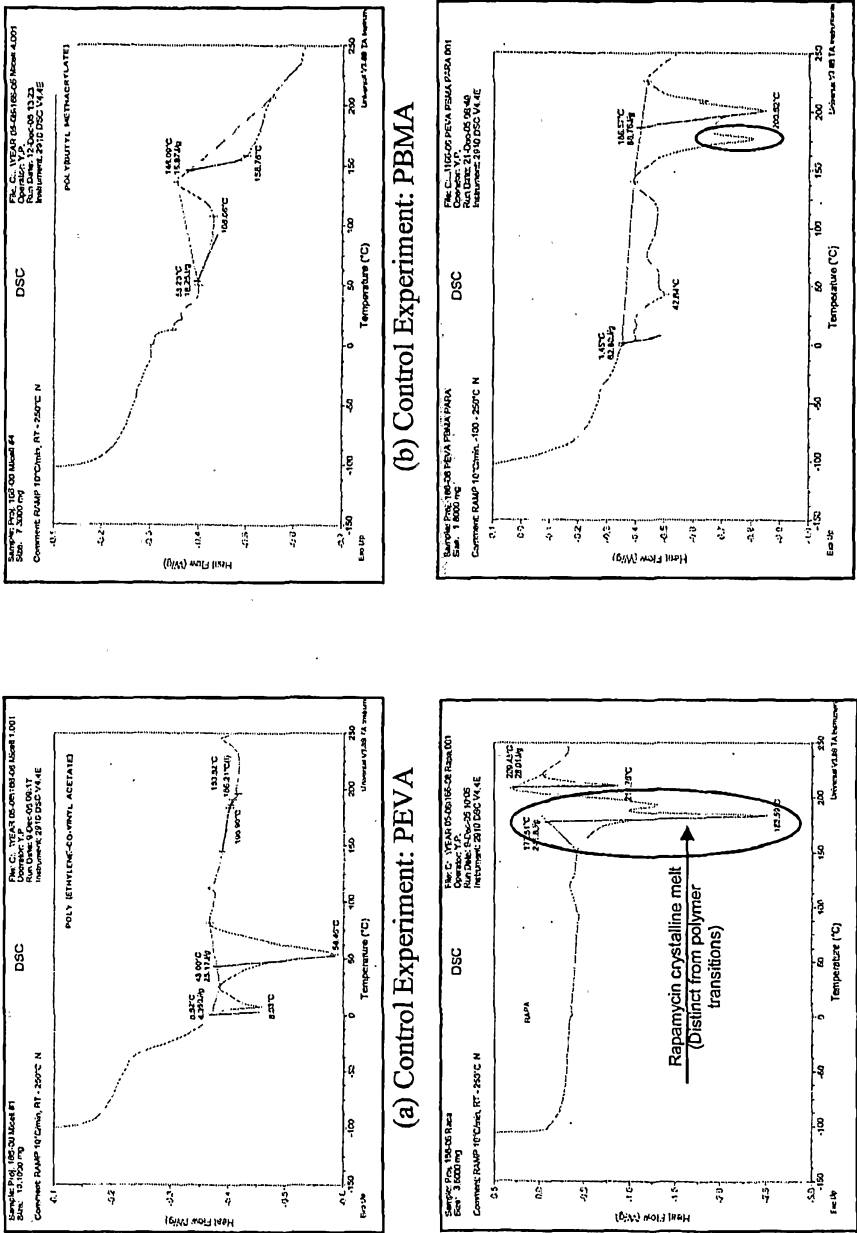



FIGURE 20

21/31

X-Ray Diffraction Analysis of Rapamycin/PEVA/PBMA Coated Stents

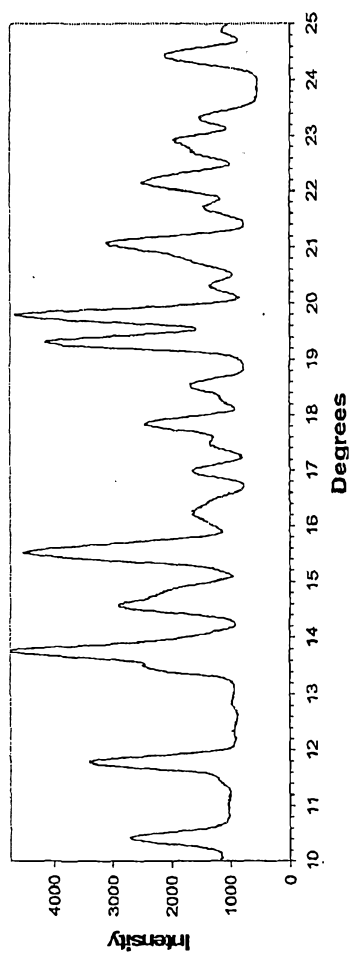


(a) AR Microionized Rapamycin Powder (Control)

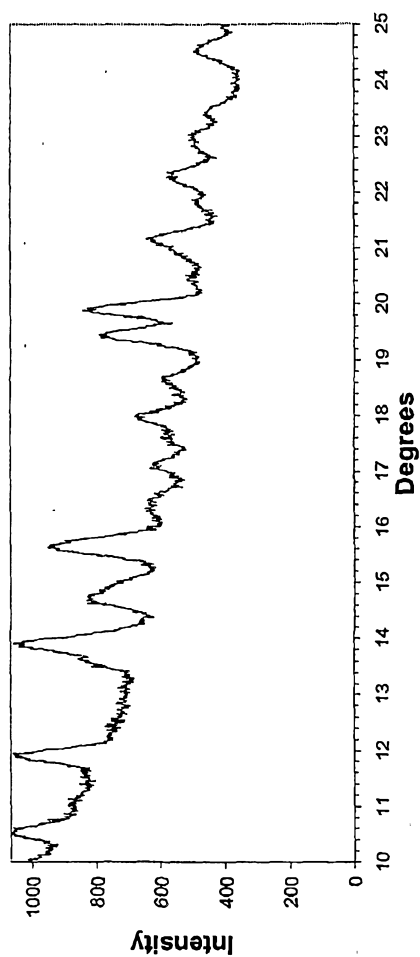

(b) Sintered Coated PEVA+PBMA+Rapamycin

FIGURE 21

Confocal Raman Analysis of Rapamycin/PEVA/PBMA Coated Stents (Depth profiling from Coating Surface to Metal Stent)

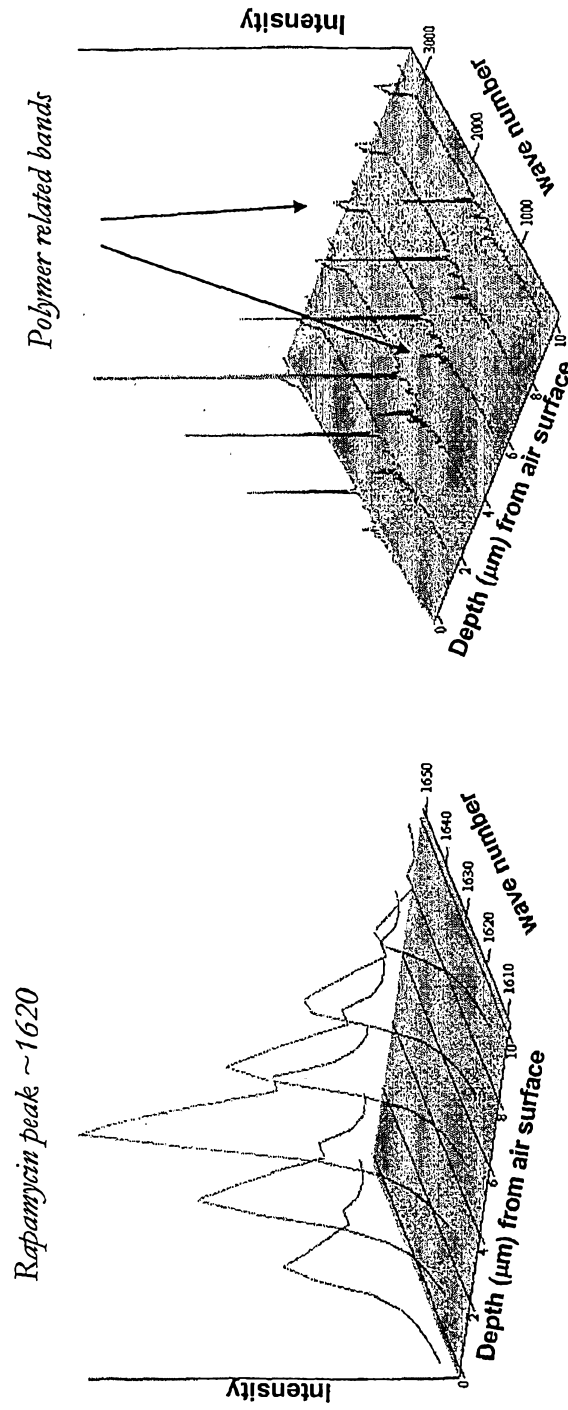


(a) Rapamycin Depth Profile Outside Circumference

(b) Polymer Depth Profile Outside Circumference

FIGURE 22

FT-IR and UV-Vis Spectrum & Calibration Curves of Rapamycin and PEVA/PBMA

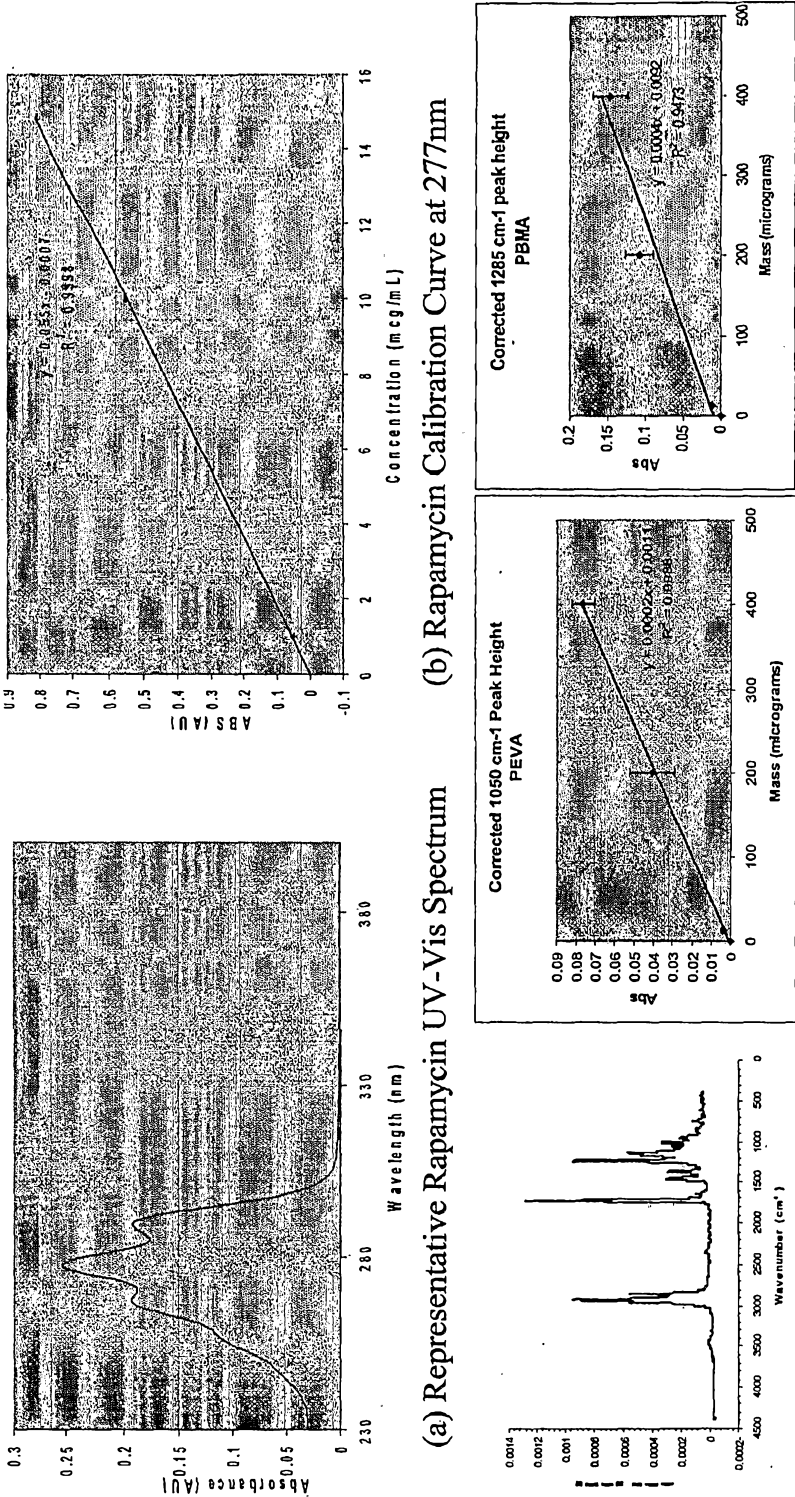

(c) Representative PEVA/PBMA FT-IR Spectrum

(d) PEVA Calibration Curve at 1050nm

(e) PBMA Calibration Curve at 1285nm

FIGURE 23

UV-Vis & FT-IR Quantification of Rapamycin, PEVA and PBMA Coating Components;
mean concentrations (3 stents each); 4 cell by 8mm parylene coated


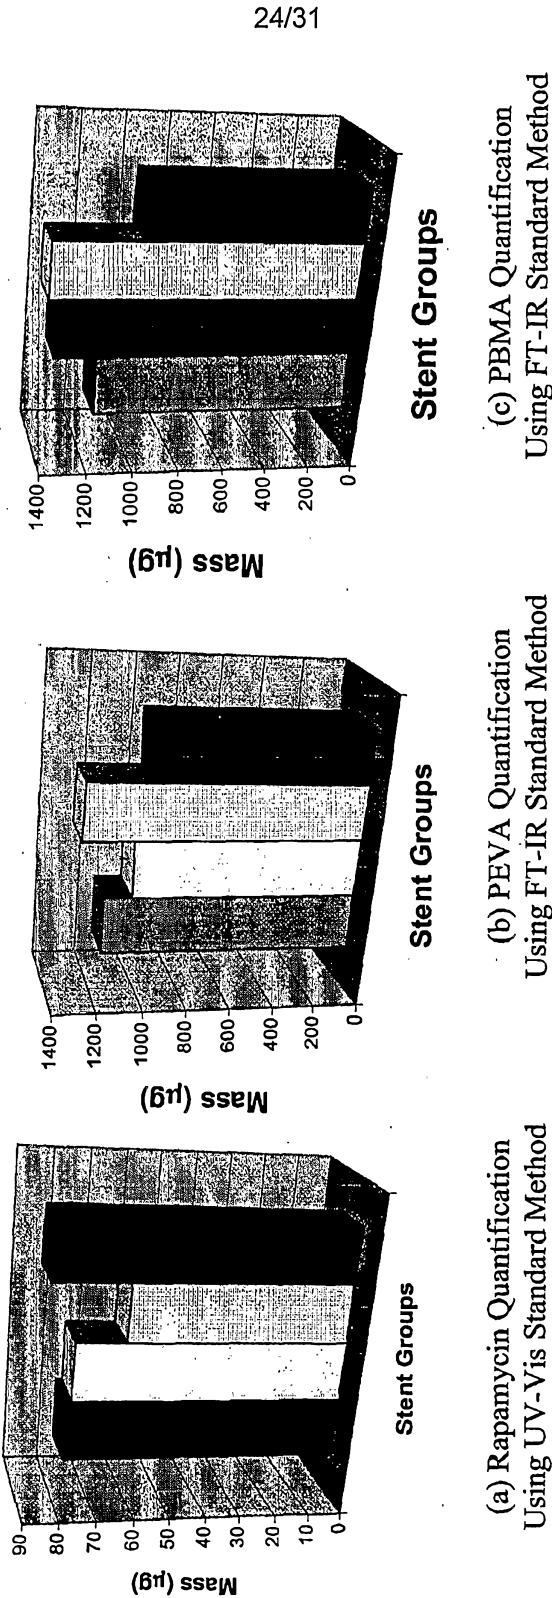


FIGURE 24

25/31

Optical Microscopy Showing the Outside Surface of
Paclitaxel-polymer Coated 3mm Guidant TriStar® Stent

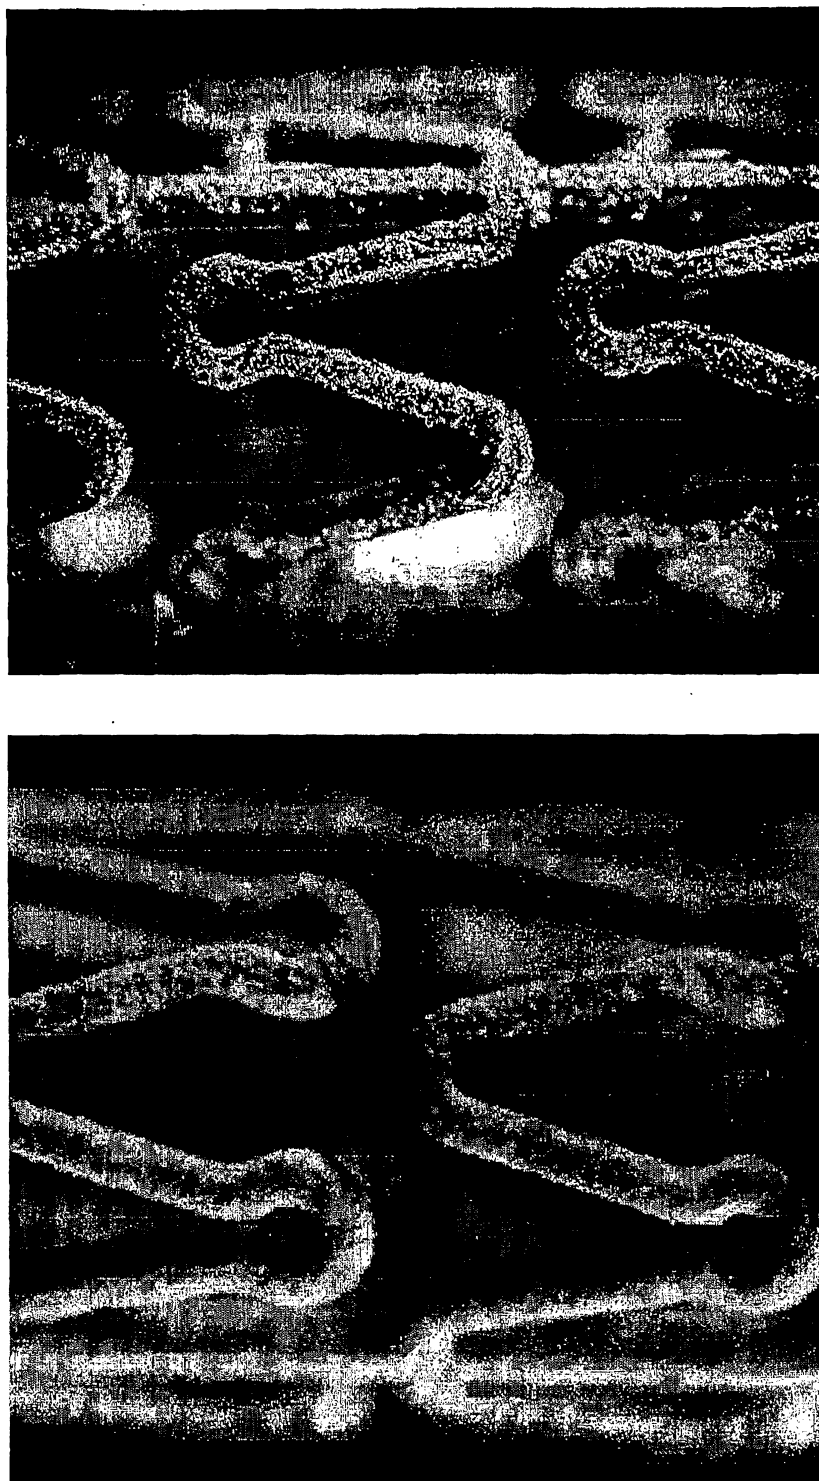


(a) before sintering

(b) after sintering

FIGURE 25

Quantification of Paclitaxel After Coating on a 3mm Guidant TriStar® Stent with Paclitaxel-polymer composite

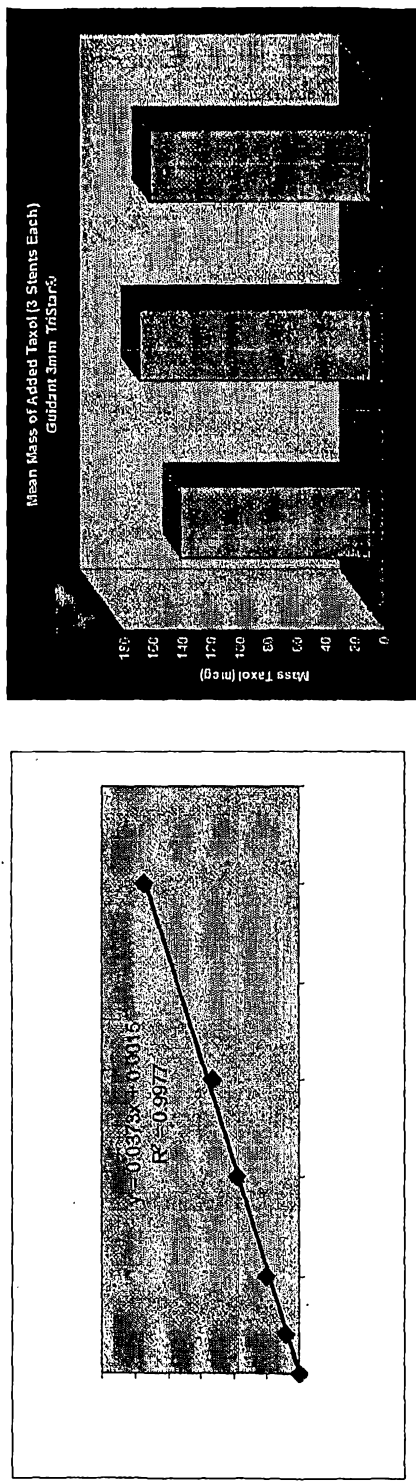

(a) Paclitaxel UV-Vis calibration curve

(b) Paclitaxel Quantification
Using UV-Vis Standard Method

FIGURE 26

UV-Vis & FT-IR Quantification of Rapamycin, PEVA and PBMA Coating Components; mean concentrations (3 stents each); 6 cell by 8mm parylene coated

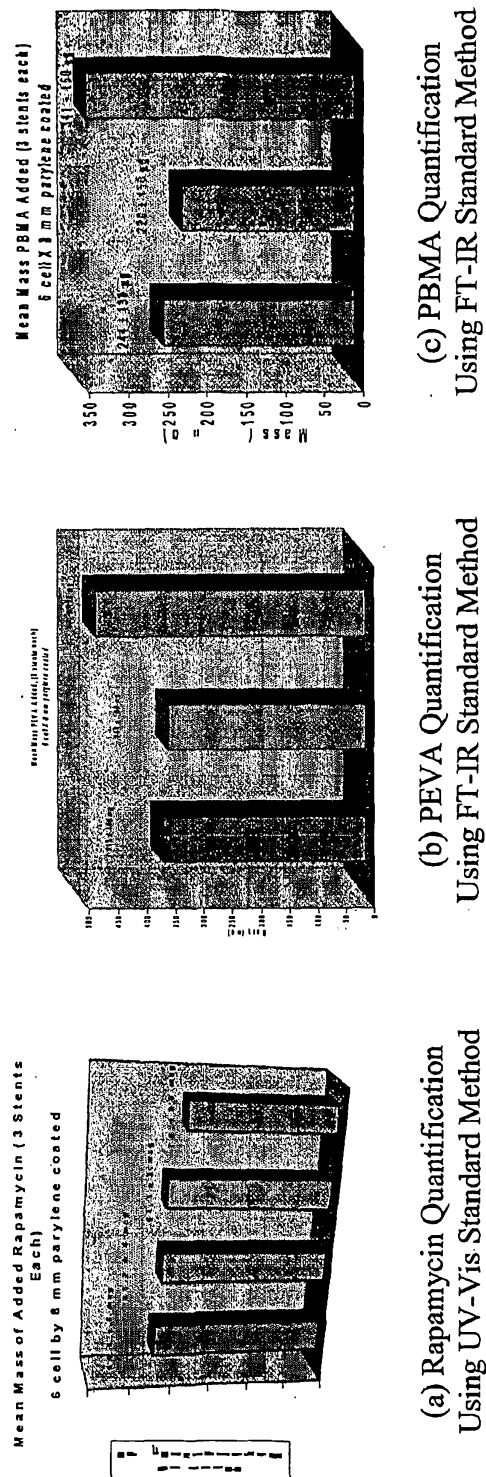


FIGURE 27

28/31

**Polymer Drug Polymer Coated on Stents and Coupons
Total PEVA & PBMA with 15 mg Rapamycin Shot
4 Hour Sintering**

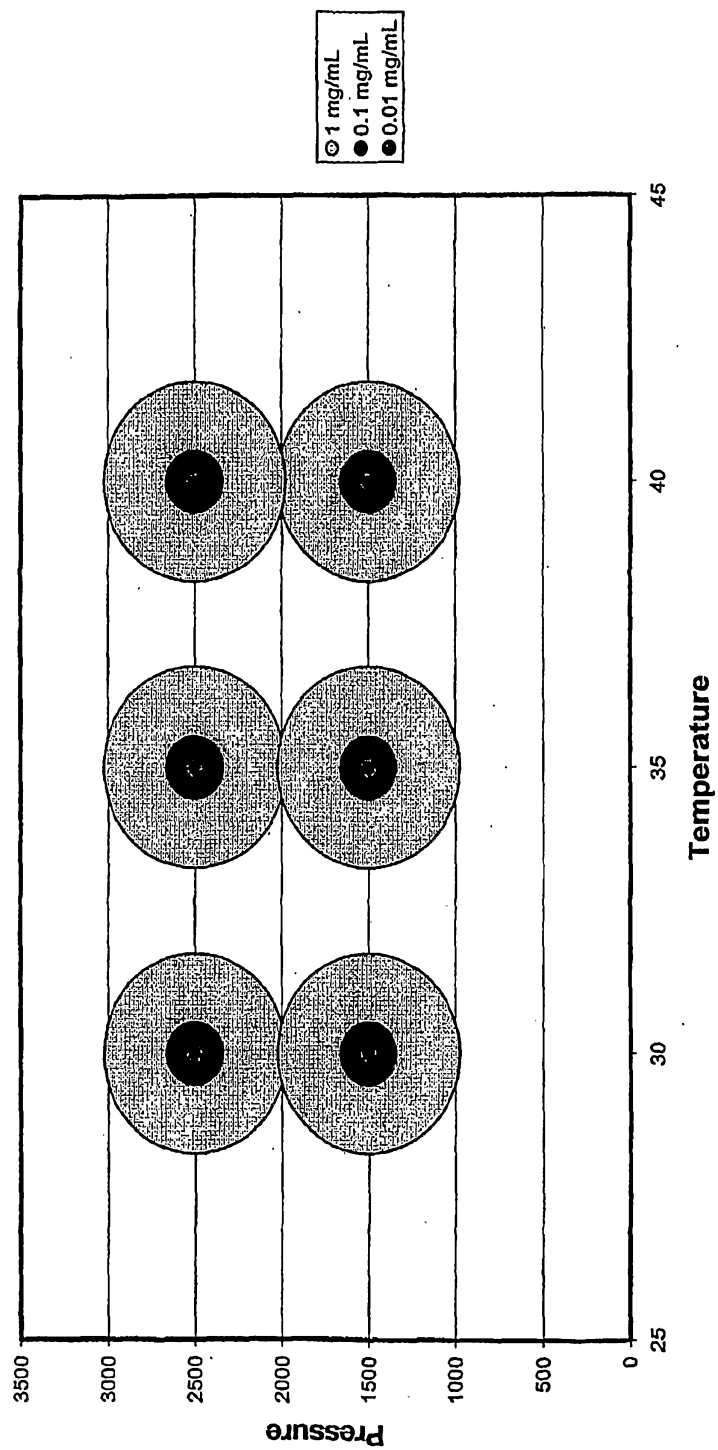


Figure 2. Graphical summary of the conditions used for the sintering experiments.

FIGURE 28

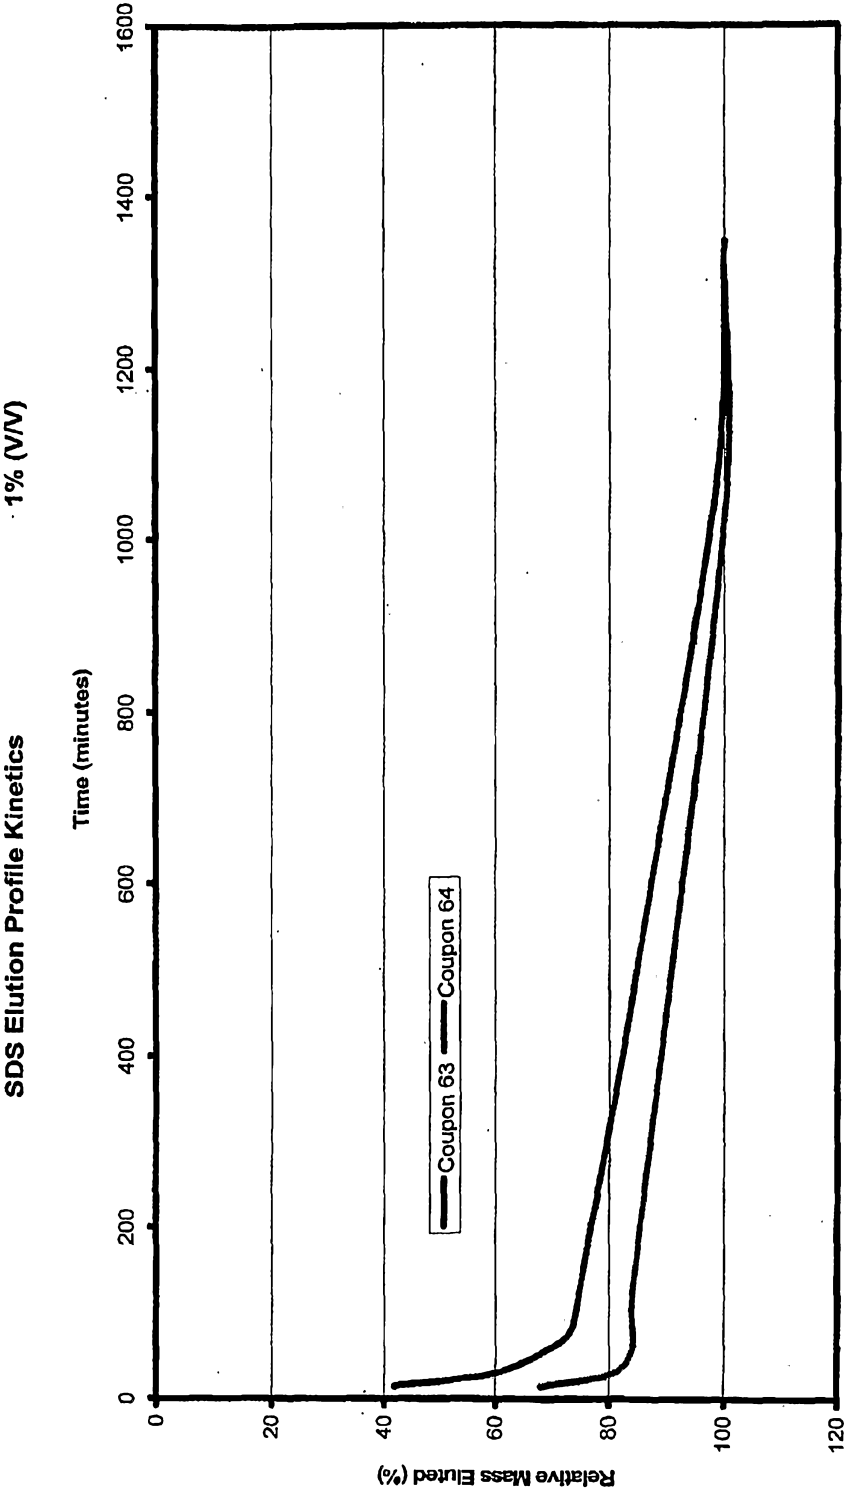


FIGURE 29


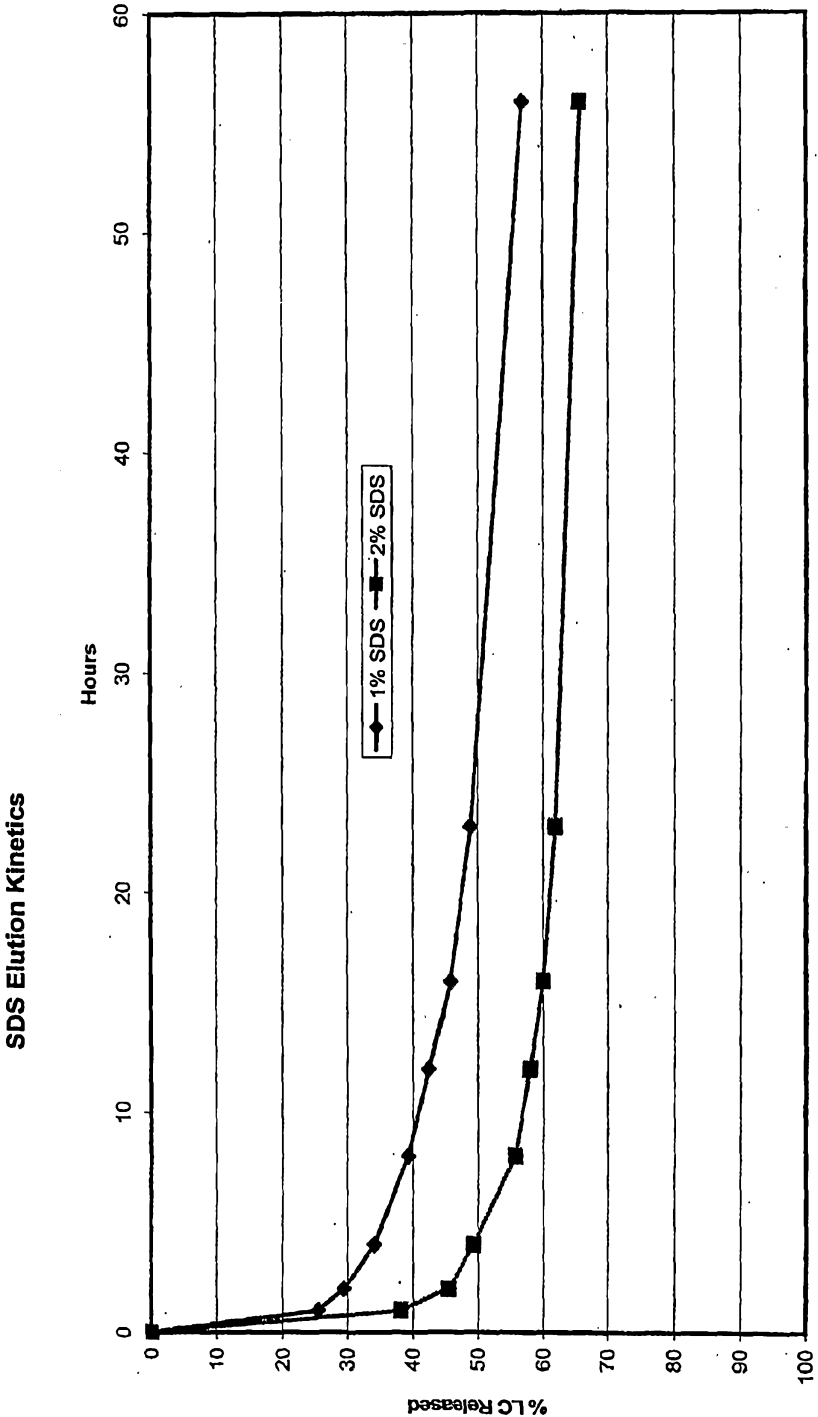


FIGURE 30

31/31

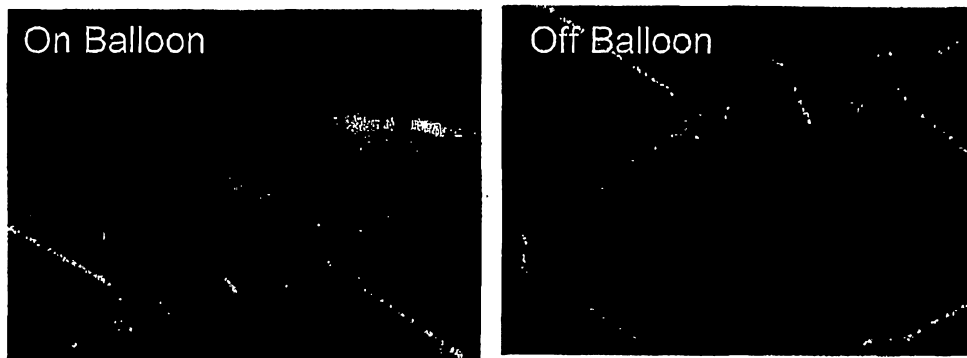

Stents exhibiting mechanically sound coating after inflation

FIGURE 31