




(86) Date de dépôt PCT/PCT Filing Date: 1997/06/10
(87) Date publication PCT/PCT Publication Date: 1998/12/10
(45) Date de délivrance/Issue Date: 2004/08/31
(85) Entrée phase nationale/National Entry: 1999/11/17
(86) N° demande PCT/PCT Application No.: US 1997/009768
(87) N° publication PCT/PCT Publication No.: 1998/055055
(30) Priorité/Priority: 1997/06/02 (08/867,294) US

(51) Cl.Int.⁷/Int.Cl.⁷ A61F 2/80
(72) Inventeur/Inventor:
CASPERS, CARL A., US
(73) Propriétaire/Owner:
OTTO BOCK HEALTHCARE LP, US
(74) Agent: OGILVY RENAULT

(54) Titre : MEMBRE ARTIFICIEL A REGULATION HYPOBARE, A DOUBLE EMBOITURE ET VERROUILLAGE
MECANIQUE

(54) Title: HYPOBARICALLY-CONTROLLED, DOUBLE-SOCKET ARTIFICIAL LIMB WITH MECHANICAL INTERLOCK

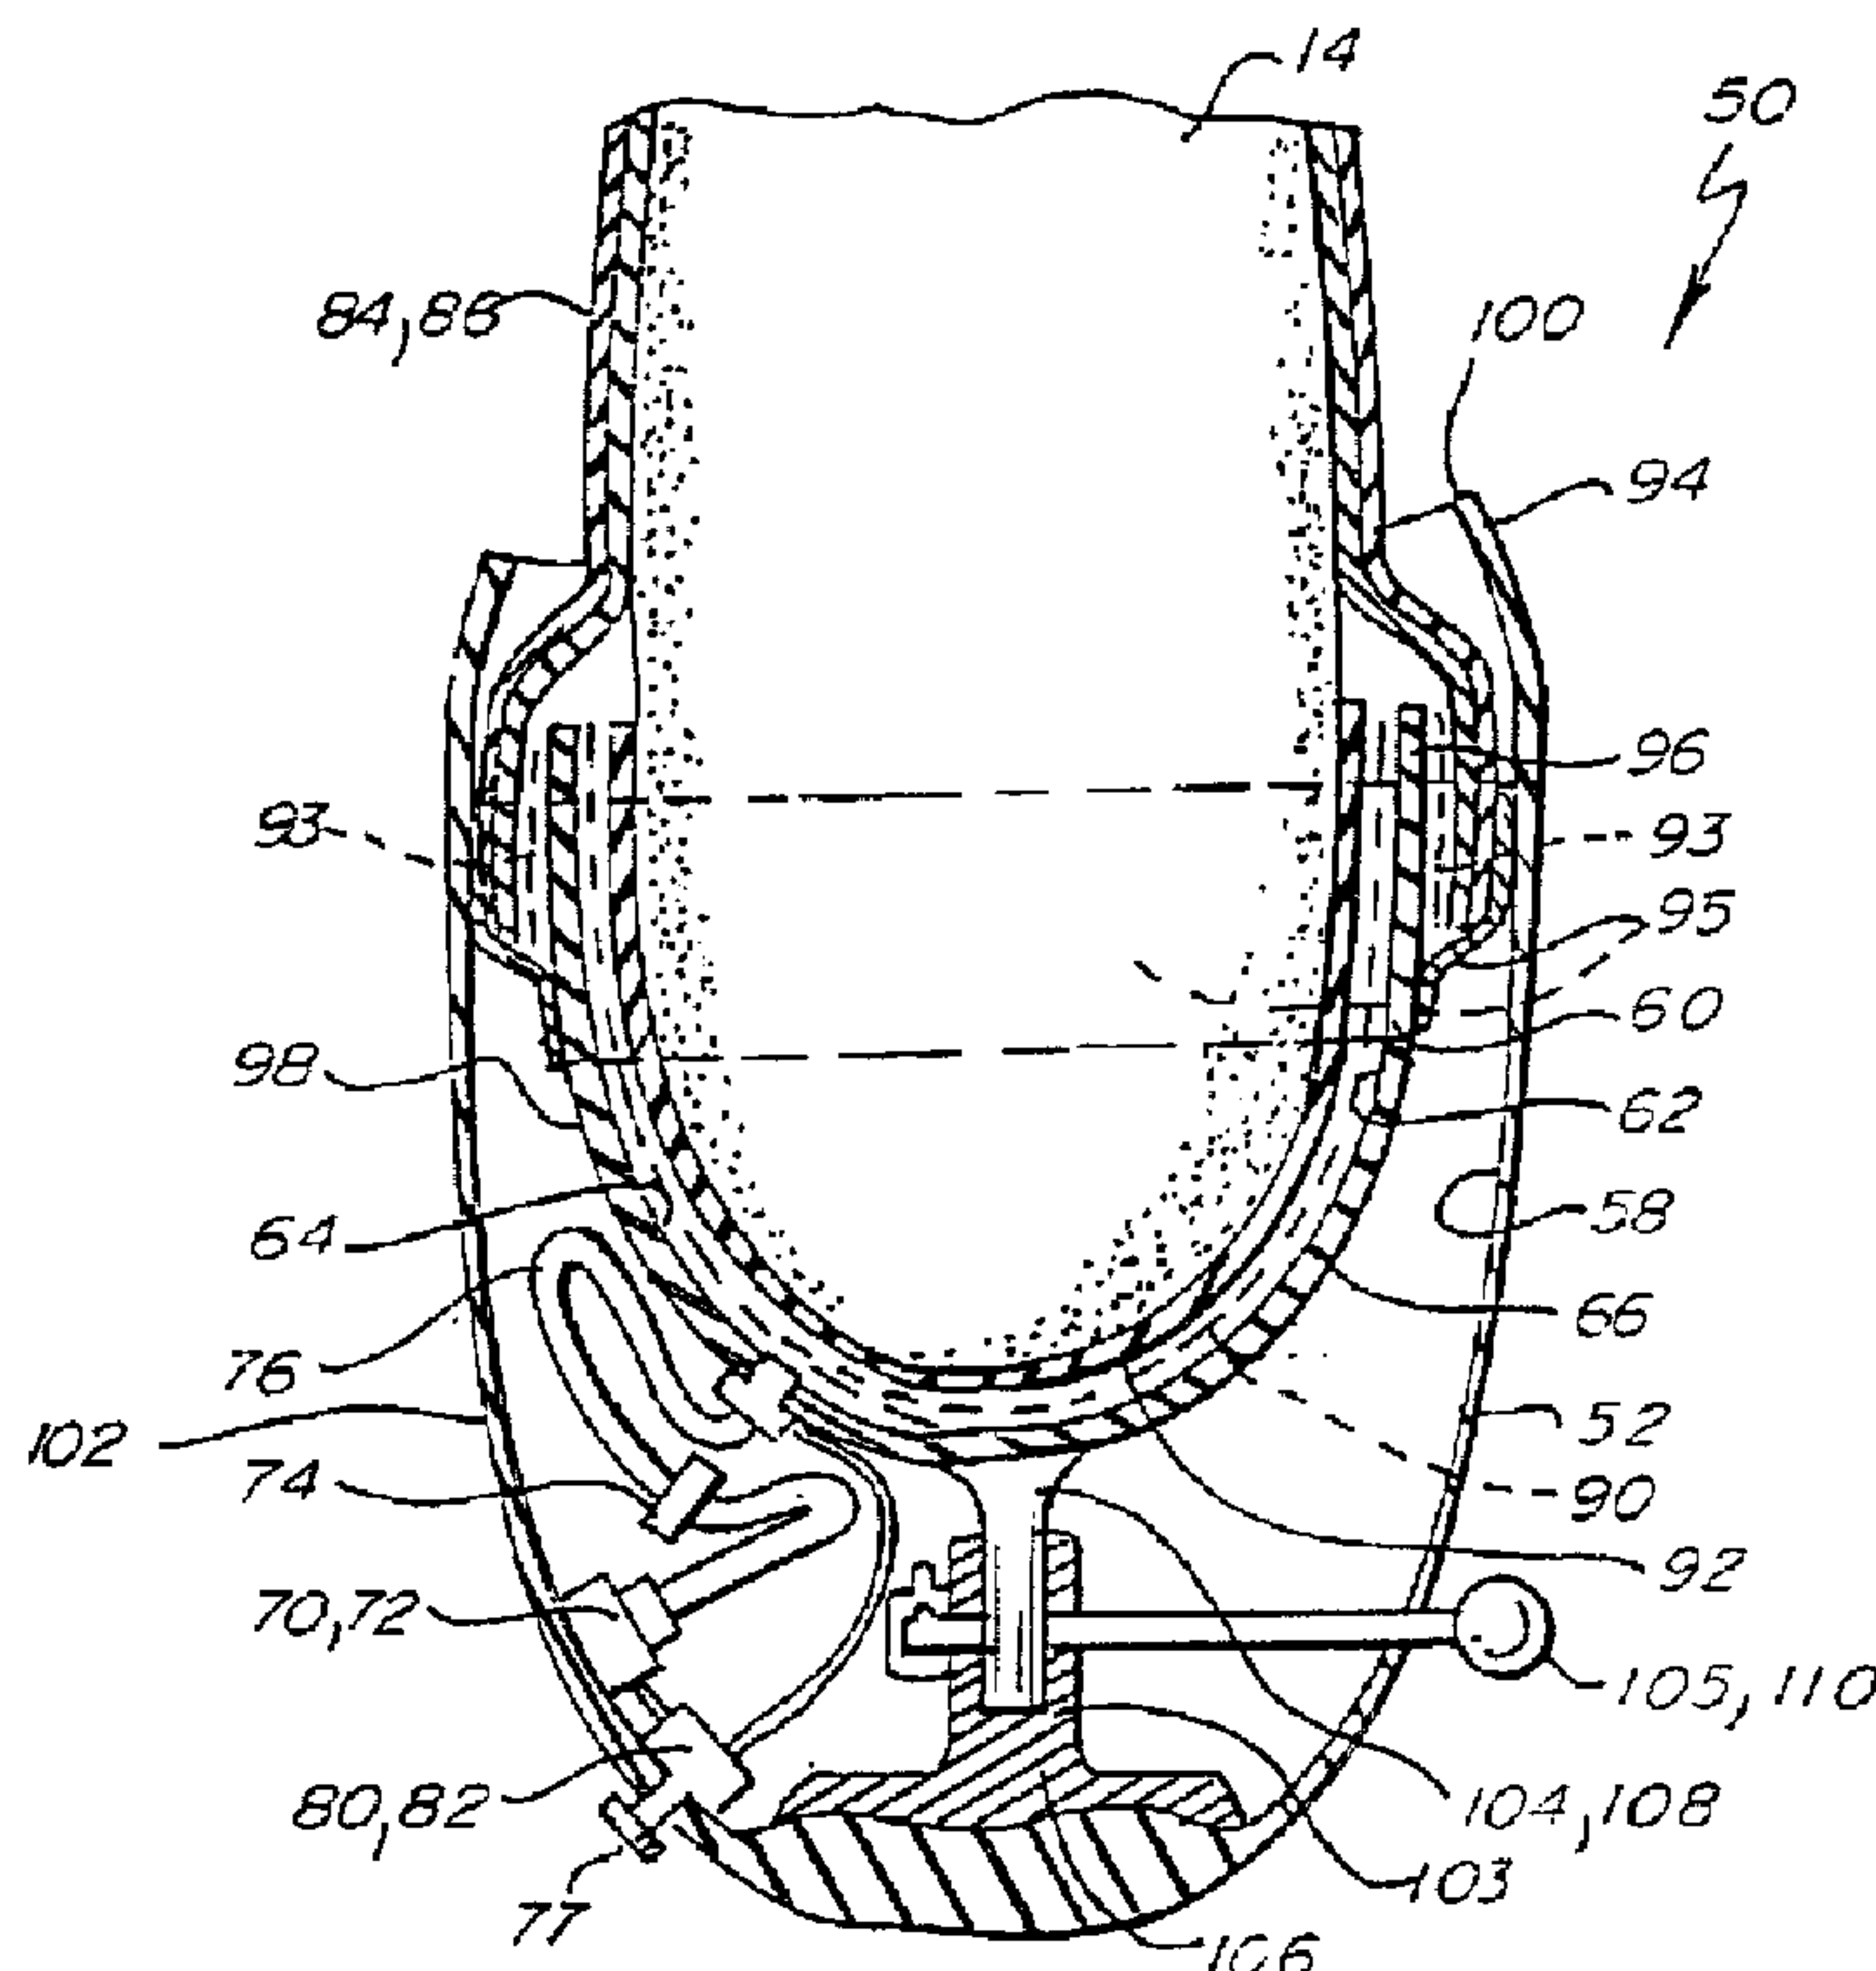

(57) Abrégé/Abstract:

A hypobarically-controlled artificial limb for amputees includes an outer socket, a flexible, compressible inner socket within the outer socket with a cavity for receiving the residual limb, a space between the inner socket and the outer socket, a vacuum source connected to the cavity, a positive pressure source connected to the space, a regulator for controlling the vacuum source and positive pressure source, and a seal for making an airtight seal between the residual limb and the socket. Another embodiment includes a semi-compressible molding material in the space to mold to the contours of the residual limb under the influence of vacuum and/or positive pressure. Another embodiment includes a positive mechanical interlock between the inner socket and the outer socket.



- 37 -

ABSTRACT OF THE DISCLOSURE

A hypobarically-controlled artificial limb for amputees includes an outer socket, a flexible, compressible inner socket within the outer socket with a cavity for receiving the residual limb, a space between the inner socket and the outer socket, a vacuum source connected to the cavity, a positive pressure source connected to the space, a regulator for controlling the vacuum source and positive pressure source, and a seal for making an airtight seal between the residual limb and the socket. Another embodiment includes a semi-compressible molding material in the space to mold to the contours of the residual limb under the influence of vacuum and/or positive pressure. Another embodiment includes a positive mechanical interlock between the inner socket and the outer socket.

HYPOBARICALLY-CONTROLLED, DOUBLE-SOCKET ARTIFICIAL LIMB WITH MECHANICAL INTERLOCK

BACKGROUND OF THE INVENTION

The present invention relates to prosthetic devices and more particularly to a hypobarically-controlled artificial limb for amputees.

An amputee is a person who has lost part of an extremity or limb such as a leg or arm which commonly may be termed as a residual limb. Residual limbs come in various sizes and shapes with respect to the stump. That is, most new amputations are either slightly bulbous or cylindrical in shape while older amputations that may have had a lot of atrophy are generally more conical in shape. Residual limbs may further be characterized by their various individual problems or configurations including the volume and shape of a stump and possible scar, skin graft, bony prominence, uneven limb volume, neuroma, pain, edema or soft tissue configurations.

Referring to FIGS. 1 and 2, a below the knee residual limb 10 is shown and described as a leg 12 having been severed below the knee terminating in a stump 14. In this case, the residual limb 10 includes soft tissue as well as the femur 16, knee joint 18, and severed tibia 20 and fibula 22. Along these bone structures surrounded by soft tissue are nerve bundles and vascular routes which must be protected against external pressure to avoid neuromas, numbness and discomfort as well as other kinds of problems. A below the knee residual limb 10 has its stump 14 generally characterized as being a more bony structure while an above the knee residual limb may be characterized as including more soft tissue as well as the vascular routes and nerve bundles.

Referring to FIG. 2, amputees who have lost a part of their arm 26, which terminates in a stump 28 also may be characterized as having vascular routes, nerve bundles as well as soft and bony tissues. The residual limb 10 includes the humerus bone 30 which extends from below the shoulder to the elbow from which the radius 34 and ulna 36 bones may pivotally extend to the point of severance. Along the humerus bone 30 are

- 2 -

the biceps muscle 38 and the triceps muscle 40 which still yet may be connected to the radius 34 and the ulna 36, respectively.

In some respects, the residual limb amputee that has a severed arm 26 does not have the pressure bearing considerations for an artificial limb but rather is concerned with having an artificial limb that is articulable to offer functions typical of a full arm, such as bending at the elbow and grasping capabilities. An individual who has a paralyzed limb would also have similar considerations wherein he or she would desire the paralyzed limb to have some degree of mobility and thus functionality.

Historically, artificial limbs typically used by a leg amputee were for the most part all made out of wood such as an Upland Willow. The limbs were hand carved with sockets for receiving the stump 14 of the residual limb 10. Below the socket would be the shin portion with the foot below the shin. These wooden artificial limbs were covered with rawhide which often were painted. The sockets of most wood limbs were hollow as the limbs were typically supported in the artificial limb by the circumferential tissue adjacent the stump 14 rather than at the distal end of the stump 14.

Some artificial limbs in Europe were also made from forged pieces of metal that were hollow. Fiber artificial limbs were also used which were stretched around a mold after which they were permitted to dry and cure. Again, these artificial limbs were hollow and pretty much supported the residual limb about the circumferential tissue adjacent the stump 14.

All of these various artificial limbs have sockets to put the amputee's stump 14 thereinto. There are generally two categories of sockets. There are hard sockets wherein the stump goes right into the socket actually touching the socket wall without any type of liner or stump sock. Another category of sockets is a socket that utilizes a liner or insert. Both categories of sockets typically were opened ended sockets where they had a hollow chamber in the bottom and no portion of the socket touched the distal end of the stump 14.

- 4 -

thigh. The sleeve suspensions have been used in combination with other forms of suspensions techniques.

Both the use of a positive pressure system and the use of a negative pressure system (or hypobaric closed chamber) have been utilized in the field of prosthetics. At one time, for pressure systems "inflatable inner tubes" were used to fit into sockets. Presently, there are pneumatic "bags" which are strategically placed over what people consider to be good weight-bearing areas to increase pressure to help accommodate for volume changes within the socket.

The problem with this is that it is a very specific pressure and creates atrophy and loss of tissue dramatically over these high pressure areas. None of these systems employs positive pressure distributed over the total contact area between the residual limb and the artificial limb socket to accommodate volume changes within the socket.

The negative pressure aspects have been utilized for a closed chamber in that a socket is donned by pulling in with a sock, pulling the sock out of the socket and then closing the opening with a valve. This creates a seal at the bottom and the stump is held into the socket by the hypobaric seal. However, there are no systems that employ a negative pressure produced by a vacuum pump to lock the residual limb to the artificial limb.

The older systems were initially started in Germany. They were an open-ended socket, meaning there was an air chamber in the bottom of the socket. This did not work particularly well because it would cause swelling of the residual limb into the chamber created by the negative draw of suspending the weight of the leg and being under a confined area. This would lead to significant edema which would be severe enough to cause stump breakdown and drainage.

It was later discovered in America that total contact was essential between the residual limb and the socket and once you had total contact the weight was distributed

(f) a seal means for making an airtight seal between the residual limb and said inner socket.

