



US00D385352S

United States Patent [19]

Bales et al.

[11] Patent Number: Des. 385,352

[45] Date of Patent: **Oct. 21, 1997

[54] SUTURE ANCHOR SCREW

[75] Inventors: Joel P. Bales, Warsaw, Ind.; S. Kyle Hayes, Laguna Niguel, Calif.

[73] Assignee: Zimmer, Inc., Warsaw, Ind.

[**] Term: 14 Years

[21] Appl. No.: 22,242

[22] Filed: May 2, 1994

[51] LOC (6) CL 24-02

[52] U.S. Cl. D24/145

[58] Field of Search D24/145, 146;
D15/138, 139; 606/67, 62, 65, 73, 232,
87, 79, 82

[56] References Cited

U.S. PATENT DOCUMENTS

| | | | |
|------------|---------|-----------------------|-----------|
| D. 331,463 | 12/1992 | Rosenberg et al. | D24/145 |
| 4,632,100 | 12/1986 | Somers et al. | 128/92 |
| 4,959,064 | 9/1990 | Engelhardt | 606/65 |
| 5,013,316 | 5/1991 | Goble et al. | D24/145 X |
| 5,098,435 | 3/1992 | Stednitz et al. | 606/79 X |
| 5,100,417 | 3/1992 | Cerier et al. | 606/139 |
| 5,102,421 | 4/1992 | Anspach, Jr. | 606/232 |
| 5,141,520 | 8/1992 | Goble et al. | 606/232 |
| 5,156,616 | 10/1992 | Meadows et al. | 606/232 |
| 5,259,398 | 11/1993 | Vrespa | 606/67 X |
| 5,268,001 | 12/1993 | Nicholson et al. | 606/72 |
| 5,364,400 | 11/1994 | Rego, Jr. et al. | D24/145 X |
| 5,370,662 | 12/1994 | Stone et al. | 606/73 X |
| 5,411,506 | 5/1995 | Goble et al. | D24/145 X |

OTHER PUBLICATIONS

Zimmer, Inc. lit.—Resistance to Suture Abrasion of the Statak Device—1993.

Linvtatec lit.—Rotator Cuff Repair With A New Twist—Orthopedics Today—Jul. 1993.

Zimmer, Inc. lit.—Mini Statak Subcortical Insertion—1993.
Arthrotek lit.—The Harpoon—JBJS, Mar. 1994.

Primary Examiner—Doris V. Coles
Assistant Examiner—I. Simmons
Attorney, Agent, or Firm—Cary R. Reeves



[57] CLAIM




The ornamental design for a suture anchor screw, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a suture anchor screw showing an embodiment our new design;
 FIG. 2 is a side elevational view thereof;
 FIG. 3 is a side elevational view thereof, rotated ninety degrees from the view of FIG. 2;
 FIG. 4 is a side elevational view thereof, rotated ninety degrees from the view of FIG. 3;
 FIG. 5 is a side elevational view thereof; rotated ninety degrees from the view of FIG. 4;
 FIG. 6 is a bottom plan view thereof; and
 FIG. 7 is a top plan view thereof;
 FIG. 8 is a perspective view of a suture anchor screw showing a second embodiment of my new design;
 FIG. 9 is a side elevational view thereof;
 FIG. 10 is a side elevational view thereof, rotated ninety degrees from the view of FIG. 2;
 FIG. 11 is a side elevational view thereof, rotated ninety degrees from the view of FIG. 3;
 FIG. 12 is a side elevational view thereof; rotated ninety degrees from the view of FIG. 4;
 FIG. 13 is a bottom plan view thereof; and,
 FIG. 14 is a top plan view thereof.

1 Claim, 4 Drawing Sheets

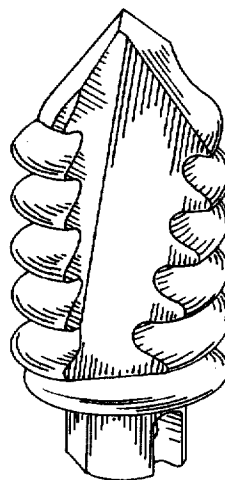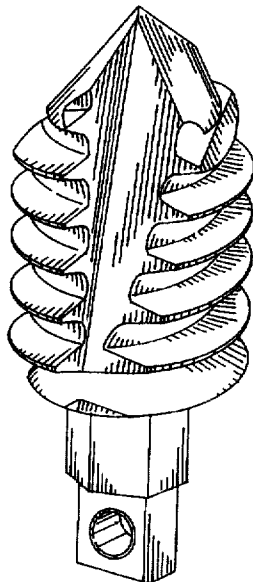

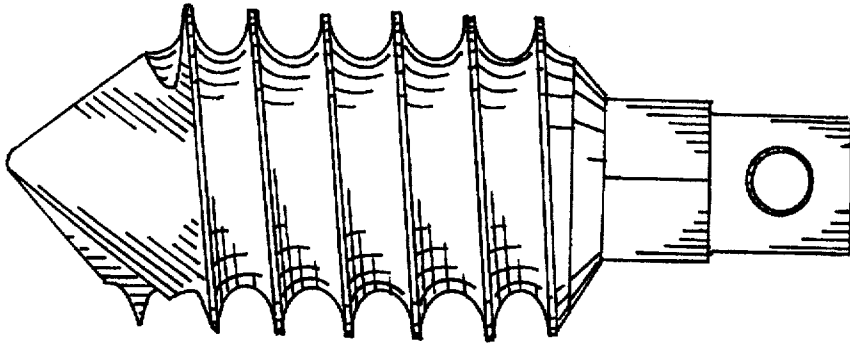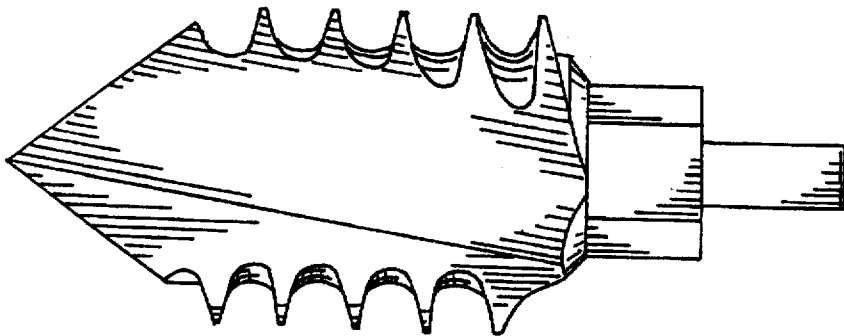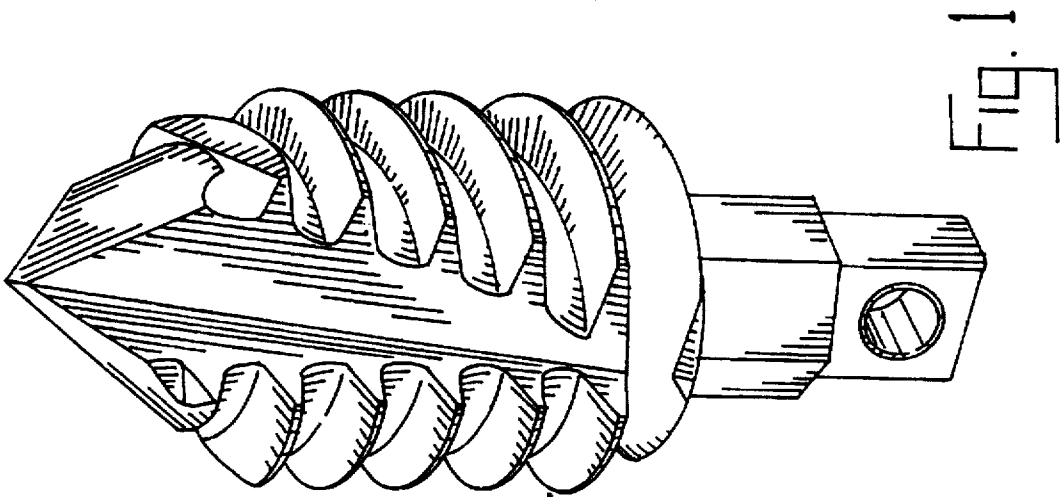

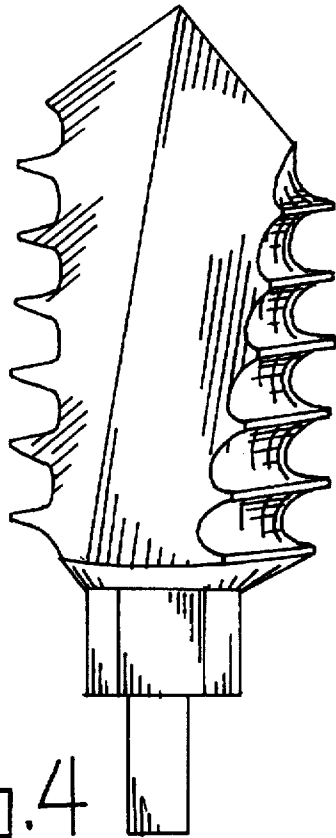


Fig. 4

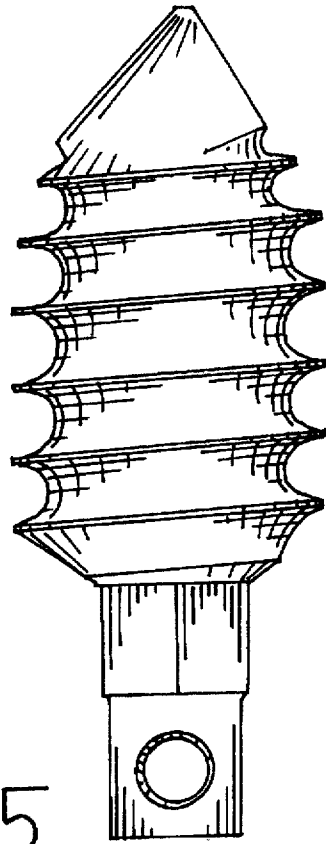


Fig. 5

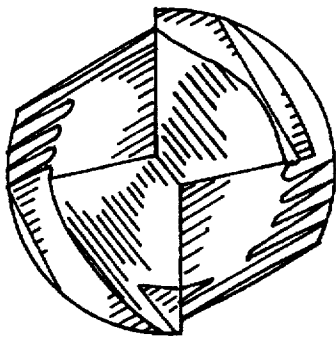


Fig. 6

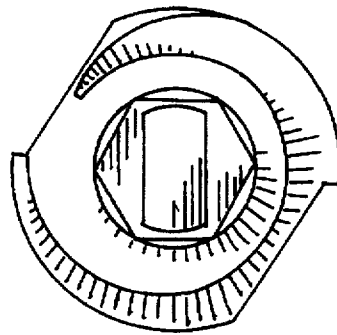


Fig. 7

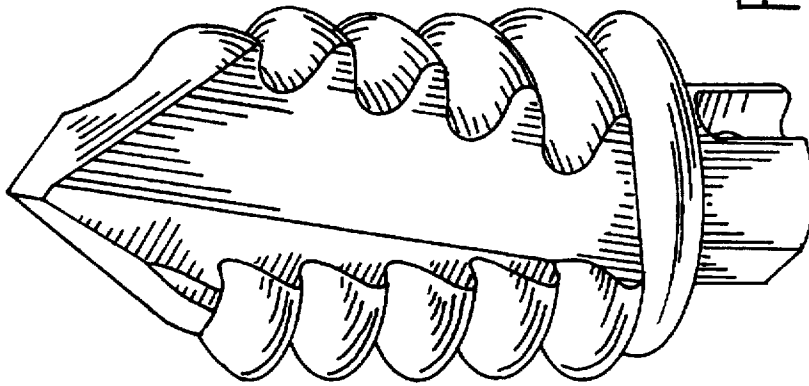


FIG. 8

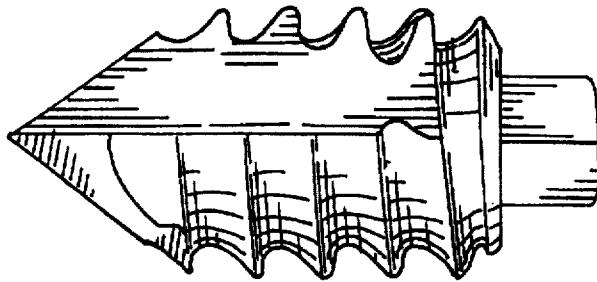


FIG. 9

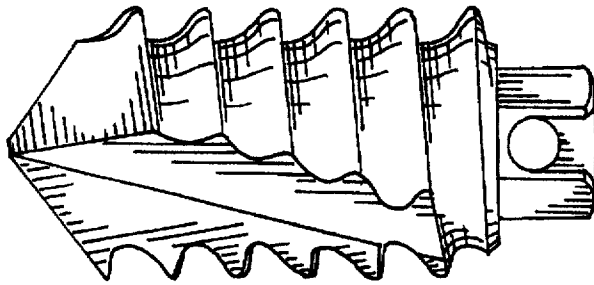


FIG. 10

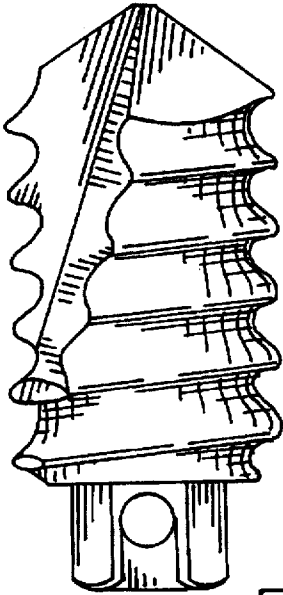


Fig. 12

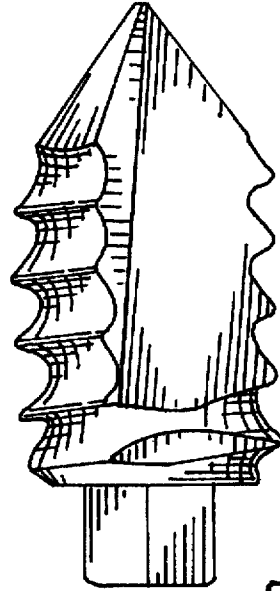


Fig. 11




Fig. 13




Fig. 14